

Thursday, February 25, 2010

LOS ALAMOS
NATIONAL LABORATORY

Page 1 of 3
REQUEST NUMBER: 10-2093

ATTN: Valerie Davis

General Engineering Laboratories, Inc., Charleston, SC.

2040 Savage Rd

Charleston, SC 29407

These Samples are on:

LANL Request Number: 10-2093

Per Agreement Number: 126310011

Project Cost Code: MR3A05529E00

Please analyse the enclosed samples
according to the schedule indicated:

SHIP DATE: 2/25/2010

TURNAROUND/REPORT DUE: 3/27/2010


TURNAROUND REQ'D: 30 Days

RAD SCREENING: Yes, Below Background

LAB REQUEST COMMENTS:

LANL ER SMO CONTACT:

Signature:

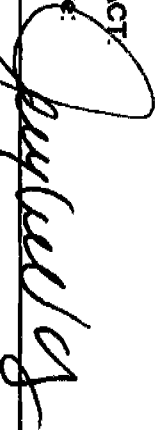

PRIORITY	METHOD CODE	CNTNR	SAMPLE ID	SAMPLE MATRIX	DATE SAMPLED	SPECIAL INSTRUCTIONS
----------	-------------	-------	-----------	---------------	--------------	----------------------

EPA:300.0	1	1	RE36-10-8448	R	2/22/2010	
-----------	---	---	--------------	---	-----------	--

	1	1	RE36-10-8449	R	2/22/2010	
--	---	---	--------------	---	-----------	--

	1	1	RE36-10-8450	R	2/22/2010	
--	---	---	--------------	---	-----------	--

	1	1	RE36-10-8451	R	2/22/2010	
--	---	---	--------------	---	-----------	--

	1	1	RE36-10-8452	R	2/22/2010	
--	---	---	--------------	---	-----------	--

	1	1	RE36-10-8453	R	2/22/2010	
--	---	---	--------------	---	-----------	--

	1	1	RE36-10-8456	R	2/22/2010	
--	---	---	--------------	---	-----------	--

EPA:353.2	1	1	RE36-10-8458	W	2/22/2010	
-----------	---	---	--------------	---	-----------	--

SW-846:6010B	1	1	RE36-10-8448	R	2/22/2010	
--------------	---	---	--------------	---	-----------	--

Thursday, February 25, 2010

REQUEST NUMBER: 10-2093

PRIORITY	METHOD CODE	CNTNR	SAMPLE ID	SAMPLE MATRIX	DATE SAMPLED	SPECIAL INSTRUCTIONS
SW-846:6010B	1	1	RE36-10-8449	R	2/22/2010	
			RE36-10-8450	R	2/22/2010	
			RE36-10-8451	R	2/22/2010	
			RE36-10-8452	R	2/22/2010	
			RE36-10-8453	R	2/22/2010	
			RE36-10-8456	R	2/22/2010	
			RE36-10-8448	R	2/22/2010	
			RE36-10-8449	R	2/22/2010	
			RE36-10-8450	R	2/22/2010	
			RE36-10-8451	R	2/22/2010	
SW-846:6020	1	1	RE36-10-8452	R	2/22/2010	
			RE36-10-8453	R	2/22/2010	
			RE36-10-8456	R	2/22/2010	
			RE36-10-8458	W	2/22/2010	
			RE36-10-8448	R	2/22/2010	
			RE36-10-8449	R	2/22/2010	
			RE36-10-8450	R	2/22/2010	
			RE36-10-8451	R	2/22/2010	
			RE36-10-8452	R	2/22/2010	
			RE36-10-8453	R	2/22/2010	
SW-846:6850	1	1	RE36-10-8456	W	2/22/2010	
			RE36-10-8458	R	2/22/2010	
			RE36-10-8448	R	2/22/2010	
			RE36-10-8449	R	2/22/2010	
			RE36-10-8450	R	2/22/2010	
			RE36-10-8451	R	2/22/2010	
			RE36-10-8452	R	2/22/2010	
			RE36-10-8453	R	2/22/2010	
			RE36-10-8456	R	2/22/2010	
			RE36-10-8458	W	2/22/2010	
SW-846:7470A	1	1	RE36-10-8458	W	2/22/2010	
			RE36-10-8456	R	2/22/2010	
			RE36-10-8448	R	2/22/2010	
			RE36-10-8449	R	2/22/2010	
			RE36-10-8450	R	2/22/2010	
			RE36-10-8451	R	2/22/2010	
			RE36-10-8452	R	2/22/2010	
			RE36-10-8453	R	2/22/2010	
			RE36-10-8456	R	2/22/2010	
			RE36-10-8458	W	2/22/2010	
SW-846:7471A	1	1	RE36-10-8458	W	2/22/2010	
			RE36-10-8456	R	2/22/2010	
			RE36-10-8448	R	2/22/2010	
			RE36-10-8449	R	2/22/2010	
			RE36-10-8450	R	2/22/2010	
			RE36-10-8451	R	2/22/2010	
			RE36-10-8452	R	2/22/2010	
			RE36-10-8453	R	2/22/2010	
			RE36-10-8456	R	2/22/2010	
			RE36-10-8458	W	2/22/2010	

Thursday, February 25, 2010

REQUEST NUMBER: 10-2093

PRIORITY	METHOD CODE	CNTNR	SAMPLE ID	SAMPLE MATRIX	DATE SAMPLED	SPECIAL INSTRUCTIONS
SW-846:9012A	SW-846:7471A	1	RE36-10-8453	R	2/22/2010	
		1	RE36-10-8456	R	2/22/2010	
		1	RE36-10-8448	R	2/22/2010	
		1	RE36-10-8449	R	2/22/2010	
		1	RE36-10-8450	R	2/22/2010	
		1	RE36-10-8451	R	2/22/2010	
		1	RE36-10-8452	R	2/22/2010	
		1	RE36-10-8453	R	2/22/2010	
		1	RE36-10-8456	R	2/22/2010	
		1	RE36-10-8458	W	2/22/2010	
SW-846:9045C	SW-846:9045C	1	RE36-10-8448	R	2/22/2010	
		1	RE36-10-8449	R	2/22/2010	
		1	RE36-10-8450	R	2/22/2010	
		1	RE36-10-8451	R	2/22/2010	
		1	RE36-10-8452	R	2/22/2010	
		1	RE36-10-8453	R	2/22/2010	
		1	RE36-10-8456	R	2/22/2010	
		1	RE36-10-8456	R	2/22/2010	
		1	RE36-10-8456	R	2/22/2010	
		1	RE36-10-8456	R	2/22/2010	

Final Page of REQUEST NUMBER 10-2093

Thursday, February 25, 2010

LAB CHAIN OF CUSTODY DOCUMENT NUMBER: 10-2093

LOS ALAMOS

REQUEST NUMBER: 10-2093

NATIONAL LABORATORY

ATTN: Valerie Davis

TURNAROUND/REPORT DUE: 3/27/2010

General Engineering Laboratories, Inc.,
Charleston, SC.

TURNAROUND REQ'D: 30

2040 Savage Rd

Charleston, SC 29407

LAB REQUEST COMMENTS:

SAMPLE ID	CTNR	CTNR DESC	ORDER	PRESERV	MATRIX
RE36-10-8458	1	POLY	METALS+U-GEL	Nitric Acid	W
RE36-10-8458	1	POLY	NO3NO2	Sulfuric Acid (Hydrogen Sulfate)	W
RE36-10-8458	1	POLY	SW-846:6850	Ice	W
RE36-10-8458	1	POLY	TCN	Sodium Hydroxide	W
RE36-10-8448	1	POLY	METALS+U-GEL	Ice	R
RE36-10-8448	1	POLY	Perchlorate+CN+N03+pH	Ice	R
RE36-10-8456	1	POLY	METALS+U-GEL	Ice	R
RE36-10-8456	1	POLY	Perchlorate+CN+N03+pH	Ice	R
RE36-10-8451	1	POLY	METALS+U-GEL	Ice	R
RE36-10-8451	1	POLY	Perchlorate+CN+N03+pH	Ice	R
RE36-10-8450	1	POLY	METALS+U-GEL	Ice	R
RE36-10-8450	1	POLY	Perchlorate+CN+N03+pH	Ice	R
RE36-10-8449	1	POLY	METALS+U-GEL	Ice	R
RE36-10-8449	1	POLY	Perchlorate+CN+N03+pH	Ice	R
RE36-10-8453	1	POLY	METALS+U-GEL	Ice	R
RE36-10-8453	1	POLY	Perchlorate+CN+N03+pH	Ice	R
RE36-10-8452	1	POLY	METALS+U-GEL	Ice	R
RE36-10-8452	1	POLY	Perchlorate+CN+N03+pH	Ice	R

Relinquished By:

Date Time

Received By:

Date Time

Printed Name

Signature

Printed Name

Signature

Printed Name

Signature

Printed Name

Signature

Printed Name

Signature

Printed Name

Signature

Received for DISPOSAL By:

Date Time

Remarks:

Printed Name

Signature

SAMPLE COLLECTION LOG/FIELD CHAIN OF CUSTODY

EVENT ID: 2510

EVENT NAME: 4th Qtr. FY09 - SWMU 36-002 - Threemile Canyon

SAMPLE ID: RE36-10-8448

WORK ORDER:

AS PLANNED		AS COLLECTED		AS PLANNED		AS COLLECTED	
DATE COLLECTED(MM/DD/YYYY):		02/22/2010		MEDIA:	QBT3	QBT 2	
TIME COLLECTED (HH:MM)		09:30		SUB-MEDIA:	TUFF 1	OK	
PRS ID:	36-002	OK		SAMPLE TECH CODE:	HA	CBS	
LOCATION ID:	36-610876			FIELD QC TYPE:	NA	OK	
LOCATION TYPE:	GENERIC			FIELD PREP:	NA		
TOP DEPTH:	0	7.5 ft		SAMPLE USAGE:	INV		
BOTTOM DEPTH:	0	10.0 ft		SCREEN/PORT DESC:		NA	
FIELD MATRIX:	R	OK		EXCAVATED: YES/NO/NA	NO/NA		
COMPOSITE TYPE:	NA			COMPOSITE TIME INTERVAL:	NA		
				WATER FLOWING: YES/NO/NA	NO/NA		
BOREHOLE: YES/NO/NA				BOREHOLE DECLINATION: -90°			
				BOREHOLE DIRECTION: NA			

#	PRIORITY	ORDER	CNTNR	PRESERVATIVE	COLLECTED Y/N	SPECIAL INSTRUCTIONS
1	Normal	8260B	125 ML SEPTUM AMBER GLASS	Ice	Y	
1		AM241+GS+ISO PU+ISOU	1 LITER POLY	None		
1		H3	500 ML POLY	Ice		
1		METALS+U-GEL	125 ML POLY	Ice		
1		Perchlorate+CN+N03+pH	500 ML POLY	Ice		
1		RADVA NA+B+G	1 EA 8 IN RESEALABLE POLY BAG	None		
1		8082+8270+NME D-EXP	500 ML AMBER GLASS	Ice		

SAMPLE DESC:

F0=36-10-8456

Light brownish gray, strongly indurated, partially welded, devitrified dry, ash flow tuff

SAMPLE COMMENTS: NA

LOCATION DESC: 2-1

FIELD SCREENING/MEASUREMENT RESULTS:

Alpha = 36 dpm
Beta/Gamma = 3332 dpm

PID ^{12m} Ambient Reading = ppm
2/22/10

COLLECTED BY (PRINT)

R. Saunders

REVIEWED BY (PRINT)

J. Marin

RELINQUISHED BY	Date/Time	RECEIVED BY	Date/Time
(Printed Name) JON MARIN	2/23/10	(Printed Name) Sherri Newwood	2/23/10
(Signature) Jon R. Marin	0812 AM	(Signature) Sherri Newwood	0812
RELINQUISHED BY	Date/Time	RECEIVED BY	Date/Time

SAMPLE COLLECTION LOG/FIELD CHAIN OF CUSTODY

EVENT ID: 2510

EVENT NAME: 4th Qtr. FY09 - SWMU 36-002 - Threemile Canyon

SAMPLE ID: RE36-10-8449

WORK ORDER:

AS PLANNED		AS COLLECTED		AS PLANNED		AS COLLECTED	
DATE COLLECTED(MM/DD/YYYY):		02/22/2010	0	MEDIA:	QBT2		QBT2
TIME COLLECTED (HH:MM)		09:50		SUB-MEDIA:	TUFF 1		OK
PRS ID:	36-002	OK		SAMPLE TECH CODE:	HA		CBS
LOCATION ID:	36-610876			FIELD QC TYPE:	NA		OK
LOCATION TYPE:	GENERIC			FIELD PREP:	NA		
TOP DEPTH:	0	15.0 ft		SAMPLE USAGE:	INV		
BOTTOM DEPTH:	0	16.0 ft		SCREEN/PORT DESC:			NA
FIELD MATRIX:	R			EXCAVATED: YES/NO/NA			
COMPOSITE TYPE:	NA			COMPOSITE TIME INTERVAL:	NA		
BOREHOLE:	YES/NO/NA			BOREHOLE DECLINATION:	-90°		
				BOREHOLE DIRECTION:	NA		

#	PRIORITY	ORDER	CNTNR	PRESERVATIVE	COLLECTED Y/N	SPECIAL INSTRUCTIONS
1	Normal	8260B	125 ML SEPTUM AMBER GLASS	Ice	Y	
1		AM241+GS+ISO PU+ISOU	1 LITER POLY	None		
1		H3	500 ML POLY	Ice		
1		METALS+U- GEL	125 ML POLY	Ice		
1		Perchlorate+CN+ N03+pH	500 ML POLY	Ice		
1		RADVANA+B+G	1 EA 8 IN RESEALABLE POLY BAG	None		
1		8082+8270+NME D-EXP	500 ML AMBER GLASS	Ice		

SAMPLE DESC:

Light brownish gray, moderately indurated, slightly welded,
detritified, dy, ash flow tuff

SAMPLE COMMENTS: NA

LOCATION DESC: 2-1

FIELD SCREENING/MEASUREMENT RESULTS:

Alpha < 41 dpm
Beta/Gamma < 2280 dpm

PID Ambient ^{7RM} 2/22/10
Reading = ppm

COLLECTED BY (PRINT)

REVIEWED BY (PRINT) J. MARIN

RELINQUISHED BY	Date/Time	RECEIVED BY	Date/Time
(Printed Name) JON MARIN	2/23/10	(Printed Name) Sherri Sherwood	2/23/10
(Signature) J. Marin	0812 AM	(Signature) Sherri Sherwood	0812
RELINQUISHED BY	Date/Time	RECEIVED BY	Date/Time

SAMPLE COLLECTION LOG/FIELD CHAIN OF CUSTODY

EVENT ID: 2510

EVENT NAME: 4th Qtr. FY09 - SWMU 36-002 - Threemile Canyon

SAMPLE ID: RE36-10-8450

WORK ORDER:

AS PLANNED		AS COLLECTED		AS PLANNED		AS COLLECTED	
DATE COLLECTED(MM/DD/YYYY):		02/22/2010	MEDIA:	QBT3		QBT2	
TIME COLLECTED (HH:MM)		10:45	SUB-MEDIA:	TUFF1		OK	
PRS ID:	36-002	OK	SAMPLE TECH CODE:	HA		CB S	
LOCATION ID:	36-610877		FIELD QC TYPE:	NA			
LOCATION TYPE:	GENERIC		FIELD PREP:	NA			
TOP DEPTH:	0	9.0 ft	SAMPLE USAGE:	INV			
BOTTOM DEPTH:	0	10.0 ft	SCREEN/PORT DESC:			NA	
FIELD MATRIX:	R	OK	EXCAVATED: YES <input checked="" type="checkbox"/> NO <input type="checkbox"/> NA				
COMPOSITE TYPE:	NA		COMPOSITE TIME INTERVAL:	NA		WATER FLOWING: YES <input checked="" type="checkbox"/> NO <input type="checkbox"/> NA	
BOREHOLE: YES <input checked="" type="checkbox"/> NO <input type="checkbox"/> NA		BOREHOLE DECLINATION: -90°		BOREHOLE DIRECTION: NA			

#	PRIORITY	ORDER	CNTNR	PRESERVATIVE	COLLECTED Y/N	SPECIAL INSTRUCTIONS
1	Normal	8260B	125 ML SEPTUM AMBER GLASS	Ice	Y	
1		AM241+GS+ISO PU+ISOU	1 LITER POLY	None		
1		H3	500 ML POLY	Ice		
1		METALS+U-GEL	125 ML POLY	Ice		
1		Perchlorate+CN+N03+pH	500 ML POLY	Ice		
1		RADVANA+B+G ARM 2/22/10	1 EA 8 IN RESEALABLE POLY BAG	None		
1		8082+8270+NME D-EXP	500 ML AMBER GLASS	Ice		

SAMPLE DESC:

Light reddish brown, moderately indurated, slightly welded, devitrified, dry, arch flow tuft with some fracture fill clay

SAMPLE COMMENTS: NA

LOCATION DESC: 2-2

FIELD SCREENING/MEASUREMENT RESULTS:

Alpha \leq 41 dpm
Beta/Gamma \leq 1976 dpm

PID $\frac{\text{Ambient Reading}}{\text{Reading}} = \text{ppm}$

COLLECTED BY (PRINT)

R. Saunders

REVIEWED BY (PRINT) J. MARIN

RELINQUISHED BY	Date/Time	RECEIVED BY	Date/Time
(Printed Name) JON MARIN	2/23/10	(Printed Name) Sherrif Herwood	2/23/10
(Signature) Jon R. Marin	0812 AM	(Signature) Sherrif Herwood	0812
RELINQUISHED BY	Date/Time	RECEIVED BY	Date/Time

SAMPLE COLLECTION LOG/FIELD CHAIN OF CUSTODY

EVENT ID: 2510

EVENT NAME: 4th Qtr. FY09 - SWMU 36-002 - Threemile Canyon

SAMPLE ID: RE36-10-8451

WORK ORDER:

AS PLANNED		AS COLLECTED		AS PLANNED		AS COLLECTED	
DATE COLLECTED(MM/DD/YYYY):		02/22/2010		MEDIA:	QBT3		QBT 2
TIME COLLECTED(HH:MM)		10:55		SUB-MEDIA:	TUFF 1		OK
PRS ID:	36-002	OK		SAMPLE TECH CODE:	HA		CB5
LOCATION ID:	36-610877			FIELD QC TYPE:	NA		OK
LOCATION TYPE:	GENERIC			FIELD PREP:	NA		
TOP DEPTH:	0	14.0 ft		SAMPLE USAGE:	INV		
BOTTOM DEPTH:	0	15.0 ft		SCREEN/PORT DESC:			NA
FIELD MATRIX:	R	OK		EXCAVATED: YES/NO/NA			
COMPOSITE TYPE:	NA			COMPOSITE TIME INTERVAL:	NA		WATER FLOWING: YES/NO/NA
BOREHOLE: YES/NO/NA		BOREHOLE DECLINATION:	-90°	BOREHOLE DIRECTION:	NA		

#	PRIORITY	ORDER	CNTNR	PRESERVATIVE	COLLECTED Y/N	SPECIAL INSTRUCTIONS
1	Normal	8260B	125 ML SEPTUM AMBER GLASS	Ice	Y	
1		AM241+GS+ISO PU+ISOU	1 LITER POLY	None		
1		H3	500 ML POLY	Ice		
1		METALS+U-GEL	125 ML POLY	Ice		
1		Perchlorate+CN+N03+pH	500 ML POLY	Ice		
1		RADVANA+B+G	1 EA 8 IN RESEALABLE POLY BAG	None		
1		2082+8270+NME D-EXP	500 ML AMBER GLASS	Ice		

SAMPLE DESC:

light brownish gray, slightly indurated, slightly welded, devitrified, dry, ash flow tuff

SAMPLE COMMENTS: NA

LOCATION DESC: 2-2

FIELD SCREENING/MEASUREMENT RESULTS:

Alpha = 36 dpm
Beta/Gamma = 2090 dpm

PID ^{Ambient} Reading = ppm

COLLECTED BY (PRINT)

R. Saunders

REVIEWED BY (PRINT)

J. MARIN

RELINQUISHED BY	Date/Time	RECEIVED BY	Date/Time
(Printed Name) JON MARIN	2/23/10	(Printed Name) Sheri Herwood	2/23/10
(Signature) J. R. Marin	08:12 AM	(Signature) Sheri Herwood	08:12
RELINQUISHED BY	Date/Time	RECEIVED BY	Date/Time

SAMPLE COLLECTION LOG/FIELD CHAIN OF CUSTODY

EVENT ID: 2510

EVENT NAME: 4th Qtr. FY09 - SWMU 36-002 - Threemile Canyon

SAMPLE ID: RE36-10-8452

WORK ORDER:

AS PLANNED		AS COLLECTED		AS PLANNED		AS COLLECTED	
DATE COLLECTED(MM/DD/YYYY):		02/22/2010		MEDIA:	QBT3	QBT2	
TIME COLLECTED (HH:MM)		11:40		SUB-MEDIA:	TUFF 1	OK	
PRS ID:	36-002	OK		SAMPLE TECH CODE:	HA	CBS	
LOCATION ID:	36-610878			FIELD QC TYPE:	NA	OK	
LOCATION TYPE:	GENERIC			FIELD PREP:	NA		
TOP DEPTH:	0	4.0 ft		SAMPLE USAGE:	INV		
BOTTOM DEPTH:	0	5.0 ft		SCREEN/PORT DESC:		NA	
FIELD MATRIX:	B	OK		EXCAVATED: YES/NO/NA	NO		
COMPOSITE TYPE:	NA			COMPOSITE TIME INTERVAL:	NA		
BOREHOLE: YES/NO/NA	NA			WATER FLOWING: YES/NO/NA	NO		
BOREHOLE DECLINATION:	-90°			BOREHOLE DIRECTION:	NA		

#	PRIORITY	ORDER	CNTNR	PRESERVATIVE	COLLECTED Y/N	SPECIAL INSTRUCTIONS
1	Normal	8260B	125 ML SEPTUM AMBER GLASS	Ice	Y	
1		8270C+NMED Exp	500 ML AMBER GLASS	Ice		
1		AM241+GS+ISO PU+ISOU	1 LITER POLY	None		
1		H3	500 ML POLY	Ice		
1		METALS+U-GEL	125 ML POLY	Ice		
1		Perchlorate+CN+N03+pH	500 ML POLY	Ice		
1		RADVANA+B+G	1 EA 8 IN RESEALABLE POLY BAG	None		

SAMPLE DESC:

Dark reddish brown, clay rich, moderately indurated, slightly welded, devitrified, moist, ash flow tuff

SAMPLE COMMENTS: NA

LOCATION DESC: 2-3

FIELD SCREENING/MEASUREMENT RESULTS:

Alpha = 56 dpm
Beta/Gamma = 2070 dpm

PID ^{from 2/23/10} Ambient Reading = ppm

COLLECTED BY (PRINT)

R. Saunders

REVIEWED BY (PRINT) J. MARIN

RELINQUISHED BY	Date/Time	RECEIVED BY	Date/Time
(Printed Name) JON MARIN	2/23/10	(Printed Name) Sherrill Sherwood	2/23/10
(Signature) Jon R. Marin	08 12 AM	(Signature) Sherrill Sherwood	08 12
RELINQUISHED BY	Date/Time	RECEIVED BY	Date/Time

SAMPLE COLLECTION LOG/FIELD CHAIN OF CUSTODY

EVENT ID: 2510

EVENT NAME: 4th Qtr. FY09 - SWMU 36-002 - Threemile Canyon

SAMPLE ID: RE36-10-8453

WORK ORDER:

AS PLANNED		AS COLLECTED		AS PLANNED		AS COLLECTED	
DATE COLLECTED(MM/DD/YYYY):		02/22/2010	MEDIA:	QBT3		QBT 2	
TIME COLLECTED (HH:MM)		11:50	SUB-MEDIA:	TUFF 1		OK	
PRS ID:	36-002	OK	SAMPLE TECH CODE:	HA		CBS	
LOCATION ID:	36-610878		FIELD QC TYPE:	NA		OK	
LOCATION TYPE:	GENERIC		FIELD PREP:	NA			
TOP DEPTH:	0	9.0 ft	SAMPLE USAGE:	INV			
BOTTOM DEPTH:	0	10.0 ft	SCREEN/PORT DESC:			NA	
FIELD MATRIX:	R	OK	EXCAVATED: YES/NO/NA				
COMPOSITE TYPE:	NA		COMPOSITE TIME INTERVAL:	NA		WATER FLOWING: YES/NO/NA	
BOREHOLE: YES/NO/NA			BOREHOLE DECLINATION: -90°			BOREHOLE DIRECTION: NA	

#	PRIORITY	ORDER	CNTNR	PRESERVATIVE	COLLECTED Y/N	SPECIAL INSTRUCTIONS
1	Normal	8260B	125 ML SEPTUM AMBER GLASS ^{from newish clear}	Ice	Y	
1		8270C+NMED Exp	500 ML AMBER GLASS	Ice	1	
1		AM241+GS+ISO PU+ISOU	1 LITER POLY	None		
1		H3	500 ML POLY	Ice		
1		METALS+U-GEL	125 ML POLY	Ice		
1		Perchlorate+CN+ N03+ph	500 ML POLY	Ice		
1		RADVANA+B+G	1 EA 8 IN RESEALABLE POLY BAG	None		

SAMPLE DESC:

Reddish brown, moderately indurated, clay rich, slightly welded, devitrified, moist, altered ash flow tuff

SAMPLE COMMENTS:

NA

LOCATION DESC:

2-3

FIELD SCREENING/MEASUREMENT RESULTS:

Alpha \leq 46 dpm
Beta/Gamma \leq 2150 dpm

PID $\frac{\text{Ambient Reading}}{\text{Reading}} = \text{ppm}$

COLLECTED BY (PRINT)

R. Saunders

REVIEWED BY (PRINT) J. MARIN

RELINQUISHED BY	Date/Time	RECEIVED BY	Date/Time
(Printed Name) JON MARIN	2/23/10	(Printed Name) Sheri Sherwood	2/23/10
(Signature) Jon R. Marin	0812 AM	(Signature) Sheri Sherwood	0812
RELINQUISHED BY	Date/Time	RECEIVED BY	Date/Time

SAMPLE COLLECTION LOG/FIELD CHAIN OF CUSTODY

EVENT ID: 2510

EVENT NAME: 4th Qtr. FY09 - SWMU 36-002 - Threemile Canyon

SAMPLE ID: RE36-10-8456

WORK ORDER:

AS PLANNED		AS COLLECTED		AS PLANNED		AS COLLECTED	
DATE COLLECTED(MM/DD/YYYY):		02/22/2010		MEDIA:	QBT3		QBT2
TIME COLLECTED(HH:MM)		09:30		SUB-MEDIA:	TUFF1		OK
PRS ID:	36-002	OK		SAMPLE TECH CODE:	HA		C13S
LOCATION ID:	UNK	36-610876		FIELD QC TYPE:	ED		OK
LOCATION TYPE:	GENERIC	OK		FIELD PREP:	NA		
TOP DEPTH:	0	7.5 ft		SAMPLE USAGE:	QC		
BOTTOM DEPTH:	0	10.0 ft		SCREEN/PORT DESC:			NA
FIELD MATRIX:	R			EXCAVATED: YES/NO/NA			
COMPOSITE TYPE:	-	NA		COMPOSITE TIME INTERVAL:	NA		WATER FLOWING: YES/NO/NA
BOREHOLE: YES/NO/NA				BOREHOLE DECLINATION: -90°			BOREHOLE DIRECTION: NA

#	PRIORITY	ORDER	CNTNR	PRESERVATIVE	COLLECTED Y/N	SPECIAL INSTRUCTIONS
1	Normal	8260B	125 ML SEPTUM AMBER GLASS	Ice	Y	
1		AM241+GS+ISO PU+ISOU	1 LITER POLY	None		
1		H3	500 ML POLY	Ice		
1		METALS+U-GEL	125 ML POLY	Ice		
1		Perchlorate+CN+N03+ph	500 ML POLY	Ice		
1		RADVANA+B+G	1 EA 8 IN RESEALABLE POLY BAG	None		
1		8082+8270+NME D-EXP	500 ML AMBER GLASS	Ice		

SAMPLE DESC: QC Sample of RE 36-10-8448

Light brown ish gray, strongly indurated, partially welded dehydrified, dry, ash flow tuff.

SAMPLE COMMENTS:

LOCATION DESC: 2-1

FIELD SCREENING/MEASUREMENT RESULTS:

Alpha = 36 dpm
Beta/Gamma = 3330 dpm

PID Ambient Reading = ppm

COLLECTED BY (PRINT)

R. Saunders

REVIEWED BY (PRINT)

J. MARIN

RELINQUISHED BY	Date/Time	RECEIVED BY	Date/Time
(Printed Name) JON MARIN	2/23/10	(Printed Name) Sherrif Newwood	2/23/10
(Signature) J. R. Marin	18:15AM	(Signature) Sherrif Newwood	0815
RELINQUISHED BY	Date/Time	RECEIVED BY	Date/Time

SAMPLE COLLECTION LOG/FIELD CHAIN OF CUSTODY

EVENT ID: 2510

EVENT NAME: 4th Qtr. FY09 - SWMU 36-002 - Threemile Canyon

SAMPLE ID: RE36-10-8458

WORK ORDER:

AS PLANNED		AS COLLECTED		AS PLANNED		AS COLLECTED	
DATE COLLECTED(MM/DD/YYYY):		02/22/2010		MEDIA:	NA		OK
TIME COLLECTED(HH:MM)		11:10		SUB-MEDIA:	OTHER		
PRS ID:	36-002	OK		SAMPLE TECH CODE:	DC		
LOCATION ID:	UNK	36-610877		FIELD QC TYPE:	ER		
LOCATION TYPE:	GENERIC	OK		FIELD PREP:	UF		
TOP DEPTH:	0			SAMPLE USAGE:	QC		
BOTTOM DEPTH:	0			SCREEN/PORT DESC:			NA
FIELD MATRIX:	W			EXCAVATED: YES/NO/NA			
COMPOSITE TYPE:	NA			COMPOSITE TIME INTERVAL:	NA		
BOREHOLE: (YES/NO/NA)				WATER FLOWING: YES/NO/NA			
BOREHOLE DECLINATION:		-90°		BOREHOLE DIRECTION:	NA		

#	PRIORITY	ORDER	CNTNR	PRESERVATIVE	COLLECTED Y/N	SPECIAL INSTRUCTIONS
1	Normal	METALS+U-GEL	1 LITER POLY	Nitric Acid	Y	
1		NO3NO2	250 ML POLY	Sulfuric Acid (Hydrogen Sulfate)	N	
1	Normal	SW-846:6850	250 ML POLY	Ice	Y	
1	Normal	TCN	500 ML POLY	Sodium Hydroxide	Y	

SAMPLE DESC: QC Sample of RE36-10-8451

SAMPLE COMMENTS: NA

LOCATION DESC: 2-2

FIELD SCREENING/MEASUREMENT RESULTS:

1/26/10 ^{LC}
 Alpha = _____ dpm
 Beta/Gamma = _____ dpm

1/26/10 ^{LC}
 PID $\frac{\text{Ambient Reading}}{\text{Reading}} = \text{ppm}$

COLLECTED BY (PRINT)

R. Saunders

REVIEWED BY (PRINT)

J. MARIN

RELINQUISHED BY (Printed Name) JON MARIN (Signature) Jon R. Marin	Date/Time 2/23/10 08:12 AM	RECEIVED BY (Printed Name) Sheri Sherwood (Signature) Sheri Sherwood	Date/Time 2/23/10 08:12
RELINQUISHED BY (Printed Name) (Signature)	Date/Time	RECEIVED BY (Printed Name) (Signature)	Date/Time

SAMPLE COLLECTION LOG/FIELD CHAIN OF CUSTODY

EVENT ID: 2510

EVENT NAME: 4th Qtr, FY09 - SWMU 36-002 - Threemile Canyon

SAMPLE ID: RE36-10-8460

WORK ORDER:

AS PLANNED		AS COLLECTED		AS PLANNED		AS COLLECTED	
DATE COLLECTED(MM/DD/YYYY):		02/22/2010		MEDIA:		NA	
TIME COLLECTED (HH:MM)		09:00		SUB-MEDIA:		OTHER	
PRS ID: 36-002		OK		SAMPLE TECH CODE:		DC	
LOCATION ID: UNK		36-610876		FIELD QC TYPE:		ETB	
LOCATION TYPE: GENERIC		OK		FIELD PREP:		NA	
TOP DEPTH: 0				SAMPLE USAGE:		QC	
BOTTOM DEPTH: 0				SCREEN/PORT DESC:		NA	
FIELD MATRIX: S				EXCAVATED: YES/NO/NA		NA	
COMPOSITE TYPE: NA		COMPOSITE TIME INTERVAL: NA		WATER FLOWING: YES/NO/NA		NA	
BOREHOLE: YES/NO/NA		BOREHOLE DECLINATION: -90°		BOREHOLE DIRECTION: NA			

#	PRIORITY	ORDER	CNTNR	PRESERVATIVE	COLLECTED Y/N	SPECIAL INSTRUCTIONS
2AM 7/2	Normal	8260B Trip Blank	40 ML SEPTUM AMBER GLASS	Ice	Y	

SAMPLE DESC: QC Sample of RE36-10-8448

SAMPLE COMMENTS: NA

LOCATION DESC: 36-610876

FIELD SCREENING/MEASUREMENT RESULTS: NA

COLLECTED BY (PRINT)

R. Saunders

REVIEWED BY (PRINT) J. MARIN

RELINQUISHED BY (Printed Name) JON MARIN (Signature) J. R. Marin	Date/Time 2/23/10 0815 AM	RECEIVED BY (Printed Name) Sheri Sherwood (Signature) Sheri Sherwood	Date/Time 2/23/10 0815
RELINQUISHED BY (Printed Name) (Signature)	Date/Time	RECEIVED BY (Printed Name) (Signature)	Date/Time

Rad Screening Data Release Form

The Following samples were received at the Field Support Facility (FSF) without screening data (list sample number):

RE36-10-8453 8456
8452
8458
8451
8450
8449
8448

These samples will not be shipped until radiological screening data documentation arrives at the FSF. I understand that it is my responsibility to ensure this information arrives at the FSF in a timely manner. If holding times are missed because screening data does not arrive, I will pick up the samples.

.....
The following samples do not require rad screening data for the reasons stated (list sample numbers):

RE36-10-8460


Reason:

Field Release

.....
Print Last Name Lujan

Signature 

Date 2/23/10

DATA VALIDATION COVER SHEET	
5121-1 <p style="text-align: center;">Data Validation Cover Sheet</p>	Records Use only 

Section I.		
REQUEST NUMBER: <u>10-2093</u>	VALIDATION DATE: <u>04/26/2010</u>	LAB CODE: <u>GEL</u>
CONTRACT LABORATORY NAME: <u>GEL Laboratories LLC</u>		
VALIDATOR: <u>Mary Donovan</u> ORGANIZATION: <u>Analytical Quality Associates, Inc.</u>		
ANALYTICAL SUITE (CHECK ALL THAT APPLY):		
<input type="checkbox"/> TPH-GRO	<input type="checkbox"/> HIGH EXPLOSIVES	<input type="checkbox"/> DIOXIN FURANS
<input type="checkbox"/> TPH-DRO	<input type="checkbox"/> METALS	<input type="checkbox"/> PCB CONGENERS
<input type="checkbox"/> GENERAL CHEMISTRY	<input type="checkbox"/> RADIOCHEMISTRY	<input type="checkbox"/> LCMSMS HIGH EXPLOSIVES
		<input checked="" type="checkbox"/> LCMSMS PERCHLORATES
		<input type="checkbox"/> ORGANOCHLORINE PESTICIDES/POLYCHLORINATED BIPHENYLS
<input type="checkbox"/> OTHER (DESCRIBE): _____		


Section II. Completeness Check							
YES	NO	N/A	(CHECK ONE)	YES	NO	N/A	(CHECK ONE)
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	1. CHAIN-OF-CUSTODY FORM(S)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	6. RAW/BSS DATA
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	2. CASE NARRATIVE	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	7. QUALITY CONTROL FORMS
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	3. SAMPLE RESULT FORMS	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	8. QUANTITATION REPORTS
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	4. SAMPLE CHROMATOGRAMS	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	9. TICS FORMS
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	5. STANDARD CHROMATOGRAMS	<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	10. TICS MASS SPECTRA

Comments/problems noted (include information about requests for further information submitted to the contract laboratory and agreed-upon date of resolution and contract laboratory point of contact):


1. The soil MSD %R was < 75% but ≥10% for perchlorate. However, the parent sample concentration was >4X the spike concentration and, thus, no sample results were qualified, based on professional judgment.
2. The MS/MSD %R calculations were performed incorrectly for the aqueous analyses. The parent sample result was < the MDL and, thus, a result of 0 ug/L should have been used to calculate the %Rs. The laboratory subtracted the parent sample concentration. The %Rs were within the acceptance limits when calculated correctly. It should be noted that the parent samples for the MS/MSD for both matrices were LANL samples from other RNs and that the raw data for the parent samples were not included in the data package. No sample data were qualified as a result.

Reviewed by: Monica Dymerski Level I Date: 04/27/10


VALIDATOR'S SIGNATURE: ## Mary A. Donovan DATE: 04/26/2010

LC/MS/MS PERCHLORATE ANALYTICAL DATA VALIDATION CHECKLIST	
5121-2 LC/MS/MS Perchlorate Analytical Data Validation Checklist	Records Use only 

Yes No N/A				Assign Qualifier Listed Below If Criterion = Yes	
(Check One)				Non-detected Analyte	Detected Analyte
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. The Internal Standard (IS) relative retention time has shifted by more than 0.98 to 1.02 seconds.	R, PERC0	J, PERC0
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. Required IS retention time documentation is missing. Data may not be acceptable for use. Contact the SMO or external laboratory for information.	R, PERC0b	R, PERC0b
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	3. The IS are count is <25% of the expected value.	UJ, PERC1a	J, PERC1a
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	4. The IS area count is <70% but >25% of the average of that obtained from the calibration standards.	UJ, PERC1b	J, PERC1b
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	5. The IS area count is >130% of the average of that obtained from the calibration standards.	UJ, PERC1c	J, PERC1c
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	6. Required IS information is missing. Data may not be acceptable for use. Contact the SMO or external laboratory for information.	R, PERC1d	R, PERC1d
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	7. The sample result is $\leq 5X$ the concentration of the related analyte in the method blank.	U, PERC4	N/A
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	8. The affected analytes are considered estimated and biased high because this analyte was identified in the method blank but was $>5X$.	N/A	J+, PERC4a
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	9. The sample result is $\leq 5X$ the concentration of the related analyte in the trip blank, rinsate blank, and/or equipment blank.	U, PERC4d	N/A
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	10. Required method blank information is missing. Data may not be acceptable for use. Contact the SMO or external laboratory for information.	R, PERC4e	R, PERC4e
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	11. The affected results were not analyzed with a valid 5-point calibration curve and/or a standard at the reporting limit.	UJ, PERC7	J, PERC7
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	12. The affected analytes were analyzed with an initial calibration curve that exceeded the %RSD criteria and/or the associated multipoint calibration correlation coefficient is <0.99 .	UJ, R, PERC7a	J, PERC7a

LC/MS/MS PERCHLORATE ANALYTICAL DATA VALIDATION CHECKLIST		
5121-2		Records Use only
LC/MS/MS Perchlorate Analytical Data Validation Checklist		

Yes No N/A				Assign Qualifier Listed Below If Criterion = Yes	
(Check One)				Non-detected Analyte	Detected Analyte
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	13. The ICV and/or CCV were recovered outside the method limits.	UJ, R, PERC7c	J, PERC7c
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	14. The ICV and/or CCV were not analyzed at the appropriate method frequency.	UJ, R, PERC7d	J, PERC7d
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	15. Required calibration information is missing or samples were analyzed on an expired calibration. Contact the SMO or external laboratory for information.	R, PERC7f	R, PERC7f
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	16. The affected analyte is considered not detected because ion abundance ratios did not meet specifications.	N/A	R, PERC8
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	17. The ion ratio documentation is missing. Data may not be acceptable for use. Contact the SMO or external laboratory for information.	N/A	R, PERC8a
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	18. The holding time was >1 and ≤2 times the applicable holding time requirement.	UJ PERC9	J-, PERC9
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	19. The holding time was > 2 times the applicable holding time requirement.	R, PERC9a	J-, PERC9a
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	20. The LCS percent recovery was <10%. Follow the external laboratory limits.	R, PERC12	J-, PERC12
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	21. The LCS percent recovery was < the Lower Acceptance Limit but >10%. Follow the external laboratory limits.	UJ, PERC12a	J-, PERC12a
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	22. The LCS percent recovery was > the Upper Acceptance Limit. Follow the external laboratory limits.	N/A	J+, PERC12b
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	23. The LCS documentation is missing. Data may not be acceptable for use. Contact the SMO or external laboratory for information.	R, PERC12c	R, PERC12c
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	24. The MS/MSD percent recovery was <10%	R, PERC12d	R, PERC12d
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	25. The MS/MSD percent recovery was >10% but <75%	UJ, PERC12e	J, PERC12e
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	26. The MS/MSD percent recovery was >125%.	N/A	J+, PERC12f

LC/MS/MS PERCHLORATE ANALYTICAL DATA VALIDATION CHECKLIST	
5121-2	Records Use only
LC/MS/MS Perchlorate Analytical Data Validation Checklist	

Yes No N/A				Assign Qualifier Listed Below If Criterion = Yes	
(Check One)				Non-detected Analyte	Detected Analyte
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	27. The MS/MSD relative percent difference was >20%.	UJ, PERC12g	J, PERC12g
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	28. The affected analytes are considered suspect because the sample was diluted without any target analytes identified due to matrix interference. Qualify as Reject if the analytical laboratory cannot provide proof for matrix interference.	UJ, R, PERC15	N/A
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	29. The sample was diluted because target analytes were > the initial verification calibration.	UJ, PERC15a	J, PERC15a
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	30. The Contract Required Detection Limit check standard (CRI) sample did not pass method-acceptance limits.	UJ, R, PERC16	J, PERC16
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	31. The Interference Check Sample was not within $\pm 20\%$ of the known value.	UJ, PERC16a	J, PERC16a
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	32. The required CRI sample information is missing. Contact the SMO or external laboratory for information.	R, PERC16c	R, PERC16c
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	33. The LANL project chemist identified quality deficiencies in the reported data that require further qualification. This code can ONLY be used and/or under advisement by the LANL project chemist.	UJ, R, PERC19	J, R, PERC19
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	34. Duplicate, dilution, or reanalysis.	UJ, PERC88	J, PERC88

Form 1

Perchlorate Analysis Data Sheet

Lab Name: GEL Laboratories LLC
 Lab Code: GEL
 Instrument: LCMSMS
 Method: SW846 6850 Modified
 Matrix: WATER
 Extraction Batch ID: 959046
 Extraction Type: Filter/DAI
 Client Sample No. RE36-10-8458
 Date Received: 26-FEB-10
 GEL Job No (SDG): 10-2093
 GEL Sample ID: 248117001
 Date Filtered: 05-MAR-10
 Injection Volume (uL): 20
 %Solids:
 Sample Volume/Weight: 10.0 mL
 Concentrated Extract Volume: 10.0

CAS No.	Analyte [^]	MDL	RL	Conc*	Units	Q	Dilution Factor	Date Analyzed	GEL File ID
14797-73-0	Perchlorate	.05	.2	0.050	ug/L	U	1	09-MAR-10 08:24	per0308111a
	Perchlorate Isotope Ratio						1	09-MAR-10 08:24	per0308111a
14797-73-0	Perchlorate-101	.05	.2	0.050	ug/L	U	1	09-MAR-10 08:24	per0308111a
	Perchlorate-O(18)			0.452	ug/L		1	09-MAR-10 08:24	per0308111a

[^] When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

*Concentration =

Instrument Value X Concentrated Extract Volume X $\frac{1}{\% \text{Solids}}$
 Aliquot

MAD
04/26/10

Form 1

Perchlorate Analysis Data Sheet

Lab Name: GEL Laboratories LLC

Lab Code: GEL

Instrument: LCMSMS

Method: SW846 6850 Modified

Matrix: SOIL

Extraction Batch ID: 959007

Extraction Type: Solid Prep

Sample Volume/Weight: 2.00 g

Concentrated Extract Volume: 20.0

Client Sample No.

RE36-10-8448

Date Received: 26-FEB-10

GEL Job No (SDG): 10-2093-1

GEL Sample ID: 248118001

Date Filtered: 12-MAR-10

Injection Volume (uL): 20

%Solids: 97.3

CAS No.	Analyte [^]	MDL	RL	Conc*	Units	Q	Dilution Factor	Date Analyzed	GEL File ID
14797-73-0	Perchlorate	.514	2.05	0.514	ug/kg	U	1	19-MAR-10 13:07	per0319015a
	Perchlorate Isotope Ratio								
14797-73-0	Perchlorate-101	.514	2.05	0.514	ug/kg	U	1	19-MAR-10 13:07	per0319015a
	Perchlorate-O(18)			4.89	ug/kg		1	19-MAR-10 13:07	per0319015a

[^] When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

*Concentration =

Instrument Value X Concentrated Extract Volume X 1
Aliquot %Solids

MAD
04/26/10

Form 1

Perchlorate Analysis Data Sheet

Lab Name: GEL Laboratories LLC

Lab Code: GEL

Instrument: LCMSMS

Method: SW846 6850 Modified

Matrix: SOIL

Extraction Batch ID: 959007

Extraction Type: Solid Prep

Sample Volume/Weight: 2.00 g

Concentrated Extract Volume: 20.0

Client Sample No.

RE36-10-8456

Date Received: 26-FEB-10

GEL Job No (SDG): 10-2093-1

GEL Sample ID: 248118002

Date Filtered: 12-MAR-10

Injection Volume (uL): 20

%Solids: 97.2

CAS No.	Analyte [^]	MDL	RL	Conc*	Units	Q	Dilution Factor	Date Analyzed	GEL File ID
14797-73-0	Perchlorate	.514	2.06	0.514	ug/kg	U	1	19-MAR-10 13:14	per0319016a
	Perchlorate Isotope Ratio						1	19-MAR-10 13:14	per0319016a
14797-73-0	Perchlorate-101	.514	2.06	0.514	ug/kg	U	1	19-MAR-10 13:14	per0319016a
	Perchlorate-Q(18)			4.99	ug/kg		1	19-MAR-10 13:14	per0319016a

[^] When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

*Concentration =

Instrument Value X $\frac{\text{Concentrated Extract Volume}}{\text{Aliquot}}$ X $\frac{1}{\% \text{Solids}}$

MAD
04/26/10

Form 1

Perchlorate Analysis Data Sheet

Lab Name: GEL Laboratories LLC
 Lab Code: GEL
 Instrument: LCMSMS
 Method: SW846 6850 Modified
 Matrix: SOIL
 Extraction Batch ID: 959007
 Extraction Type: Solid Prep
 Sample Volume/Weight: 2.00 g
 Concentrated Extract Volume: 20.0
 Client Sample No. RE36-10-8451
 Date Received: 26-FEB-10
 GEL Job No (SDG): 10-2093-1
 GEL Sample ID: 248118003
 Date Filtered: 12-MAR-10
 Injection Volume (uL): 20
 %Solids: 27

CAS No.	Analyte^	MDL	RL	Conc*	Units	Q	Dilution Factor	Date Analyzed	GEL File ID
14797-73-0	Perchlorate	.516	2.06	0.516	ug/kg	U	1	19-MAR-10 13:21	per0319017a
	Perchlorate Isotope Ratio						1	19-MAR-10 13:21	per0319017a
14797-73-0	Perchlorate-101	.516	2.06	0.516	ug/kg	U	1	19-MAR-10 13:21	per0319017a
	Perchlorate-O(18)			5.11	ug/kg		1	19-MAR-10 13:21	per0319017a

^ When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

*Concentration =
 Instrument Value X Concentrated Extract Volume X 1
 Aliquot %Solids

MAD
 04/26/10

Form 1

Perchlorate Analysis Data Sheet

Lab Name: GEL Laboratories LLC

Lab Code: GEL

Instrument: LCMSMS

Method: SW846 6850 Modified

Matrix: SOIL

Extraction Batch ID: 959007

Extraction Type: Solid Prep

Sample Volume/Weight: 2.00 g

Concentrated Extract Volume: 20.0

Client Sample No.

RE36-10-8450

Date Received: 26-FEB-10

GEL Job No (SDG): 10-2093-1

GEL Sample ID: 248118004

Date Filtered: 12-MAR-10

Injection Volume (uL): 20

% Solids: 85

CAS No.	Analyte [^]	MDL	RL	Conc*	Units	Q	Dilution Factor	Date Analyzed	GEL File ID
14797-73-0	Perchlorate	.588	2.35	1.27	ug/kg	J	1	19-MAR-10 13:28	per0319018a
	Perchlorate Isotope Ratio			3.24			1	19-MAR-10 13:28	per0319018a
14797-73-0	Perchlorate-101	.588	2.35	1.14	ug/kg	J	1	19-MAR-10 13:28	per0319018a
	Perchlorate-O(18)			5.73	ug/kg		1	19-MAR-10 13:28	per0319018a

[^] When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

*Concentration =

Instrument Value X Concentrated Extract Volume X 1
Aliquot %Solids

MAD
04/26/10

Form 1

Perchlorate Analysis Data Sheet

Lab Name: GEL Laboratories LLC

Lab Code: GEL

Instrument: LCMSMS

Method: SW846 6850 Modified

Matrix: SOIL

Extraction Batch ID: 959007

Extraction Type: Solid Prep

Sample Volume/Weight: 2.00 g

Concentrated Extract Volume: 20.0

Client Sample No.

RE36-10-8449

Date Received: 26-FEB-10

GEL Job No (SDG): 10-2093-1

GEL Sample ID: 248118005

Date Filtered: 12-MAR-10

Injection Volume (uL): 20

%Solids: 98.2

CAS No.	Analyte [^]	MDL	RL	Conc*	Units	Q	Dilution Factor	Date Analyzed	GEL File ID
14797-73-0	Perchlorate	.509	2.04	0.509	ug/kg	U	1	19-MAR-10 13:35	per0319019a
	Perchlorate Isotope Ratio						1	19-MAR-10 13:35	per0319019a
14797-73-0	Perchlorate-101	.509	2.04	0.509	ug/kg	U	1	19-MAR-10 13:35	per0319019a
	Perchlorate-O(18)			4.85	ug/kg		1	19-MAR-10 13:35	per0319019a

[^] When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

*Concentration =

Instrument Value X Concentrated Extract Volume X 1
Aliquot %Solids

MAD
04/26/10

Form 1

Perchlorate Analysis Data Sheet

Lab Name: GEL Laboratories LLC
 Lab Code: GEL
 Instrument: LCMSMS
 Method: SW846 6850 Modified
 Matrix: SOIL
 Extraction Batch ID: 959007
 Extraction Type: Solid Prep
 Sample Volume/Weight: 2.00 g
 Concentrated Extract Volume: 20.0

Client Sample No.
RE36-10-8453
 Date Received: 26-FEB-10
 GEL Job No (SDG): 10-2093-1
 GEL Sample ID: 248118006
 Date Filtered: 12-MAR-10
 Injection Volume (uL): 20
 %Solids: 95.7

CAS No.	Analyte [^]	MDL	RL	Conc*	Units	Q	Dilution Factor	Date Analyzed	GEL File ID
14797-73-0	Perchlorate	.522	2.09	3.77	ug/kg		1	19-MAR-10 13:42	per0319020a
	Perchlorate Isotope Ratio			2.99			1	19-MAR-10 13:42	per0319020a
14797-73-0	Perchlorate-101	.522	2.09	3.67	ug/kg		1	19-MAR-10 13:42	per0319020a
	Perchlorate-O(18)			5.32	ug/kg		1	19-MAR-10 13:42	per0319020a

[^] When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

*Concentration =
 Instrument Value X Concentrated Extract Volume X 1
 Aliquot %Solids

MAD
 04/26/10

Form 1

Perchlorate Analysis Data Sheet

Lab Name: GEL Laboratories LLC
 Lab Code: GEL
 Instrument: LCMSMS
 Method: SW846 6850 Modified
 Matrix: SOIL
 Extraction Batch ID: 959007
 Extraction Type: Solid Prep
 Sample Volume/Weight: 2.00 g
 Concentrated Extract Volume: 20.0
 Client Sample No. RE36-10-8452
 Date Received: 26-FEB-10
 GEL Job No (SDG): 10-2093-1
 GEL Sample ID: 248118007
 Date Filtered: 12-MAR-10
 Injection Volume (uL): 20
 %Solids: 92.9

CAS No.	Analyte [^]	MDL	RL	Conc*	Units	Q	Dilution Factor	Date Analyzed	GEL File ID
14797-73-0	Perchlorate	.538	2.15	2.32	ug/kg		1	19-MAR-10 13:49	per0319021a
	Perchlorate Isotope Ratio			3.09			1	19-MAR-10 13:49	per0319021a
14797-73-0	Perchlorate-101	.538	2.15	2.19	ug/kg		1	19-MAR-10 13:49	per0319021a
	Perchlorate-O(18)			5.53	ug/kg		1	19-MAR-10 13:49	per0319021a

[^] When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

*Concentration =
 Instrument Value X $\frac{\text{Concentrated Extract Volume}}{\text{Aliquot}}$ X $\frac{1}{\% \text{Solids}}$

MAD
 04/26/10

DATA VALIDATION COVER SHEET

5118-1

Data Validation Cover Sheet

Records Use only



Section I.

REQUEST NUMBER: 10-2093 VALIDATION DATE: 04/26/2010 LAB CODE: GEL

CONTRACT LABORATORY NAME: GEL Laboratories LLC

VALIDATOR: Mary Donovan ORGANIZATION: Analytical Quality Associates, Inc.

ANALYTICAL SUITE (CHECK ALL THAT APPLY):

- | | | | |
|--|--|---|---|
| <input type="checkbox"/> TPH-GRO | <input type="checkbox"/> HIGH EXPLOSIVES | <input type="checkbox"/> DIOXIN FURANS | <input type="checkbox"/> LCMSMS PERCHLORATES |
| <input type="checkbox"/> TPH-DRO | <input checked="" type="checkbox"/> METALS | <input type="checkbox"/> PCB CONGENERS | <input type="checkbox"/> ORGANOCHLORINE |
| <input type="checkbox"/> GENERAL CHEMISTRY | <input type="checkbox"/> RADIOCHEMISTRY | <input type="checkbox"/> LCMSMS HIGH EXPLOSIVES | <input type="checkbox"/> PESTICIDES/POLYCHLORINATED BIPHENYLS |
| <input type="checkbox"/> OTHER (DESCRIBE): _____ | | | |

Section II. Completeness Check

- | YES | NO | N/A | (CHECK ONE) | YES | NO | N/A | (CHECK ONE) |
|-------------------------------------|--------------------------|-------------------------------------|-----------------------------|-------------------------------------|--------------------------|-------------------------------------|--------------------------|
| <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | 1. CHAIN-OF-CUSTODY FORM(S) | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | 6. RAW/BSS DATA |
| <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | 2. CASE NARRATIVE | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | 7. QUALITY CONTROL FORMS |
| <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | 3. SAMPLE RESULT FORMS | <input type="checkbox"/> | <input type="checkbox"/> | <input checked="" type="checkbox"/> | 8. QUANTITATION REPORTS |
| <input type="checkbox"/> | <input type="checkbox"/> | <input checked="" type="checkbox"/> | 4. SAMPLE CHROMATOGRAMS | <input type="checkbox"/> | <input type="checkbox"/> | <input checked="" type="checkbox"/> | 9. TICS FORMS |
| <input type="checkbox"/> | <input type="checkbox"/> | <input checked="" type="checkbox"/> | 5. STANDARD CHROMATOGRAMS | <input type="checkbox"/> | <input type="checkbox"/> | <input checked="" type="checkbox"/> | 10. TICS MASS SPECTRA |

Comments/problems noted (include information about requests for further information submitted to the contract laboratory and agreed-upon date of resolution and contract laboratory point of contact):

- In the aqueous MB, Pb and Tl were detected. The associated sample result for Pb was a detect $\leq 5X$ the MB concentration and, thus, was qualified U,14. The associated sample result for Tl was an ND and, thus, was not qualified. In the soil MB, Al, Ba, Fe and Mn were detected. All associated sample results were detects $> 50X$ the MB concentrations and, thus, were not qualified, based on professional judgment.
- In the ICB or CCBs associated with the aqueous sample, Se and Tl were detected. The associated sample results were NDs and, thus, were not qualified.
- In the FR blank, sample RE36-10-8458, associated with all soil samples, Ca, Cu, K, Na and Zn were detected. The Cu results for samples -8448, -8456, -8451 and -8449 were detects $\leq 5X$ the FR blank concentration and, thus, was qualified U,14d. All other associated sample results were detects $> 5X$ the greatest FR blank concentrations and, thus, were not qualified.
- The soil LCS %R was $<$ the laboratory LAL but $\geq 10\%$ for Sb. The associated sample results were NDs and, thus, were qualified UJ,112a.
- The soil MS %Rs were $<$ the laboratory LAL but $\geq 10\%$ for Sb and Se. The associated sample results were NDs and, thus, were qualified UJ,16a. The soil MS %R was $>$ the laboratory UAL for K. The associated sample results were detects and, thus, were qualified J+,16b. The soil MS %Rs were also $>$ the laboratory UAL for Al, Ca, Fe and Mg and $<$ the laboratory LAL but $\geq 10\%$ for Mn. However, the associated parent sample concentrations were $> 4X$ the spike concentrations. Thus, the associated sample results were not qualified, based on professional judgment.
- It should be noted that the matrix QC parent samples for all analyses for both matrices were LANL samples from other RNs and that the ICP-AES and ICP-MS raw data for the parent samples were not included in the data package. No sample data were qualified as a result.

DATA VALIDATION COVER SHEET

5118-1

Data Validation Cover Sheet

Records Use only




Reviewed by: Monica Dymerski **Level I** **Date:** 04/27/10


VALIDATOR'S SIGNATURE: ## Mary A. Deane DATE: 04/26/2010

Form 5118-1, Revision 0.0


LOS ALAMOS
Environmental Restoration Project

METALS ANALYTICAL DATA VALIDATION CHECKLIST	
5118-2 Metals Analytical Data Validation Checklist	Records Use only 


Yes No N/A				Assign Qualifier Listed Below If Criterion = Yes	
(Check One)				Non-detected Analyte	Detected Analyte
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. The holding time was >1 and ≤2 times the applicable holding time requirement.	UJ, I9	J-, I9
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. The holding time was >2 times the applicable holding time requirement.	R, I9a	J-, I9a
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	3. The instrument performance sample did not pass method acceptance criteria.	R, I16	R, I16
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	4. The mass calibration is not within 0.1 amu or %RSD is >5% for any isotope (Be, Mg, Co, In, Pb).	UJ, I16a	J, I16a
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	5. Samples were analyzed outside specific method tune time criteria.	N/A	J, I16b
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	6. The required instrument performance sample information is missing. Contact the SMO or external laboratory for information.	R, I16c	R, I16c
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	7. The affected results were not analyzed with a valid 5-point calibration curve and/or a standard at the reporting limit.	UJ, R, I7	J, I7
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	8. The affected analytes were analyzed with an initial calibration curve that exceeded the %RSD criteria and/or the associated multipoint calibration correlation coefficient is <0.995.	UJ, I7a	J, I7a
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	9. The Initial Calibration Verification (ICV) and/or Continuing Calibration Verification (CCV) were recovered outside the method-specific limits.	UJ, I7c	J, I7c
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	10. The ICV and/or CCV were not analyzed at the appropriate method frequency.	UJ, I7d	J, I7d
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	11. Required calibration information is missing or samples were analyzed on an expired calibration. Contact the SMO or external laboratory for information.	R, I7f	R, I7f
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	12. Metals interference check sample percent recover value is <50%.	R, I2	J-, I2

METALS ANALYTICAL DATA VALIDATION CHECKLIST	
5118-2 Metals Analytical Data Validation Checklist	Records Use only 

Yes No N/A				Assign Qualifier Listed Below If Criterion = Yes	
(Check One)				Non-detected Analyte	Detected Analyte
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	13. Metals interference check sample percent recovery value is $\geq 50\%$ and $< 80\%$	UJ, I2a	J-, I2a
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	14. Metals interference check sample percent recovery value is $> 120\%$.	N/A	J+, I2b
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	15. Metals interference check sample was not analyzed with the samples.	R, I2c	R, I2c
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	16. The sample result is $\leq 5X$ the concentration of the related analyte in the method blank.	U, I4	N/A
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	17. The affected analytes are considered estimated and biased high because this analyte was identified in the method blank but was $> 5X$.	N/A	J, I4a
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	18. The sample result is $\leq 5X$ the concentration of the related analyte in the instrument blank and continuing calibration blank.	U, I4b	N/A
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	19. Continuing calibration blanks were not analyzed at the appropriate method frequency.	UJ, I4c	J, I4c
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	20. The sample result is $\leq 5X$ the concentration of the related analyte in the trip blank, rinsate blank, or equipment blank.	U, I4d	N/A
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	21. Required method blank information is missing. Data may not be acceptable for use. Contact the SMO or external laboratory for information.	R, I4e	R, I4e
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	22. The associated matrix spike recovery was $< 10\%$. Follow the external laboratory limits located within the associated data package.	R, I6	R, I6
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	23. The associated matrix spike recovery was $< \text{the LAL}$ but $> 10\%$. Follow the external laboratory limits located within the associated data package.	UJ, I6a	J+, I6a
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	24. The associated matrix spike recovery was $> \text{the UAL}$. Follow the external laboratory limits located within the associated data package.	UJ, I6b	J+, I6b

METALS ANALYTICAL DATA VALIDATION CHECKLIST	
5118-2 Metals Analytical Data Validation Checklist	Records Use only 

Yes No N/A				Assign Qualifier Listed Below If Criterion = Yes	
(Check One)				Non-detected Analyte	Detected Analyte
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	25. Required matrix spike information is missing. Data may not be acceptable for use. Contact the SMO or external laboratory for information. If the LCS information is present, do not Reject. Qualify data based on the LCS information.	R, I6c	R, I6c
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	26. The sample and the duplicate sample results were $\geq 5X$ the RL and the duplicate RPD was $>20\%$ for water samples and $>35\%$ for soil samples.	UJ, I10a	J, I10a
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	27. The duplicate sample was not prepared and/or analyzed with the samples for unspecified reasons. The duplicate information is missing. Data may not be acceptable for use. Contact the SMO or external laboratory for information.	UJ, I10d	J, I10d
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	28. The LCS percent recovery was $<10\%$. Follow the external laboratory limits located within the associated data package.	R, I12	R, I12
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	29. The LCS percent recover was $<$ the LAL but $>10\%$. Follow the external laboratory limits located within the associated data package.	UJ, I12a	J-, I12a
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	30. The LCS percent recovery was $>$ the UAL. Follow the external laboratory limits located within the associated data package.	N/A	J+, I12b
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	31. The LCS documentation is missing. Data may not be acceptable for use. Contact the SMO or external laboratory for information. Do not Reject if MS/MSD information is present. Qualify according to MS/MSD criteria.	R, I12c	R, I12c
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	32. The quantitating IS area count is $<10\%$ for metals window in relation to the initial calibration blank. Follow the method-specific windows.	R, I1a	J, I1a

METALS ANALYTICAL DATA VALIDATION CHECKLIST	
5118-2 Metals Analytical Data Validation Checklist	Records Use only 

Yes No N/A				Assign Qualifier Listed Below If Criterion = Yes	
(Check One)				Non-detected Analyte	Detected Analyte
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	33. The IS area count for the quantitating IS is <60% but >10% for metals window in relation to the initial calibration blank. Follow the method-specific windows.	UJ, I1b	J, I1b
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	34. The IS area count for the quantitating IS is >125% in relation to the metals initial calibration blank. Follow method-specific windows.	UJ, I1c	J, I1c
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	35. Required IS information is missing. Data may not be acceptable for use. Contact the SMO or external laboratory for information.	R, I1d	R, I1d
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	36. Serial dilution sample RPD was >10% and the sample result was >50X the MDL (>100X the MDL for ICPMS). Qualify ONLY the sample used for the serial dilution.	UJ, I18	J, I18
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	37. Serial dilution sample was not analyzed with the samples.	UJ, I18a	J, I18
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	38. The sample result was reported as detected between the IDL and the EDL.	N/A	J, I1
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	39. Duplicate, dilution, or reanalysis.	UJ, I88	J, I88
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	40. Qualification of data via data validation did not occur based on Quality Control requirements in this procedure. Adhere to the external laboratory qualifiers found within the Form I analytical data summary sheets generated by the external laboratory.	U, U_LAB	J, J_LAB, NQ, NQ
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	41. The LANL project chemist identified quality deficiencies in the reported data that require further qualification. This code can ONLY be used and/or under advisement by the LANL project chemist.	UJ, R, I19	J, R, I19

METALS
-1-
INORGANICS ANALYSIS DATA PACKAGE

SDG No: 10-2093

CONTRACT: LANL01004

METHOD TYPE: SW846

SAMPLE ID: 248117001

BASIS: As Received

DATE COLLECTED 22-FEB-10

CLIENT ID: RE36-10-8458

LEVEL: Low

DATE RECEIVED 26-FEB-10

MATRIX: WATER

%SOLIDS: 0

CAS No.	Analyte	Result	Units	Qual	MDL	PQL	CRDL	DF	M*	Analyst	Run Date	Analytical Run	Analytical Batch
7429-90-5	Aluminum	200	ug/L	U	68	200	200	1	P	HSC	03/29/10 20:44	032910C-1	959109
7440-36-0	Antimony	3	ug/L	U	1	3	3	1	MS	PRB	04/13/10 13:49	100413-3	959112
7440-38-2	Arsenic	30	ug/L	U	5	30	30	1	P	HSC	03/29/10 20:44	032910C-1	959109
7440-39-3	Barium	5	ug/L	U	1	5	5	1	P	HSC	03/29/10 20:44	032910C-1	959109
7440-41-7	Beryllium	0.50	ug/L	U	0.1	0.5	0.5	1	MS	BCD1	04/12/10 04:22	100411-2	959112
7440-43-9	Cadmium	1	ug/L	U	0.11	1	1	1	MS	BCD1	04/12/10 04:22	100411-2	959112
7440-70-2	Calcium	53	ug/L	J	50	200	200	1	P	HSC	03/29/10 20:44	032910C-1	959109
7440-47-3	Chromium	5	ug/L	U	1	5	5	1	P	HSC	03/29/10 20:44	032910C-1	959109
7440-48-4	Cobalt	5	ug/L	U	1	5	5	1	P	HSC	03/29/10 20:44	032910C-1	959109
7440-50-8	Copper	6.57	ug/L	J	3	10	10	1	P	HSC	03/29/10 20:44	032910C-1	959109
7439-89-6	Iron	100	ug/L	U	30	100	100	1	P	HSC	03/29/10 20:44	032910C-1	959109
7439-92-1	Lead U,14	0.866	ug/L	J	0.5	2	2	1	MS	BCD1	04/12/10 04:22	100411-2	959112
7439-95-4	Magnesium	300	ug/L	U	85	300	300	1	P	HSC	03/29/10 20:44	032910C-1	959109
7439-96-5	Manganese	5	ug/L	U	1	5	5	1	MS	BCD1	04/12/10 04:22	100411-2	959112
7439-97-6	Mercury	0.20	ug/L	U	0.066	0.2	0.2	1	AV	JXL1	03/02/10 11:58	030210W3-6	958951
7440-02-0	Nickel	5	ug/L	U	1.5	5	5	1	P	HSC	03/29/10 20:44	032910C-1	959109
7440-09-7	Potassium	293	ug/L		50	150	150	1	P	HSC	03/29/10 20:44	032910C-1	959109
7782-49-2	Selenium	30	ug/L	U	5	30	30	1	P	HSC	03/29/10 20:44	032910C-1	959109
7440-22-4	Silver	5	ug/L	U	1	5	5	1	P	HSC	03/29/10 20:44	032910C-1	959109
7440-23-5	Sodium	140	ug/L	J	100	300	300	1	P	HSC	03/29/10 20:44	032910C-1	959109
7440-28-0	Thallium	1	ug/L	U	0.3	1	1	1	MS	BCD1	04/12/10 04:22	100411-2	959112
7440-61-1	Uranium	0.20	ug/L	U	0.05	0.2	0.2	1	MS	PRB	04/13/10 16:22	100413-5	959112
7440-62-2	Vanadium	5	ug/L	U	1	5	5	1	P	HSC	03/29/10 20:44	032910C-1	959109
7440-66-6	Zinc	6.16	ug/L	J	3.3	10	10	1	P	HSC	03/29/10 20:44	032910C-1	959109

Prep Information:

Analytical Batch	Prep Batch	Prep Method	Initial wt./vol.	Units	Final wt./vol.	Units	Date	Analyst
958951	958949	SW846 7470A Prep	20	mL	20	mL	03/01/10	TXB3
959109	959108	SW846 3005A	50	mL	50	mL	03/04/10	FGA
959112	959110	SW846 3005A	50	mL	50	mL	03/04/10	FGA

MAD
04/26/10

METALS
-1-
INORGANICS ANALYSIS DATA PACKAGE

SDG No: 10-2093-1

CONTRACT: LANL01004

METHOD TYPE: SW846

SAMPLE ID: 248118001

BASIS: Dry Weight

DATE COLLECTED 22-FEB-10

CLIENT ID: RE36-10-8448

LEVEL: Low

DATE RECEIVED 26-FEB-10

MATRIX: SOIL

%SOLIDS: 97.3

CAS No.	Analyte	Result	Units	Qual	MDL	PQL	CRDL	DF	M*	Analyst	Run Date	Analytical Run	Analytical Batch
7429-90-5	Aluminum	1730000	ug/Kg		6900	20300	20300	1	P	HSC	03/29/10 23:24	032910C-1	959114
7440-36-0	Antimony UJ,112a	1020	ug/Kg	U	335	1020	1020	1	P	HSC	03/29/10 23:24	032910C-1	959114
7440-38-2	Arsenic	0.665	mg/kg	J	0.194	0.969	0.969	2	MS	RMJ	03/24/10 17:51	100323-2	959116
7440-39-3	Barium	20400	ug/Kg		102	508	508	1	P	HSC	03/29/10 23:24	032910C-1	959114
7440-41-7	Beryllium	0.512	mg/kg		0.0194	0.0969	0.0969	2	MS	RMJ	03/24/10 17:51	100323-2	959116
7440-43-9	Cadmium	508	ug/Kg	U	102	508	508	1	P	HSC	03/29/10 23:24	032910C-1	959114
7440-70-2	Calcium	347000	ug/Kg		8120	25400	25400	1	P	HSC	03/29/10 23:24	032910C-1	959114
7440-47-3	Chromium	2230	ug/Kg		152	508	508	1	P	HSC	03/29/10 23:24	032910C-1	959114
7440-48-4	Cobalt	657	ug/Kg		152	508	508	1	P	HSC	03/29/10 23:24	032910C-1	959114
7440-50-8	Copper U,14d	2180	ug/Kg		305	1020	1020	1	P	HSC	03/29/10 23:24	032910C-1	959114
7439-89-6	Iron	7330000	ug/Kg		8120	25400	25400	1	P	HSC	03/29/10 23:24	032910C-1	959114
7439-92-1	Lead	3720	ug/Kg		254	1020	1020	1	P	HSC	03/29/10 23:24	032910C-1	959114
7439-95-4	Magnesium	265000	ug/Kg		8630	30500	30500	1	P	HSC	03/29/10 23:24	032910C-1	959114
7439-96-5	Manganese	399000	ug/Kg		203	1020	1020	1	P	HSC	03/29/10 23:24	032910C-1	959114
7439-97-6	Mercury	11	ug/kg	U	3.76	11	11	1	AV	JXL1	03/10/10 13:22	031010S1-4	958757
7440-02-0	Nickel	1.87	mg/kg		0.0969	0.388	0.388	2	MS	RMJ	03/24/10 17:51	100323-2	959116
7440-09-7	Potassium J+,16b	364000	ug/Kg		6500	25400	25400	1	P	HSC	03/29/10 23:24	032910C-1	959114
7782-49-2	Selenium UJ,16a	0.969	mg/kg	U	0.485	0.969	0.969	2	MS	RMJ	03/24/10 17:51	100323-2	959116
7440-22-4	Silver	508	ug/Kg	U	102	508	508	1	P	HSC	03/29/10 23:24	032910C-1	959114
7440-23-5	Sodium	218000	ug/Kg		7110	25400	25400	1	P	HSC	03/29/10 23:24	032910C-1	959114
7440-28-0	Thallium	0.194	mg/kg	U	0.0582	0.194	0.194	2	MS	RMJ	03/24/10 17:51	100323-2	959116
7440-61-1	Uranium	0.613	mg/kg		0.0128	0.0388	0.0388	2	MS	RMJ	03/26/10 01:27	100325-3	959116
7440-62-2	Vanadium	3630	ug/Kg		102	508	508	1	P	HSC	03/29/10 23:24	032910C-1	959114
7440-66-6	Zinc	46600	ug/Kg		335	1020	1020	1	P	HSC	03/29/10 23:24	032910C-1	959114

Prep Information:

Analytical Batch	Prep Batch	Prep Method	Initial wt./vol.	Units	Final wt./vol.	Units	Date	Analyst
958757	958755	SW846 7471A Prep	0.558	g	30	mL	03/10/10	LXH2
959114	959113	SW846 3050B	0.506	g	50	mL	03/09/10	AXG2
959116	959115	SW846 3050B	0.53	g	50	mL	03/03/10	BXA1

MAD
04/26/10

METALS
-1-
INORGANICS ANALYSIS DATA PACKAGE

SDG No: 10-2093-1

CONTRACT: LANL01004

METHOD TYPE: SW846

SAMPLE ID: 248118002

BASIS: Dry Weight

DATE COLLECTED 22-FEB-10

CLIENT ID: RE36-10-8456

LEVEL: Low

DATE RECEIVED 26-FEB-10

MATRIX: SOIL

%SOLIDS: 97.2

CAS No.	Analyte	Result	Units	Qual	MDL	PQL	CRDL	DF	M*	Analyst	Run Date	Analytical Run	Analytical Batch
7429-90-5	Aluminum	1820000	ug/Kg		6710	19700	19700	1	P	HSC	03/29/10 23:26	032910C-1	959114
7440-38-0	Antimony UJ,112a	987	ug/Kg	U	326	987	987	1	P	HSC	03/29/10 23:26	032910C-1	959114
7440-38-2	Arsenic	0.761	mg/kg	J	0.176	0.879	0.879	2	MS	RMJ	03/24/10 17:55	100323-2	959116
7440-39-3	Barium	21800	ug/Kg		98.7	494	494	1	P	HSC	03/29/10 23:26	032910C-1	959114
7440-41-7	Beryllium	0.485	mg/kg		0.0176	0.0879	0.0879	2	MS	RMJ	03/24/10 17:55	100323-2	959116
7440-43-9	Cadmium	494	ug/Kg	U	98.7	494	494	1	P	HSC	03/29/10 23:26	032910C-1	959114
7440-70-2	Calcium	396000	ug/Kg		7900	24700	24700	1	P	HSC	03/29/10 23:26	032910C-1	959114
7440-47-3	Chromium	2740	ug/Kg		148	494	494	1	P	HSC	03/29/10 23:26	032910C-1	959114
7440-48-4	Cobalt	740	ug/Kg		148	494	494	1	P	HSC	03/29/10 23:26	032910C-1	959114
7440-50-8	Copper U,14d	2120	ug/Kg		296	987	987	1	P	HSC	03/29/10 23:26	032910C-1	959114
7439-89-6	Iron	6920000	ug/Kg		7900	24700	24700	1	P	HSC	03/29/10 23:26	032910C-1	959114
7439-92-1	Lead	3560	ug/Kg		247	987	987	1	P	HSC	03/29/10 23:26	032910C-1	959114
7439-95-4	Magnesium	295000	ug/Kg		8390	29600	29600	1	P	HSC	03/29/10 23:26	032910C-1	959114
7439-96-5	Manganese	389000	ug/Kg		197	987	987	1	P	HSC	03/29/10 23:26	032910C-1	959114
7439-97-6	Mercury	11.3	ug/kg	U	3.85	11.3	11.3	1	AV	JXL1	03/10/10 13:24	031010S1-4	958757
7440-02-0	Nickel	1.85	mg/kg		0.0879	0.352	0.352	2	MS	RMJ	03/24/10 17:55	100323-2	959116
7440-09-7	Potassium J+,16b	366000	ug/Kg		6320	24700	24700	1	P	HSC	03/29/10 23:26	032910C-1	959114
7782-49-2	Selenium UJ,16a	0.879	mg/kg	U	0.44	0.879	0.879	2	MS	RMJ	03/24/10 17:55	100323-2	959116
7440-22-4	Silver	494	ug/Kg	U	98.7	494	494	1	P	HSC	03/29/10 23:26	032910C-1	959114
7440-23-5	Sodium	209000	ug/Kg		6910	24700	24700	1	P	HSC	03/29/10 23:26	032910C-1	959114
7440-28-0	Thallium	0.176	mg/kg	U	0.0528	0.176	0.176	2	MS	RMJ	03/24/10 17:55	100323-2	959116
7440-61-1	Uranium	0.595	mg/kg		0.0116	0.0352	0.0352	2	MS	RMJ	03/26/10 01:30	100325-3	959116
7440-62-2	Vanadium	3650	ug/Kg		98.7	494	494	1	P	HSC	03/29/10 23:26	032910C-1	959114
7440-66-6	Zinc	43600	ug/Kg		326	987	987	1	P	HSC	03/29/10 23:26	032910C-1	959114

Prep Information:

Analytical Batch	Prep Batch	Prep Method	Initial wt./vol.	Units	Final wt./vol.	Units	Date	Analyst
958757	958755	SW846 7471A Prep	0.545	g	30	mL	03/10/10	LXH2
959114	959113	SW846 3050B	0.521	g	50	mL	03/09/10	AXC2
959116	959115	SW846 3050B	0.585	g	50	mL	03/03/10	BXA1

MAD
04/26/10

METALS
-1-
INORGANICS ANALYSIS DATA PACKAGE

SDG No: 10-2093-1

CONTRACT: LANL01004

METHOD TYPE: SW846

SAMPLE ID: 248118003

BASIS: Dry Weight

DATE COLLECTED 22-FEB-10

CLIENT ID: RE36-10-8451

LEVEL: Low

DATE RECEIVED 26-FEB-10

MATRIX: SOIL

%SOLIDS: 97

CAS No.	Analyte	Result	Units	Qual	MDL	PQL	CRDL	DF	M*	Analyst	Run Date	Analytical Run	Analytical Batch
7429-90-5	Aluminum	2450000	ug/Kg		6870	20200	20200	1	P	HSC	03/29/10 23:28	032910C-1	959114
7440-36-0	Antimony UJ,12a	1010	ug/Kg	U	334	1010	1010	1	P	HSC	03/29/10 23:28	032910C-1	959114
7440-38-2	Arsenic	0.644	mg/kg	J	0.2	0.999	0.999	2	MS	RMJ	03/24/10 17:59	100323-2	959116
7440-39-3	Barium	28800	ug/Kg		101	505	505	1	P	HSC	03/29/10 23:28	032910C-1	959114
7440-41-7	Beryllium	0.632	mg/kg		0.02	0.0999	0.0999	2	MS	RMJ	03/24/10 17:59	100323-2	959116
7440-43-9	Cadmium	505	ug/Kg	U	101	505	505	1	P	HSC	03/29/10 23:28	032910C-1	959114
7440-70-2	Calcium	575000	ug/Kg		8090	25300	25300	1	P	HSC	03/29/10 23:28	032910C-1	959114
7440-47-3	Chromium	3440	ug/Kg		152	505	505	1	P	HSC	03/29/10 23:28	032910C-1	959114
7440-48-4	Cobalt	1130	ug/Kg		152	505	505	1	P	HSC	03/29/10 23:28	032910C-1	959114
7440-50-8	Copper U,14d	2750	ug/Kg		303	1010	1010	1	P	HSC	03/29/10 23:28	032910C-1	959114
7439-89-6	Iron	7320000	ug/Kg		8090	25300	25300	1	P	HSC	03/29/10 23:28	032910C-1	959114
7439-92-1	Lead	6400	ug/Kg		253	1010	1010	1	P	HSC	03/29/10 23:28	032910C-1	959114
7439-95-4	Magnesium	461000	ug/Kg		8590	30300	30300	1	P	HSC	03/29/10 23:28	032910C-1	959114
7439-96-5	Manganese	362000	ug/Kg		202	1010	1010	1	P	HSC	03/29/10 23:28	032910C-1	959114
7439-97-6	Mercury	10.5	ug/kg	U	3.58	10.5	10.5	1	AV	JXL1	03/10/10 13:26	031010S1-4	958757
7440-02-0	Nickel	1.59	mg/kg		0.0999	0.4	0.4	2	MS	RMJ	03/24/10 17:59	100323-2	959116
7440-09-7	Potassium J+,16b	479000	ug/Kg		6470	25300	25300	1	P	HSC	03/29/10 23:28	032910C-1	959114
7782-49-2	Selenium UJ,16a	0.999	mg/kg	U	0.5	0.999	0.999	2	MS	RMJ	03/24/10 17:59	100323-2	959116
7440-22-4	Silver	505	ug/Kg	U	101	505	505	1	P	HSC	03/29/10 23:28	032910C-1	959114
7440-23-5	Sodium	224000	ug/Kg		7080	25300	25300	1	P	HSC	03/29/10 23:28	032910C-1	959114
7440-28-0	Thallium	0.20	mg/kg	U	0.0599	0.2	0.2	2	MS	RMJ	03/24/10 17:59	100323-2	959116
7440-61-1	Uranium	0.587	mg/kg		0.0132	0.04	0.04	2	MS	RMJ	03/26/10 01:33	100325-3	959116
7440-62-2	Vanadium	4120	ug/Kg		101	505	505	1	P	HSC	03/29/10 23:28	032910C-1	959114
7440-66-6	Zinc	38700	ug/Kg		334	1010	1010	1	P	HSC	03/29/10 23:28	032910C-1	959114

Prep Information:

Analytical Batch	Prep Batch	Prep Method	Initial wt./vol.	Units	Final wt./vol.	Units	Date	Analyst
958757	958755	SW846 7471A Prep	0.588	g	30	mL	03/10/10	LXH2
959114	959113	SW846 3050B	0.51	g	50	mL	03/09/10	AXG2
959116	959115	SW846 3050B	0.516	g	50	mL	03/03/10	BXA1

MAD
04/26/10

METALS
-1-
INORGANICS ANALYSIS DATA PACKAGE

SDG No: 10-2093-1

CONTRACT: LANL01004

METHOD TYPE: SW846

SAMPLE ID: 248118004

BASIS: Dry Weight

DATE COLLECTED 22-FEB-10

CLIENT ID: RE36-10-8450

LEVEL: Low

DATE RECEIVED 26-FEB-10

MATRIX: SOIL

%SOLIDS: 85

CAS No.	Analyte	Result	Units	Qual	MDL	PQL	CRDL	DF	M*	Analyst	Run Date	Analytical Run	Analytical Batch
7429-90-5	Aluminum	13800000	ug/Kg		7250	21300	21300	1	P	HSC	03/29/10 23:30	032910C-1	959114
7440-36-0	Antimony UJ,112a	1070	ug/Kg	U	352	1070	1070	1	P	HSC	03/29/10 23:30	032910C-1	959114
7440-38-2	Arsenic	2.07	mg/kg		0.205	1.02	1.02	2	MS	RMJ	03/24/10 18:03	100323-2	959116
7440-39-3	Barium	82200	ug/Kg		107	533	533	1	P	HSC	03/29/10 23:30	032910C-1	959114
7440-41-7	Beryllium	2.69	mg/kg		0.0205	0.102	0.102	2	MS	RMJ	03/24/10 18:03	100323-2	959116
7440-43-9	Cadmium	533	ug/Kg	U	107	533	533	1	P	HSC	03/29/10 23:30	032910C-1	959114
7440-70-2	Calcium	4700000	ug/Kg		8530	26700	26700	1	P	HSC	03/29/10 23:30	032910C-1	959114
7440-47-3	Chromium	9640	ug/Kg		160	533	533	1	P	HSC	03/29/10 23:30	032910C-1	959114
7440-48-4	Cobalt	2440	ug/Kg		160	533	533	1	P	HSC	03/29/10 23:30	032910C-1	959114
7440-50-8	Copper	9920	ug/Kg		320	1070	1070	1	P	HSC	03/29/10 23:30	032910C-1	959114
7439-89-6	Iron	12700000	ug/Kg		8530	26700	26700	1	P	HSC	03/29/10 23:30	032910C-1	959114
7439-92-1	Lead	13000	ug/Kg		267	1070	1070	1	P	HSC	03/29/10 23:30	032910C-1	959114
7439-95-4	Magnesium	3080000	ug/Kg		9070	32000	32000	1	P	HSC	03/29/10 23:30	032910C-1	959114
7439-96-5	Manganese	402000	ug/Kg		213	1070	1070	1	P	HSC	03/29/10 23:30	032910C-1	959114
7439-97-6	Mercury	56.1	ug/kg		4	11.8	11.8	1	AV	JXL1	03/10/10 13:28	031010S1-4	958757
7440-02-0	Nickel	10.6	mg/kg		0.102	0.41	0.41	2	MS	RMJ	03/24/10 18:03	100323-2	959116
7440-09-7	Potassium J+,16b	1920000	ug/Kg		6830	26700	26700	1	P	HSC	03/29/10 23:30	032910C-1	959114
7782-49-2	Selenium UJ,16a	1.02	mg/kg	U	0.512	1.02	1.02	2	MS	RMJ	03/24/10 18:03	100323-2	959116
7440-22-4	Silver	533	ug/Kg	U	107	533	533	1	P	HSC	03/29/10 23:30	032910C-1	959114
7440-23-5	Sodium	155000	ug/Kg		7470	26700	26700	1	P	HSC	03/29/10 23:30	032910C-1	959114
7440-28-0	Thallium	0.152	mg/kg	J	0.0614	0.205	0.205	2	MS	RMJ	03/24/10 18:03	100323-2	959116
7440-61-1	Uranium	1.37	mg/kg		0.0135	0.041	0.041	2	MS	RMJ	03/26/10 01:42	100325-3	959116
7440-62-2	Vanadium	16200	ug/Kg		107	533	533	1	P	HSC	03/29/10 23:30	032910C-1	959114
7440-66-6	Zinc	49600	ug/Kg		352	1070	1070	1	P	HSC	03/29/10 23:30	032910C-1	959114

Prep Information:

Analytical Batch	Prep Batch	Prep Method	Initial wt./vol.	Units	Final wt./vol.	Units	Date	Analyst
958757	958755	SW846 7471A Prep	0.599	g	30	mL	03/10/10	LXH2
959114	959113	SW846 3050B	0.551	g	50	mL	03/09/10	AXG2
959116	959115	SW846 3050B	0.574	g	50	mL	03/03/10	BXA1

MAD
04/26/10

METALS
-1-
INORGANICS ANALYSIS DATA PACKAGE

SDG No: 10-2093-1

CONTRACT: LANL01004

METHOD TYPE: SW846

SAMPLE ID: 248118005

BASIS: Dry Weight

DATE COLLECTED 22-FEB-10

CLIENT ID: RE36-10-8449

LEVEL: Low

DATE RECEIVED 26-FEB-10

MATRIX: SOIL

%SOLIDS: 98.2

CAS No.	Analyte	Result	Units	Qual	MDL	PQL	CRDL	DF	M*	Analyst	Run Date	Analytical Run	Analytical Batch
7429-90-5	Aluminum	1410000	ug/Kg		5830	17100	17100	1	P	HSC	03/29/10 23:32	032910C-1	959114
7440-36-0	Antimony UJ,112a	857	ug/Kg	U	283	857	857	1	P	HSC	03/29/10 23:32	032910C-1	959114
7440-38-2	Arsenic	0.533	mg/kg	J	0.177	0.884	0.884	2	MS	RMJ	03/24/10 18:07	100323-2	959116
7440-39-3	Barium	28200	ug/Kg		85.7	428	428	1	P	HSC	03/29/10 23:32	032910C-1	959114
7440-41-7	Beryllium	0.493	mg/kg		0.0177	0.0884	0.0884	2	MS	RMJ	03/24/10 18:07	100323-2	959116
7440-43-9	Cadmium	428	ug/Kg	U	85.7	428	428	1	P	HSC	03/29/10 23:32	032910C-1	959114
7440-70-2	Calcium	256000	ug/Kg		6850	21400	21400	1	P	HSC	03/29/10 23:32	032910C-1	959114
7440-47-3	Chromium	2240	ug/Kg		129	428	428	1	P	HSC	03/29/10 23:32	032910C-1	959114
7440-48-4	Cobalt	612	ug/Kg		129	428	428	1	P	HSC	03/29/10 23:32	032910C-1	959114
7440-50-8	Copper U,14d	2400	ug/Kg		257	857	857	1	P	HSC	03/29/10 23:32	032910C-1	959114
7439-89-6	Iron	6440000	ug/Kg		6850	21400	21400	1	P	HSC	03/29/10 23:32	032910C-1	959114
7439-92-1	Lead	6970	ug/Kg		214	857	857	1	P	HSC	03/29/10 23:32	032910C-1	959114
7439-95-4	Magnesium	160000	ug/Kg		7280	25700	25700	1	P	HSC	03/29/10 23:32	032910C-1	959114
7439-96-5	Manganese	497000	ug/Kg		171	857	857	1	P	HSC	03/29/10 23:32	032910C-1	959114
7439-97-6	Mercury	11.4	ug/kg	U	3.88	11.4	11.4	1	AV	JXLI	03/10/10 13:34	031010S1-4	958757
7440-02-0	Nickel	1.72	mg/kg		0.0884	0.353	0.353	2	MS	RMJ	03/24/10 18:07	100323-2	959116
7440-09-7	Potassium J+,16b	438000	ug/Kg		5480	21400	21400	1	P	HSC	03/29/10 23:32	032910C-1	959114
7782-49-2	Selenium UJ,16a	0.884	mg/kg	U	0.442	0.884	0.884	2	MS	RMJ	03/24/10 18:07	100323-2	959116
7440-22-4	Silver	428	ug/Kg	U	85.7	428	428	1	P	HSC	03/29/10 23:32	032910C-1	959114
7440-23-5	Sodium	332000	ug/Kg		6000	21400	21400	1	P	HSC	03/29/10 23:32	032910C-1	959114
7440-28-0	Thallium	0.177	mg/kg	U	0.053	0.177	0.177	2	MS	RMJ	03/24/10 18:07	100323-2	959116
7440-61-1	Uranium	0.687	mg/kg		0.0117	0.0353	0.0353	2	MS	RMJ	03/26/10 01:45	100325-3	959116
7440-62-2	Vanadium	2750	ug/Kg		85.7	428	428	1	P	HSC	03/29/10 23:32	032910C-1	959114
7440-66-6	Zinc	47000	ug/Kg		283	857	857	1	P	HSC	03/29/10 23:32	032910C-1	959114

Prep Information:

Analytical Batch	Prep Batch	Prep Method	Initial wt./vol.	Units	Final wt./vol.	Units	Date	Analyst
958757	958755	SW846 7471A Prep	0.535	g	30	mL	03/10/10	LXH2
959114	959113	SW846 3050B	0.594	g	50	mL	03/09/10	AXG2
959116	959115	SW846 3050B	0.576	g	50	mL	03/03/10	BXA1

MAD
04/26/10

METALS
-1-
INORGANICS ANALYSIS DATA PACKAGE

SDG No: 10-2093-1

CONTRACT: LANL01004

METHOD TYPE: SW846

SAMPLE ID: 248118006

BASIS: Dry Weight

DATE COLLECTED 22-FEB-10

CLIENT ID: RE36-10-8453

LEVEL: Low

DATE RECEIVED 26-FEB-10

MATRIX: SOIL

%SOLIDS: 95.7

CAS No.	Analyte	Result	Units	Qual	MDL	PQL	CRDL	DF	M*	Analyst	Run Date	Analytical Run	Analytical Batch
7429-90-5	Aluminum	3570000	ug/Kg		6780	19900	19900	1	P	HSC	03/29/10 23:34	032910C-1	959114
7440-36-0	Antimony UJ,112a	997	ug/Kg	U	329	997	997	1	P	HSC	03/29/10 23:34	032910C-1	959114
7440-38-2	Arsenic	0.850	mg/kg	J	0.204	1.02	1.02	2	MS	RMJ	03/24/10 18:11	100323-2	959116
7440-39-3	Barium	63700	ug/Kg		99.7	498	498	1	P	HSC	03/29/10 23:34	032910C-1	959114
7440-41-7	Beryllium	0.678	mg/kg		0.0204	0.102	0.102	2	MS	RMJ	03/24/10 18:11	100323-2	959116
7440-43-9	Cadmium	498	ug/Kg	U	99.7	498	498	1	P	HSC	03/29/10 23:34	032910C-1	959114
7440-70-2	Calcium	775000	ug/Kg		7970	24900	24900	1	P	HSC	03/29/10 23:34	032910C-1	959114
7440-47-3	Chromium	8380	ug/Kg		150	498	498	1	P	HSC	03/29/10 23:34	032910C-1	959114
7440-48-4	Cobalt	916	ug/Kg		150	498	498	1	P	HSC	03/29/10 23:34	032910C-1	959114
7440-50-8	Copper	3930	ug/Kg		299	997	997	1	P	HSC	03/29/10 23:34	032910C-1	959114
7439-89-6	Iron	10000000	ug/Kg		7970	24900	24900	1	P	HSC	03/29/10 23:34	032910C-1	959114
7439-92-1	Lead	5490	ug/Kg		249	997	997	1	P	HSC	03/29/10 23:34	032910C-1	959114
7439-95-4	Magnesium	766000	ug/Kg		8470	29900	29900	1	P	HSC	03/29/10 23:34	032910C-1	959114
7439-96-5	Manganese	359000	ug/Kg		199	997	997	1	P	HSC	03/29/10 23:34	032910C-1	959114
7439-97-6	Mercury	11.1	ug/kg	U	3.79	11.1	11.1	1	AV	JXL1	03/10/10 13:36	031010S1-4	958757
7440-02-0	Nickel	2.99	mg/kg		0.102	0.408	0.408	2	MS	RMJ	03/24/10 18:11	100323-2	959116
7440-09-7	Potassium J+,16b	601000	ug/Kg		6380	24900	24900	1	P	HSC	03/29/10 23:34	032910C-1	959114
7782-49-2	Selenium UJ,16a	1.02	mg/kg	U	0.51	1.02	1.02	2	MS	RMJ	03/24/10 18:11	100323-2	959116
7440-22-4	Silver	498	ug/Kg	U	99.7	498	498	1	P	HSC	03/29/10 23:34	032910C-1	959114
7440-23-5	Sodium	358000	ug/Kg		6980	24900	24900	1	P	HSC	03/29/10 23:34	032910C-1	959114
7440-28-0	Thallium	0.204	mg/kg	U	0.0612	0.204	0.204	2	MS	RMJ	03/24/10 18:11	100323-2	959116
7440-61-1	Uranium	0.678	mg/kg		0.0135	0.0408	0.0408	2	MS	RMJ	03/26/10 01:48	100325-3	959116
7440-62-2	Vanadium	7320	ug/Kg		99.7	498	498	1	P	HSC	03/29/10 23:34	032910C-1	959114
7440-66-6	Zinc	50500	ug/Kg		329	997	997	1	P	HSC	03/29/10 23:34	032910C-1	959114

Prep Information:

Analytical Batch	Prep Batch	Prep Method	Initial wt./vol.	Units	Final wt./vol.	Units	Date	Analyst
958757	958755	SW846 7471A Prep	0.563	g	30	mL	03/10/10	LXH2
959114	959113	SW846 3050B	0.524	g	50	mL	03/09/10	AXG2
959116	959115	SW846 3050B	0.512	g	50	mL	03/03/10	BXA1

MAD
04/26/10

METALS
-1-
INORGANICS ANALYSIS DATA PACKAGE

SDG No: 10-2093-1

CONTRACT: LANL01004

METHOD TYPE: SW846

SAMPLE ID: 248118007 BASIS: Dry Weight DATE COLLECTED 22-FEB-10
 CLIENT ID: RE36-10-8452 LEVEL: Low DATE RECEIVED 26-FEB-10
 MATRIX: SOIL %SOLIDS: 92.9

CAS No.	Analyte	Result	Units	Qual	MDL	PQL	CRDL	DF	M*	Analyst	Run Date	Analytical Run	Analytical Batch
7429-90-5	Aluminum	6940000	ug/Kg		6210	18300	18300	1	P	HSC	03/29/10 23:36	032910C-1	959114
7440-36-0	Antimony UJ,112a	913	ug/Kg	U	301	913	913	1	P	HSC	03/29/10 23:36	032910C-1	959114
7440-38-2	Arsenic	1.71	mg/kg		0.184	0.922	0.922	2	MS	RMJ	03/24/10 18:15	100323-2	959116
7440-39-3	Barium	84600	ug/Kg		91.3	456	456	1	P	HSC	03/29/10 23:36	032910C-1	959114
7440-41-7	Beryllium	0.863	mg/kg		0.0184	0.0922	0.0922	2	MS	RMJ	03/24/10 18:15	100323-2	959116
7440-43-9	Cadmium	456	ug/Kg	U	91.3	456	456	1	P	HSC	03/29/10 23:36	032910C-1	959114
7440-70-2	Calcium	1570000	ug/Kg		7300	22800	22800	1	P	HSC	03/29/10 23:36	032910C-1	959114
7440-47-3	Chromium	6860	ug/Kg		137	456	456	1	P	HSC	03/29/10 23:36	032910C-1	959114
7440-48-4	Cobalt	4200	ug/Kg		137	456	456	1	P	HSC	03/29/10 23:36	032910C-1	959114
7440-50-8	Copper	5980	ug/Kg		274	913	913	1	P	HSC	03/29/10 23:36	032910C-1	959114
7439-89-6	Iron	11100000	ug/Kg		7300	22800	22800	1	P	HSC	03/29/10 23:36	032910C-1	959114
7439-92-1	Lead	9290	ug/Kg		228	913	913	1	P	HSC	03/29/10 23:36	032910C-1	959114
7439-95-4	Magnesium	1730000	ug/Kg		7760	27400	27400	1	P	HSC	03/29/10 23:36	032910C-1	959114
7439-96-5	Manganese	359000	ug/Kg		183	913	913	1	P	HSC	03/29/10 23:36	032910C-1	959114
7439-97-6	Mercury	11.7	ug/kg	U	3.97	11.7	11.7	1	AV	JXL1	03/10/10 13:38	031010S1-4	958757
7440-02-0	Nickel	6.82	mg/kg		0.0922	0.369	0.369	2	MS	RMJ	03/24/10 18:15	100323-2	959116
7440-09-7	Potassium J+,16b	1510000	ug/Kg		5840	22800	22800	1	P	HSC	03/29/10 23:36	032910C-1	959114
7782-49-2	Selenium UJ,16a	0.922	mg/kg	U	0.461	0.922	0.922	2	MS	RMJ	03/24/10 18:15	100323-2	959116
7440-22-4	Silver	456	ug/Kg	U	91.3	456	456	1	P	HSC	03/29/10 23:36	032910C-1	959114
7440-23-5	Sodium	452000	ug/Kg		6390	22800	22800	1	P	HSC	03/29/10 23:36	032910C-1	959114
7440-28-0	Thallium	0.124	mg/kg	J	0.0553	0.184	0.184	2	MS	RMJ	03/24/10 18:15	100323-2	959116
7440-61-1	Uranium	0.688	mg/kg		0.0122	0.0369	0.0369	2	MS	RMJ	03/26/10 01:51	100325-3	959116
7440-62-2	Vanadium	15700	ug/Kg		91.3	456	456	1	P	HSC	03/29/10 23:36	032910C-1	959114
7440-66-6	Zinc	33400	ug/Kg		301	913	913	1	P	HSC	03/29/10 23:36	032910C-1	959114

Prep Information:

Analytical Batch	Prep Batch	Prep Method	Initial wt./vol.	Units	Final wt./vol.	Units	Date	Analyst
958757	958755	SW846 7471A Prep	0.554	g	30	mL	03/10/10	LXH2
959114	959113	SW846 3050B	0.59	g	50	mL	03/09/10	AXG2
959116	959115	SW846 3050B	0.584	g	50	mL	03/03/10	BXA1

MAD
04/26/10

DATA VALIDATION COVER SHEET

5120-1

Data Validation Cover Sheet

Records Use only



Section I.

REQUEST NUMBER: 10-2093 VALIDATION DATE: 04/26/2010 LAB CODE: GELCONTRACT LABORATORY NAME: GEL Laboratories LLCVALIDATOR: Mary Donovan ORGANIZATION: Analytical Quality Associates, Inc.

ANALYTICAL SUITE (CHECK ALL THAT APPLY):

- | | | | |
|---|--|---|--|
| <input type="checkbox"/> TPH-GRO | <input type="checkbox"/> HIGH EXPLOSIVES | <input type="checkbox"/> DIOXIN FURANS | <input type="checkbox"/> LCMSMS PERCHLORATES |
| <input type="checkbox"/> TPH-DRO | <input type="checkbox"/> METALS | <input type="checkbox"/> PCB CONGENERS | <input type="checkbox"/> ORGANOCHLORINE |
| <input checked="" type="checkbox"/> GENERAL CHEMISTRY | <input type="checkbox"/> RADIOCHEMISTRY | <input type="checkbox"/> LCMSMS HIGH EXPLOSIVES | PESTICIDES/POLYCHLORINATED BIPHENYLS |
| <input type="checkbox"/> OTHER (DESCRIBE): _____ | | | |


Section II. Completeness Check

- | YES | NO | N/A | (CHECK ONE) | YES | NO | N/A | (CHECK ONE) |
|-------------------------------------|--------------------------|-------------------------------------|-----------------------------|-------------------------------------|--------------------------|-------------------------------------|--------------------------|
| <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | 1. CHAIN-OF-CUSTODY FORM(S) | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | 6. RAW/BSS DATA |
| <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | 2. CASE NARRATIVE | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | 7. QUALITY CONTROL FORMS |
| <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | 3. SAMPLE RESULT FORMS | <input type="checkbox"/> | <input type="checkbox"/> | <input checked="" type="checkbox"/> | 8. QUANTITATION REPORTS |
| <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | 4. SAMPLE CHROMATOGRAMS | <input type="checkbox"/> | <input type="checkbox"/> | <input checked="" type="checkbox"/> | 9. TICS FORMS |
| <input type="checkbox"/> | <input type="checkbox"/> | <input checked="" type="checkbox"/> | 5. STANDARD CHROMATOGRAMS | <input type="checkbox"/> | <input type="checkbox"/> | <input checked="" type="checkbox"/> | 10. TICS MASS SPECTRA |


Comments/problems noted (include information about requests for further information submitted to the contract laboratory and agreed-upon date of resolution and contract laboratory point of contact):

1. In the aqueous MB, nitrate/nitrite as N was detected. The associated sample result was an ND and, thus, was not qualified.
2. It should be noted that the parent samples for the matrix QC associated with all analyses except soil nitrate-N were from other LANL RNs. No sample data were qualified as a result.


Reviewed by: Monica Dymerski Level I Date: 04/27/10VALIDATOR'S SIGNATURE: ##### Mary A. Donovan DATE: 04/26/2010

GENERAL CHEMISTRY ANALYTICAL DATA VALIDATION CHECKLIST	
5120-2 General Chemistry Analytical Data Validation Checklist	Records Use only 

Yes No N/A (Check One)				Assign Qualifier Listed Below If Criterion = Yes	
				Non-detected Analyte	Detected Analyte
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	1. The holding time was >1 and ≤2 times the applicable holding time requirement.	UJ, I9	J-, I9
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	2. The holding time was >2 times the applicable holding time requirement.	R, I9a	J-, I9a
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	3. The affected analytes are regarded as rejected because the analytical holding time was exceeded.	R, I9b	R, I9b
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	4. The affected results were not analyzed with a valid 5-point calibration curve and/or a standard at the reporting limit.	UJ, R, I7	J, I7
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	5. The affected analytes were analyzed with an initial calibration curve that exceeded the %RSD criteria and/or the associated multipoint calibration correlation coefficient is <0.995.	UJ, I7a	J, I7a
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	6. The ICV and/or CCV were recovered outside the method specific limits.	UJ, I7c	J, I7c
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	7. The ICV and/or CCV were not analyzed at the appropriate method frequency.	UJ, I7d	J, I7d
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	8. Required calibration information is missing or samples were analyzed on an expired calibration. Contact the SMO or external laboratory for information.	R, I7f	R, I7f
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	9. The interference check sample percent recovery value is <50%.	R, I2	J-, I2
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	10. The interference check sample percent recovery value is ≥50% and <80%.	UJ, I2a	J-, I2a
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	11. The interference check sample percent recovery value is >120%.	N/A	J+, I2b
<input type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	12. The interference check sample was not analyzed with the samples.	R, I2c	R, I2c
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	13. The sample result is ≤5X the concentration of the related analyte in the method blank.	U, I4	N/A

GENERAL CHEMISTRY ANALYTICAL DATA VALIDATION CHECKLIST	
5120-2 General Chemistry Analytical Data Validation Checklist	Records Use only 

Yes No N/A (Check One)				Assign Qualifier Listed Below If Criterion = Yes	
				Non-detected Analyte	Detected Analyte
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	14. The affected analytes are considered estimated and biased high because this analyte was identified in the method blank but was >5X.	N/A	J, I4a
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	15. The sample result is ≤5X the concentration of the related analyte in the instrument blank and continuing calibration blank.	U, I4b	N/A
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	16. Continuing calibration blanks were not analyzed at the appropriate method frequency.	UJ, I4c	J, I4c
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	17. The sample result is ≤5X the concentration of the related analyte in the trip blank, rinsate blank, or equipment blank.	U, I4d	N/A
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	18. Required method blank information is missing. Data may not be acceptable for use. Contact the SMO or external laboratory for information.	R, I4e	R, I4e
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	19. The associate matrix spike recovery was <10%. Follow the external laboratory limits located within the associated data package.	R, I6	R, I6
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	20. The associated matrix spike recovery was below the Lower Acceptance Limit (LAL) but >10%. Follow the external laboratory limits located within the associated data package.	UJ, I6a	J-, I6a
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	21. The associated matrix spike recovery was above the Upper Acceptance Limit (UAL). Follow the external laboratory limits located within the associated data package.	UJ, I6b	J+, I6b
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	22. Required matrix spike information is missing. Data may not be acceptable for use. Contact the SMO or external laboratory for information. If LCS information is present, do not reject. Qualify data based on LCS information.	R, I6c	R, I6c
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	23. The sample and/or the duplicate sample results RPD is not within the acceptance limits. Follow the external laboratory limits located within the associated data package.	UJ, I10b	J, I10b

GENERAL CHEMISTRY ANALYTICAL DATA VALIDATION CHECKLIST	
5120-2 General Chemistry Analytical Data Validation Checklist	Records Use only 

Yes No N/A				Assign Qualifier Listed Below If Criterion = Yes	
(Check One)				Non-detected Analyte	Detected Analyte
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	24. The duplicate sample was not prepared and/or analyzed with the samples for unspecified reasons. The duplicate information is missing. Data may not be acceptable for use. Contact the SMO or external laboratory for information.	UJ, I10d	J, I10d
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	25. The LCS percent recovery was <10%. Follow the external laboratory limits located within the associated data package.	R, I12	R, I12
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	26. The LCS percent recover was < the LAL but >10%. Follow the external laboratory limits located within the associated data package.	UJ, I12a	J-, I12a
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	27. The LCS percent recovery was > the UAL. Follow the external laboratory limits located within the associated data package.	N/A	J+, I12b
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	28. The LCS documentation is missing. Data may not be acceptable for use. Contact the SMO or external laboratory for information. Do not Reject if MS/MSD information is present. Qualify according to MS/MSD criteria.	R, I12c	R, I12c
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	29. Duplicate, dilution, or reanalysis	UJ, I88	J, I88
<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	30. The LANL project chemist identified quality deficiencies in the reported data that require further qualification. This code can ONLY be used and/or under advisement by the LANL project chemist.	UJ, R, I19	J, R, I19
<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	31. Qualification of data via data validation does not occur based on Quality Control requirements in this procedure. Adhere to the external laboratory qualifiers found within the Form I analytical data summary sheets generated by the external laboratory.	U, U_LAB	J, J_LAB NQ, NQ (no qualification)

GEL LABORATORIES LLC

2040 Savage Road Charleston SC 29407 - (843) 556-8171 - www.gel.com

Certificate of Analysis

Company : Los Alamos National Laboratory
Address : PO Box 1663
TA-03, SM271, Drop Pt. 02U, Rm111
Los Alamos, New Mexico 87545
Contact: Ms. Joylene Valdez
Project: LANL ER Project

Report Date: March 23, 2010

Client SDG: 10-2093

Client Sample ID: RE36-10-8458
Sample ID: 248117001
Matrix: W
Collect Date: 22-FEB-10 12:00
Receive Date: 26-FEB-10
Collector: Client

Project: LANL01004
Client ID: LANL010

Parameter	Qualifier	Result	DL	RL	Units	DF	Analyst	Date	Time	Batch	Method
Flow Injection Analysis											
<i>SW9012A Cyanide, Total "As Received"</i>											
Cyanide, Total	U	ND	1.66	5.00	ug/L	1	AXC2	03/08/10	1512	959217	1
Nutrient Analysis											
<i>EPA 353.2 Nitrogen, Nitrate/Nitrite "As Received"</i>											
Nitrogen, Nitrate/Nitrite	U	ND	0.050	0.250	mg/L	5	AXH3	03/03/10	1229	959199	2

The following Prep Methods were performed

Method	Description	Analyst	Date	Time	Prep Batch
SW846 9010B Prep	SW846 9010B Prep	AXS5	03/08/10	1241	959216

The following Analytical Methods were performed

Method	Description	Analyst Comments
1	SW846 9012A	
2	EPA 353.2	

GEL LABORATORIES LLC

2040 Savage Road Charleston SC 29407 - (843) 556-8171 - www.gel.com

Certificate of Analysis

Company : Los Alamos National Laboratory
Address : PO Box 1663
TA-03, SM271, Drop Pt. 02U, Rm111
Los Alamos, New Mexico 87545
Contact: Ms. Joylene Valdez
Project: LANL ER Project

Report Date: March 24, 2010

Client SDG: 10-2093-1

Client Sample ID: RE36-10-8448
Sample ID: 248118001
Matrix: R
Collect Date: 22-FEB-10 12:00
Receive Date: 26-FEB-10
Collector: Client
Moisture: 2.66%

Project: LANL01004
Client ID: LANL010

Parameter	Qualifier	Result	DL	RL	Units	DF	Analyst	Date	Time	Batch	Method
Electrode Analysis											
<i>SW9045C pH "As Received"</i>											
pH at Temp 19.8C	H	8.45	0.010	0.100	SU	1	LXA1	03/02/10	1250	959805	1
Flow Injection Analysis											
<i>SW9012A Cyanide, Total "Dry Weight Corrected"</i>											
Cyanide, Total	U	ND	64.7	238	ug/kg	1	AXC2	03/08/10	1554	959204	2
Ion Chromatography											
<i>EPA 300.0 Nitrate in Soil "Dry Weight Corrected"</i>											
Nitrate-N	U	ND	0.308	1.03	mg/kg	1	MAR1	03/21/10	1440	962078	3

The following Prep Methods were performed

Method	Description	Analyst	Date	Time	Prep Batch
EPA 300.0 PREP	EPA 300.0 Total Anions in Soil	MAR1	03/19/10	1315	962077
SW846 9010B Prep	SW846 9010B Prep	AXS5	03/08/10	1243	959203

The following Analytical Methods were performed

Method	Description	Analyst Comments
1	SW846 9045C/9045D	
2	SW846 9012A	
3	EPA 300.0	

MAD
04/26/10

GEL LABORATORIES LLC

2040 Savage Road Charleston SC 29407 - (843) 556-8171 - www.gel.com

Certificate of Analysis

Company : Los Alamos National Laboratory
Address : PO Box 1663
TA-03, SM271, Drop Pt. 02U, Rm111
Los Alamos, New Mexico 87545
Contact: Ms. Joylene Valdez
Project: LANL ER Project

Report Date: March 24, 2010

Client SDG: 10-2093-1

Client Sample ID: RE36-10-8456
Sample ID: 248118002
Matrix: R
Collect Date: 22-FEB-10 12:00
Receive Date: 26-FEB-10
Collector: Client
Moisture: 2.81%

Project: LANL01004
Client ID: LANL010

Parameter	Qualifier	Result	DL	RL	Units	DF	Analyst	Date	Time	Batch	Method
Electrode Analysis											
<i>SW9045C pH "As Received"</i>											
pH at Temp 19.7C	H	8.26	0.010	0.100	SU	1	LXA1	03/02/10	1250	959805	1
Flow Injection Analysis											
<i>SW9012A Cyanide, Total "Dry Weight Corrected"</i>											
Cyanide, Total	U	ND	66.0	243	ug/kg	1	AXC2	03/08/10	1555	959204	2
Ion Chromatography											
<i>EPA 300.0 Nitrate in Soil "Dry Weight Corrected"</i>											
Nitrate-N	U	ND	0.309	1.03	mg/kg	1	MAR1	03/21/10	1507	962078	3

The following Prep Methods were performed

Method	Description	Analyst	Date	Time	Prep Batch
EPA 300.0 PREP	EPA 300.0 Total Anions in Soil	MAR1	03/19/10	1315	962077
SW846 9010B Prep	SW846 9010B Prep	AXS5	03/08/10	1243	959203

The following Analytical Methods were performed

Method	Description	Analyst Comments
1	SW846 9045C/9045D	
2	SW846 9012A	
3	EPA 300.0	

Certificate of Analysis

Company : Los Alamos National Laboratory
Address : PO Box 1663
TA-03, SM271, Drop Pt. 02U, Rm111
Los Alamos, New Mexico 87545
Contact: Ms. Joylene Valdez
Project: LANL ER Project

Report Date: March 24, 2010

Client SDG: 10-2093-1

Client Sample ID:	RE36-10-8451	Project:	LANL01004
Sample ID:	248118003	Client ID:	LANL010
Matrix:	R		
Collect Date:	22-FEB-10 12:00		
Receive Date:	26-FEB-10		
Collector:	Client		
Moisture:	3.01%		

Parameter	Qualifier	Result	DL	RL	Units	DF	Analyst	Date	Time	Batch	Method
Electrode Analysis											
<i>SW9045C pH "As Received"</i>											
pH at Temp 20.0C	H	7.92	0.010	0.100	SU	1	LXA1	03/02/10	1250	959805	1
Flow Injection Analysis											
<i>SW9012A Cyanide, Total "Dry Weight Corrected"</i>											
Cyanide, Total	U	ND	68.7	253	ug/kg	1	AXC2	03/08/10	1556	959204	2
Ion Chromatography											
<i>EPA 300.0 Nitrate in Soil "Dry Weight Corrected"</i>											
Nitrate-N	U	ND	0.309	1.03	mg/kg	1	MAR103/21/10	1534	962078		3

The following Prep Methods were performed

Method	Description	Analyst	Date	Time	Prep Batch
EPA 300.0 PREP	EPA 300.0 Total Anions in Soil	MAR1	03/19/10	1315	962077
SW846 9010B Prep	SW846 9010B Prep	AXS5	03/08/10	1243	959203

The following Analytical Methods were performed

Method	Description	Analyst Comments
1	SW846 9045C/9045D	
2	SW846 9012A	
3	EPA 300.0	

GEL LABORATORIES LLC

2040 Savage Road Charleston SC 29407 - (843) 556-8171 - www.gel.com

Certificate of Analysis

Company: Los Alamos National Laboratory
Address: PO Box 1663
TA-03, SM271, Drop Pt. 02U, Rm111
Los Alamos, New Mexico 87545
Contact: Ms. Joylene Valdez
Project: LANL ER Project

Report Date: March 24, 2010

Client SDG: 10-2093-1

Client Sample ID: RE36-10-8450
Sample ID: 248118004
Matrix: R
Collect Date: 22-FEB-10 12:00
Receive Date: 26-FEB-10
Collector: Client
Moisture: 14.9%

Project: LANL01004
Client ID: LANL010

Parameter	Qualifier	Result	DL	RL	Units	DF	Analyst	Date	Time	Batch	Method
Electrode Analysis											
<i>SW9045C pH "As Received"</i>											
pH at Temp 19.9C	H	8.07	0.010	0.100	SU	1	LXA1	03/02/10	1250	959805	1
Flow Injection Analysis											
<i>SW9012A Cyanide, Total "Dry Weight Corrected"</i>											
Cyanide, Total	U	ND	79.9	294	ug/kg	1	AXC2	03/08/10	1557	959204	2
Ion Chromatography											
<i>EPA 300.0 Nitrate in Soil "Dry Weight Corrected"</i>											
Nitrate-N	U	ND	0.353	1.18	mg/kg	1	MAR103/21/10	1601	962078	3	

The following Prep Methods were performed

Method	Description	Analyst	Date	Time	Prep Batch
EPA 300.0 PREP	EPA 300.0 Total Anions in Soil	MAR1	03/19/10	1315	962077
SW846 9010B Prep	SW846 9010B Prep	AXS5	03/08/10	1243	959203

The following Analytical Methods were performed

Method	Description	Analyst Comments
1	SW846 9045C/9045D	
2	SW846 9012A	
3	EPA 300.0	

GEL LABORATORIES LLC

2040 Savage Road Charleston SC 29407 - (843) 556-8171 - www.gel.com

Certificate of Analysis

Company : Los Alamos National Laboratory
Address : PO Box 1663
TA-03, SM271, Drop Pt. 02U, Rm111
Los Alamos, New Mexico 87545
Contact: Ms. Joylene Valdez
Project: LANL ER Project

Report Date: March 24, 2010

Client SDG: 10-2093-1

Client Sample ID: RE36-10-8449
Sample ID: 248118005
Matrix: R
Collect Date: 22-FEB-10 12:00
Receive Date: 26-FEB-10
Collector: Client
Moisture: 1.76%

Project: LANL01004
Client ID: LANL010

Parameter	Qualifier	Result	DL	RL	Units	DF	Analyst	Date	Time	Batch	Method
Electrode Analysis											
<i>SW9045C pH "As Received"</i>											
pH at Temp 20.0C	H	8.62	0.010	0.100	SU	1	LXA1	03/02/10	1250	959805	1
Flow Injection Analysis											
<i>SW9012A Cyanide, Total "Dry Weight Corrected"</i>											
Cyanide, Total	U	ND	66.6	245	ug/kg	1	AXC2	03/08/10	1558	959204	2
Ion Chromatography											
<i>EPA 300.0 Nitrate in Soil "Dry Weight Corrected"</i>											
Nitrate-N	U	ND	0.305	1.02	mg/kg	1	MAR1	03/21/10	1627	962078	3

The following Prep Methods were performed

Method	Description	Analyst	Date	Time	Prep Batch
EPA 300.0 PREP	EPA 300.0 Total Anions in Soil	MAR1	03/19/10	1315	962077
SW846 9010B Prep	SW846 9010B Prep	AXS5	03/08/10	1243	959203

The following Analytical Methods were performed

Method	Description	Analyst Comments
1	SW846 9045C/9045D	
2	SW846 9012A	
3	EPA 300.0	

GEL LABORATORIES LLC

2040 Savage Road Charleston SC 29407 - (843) 556-8171 - www.gel.com

Certificate of Analysis

Company : Los Alamos National Laboratory
Address : PO Box 1663
TA-03, SM271, Drop Pt. 02U, Rm111
Los Alamos, New Mexico 87545
Contact: Ms. Joylene Valdez
Project: LANL ER Project

Report Date: March 24, 2010

Client SDG: 10-2093-1

Client Sample ID: RE36-10-8453
Sample ID: 248118006
Matrix: R
Collect Date: 22-FEB-10 12:00
Receive Date: 26-FEB-10
Collector: Client
Moisture: 4.28%

Project: LANL01004
Client ID: LANL010

Parameter	Qualifier	Result	DL	RL	Units	DF	Analyst	Date	Time	Batch	Method
Electrode Analysis											
<i>SW9045C pH "As Received"</i>											
pH at Temp 20.1C	H	8.60	0.010	0.100	SU	1	LXA1	03/02/10	1252	959805	1
Flow Injection Analysis											
<i>SW9012A Cyanide, Total "Dry Weight Corrected"</i>											
Cyanide, Total	U	ND	61.2	225	ug/kg	1	AXC2	03/08/10	1559	959204	2
Ion Chromatography											
<i>EPA 300.0 Nitrate in Soil "Dry Weight Corrected"</i>											
Nitrate-N	U	ND	0.313	1.04	mg/kg	1	MAR103	21/10	1748	962078	3

The following Prep Methods were performed

Method	Description	Analyst	Date	Time	Prep Batch
EPA 300.0 PREP	EPA 300.0 Total Anions in Soil	MAR1	03/19/10	1315	962077
SW846 9010B Prep	SW846 9010B Prep	AXS5	03/08/10	1243	959203

The following Analytical Methods were performed

Method	Description	Analyst Comments
1	SW846 9045C/9045D	
2	SW846 9012A	
3	EPA 300.0	

GEL LABORATORIES LLC

2040 Savage Road Charleston SC 29407 - (843) 556-8171 - www.gel.com

Certificate of Analysis

Company : Los Alamos National Laboratory
Address : PO Box 1663
TA-03, SM271, Drop Pt. 02U, Rm111
Los Alamos, New Mexico 87545
Contact: Ms. Joylene Valdez
Project: LANL ER Project

Report Date: March 24, 2010

Client SDG: 10-2093-1

Client Sample ID: RE36-10-8452
Sample ID: 248118007
Matrix: R
Collect Date: 22-FEB-10 12:00
Receive Date: 26-FEB-10
Collector: Client
Moisture: 7.14%

Project: LANL01004
Client ID: LANL010

Parameter	Qualifier	Result	DL	RL	Units	DF	Analyst	Date	Time	Batch	Method
Electrode Analysis											
<i>SW9045C pH "As Received"</i>											
pH at Temp 20.1C	H	8.23	0.010	0.100	SU	1	LXA1	03/02/10	1253	959805	1
Flow Injection Analysis											
<i>SW9012A Cyanide, Total "Dry Weight Corrected"</i>											
Cyanide, Total	U	ND	63.1	232	ug/kg	1	AXC2	03/08/10	1600	959204	2
Ion Chromatography											
<i>EPA 300.0 Nitrate in Soil "Dry Weight Corrected"</i>											
Nitrate-N	U	ND	0.323	1.08	mg/kg	1	MAR1	03/21/10	1815	962078	3

The following Prep Methods were performed

Method	Description	Analyst	Date	Time	Prep Batch
EPA 300.0 PREP	EPA 300.0 Total Anions in Soil	MAR1	03/19/10	1315	962077
SW846 9010B Prep	SW846 9010B Prep	AXS5	03/08/10	1243	959203

The following Analytical Methods were performed

Method	Description	Analyst Comments
1	SW846 9045C/9045D	
2	SW846 9012A	
3	EPA 300.0	

Thursday, February 25, 2010

LAB CHAIN OF CUSTODY DOCUMENT NUMBER: 10-2093

LOS ALAMOS

REQUEST NUMBER: 10-2093

NATIONAL LABORATORY

ATTN: Valerie Davis

TURNAROUND/REPORT DUE: 3/27/2010

General Engineering Laboratories, Inc.,
Charleston, SC.

TURNAROUND REQ'D: 30

2040 Savage Rd

Charleston, SC 29407

LAB REQUEST COMMENTS:

248117, 248118/.

SAMPLE ID	CTNR	CTNR DESC	ORDER	PRESERV	MATRIX
RE36-10-8458	1	POLY	METALS+U-GEL	Nitric Acid	W
RE36-10-8458	1	POLY	NO3NO2	Sulfuric Acid (Hydrogen Sulfate)	W
RE36-10-8458	1	POLY	SW-846:6850	Ice	W
RE36-10-8458	1	POLY	TCN	Sodium Hydroxide	W
RE36-10-8448	1	POLY	METALS+U-GEL	Ice	R
RE36-10-8448	1	POLY	Perchlorate+CN+N03+pH	Ice	R
RE36-10-8458	1	POLY	METALS+U-GEL	Ice	R
RE36-10-8458	1	POLY	Perchlorate+CN+N03+pH	Ice	R
RE36-10-8451	1	POLY	METALS+U-GEL	Ice	R
RE36-10-8451	1	POLY	Perchlorate+CN+N03+pH	Ice	R
RE36-10-8450	1	POLY	METALS+U-GEL	Ice	R
RE36-10-8450	1	POLY	Perchlorate+CN+N03+pH	Ice	R
RE36-10-8449	1	POLY	METALS+U-GEL	Ice	R
RE36-10-8449	1	POLY	Perchlorate+CN+N03+pH	Ice	R
RE36-10-8453	1	POLY	METALS+U-GEL	Ice	R
RE36-10-8453	1	POLY	Perchlorate+CN+N03+pH	Ice	R
RE36-10-8452	1	POLY	METALS+U-GEL	Ice	R
RE36-10-8452	1	POLY	Perchlorate+CN+N03+pH	Ice	R

Relinquished By:

Date Time

Received By:

Date Time

[Signature]
 Printed Name Signature

2/25/10 1400

Greg Tyler *[Signature]* 2-26-10 0845
 Printed Name Signature

Printed Name Signature

Printed Name Signature

Printed Name Signature

Printed Name Signature

Received for DISPOSAL By:

Date Time

Remarks:

Printed Name Signature

Thursday, February 25, 2010
LOS ALAMOS
NATIONAL LABORATORY


ATTN: Valerie Davis
General Engineering Laboratories, Inc., Charleston, SC.
2040 Savage Rd
Charleston, SC 29407

These Samples are on:
LANL Request Number: 10-2093
Per Agreement Number: 126310011
Project Cost Code: MR3A05529E00

Please analyse the enclosed samples
according to the schedule indicated:

SHIP DATE: 2/25/2010
TURNAROUND/REPORT DUE: 3/27/2010
TURNAROUND REQ'D: 30 Days

RAD SCREENING: Yes, Below Background
LAB REQUEST COMMENTS:

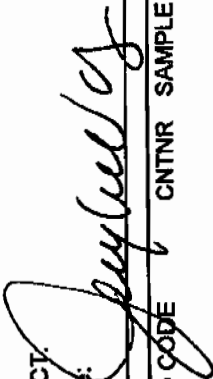LANL SMO CONTACT:
Signature: 

PRIORITY	METHOD CODE	CNTNR	SAMPLE ID	SAMPLE MATRIX	DATE SAMPLED	SPECIAL INSTRUCTIONS
	EPA:300.0	1	RE36-10-8448	R	2/22/2010	
		1	RE36-10-8449	R	2/22/2010	
		1	RE36-10-8450	R	2/22/2010	
		1	RE36-10-8451	R	2/22/2010	
		1	RE36-10-8452	R	2/22/2010	
		1	RE36-10-8453	R	2/22/2010	
		1	RE36-10-8456	R	2/22/2010	
	EPA:353.2	1	RE36-10-8458	W	2/22/2010	
	SW-846:6010B	1	RE36-10-8448	R	2/22/2010	

Thursday, February 25, 2010 Page 2 of 3
 REQUEST NUMBER: 10-2093

PRIORITY	METHOD CODE	CNTNR	SAMPLE ID	SAMPLE MATRIX	DATE SAMPLED	SPECIAL INSTRUCTIONS
	SW-846:6010B	1	RE36-10-8449	R	2/22/2010	
		1	RE36-10-8450	R	2/22/2010	
		1	RE36-10-8451	R	2/22/2010	
		1	RE36-10-8452	R	2/22/2010	
		1	RE36-10-8453	R	2/22/2010	
		1	RE36-10-8456	R	2/22/2010	
	SW-846:6020	1	RE36-10-8448	R	2/22/2010	
		1	RE36-10-8449	R	2/22/2010	
		1	RE36-10-8450	R	2/22/2010	
		1	RE36-10-8451	R	2/22/2010	
		1	RE36-10-8452	R	2/22/2010	
		1	RE36-10-8453	R	2/22/2010	
		1	RE36-10-8456	R	2/22/2010	
	SW-846:6850	1	RE36-10-8458	W	2/22/2010	
		1	RE36-10-8448	R	2/22/2010	
		1	RE36-10-8449	R	2/22/2010	
		1	RE36-10-8450	R	2/22/2010	
		1	RE36-10-8451	R	2/22/2010	
		1	RE36-10-8452	R	2/22/2010	
		1	RE36-10-8453	R	2/22/2010	
		1	RE36-10-8456	R	2/22/2010	
		1	RE36-10-8458	W	2/22/2010	
	SW-846:7470A	1	RE36-10-8458	W	2/22/2010	
	SW-846:7471A	1	RE36-10-8448	R	2/22/2010	
		1	RE36-10-8449	R	2/22/2010	
		1	RE36-10-8450	R	2/22/2010	
		1	RE36-10-8451	R	2/22/2010	
		1	RE36-10-8452	R	2/22/2010	

REQUEST NUMBER: 10-2093

Thursday, February 25, 2010

PRIORITY	METHOD CODE	CNTNR	SAMPLE ID	SAMPLE MATRIX	DATE SAMPLED	SPECIAL INSTRUCTIONS
	SW-846:7471A	1	RE36-10-8453	R	2/22/2010	
		1	RE36-10-8456	R	2/22/2010	
	SW-846:9012A	1	RE36-10-8448	R	2/22/2010	
		1	RE36-10-8449	R	2/22/2010	
		1	RE36-10-8450	R	2/22/2010	
		1	RE36-10-8451	R	2/22/2010	
		1	RE36-10-8452	R	2/22/2010	
		1	RE36-10-8453	R	2/22/2010	
		1	RE36-10-8456	R	2/22/2010	
		1	RE36-10-8458	W	2/22/2010	
	SW-846:9045C	1	RE36-10-8448	R	2/22/2010	
		1	RE36-10-8449	R	2/22/2010	
		1	RE36-10-8450	R	2/22/2010	
		1	RE36-10-8451	R	2/22/2010	
		1	RE36-10-8452	R	2/22/2010	
		1	RE36-10-8453	R	2/22/2010	
		1	RE36-10-8456	R	2/22/2010	

Final Page of REQUEST NUMBER 10-2093



March 04, 2010

www.gel.com

Ms. Joylene Valdez
Los Alamos National Laboratory
PO Box 1663
TA-03, SM271, Drop Pt. 02U, Rm111
Los Alamos, New Mexico 87545

Re: LANL ER Project
Work Orders: 248117 248118
SDG: 10-2093

Dear Ms. Valdez:

GEL Laboratories, LLC (GEL) appreciates the opportunity to provide the following analytical results for the sample(s) we received on February 26, 2010, and analyzed for General Chemistry, Metals and Perchlorates by LCMSMS. This original data report has been prepared and reviewed in accordance with GEL's standard operating procedures.

Our policy is to provide high quality, personalized analytical services to enable you to meet your analytical needs on time every time. We trust that you will find everything in order and to your satisfaction. If you have any questions, please do not hesitate to call me at (843) 556-8171, ext. 4485.

Sincerely,

Valerie Davis
Project Manager

Purchase Order: 72733-001-09
Chain of Custody: 10-2093
Enclosures

Los Alamos National Laboratory (72733-001-09)

LANL ER Project

Work Order #: 248117 and 248118

SDG: 10-2093

Table of Contents

Case Narrative.....	1
Chain of Custody and Supporting Documentation	4
Data Review Qualifier Flag Definition Sheet	17
LC/MS/MS Perchlorate Analysis.....	19
Sample Data Summary	24
Quality Control Summary	26
Sample Data	57
Standards Data.....	60
Quality Control	89
Miscellaneous Data	94
LC/MS/MS Perchlorate Analysis.....	103
Sample Data Summary	108
Quality Control Summary.....	116
Sample Data	138
Standards Data.....	153
Quality Control	165
Miscellaneous Data	170
Metals Analysis	178
Case Narrative	179
Sample Data Summary	185
Quality Control Summary.....	187
Standards	234
Raw Data	247
Miscellaneous	488
Metals Analysis	527
Case Narrative	528
Sample Data Summary	534
Quality Control Summary.....	542
Standards	601
Raw Data	613
Miscellaneous	856
General Chemistry Analysis	900
Case Narrative	901
Sample Data Summary	908

Quality Control Summary.....	911
Instrument QC Data Summary	914
Cyanide, Total	917
Nitrate Nitrite by Cadmium Reduction	936
General Chemistry Analysis	947
Case Narrative	948
Sample Data Summary	958
Quality Control Summary.....	967
Instrument QC Data Summary	971
Cyanide, Total	974
Ion Chromatography	993
pH	1042
Miscellaneous	1046

Case Narrative

**Case Narrative for
Los Alamos National Laboratory (72733-001-09)
LANL ER Project
Workorder #: 248117 and 248118
SDG # : 10-2093**

March 04, 2010

Laboratory Identification:

GEL Laboratories LLC
2040 Savage Road
Charleston, South Carolina 29407
(843) 556-8171

Summary

Sample receipt The samples arrived at GEL Laboratories LLC, Charleston, South Carolina on February 26, 2010 for analysis. The sample was prepared/analyzed within the required holding time. Shipping container temperature was checked, documented, and within specifications. The samples were screened according to GEL Standard Operating Procedure. The lab did not receive the NO3NO2 container for sample RE36-10-8458. Los Alamos was notified. All sample containers arrived without any visible signs of tampering or breakage. Containers were checked for pH, where appropriate, and matched the preservative as documented on the accompanying chain of custody. Shipping container temperature was within specification (0 - 6C).

Sample Identification The laboratory received the following samples:

<u>Laboratory ID</u>	<u>Client ID</u>
248117001	RE36-10-8458
248118001	RE36-10-8448
248118002	RE36-10-8456
248118003	RE36-10-8451
248118004	RE36-10-8450
248118005	RE36-10-8449
248118006	RE36-10-8453
248118007	RE36-10-8452

Case Narrative

Sample analyses were conducted using methodology as outlined in GEL Laboratories, LLC (GEL) Standard Operating Procedures. Any technical or administrative problems during analysis, data review, and reduction are contained in the analytical case narratives in the enclosed data package.

Data Package The enclosed data package contains the following sections: Case Narrative, Chain of Custody, Cooler Receipt Checklist, Data Package Qualifier Definitions and data from the following fractions: General Chemistry, Metals and Perchlorates by LCMSMS.

I certify that this data report is in compliance with the terms and conditions of the subcontract and task order, both technically and for completeness, for other than the conditions detailed in the attached case narrative.

Valerie Davis

Valerie Davis
Project Manager

List of current GEL Certifications as of 04 March 2010

State	Certification
Arizona	AZ0668
Arkansas	88-0651
CLIA	42D0904046
California – NELAP	01151CA
Colorado	GEL
Connecticut	PH-0169
Dept. of Navy	NFESC 413
EPA Region 5	WG-15J
Florida – NELAP	E87156
Georgia	E87156 (FL/NELAP)
Georgia DW	967
Hawaii	N/A
ISO 17025	2567.01
Idaho	SC00012
Illinois – NELAP	200029
Indiana	C-SC-01
Kansas – NELAP	E-10332
Kentucky	90129
Louisiana – NELAP	03046
Maryland	270
Massachusetts	M-SC012
Nevada	SC00012
New Jersey – NELAP	SC002
New Mexico	FL NELAP E87156
New York – NELAP	11501
North Carolina	233
North Carolina DW	45709
Oklahoma	9904
Pennsylvania – NELAP	68-00485
South Carolina	10120001/10120002
Tennessee	TN 02934
Texas – NELAP	T104704235-07B-TX
U.S. Dept. of Agriculture	S-52597
Utah – NELAP	GEL
Vermont	VT87156
Virginia	00151
Washington	C1641

Chain of Custody and Supporting Documentation

Thursday, February 25, 2010

LAB CHAIN OF CUSTODY DOCUMENT NUMBER: 10-2093

LOS ALAMOS

REQUEST NUMBER: 10-2093

NATIONAL LABORATORY

ATTN: Valerie Davis

TURNAROUND/REPORT DUE: 3/27/2010

General Engineering Laboratories, Inc.,
Charleston, SC.

TURNAROUND REQ'D: 30

2040 Savage Rd

Charleston, SC 29407

LAB REQUEST COMMENTS:

248117, 248118/.

SAMPLE ID	CTNR	CTNR DESC	ORDER	PRESERV	MATRIX
RE36-10-8458	1	POLY	METALS+U-GEL	Nitric Acid	W
RE36-10-8458	1	POLY	NO3NO2	Sulfuric Acid (Hydrogen Sulfate)	W
RE36-10-8458	1	POLY	SW-846:6850	Ice	W
RE36-10-8458	1	POLY	TCN	Sodium Hydroxide	W
RE36-10-8448	1	POLY	METALS+U-GEL	Ice	R
RE36-10-8448	1	POLY	Perchlorate+CN+N03+pH	Ice	R
RE36-10-8456	1	POLY	METALS+U-GEL	Ice	R
RE36-10-8456	1	POLY	Perchlorate+CN+N03+pH	Ice	R
RE36-10-8451	1	POLY	METALS+U-GEL	Ice	R
RE36-10-8451	1	POLY	Perchlorate+CN+N03+pH	Ice	R
RE36-10-8450	1	POLY	METALS+U-GEL	Ice	R
RE36-10-8450	1	POLY	Perchlorate+CN+N03+pH	Ice	R
RE36-10-8449	1	POLY	METALS+U-GEL	Ice	R
RE36-10-8449	1	POLY	Perchlorate+CN+N03+pH	Ice	R
RE36-10-8453	1	POLY	METALS+U-GEL	Ice	R
RE36-10-8453	1	POLY	Perchlorate+CN+N03+pH	Ice	R
RE36-10-8452	1	POLY	METALS+U-GEL	Ice	R
RE36-10-8452	1	POLY	Perchlorate+CN+N03+pH	Ice	R

Relinquished By:

Date Time

Received By:

Date Time

Printed Name

Signature

2/25/10 1400

Printed Name

Signature

Greg Tyler Greg Tyler 2-26-10 0845

Printed Name

Signature

Printed Name

Signature

Printed Name

Signature

Printed Name

Signature

Received for DISPOSAL By:

Date Time

Remarks:

Printed Name

Signature

Thursday, February 25, 2010

LOS ALAMOS
NATIONAL LABORATORY

ATTN: Valerie Davis

General Engineering Laboratories, Inc., Charleston, SC.

2040 Savage Rd

Charleston, SC 29407

Please analyse the enclosed samples
according to the schedule indicated:

SHIP DATE: 2/25/2010

TURNAROUND/REPORT DUE: 3/27/2010


TURNAROUND REQ'D: 30 Days

RAD SCREENING: Yes, Below Background

LAB REQUEST COMMENTS:

LANL ER SMO CONTACT:

Signature:

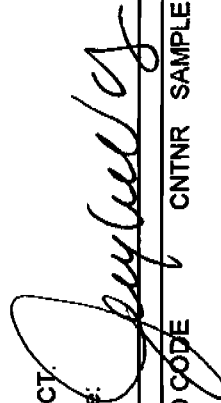

These Samples are on:
LANL Request Number: 10-2093
Per Agreement Number: 126310011
Project Cost Code: MR3A05529E00

Page 1 of 3
REQUEST NUMBER: 10-2093

PRIORITY	METHOD CODE	CNTNR	SAMPLE ID	SAMPLE MATRIX	DATE SAMPLED	SPECIAL INSTRUCTIONS
	EPA-300.0	1	RE36-10-8448	R	2/22/2010	
		1	RE36-10-8449	R	2/22/2010	
		1	RE36-10-8450	R	2/22/2010	
		1	RE36-10-8451	R	2/22/2010	
		1	RE36-10-8452	R	2/22/2010	
		1	RE36-10-8453	R	2/22/2010	
		1	RE36-10-8456	R	2/22/2010	
	EPA-353.2	1	RE36-10-8458	W	2/22/2010	
	SW-846:6010B	1	RE36-10-8448	R	2/22/2010	

Thursday, February 25, 2010

REQUEST NUMBER: 10-2093

PRIORITY	METHOD CODE	CNTNR	SAMPLE ID	SAMPLE MATRIX	DATE SAMPLED	SPECIAL INSTRUCTIONS
	SW-846:6010B	1	RE36-10-8449	R	2/22/2010	
		1	RE36-10-8450	R	2/22/2010	
		1	RE36-10-8451	R	2/22/2010	
		1	RE36-10-8452	R	2/22/2010	
		1	RE36-10-8453	R	2/22/2010	
		1	RE36-10-8456	R	2/22/2010	
	SW-846:6020	1	RE36-10-8448	R	2/22/2010	
		1	RE36-10-8449	R	2/22/2010	
		1	RE36-10-8450	R	2/22/2010	
		1	RE36-10-8451	R	2/22/2010	
		1	RE36-10-8452	R	2/22/2010	
		1	RE36-10-8453	R	2/22/2010	
		1	RE36-10-8456	R	2/22/2010	
		1	RE36-10-8458	W	2/22/2010	
	SW-846:6850	1	RE36-10-8448	R	2/22/2010	
		1	RE36-10-8449	R	2/22/2010	
		1	RE36-10-8450	R	2/22/2010	
		1	RE36-10-8451	R	2/22/2010	
		1	RE36-10-8452	R	2/22/2010	
		1	RE36-10-8453	R	2/22/2010	
		1	RE36-10-8456	R	2/22/2010	
		1	RE36-10-8458	W	2/22/2010	
	SW-846:7470A	1	RE36-10-8458	W	2/22/2010	
	SW-846:7471A	1	RE36-10-8448	R	2/22/2010	
		1	RE36-10-8449	R	2/22/2010	
		1	RE36-10-8450	R	2/22/2010	
		1	RE36-10-8451	R	2/22/2010	
		1	RE36-10-8452	R	2/22/2010	

Thursday, February 25, 2010

Page 3 of 3

REQUEST NUMBER: 10-2093

PRIORITY	METHOD CODE	CNTNR	SAMPLE ID	SAMPLE MATRIX	DATE SAMPLED	SPECIAL INSTRUCTIONS
	SW-846:7471A	1	RE36-10-8453	R	2/22/2010	
		1	RE36-10-8456	R	2/22/2010	
	SW-846:9012A	1	RE36-10-8448	R	2/22/2010	
		1	RE36-10-8449	R	2/22/2010	
		1	RE36-10-8450	R	2/22/2010	
		1	RE36-10-8451	R	2/22/2010	
		1	RE36-10-8452	R	2/22/2010	
		1	RE36-10-8453	R	2/22/2010	
		1	RE36-10-8456	R	2/22/2010	
		1	RE36-10-8458	W	2/22/2010	
	SW-846:9045C	1	RE36-10-8448	R	2/22/2010	
		1	RE36-10-8449	R	2/22/2010	
		1	RE36-10-8450	R	2/22/2010	
		1	RE36-10-8451	R	2/22/2010	
		1	RE36-10-8452	R	2/22/2010	
		1	RE36-10-8453	R	2/22/2010	
		1	RE36-10-8456	R	2/22/2010	

Final Page of REQUEST NUMBER 10-2093

SAMPLE RECEIPT & REVIEW FORM

Client: LANL		SDG/ARCOC/Work Order: 10-2093	
Received By: Greg Tyler		Date Received: 2/26/10	
Suspected Hazard Information	Yes	No	*If Counts > x2 area background on samples not marked "radioactive", contact the Radiation Safety Group of further investigation.
COC/Samples marked as radioactive?		X	Maximum Counts Observed*: 60cpm
Classified Radioactive II by RSO?		X	
COC/Samples marked containing PCBs?		X	
Shipped as a DOT Hazardous?		X	Hazard Class Shipped: UN#:
Samples identified as Foreign Soil?		X	

Sample Receipt Criteria	Yes	NA	No	Comments/Qualifiers (Required for Non-Conforming Items)
1 Shipping containers received intact and sealed?	X			Circle Applicable: seals broken damaged container leaking container other (describe)
2 Samples requiring cold preservation within 0 ≤ 6 deg. C?	X			Preservation Method: ice bags blue ice dry ice none other 1-3,6C 11-14,17
3 Chain of custody documents included with shipment?	X			
4 Sample containers intact and sealed?	X			Circle Applicable: seals broken damaged container leaking container other (describe)
5 Samples requiring chemical preservation at proper pH?	X			Sample ID's, containers affected and observed pH: If Preservation added, Lot#:
6 VOA vials free of headspace (defined as < 6mm bubble)?		X		Sample ID's and containers affected:
7 Are Encore containers present?			X	(If yes, immediately deliver to Volatiles laboratory)
8 Samples received within holding time?	X			Id's and tests affected:
9 Sample ID's on COC match ID's on bottles?	X			Sample ID's and containers affected:
10 Date & time on COC match date & time on bottles?		X		Sample ID's affected: No time on Chain of Custody.
11 Number of containers received match number indicated on COC?			X	Sample ID's affected: RE36-10-8458 The lab did not receive the (1) 250 Ml Poly for N03N02 as indicated on COC.
12 COC form is properly signed in relinquished/received sections?	X			

Comments:

Fed Ex Tracking Numbers:

7209 7850 2341 1C 7209 7850 2319 2C 7209 7850 2352 12C
 7209 7850 2320 1C 7209 7850 2422 3C 7209 7850 2271 13C
 7209 7850 2396 2C 7209 7850 2385 3C 7209 7850 2466 13C
 7209 7850 2374 2C 7209 7850 2444 6C 7209 7850 2282 14C
 7209 7850 2330 2C 7209 7850 2400 6C 7209 7850 2293 17C
 7209 7850 2455 2C 7209 7850 2477 6C
 7209 7850 2308 2C 7209 7850 2433 6C
 7209 7850 2411 2C 7209 7850 2260 11C

PM (or PMA) review: Initials *gt*

Date 3/1/10

Subject: Sample Receipt for 2/26/10

From: Dionne Francis <Dionne.Francis@gel.com>

Date: Mon, 01 Mar 2010 10:54:43 -0500

To: "Keith R. Greene" <kgreene@lanl.gov>, Joylene Valdez <joylenev@lanl.gov>, Valerie Davis <vsd@gel.com>

Keith,

RN 10-2096: the Gross A/B containers will be preserved prior to analysis.

RN 10-2108: the Gross A/B, Metals, Rad and CN will be preserved prior to analysis.

RN 10-2101: the lab rec'd (1) 1L amber glass HEXP container for sample CAPA-10-12847 instead of (3) as indicated on the COC.

RN 10-2122: the lab did not receive a NO3NO2 container for sample RE36-10-7529.

RN 10-2090: the lab did not receive a NO3NO2 container for sample RE15-10-8407.

RN 10-2093: the lab did not receive a NO3NO2 container for sample RE36-10-8458.

An aliquot will be taken from the perchlorate container and preserved.

RN 10-2102: the lab rec'd (1) 40ml vial 8260B container for sample RE46-10-13207 instead of (2) as indicated on the COC.

RN 10-2107: the Ra226+228, Rad, Gross A/B, Metals and CN containers will be preserved prior to analysis.

RN 10-2110: the TKN+TOC container for sample CAPA-10-12823 will be preserved prior to analysis.

The lab did not receive any containers for RN#s 10-2097 and 10-2098.

The following containers rec'd without a COC:

WST51-10-13119 - LL-H3 1L poly

RE11-10-1654 - RADVANA+B+G 250ml poly

Thanks,

Dionne

--

Dionne Francis
Project Manager Assistant
GEL Laboratories, LLC
2040 Savage Road
Charleston, SC (USA) 29407
Direct: 843.769.7376 Ext. 4432
Main: 843.556.8171
Fax: 843.766.1178
E-mail: daf@gel.com
Web: www.gel.com

Let the Bible fill the memory, rule the heart, and guide the feet.

ORIGIN ID: SAFA (505) 665-9968
JOYLENE VALDEZ
LOS ALAMOS NATL LAB
TA00 BLDG 1237 DPU 03

SHIP DATE: 25FEB10
ACTWGT: 57.0 LB MAN
CAD: 0014176/CAFE2450

LOS ALAMOS, NM 87545
UNITED STATES US

BILL SENDER


TO VALERIE DAVIS
GENERAL ENGINEERING LAB
2040 SAVAGE RD

CHARLESTON SC 29407

(843) 556-8171

REF: 6B010AMR3A022DXL00

10

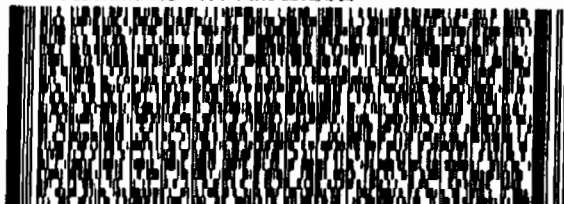

FedEx
Express



ORIGIN ID: SAFA (505) 665-9968
JOYLENE VALDEZ
LOS ALAMOS NATL LAB
TA00 BLDG 1237 DPU 03

SHIP DATE: 25FEB10
ACTWGT: 48.0 LB MAN
CAD: 0014176/CAFE2450

LOS ALAMOS, NM 87545
UNITED STATES US

BILL SENDER

TO VALERIE DAVIS
GENERAL ENGINEERING LAB
2040 SAVAGE RD

CHARLESTON SC 29407

(843) 556-8171

REF: 6B010AMR1A015AGNMO

1c



FedEx
Express




1 of 2
TRKH 7209 7850 2341
0201
MM MASTER MM

FRI - 26FEB A
PRIORITY OVERNIGHT

XX CHSA

29407
SC-US
CHS

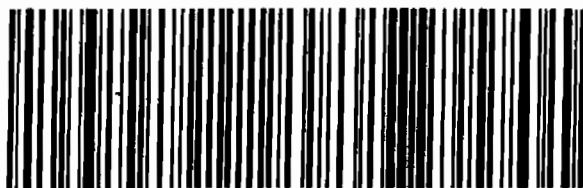

1 of 2
TRKH 7209 7850 2320
0201
MM MASTER MM

FRI - 26FEB A1
PRIORITY OVERNIGHT

XX CHSA

29407
SC-US
CHS



ORIGIN ID: SAFA (505) 665-9968
JOYLENE VALDEZ
LOS ALAMOS NATL LAB
TA00 BLDG 1237 DPU 03

SHIP DATE: 25FEB10
ACTWGT: 58.0 LB MAN
CAD: 0014176/CAFE2450

LOS ALAMOS, NM 87545
UNITED STATES US

BILL SENDER


TO VALERIE DAVIS
GENERAL ENGINEERING LAB
2040 SAVAGE RD

CHARLESTON SC 29407

(843) 556-8171

REF: 6B010AARDW01EA1S00

2°

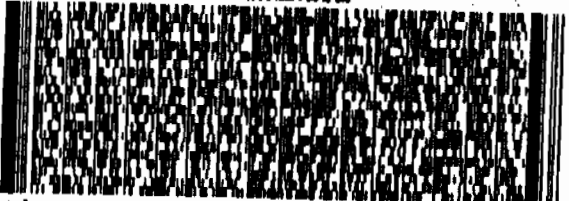

FedEx
Express



JOYLENE VALDEZ
LOS ALAMOS NATL LAB
TA00 BLDG 1237 DPU 03

SHIP DATE: 25FEB10
ACTWGT: 48.0 LB MAN
CAD: 0014176/CAFE2450

LOS ALAMOS, NM 87545
UNITED STATES US

BILL SENDER


TO VALERIE DAVIS
GENERAL ENGINEERING LAB
2040 SAVAGE RD

CHARLESTON SC 29407

(843) 556-8171

REF: 6B010AMR3A0532VA00

2°

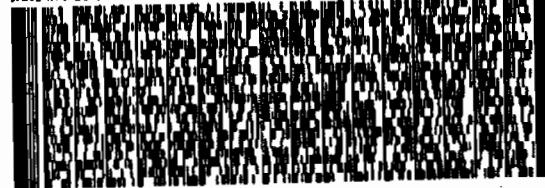

FedEx
Express



2 of 2
MPS# 7209 7850 2396
0263

FRI - 26FEB A1
PRIORITY OVERNIGHT

Matr# 7209 7850 2385 0201

XX CHSA

29407
SC-US

TRKH 7209 7850 2374
0201

FRI - 26FEB A1
PRIORITY OVERNIGHT

XX CHSA

29407
SC-US
CHS

11

ORIGIN ID: SAFA (06) 665-9968
JOYLENE VALDEZ
LOS ALAMOS NATL LAB
TA00 BLDG 1237 DPU 03

SHIP DATE: 25FEB10
ACTWGT: 49.0 LB MAN
CAD: 0014176/CAFE2450

LOS ALAMOS, NM 87545
UNITED STATES US

BILL SENDER

TO VALERIE DAVIS
GENERAL ENGINEERING LAB
2040 SAVAGE RD

CHARLESTON SC 29407

(843) 556-8171
REF: 6B010AMR1A03AGWMO



J052009111302223

2 of 2


FRI - 26FEB A1

FRI - 26 FEB A1
PRIORITY OVERNIGHT

FedEx
TRK# 7209 7850 2330
0201

XX CHSA

29407
SC-US
CHS

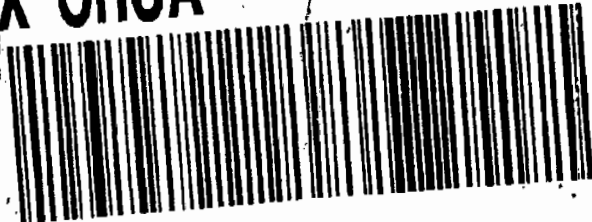

Emp# 133998 25FEB10 SAFA

TA00 BLDG 1237 DPU 03

LOS ALAMOS, NM 87545
UNITED STATES US

ACTWGT: 52.0 LB MAN
CAD: 0014176/CAFE2450

BILL SENDER

TO VALERIE DAVIS
GENERAL ENGINEERING LAB
2040 SAVAGE RD

CHARLESTON SC 29407

(843) 556-8171
REF: 6B010AMR1A015AGWMO



J052009111302223

1 of 2

TRK# 7209 7850 2308
0201

NN MASTER NN

XX CHSA

FRI - 26FEB A1
PRIORITY OVERNIGHT

29407
SC-US
CHS

ORIGIN ID: SAFA (505) 665-9968
JOYLENE VALDEZ
LOS ALAMOS NATL LAB
TA00 BLDG 1237 DPU 03

SHIP DATE: 25FEB10
ACTWGT: 50.0 LB MAN
CAD: 0014176/CAFE2450


LOS ALAMOS, NM 87545
UNITED STATES US

BILL SENDER

TO VALERIE DAVIS
GENERAL ENGINEERING LAB
2040 SAVAGE RD

CHARLESTON SC 29407

(843) 556-8171
REF: 6B010AMR3A05529E00

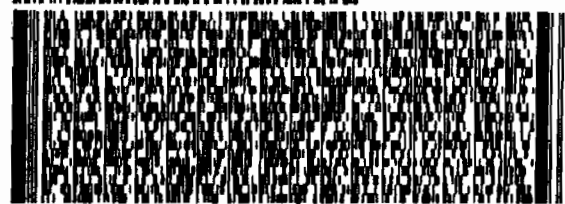

J052009111302223

1 of 3


TRK# 7209 7850 2455
0201

NN MASTER NN

XX CHSA

FRI - 26FEB A1
PRIORITY OVERNIGHT

29407
SC-US
CHS

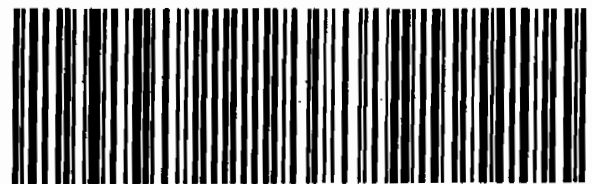

ORIGIN ID: SAFA (505) 665-9968
JOYLENE VALDEZ
LOS ALAMOS NATL LAB
TA00 BLDG 1237 DPU 03

SHIP DATE: 25FEB10
ACTWGT: 60.0 LB MAN
CAD: 0014176/CAFE2450

LOS ALAMOS, NM 87545
UNITED STATES US

BILL SENDER

TO VALERIE DAVIS
GENERAL ENGINEERING LAB
2040 SAVAGE RD

CHARLESTON SC 29407

(843) 556-8171
REF: 6B010AMR3A05529E00



J052009111302223

2 of 2

MPS# 7209 7850 2411
0263

Matr# 7209 7850 2400 0201

XX CHSA

FRI - 26FEB A1
PRIORITY OVERNIGHT

29407.
SC-US
CHS

ORIGIN ID: SAFA (505) 665-9968
JOYLENE VALDEZ
LOS ALAMOS NATL LAB.
TA00 BLDG 1237 DPU 03

LOS ALAMOS, NM 87545
UNITED STATES US


SHIP DATE: 25FEB10
ACTWGT: 53.0 LB MAN
CAD: 0014176/CAFE2450

BILL SENDER

VALERIE DAVIS
GENERAL ENGINEERING LAB
2040 SAVAGE RD

CHARLESTON SC 29407
(843) 556-8171
REF: 6B010AMR1A015AGWMO

2C

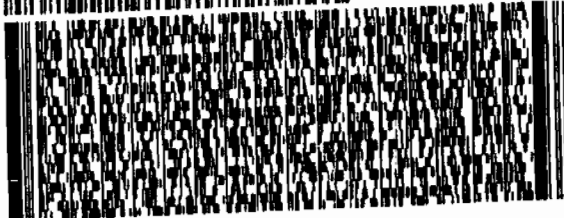

FedEx
Express



2 of 2
MPS# 7209 7850 2319
Matr# 7209 7850 2308 0201

FRI - 26FEB A1
PRIORITY OVERNIGHT

29407
SC-US
CHS

XX CHSA



ORIGIN ID: SAFA (505) 665-9968
JOYLENE VALDEZ
LOS ALAMOS NATL LAB.
TA00 BLDG 1237 DPU 03

LOS ALAMOS, NM 87545
UNITED STATES US


SHIP DATE: 25FEB10
ACTWGT: 52.0 LB MAN
CAD: 0014176/CAFE2450

BILL SENDER

TO VALERIE DAVIS
GENERAL ENGINEERING LAB
2040 SAVAGE RD

CHARLESTON SC 29407
(843) 556-8171
REF: 6B010AARDW01EA1S00

3C

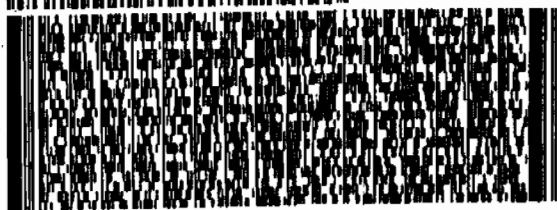

FedEx
Express



1 of 2
FedEx
TRK# 7209 7850 2385
0201

FRI - 26FEB
FRI - 26 FEB A1
PRIORITY OVERNIGHT

29407

XX CHSA

ORIGIN ID: SAFA (505) 665-9968
JOYLENE VALDEZ
LOS ALAMOS NATL LAB.
TA00 BLDG 1237 DPU 03

LOS ALAMOS, NM 87545
UNITED STATES US


SHIP DATE: 25FEB10
ACTWGT: 58.0 LB MAN
CAD: 0014176/CAFE2450

BILL SENDER

TO VALERIE DAVIS
GENERAL ENGINEERING LAB
2040 SAVAGE RD

CHARLESTON SC 29407
(843) 556-8171
REF: 6B010AMR3A05529E00

3C

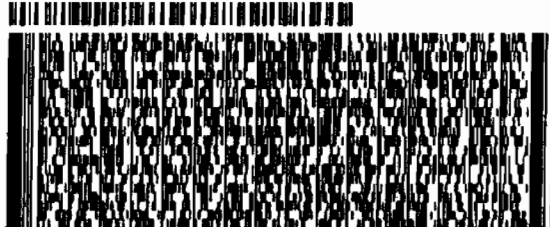

FedEx
Express




1 of 2
TRK# 7209 7850 2422
0201
MASTER

FRI - 26FEB A1
PRIORITY OVERNIGHT

29407
SC-US
CHS

XX CHSA

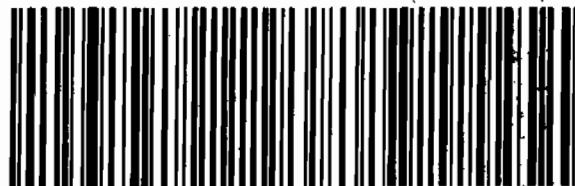

ORIGIN ID: SAFA (505) 665-9968
JOYLENE VALDEZ
LOS ALAMOS NATL LAB.
TA00 BLDG 1237 DPU 03

LOS ALAMOS, NM 87545
UNITED STATES US

SHIP DATE: 25FEB10
ACTWGT: 53.0 LB MAN
CAD: 0014176/CAFE2450

BILL SENDER

TO VALERIE DAVIS
GENERAL ENGINEERING LAB
2040 SAVAGE RD

CHARLESTON SC 29407
(843) 556-8171
REF: 6B010AMR3A05529E00

6



FedEx
Express



FRI - 26FEB
FRI - 26 FEB A1
PRIORITY OVERNIGHT

A1
PRIORITY OVERNIGHT

29407
SC-US
CHS

XX CHSA

ORIGIN ID: SAFA (505) 665-9968
JOYLENE VALDEZ
LOS ALAMOS NATL LAB
TA00 BLDG 1237 DPU 03

LOS ALAMOS, NM 87545
UNITED STATES US

SHIP DATE: 25FEB10
ACTWGT: 54.0 LB MAN
CAD: 0014176/CAFE2450

BILL SENDER

ORIGIN ID: SAFA (505) 665-9968
JOYLENE VALDEZ
LOS ALAMOS NATL LAB
TA00 BLDG 1237 DPU 03

LOS ALAMOS, NM 87545
UNITED STATES US

SHIP DATE: 25FEB10
ACTWGT: 45.0 LB MAN
CAD: 0014176/CAFE2450

BILL SENDER

TO VALERIE DAVIS
GENERAL ENGINEERING LAB
2040 SAVAGE RD

CHARLESTON SC 29407

(843) 556-8171



REF: 6B010AMR3A05529E00

TO VALERIE DAVIS
GENERAL ENGINEERING LAB
2040 SAVAGE RD

CHARLESTON SC 29407



(843) 556-8171

REF: 6B010AMR3A05529E00

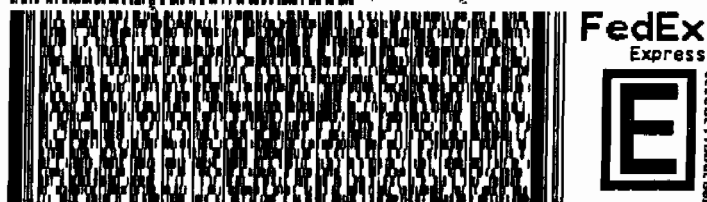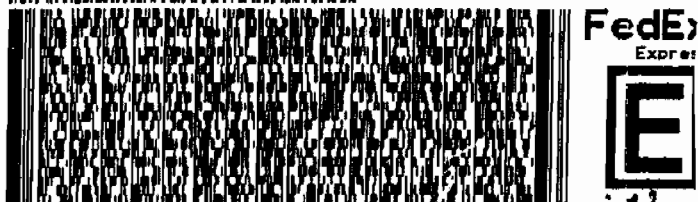

1 of 2 FRI - 26FEB A1
TRKH 7209 7850 2400
0201
MM MASTER MM
XX CHSA
29407
SC-U
CHS

3 of 3 FRI - 26FEB A1
MPSH 7209 7850 2477
0263
MstrM 7209 7850 2455 0201
29407
SC-US
CHS

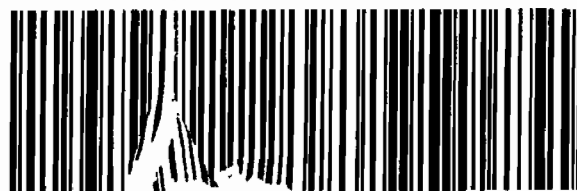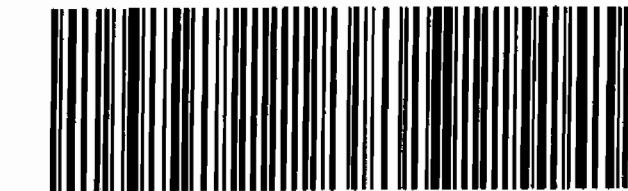

ORIGIN ID: SAFA (505)
JOYLENE VALDEZ
LOS ALAMOS NATL LAB
TA00 BLDG 1237 DPU 03

LOS ALAMOS, NM 87545
UNITED STATES US

ACTWGT: 53.0 LB MAN
CAD: 0014176/CAFE2450

BILL SENDER

ORIGIN ID: SAFA (505)
JOYLENE VALDEZ
LOS ALAMOS NATL LAB
TA00 BLDG 1237 DPU 03

LOS ALAMOS, NM 87545
UNITED STATES US

ACTWGT: 45.0 LB MAN
CAD: 0014176/CAFE2450

BILL SENDER

TO VALERIE DAVIS
GENERAL ENGINEERING LAB
2040 SAVAGE RD

CHARLESTON SC 29407

(843) 556-8171


REF: 6B010AMR3A05529E00

TO VALERIE DAVIS
GENERAL ENGINEERING LAB
2040 SAVAGE RD

CHARLESTON SC 29407

(843) 556-8171

REF: 6B010AMR2A0515BYDO

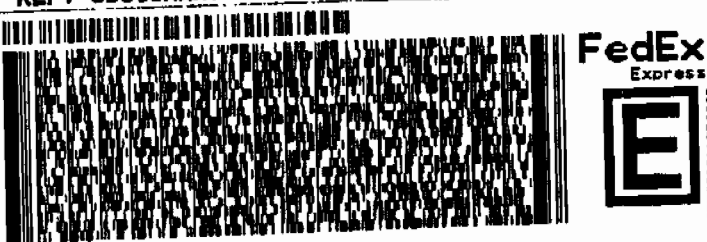

2 of 2 FRI - 26FEB A1
MPSH 7209 7850 2433
0263
MstrM 7209 7850 2422 0201
XX CHSA
29407
SC-US
CHS

2 of 3 FRI - 26FEB A1
MPSH 7209 7850 2260
0263
MstrM 7209 7850 2250 0201
XX CHSA
29407
SC-US
CHS



ORIGIN ID: SAFA (505) 665-9968
JOYLENE VALDEZ
LOS ALAMOS NATL LAB
TA00 BLDG 1237 DPU 03
LOS ALAMOS, NM 87545
UNITED STATES US

SHIP DATE: 25FEB10
ACTWGT: 59.0 LB MAN
CAD: 0014176/CAFE2450


BILL SENDER

TO VALERIE DAVIS
GENERAL ENGINEERING LAB
2040 SAVAGE RD

CHARLESTON SC 29407

(843) 656-8171
REF: 6B010AMR3A022DXL00

0014176/CAFE2450

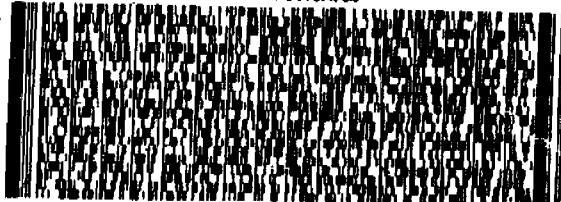

FedEx
Express




J09280911302271

2 of 2
MPS# 0263 7209 7850 2352
Mstr# 7209 7850 2341 0201

FRI - 26FEB A1
PRIORITY OVERNIGHT

XX CHSA

29407
SC-US
CHS

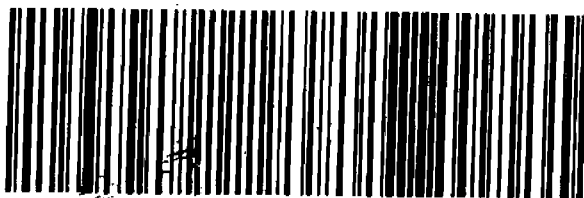

LOS ALAMOS NATL LAB
TA00 BLDG 1237 DPU 03
LOS ALAMOS, NM 87545
UNITED STATES US

CAD: 0014176/CAFE2450


BILL SENDER

TO VALERIE DAVIS
GENERAL ENGINEERING LAB
2040 SAVAGE RD

CHARLESTON SC 29407

(843) 656-8171
REF: 6B010AMR2A0515BYDO

0014176/CAFE2450

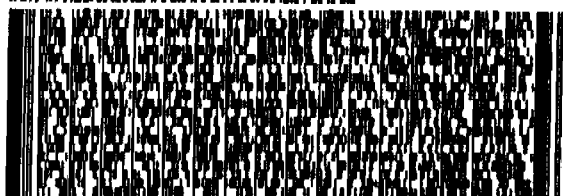

FedEx
Express



J09280911302271

1 of 2
TRK# 0201 7209 7850 2282
NN MASTER NN

FRI - 26FEB A1
PRIORITY OVERNIGHT

XX CHSA

29407
SC-US
CHS

ORIGIN ID: SAFA (505) 665-9968
JOYLENE VALDEZ
LOS ALAMOS NATL LAB
TA00 BLDG 1237 DPU 03
LOS ALAMOS, NM 87545
UNITED STATES US

SHIP DATE: 25FEB10
ACTWGT: 60.0 LB MAN
CAD: 0014176/CAFE2450


BILL SENDER

TO VALERIE DAVIS
GENERAL ENGINEERING LAB
2040 SAVAGE RD

CHARLESTON SC 29407

(843) 656-8171
REF: 6B010AMR2A0515BYDO

0014176/CAFE2450

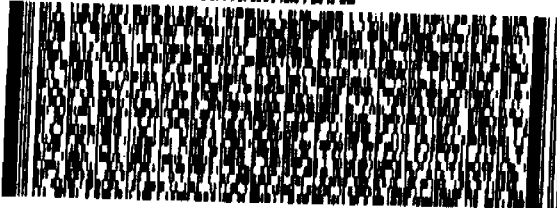

FedEx
Express




J09280911302271

3 of 3
MPS# 0263 7209 7850 2271
Mstr# 7209 7850 2250 0201

FRI - 26FEB A1
PRIORITY OVERNIGHT

XX CHSA

29407
SC-US
CHS

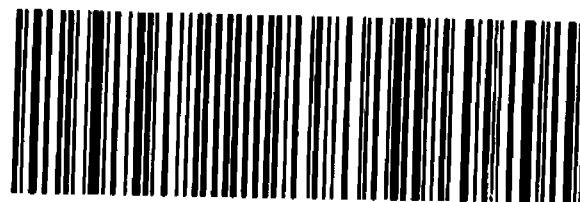

ORIGIN ID: SAFA (505) 665-9968
JOYLENE VALDEZ
LOS ALAMOS NATL LAB
TA00 BLDG 1237 DPU 03
LOS ALAMOS, NM 87545
UNITED STATES US

SHIP DATE: 25FEB10
ACTWGT: 58.0 LB MAN
CAD: 0014176/CAFE2450


BILL SENDER

TO VALERIE DAVIS
GENERAL ENGINEERING LAB
2040 SAVAGE RD

CHARLESTON SC 29407

(843) 656-8171
REF: 6B010AMR3A05529E00

0014176/CAFE2450

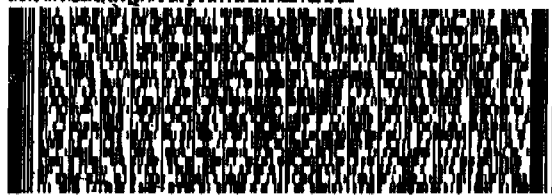

FedEx
Express



J09280911302271

2 of 3
MPS# 0263 7209 7850 2466
Mstr# 7209 7850 2455 0201

FRI - 26FEB A1
PRIORITY OVERNIGHT

XX CHSA

29407
SC-US
CHS


ORIGIN ID: SAFA (505) 665-9968
JOYLENE VALDEZ
LOS ALAMOS NATL LAB
TA00 BLDG 1237 DPU 03
LOS ALAMOS, NM 87545
UNITED STATES US

SHIP DATE: 25FEB10
ACTWGT: 40.0 LB MAN
CAD: 0014176/CAFE2450
BILL SENDER

TO VALERIE DAVIS
GENERAL ENGINEERING LAB
2040 SAVAGE RD

CHARLESTON SC 29407
(843) 556-8171
REF: 6B010AMR2A0515BYDO

|||||

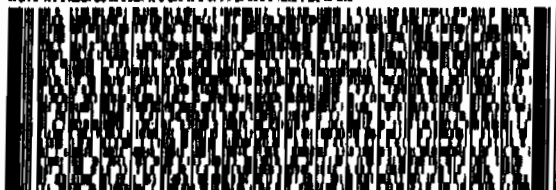

FedEx
Express




J0829081130223

2 of 2
NPS# 7209 7850 2293
0263
Mstr# 7209 7850 2282 0201

FRI - 26FEB A1
PRIORITY OVERNIGHT

XX CHSA

29407
SC-US
CHS

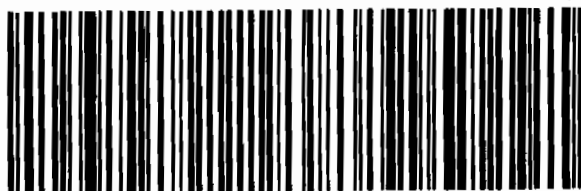

Data Review Qualifier Flag Definition Sheet

Data Review Qualifier Definitions

Qualifier	Explanation
-----------	-------------

*	A quality control analyte recovery is outside of specified acceptance criteria
**	Analyte is a surrogate compound
<	Result is less than value reported
>	Result is greater than value reported
^	RPD of sample and duplicate evaluated using +/-RL. Concentrations are <5X the RL
A	The TIC is a suspected aldol-condensation product
B	Target analyte was detected in the associated blank
B	Metals-Either presence of analyte detected in the associated blank, or MDL/IDL < sample value < PQL
BD	Results are either below the MDC or tracer recovery is low
C	Analyte has been confirmed by GC/MS analysis
D	Results are reported from a diluted aliquot of the sample
d	5-day BOD-The 2:1 depletion requirement was not met for this sample
E	Organics-Concentration of the target analyte exceeds the instrument calibration range
E	Metals-%difference of sample and SD is >10%. Sample concentration must meet flagging criteria
H	Analytical holding time was exceeded
h	Preparation or preservation holding time was exceeded
J	Value is estimated
N	Metals-The Matrix spike sample recovery is not within specified control limits
N	Organics-Presumptive evidence based on mass spectral library search to make a tentative identification of the analyte (TIC). Quantitation is based on nearest internal standard response factor
N/A	Spike recovery limits do not apply. Sample concentration exceeds spike concentration by 4X or more
ND	Analyte concentration is not detected above the reporting limit
UI	Gamma Spectroscopy-Uncertain identification
X	Consult Case Narrative, Data Summary package, or Project Manager concerning this qualifier
Y	QC Samples were not spiked with this compound
Z	Paint Filter Test-Particulates passed through the filter, however no free liquids were observed.

LC/MS/MS PERCHLORATE ANALYSIS

**Perchlorate by LC/MSMS
Los Alamos National Laboratory (LANL)
SDG 10-2093**

Method/Analysis Information

Procedure: **Definitive Low Level Perchlorate Analysis Utilizing Liquid Chromatography/Mass Spectrometry/Mass Spectrometry (LC/MS/MS) by EPA Method 6850 Modified (6850M)**

Analytical Method: SW846 6850 Modified

Prep Method: SW846 6850 Modified

Analytical Batch Number: 959047

Prep Batch Number: 959046

Sample Analysis

Sample ID	Client ID
248117001	RE36-10-8458
1202056719	Interference Check Sample (ICS)
1202056715	Method Blank (MB)
1202056716	Laboratory Control Sample (LCS)
1202056717	248162002(RE46-10-13209) Matrix Spike (MS)
1202056718	248162002(RE46-10-13209) Matrix Spike Duplicate (MSD)

The samples in this SDG were analyzed on an "as received" basis.

Preparation/Analytical Method Verification

SOP Reference

Procedure for preparation, analysis and reporting of analytical data are controlled by GEL Laboratories LLC as Standard Operating Procedure (SOP). The data discussed in this narrative has been analyzed in accordance with GL-OA-E-067 REV# 6.

Calibration Information

Initial Calibration

All initial calibration requirements have been met for this SDG. Due to software constraints, all Initial Calibration Blanks must be designated as IPB001.

10-2093-PERLCMS

Page 1 of 4

CCV Requirements

All associated calibration verification standard(s) (ICV or CCV) met the acceptance criteria.

CCB Requirements

All continuing calibration blanks (CCB) bracketing the analyses associated with this batch were within acceptance criteria.

CCV Requirements

All continuing calibration checks (CCV) requirements were met by all bracketing CCV standards.

Low Level Standard (CRI) Requirements

All low level calibration verification (CRI) requirements were met by all bracketing CRI standards.

Quality Control (QC) Information**Method Blank (MB) Statement**

The MB(s) analyzed with this SDG met the acceptance criteria.

Interference Check Sample (ICS)

The interference check sample (ICS) met all recovery acceptance criteria.

Laboratory Control Sample (LCS) Recovery

The LCS spike recoveries met the acceptance limits.

QC Sample Designation

Client sample 248162002 (RE46-10-13209) from SDG 10-2103 was chosen for matrix spike and matrix spike duplicate analysis. Please see the raw data in the Miscellaneous Section.

Matrix Spike (MS) Recovery Statement

The MS recoveries were within the established acceptance limits.

Matrix Spike Duplicate (MSD) Recovery Statement

The MSD recoveries were within the established acceptance limits.

MS/MSD Relative Percent Difference (RPD) Statement

The RPD(s) between the MS and MSD met the acceptance limits.

Retention Time Standard Area Acceptance

The retention time standard areas were within the required acceptance criteria for all samples and QC.

Retention Time

During the analysis of Perchlorate by LC/MS/MS, retention time shifts are commonly observed. These retention time shifts, which are caused by fouling of the column by the sample matrices, are problematic when the retention time is used as one of the criterion for confirmation. To overcome this problem, a known amount of O(18) labeled Perchlorate was added to each sample as a retention time standard. The presence of Perchlorate was confirmed by the relative retention time (RRT) of the Perchlorate peak and the O(18) standard. A RRT window of 0.98 to 1.02, as required by Method 332.0, has been used. In addition to the isotopic ratio, the presence of Perchlorate in the samples associated with this data package have been confirmed using the relative retention criteria stated above, not the absolute retention time.

10-2093-PERLCMS

Page 2 of 4

Technical Information

Holding Time Specifications

All samples in this SDG in this analytical batch met the specified holding time. GEL assigns holding times based on the associated methodology, which assigns the date and time from sample collection of sample receipt. Those holding times expressed in hours are calculated in the AlphaLIMS system. Those holding times expressed as days expire at midnight on the day of expiration.

Preparation/Analytical Method Verification

All procedures were performed as stated in the SOP.

Sample Dilutions

The samples in this SDG did not require dilutions.

Sample Re-extraction/Re-analysis

Re-extractions or re-analyses were not required in this SDG except for dilutions.

Miscellaneous Information

Data Exception (DER) Documentation

Data exception reports (DERs) are generated to document procedural anomalies that may deviate from referenced SOP or contractual documents. A data exception report (DER) was not generated for this SDG.

Manual Integrations

Some initial calibration standards, continuing calibration standards, and/or samples may require manual integrations due to software limitations.

Method Comments

The sample in this SDG was not originally analyzed using EPA Method 314.0.

Additional Comments

The Perchlorate Isotope Ratio on the Form I may differ slightly from the ratio on the corresponding raw data due to rounding rules and/or significant figures or due to software limitations when there are manual integrations, dilutions or other factors. The ratio value of the Form I is the correct value.

The retention time marker, Perchlorate-O (18), is added to all samples, instrument blanks, and standards prior to injection. It is used to verify the retention time of Perchlorate and Perchlorate-101 and to insure an accurate injection occurred. Due to various anions affecting the recovery of Perchlorate-O (18) and not Perchlorate and Perchlorate-101, the calibration curves of Perchlorate and Perchlorate-101 are not internally corrected for using Perchlorate-O (18). They are external calibrations.

Perchlorate Isotope Ratio

The Perchlorate isotope ratio met acceptance criteria for all samples and QC samples. Please see the isotope ratio criteria in the Miscellaneous Section.

System Configuration

The laboratory utilizes a Waters LC 2795 liquid chromatography instrument for perchlorate analysis. It is coupled with either a Micromass Quattro Micro Mass Spectrometer/ Mass Spectrometer, or a Micromass Quattro Ultima Mass Spectrometer/ Mass Spectrometer. Each being designated as LCMSMS #1, and LCMSMS #2, respectively. It is fitted with an electrospray probe that is operated in the negative electrospray ionization mode for perchlorate analysis. The laboratory may also utilize an Agilent 1100 liquid chromatography instrument for perchlorate analysis. It is coupled with an Applied Biosystems 4000 Mass Spectrometer/ Mass Spectrometer, designated as LCMSMS #3 or LCMSMS #4. It is also fitted with an electrospray probe that is operated in the negative electrospray ionization mode for perchlorate analysis.

Chromatographic Columns

Chromatographic separation of perchlorate is accomplished through analysis on the following anion column:

Dionex: IonPac AG-16 2 x 50 mm.

Certification Statement

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless otherwise noted in the analytical case narrative.

Review Validation:

GEL requires all analytical data to be verified by a qualified data validator. In addition, all data designated for CLP or CLP-like packaging will receive a third level validation upon completion of the data package.

The following data validator verified the information presented in this case narrative:

Reviewer: Herbert M. Mauer Date: 03/16/10

SAMPLE DATA SUMMARY

Perchlorate Analysis Data Sheet

Lab Name: GEL Laboratories LLC

Lab Code: GEL

Instrument: LCMSMS

Method: SW846 6850 Modified

Matrix: WATER

Extraction Batch ID: 959046

Extraction Type: Filter/DAI

Client Sample No.

RE36-10-8458

Date Received: 26-FEB-10

GEL Job No (SDG): 10-2093

GEL Sample ID: 248117001

Date Filtered: 05-MAR-10

Injection Volume (uL): 20

%Solids:

Sample Volume/Weight: 10.0 mL

Concentrated Extract Volume: 10.0

CAS No.	Analyte^	MDL	RL	Conc*	Units	Q	Dilution Factor	Date Analyzed	GEL File ID
14797-73-0	Perchlorate	.05	.2	0.050	ug/L	U	1	09-MAR-10 08:24	per0308111a
	Perchlorate Isotope Ratio						1	09-MAR-10 08:24	per0308111a
14797-73-0	Perchlorate-101	.05	.2	0.050	ug/L	U	1	09-MAR-10 08:24	per0308111a
	Perchlorate-O(18)			0.452	ug/L		1	09-MAR-10 08:24	per0308111a

^ When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

*Concentration =

Instrument Value X Concentrated Extract Volume X %Solids
Aliquot

QUALITY CONTROL SUMMARY

Perchlorate Laboratory Control Sample

Lab Name: General Engineering Laboratories

Lab Code: GEL

GEL Job No. (SDG): 10-2093

Extract Batch Code: 959046

Date Filtered: 05-MAR-10

Matrix: WATER

Sample ID: 1202056716

Analyte [^]	True	Found	Units	%Rec	Q	Control Limits
Perchlorate	0.200	.187	ug/L	93.6		85 - 115
Perchlorate Isotope Ratio		3.13				-
Perchlorate-101	0.200	.197	ug/L	98.4		85 - 115
Perchlorate-O(18)		.45	ug/L			-

[^] When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

Perchlorate Interference Check Sample

Lab Name: General Engineering Laboratories

Lab Code: GEL GEL Job No. (SDG): 10-2093

Extract Batch Code: 959046 Date Filtered: 05-MAR-10

Matrix: WATER Sample ID: 1202056719

Analyte [^]	True	Found	Units	%Rec	Q	Control Limits
Perchlorate	0.200	.197	ug/L	98.5		70 -- 130
Perchlorate Isotope Ratio		3.09				
Perchlorate-101	0.200	.21	ug/L	105		70 -- 130
Perchlorate-O(18)		.463	ug/L			

[^] When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charlers W. Wilson


Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308109a
Date: 09-Mar-2010
Time: 08:06:14
ID: 1202056719
Vial: 3:1,C

03-09-10

1202056719 | 1202056719 | 1202056719

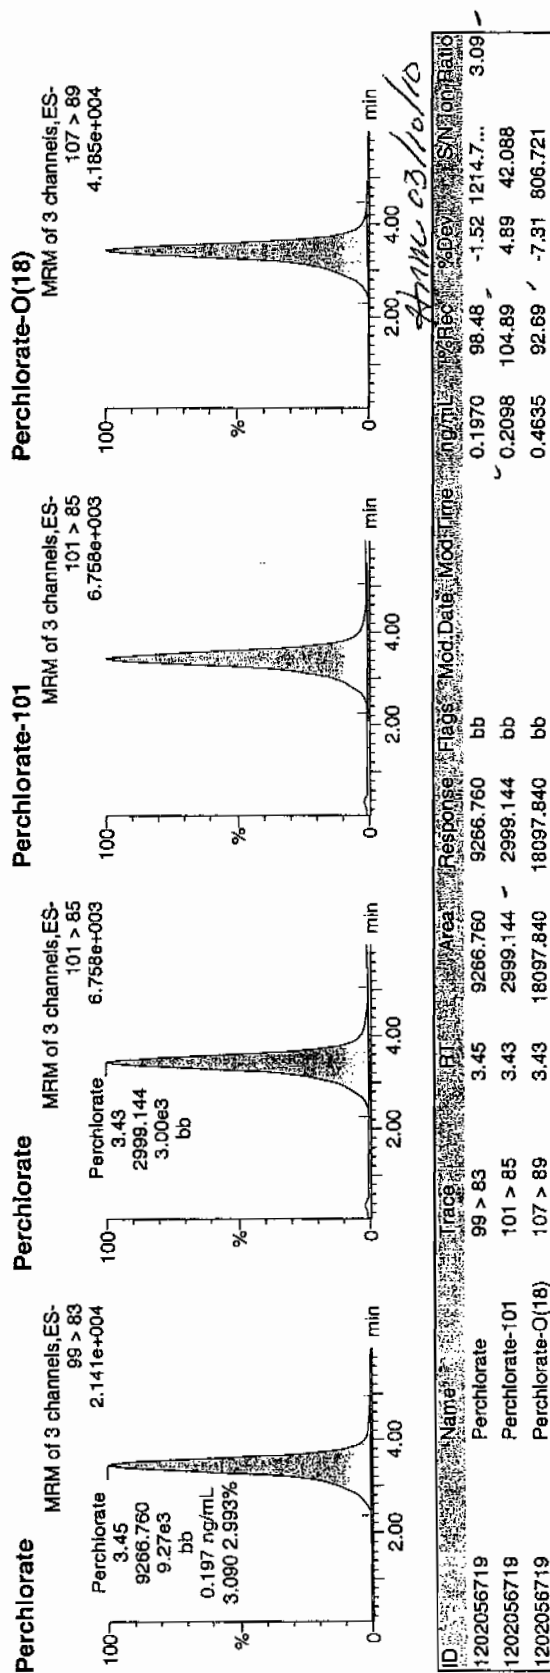

Perchlorate Spike/Spike Duplicate Summary

Lab Name: General Engineering Laboratories

Lab Code: GEL

GEL Job No (SDG): 10-2093

Extract Batch Code: 959046

Date Extracted: 05-MAR-10

GEL MS/PS ID: 1202056717

Client ID: RE46-10-13209

GEL MSD/PSD ID: 1202056718

QC Type: MS

Compound [^]	Spike Added	Sample Conc	Units	MS Conc	MS Rec	#	MSD Conc	MSD Rec	#	RPD	#	RPD Limit	Recovery Limit
Perchlorate	0.200	0.00772	ug/L	0.190	91.1		.191	91.9		.803		30	75 - 125
Perchlorate Isotope Ratio	0	0.00		3.14			3.05			0			-
Perchlorate-101	0.200	0.0102	ug/L	0.199	94.3		.207	98.3		3.87		30	75 - 125
Perchlorate-O(18)	0	0.435	ug/L	0.461			.46			.13			-

[^] When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

Comments:

Form 4

Perchlorate Initial Calibration Blank

GEL Job No.(SDG): 10-2093

Lab Name: General Engineering Laboratories

Lab Code: GEL

Reporting Units: ug/L

Analyte	True	Found	%Rec	Date Analyzed	GEL File Id	GEL Sample ID
Perchlorate	0.00	0	NA	08-MAR-10	per0308001a	IPB001
Perchlorate-101	0.00	0	NA	08-MAR-10	per0308001a	IPB001
Perchlorate	0.00	0	NA	08-MAR-10	per0308002a	IPB001
Perchlorate-101	0.00	0	NA	08-MAR-10	per0308002a	IPB001

Quantify Sample Report MassLynx 4.0-SP4
The GEL Group, LLC Analyst: Charfers W. Wilson


Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Method: C:\MassLynx\Perchlorate.PRO\MethDB\per030810a.mdb 09 Mar 2010 12:48:33
Calibration: C:\MassLynx\Perchlorate.PRO\CurveDB\per030810a.cdb 09 Mar 2010 12:48:47

Name: per0308001a
Date: 08-Mar-2010
Time: 15:44:43
D: IPB001
File: 1:1,A

03-09-10

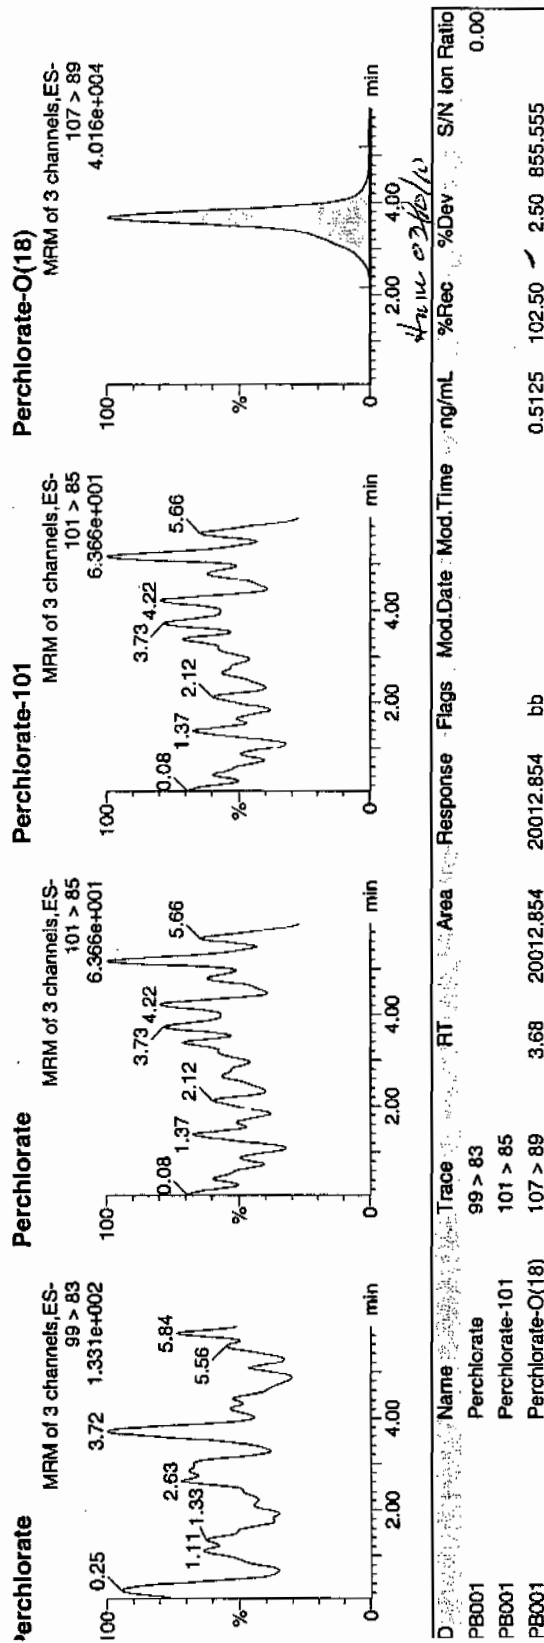


Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charles W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308002a
Date: 08-Mar-2010
Time: 15:53:45
D: IPB001
Vial: 1:1,A

03-04-10

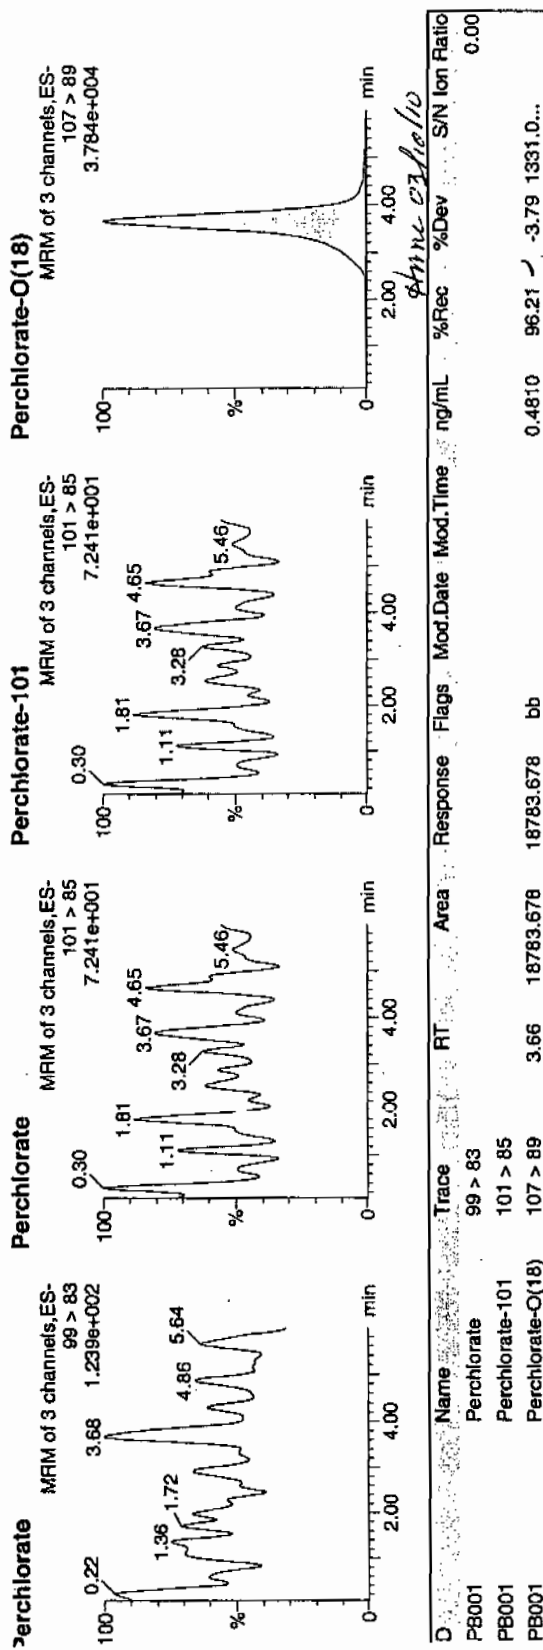

Perchlorate Continuing Calibration Blank

GEL Job No.(SDG): 10-2093

Lab Name: General Engineering Laboratories

Lab Code: GEL

Reporting Units: ug/L

Analyte	True	Found	%Rec	Date Analyzed	GEL File Id	GEL Sample ID
Perchlorate	0.00	0	NA	08-MAR-10	per0308008a	IPB002
Perchlorate-101	0.00	0	NA	08-MAR-10	per0308008a	IPB002
Perchlorate	0.00	0	NA	08-MAR-10	per0308010a	IPB003
Perchlorate-101	0.00	0	NA	08-MAR-10	per0308010a	IPB003
Perchlorate	0.00	0	NA	08-MAR-10	per0308022a	IPB004
Perchlorate-101	0.00	0	NA	08-MAR-10	per0308022a	IPB004
Perchlorate	0.00	0	NA	08-MAR-10	per0308035a	IPB005
Perchlorate-101	0.00	0	NA	08-MAR-10	per0308035a	IPB005
Perchlorate	0.00	0	NA	08-MAR-10	per0308048a	IPB006
Perchlorate-101	0.00	0	NA	08-MAR-10	per0308048a	IPB006
Perchlorate	0.00	0	NA	08-MAR-10	per0308052a	IPB007
Perchlorate-101	0.00	0	NA	08-MAR-10	per0308052a	IPB007
Perchlorate	0.00	0	NA	09-MAR-10	per0308061a	IPB008

Perchlorate Continuing Calibration Blank

Lab Name: General Engineering Laboratories GEL Job No.(SDG): 10-2093

Lab Code: GEL

Reporting Units: ug/L

Analyte	True	Found	%Rec	Date Analyzed	GEL File Id	GEL Sample ID
Perchlorate-101	0.00	0	NA	09-MAR-10	per0308061a	IPB008
Perchlorate	0.00	0	NA	09-MAR-10	per0308074a	IPB009
Perchlorate-101	0.00	0	NA	09-MAR-10	per0308074a	IPB009
Perchlorate	0.00	0	NA	09-MAR-10	per0308087a	IPB010
Perchlorate-101	0.00	0	NA	09-MAR-10	per0308087a	IPB010
Perchlorate	0.00	0	NA	09-MAR-10	per0308100a	IPB011
Perchlorate-101	0.00	0	NA	09-MAR-10	per0308100a	IPB011
Perchlorate	0.00	0	NA	09-MAR-10	per0308106a	IPB012
Perchlorate-101	0.00	0	NA	09-MAR-10	per0308106a	IPB012
Perchlorate	0.00	0	NA	09-MAR-10	per0308113a	IPB013
Perchlorate-101	0.00	0	NA	09-MAR-10	per0308113a	IPB013


Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charlers W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308008a
Date: 08-Mar-2010
Time: 16:48:15
ID: IPB002
Vial: 1:1,A

W3-01-10

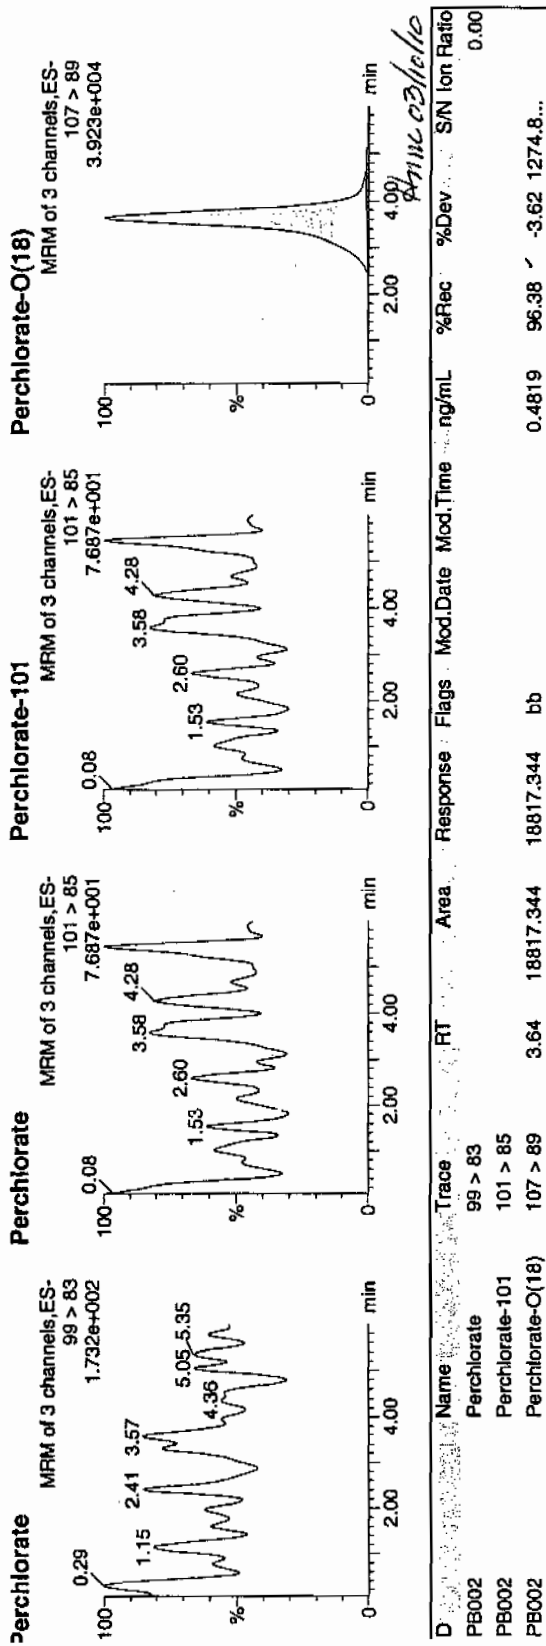

D	Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	S/N	Ion Ratio
PB002	Perchlorate	99 > 83											0.00
PB002	Perchlorate-101	101 > 85	3.64	18817.344	18817.344	bb			0.4819	96.38	-3.62	1274.8...	
PB002	Perchlorate-O(18)	107 > 89											


Quantity Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charters W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308010a
Date: 08-Mar-2010
Time: 17:06:27
ID: IPB003
Vial: 1:1,A

03-09-10

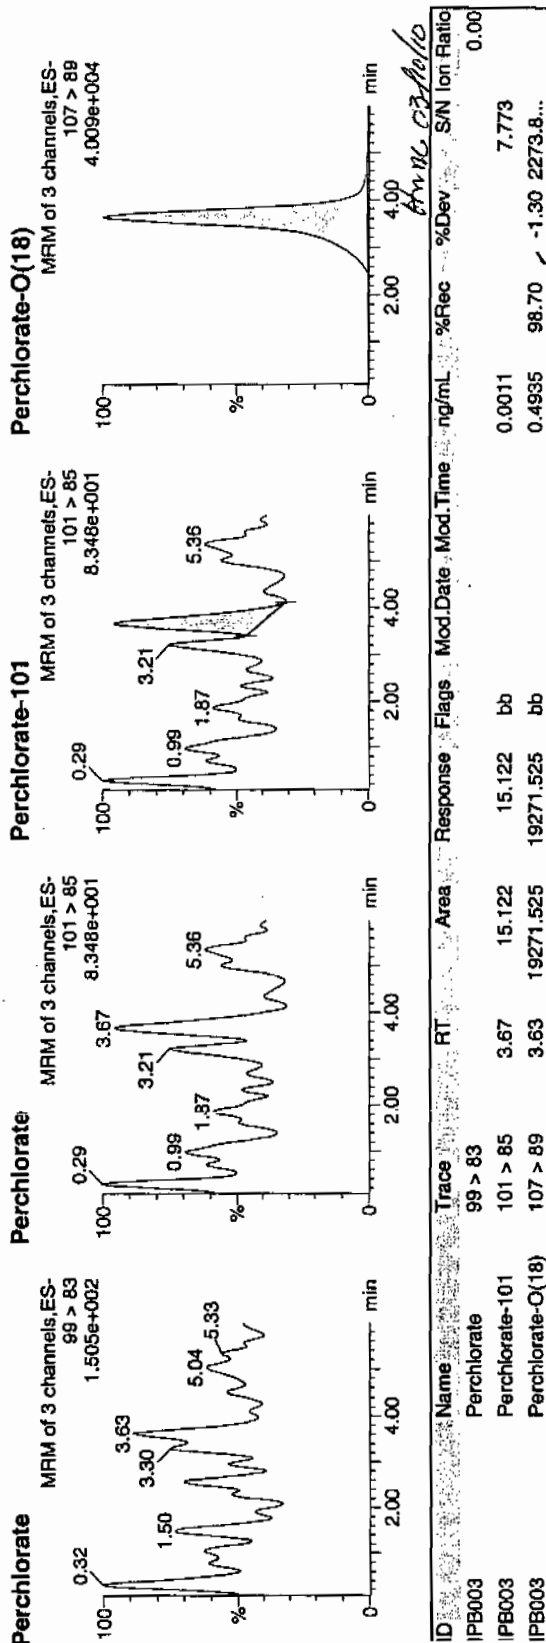


Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charters W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308022a
Date: 08-Mar-2010
Time: 18:55:24
D: IPB004
/lal: 1:1.A

03-09-10

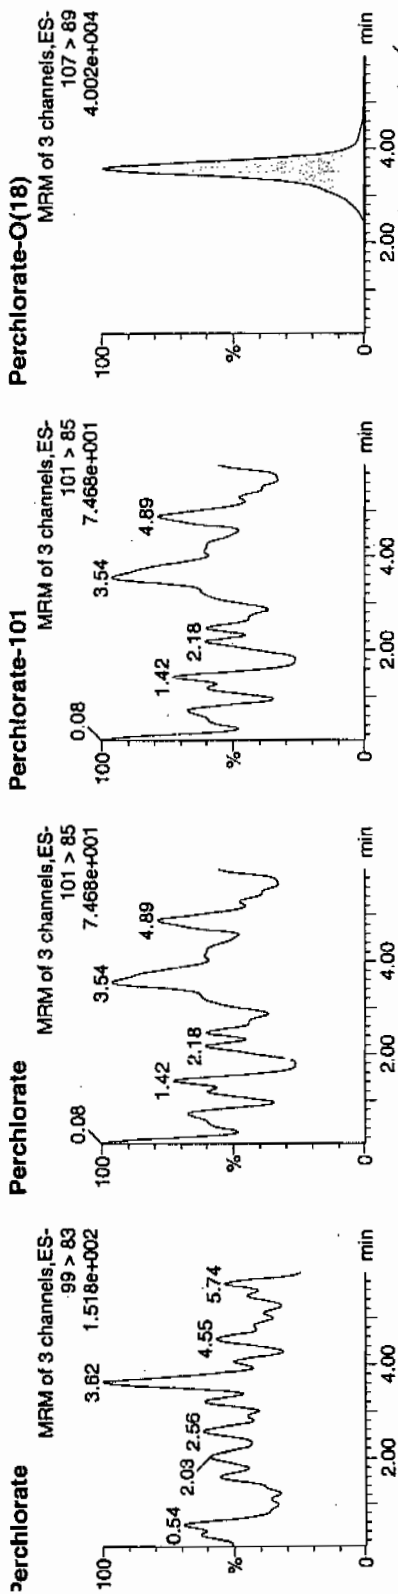

D	Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	S/N	Ion Ratio
PB004	Perchlorate	99 > 83											0.00
PB004	Perchlorate-101	101 > 85											
PB004	Perchlorate-O(18)	107 > 89	3.58	19034.945	19034.945	bb			0.4875	97.49	-2.51	1930.8...	


Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charlers W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308035a
Date: 08-Mar-2010
Time: 20:53:11
ID: IPB005
Vial: 1:1,A

0309-10

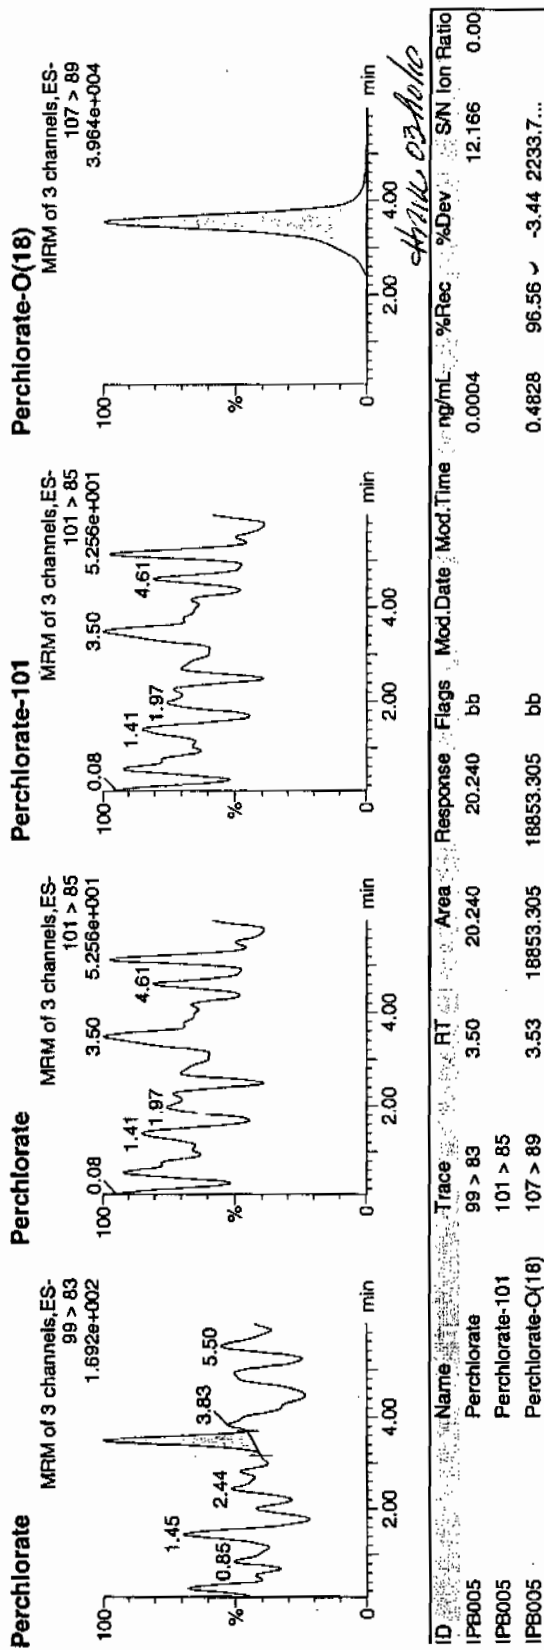

ID	Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	S/N	Ion Ratio
IPB005	Perchlorate	99 > 83	3.50	20.240	20.240	bb			0.0004			12.166	0.00
IPB005	Perchlorate-101	101 > 85											
IPB005	Perchlorate-O(18)	107 > 89	3.53	18853.305	18853.305	bb			0.4828	96.56	-3.44	2233.7...	


Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charlers W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308048a
Date: 08-Mar-2010
Time: 22:51:21
D: IPB006
Vial: 1:1,A

03-09-10

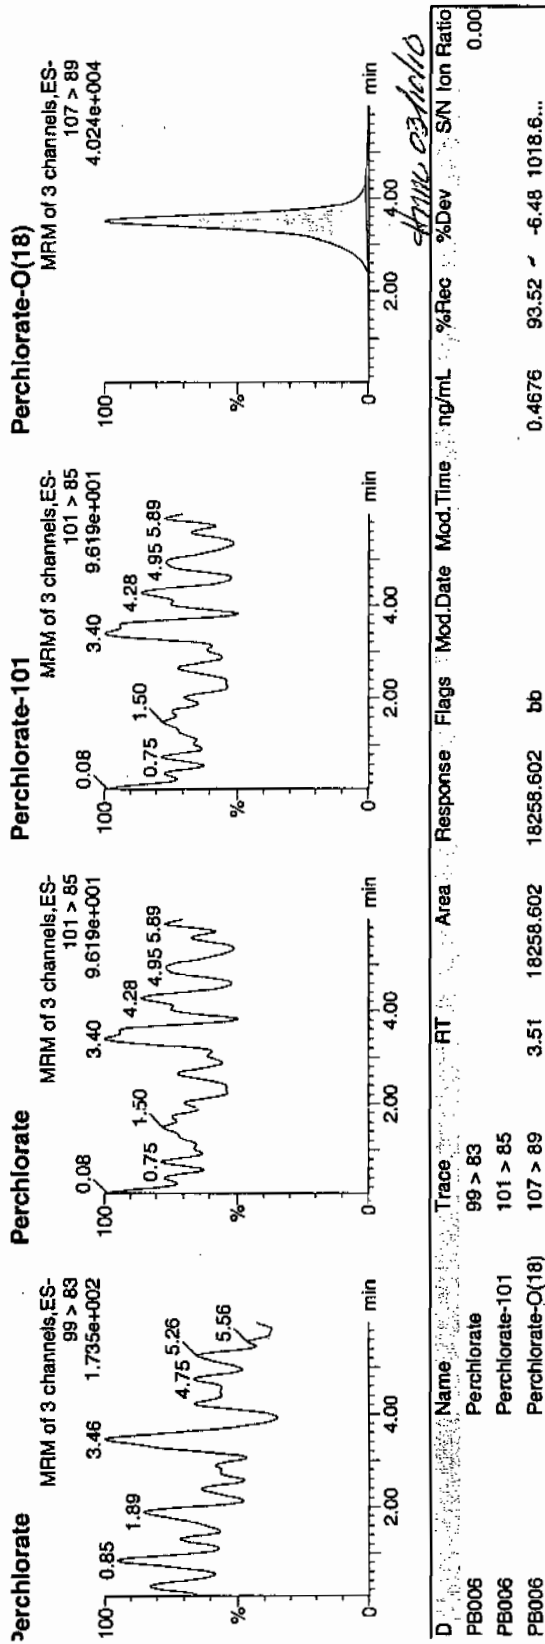

D	Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	S/N	Ion Ratio
PB006	Perchlorate	99 > 83											0.00
PB006	Perchlorate-101	101 > 85											
PB006	Perchlorate-O(18)	107 > 89	3.51	18258.602	18258.602	bb			0.4676	93.52	-6.48	1018.6...	


Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charles W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308052a
Date: 08-Mar-2010
Time: 23:27:41
D: IPB007
/fal: 1:1,A

CWJ
03-04-10

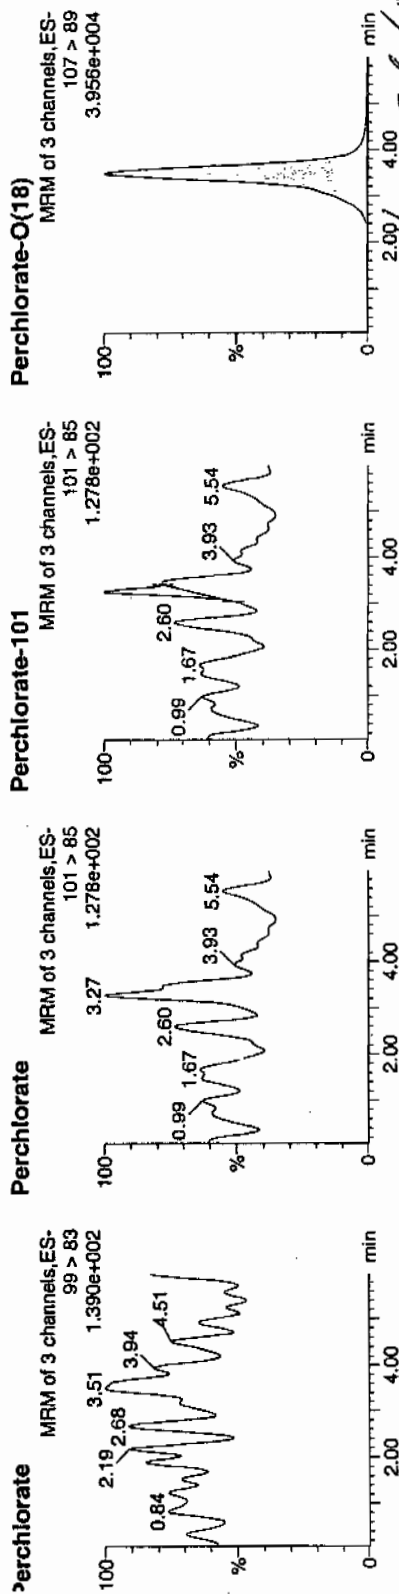

D	Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	S/N	Ion Ratio
PB007	Perchlorate	99 > 83	3.27	7.250	7.250	bb			0.0005	94.73	-5.27	11.574	0.00
PB007	Perchlorate-101	101 > 85	3.50	18495.547	18495.547	bb			0.4736			613.571	
PB007	Perchlorate-O(18)	107 > 89											


Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charliers W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308061a
Date: 09-Mar-2010
Time: 00:50:02
ID: IPB008
Vial: 1:1,A

03-09-10

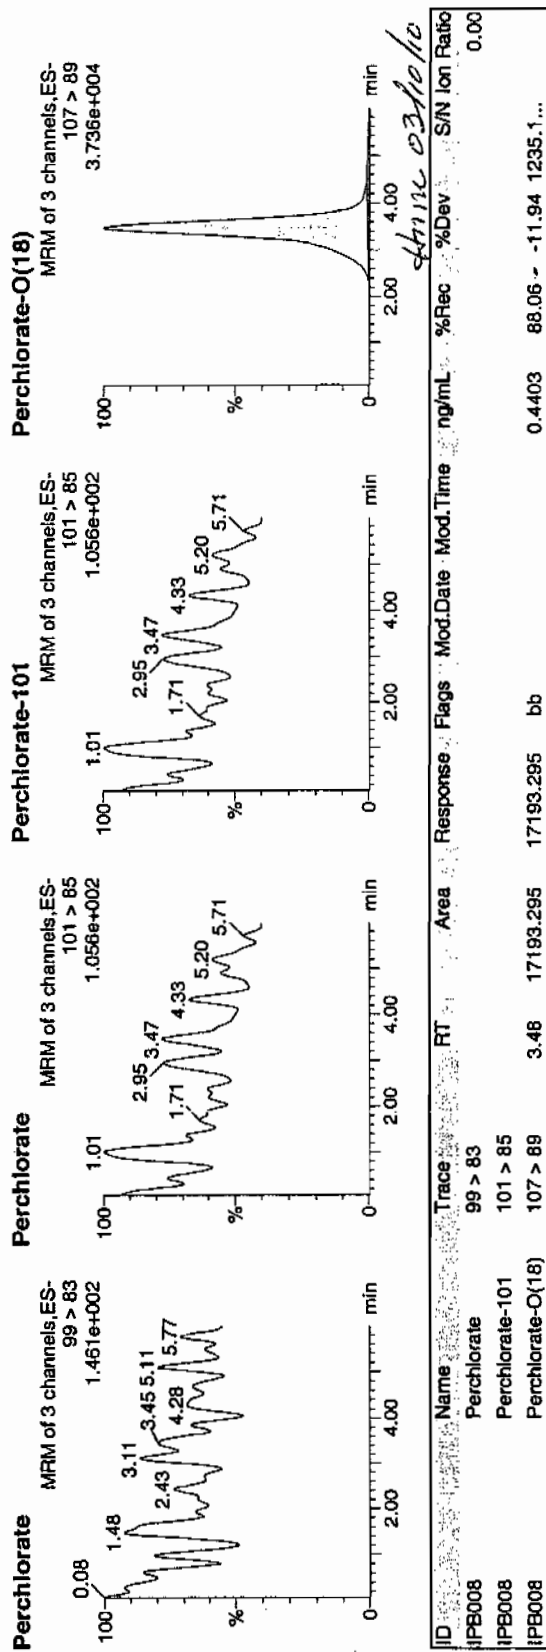


Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charles W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308074a
Date: 09-Mar-2010
Time: 02:48:02
D: IPB009
/al: 1:1,A

03-04-10

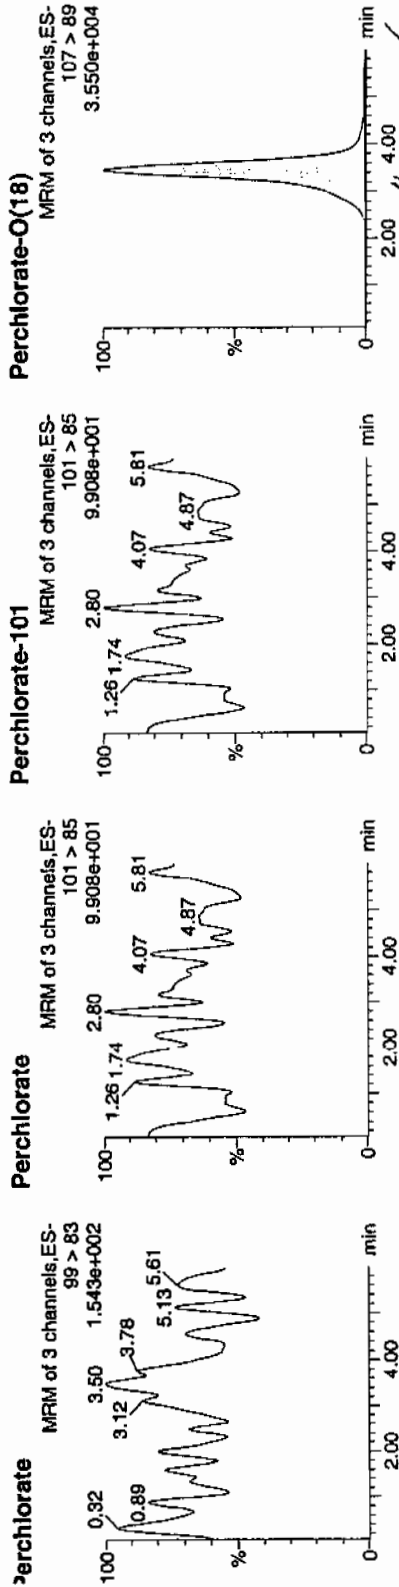

ID	Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	S/N	Ion Ratio
IPB009	Perchlorate	99 > 83											0.00
IPB009	Perchlorate-101	101 > 85	3.47	16711.643	16711.643	bb			0.4280	85.59	-14.41	2348.6...	
IPB009	Perchlorate-O(18)	107 > 89											


Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charters W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308087a
Date: 09-Mar-2010
Time: 04:46:06
ID: IPB010
Vial: 1:1,A

03 04-10

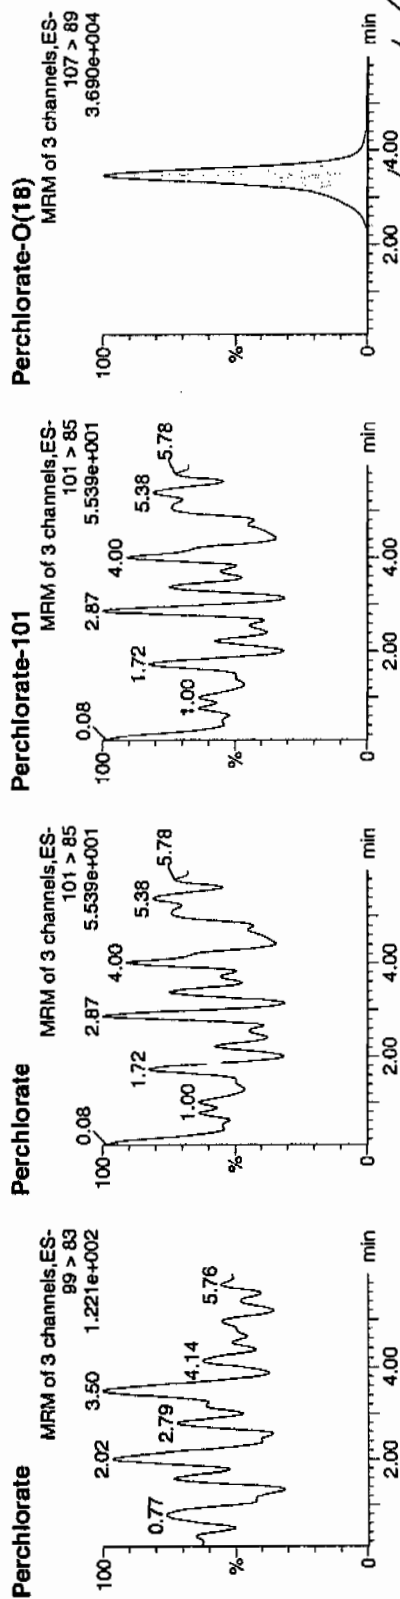

ID	Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	S/N	Ion Ratio
IPB010	Perchlorate	99 > 83											0.00
IPB010	Perchlorate-101	101 > 85	3.46	16789.424	16789.424	bb			0.4300	85.99	-14.01	1743.0...	
IPB010	Perchlorate-O(18)	107 > 89											


Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charlers W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308100a
Date: 09-Mar-2010
Time: 06:44:12
ID: IPB011
Vial: 1:1,A

03.04-10

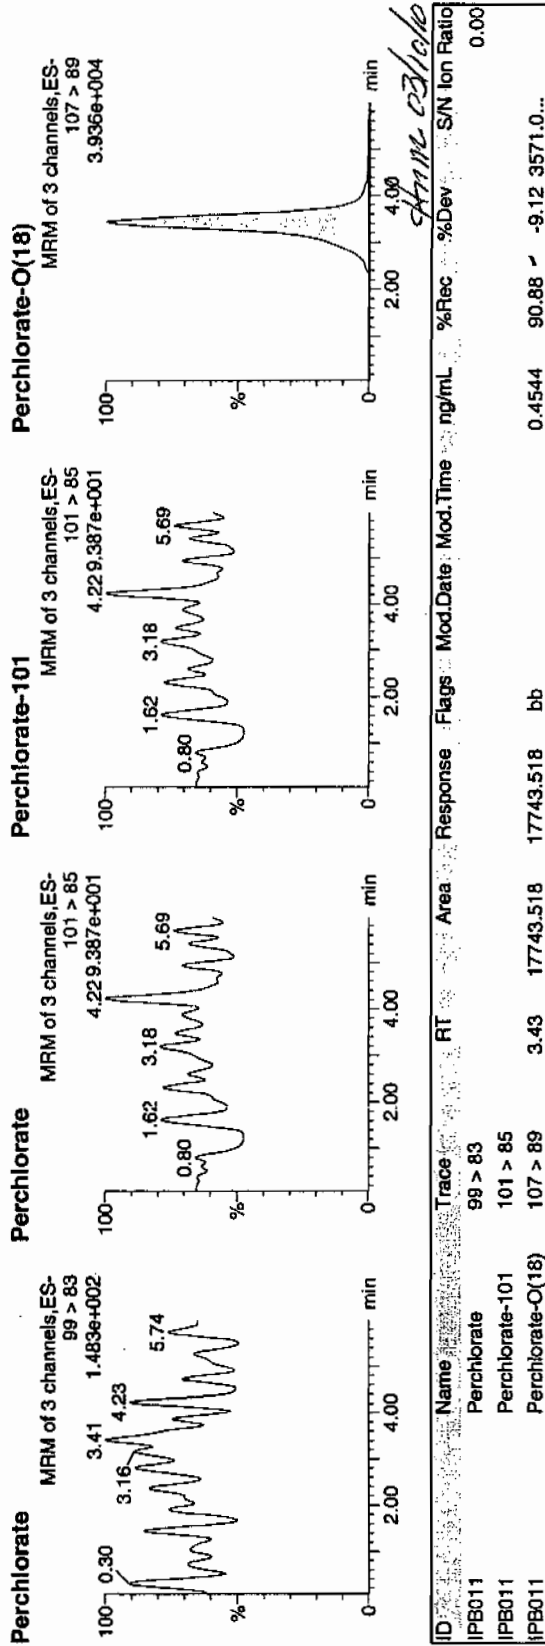

ID	Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	S/N	Ion Ratio
IPB011	Perchlorate	99 > 83											0.00
IPB011	Perchlorate-101	101 > 85	3.43	17743.518	17743.518	bb			0.4544	90.88	-	-9.12	3571.0...
IPB011	Perchlorate-O(18)	107 > 89											


Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charles W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308106a
Date: 09-Mar-2010
Time: 07:38:40
D: IPB012
Vial: 1:1,A

03-09-10

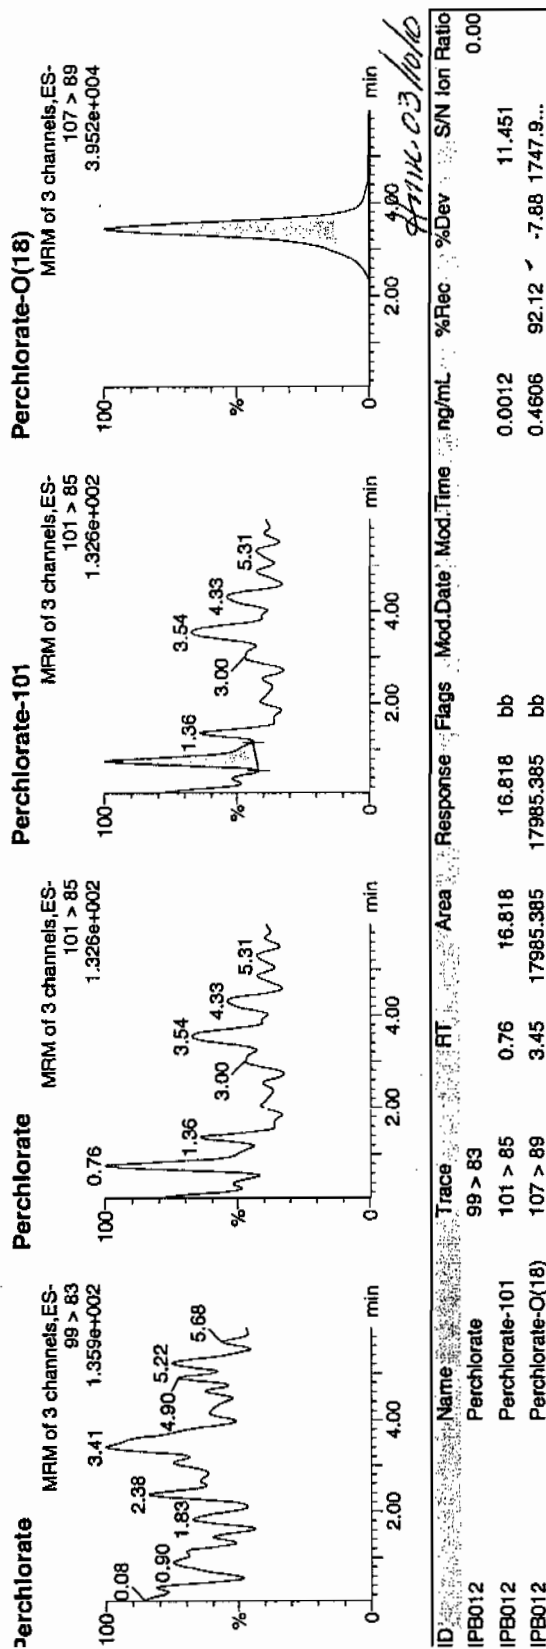


Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charlers W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308113a
Date: 09-Mar-2010
Time: 08:42:34
ID: IPB013
Vial: 1:1,A

03-04-10

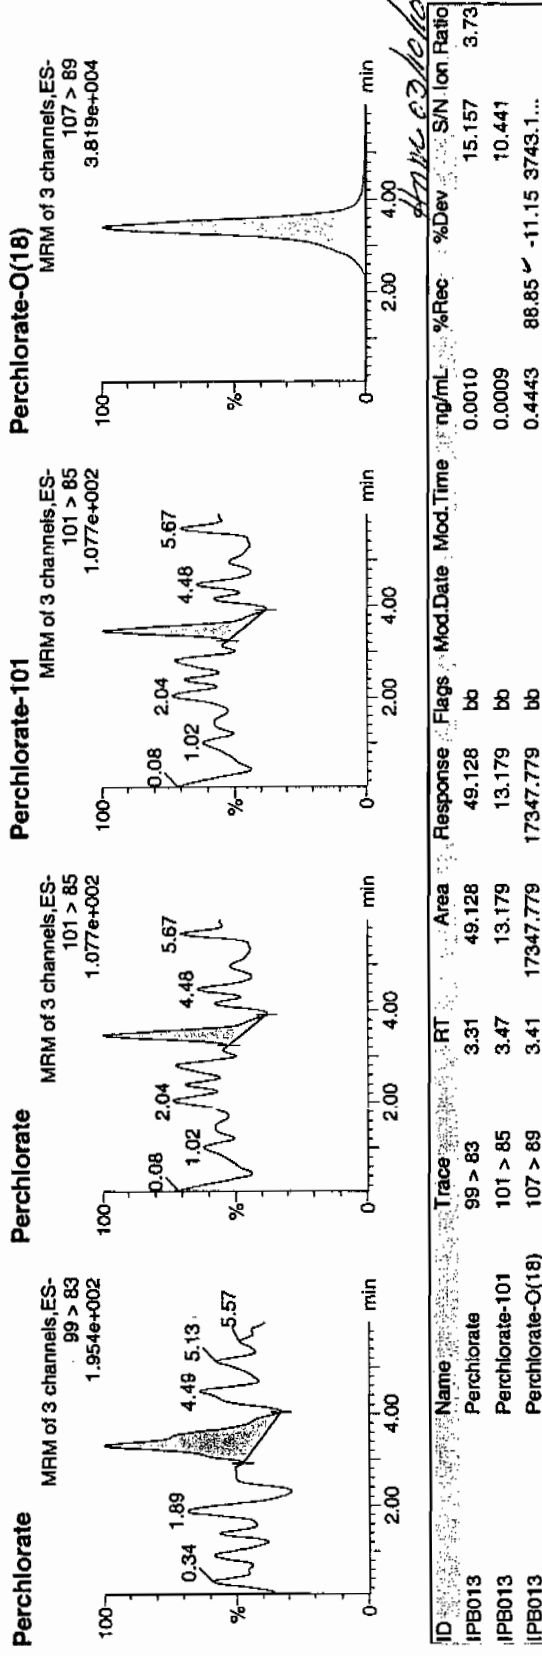

Nairb.ref

;Positive ion monoisotopic and average masses from solution
 ;of NaI/Rbi (2.0/0.05ug/ul) in 50/20 2-propanol/H2O.
 ;Most useful general purpose calibrant for all low
 ;MW applications, including MS/MS work.
 ;At high resolution, readily covers from m/z 50-2000.
 ;At reduced resolution, can be used to over m/z 3000.
 ;NOT RECOMMENDED FOR PROTEIN WORK. USE MYO, MYOTRP or TRP.
 Updated 20 April '95

22.9898	100
84.9118	100
172.8840	100
322.7782	100
472.6725	100
622.5667	100
772.4610	100
922.3552	100
1072.2494	100
; 1222.1437	100
; 1372.0379	100
; 1521.9321	100
; 1671.8264	100
; 1821.7206	100
; 1971.6149	100
; 2121.5091	100
; 2271.4033	100
; 2421.2976	100
; 2571.1918	100
; 2721.0861	100
; 2870.9803	100
; 3020.8745	100
; 3170.7688	100
; 3320.6630	100
; 3470.5572	100
; 3620.4515	100
; 3770.3457	100
; 3920.2400	100


QUATRO ULTIMA: nairb_01_08_08.cal

Calibration Report - MS1 Static

Page 1 of 1

Printed: Tue Jan 08 12:19:12 2008


POINTS HIGHLIGHTED BY CURV 01-09-08

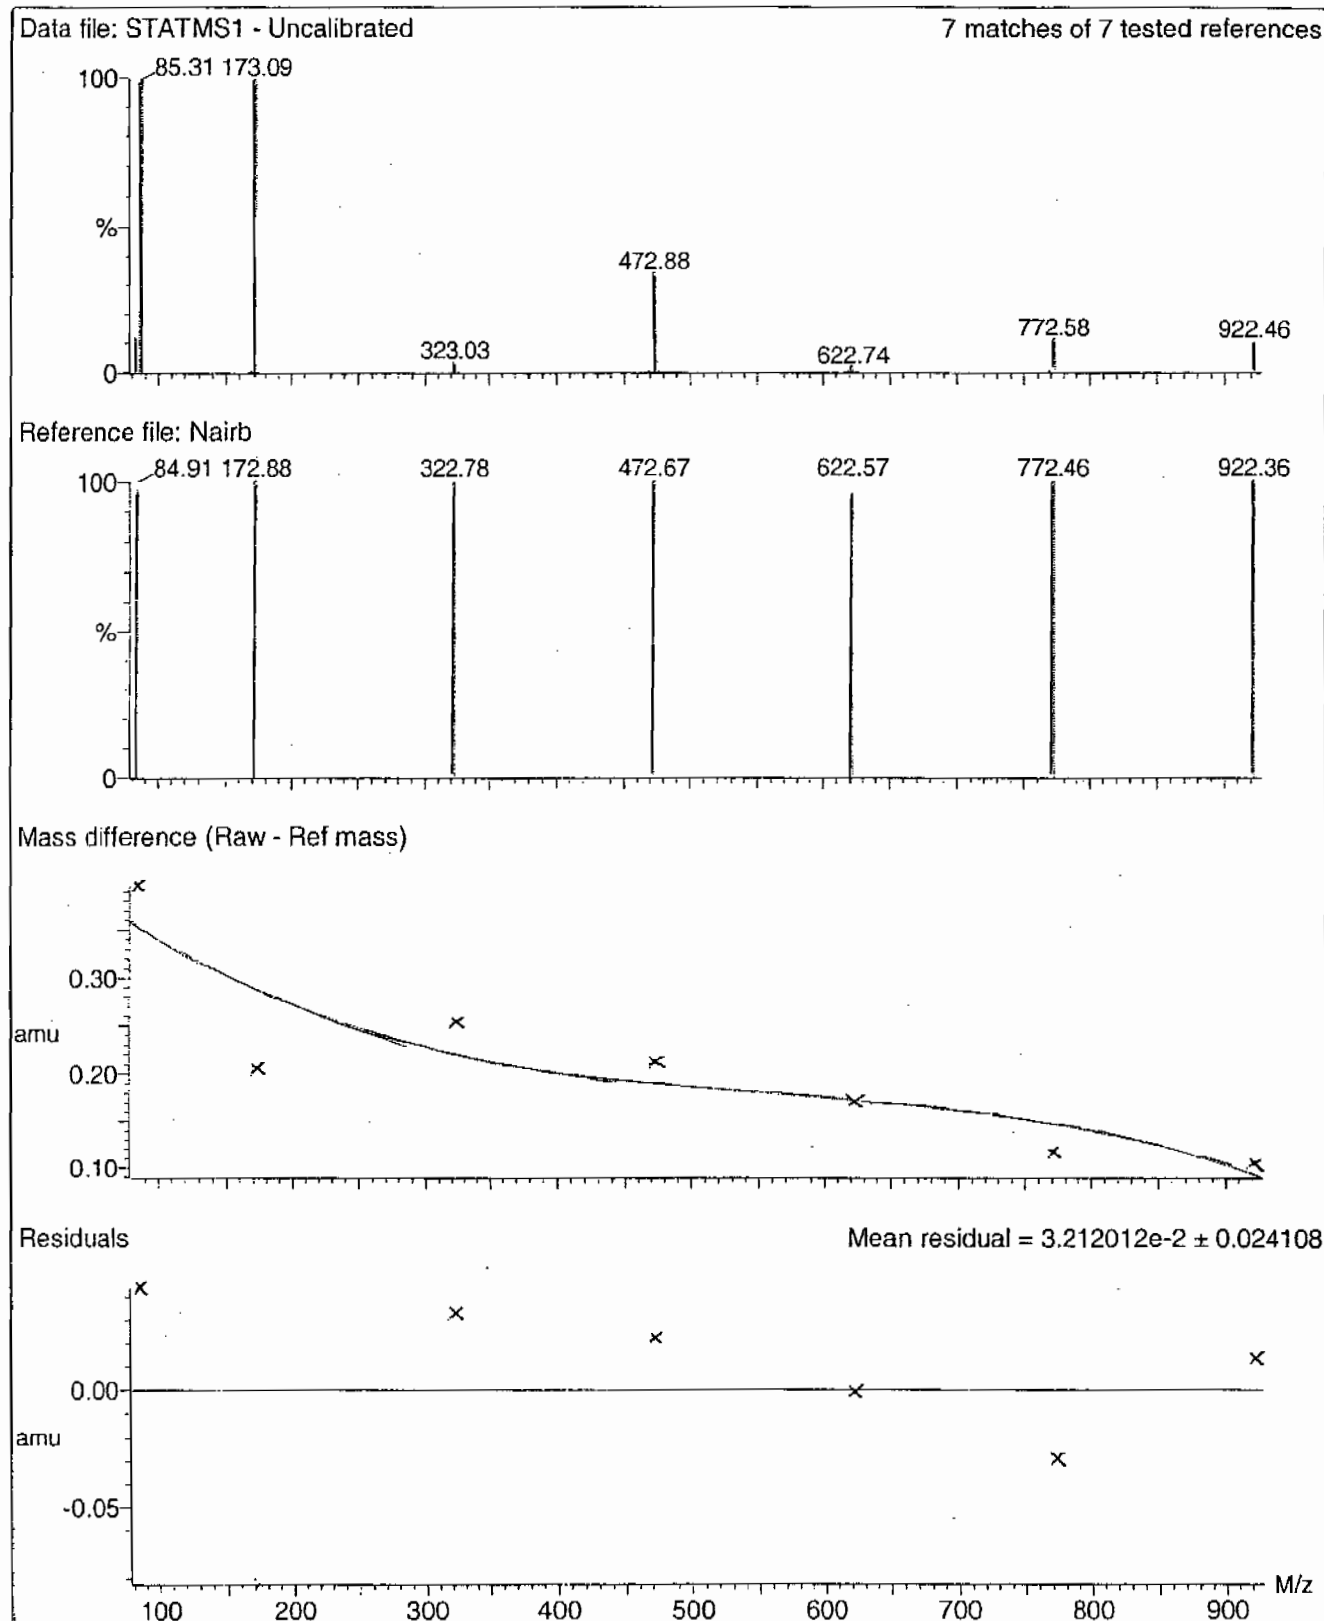

Calibration Report - MS1 Scanning

Page 1 of 1


Printed: Tue Jan 08 12:20:09 2008

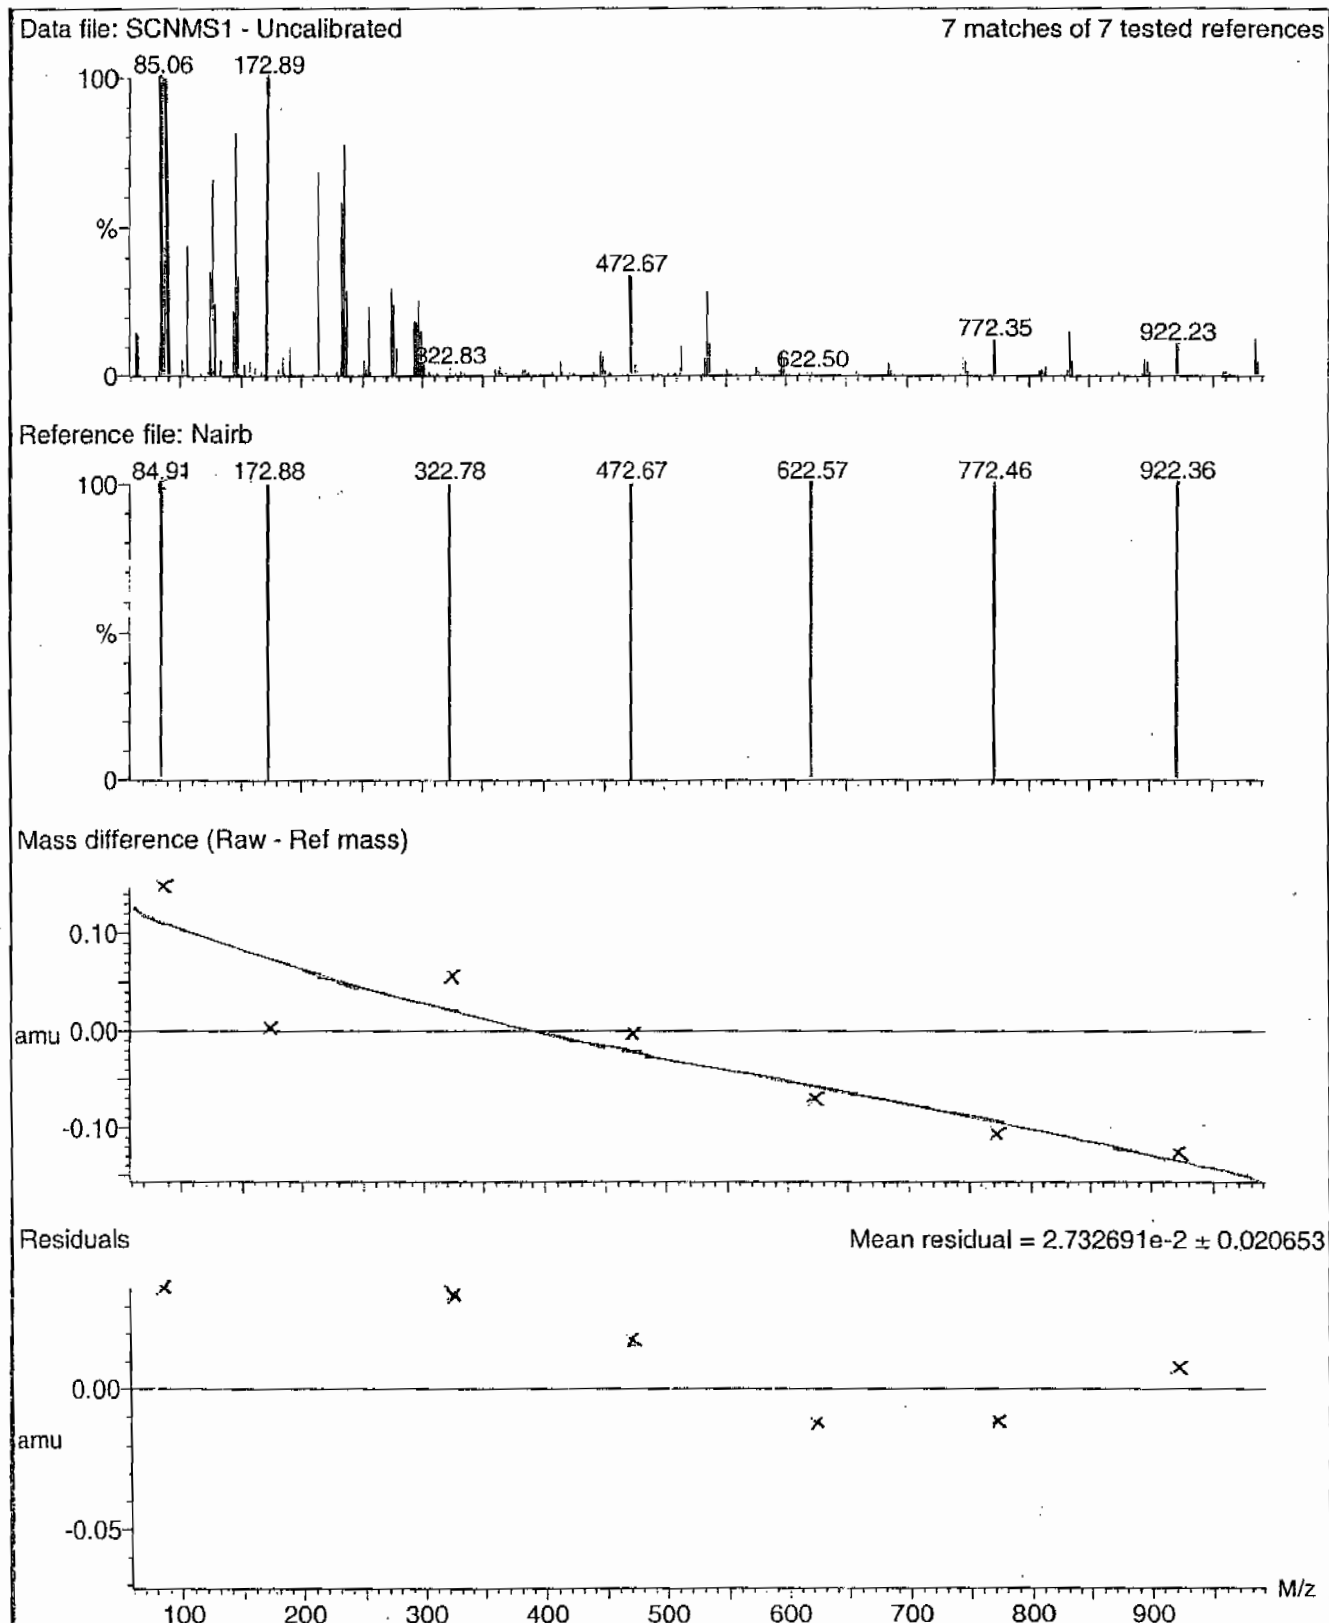

Calibration Report - MS1 Scan Speed Compensation

Page 1 of 1


Printed: Tue Jan 08 12:21:04 2008

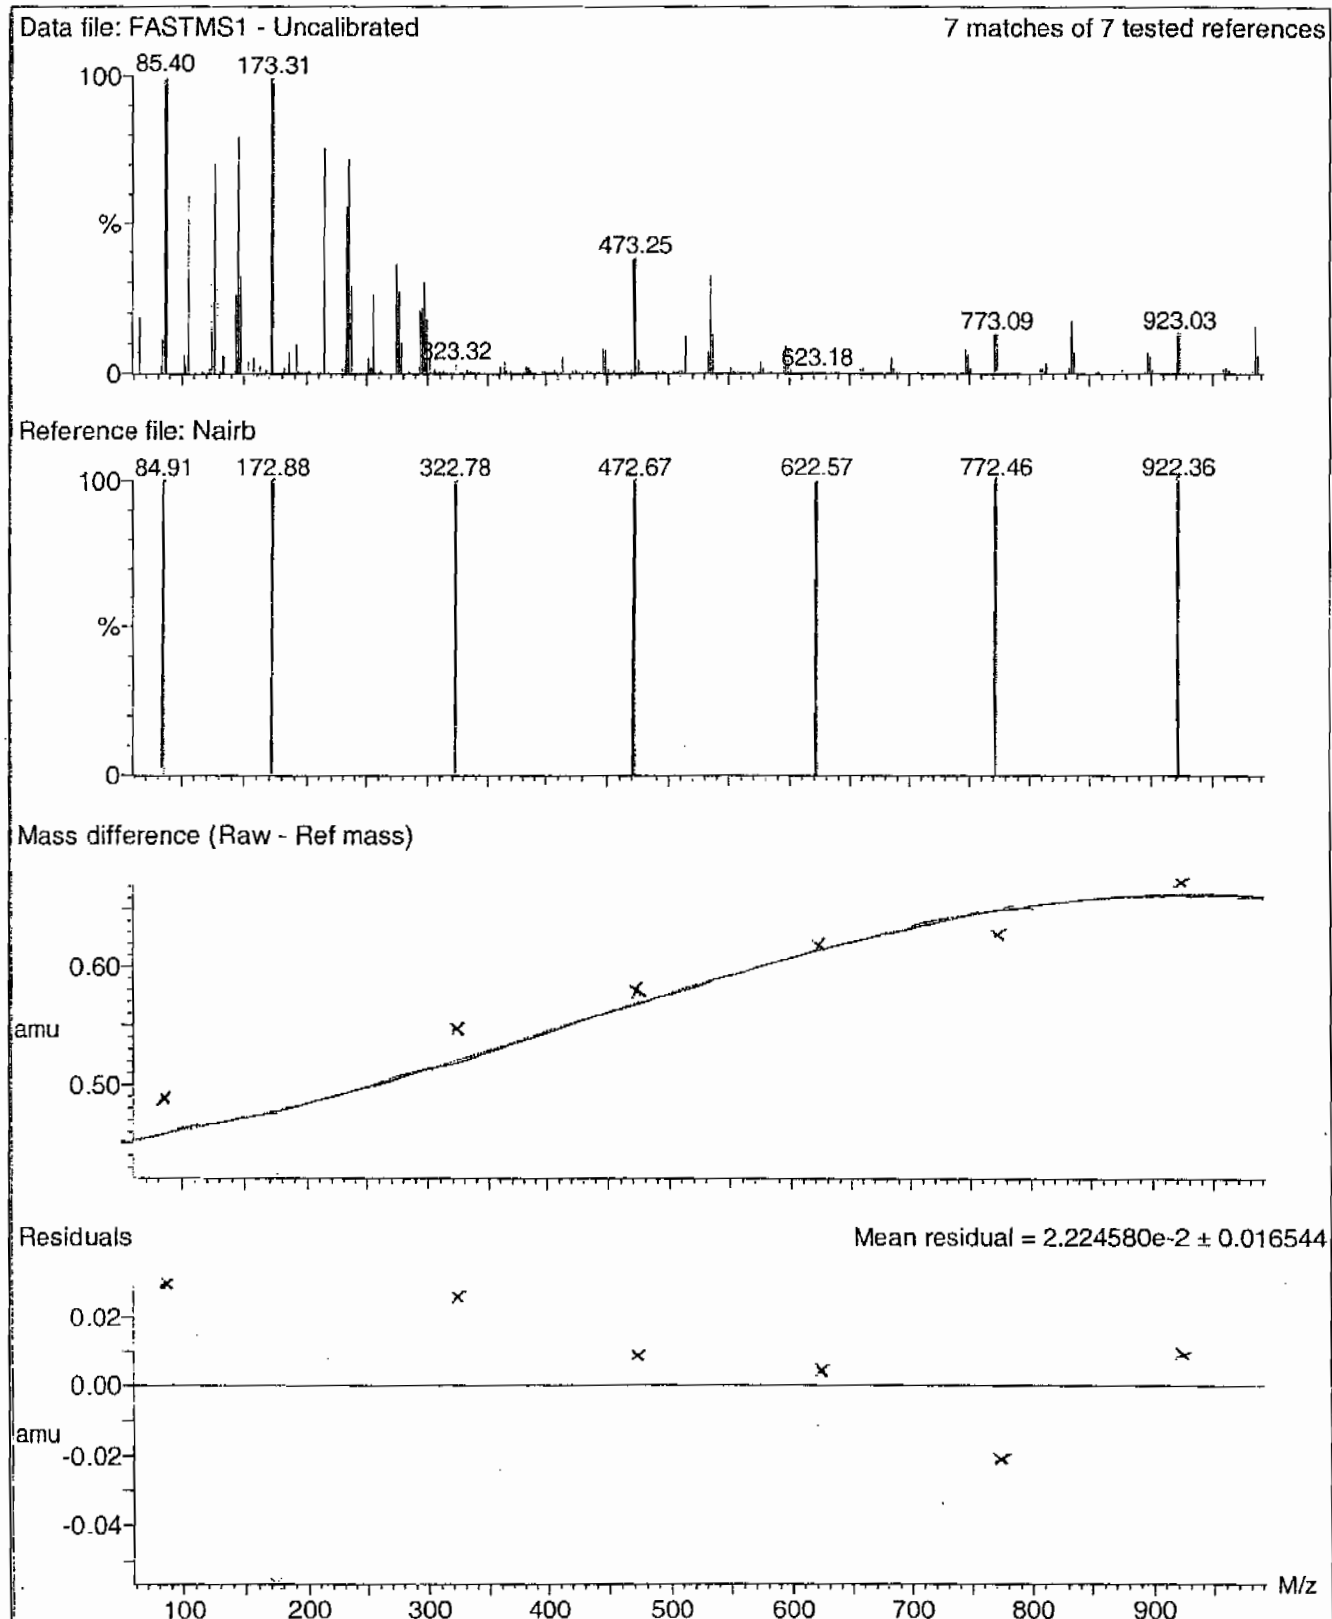

Calibration Report - MS2 Scan Speed Compensation

Page 1 of 1


Printed: Tue Jan 08 12:23:51 2008

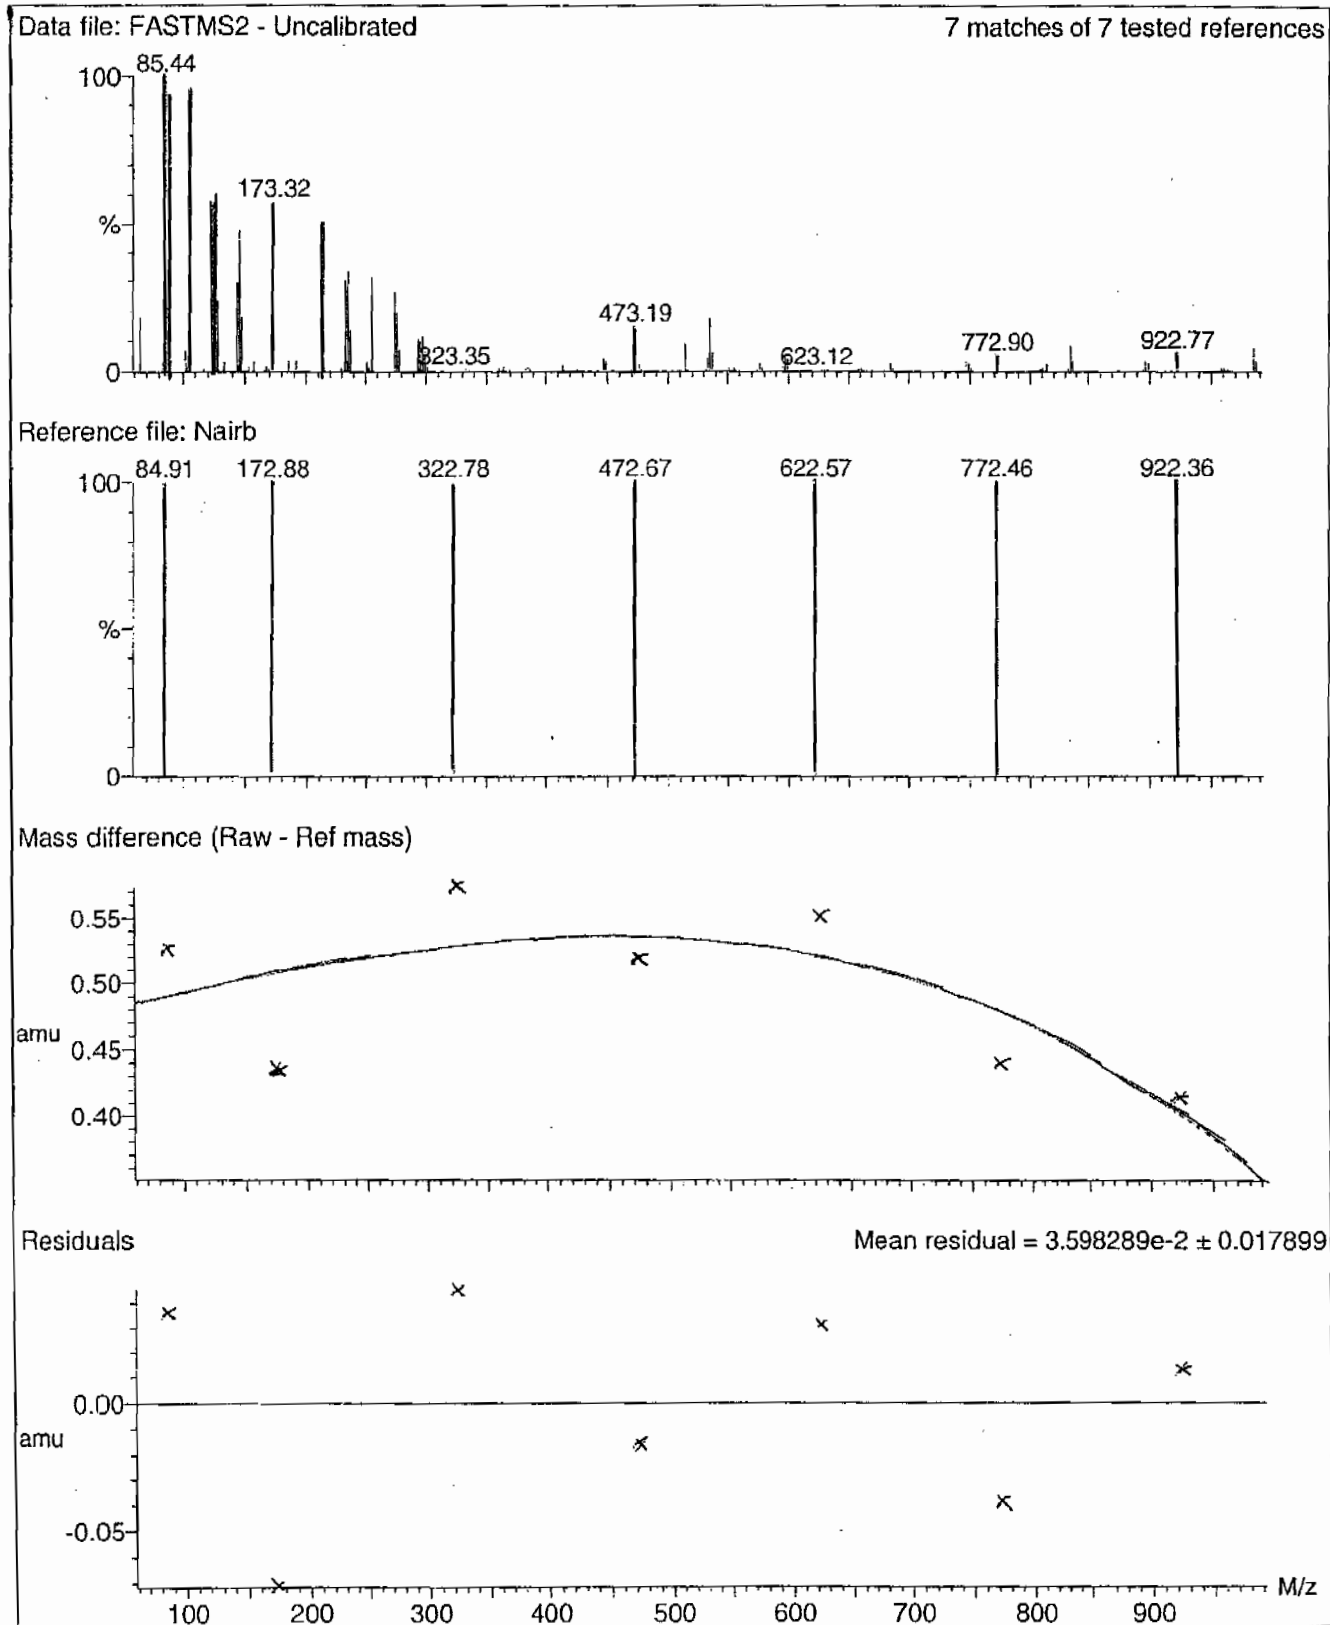

Calibration Report - MS2 Scanning

Page 1 of 1

Printed: Tue Jan 08 12:22:56 2008

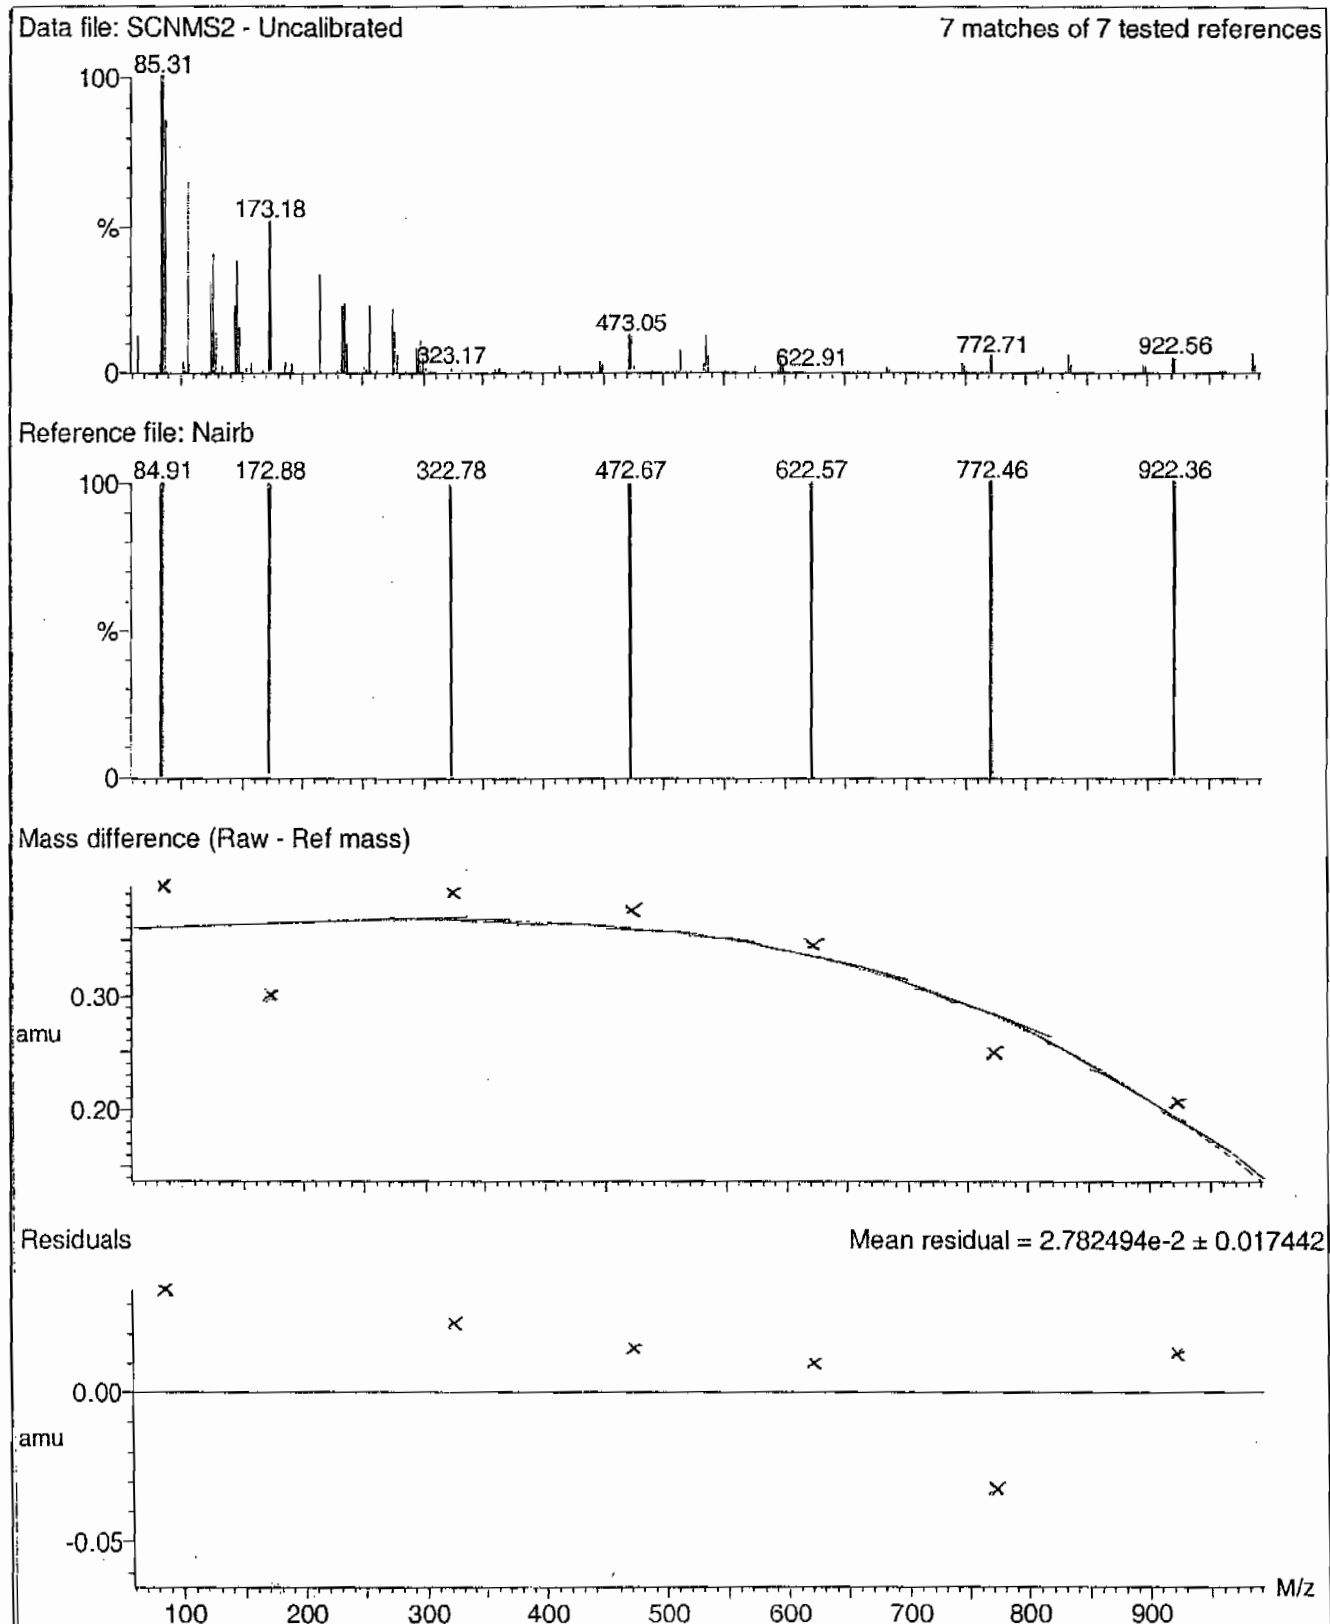


Calibration Report - MS2 Static

Page 1 of 1


Printed: Tue Jan 08 12:21:59 2008

Data file: STATMS2 - Uncalibrated


7 matches of 7 tested references

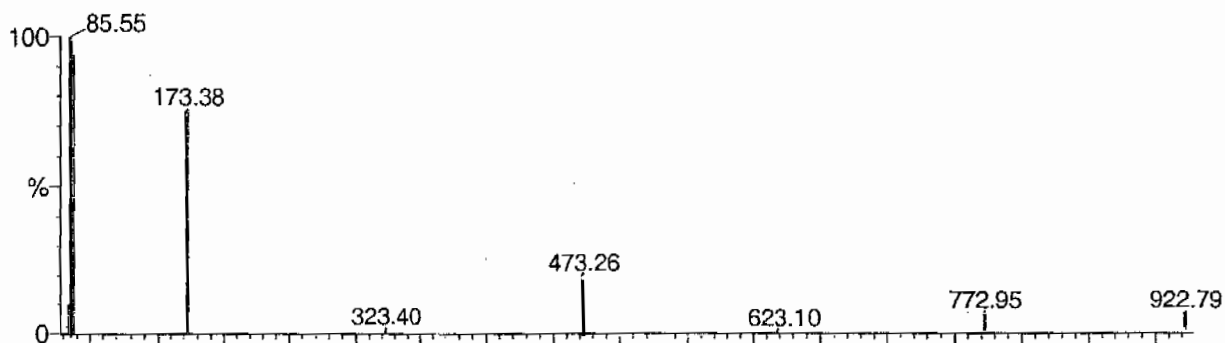

Reference file: Nairb

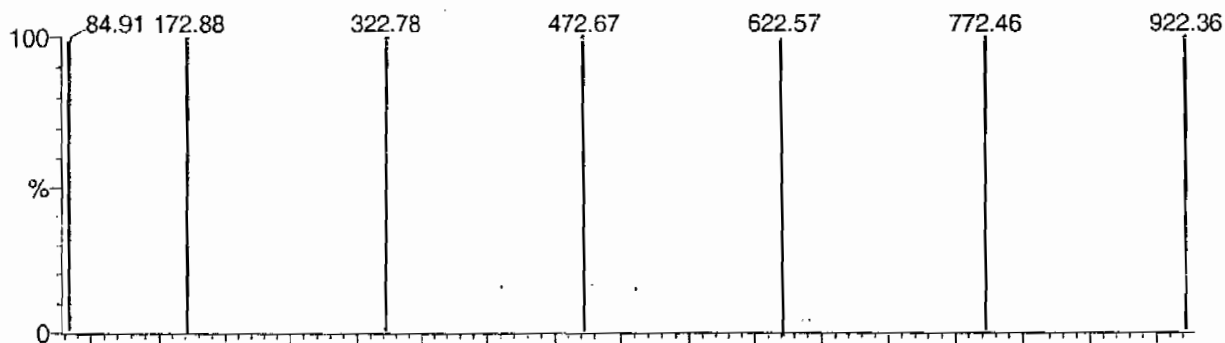


Mass difference (Raw - Ref mass)

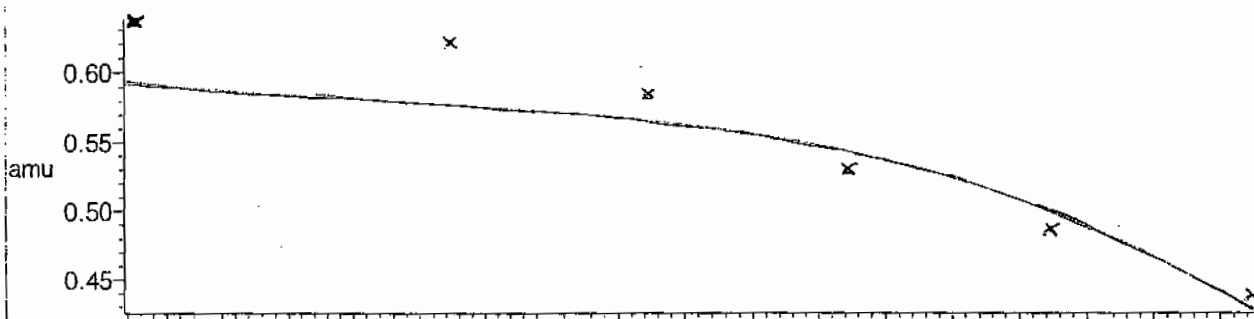

Residuals

Mean residual = $3.295980 \times 10^{-2} \pm 0.025603$

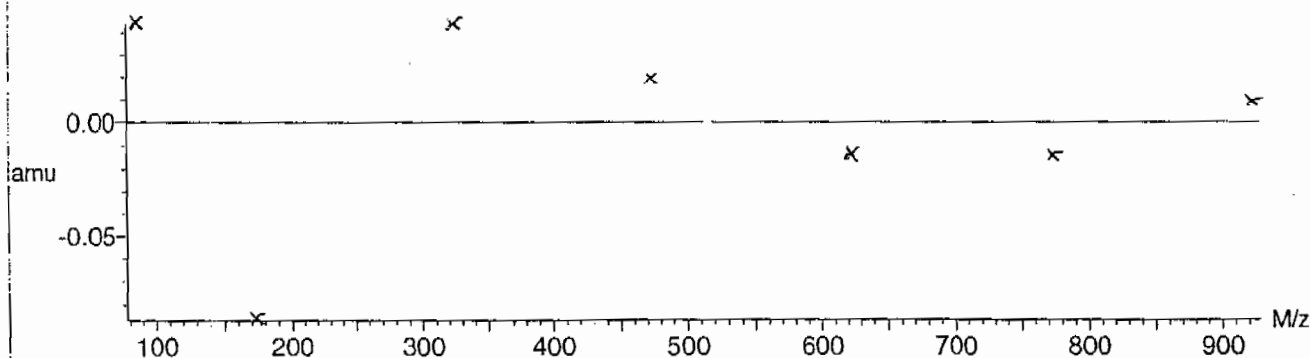


Tune Parameters

MassLynx 4.0 SP4

Page 1 of 1

File: C:\MassLynx\Perchlorate.PRO\ACQUDB\Perchlorate.IPR

Printed: Monday, March 08, 2010 10:18:13 Eastern Standard Time

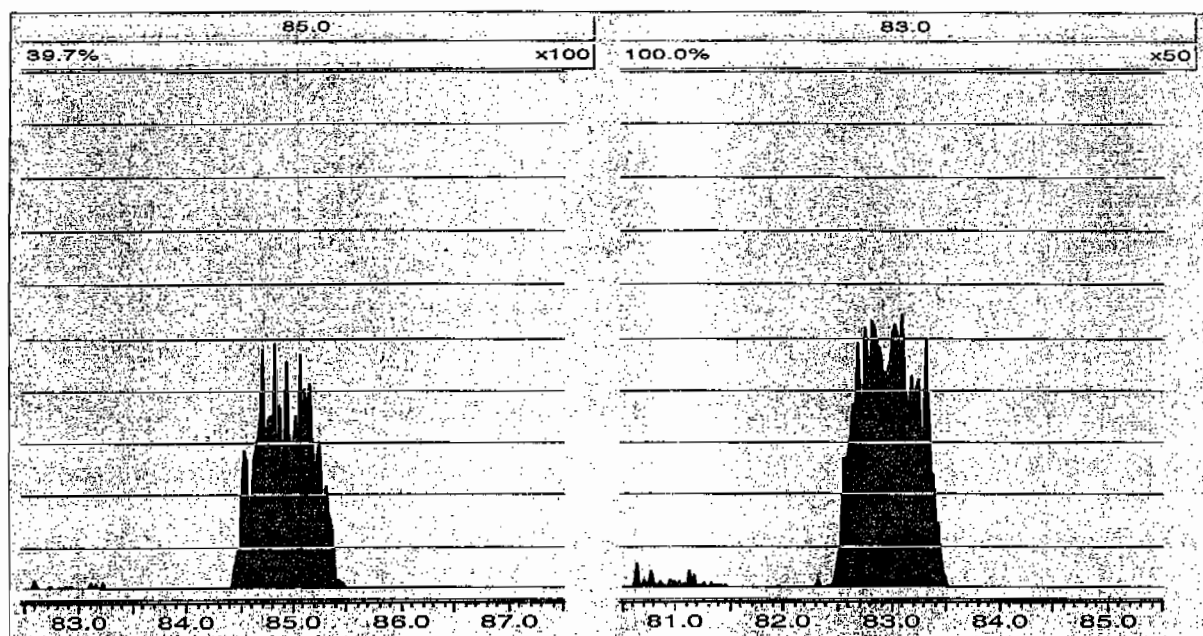

Perchlorate RT And Area Summary

Lab Name: General Engineering Laboratories
GEL Job No.(SDG): 10-2093

Lab Code: GEL

Instrument ID: LCMSMS

HPLC Column: Phenomenex Ion Pac AG-16 2 X 50 mm

Sample ID	Datafile	Run Date	Area	RT	RT CLO4	RRT	Q 0.98-1.02
MidLevel Standard Area	per0308006a	08-MAR-10	19792.7				
Lower Area Limit			9896.35				
Upper Area Limit			39585.4				
1202056715	per0308107a	09-MAR-10 07:47	17439.3	3.43	3.44547	1.005	
1202056716	per0308108a	09-MAR-10 07:57	17560.8	3.43	3.44552	1.005	
1202056719	per0308109a	09-MAR-10 08:06	18097.8	3.43	3.44547	1.005	
248117001	per0308111a	09-MAR-10 08:24	17642	3.42	3.45797	1.011	

SAMPLE DATA

P perchlorate Analysis Data Sheet

Lab Name: GEL Laboratories LLC
 Lab Code: GEL
 Instrument: LCMSMS
 Method: SW846 6850 Modified
 Matrix: WATER
 Extraction Batch ID: 259046
 Extraction Type: Filter/DAI
 Client Sample No. RE36-10-8458
 Date Received: 26-FEB-10
 GEL Job No (SDG): 10-2093
 GEL Sample ID: 248117001
 Date Filtered: 05-MAR-10
 Injection Volume (uL): 20

Sample Volume/Weight: 10.0 mL

%Solids:

Concentrated Extract Volume: 10.0

CAS No.	Analyte^	MDL	RL	Conc*	Units	Q	Dilution Factor	Date Analyzed	GEL File ID
14797-73-0	Perchlorate	.05	.2	0.050	ug/L	U	1	09-MAR-10 08:24	per0308111a
	Perchlorate Isotope Ratio						1	09-MAR-10 08:24	per0308111a
14797-73-0	Perchlorate-101	.05	.2	0.050	ug/L	U	1	09-MAR-10 08:24	per0308111a
	Perchlorate-O(18)			0.452	ug/L		1	09-MAR-10 08:24	per0308111a

^ When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

*Concentration =

Instrument Value X Concentrated Extract Volume X 1
 Aliquot %Solids

Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charliers W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308111a

Date: 09-Mar-2010


Time: 08:24:17

ID: 248117001

Vial: 3:1,E

03-04-10

12207 | 12207 | 11

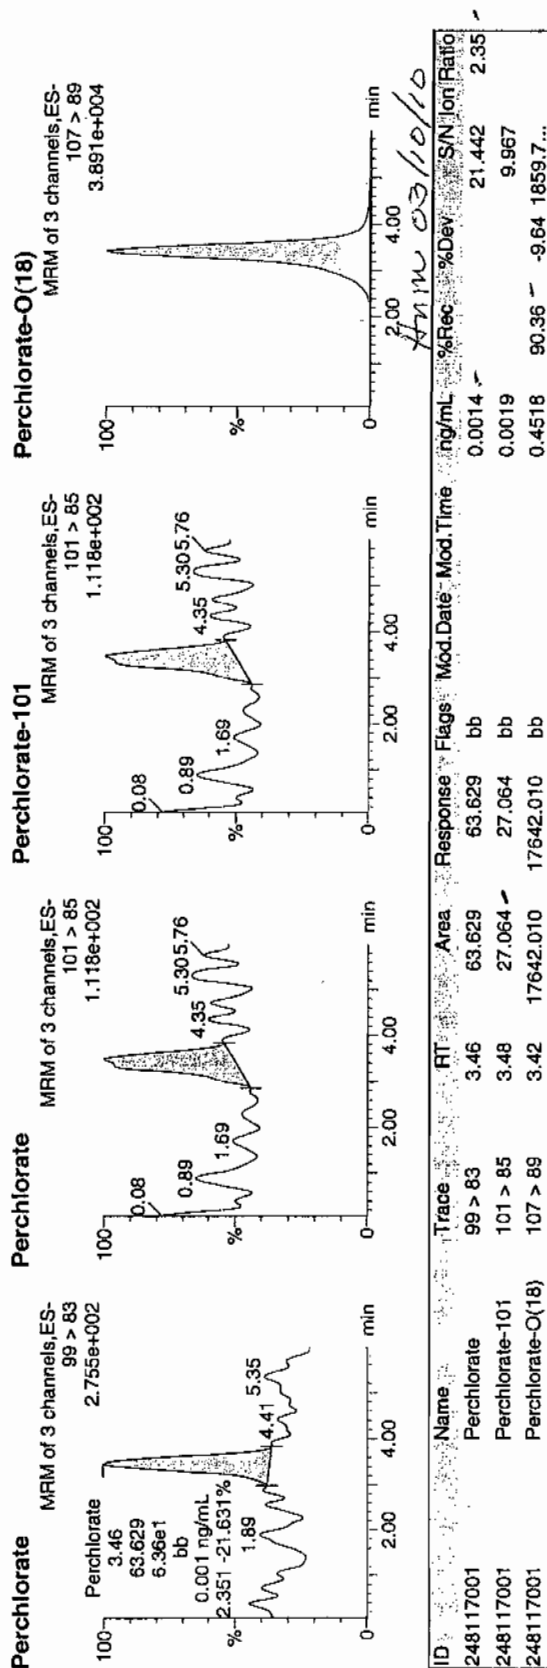

STANDARDS DATA

Perchlorate Initial Calibration

GEL Job No.(SDG): 10-2093

Lab Name: General Engineering Laboratories

Lab Code: GEL

Instrument ID: LCMSMS Date Analyzed: 08-MAR-10

HPLC Column: Phenomenex Ion Pac AG-16 2 X 50 mm

Calibration Level	1	2	3	4	5
Cal Concentration (ug/L)	0.05	0.1	0.25	0.50	1.0

Parname Perchlorate

Coefficient of Determination:

Calibration Curve: 47047.38

Response Type: External Standard

Curve Type: RF

P perchlorate Initial Calibration

Lab Name: General Engineering Laboratories GEL Job No.(SDG): 10-2093

Lab Code: GEL

Instrument ID: LCMSMS Date Analyzed: 08-MAR-10

HPLC Column: Phenomenex Ion Pac AG-16 2 X 50 mm

Calibration Level	1	2	3	4	5
Cal Concentration (ug/L)	0.05	0.1	0.25	0.50	1.0

Parname Perchlorate-101

Coefficient of Determination:

Calibration Curve: 14296.94

Response Type: External Standard

Curve Type: RF

Quantify Calibration Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charles W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Method: C:\MassLynx\Perchlorate.PRO\MethDB\per030810a.mdb 09 Mar 2010 12:48:33
Calibration: C:\MassLynx\Perchlorate.PRO\CurveDB\per030810a.cdb 09 Mar 2010 12:48:47


Compound name: Perchlorate

Response Factor: 47047.4

RF SD: 838.521, % Relative SD: 1.78229

Response type: External Std, Area

Curve type: RF

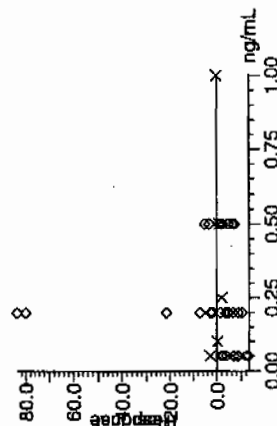


Compound name: Perchlorate-101

Response Factor: 14297



RF SD: 749.315, % Relative SD: 5.24108

Response type: External Std, Area

Curve type: RF

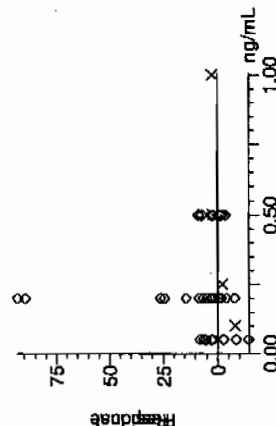

03-09-10

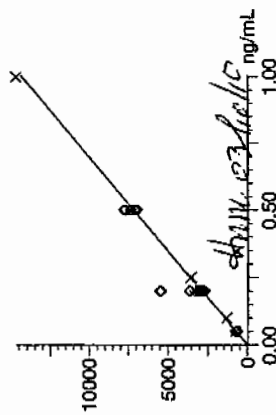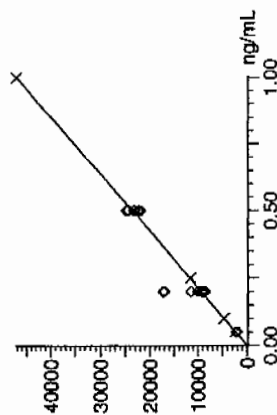

Quantify Calibration Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charles W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time


Compound name: Perchlorate-O(18)

Response Factor: 39049

RF SD: 832.552, % Relative SD: 2.13207

Response type: External Std, Area

Curve type: RF

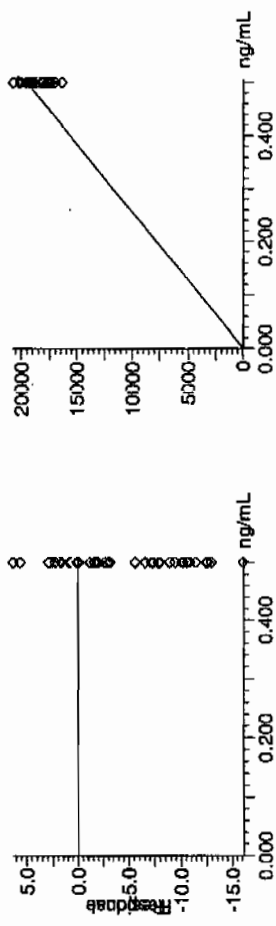

Form 3

Perchlorate Initial Calibration Verification

Lab Name: General Engineering Laboratories

GEL Job No.(SDG): 10-2093

Lab Code: GEL

Reporting Units: ug/L

Analyte	True	Found	%Rec	Date Analyzed	GEL File Id
Perchlorate	.5	.53	105.14	08-MAR-10 16:57	per0308009a
Perchlorate Isotope Ratio		3.18		08-MAR-10 16:57	per0308009a
Perchlorate-101	.5	.54	108.66	08-MAR-10 16:57	per0308009a


Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charfers W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308009a
Date: 08-Mar-2010
Time: 16:57:17
ID: WCL100227-06ICV
Vial: 1:2,A

Per
0308-10

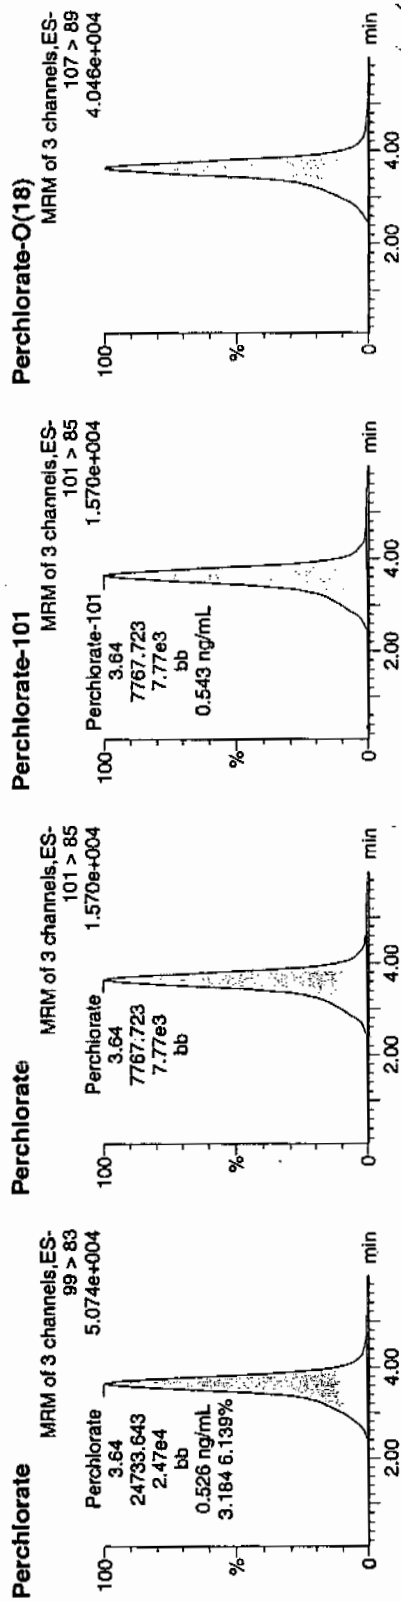

ID	Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	S/N	Ion Ratio
WCL100227-06ICV	Perchlorate	99 > 83	3.64	24733.643	24733.643	bb			0.5257	105.14	5.14	543.107	3.18
WCL100227-06ICV	Perchlorate-101	101 > 85	3.64	7767.723	7767.723	bb			0.5433	108.66	8.66	159.570	
WCL100227-06ICV	Perchlorate-O(18)	107 > 89	3.63	19967.303	19967.303	bb			0.5113	102.27	2.27	1535.3...	

Perchlorate Continuing Calibration Verification

Lab Name: General Engineering Laboratories

GEL Job No.(SDG): 10-2093

Lab Code: GEL

Reporting Units: ug/L

Analyte	True	Found	%Rec	Date Analyzed	GEL File Id
Perchlorate	.5	.52	103.28	08-MAR-10 18:46	per0308021a
Perchlorate Isotope Ratio		3.14		08-MAR-10 18:46	per0308021a
Perchlorate-101	.5	.54	108.41	08-MAR-10 18:46	per0308021a
Perchlorate	.5	.53	105.15	08-MAR-10 20:44	per0308034a
Perchlorate Isotope Ratio		3.23		08-MAR-10 20:44	per0308034a
Perchlorate-101	.5	.54	107.08	08-MAR-10 20:44	per0308034a
Perchlorate	.5	.52	103.16	08-MAR-10 22:42	per0308047a
Perchlorate Isotope Ratio		3.13		08-MAR-10 22:42	per0308047a
Perchlorate-101	.5	.54	108.56	08-MAR-10 22:42	per0308047a
Perchlorate	.5	.5	99.29	09-MAR-10 00:40	per0308060a
Perchlorate Isotope Ratio		3.17		09-MAR-10 00:40	per0308060a
Perchlorate-101	.5	.51	102.95	09-MAR-10 00:40	per0308060a
Perchlorate	.5	.48	95.1	09-MAR-10 02:38	per0308073a

Perchlorate Continuing Calibration Verification

Lab Name: General Engineering Laboratories

GEL Job No.(SDG): 10-2093

Lab Code: GEL

Reporting Units: ug/L

Perchlorate Isotope Ratio		3.07		09-MAR-10 02:38	per0308073a
Perchlorate-101	.5	.51	101.9	09-MAR-10 02:38	per0308073a
Perchlorate	.5	.46	92.67	09-MAR-10 04:36	per0308086a
Perchlorate Isotope Ratio		3.1		09-MAR-10 04:36	per0308086a
Perchlorate-101	.5	.49	98.48	09-MAR-10 04:36	per0308086a
Perchlorate	.5	.47	93.76	09-MAR-10 06:34	per0308099a
Perchlorate Isotope Ratio		3.2		09-MAR-10 06:34	per0308099a
Perchlorate-101	.5	.48	96.42	09-MAR-10 06:34	per0308099a
Perchlorate	.5	.48	95.65	09-MAR-10 08:33	per0308112a
Perchlorate Isotope Ratio		3.22		09-MAR-10 08:33	per0308112a
Perchlorate-101	.5	.49	97.77	09-MAR-10 08:33	per0308112a


Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charlers W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308021a
Date: 08-Mar-2010
Time: 18:46:13
ID: WCL100227-06CCV
Vial: 1:2,A

Pure
0309-10

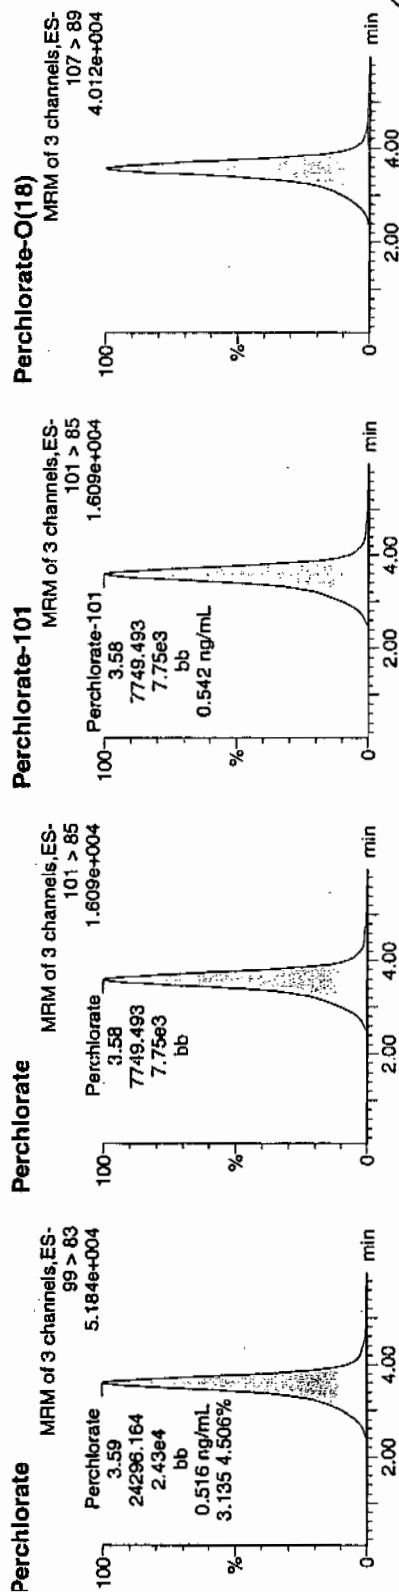

D	Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	S/N	Ion Ratio
WCL100227-06CCV	Perchlorate	99 > 83	3.59	24296.164	24296.164	bb			0.5164	103.28	3.28	2058.4...	3.14
WCL100227-06CCV	Perchlorate-101	101 > 85	3.58	7749.493	7749.493	bb			0.5420	108.41	8.41	842.163	
WCL100227-06CCV	Perchlorate-O(18)	107 > 89	3.57	18892.500	18892.500	bb			0.4838	96.76	-3.24	3961.4...	


Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charles W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308034a
Date: 08-Mar-2010
Time: 20:44:08
ID: WCL100227-06CCV
Vial: 1:2,A

Pure
03-29-10

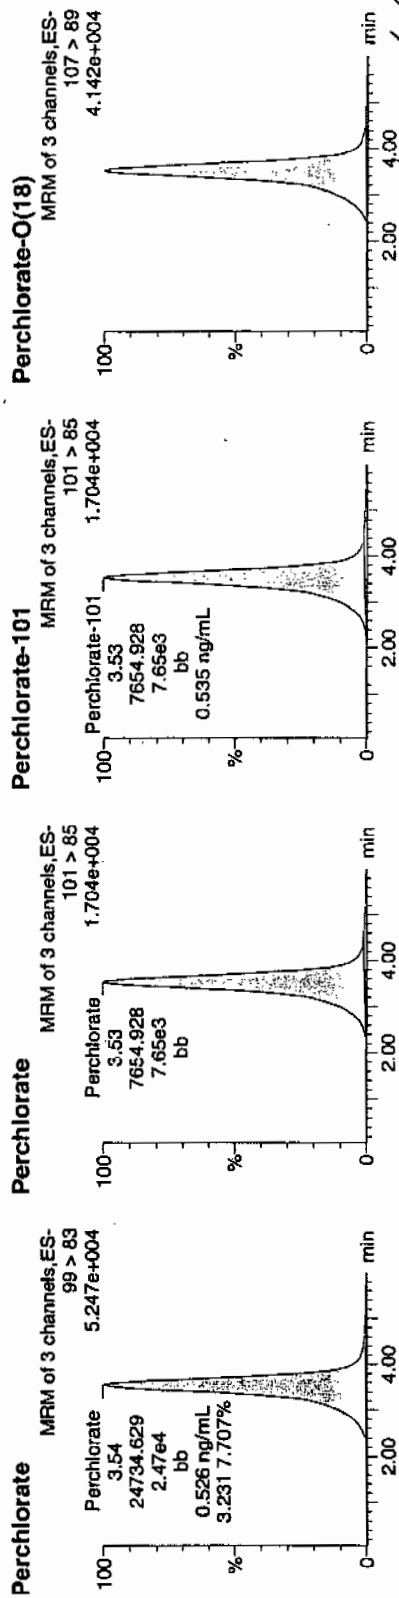

ID	Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	S/N	Ion Ratio
WCL100227-06CCV	Perchlorate	99 > 83	3.54	24734.629	24734.629	bb			0.5257	105.15	5.15	2200.8...	3.23
WCL100227-06CCV	Perchlorate-101	101 > 85	3.53	7654.928	7654.928	bb			0.5354	107.08	7.08	2331.6...	
WCL100227-06CCV	Perchlorate-O(18)	107 > 89	3.53	19141.506	19141.506	bb			0.4902	98.04	-1.96	1232.7...	


Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charlers W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308047a
Date: 08-Mar-2010
Time: 22:42:18
ID: WCL100227-06CCV
Vial: 1:2,A

Runs and 03-24-10

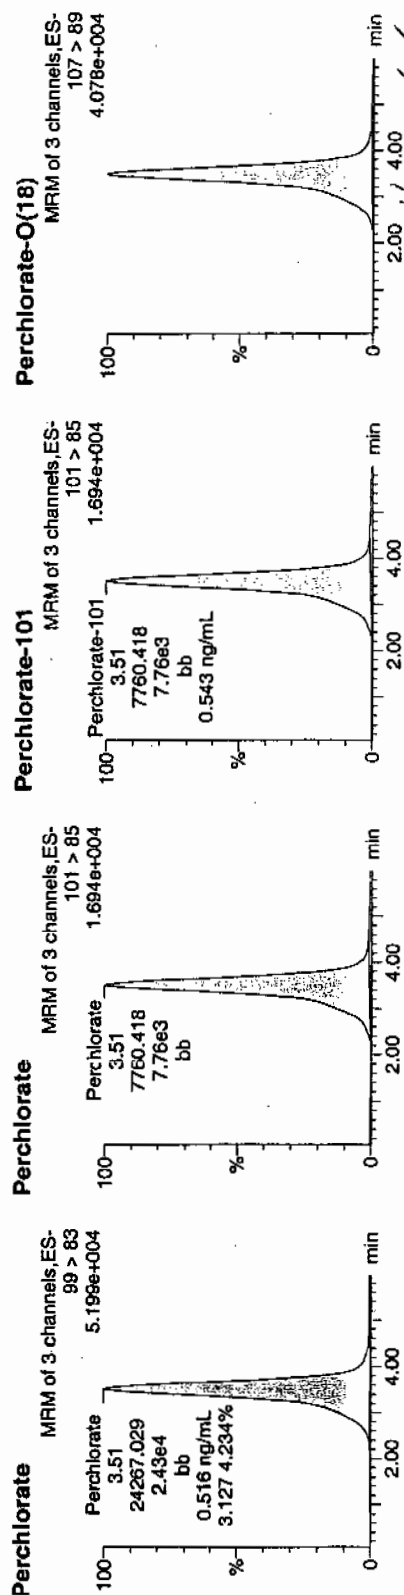

ID	Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	S/N	Ion Ratio
WCL100227-06CCV	Perchlorate	99 > 83	3.51	24267.029	24267.029	bb			0.5158	103.16	3.16	1490.7...	3.13
WCL100227-06CCV	Perchlorate-101	101 > 85	3.51	7760.418	7760.418	bb			0.5428	108.56	8.56	1343.7...	
WCL100227-06CCV	Perchlorate-O(18)	107 > 89	3.50	18936.834	18936.834	bb			0.4849	96.99	-3.01	1821.0...	


Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charliers W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308060a
Date: 09-Mar-2010
Time: 00:40:46
ID: WCL100227-06CCV
Vial: 1:2,A

*Run
WCL
03-01-10*

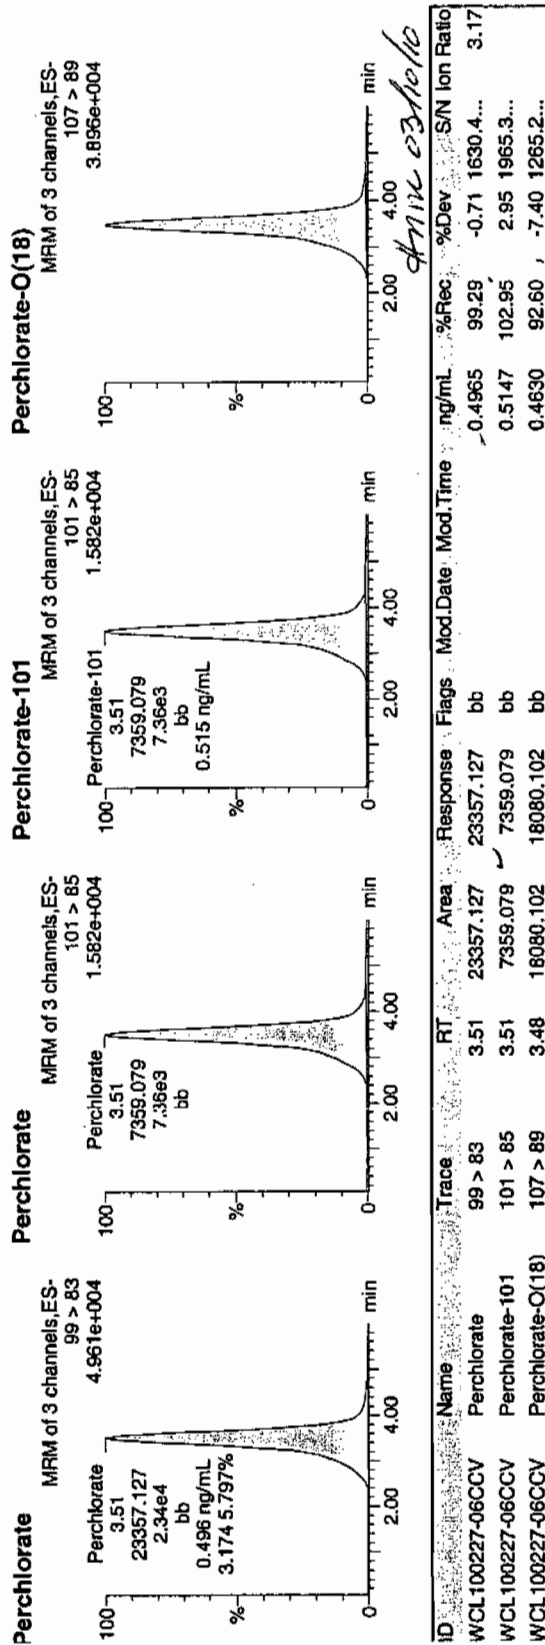





Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charlers W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308073a
Date: 09-Mar-2010
Time: 02:38:45
ID: WCL100227-06CCV
Vial: 1:2,A

Purs
03-04-10

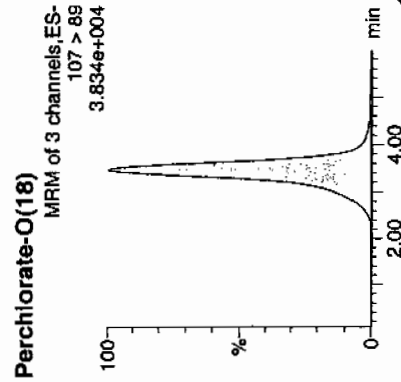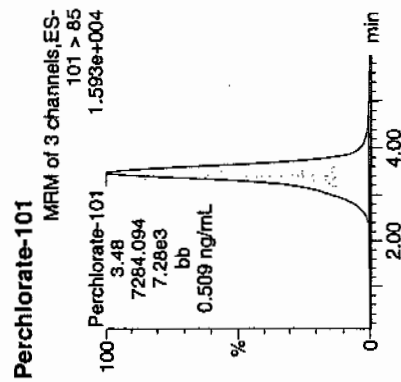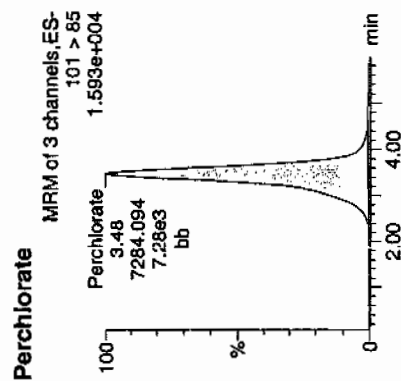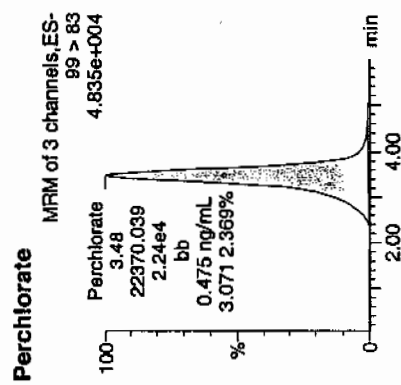

ID	Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	SN	Ion Ratio
WCL100227-06CCV	Perchlorate	99 > 83	3.48	22370.039	22370.039	bb			0.4755	95.10	-4.90	2051.0...	3.07
WCL100227-06CCV	Perchlorate-101	101 > 85	3.48	7284.094	7284.094	bb			0.5095	101.90	1.90	930.289	
WCL100227-06CCV	Perchlorate-O(18)	107 > 89	3.47	17683.076	17683.076	bb			0.4528	90.57	-9.43	2477.5...	


Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charlers W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308086a
Date: 09-Mar-2010
Time: 04:36:48
ID: WCL100227-06CCV
Vial: 1:2,A

Per030810

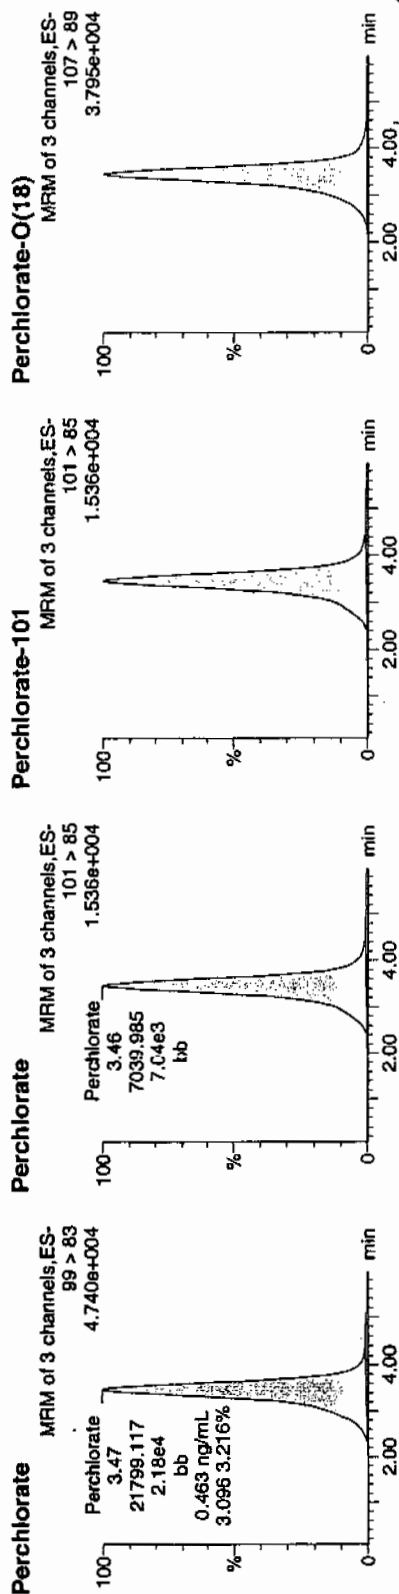

ID	Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	S/N	Ion Ratio
WCL100227-06CCV	Perchlorate	99 > 83	3.47	21799.117	21799.117	bb			0.4633	92.67	-7.33	1295.8...	3.10
WCL100227-06CCV	Perchlorate-101	101 > 85	3.46	7039.985	7039.985	bb			0.4924	98.48	-1.52	178.389	
WCL100227-06CCV	Perchlorate-O(18)	107 > 89	3.45	17451.631	17451.631	bb			0.4469	89.38	-10.62	1763.3...	

Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charliers W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308099a


Date: 09-Mar-2010

Time: 06:34:54

ID: WCL100227-06CCV

Vial: 1:2,A

Run and 03-04-10

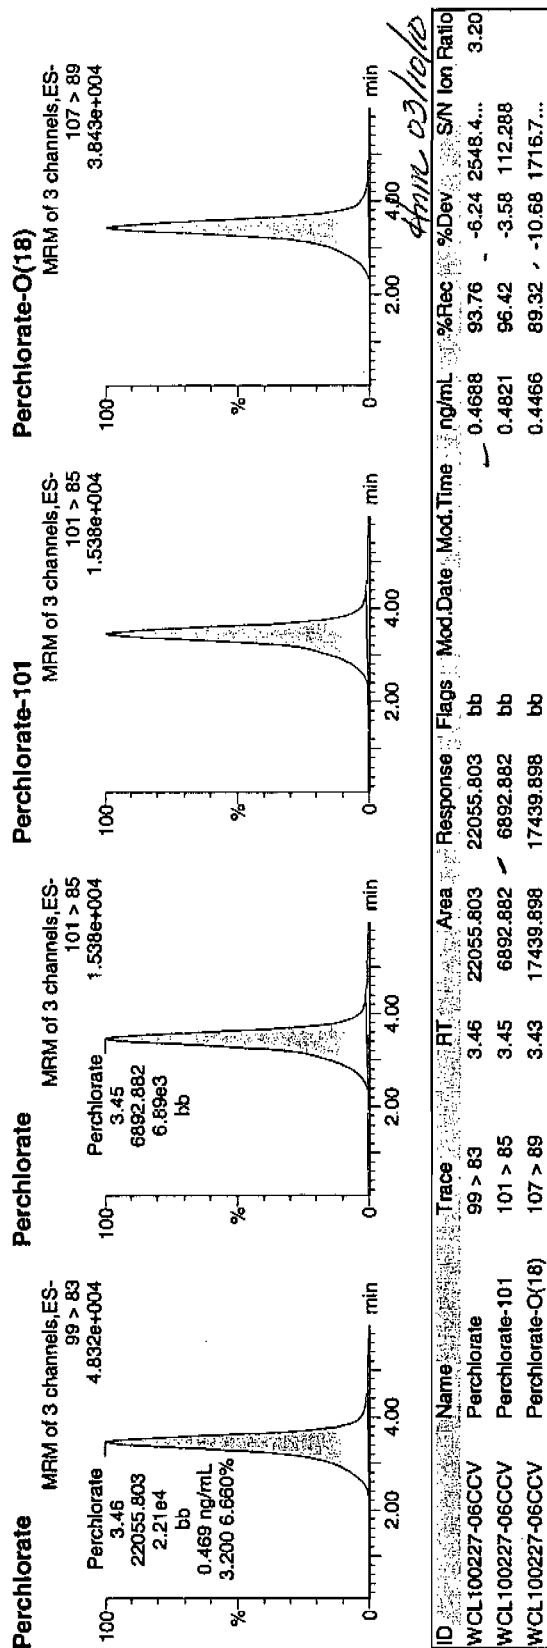


Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charlers W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308112a
Date: 09-Mar-2010
Time: 08:33:18
ID: WCL100227-06CCV
Vial: 1:2,A

*Perchlorate
03-09-10*

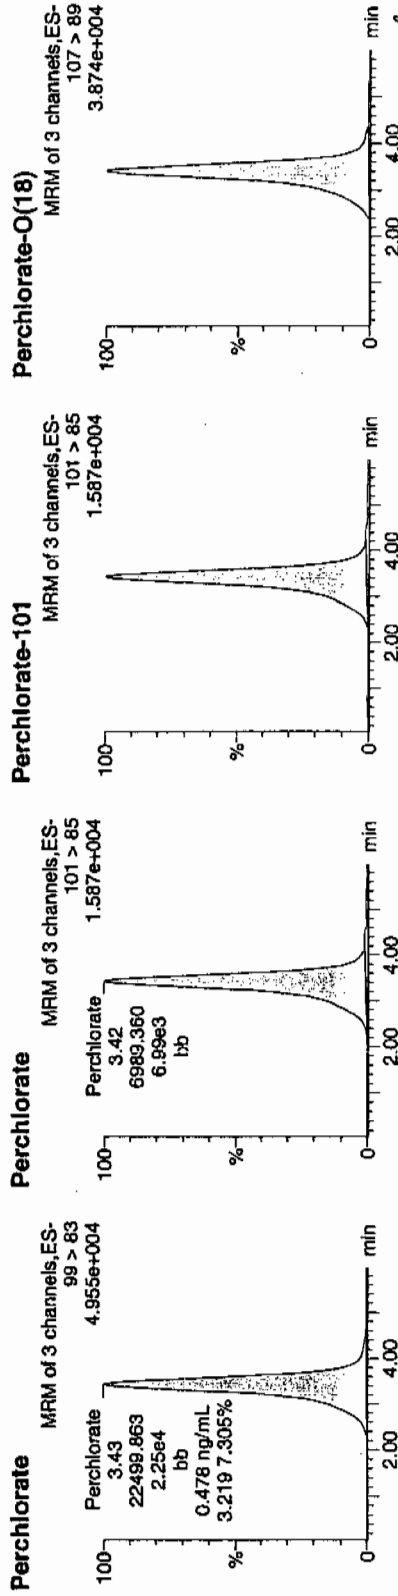

ID	Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	S/N	Ion Ratio
WCL100227-06CCV	Perchlorate	99 > 83	3.43	22499.863	22499.863	bb			0.4782	95.65	-4.35	1163.4...	3.22
WCL100227-06CCV	Perchlorate-101	101 > 85	3.42	6989.360	6989.360	bb			0.4889	97.77	-2.23	1178.6...	
WCL100227-06CCV	Perchlorate-O(18)	107 > 89	3.42	17548.695	17548.695	bb			0.4494	89.88	-10.12	1305.7...	

Perchlorate MDL Verification

GEL Job No.(SDG): 10-2093

Lab Name: General Engineering Laboratories

Lab Code: GEL

Reporting Units: ug/L

Analyte	True	Found	%Rec	Date Analyzed	GEL File Id
Perchlorate	.05	.05	91.57	08-MAR-10 17:15	per0308011a
Perchlorate Isotope Ratio		2.95		08-MAR-10 17:15	per0308011a
Perchlorate-101	.05	.05	102.06	08-MAR-10 17:15	per0308011a
Perchlorate	.05	.05	97.28	08-MAR-10 19:04	per0308023a
Perchlorate Isotope Ratio		2.97		08-MAR-10 19:04	per0308023a
Perchlorate-101	.05	.05	107.82	08-MAR-10 19:04	per0308023a
Perchlorate	.05	.05	97.48	08-MAR-10 21:02	per0308036a
Perchlorate Isotope Ratio		3.14		08-MAR-10 21:02	per0308036a
Perchlorate-101	.05	.05	102.17	08-MAR-10 21:02	per0308036a
Perchlorate	.05	.05	98.41	08-MAR-10 23:00	per0308049a
Perchlorate Isotope Ratio		3.08		08-MAR-10 23:00	per0308049a

Perchlorate MDL Verification

GEL Job No.(SDG): 10-2093

Lab Name: General Engineering Laboratories

Lab Code: GEL

Reporting Units: ug/L

Perchlorate-101	.05	.05	105.1	08-MAR-10 23:00	per0308049a
Perchlorate	.05	.05	92.76	09-MAR-10 00:59	per0308062a
Perchlorate Isotope Ratio		3.13		09-MAR-10 00:59	per0308062a
Perchlorate-101	.05	.05	97.6	09-MAR-10 00:59	per0308062a
Perchlorate	.05	.04	87.02	09-MAR-10 02:57	per0308075a
Perchlorate Isotope Ratio		2.95		09-MAR-10 02:57	per0308075a
Perchlorate-101	.05	.05	97.15	09-MAR-10 02:57	per0308075a
Perchlorate	.05	.04	88.07	09-MAR-10 04:55	per0308088a
Perchlorate Isotope Ratio		2.98		09-MAR-10 04:55	per0308088a
Perchlorate-101	.05	.05	97.34	09-MAR-10 04:55	per0308088a
Perchlorate	.05	.05	93.32	09-MAR-10 06:53	per0308101a

Perchlorate MDL Verification

Lab Name: General Engineering Laboratories GEL Job No.(SDG): 10-2093

Lab Code: GEL

Reporting Units: ug/L

Perchlorate Isotope Ratio		3.36		09-MAR-10 06:53	per0308101a
Perchlorate-101	.05	.05	91.41	09-MAR-10 06:53	per0308101a
Perchlorate	.05	.05	96.02	09-MAR-10 08:51	per0308114a
Perchlorate Isotope Ratio		3.69		09-MAR-10 08:51	per0308114a
Perchlorate-101	.05	.04	85.66	09-MAR-10 08:51	per0308114a


Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charles W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Sample Name: per0308011a
Date: 08-Mar-2010
Time: 17:15:29
D: WCL100227-07CRI
Vial: 1:2,B

Per
03-09-10

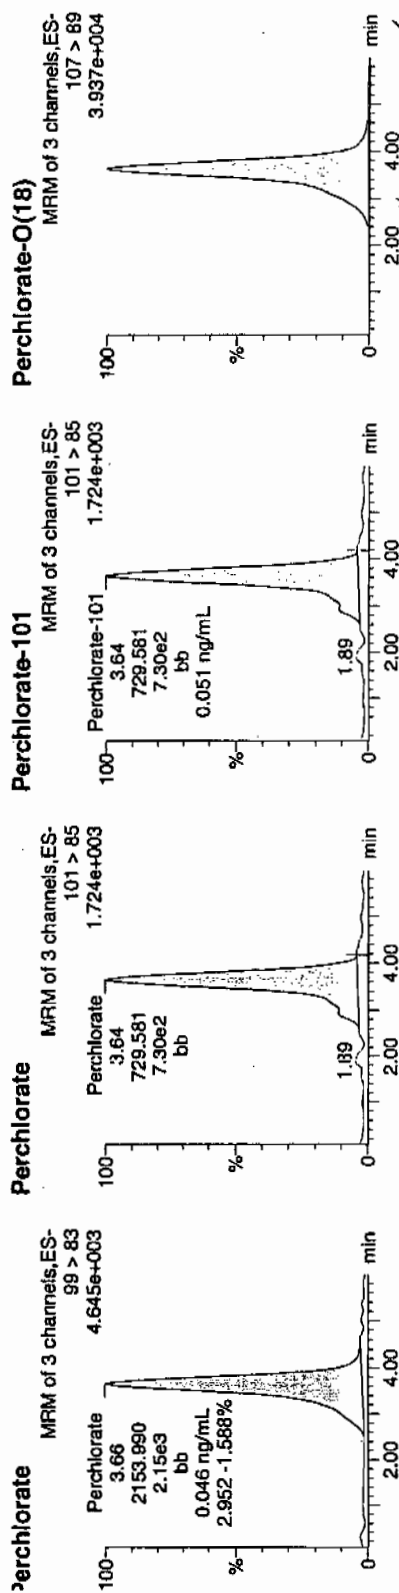

Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	S/N	Ion Ratio
Perchlorate	99 > 83	3.66	2153.990	2153.990	bb			0.0458	91.57	-8.43	192.273	2.95
Perchlorate-101	101 > 85	3.64	729.581	729.581	bb			0.0510	102.06	2.06	143.835	
Perchlorate-O(18)	107 > 89	3.63	19505.877	19505.877	bb			0.4995	99.90	-0.10	1304.1...	

Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charlers W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308023a





Date: 08-Mar-2010

Time: 19:04:27

ID: WCL100227-07CRI

Vial: 1:2,B

per
03-09-10

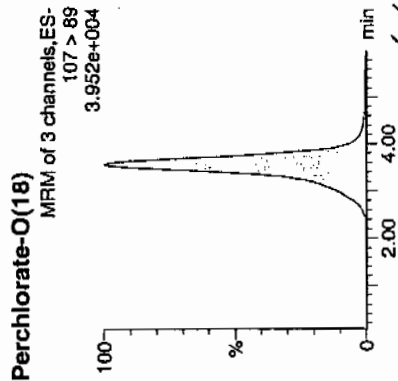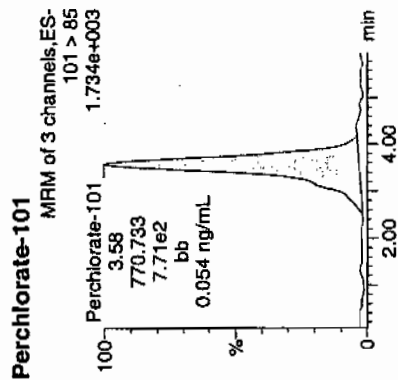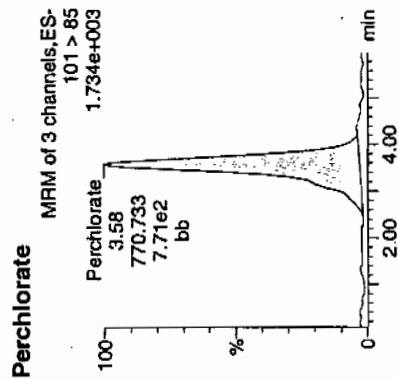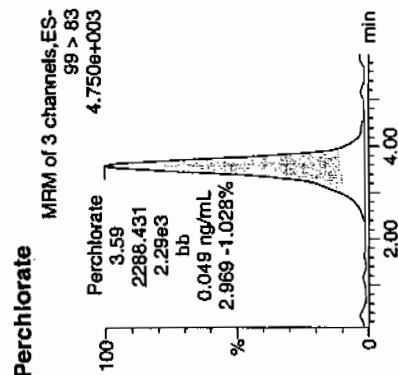

ID	Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	S/N	Ion Ratio
WCL100227-07CRI	Perchlorate	99 > 83	3.59	2288.431	2288.431	bb			0.0486	97.28	-2.72	379.669	2.97
WCL100227-07CRI	Perchlorate-101	101 > 85	3.58	770.733	770.733	bb			0.0539	107.82	7.82	84.015	
WCL100227-07CRI	Perchlorate-O(18)	107 > 89	3.57	18985.990	18985.990	bb			0.4862	97.24	-2.76	3992.9...	

Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charles W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308036a


Date: 08-Mar-2010

Time: 21:02:14

ID: WCL100227-07CRI

Vial: 1:2,B

*Pure
conc
03-04-10*

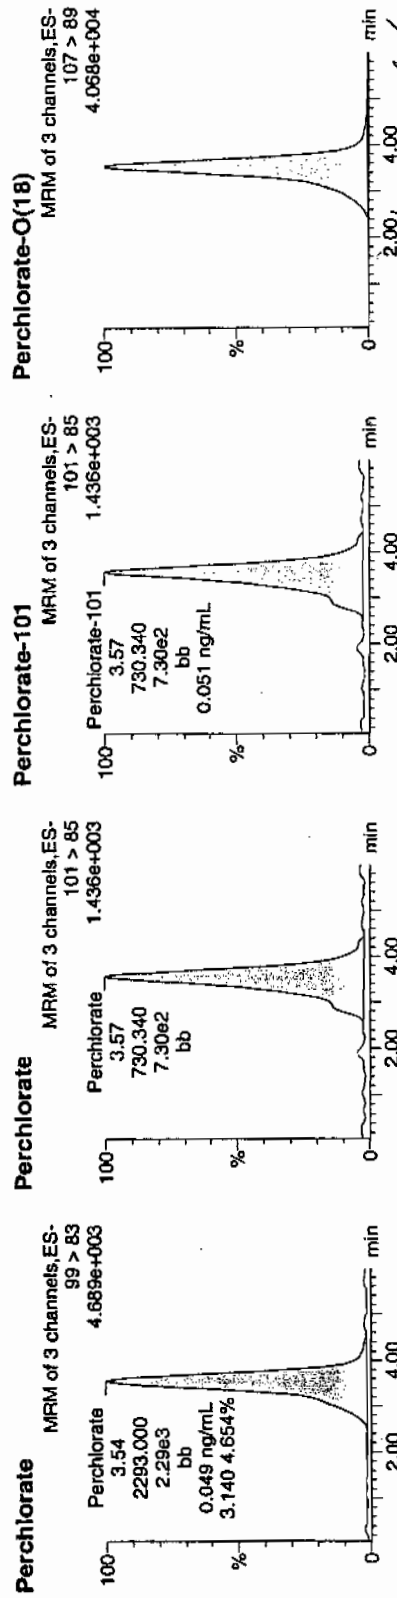

ID	Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	SN	Ion Ratio
WCL100227-07CRI	Perchlorate	99 > 83	3.54	2293.000	2293.000	bb			0.0487	97.48	-2.52	112.560	3.14
WCL100227-07CRI	Perchlorate-101	101 > 85	3.57	730.340	730.340	bb			0.0511	102.17	2.17	21.006	
WCL100227-07CRI	Perchlorate-O(18)	107 > 89	3.53	19152.959	19152.959	bb			0.4905	98.10	-1.90	2778.2...	

Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charfers W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308049a


Date: 08-Mar-2010

Time: 23:00:24

D: WCL100227-07CRI

/lal: 1:2,B

Pur
Ans
03-04-10

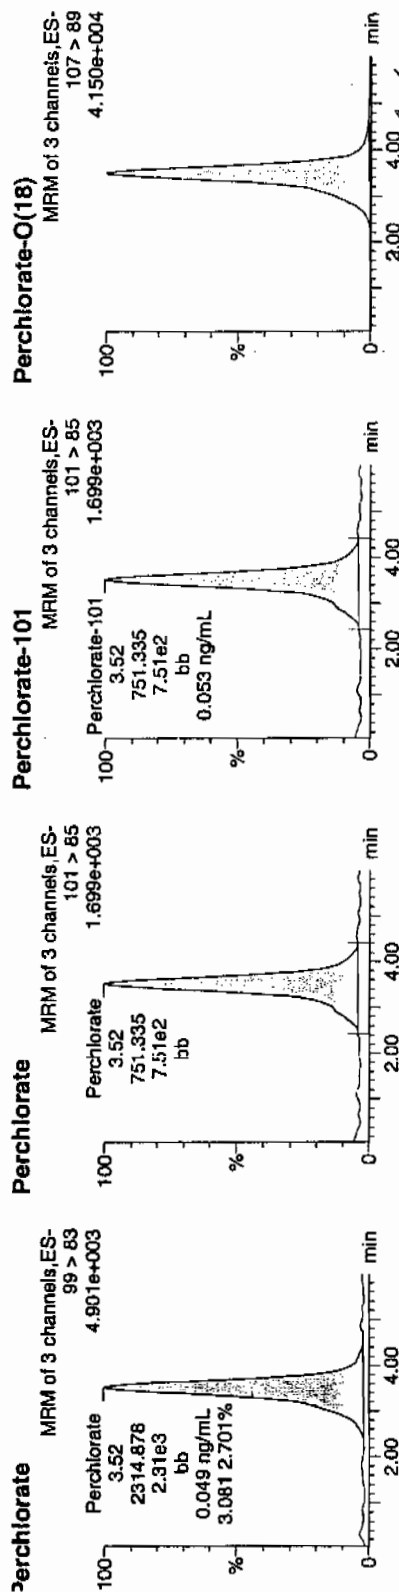

ID	Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	S/N	Ion Ratio
WCL100227-07CRI	Perchlorate	99 > 83	3.52	2314.878	2314.878	bb			0.0492	98.41	-1.59	318.865	3.08
WCL100227-07CRI	Perchlorate-101	101 > 85	3.52	751.335	751.335	bb			0.0526	105.10	5.10	86.661	
WCL100227-07CRI	Perchlorate-O(18)	107 > 89	3.51	19220.762	19220.762	bb			0.4922	98.44	-1.56	1856.7...	


Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charliers W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308062a
Date: 09-Mar-2010
Time: 00:59:13
ID: WCL100227-07CRI
Vial: 1:2,B

*Run
623
03-09-10*

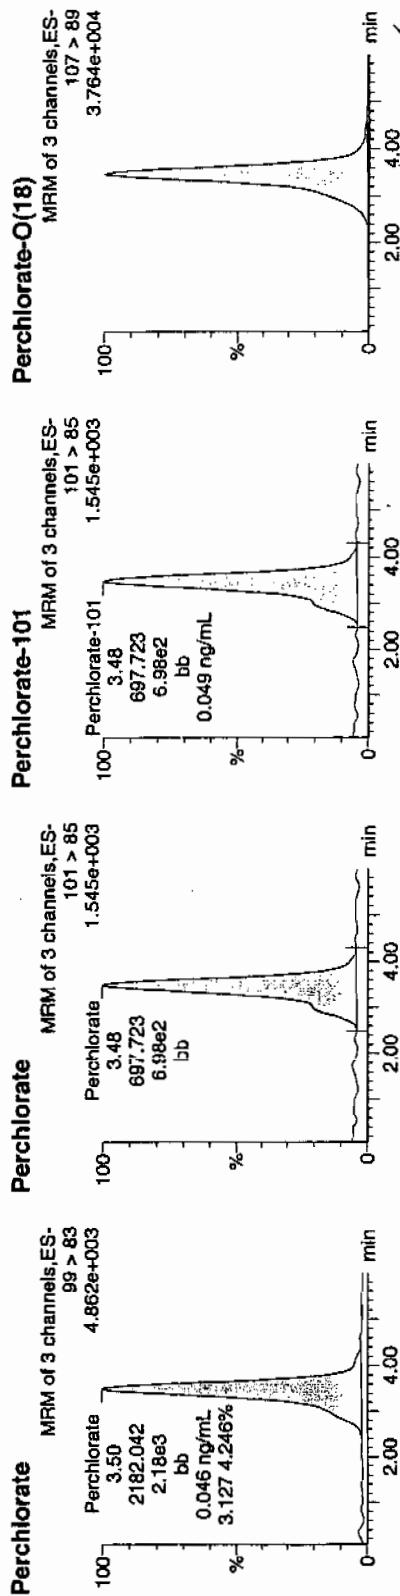

ID	Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	S/N	Ion Ratio
WCL100227-07CRI	Perchlorate	99 > 83	3.50	2182.042	2182.042	bb			0.0464	92.76	-7.24	176.942	3.13
WCL100227-07CRI	Perchlorate-101	101 > 85	3.48	697.723	697.723	bb			0.0488	97.60	-2.40	55.243	
WCL100227-07CRI	Perchlorate-O(18)	107 > 89	3.47	17393.770	17393.770	bb			0.4454	89.09	-10.91	764.961	

Amu 03/09/10


Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charlers W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308075a
Date: 09-Mar-2010
Time: 02:57:04
ID: WCL100227-07CRI
Vial: 1:2,B

Pure
and
03-09-10

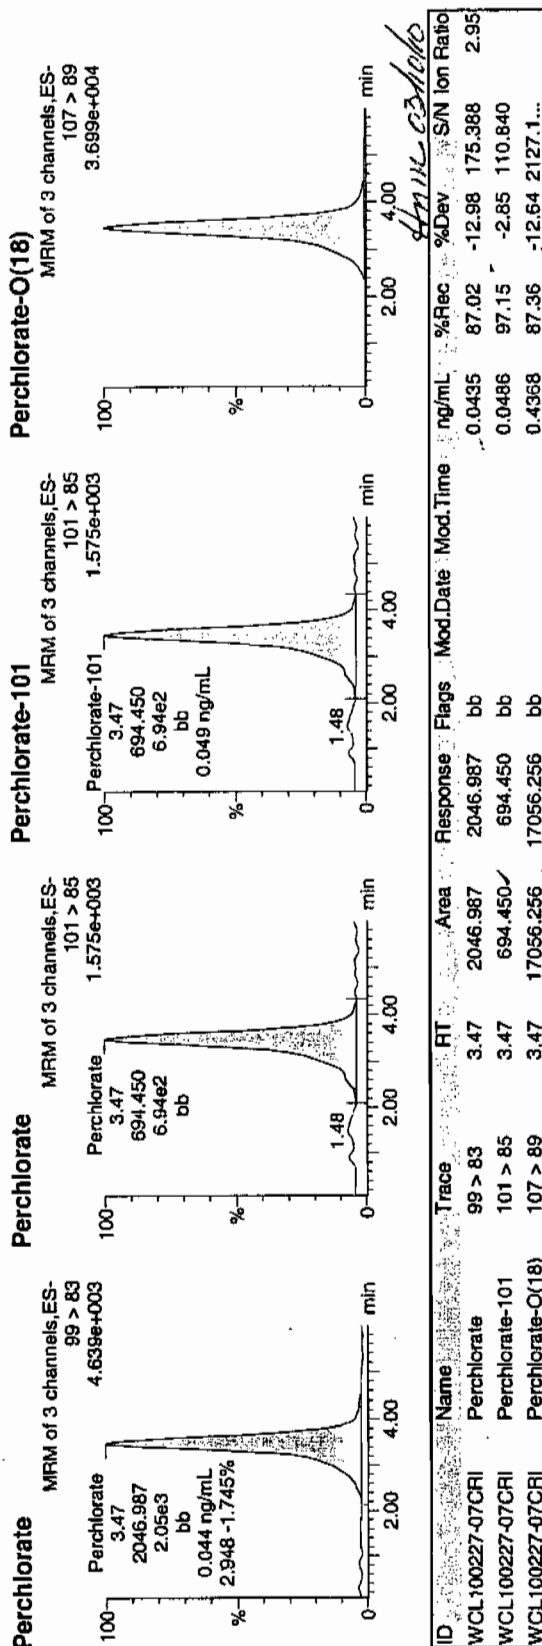





Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charles W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308088a
Date: 09-Mar-2010
Time: 04:55:08
ID: WCL100227-07CRI
Vial: 1:2,B

Run and 03-09-10

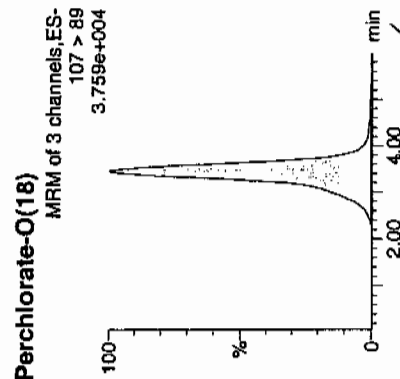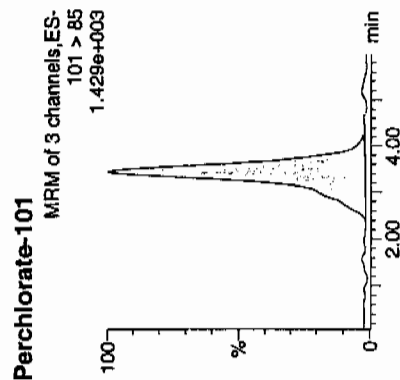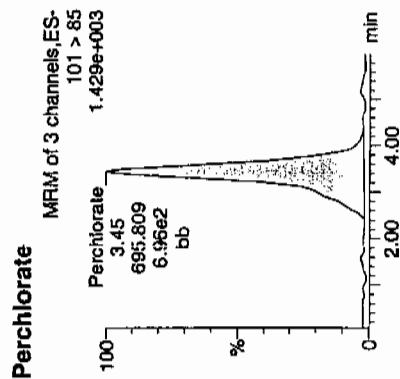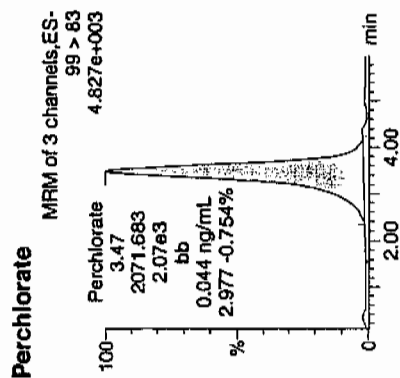


ID	Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	S/N	Ion Ratio
WCL100227-07CRI	Perchlorate	99 > 83	3.47	2071.683	2071.683	bb			0.0440	88.07	-11.93	130.882	2.98
WCL100227-07CRI	Perchlorate-101	101 > 85	3.45	695.809	695.809	bb			0.0487	97.34	-2.66	110.757	
WCL100227-07CRI	Perchlorate-O(18)	107 > 89	3.45	17290.361	17290.361	bb			0.4428	88.56	-11.44	1467.3...	

Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charlers W. Wilson
Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308101a
Date: 09-Mar-2010
Time: 06:53:14
ID: WCL100227-07CRI
Vial: 1;2,B

Purs
and
03-04-10

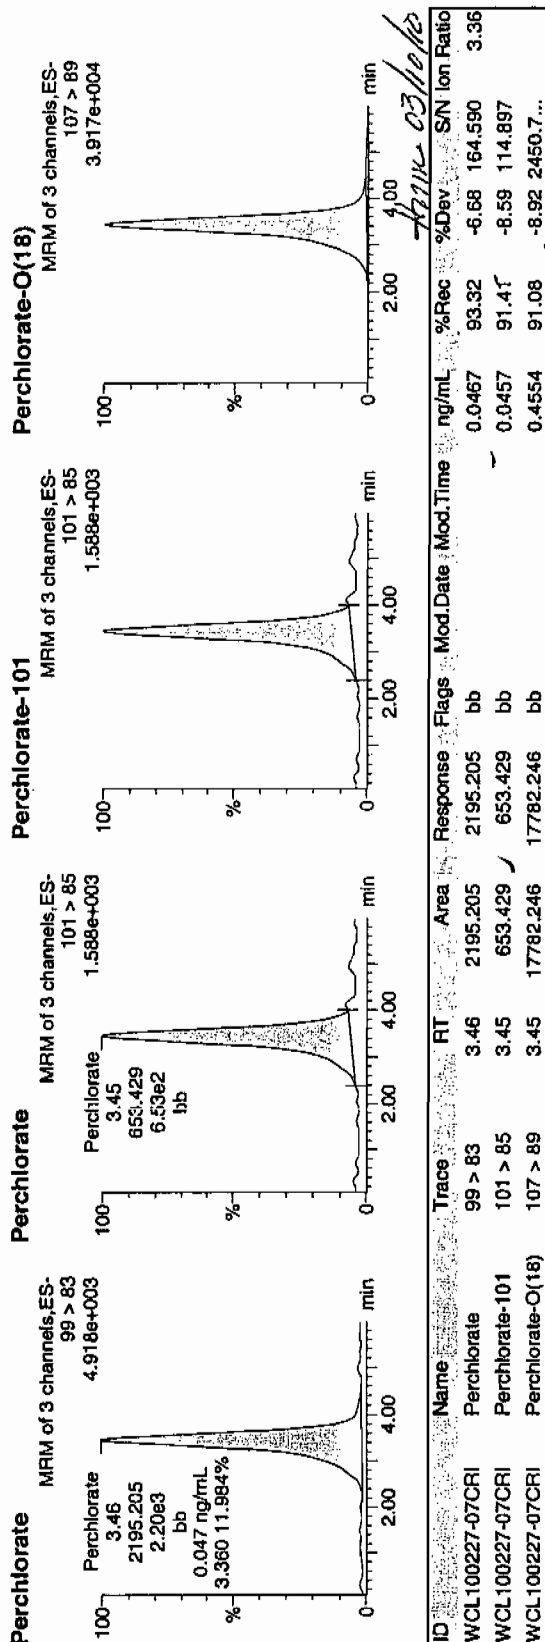

Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charfers W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308114a


Date: 09-Mar-2010

Time: 08:51:36

D: WCL100227-07CRI

/lat: 1:2,B

Per
03-04-10

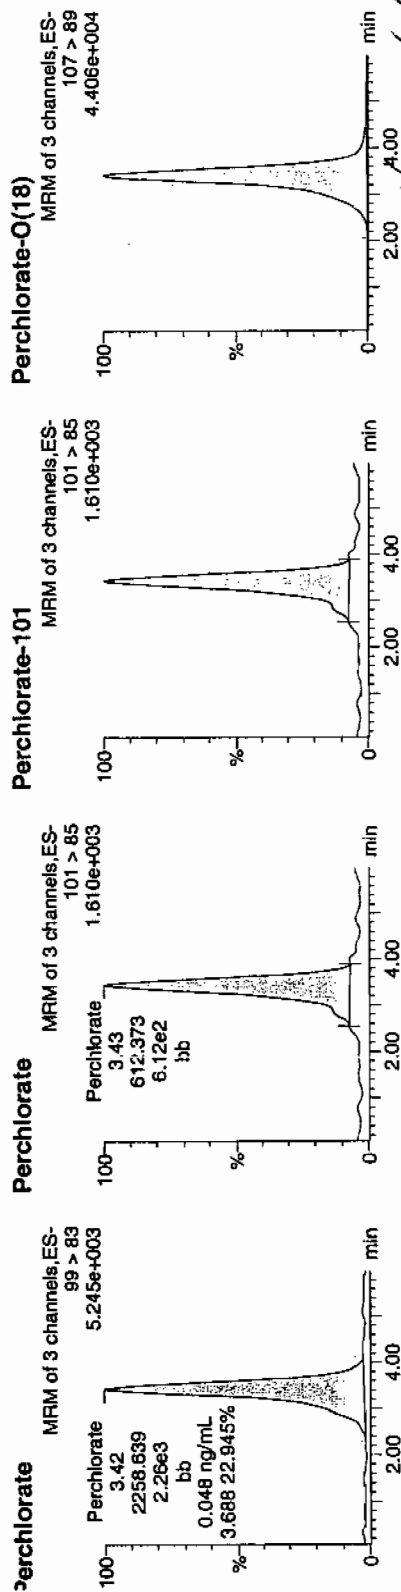

ID	Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	S/N	Ion Ratio
WCL100227-07CRI	Perchlorate	99 > 83	3.42	2258.639	2258.639	bb			0.0480	96.02	-3.98	390.282	3.69
WCL100227-07CRI	Perchlorate-101	101 > 85	3.43	612.373	612.373	bb			0.0428	85.66	-14.34	48.257	
WCL100227-07CRI	Perchlorate-O(18)	107 > 89	3.42	20100.334	20100.334	bb			0.5147	102.95	2.95	5432.1...	

QUALITY CONTROL

Form 1

Perchlorate Analysis Data Sheet

Lab Name: GEL Laboratories LLC
 Lab Code: GEL
 Instrument: LCMSMS
 Method: EPA 6850 Modified
 Matrix: WATER
 Extraction Batch ID: 959046
 Extraction Type: Filter/DAI
 Client Sample No. MB
 Date Received: 05-MAR-10
 GEL Job No (SDG): 10-2093
 GEL Sample ID: 1202056715
 Date Filtered: 05-MAR-10
 Injection Volume (uL): 20
 %Solids:

Sample Volume/Weight: 10.0 mL

Concentrated Extract Volume: 10.0

CAS No.	Analyte [^]	MDL	RL	Conc*	Units	Q	Dilution Factor	Date Analyzed	GEL File ID
14797-73-0	Perchlorate	.05	.2	0.050	ug/L	U	1	09-MAR-10 07:47	per0308107a
	Perchlorate Isotope Ratio						1	09-MAR-10 07:47	per0308107a
14797-73-0	Perchlorate-101	.05	.2	0.050	ug/L	U	1	09-MAR-10 07:47	per0308107a
	Perchlorate-O(18)			0.447	ug/L		1	09-MAR-10 07:47	per0308107a

[^] When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

*Concentration =
 Instrument Value X Concentrated Extract Volume X ¹
 Aliquot %Solids

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time


Name: per0308107a

Date: 09-Mar-2010

Time: 07:47:57

ID: 1202056715

Vial: 3:1,A

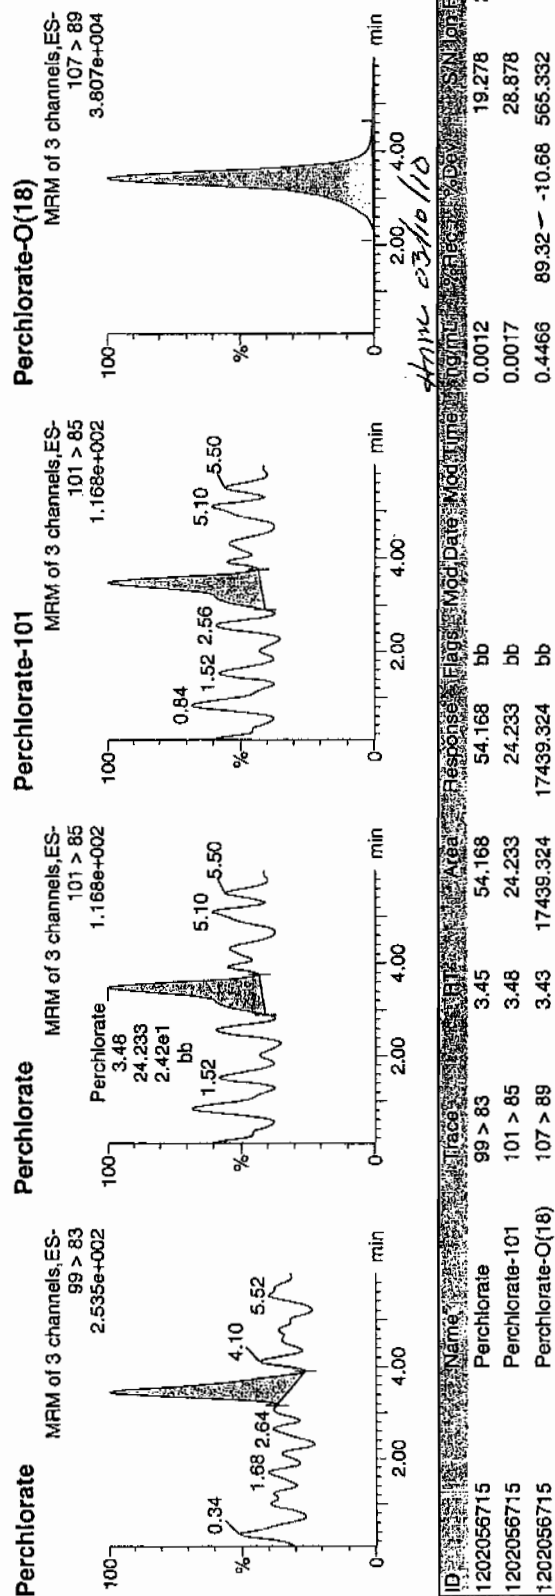

00507
4672

Perchlorate Analysis Data Sheet

Lab Name: GEL Laboratories LLC

Lab Code: GEL

Instrument: LCMSMS

Method: EPA 6850 Modified

Matrix: WATER

Extraction Batch ID: 959046

Extraction Type: Filter/DAI

Sample Volume/Weight: 10.0 mL

Concentrated Extract Volume: 10.0

Client Sample No.

LCS

Date Received: 05-MAR-10

GEL Job No (SDG): 10-2093

GEL Sample ID: 1202056716

Date Filtered: 05-MAR-10

Injection Volume (uL): 20

%Solids:

CAS No.	Analyte [^]	MDL	RL	Conc*	Units	Q	Dilution Factor	Date Analyzed	GEL File ID
14797-73-0	Perchlorate	.05	.2	0.187	ug/L	J	1	09-MAR-10 07:57	per0308108a
	Perchlorate Isotope Ratio			3.13			1	09-MAR-10 07:57	per0308108a
14797-73-0	Perchlorate-101	.05	.2	0.197	ug/L	J	1	09-MAR-10 07:57	per0308108a
	Perchlorate-O(18)			0.450	ug/L		1	09-MAR-10 07:57	per0308108a

[^] When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

*Concentration =

Instrument Value X Concentrated Extract Volume X 1 %Solids
Aliquot

Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charlers W. Wilson


Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308108a
Date: 09-Mar-2010
Time: 07:57:12
ID: 1202056716
Vial: 3:1,B

Lawrence / 12/22/10

03-01-10

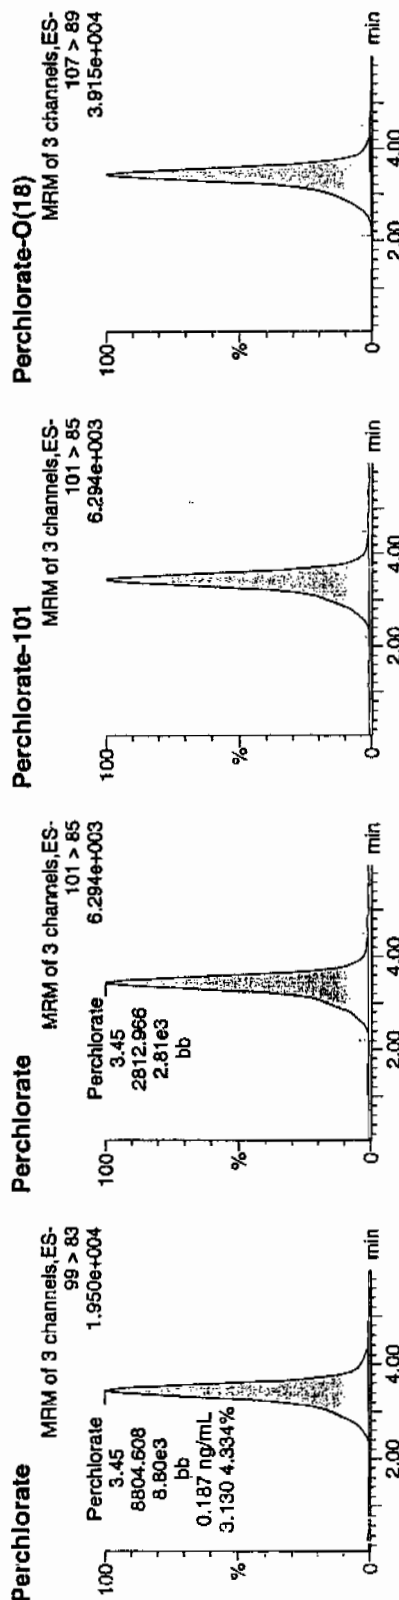

ID	Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	S/N	Ion Ratio
1202056716	Perchlorate	99 > 83	3.45	8804.608	8804.608	bb			0.1871	93.57	-6.43	837.751	3.13
1202056716	Perchlorate-101	101 > 85	3.45	2812.966	2812.966	bb			0.1968	98.38	-1.62	753.206	
1202056716	Perchlorate-O(18)	107 > 89	3.43	17560.795	17560.795	bb			0.4497	89.94	-10.06	1081.8...	

8804.608
47047.4
= 0.1871
HMP 03/10/10

MISCELLANEOUS DATA

Prep Logbook

Definitive Low Level Perchlorate Analysis Utilizing Liquid Chromatography/Mass Spectrometry/Mass Spectrometry (LC/MS/MS) by EPA Method 6850 Modified (6850M)

Batch ID: 959046
 Analyst: Kaylie Westmoreland
 Method: SW846 6850 Modified
 Verified by:
 Lab SOP: GL-OA-E-067 REV# 6
 Instrument: MicroMass Quattro Ultima

Sample ID	Run Date	Initial Volume (mL)	Final Volume (mL)	Prepped Factor (mL/mL)
1203056715 MB	05-MAR-2010 15:17:00	10	10	1
1203056716 LCS	05-MAR-2010 15:17:00	10	10	1
248108001	05-MAR-2010 15:17:00	10	10	1
248117001	05-MAR-2010 15:17:00	10	10	1
248127001	05-MAR-2010 15:17:00	10	10	1
248127002	05-MAR-2010 15:17:00	10	10	1
248162001	05-MAR-2010 15:17:00	10	10	1
248162002	05-MAR-2010 15:17:00	10	10	1
1203056717 MS (248162002)	05-MAR-2010 15:17:00	10	10	1
1203056718 MSD (248162002)	05-MAR-2010 15:17:00	10	10	1
248162003	05-MAR-2010 15:17:00	10	10	1
248162004	05-MAR-2010 15:17:00	10	10	1
248168006	05-MAR-2010 15:17:00	10	10	1
248169004	05-MAR-2010 15:17:00	10	10	1
248188001	05-MAR-2010 15:17:00	10	10	1
248199001	05-MAR-2010 15:17:00	10	10	1
248238001	05-MAR-2010 15:17:00	10	10	1
248238002	05-MAR-2010 15:17:00	10	10	1
248242001	05-MAR-2010 15:17:00	10	10	1
248245001	05-MAR-2010 15:17:00	10	10	1
248257001	05-MAR-2010 15:17:00	10	10	1
248257002	05-MAR-2010 15:17:00	10	10	1
248261001	05-MAR-2010 15:17:00	10	10	1
1203056719 LCS	05-MAR-2010 15:17:00	10	10	1

Comments:

Desulphing Cartridges used: 100224-1-Ba & 100217-1-H

Type	Sample Id	Description	Serial Number	Spike Amt	Units
ICS	1203056719	10 ug/L ICVACV Second Source	UCL100226-01.1	2	mL
LCS	1203056716	10 ug/L ICVACV Second Source	UCL100226-01.1	2	mL
MS	1203056717	10 ug/L ICVACV Second Source	UCL100226-01.1	2	mL
MSD	1203056718	10 ug/L ICVACV Second Source	UCL100226-01.1	2	mL
ICVACV	All	500 ppm Carbonate, Bicarbonate, Chloride, Sulfate	1267890	10	mL
ICVACV	All	0.25M HCl (Grade Water)	1271940	10	mL

GEL ORGANIC RUN LOG

INSTRUMENT ID: LCMSMS#2

Date: 03/07/10

Extr. Injection Volume: 20uL

Sequence Number: per030710a

Initial Calibration Date: 03/07/10

Method: EPA 6850-Modified

Int. Std.: UCL100126-01

Mobile Phase Lot#: 1278688, 1271949

Standard-Samp Reagent Lot#: 1271949

Reviewed BY: *Ham*
Date: 03/10/10
SOP: GL-OA-E-067 Rev.6
Alt Check Std. ID: WCL100227-06

DataFile	Sample	Analyst	Injection Date	Batch	SDG	Dilution	Client	Comments	QC_Flag
per0308001a	IPB001	CWW	3/8/2010 15:44			1		USE	B
per0308002a	IPB001	CWW	3/8/2010 15:53			1		USE	B
per0308003a	WCLICAL-01	CWW	3/8/2010 16:02			1		USE	I
per0308004a	WCLICAL-02	CWW	3/8/2010 16:11			1		USE	I
per0308005a	WCLICAL-03	CWW	3/8/2010 16:20			1		USE	I
per0308006a	WCLICAL-04	CWW	3/8/2010 16:29			1		USE	I
per0308007a	WCLICAL-05	CWW	3/8/2010 16:39			1		USE	I
per0308008a	IPB002	CWW	3/8/2010 16:48			1		USE	B
per0308009a	WCLICV	CWW	3/8/2010 16:57			1		USE	C
per0308010a	IPB003	CWW	3/8/2010 17:06			1		USE	B
per0308011a	WCLCRI	CWW	3/8/2010 17:15			1		USE	C
per0308012a	246870009	CWW	3/8/2010 17:24	955688	10-1782	1	LANL	USE	S
per0308013a	246870010	CWW	3/8/2010 17:33	955688	10-1782	1	LANL	USE	S
per0308014a	246982001	CWW	3/8/2010 17:42	955688	10-1812	1	LANL	USE	S
per0308015a	246982002	CWW	3/8/2010 17:51	955688	10-1812	1	LANL	USE	S
per0308016a	246982003	CWW	3/8/2010 18:01	955688	10-1812	1	LANL	USE	S
per0308017a	246982004	CWW	3/8/2010 18:10	955688	10-1812	1	LANL	USE	S
per0308018a	246982005	CWW	3/8/2010 18:19	955688	10-1812	1	LANL	USE	S
per0308019a	246982006	CWW	3/8/2010 18:28	955688	10-1812	1	LANL	USE	S
per0308020a	246982007	CWW	3/8/2010 18:37	955688	10-1812	1	LANL	USE	S
per0308021a	WCLCCV	CWW	3/8/2010 18:46			1		USE	C
per0308022a	IPB004	CWW	3/8/2010 18:55			1		USE	B
per0308023a	WCLCRI	CWW	3/8/2010 19:04			1		USE	C
per0308024a	1202049003	CWW	3/8/2010 19:13	955691	10-1809	1	LANL	USE	S
per0308025a	1202049004	CWW	3/8/2010 19:22	955691	10-1809	1	LANL	USE	S
per0308026a	1202049007	CWW	3/8/2010 19:31	955691	10-1809	1	LANL	USE	S
per0308027a	246974001	CWW	3/8/2010 19:40	955691	10-1809	1	LANL	USE	S
per0308028a	1202049005	CWW	3/8/2010 19:49	955691	10-1809	1	LANL	USE	S
per0308029a	1202049006	CWW	3/8/2010 19:58	955691	10-1809	1	LANL	USE	S

per0308030a	246974002	CWW	3/8/2010 20:07	955691	10-1809	1	LANL	USE	S
per0308031a	246974003	CWW	3/8/2010 20:16	955691	10-1809	1	LANL	USE	S
per0308032a	246974004	CWW	3/8/2010 20:26	955691	10-1809	1	LANL	USE	S
per0308033a	246974005	CWW	3/8/2010 20:35	955691	10-1809	1	LANL	USE	S
per0308034a	WCLCCV	CWW	3/8/2010 20:44			1		USE	C
per0308035a	IPB005	CWW	3/8/2010 20:53			1		USE	B
per0308036a	WCLCRI	CWW	3/8/2010 21:02			1		USE	C
per0308037a	246974006	CWW	3/8/2010 21:11	955691	10-1809	1	LANL	USE	S
per0308038a	246974007	CWW	3/8/2010 21:20	955691	10-1809	1	LANL	USE	S
per0308039a	246974008	CWW	3/8/2010 21:29	955691	10-1809	1	LANL	USE	S
per0308040a	246974009	CWW	3/8/2010 21:38	955691	10-1809	1	LANL	USE	S
per0308041a	246974010	CWW	3/8/2010 21:47	955691	10-1809	1	LANL	USE	S
per0308042a	246974011	CWW	3/8/2010 21:56	955691	10-1809	1	LANL	USE	S
per0308043a	246974012	CWW	3/8/2010 22:05	955691	10-1809	1	LANL	USE	S
per0308044a	246974013	CWW	3/8/2010 22:14	955691	10-1809	1	LANL	USE	S
per0308045a	246974014	CWW	3/8/2010 22:23	955691	10-1809	1	LANL	USE	S
per0308046a	246974015	CWW	3/8/2010 22:32	955691	10-1809	1	LANL	USE	S
per0308047a	WCLCCV	CWW	3/8/2010 22:42			1		USE	C
per0308048a	IPB006	CWW	3/8/2010 22:51			1		USE	B
per0308049a	WCLCRI	CWW	3/8/2010 23:00			1		USE	C
per0308050a	246974016	CWW	3/8/2010 23:09	955691	10-1809	1	LANL	USE	S
per0308051a	246974017	CWW	3/8/2010 23:18	955691	10-1809	1	LANL	USE	S
per0308052a	IPB007	CWW	3/8/2010 23:27			1		USE	B
per0308053a	1202049064	CWW	3/8/2010 23:36	955724	VARIOUS	1	LANL	USE	S
per0308054a	1202049065	CWW	3/8/2010 23:46	955724	VARIOUS	1	LANL	USE	S
per0308055a	1202049068	CWW	3/8/2010 23:55	955724	VARIOUS	1	LANL	USE	S
per0308056a	246964002	CWW	3/9/2010 0:04	955724	10-1802	1	LANL	USE	S
per0308057a	246964004	CWW	3/9/2010 0:13	955724	10-1802	1	LANL	USE	S
per0308058a	246967001	CWW	3/9/2010 0:22	955724	10-1807	1	LANL	USE	S
per0308059a	246967004	CWW	3/9/2010 0:31	955724	10-1807	1	LANL	DUSE-DL	S
per0308060a	WCLCCV	CWW	3/9/2010 0:40			1		USE	C
per0308061a	IPB008	CWW	3/9/2010 0:50			1		USE	B
per0308062a	WCLCRI	CWW	3/9/2010 0:59			1		USE	C
per0308063a	247036002	CWW	3/9/2010 1:08	955724	10-1826	1	LANL	USE	S
per0308064a	247036003	CWW	3/9/2010 1:17	955724	10-1826	1	LANL	USE	S
per0308065a	247036006	CWW	3/9/2010 1:26	955724	10-1826	1	LANL	USE	S
per0308066a	247037001	CWW	3/9/2010 1:35	955724	10-1823	1	LANL	DUSE-DL	S

per0308067a	247042002	CWW	3/9/2010 1:44	955724	10-1817	1	LANL	DUSE-RA	S
per0308068a	247042004	CWW	3/9/2010 1:53	955724	10-1817	1	LANL	USE	S
per0308069a	247042006	CWW	3/9/2010 2:02	955724	10-1817	1	LANL	USE	S
per0308070a	247261004	CWW	3/9/2010 2:11	955724	10-1886	1	LANL	USE	S
per0308071a	1202049066	CWW	3/9/2010 2:20	955724	10-1886	1	LANL	USE	S
per0308072a	1202049067	CWW	3/9/2010 2:29	955724	10-1886	1	LANL	USE	S
per0308073a	WCLCCV	CWW	3/9/2010 2:38			1		USE	C
per0308074a	IPB009	CWW	3/9/2010 2:48			1		USE	B
per0308075a	WCLCRI	CWW	3/9/2010 2:57			1		USE	C
per0308076a	1202056710	CWW	3/9/2010 3:06	959044	VARIOUS	1	LANL	USE	S
per0308077a	1202056711	CWW	3/9/2010 3:15	959044	VARIOUS	1	LANL	USE	S
per0308078a	1202056714	CWW	3/9/2010 3:24	959044	VARIOUS	1	LANL	USE	S
per0308079a	247908001	CWW	3/9/2010 3:33	959044	10-2013-1	1	LANL	USE	S
per0308080a	1202056712	CWW	3/9/2010 3:42	959044	10-2013-1	1	LANL	USE	S
per0308081a	1202056713	CWW	3/9/2010 3:51	959044	10-2013-1	1	LANL	USE	S
per0308082a	247908002	CWW	3/9/2010 4:00	959044	10-2013-1	1	LANL	USE	S
per0308083a	247908003	CWW	3/9/2010 4:09	959044	10-2013-1	1	LANL	USE	S
per0308084a	247919001	CWW	3/9/2010 4:18	959044	10-2016-1	1	LANL	USE	S
per0308085a	247919002	CWW	3/9/2010 4:27	959044	10-2016-1	1	LANL	USE	S
per0308086a	WCLCCV	CWW	3/9/2010 4:36			1		USE	C
per0308087a	IPB010	CWW	3/9/2010 4:46			1		USE	B
per0308088a	WCLCRI	CWW	3/9/2010 4:55			1		USE	C
per0308089a	247922004	CWW	3/9/2010 5:04	959044	10-2022	1	LANL	USE	S
per0308090a	247997001	CWW	3/9/2010 5:13	959044	10-2025	1	LANL	USE	S
per0308091a	248001001	CWW	3/9/2010 5:22	959044	10-2028	1	LANL	USE	S
per0308092a	248019001	CWW	3/9/2010 5:31	959044	10-2052	1	LANL	USE	S
per0308093a	248019002	CWW	3/9/2010 5:40	959044	10-2052	1	LANL	USE	S
per0308094a	248034001	CWW	3/9/2010 5:49	959044	10-2072-1	1	LANL	USE	S
per0308095a	248038001	CWW	3/9/2010 5:58	959044	10-2066-1	1	LANL	USE	S
per0308096a	248038002	CWW	3/9/2010 6:07	959044	10-2066-1	1	LANL	USE	S
per0308097a	248039001	CWW	3/9/2010 6:16	959044	10-2069	1	LANL	USE	S
per0308098a	248046001	CWW	3/9/2010 6:25	959044	10-2075-1	1	LANL	USE	S
per0308099a	WCLCCV	CWW	3/9/2010 6:34			1		USE	C
per0308100a	IPB011	CWW	3/9/2010 6:44			1		USE	B
per0308101a	WCLCRI	CWW	3/9/2010 6:53			1		USE	C
per0308102a	248046002	CWW	3/9/2010 7:02	959044	10-2075-1	1	LANL	USE	S
per0308103a	248053001	CWW	3/9/2010 7:11	959044	10-2081	1	LANL	USE	S

per0308104a	248053002	CWW	3/9/2010 7:20	959044	10-2081	1	LANL	USE	S
per0308105a	248053003	CWW	3/9/2010 7:29	959044	10-2081	1	LANL	USE	S
per0308106a	IPB012	CWW	3/9/2010 7:38			1		USE	B
per0308107a	1202056715	CWW	3/9/2010 7:47	959047	VARIOUS	1	LANL	USE	S
per0308108a	1202056716	CWW	3/9/2010 7:57	959047	VARIOUS	1	LANL	USE	S
per0308109a	1202056719	CWW	3/9/2010 8:06	959047	VARIOUS	1	LANL	USE	S
per0308110a	248108001	CWW	3/9/2010 8:15	959047	10-2090	1	LANL	USE	S
per0308111a	248117001	CWW	3/9/2010 8:24	959047	10-2093	1	LANL	USE	S
per0308112a	WCLCCV	CWW	3/9/2010 8:33			1		USE	C
per0308113a	IPB013	CWW	3/9/2010 8:42			1		USE	B
per0308114a	WCLCRI	CWW	3/9/2010 8:51			1		USE	C
per0308115a	248127001	CWW	3/9/2010 9:00	959047	10-2096	1	LANL	USE	S
per0308116a	248127002	CWW	3/9/2010 9:09	959047	10-2096	1	LANL	USE	S
per0308117a	248162001	CWW	3/9/2010 9:18	959047	10-2103	1	LANL	USE	S
per0308118a	248162002	CWW	3/9/2010 9:27	959047	10-2103	1	LANL	USE	S
per0308119a	1202056717	CWW	3/9/2010 9:37	959047	10-2103	1	LANL	USE	S
per0308120a	1202056718	CWW	3/9/2010 9:46	959047	10-2103	1	LANL	USE	S
per0308121a	248162003	CWW	3/9/2010 9:55	959047	10-2103	1	LANL	USE	S
per0308122a	248162004	CWW	3/9/2010 10:04	959047	10-2103	1	LANL	USE	S
per0308123a	248168006	CWW	3/9/2010 10:13	959047	10-2107	1	LANL	USE	S
per0308124a	248169004	CWW	3/9/2010 10:22	959047	10-2108	1	LANL	USE	S
per0308125a	WCLCCV	CWW	3/9/2010 10:31			1		USE	C
per0308126a	IPB014	CWW	3/9/2010 10:40			1		USE	B
per0308127a	WCLCRI	CWW	3/9/2010 10:49			1		USE	C
per0308128a	248188001	CWW	3/9/2010 10:58	959047	10-2120	1	LANL	USE	S
per0308129a	248199001	CWW	3/9/2010 11:07	959047	10-2122-1	1	LANL	USE	S
per0308130a	248238001	CWW	3/9/2010 11:16	959047	10-2132-1	1	LANL	USE	S
per0308131a	248238002	CWW	3/9/2010 11:25	959047	10-2132-1	1	LANL	USE	S
per0308132a	248242001	CWW	3/9/2010 11:34	959047	10-2135-1	1	LANL	USE	S
per0308133a	248245001	CWW	3/9/2010 11:43	959047	10-2138	1	LANL	USE	S
per0308134a	248257001	CWW	3/9/2010 11:52	959047	10-2146-1	1	LANL	USE	S
per0308135a	248257002	CWW	3/9/2010 12:02	959047	10-2146-1	1	LANL	USE	S
per0308136a	248261001	CWW	3/9/2010 12:11	959047	10-2149	1	LANL	USE	S
per0308137a	WCLCCV	CWW	3/9/2010 12:20			1		USE	C
per0308138a	IPB015	CWW	3/9/2010 12:29			1		USE	B
per0308139a	WCLCRI	CWW	3/9/2010 12:38			1		USE	C

Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charfers W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308119a

Date: 09-Mar-2010


Time: 09:37:00

ID: 1202056717

Vial: 3:2,D

03-09-10

1202056717 1202056717 1202056717

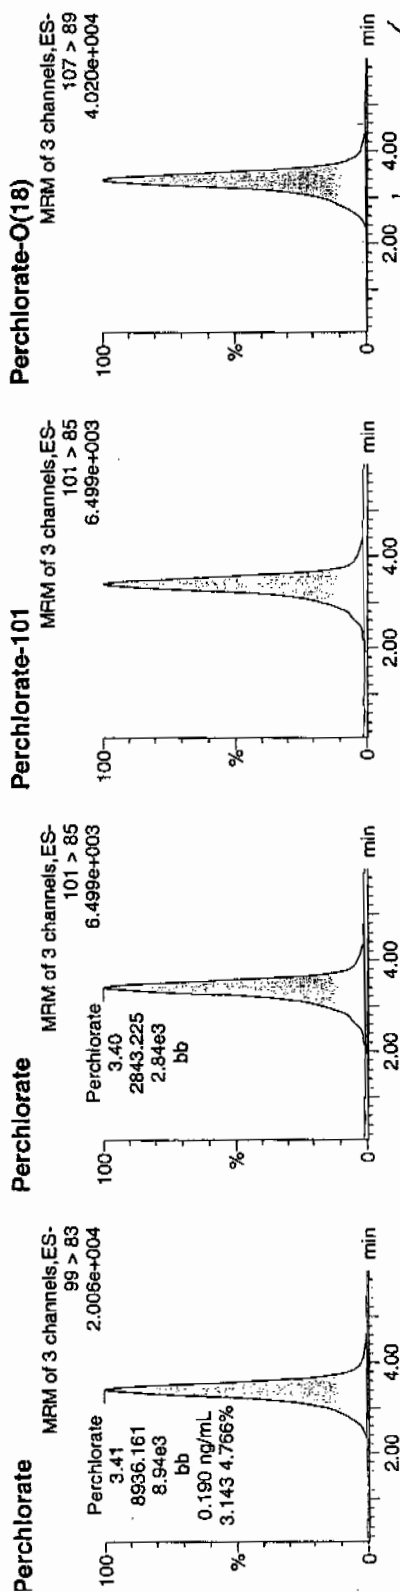

ID	Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	S/N	Ion Ratio
1202056717	Perchlorate	99 > 83	3.41	8936.161	8936.161	bb			0.1899	94.97	-5.03	309.674	3.14
1202056717	Perchlorate-101	101 > 85	3.40	2843.225	2843.225	bb			0.1989	99.43	-0.57	415.047	
1202056717	Perchlorate-O(18)	107 > 89	3.38	17994.619	17994.619	bb			0.4608	92.16	-7.84	888.553	

Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charlers W. Wilson


Dataset: C:\MassLynx\Perchlorate.PRO\per030810a.qld

Last Altered: Tuesday, March 09, 2010 12:57:27 PM Eastern Standard Time
Printed: Tuesday, March 09, 2010 1:04:52 PM Eastern Standard Time

Name: per0308120a
Date: 09-Mar-2010
Time: 09:46:02
ID: 1202056718
Vial: 3:2,E

03 29-10

1202056718 | 1202056718 | 1202056718

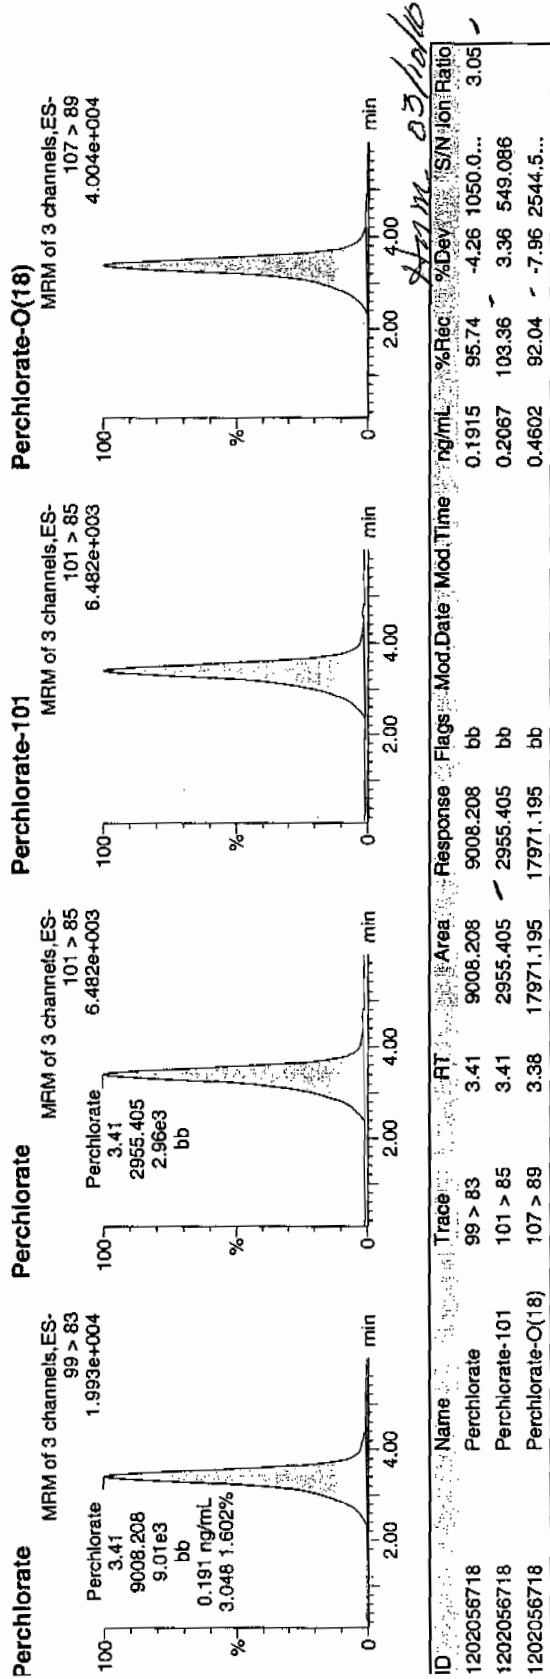

Isotope Ratio Criteria

Isotope Ratio $^{35}\text{Cl}/^{37}\text{Cl}$

2.31-3.85

Tune Criteria

The tuning solution is introduced directly into the mass spectrometer using the ESI interface in the positive ion mode. The mass range scanned is 20 to 1100 amu using at least six scans. The observed mass for the target compound in the daily calibration standards must be within 0.2 amu of the expected value. If it is greater than 0.2 amu, then a mass calibration is performed and the instrument is re-calibrated.

LC/MS/MS PERCHLORATE ANALYSIS

**Perchlorate by LC/MSMS
Los Alamos National Laboratory (LANL)
SDG 10-2093-1**

Method/Analysis Information

Procedure: **Definitive Low Level Perchlorate Analysis Utilizing Liquid Chromatography/Mass Spectrometry/Mass Spectrometry (LC/MS/MS) by EPA Method 6850 Modified (6850M)**

Analytical Method: SW846 6850 Modified

Prep Method: SW846 6850 Modified

Analytical Batch Number: 959012

Prep Batch Number: 959007

Sample Analysis

Sample ID	Client ID
248118001	RE36-10-8448
248118002	RE36-10-8456
248118003	RE36-10-8451
248118004	RE36-10-8450
248118005	RE36-10-8449
248118006	RE36-10-8453
248118007	RE36-10-8452
1202056681	Interference Check Sample (ICS)
1202056676	Method Blank (MB)
1202056677	Laboratory Control Sample (LCS)
1202056678	248198001(RE36-10-7405) Matrix Spike (MS)
1202056679	248198001(RE36-10-7405) Matrix Spike Duplicate (MSD)

The samples in this SDG were analyzed on a "dry weight" basis.

10-2093-1-PERLCMS

Page 1 of 4

Preparation/Analytical Method Verification

SOP Reference

Procedure for preparation, analysis and reporting of analytical data are controlled by GEL Laboratories LLC as Standard Operating Procedure (SOP). The data discussed in this narrative has been analyzed in accordance with GL-OA-E-067 REV# 6.

Calibration Information

Initial Calibration

All initial calibration requirements have been met for this SDG. Due to software constraints, all Initial Calibration Blanks must be designated as IPB001.

CCV Requirements

All associated calibration verification standard(s) (ICV or CCV) met the acceptance criteria.

CCB Requirements

All continuing calibration blanks (CCB) bracketing the analyses associated with this batch were within acceptance criteria.

CCV Requirements

All continuing calibration checks (CCV) requirements were met by all bracketing CCV standards.

Low Level Standard (CRI) Requirements

All low level calibration verification (CRI) requirements were met by all bracketing CRI standards.

Quality Control (QC) Information

Method Blank (MB) Statement

The MB(s) analyzed with this SDG met the acceptance criteria.

Interference Check Sample (ICS)

The interference check sample (ICS) met all recovery acceptance criteria.

Laboratory Control Sample (LCS) Recovery

The LCS spike recoveries met the acceptance limits.

QC Sample Designation

Client sample 248198001 (RE36-10-7405) from SDG 10-2122 was chosen for matrix spike and matrix spike duplicate analysis. Please see the raw data in the Miscellaneous Section.

Matrix Spike (MS) Recovery Statement

The MS recovered Perchlorate-101 at 127% and the acceptance range is 75-125%. The high recovery may be the result of the background concentration present in the parent sample, 248198001 (RE36-10-7405), and the need to dilute all at 1:2 prior to analysis. Please see data exception report 807337.

Matrix Spike Duplicate (MSD) Recovery Statement

The MSD recoveries were within the established acceptance limits.

MS/MSD Relative Percent Difference (RPD) Statement

The RPD(s) between the MS and MSD met the acceptance limits.

10-2093-1-PERLCMS

Page 2 of 4

Retention Time Standard Area Acceptance

The retention time standard areas were within the required acceptance criteria for all samples and QC.

Retention Time

During the analysis of Perchlorate by LC/MS/MS, retention time shifts are commonly observed. These retention time shifts, which are caused by fouling of the column by the sample matrices, are problematic when the retention time is used as one of the criterion for confirmation. To overcome this problem, a known amount of O(18) labeled Perchlorate was added to each sample as a retention time standard. The presence of Perchlorate was confirmed by the relative retention time (RRT) of the Perchlorate peak and the O(18) standard. A RRT window of 0.98 to 1.02, as required by Method 332.0, has been used. In addition to the isotopic ratio, the presence of Perchlorate in the samples associated with this data package have been confirmed using the relative retention criteria stated above, not the absolute retention time.

Technical Information

Holding Time Specifications

All samples in this SDG in this analytical batch met the specified holding time. GEL assigns holding times based on the associated methodology, which assigns the date and time from sample collection of sample receipt. Those holding times expressed in hours are calculated in the AlphaLIMS system. Those holding times expressed as days expire at midnight on the day of expiration.

Preparation/Analytical Method Verification

All procedures were performed as stated in the SOP.

Sample Dilutions

The samples in this SDG did not require dilutions.

Sample Re-extraction/Re-analysis

Re-extractions or re-analyses were not required in this SDG except for dilutions.

Miscellaneous Information

Data Exception (DER) Documentation

Data exception report 807337 was generated for this SDG.

The MS recovered Perchlorate-101 at 127% and the acceptance range is 75-125%. The high recovery may be the result of the background concentration present in the parent sample, 248198001 (RE36-10-7405), and the need to dilute all at 1:2 prior to analysis.

Manual Integrations

Some initial calibration standards, continuing calibration standards, and/or samples may require manual integrations due to software limitations.

Method Comments

The samples in this SDG were not originally analyzed using EPA Method 314.0.

Additional Comments

The Perchlorate Isotope Ratio on the Form I may differ slightly from the ratio on the corresponding raw data due to rounding rules and/or significant figures or due to software limitations when there are manual integrations, dilutions or other factors. The ratio value of the Form I is the correct value.

The retention time marker, Perchlorate-O (18), is added to all samples, instrument blanks, and standards prior to injection. It is used to verify the retention time of Perchlorate and Perchlorate-101 and to insure an accurate injection occurred. Due to various anions affecting the recovery of Perchlorate-O (18) and not Perchlorate and Perchlorate-101, the calibration curves of Perchlorate and Perchlorate-101 are not internally corrected for using Perchlorate-O (18). They are external calibrations.

Perchlorate Isotope Ratio

The Perchlorate isotope ratio met acceptance criteria for all samples and QC samples. Please see the isotope ratio criteria in the Miscellaneous Section.

System Configuration

The laboratory utilizes a Waters LC 2795 liquid chromatography instrument for perchlorate analysis. It is coupled with either a Micromass Quattro Micro Mass Spectrometer/ Mass Spectrometer, or a Micromass Quattro Ultima Mass Spectrometer/ Mass Spectrometer. Each being designated as LCMSMS #1, and LCMSMS #2, respectively. It is fitted with an electrospray probe that is operated in the negative electrospray ionization mode for perchlorate analysis. The laboratory may also utilize an Agilent 1100 liquid chromatography instrument for perchlorate analysis. It is coupled with an Applied Biosystems 4000 Mass Spectrometer/ Mass Spectrometer, designated as LCMSMS #3 or LCMSMS #4. It is also fitted with an electrospray probe that is operated in the negative electrospray ionization mode for perchlorate analysis.

Chromatographic Columns

Chromatographic separation of perchlorate is accomplished through analysis on the following anion column:

Dionex: IonPac AG-16 2 x 50 mm.

Certification Statement

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless otherwise noted in the analytical case narrative.

Review Validation:

GEL requires all analytical data to be verified by a qualified data validator. In addition, all data designated for CLP or CLP-like packaging will receive a third level validation upon completion of the data package.

The following data validator verified the information presented in this case narrative:

Reviewer: Heather K. Mauer

Date: 03/23/10

10-2093-1-PERLCMS

Page 4 of 4

SAMPLE DATA SUMMARY

Perchlorate Analysis Data Sheet

Lab Name: GEL Laboratories LLC
 Lab Code: GEL
 Instrument: LCMSMS
 Method: SW846 6850 Modified
 Matrix: SOIL
 Extraction Batch ID: 959007
 Extraction Type: Solid Prep
 Client Sample No. RE36-10-8448
 Date Received: 26-FEB-10
 GEL Job No (SDG): 10-2093-1
 GEL Sample ID: 248118001
 Date Filtered: 12-MAR-10
 Injection Volume (uL): 20
 % Solids: 97.3

Sample Volume/Weight: 2.00 g

Concentrated Extract Volume: 20.0

CAS No.	Analyte [^]	MDL	RL	Conc*	Units	Q	Dilution Factor	Date Analyzed	GEL File ID
14797-73-0	Perchlorate	.514	2.05	0.514	ug/kg	U	1	19-MAR-10 13:07	per0319015a
	Perchlorate Isotope Ratio						1	19-MAR-10 13:07	per0319015a
14797-73-0	Perchlorate-101	.514	2.05	0.514	ug/kg	U	1	19-MAR-10 13:07	per0319015a
	Perchlorate-O(18)			4.89	ug/kg		1	19-MAR-10 13:07	per0319015a

[^] When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

*Concentration =

Instrument Value X $\frac{\text{Concentrated Extract Volume}}{\text{Aliquot}}$ X $\frac{1}{\% \text{Solids}}$

Form 1

Perchlorate Analysis Data Sheet

Lab Name: GEL Laboratories LLC

Lab Code: GEL

Instrument: LCMSMS

Method: SW846 6850 Modified

Matrix: SOIL

Extraction Batch ID: 959007

Extraction Type: Solid Prep

Sample Volume/Weight: 2.00 g

Concentrated Extract Volume: 20.0

Client Sample No.

RE36-10-8456

Date Received: 26-FEB-10

GEL Job No (SDG): 10-2093-1

GEL Sample ID: 248118002

Date Filtered: 12-MAR-10

Injection Volume (uL): 20

%Solids: 97.2

CAS No.	Analyte [^]	MDL	RL	Conc*	Units	Q	Dilution Factor	Date Analyzed	GEL File ID
14797-73-0	Perchlorate	.514	2.06	0.514	ug/kg	U	1	19-MAR-10 13:14	per0319016a
	Perchlorate Isotope Ratio						1	19-MAR-10 13:14	per0319016a
14797-73-0	Perchlorate-101	.514	2.06	0.514	ug/kg	U	1	19-MAR-10 13:14	per0319016a
	Perchlorate-O(18)			4.99	ug/kg		1	19-MAR-10 13:14	per0319016a

[^] When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

*Concentration =

Instrument Value X Concentrated Extract Volume X 1
Aliquot %Solids

Form 1

Perchlorate Analysis Data Sheet

Lab Name: GEL Laboratories LLC

Lab Code: GEL

Instrument: LCMSMS

Method: SW846 6850 Modified

Matrix: SOIL

Extraction Batch ID: 959007

Extraction Type: Solid Prep

Sample Volume/Weight: 2.00 g

Concentrated Extract Volume: 20.0

Client Sample No.

RE36-10-8451

Date Received: 26-FEB-10

GEL Job No (SDG): 10-2093-1

GEL Sample ID: 248118003

Date Filtered: 12-MAR-10

Injection Volume (uL): 20

%Solids: 97

CAS No.	Analyte [^]	MDL	RL	Conc*	Units	Q	Dilution Factor	Date Analyzed	GEL File ID
14797-73-0	Perchlorate	.516	2.06	0.516	ug/kg	U	1	19-MAR-10 13:21	per0319017a
	Perchlorate Isotope Ratio						1	19-MAR-10 13:21	per0319017a
14797-73-0	Perchlorate-101	.516	2.06	0.516	ug/kg	U	1	19-MAR-10 13:21	per0319017a
	Perchlorate-O(18)			5.11	ug/kg		1	19-MAR-10 13:21	per0319017a

[^] When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

*Concentration =

Instrument Value X $\frac{\text{Concentrated Extract Volume}}{\text{Aliquot}}$ X $\frac{1}{\% \text{Solids}}$

Form 1

Perchlorate Analysis Data Sheet

Lab Name: GEL Laboratories LLC
 Lab Code: GEL
 Instrument: LCMSMS
 Method: SW846 6850 Modified
 Matrix: SOIL
 Extraction Batch ID: 959007
 Extraction Type: Solid Prep
 Sample Volume/Weight: 2.00 g
 Concentrated Extract Volume: 20.0
 Client Sample No. RE36-10-8450
 Date Received: 26-FEB-10
 GEL Job No (SDG): 10-2093-1
 GEL Sample ID: 248118004
 Date Filtered: 12-MAR-10
 Injection Volume (uL): 20
 %Solids: 85

CAS No.	Analyte [^]	MDL	RL	Conc*	Units	Q	Dilution Factor	Date Analyzed	GEL File ID
14797-73-0	Perchlorate	.588	2.35	1.27	ug/kg	J	1	19-MAR-10 13:28	per0319018a
	Perchlorate Isotope Ratio			3.24			1	19-MAR-10 13:28	per0319018a
14797-73-0	Perchlorate-101	.588	2.35	1.14	ug/kg	J	1	19-MAR-10 13:28	per0319018a
	Perchlorate-O(18)			5.73	ug/kg		1	19-MAR-10 13:28	per0319018a

[^] When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

*Concentration =

Instrument Value X $\frac{\text{Concentrated Extract Volume}}{\text{Aliquot}}$ X $\frac{1}{\% \text{Solids}}$

Form 1

Perchlorate Analysis Data Sheet

Lab Name: GEL Laboratories LLC

Lab Code: GEL

Instrument: LCMSMS

Method: SW846 6850 Modified

Matrix: SOIL

Extraction Batch ID: 959007

Extraction Type: Solid Prep

Sample Volume/Weight: 2.00 g

Concentrated Extract Volume: 20.0

Client Sample No.

RE36-10-8449

Date Received: 26-FEB-10

GEL Job No (SDG): 10-2093-1

GEL Sample ID: 248118005

Date Filtered: 12-MAR-10

Injection Volume (uL): 20

%Solids: 98.2

CAS No.	Analyte [^]	MDL	RL	Conc*	Units	Q	Dilution Factor	Date Analyzed	GEL File ID
14797-73-0	Perchlorate	.509	2.04	0.509	ug/kg	U	1	19-MAR-10 13:35	per0319019a
	Perchlorate Isotope Ratio						1	19-MAR-10 13:35	per0319019a
14797-73-0	Perchlorate-101	.509	2.04	0.509	ug/kg	U	1	19-MAR-10 13:35	per0319019a
	Perchlorate-O(18)			4.85	ug/kg		1	19-MAR-10 13:35	per0319019a

[^] When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

*Concentration =

Instrument Value X Concentrated Extract Volume X 1
Aliquot %Solids

Form 1

Perchlorate Analysis Data Sheet

Lab Name: GEL Laboratories LLC
 Lab Code: GEL
 Instrument: LCMSMS
 Method: SW846 6850 Modified
 Matrix: SOIL
 Extraction Batch ID: 959007
 Extraction Type: Solid Prep
 Sample Volume/Weight: 2.00 g
 Concentrated Extract Volume: 20.0
 Client Sample No. RE36-10-8453
 Date Received: 26-FEB-10
 GEL Job No (SDG): 10-2093-1
 GEL Sample ID: 248118006
 Date Filtered: 12-MAR-10
 Injection Volume (uL): 20
 %Solids: 95.7

CAS No.	Analyte [^]	MDL	RL	Conc*	Units	Q	Dilution Factor	Date Analyzed	GEL File ID
14797-73-0	Perchlorate	.522	2.09	3.77	ug/kg		1	19-MAR-10 13:42	per0319020a
	Perchlorate Isotope Ratio			2.99			1	19-MAR-10 13:42	per0319020a
14797-73-0	Perchlorate-101	.522	2.09	3.67	ug/kg		1	19-MAR-10 13:42	per0319020a
	Perchlorate-O(18)			5.32	ug/kg		1	19-MAR-10 13:42	per0319020a

[^] When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

*Concentration =

Instrument Value X $\frac{\text{Concentrated Extract Volume}}{\text{Aliquot}}$ X $\frac{1}{\% \text{Solids}}$

Perchlorate Analysis Data Sheet

Lab Name: GEL Laboratories LLC

Lab Code: GEL

Instrument: LCMSMS

Method: SW846 6850 Modified

Matrix: SOIL

Extraction Batch ID: 959007

Extraction Type: Solid Prep

Sample Volume/Weight: 2.00 g

Concentrated Extract Volume: 20.0

Client Sample No.

RE36-10-8452

Date Received: 26-FEB-10

GEL Job No (SDG): 10-2093-1

GEL Sample ID: 248118007

Date Filtered: 12-MAR-10

Injection Volume (uL): 20

%Solids: 92.9

CAS No.	Analyte [^]	MDL	RL	Conc*	Units	Q	Dilution Factor	Date Analyzed	GEL File ID
14797-73-0	Perchlorate	.538	2.15	2.32	ug/kg		1	19-MAR-10 13:49	per0319021a
	Perchlorate Isotope Ratio			3.09			1	19-MAR-10 13:49	per0319021a
14797-73-0	Perchlorate-101	.538	2.15	2.19	ug/kg		1	19-MAR-10 13:49	per0319021a
	Perchlorate-O(18)			5.53	ug/kg		1	19-MAR-10 13:49	per0319021a

[^] When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

*Concentration =

Instrument Value X Concentrated Extract Volume X 1 %Solids
Aliquot

QUALITY CONTROL SUMMARY

Perchlorate Laboratory Control Sample

Lab Name: General Engineering Laboratories

Lab Code: GEL

GEL Job No. (SDG): 10-2093-1

Extract Batch Code: 959007

Date Filtered: 12-MAR-10

Matrix: SOIL

Sample ID: 1202056677

Analyte^	True	Found	Units	%Rec	Q	Control Limits
Perchlorate	2.00	2.03	ug/kg	101		70 - 130
Perchlorate Isotope Ratio		3.05				-
Perchlorate-101	2.00	1.94	ug/kg	96.8		70 - 130
Perchlorate-O(18)		4.91	ug/kg			-

^ When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

Perchlorate Interference Check Sample

Lab Name: General Engineering Laboratories

Lab Code: GEL

GEL Job No. (SDG): 10-2093-1

Extract Batch Code: 959007

Date Filtered: 12-MAR-10

Matrix: SOIL

Sample ID: 1202056681

Analyte [^]	True	Found	Units	%Rec	Q	Control Limits
Perchlorate	2.00	2.14	ug/kg	107		70 - 130
Perchlorate Isotope Ratio		2.88				
Perchlorate-101	2.00	2.16	ug/kg	108		70 - 130
Perchlorate-O(18)		5.05	ug/kg			

[^] When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

Dataset: C:\MassLynx\Perchlorate.PRO\per031910a.qld

Last Altered: Saturday, March 20, 2010 1:22:43 PM Eastern Standard Time
 Printed: Saturday, March 20, 2010 1:32:33 PM Eastern Standard Time

Name: per0319014a

Date: 19-Mar-2010


Time: 13:00:23

D: 1202056681

vial: 1:3,C

302210

11	ST	C2205	710656	7267
----	----	-------	--------	------

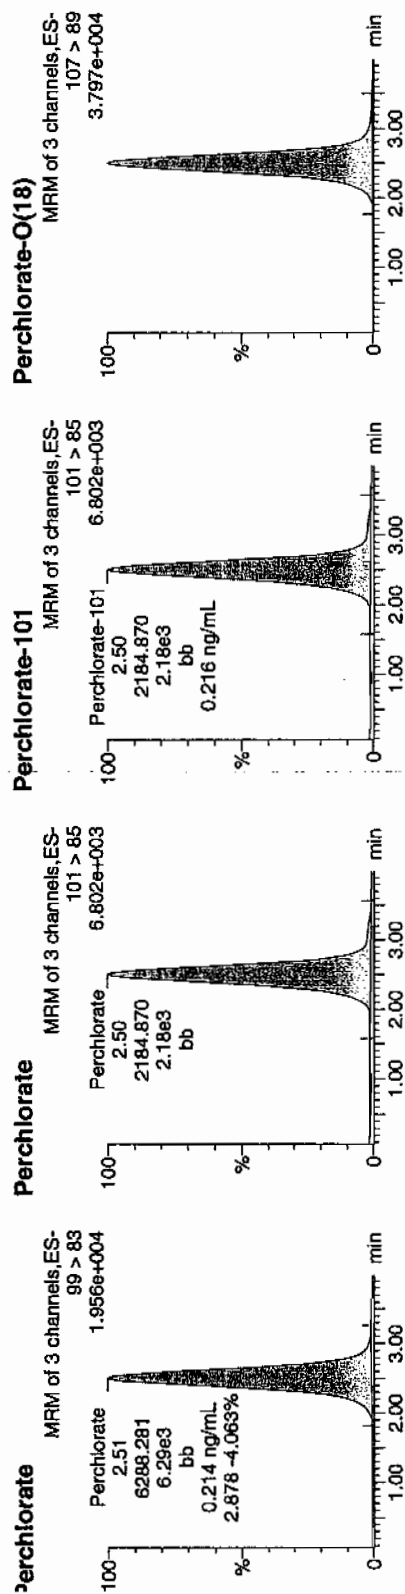

PC	Sample	Trace	RT	Area	Response	Flags	ModDate	ModTime	Op	PL	Req	De	SS	SN	OnRatio
1202056681	Perchlorate	99 > 83	2.51	6288.281	6288.281	bb			✓	0.2137	106.85	6.85	1124.6...		2.88
1202056681	Perchlorate-101	101 > 85	2.50	2184.870	2184.870	bb				0.2165	108.25	8.25	572.846		
1202056681	Perchlorate-O'(18)	107 > 89	2.50	12272.666	12272.666	bb				0.5053	101.05	1.05	3592.8...		

$$\frac{6285.281}{2184.970} = 2.8781$$

not
3/22/10

Perchlorate Spike/Spike Duplicate Summary

Lab Name: General Engineering Laboratories

Lab Code: GEL

Extract Batch Code: 959007

GEL MS/PS ID: 1202056678

GEL MSD/PSD ID: 1202056679

GEL Job No (SDG): 10-2093-1

Date Extracted: 12-MAR-10

Client ID: RE36-10-7405

QC Type: MS

Compound^	Spike Added	Sample Conc	Units	MS Conc	MS Rec	#	MSD Conc	MSD Rec	#	RPD	#	RPD Limit	Recovery Limit
Perchlorate	2.42	13.6	ug/kg	16.1	105		15.4	75.2		4.63		30	75 - 125
Perchlorate Isotope Ratio	0	0.00		3.05			3.09			0			-
Perchlorate-101	2.42	12.9	ug/kg	16.0	127 *		15.1	89.2		5.96		30	75 - 125
Perchlorate-O(18)	0	12.0	ug/kg	13.0			13			.177			-

^ When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

Comments:

Perchlorate Initial Calibration Blank

GEL Job No.(SDG): 10-2093-1

Lab Name: General Engineering Laboratories

Lab Code: GEL

Reporting Units: ug/kg

Analyte	True	Found	%Rec	Date Analyzed	GEL File Id	GEL Sample ID
Perchlorate	0.00	0	NA	19-MAR-10	per0319001a	IPB001
Perchlorate-101	0.00	0	NA	19-MAR-10	per0319001a	IPB001
Perchlorate	0.00	0	NA	19-MAR-10	per0319002a	IPB001
Perchlorate-101	0.00	0	NA	19-MAR-10	per0319002a	IPB001

Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charles W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per031910a.qld

Last Altered: Saturday, March 20, 2010 1:22:43 PM Eastern Standard Time
Printed: Saturday, March 20, 2010 1:32:33 PM Eastern Standard Time

Method: C:\MassLynx\Perchlorate.PRO\MethDB\per031910a.mdb 20 Mar 2010 13:21:43
Calibration: C:\MassLynx\Perchlorate.PRO\CurveDB\per031910a.cdb 20 Mar 2010 13:22:42

Name: per0319001a

Date: 19-Mar-2010


Time: 11:27:17

ID: 128007-172001


Vial: 1:1A

HMW 03/20/10


Perchlorate

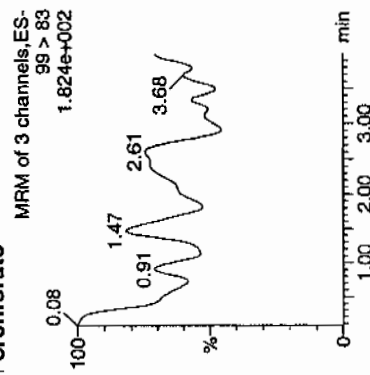


Perchlorate

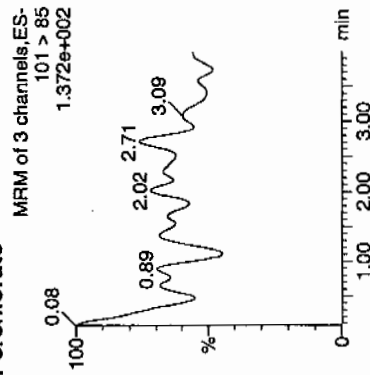

Perchlorate-101

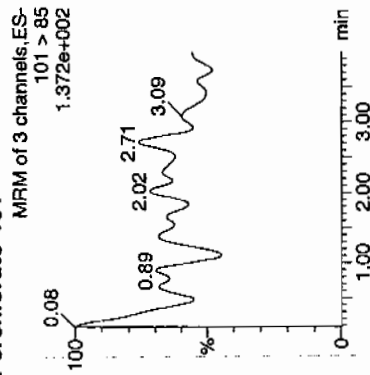

Perchlorate-O(18)

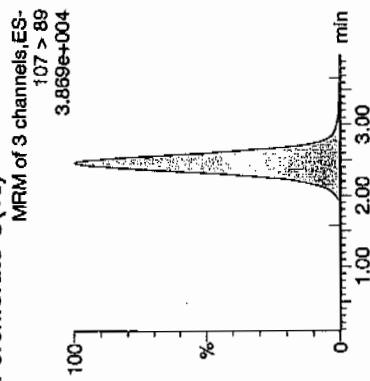

03/20/10

ID	Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	S/N	Ion Ratio
128007	Perchlorate	99 > 83											
128007	Perchlorate-101	101 > 85											
128007	Perchlorate-O(18)	107 > 89	2.46	12680.074	12680.074	bb			0.5220	104.41	4.41	1666.8...	

128007
3/22/10


128007
HMW
03/20/10

Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charles W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per031910a.qld
Last Altered: Saturday, March 20, 2010 1:22:43 PM Eastern Standard Time
Printed: Saturday, March 20, 2010 1:32:33 PM Eastern Standard Time

Name: per0319002a
Date: 19-Mar-2010
Time: 11:34:49
ID: IPB001
Vial: 1:1,A

03-20-10

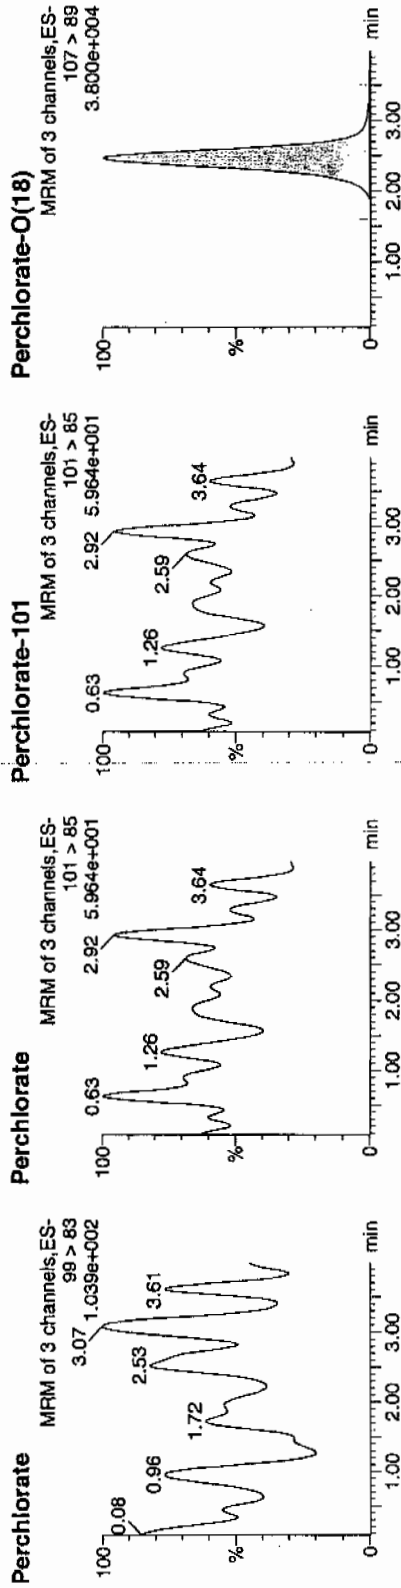

ID	Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	S/N	Ion Ratio
IPB001	Perchlorate	99 > 83											
IPB001	Perchlorate-101	101 > 85											
IPB001	Perchlorate-O(18)	107 > 89	2.46	12482.422	12482.422	bb			0.5139	102.78	✓	2.78	1649.8...

1477
3/22/10

Perchlorate Continuing Calibration Blank

GEL Job No.(SDG): 10-2093-1

Lab Name: General Engineering Laboratories

Lab Code: GEL

Reporting Units: ug/kg

Analyte	True	Found	%Rec	Date Analyzed	GEL File Id	GEL Sample ID
Perchlorate	0.00	0	NA	19-MAR-10	per0319008a	IPB002
Perchlorate-101	0.00	0	NA	19-MAR-10	per0319008a	IPB002
Perchlorate	0.00	0	NA	19-MAR-10	per0319010a	IPB003
Perchlorate-101	0.00	0	NA	19-MAR-10	per0319010a	IPB003
Perchlorate	0.00	0	NA	19-MAR-10	per0319023a	IPB004
Perchlorate-101	0.00	0	NA	19-MAR-10	per0319023a	IPB004





Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charfers W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per031910a.qld

Last Altered: Saturday, March 20, 2010 1:22:43 PM Eastern Standard Time
Printed: Saturday, March 20, 2010 1:32:33 PM Eastern Standard Time

Name: per0319008a
Date: 19-Mar-2010
Time: 12:17:20
ID: IPB002
Vial: 1:1,A

03-20-10

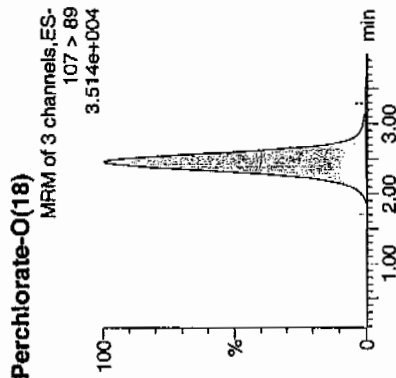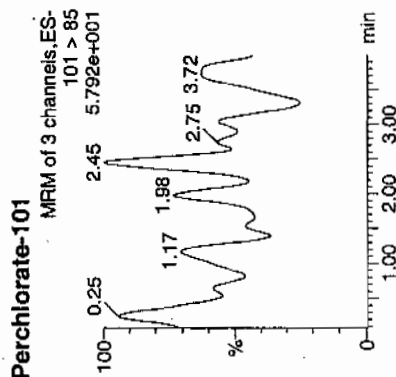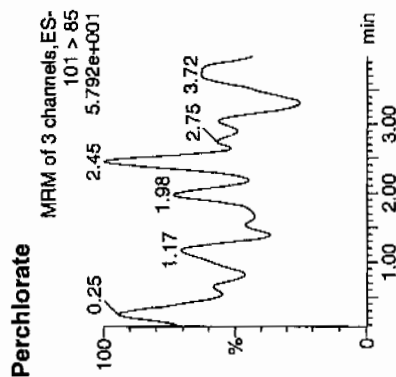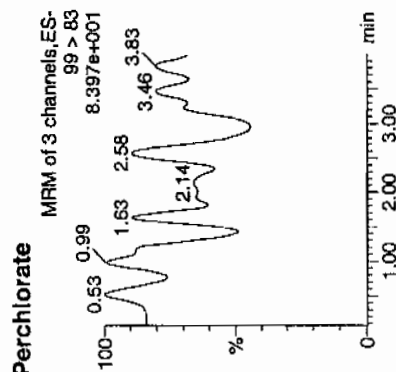

ID	Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	S/N	Ion Ratio
IPB002	Perchlorate	99 > 83											0.00
PB002	Perchlorate-101	101 > 85											
PB002	Perchlorate-O(18)	107 > 89	2.45	11463.639	11463.639	bb			0.4720	94.39	-5.61	3179.8...	

3/22/10

Quantify Sample Report MassLynx 4.0 SP4

The GEL Group, LLC Analyst: Charlers W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per031910a.qtd

Last Altered: Saturday, March 20, 2010 1:22:43 PM Eastern Standard Time

Printed: Saturday, March 20, 2010 1:32:33 PM Eastern Standard Time

Name: per0319010a

Date: 19-Mar-2010


Time: 12:31:39

ID: IPB003


Vial: 1:1,A

03-20-10


Perchlorate

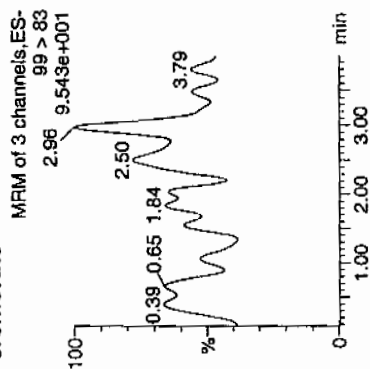


Perchlorate

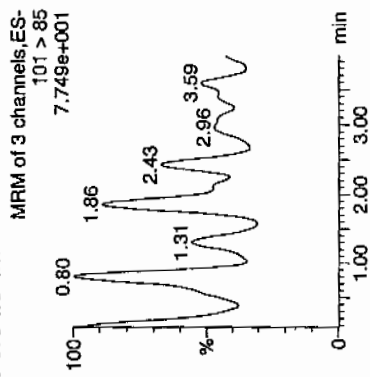

Perchlorate-101

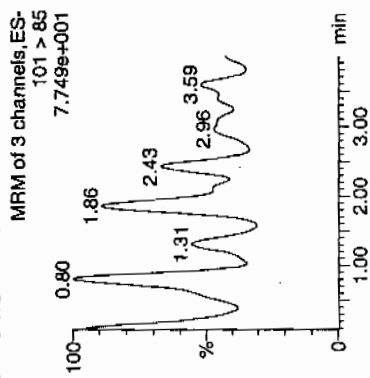

Perchlorate-O(18)

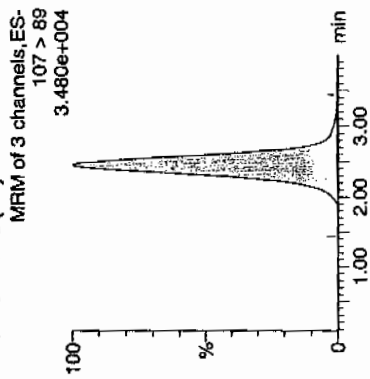

ID	Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	S/N	Ion Ratio
IPB003	Perchlorate	99 > 83											0.00
IPB003	Perchlorate-101	101 > 85											
IPB003	Perchlorate-O(18)	107 > 89	2.45	11371.736	11371.736	bb			0.4682	93.63	-6.37	1451.8...	

1451.8
3/20/10


Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charles W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per031910a.qld

Last Altered: Saturday, March 20, 2010 1:22:43 PM Eastern Standard Time
Printed: Saturday, March 20, 2010 1:32:33 PM Eastern Standard Time

Name: per0319023a
Date: 19-Mar-2010
Time: 14:04:02
ID: IPB004
Vial: 1:1,A

03-20-10

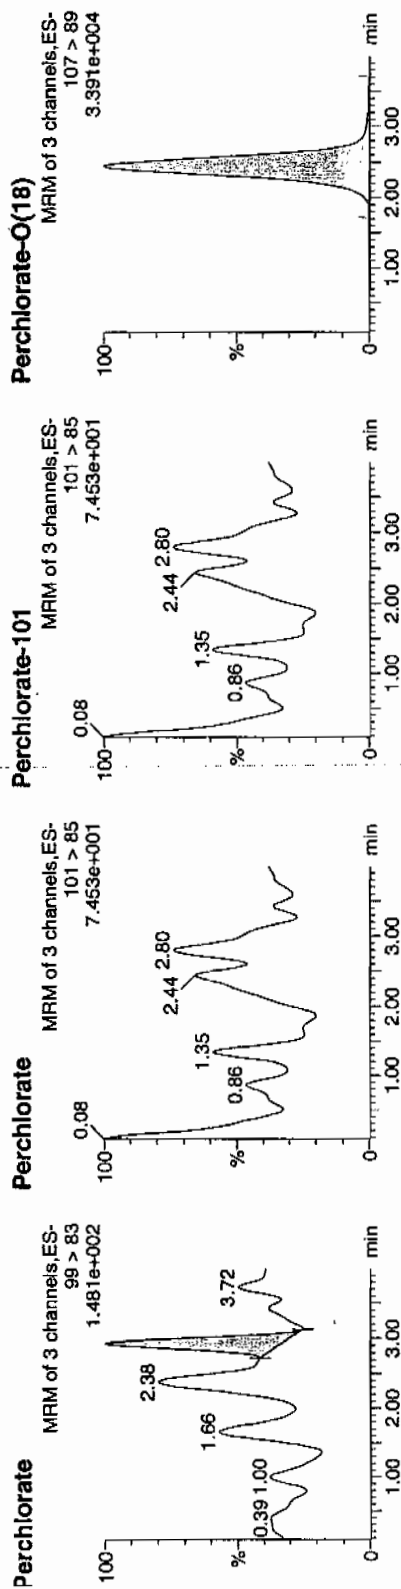

ID	Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	SN	Ion Ratio
IPB004	Perchlorate	99 > 83	2.92	17.504	17.504	bb			0.0006			18.535	0.00
IPB004	Perchlorate-101	101 > 85											
IPB004	Perchlorate-O(18)	107 > 89	2.45	11083.563	11083.563	bb			0.4563	91.26	-8.74	1886.8...	

not
3/22/10

Nairb.ref

; Positive ion monoisotopic and average masses from solution
 ; of NaI/Rbi (2.0/0.05ug/ul) in 50/20 2-propanol/H₂O.
 ; Most useful general purpose calibrant for all low
 ; MW applications, including MS/MS work.
 ; At high resolution, readily covers from m/z 50-2000.
 ; At reduced resolution, can be used to over m/z 3000.
 ; NOT RECOMMENDED FOR PROTEIN WORK. USE MYO, MYOTRP or TRP.

Updated 20 April '95

22.9898	100
84.9118	100
172.8840	100
322.7782	100
472.6725	100
622.5667	100
772.4610	100
922.3552	100
1072.2494	100
; 1222.1437	100
; 1372.0379	100
; 1521.9321	100
; 1671.8264	100
; 1821.7206	100
; 1971.6149	100
; 2121.5091	100
; 2271.4033	100
; 2421.2976	100
; 2571.1918	100
; 2721.0861	100
; 2870.9803	100
; 3020.8745	100
; 3170.7688	100
; 3320.6630	100
; 3470.5572	100
; 3620.4515	100
; 3770.3457	100
; 3920.2400	100

QUANTO ULTIMA: nairb 01.08.08.ca

Calibration Report - MS1 Static


Page 1 of 1

Printed: Tue Jan 08 12:19:12 2008


DATA HIGHLIGHTED BY CURVED 01-09-08

Data file: STATMS1 - Uncalibrated


7 matches of 7 tested references

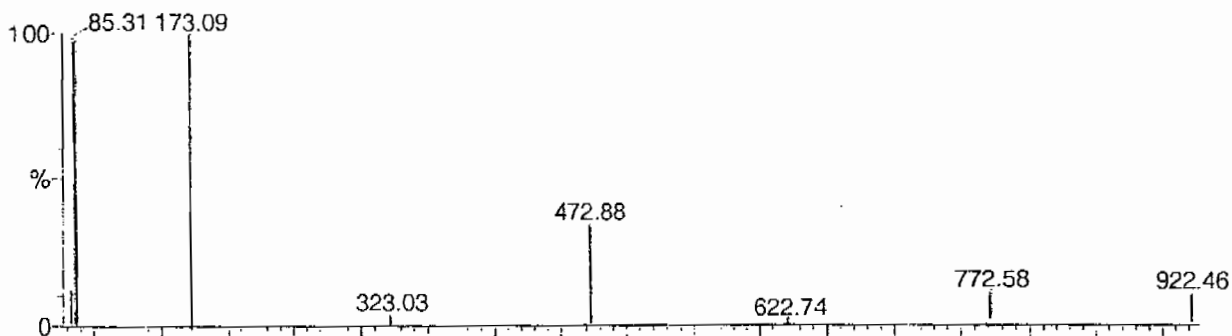

Reference file: Nairb

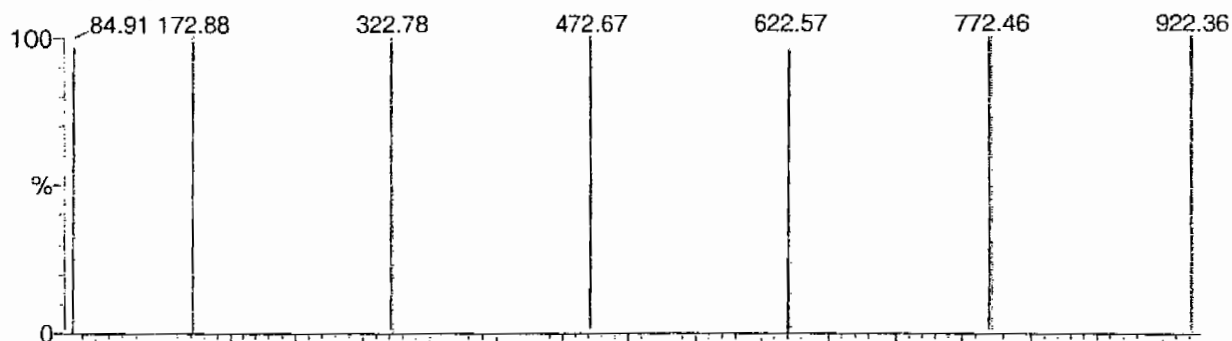


Mass difference (Raw - Ref mass)

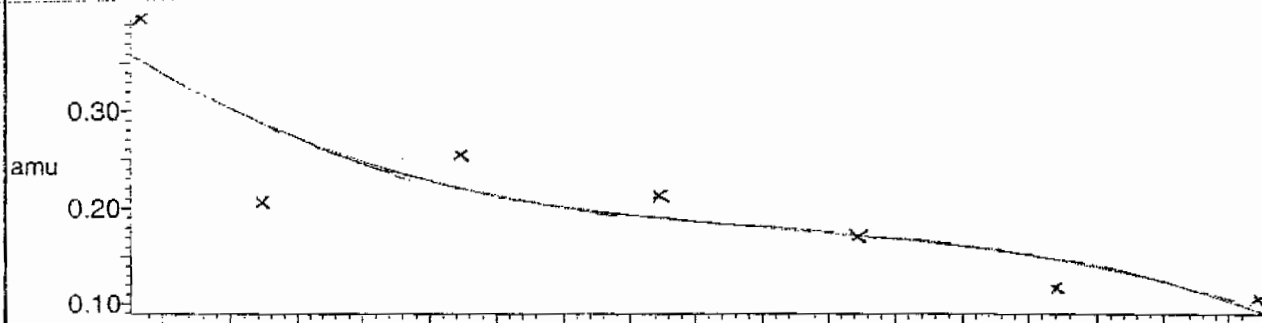

Residuals

Mean residual = $3.212012 \times 10^{-2} \pm 0.024108$

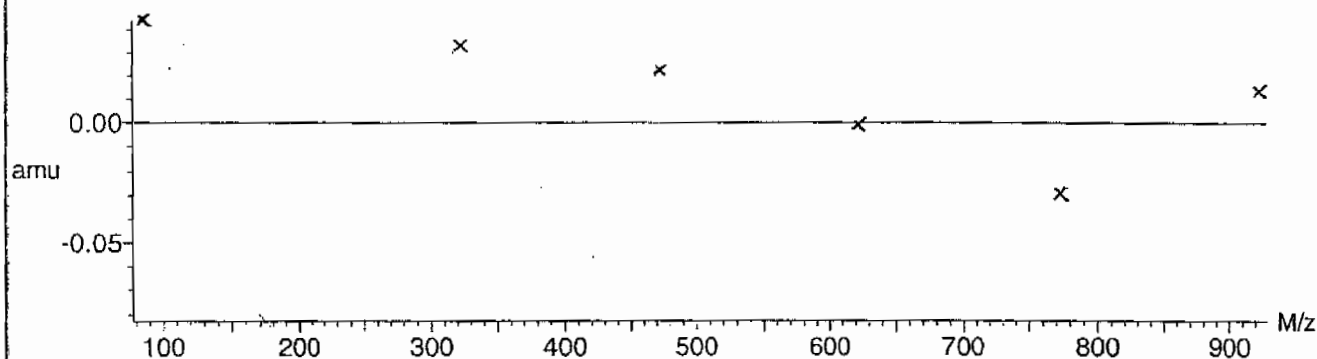


Calibration Report - MS1 Scanning

Page 1 of 1


Printed: Tue Jan 08 12:20:09 2008

Data file: SCNMS1 - Uncalibrated


7 matches of 7 tested references

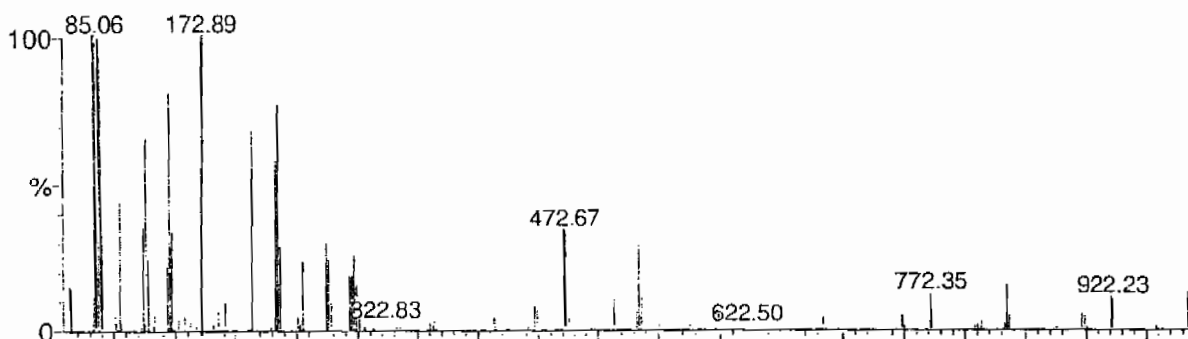

Reference file: Nairb

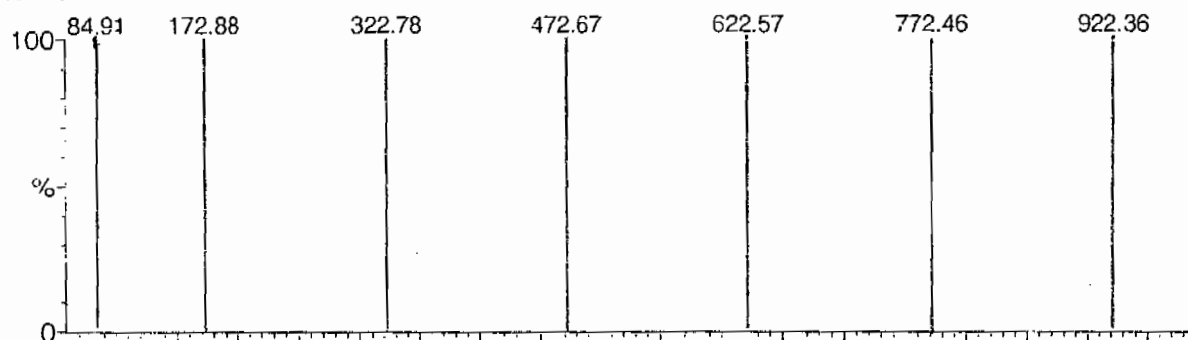


Mass difference (Raw - Ref mass)

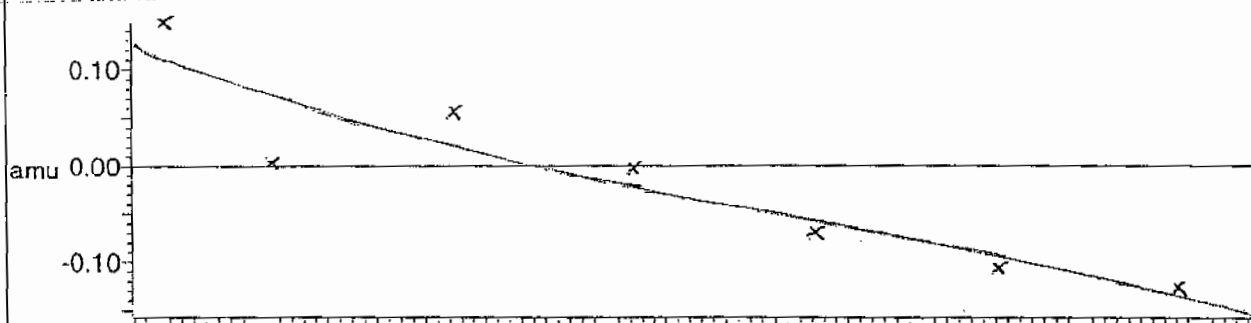

Residuals

Mean residual = $2.732691 \times 10^{-2} \pm 0.020653$

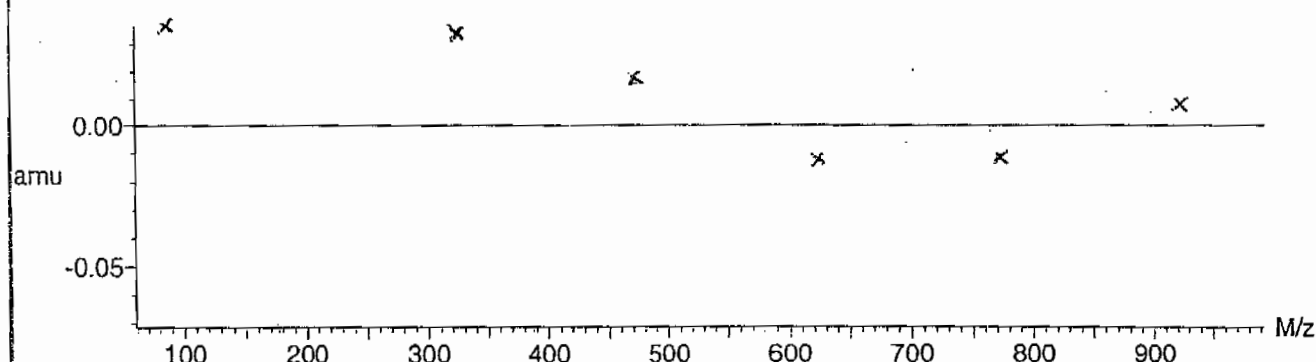


Calibration Report - MS1 Scan Speed Compensation

Page 1 of 1


Printed: Tue Jan 08 12:21:04 2008

Data file: FASTMS1 - Uncalibrated


7 matches of 7 tested references

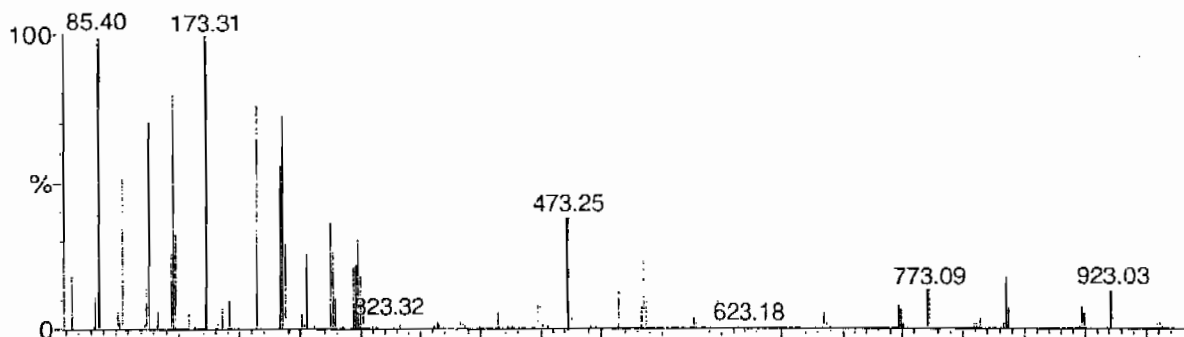

Reference file: Nairb

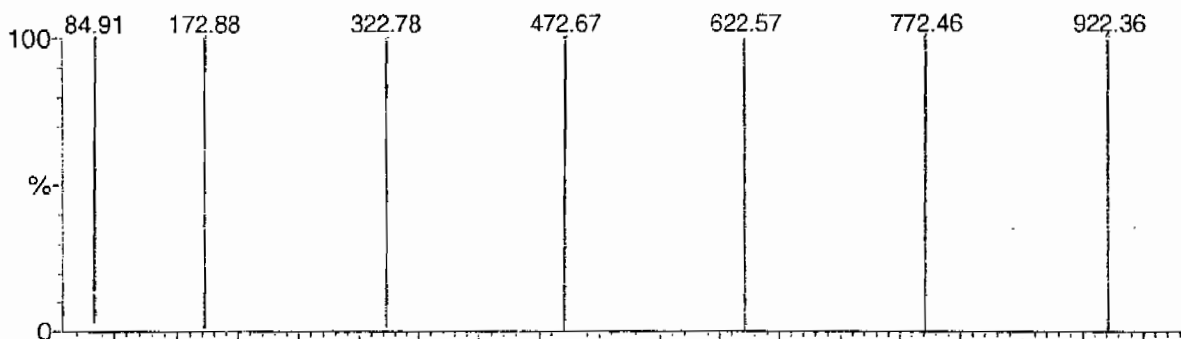


Mass difference (Raw - Ref mass)

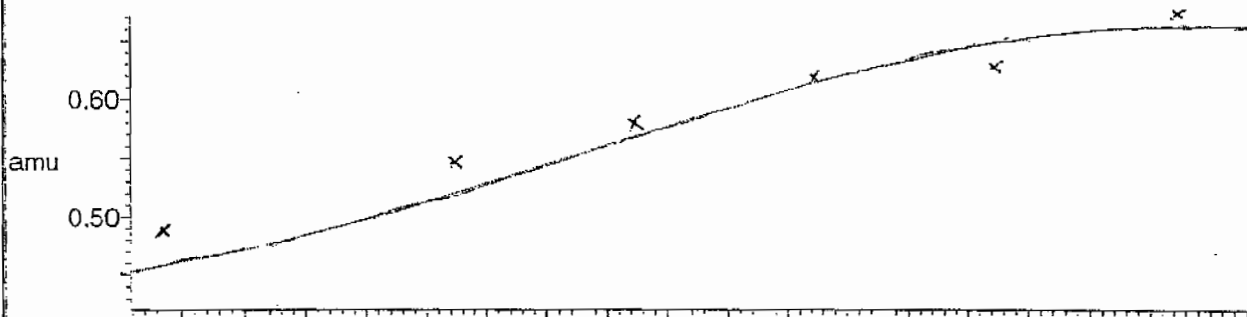

Residuals


Mean residual = $2.224580 \times 10^{-2} \pm 0.016544$

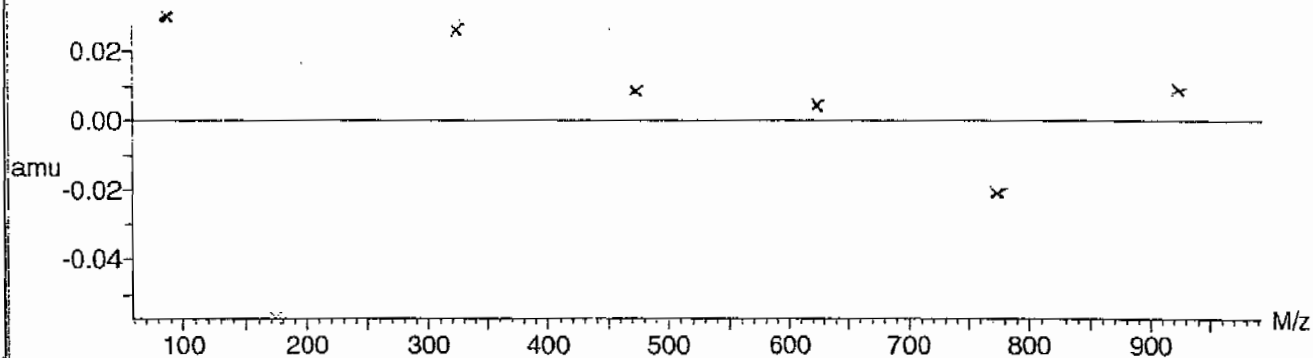

Calibration Report - MS2 Scan Speed Compensation

Page 1 of 1


Printed: Tue Jan 08 12:23:51 2008

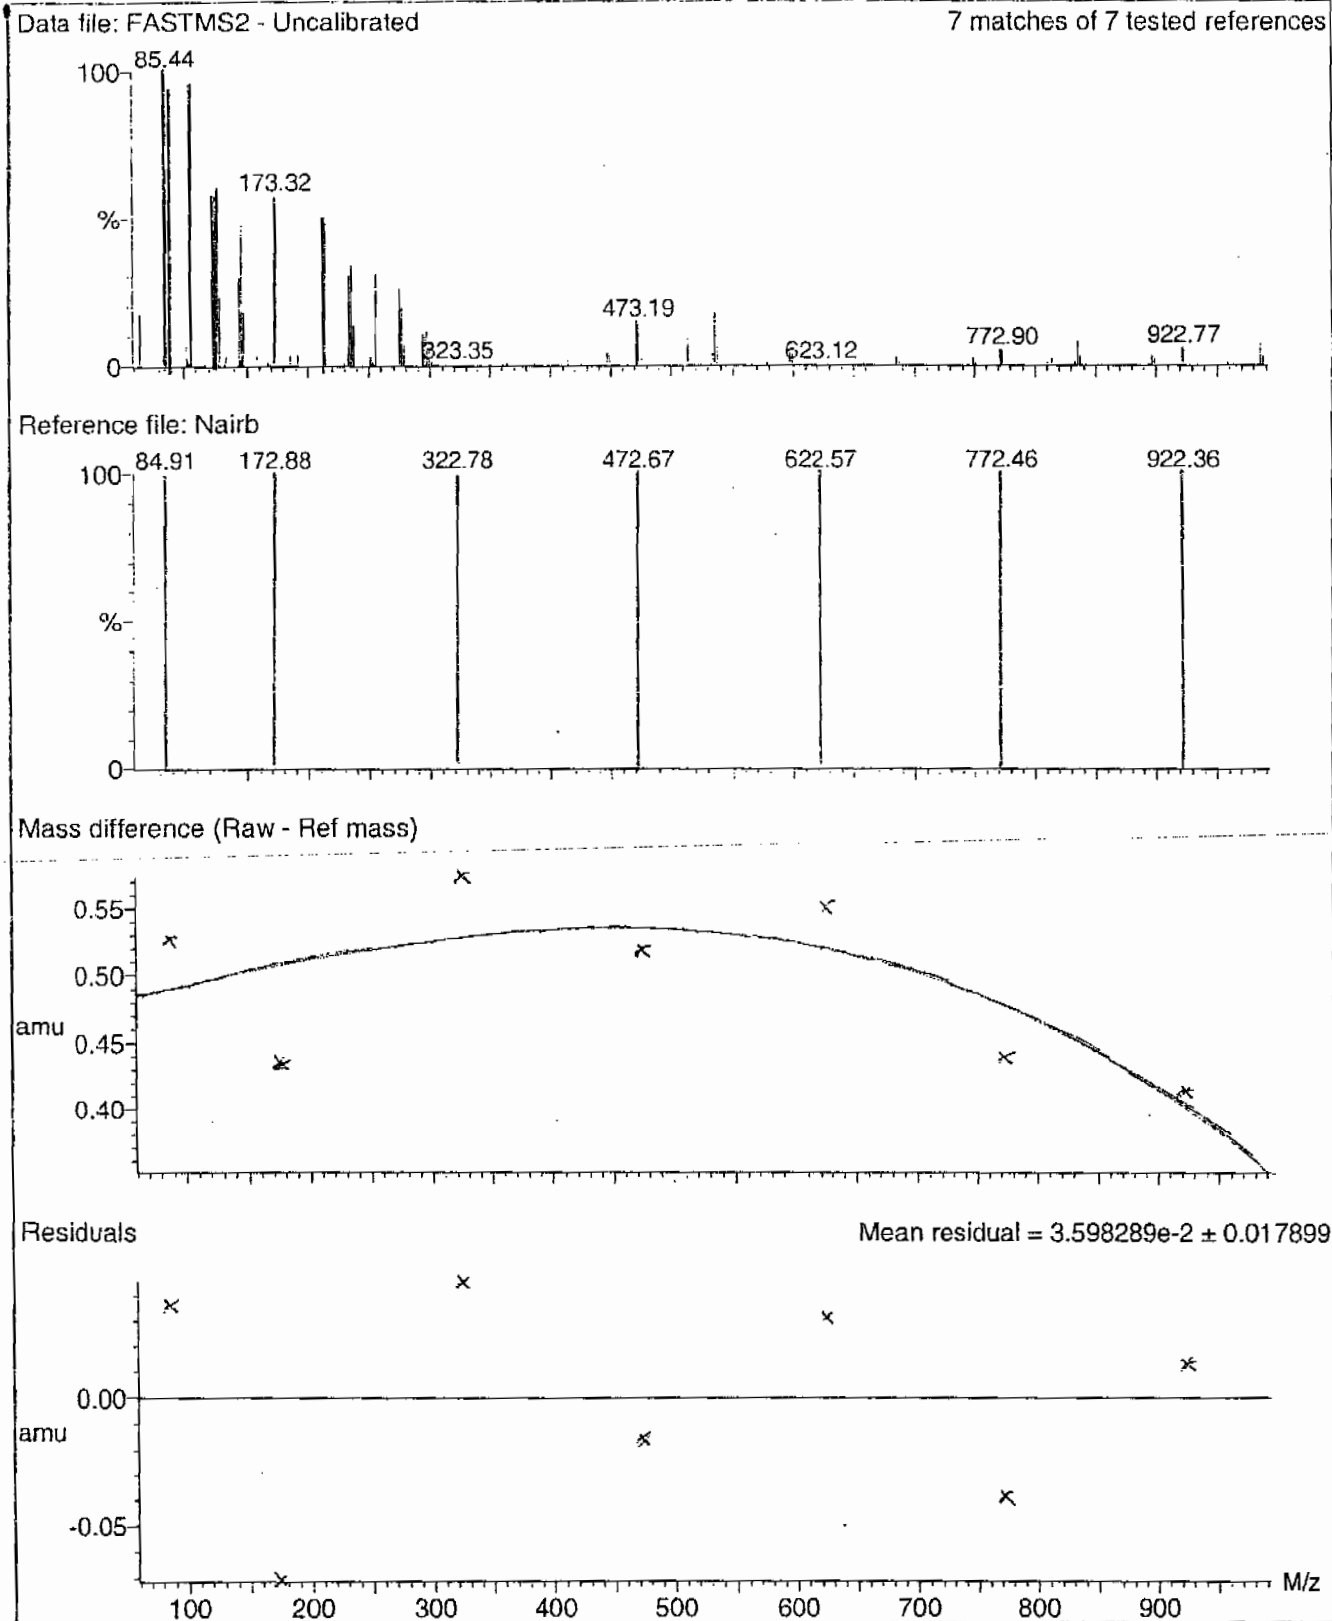

Calibration Report - MS2 Scanning

Page 1 of 1

Printed: Tue Jan 08 12:22:56 2008

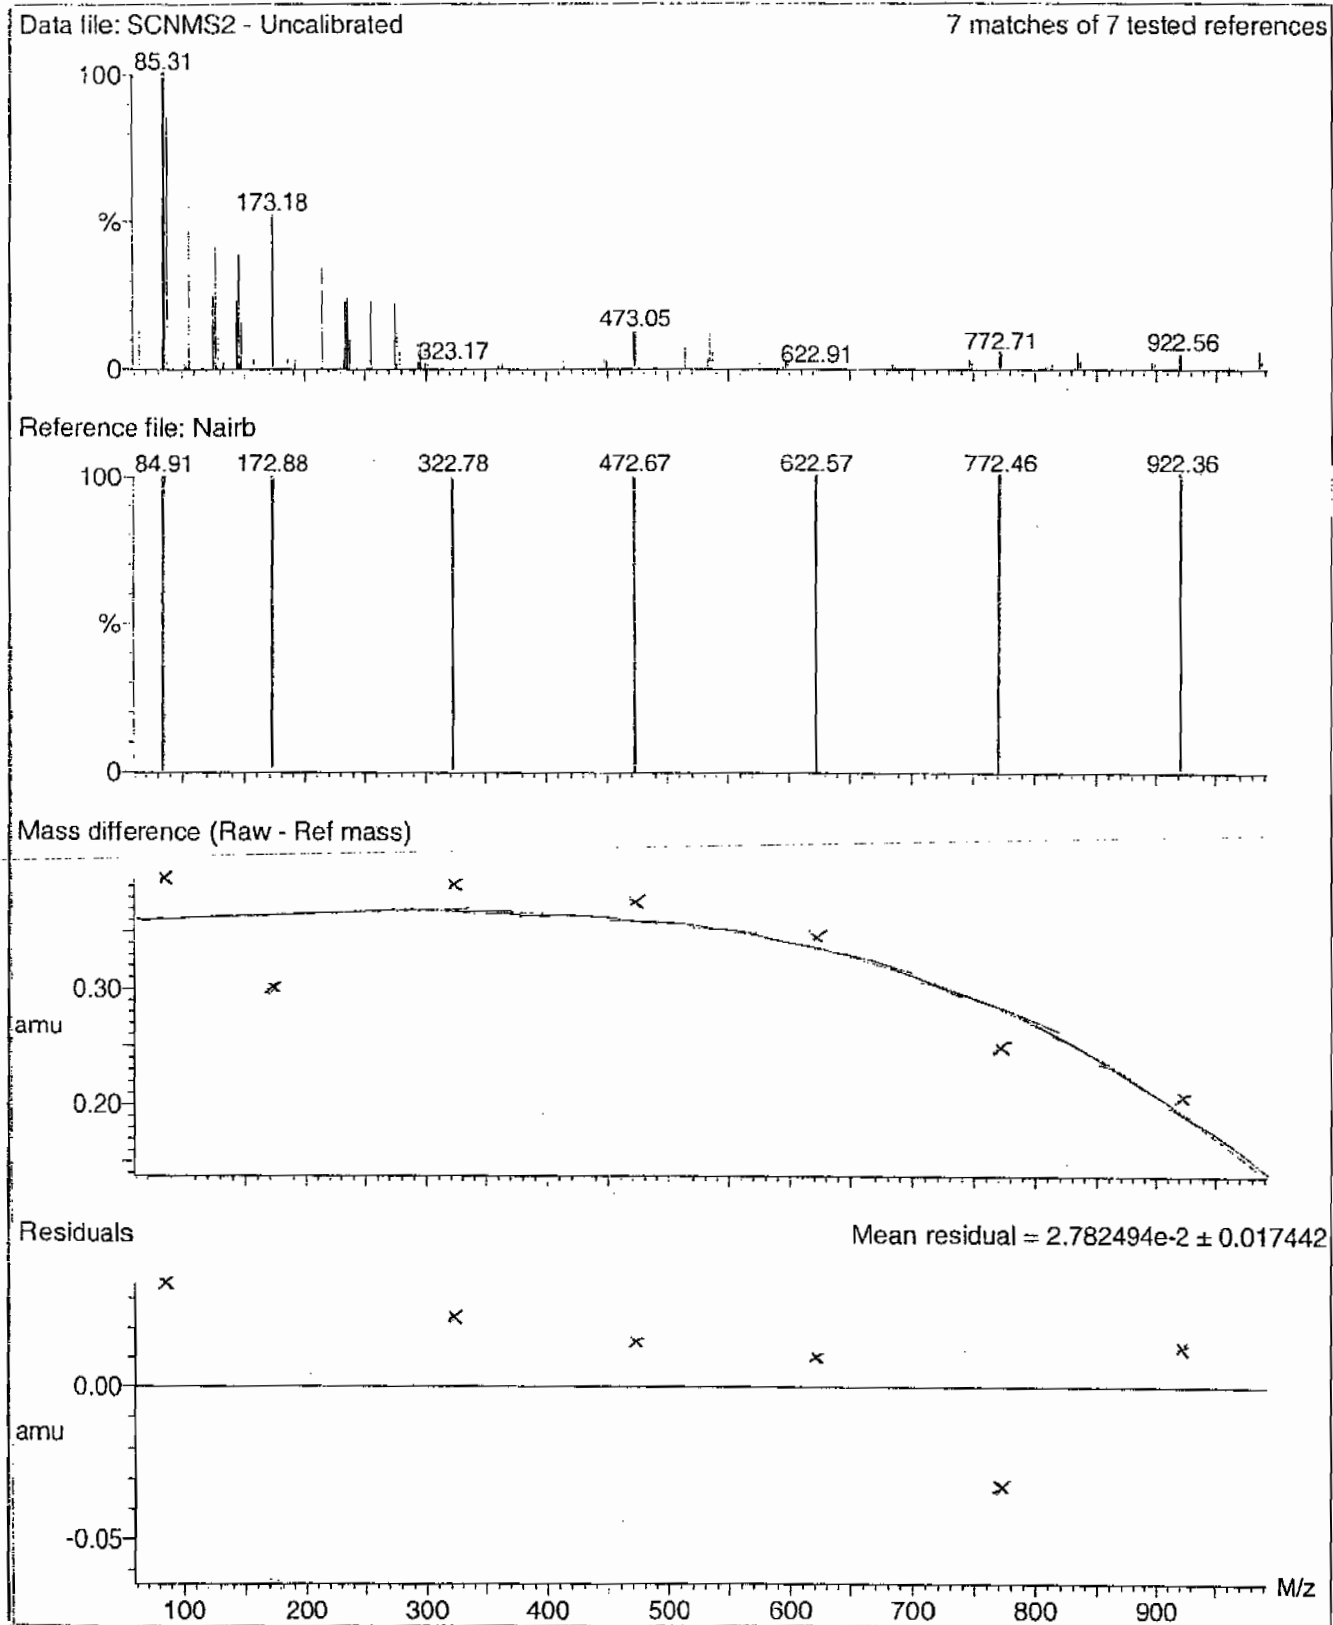


Calibration Report - MS2 Static

Page 1 of 1


Printed: Tue Jan 08 12:21:59 2008

Data file: STATMS2 - Uncalibrated


7 matches of 7 tested references

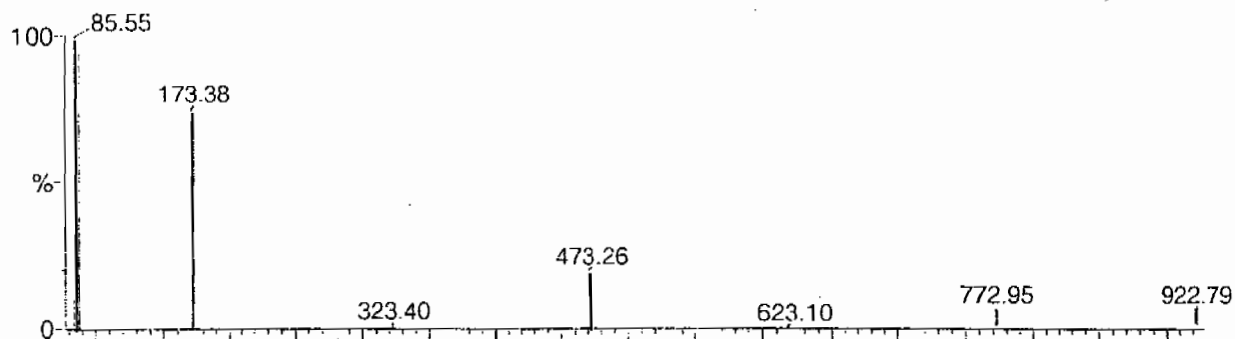

Reference file: Nairb

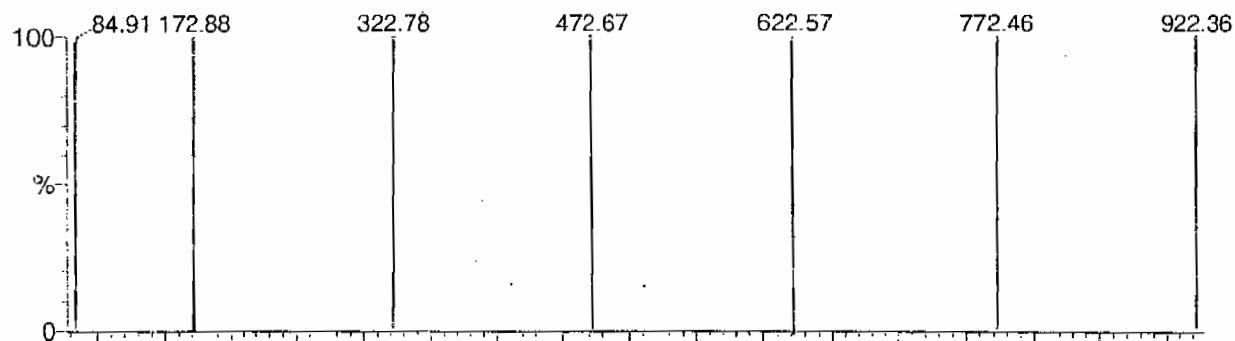


Mass difference (Raw - Ref mass)

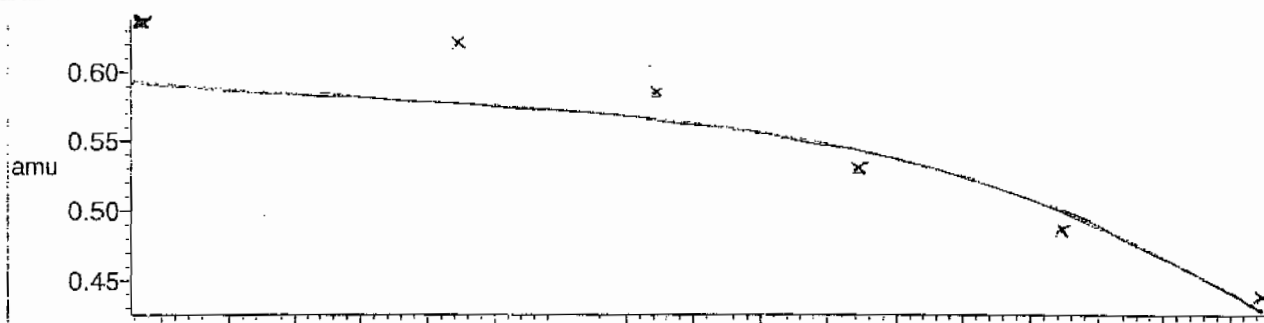

Residuals

Mean residual = $3.295980 \times 10^{-2} \pm 0.025603$

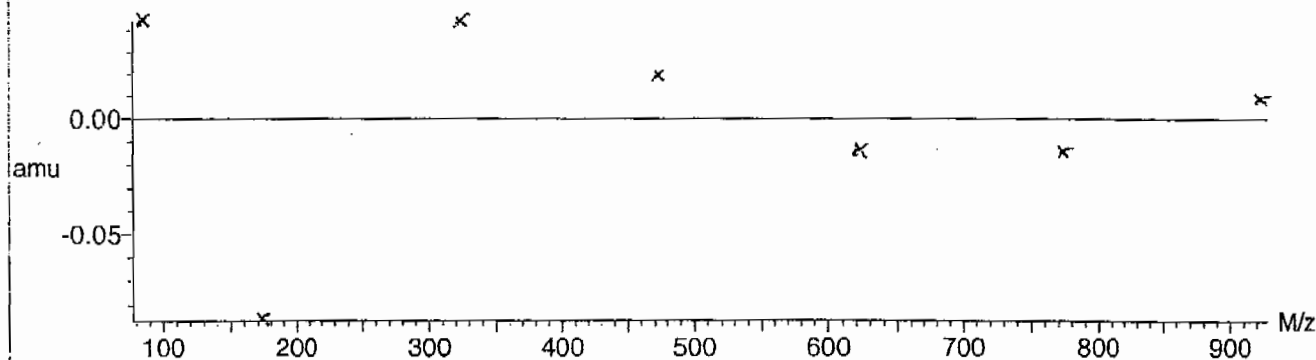


File Parameters

MassLynx 4.0 SP4

Page 1 of 1

File: C:\MassLynx\Perchlorate.PRO\ACQUDB\Perchlorate.IPR

Printed: Friday, March 19, 2010 07:16:27 Eastern Standard Time

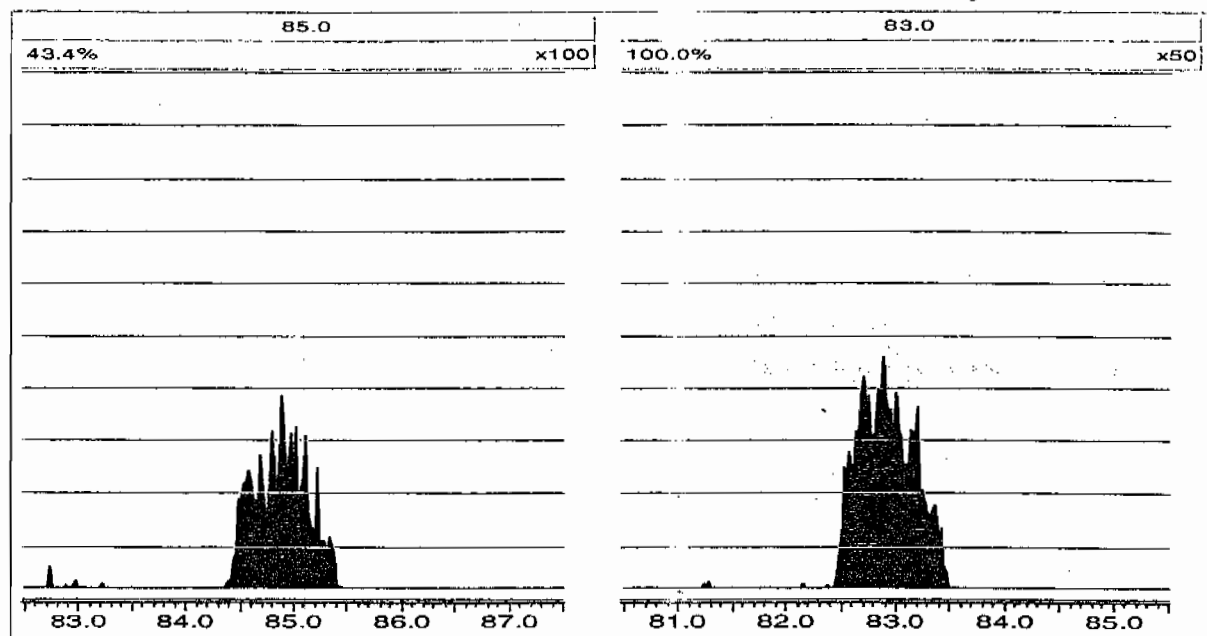

Perchlorate RT And Area Summary

GEL Job No.(SDG): 10-2093-1

Lab Name: General Engineering Laboratories

Lab Code: GEL

Instrument ID: LCMSMS

HPLC Column: Phenomenex Ion Pac AG-16 2 X 50 mm

Sample ID	Datafile	Run Date	Area	RT	RT CLO4	RRT	Q 0.98-1.02
MidLevel Standard Area	per0319006a	19-MAR-10	11968.7				
Lower Area Limit			5984.35				
Upper Area Limit			23937.4				
1202056676	per0319012a	19-MAR-10 12:46	10813.9	2.45	2.42698	.991	
1202056677	per0319013a	19-MAR-10 12:53	11935.6	2.45	2.46423	1.006	
1202056681	per0319014a	19-MAR-10 13:00	12272.7	2.5	2.51383	1.006	
248118001	per0319015a	19-MAR-10 13:07	11566.5	2.45	2.46422	1.006	
248118002	per0319016a	19-MAR-10 13:14	11770.3	2.45	2.4766	1.011	
248118003	per0319017a	19-MAR-10 13:21	12042.1	2.45	2.46427	1.006	
248118004	per0319018a	19-MAR-10 13:28	11849.9	2.45	2.46427	1.006	
248118005	per0319019a	19-MAR-10 13:35	11576.7	2.46	2.46423	1.002	

Perchlorate RT And Area Summary

Lab Name: General Engineering Laboratories

GEL Job No.(SDG): 10-2093-1

Lab Code: GEL

Instrument ID: LCMSMS

HPLC Column: Phenomenex Ion Pac AG-16 2 X 50 mm

Sample ID	Datafile	Run Date	Area	RT	RT CLO4	RRT	Q 0.98-1.02
MidLevel Standard Area	per0319006a	19-MAR-10	11968.7				
Lower Area Limit			5984.35				
Upper Area Limit			23937.4				
248118006	per0319020a	19-MAR-10 13:42	12374.8	2.44	2.46432	1.01	
248118007	per0319021a	19-MAR-10 13:49	12472.3	2.45	2.46425	1.006	

SAMPLE DATA

Perchlorate Analysis Data Sheet

Lab Name: GEL Laboratories LLC

Lab Code: GEL

Instrument: LCMSMS

Method: SW846 6850 Modified

Matrix: SOIL

Extraction Batch ID: 259007

Extraction Type: Solid Prep

Sample Volume/Weight: 2.00 g

Concentrated Extract Volume: 20.0

Client Sample No.

RE36-10-8448

Date Received: 26-FEB-10

GEL Job No (SDG): 10-2093-1

GEL Sample ID: 248118001

Date Filtered: 12-MAR-10

Injection Volume (uL): 20

% Solids: 97.3

CAS No.	Analyte [^]	MDL	RL	Conc*	Units	Q	Dilution Factor	Date Analyzed	GEL File ID
14797-73-0	Perchlorate	.514	2.05	0.514	ug/kg	U	1	19-MAR-10 13:07	per0319015a
	Perchlorate Isotope Ratio						1	19-MAR-10 13:07	per0319015a
14797-73-0	Perchlorate-101	.514	2.05	0.514	ug/kg	U	1	19-MAR-10 13:07	per0319015a
	Perchlorate-O(18)			4.89	ug/kg		1	19-MAR-10 13:07	per0319015a

[^] When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

*Concentration =

Instrument Value X $\frac{\text{Concentrated Extract Volume}}{\text{Aliquot}}$ X $\frac{1}{\% \text{Solids}}$

Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charlers W. Wilson


Dataset: C:\MassLynx\Perchlorate.PRO\per031910a.qld

Last Altered: Saturday, March 20, 2010 1:22:43 PM Eastern Standard Time
Printed: Saturday, March 20, 2010 1:32:33 PM Eastern Standard Time

Name: per0319015a
Date: 19-Mar-2010
Time: 13:07:25
DI: 248118001
/al: 1:3,D

0320-10

122-1959012 | 3220 | 11

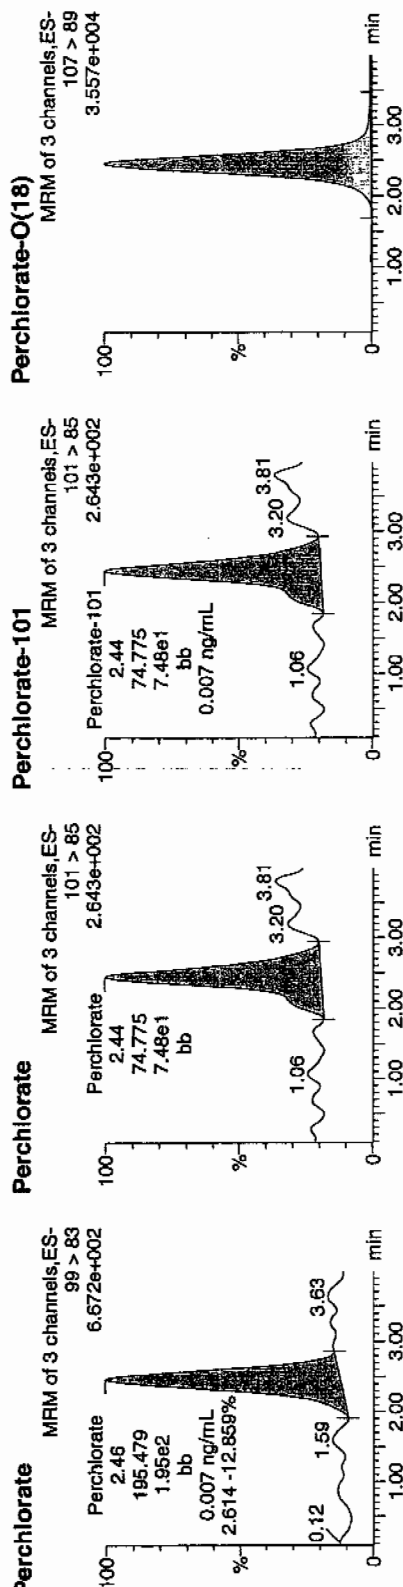

Name	Trace	Area	Response	Flags	Mod Date	Mod Time	Mod User	%Area	%Dev	S/N	Ion Ratio
248118001	Perchlorate	99 > 83	2.46	195.479	bb			0.0086		105.440	2.61
248118001	Perchlorate-101	101 > 85	2.44	74.775	bb			0.0074		21.603	
248118001	Perchlorate-O(18)	107 > 89	2.45	11566.496	bb			0.4762	95.24	-4.76	2246.4...

122
3/22/10

Form 1

Perchlorate Analysis Data Sheet

Lab Name: GEL Laboratories LLC

Lab Code: GEL

Instrument: LCMSMS

Method: SW846 6850 Modified

Matrix: SOIL

Extraction Batch ID: 959007

Extraction Type: Solid Prep

Sample Volume/Weight: 2.00 g

Concentrated Extract Volume: 20.0

Client Sample No.

RE36-10-8456

Date Received: 26-FEB-10

GEL Job No (SDG): 10-2093-1

GEL Sample ID: 248118002

Date Filtered: 12-MAR-10

Injection Volume (uL): 20

%Solids: 97.2

CAS No.	Analyte [^]	MDL	RL	Conc*	Units	Q	Dilution Factor	Date Analyzed	GEL File ID
14797-73-0	Perchlorate	.514	2.06	0.514	ug/kg	U	1	19-MAR-10 13:14	per0319016a
	Perchlorate Isotope Ratio						1	19-MAR-10 13:14	per0319016a
14797-73-0	Perchlorate-101	.514	2.06	0.514	ug/kg	U	1	19-MAR-10 13:14	per0319016a
	Perchlorate-O(18)			4.99	ug/kg		1	19-MAR-10 13:14	per0319016a

[^] When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

*Concentration =

Instrument Value X $\frac{\text{Concentrated Extract Volume}}{\text{Aliquot}}$ X $\frac{1}{\% \text{Solids}}$

Dataset: C:\MassLynx\Perchlorate.PRO\per031910a.qld

Last Altered: Saturday, March 20, 2010 1:22:43 PM Eastern Standard Time
Printed: Saturday, March 20, 2010 1:32:33 PM Eastern Standard Time





Name: per0319016a

Date: 19-Mar-2010

Time: 13:14:41

D: 248118002

Vial: 1:3,E

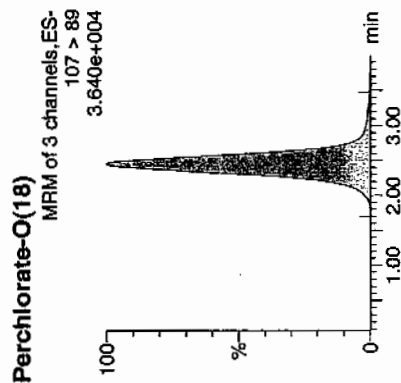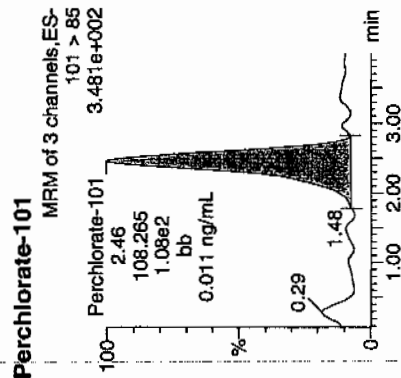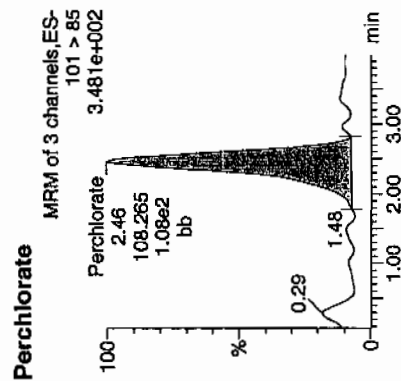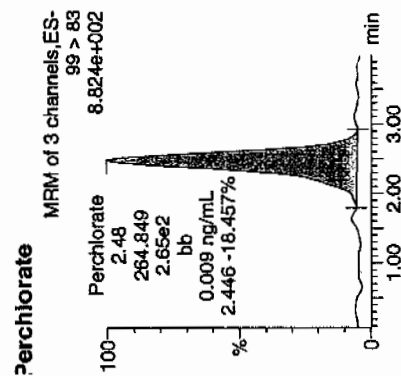

Dr. No.	Name	Trace	211	Mean	Response	FAUS	Mod. rate	Mod. time	no. of	% res.	20 day	SN Ion Ratio
2481118002	Perchlorate	99 > 83	2.48	264.849	264.849	bb			0.0090		32.924	2.45
2481118002	Perchlorate-101	101 > 85	2.46	108.265	108.265	bb			0.0107		58.603	
2481118002	Perchlorate-O(18)	107 > 89	2.45	11770.317	11770.317	bb			0.4846	96.92	-3.08	1218.8...

3/22/20
part 7

Form 1

Perchlorate Analysis Data Sheet

Lab Name: GEL Laboratories LLC

Lab Code: GEL

Instrument: LCMSMS

Method: SW846 6850 Modified

Matrix: SOIL

Extraction Batch ID: 959007

Extraction Type: Solid Prep

Sample Volume/Weight: 2.00 g

Concentrated Extract Volume: 20.0

Client Sample No.

RE36-10-8451

Date Received: 26-FEB-10

GEL Job No (SDG): 10-2093-1

GEL Sample ID: 248118003

Date Filtered: 12-MAR-10

Injection Volume (uL): 20

% Solids: 97

CAS No.	Analyte [^]	MDL	RL	Conc*	Units	Q	Dilution Factor	Date Analyzed	GEL File ID
14797-73-0	Perchlorate	.516	2.06	0.516	ug/kg	U	1	19-MAR-10 13:21	per0319017a
	Perchlorate Isotope Ratio						1	19-MAR-10 13:21	per0319017a
14797-73-0	Perchlorate-101	.516	2.06	0.516	ug/kg	U	1	19-MAR-10 13:21	per0319017a
	Perchlorate-O(18)			5.11	ug/kg		1	19-MAR-10 13:21	per0319017a

[^] When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

*Concentration =

Instrument Value X $\frac{\text{Concentrated Extract Volume}}{\text{Aliquot}}$ X $\frac{1}{\% \text{ Solids}}$

Dataset: C:\MassLynx\Perchlorate.PRO\per031910a.qld

Last Altered: Saturday, March 20, 2010 1:22:43 PM Eastern Standard Time
Printed: Saturday, March 20, 2010 1:32:33 PM Eastern Standard Time







Name: per0319017a

Date: 19-Mar-2010

Time: 13:21:42

ID: 248118003

Vial: 1:3,F

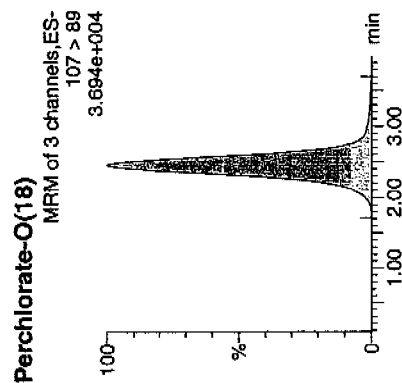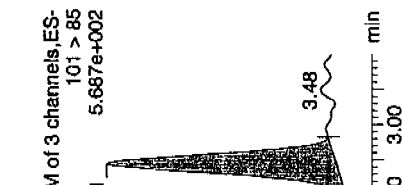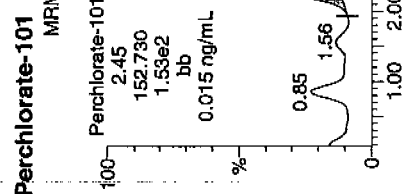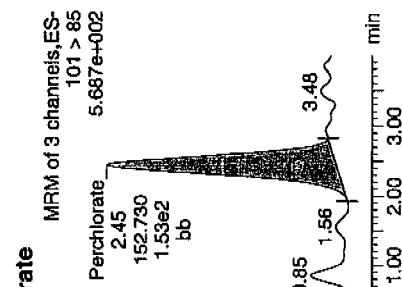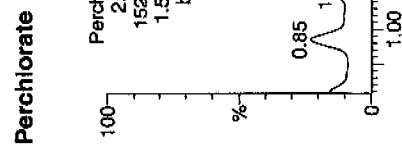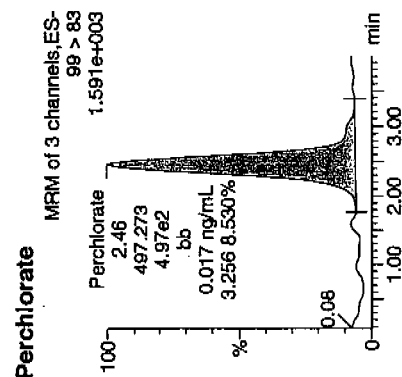

ID	Name	Trace	HT	Area	Response	Flags	Mod	Date	Mod	Time	%Rec	%Dev	SN	Ion	Ratio
248118003	Perchlorate	99 > 83	2.46	497.273	497.273	bb					0.0169		86.004		3.26
248118003	Perchlorate-101	101 > 85	2.45	✓ 152.730	✓ 152.730	bb					0.0151		11.945		
248118003	Perchlorate-O(18)	107 > 89	2.45	12042.129	12042.129	bb					0.4958	99.15	-0.85	848.758	

3/22/10
12077

Perchlorate Analysis Data Sheet

Lab Name: GEL Laboratories LLC
 Lab Code: GEL
 Instrument: LCMSMS
 Method: SW846 6850 Modified
 Matrix: SOIL
 Extraction Batch ID: 959007
 Extraction Type: Solid Prep
 Sample Volume/Weight: 2.00 g
 Concentrated Extract Volume: 20.0
 Client Sample No. RE36-10-8450
 Date Received: 26-FEB-10
 GEL Job No (SDG): 10-2093-1
 GEL Sample ID: 248118004
 Date Filtered: 12-MAR-10
 Injection Volume (uL): 20
 %Solids: 85

CAS No.	Analyte [^]	MDL	RL	Conc*	Units	Q	Dilution Factor	Date Analyzed	GEL File ID
14797-73-0	Perchlorate	.588	2.35	1.27	ug/kg	J	1	19-MAR-10 13:28	per0319018a
	Perchlorate Isotope Ratio			3.24			1	19-MAR-10 13:28	per0319018a
14797-73-0	Perchlorate-101	.588	2.35	1.14	ug/kg	J	1	19-MAR-10 13:28	per0319018a
	Perchlorate-O(18)			5.73	ug/kg		1	19-MAR-10 13:28	per0319018a

[^] When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

*Concentration =

Instrument Value X Concentrated Extract Volume X 1
 Aliquot %Solids

Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charfers W. Wilson


Dataset: C:\MassLynx\Perchlorate.PRO\per031910a.qld

Last Altered: Saturday, March 20, 2010 1:22:43 PM Eastern Standard Time
Printed: Saturday, March 20, 2010 1:32:33 PM Eastern Standard Time

Name: per0319018a
Date: 19-Mar-2010
Time: 13:28:43
ID: 248118004
Vial: 1:4,A

002
03-20-10

112201954012 / 2420 / 11

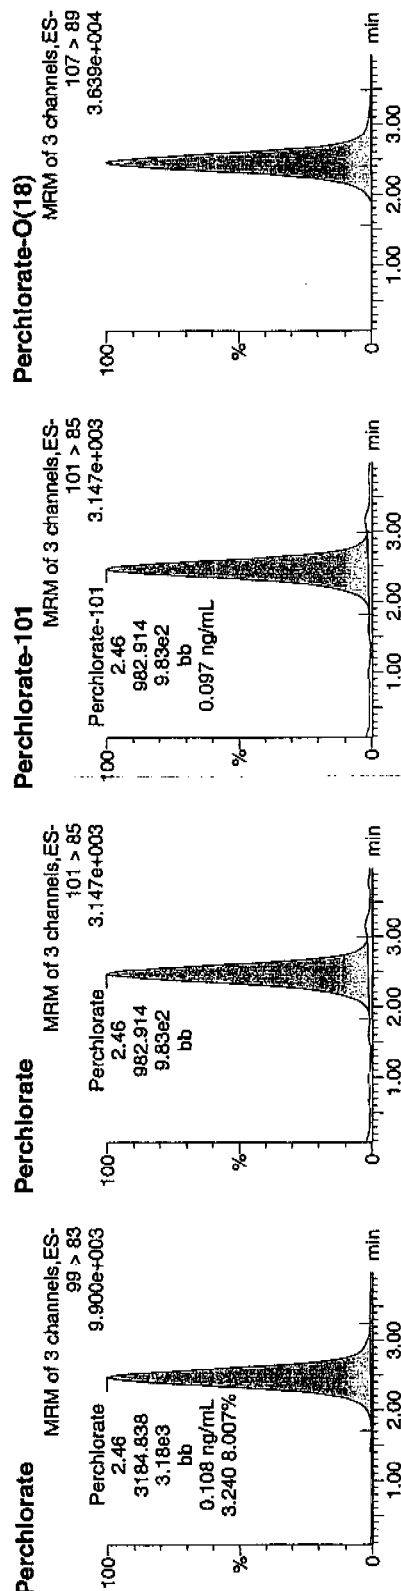

ID	Name	Trace	Area	Response	Flags	ModDate	ModTime	ng/mL	%Rec	%Dev	S/N	Ion Ratio
248118004	Perchlorate	99 > 83	2.46	3184.838	bb				0.1082		834.775	3.24
248118004	Perchlorate-101	101 > 85	2.46	982.914	bb				0.0974		438.182	
248118004	Perchlorate-O(18)	107 > 89	2.45	11849.896	bb				0.4879	97.57	-2.43	2304.4...

$$\frac{3184.838}{2420} = 1.27$$

not
3/22/10

Form 1

Perchlorate Analysis Data Sheet

Lab Name: GEL Laboratories LLC

Lab Code: GEL

Instrument: LCMSMS

Method: SW846 6850 Modified

Matrix: SOIL

Extraction Batch ID: 959007

Extraction Type: Solid Prep

Sample Volume/Weight: 2.00 g

Concentrated Extract Volume: 20.0

Client Sample No.

RE36-10-8449

Date Received: 26-FEB-10

GEL Job No (SDG): 10-2093-1

GEL Sample ID: 248118005

Date Filtered: 12-MAR-10

Injection Volume (uL): 20

%Solids: 98.2

CAS No.	Analyte [^]	MDL	RL	Conc*	Units	Q	Dilution Factor	Date Analyzed	GEL File ID
14797-73-0	Perchlorate	.509	2.04	0.509	ug/kg	U	1	19-MAR-10 13:35	per0319019a
	Perchlorate Isotope Ratio						1	19-MAR-10 13:35	per0319019a
14797-73-0	Perchlorate-101	.509	2.04	0.509	ug/kg	U	1	19-MAR-10 13:35	per0319019a
	Perchlorate-O(18)			4.85	ug/kg		1	19-MAR-10 13:35	per0319019a

[^] When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

*Concentration =

Instrument Value X $\frac{\text{Concentrated Extract Volume}}{\text{Aliquot}}$ X $\frac{1}{\% \text{Solids}}$

Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charlers W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per031910a.qld


Last Altered: Saturday, March 20, 2010 1:22:43 PM Eastern Standard Time
Printed: Saturday, March 20, 2010 1:32:33 PM Eastern Standard Time

Name: per0319019a
Date: 19-Mar-2010
Time: 13:35:46
ID: 248118005
Vial: 1:4,B


122-1954012 | 3020 | 11

0320-10


Perchlorate

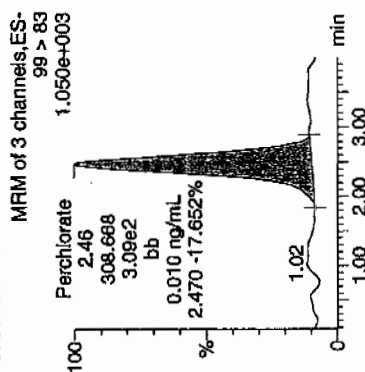


Perchlorate

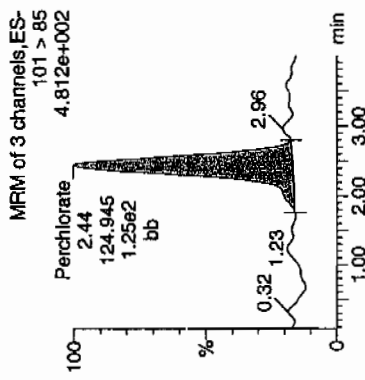

Perchlorate-101

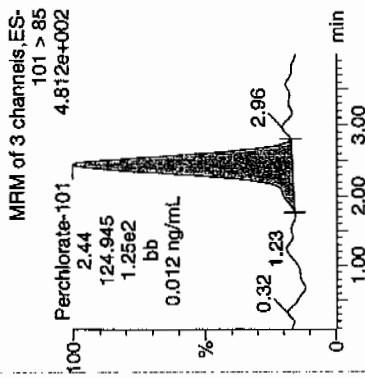

Perchlorate-O(18)

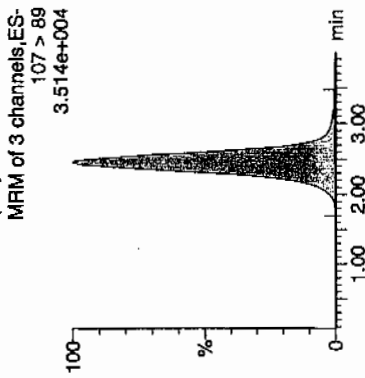

ID	Name	Trace	Area	Flag	Mod	Time	Conc	Res	Day	SN	Ratio
248118005	Perchlorate	99 > 83	2.46		308.668	bb	0.0105	222.519	2.47		
248118005	Perchlorate-101	101 > 85	2.44		124.945	bb	0.0124	70.180			
248118005	Perchlorate-O(18)	107 > 89	2.46		11576.663	bb	0.4766	95.32	-4.68	1731.3...	

107
3/20/10

Form 1

Perchlorate Analysis Data Sheet

Lab Name: GEL Laboratories LLC

Lab Code: GEL

Instrument: LCMSMS

Method: SW846 6850 Modified

Matrix: SOIL

Extraction Batch ID: 959007

Extraction Type: Solid Prep

Sample Volume/Weight: 2.00 g

Concentrated Extract Volume: 20.0

Client Sample No.

RE36-10-8453

Date Received: 26-FEB-10

GEL Job No (SDG): 10-2093-1

GEL Sample ID: 248118006

Date Filtered: 12-MAR-10

Injection Volume (uL): 20

%Solids: 95.7

CAS No.	Analyte [^]	MDL	RL	Conc*	Units	Q	Dilution Factor	Date Analyzed	GEL File ID
14797-73-0	Perchlorate	.522	2.09	3.77	ug/kg		1	19-MAR-10 13:42	per0319020a
	Perchlorate Isotope Ratio			2.99			1	19-MAR-10 13:42	per0319020a
14797-73-0	Perchlorate-101	.522	2.09	3.67	ug/kg		1	19-MAR-10 13:42	per0319020a
	Perchlorate-O(18)			5.32	ug/kg		1	19-MAR-10 13:42	per0319020a

[^] When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

*Concentration =

Instrument Value X Concentrated Extract Volume X 1 %Solids
Aliquot

Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charlers W. Wilson


Dataset: C:\MassLynx\Perchlorate.PRO\per031910a.qld

Last Altered: Saturday, March 20, 2010 1:22:43 PM Eastern Standard Time
Printed: Saturday, March 20, 2010 1:32:33 PM Eastern Standard Time

Name: per0319020a
Date: 19-Mar-2010
Time: 13:42:49
ID: 248118006
Vial: 1-4,C

03-20-10

LANC | 954012 | 5070 | 11

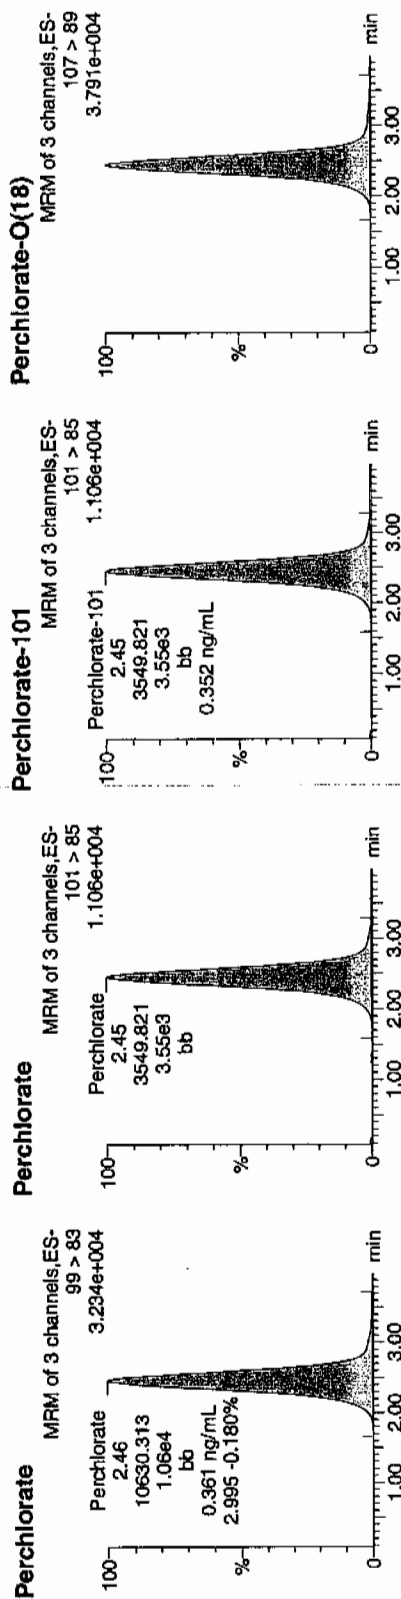

ID	Name	Trace	Area	Response	Flags	Mod Time	% Rec	% Dev	S/N	Ratio
248118006	Perchlorate	99 > 83	2.46	10630.313	bb		0.3612	7985.2...	2.99	
248118006	Perchlorate-101	101 > 85	2.45	3549.821	bb		0.3517	1000.5...		
248118006	Perchlorate-O(18)	107 > 89	2.44	12374.818	bb		0.5095	101.89	1.89	2404.9...

10630.313
29427 ~ 0.3612

not
3/20/10

Perchlorate Analysis Data Sheet

Lab Name: GEL Laboratories LLC
Lab Code: GEL
Instrument: LCMSMS
Method: SW846 6850 Modified
Matrix: SOIL
Extraction Batch ID: 959007
Extraction Type: Solid Prep
Sample Volume/Weight: 2.00 g
Concentrated Extract Volume: 20.0
Client Sample No. RE36-10-8452
Date Received: 26-FEB-10
GEL Job No (SDG): 10-2093-1
GEL Sample ID: 248118007
Date Filtered: 12-MAR-10
Injection Volume (uL): 20
%Solids: 92.9

CAS No.	Analyte [^]	MDL	RL	Conc*	Units	Q	Dilution Factor	Date Analyzed	GEL File ID
14797-73-0	Perchlorate	.538	2.15	2.32	ug/kg		1	19-MAR-10 13:49	per0319021a
	Perchlorate Isotope Ratio			3.09			1	19-MAR-10 13:49	per0319021a
14797-73-0	Perchlorate-101	.538	2.15	2.19	ug/kg		1	19-MAR-10 13:49	per0319021a
	Perchlorate-O(18)			5.53	ug/kg		1	19-MAR-10 13:49	per0319021a

[^] When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

*Concentration =

Instrument Value X $\frac{\text{Concentrated Extract Volume}}{\text{Aliquot}}$ X $\frac{1}{\% \text{Solids}}$

Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charliers W. Wilson





Dataset: C:\MassLynx\Perchlorate.PRO\per031910a.qld

Last Altered: Saturday, March 20, 2010 1:22:43 PM Eastern Standard Time
Printed: Saturday, March 20, 2010 1:32:33 PM Eastern Standard Time

Name: per0319021a
Date: 19-Mar-2010
Time: 13:49:50
ID: 248118007
Vial: 1:4,D

152-959012 | 30750 | 11

03-20-10

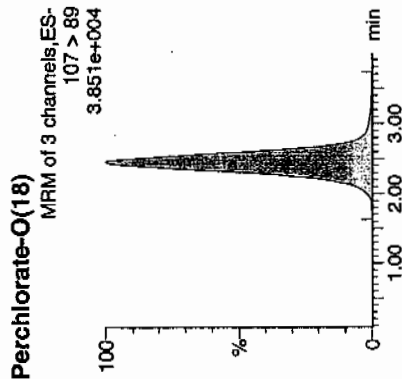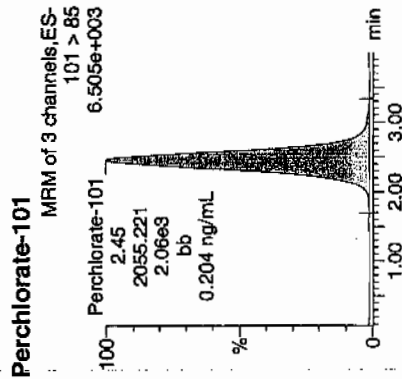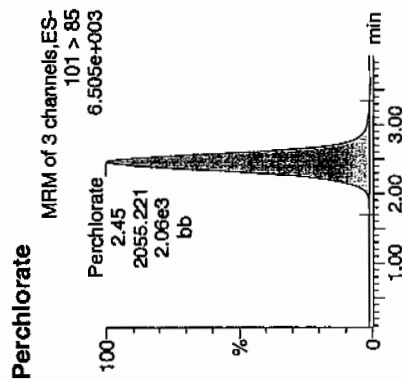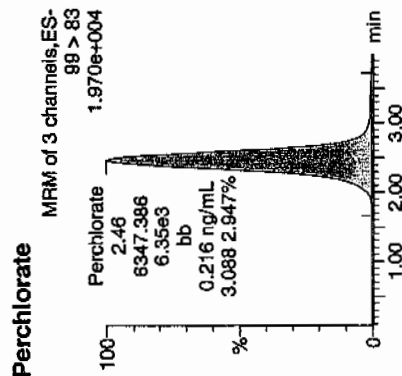

ID	Name	Area	Response	Flags	Mod	Time	ng/mL	%Rec	%Dev	S/N	Ratio
248118007	Perchlorate	99 > 83	2.46	6347.386	bb	2.45	0.2157	1655.6...		3.09	
248118007	Perchlorate-101	101 > 85	2.45	2055.221	bb	2.45	0.2036	104.323			
248118007	Perchlorate-O(18)	107 > 89	2.45	12472.345	bb	2.70	0.5135	5190.0...			

6347.386
29427
= 0.2157

3/22/10

STANDARDS DATA

Perchlorate Initial Calibration

GEL Job No.(SDG): 10-2093-1

Lab Name: General Engineering Laboratories

Lab Code: GEL

Instrument ID: LCMSMS Date Analyzed: 19-MAR-10

HPLC Column: Phenomenex Ion Pac AG-16 2 X 50 mm

Calibration Level	1	2	3	4	5
Cal Concentration (ug/L)	0.05	0.1	0.25	0.50	1.0

Parname Perchlorate

Coefficient of Determination:

Calibration Curve: 29426.98

Response Type: External Standard

Curve Type: RF

Perchlorate Initial Calibration

Lab Name: General Engineering Laboratories GEL Job No.(SDG): 10-2093-1

Lab Code: GEL

Instrument ID: LCMSMS Date Analyzed: 19-MAR-10

HPLC Column: Phenomenex Ion Pac AG-16.2 X 50 mm

Calibration Level	1	2	3	4	5
Cal Concentration (ug/L)	0.05	0.1	0.25	0.50	1.0

Paramname Perchlorate-101

Coefficient of Determination:

Calibration Curve: 10091.948

Response Type: External Standard

Curve Type: RF

Quantify Calibration Report MassLynx 4.0 SP4


The GEL Group, LLC Analyst: Charles W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per031910a.qld




Last Altered: Saturday, March 20, 2010 1:22:43 PM Eastern Standard Time
Printed: Saturday, March 20, 2010 1:32:33 PM Eastern Standard Time

Method: C:\MassLynx\Perchlorate.PRO\MethDB\per031910a.mdb 20 Mar 2010 13:21:43
Calibration: C:\MassLynx\Perchlorate.PRO\CurveDB\per031910a.cdb 20 Mar 2010 13:22:42

Compound name: Perchlorate
Response Factor: 29427
IRF SD: 1177.51, % Relative SD: 4.00146
Response type: External Std, Area
Curve type: RF

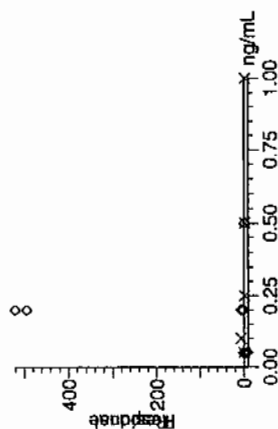

Compound name: Perchlorate-101
Response Factor: 10092
IRF SD: 664.55, % Relative SD: 6.58495
Response type: External Std, Area
Curve type: RF

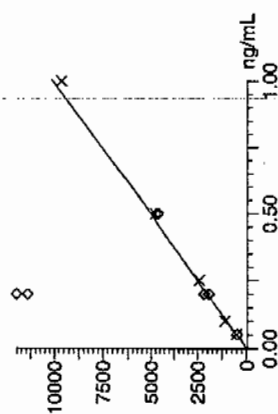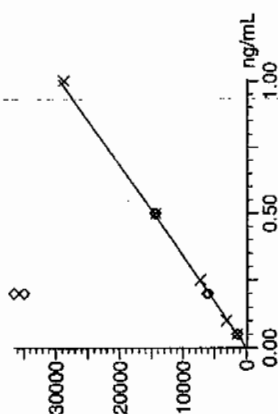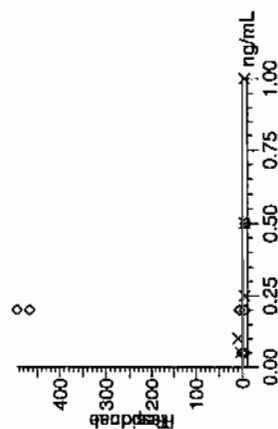

iEL SOP GL-OA-E-067, Method 6850-Modified / MM = Manual Modification


Quantify Calibration Report MassLynx 4.0 SP4

The GEL Group, LLC Analyst: Charles W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per031910a.qld

Last Altered: Saturday, March 20, 2010 1:22:43 PM Eastern Standard Time
Printed: Saturday, March 20, 2010 1:32:33 PM Eastern Standard Time

Compound name: Perchlorate-O(18) ✓
Response Factor: 24289.8 ✓
RF SD: 695.197, % Relative SD: 2.86209 ✓
Response type: External Std, Area
Curve type: RF

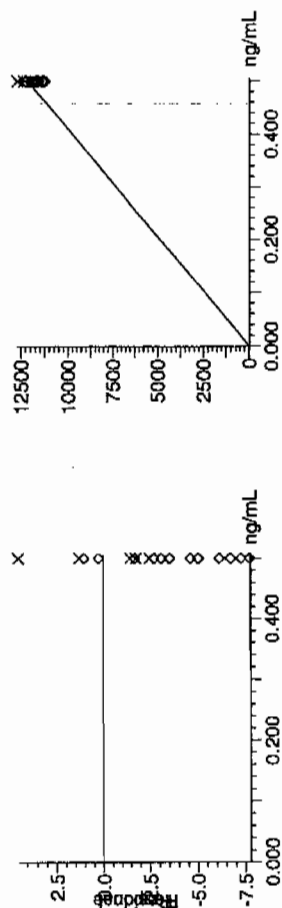

GEL SOP GL-OA-E-067, Method 6850-Modified / MM = Manual Modification

Perchlorate Initial Calibration Verification

GEL Job No.(SDG): 10-2093-1

Lab Name: General Engineering Laboratories

Lab Code: GEL

Reporting Units: ug/kg

Analyte	True	Found	%Rec	Date Analyzed	GEL File Id
Perchlorate	.5	.5	99.27	19-MAR-10 12:24	per0319009a
Perchlorate Isotope Ratio		3.08		19-MAR-10 12:24	per0319009a
Perchlorate-101	.5	.47	93.84	19-MAR-10 12:24	per0319009a

Quantify Sample Report MassLynx 4.0 SP4





The GEL Group, LLC Analyst: Charliers W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per031910a.qld

Last Altered: Saturday, March 20, 2010 1:22:43 PM Eastern Standard Time
Printed: Saturday, March 20, 2010 1:32:33 PM Eastern Standard Time

Sample Name: per0319009a
Date: 19-Mar-2010
Time: 12:24:29
D: WCL100318-06ICV
File: 1:2,A

*per
0319009a
3/20/10*

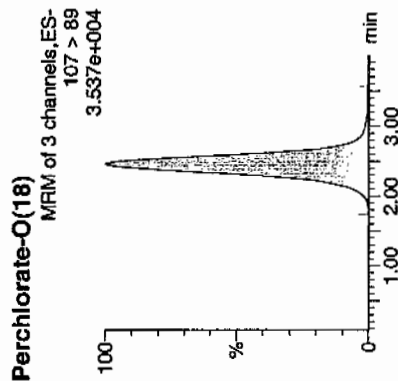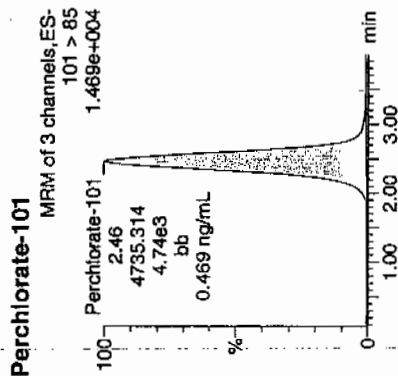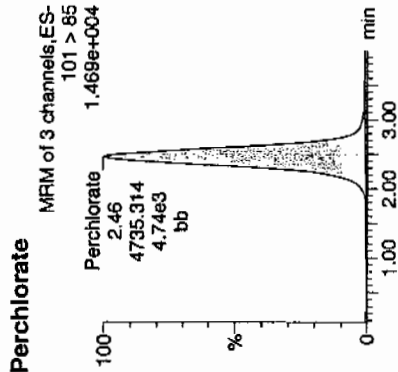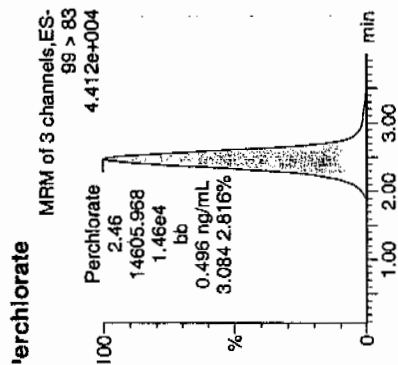

Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	S/N	Ion Ratio
VCL100318-06ICV	98 > 83	2.46	14605.968	14605.968	bb			0.4963	99.27	-0.73	2776.0...	3.08
VCL100318-06ICV	101 > 85	2.46	4735.314	4735.314	bb			0.4692	93.84	-6.16	442.320	
VCL100318-06ICV	107 > 89	2.45	11529.493	11529.493	bb			0.4747	94.93	-5.07	2669.5...	

$$\frac{14605.968}{29427} = 0.4963$$

*not
3/20/10*

Perchlorate Continuing Calibration Verification

Lab Name: General Engineering Laboratories

GEL Job No.(SDG): 10-2093-1

Lab Code: GEL

Reporting Units: ug/kg

Analyte	True	Found	%Rec	Date Analyzed	GEL File Id
Perchlorate	.5	.49	98.34	19-MAR-10 13:56	per0319022a
Perchlorate Isotope Ratio		3.13		19-MAR-10 13:56	per0319022a
Perchlorate-101	.5	.46	91.49	19-MAR-10 13:56	per0319022a

Quantify Sample Report MassLynx 4.0 SP4


The GEL Group, LLC Analyst: Charlers W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per031910a.qld

Last Altered: Saturday, March 20, 2010 1:22:43 PM Eastern Standard Time
Printed: Saturday, March 20, 2010 1:32:33 PM Eastern Standard Time

Name: per0319022a
Date: 19-Mar-2010
Time: 13:56:52
D: WCL100318-06CCV
/ial: 1:2,A

per0319022a
03-20-10

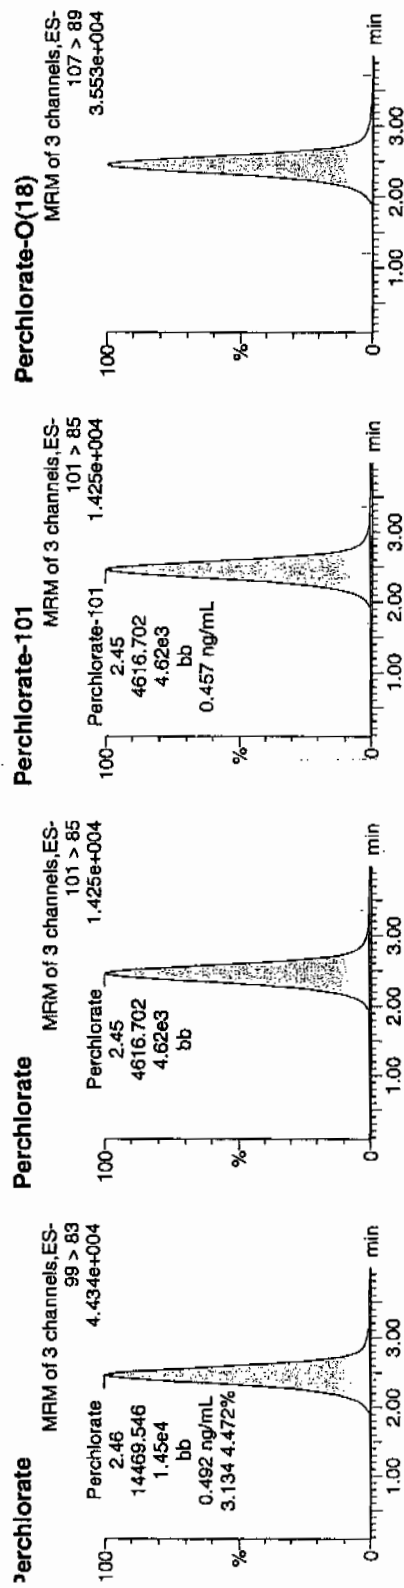

Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	S/N	Ion.Ratio
VCL100318-06CCV	Perchlorate	99 > 83	2.46	14469.546	14469.546	bb		0.4917	98.34	-1.66	1562.4...	3.13
VCL100318-06CCV	Perchlorate-101	101 > 85	2.45	4616.702	4616.702	bb		0.4575	91.49	-8.51	2931.0...	
VCL100318-06CCV	Perchlorate-O(18)	107 > 89	2.45	11718.223	11718.223	bb		0.4824	96.49	-3.51	912.670	

107
3/22/10

Perchlorate MDL Verification

Lab Name: General Engineering Laboratories

GEL Job No.(SDG): 10-2093-1

Lab Code: GEL

Reporting Units: ug/kg

Analyte	True	Found	%Rec	Date Analyzed	GEL File Id
Perchlorate	.05	.05	98.34	19-MAR-10 12:38	per0319011a
Perchlorate Isotope Ratio		3.07		19-MAR-10 12:38	per0319011a
Perchlorate-101	.05	.05	93.42	19-MAR-10 12:38	per0319011a
Perchlorate	.05	.05	92.33	19-MAR-10 14:11	per0319024a
Perchlorate Isotope Ratio		2.86		19-MAR-10 14:11	per0319024a
Perchlorate-101	.05	.05	94.1	19-MAR-10 14:11	per0319024a


Quantity Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charliers W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per031910a.qld

Last Altered: Saturday, March 20, 2010 1:22:43 PM Eastern Standard Time
Printed: Saturday, March 20, 2010 1:32:33 PM Eastern Standard Time

Sample Name: per0319011a
Date: 19-Mar-2010
Time: 12:38:41
File: WCL100318-07CRI
Label: 1:2,B

Res
603
20.20.10

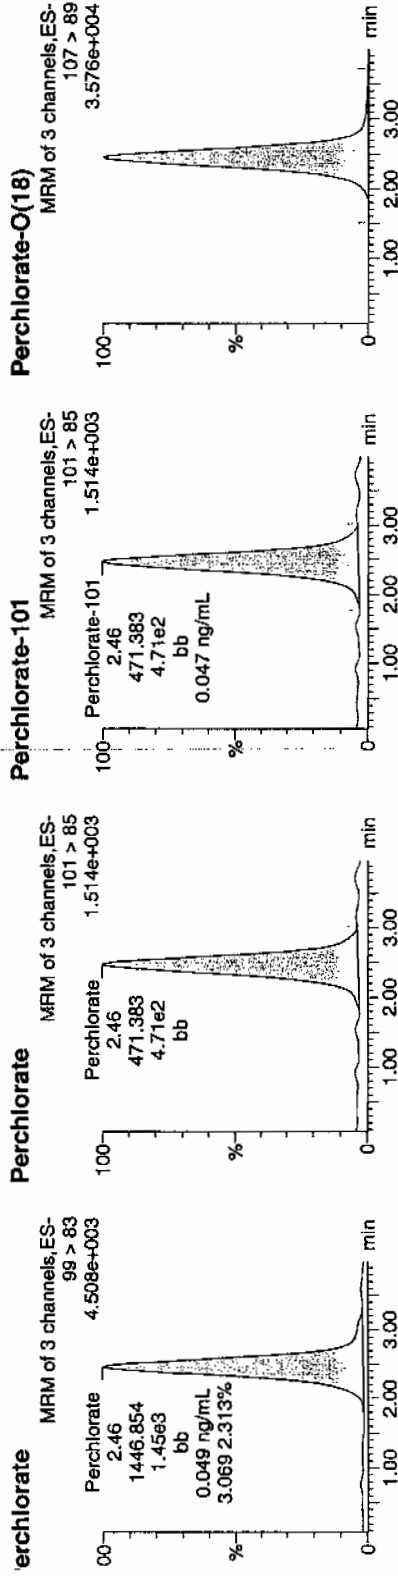

Name	Trace	RT	Area	Response	Flags	Mod.Date	Mod.Time	ng/mL	%Rec	%Dev	S/N	Ion Ratio
per0319011a	99 > 83	2.46	1446.854	1446.854	bb			0.0492	98.34	-1.66	227.011	3.07
per0319011a	101 > 85	2.46	471.383	471.383	bb			0.0467	93.42	-6.58	230.390	
per0319011a	107 > 89	2.45	11715.260	11715.260	bb			0.4823	96.46	-3.54	5477.3...	

$$\frac{1446.854}{471.383} = 3.0694$$

Aut
3/20/10





Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charles W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per031910a.qld

Last Altered: Saturday, March 20, 2010 1:22:43 PM Eastern Standard Time
Printed: Saturday, March 20, 2010 1:32:33 PM Eastern Standard Time

Sample Name: per0319024a
Date: 19-Mar-2010
Time: 14:11:04
Job: WCL100318-07CRI
Vial: 1:2,B

Page 30
03-20-10

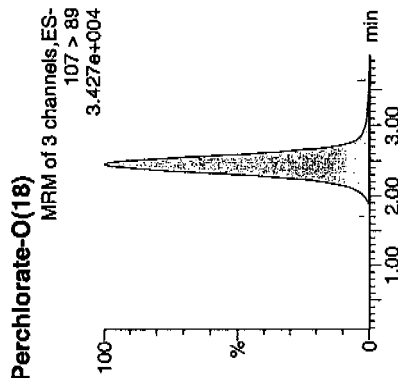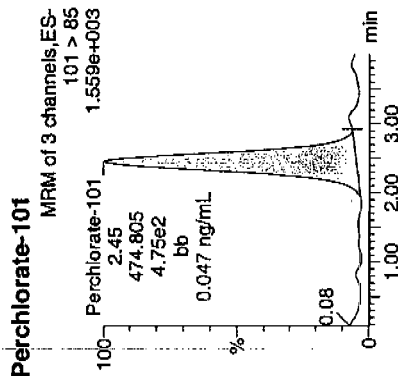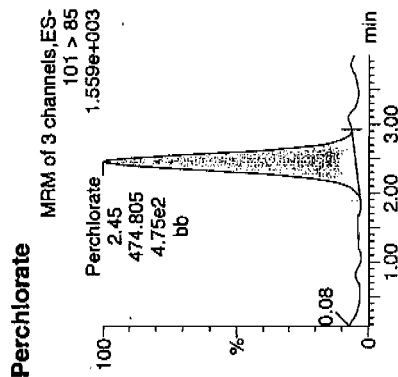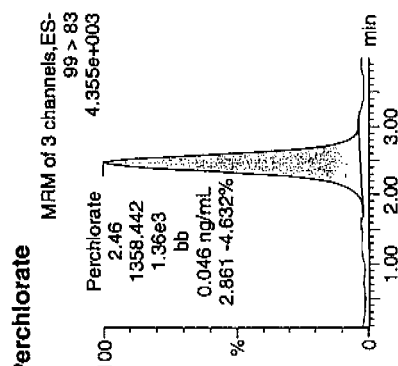

Name	Trace	RT	Area	Response	Flags	Mod Date	Mod Time	ng/mL	%Rec	%Dev	S/N	Ion Ratio
VCL100318-07CRI	Perchlorate	99 > 83	2.46	1358.442	bb			0.0462	92.33	-7.67	252.858	2.86
VCL100318-07CRI	Perchlorate-101	101 > 85	2.45	474.805	bb			0.0470	94.10	-5.90	180.052	
VCL100318-07CRI	Perchlorate-Q(18)	107 > 89	2.44	11259.898	bb			0.4636	92.71	-7.29	2545.0...	

MT
3/22/10

IEL SOP GL-OA-E-067, Method 6850-Modified / MM = Manual Modification

QUALITY CONTROL

Perchlorate Analysis Data Sheet

Lab Name: GEL Laboratories LLC

Lab Code: GEL

Instrument: LCMSMS

Method: EPA 6850 Modified

Matrix: SOIL

Extraction Batch ID: 959007

Extraction Type: Solid Prep

Sample Volume/Weight: 2.00 g

Concentrated Extract Volume: 20.0

Client Sample No.

MB

Date Received: 12-MAR-10

GEL Job No (SDG): 10-2093-1

GEL Sample ID: 1202056676

Date Filtered: 12-MAR-10

Injection Volume (uL): 20

%Solids: 100

CAS No.	Analyte [^]	MDL	RL	Conc*	Units	Q	Dilution Factor	Date Analyzed	GEL File ID
14797-73-0	Perchlorate	.5	2	0.500	ug/kg	U	1	19-MAR-10 12:46	per0319012a
	Perchlorate Isotope Ratio						1	19-MAR-10 12:46	per0319012a
14797-73-0	Perchlorate-101	.5	2	0.500	ug/kg	U	1	19-MAR-10 12:46	per0319012a
	Perchlorate-O(18)			4.45	ug/kg		1	19-MAR-10 12:46	per0319012a

[^] When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

*Concentration =

Instrument Value X $\frac{\text{Concentrated Extract Volume}}{\text{Aliquot}}$ X $\frac{1}{\% \text{Solids}}$


Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charlers W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per031910a.qld

Last Altered: Saturday, March 20, 2010 1:22:43 PM Eastern Standard Time
Printed: Saturday, March 20, 2010 1:32:33 PM Eastern Standard Time

Name: per0319012a
Date: 19-Mar-2010
Time: 12:46:18
ID: 1202056676
Vial: 1:3,A

1202056676 | 954012 | 3020 | MB | 1 | 1
03-20-10

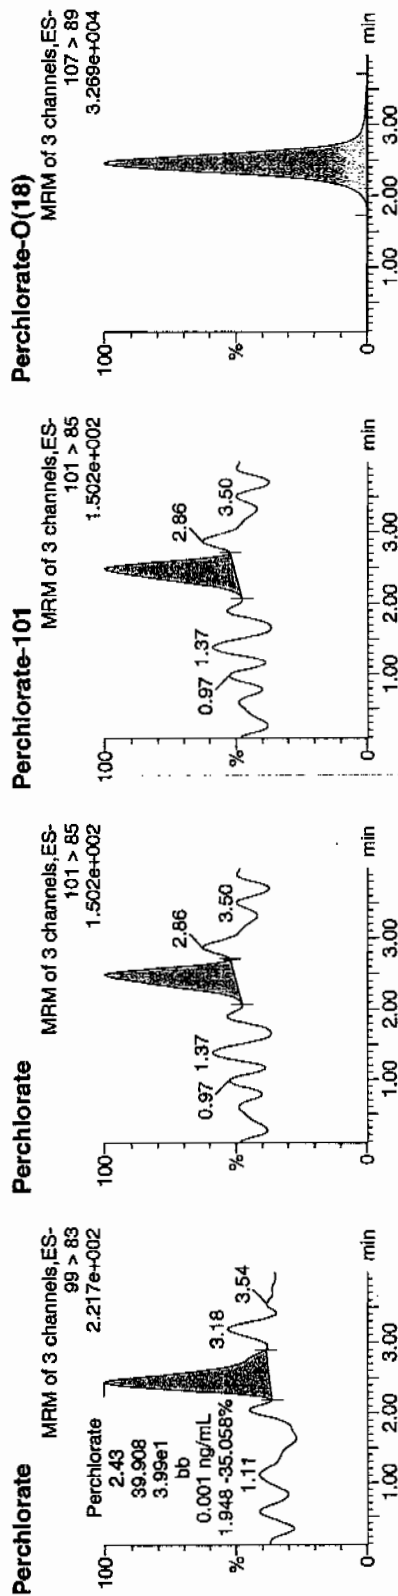

Name	Trace	RT	Area	Response	Flags	Mod	Date	Time	File	Rec	Area	SN	Ratio
1202056676	Perchlorate	99 > 83	2.43	39.908	bb					0.0014	9.348	1.95	
1202056676	Perchlorate-101	101 > 85	2.48	20.484	bb					0.0020	14.470		
1202056676	Perchlorate-O(18)	107 > 89	2.45	10813.935	bb					0.4452	89.04	2410.7...	

OKAY
24.0300
not
312660

Form 1

Perchlorate Analysis Data Sheet

Lab Name: GEL Laboratories LLC

Lab Code: GEL

Instrument: LCMSMS

Method: EPA 6850 Modified

Matrix: SOIL

Extraction Batch ID: 959007

Extraction Type: Solid Prep

Sample Volume/Weight: 2.00 g

Concentrated Extract Volume: 20.0

Client Sample No.

LCS

Date Received: 12-MAR-10

GEL Job No (SDG): 10-2093-1

GEL Sample ID: 1202056677

Date Filtered: 12-MAR-10

Injection Volume (uL): 20

%Solids: 100

CAS No.	Analyte [^]	MDL	RL	Conc*	Units	Q	Dilution Factor	Date Analyzed	GEL File ID
14797-73-0	Perchlorate	.5	2	2.03	ug/kg		1	19-MAR-10 12:53	per0319013a
	Perchlorate Isotope Ratio			3.05			1	19-MAR-10 12:53	per0319013a
14797-73-0	Perchlorate-101	.5	2	1.94	ug/kg	J	1	19-MAR-10 12:53	per0319013a
	Perchlorate-O(18)			4.91	ug/kg		1	19-MAR-10 12:53	per0319013a

[^] When the analyte name is Perchlorate Isotope Ratio the concentration is a unitless value calculated from the ratio of Perchlorate peak area to Perchlorate-101 peak area. The Perchlorate-101 and isotopic ratio results are provided for qualitative purposes only. The results are used to verify the presence and quantitation of Perchlorate.

*Concentration =

Instrument Value X Concentrated Extract Volume X 1 %Solids
Aliquot

Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charlers W. Wilson


Dataset: C:\MassLynx\Perchlorate.PRO\per031910a.qld

Last Altered: Saturday, March 20, 2010 1:22:43 PM Eastern Standard Time
Printed: Saturday, March 20, 2010 1:32:33 PM Eastern Standard Time

Name: per0319013a
Date: 19-Mar-2010
Time: 12:53:21
ID: 1202056677
Vial: 1:3,B

603
30.20.10

1202056677 | 30.20 | LUS | 11

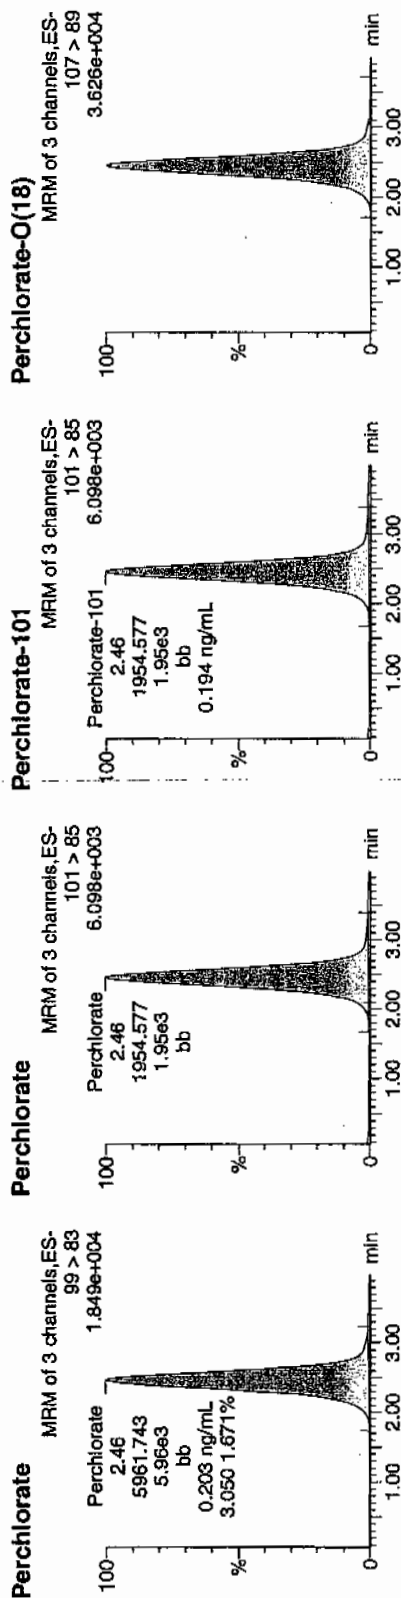

Name	Trace	Area	Response	Flags	Mod Date	Mod Time	Mod User	Rec	Day	SIN	Ratio
1202056677	Perchlorate	99 > 83	2.46	5961.743	5961.743	bb		0.2026	101.30	1.30	2435.2...
1202056677	Perchlorate-101	101 > 85	2.46	1954.577	1954.577	bb		0.1937	96.84	-3.16	920.075
1202056677	Perchlorate-O(18)	107 > 89	2.45	11935.557	11935.557	bb		0.4914	98.28	-1.72	3385.6...

5961.743
29427
= 0.2026

not
3/22/10

GEL SOP GL-OA-E-067, Method 6850-Modified / MM = Manual Modification

MISCELLANEOUS DATA

Prep Logbook

Definitive Low Level Perchlorate Analysis Utilizing Liquid Chromatography/Mass Spectrometry/Mass Spectrometry (LC/MS/MS) by EPA Method 6850 Modified (6850M)

Batch ID: 959007 Verified by: _____
 Analyst: Kaylie Westmoreland
 Method: SW846 6850 Modified
 Lab SOP: GL-OA-E-067 REV# 6
 Instrument: MicroMass Quattro Ultima

Sample ID	Run Date	Allquot (g)	Prepped Aliquot (mL)	Prepped Factor (mL/g)
1202056676 MB	12-MAR-2010 14:07:00	2	20	10
1202056677 LCS	12-MAR-2010 14:07:00	2	20	10
248118001	12-MAR-2010 14:07:00	2	20	10
248118002	12-MAR-2010 14:07:00	2	20	10
248118003	12-MAR-2010 14:07:00	2	20	10
248118004	12-MAR-2010 14:07:00	2	20	10
248118005	12-MAR-2010 14:07:00	2	20	10
248118006	12-MAR-2010 14:07:00	2	20	10
248118007	12-MAR-2010 14:07:00	2	20	10
248198001	12-MAR-2010 14:07:00	2	20	10
1202056678 MS (248198001)	12-MAR-2010 14:07:00	2	20	10
1202056679 MSD (248198001)	12-MAR-2010 14:07:00	2	20	10
248198002	12-MAR-2010 14:07:00	2	20	10
248198003	12-MAR-2010 14:07:00	2	20	10
248198004	12-MAR-2010 14:07:00	2	20	10
248198005	12-MAR-2010 14:07:00	2	20	10
248198006	12-MAR-2010 14:07:00	2	20	10
248198007	12-MAR-2010 14:07:00	2	20	10
248198008	12-MAR-2010 14:07:00	2	20	10
248198009	12-MAR-2010 14:07:00	2	20	10
248198010	12-MAR-2010 14:07:00	2	20	10
248198011	12-MAR-2010 14:07:00	2	20	10
248198012	12-MAR-2010 14:07:00	2	20	10
1202056681 ICS	12-MAR-2010 14:07:00	2	20	10

Comments:

Type	Sample Id	Description	Serial Number	Spike Amt	Units
ICS	1202056681	10 ug/L ICV/CCV Second Source	UCL100311-01.1	.4	mL
LCS	1202056677	10 ug/L ICV/CCV Second Source	UCL100311-01.1	.4	mL
MSD	1202056679	10 ug/L ICV/CCV Second Source	UCL100311-01.1	.4	mL

Desalting Cartridges used: 100216-1-H & 100211-1-Ba

GEL ORGANIC RUN LOG

INSTRUMENT ID: LCMSMS#2

Date: 03/19/10
 Extr. Injection Volume: 20uL
 Sequence Number: per031910a
 Initial Calibration Date: 03/19/10

Method: EPA 6850-Modified
 Int. Std.: UCL100210-01
 Mobile Phase Lot#: 1278668, 1271949
 Standard-Samp Reagent Lot#: 1271949

Reviewed BY: mta
 Date: 3/22/10
 SOP: GL-OA-E-067 Rev.6
 Alt Check Std. ID: WCL100318-06

DataFile	Sample	Analyst	Injection Date	Batch	SDG	Dilution	Client	Comments	QC_Flag
per0319001a	IPB001	CWW	3/19/2010 11:27			1		USE	B
per0319002a	IPB001	CWW	3/19/2010 11:34			1		USE	B
per0319003a	WCLICAL-01	CWW	3/19/2010 11:41			1		USE	I
per0319004a	WCLICAL-02	CWW	3/19/2010 11:48			1		USE	I
per0319005a	WCLICAL-03	CWW	3/19/2010 11:55			1		USE	I
per0319006a	WCLICAL-04	CWW	3/19/2010 12:03			1		USE	I
per0319007a	WCLICAL-05	CWW	3/19/2010 12:10			1		USE	I
per0319008a	IPB002	CWW	3/19/2010 12:17			1		USE	B
per0319009a	WCLICV	CWW	3/19/2010 12:24			1		USE	C
per0319010a	IPB003	CWW	3/19/2010 12:31			1		USE	B
per0319011a	WCLCRI	CWW	3/19/2010 12:38			1		USE	C
per0319012a	1202056676	CWW	3/19/2010 12:46	959012	VARIOUS	1	LANL	USE	S
per0319013a	1202056677	CWW	3/19/2010 12:53	959012	VARIOUS	1	LANL	USE	S
per0319014a	1202056681	CWW	3/19/2010 13:00	959012	VARIOUS	1	LANL	USE	S
per0319015a	248118001	CWW	3/19/2010 13:07	959012	10-2093-1	1	LANL	USE	S
per0319016a	248118002	CWW	3/19/2010 13:14	959012	10-2093-1	1	LANL	USE	S
per0319017a	248118003	CWW	3/19/2010 13:21	959012	10-2093-1	1	LANL	USE	S
per0319018a	248118004	CWW	3/19/2010 13:28	959012	10-2093-1	1	LANL	USE	S
per0319019a	248118005	CWW	3/19/2010 13:35	959012	10-2093-1	1	LANL	USE	S
per0319020a	248118006	CWW	3/19/2010 13:42	959012	10-2093-1	1	LANL	USE	S
per0319021a	248118007	CWW	3/19/2010 13:49	959012	10-2093-1	1	LANL	USE	S
per0319022a	WCLCCV	CWW	3/19/2010 13:56			1		USE	C
per0319023a	IPB004	CWW	3/19/2010 14:04			1		USE	B
per0319024a	WCLCRI	CWW	3/19/2010 14:11			1		USE	C
per0319025a	248198001	CWW	3/19/2010 14:18	959012	10-2122	1	LANL	DUSE-DL	S
per0319026a	1202056678	CWW	3/19/2010 14:25	959012	10-2122	1	LANL	DUSE-DL	S
per0319027a	1202056679	CWW	3/19/2010 14:32	959012	10-2122	1	LANL	DUSE-DL	S
per0319028a	248198002	CWW	3/19/2010 14:39	959012	10-2122	1	LANL	DUSE-DL	S
per0319029a	248198003	CWW	3/19/2010 14:46	959012	10-2122	1	LANL	DUSE-DL	S

per0319030a	248198004	CWW	3/19/2010 14:53	959012	10-2122	1	LANL	DUSE-DL	S
per0319031a	248198005	CWW	3/19/2010 15:00	959012	10-2122	1	LANL	DUSE-DL	S
per0319032a	248198006	CWW	3/19/2010 15:07	959012	10-2122	1	LANL	DUSE-RA	S
per0319033a	248198007	CWW	3/19/2010 15:14	959012	10-2122	1	LANL	DUSE-DL	S
per0319034a	248198008	CWW	3/19/2010 15:21	959012	10-2122	1	LANL	DUSE-RA	S
per0319035a	WCLCCV	CWW	3/19/2010 15:28			1		USE	C
per0319036a	IPB005	CWW	3/19/2010 15:35			1		USE	B
per0319037a	WCLCRI	CWW	3/19/2010 15:42			1		USE	C
per0319038a	248198009	CWW	3/19/2010 15:49	959012	10-2122	1	LANL	USE	S
per0319039a	248198010	CWW	3/19/2010 15:56	959012	10-2122	1	LANL	USE	S
per0319040a	248198011	CWW	3/19/2010 16:03	959012	10-2122	1	LANL	USE	S
per0319041a	248198012	CWW	3/19/2010 16:11	959012	10-2122	1	LANL	USE	S
per0319042a	IPB006	CWW	3/19/2010 16:18			1		USE	B
per0319043a	1202056685	CWW	3/19/2010 16:25	959022	10-2129	1	LANL	USE	S
per0319044a	1202056686	CWW	3/19/2010 16:32	959022	10-2129	1	LANL	USE	S
per0319045a	1202056689	CWW	3/19/2010 16:39	959022	10-2129	1	LANL	USE	S
per0319046a	248233001	CWW	3/19/2010 16:46	959022	10-2129	1	LANL	USE	S
per0319047a	1202056687	CWW	3/19/2010 16:54	959022	10-2129	1	LANL	USE	S
per0319048a	WCLCCV	CWW	3/19/2010 17:01			1		USE	C
per0319049a	IPB007	CWW	3/19/2010 17:08			1		USE	B
per0319050a	WCLCRI	CWW	3/19/2010 17:16			1		USE	C
								USE	
								DUSE-RA	
								DUSE-RA	
								DUSE-RA	
								DUSE-RA	
								DUSE-RA	
								USE	
								USE	
								USE	

Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charlers W. Wilson

Dataset: C:\MassLynx\Perchlorate.PRO\per032010a.qld

Last Altered: Sunday, March 21, 2010 8:29:18 AM Eastern Standard Time
Printed: Sunday, March 21, 2010 8:43:52 AM Eastern Standard Time

Name: per0320013a

Date: 20-Mar-2010

Time: 19:06:57


ID: 1202056678

Vial: 1:3,B


03-21-10

1202056678 | 959012 | 30020 | MS | 2/10


Perchlorate

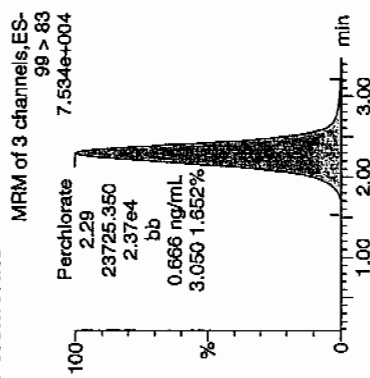


Perchlorate

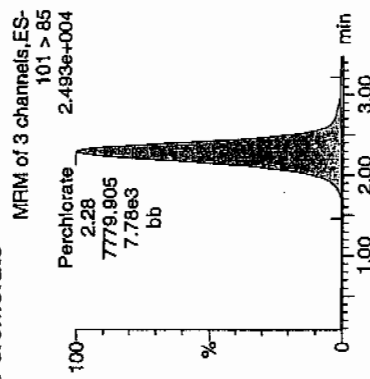

Perchlorate-101

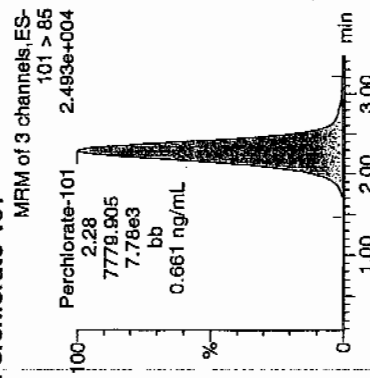

Perchlorate-O(18)

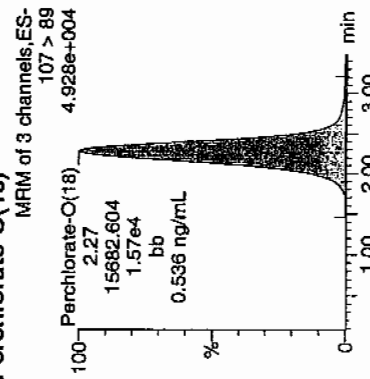

File	RT	Mass	Response	Area	Conc	SN	Ratio
1202056678	Perchlorate	99 > 83	2.29	23725.350	bb	0.6660	332.99 232.99 4539.0...
1202056678	Perchlorate-101	101 > 85	2.28	7779.905	bb	0.6612	330.62 230.62 455.893
1202056678	Perchlorate-O(18)	107 > 89	2.27	15682.604	bb	0.5363	107.27 7.27 8031.3...

- 1.33
x2
= 1.32
WAT
3/22/10

Quantify Sample Report MassLynx 4.0 SP4
The GEL Group, LLC Analyst: Charlers W. Wilson


Dataset: C:\MassLynx\Perchlorate.PRO\per032010a.qld

Last Altered: Sunday, March 21, 2010 8:29:18 AM Eastern Standard Time
Printed: Sunday, March 21, 2010 8:43:52 AM Eastern Standard Time

Name: per0320014a
Date: 20-Mar-2010
Time: 19:13:30
ID: 1202056679
Vial: 1:3,C

03-24-10

1202056679 | 959012 | 30020 | 150 | 2 | 0

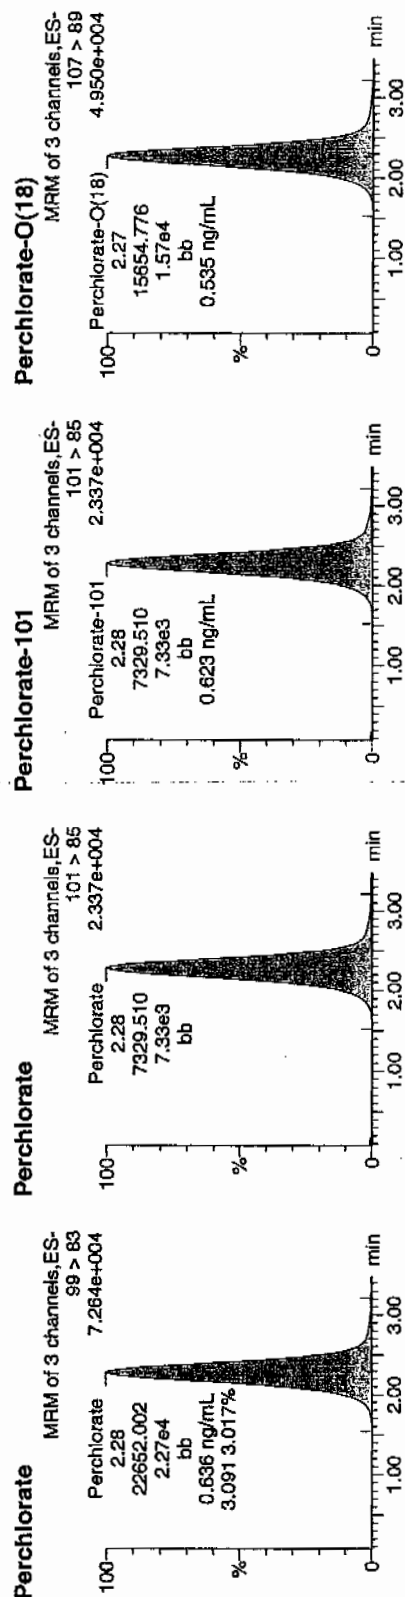

ID	Name	Area	Ratio	Response	Mass	Weight	Volume	Conc	Ratio	SN	Ratio
1202056679	Perchlorate	99 > 83	2.28	22652.002	22652.002	bb		0.6359	317.93	217.93	772.708
1202056679	Perchlorate-101	101 > 85	2.28	7329.510	7329.510	bb		0.6230	311.48	211.48	4082.1...
1202056679	Perchlorate-O(18)	107 > 89	2.27	15654.776	15654.776	bb		0.5354	107.07	7.07	1018.0...

✓ = 1.27
x2
= 1.25
100%
3/24/10

GEL Laboratories LLC
Form GEL-DER

DER Report No.: 807337

Revision No.: 2

DATA EXCEPTION REPORT

Mo.Day Yr. 21-MAR-10	Division: Federal	Quality Criteria: Specifications	Type: Process
Instrument Type: LC-MS/MS	Test / Method: SW846 6850 Modified	Matrix Type: Solid	Client Code: LANL010
Batch ID: 959012	Sample Numbers: See below		
Potentially affected work order(s)(SDG): 248118(10-2093-1),248198(10-2122) Application Issues: Failed Recovery for MS/PS			
Specification and Requirements		DER Disposition:	
Exception Description: 1. High recovery of Perchlorate-101 was observed in 1202056678 (MS). The recovery was 127% and the acceptance range is 75-125%.		1. The high recovery may be the result of the background concentration present in the parent sample, 248198001, and the need to dilute all at 1:2 prior to analysis.	

Originator's Name:

Charles Wilson 21-MAR-10

Data Validator/Group Leader:

Herbert Maier 23-MAR-10

Isotope Ratio Criteria

Isotope Ratio $^{35}\text{Cl}/^{37}\text{Cl}$

2.31-3.85

Tune Criteria

The tuning solution is introduced directly into the mass spectrometer using the ESI interface in the positive ion mode. The mass range scanned is 20 to 1100 amu using at least six scans. The observed mass for the target compound in the daily calibration standards must be within 0.2 amu of the expected value. If it is greater than 0.2 amu, then a mass calibration is performed and the instrument is re-calibrated.

Metals Analysis

Case Narrative

**Metals Fractional Narrative
Los Alamos National Laboratory (LANL)
SDG 10-2093**

Sample Analysis

Sample ID	Client ID
248117001	RE36-10-8458
1202056866	Method Blank (MB) ICP
1202056867	Laboratory Control Sample (LCS)
1202056870	248199001(RE36-10-7529L) Serial Dilution (SD)
1202056868	248199001(RE36-10-7529D) Sample Duplicate (DUP)
1202056869	248199001(RE36-10-7529S) Matrix Spike (MS)
1202056872	Method Blank (MB) ICP-MS
1202056873	Laboratory Control Sample (LCS)
1202056876	248199001(RE36-10-7529L) Serial Dilution (SD)
1202056874	248199001(RE36-10-7529D) Sample Duplicate (DUP)
1202056875	248199001(RE36-10-7529S) Matrix Spike (MS)
1202056573	Method Blank (MB) CVAA
1202056574	Laboratory Control Sample (LCS)
1202056577	248145001(WST16-10-12239L) Serial Dilution (SD)
1202056575	248145001(WST16-10-12239D) Sample Duplicate (DUP)
1202056576	248145001(WST16-10-12239S) Matrix Spike (MS)

The samples in this SDG were analyzed on an "as received" basis.

Method/Analysis Information

Analytical Batch:	959109, 959112 and 958951
Prep Batch :	959108, 959110 and 958949
Standard Operating Procedures:	GL-MA-E-013 REV# 20, GL-MA-E-006 REV# 9, GL-MA-E-014 REV# 21 and GL-MA-E-010 REV# 23
Analytical Method:	SW846 3005/6010B, SW846 3005/6020 and SW846 7470A
Prep Method :	SW846 3005A and SW846 7470A Prep

Preparation/Analytical Method Verification

The SOP stated above has been prepared based on technical research and testing conducted by GEL Laboratories, LLC. and with guidance from the regulatory documents listed in this "Method/Analysis Information" section.

System Configuration

The Metals analysis-ICP was performed on a P E 7300 Optima radial/axial-viewing inductively coupled plasma atomic emission spectrometer. The instrument is equipped with a Burgener nebulizer, cyclonic spray chamber, and yttrium or scandium internal standard. Operating conditions for the ICP are set at a power level of 1500 watts. The instrument has a peristaltic pump flow rate of 1.4L/min, argon gas flows of 15 L/min and 0.2 L/min for the torch and auxiliary gases, and a flow setting of 0.65L/min for the nebulizer.

The Metals analysis - ICPMS was performed on a Perkin Elmer ELAN 6100E inductively coupled plasma mass spectrometer (ICP-MS). The instrument is equipped with a cross-flow nebulizer, quadrupole mass spectrometer, and dual mode electron multiplier detector. Internal standards of scandium, germanium, indium, tantalum, and/or lutetium were utilized to cover the mass spectrum. Operating conditions are set at 1400W power and combined argon pressures of 360+/-7 kPa for the plasma and auxiliary gases, and 0.85 L/min carrier gas flow, and an initial lens voltage of 5.2.

The Metals analysis - ICPMS was performed on a Perkin Elmer ELAN 9000 inductively coupled plasma mass spectrometer (ICP-MS). The instrument is equipped with a cross-flow nebulizer, quadrupole mass spectrometer, and dual mode electron multiplier detector. Internal standards of scandium, germanium, indium, tantalum, and/or lutetium were utilized to cover the mass spectrum. Operating conditions are set at 1400W power and combined argon pressures of 360+/-7 kPa for the plasma and auxiliary gases, and 0.85 L/min carrier gas flow, and an initial lens voltage of 5.2.

The Metals analysis-Mercury was performed on a Perkin-Elmer Flow Injection Mercury System (FIMS-100) automated mercury analyzer. The instrument consists of a cold vapor atomic absorption spectrometer set to detect mercury at a wavelength of 253.7 nm. Sample introduction through the flow injection system is performed via a peristaltic pump at 9 mL/min and nitrogen carrier gas rate of 80 mL/min.

Calibration Information

Instrument Calibration

All initial calibration requirements have been met for this sample delivery group (SDG).

CRDL Requirements

All CRDL standard(s) met the referenced advisory control limits.

ICSA/ICSAB Statement

All interference check samples (ICSA and ICSAB) associated with this SDG met the established acceptance criteria.

Continuing Calibration Blank (CCB) Requirements

All continuing calibration blanks (CCB) bracketing this batch met the established acceptance criteria with the exception of thallium in CCB04.

Continuing Calibration Verification (CCV) Requirements

All continuing calibration verifications (CCV) bracketing this SDG met the acceptance criteria.

Quality Control (QC) Information**Method Blank (MB) Statement**

The MBs analyzed with this SDG met the acceptance criteria.

Laboratory Control Sample (LCS) Recovery

The LCS spike recoveries met the acceptance limits.

Quality Control (QC) Sample Statement

The following samples were selected as the quality control (QC) samples for this SDG: 248199001 (RE36-10-7529)-ICP and ICP-MS and 248145001 (WST16-10-12239)-CVAA.

Matrix Spike (MS) Recovery Statement

The percent recoveries (%R) obtained from the MS analyses are evaluated when the sample concentration is less than four times (4X) the spike concentration added. All applicable elements met the acceptance criteria.

Duplicate Relative Percent Difference (RPD) Statement

The RPD obtained from the designated sample duplicate (DUP) is evaluated based on acceptance criteria of 20% when the sample is >5X the contract required detection limit (RL). In cases where either the sample or duplicate value is less than 5X the RL, a control of +/-RL is used to evaluate the DUP results. All applicable analytes met these requirements.

Serial Dilution % Difference Statement

The serial dilution is used to assess matrix suppression or enhancement. Raw element concentrations that are 25X the IDL/MDL for CVAA, 50X the IDL/MDL for ICP, and 100X the IDL/MDL for ICP-MS analyses are applicable for serial dilution assessment. All applicable analytes met the acceptance criteria of less than 10% difference (%D).

Technical Information**Holding Time Specifications**

GEL assigns holding times based on the associated methodology, which assigns the date and time from sample collection of sample receipt. Those holding times expressed in hours are calculated in the AlphaLIMS system. Those holding times expressed as days expire at midnight

on the day of expiration. All samples in this SDG met the specified holding time.

Sample Dilutions

Dilutions are performed to minimize matrix interferences resulting from elevated mineral element concentrations present in solid samples and/or to bring over range target analyte concentrations into the linear calibration range of the instrument. The samples in this SDG did not require dilutions.

Preparation Information

The samples in this SDG were prepared exactly according to the cited SOP.

Miscellaneous Information

Electronic Packaging Comment

This data package was generated using an electronic data processing program referred to as virtual packaging. In an effort to increase quality and efficiency, the laboratory has developed systems to generate all data packages electronically. The following change from traditional packages should be noted:

Analyst/peer reviewer initials and dates are not present on the electronic data files. Presently, all initials and dates are present on the original raw data. These hard copies are temporarily stored in the laboratory. The data validator will always sign and date the case narrative. Data that are not generated electronically, such as hand written pages, will be scanned and inserted into the electronic package.

Data Exception (DER) Documentation

Data exception reports (DERs) are generated to document procedural anomalies that may deviate from referenced SOP or contractual documents. A data exception report (DER) was not generated for this SDG.

Additional Comments

Additional comments were not required for this SDG.

Certification Statement

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless otherwise noted in the analytical case narrative.

Review Validation:

GEL requires all analytical data to be verified by a qualified data validator. In addition, all data designated for CLP or CLP-like packaging will receive a third level validation upon completion of the data package.

The following data validator verified the information presented in this case narrative:

Reviewer: Nikhil A. Emre Date: 4.17.10

Sample Data Summary

METALS
-1-
INORGANICS ANALYSIS DATA PACKAGE

SDG No: 10-2093

CONTRACT: LANL01004

METHOD TYPE: SW846

SAMPLE ID: 248117001

BASIS: As Received

DATE COLLECTED 22-FEB-10

CLIENT ID: RE36-10-8458

LEVEL: Low

DATE RECEIVED 26-FEB-10

MATRIX: WATER

%SOLIDS: 0

CAS No.	Analyte	Result	Units	Qual	MDL	PQL	CRDL	DF	M*	Analyst	Run Date	Analytical Run	Analytical Batch
7429-90-5	Aluminum	200	ug/L	U	68	200	200	1	P	HSC	03/29/10 20:44	032910C-1	959109
7440-36-0	Antimony	3	ug/L	U	1	3	3	1	MS	PRB	04/13/10 13:49	100413-3	959112
7440-38-2	Arsenic	30	ug/L	U	5	30	30	1	P	HSC	03/29/10 20:44	032910C-1	959109
7440-39-3	Barium	5	ug/L	U	1	5	5	1	P	HSC	03/29/10 20:44	032910C-1	959109
7440-41-7	Beryllium	0.50	ug/L	U	0.1	0.5	0.5	1	MS	BCD1	04/12/10 04:22	100411-2	959112
7440-43-9	Cadmium	1	ug/L	U	0.11	1	1	1	MS	BCD1	04/12/10 04:22	100411-2	959112
7440-70-2	Calcium	53	ug/L	J	50	200	200	1	P	HSC	03/29/10 20:44	032910C-1	959109
7440-47-3	Chromium	5	ug/L	U	1	5	5	1	P	HSC	03/29/10 20:44	032910C-1	959109
7440-48-4	Cobalt	5	ug/L	U	1	5	5	1	P	HSC	03/29/10 20:44	032910C-1	959109
7440-50-8	Copper	6.57	ug/L	J	3	10	10	1	P	HSC	03/29/10 20:44	032910C-1	959109
7439-89-6	Iron	100	ug/L	U	30	100	100	1	P	HSC	03/29/10 20:44	032910C-1	959109
7439-92-1	Lead	0.866	ug/L	J	0.5	2	2	1	MS	BCD1	04/12/10 04:22	100411-2	959112
7439-95-4	Magnesium	300	ug/L	U	85	300	300	1	P	HSC	03/29/10 20:44	032910C-1	959109
7439-96-5	Manganese	5	ug/L	U	1	5	5	1	MS	BCD1	04/12/10 04:22	100411-2	959112
7439-97-6	Mercury	0.20	ug/L	U	0.066	0.2	0.2	1	AV	JXL1	03/02/10 11:58	030210W3-6	958951
7440-02-0	Nickel	5	ug/L	U	1.5	5	5	1	P	HSC	03/29/10 20:44	032910C-1	959109
7440-09-7	Potassium	293	ug/L		50	150	150	1	P	HSC	03/29/10 20:44	032910C-1	959109
7782-49-2	Selenium	30	ug/L	U	5	30	30	1	P	HSC	03/29/10 20:44	032910C-1	959109
7440-22-4	Silver	5	ug/L	U	1	5	5	1	P	HSC	03/29/10 20:44	032910C-1	959109
7440-23-5	Sodium	140	ug/L	J	100	300	300	1	P	HSC	03/29/10 20:44	032910C-1	959109
7440-28-0	Thallium	1	ug/L	U	0.3	1	1	1	MS	BCD1	04/12/10 04:22	100411-2	959112
7440-61-1	Uranium	0.20	ug/L	U	0.05	0.2	0.2	1	MS	PRB	04/13/10 16:22	100413-5	959112
7440-62-2	Vanadium	5	ug/L	U	1	5	5	1	P	HSC	03/29/10 20:44	032910C-1	959109
7440-66-6	Zinc	6.16	ug/L	J	3.3	10	10	1	P	HSC	03/29/10 20:44	032910C-1	959109

Prep Information:

Analytical Batch	Prep Batch	Prep Method	Initial wt./vol.	Units	Final wt./vol.	Units	Date	Analyst
958951	958949	SW846 7470A Prep	20	mL	20	mL	03/01/10	TXB3
959109	959108	SW846 3005A	50	mL	50	mL	03/04/10	FGA
959112	959110	SW846 3005A	50	mL	50	mL	03/04/10	FGA

Quality Control Summary

METALS
-2a-
Initial and Continuing Calibration Verification

SDG No: 10-2093

Contract: LANL01004

Lab Code: GEL

Initial Calibration Source: Solutions Plus

Continuing Calibration Source: O2Si

Instrument ID: HG3,ICPMS4,ICPMS5,OPTIMA4

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>True Value</u>	<u>Units</u>	<u>% Recovery</u>	<u>Acceptance Window (%R)</u>	<u>M</u>	<u>Analysis Date/Time</u>	<u>Run Number</u>
ICV01										
	Mercury	5.2	ug/L	5	ug/L	104	90.0 – 110.0	AV	02-MAR-10 08:39	030210W3-6
	Aluminum	5140	ug/L	5000	ug/L	102.7	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Arsenic	479	ug/L	500	ug/L	95.8	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Barium	508	ug/L	500	ug/L	101.6	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Calcium	5000	ug/L	5000	ug/L	100	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Chromium	488	ug/L	500	ug/L	97.6	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Cobalt	506	ug/L	500	ug/L	101.3	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Copper	510	ug/L	500	ug/L	102	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Iron	5010	ug/L	5000	ug/L	100.3	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Magnesium	5200	ug/L	5000	ug/L	103.9	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Nickel	495	ug/L	500	ug/L	99	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Potassium	2470	ug/L	2500	ug/L	98.7	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Selenium	2470	ug/L	2500	ug/L	98.8	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Silver	257	ug/L	250	ug/L	102.8	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Sodium	2460	ug/L	2500	ug/L	98.5	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Vanadium	505	ug/L	500	ug/L	100.9	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Zinc	497	ug/L	500	ug/L	99.4	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Beryllium	51.8	ug/L	50	ug/L	103.6	90.0 – 110.0	MS	12-APR-10 03:01	100411-2
	Cadmium	51.2	ug/L	50	ug/L	102.5	90.0 – 110.0	MS	12-APR-10 03:01	100411-2
	Lead	51.3	ug/L	50	ug/L	102.6	90.0 – 110.0	MS	12-APR-10 03:01	100411-2
	Manganese	53.3	ug/L	50	ug/L	106.6	90.0 – 110.0	MS	12-APR-10 03:01	100411-2
	Thallium	50	ug/L	50	ug/L	99.9	90.0 – 110.0	MS	12-APR-10 03:01	100411-2
	Antimony	53.1	ug/L	50	ug/L	106.3	90.0 – 110.0	MS	13-APR-10 11:52	100413-3
	Uranium	49.6	ug/L	50	ug/L	99.3	90.0 – 110.0	MS	13-APR-10 15:17	100413-5
CCV01										
	Mercury	5.16	ug/L	5	ug/L	103.1	80.0 – 120.0	AV	02-MAR-10 08:45	030210W3-6
	Aluminum	5090	ug/L	5000	ug/L	101.7	90.0 – 110.0	P	29-MAR-10 18:49	032910C-1
	Arsenic	507	ug/L	500	ug/L	101.4	90.0 – 110.0	P	29-MAR-10 18:49	032910C-1
	Barium	498	ug/L	500	ug/L	99.6	90.0 – 110.0	P	29-MAR-10 18:49	032910C-1
	Calcium	4990	ug/L	5000	ug/L	99.8	90.0 – 110.0	P	29-MAR-10 18:49	032910C-1

METALS

-2a-

Initial and Continuing Calibration Verification

SDG No: 10-2093

Contract: LANL01004

Lab Code: GEL

Initial Calibration Source: Solutions Plus

Continuing Calibration Source: O2Si

Instrument ID: HG3,ICPMS4,ICPMS5,OPTIMA4

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>True Value</u>	<u>Units</u>	<u>% Recovery</u>	<u>Acceptance Window (%R)</u>	<u>M</u>	<u>Analysis Date/Time</u>	<u>Run Number</u>
	Chromium	493	ug/L	500	ug/L	98.6	90.0 - 110.0	P	29-MAR-10 18:49	032910C-1
	Cobalt	491	ug/L	500	ug/L	98.2	90.0 - 110.0	P	29-MAR-10 18:49	032910C-1
	Copper	496	ug/L	500	ug/L	99.3	90.0 - 110.0	P	29-MAR-10 18:49	032910C-1
	Iron	4940	ug/L	5000	ug/L	98.8	90.0 - 110.0	P	29-MAR-10 18:49	032910C-1
	Magnesium	5080	ug/L	5000	ug/L	101.5	90.0 - 110.0	P	29-MAR-10 18:49	032910C-1
	Nickel	492	ug/L	500	ug/L	98.4	90.0 - 110.0	P	29-MAR-10 18:49	032910C-1
	Potassium	5440	ug/L	5000	ug/L	108.7	90.0 - 110.0	P	29-MAR-10 18:49	032910C-1
	Selenium	488	ug/L	500	ug/L	97.6	90.0 - 110.0	P	29-MAR-10 18:49	032910C-1
	Silver	498	ug/L	500	ug/L	99.6	90.0 - 110.0	P	29-MAR-10 18:49	032910C-1
	Sodium	10000	ug/L	10000	ug/L	100	90.0 - 110.0	P	29-MAR-10 18:49	032910C-1
	Vanadium	499	ug/L	500	ug/L	99.8	90.0 - 110.0	P	29-MAR-10 18:49	032910C-1
	Zinc	488	ug/L	500	ug/L	97.7	90.0 - 110.0	P	29-MAR-10 18:49	032910C-1
	Beryllium	49	ug/L	50	ug/L	98	90.0 - 110.0	MS	12-APR-10 03:32	100411-2
	Cadmium	50.8	ug/L	50	ug/L	101.7	90.0 - 110.0	MS	12-APR-10 03:32	100411-2
	Lead	51.3	ug/L	50	ug/L	102.7	90.0 - 110.0	MS	12-APR-10 03:32	100411-2
	Manganese	52.9	ug/L	50	ug/L	105.8	90.0 - 110.0	MS	12-APR-10 03:32	100411-2
	Thallium	50.3	ug/L	50	ug/L	100.6	90.0 - 110.0	MS	12-APR-10 03:32	100411-2
	Antimony	52.6	ug/L	50	ug/L	105.1	90.0 - 110.0	MS	13-APR-10 12:04	100413-3
	Uranium	49.3	ug/L	50	ug/L	98.6	90.0 - 110.0	MS	13-APR-10 15:26	100413-5
CCV02	Mercury	5.13	ug/L	5	ug/L	102.6	80.0 - 120.0	AV	02-MAR-10 09:08	030210W3-6
	Aluminum	5100	ug/L	5000	ug/L	102	90.0 - 110.0	P	29-MAR-10 18:57	032910C-1
	Arsenic	507	ug/L	500	ug/L	101.4	90.0 - 110.0	P	29-MAR-10 18:57	032910C-1
	Barium	497	ug/L	500	ug/L	99.4	90.0 - 110.0	P	29-MAR-10 18:57	032910C-1
	Calcium	4970	ug/L	5000	ug/L	99.4	90.0 - 110.0	P	29-MAR-10 18:57	032910C-1
	Chromium	492	ug/L	500	ug/L	98.5	90.0 - 110.0	P	29-MAR-10 18:57	032910C-1
	Cobalt	490	ug/L	500	ug/L	98	90.0 - 110.0	P	29-MAR-10 18:57	032910C-1
	Copper	495	ug/L	500	ug/L	99	90.0 - 110.0	P	29-MAR-10 18:57	032910C-1
	Iron	4920	ug/L	5000	ug/L	98.4	90.0 - 110.0	P	29-MAR-10 18:57	032910C-1
	Magnesium	5070	ug/L	5000	ug/L	101.5	90.0 - 110.0	P	29-MAR-10 18:57	032910C-1

METALS

-2a-

Initial and Continuing Calibration Verification

SDG No: 10-2093

Contract: LANL01004

Lab Code: GEL

Initial Calibration Source: Solutions Plus

Continuing Calibration Source: O2Si

Instrument ID: HG3,ICPMS4,ICPMS5,OPTIMA4

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>True Value</u>	<u>Units</u>	<u>% Recovery</u>	<u>Acceptance Window (%R)</u>	<u>M</u>	<u>Analysis Date/Time</u>	<u>Run Number</u>
	Nickel	491	ug/L	500	ug/L	98.3	90.0 – 110.0	P	29-MAR-10 18:57	032910C-1
	Potassium	4890	ug/L	5000	ug/L	97.8	90.0 – 110.0	P	29-MAR-10 18:57	032910C-1
	Selenium	483	ug/L	500	ug/L	96.6	90.0 – 110.0	P	29-MAR-10 18:57	032910C-1
	Silver	498	ug/L	500	ug/L	99.6	90.0 – 110.0	P	29-MAR-10 18:57	032910C-1
	Sodium	9880	ug/L	10000	ug/L	98.8	90.0 – 110.0	P	29-MAR-10 18:57	032910C-1
	Vanadium	500	ug/L	500	ug/L	100	90.0 – 110.0	P	29-MAR-10 18:57	032910C-1
	Zinc	484	ug/L	500	ug/L	96.8	90.0 – 110.0	P	29-MAR-10 18:57	032910C-1
	Beryllium	49.9	ug/L	50	ug/L	99.9	90.0 – 110.0	MS	12-APR-10 03:51	100411-2
	Cadmium	52.1	ug/L	50	ug/L	104.2	90.0 – 110.0	MS	12-APR-10 03:51	100411-2
	Lead	52.4	ug/L	50	ug/L	104.8	90.0 – 110.0	MS	12-APR-10 03:51	100411-2
	Manganese	53.6	ug/L	50	ug/L	107.2	90.0 – 110.0	MS	12-APR-10 03:51	100411-2
	Thallium	50.8	ug/L	50	ug/L	101.7	90.0 – 110.0	MS	12-APR-10 03:51	100411-2
	Antimony	52.9	ug/L	50	ug/L	105.8	90.0 – 110.0	MS	13-APR-10 12:31	100413-3
	Uranium	50.4	ug/L	50	ug/L	100.7	90.0 – 110.0	MS	13-APR-10 15:44	100413-5
CCV03										
	Mercury	5.06	ug/L	5	ug/L	101.1	80.0 – 120.0	AV	02-MAR-10 09:31	030210W3-6
	Aluminum	5160	ug/L	5000	ug/L	103.3	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Arsenic	515	ug/L	500	ug/L	103	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Barium	498	ug/L	500	ug/L	99.6	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Calcium	4960	ug/L	5000	ug/L	99.2	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Chromium	488	ug/L	500	ug/L	97.7	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Cobalt	487	ug/L	500	ug/L	97.5	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Copper	493	ug/L	500	ug/L	98.6	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Iron	4930	ug/L	5000	ug/L	98.5	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Magnesium	5060	ug/L	5000	ug/L	101.2	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Nickel	490	ug/L	500	ug/L	98.1	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Potassium	4830	ug/L	5000	ug/L	96.6	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Selenium	476	ug/L	500	ug/L	95.2	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Silver	496	ug/L	500	ug/L	99.2	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Sodium	9860	ug/L	10000	ug/L	98.6	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1

SW846

METALS
-2a-
Initial and Continuing Calibration Verification

SDG No: 10-2093

Contract: LANL01004

Lab Code: GEL

Initial Calibration Source: Solutions Plus

Continuing Calibration Source: O2Si

Instrument ID: HG3,ICPMS4,ICPMS5,OPTIMA4

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>True Value</u>	<u>Units</u>	<u>% Recovery</u>	<u>Acceptance Window (%R)</u>	<u>M</u>	<u>Analysis Date/Time</u>	<u>Run Number</u>
	Vanadium	498	ug/L	500	ug/L	99.6	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Zinc	480	ug/L	500	ug/L	96.1	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Beryllium	49.2	ug/L	50	ug/L	98.4	90.0 – 110.0	MS	12-APR-10 05:05	100411-2
	Cadmium	50.4	ug/L	50	ug/L	100.8	90.0 – 110.0	MS	12-APR-10 05:05	100411-2
	Lead	50.7	ug/L	50	ug/L	101.4	90.0 – 110.0	MS	12-APR-10 05:05	100411-2
	Manganese	51.8	ug/L	50	ug/L	103.6	90.0 – 110.0	MS	12-APR-10 05:05	100411-2
	Thallium	48	ug/L	50	ug/L	96	90.0 – 110.0	MS	12-APR-10 05:05	100411-2
	Antimony	52.3	ug/L	50	ug/L	104.6	90.0 – 110.0	MS	13-APR-10 12:53	100413-3
	Uranium	48.8	ug/L	50	ug/L	97.6	90.0 – 110.0	MS	13-APR-10 15:59	100413-5
CCV04	Mercury	5.02	ug/L	5	ug/L	100.3	80.0 – 120.0	AV	02-MAR-10 09:54	030210W3-6
	Aluminum	5160	ug/L	5000	ug/L	103.1	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Arsenic	520	ug/L	500	ug/L	104.1	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Barium	498	ug/L	500	ug/L	99.5	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Calcium	4950	ug/L	5000	ug/L	98.9	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Chromium	488	ug/L	500	ug/L	97.6	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Cobalt	486	ug/L	500	ug/L	97.1	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Copper	492	ug/L	500	ug/L	98.4	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Iron	4910	ug/L	5000	ug/L	98.3	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Magnesium	5060	ug/L	5000	ug/L	101.2	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Nickel	487	ug/L	500	ug/L	97.5	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Potassium	4830	ug/L	5000	ug/L	96.7	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Selenium	476	ug/L	500	ug/L	95.2	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Silver	495	ug/L	500	ug/L	99.1	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Sodium	9860	ug/L	10000	ug/L	98.6	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Vanadium	498	ug/L	500	ug/L	99.7	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Zinc	479	ug/L	500	ug/L	95.8	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Beryllium	50.9	ug/L	50	ug/L	101.8	90.0 – 110.0	MS	12-APR-10 05:42	100411-2
	Cadmium	50	ug/L	50	ug/L	100	90.0 – 110.0	MS	12-APR-10 05:42	100411-2
	Lead	50.4	ug/L	50	ug/L	100.8	90.0 – 110.0	MS	12-APR-10 05:42	100411-2

METALS
-2a-
Initial and Continuing Calibration Verification

SDG No: 10-2093

Contract: LANL01004

Lab Code: GEL

Initial Calibration Source: Solutions Plus

Continuing Calibration Source: O2Si

Instrument ID: HG3,ICPMS4,ICPMS5,OPTIMA4

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>True Value</u>	<u>Units</u>	<u>% Recovery</u>	<u>Acceptance Window (%R)</u>	<u>M</u>	<u>Analysis Date/Time</u>	<u>Run Number</u>
	Manganese	52	ug/L	50	ug/L	104.1	90.0 - 110.0	MS	12-APR-10 05:42	100411-2
	Thallium	48.2	ug/L	50	ug/L	96.5	90.0 - 110.0	MS	12-APR-10 05:42	100411-2
	Antimony	51.4	ug/L	50	ug/L	102.7	90.0 - 110.0	MS	13-APR-10 13:21	100413-3
	Uranium	50.4	ug/L	50	ug/L	100.8	90.0 - 110.0	MS	13-APR-10 16:14	100413-5
CCV05										
	Mercury	5	ug/L	5	ug/L	99.9	80.0 - 120.0	AV	02-MAR-10 10:17	030210W3-6
	Aluminum	5180	ug/L	5000	ug/L	103.6	90.0 - 110.0	P	29-MAR-10 20:14	032910C-1
	Arsenic	532	ug/L	500	ug/L	106.5	90.0 - 110.0	P	29-MAR-10 20:14	032910C-1
	Barium	502	ug/L	500	ug/L	100.4	90.0 - 110.0	P	29-MAR-10 20:14	032910C-1
	Calcium	4930	ug/L	5000	ug/L	98.6	90.0 - 110.0	P	29-MAR-10 20:14	032910C-1
	Chromium	492	ug/L	500	ug/L	98.3	90.0 - 110.0	P	29-MAR-10 20:14	032910C-1
	Cobalt	489	ug/L	500	ug/L	97.8	90.0 - 110.0	P	29-MAR-10 20:14	032910C-1
	Copper	495	ug/L	500	ug/L	99	90.0 - 110.0	P	29-MAR-10 20:14	032910C-1
	Iron	4900	ug/L	5000	ug/L	98	90.0 - 110.0	P	29-MAR-10 20:14	032910C-1
	Magnesium	5040	ug/L	5000	ug/L	100.7	90.0 - 110.0	P	29-MAR-10 20:14	032910C-1
	Nickel	490	ug/L	500	ug/L	98.1	90.0 - 110.0	P	29-MAR-10 20:14	032910C-1
	Potassium	4780	ug/L	5000	ug/L	95.7	90.0 - 110.0	P	29-MAR-10 20:14	032910C-1
	Selenium	479	ug/L	500	ug/L	95.8	90.0 - 110.0	P	29-MAR-10 20:14	032910C-1
	Silver	498	ug/L	500	ug/L	99.6	90.0 - 110.0	P	29-MAR-10 20:14	032910C-1
	Sodium	9800	ug/L	10000	ug/L	98	90.0 - 110.0	P	29-MAR-10 20:14	032910C-1
	Vanadium	501	ug/L	500	ug/L	100.2	90.0 - 110.0	P	29-MAR-10 20:14	032910C-1
	Zinc	482	ug/L	500	ug/L	96.5	90.0 - 110.0	P	29-MAR-10 20:14	032910C-1
	Antimony	52.7	ug/L	50	ug/L	105.4	90.0 - 110.0	MS	13-APR-10 13:36	100413-3
	Uranium	49.5	ug/L	50	ug/L	98.9	90.0 - 110.0	MS	13-APR-10 16:29	100413-5
CCV06										
	Mercury	5.06	ug/L	5	ug/L	101.2	80.0 - 120.0	AV	02-MAR-10 10:41	030210W3-6
	Aluminum	5180	ug/L	5000	ug/L	103.7	90.0 - 110.0	P	29-MAR-10 20:39	032910C-1
	Arsenic	533	ug/L	500	ug/L	106.7	90.0 - 110.0	P	29-MAR-10 20:39	032910C-1
	Barium	500	ug/L	500	ug/L	100	90.0 - 110.0	P	29-MAR-10 20:39	032910C-1
	Calcium	4890	ug/L	5000	ug/L	97.8	90.0 - 110.0	P	29-MAR-10 20:39	032910C-1

METALS
-2a-
Initial and Continuing Calibration Verification

SDG No: 10-2093

Contract: LANL01004

Lab Code: GEL

Initial Calibration Source: Solutions Plus

Continuing Calibration Source: O2Si

Instrument ID: HG3,ICPMS4,ICPMS5,OPTIMA4

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>True Value</u>	<u>Units</u>	<u>% Recovery</u>	<u>Acceptance Window (%R)</u>	<u>M</u>	<u>Analysis Date/Time</u>	<u>Run Number</u>
	Chromium	488	ug/L	500	ug/L	97.6	90.0 – 110.0	P	29-MAR-10 20:39	032910C-1
	Cobalt	485	ug/L	500	ug/L	97.1	90.0 – 110.0	P	29-MAR-10 20:39	032910C-1
	Copper	493	ug/L	500	ug/L	98.7	90.0 – 110.0	P	29-MAR-10 20:39	032910C-1
	Iron	4870	ug/L	5000	ug/L	97.5	90.0 – 110.0	P	29-MAR-10 20:39	032910C-1
	Magnesium	5020	ug/L	5000	ug/L	100.3	90.0 – 110.0	P	29-MAR-10 20:39	032910C-1
	Nickel	487	ug/L	500	ug/L	97.4	90.0 – 110.0	P	29-MAR-10 20:39	032910C-1
	Potassium	4730	ug/L	5000	ug/L	94.6	90.0 – 110.0	P	29-MAR-10 20:39	032910C-1
	Selenium	471	ug/L	500	ug/L	94.2	90.0 – 110.0	P	29-MAR-10 20:39	032910C-1
	Silver	495	ug/L	500	ug/L	98.9	90.0 – 110.0	P	29-MAR-10 20:39	032910C-1
	Sodium	9760	ug/L	10000	ug/L	97.6	90.0 – 110.0	P	29-MAR-10 20:39	032910C-1
	Vanadium	499	ug/L	500	ug/L	99.8	90.0 – 110.0	P	29-MAR-10 20:39	032910C-1
	Zinc	478	ug/L	500	ug/L	95.7	90.0 – 110.0	P	29-MAR-10 20:39	032910C-1
	Antimony	52.1	ug/L	50	ug/L	104.2	90.0 – 110.0	MS	13-APR-10 13:59	100413-3
	Uranium	48.8	ug/L	50	ug/L	97.6	90.0 – 110.0	MS	13-APR-10 16:44	100413-5
CCV07										
	Mercury	5.01	ug/L	5	ug/L	100.3	80.0 – 120.0	AV	02-MAR-10 11:04	030210W3-6
	Aluminum	5210	ug/L	5000	ug/L	104.3	90.0 – 110.0	P	29-MAR-10 21:03	032910C-1
	Arsenic	534	ug/L	500	ug/L	106.8	90.0 – 110.0	P	29-MAR-10 21:03	032910C-1
	Barium	500	ug/L	500	ug/L	100.1	90.0 – 110.0	P	29-MAR-10 21:03	032910C-1
	Calcium	4930	ug/L	5000	ug/L	98.6	90.0 – 110.0	P	29-MAR-10 21:03	032910C-1
	Chromium	488	ug/L	500	ug/L	97.7	90.0 – 110.0	P	29-MAR-10 21:03	032910C-1
	Cobalt	486	ug/L	500	ug/L	97.2	90.0 – 110.0	P	29-MAR-10 21:03	032910C-1
	Copper	494	ug/L	500	ug/L	98.8	90.0 – 110.0	P	29-MAR-10 21:03	032910C-1
	Iron	4910	ug/L	5000	ug/L	98.2	90.0 – 110.0	P	29-MAR-10 21:03	032910C-1
	Magnesium	5070	ug/L	5000	ug/L	101.4	90.0 – 110.0	P	29-MAR-10 21:03	032910C-1
	Nickel	487	ug/L	500	ug/L	97.4	90.0 – 110.0	P	29-MAR-10 21:03	032910C-1
	Potassium	4790	ug/L	5000	ug/L	95.9	90.0 – 110.0	P	29-MAR-10 21:03	032910C-1
	Selenium	476	ug/L	500	ug/L	95.2	90.0 – 110.0	P	29-MAR-10 21:03	032910C-1
	Silver	496	ug/L	500	ug/L	99.2	90.0 – 110.0	P	29-MAR-10 21:03	032910C-1
	Sodium	9820	ug/L	10000	ug/L	98.3	90.0 – 110.0	P	29-MAR-10 21:03	032910C-1

METALS
-2a-
Initial and Continuing Calibration Verification

SDG No: 10-2093

Contract: LANL01004

Lab Code: GEL

Initial Calibration Source: Solutions Plus

Continuing Calibration Source: O2Si

Instrument ID: HG3,ICPMS4,ICPMS5,OPTIMA4

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>True Value</u>	<u>Units</u>	<u>% Recovery</u>	<u>Acceptance Window (%R)</u>	<u>M</u>	<u>Analysis Date/Time</u>	<u>Run Number</u>
CCV08	Vanadium	499	ug/L	500	ug/L	99.8	90.0 – 110.0	P	29-MAR-10 21:03	032910C-1
	Zinc	478	ug/L	500	ug/L	95.6	90.0 – 110.0	P	29-MAR-10 21:03	032910C-1
	Antimony	51	ug/L	50	ug/L	102.1	90.0 – 110.0	MS	13-APR-10 14:21	100413-3
	Mercury	5.21	ug/L	5	ug/L	104.3	80.0 – 120.0	AV	02-MAR-10 11:27	030210W3-6
	Mercury	4.93	ug/L	5	ug/L	98.7	80.0 – 120.0	AV	02-MAR-10 11:50	030210W3-6
CCV10	Mercury	5.01	ug/L	5	ug/L	100.1	80.0 – 120.0	AV	02-MAR-10 12:14	030210W3-6

METALS
-2b-
CRDL Standard for AA & ICP

SDG No: 10-2093

Contract: LANL01004

Lab Code: GEL

AA CRDL Standard Source: SPEX

ICP CRDL Standard Source Solutions Plus

Instrument ID: HG3,ICPMS4,ICPMS5,OPTIMA4

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>True Value</u>	<u>Units</u>	<u>% Recovery</u>	<u>Advisory Limits (%R)</u>	<u>M</u>	<u>Analysis Date/Time</u>	<u>Run Number</u>
CRDL01										
	Mercury	.24	ug/L	.2	ug/L	120	70.0 - 130.0	AV	02-MAR-10 08:43	030210W3-6
	Lead	2.32	ug/L	2	ug/L	115.8	70.0 - 130.0	MS	12-APR-10 03:14	100411-2
	Thallium	1.14	ug/L	1	ug/L	114.3	70.0 - 130.0	MS	12-APR-10 03:14	100411-2
	Manganese	6.18	ug/L	5	ug/L	123.5	70.0 - 130.0	MS	12-APR-10 03:14	100411-2
	Cadmium	1.19	ug/L	1	ug/L	119	70.0 - 130.0	MS	12-APR-10 03:14	100411-2
	Beryllium	.545	ug/L	.5	ug/L	109	70.0 - 130.0	MS	12-APR-10 03:14	100411-2
	Antimony	2.94	ug/L	3	ug/L	98.1	70.0 - 130.0	MS	13-APR-10 11:57	100413-3
	Uranium	.216	ug/L	.2	ug/L	108	70.0 - 130.0	MS	13-APR-10 15:21	100413-5
PQL01										
	Aluminum	201	ug/L	200	ug/L	100.4	70.0 - 130.0	P	29-MAR-10 18:40	032910C-1
	Iron	103	ug/L	100	ug/L	103.4	70.0 - 130.0	P	29-MAR-10 18:40	032910C-1
	Magnesium	303	ug/L	300	ug/L	101.1	70.0 - 130.0	P	29-MAR-10 18:40	032910C-1
	Nickel	5.03	ug/L	5	ug/L	100.7	70.0 - 130.0	P	29-MAR-10 18:40	032910C-1
	Potassium	170	ug/L	150	ug/L	113.4	70.0 - 130.0	P	29-MAR-10 18:40	032910C-1
	Silver	4.62	ug/L	5	ug/L	92.4	70.0 - 130.0	P	29-MAR-10 18:40	032910C-1
	Sodium	260	ug/L	300	ug/L	86.8	70.0 - 130.0	P	29-MAR-10 18:40	032910C-1
	Arsenic	29.8	ug/L	30	ug/L	99.4	70.0 - 130.0	P	29-MAR-10 18:40	032910C-1
	Barium	5.16	ug/L	5	ug/L	103.1	70.0 - 130.0	P	29-MAR-10 18:40	032910C-1
	Chromium	4.84	ug/L	5	ug/L	96.8	70.0 - 130.0	P	29-MAR-10 18:40	032910C-1
	Cobalt	5.14	ug/L	5	ug/L	102.7	70.0 - 130.0	P	29-MAR-10 18:40	032910C-1
	Copper	10.1	ug/L	10	ug/L	101.4	70.0 - 130.0	P	29-MAR-10 18:40	032910C-1
	Vanadium	4.53	ug/L	5	ug/L	90.6	70.0 - 130.0	P	29-MAR-10 18:40	032910C-1
	Zinc	9.92	ug/L	10	ug/L	99.2	70.0 - 130.0	P	29-MAR-10 18:40	032910C-1
	Calcium	204	ug/L	200	ug/L	101.8	70.0 - 130.0	P	29-MAR-10 18:40	032910C-1
	Selenium	29.5	ug/L	30	ug/L	98.3	70.0 - 130.0	P	29-MAR-10 18:40	032910C-1

Metals
-3a-
Initial and Continuing Calibration Blank Summary

SDG No.: 10-2093

Contract: LANL01004

Lab Code: GEL

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u> <u>ug/L</u>	<u>Acceptance</u>	<u>Conc</u> <u>Qual</u>	<u>MDL</u>	<u>RDL</u>	<u>Matrix</u>	<u>M</u>	<u>Analysis</u> <u>Date/Time</u>	<u>Run</u>
ICB01										
	Mercury	0.066	+/- .2	U	0.066	0.2	LIQ	AV	02-MAR-10 08:41	030210W3-6
	Aluminum	68.0	+/-200	U	68.0	200	LIQ	P	29-MAR-10 18:37	032910C-1
	Arsenic	5.0	+/-30	U	5.0	30.0	LIQ	P	29-MAR-10 18:37	032910C-1
	Barium	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 18:37	032910C-1
	Calcium	50.0	+/-200	U	50.0	200	LIQ	P	29-MAR-10 18:37	032910C-1
	Chromium	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 18:37	032910C-1
	Cobalt	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 18:37	032910C-1
	Copper	3.0	+/-10	U	3.0	10.0	LIQ	P	29-MAR-10 18:37	032910C-1
	Iron	30.0	+/-100	U	30.0	100	LIQ	P	29-MAR-10 18:37	032910C-1
	Magnesium	85.0	+/-300	U	85.0	300	LIQ	P	29-MAR-10 18:37	032910C-1
	Nickel	1.5	+/-5	U	1.5	5.0	LIQ	P	29-MAR-10 18:37	032910C-1
	Potassium	50.0	+/-150	U	50.0	150	LIQ	P	29-MAR-10 18:37	032910C-1
	Selenium	5.57	+/-30	J	5.0	30.0	LIQ	P	29-MAR-10 18:37	032910C-1
	Silver	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 18:37	032910C-1
	Sodium	100	+/-300	U	100	300	LIQ	P	29-MAR-10 18:37	032910C-1
	Vanadium	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 18:37	032910C-1
	Zinc	3.3	+/-10	U	3.3	10.0	LIQ	P	29-MAR-10 18:37	032910C-1
	Beryllium	0.1	+/- .5	U	0.1	0.5	LIQ	MS	12-APR-10 03:08	100411-2
	Cadmium	0.11	+/-1	U	0.11	1.0	LIQ	MS	12-APR-10 03:08	100411-2
	Lead	0.5	+/-2	U	0.5	2.0	LIQ	MS	12-APR-10 03:08	100411-2
	Manganese	1.0	+/-5	U	1.0	5.0	LIQ	MS	12-APR-10 03:08	100411-2
	Thallium	0.3	+/-1	U	0.3	1.0	LIQ	MS	12-APR-10 03:08	100411-2
	Antimony	1.0	+/-3	U	1.0	3.0	LIQ	MS	13-APR-10 11:54	100413-3
	Uranium	0.05	+/- .2	U	0.05	0.2	LIQ	MS	13-APR-10 15:19	100413-5
CCB01										
	Mercury	0.066	+/- .2	U	0.066	0.2	LIQ	AV	02-MAR-10 08:47	030210W3-6
	Aluminum	68.0	+/-200	U	68.0	200	LIQ	P	29-MAR-10 18:51	032910C-1
	Arsenic	5.0	+/-30	U	5.0	30.0	LIQ	P	29-MAR-10 18:51	032910C-1
	Barium	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 18:51	032910C-1
	Calcium	50.0	+/-200	U	50.0	200	LIQ	P	29-MAR-10 18:51	032910C-1
	Chromium	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 18:51	032910C-1

Metals
-3a-
Initial and Continuing Calibration Blank Summary

SDG No.: 10-2093

Contract: LANL01004

Lab Code: GEL

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u> <u>ug/L</u>	<u>Acceptance</u>	<u>Conc</u> <u>Qual</u>	<u>MDL</u>	<u>RDL</u>	<u>Matrix</u>	<u>M</u>	<u>Analysis</u> <u>Date/Time</u>	<u>Run</u>
	Cobalt	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 18:51	032910C-1
	Copper	3.0	+/-10	U	3.0	10.0	LIQ	P	29-MAR-10 18:51	032910C-1
	Iron	30.0	+/-100	U	30.0	100	LIQ	P	29-MAR-10 18:51	032910C-1
	Magnesium	85.0	+/-300	U	85.0	300	LIQ	P	29-MAR-10 18:51	032910C-1
	Nickel	1.5	+/-5	U	1.5	5.0	LIQ	P	29-MAR-10 18:51	032910C-1
	Potassium	152.39	+/-150		50.0	150	LIQ	P	29-MAR-10 18:51	032910C-1
	Selenium	5.0	+/-30	U	5.0	30.0	LIQ	P	29-MAR-10 18:51	032910C-1
	Silver	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 18:51	032910C-1
	Sodium	100	+/-300	U	100	300	LIQ	P	29-MAR-10 18:51	032910C-1
	Vanadium	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 18:51	032910C-1
	Zinc	3.3	+/-10	U	3.3	10.0	LIQ	P	29-MAR-10 18:51	032910C-1
	Beryllium	0.1	+/-5	U	0.1	0.5	LIQ	MS	12-APR-10 03:38	100411-2
	Cadmium	0.11	+/-1	U	0.11	1.0	LIQ	MS	12-APR-10 03:38	100411-2
	Lead	0.5	+/-2	U	0.5	2.0	LIQ	MS	12-APR-10 03:38	100411-2
	Manganese	1.0	+/-5	U	1.0	5.0	LIQ	MS	12-APR-10 03:38	100411-2
	Thallium	0.3	+/-1	U	0.3	1.0	LIQ	MS	12-APR-10 03:38	100411-2
	Antimony	1.0	+/-3	U	1.0	3.0	LIQ	MS	13-APR-10 12:07	100413-3
	Uranium	0.05	+/-2	U	0.05	0.2	LIQ	MS	13-APR-10 15:27	100413-5
CCB02	Mercury	0.066	+/-2	U	0.066	0.2	LIQ	AV	02-MAR-10 09:10	030210W3-6
	Aluminum	68.0	+/-200	U	68.0	200	LIQ	P	29-MAR-10 18:59	032910C-1
	Arsenic	5.0	+/-30	U	5.0	30.0	LIQ	P	29-MAR-10 18:59	032910C-1
	Barium	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 18:59	032910C-1
	Calcium	50.0	+/-200	U	50.0	200	LIQ	P	29-MAR-10 18:59	032910C-1
	Chromium	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 18:59	032910C-1
	Cobalt	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 18:59	032910C-1
	Copper	3.0	+/-10	U	3.0	10.0	LIQ	P	29-MAR-10 18:59	032910C-1
	Iron	30.0	+/-100	U	30.0	100	LIQ	P	29-MAR-10 18:59	032910C-1
	Magnesium	85.0	+/-300	U	85.0	300	LIQ	P	29-MAR-10 18:59	032910C-1
	Nickel	1.5	+/-5	U	1.5	5.0	LIQ	P	29-MAR-10 18:59	032910C-1
	Potassium	50.0	+/-150	U	50.0	150	LIQ	P	29-MAR-10 18:59	032910C-1

Metals
-3a-
Initial and Continuing Calibration Blank Summary

SDG No.: 10-2093

Contract: LANL01004

Lab Code: GEL

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u> <u>ug/L</u>	<u>Acceptance</u>	<u>Conc</u> <u>Qual</u>	<u>MDL</u>	<u>RDL</u>	<u>Matrix</u>	<u>M</u>	<u>Analysis</u> <u>Date/Time</u>	<u>Run</u>
	Selenium	5.0	+/-30	U	5.0	30.0	LIQ	P	29-MAR-10 18:59	032910C-1
	Silver	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 18:59	032910C-1
	Sodium	100	+/-300	U	100	300	LIQ	P	29-MAR-10 18:59	032910C-1
	Vanadium	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 18:59	032910C-1
	Zinc	3.3	+/-10	U	3.3	10.0	LIQ	P	29-MAR-10 18:59	032910C-1
	Beryllium	0.1	+/-5	U	0.1	0.5	LIQ	MS	12-APR-10 03:57	100411-2
	Cadmium	0.11	+/-1	U	0.11	1.0	LIQ	MS	12-APR-10 03:57	100411-2
	Lead	0.5	+/-2	U	0.5	2.0	LIQ	MS	12-APR-10 03:57	100411-2
	Manganese	1.0	+/-5	U	1.0	5.0	LIQ	MS	12-APR-10 03:57	100411-2
	Thallium	0.597	+/-1	J	0.3	1.0	LIQ	MS	12-APR-10 03:57	100411-2
	Antimony	1.0	+/-3	U	1.0	3.0	LIQ	MS	13-APR-10 12:34	100413-3
	Uranium	0.05	+/-2	U	0.05	0.2	LIQ	MS	13-APR-10 15:45	100413-5
CCB03	Mercury	0.066	+/-2	U	0.066	0.2	LIQ	AV	02-MAR-10 09:33	030210W3-6
	Aluminum	68.0	+/-200	U	68.0	200	LIQ	P	29-MAR-10 19:33	032910C-1
	Arsenic	5.0	+/-30	U	5.0	30.0	LIQ	P	29-MAR-10 19:33	032910C-1
	Barium	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 19:33	032910C-1
	Calcium	50.0	+/-200	U	50.0	200	LIQ	P	29-MAR-10 19:33	032910C-1
	Chromium	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 19:33	032910C-1
	Cobalt	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 19:33	032910C-1
	Copper	3.0	+/-10	U	3.0	10.0	LIQ	P	29-MAR-10 19:33	032910C-1
	Iron	30.0	+/-100	U	30.0	100	LIQ	P	29-MAR-10 19:33	032910C-1
	Magnesium	85.0	+/-300	U	85.0	300	LIQ	P	29-MAR-10 19:33	032910C-1
	Nickel	1.5	+/-5	U	1.5	5.0	LIQ	P	29-MAR-10 19:33	032910C-1
	Potassium	50.0	+/-150	U	50.0	150	LIQ	P	29-MAR-10 19:33	032910C-1
	Selenium	5.0	+/-30	U	5.0	30.0	LIQ	P	29-MAR-10 19:33	032910C-1
	Silver	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 19:33	032910C-1
	Sodium	100	+/-300	U	100	300	LIQ	P	29-MAR-10 19:33	032910C-1
	Vanadium	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 19:33	032910C-1
	Zinc	3.3	+/-10	U	3.3	10.0	LIQ	P	29-MAR-10 19:33	032910C-1
	Beryllium	0.1	+/-5	U	0.1	0.5	LIQ	MS	12-APR-10 05:11	100411-2

SW846

Metals
-3a-
Initial and Continuing Calibration Blank Summary

SDG No.: 10-2093

Contract: LANL01004

Lab Code: GEL

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u> <u>ug/L</u>	<u>Acceptance</u>	<u>Conc</u> <u>Qual</u>	<u>MDL</u>	<u>RDL</u>	<u>Matrix</u>	<u>M</u>	<u>Analysis</u> <u>Date/Time</u>	<u>Run</u>
	Cadmium	0.11	+/-1	U	0.11	1.0	LIQ	MS	12-APR-10 05:11	100411-2
	Lead	0.5	+/-2	U	0.5	2.0	LIQ	MS	12-APR-10 05:11	100411-2
	Manganese	1.0	+/-5	U	1.0	5.0	LIQ	MS	12-APR-10 05:11	100411-2
	Thallium	0.37	+/-1	J	0.3	1.0	LIQ	MS	12-APR-10 05:11	100411-2
	Antimony	1.0	+/-3	U	1.0	3.0	LIQ	MS	13-APR-10 12:56	100413-3
	Uranium	0.05	+/-2	U	0.05	0.2	LIQ	MS	13-APR-10 16:00	100413-5
CCB04	Mercury	0.066	+/-2	U	0.066	0.2	LIQ	AV	02-MAR-10 09:56	030210W3-6
	Aluminum	68.0	+/-200	U	68.0	200	LIQ	P	29-MAR-10 19:54	032910C-1
	Arsenic	5.0	+/-30	U	5.0	30.0	LIQ	P	29-MAR-10 19:54	032910C-1
	Barium	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 19:54	032910C-1
	Calcium	50.0	+/-200	U	50.0	200	LIQ	P	29-MAR-10 19:54	032910C-1
	Chromium	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 19:54	032910C-1
	Cobalt	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 19:54	032910C-1
	Copper	3.0	+/-10	U	3.0	10.0	LIQ	P	29-MAR-10 19:54	032910C-1
	Iron	30.0	+/-100	U	30.0	100	LIQ	P	29-MAR-10 19:54	032910C-1
	Magnesium	85.0	+/-300	U	85.0	300	LIQ	P	29-MAR-10 19:54	032910C-1
	Nickel	1.5	+/-5	U	1.5	5.0	LIQ	P	29-MAR-10 19:54	032910C-1
	Potassium	50.0	+/-150	U	50.0	150	LIQ	P	29-MAR-10 19:54	032910C-1
	Selenium	5.0	+/-30	U	5.0	30.0	LIQ	P	29-MAR-10 19:54	032910C-1
	Silver	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 19:54	032910C-1
	Sodium	100	+/-300	U	100	300	LIQ	P	29-MAR-10 19:54	032910C-1
	Vanadium	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 19:54	032910C-1
	Zinc	3.3	+/-10	U	3.3	10.0	LIQ	P	29-MAR-10 19:54	032910C-1
	Beryllium	0.1	+/-5	U	0.1	0.5	LIQ	MS	12-APR-10 05:49	100411-2
	Cadmium	0.11	+/-1	U	0.11	1.0	LIQ	MS	12-APR-10 05:49	100411-2
	Lead	0.5	+/-2	U	0.5	2.0	LIQ	MS	12-APR-10 05:49	100411-2
	Manganese	1.0	+/-5	U	1.0	5.0	LIQ	MS	12-APR-10 05:49	100411-2
	Thallium	1.12	+/-1		0.3	1.0	LIQ	MS	12-APR-10 05:49	100411-2
	Antimony	1.0	+/-3	U	1.0	3.0	LIQ	MS	13-APR-10 13:24	100413-3
	Uranium	0.05	+/-2	U	0.05	0.2	LIQ	MS	13-APR-10 16:15	100413-5

SW846

Metals
-3a-
Initial and Continuing Calibration Blank Summary

SDG No.: 10-2093

Contract: LANL01004

Lab Code: GEL

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u> <u>ug/L</u>	<u>Acceptance</u>	<u>Conc</u> <u>Qual</u>	<u>MDL</u>	<u>RDL</u>	<u>Matrix</u>	<u>M</u>	<u>Analysis</u> <u>Date/Time</u>	<u>Run</u>
CCB05	Mercury	0.066	+/-2	U	0.066	0.2	LIQ	AV	02-MAR-10 10:19	030210W3-6
	Aluminum	68.0	+/-200	U	68.0	200	LIQ	P	29-MAR-10 20:16	032910C-1
	Arsenic	5.0	+/-30	U	5.0	30.0	LIQ	P	29-MAR-10 20:16	032910C-1
	Barium	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 20:16	032910C-1
	Calcium	50.0	+/-200	U	50.0	200	LIQ	P	29-MAR-10 20:16	032910C-1
	Chromium	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 20:16	032910C-1
	Cobalt	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 20:16	032910C-1
	Copper	3.0	+/-10	U	3.0	10.0	LIQ	P	29-MAR-10 20:16	032910C-1
	Iron	30.0	+/-100	U	30.0	100	LIQ	P	29-MAR-10 20:16	032910C-1
	Magnesium	85.0	+/-300	U	85.0	300	LIQ	P	29-MAR-10 20:16	032910C-1
	Nickel	1.5	+/-5	U	1.5	5.0	LIQ	P	29-MAR-10 20:16	032910C-1
	Potassium	50.0	+/-150	U	50.0	150	LIQ	P	29-MAR-10 20:16	032910C-1
	Selenium	5.0	+/-30	U	5.0	30.0	LIQ	P	29-MAR-10 20:16	032910C-1
	Silver	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 20:16	032910C-1
	Sodium	100	+/-300	U	100	300	LIQ	P	29-MAR-10 20:16	032910C-1
	Vanadium	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 20:16	032910C-1
	Zinc	3.3	+/-10	U	3.3	10.0	LIQ	P	29-MAR-10 20:16	032910C-1
	Antimony	1.0	+/-3	U	1.0	3.0	LIQ	MS	13-APR-10 13:39	100413-3
	Uranium	0.05	+/-2	U	0.05	0.2	LIQ	MS	13-APR-10 16:30	100413-5
CCB06	Mercury	0.066	+/-2	U	0.066	0.2	LIQ	AV	02-MAR-10 10:42	030210W3-6
	Aluminum	68.0	+/-200	U	68.0	200	LIQ	P	29-MAR-10 20:41	032910C-1
	Arsenic	5.0	+/-30	U	5.0	30.0	LIQ	P	29-MAR-10 20:41	032910C-1
	Barium	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 20:41	032910C-1
	Calcium	50.0	+/-200	U	50.0	200	LIQ	P	29-MAR-10 20:41	032910C-1
	Chromium	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 20:41	032910C-1
	Cobalt	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 20:41	032910C-1
	Copper	3.0	+/-10	U	3.0	10.0	LIQ	P	29-MAR-10 20:41	032910C-1
	Iron	30.0	+/-100	U	30.0	100	LIQ	P	29-MAR-10 20:41	032910C-1
	Magnesium	85.0	+/-300	U	85.0	300	LIQ	P	29-MAR-10 20:41	032910C-1
	Nickel	1.5	+/-5	U	1.5	5.0	LIQ	P	29-MAR-10 20:41	032910C-1

Metals
-3a-
Initial and Continuing Calibration Blank Summary

SDG No.: 10-2093

Contract: LANL01004

Lab Code: GEL

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u> <u>ug/L</u>	<u>Acceptance</u>	<u>Conc</u> <u>Qual</u>	<u>MDL</u>	<u>RDL</u>	<u>Matrix</u>	<u>M</u>	<u>Analysis</u> <u>Date/Time</u>	<u>Run</u>
	Potassium	50.0	+/-150	U	50.0	150	LIQ	P	29-MAR-10 20:41	032910C-1
	Selenium	5.0	+/-30	U	5.0	30.0	LIQ	P	29-MAR-10 20:41	032910C-1
	Silver	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 20:41	032910C-1
	Sodium	100	+/-300	U	100	300	LIQ	P	29-MAR-10 20:41	032910C-1
	Vanadium	-1.05	+/-5	J	1.0	5.0	LIQ	P	29-MAR-10 20:41	032910C-1
	Zinc	3.3	+/-10	U	3.3	10.0	LIQ	P	29-MAR-10 20:41	032910C-1
	Antimony	1.0	+/-3	U	1.0	3.0	LIQ	MS	13-APR-10 14:01	100413-3
	Uranium	0.05	+/-2	U	0.05	0.2	LIQ	MS	13-APR-10 16:45	100413-5
CCB07	Mercury	0.066	+/-2	U	0.066	0.2	LIQ	AV	02-MAR-10 11:06	030210W3-6
	Aluminum	68.0	+/-200	U	68.0	200	LIQ	P	29-MAR-10 21:05	032910C-1
	Arsenic	5.0	+/-30	U	5.0	30.0	LIQ	P	29-MAR-10 21:05	032910C-1
	Barium	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 21:05	032910C-1
	Calcium	50.0	+/-200	U	50.0	200	LIQ	P	29-MAR-10 21:05	032910C-1
	Chromium	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 21:05	032910C-1
	Cobalt	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 21:05	032910C-1
	Copper	3.0	+/-10	U	3.0	10.0	LIQ	P	29-MAR-10 21:05	032910C-1
	Iron	30.0	+/-100	U	30.0	100	LIQ	P	29-MAR-10 21:05	032910C-1
	Magnesium	85.0	+/-300	U	85.0	300	LIQ	P	29-MAR-10 21:05	032910C-1
	Nickel	1.5	+/-5	U	1.5	5.0	LIQ	P	29-MAR-10 21:05	032910C-1
	Potassium	50.0	+/-150	U	50.0	150	LIQ	P	29-MAR-10 21:05	032910C-1
	Selenium	5.0	+/-30	U	5.0	30.0	LIQ	P	29-MAR-10 21:05	032910C-1
	Silver	1.0	+/-5	U	1.0	5.0	LIQ	P	29-MAR-10 21:05	032910C-1
	Sodium	100	+/-300	U	100	300	LIQ	P	29-MAR-10 21:05	032910C-1
	Vanadium	-1.02	+/-5	J	1.0	5.0	LIQ	P	29-MAR-10 21:05	032910C-1
	Zinc	3.3	+/-10	U	3.3	10.0	LIQ	P	29-MAR-10 21:05	032910C-1
	Antimony	1.0	+/-3	U	1.0	3.0	LIQ	MS	13-APR-10 14:23	100413-3
CCB08	Mercury	0.066	+/-2	U	0.066	0.2	LIQ	AV	02-MAR-10 11:29	030210W3-6
CCB09	Mercury	0.066	+/-2	U	0.066	0.2	LIQ	AV	02-MAR-10 11:52	030210W3-6

Metals
-3a-
Initial and Continuing Calibration Blank Summary

SDG No.: 10-2093

Contract: LANL01004

Lab Code: GEL

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u> <u>ng/L</u>	<u>Acceptance</u>	<u>Conc</u> <u>Qual</u>	<u>MDL</u>	<u>RDL</u>	<u>Matrix</u>	<u>M</u>	<u>Analysis</u> <u>Date/Time</u>	<u>Run</u>
CCB10	Mercury	0.066	+/- .2	U	0.066	0.2	LIQ	AV	02-MAR-10 12:15	030210W3-6

METALS
-3b-
PREPARATION BLANK SUMMARY

SDG NO. 10-2093

Contract: LANL01004

Matrix: WATER

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>Acceptance Window</u>	<u>Conc Qual</u>	<u>M</u>	<u>MDL</u>	<u>RDL</u>
1202056573	Mercury	0.066	ug/L	+/-0.2	U	AV	0.066	0.2
1202056866	Aluminum	68	ug/L	+/-200	U	P	68	200
	Arsenic	5	ug/L	+/-30	U	P	5	30
	Calcium	50	ug/L	+/-200	U	P	50	200
	Copper	3	ug/L	+/-10	U	P	3	10
	Cobalt	1	ug/L	+/-5	U	P	1	5
	Chromium	1	ug/L	+/-5	U	P	1	5
	Barium	1	ug/L	+/-5	U	P	1	5
	Iron	30	ug/L	+/-100	U	P	30	100
	Zinc	3.3	ug/L	+/-10	U	P	3.3	10
	Vanadium	1	ug/L	+/-5	U	P	1	5
	Sodium	100	ug/L	+/-300	U	P	100	300
	Silver	1	ug/L	+/-5	U	P	1	5
	Selenium	5	ug/L	+/-30	U	P	5	30
	Potassium	50	ug/L	+/-150	U	P	50	150
	Nickel	1.5	ug/L	+/-5	U	P	1.5	5
	Magnesium	85	ug/L	+/-300	U	P	85	300
1202056872	Antimony	1	ug/L	+/-3	U	MS	1	3
	Beryllium	0.1	ug/L	+/-0.5	U	MS	0.1	0.5
	Cadmium	0.11	ug/L	+/-1	U	MS	0.11	1
	Lead	1.11	ug/L	+/-2	J	MS	0.5	2
	Manganese	1	ug/L	+/-5	U	MS	1	5
	Thallium	0.338	ug/L	+/-1	J	MS	0.3	1
	Uranium	0.05	ug/L	+/-0.2	U	MS	0.05	0.2

METALS
-4-
Interference Check Sample

SDG No: 10-2093

Contract: LANL01004

Lab Code: GEL

ICS: O2Si

Instrument: OPTIMA4

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>True Value</u>	<u>Units</u>	<u>% Recovery</u>	<u>Acceptance Window (%R)</u>	<u>Analysis Date/Time</u>	<u>Run Number</u>
ICSA01									
	Aluminum	511000	ug/L	500000	ug/L	102	80.0 – 120.0	29-MAR-10 18:43	032910C-1
	Arsenic	4.51	ug/L					29-MAR-10 18:43	032910C-1
	Barium	0.49	ug/L					29-MAR-10 18:43	032910C-1
	Calcium	479000	ug/L	500000	ug/L	95.7	80.0 – 120.0	29-MAR-10 18:43	032910C-1
	Chromium	1.9	ug/L					29-MAR-10 18:43	032910C-1
	Cobalt	-6.27	ug/L					29-MAR-10 18:43	032910C-1
	Copper	-2.45	ug/L					29-MAR-10 18:43	032910C-1
	Iron	189000	ug/L	200000	ug/L	94.6	80.0 – 120.0	29-MAR-10 18:43	032910C-1
	Magnesium	481000	ug/L	500000	ug/L	96.2	80.0 – 120.0	29-MAR-10 18:43	032910C-1
	Nickel	2.89	ug/L					29-MAR-10 18:43	032910C-1
	Potassium	-157.0	ug/L					29-MAR-10 18:43	032910C-1
	Selenium	-3.7	ug/L					29-MAR-10 18:43	032910C-1
	Silver	0.683	ug/L					29-MAR-10 18:43	032910C-1
	Sodium	12.5	ug/L					29-MAR-10 18:43	032910C-1
	Vanadium	1.57	ug/L					29-MAR-10 18:43	032910C-1
	Zinc	7.6	ug/L					29-MAR-10 18:43	032910C-1
ICSAB01									
	Aluminum	520000	ug/L	500000	ug/L	104	80.0 – 120.0	29-MAR-10 18:45	032910C-1
	Arsenic	526	ug/L	500	ug/L	105	80.0 – 120.0	29-MAR-10 18:45	032910C-1
	Barium	500	ug/L	500	ug/L	100	80.0 – 120.0	29-MAR-10 18:45	032910C-1
	Calcium	487000	ug/L	500000	ug/L	97.4	80.0 – 120.0	29-MAR-10 18:45	032910C-1
	Chromium	485	ug/L	500	ug/L	96.9	80.0 – 120.0	29-MAR-10 18:45	032910C-1
	Cobalt	437	ug/L	500	ug/L	87.5	80.0 – 120.0	29-MAR-10 18:45	032910C-1
	Copper	537	ug/L	500	ug/L	107	80.0 – 120.0	29-MAR-10 18:45	032910C-1
	Iron	191000	ug/L	200000	ug/L	95.3	80.0 – 120.0	29-MAR-10 18:45	032910C-1
	Magnesium	483000	ug/L	500000	ug/L	96.6	80.0 – 120.0	29-MAR-10 18:45	032910C-1
	Nickel	451	ug/L	500	ug/L	90.1	80.0 – 120.0	29-MAR-10 18:45	032910C-1
	Potassium	5450	ug/L	5000	ug/L	109	80.0 – 120.0	29-MAR-10 18:45	032910C-1
	Selenium	2360	ug/L	2500	ug/L	94.4	80.0 – 120.0	29-MAR-10 18:45	032910C-1

SW846

METALS

-4-

Interference Check Sample

SDG No: 10-2093

Contract: LANL01004

Lab Code: GEL

ICS:

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>True Value</u>	<u>Units</u>	<u>% Recovery</u>	<u>Acceptance Window (%R)</u>	<u>Analysis Date/Time</u>	<u>Run Number</u>
	Silver	271	ug/L	250	ug/L	108	80.0 – 120.0	29-MAR-10 18:45	032910C-1
	Sodium	5320	ug/L	5000	ug/L	106	80.0 – 120.0	29-MAR-10 18:45	032910C-1
	Vanadium	517	ug/L	500	ug/L	103	80.0 – 120.0	29-MAR-10 18:45	032910C-1
	Zinc	484	ug/L	500	ug/L	96.8	80.0 – 120.0	29-MAR-10 18:45	032910C-1

METALS

-4-

Interference Check Sample

SDG No: 10-2093

Contract: LANL01004

Lab Code: GEL

ICS: O2Si

Instrument: ICPMS4

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>True Value</u>	<u>Units</u>	<u>% Recovery</u>	<u>Acceptance Window (%R)</u>	<u>Analysis Date/Time</u>	<u>Run Number</u>
ICSA01									
	Beryllium	0.135	ug/L					12-APR-10 03:20	100411-2
	Cadmium	0.235	ug/L					12-APR-10 03:20	100411-2
	Lead	0.207	ug/L					12-APR-10 03:20	100411-2
	Manganese	5.81	ug/L					12-APR-10 03:20	100411-2
	Thallium	-0.037	ug/L					12-APR-10 03:20	100411-2
ICSAB01									
	Beryllium	17.9	ug/L	20	ug/L	89.5	80.0 - 120.0	12-APR-10 03:26	100411-2
	Cadmium	19.0	ug/L	20.44	ug/L	92.7	80.0 - 120.0	12-APR-10 03:26	100411-2
	Lead	18.5	ug/L	20.19	ug/L	91.7	80.0 - 120.0	12-APR-10 03:26	100411-2
	Manganese	25.4	ug/L	25.8	ug/L	98.4	80.0 - 120.0	12-APR-10 03:26	100411-2
	Thallium	17.7	ug/L	20	ug/L	88.5	80.0 - 120.0	12-APR-10 03:26	100411-2

METALS

-4-

Interference Check Sample

SDG No: 10-2093

Contract: LANL01004

Lab Code: GEL

ICS: O2Si

Instrument: ICPMS5

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>True Value</u>	<u>Units</u>	<u>% Recovery</u>	<u>Acceptance Window (%R)</u>	<u>Analysis Date/Time</u>	<u>Run Number</u>
ICSA01	Antimony	0.265	ug/L					13-APR-10 11:59	100413-3
ICSAB01	Antimony	20.3	ug/L	20	ug/L	101	80.0 - 120.0	13-APR-10 12:02	100413-3

METALS
-4-
Interference Check Sample

SDG No: 10-2093

Contract: LANL01004

Lab Code: GEL

ICS: O2Si

Instrument: ICPMS5

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>True Value</u>	<u>Units</u>	<u>% Recovery</u>	<u>Acceptance Window (%R)</u>	<u>Analysis Date/Time</u>	<u>Run Number</u>
ICSA01	Uranium	-0.002	ug/L					13-APR-10 15:22	100413-5
ICSAB01	Uranium	21.0	ug/L	20	ug/L	105	80.0 - 120.0	13-APR-10 15:24	100413-5

METALS

-5a-

Matrix Spike Summary

SDG NO. 10-2093 **Client ID** WST16-10-12239S**Contract:** LANL01004 **Level:** Low**Matrix:** WATER **% Solids:****Sample ID:** 248145001 **Spike ID:** 1202056576

Analyte	Units	Acceptance Limit	Spiked Result	C	Sample Result	C	Spike Added	% Recovery	Qual	M
Mercury	ug/L	75-125	2.27		0.066	U	2	112		AV

METALS

-5a-

Matrix Spike Summary

SDG NO. 10-2093 Client ID RE36-10-7529S

Contract: LANL01004 Level: Low

Matrix: WATER % Solids:

Sample ID: 248199001 Spike ID: 1202056869

Analyte	Units	Acceptance Limit	Spiked Result	C	Sample Result	C	Spike Added	% Recovery	Qual	M
Calcium	ug/L	75-125	4930		50	U	5000	97.8		P
Chromium	ug/L	75-125	486		1	U	500	97.1		P
Cobalt	ug/L	75-125	474		1	U	500	94.8		P
Copper	ug/L	75-125	496		3	U	500	99		P
Iron	ug/L	75-125	4880		30	U	5000	97.1		P
Magnesium	ug/L	75-125	5060		85	U	5000	101		P
Nickel	ug/L	75-125	487		1.5	U	500	97.4		P
Potassium	ug/L	75-125	4860		50	U	5000	96.2		P
Selenium	ug/L	75-125	461		5	U	500	92.2		P
Silver	ug/L	75-125	476		1	U	500	95.1		P
Sodium	ug/L	75-125	5030		115	J	5000	98.3		P
Vanadium	ug/L	75-125	497		1	U	500	99.4		P
Zinc	ug/L	75-125	467		3.3	U	500	93.1		P
Aluminum	ug/L	75-125	5190		68	U	5000	104		P
Arsenic	ug/L	75-125	535		5	U	500	107		P
Barium	ug/L	75-125	502		1	U	500	100		P

METALS

-5a-

Matrix Spike Summary

SDG NO. 10-2093

Client ID RE36-10-7529S

Contract: LANL01004

Level: Low

Matrix: WATER

% Solids:

Sample ID: 248199001

Spike ID: 1202056875

<u>Analyte</u>	<u>Units</u>	<u>Acceptance Limit</u>	<u>Spiked Result</u>	<u>C</u>	<u>Sample Result</u>	<u>C</u>	<u>Spike Added</u>	<u>% Recovery</u>	<u>Qual</u>	<u>M</u>
Antimony	ug/L	75-125	206		1	U	200	103		MS
Beryllium	ug/L	75-125	48.6		0.1	U	50	97.2		MS
Cadmium	ug/L	75-125	9.94		0.11	U	10	99.4		MS
Lead	ug/L	75-125	41.5		1.43	J	40	100		MS
Manganese	ug/L	75-125	51.9		1	U	50	103		MS
Thallium	ug/L	75-125	84.4		0.3	U	100	84.1		MS
Uranium	ug/L	75-125	45.2		0.05	U	50	90.4		MS

Metals
-6-
Duplicate Sample Summary

SDG No.: 10-2093

Contract: LANL01004

Lab Code: GEL

Matrix: LIQUID

Level: Low

Client ID: WST16-10-12239D

Sample ID: 248145001

Duplicate ID: 1202056575

Percent Solids for Dup: N/A

Analyte	Units	Acceptance Limit	Sample Result	C	Duplicate Result	C	RPD	Qual	M
Mercury	ug/L		0.066 U		0.066 U				AV

Metals
-6-
Duplicate Sample Summary

SDG No.: 10-2093

Contract: LANL01004

Lab Code: GEL

Matrix: LIQUID

Level: Low

Client ID: RE36-10-7529D

Sample ID: 248199001

Duplicate ID: 1202056868

Percent Solids for Dup: N/A

Analyte	Units	Acceptance Limit	Sample Result	C	Duplicate Result	C	RPD	Qual	M
Aluminum	ug/L		68 U		68 U				P
Arsenic	ug/L		5 U		5 U				P
Barium	ug/L		1 U		1 U				P
Calcium	ug/L		50 U		50 U				P
Chromium	ug/L		1 U		1 U				P
Cobalt	ug/L		1 U		1 U				P
Copper	ug/L		3 U		3 U				P
Iron	ug/L		30 U		30 U				P
Magnesium	ug/L		85 U		85 U				P
Nickel	ug/L		1.5 U		1.5 U				P
Potassium	ug/L		50 U		50 U				P
Selenium	ug/L		5 U		5 U				P
Silver	ug/L		1 U		1 U				P
Sodium	ug/L	+/-300	115 J		105 J		9.86		P
Vanadium	ug/L		1 U		1 U				P
Zinc	ug/L		3.3 U		3.3 U				P

Metals

-6-

Duplicate Sample Summary

SDG No.: 10-2093

Contract: LANL01004

Lab Code: GEL

Matrix: LIQUID

Level: Low

Client ID: RE36-10-7529D

Sample ID: 248199001

Duplicate ID: 1202056874

Percent Solids for Dup: N/A

Analyte	Units	Acceptance Limit	Sample Result	C	Duplicate Result	C	RPD	Qual	M
Antimony	ug/L		1 U		1 U				MS
Beryllium	ug/L		0.1 U		0.1 U				MS
Cadmium	ug/L		0.11 U		0.11 U				MS
Lead	ug/L	+/-2	1.43 J		0.631 J		77.4		MS
Manganese	ug/L		1 U		1 U				MS
Thallium	ug/L		0.3 U		0.3 U				MS
Uranium	ug/L		0.05 U		0.05 U				MS

METALS

-7-

Laboratory Control Sample Summary

SDG NO. 10-2093

Contract: LANL01004

Aqueous LCS Source:GEL

Solid LCS Source:

<u>Sample ID</u>	<u>Analyte</u>	<u>Units</u>	<u>True Value</u>	<u>Result</u>	<u>C</u>	<u>% Recovery</u>	<u>Acceptance Limit</u>	<u>M</u>
1202056574	Mercury	ug/L	2	2.21		110	80-120	AV

METALS
-7-
Laboratory Control Sample Summary

SDG NO. 10-2093

Contract: LANL01004

Aqueous LCS Source: OS2I

Solid LCS Source:

<u>Sample ID</u>	<u>Analyte</u>	<u>Units</u>	<u>True Value</u>	<u>Result</u>	<u>C</u>	<u>% Recovery</u>	<u>Acceptance Limit</u>	<u>M</u>
1202056867								
	Aluminum	ug/L	5000	5200		104	80-120	P
	Arsenic	ug/L	500	539		108	80-120	P
	Barium	ug/L	500	509		102	80-120	P
	Calcium	ug/L	5000	4960		99.1	80-120	P
	Chromium	ug/L	500	492		98.3	80-120	P
	Cobalt	ug/L	500	481		96.2	80-120	P
	Copper	ug/L	500	502		100	80-120	P
	Iron	ug/L	5000	4920		98.3	80-120	P
	Magnesium	ug/L	5000	5110		102	80-120	P
	Nickel	ug/L	500	496		99.2	80-120	P
	Potassium	ug/L	5000	4810		96.2	80-120	P
	Selenium	ug/L	500	475		95	80-120	P
	Silver	ug/L	500	482		96.5	80-120	P
	Sodium	ug/L	5000	4930		98.6	80-120	P
	Vanadium	ug/L	500	504		101	80-120	P
	Zinc	ug/L	500	477		95.3	80-120	P

METALS

-7-

Laboratory Control Sample Summary

SDG NO. 10-2093

Contract: LANL01004

Aqueous LCS Source:O2si

Solid LCS Source:

<u>Sample ID</u>	<u>Analyte</u>	<u>Units</u>	<u>True Value</u>	<u>Result</u>	<u>C</u>	<u>% Recovery</u>	<u>Acceptance Limit</u>	<u>M</u>
1202056873								
	Antimony	ug/L	50	55.1		110	80-120	MS
	Beryllium	ug/L	50	48.6		97.1	80-120	MS
	Cadmium	ug/L	50	48.2		96.4	80-120	MS
	Lead	ug/L	50	52.2		104	80-120	MS
	Manganese	ug/L	50	53.8		108	80-120	MS
	Thallium	ug/L	50	47.8		95.6	80-120	MS
	Uranium	ug/L	50	44.9		89.7	80-120	MS

METALS

-9-

Serial Dilution Sample Summary

SDG NO. 10-2093 Client ID WST16-10-12239L

Contract: LANL01004

Matrix: LIQUID Level: Low

Sample ID: 248145001 Serial Dilution ID: 1202056577

<u>Analyte</u>	<u>Initial Value ug/L</u>	<u>C</u>	<u>Serial Value ug/L</u>	<u>C</u>	<u>% Difference</u>	<u>Qual</u>	<u>Acceptance Limit</u>	<u>M</u>
Mercury	.066	U	.33	U				AV

METALS

-9-

Serial Dilution Sample Summary

SDG NO. 10-2093

Client ID RE36-10-7529L

Contract: LANL01004

Matrix: LIQUID

Level: Low

Sample ID: 248199001

Serial Dilution ID: 1202056870

Analyte	Initial Value ug/L	C	Serial Value ug/L	C	% Difference	Qual	Acceptance Limit	M
Aluminum	68	U	340	U				P
Arsenic	5	U	25	U				P
Barium	1	U	5	U				P
Calcium	50	U	250	U				P
Chromium	1	U	5	U				P
Cobalt	1	U	5	U				P
Copper	3	U	15	U				P
Iron	30	U	150	U				P
Magnesium	85	U	425	U				P
Nickel	1.5	U	7.5	U				P
Potassium	50	U	250	U				P
Selenium	5	U	25	U				P
Silver	1	U	5	U				P
Sodium	115	J	500	U	100			P
Vanadium	1	U	5	U				P
Zinc	3.3	U	16.5	U				P

METALS

-9-

Serial Dilution Sample Summary

SDG NO. 10-2093 Client ID RE36-10-7529L

Contract: LANL01004

Matrix: LIQUID Level: Low

Sample ID: 248199001 Serial Dilution ID: 1202056876

Analyte	Initial Value ug/L	C	Serial Value ug/L	C	% Difference	Qual	Acceptance Limit	M
Antimony	1	U	5	U				MS
Beryllium	.1	U	.5	U				MS
Cadmium	.11	U	.55	U				MS
Lead	1.43	J	2.5	U	100			MS
Manganese	1	U	5	U				MS
Thallium	.3	U	13.4					MS
Uranium	.05	U	.25	U				MS

METALS
-13-
SAMPLE PREPARATION SUMMARY

SDG No: 10-2093

Method Type: P

Contract: LANL01004

Lab Code: GEL

<u>Sample ID</u>	<u>Client ID</u>	<u>Sample Type</u>	<u>Matrix</u>	<u>Prep Date</u>	<u>Initial Sample Size</u>	<u>Final Sample Volume</u>	<u>Percent Solids</u>
Batch Number	959108						
1202056866	MB for batch 959108	MB	W	04-MAR-10	50mL	50mL	
1202056867	LCS for batch 959108	LCS	W	04-MAR-10	50mL	50mL	
1202056869	RE36-10-7529S	MS	W	04-MAR-10	50mL	50mL	
1202056868	RE36-10-7529D	DUP	W	04-MAR-10	50mL	50mL	
248117001	RE36-10-8458	SAMPLE	W	04-MAR-10	50mL	50mL	

SW846

METALS
-13-
SAMPLE PREPARATION SUMMARY

SDG No: 10-2093

Method Type: MS

Contract: LANL01004

Lab Code: GEL

<u>Sample ID</u>	<u>Client ID</u>	<u>Sample Type</u>	<u>Matrix</u>	<u>Prep Date</u>	<u>Initial Sample Size</u>	<u>Final Sample Volume</u>	<u>Percent Solids</u>
Batch Number	959110						
1202056872	MB for batch 959110	MB	W	04-MAR-10	50mL	50mL	
1202056873	LCS for batch 959110	LCS	W	04-MAR-10	50mL	50mL	
1202056875	RE36-10-7529S	MS	W	04-MAR-10	50mL	50mL	
1202056874	RE36-10-7529D	DUP	W	04-MAR-10	50mL	50mL	
248117001	RE36-10-8458	SAMPLE	W	04-MAR-10	50mL	50mL	

SW846

METALS
-13-
SAMPLE PREPARATION SUMMARY

SDG No: 10-2093

Method Type: AV

Contract: LANL01004

Lab Code: GEL

<u>Sample ID</u>	<u>Client ID</u>	<u>Sample Type</u>	<u>Matrix</u>	<u>Prep Date</u>	<u>Initial Sample Size</u>	<u>Final Sample Volume</u>	<u>Percent Solids</u>
Batch Number	958949						
1202056573	MB for batch 958949	MB	W	01-MAR-10	20mL	20mL	
1202056574	LCS for batch 958949	LCS	W	01-MAR-10	20mL	20mL	
1202056576	WST16-10-12239S	MS	W	01-MAR-10	20mL	20mL	
1202056575	WST16-10-12239D	DUP	W	01-MAR-10	20mL	20mL	
248117001	RE36-10-8458	SAMPLE	W	01-MAR-10	20mL	20mL	

SW846

Metals
-14-
Analysis Run Log

Contract: LANL01004

Lab Code: GEL

Inst Name: ICPMS5

Start Date: 13-APR-10

End Date: 13-APR-10

Client Sdg: 10-2093

Method MS

Data File: 100413-3

Samp No.	D/F	Run Time	Al	Sb	As	Ba	Be	Cd	Ca	Cr	Co	Cu	Fe	Pb	Mg	Mn	Hg	Ni	K	Se	Ag	Na	Tl	U	V	Zn
S0.0	1	11:45:00		X																						
S10	1	11:47:00		X																						
S100	1	11:49:00		X																						
ICV01	1	11:52:00		X																						
ICB01	1	11:54:00		X																						
CRDL01	1	11:57:00		X																						
ICSA01	1	11:59:00		X																						
ICSAB01	1	12:02:00		X																						
CCV01	1	12:04:00		X																						
CCB01	1	12:07:00		X																						
ZZZZZZ	1	12:09:00																								
ZZZZZZ	1	12:12:00																								
ZZZZZZ	1	12:14:00																								
ZZZZZZ	1	12:16:00																								
ZZZZZZ	1	12:19:00																								
ZZZZZZ	1	12:21:00																								
ZZZZZZ	1	12:24:00																								
ZZZZZZ	5	12:26:00																								
ZZZZZZ	1	12:29:00																								
CCV02	1	12:31:00		X																						
CCB02	1	12:34:00		X																						
ZZZZZZ	1	12:36:00																								
ZZZZZZ	1	12:39:00																								
ZZZZZZ	1	12:41:00																								
ZZZZZZ	1	12:44:00																								
ZZZZZZ	1	12:46:00																								
ZZZZZZ	1	12:48:00																								
ZZZZZZ	1	12:51:00																								
CCV03	1	12:53:00		X																						
CCB03	1	12:56:00		X																						
ZZZZZZ	1	12:58:00																								
ZZZZZZ	1	13:01:00																								
ZZZZZZ	1	13:03:00																								
ZZZZZZ	1	13:06:00																								
ZZZZZZ	1	13:08:00																								
ZZZZZZ	1	13:11:00																								
ZZZZZZ	5	13:13:00																								
ZZZZZZ	1	13:19:00																								
CCV04	1	13:21:00		X																						
CCB04	1	13:24:00		X																						

Metals
-14-
Analysis Run Log

Samp No.	D/F	Run Time
ZZZZZZ	1	13:26:00
ZZZZZZ	1	13:29:00
ZZZZZZ	1	13:31:00
ZZZZZZ	5	13:34:00
CCV05	1	13:36:00
CCB05	1	13:39:00
1202056872	1	13:41:00
1202056873	1	13:44:00
ZZZZZZ	1	13:46:00
248117001	1	13:49:00
ZZZZZZ	1	13:51:00
ZZZZZZ	1	13:54:00
ZZZZZZ	1	13:56:00
CCV06	1	13:59:00
CCB06	1	14:01:00
ZZZZZZ	1	14:04:00
ZZZZZZ	1	14:06:00
ZZZZZZ	1	14:08:00
ZZZZZZ	1	14:11:00
1202056874	1	14:13:00
1202056875	1	14:16:00
1202056876	5	14:18:00
CCV07	1	14:21:00
CCB07	1	14:23:00

Metals
-14-
Analysis Run Log

Contract: LANL01004

Lab Code: GEL

Inst Name: ICPMS5

Start Date: 13-APR-10

Client Sdg: 10-2093

Method MS

Data File: 100413-5

End Date: 13-APR-10

Samp No.	D/F	Run Time	Al	Sb	As	Ba	Be	Cd	Ca	Cr	Co	Cu	Fe	Pb	Mg	Mn	Hg	Ni	K	Se	Ag	Na	Tl	U	V	Zn
S0.0	1	15:12:00																						X		
S10	1	15:14:00																						X		
S100	1	15:16:00																						X		
ICV01	1	15:17:00																						X		
ICB01	1	15:19:00																						X		
CRDL01	1	15:21:00																						X		
ICSA01	1	15:22:00																						X		
ICSAB01	1	15:24:00																						X		
CCV01	1	15:26:00																						X		
CCB01	1	15:27:00																						X		
ZZZZZZ	1	15:29:00																								
ZZZZZZ	1	15:31:00																								
ZZZZZZ	1	15:32:00																								
ZZZZZZ	1	15:34:00																								
ZZZZZZ	1	15:35:00																								
ZZZZZZ	1	15:37:00																								
ZZZZZZ	1	15:39:00																								
ZZZZZZ	5	15:40:00																								
ZZZZZZ	1	15:42:00																								
CCV02	1	15:44:00																						X		
CCB02	1	15:45:00																						X		
ZZZZZZ	1	15:47:00																								
ZZZZZZ	1	15:49:00																								
ZZZZZZ	1	15:50:00																								
ZZZZZZ	1	15:52:00																								
ZZZZZZ	1	15:54:00																								
ZZZZZZ	1	15:55:00																								
ZZZZZZ	1	15:57:00																								
CCV03	1	15:59:00																						X		
CCB03	1	16:00:00																						X		
ZZZZZZ	1	16:02:00																								
ZZZZZZ	1	16:04:00																								
ZZZZZZ	1	16:05:00																								
ZZZZZZ	1	16:07:00																								
ZZZZZZ	1	16:09:00																								
ZZZZZZ	1	16:10:00																								
ZZZZZZ	5	16:12:00																								
CCV04	1	16:14:00																						X		
CCB04	1	16:15:00																						X		
1202056872	1	16:17:00																						X		

[illegible]

Metals
-14-
Analysis Run Log

Contract: LANL01004

Lab Code: GEL

Inst Name: HG3

Start Date: 02-MAR-10

End Date: 02-MAR-10

Client Sdg: 10-2093

Method AV

Data File: 030210W3-6

Samp No.	D/F	Run Time	Al	Sb	As	Ba	Be	Cd	Ca	Cr	Co	Cu	Fe	Pb	Mg	Mn	Hg	Ni	K	Se	Ag	Na	Tl	U	V	Zn
S0.0	1	08:28:00															X									
S0.2	1	08:30:00															X									
S0.5	1	08:31:00															X									
S2.0	1	08:33:00															X									
S5.0	1	08:35:00															X									
S10.0	1	08:37:00															X									
ICV01	1	08:39:00															X									
ICB01	1	08:41:00															X									
CRDL01	1	08:43:00															X									
CCV01	1	08:45:00															X									
CCB01	1	08:47:00															X									
ZZZZZZ	1	08:49:00																								
ZZZZZZ	1	08:51:00																								
ZZZZZZ	1	08:53:00																								
ZZZZZZ	1	08:55:00																								
ZZZZZZ	1	08:57:00																								
ZZZZZZ	5	08:58:00																								
ZZZZZZ	1	09:00:00																								
ZZZZZZ	1	09:02:00																								
ZZZZZZ	1	09:04:00																								
ZZZZZZ	1	09:06:00																								
CCV02	1	09:08:00															X									
CCB02	1	09:10:00															X									
ZZZZZZ	1	09:12:00																								
ZZZZZZ	1	09:14:00																								
ZZZZZZ	1	09:16:00																								
ZZZZZZ	1	09:18:00																								
ZZZZZZ	1	09:20:00																								
ZZZZZZ	1	09:21:00																								
ZZZZZZ	1	09:23:00																								
ZZZZZZ	1	09:25:00																								
ZZZZZZ	5	09:27:00																								
ZZZZZZ	1	09:29:00																								
CCV03	1	09:31:00															X									
CCB03	1	09:33:00															X									
ZZZZZZ	1	09:35:00																								
ZZZZZZ	1	09:37:00																								
ZZZZZZ	1	09:39:00																								
ZZZZZZ	1	09:41:00																								
ZZZZZZ	1	09:43:00																								

Metals
-14-
Analysis Run Log

Samp No.	D/F	Run Time
ZZZZZZ	1	09:45:00
ZZZZZZ	1	09:47:00
ZZZZZZ	1	09:48:00
ZZZZZZ	1	09:50:00
ZZZZZZ	1	09:52:00
CCV04	1	09:54:00
CCB04	1	09:56:00
ZZZZZZ	1	09:58:00
ZZZZZZ	1	10:00:00
ZZZZZZ	1	10:02:00
ZZZZZZ	5	10:04:00
ZZZZZZ	1	10:06:00
ZZZZZZ	1	10:08:00
ZZZZZZ	1	10:10:00
ZZZZZZ	1	10:12:00
ZZZZZZ	1	10:13:00
ZZZZZZ	1	10:15:00
CCV05	1	10:17:00
CCB05	1	10:19:00
ZZZZZZ	1	10:21:00
ZZZZZZ	1	10:23:00
ZZZZZZ	1	10:25:00
ZZZZZZ	1	10:27:00
ZZZZZZ	1	10:29:00
ZZZZZZ	5	10:31:00
ZZZZZZ	1	10:33:00
ZZZZZZ	1	10:35:00
ZZZZZZ	1	10:37:00
ZZZZZZ	1	10:39:00
CCV06	1	10:41:00
CCB06	1	10:42:00
ZZZZZZ	1	10:44:00
ZZZZZZ	1	10:46:00
ZZZZZZ	1	10:48:00
ZZZZZZ	1	10:50:00
ZZZZZZ	1	10:52:00
ZZZZZZ	1	10:54:00
ZZZZZZ	1	10:56:00
ZZZZZZ	1	10:58:00
ZZZZZZ	1	11:00:00

Metals
-14-
Analysis Run Log

Samp No.	D/F	Run Time	Al	Sb	As	Ba	Be	Cd	Ca	Cr	Co	Cu	Fe	Pb	Mg	Mn	Hg	Ni	K	Se	Ag	Na	Tl	U	V	Zn
ZZZZZZ	5	11:02:00																								
CCV07	1	11:04:00															X									
CCB07	1	11:06:00															X									
ZZZZZZ	1	11:08:00																								
ZZZZZZ	1	11:09:00																								
ZZZZZZ	1	11:11:00																								
ZZZZZZ	1	11:13:00																								
1202056573	1	11:15:00															X									
1202056574	1	11:17:00															X									
ZZZZZZ	1	11:19:00																								
ZZZZZZ	1	11:21:00																								
ZZZZZZ	1	11:23:00																								
ZZZZZZ	1	11:25:00																								
CCV08	1	11:27:00															X									
CCB08	1	11:29:00															X									
ZZZZZZ	1	11:31:00																								
ZZZZZZ	1	11:33:00																								
ZZZZZZ	1	11:35:00																								
ZZZZZZ	1	11:37:00																								
ZZZZZZ	1	11:39:00																								
ZZZZZZ	1	11:40:00																								
ZZZZZZ	1	11:42:00																								
ZZZZZZ	1	11:44:00																								
ZZZZZZ	1	11:46:00																								
ZZZZZZ	1	11:48:00																								
CCV09	1	11:50:00															X									
CCB09	1	11:52:00															X									
ZZZZZZ	1	11:54:00																								
ZZZZZZ	1	11:56:00																								
248117001	1	11:58:00															X									
ZZZZZZ	1	12:00:00																								
1202056575	1	12:02:00															X									
1202056576	1	12:04:00															X									
1202056577	5	12:06:00															X									
ZZZZZZ	1	12:08:00																								
ZZZZZZ	1	12:10:00																								
ZZZZZZ	1	12:12:00																								
CCV10	1	12:14:00															X									
CCB10	1	12:15:00															X									

Metals
-14-
Analysis Run Log

Contract: LANL01004

Lab Code: GEL

Inst Name: OPTIMA4

Start Date: 29-MAR-10

End Date: 29-MAR-10

Client Sdg: 10-2093

Method: P

Data File: 032910C-1

Samp No.	D/F	Run Time	Al	Sb	As	Ba	Be	Cd	Ca	Cr	Co	Cu	Fe	Pb	Mg	Mn	Hg	Ni	K	Se	Ag	Na	Tl	U	V	Zn
S0.0	1	18:25:00	X		X	X			X	X	X	X	X		X			X	X	X	X	X			X	X
S0.1	1	18:28:00			X	X				X	X	X						X	X	X	X				X	X
S0.5	1	18:30:00	X		X	X			X	X	X	X			X			X	X	X	X				X	X
SCAL	1	18:32:00	X		X	X			X	X	X	X	X		X			X	X	X	X	X			X	X
S10	1	18:34:00	X						X				X		X							X				
ICV01	1	18:35:00	X		X	X			X	X	X	X	X		X			X	X	X	X	X			X	X
ICB01	1	18:37:00	X		X	X			X	X	X	X	X		X			X	X	X	X	X			X	X
PQL01	1	18:40:00	X		X	X			X	X	X	X	X		X			X	X	X	X	X			X	X
ICSA01	1	18:43:00	X		X	X			X	X	X	X	X		X			X	X	X	X	X			X	X
ICSAB01	1	18:45:00	X		X	X			X	X	X	X	X		X			X	X	X	X	X			X	X
LR01	1	18:46:00	X		X	X			X	X	X	X	X		X			X	X	X	X	X			X	X
LR02	1	18:48:00	X		X	X			X	X	X	X	X		X			X	X	X	X	X			X	X
CCV01	1	18:49:00	X		X	X			X	X	X	X	X		X			X	X	X	X	X			X	X
CCB01	1	18:51:00	X		X	X			X	X	X	X	X		X			X	X	X	X	X			X	X
CCV02	1	18:57:00	X		X	X			X	X	X	X	X		X			X	X	X	X	X			X	X
CCB02	1	18:59:00	X		X	X			X	X	X	X	X		X			X	X	X	X	X			X	X
ZZZZZZ	1	19:17:00																								
ZZZZZZ	1	19:20:00																								
ZZZZZZ	1	19:21:00																								
ZZZZZZ	1	19:23:00																								
ZZZZZZ	1	19:25:00																								
ZZZZZZ	1	19:26:00																								
ZZZZZZ	5	19:29:00																								
CCV03	1	19:31:00	X		X	X			X	X	X	X	X		X			X	X	X	X	X			X	X
CCB03	1	19:33:00	X		X	X			X	X	X	X	X		X			X	X	X	X	X			X	X
ZZZZZZ	1	19:36:00																								
ZZZZZZ	1	19:38:00																								
ZZZZZZ	1	19:40:00																								
ZZZZZZ	1	19:42:00																								
ZZZZZZ	1	19:44:00																								
ZZZZZZ	1	19:46:00																								
ZZZZZZ	1	19:48:00																								
ZZZZZZ	1	19:50:00																								
CCV04	1	19:52:00	X		X	X			X	X	X	X	X		X			X	X	X	X	X			X	X
CCB04	1	19:54:00	X		X	X			X	X	X	X	X		X			X	X	X	X	X			X	X
ZZZZZZ	1	19:57:00																								
ZZZZZZ	1	19:59:00																								
ZZZZZZ	1	20:02:00																								
ZZZZZZ	1	20:04:00																								
ZZZZZZ	1	20:06:00																								

Samp No.	D/F	Run Time																								
ZZZZZZ	1	20:08:00																								
ZZZZZZ	1	20:10:00																								
ZZZZZZ	1	20:12:00																								
CCV05	1	20:14:00	X		X	X			X	X	X	X	X		X			X	X	X	X	X			X	X
CCB05	1	20:16:00	X		X	X			X	X	X	X	X		X			X	X	X	X	X			X	X
1202056866	1	20:20:00	X		X	X			X	X	X	X	X		X			X	X	X	X	X			X	X
1202056867	1	20:23:00	X		X	X			X	X	X	X	X		X			X	X	X	X	X			X	X
ZZZZZZ	1	20:25:00																								
1202056868	1	20:28:00	X		X	X			X	X	X	X	X		X			X	X	X	X	X			X	X
1202056869	1	20:31:00	X		X	X			X	X	X	X	X		X			X	X	X	X	X			X	X
1202056870	5	20:33:00	X		X	X			X	X	X	X	X		X			X	X	X	X	X			X	X
ZZZZZZ	1	20:36:00																								
CCV06	1	20:39:00	X		X	X			X	X	X	X	X		X			X	X	X	X	X			X	X
CCB06	1	20:41:00	X		X	X			X	X	X	X	X		X			X	X	X	X	X			X	X
248117001	1	20:44:00	X		X	X			X	X	X	X	X		X			X	X	X	X	X			X	X
ZZZZZZ	1	20:47:00																								
ZZZZZZ	1	20:50:00																								
ZZZZZZ	1	20:52:00																								
ZZZZZZ	1	20:55:00																								
ZZZZZZ	1	20:57:00																								
ZZZZZZ	1	21:00:00																								
CCV07	1	21:03:00	X		X	X			X	X	X	X	X		X			X	X	X	X	X			X	X
CCB07	1	21:05:00	X		X	X			X	X	X	X	X		X			X	X	X	X	X			X	X

Metals
-14-
Analysis Run Log

Contract: LANL01004

Lab Code: GEL

Inst Name: ICPMS4

Start Date: 12-APR-10

End Date: 12-APR-10

Client Sdg: 10-2093

Method MS

Data File: 100411-2

Samp No.	D/F	Run Time	Al	Sb	As	Ba	Be	Cd	Ca	Cr	Co	Cu	Fe	Pb	Mg	Mn	Hg	Ni	K	Se	Ag	Na	Tl	U	V	Zn
S0.0	1	02:43:00					X	X						X		X							X			
S10	1	02:49:00					X	X						X		X							X			
S100	1	02:55:00					X	X						X		X							X			
ICV01	1	03:01:00					X	X						X		X							X			
ICB01	1	03:08:00					X	X						X		X							X			
CRDL01	1	03:14:00					X	X						X		X							X			
ICSA01	1	03:20:00					X	X						X		X							X			
ICSAB01	1	03:26:00					X	X						X		X							X			
CCV01	1	03:32:00					X	X						X		X							X			
CCB01	1	03:38:00					X	X						X		X							X			
LR01	1	03:44:00					X	X						X		X							X			
CCV02	1	03:51:00					X	X						X		X							X			
CCB02	1	03:57:00					X	X						X		X							X			
1202056872	1	04:03:00					X	X						X		X							X			
1202056873	1	04:09:00					X	X						X		X							X			
ZZZZZZ	1	04:15:00																								
248117001	1	04:22:00					X	X						X		X							X			
ZZZZZZ	1	04:28:00																								
ZZZZZZ	1	04:34:00																								
ZZZZZZ	1	04:40:00																								
ZZZZZZ	1	04:46:00																								
ZZZZZZ	1	04:53:00																								
ZZZZZZ	1	04:59:00																								
CCV03	1	05:05:00					X	X						X		X							X			
CCB03	1	05:11:00					X	X						X		X							X			
ZZZZZZ	1	05:18:00																								
1202056874	1	05:24:00					X	X						X		X							X			
1202056875	1	05:30:00					X	X						X		X							X			
1202056876	5	05:36:00					X	X						X		X							X			
CCV04	1	05:42:00					X	X						X		X							X			
CCB04	1	05:49:00					X	X						X		X							X			

Standards

METALS
-10-
Instrument Detection Limits

SDG NO. 10-2093

Contract: LANL01004

Lab Code: GEL

MDL Effective Date: 01-JUL-09

ICP/MS	<u>Analyte</u>	<u>Wavelength</u>	<u>MDL</u>	<u>RDL</u>
		<u>(nm)</u>	<u>ug/L</u>	<u>ug/L</u>
LIQUID	Aluminum		15.0	30
	Antimony		1.0	3
	Arsenic		1.6	5
	Barium		0.6	2
	Beryllium		0.1	.5
	Cadmium		0.11	1
	Calcium		65.0	200
	Chromium		2.0	10
	Cobalt		0.1	1
	Copper		0.33	1
	Iron		33.0	100
	Lead		0.5	2
	Magnesium		5.2	15
	Manganese		1.0	5
	Nickel		0.5	2
	Potassium		80.0	300
	Selenium		1.0	5
	Silver		0.2	1
	Sodium		80.0	250
	Thallium		0.3	1
	Uranium		0.05	.2
	Vanadium		3.0	10
	Zinc		3.0	10

METALS
-10-
Instrument Detection Limits

SDG NO. 10-2093

Contract: LANL01004

Lab Code: GEL

MDL Effective Date: 01-JUL-09

	<u>Analyte</u>	<u>Wavelength</u> <u>(nm)</u>	<u>MDL</u> <u>ug/L</u>	<u>RDL</u> <u>ug/L</u>
MERCURY				
LIQUID	Mercury		0.066	.2

METALS
-10-
Instrument Detection Limits

SDG NO. 10-2093

Contract: LANL01004

Lab Code: GEL

MDL Effective Date: 01-JUL-09

ICP	<u>Analyte</u>	<u>Wavelength</u> (nm)	<u>MDL</u>	<u>RDL</u>
			<u>ug/L</u>	<u>ug/L</u>
LIQUID	Aluminum	396.153	68.0	200
	Antimony	206.836	3.0	10
	Arsenic	188.979	5.0	30
	Barium	233.527	1.0	5
	Beryllium	313.107	1.0	5
	Cadmium	226.502	1.0	5
	Calcium	317.933	50.0	200
	Chromium	267.716	1.0	5
	Cobalt	228.616	1.0	5
	Copper	324.752	3.0	10
	Iron	238.204	30.0	100
	Lead	220.353	3.3	10
	Magnesium	279.077	85.0	300
	Manganese	257.61	2.0	10
	Nickel	231.604	1.5	5
	Potassium	766.49	50.0	150
	Selenium	196.026	5.0	30
	Silver	328.068	1.0	5
	Sodium	589.592	100	300
	Thallium	190.801	5.0	20
	Uranium	409.014	10.0	50
	Vanadium	292.402	1.0	5
	Zinc	213.857	3.3	10

METALS
-11-
Interelement Correction Factors

Lab Code: GEL

GEL Job No: 10-2093

Contract: LANL01004

Instrument: OPTIMA4

Effective Dates: 22-MAR-10

Interelement Correction Factors (apparent ppb analyte/ppm interferent)

Parmname	Wavelength	Aluminum	Antimony	Arsenic	Barium	Beryllium
Aluminum	396.153	0.00000	0.00000	0.00000	0.00000	0.00000
Antimony	206.836	0.00676	0.00000	0.00000	0.00000	0.00000
Arsenic	188.979	0.00000	0.00000	0.00000	0.00000	0.00000
Barium	233.527	0.00000	0.00000	0.00000	0.00000	0.00000
Beryllium	313.107	0.00000	0.00000	0.00000	0.00000	0.00000
Boron	249.677	0.00000	0.00000	0.00000	0.00000	0.00000
Cadmium	226.502	0.00000	0.00000	0.00000	0.00000	0.00000
Chromium	267.716	0.00000	0.00000	0.00000	0.00000	0.00000
Cobalt	228.616	0.00000	0.00000	0.00000	-0.98369	0.00000
Copper	324.752	0.00000	0.00000	0.00000	0.00000	0.00000
Lead	220.353	-0.06206	0.00000	0.00000	0.00000	0.00000
Magnesium	279.077	0.00000	0.00000	0.00000	0.00000	0.00000
Manganese	257.61	0.00000	0.00000	0.00000	0.00000	0.00000
Molybdenum	202.031	0.00000	0.00000	0.00000	0.00000	0.00000
Phosphorous	214.914	-0.22134	0.00000	0.00000	0.00000	0.00000
Potassium	766.49	0.22220	0.00000	0.00000	0.00000	0.00000
Selenium	196.026	0.00000	0.00000	0.00000	0.00000	0.00000
Silicon	251.611	0.00000	0.00000	0.00000	0.00000	0.00000
Silver	328.068	0.00000	0.00000	0.00000	0.00000	0.00000
Sodium	589.592	0.00000	0.00000	0.00000	0.00000	0.00000
Strontium	421.552	0.00000	0.00000	0.00000	0.00000	0.00000
Sulfur	181.975	0.00000	0.00000	0.00000	0.00000	0.00000
Thallium	190.801	0.00000	0.00000	0.00000	0.00000	0.00000
Tin	189.927	0.00000	0.00000	0.00000	0.00000	0.00000
Titanium	334.94	0.00000	0.00000	0.00000	0.00000	0.00000
Uranium	409.014	0.00000	0.00000	0.00000	0.00000	0.00000
Vanadium	292.402	0.00000	0.00000	0.00000	0.00000	0.00000
Zinc	213.857	-0.01674	0.00000	0.00000	0.00000	0.00000

METALS
-11-
Interelement Correction Factors

Lab Code: GELGEL Job No: **10-2093**

Contract: LANL01004

Instrument: OPTIMA4

Effective Dates: **22-MAR-10**

Interelement Correction Factors (apparent ppb analyte/ppm interferent)

Parmname	Wavelength	Boron	Cadmium	Chromium	Cobalt	Copper
Aluminum	396.153	0.00000	0.00000	0.00000	0.00000	0.00000
Antimony	206.836	0.00000	0.00000	14.9992	0.00000	0.00000
Arsenic	188.979	0.00000	0.00000	-9.49960	0.00000	0.00000
Barium	233.527	0.00000	0.00000	0.00000	0.00000	0.00000
Beryllium	313.107	0.00000	0.00000	0.00000	0.00000	0.00000
Boron	249.677	0.00000	0.00000	0.00000	3.47778	0.00000
Cadmium	226.502	0.00000	0.00000	0.00000	0.00000	0.00000
Chromium	267.716	0.00000	0.00000	0.00000	0.00000	0.00000
Cobalt	228.616	0.00000	0.00000	-0.18390	0.00000	0.00000
Copper	324.752	0.00000	0.00000	0.00000	-0.60088	0.00000
Lead	220.353	0.00000	0.00000	0.00000	0.04741	0.32747
Magnesium	279.077	0.00000	0.00000	0.00000	0.00000	0.00000
Manganese	257.61	0.00000	0.00000	0.00000	0.00000	0.00000
Molybdenum	202.031	0.00000	0.00000	0.00000	0.00000	0.00000
Phosphorous	214.914	0.00000	0.00000	0.00000	0.00000	10.9289
Potassium	766.49	0.00000	0.00000	0.00000	0.00000	0.00000
Selenium	196.026	0.00000	0.00000	0.00000	0.00000	0.00000
Silicon	251.611	0.00000	0.00000	0.00000	0.00000	0.00000
Silver	328.068	0.00000	0.00000	-0.07359	0.00000	0.00000
Sodium	589.592	0.00000	0.00000	0.00000	0.00000	0.00000
Strontium	421.552	0.00000	0.00000	0.00000	0.00000	0.00000
Sulfur	181.975	0.00000	0.00000	0.00000	0.00000	0.00000
Thallium	190.801	0.00000	0.00000	0.00000	5.02864	0.00000
Tin	189.927	0.00000	0.00000	0.00000	0.00000	0.00000
Titanium	334.94	0.00000	0.00000	0.33675	0.00000	0.00000
Uranium	409.014	0.00000	0.00000	1.18768	0.00000	0.00000
Vanadium	292.402	0.00000	0.00000	-4.30004	0.00000	0.00000
Zinc	213.857	0.00000	0.00000	0.03286	0.12442	0.79397

METALS
-11-
Interelement Correction Factors

Lab Code: GELGEL Job No: **10-2093**

Contract: LANL01004

Instrument: OPTIMA4

Effective Dates: **22-MAR-10**

Interelement Correction Factors (apparent ppb analyte/ppm interferent)

Parmname	Wavelength	Lead	Magnesium	Manganese	Molybdenum	Phosphorous
Aluminum	396.153	0.00000	0.00000	0.00000	46.4438	0.00000
Antimony	206.836	0.00000	0.00000	0.00000	-14.0269	0.00000
Arsenic	188.979	0.00000	0.00000	0.00000	-2.84596	0.00000
Barium	233.527	0.00000	0.00000	0.00000	-0.32136	0.00000
Beryllium	313.107	0.00000	0.00000	0.00000	0.00000	0.00000
Boron	249.677	0.00000	0.00000	0.00000	0.00000	0.00000
Cadmium	226.502	0.00000	0.00000	0.00000	0.00000	0.00000
Chromium	267.716	0.00000	0.01216	0.24903	0.00000	0.00000
Cobalt	228.616	0.00000	0.00000	0.00000	0.00000	0.00000
Copper	324.752	0.00000	-0.02702	0.00000	0.00000	0.00000
Lead	220.353	0.00000	0.00000	0.00000	-2.77286	0.00000
Magnesium	279.077	0.00000	0.00000	0.00000	-24.4630	0.00000
Manganese	257.61	0.00000	0.03966	0.00000	0.00000	0.00000
Molybdenum	202.031	0.00000	-0.01826	0.00000	0.00000	0.00000
Phosphorous	214.914	0.00000	0.00000	0.00000	10.3832	0.00000
Potassium	766.49	0.00000	0.07568	0.00000	0.00000	0.00000
Selenium	196.026	0.00000	0.00000	0.00000	0.00000	0.00000
Silicon	251.611	0.00000	0.00000	0.00000	13.3443	0.00000
Silver	328.068	0.00000	0.00000	0.28019	-0.03095	0.00000
Sodium	589.592	0.00000	0.00000	0.00000	0.00000	0.00000
Strontium	421.552	0.00000	0.00000	0.00000	0.00000	0.00000
Sulfur	181.975	0.00000	0.00000	0.00000	-8.43314	0.00000
Thallium	190.801	0.00000	0.00000	-2.58065	0.00000	0.00000
Tin	189.927	0.00000	0.00000	0.00000	0.00000	0.00000
Titanium	334.94	0.00000	0.08144	0.00000	0.00000	0.00000
Uranium	409.014	0.00000	0.00000	-6.48399	0.00000	0.00000
Vanadium	292.402	0.00000	0.00000	0.00000	-10.3466	0.00000
Zinc	213.857	0.00000	0.00000	0.06887	-0.04597	0.00000

METALS
-11-
Interelement Correction Factors

Lab Code: GELGEL Job No: **10-2093**

Contract: LANL01004

Instrument: OPTIMA4

Effective Dates: **22-MAR-10**

Interelement Correction Factors (apparent ppb analyte/ppm interferent)

Parmname	Wavelength	Potassium	Selenium	Silicon	Silver	Sodium
Aluminum	396.153	0.00000	0.00000	0.00000	0.00000	0.00000
Antimony	206.836	0.00000	0.00000	0.00000	0.00000	0.00000
Arsenic	188.979	0.00000	0.00000	0.00000	0.00000	0.00000
Barium	233.527	0.00000	0.00000	0.00000	0.00000	0.00000
Beryllium	313.107	0.00000	0.00000	0.00000	0.00000	0.00000
Boron	249.677	0.00000	0.00000	0.00000	0.00000	0.00000
Cadmium	226.502	0.00000	0.00000	0.00000	0.00000	0.00000
Chromium	267.716	0.00000	0.00000	0.00000	0.00000	0.00000
Cobalt	228.616	0.00000	0.00000	0.00000	0.00000	0.00000
Copper	324.752	0.00000	0.00000	0.00000	0.00000	0.00000
Lead	220.353	0.00000	0.00000	0.00000	0.00000	0.00000
Magnesium	279.077	0.00000	0.00000	0.00000	0.00000	0.00000
Manganese	257.61	0.00000	0.00000	0.00000	0.00000	0.00000
Molybdenum	202.031	0.00000	0.00000	0.00000	0.00000	0.00000
Phosphorous	214.914	0.00000	0.00000	0.00000	0.00000	0.00000
Potassium	766.49	0.00000	0.00000	0.00000	0.00000	0.16274
Selenium	196.026	0.00000	0.00000	0.00000	0.00000	0.00000
Silicon	251.611	0.00000	0.00000	0.00000	0.00000	0.00000
Silver	328.068	0.00000	0.00000	0.00000	0.00000	0.00000
Sodium	589.592	0.88937	0.00000	0.00000	0.00000	0.00000
Strontium	421.552	0.00000	0.00000	0.00000	0.00000	0.00000
Sulfur	181.975	0.00000	0.00000	0.00000	0.00000	0.00000
Thallium	190.801	0.00000	0.00000	0.00000	0.00000	0.00000
Tin	189.927	0.00000	0.00000	0.00000	0.00000	0.00000
Titanium	334.94	0.00000	0.00000	0.00000	0.00000	0.00000
Uranium	409.014	0.00000	0.00000	0.00000	0.00000	0.00000
Vanadium	292.402	0.00000	0.00000	0.00000	0.00000	0.00000
Zinc	213.857	0.00000	0.00000	0.00000	0.00000	0.00000

METALS
-11-
Interelement Correction Factors

Lab Code: GEL

GEL Job No: 10-2093

Contract: LANI.01004

Instrument: OPTIMA4

Effective Dates: 22-MAR-10

Interelement Correction Factors (apparent ppb analyte/ppm interferent)

Parmname	Wavelength	Strontium	Sulfur	Thallium	Tin	Titanium
Aluminum	396.153	0.00000	0.00000	0.00000	0.00000	0.00000
Antimony	206.836	0.00000	0.00000	0.00000	-1.82716	0.00000
Arsenic	188.979	0.00000	0.00000	0.00000	0.00000	0.00000
Barium	233.527	0.00000	0.00000	0.00000	0.00000	0.00000
Beryllium	313.107	0.00000	0.00000	0.00000	0.00000	0.00000
Boron	249.677	0.00000	0.00000	0.00000	0.00000	0.00000
Cadmium	226.502	0.00000	0.00000	0.00000	0.00000	0.00000
Chromium	267.716	0.00000	0.00000	0.00000	0.00000	0.00000
Cobalt	228.616	0.00000	0.00000	0.00000	0.00000	0.00000
Copper	324.752	0.00000	0.00000	0.00000	0.00000	0.00000
Lead	220.353	0.00000	0.00000	0.00000	0.00000	-1.32991
Magnesium	279.077	0.00000	0.00000	0.00000	0.00000	0.00000
Manganese	257.61	0.00000	0.00000	0.00000	0.00000	0.00000
Molybdenum	202.031	0.00000	0.00000	0.00000	0.00000	0.00000
Phosphorous	214.914	0.00000	0.00000	0.00000	-8.61809	0.00000
Potassium	766.49	0.00000	0.00000	0.00000	0.00000	0.00000
Selenium	196.026	0.00000	0.00000	0.00000	0.00000	0.00000
Silicon	251.611	0.00000	0.00000	0.00000	6.59640	0.00000
Silver	328.068	0.00000	0.00000	0.00000	0.00000	0.00000
Sodium	589.592	0.00000	0.00000	0.00000	0.00000	0.00000
Strontium	421.552	0.00000	0.00000	0.00000	0.00000	0.00000
Sulfur	181.975	0.00000	0.00000	0.00000	0.00000	0.00000
Thallium	190.801	0.00000	0.00000	0.00000	0.00000	-10.0432
Tin	189.927	0.00000	0.00000	0.00000	0.00000	-3.37234
Titanium	334.94	0.00000	0.00000	0.00000	0.00000	0.00000
Uranium	409.014	0.00000	0.00000	0.00000	0.00000	0.00000
Vanadium	292.402	0.00000	0.00000	0.00000	0.00000	0.92753
Zinc	213.857	0.00000	0.00000	0.00000	0.00000	-0.56798

METALS
-11-
Interelement Correction Factors

Lab Code: GEL

GEL Job No: 10-2093

Contract: LANL01004

Instrument: OPTIMA4

Effective Dates: 22-MAR-10

Interelement Correction Factors (apparent ppb analyte/ppm interferent)

Parmname	Wavelength	Uranium	Vanadium	Zinc
Aluminum	396.153	0.00000	0.00000	0.00000
Antimony	206.836	0.00000	-1.62578	0.00000
Arsenic	188.979	0.00000	0.00000	0.00000
Barium	233.527	0.00000	-0.63442	0.00000
Beryllium	313.107	-0.30229	0.00000	0.00000
Boron	249.677	0.00000	0.00000	0.00000
Cadmium	226.502	0.00000	0.00000	0.00000
Chromium	267.716	0.78601	-0.47146	0.00000
Cobalt	228.616	0.00000	0.00000	0.00000
Copper	324.752	-0.82619	0.00000	0.00000
Lead	220.353	0.74521	0.00000	0.00000
Magnesium	279.077	0.00000	0.00000	0.00000
Manganese	257.61	0.00000	0.00000	0.00000
Molybdenum	202.031	0.00000	-0.33953	0.00000
Phosphorous	214.914	0.00000	0.00000	0.00000
Potassium	766.49	0.00000	0.00000	0.00000
Selenium	196.026	-0.96499	0.00000	0.00000
Silicon	251.611	0.00000	0.00000	0.00000
Silver	328.068	-1.22996	-11.9401	0.00000
Sodium	589.592	0.00000	0.00000	0.00000
Strontium	421.552	0.00000	0.00000	0.00000
Sulfur	181.975	0.00000	0.00000	0.00000
Thallium	190.801	0.00000	-7.37871	0.00000
Tin	189.927	0.00000	0.00000	0.00000
Titanium	334.94	0.40930	0.00000	0.00000
Uranium	409.014	0.00000	-57.5852	0.00000
Vanadium	292.402	-0.67226	0.00000	0.00000
Zinc	213.857	0.00000	0.00000	0.00000

METALS
-12-
Linear Ranges

SDG NO. 10-2093

Contract: LANL01004

Lab Code: GEL

Instrument IDICPMS5

<u>Analyte</u>	<u>Integration Time (msec)</u>	<u>LDR</u>	<u>Units</u>	<u>Effective Date</u>
Aluminum	1	50000	ug/L	01-FEB-10
Antimony	1000	250	ug/L	01-FEB-10
Arsenic	1000	1000	ug/L	01-FEB-10
Barium	1000	1000	ug/L	01-FEB-10
Beryllium	1000	1000	ug/L	01-FEB-10
Cadmium	1000	1000	ug/L	01-FEB-10
Calcium	500	50000	ug/L	01-FEB-10
Chromium	1000	1000	ug/L	01-FEB-10
Cobalt	1000	1000	ug/L	01-FEB-10
Copper	1000	1000	ug/L	01-FEB-10
Iron	500	50000	ug/L	01-FEB-10
Lead	1000	5000	ug/L	01-FEB-10
Magnesium	1	50000	ug/L	01-FEB-10
Manganese	1000	1000	ug/L	01-FEB-10
Nickel	1000	1000	ug/L	01-FEB-10
Potassium	1	50000	ug/L	01-FEB-10
Selenium	1000	500	ug/L	01-FEB-10
Silver	1000	250	ug/L	01-FEB-10
Sodium	1	50000	ug/L	01-FEB-10
Thallium	1000	500	ug/L	01-FEB-10
Uranium	1000	5000	ug/L	01-FEB-10
Vanadium	1000	100	ug/L	01-FEB-10
Zinc	1000	2500	ug/L	01-FEB-10

METALS
-12-
Linear Ranges

SDG NO. 10-2093

Contract: LANL01004

Lab Code: GEL

Instrument ID OPTIMA4

<u>Analyte</u>	<u>Integration Time (sec)</u>	<u>LDR</u>	<u>Units</u>	<u>Effective Date</u>
Aluminum	20	500000	ug/L	01-FEB-10
Antimony	20	10000	ug/L	01-FEB-10
Arsenic	20	10000	ug/L	01-FEB-10
Barium	20	15000	ug/L	01-FEB-10
Beryllium	20	3000	ug/L	01-FEB-10
Cadmium	20	10000	ug/L	01-FEB-10
Calcium	20	500000	ug/L	01-FEB-10
Chromium	20	25000	ug/L	01-FEB-10
Cobalt	20	10000	ug/L	01-FEB-10
Copper	20	20000	ug/L	01-FEB-10
Iron	20	500000	ug/L	01-FEB-10
Lead	20	25000	ug/L	01-FEB-10
Magnesium	20	500000	ug/L	01-FEB-10
Manganese	20	10000	ug/L	01-FEB-10
Nickel	20	10000	ug/L	01-FEB-10
Potassium	20	300000	ug/L	01-FEB-10
Selenium	20	10000	ug/L	01-FEB-10
Silver	20	1000	ug/L	01-FEB-10
Sodium	20	500000	ug/L	01-FEB-10
Thallium	20	10000	ug/L	01-FEB-10
Uranium	20	15000	ug/L	01-FEB-10
Vanadium	20	10000	ug/L	01-FEB-10
Zinc	20	15000	ug/L	01-FEB-10

METALS
-12-
Linear Ranges

SDG NO. 10-2093

Contract: LANL01004

Lab Code: GEL

Instrument ID ICPMS4

<u>Analyte</u>	<u>Integration Time (msec)</u>	<u>LDR</u>	<u>Units</u>	<u>Effective Date</u>
Aluminum	1	50000	ug/L	01-FEB-10
Antimony	1000	250	ug/L	01-FEB-10
Arsenic	1000	1000	ug/L	01-FEB-10
Barium	1000	1000	ug/L	01-FEB-10
Beryllium	1000	1000	ug/L	01-FEB-10
Cadmium	1000	1000	ug/L	01-FEB-10
Calcium	500	50000	ug/L	01-FEB-10
Chromium	1000	1000	ug/L	01-FEB-10
Cobalt	1000	1000	ug/L	01-FEB-10
Copper	1000	1000	ug/L	01-FEB-10
Iron	500	50000	ug/L	01-FEB-10
Lead	1000	5000	ug/L	01-FEB-10
Magnesium	1	50000	ug/L	01-FEB-10
Manganese	1000	1000	ug/L	01-FEB-10
Nickel	1000	1000	ug/L	01-FEB-10
Potassium	1	50000	ug/L	01-FEB-10
Selenium	1000	500	ug/L	01-FEB-10
Silver	1000	250	ug/L	01-FEB-10
Sodium	1	50000	ug/L	01-FEB-10
Thallium	1000	500	ug/L	01-FEB-10
Uranium	1000	5000	ug/L	01-FEB-10
Vanadium	1000	100	ug/L	01-FEB-10
Zinc	1000	2500	ug/L	01-FEB-10

Raw Data

=====

Reprocessing Begun

Logged In Analyst: optima4

Technique: ICP Continuous

Results Data Set (original): 032910B

Results Library (original): C:\pe\optima4\Results\Results.mdb

Results Data Set (reprocessed): 032910C

Results Library (reprocessed): C:\pe\optima4\Results\Results.mdb

=====

Method Loaded

Method Name: Gen Eng fast_new Si

Method Last Saved: 3/29/2010 19:12:39

IEC File: 031810.iec

MSF File:

Method Description:

Analyte	Calibration Equation	Processing	View	Internal Standard	IEC
Ag 328.068	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Al 396.153Radial	Lin Thru 0	Peak Area	Radial	Sc RADIAL	Yes
As 188.979	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
B 249.677	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Ba 233.527	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Be 313.107	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Ca 317.933Radial	Lin Thru 0	Peak Area	Radial	Sc RADIAL	No
Cd 226.502	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Co 228.616	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Cr 267.716	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Cu 324.752	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Fe 238.204 Radial	Lin Thru 0	Peak Area	Radial	Sc RADIAL	No
K 766.490 Radial	Lin Thru 0	Peak Area	Radial	Sc RADIAL	Yes
Mg 279.077 IEC	Lin Thru 0	Peak Area	Radial	Sc RADIAL	Yes
Mn 257.610	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Mo 202.031	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Na 589.592 Radial	Lin Thru 0	Peak Area	Radial	Sc RADIAL	Yes
Ni 231.604	Lin Thru 0	Peak Area	Axial	Sc 361.383	No
P 214.914	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Pb 220.353	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
S 181.975 Axial	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Sb 206.836	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Sc 361.383	Lin Thru 0	Peak Area	Axial	n/a	n/a
Sc RADIAL	Lin, Calc Int	Peak Area	Radial	n/a	n/a
Se 196.026	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
SiO2	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Si 251.611	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Sn 189.927	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Sr 421.552	Lin Thru 0	Peak Area	Radial	Sc RADIAL	Yes
Ti 334.940	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Tl 190.801	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
U 409.014	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
V 292.402	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Y 371.029	Lin, Calc Int	Peak Area	Axial	n/a	n/a
Zn 213.857	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes

=====

Sequence No.: 1

Autosampler Location: 8

Sample ID: S0

Date Collected: 3/29/2010 18:25:17

Analyst:

Data Type: Reprocessed on 3/29/2010 19:14:31

Logged In Analyst (Original) : optima4

Initial Sample Wt:

Initial Sample Vol:

Dilution:

Sample Prep Vol:

Replicate Data: S0

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Analysis Time
1	Sc 361.383	1675486.4	1675486.4	100.16 %	18:27:09
1	Sc RADIAL	146509.4	146509.4	101 %	18:25:47
1	Y 371.029	1022720.1	1022720.1	100.01 %	18:27:09
1	Ag 328.068†	2983.2	2978.4	[0.00] µg/L	18:27:11
1	Al 396.153Radial†	-35.1	-35.0	[0.00] µg/L	18:26:07
1	As 188.979†	-19.2	-19.2	[0.00] µg/L	18:27:31

1	B 249.677†	3447.9	3442.3	[0.00]	µg/L	18:27:11
1	Ba 233.527†	-170.9	-170.6	[0.00]	µg/L	18:27:31
1	Be 313.107†	-760.2	-759.0	[0.00]	µg/L	18:27:11
1	Ca 317.933Radial†	609.6	606.5	[0.00]	µg/L	18:26:07
1	Cd 226.502†	-94.3	-94.2	[0.00]	µg/L	18:27:31
1	Co 228.616†	-177.2	-176.9	[0.00]	µg/L	18:27:31
1	Cr 267.716†	191.1	190.8	[0.00]	µg/L	18:27:31
1	Cu 324.752†	2447.0	2443.1	[0.00]	µg/L	18:27:11
1	Fe 238.204 Radial†	120.7	120.1	[0.00]	µg/L	18:26:07
1	K 766.490 Radial†	1409.9	1402.7	[0.00]	µg/L	18:25:47
1	Mg 279.077 IEC†	182.4	181.4	[0.00]	µg/L	18:26:07
1	Mn 257.610†	83.5	83.4	[0.00]	µg/L	18:27:31
1	Mo 202.031†	-61.5	-61.4	[0.00]	µg/L	18:27:31
1	Na 589.592 Radial†	1727.7	1718.8	[0.00]	µg/L	18:25:47
1	Ni 231.604†	-12.7	-12.7	[0.00]	µg/L	18:27:31
1	P 214.914†	74.6	74.5	[0.00]	µg/L	18:27:31
1	Pb 220.353†	124.0	123.8	[0.00]	µg/L	18:27:31
1	S 181.975 Axial†	92.2	92.1	[0.00]	µg/L	18:27:31
1	Sb 206.836†	94.8	94.7	[0.00]	µg/L	18:27:31
1	Se 196.026†	10.9	10.9	[0.00]	µg/L	18:27:31
1	SiO2†	1567.1	1564.5	[0.00]	µg/L	18:27:31
1	Si 251.611†	683.3	682.2	[0.00]	µg/L	18:27:11
1	Sn 189.927†	-0.3	-0.3	[0.00]	µg/L	18:27:31
1	Sr 421.552†	-242.7	-241.5	[0.00]	µg/L	18:25:47
1	Ti 334.940†	661.0	659.9	[0.00]	µg/L	18:27:11
1	Tl 190.801†	-125.7	-125.5	[0.00]	µg/L	18:27:31
1	U 409.014†	-452.8	-452.0	[0.00]	µg/L	18:27:11
1	V 292.402†	515.3	514.5	[0.00]	µg/L	18:27:11
1	Zn 213.857†	458.0	457.2	[0.00]	µg/L	18:27:31
2	Sc 361.383	1673882.1	1673882.1	100.07	%	18:27:33
2	Sc RADIAL	143614.2	143614.2	98.5	%	18:26:09
2	Y 371.029	1022767.5	1022767.5	100.02	%	18:27:33
2	Ag 328.068†	3053.8	3051.7	[0.00]	µg/L	18:27:35
2	Al 396.153Radial†	-38.9	-39.5	[0.00]	µg/L	18:26:29
2	As 188.979†	-15.1	-15.1	[0.00]	µg/L	18:27:55
2	B 249.677†	3293.2	3291.1	[0.00]	µg/L	18:27:35
2	Ba 233.527†	-175.9	-175.8	[0.00]	µg/L	18:27:55
2	Be 313.107†	-530.4	-530.1	[0.00]	µg/L	18:27:35
2	Ca 317.933Radial†	602.3	611.3	[0.00]	µg/L	18:26:29
2	Cd 226.502†	-94.9	-94.9	[0.00]	µg/L	18:27:55
2	Co 228.616†	-169.1	-169.0	[0.00]	µg/L	18:27:55
2	Cr 267.716†	157.6	157.5	[0.00]	µg/L	18:27:55
2	Cu 324.752†	2326.2	2324.7	[0.00]	µg/L	18:27:35
2	Fe 238.204 Radial†	112.7	114.4	[0.00]	µg/L	18:26:29
2	K 766.490 Radial†	1475.1	1497.1	[0.00]	µg/L	18:26:09
2	Mg 279.077 IEC†	191.8	194.7	[0.00]	µg/L	18:26:29
2	Mn 257.610†	69.4	69.3	[0.00]	µg/L	18:27:55
2	Mo 202.031†	-55.1	-55.0	[0.00]	µg/L	18:27:55
2	Na 589.592 Radial†	1691.1	1716.3	[0.00]	µg/L	18:26:09
2	Ni 231.604†	-51.5	-51.5	[0.00]	µg/L	18:27:55
2	P 214.914†	99.0	98.9	[0.00]	µg/L	18:27:55
2	Pb 220.353†	108.5	108.4	[0.00]	µg/L	18:27:55
2	S 181.975 Axial†	90.3	90.2	[0.00]	µg/L	18:27:55
2	Sb 206.836†	81.0	81.0	[0.00]	µg/L	18:27:55
2	Se 196.026†	15.5	15.5	[0.00]	µg/L	18:27:55
2	SiO2†	1541.6	1540.6	[0.00]	µg/L	18:27:55
2	Si 251.611†	721.8	721.4	[0.00]	µg/L	18:27:35
2	Sn 189.927†	7.0	7.0	[0.00]	µg/L	18:27:55
2	Sr 421.552†	-264.2	-268.1	[0.00]	µg/L	18:26:09
2	Ti 334.940†	533.5	533.1	[0.00]	µg/L	18:27:35
2	Tl 190.801†	-121.5	-121.4	[0.00]	µg/L	18:27:55
2	U 409.014†	-565.6	-565.2	[0.00]	µg/L	18:27:35
2	V 292.402†	425.8	425.5	[0.00]	µg/L	18:27:35
2	Zn 213.857†	466.7	466.4	[0.00]	µg/L	18:27:55
3	Sc 361.383	1668955.0	1668955.0	99.772	%	18:27:57
3	Sc RADIAL	147139.1	147139.1	101	%	18:26:31
3	Y 371.029	1022257.2	1022257.2	99.968	%	18:27:57
3	Ag 328.068†	2864.4	2871.0	[0.00]	µg/L	18:27:59
3	Al 396.153Radial†	-21.4	-21.2	[0.00]	µg/L	18:26:51
3	As 188.979†	-8.4	-8.4	[0.00]	µg/L	18:28:20
3	B 249.677†	3326.1	3333.7	[0.00]	µg/L	18:27:59

3	Ba 233.527†	-178.4	-178.8	[0.00]	µg/L	18:28:20
3	Be 313.107†	-689.7	-691.3	[0.00]	µg/L	18:27:59
3	Ca 317.933 Radial†	636.8	630.8	[0.00]	µg/L	18:26:51
3	Cd 226.502†	-94.0	-94.2	[0.00]	µg/L	18:28:20
3	Co 228.616†	-183.5	-183.9	[0.00]	µg/L	18:28:20
3	Cr 267.716†	132.1	132.4	[0.00]	µg/L	18:28:20
3	Cu 324.752†	2501.2	2506.9	[0.00]	µg/L	18:27:59
3	Fe 238.204 Radial†	106.3	105.3	[0.00]	µg/L	18:26:51
3	K 766.490 Radial†	1479.1	1465.2	[0.00]	µg/L	18:26:31
3	Mg 279.077 IEC†	185.6	183.9	[0.00]	µg/L	18:26:51
3	Mn 257.610†	87.1	87.3	[0.00]	µg/L	18:28:20
3	Mo 202.031†	-49.1	-49.2	[0.00]	µg/L	18:28:20
3	Na 589.592 Radial†	1664.8	1649.1	[0.00]	µg/L	18:26:31
3	Ni 231.604†	-58.4	-58.5	[0.00]	µg/L	18:28:20
3	P 214.914†	65.2	65.3	[0.00]	µg/L	18:28:20
3	Pb 220.353†	104.9	105.1	[0.00]	µg/L	18:28:20
3	S 181.975 Axial†	101.9	102.2	[0.00]	µg/L	18:28:20
3	Sb 206.836†	84.1	84.3	[0.00]	µg/L	18:28:20
3	Se 196.026†	6.3	6.3	[0.00]	µg/L	18:28:20
3	SiO2†	1609.7	1613.4	[0.00]	µg/L	18:28:20
3	Si 251.611†	624.2	625.6	[0.00]	µg/L	18:27:59
3	Sn 189.927†	-0.6	-0.6	[0.00]	µg/L	18:28:20
3	Sr 421.552†	-327.4	-324.4	[0.00]	µg/L	18:26:31
3	Ti 334.940†	714.3	716.0	[0.00]	µg/L	18:27:59
3	Tl 190.801†	-113.7	-113.9	[0.00]	µg/L	18:28:20
3	U 409.014†	-419.1	-420.1	[0.00]	µg/L	18:27:59
3	V 292.402†	354.6	355.5	[0.00]	µg/L	18:27:59
3	Zn 213.857†	468.5	469.6	[0.00]	µg/L	18:28:20

Mean Data: S0

Analyte	Mean Corrected Intensity	Std.Dev.	RSD	Calib Conc.	Units
Sc 361.383	1672774.5	3403.67	0.20%	100.00	%
Sc RADIAL	145754.2	1879.88	1.29%	100	%
Y 371.029	1022581.6	281.95	0.03%	100.00	%
Ag 328.068†	2967.0	90.92	3.06%	[0.00]	µg/L
Al 396.153 Radial†	-31.9	9.54	29.92%	[0.00]	µg/L
As 188.979†	-14.2	5.41	37.98%	[0.00]	µg/L
B 249.677†	3355.7	78.00	2.32%	[0.00]	µg/L
Ba 233.527†	-175.1	4.13	2.36%	[0.00]	µg/L
Be 313.107†	-660.1	117.60	17.82%	[0.00]	µg/L
Ca 317.933 Radial†	616.2	12.87	2.09%	[0.00]	µg/L
Cd 226.502†	-94.4	0.38	0.41%	[0.00]	µg/L
Co 228.616†	-176.6	7.48	4.23%	[0.00]	µg/L
Cr 267.716†	160.2	29.32	18.30%	[0.00]	µg/L
Cu 324.752†	2424.9	92.45	3.81%	[0.00]	µg/L
Fe 238.204 Radial†	113.3	7.45	6.58%	[0.00]	µg/L
K 766.490 Radial†	1455.0	48.06	3.30%	[0.00]	µg/L
Mg 279.077 IEC†	186.7	7.04	3.77%	[0.00]	µg/L
Mn 257.610†	80.0	9.46	11.83%	[0.00]	µg/L
Mo 202.031†	-55.2	6.06	10.98%	[0.00]	µg/L
Na 589.592 Radial†	1694.7	39.52	2.33%	[0.00]	µg/L
Ni 231.604†	-40.9	24.66	60.28%	[0.00]	µg/L
P 214.914†	79.6	17.37	21.83%	[0.00]	µg/L
Pb 220.353†	112.4	9.96	8.86%	[0.00]	µg/L
S 181.975 Axial†	94.8	6.43	6.78%	[0.00]	µg/L
Sb 206.836†	86.6	7.13	8.23%	[0.00]	µg/L
Se 196.026†	10.9	4.59	42.08%	[0.00]	µg/L
SiO2†	1572.9	37.13	2.36%	[0.00]	µg/L
Si 251.611†	676.4	48.15	7.12%	[0.00]	µg/L
Sn 189.927†	2.0	4.32	214.20%	[0.00]	µg/L
Sr 421.552†	-278.0	42.30	15.22%	[0.00]	µg/L
Ti 334.940†	636.3	93.67	14.72%	[0.00]	µg/L
Tl 190.801†	-120.3	5.87	4.88%	[0.00]	µg/L
U 409.014†	-479.1	76.26	15.92%	[0.00]	µg/L
V 292.402†	431.8	79.70	18.46%	[0.00]	µg/L
Zn 213.857†	464.4	6.40	1.38%	[0.00]	µg/L

Sequence No.: 2
 Sample ID: S0.1
 Analyst:
 Logged In Analyst (Original) : optima4
 Initial Sample Wt:
 Dilution:

Autosampler Location: 2
 Date Collected: 3/29/2010 18:28:28
 Data Type: Reprocessed on 3/29/2010 19:14:33
 Initial Sample Vol:
 Sample Prep Vol:

Replicate Data: S0.1

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Analysis Time
1	Sc 361.383	1661946.1	1661946.1	99.353 %	18:29:20
1	Sc RADIAL	142262.8	142262.8	97.6 %	18:28:58
1	Y 371.029	1013636.7	1013636.7	99.125 %	18:29:20
1	Ag 328.068†	28004.5	25219.9	[100] µg/L	18:29:22
1	As 188.979†	214.7	230.4	[100] µg/L	18:29:42
1	B 249.677†	9080.8	5784.2	[100] µg/L	18:29:22
1	Ba 233.527†	21988.9	22307.2	[100] µg/L	18:29:22
1	Be 313.107†	303759.0	306398.2	[100] µg/L	18:29:20
1	Cd 226.502†	14418.1	14606.5	[100] µg/L	18:29:22
1	Co 228.616†	7233.5	7457.2	[100] µg/L	18:29:42
1	Cr 267.716†	11824.2	11741.0	[100] µg/L	18:29:22
1	Cu 324.752†	25515.5	23256.9	[100] µg/L	18:29:22
1	K 766.490 Radial†	3700.4	2336.2	[1000] µg/L	18:28:58
1	Mn 257.610†	75396.6	75807.8	[100] µg/L	18:29:22
1	Mo 202.031†	3080.8	3156.1	[100] µg/L	18:29:42
1	Ni 231.604†	8001.7	8094.7	[100] µg/L	18:29:22
1	P 214.914†	2111.9	2046.0	[500] µg/L	18:29:42
1	Pb 220.353†	1769.2	1668.3	[100] µg/L	18:29:42
1	S 181.975 Axial†	329.8	237.2	[200] µg/L	18:29:42
1	Sb 206.836†	823.1	741.9	[100] µg/L	18:29:42
1	Se 196.026†	270.2	261.0	[100] µg/L	18:29:42
1	SiO2†	11219.8	9720.0	[1069.5] µg/L	18:29:22
1	Si 251.611†	30808.9	30333.3	[500] µg/L	18:29:22
1	Sn 189.927†	1389.8	1396.8	[100] µg/L	18:29:42
1	Sr 421.552†	43261.6	44601.3	[100] µg/L	18:28:58
1	Ti 334.940†	97625.2	97625.0	[100] µg/L	18:29:22
1	Tl 190.801†	629.9	754.3	[100] µg/L	18:29:42
1	U 409.014†	1288.2	1775.7	[100] µg/L	18:29:22
1	V 292.402†	18219.3	17906.2	[100] µg/L	18:29:22
1	Zn 213.857†	16338.0	15980.0	[100] µg/L	18:29:22
2	Sc 361.383	1666549.8	1666549.8	99.628 %	18:29:44
2	Sc RADIAL	146980.5	146980.5	101 %	18:29:00
2	Y 371.029	1017353.0	1017353.0	99.489 %	18:29:44
2	Ag 328.068†	28245.8	25384.2	[100] µg/L	18:29:47
2	As 188.979†	216.8	231.9	[100] µg/L	18:30:07
2	B 249.677†	9095.6	5773.9	[100] µg/L	18:29:47
2	Ba 233.527†	22220.1	22478.2	[100] µg/L	18:29:47
2	Be 313.107†	301592.1	303378.7	[100] µg/L	18:29:44
2	Cd 226.502†	14444.4	14592.7	[100] µg/L	18:29:47
2	Co 228.616†	7194.5	7397.9	[100] µg/L	18:30:07
2	Cr 267.716†	11989.4	11874.0	[100] µg/L	18:29:47
2	Cu 324.752†	25454.5	23124.7	[100] µg/L	18:29:47
2	K 766.490 Radial†	3828.6	2341.7	[1000] µg/L	18:29:00
2	Mn 257.610†	75955.3	76159.0	[100] µg/L	18:29:47
2	Mo 202.031†	3072.9	3139.6	[100] µg/L	18:30:07
2	Ni 231.604†	7945.1	8015.7	[100] µg/L	18:29:47
2	P 214.914†	2095.0	2023.3	[500] µg/L	18:30:07
2	Pb 220.353†	1806.4	1700.7	[100] µg/L	18:30:07
2	S 181.975 Axial†	328.8	235.2	[200] µg/L	18:30:07
2	Sb 206.836†	831.1	747.6	[100] µg/L	18:30:07
2	Se 196.026†	268.7	258.8	[100] µg/L	18:30:07
2	SiO2†	11380.9	9850.6	[1069.5] µg/L	18:29:47
2	Si 251.611†	30908.3	30347.4	[500] µg/L	18:29:47
2	Sn 189.927†	1386.9	1390.0	[100] µg/L	18:30:07
2	Sr 421.552†	43897.3	43809.0	[100] µg/L	18:29:00
2	Ti 334.940†	97949.2	97678.7	[100] µg/L	18:29:47
2	Tl 190.801†	629.9	752.6	[100] µg/L	18:30:07
2	U 409.014†	1127.3	1610.7	[100] µg/L	18:29:47

2	V 292.402†	18287.8	17924.3	[100] µg/L	18:29:47
2	Zn 213.857†	16478.9	16076.1	[100] µg/L	18:29:47
3	Sc 361.383	1678711.7	1678711.7	100.35 %	18:30:09
3	Sc RADIAL	143945.0	143945.0	98.8 %	18:29:02
3	Y 371.029	1024374.9	1024374.9	100.18 %	18:30:09
3	Ag 328.068†	27960.9	24894.9	[100] µg/L	18:30:11
3	As 188.979†	221.3	234.7	[100] µg/L	18:30:31
3	B 249.677†	9088.4	5700.5	[100] µg/L	18:30:11
3	Ba 233.527†	21982.2	22079.5	[100] µg/L	18:30:11
3	Be 313.107†	305374.6	304954.6	[100] µg/L	18:30:09
3	Cd 226.502†	14449.3	14492.6	[100] µg/L	18:30:11
3	Co 228.616†	7225.7	7376.7	[100] µg/L	18:30:31
3	Cr 267.716†	11783.4	11581.4	[100] µg/L	18:30:11
3	Cu 324.752†	25635.6	23120.1	[100] µg/L	18:30:11
3	K 766.490 Radial†	3785.9	2378.5	[1000] µg/L	18:29:02
3	Mn 257.610†	75567.2	75219.9	[100] µg/L	18:30:11
3	Mo 202.031†	3088.5	3132.8	[100] µg/L	18:30:31
3	Ni 231.604†	7999.7	8012.3	[100] µg/L	18:30:11
3	P 214.914†	2091.9	2004.9	[500] µg/L	18:30:31
3	Pb 220.353†	1784.3	1665.6	[100] µg/L	18:30:31
3	S 181.975 Axial†	327.0	231.0	[200] µg/L	18:30:31
3	Sb 206.836†	817.3	727.8	[100] µg/L	18:30:31
3	Se 196.026†	251.7	239.9	[100] µg/L	18:30:31
3	SiO2†	11327.9	9715.0	[1069.5] µg/L	18:30:11
3	Si 251.611†	30819.3	30033.9	[500] µg/L	18:30:11
3	Sn 189.927†	1401.4	1394.4	[100] µg/L	18:30:31
3	Sr 421.552†	43851.5	44680.7	[100] µg/L	18:29:02
3	Ti 334.940†	97740.3	96758.3	[100] µg/L	18:30:11
3	Tl 190.801†	620.5	738.6	[100] µg/L	18:30:31
3	U 409.014†	1269.9	1744.5	[100] µg/L	18:30:11
3	V 292.402†	18059.5	17563.8	[100] µg/L	18:30:11
3	Zn 213.857†	16510.7	15987.9	[100] µg/L	18:30:11

Mean Data: S0.1

Analyte	Mean Corrected Intensity	Std.Dev.	RSD	Calib Conc. Units
Sc 361.383	1669069.2	8662.09	0.52%	99.778 %
Sc RADIAL	144396.1	2390.99	1.66%	99.1 %
Y 371.029	1018454.9	5453.26	0.54%	99.596 %
Ag 328.068†	25166.4	249.02	0.99%	[100] µg/L
As 188.979†	232.3	2.20	0.95%	[100] µg/L
B 249.677†	5752.9	45.63	0.79%	[100] µg/L
Ba 233.527†	22288.3	200.02	0.90%	[100] µg/L
Be 313.107†	304910.5	1510.27	0.50%	[100] µg/L
Cd 226.502†	14563.9	62.13	0.43%	[100] µg/L
Co 228.616†	7410.6	41.70	0.56%	[100] µg/L
Cr 267.716†	11732.1	146.47	1.25%	[100] µg/L
Cu 324.752†	23167.2	77.70	0.34%	[100] µg/L
K 766.490 Radial†	2352.1	22.98	0.98%	[1000] µg/L
Mn 257.610†	75728.9	474.50	0.63%	[100] µg/L
Mo 202.031†	3142.8	11.99	0.38%	[100] µg/L
Ni 231.604†	8040.9	46.63	0.58%	[100] µg/L
P 214.914†	2024.7	20.61	1.02%	[500] µg/L
Pb 220.353†	1678.2	19.56	1.17%	[100] µg/L
S 181.975 Axial†	234.4	3.15	1.34%	[200] µg/L
Sb 206.836†	739.1	10.21	1.38%	[100] µg/L
Se 196.026†	253.2	11.62	4.59%	[100] µg/L
SiO2†	9761.9	76.87	0.79%	[1069.5] µg/L
Si 251.611†	30238.2	177.02	0.59%	[500] µg/L
Sn 189.927†	1393.8	3.45	0.25%	[100] µg/L
Sr 421.552†	44363.6	481.98	1.09%	[100] µg/L
Ti 334.940†	97354.0	516.57	0.53%	[100] µg/L
Tl 190.801†	748.5	8.62	1.15%	[100] µg/L
U 409.014†	1710.3	87.69	5.13%	[100] µg/L
V 292.402†	17798.1	203.14	1.14%	[100] µg/L
Zn 213.857†	16014.7	53.32	0.33%	[100] µg/L

Sequence No.: 3
 Sample ID: S0.5
 Analyst:
 Logged In Analyst (Original) : optima4
 Initial Sample Wt:
 Dilution:

Autosampler Location: 3
 Date Collected: 3/29/2010 18:30:39
 Data Type: Reprocessed on 3/29/2010 19:14:34

Initial Sample Vol:
 Sample Prep Vol:

Replicate Data: S0.5

Repl#	Analyte	Net Intensity	Corrected Intensity	Conc. Units	Analysis Time
1	Sc 361.383	1666330.4	1666330.4	99.615 %	18:31:37
1	Sc RADIAL	146255.9	146255.9	100 %	18:31:10
1	Y 371.029	1010770.4	1010770.4	98.845 %	18:31:37
1	Ag 328.068†	124810.0	122325.6	[500] µg/L	18:31:37
1	Al 396.153Radial†	22730.9	22684.8	[5000] µg/L	18:31:10
1	As 188.979†	1130.3	1148.9	[500] µg/L	18:31:57
1	B 249.677†	32443.2	29213.0	[500] µg/L	18:31:37
1	Ba 233.527†	108021.9	108614.7	[500] µg/L	18:31:37
1	Be 313.107†	1516563.3	1523088.3	[500] µg/L	18:31:37
1	Ca 317.933Radial†	86179.3	85267.4	[5000] µg/L	18:31:10
1	Cd 226.502†	71219.1	71589.0	[500] µg/L	18:31:37
1	Co 228.616†	35394.0	35707.4	[500] µg/L	18:31:57
1	Cr 267.716†	57615.1	57677.6	[500] µg/L	18:31:37
1	Cu 324.752†	116290.7	114315.5	[500] µg/L	18:31:37
1	K 766.490 Radial†	13629.8	12128.1	[5000] µg/L	18:31:10
1	Mg 279.077 IEC†	12468.2	12238.8	[5000] µg/L	18:31:10
1	Mn 257.610†	362696.8	364019.5	[500] µg/L	18:31:37
1	Mo 202.031†	15371.1	15485.8	[500] µg/L	18:31:57
1	Ni 231.604†	38767.1	38957.9	[500] µg/L	18:31:37
1	P 214.914†	10122.4	10082.0	[2500] µg/L	18:31:57
1	Pb 220.353†	8161.6	8080.8	[500] µg/L	18:31:57
1	S 181.975 Axial†	1278.6	1188.7	[1000] µg/L	18:31:57
1	Sb 206.836†	3687.2	3614.8	[500] µg/L	18:31:57
1	Se 196.026†	1225.0	1218.8	[500] µg/L	18:31:57
1	SiO2†	49926.4	48546.6	[5347.5] µg/L	18:31:37
1	Si 251.611†	150511.0	150416.7	[2500] µg/L	18:31:37
1	Sn 189.927†	6828.0	6852.4	[500] µg/L	18:31:57
1	Sr 421.552†	212817.9	212365.9	[500] µg/L	18:31:08
1	Ti 334.940†	484276.9	485513.3	[500] µg/L	18:31:37
1	Tl 190.801†	3503.2	3637.1	[500] µg/L	18:31:57
1	U 409.014†	6910.1	7415.9	[500] µg/L	18:31:37
1	V 292.402†	89155.4	89068.4	[500] µg/L	18:31:37
1	Zn 213.857†	79249.5	79091.5	[500] µg/L	18:31:37
2	Sc 361.383	1656377.5	1656377.5	99.020 %	18:32:00
2	Sc RADIAL	143364.9	143364.9	98.4 %	18:31:14
2	Y 371.029	1005040.5	1005040.5	98.285 %	18:32:00
2	Ag 328.068†	123893.4	122152.8	[500] µg/L	18:32:00
2	Al 396.153Radial†	22411.8	22817.2	[5000] µg/L	18:31:14
2	As 188.979†	1160.9	1186.7	[500] µg/L	18:32:21
2	B 249.677†	32166.0	29128.7	[500] µg/L	18:32:00
2	Ba 233.527†	106821.0	108053.5	[500] µg/L	18:32:00
2	Be 313.107†	1497872.7	1513360.7	[500] µg/L	18:32:00
2	Ca 317.933Radial†	83955.9	84739.0	[5000] µg/L	18:31:14
2	Cd 226.502†	70376.7	71167.8	[500] µg/L	18:32:00
2	Co 228.616†	35865.0	36396.7	[500] µg/L	18:32:21
2	Cr 267.716†	57094.1	57499.1	[500] µg/L	18:32:00
2	Cu 324.752†	115218.7	113934.4	[500] µg/L	18:32:00
2	K 766.490 Radial†	13146.4	11910.5	[5000] µg/L	18:31:14
2	Mg 279.077 IEC†	12081.5	12096.2	[5000] µg/L	18:31:14
2	Mn 257.610†	359096.8	362571.6	[500] µg/L	18:32:00
2	Mo 202.031†	15556.5	15765.7	[500] µg/L	18:32:21
2	Ni 231.604†	38151.2	38569.7	[500] µg/L	18:32:00
2	P 214.914†	10250.6	10272.5	[2500] µg/L	18:32:21
2	Pb 220.353†	8247.6	8216.9	[500] µg/L	18:32:21
2	S 181.975 Axial†	1295.5	1213.5	[1000] µg/L	18:32:21
2	Sb 206.836†	3729.7	3679.9	[500] µg/L	18:32:21
2	Se 196.026†	1259.6	1261.2	[500] µg/L	18:32:21
2	SiO2†	49488.1	48405.1	[5347.5] µg/L	18:32:00

2	Si 251.611†	149066.4	149865.6	[2500] µg/L	18:32:00
2	Sn 189.927†	6928.0	6994.5	[500] µg/L	18:32:21
2	Sr 421.552†	210571.1	214358.5	[500] µg/L	18:31:12
2	Ti 334.940†	480119.5	484236.0	[500] µg/L	18:32:00
2	Tl 190.801†	3520.8	3676.0	[500] µg/L	18:32:21
2	U 409.014†	6871.4	7418.6	[500] µg/L	18:32:00
2	V 292.402†	88228.0	88669.5	[500] µg/L	18:32:00
2	Zn 213.857†	78116.6	78425.5	[500] µg/L	18:32:00
3	Sc 361.383	1678591.9	1678591.9	100.35 %	18:32:24
3	Sc RADIAL	148088.8	148088.8	102 %	18:31:18
3	Y 371.029	1018746.9	1018746.9	99.625 %	18:32:24
3	Ag 328.068†	125886.3	122483.0	[500] µg/L	18:32:24
3	Al 396.153Radial†	22914.6	22585.2	[5000] µg/L	18:31:18
3	As 188.979†	1161.2	1171.4	[500] µg/L	18:32:44
3	B 249.677†	32821.8	29352.3	[500] µg/L	18:32:24
3	Ba 233.527†	108685.7	108484.1	[500] µg/L	18:32:24
3	Be 313.107†	1528160.6	1523524.6	[500] µg/L	18:32:24
3	Ca 317.933Radial†	86630.7	84648.8	[5000] µg/L	18:31:18
3	Cd 226.502†	72351.9	72195.6	[500] µg/L	18:32:24
3	Co 228.616†	36165.4	36216.7	[500] µg/L	18:32:44
3	Cr 267.716†	58224.7	57862.7	[500] µg/L	18:32:24
3	Cu 324.752†	117068.1	114237.5	[500] µg/L	18:32:24
3	K 766.490 Radial†	13544.3	11875.7	[5000] µg/L	18:31:18
3	Mg 279.077 IEC†	12711.0	12323.9	[5000] µg/L	18:31:18
3	Mn 257.610†	365977.4	364629.0	[500] µg/L	18:32:24
3	Mo 202.031†	15658.0	15658.9	[500] µg/L	18:32:44
3	Ni 231.604†	38949.9	38855.9	[500] µg/L	18:32:24
3	P 214.914†	10378.5	10262.9	[2500] µg/L	18:32:44
3	Pb 220.353†	8301.3	8160.1	[500] µg/L	18:32:44
3	S 181.975 Axial†	1298.3	1199.0	[1000] µg/L	18:32:44
3	Sb 206.836†	3757.3	3657.7	[500] µg/L	18:32:44
3	Se 196.026†	1268.4	1253.0	[500] µg/L	18:32:44
3	SiO2†	50453.3	48705.6	[5347.5] µg/L	18:32:24
3	Si 251.611†	151847.8	150645.2	[2500] µg/L	18:32:24
3	Sn 189.927†	6976.6	6950.4	[500] µg/L	18:32:44
3	Sr 421.552†	212729.2	209653.5	[500] µg/L	18:31:16
3	Ti 334.940†	487904.2	485577.0	[500] µg/L	18:32:24
3	Tl 190.801†	3573.5	3681.5	[500] µg/L	18:32:44
3	U 409.014†	7083.7	7538.2	[500] µg/L	18:32:24
3	V 292.402†	89928.1	89184.6	[500] µg/L	18:32:24
3	Zn 213.857†	79862.3	79121.1	[500] µg/L	18:32:24

Mean Data: S0.5

Analyte	Mean Corrected Intensity	Std.Dev.	RSD	Calib Conc. Units
Sc 361.383	1667099.9	11127.18	0.67%	99.661 %
Sc RADIAL	145903.2	2381.65	1.63%	100 %
Y 371.029	1011519.3	6883.81	0.68%	98.918 %
Ag 328.068†	122320.5	165.15	0.14%	[500] µg/L
Al 396.153Radial†	22695.7	116.36	0.51%	[5000] µg/L
As 188.979†	1169.0	19.01	1.63%	[500] µg/L
B 249.677†	29231.4	112.94	0.39%	[500] µg/L
Ba 233.527†	108384.1	293.66	0.27%	[500] µg/L
Be 313.107†	1519991.2	5746.30	0.38%	[500] µg/L
Ca 317.933Radial†	84885.1	334.21	0.39%	[5000] µg/L
Cd 226.502†	71650.8	516.66	0.72%	[500] µg/L
Co 228.616†	36106.9	357.49	0.99%	[500] µg/L
Cr 267.716†	57679.8	181.81	0.32%	[500] µg/L
Cu 324.752†	114162.5	201.35	0.18%	[500] µg/L
K 766.490 Radial†	11971.4	136.75	1.14%	[5000] µg/L
Mg 279.077 IEC†	12219.6	115.04	0.94%	[5000] µg/L
Mn 257.610†	363740.0	1056.77	0.29%	[500] µg/L
Mo 202.031†	15636.8	141.25	0.90%	[500] µg/L
Ni 231.604†	38794.5	201.22	0.52%	[500] µg/L
P 214.914†	10205.8	107.31	1.05%	[2500] µg/L
Pb 220.353†	8152.6	68.35	0.84%	[500] µg/L
S 181.975 Axial†	1200.4	12.45	1.04%	[1000] µg/L
Sb 206.836†	3650.8	33.08	0.91%	[500] µg/L
Se 196.026†	1244.3	22.47	1.81%	[500] µg/L
SiO2†	48552.4	150.29	0.31%	[5347.5] µg/L

Si 251.611†	150309.2	400.75	0.27%	[2500]	µg/L
Sn 189.927†	6932.4	72.76	1.05%	[500]	µg/L
Sr 421.552†	212126.0	2361.66	1.11%	[500]	µg/L
Ti 334.940†	485108.8	756.53	0.16%	[500]	µg/L
Tl 190.801†	3664.9	24.20	0.66%	[500]	µg/L
U 409.014†	7457.6	69.86	0.94%	[500]	µg/L
V 292.402†	88974.2	270.15	0.30%	[500]	µg/L
Zn 213.857†	78879.4	393.36	0.50%	[500]	µg/L

Sequence No.: 4
 Sample ID: SCAL
 Analyst:
 Logged In Analyst (Original) : optima4
 Initial Sample Wt:
 Dilution:

Autosampler Location: 4
 Date Collected: 3/29/2010 18:32:52
 Data Type: Reprocessed on 3/29/2010 19:14:34

Initial Sample Vol:
 Sample Prep Vol:

Replicate Data: SCAL

Repl#	Analyte	Net Intensity	Corrected Intensity	Conc. Units	Calib.	Analysis Time
1	Sc 361.383	1695274.3	1695274.3	101.35 %		18:33:51
1	Sc RADIAL	148093.8	148093.8	102 %		18:33:23
1	Y 371.029	1024428.2	1024428.2	100.18 %		18:33:51
1	Ag 328.068†	253437.3	247106.6	[1000] µg/L		18:33:51
1	Al 396.153Radial†	47074.8	46363.0	[10000] µg/L		18:33:23
1	As 188.979†	2423.7	2405.8	[1000] µg/L		18:33:53
1	B 249.677†	64171.5	59964.1	[1000] µg/L		18:33:51
1	Ba 233.527†	222696.0	219915.4	[1000] µg/L		18:33:51
1	Be 313.107†	3125497.2	3084675.4	[1000] µg/L		18:33:51
1	Ca 317.933Radial†	175989.6	172593.1	[10000] µg/L		18:33:23
1	Cd 226.502†	147319.9	145459.1	[1000] µg/L		18:33:51
1	Co 228.616†	73285.4	72489.3	[1000] µg/L		18:33:53
1	Cr 267.716†	118453.3	116720.9	[1000] µg/L		18:33:51
1	Cu 324.752†	236158.0	230598.8	[1000] µg/L		18:33:51
1	Fe 238.204 Radial†	153305.8	150770.6	[10000] µg/L		18:33:23
1	K 766.490 Radial†	26333.7	24462.7	[10000] µg/L		18:33:23
1	Mg 279.077 IEC†	25539.7	24949.5	[10000] µg/L		18:33:23
1	Mn 257.610†	742700.4	732763.2	[1000] µg/L		18:33:51
1	Mo 202.031†	31916.7	31548.3	[1000] µg/L		18:33:53
1	Na 589.592 Radial†	67840.0	65073.6	[10000] µg/L		18:33:23
1	Ni 231.604†	79543.1	78528.3	[1000] µg/L		18:33:51
1	P 214.914†	21051.1	20692.1	[5000] µg/L		18:33:53
1	Pb 220.353†	16751.4	16416.6	[1000] µg/L		18:33:53
1	S 181.975 Axial†	2600.1	2470.7	[2000] µg/L		18:33:53
1	Sb 206.836†	7615.0	7427.3	[1000] µg/L		18:33:53
1	Se 196.026†	2517.5	2473.2	[1000] µg/L		18:33:53
1	SiO2†	101024.7	98111.1	[10695] µg/L		18:33:51
1	Si 251.611†	307939.1	303175.7	[5000] µg/L		18:33:51
1	Sn 189.927†	14211.0	14020.4	[1000] µg/L		18:33:53
1	Sr 421.552†	434456.1	427870.5	[1000] µg/L		18:33:21
1	Ti 334.940†	997481.3	983606.3	[1000] µg/L		18:33:51
1	Tl 190.801†	7335.9	7358.9	[1000] µg/L		18:33:53
1	U 409.014†	16212.4	16476.3	[1000] µg/L		18:33:51
1	V 292.402†	183867.8	180995.7	[1000] µg/L		18:33:51
1	Zn 213.857†	161925.8	159312.2	[1000] µg/L		18:33:51
2	Sc 361.383	1690996.4	1690996.4	101.09 %		18:33:57
2	Sc RADIAL	145999.7	145999.7	100 %		18:33:27
2	Y 371.029	1021922.1	1021922.1	99.936 %		18:33:57
2	Ag 328.068†	252044.6	246361.5	[1000] µg/L		18:33:57
2	Al 396.153Radial†	46624.8	46578.3	[10000] µg/L		18:33:27
2	As 188.979†	2403.1	2391.4	[1000] µg/L		18:33:59
2	B 249.677†	63843.6	59800.0	[1000] µg/L		18:33:57
2	Ba 233.527†	221227.7	219018.9	[1000] µg/L		18:33:57
2	Be 313.107†	3107291.9	3074468.3	[1000] µg/L		18:33:57
2	Ca 317.933Radial†	173656.9	172748.8	[10000] µg/L		18:33:27
2	Cd 226.502†	146575.4	145090.3	[1000] µg/L		18:33:57
2	Co 228.616†	74805.8	74176.3	[1000] µg/L		18:33:59
2	Cr 267.716†	118015.5	116583.5	[1000] µg/L		18:33:57
2	Cu 324.752†	235118.6	230160.1	[1000] µg/L		18:33:57
2	Fe 238.204 Radial†	151211.1	150843.6	[10000] µg/L		18:33:27
2	K 766.490 Radial†	25931.4	24432.8	[10000] µg/L		18:33:27
2	Mg 279.077 IEC†	24969.0	24740.4	[10000] µg/L		18:33:27
2	Mn 257.610†	740445.3	732386.4	[1000] µg/L		18:33:57
2	Mo 202.031†	32495.1	32200.2	[1000] µg/L		18:33:59
2	Na 589.592 Radial†	67249.4	65441.6	[10000] µg/L		18:33:27
2	Ni 231.604†	79100.3	78288.9	[1000] µg/L		18:33:57
2	P 214.914†	21690.5	21377.2	[5000] µg/L		18:33:59
2	Pb 220.353†	17172.9	16875.4	[1000] µg/L		18:33:59

2	S 181.975 Axial†	2679.6	2555.9	[2000]	µg/L	18:33:59
2	Sb 206.836†	7635.7	7466.8	[1000]	µg/L	18:33:59
2	Se 196.026†	2666.5	2626.9	[1000]	µg/L	18:33:59
2	SiO2†	100664.8	98007.2	[10695]	µg/L	18:33:57
2	Si 251.611†	306502.8	302523.6	[5000]	µg/L	18:33:57
2	Sn 189.927†	14443.7	14286.0	[1000]	µg/L	18:33:59
2	Sr 421.552†	430963.7	430517.1	[1000]	µg/L	18:33:25
2	Ti 334.940†	993955.9	982608.8	[1000]	µg/L	18:33:57
2	Tl 190.801†	7531.3	7570.4	[1000]	µg/L	18:33:59
2	U 409.014†	16040.6	16346.9	[1000]	µg/L	18:33:57
2	V 292.402†	183235.5	180829.1	[1000]	µg/L	18:33:57
2	Zn 213.857†	161264.5	159062.3	[1000]	µg/L	18:33:57
3	Sc 361.383	1679595.4	1679595.4	100.41	%	18:34:04
3	Sc RADIAL	149693.3	149693.3	103	%	18:33:31
3	Y 371.029	1015550.9	1015550.9	99.312	%	18:34:04
3	Ag 328.068†	251016.5	247030.1	[1000]	µg/L	18:34:04
3	Al 396.153Radial†	47551.4	46332.0	[10000]	µg/L	18:33:31
3	As 188.979†	2421.2	2425.6	[1000]	µg/L	18:34:06
3	B 249.677†	63426.3	59813.0	[1000]	µg/L	18:34:04
3	Ba 233.527†	219963.3	219245.0	[1000]	µg/L	18:34:04
3	Be 313.107†	3093622.9	3081719.7	[1000]	µg/L	18:34:04
3	Ca 317.933Radial†	178184.0	172879.1	[10000]	µg/L	18:33:31
3	Cd 226.502†	145509.3	145012.8	[1000]	µg/L	18:34:04
3	Co 228.616†	73160.7	73040.2	[1000]	µg/L	18:34:06
3	Cr 267.716†	117369.2	116732.4	[1000]	µg/L	18:34:04
3	Cu 324.752†	233979.9	230604.8	[1000]	µg/L	18:34:04
3	Fe 238.204 Radial†	154947.1	150756.5	[10000]	µg/L	18:33:31
3	K 766.490 Radial†	26410.5	24260.6	[10000]	µg/L	18:33:31
3	Mg 279.077 IEC†	25740.2	24876.2	[10000]	µg/L	18:33:31
3	Mn 257.610†	735902.7	732834.1	[1000]	µg/L	18:34:04
3	Mo 202.031†	31675.9	31602.5	[1000]	µg/L	18:34:06
3	Na 589.592 Radial†	68591.3	65091.7	[10000]	µg/L	18:33:31
3	Ni 231.604†	78372.8	78095.4	[1000]	µg/L	18:34:04
3	P 214.914†	21100.1	20934.8	[5000]	µg/L	18:34:06
3	Pb 220.353†	16565.8	16386.1	[1000]	µg/L	18:34:06
3	S 181.975 Axial†	2538.8	2433.7	[2000]	µg/L	18:34:06
3	Sb 206.836†	7547.1	7429.8	[1000]	µg/L	18:34:06
3	Se 196.026†	2534.8	2513.6	[1000]	µg/L	18:34:06
3	SiO2†	99973.5	97994.7	[10695]	µg/L	18:34:04
3	Si 251.611†	304718.9	302805.0	[5000]	µg/L	18:34:04
3	Sn 189.927†	14107.2	14047.9	[1000]	µg/L	18:34:06
3	Sr 421.552†	434068.2	422924.1	[1000]	µg/L	18:33:29
3	Ti 334.940†	988596.9	983945.8	[1000]	µg/L	18:34:04
3	Tl 190.801†	7419.8	7510.0	[1000]	µg/L	18:34:06
3	U 409.014†	16237.0	16650.2	[1000]	µg/L	18:34:04
3	V 292.402†	181988.8	180817.9	[1000]	µg/L	18:34:04
3	Zn 213.857†	160057.9	158943.5	[1000]	µg/L	18:34:04

Mean Data: SCAL

Analyte	Mean Corrected Intensity	Std.Dev.	RSD	Calib Conc. Units
Sc 361.383	1688622.0	8104.65	0.48%	100.95 %
Sc RADIAL	147928.9	1852.30	1.25%	101 %
Y 371.029	1020633.7	4576.76	0.45%	99.810 %
Ag 328.068†	246832.7	409.85	0.17%	[1000] µg/L
Al 396.153Radial†	46424.4	134.12	0.29%	[10000] µg/L
As 188.979†	2407.6	17.16	0.71%	[1000] µg/L
B 249.677†	59859.0	91.23	0.15%	[1000] µg/L
Ba 233.527†	219393.1	466.22	0.21%	[1000] µg/L
Be 313.107†	3080287.8	5252.04	0.17%	[1000] µg/L
Ca 317.933Radial†	172740.3	143.17	0.08%	[10000] µg/L
Cd 226.502†	145187.4	238.43	0.16%	[1000] µg/L
Co 228.616†	73235.3	860.22	1.17%	[1000] µg/L
Cr 267.716†	116678.9	82.81	0.07%	[1000] µg/L
Cu 324.752†	230454.6	255.03	0.11%	[1000] µg/L
Fe 238.204 Radial†	150790.2	46.73	0.03%	[10000] µg/L
K 766.490 Radial†	24385.4	109.10	0.45%	[10000] µg/L
Mg 279.077 IEC†	24855.4	106.12	0.43%	[10000] µg/L
Mn 257.610†	732661.3	240.63	0.03%	[1000] µg/L
Mo 202.031†	31783.7	361.73	1.14%	[1000] µg/L

Na 589.592 Radial†	65202.3	207.44	0.32%	[10000]	µg/L
Ni 231.604†	78304.2	216.83	0.28%	[1000]	µg/L
P 214.914†	21001.4	347.34	1.65%	[5000]	µg/L
Pb 220.353†	16559.4	274.11	1.66%	[1000]	µg/L
S 181.975 Axial†	2486.8	62.65	2.52%	[2000]	µg/L
Sb 206.836†	7441.3	22.10	0.30%	[1000]	µg/L
Se 196.026†	2537.9	79.67	3.14%	[1000]	µg/L
SiO2†	98037.6	63.89	0.07%	[10695]	µg/L
Si 251.611†	302834.8	327.07	0.11%	[5000]	µg/L
Sn 189.927†	14118.1	146.08	1.03%	[1000]	µg/L
Sr 421.552†	427103.9	3854.12	0.90%	[1000]	µg/L
Ti 334.940†	983387.0	694.94	0.07%	[1000]	µg/L
Tl 190.801†	7479.8	108.97	1.46%	[1000]	µg/L
U 409.014†	16491.1	152.21	0.92%	[1000]	µg/L
V 292.402†	180880.9	99.54	0.06%	[1000]	µg/L
Zn 213.857†	159106.0	188.24	0.12%	[1000]	µg/L

Sequence No.: 5

Sample ID: S10

Analyst:

Logged In Analyst (Original) : optima4

Initial Sample Wt:

Dilution:

Autosampler Location: 5

Date Collected: 3/29/2010 18:34:14

Data Type: Reprocessed on 3/29/2010 19:14:35

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: S10

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Analysis Time
1	Sc 361.383	1647889.5	1647889.5	98.512 %	18:35:05
1	Sc RADIAL	147922.0	147922.0	101 %	18:34:43
1	Y 371.029	997984.1	997984.1	97.595 %	18:35:05
1	Al 396.153Radial†	231630.6	228268.0	[50000] µg/L	18:34:43
1	Ca 317.933Radial†	864405.0	851121.2	[50000] µg/L	18:34:43
1	Fe 238.204 Radial†	304562.8	299986.3	[20000] µg/L	18:34:43
1	Mg 279.077 IEC†	122786.4	120800.3	[50000] µg/L	18:34:43
1	Na 589.592 Radial†	134121.8	130461.6	[20000] µg/L	18:34:43
2	Sc 361.383	1646965.2	1646965.2	98.457 %	18:35:08
2	Sc RADIAL	147135.1	147135.1	101 %	18:34:45
2	Y 371.029	998151.2	998151.2	97.611 %	18:35:08
2	Al 396.153Radial†	231070.3	228933.5	[50000] µg/L	18:34:45
2	Ca 317.933Radial†	860622.6	851929.2	[50000] µg/L	18:34:45
2	Fe 238.204 Radial†	303079.0	300121.2	[20000] µg/L	18:34:45
2	Mg 279.077 IEC†	122393.7	121058.3	[50000] µg/L	18:34:45
2	Na 589.592 Radial†	133483.0	130535.5	[20000] µg/L	18:34:45
3	Sc 361.383	1642134.3	1642134.3	98.168 %	18:35:10
3	Sc RADIAL	146873.2	146873.2	101 %	18:34:47
3	Y 371.029	994617.7	994617.7	97.265 %	18:35:10
3	Al 396.153Radial†	231391.3	229660.2	[50000] µg/L	18:34:47
3	Ca 317.933Radial†	862939.8	855749.1	[50000] µg/L	18:34:47
3	Fe 238.204 Radial†	304238.1	301806.9	[20000] µg/L	18:34:47
3	Mg 279.077 IEC†	122676.5	121555.2	[50000] µg/L	18:34:47
3	Na 589.592 Radial†	134070.7	131354.5	[20000] µg/L	18:34:47

Mean Data: S10

Analyte	Mean Corrected Intensity	Std.Dev.	RSD	Calib Conc. Units
Sc 361.383	1645663.0	3090.68	0.19%	98.379 %
Sc RADIAL	147310.1	545.84	0.37%	101 %
Y 371.029	996917.7	1993.60	0.20%	97.490 %
Al 396.153Radial†	228953.9	696.32	0.30%	[50000] µg/L
Ca 317.933Radial†	852933.2	2471.89	0.29%	[50000] µg/L
Fe 238.204 Radial†	300638.1	1014.46	0.34%	[20000] µg/L
Mg 279.077 IEC†	121137.9	383.71	0.32%	[50000] µg/L
Na 589.592 Radial†	130783.9	495.57	0.38%	[20000] µg/L

Calibration Summary

Analyte	Stds.	Equation	Intercept	Slope	Curvature	Corr. Coef.	Reslope
Ag 328.068	3	Lin Thru 0	0.0	246.4	0.00000	0.999992	
Al 396.153Radial	3	Lin Thru 0	0.0	4.581	0.00000	0.999996	
As 188.979	3	Lin Thru 0	0.0	2.393	0.00000	0.999929	
B 249.677	3	Lin Thru 0	0.0	59.56	0.00000	0.999952	
Ba 233.527	3	Lin Thru 0	0.0	218.9	0.00000	0.999987	
Be 313.107	3	Lin Thru 0	0.0	3072	0.00000	0.999986	
Ca 317.933Radial	3	Lin Thru 0	0.0	17.07	0.00000	0.999997	
Cd 226.502	3	Lin Thru 0	0.0	144.8	0.00000	0.999986	
Co 228.616	3	Lin Thru 0	0.0	73.04	0.00000	0.999984	
Cr 267.716	3	Lin Thru 0	0.0	116.4	0.00000	0.999990	
Cu 324.752	3	Lin Thru 0	0.0	230.0	0.00000	0.999993	
Fe 238.204 Radia	2	Lin Thru 0	0.0	15.04	0.00000	0.999999	
K 766.490 Radial	3	Lin Thru 0	0.0	2.429	0.00000	0.999970	
Mg 279.077 IEC	3	Lin Thru 0	0.0	2.425	0.00000	0.999987	
Mn 257.610	3	Lin Thru 0	0.0	731.8	0.00000	0.999991	
Mo 202.031	3	Lin Thru 0	0.0	31.68	0.00000	0.999979	

Na 589.592 Radia	2	Lin Thru 0	0.0	6.535	0.00000	0.999999
Ni 231.604	3	Lin Thru 0	0.0	78.18	0.00000	0.999990
P 214.914	3	Lin Thru 0	0.0	4.176	0.00000	0.999933
Pb 220.353	3	Lin Thru 0	0.0	16.51	0.00000	0.999980
S 181.975 Axial	3	Lin Thru 0	0.0	1.234	0.00000	0.999894
Sb 206.836	3	Lin Thru 0	0.0	7.413	0.00000	0.999972
Se 196.026	3	Lin Thru 0	0.0	2.528	0.00000	0.999970
SiO2	3	Lin Thru 0	0.0	9.149	0.00000	0.999993
Si 251.611	3	Lin Thru 0	0.0	60.48	0.00000	0.999996
Sn 189.927	3	Lin Thru 0	0.0	14.07	0.00000	0.999974
Sr 421.552	3	Lin Thru 0	0.0	426.7	0.00000	0.999990
Ti 334.940	3	Lin Thru 0	0.0	980.7	0.00000	0.999985
Tl 190.801	3	Lin Thru 0	0.0	7.450	0.00000	0.999968
U 409.014	3	Lin Thru 0	0.0	16.18	0.00000	0.999235
V 292.402	3	Lin Thru 0	0.0	180.3	0.00000	0.999978
Zn 213.857	3	Lin Thru 0	0.0	158.8	0.00000	0.999994

Sequence No.: 6

Sample ID: ICV

Analyst:

Logged In Analyst (Original) : optima4

Initial Sample Wt:

Dilution:

Autosampler Location: 9

Date Collected: 3/29/2010 18:35:18

Data Type: Reprocessed on 3/29/2010 19:14:36

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: ICV

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc 361.383	1701844.8	1701844.8	101.74 %		18:36:17
1	Sc RADIAL	151216.0	151216.0	104 %		18:35:50
1	Y 371.029	1036585.9	1036585.9	101.37 %		18:36:17
1	Ag 328.068†	65858.6	61766.5	256.87 µg/L	256.87 ppb	18:36:17
1	Al 396.153Radial†	24486.5	23634.0	5134.9 µg/L	5134.9 ppb	18:35:50
1	As 188.979†	1140.6	1135.4	481.67 µg/L	481.67 ppb	18:36:37
1	B 249.677†	34168.2	30228.9	505.75 µg/L	505.75 ppb	18:36:17
1	Ba 233.527†	112714.3	110964.0	507.33 µg/L	507.33 ppb	18:36:17
1	Be 313.107†	798269.6	785294.0	255.76 µg/L	255.76 ppb	18:36:17
1	Ca 317.933Radial†	89164.4	85327.7	4999.8 µg/L	4999.8 ppb	18:35:50
1	Cd 226.502†	72993.3	71840.9	495.79 µg/L	495.79 ppb	18:36:17
1	Co 228.616†	37444.2	36981.2	506.64 µg/L	506.64 ppb	18:36:17
1	Cr 267.716†	57873.1	56724.3	487.10 µg/L	487.10 ppb	18:36:17
1	Cu 324.752†	121386.5	116888.2	509.66 µg/L	509.66 ppb	18:36:17
1	Fe 238.204 Radial†	78431.6	75485.5	5018.5 µg/L	5018.5 ppb	18:35:50
1	K 766.490 Radial†	7725.2	5991.2	2463.6 µg/L	2463.6 ppb	18:35:50
1	Mg 279.077 IEC†	13310.9	12643.4	5221.4 µg/L	5221.4 ppb	18:35:50
1	Mn 257.610†	376288.9	369781.3	505.06 µg/L	505.06 ppb	18:36:17
1	Mo 202.031†	16673.6	16444.0	519.54 µg/L	519.54 ppb	18:36:37
1	Na 589.592 Radial†	18471.5	16109.6	2462.8 µg/L	2462.8 ppb	18:35:50
1	Ni 231.604†	39283.0	38652.9	494.42 µg/L	494.42 ppb	18:36:17
1	P 214.914†	10554.2	10294.3	2456.6 µg/L	2456.6 ppb	18:36:37
1	Pb 220.353†	8472.5	8215.3	499.30 µg/L	499.30 ppb	18:36:37
1	S 181.975 Axial†	3123.6	2975.4	2415.0 µg/L	2415.0 ppb	18:36:37
1	Sb 206.836†	3775.1	3624.0	490.49 µg/L	490.49 ppb	18:36:37
1	Se 196.026†	6364.3	6244.7	2470 µg/L	2470 ppb	18:36:37
1	SiO2†	99568.8	96295.2	10503 µg/L	10503 ppb	18:36:17
1	Si 251.611†	303093.3	297239.6	4904.5 µg/L	4904.5 ppb	18:36:17
1	Sn 189.927†	7432.7	7303.7	520.86 µg/L	520.86 ppb	18:36:37
1	Sr 421.552†	233447.1	225293.2	527.99 µg/L	527.99 ppb	18:35:48
1	Ti 334.940†	482527.6	473648.9	482.33 µg/L	482.33 ppb	18:36:17
1	Tl 190.801†	3799.6	3855.0	524.73 µg/L	524.73 ppb	18:36:37
1	U 409.014†	6773.0	7136.4	471.37 µg/L	471.37 ppb	18:36:17
1	V 292.402†	91625.4	89628.5	503.69 µg/L	503.69 ppb	18:36:17
1	Zn 213.857†	81346.1	79492.2	496.47 µg/L	496.47 ppb	18:36:17
2	Sc 361.383	1701980.9	1701980.9	101.75 %		18:36:40
2	Sc RADIAL	148848.9	148848.9	102 %		18:35:54
2	Y 371.029	1036246.9	1036246.9	101.34 %		18:36:40
2	Ag 328.068†	66063.0	61962.3	257.67 µg/L	257.67 ppb	18:36:40
2	Al 396.153Radial†	24189.6	23718.6	5153.2 µg/L	5153.2 ppb	18:35:54
2	As 188.979†	1141.1	1135.8	481.85 µg/L	481.85 ppb	18:37:00
2	B 249.677†	34342.1	30397.1	508.57 µg/L	508.57 ppb	18:36:40
2	Ba 233.527†	113003.6	111239.5	508.60 µg/L	508.60 ppb	18:36:40
2	Be 313.107†	803326.2	790201.1	257.35 µg/L	257.35 ppb	18:36:40
2	Ca 317.933Radial†	87776.3	85335.2	5000.3 µg/L	5000.3 ppb	18:35:54
2	Cd 226.502†	73305.6	72142.1	497.87 µg/L	497.87 ppb	18:36:40
2	Co 228.616†	37456.8	36990.6	506.77 µg/L	506.77 ppb	18:36:40
2	Cr 267.716†	58033.0	56876.9	488.42 µg/L	488.42 ppb	18:36:40
2	Cu 324.752†	121826.1	117310.6	511.48 µg/L	511.48 ppb	18:36:40
2	Fe 238.204 Radial†	77113.3	75396.8	5012.6 µg/L	5012.6 ppb	18:35:54
2	K 766.490 Radial†	7618.8	6005.4	2469.4 µg/L	2469.4 ppb	18:35:54
2	Mg 279.077 IEC†	12970.7	12514.3	5168.3 µg/L	5168.3 ppb	18:35:54
2	Mn 257.610†	377832.0	371268.3	507.10 µg/L	507.10 ppb	18:36:40
2	Mo 202.031†	16755.0	16522.7	522.02 µg/L	522.02 ppb	18:37:00
2	Na 589.592 Radial†	18069.9	15999.5	2445.9 µg/L	2445.9 ppb	18:35:54
2	Ni 231.604†	39447.3	38811.3	496.44 µg/L	496.44 ppb	18:36:40
2	P 214.914†	10626.3	10364.3	2473.3 µg/L	2473.3 ppb	18:37:00
2	Pb 220.353†	8494.9	8236.7	500.61 µg/L	500.61 ppb	18:37:00

2	S 181.975 Axial†	3125.4	2976.9	2416.3 µg/L	2416.3 ppb	18:37:00
2	Sb 206.836†	3806.5	3654.5	494.63 µg/L	494.63 ppb	18:37:00
2	Se 196.026†	6410.3	6289.4	2490 µg/L	2490 ppb	18:37:00
2	SiO2†	100159.6	96868.0	10565 µg/L	10565 ppb	18:36:40
2	Si 251.611†	304136.0	298240.5	4921.0 µg/L	4921.0 ppb	18:36:40
2	Sn 189.927†	7468.1	7337.9	523.29 µg/L	523.29 ppb	18:37:00
2	Sr 421.552†	233080.0	228512.0	535.53 µg/L	535.53 ppb	18:35:52
2	Ti 334.940†	484116.4	475172.5	483.90 µg/L	483.90 ppb	18:36:40
2	Tl 190.801†	3811.9	3866.8	526.34 µg/L	526.34 ppb	18:37:00
2	U 409.014†	6593.5	6959.4	460.57 µg/L	460.57 ppb	18:36:40
2	V 292.402†	92020.5	90009.6	505.83 µg/L	505.83 ppb	18:36:40
2	Zn 213.857†	81495.2	79632.3	497.34 µg/L	497.34 ppb	18:36:40
3	Sc 361.383	1720635.0	1720635.0	102.86 %		18:37:03
3	Sc RADIAL	149044.6	149044.6	102 %		18:35:58
3	Y 371.029	1046771.8	1046771.8	102.37 %		18:37:03
3	Ag 328.068†	66524.8	61707.3	256.63 µg/L	256.63 ppb	18:37:03
3	Al 396.153Radial†	24064.3	23565.0	5120.0 µg/L	5120.0 ppb	18:35:58
3	As 188.979†	1131.9	1114.6	473.00 µg/L	473.00 ppb	18:37:23
3	B 249.677†	34751.0	30428.7	509.10 µg/L	509.10 ppb	18:37:03
3	Ba 233.527†	114119.3	111120.0	508.05 µg/L	508.05 ppb	18:37:03
3	Be 313.107†	809136.9	787290.3	256.41 µg/L	256.41 ppb	18:37:03
3	Ca 317.933Radial†	87762.2	85208.6	4992.9 µg/L	4992.9 ppb	18:35:58
3	Cd 226.502†	74233.6	72263.2	498.71 µg/L	498.71 ppb	18:37:03
3	Co 228.616†	37810.4	36935.2	506.02 µg/L	506.02 ppb	18:37:03
3	Cr 267.716†	58579.7	56790.0	487.67 µg/L	487.67 ppb	18:37:03
3	Cu 324.752†	122627.9	116792.1	509.24 µg/L	509.24 ppb	18:37:03
3	Fe 238.204 Radial†	77211.6	75393.8	5012.4 µg/L	5012.4 ppb	18:35:58
3	K 766.490 Radial†	7631.8	6008.3	2470.6 µg/L	2470.6 ppb	18:35:58
3	Mg 279.077 IEC†	13062.0	12587.0	5198.1 µg/L	5198.1 ppb	18:35:58
3	Mn 257.610†	380724.0	370053.9	505.44 µg/L	505.44 ppb	18:37:03
3	Mo 202.031†	16767.7	16356.5	516.77 µg/L	516.77 ppb	18:37:23
3	Na 589.592 Radial†	18288.4	16189.9	2475.1 µg/L	2475.1 ppb	18:35:58
3	Ni 231.604†	39680.9	38618.1	493.97 µg/L	493.97 ppb	18:37:03
3	P 214.914†	10598.2	10223.8	2439.7 µg/L	2439.7 ppb	18:37:23
3	Pb 220.353†	8535.0	8185.1	497.46 µg/L	497.46 ppb	18:37:23
3	S 181.975 Axial†	3153.8	2971.2	2411.6 µg/L	2411.6 ppb	18:37:23
3	Sb 206.836†	3795.0	3602.8	487.58 µg/L	487.58 ppb	18:37:23
3	Se 196.026†	6408.5	6219.4	2460 µg/L	2460 ppb	18:37:23
3	SiO2†	100969.8	96588.4	10535 µg/L	10535 ppb	18:37:03
3	Si 251.611†	306927.5	297713.8	4912.4 µg/L	4912.4 ppb	18:37:03
3	Sn 189.927†	7476.5	7266.5	518.21 µg/L	518.21 ppb	18:37:23
3	Sr 421.552†	230245.5	225440.5	528.33 µg/L	528.33 ppb	18:35:56
3	Ti 334.940†	487355.2	473162.7	481.84 µg/L	481.84 ppb	18:37:03
3	Tl 190.801†	3807.3	3821.7	520.26 µg/L	520.26 ppb	18:37:23
3	U 409.014†	6788.8	7079.0	467.87 µg/L	467.87 ppb	18:37:03
3	V 292.402†	92755.7	89743.8	504.30 µg/L	504.30 ppb	18:37:03
3	Zn 213.857†	82290.5	79537.1	496.75 µg/L	496.75 ppb	18:37:03

Mean Data: ICV

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1708153.5	102.11 %	0.646			0.63%
Sc RADIAL	149703.2	103 %	0.9			0.88%
Y 371.029	1039868.2	101.69 %	0.585			0.58%
Ag 328.068†	61812.1	257.06 µg/L	0.547	257.06 ppb	0.547	0.21%
QC value within limits for Ag 328.068 Recovery = 102.82%						
Al 396.153Radial†	23639.2	5136.0 µg/L	16.67	5136.0 ppb	16.67	0.32%
QC value within limits for Al 396.153Radial Recovery = 102.72%						
As 188.979†	1128.6	478.84 µg/L	5.057	478.84 ppb	5.057	1.06%
QC value within limits for As 188.979 Recovery = 95.77%						
B 249.677†	30351.6	507.81 µg/L	1.804	507.81 ppb	1.804	0.36%
QC value within limits for B 249.677 Recovery = 101.56%						
Ba 233.527†	111107.9	507.99 µg/L	0.632	507.99 ppb	0.632	0.12%
QC value within limits for Ba 233.527 Recovery = 101.60%						
Be 313.107†	787595.1	256.51 µg/L	0.802	256.51 ppb	0.802	0.31%
QC value within limits for Be 313.107 Recovery = 102.60%						
Ca 317.933Radial†	85290.5	4997.7 µg/L	4.16	4997.7 ppb	4.16	0.08%
QC value within limits for Ca 317.933Radial Recovery = 99.95%						
Cd 226.502†	72082.0	497.46 µg/L	1.502	497.46 ppb	1.502	0.30%
QC value within limits for Cd 226.502 Recovery = 99.49%						

Co 228.616†	36969.0	506.48 µg/L	0.406	506.48 ppb	0.406	0.08%
QC value within limits for Co 228.616 Recovery = 101.30%						
Cr 267.716†	56797.1	487.73 µg/L	0.662	487.73 ppb	0.662	0.14%
QC value within limits for Cr 267.716 Recovery = 97.55%						
Cu 324.752†	116997.0	510.13 µg/L	1.195	510.13 ppb	1.195	0.23%
QC value within limits for Cu 324.752 Recovery = 102.03%						
Fe 238.204 Radial†	75425.3	5014.5 µg/L	3.46	5014.5 ppb	3.46	0.07%
QC value within limits for Fe 238.204 Radial Recovery = 100.29%						
K 766.490 Radial†	6001.6	2467.9 µg/L	3.77	2467.9 ppb	3.77	0.15%
QC value within limits for K 766.490 Radial Recovery = 98.71%						
Mg 279.077 IEC†	12581.6	5195.9 µg/L	26.65	5195.9 ppb	26.65	0.51%
QC value within limits for Mg 279.077 IEC Recovery = 103.92%						
Mn 257.610†	370367.8	505.87 µg/L	1.083	505.87 ppb	1.083	0.21%
QC value within limits for Mn 257.610 Recovery = 101.17%						
Mo 202.031†	16441.1	519.44 µg/L	2.624	519.44 ppb	2.624	0.51%
QC value within limits for Mo 202.031 Recovery = 103.89%						
Na 589.592 Radial†	16099.7	2461.3 µg/L	14.63	2461.3 ppb	14.63	0.59%
QC value within limits for Na 589.592 Radial Recovery = 98.45%						
Ni 231.604†	38694.1	494.94 µg/L	1.317	494.94 ppb	1.317	0.27%
QC value within limits for Ni 231.604 Recovery = 98.99%						
P 214.914†	10294.2	2456.5 µg/L	16.81	2456.5 ppb	16.81	0.68%
QC value within limits for P 214.914 Recovery = 98.26%						
Pb 220.353†	8212.4	499.12 µg/L	1.581	499.12 ppb	1.581	0.32%
QC value within limits for Pb 220.353 Recovery = 99.82%						
S 181.975 Axial†	2974.5	2414.3 µg/L	2.40	2414.3 ppb	2.40	0.10%
QC value within limits for S 181.975 Axial Recovery = 96.57%						
Sb 206.836†	3627.1	490.90 µg/L	3.546	490.90 ppb	3.546	0.72%
QC value within limits for Sb 206.836 Recovery = 98.18%						
Se 196.026†	6251.2	2470 µg/L	14.0	2470 ppb	14.0	0.57%
QC value within limits for Se 196.026 Recovery = 98.99%						
SiO2†	96583.8	10534 µg/L	31.3	10534 ppb	31.3	0.30%
QC value within limits for SiO2 Recovery = 98.50%						
Si 251.611†	297731.3	4912.6 µg/L	8.25	4912.6 ppb	8.25	0.17%
QC value within limits for Si 251.611 Recovery = 98.25%						
Sn 189.927†	7302.7	520.79 µg/L	2.541	520.79 ppb	2.541	0.49%
QC value within limits for Sn 189.927 Recovery = 104.16%						
Sr 421.552†	226415.3	530.62 µg/L	4.259	530.62 ppb	4.259	0.80%
QC value within limits for Sr 421.552 Recovery = 106.12%						
Ti 334.940†	473994.7	482.69 µg/L	1.073	482.69 ppb	1.073	0.22%
QC value within limits for Ti 334.940 Recovery = 96.54%						
Tl 190.801†	3847.8	523.78 µg/L	3.151	523.78 ppb	3.151	0.60%
QC value within limits for Tl 190.801 Recovery = 104.76%						
U 409.014†	7058.3	466.61 µg/L	5.511	466.61 ppb	5.511	1.18%
QC value within limits for U 409.014 Recovery = 93.32%						
V 292.402†	89793.9	504.61 µg/L	1.101	504.61 ppb	1.101	0.22%
QC value within limits for V 292.402 Recovery = 100.92%						
Zn 213.857†	79553.9	496.85 µg/L	0.443	496.85 ppb	0.443	0.09%
QC value within limits for Zn 213.857 Recovery = 99.37%						
All analyte(s) passed QC.						

Sequence No.: 7

Sample ID: ICB

Analyst:

Logged In Analyst (Original) : optima4

Initial Sample Wt:

Dilution:

Autosampler Location: 10

Date Collected: 3/29/2010 18:37:32

Data Type: Reprocessed on 3/29/2010 19:14:36

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: ICB

Repl#	Analyte	Net Intensity	Corrected Intensity	Conc. Units	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc 361.383	1718110.5	1718110.5	102.71 %			18:39:24
1	Sc RADIAL	149870.1	149870.1	103 %			18:38:01
1	Y 371.029	1056124.6	1056124.6	103.28 %			18:39:24
1	Ag 328.068†	2764.1	-275.9	-1.1170 µg/L		-1.1170 ppb	18:39:26
1	Al 396.153Radial†	-34.1	-1.3	-0.3025 µg/L		-0.3025 ppb	18:38:21
1	As 188.979†	-13.9	0.8	0.3158 µg/L		0.3158 ppb	18:39:46
1	B 249.677†	3290.8	-151.7	-2.5477 µg/L		-2.5477 ppb	18:39:46
1	Ba 233.527†	-149.3	29.7	0.1352 µg/L		0.1352 ppb	18:39:46
1	Be 313.107†	-642.8	34.2	0.0134 µg/L		0.0134 ppb	18:39:26
1	Ca 317.933Radial†	601.2	-31.5	-1.8457 µg/L		-1.8457 ppb	18:38:21
1	Cd 226.502†	-82.2	14.4	0.0988 µg/L		0.0988 ppb	18:39:46
1	Co 228.616†	-179.0	2.3	0.0321 µg/L		0.0321 ppb	18:39:46
1	Cr 267.716†	164.4	-0.2	-0.0075 µg/L		-0.0075 ppb	18:39:46
1	Cu 324.752†	2372.4	-115.1	-0.4939 µg/L		-0.4939 ppb	18:39:26
1	Fe 238.204 Radial†	141.5	24.3	1.6170 µg/L		1.6170 ppb	18:38:21
1	K 766.490 Radial†	1569.1	71.0	29.223 µg/L		29.223 ppb	18:38:01
1	Mg 279.077 IEC†	162.3	-28.9	-11.902 µg/L		-11.902 ppb	18:38:21
1	Mn 257.610†	162.2	77.9	0.1069 µg/L		0.1069 ppb	18:39:46
1	Mo 202.031†	-48.8	7.7	0.2416 µg/L		0.2416 ppb	18:39:46
1	Na 589.592 Radial†	1595.3	-143.3	-21.948 µg/L		-21.948 ppb	18:38:01
1	Ni 231.604†	-74.2	-31.3	-0.4003 µg/L		-0.4003 ppb	18:39:46
1	P 214.914†	77.1	-4.5	-1.0788 µg/L		-1.0788 ppb	18:39:46
1	Pb 220.353†	105.8	-9.5	-0.5776 µg/L		-0.5776 ppb	18:39:46
1	S 181.975 Axial†	96.4	-1.0	-0.8082 µg/L		-0.8082 ppb	18:39:46
1	Sb 206.836†	76.9	-11.8	-1.5863 µg/L		-1.5863 ppb	18:39:46
1	Se 196.026†	30.3	18.6	7.35 µg/L		7.35 ppb	18:39:46
1	SiO2†	1615.4	-0.1	-0.0156 µg/L		-0.0156 ppb	18:39:46
1	Si 251.611†	756.3	60.0	0.9881 µg/L		0.9881 ppb	18:39:26
1	Sn 189.927†	2.2	0.2	0.0117 µg/L		0.0117 ppb	18:39:46
1	Sr 421.552†	-232.4	51.9	0.1217 µg/L		0.1217 ppb	18:38:01
1	Ti 334.940†	823.7	165.6	0.1667 µg/L		0.1667 ppb	18:39:26
1	Tl 190.801†	-129.5	-5.8	-0.7821 µg/L		-0.7821 ppb	18:39:46
1	U 409.014†	-365.4	123.4	7.5895 µg/L		7.5895 ppb	18:39:26
1	V 292.402†	336.7	-104.0	-0.5695 µg/L		-0.5695 ppb	18:39:26
1	Zn 213.857†	481.8	4.7	0.0326 µg/L		0.0326 ppb	18:39:46
2	Sc 361.383	1718304.1	1718304.1	102.72 %			18:39:48
2	Sc RADIAL	149819.8	149819.8	103 %			18:38:23
2	Y 371.029	1056622.1	1056622.1	103.33 %			18:39:48
2	Ag 328.068†	3062.4	14.3	0.0846 µg/L		0.0846 ppb	18:39:50
2	Al 396.153Radial†	-45.4	-12.3	-2.7171 µg/L		-2.7171 ppb	18:38:44
2	As 188.979†	-10.9	3.6	1.5162 µg/L		1.5162 ppb	18:40:10
2	B 249.677†	3277.0	-165.5	-2.7792 µg/L		-2.7792 ppb	18:40:10
2	Ba 233.527†	-168.1	11.4	0.0526 µg/L		0.0526 ppb	18:40:10
2	Be 313.107†	-415.9	255.2	0.0882 µg/L		0.0882 ppb	18:39:50
2	Ca 317.933Radial†	633.4	0.0	0.0016 µg/L		0.0016 ppb	18:38:44
2	Cd 226.502†	-115.3	-17.9	-0.1235 µg/L		-0.1235 ppb	18:40:10
2	Co 228.616†	-162.9	18.1	0.2472 µg/L		0.2472 ppb	18:40:10
2	Cr 267.716†	189.3	24.1	0.1939 µg/L		0.1939 ppb	18:40:10
2	Cu 324.752†	2490.6	-0.2	0.0132 µg/L		0.0132 ppb	18:39:50
2	Fe 238.204 Radial†	132.2	15.4	1.0215 µg/L		1.0215 ppb	18:38:44
2	K 766.490 Radial†	1519.5	23.3	9.5884 µg/L		9.5884 ppb	18:38:23
2	Mg 279.077 IEC†	195.8	3.8	1.5733 µg/L		1.5733 ppb	18:38:44
2	Mn 257.610†	168.0	83.5	0.1141 µg/L		0.1141 ppb	18:40:10
2	Mo 202.031†	-35.6	20.5	0.6489 µg/L		0.6489 ppb	18:40:10
2	Na 589.592 Radial†	1651.7	-87.8	-13.450 µg/L		-13.450 ppb	18:38:23
2	Ni 231.604†	-55.2	-12.8	-0.1641 µg/L		-0.1641 ppb	18:40:10
2	P 214.914†	83.6	1.8	0.4344 µg/L		0.4344 ppb	18:40:10
2	Pb 220.353†	94.6	-20.3	-1.2399 µg/L		-1.2399 ppb	18:40:10

2	S 181.975 Axial†	84.2	-12.9	-10.416 µg/L	-10.416 ppb	18:40:10
2	Sb 206.836†	72.7	-15.8	-2.1296 µg/L	-2.1296 ppb	18:40:10
2	Se 196.026†	25.1	13.5	5.37 µg/L	5.37 ppb	18:40:10
2	SiO2†	1629.2	13.2	1.4227 µg/L	1.4227 ppb	18:40:10
2	Si 251.611†	776.2	79.3	1.3023 µg/L	1.3023 ppb	18:39:50
2	Sn 189.927†	1.7	-0.4	-0.0258 µg/L	-0.0258 ppb	18:40:10
2	Sr 421.552†	-119.9	161.3	0.3781 µg/L	0.3781 ppb	18:38:23
2	Ti 334.940†	906.1	245.8	0.2435 µg/L	0.2435 ppb	18:39:50
2	Tl 190.801†	-120.0	3.5	0.4698 µg/L	0.4698 ppb	18:40:10
2	U 409.014†	-211.2	273.5	16.929 µg/L	16.929 ppb	18:39:50
2	V 292.402†	536.3	90.3	0.5193 µg/L	0.5193 ppb	18:39:50
2	Zn 213.857†	461.1	-15.5	-0.0967 µg/L	-0.0967 ppb	18:40:10
3	Sc 361.383	1698930.8	1698930.8	101.56 %		18:40:12
3	Sc RADIAL	152143.2	152143.2	104 %		18:38:46
3	Y 371.029	1045315.3	1045315.3	102.22 %		18:40:12
3	Ag 328.068†	3085.7	71.1	0.2837 µg/L	0.2837 ppb	18:40:14
3	Al 396.153Radial†	-62.8	-28.3	-6.2230 µg/L	-6.2230 ppb	18:39:06
3	As 188.979†	-25.2	-10.6	-4.4173 µg/L	-4.4173 ppb	18:40:34
3	B 249.677†	3266.7	-139.3	-2.3411 µg/L	-2.3411 ppb	18:40:34
3	Ba 233.527†	-163.9	13.7	0.0623 µg/L	0.0623 ppb	18:40:34
3	Be 313.107†	-627.7	42.1	0.0141 µg/L	0.0141 ppb	18:40:14
3	Ca 317.933Radial†	630.0	-12.6	-0.7399 µg/L	-0.7399 ppb	18:39:06
3	Cd 226.502†	-76.1	19.4	0.1339 µg/L	0.1339 ppb	18:40:34
3	Co 228.616†	-133.4	45.2	0.6195 µg/L	0.6195 ppb	18:40:34
3	Cr 267.716†	156.7	-5.9	-0.0523 µg/L	-0.0523 ppb	18:40:34
3	Cu 324.752†	2540.5	76.5	0.3341 µg/L	0.3341 ppb	18:40:14
3	Fe 238.204 Radial†	134.4	15.5	1.0313 µg/L	1.0313 ppb	18:39:06
3	K 766.490 Radial†	1520.9	2.1	0.8535 µg/L	0.8535 ppb	18:38:46
3	Mg 279.077 IEC†	186.1	-8.4	-3.4269 µg/L	-3.4269 ppb	18:39:06
3	Mn 257.610†	142.8	60.6	0.0829 µg/L	0.0829 ppb	18:40:34
3	Mo 202.031†	-28.7	26.9	0.8495 µg/L	0.8495 ppb	18:40:34
3	Na 589.592 Radial†	1594.0	-167.7	-25.662 µg/L	-25.662 ppb	18:38:46
3	Ni 231.604†	-74.3	-32.3	-0.4127 µg/L	-0.4127 ppb	18:40:34
3	P 214.914†	71.0	-9.6	-2.3151 µg/L	-2.3151 ppb	18:40:34
3	Pb 220.353†	138.9	24.3	1.4738 µg/L	1.4738 ppb	18:40:34
3	S 181.975 Axial†	87.7	-8.5	-6.8917 µg/L	-6.8917 ppb	18:40:34
3	Sb 206.836†	71.9	-15.8	-2.1234 µg/L	-2.1234 ppb	18:40:34
3	Se 196.026†	21.3	10.1	3.99 µg/L	3.99 ppb	18:40:34
3	SiO2†	1618.8	21.0	2.2686 µg/L	2.2686 ppb	18:40:34
3	Si 251.611†	788.9	100.3	1.6458 µg/L	1.6458 ppb	18:40:14
3	Sn 189.927†	6.3	4.2	0.2956 µg/L	0.2956 ppb	18:40:34
3	Sr 421.552†	-237.8	50.2	0.1176 µg/L	0.1176 ppb	18:38:46
3	Ti 334.940†	556.8	-88.1	-0.0902 µg/L	-0.0902 ppb	18:40:14
3	Tl 190.801†	-119.8	2.3	0.3073 µg/L	0.3073 ppb	18:40:34
3	U 409.014†	-464.1	22.2	1.3392 µg/L	1.3392 ppb	18:40:14
3	V 292.402†	338.6	-98.5	-0.5367 µg/L	-0.5367 ppb	18:40:14
3	Zn 213.857†	460.6	-10.9	-0.0662 µg/L	-0.0662 ppb	18:40:34

Mean Data: ICB

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1711781.8	102.33 %	0.665			0.65%
Sc RADIAL	150611.1	103 %	0.9			0.88%
Y 371.029	1052687.3	102.94 %	0.625			0.61%
Ag 328.068†	-63.5	-0.2496 µg/L	0.75780	-0.2496 ppb	0.75780	303.64%
QC value within limits for Ag 328.068 Recovery = Not calculated						
Al 396.153Radial†	-14.0	-3.0809 µg/L	2.97697	-3.0809 ppb	2.97697	96.63%
QC value within limits for Al 396.153Radial Recovery = Not calculated						
As 188.979†	-2.1	-0.8618 µg/L	3.13716	-0.8618 ppb	3.13716	364.04%
QC value within limits for As 188.979 Recovery = Not calculated						
B 249.677†	-152.2	-2.5560 µg/L	0.21918	-2.5560 ppb	0.21918	8.58%
QC value within limits for B 249.677 Recovery = Not calculated						
Ba 233.527†	18.2	0.0834 µg/L	0.04516	0.0834 ppb	0.04516	54.17%
QC value within limits for Ba 233.527 Recovery = Not calculated						
Be 313.107†	110.5	0.0386 µg/L	0.04296	0.0386 ppb	0.04296	111.35%
QC value within limits for Be 313.107 Recovery = Not calculated						
Ca 317.933Radial†	-14.7	-0.8613 µg/L	0.92961	-0.8613 ppb	0.92961	107.93%
QC value within limits for Ca 317.933Radial Recovery = Not calculated						
Cd 226.502†	5.3	0.0364 µg/L	0.13959	0.0364 ppb	0.13959	383.42%
QC value within limits for Cd 226.502 Recovery = Not calculated						

Co 228.616†	21.9	0.2996 µg/L	0.29720	0.2996 ppb	0.29720	99.21%
QC value within limits for Co 228.616 Recovery = Not calculated						
Cr 267.716†	6.0	0.0447 µg/L	0.13112	0.0447 ppb	0.13112	293.47%
QC value within limits for Cr 267.716 Recovery = Not calculated						
Cu 324.752†	-12.9	-0.0489 µg/L	0.41746	-0.0489 ppb	0.41746	854.27%
QC value within limits for Cu 324.752 Recovery = Not calculated						
Fe 238.204 Radial†	18.4	1.2233 µg/L	0.34099	1.2233 ppb	0.34099	27.88%
QC value within limits for Fe 238.204 Radial Recovery = Not calculated						
K 766.490 Radial†	32.1	13.222 µg/L	14.5294	13.222 ppb	14.5294	109.89%
QC value within limits for K 766.490 Radial Recovery = Not calculated						
Mg 279.077 IEC†	-11.2	-4.5853 µg/L	6.81203	-4.5853 ppb	6.81203	148.56%
QC value within limits for Mg 279.077 IEC Recovery = Not calculated						
Mn 257.610†	74.0	0.1013 µg/L	0.01630	0.1013 ppb	0.01630	16.09%
QC value within limits for Mn 257.610 Recovery = Not calculated						
Mo 202.031†	18.4	0.5800 µg/L	0.30975	0.5800 ppb	0.30975	53.40%
QC value within limits for Mo 202.031 Recovery = Not calculated						
Na 589.592 Radial†	-132.9	-20.353 µg/L	6.2604	-20.353 ppb	6.2604	30.76%
QC value within limits for Na 589.592 Radial Recovery = Not calculated						
Ni 231.604†	-25.5	-0.3257 µg/L	0.14010	-0.3257 ppb	0.14010	43.01%
QC value within limits for Ni 231.604 Recovery = Not calculated						
P 214.914†	-4.1	-0.9865 µg/L	1.37705	-0.9865 ppb	1.37705	139.59%
QC value within limits for P 214.914 Recovery = Not calculated						
Pb 220.353†	-1.8	-0.1146 µg/L	1.41489	-0.1146 ppb	1.41489	>999.9%
QC value within limits for Pb 220.353 Recovery = Not calculated						
S 181.975 Axial†	-7.5	-6.0387 µg/L	4.86046	-6.0387 ppb	4.86046	80.49%
QC value within limits for S 181.975 Axial Recovery = Not calculated						
Sb 206.836†	-14.5	-1.9465 µg/L	0.31193	-1.9465 ppb	0.31193	16.03%
QC value within limits for Sb 206.836 Recovery = Not calculated						
Se 196.026†	14.1	5.57 µg/L	1.688	5.57 ppb	1.688	30.30%
QC value within limits for Se 196.026 Recovery = Not calculated						
SiO2†	11.4	1.2252 µg/L	1.15483	1.2252 ppb	1.15483	94.25%
QC value within limits for SiO2 Recovery = Not calculated						
Si 251.611†	79.9	1.3121 µg/L	0.32896	1.3121 ppb	0.32896	25.07%
QC value within limits for Si 251.611 Recovery = Not calculated						
Sn 189.927†	1.3	0.0938 µg/L	0.17571	0.0938 ppb	0.17571	187.29%
QC value within limits for Sn 189.927 Recovery = Not calculated						
Sr 421.552†	87.8	0.2058 µg/L	0.14923	0.2058 ppb	0.14923	72.50%
QC value within limits for Sr 421.552 Recovery = Not calculated						
Ti 334.940†	107.7	0.1067 µg/L	0.17474	0.1067 ppb	0.17474	163.81%
QC value within limits for Ti 334.940 Recovery = Not calculated						
Tl 190.801†	0.0	-0.0017 µg/L	0.68072	-0.0017 ppb	0.68072	>999.9%
QC value within limits for Tl 190.801 Recovery = Not calculated						
U 409.014†	139.7	8.6193 µg/L	7.84577	8.6193 ppb	7.84577	91.03%
QC value within limits for U 409.014 Recovery = Not calculated						
V 292.402†	-37.4	-0.1957 µg/L	0.61936	-0.1957 ppb	0.61936	316.55%
QC value within limits for V 292.402 Recovery = Not calculated						
Zn 213.857†	-7.2	-0.0435 µg/L	0.06758	-0.0435 ppb	0.06758	155.53%
QC value within limits for Zn 213.857 Recovery = Not calculated						

All analyte(s) passed QC.

Sequence No.: 8

Sample ID: PQL

Analyst:

Logged In Analyst (Original) : optima4

Initial Sample Wt:

Dilution:

Autosampler Location: 101

Date Collected: 3/29/2010 18:40:43

Data Type: Reprocessed on 3/29/2010 19:14:37

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: PQL

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc 361.383	1721442.6	1721442.6	102.91 %		18:41:40
1	Sc RADIAL	147903.8	147903.8	101 %		18:41:13
1	Y 371.029	1058404.9	1058404.9	103.50 %		18:41:40
1	Ag 328.068†	4025.6	944.7	3.9659 µg/L	3.9659 ppb	18:41:43
1	Al 396.153Radial†	922.6	941.1	204.98 µg/L	204.98 ppb	18:41:15
1	As 188.979†	70.2	82.5	34.551 µg/L	34.551 ppb	18:42:03
1	B 249.677†	6252.3	2719.8	45.645 µg/L	45.645 ppb	18:41:43
1	Ba 233.527†	968.6	1116.3	5.1042 µg/L	5.1042 ppb	18:42:03
1	Be 313.107†	14893.3	15132.4	4.9477 µg/L	4.9477 ppb	18:41:43
1	Ca 317.933Radial†	4243.5	3565.6	208.93 µg/L	208.93 ppb	18:41:15
1	Cd 226.502†	637.3	713.7	4.9197 µg/L	4.9197 ppb	18:42:03
1	Co 228.616†	202.6	373.5	5.1141 µg/L	5.1141 ppb	18:42:03
1	Cr 267.716†	729.0	548.1	4.6505 µg/L	4.6505 ppb	18:42:03
1	Cu 324.752†	4895.4	2332.1	10.224 µg/L	10.224 ppb	18:41:43
1	Fe 238.204 Radial†	1705.5	1567.4	104.21 µg/L	104.21 ppb	18:41:15
1	K 766.490 Radial†	1904.1	421.4	173.34 µg/L	173.34 ppb	18:41:13
1	Mg 279.077 IEC†	935.0	734.7	303.09 µg/L	303.09 ppb	18:41:15
1	Mn 257.610†	7824.8	7523.6	10.268 µg/L	10.268 ppb	18:41:43
1	Mo 202.031†	258.6	306.5	9.6870 µg/L	9.6870 ppb	18:42:03
1	Na 589.592 Radial†	3412.3	1667.9	255.06 µg/L	255.06 ppb	18:41:15
1	Ni 231.604†	353.8	384.7	4.9210 µg/L	4.9210 ppb	18:42:03
1	P 214.914†	701.3	601.9	143.99 µg/L	143.99 ppb	18:42:03
1	Pb 220.353†	285.3	164.8	9.9640 µg/L	9.9640 ppb	18:42:03
1	S 181.975 Axial†	217.5	116.6	94.518 µg/L	94.518 ppb	18:42:03
1	Sb 206.836†	151.7	60.8	8.2873 µg/L	8.2873 ppb	18:42:03
1	Se 196.026†	93.5	79.9	31.7 µg/L	31.7 ppb	18:42:03
1	SiO2†	3528.6	1856.0	202.45 µg/L	202.45 ppb	18:41:43
1	Si 251.611†	7008.2	6133.7	101.23 µg/L	101.23 ppb	18:41:43
1	Sn 189.927†	141.3	135.3	9.6379 µg/L	9.6379 ppb	18:42:03
1	Sr 421.552†	2328.3	2572.4	6.0274 µg/L	6.0274 ppb	18:41:15
1	Ti 334.940†	5694.2	4896.9	4.9428 µg/L	4.9428 ppb	18:41:43
1	Tl 190.801†	28.4	147.9	19.934 µg/L	19.934 ppb	18:42:03
1	U 409.014†	713.0	1172.0	72.715 µg/L	72.715 ppb	18:41:43
1	V 292.402†	1246.9	779.8	4.4736 µg/L	4.4736 ppb	18:41:43
1	Zn 213.857†	2077.4	1554.3	9.7365 µg/L	9.7365 ppb	18:42:03
2	Sc 361.383	1724623.2	1724623.2	103.10 %		18:42:05
2	Sc RADIAL	148676.2	148676.2	102 %		18:41:17
2	Y 371.029	1060877.7	1060877.7	103.75 %		18:42:05
2	Ag 328.068†	4441.5	1340.9	5.5444 µg/L	5.5444 ppb	18:42:07
2	Al 396.153Radial†	882.0	896.6	195.25 µg/L	195.25 ppb	18:41:19
2	As 188.979†	60.0	72.5	30.385 µg/L	30.385 ppb	18:42:27
2	B 249.677†	6195.0	2653.1	44.524 µg/L	44.524 ppb	18:42:07
2	Ba 233.527†	972.4	1118.3	5.1130 µg/L	5.1130 ppb	18:42:27
2	Be 313.107†	15035.6	15243.7	4.9775 µg/L	4.9775 ppb	18:42:07
2	Ca 317.933Radial†	4053.9	3358.0	196.76 µg/L	196.76 ppb	18:41:19
2	Cd 226.502†	642.0	717.1	4.9432 µg/L	4.9432 ppb	18:42:27
2	Co 228.616†	195.2	365.9	5.0104 µg/L	5.0104 ppb	18:42:27
2	Cr 267.716†	741.9	559.4	4.7640 µg/L	4.7640 ppb	18:42:27
2	Cu 324.752†	4804.6	2235.3	9.7851 µg/L	9.7851 ppb	18:42:07
2	Fe 238.204 Radial†	1689.7	1543.2	102.60 µg/L	102.60 ppb	18:41:19
2	K 766.490 Radial†	1941.0	447.8	184.20 µg/L	184.20 ppb	18:41:17
2	Mg 279.077 IEC†	934.9	729.8	301.08 µg/L	301.08 ppb	18:41:19
2	Mn 257.610†	7840.1	7524.4	10.269 µg/L	10.269 ppb	18:42:07
2	Mo 202.031†	268.7	315.9	9.9813 µg/L	9.9813 ppb	18:42:27
2	Na 589.592 Radial†	3585.8	1820.6	278.41 µg/L	278.41 ppb	18:41:19
2	Ni 231.604†	360.6	390.7	4.9969 µg/L	4.9969 ppb	18:42:27
2	P 214.914†	704.9	604.1	144.53 µg/L	144.53 ppb	18:42:27
2	Pb 220.353†	256.9	136.7	8.2831 µg/L	8.2831 ppb	18:42:27

2	S 181.975 Axial†	211.0	109.8	89.075 µg/L	89.075 ppb	18:42:27
2	Sb 206.836†	139.1	48.3	6.6025 µg/L	6.6025 ppb	18:42:27
2	Se 196.026†	85.2	71.7	28.4 µg/L	28.4 ppb	18:42:27
2	SiO2†	3666.3	1983.3	216.34 µg/L	216.34 ppb	18:42:07
2	Si 251.611†	6987.0	6100.5	100.67 µg/L	100.67 ppb	18:42:07
2	Sn 189.927†	148.9	142.4	10.142 µg/L	10.142 ppb	18:42:27
2	Sr 421.552†	2257.8	2491.4	5.8378 µg/L	5.8378 ppb	18:41:19
2	Ti 334.940†	5599.5	4794.8	4.8474 µg/L	4.8474 ppb	18:42:07
2	Tl 190.801†	28.5	147.9	19.938 µg/L	19.938 ppb	18:42:27
2	U 409.014†	356.1	824.5	51.229 µg/L	51.229 ppb	18:42:07
2	V 292.402†	1199.8	731.9	4.1969 µg/L	4.1969 ppb	18:42:07
2	Zn 213.857†	2110.9	1583.0	9.9172 µg/L	9.9172 ppb	18:42:27
3	Sc 361.383	1709181.0	1709181.0	102.18 %		18:42:29
3	Sc RADIAL	148765.1	148765.1	102 %		18:41:21
3	Y 371.029	1051117.1	1051117.1	102.79 %		18:42:29
3	Ag 328.068†	4096.5	1042.2	4.3518 µg/L	4.3518 ppb	18:42:31
3	Al 396.153Radial†	913.9	927.3	201.93 µg/L	201.93 ppb	18:41:23
3	As 188.979†	45.1	58.4	24.503 µg/L	24.503 ppb	18:42:51
3	B 249.677†	6365.0	2873.8	48.229 µg/L	48.229 ppb	18:42:31
3	Ba 233.527†	993.8	1147.7	5.2479 µg/L	5.2479 ppb	18:42:51
3	Be 313.107†	15404.4	15736.4	5.1406 µg/L	5.1406 ppb	18:42:31
3	Ca 317.933Radial†	4204.3	3503.0	205.26 µg/L	205.26 ppb	18:41:23
3	Cd 226.502†	656.9	737.3	5.0831 µg/L	5.0831 ppb	18:42:51
3	Co 228.616†	214.1	386.1	5.2868 µg/L	5.2868 ppb	18:42:51
3	Cr 267.716†	776.9	600.1	5.1070 µg/L	5.1070 ppb	18:42:51
3	Cu 324.752†	4905.4	2376.0	10.405 µg/L	10.405 ppb	18:42:31
3	Fe 238.204 Radial†	1701.7	1554.0	103.31 µg/L	103.31 ppb	18:41:23
3	K 766.490 Radial†	1863.7	371.0	152.58 µg/L	152.58 ppb	18:41:21
3	Mg 279.077 IEC†	946.2	740.4	305.43 µg/L	305.43 ppb	18:41:23
3	Mn 257.610†	7932.9	7683.9	10.487 µg/L	10.487 ppb	18:42:31
3	Mo 202.031†	276.9	326.2	10.308 µg/L	10.308 ppb	18:42:51
3	Na 589.592 Radial†	3380.4	1617.2	247.32 µg/L	247.32 ppb	18:41:23
3	Ni 231.604†	372.2	405.1	5.1823 µg/L	5.1823 ppb	18:42:51
3	P 214.914†	693.9	599.5	143.42 µg/L	143.42 ppb	18:42:51
3	Pb 220.353†	299.1	180.3	10.914 µg/L	10.914 ppb	18:42:51
3	S 181.975 Axial†	216.9	117.4	95.241 µg/L	95.241 ppb	18:42:51
3	Sb 206.836†	178.2	87.8	11.935 µg/L	11.935 ppb	18:42:51
3	Se 196.026†	84.3	71.6	28.4 µg/L	28.4 ppb	18:42:51
3	SiO2†	3665.9	2015.0	219.80 µg/L	219.80 ppb	18:42:31
3	Si 251.611†	7292.1	6460.4	106.62 µg/L	106.62 ppb	18:42:31
3	Sn 189.927†	146.0	140.9	10.035 µg/L	10.035 ppb	18:42:51
3	Sr 421.552†	2185.8	2419.5	5.6692 µg/L	5.6692 ppb	18:41:23
3	Ti 334.940†	5763.7	5004.6	5.0573 µg/L	5.0573 ppb	18:42:31
3	Tl 190.801†	37.2	156.7	21.117 µg/L	21.117 ppb	18:42:51
3	U 409.014†	504.2	972.6	60.421 µg/L	60.421 ppb	18:42:31
3	V 292.402†	1321.2	861.3	4.9254 µg/L	4.9254 ppb	18:42:31
3	Zn 213.857†	2122.4	1612.8	10.103 µg/L	10.103 ppb	18:42:51

Mean Data: PQL

Analyte	Mean Corrected Intensity	Conc. Units	Calib. Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1718415.6	102.73 %	0.487			0.47%
Sc RADIAL	148448.4	102 %	0.3			0.32%
Y 371.029	1056799.9	103.35 %	0.496			0.48%
Ag 328.068†	1109.3	4.6207 µg/L	0.82285	4.6207 ppb	0.82285	17.81%
QC value within limits for Ag 328.068 Recovery = 92.41%						
Al 396.153Radial†	921.7	200.72 µg/L	4.978	200.72 ppb	4.978	2.48%
QC value within limits for Al 396.153Radial Recovery = 100.36%						
As 188.979†	71.1	29.813 µg/L	5.0483	29.813 ppb	5.0483	16.93%
QC value within limits for As 188.979 Recovery = 99.38%						
B 249.677†	2748.9	46.133 µg/L	1.8998	46.133 ppb	1.8998	4.12%
QC value within limits for B 249.677 Recovery = 92.27%						
Ba 233.527†	1127.4	5.1550 µg/L	0.08056	5.1550 ppb	0.08056	1.56%
QC value within limits for Ba 233.527 Recovery = 103.10%						
Be 313.107†	15370.8	5.0219 µg/L	0.10386	5.0219 ppb	0.10386	2.07%
QC value within limits for Be 313.107 Recovery = 100.44%						
Ca 317.933Radial†	3475.5	203.65 µg/L	6.241	203.65 ppb	6.241	3.06%
QC value within limits for Ca 317.933Radial Recovery = 101.83%						
Cd 226.502†	722.7	4.9820 µg/L	0.08834	4.9820 ppb	0.08834	1.77%
QC value within limits for Cd 226.502 Recovery = 99.64%						

Co 228.616†	375.2	5.1371 µg/L	0.13962	5.1371 ppb	0.13962	2.72%
QC value within limits for Co 228.616 Recovery = 102.74%						
Cr 267.716†	569.2	4.8405 µg/L	0.23770	4.8405 ppb	0.23770	4.91%
QC value within limits for Cr 267.716 Recovery = 96.81%						
Cu 324.752†	2314.5	10.138 µg/L	0.3187	10.138 ppb	0.3187	3.14%
QC value within limits for Cu 324.752 Recovery = 101.38%						
Fe 238.204 Radial†	1554.9	103.37 µg/L	0.806	103.37 ppb	0.806	0.78%
QC value within limits for Fe 238.204 Radial Recovery = 103.37%						
K 766.490 Radial†	413.4	170.04 µg/L	16.070	170.04 ppb	16.070	9.45%
QC value within limits for K 766.490 Radial Recovery = 113.36%						
Mg 279.077 IEC†	735.0	303.20 µg/L	2.180	303.20 ppb	2.180	0.72%
QC value within limits for Mg 279.077 IEC Recovery = 101.07%						
Mn 257.610†	7577.3	10.342 µg/L	0.1261	10.342 ppb	0.1261	1.22%
QC value within limits for Mn 257.610 Recovery = 103.42%						
Mo 202.031†	316.2	9.9921 µg/L	0.31074	9.9921 ppb	0.31074	3.11%
QC value within limits for Mo 202.031 Recovery = 99.92%						
Na 589.592 Radial†	1701.9	260.27 µg/L	16.186	260.27 ppb	16.186	6.22%
QC value within limits for Na 589.592 Radial Recovery = 86.76%						
Ni 231.604†	393.5	5.0334 µg/L	0.13439	5.0334 ppb	0.13439	2.67%
QC value within limits for Ni 231.604 Recovery = 100.67%						
P 214.914†	601.9	143.98 µg/L	0.554	143.98 ppb	0.554	0.38%
QC value within limits for P 214.914 Recovery = 95.99%						
Pb 220.353†	160.6	9.7204 µg/L	1.33235	9.7204 ppb	1.33235	13.71%
QC value within limits for Pb 220.353 Recovery = 97.20%						
S 181.975 Axial†	114.6	92.945 µg/L	3.3708	92.945 ppb	3.3708	3.63%
QC value within limits for S 181.975 Axial Recovery = 92.94%						
Sb 206.836†	65.6	8.9415 µg/L	2.72562	8.9415 ppb	2.72562	30.48%
QC value within limits for Sb 206.836 Recovery = 89.41%						
Se 196.026†	74.4	29.5 µg/L	1.90	29.5 ppb	1.90	6.42%
QC value within limits for Se 196.026 Recovery = 98.43%						
SiO2†	1951.4	212.86 µg/L	9.186	212.86 ppb	9.186	4.32%
QC value within limits for SiO2 Recovery = 99.94%						
Si 251.611†	6231.5	102.84 µg/L	3.285	102.84 ppb	3.285	3.19%
QC value within limits for Si 251.611 Recovery = 102.84%						
Sn 189.927†	139.6	9.9381 µg/L	0.26552	9.9381 ppb	0.26552	2.67%
QC value within limits for Sn 189.927 Recovery = 99.38%						
Sr 421.552†	2494.5	5.8448 µg/L	0.17922	5.8448 ppb	0.17922	3.07%
QC value within limits for Sr 421.552 Recovery = 116.90%						
Ti 334.940†	4898.8	4.9492 µg/L	0.10510	4.9492 ppb	0.10510	2.12%
QC value within limits for Ti 334.940 Recovery = 98.98%						
Tl 190.801†	150.8	20.330 µg/L	0.6817	20.330 ppb	0.6817	3.35%
QC value within limits for Tl 190.801 Recovery = 101.65%						
U 409.014†	989.7	61.455 µg/L	10.7804	61.455 ppb	10.7804	17.54%
QC value within limits for U 409.014 Recovery = 122.91%						
V 292.402†	791.0	4.5320 µg/L	0.36774	4.5320 ppb	0.36774	8.11%
QC value within limits for V 292.402 Recovery = 90.64%						
Zn 213.857†	1583.4	9.9190 µg/L	0.18336	9.9190 ppb	0.18336	1.85%
QC value within limits for Zn 213.857 Recovery = 99.19%						
All analyte(s) passed QC.						

Sequence No.: 9
 Sample ID: IC5A
 Analyst:
 Logged In Analyst (Original) : optima4
 Initial Sample Wt:
 Dilution:

Autosampler Location: 103
 Date Collected: 3/29/2010 18:43:01
 Data Type: Reprocessed on 3/29/2010 19:14:38
 Initial Sample Vol:
 Sample Prep Vol:

Replicate Data: IC5A

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc 361.383	1519975.5	1519975.5	90.866 %		18:44:01
1	Sc RADIAL	137750.3	137750.3	94.5 %		18:43:34
1	Y 371.029	919968.6	919968.6	89.965 %		18:44:01
1	Ag 328.068†	5916.7	3544.4	1.2267 µg/L	1.2267 ppb	18:44:01
1	Al 396.153Radial†	2228558.9	2358079.9	514740 µg/L	514740 ppb	18:43:31
1	As 188.979†	-88.3	-82.9	8.1301 µg/L	8.1301 ppb	18:44:21
1	B 249.677†	3032.6	-18.3	-0.3191 µg/L	-0.3191 ppb	18:44:01
1	Ba 233.527†	439.8	659.1	0.5804 µg/L	0.5804 ppb	18:44:21
1	Be 313.107†	-620.0	-22.3	0.0066 µg/L	0.0066 ppb	18:44:01
1	Ca 317.933Radial†	7783821.6	8235480.1	482560 µg/L	482560 ppb	18:43:31
1	Cd 226.502†	2257.8	2579.2	-2.2506 µg/L	-2.2506 ppb	18:44:21
1	Co 228.616†	76.3	260.5	-6.3814 µg/L	-6.3814 ppb	18:44:21
1	Cr 267.716†	306.4	176.9	2.2002 µg/L	2.2002 ppb	18:44:21
1	Cu 324.752†	-6875.9	-9992.0	-2.5122 µg/L	-2.5122 ppb	18:44:01
1	Fe 238.204 Radial†	2712004.8	2869471.1	190770 µg/L	190770 ppb	18:43:31
1	K 766.490 Radial†	1538.5	172.9	-171.54 µg/L	-171.54 ppb	18:43:34
1	Mg 279.077 IEC†	1111575.2	1175976.0	484700 µg/L	484700 ppb	18:43:31
1	Mn 257.610†	14620.3	16010.1	2.1476 µg/L	2.1476 ppb	18:44:01
1	Mo 202.031†	-501.7	-496.9	0.7251 µg/L	0.7251 ppb	18:44:01
1	Na 589.592 Radial†	1635.3	35.6	5.3873 µg/L	5.3873 ppb	18:43:34
1	Ni 231.604†	146.0	201.6	2.5791 µg/L	2.5791 ppb	18:44:21
1	P 214.914†	148.1	83.5	4.8563 µg/L	4.8563 ppb	18:44:21
1	Pb 220.353†	-247.5	-384.9	2.4276 µg/L	2.4276 ppb	18:44:21
1	S 181.975 Axial†	166.5	88.4	71.471 µg/L	71.471 ppb	18:44:21
1	Sb 206.836†	109.8	34.2	-1.4541 µg/L	-1.4541 ppb	18:44:21
1	Se 196.026†	-143.9	-169.3	-0.728 µg/L	-0.728 ppb	18:44:21
1	SiO2†	1500.4	78.4	8.9950 µg/L	8.9950 ppb	18:44:21
1	Si 251.611†	379.6	-258.7	-4.0756 µg/L	-4.0756 ppb	18:44:21
1	Sn 189.927†	17.0	16.7	1.2650 µg/L	1.2650 ppb	18:44:21
1	Sr 421.552†	1360.0	1717.1	0.2472 µg/L	0.2472 ppb	18:43:34
1	Ti 334.940†	20973.2	22445.2	-4.0421 µg/L	-4.0421 ppb	18:44:01
1	Tl 190.801†	-165.7	-62.0	-7.8287 µg/L	-7.8287 ppb	18:44:21
1	U 409.014†	239.9	743.1	25.180 µg/L	25.180 ppb	18:44:01
1	V 292.402†	5463.3	5580.7	0.4848 µg/L	0.4848 ppb	18:44:01
1	Zn 213.857†	3868.4	3792.8	7.6857 µg/L	7.6857 ppb	18:44:21
2	Sc 361.383	1532514.6	1532514.6	91.615 %		18:44:24
2	Sc RADIAL	139244.5	139244.5	95.5 %		18:43:38
2	Y 371.029	927898.5	927898.5	90.741 %		18:44:24
2	Ag 328.068†	5725.2	3282.1	0.2956 µg/L	0.2956 ppb	18:44:24
2	Al 396.153Radial†	2228857.8	2333088.7	509290 µg/L	509290 ppb	18:43:36
2	As 188.979†	-96.0	-90.5	4.5139 µg/L	4.5139 ppb	18:44:44
2	B 249.677†	3203.6	141.1	2.3574 µg/L	2.3574 ppb	18:44:24
2	Ba 233.527†	417.7	631.0	0.4768 µg/L	0.4768 ppb	18:44:44
2	Be 313.107†	-855.2	-273.4	-0.0781 µg/L	-0.0781 ppb	18:44:24
2	Ca 317.933Radial†	7791433.2	8155066.3	477850 µg/L	477850 ppb	18:43:36
2	Cd 226.502†	2233.3	2532.1	-2.3767 µg/L	-2.3767 ppb	18:44:44
2	Co 228.616†	66.6	249.3	-6.4368 µg/L	-6.4368 ppb	18:44:44
2	Cr 267.716†	246.3	108.6	1.6057 µg/L	1.6057 ppb	18:44:44
2	Cu 324.752†	-6872.9	-9926.8	-2.6212 µg/L	-2.6212 ppb	18:44:24
2	Fe 238.204 Radial†	2714288.8	2841068.4	188880 µg/L	188880 ppb	18:43:36
2	K 766.490 Radial†	1618.0	238.7	-142.04 µg/L	-142.04 ppb	18:43:38
2	Mg 279.077 IEC†	1114260.0	1166165.0	480660 µg/L	480660 ppb	18:43:36
2	Mn 257.610†	14586.8	15841.8	2.0830 µg/L	2.0830 ppb	18:44:24
2	Mo 202.031†	-508.1	-499.4	0.4957 µg/L	0.4957 ppb	18:44:24
2	Na 589.592 Radial†	1714.1	99.5	15.141 µg/L	15.141 ppb	18:43:38
2	Ni 231.604†	152.3	207.2	2.6500 µg/L	2.6500 ppb	18:44:44
2	P 214.914†	105.5	35.5	-6.5606 µg/L	-6.5606 ppb	18:44:44
2	Pb 220.353†	-290.5	-429.6	-0.5500 µg/L	-0.5500 ppb	18:44:44

2	S 181.975 Axial†	171.6	92.5	74.799 µg/L	74.799 ppb	18:44:44
2	Sb 206.836†	130.7	56.0	1.5606 µg/L	1.5606 ppb	18:44:44
2	Se 196.026†	-155.0	-180.1	-5.67 µg/L	-5.67 ppb	18:44:44
2	SiO2†	1504.6	69.4	8.0425 µg/L	8.0425 ppb	18:44:44
2	Si 251.611†	375.1	-267.0	-4.2014 µg/L	-4.2014 ppb	18:44:44
2	Sn 189.927†	-4.2	-6.6	-0.3924 µg/L	-0.3924 ppb	18:44:44
2	Sr 421.552†	1366.5	1708.4	0.2637 µg/L	0.2637 ppb	18:43:38
2	Ti 334.940†	21214.1	22519.4	-3.7556 µg/L	-3.7556 ppb	18:44:24
2	Tl 190.801†	-155.0	-48.9	-6.0537 µg/L	-6.0537 ppb	18:44:44
2	U 409.014†	96.2	584.1	15.646 µg/L	15.646 ppb	18:44:24
2	V 292.402†	5684.6	5773.1	1.8417 µg/L	1.8417 ppb	18:44:24
2	Zn 213.857†	3858.3	3747.0	7.5506 µg/L	7.5506 ppb	18:44:44
3	Sc 361.383	1531662.1	1531662.1	91.564 %		18:44:46
3	Sc RADIAL	139848.7	139848.7	95.9 %		18:43:42
3	Y 371.029	927170.5	927170.5	90.670 %		18:44:46
3	Ag 328.068†	5762.9	3326.8	0.5251 µg/L	0.5251 ppb	18:44:46
3	Al 396.153Radial†	2231390.2	2325648.7	507660 µg/L	507660 ppb	18:43:40
3	As 188.979†	-103.4	-98.7	0.8735 µg/L	0.8735 ppb	18:45:06
3	B 249.677†	3235.4	177.8	2.9710 µg/L	2.9710 ppb	18:44:46
3	Ba 233.527†	402.4	614.5	0.4137 µg/L	0.4137 ppb	18:45:06
3	Be 313.107†	-678.3	-80.7	-0.0209 µg/L	-0.0209 ppb	18:44:46
3	Ca 317.933Radial†	7787439.6	8115669.6	475540 µg/L	475540 ppb	18:43:40
3	Cd 226.502†	2245.5	2546.8	-2.1709 µg/L	-2.1709 ppb	18:45:06
3	Co 228.616†	93.2	278.4	-5.9871 µg/L	-5.9871 ppb	18:45:06
3	Cr 267.716†	275.9	141.1	1.8999 µg/L	1.8999 ppb	18:45:06
3	Cu 324.752†	-6732.3	-9777.4	-2.2074 µg/L	-2.2074 ppb	18:44:46
3	Fe 238.204 Radial†	2711795.4	2826195.2	187900 µg/L	187900 ppb	18:43:40
3	K 766.490 Radial†	1584.0	195.9	-158.63 µg/L	-158.63 ppb	18:43:42
3	Mg 279.077 IEC†	1112495.6	1159287.1	477830 µg/L	477830 ppb	18:43:40
3	Mn 257.610†	14462.2	15714.6	2.0242 µg/L	2.0242 ppb	18:44:46
3	Mo 202.031†	-593.4	-592.8	-2.5422 µg/L	-2.5422 ppb	18:44:46
3	Na 589.592 Radial†	1732.7	111.2	16.939 µg/L	16.939 ppb	18:43:42
3	Ni 231.604†	209.1	269.3	3.4450 µg/L	3.4450 ppb	18:45:06
3	P 214.914†	118.4	49.8	-2.8056 µg/L	-2.8056 ppb	18:45:06
3	Pb 220.353†	-264.9	-401.8	1.0704 µg/L	1.0704 ppb	18:45:06
3	S 181.975 Axial†	171.3	92.2	74.546 µg/L	74.546 ppb	18:45:06
3	Sb 206.836†	101.8	24.6	-2.6986 µg/L	-2.6986 ppb	18:45:06
3	Se 196.026†	-151.8	-176.7	-4.70 µg/L	-4.70 ppb	18:45:06
3	SiO2†	1457.7	19.2	2.6178 µg/L	2.6178 ppb	18:45:06
3	Si 251.611†	375.6	-266.2	-4.1555 µg/L	-4.1555 ppb	18:45:06
3	Sn 189.927†	9.2	8.1	0.6527 µg/L	0.6527 ppb	18:45:06
3	Sr 421.552†	1404.5	1741.8	0.3601 µg/L	0.3601 ppb	18:43:42
3	Ti 334.940†	21500.8	22845.3	-3.2450 µg/L	-3.2450 ppb	18:44:46
3	Tl 190.801†	-148.3	-41.6	-5.0807 µg/L	-5.0807 ppb	18:45:06
3	U 409.014†	-176.5	286.3	-2.6068 µg/L	-2.6068 ppb	18:44:46
3	V 292.402†	5753.1	5851.3	2.3911 µg/L	2.3911 ppb	18:44:46
3	Zn 213.857†	3845.3	3735.2	7.5699 µg/L	7.5699 ppb	18:45:06

Mean Data: ICSEA

Analyte	Mean Corrected Intensity	Conc. Units	Calib. Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1528050.7	91.348 %	0.4188			0.46%
Sc RADIAL	138947.9	95.3 %	0.74			0.78%
Y 371.029	925012.6	90.459 %	0.4287			0.47%
Ag 328.068†	3384.5	0.6825 µg/L	0.48505	0.6825 ppb	0.48505	71.07%
QC value within limits for Ag 328.068 Recovery = Not calculated						
Al 396.153Radial†	2338939.1	510560 µg/L	3708.4	510560 ppb	3708.4	0.73%
QC value within limits for Al 396.153Radial Recovery = 102.11%						
As 188.979†	-90.7	4.5059 µg/L	3.62830	4.5059 ppb	3.62830	80.52%
QC value within limits for As 188.979 Recovery = Not calculated						
B 249.677†	100.2	1.6697 µg/L	1.74948	1.6697 ppb	1.74948	104.78%
QC value within limits for B 249.677 Recovery = Not calculated						
Ba 233.527†	634.8	0.4903 µg/L	0.08415	0.4903 ppb	0.08415	17.16%
QC value within limits for Ba 233.527 Recovery = Not calculated						
Be 313.107†	-125.5	-0.0308 µg/L	0.04321	-0.0308 ppb	0.04321	140.33%
QC value within limits for Be 313.107 Recovery = Not calculated						
Ca 317.933Radial†	8168738.7	478650 µg/L	3578.1	478650 ppb	3578.1	0.75%
QC value within limits for Ca 317.933Radial Recovery = 95.73%						
Cd 226.502†	2552.7	-2.2661 µg/L	0.10379	-2.2661 ppb	0.10379	4.58%
QC value within limits for Cd 226.502 Recovery = Not calculated						

Co 228.616†	262.7	-6.2685 µg/L	0.24520	-6.2685 ppb	0.24520	3.91%
QC value within limits for Co 228.616 Recovery = Not calculated						
Cr 267.716†	142.2	1.9019 µg/L	0.29723	1.9019 ppb	0.29723	15.63%
QC value within limits for Cr 267.716 Recovery = Not calculated						
Cu 324.752†	-9898.7	-2.4469 µg/L	0.21446	-2.4469 ppb	0.21446	8.76%
QC value within limits for Cu 324.752 Recovery = Not calculated						
Fe 238.204 Radial†	2845578.2	189180 µg/L	1461.8	189180 ppb	1461.8	0.77%
QC value within limits for Fe 238.204 Radial Recovery = 94.59%						
K 766.490 Radial†	202.5	-157.40 µg/L	14.790	-157.40 ppb	14.790	9.40%
QC value within limits for K 766.490 Radial Recovery = Not calculated						
Mg 279.077 IEC†	1167142.7	481060 µg/L	3456.9	481060 ppb	3456.9	0.72%
QC value within limits for Mg 279.077 IEC Recovery = 96.21%						
Mn 257.610†	15855.5	2.0849 µg/L	0.06170	2.0849 ppb	0.06170	2.96%
QC value within limits for Mn 257.610 Recovery = Not calculated						
Mo 202.031†	-529.7	-0.4405 µg/L	1.82378	-0.4405 ppb	1.82378	414.05%
QC value within limits for Mo 202.031 Recovery = Not calculated						
Na 589.592 Radial†	82.1	12.489 µg/L	6.2157	12.489 ppb	6.2157	49.77%
QC value within limits for Na 589.592 Radial Recovery = Not calculated						
Ni 231.604†	226.0	2.8914 µg/L	0.48079	2.8914 ppb	0.48079	16.63%
QC value within limits for Ni 231.604 Recovery = Not calculated						
P 214.914†	56.3	-1.5033 µg/L	5.81883	-1.5033 ppb	5.81883	387.07%
QC value within limits for P 214.914 Recovery = Not calculated						
Pb 220.353†	-405.4	0.9827 µg/L	1.49074	0.9827 ppb	1.49074	151.70%
QC value within limits for Pb 220.353 Recovery = Not calculated						
S 181.975 Axial†	91.0	73.605 µg/L	1.8528	73.605 ppb	1.8528	2.52%
QC value within limits for S 181.975 Axial Recovery = Not calculated						
Sb 206.836†	38.3	-0.8640 µg/L	2.19006	-0.8640 ppb	2.19006	253.47%
QC value within limits for Sb 206.836 Recovery = Not calculated						
Se 196.026†	-175.4	-3.70 µg/L	2.618	-3.70 ppb	2.618	70.77%
QC value within limits for Se 196.026 Recovery = Not calculated						
SiO2†	55.7	6.5518 µg/L	3.44005	6.5518 ppb	3.44005	52.51%
QC value within limits for SiO2 Recovery = Not calculated						
Si 251.611†	-264.0	-4.1441 µg/L	0.06368	-4.1441 ppb	0.06368	1.54%
QC value within limits for Si 251.611 Recovery = Not calculated						
Sn 189.927†	6.1	0.5084 µg/L	0.83805	0.5084 ppb	0.83805	164.84%
QC value within limits for Sn 189.927 Recovery = Not calculated						
Sr 421.552†	1722.4	0.2904 µg/L	0.06098	0.2904 ppb	0.06098	21.00%
QC value within limits for Sr 421.552 Recovery = Not calculated						
Ti 334.940†	22603.3	-3.6809 µg/L	0.40375	-3.6809 ppb	0.40375	10.97%
QC value within limits for Ti 334.940 Recovery = Not calculated						
Tl 190.801†	-50.8	-6.3210 µg/L	1.39339	-6.3210 ppb	1.39339	22.04%
QC value within limits for Tl 190.801 Recovery = Not calculated						
U 409.014†	537.8	12.740 µg/L	14.1197	12.740 ppb	14.1197	110.83%
QC value within limits for U 409.014 Recovery = Not calculated						
V 292.402†	5735.0	1.5725 µg/L	0.98127	1.5725 ppb	0.98127	62.40%
QC value within limits for V 292.402 Recovery = Not calculated						
Zn 213.857†	3758.3	7.6020 µg/L	0.07306	7.6020 ppb	0.07306	0.96%
QC value within limits for Zn 213.857 Recovery = Not calculated						
All analyte(s) passed QC.						

Sequence No.: 10

Sample ID: ICSAB

Analyst:

Logged In Analyst (Original) : optima4

Initial Sample Wt:

Dilution:

Autosampler Location: 104

Date Collected: 3/29/2010 18:45:15

Data Type: Reprocessed on 3/29/2010 19:14:39

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: ICSAB

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc 361.383	1510684.4	1510684.4	90.310 %		18:46:21
1	Sc RADIAL	137128.2	137128.2	94.1 %		18:45:49
1	Y 371.029	915417.0	915417.0	89.520 %		18:46:21
1	Ag 328.068†	64579.9	68542.0	271.32 µg/L	271.32 ppb	18:46:21
1	Al 396.153Radial†	2257035.7	2399046.7	523660 µg/L	523660 ppb	18:45:45
1	As 188.979†	1040.4	1166.3	536.34 µg/L	536.34 ppb	18:46:23
1	B 249.677†	30637.0	30568.6	511.66 µg/L	511.66 ppb	18:46:21
1	Ba 233.527†	99072.5	109877.7	499.99 µg/L	499.99 ppb	18:46:21
1	Be 313.107†	681148.0	754892.4	245.89 µg/L	245.89 ppb	18:46:21
1	Ca 317.933Radial†	7888724.1	8384349.0	491290 µg/L	491290 ppb	18:45:45
1	Cd 226.502†	63574.5	70490.2	466.80 µg/L	466.80 ppb	18:46:21
1	Co 228.616†	29268.7	32585.7	436.71 µg/L	436.71 ppb	18:46:23
1	Cr 267.716†	51261.8	56601.7	486.64 µg/L	486.64 ppb	18:46:23
1	Cu 324.752†	105042.3	113888.0	536.82 µg/L	536.82 ppb	18:46:21
1	Fe 238.204 Radial†	2714615.2	2885265.2	191820 µg/L	191820 ppb	18:45:47
1	K 766.490 Radial†	14492.6	13949.3	5495.4 µg/L	5495.4 ppb	18:45:49
1	Mg 279.077 IEC†	1107607.9	1177095.4	485180 µg/L	485180 ppb	18:45:49
1	Mn 257.610†	329092.8	364323.1	478.08 µg/L	478.08 ppb	18:46:21
1	Mo 202.031†	13229.8	14704.5	480.80 µg/L	480.80 ppb	18:46:23
1	Na 589.592 Radial†	34394.1	34862.9	5329.4 µg/L	5329.4 ppb	18:45:49
1	Ni 231.604†	31853.0	35311.6	451.68 µg/L	451.68 ppb	18:46:23
1	P 214.914†	9576.1	10524.0	2499.6 µg/L	2499.6 ppb	18:46:23
1	Pb 220.353†	6597.4	7192.9	463.36 µg/L	463.36 ppb	18:46:23
1	S 181.975 Axial†	3009.0	3237.0	2626.5 µg/L	2626.5 ppb	18:46:23
1	Sb 206.836†	3499.0	3787.8	505.98 µg/L	505.98 ppb	18:46:23
1	Se 196.026†	5309.9	5868.7	2390 µg/L	2390 ppb	18:46:23
1	SiO2†	92256.7	100582.6	10974 µg/L	10974 ppb	18:46:21
1	Si 251.611†	281270.8	310773.6	5129.3 µg/L	5129.3 ppb	18:46:21
1	Sn 189.927†	6022.0	6666.1	475.68 µg/L	475.68 ppb	18:46:23
1	Sr 421.552†	210049.1	223540.3	520.07 µg/L	520.07 ppb	18:45:49
1	Ti 334.940†	468269.2	517876.1	500.97 µg/L	500.97 ppb	18:46:21
1	Tl 190.801†	2818.9	3241.7	443.45 µg/L	443.45 ppb	18:46:23
1	U 409.014†	7133.6	8378.1	528.93 µg/L	528.93 ppb	18:46:21
1	V 292.402†	88326.4	97371.6	516.38 µg/L	516.38 ppb	18:46:21
1	Zn 213.857†	72620.0	79947.4	483.88 µg/L	483.88 ppb	18:46:21
2	Sc 361.383	1518034.6	1518034.6	90.750 %		18:46:26
2	Sc RADIAL	136837.3	136837.3	93.9 %		18:45:56
2	Y 371.029	919619.6	919619.6	89.931 %		18:46:26
2	Ag 328.068†	64494.6	68101.8	269.69 µg/L	269.69 ppb	18:46:26
2	Al 396.153Radial†	2229777.5	2375110.8	518440 µg/L	518440 ppb	18:45:52
2	As 188.979†	1016.8	1134.7	522.67 µg/L	522.67 ppb	18:46:28
2	B 249.677†	30917.4	30713.3	514.09 µg/L	514.09 ppb	18:46:26
2	Ba 233.527†	99392.7	109699.3	499.19 µg/L	499.19 ppb	18:46:26
2	Be 313.107†	684598.1	755042.2	245.93 µg/L	245.93 ppb	18:46:26
2	Ca 317.933Radial†	7784991.4	8291677.2	485860 µg/L	485860 ppb	18:45:52
2	Cd 226.502†	63805.9	70404.3	466.38 µg/L	466.38 ppb	18:46:26
2	Co 228.616†	29275.9	32436.7	434.76 µg/L	434.76 ppb	18:46:28
2	Cr 267.716†	50741.5	55753.6	479.35 µg/L	479.35 ppb	18:46:28
2	Cu 324.752†	105439.6	113762.6	535.91 µg/L	535.91 ppb	18:46:26
2	Fe 238.204 Radial†	2684811.7	2859651.8	190120 µg/L	190120 ppb	18:45:54
2	K 766.490 Radial†	14227.4	13699.5	5395.1 µg/L	5395.1 ppb	18:45:56
2	Mg 279.077 IEC†	1095117.9	1166293.6	480720 µg/L	480720 ppb	18:45:56
2	Mn 257.610†	330574.5	364191.4	478.08 µg/L	478.08 ppb	18:46:26
2	Mo 202.031†	13322.6	14735.9	481.64 µg/L	481.64 ppb	18:46:28
2	Na 589.592 Radial†	34233.3	34769.4	5315.2 µg/L	5315.2 ppb	18:45:56
2	Ni 231.604†	31592.4	34853.7	445.82 µg/L	445.82 ppb	18:46:28
2	P 214.914†	9407.5	10286.9	2442.8 µg/L	2442.8 ppb	18:46:28
2	Pb 220.353†	6453.4	6998.8	451.34 µg/L	451.34 ppb	18:46:28

2	S 181.975 Axial†	2940.7	3145.6	2552.4 µg/L	2552.4 ppb	18:46:28
2	Sb 206.836†	3475.9	3743.6	500.18 µg/L	500.18 ppb	18:46:28
2	Se 196.026†	5145.8	5659.4	2310 µg/L	2310 ppb	18:46:28
2	SiO2†	92799.3	100685.9	10985 µg/L	10985 ppb	18:46:26
2	Si 251.611†	282521.5	310643.8	5127.1 µg/L	5127.1 ppb	18:46:26
2	Sn 189.927†	5996.0	6605.2	471.35 µg/L	471.35 ppb	18:46:28
2	Sr 421.552†	208807.5	222692.2	518.13 µg/L	518.13 ppb	18:45:56
2	Ti 334.940†	470515.6	517840.9	501.16 µg/L	501.16 ppb	18:46:26
2	Tl 190.801†	2878.3	3292.0	450.21 µg/L	450.21 ppb	18:46:28
2	U 409.014†	7163.0	8372.3	528.73 µg/L	528.73 ppb	18:46:26
2	V 292.402†	88754.8	97370.2	516.63 µg/L	516.63 ppb	18:46:26
2	Zn 213.857†	72903.7	79870.6	483.58 µg/L	483.58 ppb	18:46:26
3	Sc 361.383	1509678.5	1509678.5	90.250 %		18:46:31
3	Sc RADIAL	138373.5	138373.5	94.9 %		18:46:03
3	Y 371.029	914674.1	914674.1	89.448 %		18:46:31
3	Ag 328.068†	64587.4	68598.0	271.77 µg/L	271.77 ppb	18:46:31
3	Al 396.153Radial†	2250390.9	2370456.7	517420 µg/L	517420 ppb	18:45:58
3	As 188.979†	1006.1	1129.0	520.40 µg/L	520.40 ppb	18:46:33
3	B 249.677†	30857.6	30835.5	516.13 µg/L	516.13 ppb	18:46:31
3	Ba 233.527†	99227.6	110122.6	501.13 µg/L	501.13 ppb	18:46:31
3	Be 313.107†	682431.3	756816.9	246.51 µg/L	246.51 ppb	18:46:31
3	Ca 317.933Radial†	7834035.4	8251280.0	483490 µg/L	483490 ppb	18:45:58
3	Cd 226.502†	63517.1	70473.5	466.87 µg/L	466.87 ppb	18:46:31
3	Co 228.616†	29487.3	32849.5	440.42 µg/L	440.42 ppb	18:46:33
3	Cr 267.716†	51368.6	56757.9	487.95 µg/L	487.95 ppb	18:46:33
3	Cu 324.752†	105432.6	114397.9	538.71 µg/L	538.71 ppb	18:46:31
3	Fe 238.204 Radial†	2714742.3	2859431.1	190100 µg/L	190100 ppb	18:46:01
3	K 766.490 Radial†	14507.9	13826.8	5448.0 µg/L	5448.0 ppb	18:46:03
3	Mg 279.077 IEC†	1111196.5	1170280.1	482370 µg/L	482370 ppb	18:46:03
3	Mn 257.610†	329292.9	364787.6	478.83 µg/L	478.83 ppb	18:46:31
3	Mo 202.031†	13311.3	14804.5	483.83 µg/L	483.83 ppb	18:46:33
3	Na 589.592 Radial†	34668.7	34823.2	5323.3 µg/L	5323.3 ppb	18:46:03
3	Ni 231.604†	31996.5	35494.2	454.01 µg/L	454.01 ppb	18:46:33
3	P 214.914†	9605.6	10563.7	2508.9 µg/L	2508.9 ppb	18:46:33
3	Pb 220.353†	6567.4	7164.5	461.32 µg/L	461.32 ppb	18:46:33
3	S 181.975 Axial†	2974.8	3201.4	2597.7 µg/L	2597.7 ppb	18:46:33
3	Sb 206.836†	3463.3	3750.8	501.08 µg/L	501.08 ppb	18:46:33
3	Se 196.026†	5291.7	5852.5	2380 µg/L	2380 ppb	18:46:33
3	SiO2†	92489.2	100908.3	11009 µg/L	11009 ppb	18:46:31
3	Si 251.611†	281639.3	311389.5	5139.4 µg/L	5139.4 ppb	18:46:31
3	Sn 189.927†	6087.5	6743.1	481.17 µg/L	481.17 ppb	18:46:33
3	Sr 421.552†	210738.5	222257.1	517.13 µg/L	517.13 ppb	18:46:03
3	Ti 334.940†	470683.6	520896.9	504.08 µg/L	504.08 ppb	18:46:31
3	Tl 190.801†	2864.6	3294.4	450.54 µg/L	450.54 ppb	18:46:33
3	U 409.014†	7145.1	8396.1	530.14 µg/L	530.14 ppb	18:46:31
3	V 292.402†	88390.3	97507.5	517.45 µg/L	517.45 ppb	18:46:31
3	Zn 213.857†	72542.0	79914.6	483.81 µg/L	483.81 ppb	18:46:31

Mean Data: ICSAB

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1512799.2	90.437 %	0.2727			0.30%
Sc RADIAL	137446.3	94.3 %	0.56			0.59%
Y 371.029	916570.2	89.633 %	0.2608			0.29%
Ag 328.068†	68413.9	270.93 µg/L	1.098	270.93 ppb	1.098	0.41%
QC value within limits for Ag 328.068 Recovery = 108.37%						
Al 396.153Radial†	2381538.1	519840 µg/L	3348.7	519840 ppb	3348.7	0.64%
QC value within limits for Al 396.153Radial Recovery = 103.97%						
As 188.979†	1143.3	526.47 µg/L	8.621	526.47 ppb	8.621	1.64%
QC value within limits for As 188.979 Recovery = 105.29%						
B 249.677†	30705.8	513.96 µg/L	2.238	513.96 ppb	2.238	0.44%
QC value within limits for B 249.677 Recovery = 102.79%						
Ba 233.527†	109899.8	500.10 µg/L	0.973	500.10 ppb	0.973	0.19%
QC value within limits for Ba 233.527 Recovery = 100.02%						
Be 313.107†	755583.8	246.11 µg/L	0.349	246.11 ppb	0.349	0.14%
QC value within limits for Be 313.107 Recovery = 98.44%						
Ca 317.933Radial†	8309102.1	486880 µg/L	3997.7	486880 ppb	3997.7	0.82%
QC value within limits for Ca 317.933Radial Recovery = 97.38%						
Cd 226.502†	70456.0	466.68 µg/L	0.262	466.68 ppb	0.262	0.06%
QC value within limits for Cd 226.502 Recovery = 93.34%						

Co 228.616†	32623.9	437.30 µg/L	2.873	437.30 ppb	2.873	0.66%
QC value within limits for Co 228.616 Recovery = 87.46%						
Cr 267.716†	56371.1	484.65 µg/L	4.635	484.65 ppb	4.635	0.96%
QC value within limits for Cr 267.716 Recovery = 96.93%						
Cu 324.752†	114016.2	537.15 µg/L	1.432	537.15 ppb	1.432	0.27%
QC value within limits for Cu 324.752 Recovery = 107.43%						
Fe 238.204 Radial†	2868116.0	190680 µg/L	987.4	190680 ppb	987.4	0.52%
QC value within limits for Fe 238.204 Radial Recovery = 95.34%						
K 766.490 Radial†	13825.2	5446.2 µg/L	50.18	5446.2 ppb	50.18	0.92%
QC value within limits for K 766.490 Radial Recovery = 108.92%						
Mg 279.077 IEC†	1171223.1	482760 µg/L	2251.4	482760 ppb	2251.4	0.47%
QC value within limits for Mg 279.077 IEC Recovery = 96.55%						
Mn 257.610†	364434.0	478.33 µg/L	0.433	478.33 ppb	0.433	0.09%
QC value within limits for Mn 257.610 Recovery = 95.67%						
Mo 202.031†	14748.3	482.09 µg/L	1.569	482.09 ppb	1.569	0.33%
QC value within limits for Mo 202.031 Recovery = 96.42%						
Na 589.592 Radial†	34818.5	5322.6 µg/L	7.14	5322.6 ppb	7.14	0.13%
QC value within limits for Na 589.592 Radial Recovery = 106.45%						
Ni 231.604†	35219.8	450.50 µg/L	4.221	450.50 ppb	4.221	0.94%
QC value within limits for Ni 231.604 Recovery = 90.10%						
P 214.914†	10458.2	2483.8 µg/L	35.79	2483.8 ppb	35.79	1.44%
QC value within limits for P 214.914 Recovery = 99.35%						
Pb 220.353†	7118.7	458.68 µg/L	6.431	458.68 ppb	6.431	1.40%
QC value within limits for Pb 220.353 Recovery = 91.74%						
S 181.975 Axial†	3194.7	2592.2 µg/L	37.32	2592.2 ppb	37.32	1.44%
QC value within limits for S 181.975 Axial Recovery = 103.69%						
Sb 206.836†	3760.7	502.41 µg/L	3.120	502.41 ppb	3.120	0.62%
QC value within limits for Sb 206.836 Recovery = 100.48%						
Se 196.026†	5793.5	2360 µg/L	46.2	2360 ppb	46.2	1.96%
QC value within limits for Se 196.026 Recovery = 94.33%						
SiO2†	100725.6	10989 µg/L	18.1	10989 ppb	18.1	0.16%
QC value within limits for SiO2 Recovery = 102.75%						
Si 251.611†	310935.6	5131.9 µg/L	6.54	5131.9 ppb	6.54	0.13%
QC value within limits for Si 251.611 Recovery = 102.64%						
Sn 189.927†	6671.5	476.07 µg/L	4.919	476.07 ppb	4.919	1.03%
QC value within limits for Sn 189.927 Recovery = 95.21%						
Sr 421.552†	222829.9	518.44 µg/L	1.498	518.44 ppb	1.498	0.29%
QC value within limits for Sr 421.552 Recovery = 103.69%						
Ti 334.940†	518871.3	502.07 µg/L	1.741	502.07 ppb	1.741	0.35%
QC value within limits for Ti 334.940 Recovery = 100.41%						
Tl 190.801†	3276.0	448.07 µg/L	4.004	448.07 ppb	4.004	0.89%
QC value within limits for Tl 190.801 Recovery = 89.61%						
U 409.014†	8382.2	529.27 µg/L	0.763	529.27 ppb	0.763	0.14%
QC value within limits for U 409.014 Recovery = 105.85%						
V 292.402†	97416.4	516.82 µg/L	0.558	516.82 ppb	0.558	0.11%
QC value within limits for V 292.402 Recovery = 103.36%						
Zn 213.857†	79910.9	483.76 µg/L	0.156	483.76 ppb	0.156	0.03%
QC value within limits for Zn 213.857 Recovery = 96.75%						
All analyte(s) passed QC.						

Sequence No.: 11

Sample ID: LR1

Analyst:

Logged In Analyst (Original) : optima4

Initial Sample Wt:

Dilution:

Autosampler Location: 105

Date Collected: 3/29/2010 18:46:42

Data Type: Reprocessed on 3/29/2010 19:14:40

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: LR1

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc 361.383	1475217.1	1475217.1	88.190 %		18:47:41
1	Sc RADIAL	134988.0	134988.0	92.6 %		18:47:14
1	Y 371.029	890652.0	890652.0	87.098 %		18:47:41
1	Ag 328.068†	2600.2	-18.7	4.2300 µg/L	4.2300 ppb	18:47:41
1	Al 396.153Radial†	2173247.9	2346612.0	512240 µg/L	512240 ppb	18:47:12
1	As 188.979†	-221.7	-237.2	2.3463 µg/L	2.3463 ppb	18:47:43
1	B 249.677†	3640.1	771.9	12.918 µg/L	12.918 ppb	18:47:41
1	Ba 233.527†	451.6	687.2	-2.6252 µg/L	-2.6252 ppb	18:47:43
1	Be 313.107†	-13095.3	-14188.9	-0.0322 µg/L	-0.0322 ppb	18:47:41
1	Ca 317.933Radial†	7559025.2	8161296.1	478220 µg/L	478220 ppb	18:47:12
1	Cd 226.502†	5610.9	6456.7	-2.9745 µg/L	-2.9745 ppb	18:47:43
1	Co 228.616†	613.3	872.0	-11.650 µg/L	-11.650 ppb	18:47:43
1	Cr 267.716†	908.0	869.3	5.4318 µg/L	5.4318 ppb	18:47:43
1	Cu 324.752†	-17506.0	-22275.2	-5.5587 µg/L	-5.5587 ppb	18:47:43
1	Fe 238.204 Radial†	6300456.2	6802850.0	452280 µg/L	452280 ppb	18:47:12
1	K 766.490 Radial†	1898.7	595.1	-78.007 µg/L	-78.007 ppb	18:47:14
1	Mg 279.077 IEC†	1069506.5	1154620.7	475670 µg/L	475670 ppb	18:47:12
1	Mn 257.610†	14951.4	16873.6	2.9939 µg/L	2.9939 ppb	18:47:41
1	Mo 202.031†	-853.5	-912.6	-2.2055 µg/L	-2.2055 ppb	18:47:41
1	Na 589.592 Radial†	3064907.6	3307661.5	506110 µg/L	506110 ppb	18:47:12
1	Ni 231.604†	241.8	315.0	4.0298 µg/L	4.0298 ppb	18:47:43
1	P 214.914†	851.2	885.7	19.361 µg/L	19.361 ppb	18:47:43
1	Pb 220.353†	111.2	13.7	6.6643 µg/L	6.6643 ppb	18:47:43
1	S 181.975 Axial†	199.5	131.4	106.18 µg/L	106.18 ppb	18:47:43
1	Sb 206.836†	173.5	110.1	5.3162 µg/L	5.3162 ppb	18:47:43
1	Se 196.026†	-269.6	-316.6	46.3 µg/L	46.3 ppb	18:47:43
1	SiO2†	1875.2	553.5	61.247 µg/L	61.247 ppb	18:47:43
1	Si 251.611†	-2234.1	-3209.7	-52.717 µg/L	-52.717 ppb	18:47:43
1	Sn 189.927†	58.5	64.3	4.6670 µg/L	4.6670 ppb	18:47:43
1	Sr 421.552†	4787.3	5447.1	9.0235 µg/L	9.0235 ppb	18:47:14
1	Ti 334.940†	25472.1	28246.9	-3.7159 µg/L	-3.7159 ppb	18:47:41
1	Tl 190.801†	-294.1	-213.1	-27.836 µg/L	-27.836 ppb	18:47:43
1	U 409.014†	216123.9	245545.7	15094 µg/L	15094 ppb	18:47:41
1	V 292.402†	10776.3	11787.7	3.3989 µg/L	3.3989 ppb	18:47:43
1	Zn 213.857†	7832.8	8417.4	9.2023 µg/L	9.2023 ppb	18:47:43
2	Sc 361.383	1474797.5	1474797.5	88.165 %		18:47:46
2	Sc RADIAL	136487.8	136487.8	93.6 %		18:47:19
2	Y 371.029	890090.9	890090.9	87.044 %		18:47:46
2	Ag 328.068†	2591.0	-28.2	4.2336 µg/L	4.2336 ppb	18:47:46
2	Al 396.153Radial†	2181204.6	2329323.3	508460 µg/L	508460 ppb	18:47:17
2	As 188.979†	-251.7	-271.3	-12.460 µg/L	-12.460 ppb	18:47:48
2	B 249.677†	3729.3	874.2	14.628 µg/L	14.628 ppb	18:47:46
2	Ba 233.527†	527.6	773.5	-2.2009 µg/L	-2.2009 ppb	18:47:46
2	Be 313.107†	-13474.2	-14622.9	-0.1807 µg/L	-0.1807 ppb	18:47:48
2	Ca 317.933Radial†	7600178.4	8115555.5	475540 µg/L	475540 ppb	18:47:17
2	Cd 226.502†	5683.2	6540.6	-2.1393 µg/L	-2.1393 ppb	18:47:48
2	Co 228.616†	752.5	1030.1	-9.3590 µg/L	-9.3590 ppb	18:47:48
2	Cr 267.716†	724.6	661.7	3.6080 µg/L	3.6080 ppb	18:47:48
2	Cu 324.752†	-17459.2	-22227.9	-5.7811 µg/L	-5.7811 ppb	18:47:48
2	Fe 238.204 Radial†	6336284.1	6766355.5	449850 µg/L	449850 ppb	18:47:17
2	K 766.490 Radial†	1981.3	660.8	-49.077 µg/L	-49.077 ppb	18:47:19
2	Mg 279.077 IEC†	1076643.1	1149552.1	473590 µg/L	473590 ppb	18:47:17
2	Mn 257.610†	15045.5	16985.2	3.2356 µg/L	3.2356 ppb	18:47:46
2	Mo 202.031†	-881.3	-944.4	-3.3453 µg/L	-3.3453 ppb	18:47:46
2	Na 589.592 Radial†	3084400.4	3292112.6	503740 µg/L	503740 ppb	18:47:17
2	Ni 231.604†	341.9	428.7	5.4833 µg/L	5.4833 ppb	18:47:48
2	P 214.914†	888.6	928.3	30.390 µg/L	30.390 ppb	18:47:48
2	Pb 220.353†	63.3	-40.6	3.2317 µg/L	3.2317 ppb	18:47:48

2	S 181.975 Axial†	169.7	97.6	78.843 µg/L	78.843 ppb	18:47:48
2	Sb 206.836†	95.2	21.4	-6.5888 µg/L	-6.5888 ppb	18:47:48
2	Se 196.026†	-403.3	-468.4	-14.6 µg/L	-14.6 ppb	18:47:48
2	SiO2†	1816.0	486.9	54.020 µg/L	54.020 ppb	18:47:48
2	Si 251.611†	-2084.7	-3041.0	-49.906 µg/L	-49.906 ppb	18:47:48
2	Sn 189.927†	43.9	47.8	3.4920 µg/L	3.4920 ppb	18:47:48
2	Sr 421.552†	4824.6	5430.1	9.0047 µg/L	9.0047 ppb	18:47:19
2	Ti 334.940†	25083.7	27814.6	-4.0459 µg/L	-4.0459 ppb	18:47:46
2	Tl 190.801†	-241.3	-153.4	-19.840 µg/L	-19.840 ppb	18:47:48
2	U 409.014†	215721.0	245158.5	15071 µg/L	15071 ppb	18:47:46
2	V 292.402†	10612.7	11605.5	2.7405 µg/L	2.7405 ppb	18:47:48
2	Zn 213.857†	7898.7	8494.6	9.8973 µg/L	9.8973 ppb	18:47:48
3	Sc 361.383	1482973.9	1482973.9	88.654 %		18:47:51
3	Sc RADIAL	135581.7	135581.7	93.0 %		18:47:23
3	Y 371.029	894893.3	894893.3	87.513 %		18:47:51
3	Ag 328.068†	2907.1	312.1	5.3159 µg/L	5.3159 ppb	18:47:51
3	Al 396.153Radial†	2198157.6	2363115.2	515840 µg/L	515840 ppb	18:47:21
3	As 188.979†	-166.7	-173.8	30.035 µg/L	30.035 ppb	18:47:53
3	B 249.677†	3819.0	952.0	15.940 µg/L	15.940 ppb	18:47:51
3	Ba 233.527†	467.2	702.0	-2.6283 µg/L	-2.6283 ppb	18:47:53
3	Be 313.107†	-13583.2	-14661.6	-0.1997 µg/L	-0.1997 ppb	18:47:51
3	Ca 317.933Radial†	7679845.3	8255440.6	483730 µg/L	483730 ppb	18:47:21
3	Cd 226.502†	5523.3	6324.6	-4.4547 µg/L	-4.4547 ppb	18:47:53
3	Co 228.616†	665.1	926.8	-11.181 µg/L	-11.181 ppb	18:47:53
3	Cr 267.716†	895.3	849.6	5.3942 µg/L	5.3942 ppb	18:47:53
3	Cu 324.752†	-17409.5	-22062.6	-3.6839 µg/L	-3.6839 ppb	18:47:53
3	Fe 238.204 Radial†	6403813.8	6884172.5	457680 µg/L	457680 ppb	18:47:21
3	K 766.490 Radial†	2077.2	778.0	-6.1386 µg/L	-6.1386 ppb	18:47:23
3	Mg 279.077 IEC†	1090892.1	1172554.0	483060 µg/L	483060 ppb	18:47:21
3	Mn 257.610†	15096.7	16948.9	2.7894 µg/L	2.7894 ppb	18:47:51
3	Mo 202.031†	-879.5	-936.8	-2.6225 µg/L	-2.6225 ppb	18:47:51
3	Na 589.592 Radial†	3116499.7	3348632.9	512380 µg/L	512380 ppb	18:47:21
3	Ni 231.604†	249.4	322.2	4.1219 µg/L	4.1219 ppb	18:47:53
3	P 214.914†	734.4	748.9	-16.245 µg/L	-16.245 ppb	18:47:53
3	Pb 220.353†	-96.4	-221.1	-7.4793 µg/L	-7.4793 ppb	18:47:53
3	S 181.975 Axial†	169.9	96.8	78.205 µg/L	78.205 ppb	18:47:53
3	Sb 206.836†	73.9	-3.3	-10.074 µg/L	-10.074 ppb	18:47:53
3	Se 196.026†	-324.5	-376.9	24.3 µg/L	24.3 ppb	18:47:53
3	SiO2†	1980.5	661.1	72.973 µg/L	72.973 ppb	18:47:53
3	Si 251.611†	-1826.1	-2736.2	-44.905 µg/L	-44.905 ppb	18:47:53
3	Sn 189.927†	110.7	122.9	8.8298 µg/L	8.8298 ppb	18:47:53
3	Sr 421.552†	4811.0	5449.9	8.9869 µg/L	8.9869 ppb	18:47:23
3	Ti 334.940†	25226.4	27818.7	-4.5924 µg/L	-4.5924 ppb	18:47:51
3	Tl 190.801†	-184.7	-88.0	-11.070 µg/L	-11.070 ppb	18:47:53
3	U 409.014†	216613.9	244816.6	15048 µg/L	15048 ppb	18:47:51
3	V 292.402†	10498.6	11410.5	0.4086 µg/L	0.4086 ppb	18:47:53
3	Zn 213.857†	7725.4	8249.7	7.5805 µg/L	7.5805 ppb	18:47:53

Mean Data: LR1

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1477662.9	88.336 %	0.2752			0.31%
Sc RADIAL	135685.8	93.1 %	0.52			0.56%
Y 371.029	891878.7	87.218 %	0.2568			0.29%
Ag 328.068†	88.4	4.5932 µg/L	0.62588	4.5932 ppb	0.62588	13.63%
Al 396.153Radial†	2346350.2	512180 µg/L	3688.5	512180 ppb	3688.5	0.72%
QC value within limits for Al 396.153Radial Recovery = 102.44%						
As 188.979†	-227.4	6.6405 µg/L	21.57070	6.6405 ppb	21.57070	324.83%
B 249.677†	866.1	14.495 µg/L	1.5153	14.495 ppb	1.5153	10.45%
Ba 233.527†	720.9	-2.4848 µg/L	0.24586	-2.4848 ppb	0.24586	9.89%
Be 313.107†	-14491.1	-0.1375 µg/L	0.09171	-0.1375 ppb	0.09171	66.68%
Ca 317.933Radial†	8177430.7	479160 µg/L	4179.3	479160 ppb	4179.3	0.87%
QC value within limits for Ca 317.933Radial Recovery = 95.83%						
Cd 226.502†	6440.6	-3.1895 µg/L	1.17255	-3.1895 ppb	1.17255	36.76%
Co 228.616†	943.0	-10.730 µg/L	1.2103	-10.730 ppb	1.2103	11.28%
Cr 267.716†	793.5	4.8113 µg/L	1.04230	4.8113 ppb	1.04230	21.66%
Cu 324.752†	-22188.5	-5.0079 µg/L	1.15199	-5.0079 ppb	1.15199	23.00%
Fe 238.204 Radial†	6817792.7	453270 µg/L	4009.8	453270 ppb	4009.8	0.88%
QC value within limits for Fe 238.204 Radial Recovery = 90.65%						
K 766.490 Radial†	678.0	-44.408 µg/L	36.1609	-44.408 ppb	36.1609	81.43%

Mg 279.077 IEC†	1158908.9	477440 µg/L	4979.6	477440 ppb	4979.6	1.04%
QC value within limits for Mg 279.077 IEC Recovery = 95.49%						
Mn 257.610†	16935.9	3.0063 µg/L	0.22334	3.0063 ppb	0.22334	7.43%
Mo 202.031†	-931.3	-2.7244 µg/L	0.57668	-2.7244 ppb	0.57668	21.17%
Na 589.592 Radial†	3316135.7	507410 µg/L	4467.6	507410 ppb	4467.6	0.88%
QC value within limits for Na 589.592 Radial Recovery = 101.48%						
Ni 231.604†	355.3	4.5450 µg/L	0.81388	4.5450 ppb	0.81388	17.91%
P 214.914†	854.3	11.169 µg/L	24.3729	11.169 ppb	24.3729	218.22%
Pb 220.353†	-82.7	0.8056 µg/L	7.37729	0.8056 ppb	7.37729	915.80%
S 181.975 Axial†	108.6	87.742 µg/L	15.9697	87.742 ppb	15.9697	18.20%
Sb 206.836†	42.7	-3.7822 µg/L	8.06989	-3.7822 ppb	8.06989	213.36%
Se 196.026†	-387.3	18.7 µg/L	30.84	18.7 ppb	30.84	165.04%
SiO2†	567.2	62.747 µg/L	9.5648	62.747 ppb	9.5648	15.24%
Si 251.611†	-2995.6	-49.176 µg/L	3.9567	-49.176 ppb	3.9567	8.05%
Sn 189.927†	78.3	5.6629 µg/L	2.80476	5.6629 ppb	2.80476	49.53%
Sr 421.552†	5442.4	9.0050 µg/L	0.01831	9.0050 ppb	0.01831	0.20%
Ti 334.940†	27960.1	-4.1181 µg/L	0.44268	-4.1181 ppb	0.44268	10.75%
Tl 190.801†	-151.5	-19.582 µg/L	8.3859	-19.582 ppb	8.3859	42.82%
U 409.014†	245173.6	15071 µg/L	23.1	15071 ppb	23.1	0.15%
QC value within limits for U 409.014 Recovery = 100.47%						
V 292.402†	11601.2	2.1827 µg/L	1.57124	2.1827 ppb	1.57124	71.99%
Zn 213.857†	8387.2	8.8934 µg/L	1.18890	8.8934 ppb	1.18890	13.37%
All analyte(s) passed QC.						

Sequence No.: 12

Sample ID: LR2

Analyst:

Logged In Analyst (Original) : optima4

Initial Sample Wt:

Dilution:

Autosampler Location: 108

Date Collected: 3/29/2010 18:48:01

Data Type: Reprocessed on 3/29/2010 19:14:40

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: LR2

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc 361.383	1698380.4	1698380.4	101.53 %		18:49:13
1	Sc RADIAL	151205.1	151205.1	104 %		18:48:34
1	Y 371.029	1017103.0	1017103.0	99.464 %		18:49:13
1	Ag 328.068†	-18686.1	-21371.4	31.131 µg/L	31.131 ppb	18:49:15
1	Al 396.153Radial†	2338.4	2286.0	66.356 µg/L	66.356 ppb	18:48:36
1	As 188.979†	24060.3	23711.8	10160 µg/L	10160 ppb	18:49:15
1	B 249.677†	302290.6	294377.4	4910.3 µg/L	4910.3 ppb	18:49:13
1	Ba 233.527†	3091920.0	3045479.3	13922 µg/L	13922 ppb	18:49:13
1	Be 313.107†	8967503.4	8832963.6	2875.2 µg/L	2875.2 ppb	18:49:09
1	Ca 317.933Radial†	1386.8	720.6	42.226 µg/L	42.226 ppb	18:48:36
1	Cd 226.502†	1391850.4	1370960.3	9471.5 µg/L	9471.5 ppb	18:49:13
1	Co 228.616†	680530.5	670447.0	9197.3 µg/L	9197.3 ppb	18:49:13
1	Cr 267.716†	2796482.2	2754160.4	23659 µg/L	23659 ppb	18:49:13
1	Cu 324.752†	4652514.4	4579945.2	19914 µg/L	19914 ppb	18:49:13
1	Fe 238.204 Radial†	-1093.2	-1167.1	-77.594 µg/L	-77.594 ppb	18:48:36
1	K 766.490 Radial†	735082.9	707128.4	291110 µg/L	291110 ppb	18:48:34
1	Mg 279.077 IEC†	-573.2	-739.2	-76.817 µg/L	-76.817 ppb	18:48:36
1	Mn 257.610†	6850554.7	6747191.3	9219.6 µg/L	9219.6 ppb	18:49:13
1	Mo 202.031†	299568.0	295106.7	9318.7 µg/L	9318.7 ppb	18:49:15
1	Na 589.592 Radial†	4106.1	2263.3	87.417 µg/L	87.417 ppb	18:48:36
1	Ni 231.604†	759020.4	747617.8	9562.9 µg/L	9562.9 ppb	18:49:13
1	P 214.914†	61793.1	60781.8	14324 µg/L	14324 ppb	18:49:15
1	Pb 220.353†	385088.4	379170.1	22997 µg/L	22997 ppb	18:49:13
1	S 181.975 Axial†	62300.3	61266.2	49715 µg/L	49715 ppb	18:49:15
1	Sb 206.836†	72365.8	71188.1	9412.3 µg/L	9412.3 ppb	18:49:15
1	Se 196.026†	23983.3	23610.8	9340 µg/L	9340 ppb	18:49:15
1	SiO2†	927224.5	911672.2	99243 µg/L	99243 ppb	18:49:13
1	Si 251.611†	2845330.8	2801756.4	46140 µg/L	46140 ppb	18:49:13
1	Sn 189.927†	135952.5	133900.7	9552.3 µg/L	9552.3 ppb	18:49:15
1	Sr 421.552†	4291141.6	4136725.5	9695.4 µg/L	9695.4 ppb	18:48:32
1	Ti 334.940†	9795412.6	9647094.3	9829.2 µg/L	9829.2 ppb	18:49:09
1	Tl 190.801†	68839.1	67921.6	9266.8 µg/L	9266.8 ppb	18:49:15
1	U 409.014†	-6352.9	-5778.0	247.84 µg/L	247.84 ppb	18:49:15
1	V 292.402†	1822287.8	1794382.0	10142 µg/L	10142 ppb	18:49:13
1	Zn 213.857†	2271454.5	2236744.1	14006 µg/L	14006 ppb	18:49:13
2	Sc 361.383	1692355.1	1692355.1	101.17 %		18:49:22
2	Sc RADIAL	148148.5	148148.5	102 %		18:48:40
2	Y 371.029	1013670.4	1013670.4	99.129 %		18:49:22
2	Ag 328.068†	-18902.0	-21650.3	30.241 µg/L	30.241 ppb	18:49:25
2	Al 396.153Radial†	2166.1	2162.9	32.480 µg/L	32.480 ppb	18:48:43
2	As 188.979†	24382.8	24114.9	10329 µg/L	10329 ppb	18:49:25
2	B 249.677†	301947.2	295098.0	4922.4 µg/L	4922.4 ppb	18:49:22
2	Ba 233.527†	3087006.8	3051465.1	13949 µg/L	13949 ppb	18:49:22
2	Be 313.107†	8888938.4	8786753.2	2860.1 µg/L	2860.1 ppb	18:49:19
2	Ca 317.933Radial†	1193.0	557.5	32.668 µg/L	32.668 ppb	18:48:43
2	Cd 226.502†	1387271.1	1371314.7	9474.0 µg/L	9474.0 ppb	18:49:22
2	Co 228.616†	679503.2	671817.9	9216.1 µg/L	9216.1 ppb	18:49:22
2	Cr 267.716†	2791317.7	2758861.8	23700 µg/L	23700 ppb	18:49:22
2	Cu 324.752†	4645173.2	4589003.5	19954 µg/L	19954 ppb	18:49:22
2	Fe 238.204 Radial†	-1141.0	-1235.9	-82.165 µg/L	-82.165 ppb	18:48:43
2	K 766.490 Radial†	723724.6	710573.4	292530 µg/L	292530 ppb	18:48:40
2	Mg 279.077 IEC†	-594.9	-771.9	-86.616 µg/L	-86.616 ppb	18:48:43
2	Mn 257.610†	6838819.1	6759613.7	9236.6 µg/L	9236.6 ppb	18:49:22
2	Mo 202.031†	303352.5	299897.9	9470.0 µg/L	9470.0 ppb	18:49:25
2	Na 589.592 Radial†	3886.9	2129.3	65.648 µg/L	65.648 ppb	18:48:43
2	Ni 231.604†	757365.3	748643.5	9576.0 µg/L	9576.0 ppb	18:49:22
2	P 214.914†	62941.1	62133.3	14647 µg/L	14647 ppb	18:49:25
2	Pb 220.353†	383628.9	379077.8	22992 µg/L	22992 ppb	18:49:22

2	S 181.975 Axial†	63093.2	62268.3	50529 µg/L	50529 ppb	18:49:25
2	Sb 206.836†	73391.6	72455.9	9585.2 µg/L	9585.2 ppb	18:49:25
2	Se 196.026†	24264.9	23973.2	9480 µg/L	9480 ppb	18:49:25
2	SiO2†	925612.2	913330.0	99418 µg/L	99418 ppb	18:49:22
2	Si 251.611†	2841383.2	2807831.9	46237 µg/L	46237 ppb	18:49:22
2	Sn 189.927†	137626.2	136031.8	9703.7 µg/L	9703.7 ppb	18:49:25
2	Sr 421.552†	4251704.3	4183270.4	9804.5 µg/L	9804.5 ppb	18:48:38
2	Ti 334.940†	9732958.3	9619711.2	9801.3 µg/L	9801.3 ppb	18:49:19
2	Tl 190.801†	69796.1	69108.9	9426.0 µg/L	9426.0 ppb	18:49:25
2	U 409.014†	-6518.6	-5964.1	237.63 µg/L	237.63 ppb	18:49:25
2	V 292.402†	1819682.2	1798196.6	10165 µg/L	10165 ppb	18:49:22
2	Zn 213.857†	2265596.7	2238919.2	14019 µg/L	14019 ppb	18:49:22
3	Sc 361.383	1700875.8	1700875.8	101.68 %		18:49:32
3	Sc RADIAL	149241.8	149241.8	102 %		18:48:47
3	Y 371.029	1018743.4	1018743.4	99.625 %		18:49:32
3	Ag 328.068†	-19043.0	-21695.4	29.614 µg/L	29.614 ppb	18:49:34
3	Al 396.153Radial†	2183.6	2164.5	34.118 µg/L	34.118 ppb	18:48:49
3	As 188.979†	24384.9	23996.2	10278 µg/L	10278 ppb	18:49:34
3	B 249.677†	302272.0	293922.3	4902.7 µg/L	4902.7 ppb	18:49:32
3	Ba 233.527†	3092416.4	3041499.6	13904 µg/L	13904 ppb	18:49:32
3	Be 313.107†	8907241.5	8760739.0	2851.7 µg/L	2851.7 ppb	18:49:28
3	Ca 317.933Radial†	1218.9	574.2	33.647 µg/L	33.647 ppb	18:48:49
3	Cd 226.502†	1391102.2	1368213.3	9452.5 µg/L	9452.5 ppb	18:49:32
3	Co 228.616†	681435.9	670354.0	9196.0 µg/L	9196.0 ppb	18:49:32
3	Cr 267.716†	2794875.2	2748538.9	23611 µg/L	23611 ppb	18:49:32
3	Cu 324.752†	4650199.8	4570945.8	19875 µg/L	19875 ppb	18:49:32
3	Fe 238.204 Radial†	-1251.6	-1335.7	-88.800 µg/L	-88.800 ppb	18:48:49
3	K 766.490 Radial†	729684.2	711177.7	292780 µg/L	292780 ppb	18:48:47
3	Mg 279.077 IEC†	-664.5	-835.6	-113.55 µg/L	-113.55 ppb	18:48:49
3	Mn 257.610†	6850008.1	6736754.4	9205.4 µg/L	9205.4 ppb	18:49:32
3	Mo 202.031†	303976.8	299009.8	9441.9 µg/L	9441.9 ppb	18:49:34
3	Na 589.592 Radial†	3504.7	1728.1	4.0327 µg/L	4.0327 ppb	18:48:49
3	Ni 231.604†	758972.5	746473.9	9548.3 µg/L	9548.3 ppb	18:49:32
3	P 214.914†	62994.4	61874.1	14586 µg/L	14586 ppb	18:49:34
3	Pb 220.353†	384992.3	378519.2	22958 µg/L	22958 ppb	18:49:32
3	S 181.975 Axial†	63225.2	62085.8	50381 µg/L	50381 ppb	18:49:34
3	Sb 206.836†	73461.5	72161.1	9546.2 µg/L	9546.2 ppb	18:49:34
3	Se 196.026†	24345.1	23931.9	9470 µg/L	9470 ppb	18:49:34
3	SiO2†	927967.0	911062.6	99172 µg/L	99172 ppb	18:49:32
3	Si 251.611†	2848954.5	2801208.6	46128 µg/L	46128 ppb	18:49:32
3	Sn 189.927†	137708.4	135431.2	9660.9 µg/L	9660.9 ppb	18:49:34
3	Sr 421.552†	4283363.5	4183546.2	9805.1 µg/L	9805.1 ppb	18:48:45
3	Ti 334.940†	9739101.8	9577559.1	9758.3 µg/L	9758.3 ppb	18:49:28
3	Tl 190.801†	69743.1	68711.1	9371.9 µg/L	9371.9 ppb	18:49:34
3	U 409.014†	-6372.0	-5787.7	246.22 µg/L	246.22 ppb	18:49:34
3	V 292.402†	1821804.8	1791273.7	10126 µg/L	10126 ppb	18:49:32
3	Zn 213.857†	2271404.4	2233412.6	13985 µg/L	13985 ppb	18:49:32

Mean Data: LR2

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1697203.7	101.46 %	0.262			0.26%
Sc RADIAL	149531.8	103 %	1.1			1.04%
Y 371.029	1016505.6	99.406 %	0.2532			0.25%
Ag 328.068†	-21572.4	30.328 µg/L	0.7622	30.328 ppb	0.7622	2.51%
Al 396.153Radial†	2204.5	44.318 µg/L	19.1029	44.318 ppb	19.1029	43.10%
As 188.979†	23941.0	10256 µg/L	86.9	10256 ppb	86.9	0.85%
QC value within limits for As 188.979 Recovery = 102.56%						
B 249.677†	294465.9	4911.8 µg/L	9.92	4911.8 ppb	9.92	0.20%
QC value within limits for B 249.677 Recovery = 98.24%						
Ba 233.527†	3046148.0	13925 µg/L	22.9	13925 ppb	22.9	0.16%
QC value within limits for Ba 233.527 Recovery = 92.83%						
Be 313.107†	8793485.2	2862.3 µg/L	11.91	2862.3 ppb	11.91	0.42%
QC value within limits for Be 313.107 Recovery = 95.41%						
Ca 317.933Radial†	617.5	36.181 µg/L	5.2587	36.181 ppb	5.2587	14.53%
Cd 226.502†	1370162.8	9466.0 µg/L	11.73	9466.0 ppb	11.73	0.12%
QC value within limits for Cd 226.502 Recovery = 94.66%						
Co 228.616†	670873.0	9203.1 µg/L	11.25	9203.1 ppb	11.25	0.12%
QC value within limits for Co 228.616 Recovery = 92.03%						
Cr 267.716†	2753853.7	23657 µg/L	44.4	23657 ppb	44.4	0.19%

QC value within limits for Cr 267.716 Recovery = 94.63%						
Cu 324.752†	4579964.8	19914 µg/L	39.3	19914 ppb	39.3	0.20%
QC value within limits for Cu 324.752 Recovery = 99.57%						
Fe 238.204 Radial†	-1246.2	-82.853 µg/L	5.6347	-82.853 ppb	5.6347	6.80%
K 766.490 Radial†	709626.5	292140 µg/L	899.3	292140 ppb	899.3	0.31%
QC value within limits for K 766.490 Radial Recovery = 97.38%						
Mg 279.077 IEC†	-782.2	-92.329 µg/L	19.0229	-92.329 ppb	19.0229	20.60%
Mn 257.610†	6747853.1	9220.5 µg/L	15.64	9220.5 ppb	15.64	0.17%
QC value within limits for Mn 257.610 Recovery = 92.21%						
Mo 202.031†	298004.8	9410.2 µg/L	80.46	9410.2 ppb	80.46	0.86%
QC value within limits for Mo 202.031 Recovery = 94.10%						
Na 589.592 Radial†	2040.3	52.366 µg/L	43.2497	52.366 ppb	43.2497	82.59%
Ni 231.604†	747578.4	9562.4 µg/L	13.88	9562.4 ppb	13.88	0.15%
QC value within limits for Ni 231.604 Recovery = 95.62%						
P 214.914†	61596.4	14519 µg/L	171.5	14519 ppb	171.5	1.18%
QC value within limits for P 214.914 Recovery = 96.79%						
Pb 220.353†	378922.4	22983 µg/L	21.3	22983 ppb	21.3	0.09%
QC value within limits for Pb 220.353 Recovery = 91.93%						
S 181.975 Axial†	61873.4	50208 µg/L	433.1	50208 ppb	433.1	0.86%
QC value within limits for S 181.975 Axial Recovery = 100.42%						
Sb 206.836†	71935.0	9514.6 µg/L	90.66	9514.6 ppb	90.66	0.95%
QC value within limits for Sb 206.836 Recovery = 95.15%						
Se 196.026†	23838.7	9430 µg/L	78.5	9430 ppb	78.5	0.83%
QC value within limits for Se 196.026 Recovery = 94.29%						
SiO2†	912021.6	99278 µg/L	126.7	99278 ppb	126.7	0.13%
QC value within limits for SiO2 Recovery = 92.78%						
Si 251.611†	2803599.0	46168 µg/L	59.8	46168 ppb	59.8	0.13%
QC value within limits for Si 251.611 Recovery = 92.34%						
Sn 189.927†	135121.2	9639.0 µg/L	78.05	9639.0 ppb	78.05	0.81%
QC value within limits for Sn 189.927 Recovery = 96.39%						
Sr 421.552†	4167847.3	9768.3 µg/L	63.17	9768.3 ppb	63.17	0.65%
QC value within limits for Sr 421.552 Recovery = 97.68%						
Ti 334.940†	9614788.2	9796.3 µg/L	35.71	9796.3 ppb	35.71	0.36%
QC value within limits for Ti 334.940 Recovery = 97.96%						
Tl 190.801†	68580.5	9354.9 µg/L	80.95	9354.9 ppb	80.95	0.87%
QC value within limits for Tl 190.801 Recovery = 93.55%						
U 409.014†	-5843.2	243.90 µg/L	5.490	243.90 ppb	5.490	2.25%
V 292.402†	1794617.4	10145 µg/L	19.6	10145 ppb	19.6	0.19%
QC value within limits for V 292.402 Recovery = 101.45%						
Zn 213.857†	2236358.7	14003 µg/L	17.3	14003 ppb	17.3	0.12%
QC value within limits for Zn 213.857 Recovery = 93.36%						

All analyte(s) passed QC.

Sequence No.: 13

Sample ID: CCV

Analyst:

Logged In Analyst (Original) : optima4

Initial Sample Wt:

Dilution:

Autosampler Location: 7

Date Collected: 3/29/2010 18:49:43

Data Type: Reprocessed on 3/29/2010 19:14:41

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCV

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc 361.383	1716469.7	1716469.7	102.61 %		18:50:43
1	Sc RADIAL	154139.7	154139.7	106 %		18:50:16
1	Y 371.029	1044074.8	1044074.8	102.10 %		18:50:43
1	Ag 328.068†	127602.5	121387.1	498.79 µg/L	498.79 ppb	18:50:43
1	Al 396.153Radial†	24715.7	23403.0	5085.7 µg/L	5085.7 ppb	18:50:16
1	As 188.979†	1226.4	1209.4	512.57 µg/L	512.57 ppb	18:51:03
1	B 249.677†	33333.5	29129.3	487.34 µg/L	487.34 ppb	18:50:43
1	Ba 233.527†	111436.2	108774.4	497.32 µg/L	497.32 ppb	18:50:43
1	Be 313.107†	1573483.9	1534088.7	499.51 µg/L	499.51 ppb	18:50:43
1	Ca 317.933Radial†	90206.4	84682.8	4962.0 µg/L	4962.0 ppb	18:50:16
1	Cd 226.502†	72401.2	70652.6	487.60 µg/L	487.60 ppb	18:50:43
1	Co 228.616†	36477.3	35725.3	489.45 µg/L	489.45 ppb	18:50:43
1	Cr 267.716†	59006.8	57344.5	492.41 µg/L	492.41 ppb	18:50:43
1	Cu 324.752†	119200.3	113741.0	495.97 µg/L	495.97 ppb	18:50:43
1	Fe 238.204 Radial†	78399.3	74021.0	4921.2 µg/L	4921.2 ppb	18:50:16
1	K 766.490 Radial†	15543.8	13243.2	5447.9 µg/L	5447.9 ppb	18:50:16
1	Mg 279.077 IEC†	13152.3	12250.1	5058.7 µg/L	5058.7 ppb	18:50:16
1	Mn 257.610†	370669.7	361153.8	493.28 µg/L	493.28 ppb	18:50:43
1	Mo 202.031†	15969.2	15617.9	493.45 µg/L	493.45 ppb	18:51:03
1	Na 589.592 Radial†	70596.7	65061.3	9950.4 µg/L	9950.4 ppb	18:50:16
1	Ni 231.604†	39349.5	38388.8	491.04 µg/L	491.04 ppb	18:50:43
1	P 214.914†	10515.6	10168.3	2426.7 µg/L	2426.7 ppb	18:51:03
1	Pb 220.353†	8561.1	8230.7	500.15 µg/L	500.15 ppb	18:51:03
1	S 181.975 Axial†	1372.2	1242.5	1010.8 µg/L	1010.8 ppb	18:51:03
1	Sb 206.836†	3825.6	3641.6	492.37 µg/L	492.37 ppb	18:51:03
1	Se 196.026†	1275.8	1232.4	490 µg/L	490 ppb	18:51:03
1	SiO2†	51362.9	48482.5	5278.0 µg/L	5278.0 ppb	18:50:43
1	Si 251.611†	154098.4	149499.2	2462.1 µg/L	2462.1 ppb	18:50:43
1	Sn 189.927†	7147.3	6963.3	496.69 µg/L	496.69 ppb	18:51:03
1	Sr 421.552†	225096.8	213129.1	499.48 µg/L	499.48 ppb	18:50:14
1	Ti 334.940†	496998.7	483710.6	492.59 µg/L	492.59 ppb	18:50:43
1	Tl 190.801†	3658.8	3685.9	502.16 µg/L	502.16 ppb	18:51:03
1	U 409.014†	7304.5	7597.6	499.58 µg/L	499.58 ppb	18:50:43
1	V 292.402†	91666.3	88901.0	499.43 µg/L	499.43 ppb	18:50:43
1	Zn 213.857†	80718.2	78199.0	488.38 µg/L	488.38 ppb	18:50:43
2	Sc 361.383	1735506.8	1735506.8	103.75 %		18:51:06
2	Sc RADIAL	152000.4	152000.4	104 %		18:50:20
2	Y 371.029	1054226.6	1054226.6	103.09 %		18:51:06
2	Ag 328.068†	129107.7	121473.9	499.12 µg/L	499.12 ppb	18:51:06
2	Al 396.153Radial†	24426.5	23454.6	5097.3 µg/L	5097.3 ppb	18:50:20
2	As 188.979†	1211.7	1182.2	501.18 µg/L	501.18 ppb	18:51:26
2	B 249.677†	33876.9	29296.7	490.15 µg/L	490.15 ppb	18:51:06
2	Ba 233.527†	112976.1	109067.5	498.66 µg/L	498.66 ppb	18:51:06
2	Be 313.107†	1597015.9	1539949.6	501.42 µg/L	501.42 ppb	18:51:06
2	Ca 317.933Radial†	89516.0	85221.3	4993.6 µg/L	4993.6 ppb	18:50:20
2	Cd 226.502†	73594.6	71028.9	490.19 µg/L	490.19 ppb	18:51:06
2	Co 228.616†	37103.5	35939.0	492.37 µg/L	492.37 ppb	18:51:06
2	Cr 267.716†	59788.6	57467.2	493.47 µg/L	493.47 ppb	18:51:06
2	Cu 324.752†	121059.6	114258.9	498.22 µg/L	498.22 ppb	18:51:06
2	Fe 238.204 Radial†	77655.1	74350.7	4943.1 µg/L	4943.1 ppb	18:50:20
2	K 766.490 Radial†	15260.2	13178.1	5421.1 µg/L	5421.1 ppb	18:50:20
2	Mg 279.077 IEC†	13002.7	12281.7	5071.5 µg/L	5071.5 ppb	18:50:20
2	Mn 257.610†	375944.4	362275.4	494.81 µg/L	494.81 ppb	18:51:06
2	Mo 202.031†	15890.3	15371.2	485.66 µg/L	485.66 ppb	18:51:26
2	Na 589.592 Radial†	70215.3	65635.2	10038 µg/L	10038 ppb	18:50:20
2	Ni 231.604†	40047.6	38641.0	494.26 µg/L	494.26 ppb	18:51:06
2	P 214.914†	10471.7	10013.6	2389.6 µg/L	2389.6 ppb	18:51:26
2	Pb 220.353†	8484.3	8065.2	490.12 µg/L	490.12 ppb	18:51:26

2	S 181.975 Axial†	1365.8	1221.6	993.82 µg/L	993.82 ppb	18:51:26
2	Sb 206.836†	3834.3	3609.1	487.85 µg/L	487.85 ppb	18:51:26
2	Se 196.026†	1280.6	1223.4	486 µg/L	486 ppb	18:51:26
2	SiO2†	52085.9	48630.3	5294.5 µg/L	5294.5 ppb	18:51:06
2	Si 251.611†	156279.7	149954.3	2469.8 µg/L	2469.8 ppb	18:51:06
2	Sn 189.927†	7113.5	6854.4	488.96 µg/L	488.96 ppb	18:51:26
2	Sr 421.552†	226242.9	217223.8	509.08 µg/L	509.08 ppb	18:50:18
2	Ti 334.940†	504866.7	485981.2	494.91 µg/L	494.91 ppb	18:51:06
2	Tl 190.801†	3631.8	3620.9	493.44 µg/L	493.44 ppb	18:51:26
2	U 409.014†	7123.0	7344.6	483.95 µg/L	483.95 ppb	18:51:06
2	V 292.402†	92685.9	88903.8	499.36 µg/L	499.36 ppb	18:51:06
2	Zn 213.857†	81781.8	78361.2	489.37 µg/L	489.37 ppb	18:51:06
3	Sc 361.383	1735485.3	1735485.3	103.75 %		18:51:29
3	Sc RADIAL	153403.0	153403.0	105 %		18:50:24
3	Y 371.029	1055021.0	1055021.0	103.17 %		18:51:29
3	Ag 328.068†	128496.4	120886.2	496.73 µg/L	496.73 ppb	18:51:29
3	Al 396.153Radial†	24553.1	23360.7	5076.8 µg/L	5076.8 ppb	18:50:24
3	As 188.979†	1228.3	1198.2	507.85 µg/L	507.85 ppb	18:51:49
3	B 249.677†	33764.7	29188.9	488.34 µg/L	488.34 ppb	18:51:29
3	Ba 233.527†	112730.4	108832.0	497.58 µg/L	497.58 ppb	18:51:29
3	Be 313.107†	1593609.1	1536684.9	500.35 µg/L	500.35 ppb	18:51:29
3	Ca 317.933Radial†	90597.1	85463.7	5007.8 µg/L	5007.8 ppb	18:50:24
3	Cd 226.502†	73406.3	70848.2	488.94 µg/L	488.94 ppb	18:51:29
3	Co 228.616†	37011.7	35850.9	491.16 µg/L	491.16 ppb	18:51:29
3	Cr 267.716†	59666.8	57350.6	492.47 µg/L	492.47 ppb	18:51:29
3	Cu 324.752†	120307.7	113535.5	495.08 µg/L	495.08 ppb	18:51:29
3	Fe 238.204 Radial†	78518.4	74490.1	4952.4 µg/L	4952.4 ppb	18:50:24
3	K 766.490 Radial†	15451.9	13226.5	5441.0 µg/L	5441.0 ppb	18:50:24
3	Mg 279.077 IEC†	13189.3	12345.0	5097.6 µg/L	5097.6 ppb	18:50:24
3	Mn 257.610†	374488.1	360876.2	492.90 µg/L	492.90 ppb	18:51:29
3	Mo 202.031†	15929.3	15408.9	486.85 µg/L	486.85 ppb	18:51:49
3	Na 589.592 Radial†	70596.2	65381.5	9999.4 µg/L	9999.4 ppb	18:50:24
3	Ni 231.604†	39740.3	38345.2	490.48 µg/L	490.48 ppb	18:51:29
3	P 214.914†	10488.7	10030.1	2393.6 µg/L	2393.6 ppb	18:51:49
3	Pb 220.353†	8512.5	8092.5	491.77 µg/L	491.77 ppb	18:51:49
3	S 181.975 Axial†	1342.5	1199.2	975.68 µg/L	975.68 ppb	18:51:49
3	Sb 206.836†	3856.9	3630.9	490.82 µg/L	490.82 ppb	18:51:49
3	Se 196.026†	1283.1	1225.8	487 µg/L	487 ppb	18:51:49
3	SiO2†	51906.7	48458.3	5275.6 µg/L	5275.6 ppb	18:51:29
3	Si 251.611†	155757.0	149452.4	2461.5 µg/L	2461.5 ppb	18:51:29
3	Sn 189.927†	7131.5	6871.8	490.19 µg/L	490.19 ppb	18:51:49
3	Sr 421.552†	223596.8	212726.1	498.53 µg/L	498.53 ppb	18:50:22
3	Ti 334.940†	502794.3	483989.7	492.88 µg/L	492.88 ppb	18:51:29
3	Tl 190.801†	3635.4	3624.3	493.87 µg/L	493.87 ppb	18:51:49
3	U 409.014†	7197.3	7416.4	488.32 µg/L	488.32 ppb	18:51:29
3	V 292.402†	92498.4	88724.2	498.37 µg/L	498.37 ppb	18:51:29
3	Zn 213.857†	81445.8	78038.4	487.36 µg/L	487.36 ppb	18:51:29

Mean Data: CCV

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1729154.0	103.37 %	0.657			0.64%
Sc RADIAL	153181.0	105 %	0.7			0.71%
Y 371.029	1051107.5	102.79 %	0.597			0.58%
Ag 328.068†	121249.1	498.21 µg/L	1.295	498.21 ppb	1.295	0.26%
QC value within limits for Ag 328.068 Recovery = 99.64%						
Al 396.153Radial†	23406.1	5086.6 µg/L	10.30	5086.6 ppb	10.30	0.20%
QC value within limits for Al 396.153Radial Recovery = 101.73%						
As 188.979†	1196.6	507.20 µg/L	5.724	507.20 ppb	5.724	1.13%
QC value within limits for As 188.979 Recovery = 101.44%						
B 249.677†	29205.0	488.61 µg/L	1.419	488.61 ppb	1.419	0.29%
QC value within limits for B 249.677 Recovery = 97.72%						
Ba 233.527†	108891.3	497.85 µg/L	0.708	497.85 ppb	0.708	0.14%
QC value within limits for Ba 233.527 Recovery = 99.57%						
Be 313.107†	1536907.7	500.43 µg/L	0.954	500.43 ppb	0.954	0.19%
QC value within limits for Be 313.107 Recovery = 100.09%						
Ca 317.933Radial†	85122.6	4987.8 µg/L	23.42	4987.8 ppb	23.42	0.47%
QC value within limits for Ca 317.933Radial Recovery = 99.76%						
Cd 226.502†	70843.2	488.91 µg/L	1.299	488.91 ppb	1.299	0.27%
QC value within limits for Cd 226.502 Recovery = 97.78%						

Co 228.616†	35838.4	490.99 µg/L	1.470	490.99 ppb	1.470	0.30%
QC value within limits for Co 228.616 Recovery = 98.20%						
Cr 267.716†	57387.4	492.78 µg/L	0.599	492.78 ppb	0.599	0.12%
QC value within limits for Cr 267.716 Recovery = 98.56%						
Cu 324.752†	113845.1	496.42 µg/L	1.617	496.42 ppb	1.617	0.33%
QC value within limits for Cu 324.752 Recovery = 99.28%						
Fe 238.204 Radial†	74287.3	4938.9 µg/L	16.02	4938.9 ppb	16.02	0.32%
QC value within limits for Fe 238.204 Radial Recovery = 98.78%						
K 766.490 Radial†	13215.9	5436.6 µg/L	13.92	5436.6 ppb	13.92	0.26%
QC value within limits for K 766.490 Radial Recovery = 108.73%						
Mg 279.077 IEC†	12292.3	5076.0 µg/L	19.85	5076.0 ppb	19.85	0.39%
QC value within limits for Mg 279.077 IEC Recovery = 101.52%						
Mn 257.610†	361435.1	493.67 µg/L	1.013	493.67 ppb	1.013	0.21%
QC value within limits for Mn 257.610 Recovery = 98.73%						
Mo 202.031†	15466.0	488.65 µg/L	4.194	488.65 ppb	4.194	0.86%
QC value within limits for Mo 202.031 Recovery = 97.73%						
Na 589.592 Radial†	65359.4	9996.0 µg/L	44.02	9996.0 ppb	44.02	0.44%
QC value within limits for Na 589.592 Radial Recovery = 99.96%						
Ni 231.604†	38458.3	491.93 µg/L	2.043	491.93 ppb	2.043	0.42%
QC value within limits for Ni 231.604 Recovery = 98.39%						
P 214.914†	10070.7	2403.3 µg/L	20.35	2403.3 ppb	20.35	0.85%
QC value within limits for P 214.914 Recovery = 96.13%						
Pb 220.353†	8129.5	494.02 µg/L	5.379	494.02 ppb	5.379	1.09%
QC value within limits for Pb 220.353 Recovery = 98.80%						
S 181.975 Axial†	1221.1	993.43 µg/L	17.559	993.43 ppb	17.559	1.77%
QC value within limits for S 181.975 Axial Recovery = 99.34%						
Sb 206.836†	3627.2	490.35 µg/L	2.300	490.35 ppb	2.300	0.47%
QC value within limits for Sb 206.836 Recovery = 98.07%						
Se 196.026†	1227.2	488 µg/L	1.8	488 ppb	1.8	0.38%
QC value within limits for Se 196.026 Recovery = 97.52%						
SiO2†	48523.7	5282.7 µg/L	10.27	5282.7 ppb	10.27	0.19%
QC value within limits for SiO2 Recovery = 98.79%						
Si 251.611†	149635.3	2464.5 µg/L	4.63	2464.5 ppb	4.63	0.19%
QC value within limits for Si 251.611 Recovery = 98.58%						
Sn 189.927†	6896.5	491.95 µg/L	4.158	491.95 ppb	4.158	0.85%
QC value within limits for Sn 189.927 Recovery = 98.39%						
Sr 421.552†	214359.7	502.36 µg/L	5.833	502.36 ppb	5.833	1.16%
QC value within limits for Sr 421.552 Recovery = 100.47%						
Ti 334.940†	484560.5	493.46 µg/L	1.265	493.46 ppb	1.265	0.26%
QC value within limits for Ti 334.940 Recovery = 98.69%						
Tl 190.801†	3643.7	496.49 µg/L	4.915	496.49 ppb	4.915	0.99%
QC value within limits for Tl 190.801 Recovery = 99.30%						
U 409.014†	7452.9	490.62 µg/L	8.063	490.62 ppb	8.063	1.64%
QC value within limits for U 409.014 Recovery = 98.12%						
V 292.402†	88843.0	499.05 µg/L	0.592	499.05 ppb	0.592	0.12%
QC value within limits for V 292.402 Recovery = 99.81%						
Zn 213.857†	78199.5	488.37 µg/L	1.004	488.37 ppb	1.004	0.21%
QC value within limits for Zn 213.857 Recovery = 97.67%						
All analyte(s) passed QC.						

Sequence No.: 14

Sample ID: CCB

Analyst:

Logged In Analyst (Original) : optima4

Initial Sample Wt:

Dilution:

Autosampler Location: 8

Date Collected: 3/29/2010 18:51:58

Data Type: Reprocessed on 3/29/2010 19:14:42

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCB

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc 361.383	1728897.1	1728897.1	103.36 %		18:53:35
1	Sc RADIAL	154974.9	154974.9	106 %		18:52:27
1	Y 371.029	1063835.8	1063835.8	104.03 %		18:53:35
1	Ag 328.068†	3134.9	66.1	0.2939 µg/L	0.2939 ppb	18:53:37
1	Al 396.153Radial†	-26.1	7.3	1.5617 µg/L	1.5617 ppb	18:52:47
1	As 188.979†	-6.1	8.3	3.4794 µg/L	3.4794 ppb	18:53:57
1	B 249.677†	3279.3	-182.9	-3.0715 µg/L	-3.0715 ppb	18:53:57
1	Ba 233.527†	-172.5	8.1	0.0372 µg/L	0.0372 ppb	18:53:57
1	Be 313.107†	-265.8	402.9	0.1379 µg/L	0.1379 ppb	18:53:37
1	Ca 317.933Radial†	701.7	43.7	2.5615 µg/L	2.5615 ppb	18:52:47
1	Cd 226.502†	-78.0	18.9	0.1302 µg/L	0.1302 ppb	18:53:57
1	Co 228.616†	-150.4	31.1	0.4253 µg/L	0.4253 ppb	18:53:57
1	Cr 267.716†	165.7	0.1	-0.0163 µg/L	-0.0163 ppb	18:53:57
1	Cu 324.752†	2708.5	195.7	0.8692 µg/L	0.8692 ppb	18:53:37
1	Fe 238.204 Radial†	162.5	39.6	2.6306 µg/L	2.6306 ppb	18:52:47
1	K 766.490 Radial†	1937.4	367.1	151.11 µg/L	151.11 ppb	18:52:27
1	Mg 279.077 IEC†	162.4	-33.9	-13.972 µg/L	-13.972 ppb	18:52:47
1	Mn 257.610†	174.4	88.7	0.1218 µg/L	0.1218 ppb	18:53:57
1	Mo 202.031†	-30.8	25.4	0.8010 µg/L	0.8010 ppb	18:53:57
1	Na 589.592 Radial†	2342.1	508.0	77.603 µg/L	77.603 ppb	18:52:27
1	Ni 231.604†	-58.4	-15.6	-0.1996 µg/L	-0.1996 ppb	18:53:57
1	P 214.914†	71.2	-10.7	-2.5700 µg/L	-2.5700 ppb	18:53:57
1	Pb 220.353†	154.2	36.7	2.2095 µg/L	2.2095 ppb	18:53:57
1	S 181.975 Axial†	101.6	3.4	2.7893 µg/L	2.7893 ppb	18:53:57
1	Sb 206.836†	90.3	0.8	0.1164 µg/L	0.1164 ppb	18:53:57
1	Se 196.026†	18.0	6.5	2.59 µg/L	2.59 ppb	18:53:57
1	SiO2†	1694.9	67.0	7.2702 µg/L	7.2702 ppb	18:53:57
1	Si 251.611†	856.4	152.3	2.4932 µg/L	2.4932 ppb	18:53:57
1	Sn 189.927†	32.2	29.2	2.0730 µg/L	2.0730 ppb	18:53:57
1	Sr 421.552†	-130.0	155.7	0.3650 µg/L	0.3650 ppb	18:52:27
1	Ti 334.940†	561.4	-93.1	-0.1029 µg/L	-0.1029 ppb	18:53:37
1	Tl 190.801†	-112.5	11.5	1.5393 µg/L	1.5393 ppb	18:53:57
1	U 409.014†	-122.5	360.6	22.274 µg/L	22.274 ppb	18:53:37
1	V 292.402†	422.0	-23.5	-0.1074 µg/L	-0.1074 ppb	18:53:37
1	Zn 213.857†	665.5	179.5	1.1304 µg/L	1.1304 ppb	18:53:57
2	Sc 361.383	1739415.6	1739415.6	103.98 %		18:53:59
2	Sc RADIAL	153949.0	153949.0	106 %		18:52:49
2	Y 371.029	1070599.7	1070599.7	104.70 %		18:53:59
2	Ag 328.068†	3011.7	-70.7	-0.2648 µg/L	-0.2648 ppb	18:54:01
2	Al 396.153Radial†	-22.1	11.0	2.3766 µg/L	2.3766 ppb	18:53:09
2	As 188.979†	-13.6	1.2	0.4948 µg/L	0.4948 ppb	18:54:21
2	B 249.677†	3226.1	-253.2	-4.2510 µg/L	-4.2510 ppb	18:54:21
2	Ba 233.527†	-183.8	-1.7	-0.0082 µg/L	-0.0082 ppb	18:54:21
2	Be 313.107†	-497.9	181.3	0.0661 µg/L	0.0661 ppb	18:54:01
2	Ca 317.933Radial†	683.5	30.9	1.8113 µg/L	1.8113 ppb	18:53:09
2	Cd 226.502†	-81.2	16.3	0.1120 µg/L	0.1120 ppb	18:54:21
2	Co 228.616†	-169.3	13.8	0.1886 µg/L	0.1886 ppb	18:54:21
2	Cr 267.716†	203.3	35.3	0.2845 µg/L	0.2845 ppb	18:54:21
2	Cu 324.752†	2932.9	395.7	1.7397 µg/L	1.7397 ppb	18:54:01
2	Fe 238.204 Radial†	156.9	35.2	2.3419 µg/L	2.3419 ppb	18:53:09
2	K 766.490 Radial†	1851.5	297.9	122.64 µg/L	122.64 ppb	18:52:49
2	Mg 279.077 IEC†	181.3	-15.0	-6.1810 µg/L	-6.1810 ppb	18:53:09
2	Mn 257.610†	185.1	98.0	0.1342 µg/L	0.1342 ppb	18:54:21
2	Mo 202.031†	-40.6	16.1	0.5093 µg/L	0.5093 ppb	18:54:21
2	Na 589.592 Radial†	2203.5	391.5	59.792 µg/L	59.792 ppb	18:52:49
2	Ni 231.604†	-87.1	-42.9	-0.5483 µg/L	-0.5483 ppb	18:54:21
2	P 214.914†	70.7	-11.6	-2.7920 µg/L	-2.7920 ppb	18:54:21
2	Pb 220.353†	120.5	3.4	0.1904 µg/L	0.1904 ppb	18:54:21

2	S 181.975 Axial†	93.2	-5.2	-4.2193 µg/L	-4.2193 ppb	18:54:21
2	Sb 206.836†	93.2	3.0	0.4017 µg/L	0.4017 ppb	18:54:21
2	Se 196.026†	16.5	5.0	1.99 µg/L	1.99 ppb	18:54:21
2	SiO2†	1661.9	25.3	2.7424 µg/L	2.7424 ppb	18:54:21
2	Si 251.611†	798.6	91.6	1.5029 µg/L	1.5029 ppb	18:54:21
2	Sn 189.927†	13.9	11.4	0.8082 µg/L	0.8082 ppb	18:54:21
2	Sr 421.552†	-162.3	124.3	0.2914 µg/L	0.2914 ppb	18:52:49
2	Ti 334.940†	589.0	-69.9	-0.0804 µg/L	-0.0804 ppb	18:54:01
2	Tl 190.801†	-123.3	1.7	0.2267 µg/L	0.2267 ppb	18:54:21
2	U 409.014†	-105.6	377.6	23.300 µg/L	23.300 ppb	18:54:01
2	V 292.402†	344.7	-100.3	-0.5347 µg/L	-0.5347 ppb	18:54:01
2	Zn 213.857†	642.6	153.6	0.9689 µg/L	0.9689 ppb	18:54:21
3	Sc 361.383	1736015.7	1736015.7	103.78 %		18:54:23
3	Sc RADIAL	153754.9	153754.9	105 %		18:53:11
3	Y 371.029	1068282.8	1068282.8	104.47 %		18:54:23
3	Ag 328.068†	2964.9	-110.2	-0.4509 µg/L	-0.4509 ppb	18:54:26
3	Al 396.153Radial†	-16.1	16.6	3.5986 µg/L	3.5986 ppb	18:53:31
3	As 188.979†	-20.3	-5.3	-2.2272 µg/L	-2.2272 ppb	18:54:46
3	B 249.677†	3208.4	-264.2	-4.4364 µg/L	-4.4364 ppb	18:54:46
3	Ba 233.527†	-175.6	5.8	0.0262 µg/L	0.0262 ppb	18:54:46
3	Be 313.107†	-146.9	518.6	0.1704 µg/L	0.1704 ppb	18:54:26
3	Ca 317.933Radial†	709.7	56.6	3.3147 µg/L	3.3147 ppb	18:53:31
3	Cd 226.502†	-66.7	30.1	0.2078 µg/L	0.2078 ppb	18:54:46
3	Co 228.616†	-149.7	32.3	0.4424 µg/L	0.4424 ppb	18:54:46
3	Cr 267.716†	183.5	16.6	0.1380 µg/L	0.1380 ppb	18:54:46
3	Cu 324.752†	2785.8	259.4	1.1323 µg/L	1.1323 ppb	18:54:26
3	Fe 238.204 Radial†	167.4	45.4	3.0195 µg/L	3.0195 ppb	18:53:31
3	K 766.490 Radial†	2004.9	445.6	183.43 µg/L	183.43 ppb	18:53:11
3	Mg 279.077 IEC†	164.0	-31.2	-12.871 µg/L	-12.871 ppb	18:53:31
3	Mn 257.610†	141.8	56.6	0.0779 µg/L	0.0779 ppb	18:54:46
3	Mo 202.031†	-43.5	13.3	0.4189 µg/L	0.4189 ppb	18:54:46
3	Na 589.592 Radial†	2025.0	224.9	34.251 µg/L	34.251 ppb	18:53:11
3	Ni 231.604†	-54.8	-11.9	-0.1527 µg/L	-0.1527 ppb	18:54:46
3	P 214.914†	63.8	-18.1	-4.3341 µg/L	-4.3341 ppb	18:54:46
3	Pb 220.353†	149.8	31.9	1.9285 µg/L	1.9285 ppb	18:54:46
3	S 181.975 Axial†	104.0	5.4	4.3655 µg/L	4.3655 ppb	18:54:46
3	Sb 206.836†	91.0	1.1	0.1457 µg/L	0.1457 ppb	18:54:46
3	Se 196.026†	19.4	7.7	3.06 µg/L	3.06 ppb	18:54:46
3	SiO2†	1644.1	11.4	1.2195 µg/L	1.2195 ppb	18:54:46
3	Si 251.611†	797.5	92.1	1.5112 µg/L	1.5112 ppb	18:54:46
3	Sn 189.927†	13.8	11.3	0.8038 µg/L	0.8038 ppb	18:54:46
3	Sr 421.552†	-194.0	94.1	0.2206 µg/L	0.2206 ppb	18:53:11
3	Ti 334.940†	849.4	182.1	0.1846 µg/L	0.1846 ppb	18:54:26
3	Tl 190.801†	-118.6	6.0	0.7978 µg/L	0.7978 ppb	18:54:46
3	U 409.014†	-409.0	85.0	5.2024 µg/L	5.2024 ppb	18:54:26
3	V 292.402†	290.0	-152.4	-0.8373 µg/L	-0.8373 ppb	18:54:26
3	Zn 213.857†	615.7	128.9	0.8114 µg/L	0.8114 ppb	18:54:46

Mean Data: CCB

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1734776.2	103.71 %	0.321			0.31%
Sc RADIAL	154226.3	106 %	0.4			0.43%
Y 371.029	1067572.8	104.40 %	0.336			0.32%
Ag 328.068†	-38.3	-0.1406 µg/L	0.38763	-0.1406 ppb	0.38763	275.71%
QC value within limits for Ag 328.068 Recovery = Not calculated						
Al 396.153Radial†	11.6	2.5123 µg/L	1.02521	2.5123 ppb	1.02521	40.81%
QC value within limits for Al 396.153Radial Recovery = Not calculated						
As 188.979†	1.4	0.5823 µg/L	2.85430	0.5823 ppb	2.85430	490.14%
QC value within limits for As 188.979 Recovery = Not calculated						
B 249.677†	-233.4	-3.9196 µg/L	0.74029	-3.9196 ppb	0.74029	18.89%
QC value within limits for B 249.677 Recovery = Not calculated						
Ba 233.527†	4.1	0.0184 µg/L	0.02367	0.0184 ppb	0.02367	128.49%
QC value within limits for Ba 233.527 Recovery = Not calculated						
Be 313.107†	367.6	0.1248 µg/L	0.05339	0.1248 ppb	0.05339	42.78%
QC value within limits for Be 313.107 Recovery = Not calculated						
Ca 317.933Radial†	43.7	2.5625 µg/L	0.75170	2.5625 ppb	0.75170	29.33%
QC value within limits for Ca 317.933Radial Recovery = Not calculated						
Cd 226.502†	21.8	0.1500 µg/L	0.05085	0.1500 ppb	0.05085	33.90%
QC value within limits for Cd 226.502 Recovery = Not calculated						

Co 228.616†	25.7	0.3521 µg/L	0.14188	0.3521 ppb	0.14188	40.30%
QC value within limits for Co 228.616 Recovery = Not calculated						
Cr 267.716†	17.3	0.1354 µg/L	0.15041	0.1354 ppb	0.15041	111.10%
QC value within limits for Cr 267.716 Recovery = Not calculated						
Cu 324.752†	283.6	1.2471 µg/L	0.44643	1.2471 ppb	0.44643	35.80%
QC value within limits for Cu 324.752 Recovery = Not calculated						
Fe 238.204 Radial†	40.1	2.6640 µg/L	0.34002	2.6640 ppb	0.34002	12.76%
QC value within limits for Fe 238.204 Radial Recovery = Not calculated						
K 766.490 Radial†	370.2	152.39 µg/L	30.414	152.39 ppb	30.414	19.96%
QC value greater than the upper limit for K 766.490 Radial Recovery = Not calculated						
Mg 279.077 IEC†	-26.7	-11.008 µg/L	4.2166	-11.008 ppb	4.2166	38.30%
QC value within limits for Mg 279.077 IEC Recovery = Not calculated						
Mn 257.610†	81.1	0.1113 µg/L	0.02959	0.1113 ppb	0.02959	26.59%
QC value within limits for Mn 257.610 Recovery = Not calculated						
Mo 202.031†	18.3	0.5764 µg/L	0.19971	0.5764 ppb	0.19971	34.65%
QC value within limits for Mo 202.031 Recovery = Not calculated						
Na 589.592 Radial†	374.8	57.216 µg/L	21.7906	57.216 ppb	21.7906	38.09%
QC value within limits for Na 589.592 Radial Recovery = Not calculated						
Ni 231.604†	-23.5	-0.3002 µg/L	0.21614	-0.3002 ppb	0.21614	72.00%
QC value within limits for Ni 231.604 Recovery = Not calculated						
P 214.914†	-13.5	-3.2320 µg/L	0.96088	-3.2320 ppb	0.96088	29.73%
QC value within limits for P 214.914 Recovery = Not calculated						
Pb 220.353†	24.0	1.4428 µg/L	1.09369	1.4428 ppb	1.09369	75.80%
QC value within limits for Pb 220.353 Recovery = Not calculated						
S 181.975 Axial†	1.2	0.9785 µg/L	4.56987	0.9785 ppb	4.56987	467.04%
QC value within limits for S 181.975 Axial Recovery = Not calculated						
Sb 206.836†	1.6	0.2213 µg/L	0.15695	0.2213 ppb	0.15695	70.93%
QC value within limits for Sb 206.836 Recovery = Not calculated						
Se 196.026†	6.4	2.55 µg/L	0.537	2.55 ppb	0.537	21.07%
QC value within limits for Se 196.026 Recovery = Not calculated						
SiO2†	34.6	3.7440 µg/L	3.14725	3.7440 ppb	3.14725	84.06%
QC value within limits for SiO2 Recovery = Not calculated						
Si 251.611†	112.0	1.8358 µg/L	0.56935	1.8358 ppb	0.56935	31.01%
QC value within limits for Si 251.611 Recovery = Not calculated						
Sn 189.927†	17.3	1.2284 µg/L	0.73152	1.2284 ppb	0.73152	59.55%
QC value within limits for Sn 189.927 Recovery = Not calculated						
Sr 421.552†	124.7	0.2923 µg/L	0.07221	0.2923 ppb	0.07221	24.70%
QC value within limits for Sr 421.552 Recovery = Not calculated						
Ti 334.940†	6.3	0.0004 µg/L	0.15987	0.0004 ppb	0.15987	>999.9%
QC value within limits for Ti 334.940 Recovery = Not calculated						
Tl 190.801†	6.4	0.8546 µg/L	0.65815	0.8546 ppb	0.65815	77.01%
QC value within limits for Tl 190.801 Recovery = Not calculated						
U 409.014†	274.4	16.925 µg/L	10.1653	16.925 ppb	10.1653	60.06%
QC value within limits for U 409.014 Recovery = Not calculated						
V 292.402†	-92.1	-0.4931 µg/L	0.36672	-0.4931 ppb	0.36672	74.37%
QC value within limits for V 292.402 Recovery = Not calculated						
Zn 213.857†	154.0	0.9702 µg/L	0.15951	0.9702 ppb	0.15951	16.44%
QC value within limits for Zn 213.857 Recovery = Not calculated						
QC Failed. Continue with analysis.						

Sequence No.: 15

Sample ID: CCV

Analyst:

Logged In Analyst (Original) : optima4

Initial Sample Wt:

Dilution:

Autosampler Location: 7

Date Collected: 3/29/2010 18:57:39

Data Type: Reprocessed on 3/29/2010 19:14:43

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCV

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc 361.383	1742170.7	1742170.7	104.15 %		18:58:39
1	Sc RADIAL	154515.3	154515.3	106 %		18:58:11
1	Y 371.029	1059060.1	1059060.1	103.57 %		18:58:39
1	Ag 328.068†	129322.6	121204.2	498.05 µg/L	498.05 ppb	18:58:39
1	Al 396.153Radial†	24823.0	23447.4	5095.8 µg/L	5095.8 ppb	18:58:11
1	As 188.979†	1217.4	1183.1	501.56 µg/L	501.56 ppb	18:58:59
1	B 249.677†	33548.3	28856.2	482.76 µg/L	482.76 ppb	18:58:39
1	Ba 233.527†	113126.0	108794.9	497.41 µg/L	497.41 ppb	18:58:39
1	Be 313.107†	1604803.7	1541539.3	501.94 µg/L	501.94 ppb	18:58:39
1	Ca 317.933Radial†	90245.5	84512.4	4952.1 µg/L	4952.1 ppb	18:58:11
1	Cd 226.502†	73575.0	70738.7	488.19 µg/L	488.19 ppb	18:58:39
1	Co 228.616†	37114.9	35813.1	490.65 µg/L	490.65 ppb	18:58:39
1	Cr 267.716†	59986.2	57436.6	493.20 µg/L	493.20 ppb	18:58:39
1	Cu 324.752†	120959.5	113716.5	495.86 µg/L	495.86 ppb	18:58:39
1	Fe 238.204 Radial†	78194.0	73647.1	4896.3 µg/L	4896.3 ppb	18:58:11
1	K 766.490 Radial†	14176.6	11917.8	4902.2 µg/L	4902.2 ppb	18:58:11
1	Mg 279.077 IEC†	13187.4	12253.0	5059.7 µg/L	5059.7 ppb	18:58:11
1	Mn 257.610†	376145.4	361082.3	493.18 µg/L	493.18 ppb	18:58:39
1	Mo 202.031†	15919.4	15340.5	484.69 µg/L	484.69 ppb	18:58:59
1	Na 589.592 Radial†	70146.9	64474.8	9861.1 µg/L	9861.1 ppb	18:58:11
1	Ni 231.604†	39988.6	38436.6	491.65 µg/L	491.65 ppb	18:58:39
1	P 214.914†	10512.2	10013.9	2389.7 µg/L	2389.7 ppb	18:58:59
1	Pb 220.353†	8436.4	7988.0	485.43 µg/L	485.43 ppb	18:58:59
1	S 181.975 Axial†	1318.2	1170.9	952.74 µg/L	952.74 ppb	18:58:59
1	Sb 206.836†	3856.6	3616.3	488.81 µg/L	488.81 ppb	18:58:59
1	Se 196.026†	1269.9	1208.4	480 µg/L	480 ppb	18:58:59
1	SiO2†	51891.1	48251.3	5253.1 µg/L	5253.1 ppb	18:58:39
1	Si 251.611†	155814.4	148931.5	2452.9 µg/L	2452.9 ppb	18:58:39
1	Sn 189.927†	7088.8	6804.4	485.40 µg/L	485.40 ppb	18:58:59
1	Sr 421.552†	226055.0	213515.6	500.39 µg/L	500.39 ppb	18:58:09
1	Ti 334.940†	505203.6	484443.4	493.34 µg/L	493.34 ppb	18:58:39
1	Tl 190.801†	3627.2	3603.0	491.03 µg/L	491.03 ppb	18:58:59
1	U 409.014†	7391.3	7576.0	498.27 µg/L	498.27 ppb	18:58:39
1	V 292.402†	93133.5	88991.9	499.85 µg/L	499.85 ppb	18:58:39
1	Zn 213.857†	81243.9	77543.3	484.25 µg/L	484.25 ppb	18:58:39
2	Sc 361.383	1731918.8	1731918.8	103.54 %		18:59:02
2	Sc RADIAL	153334.6	153334.6	105 %		18:58:15
2	Y 371.029	1053099.9	1053099.9	102.98 %		18:59:02
2	Ag 328.068†	128679.2	121317.8	498.52 µg/L	498.52 ppb	18:59:02
2	Al 396.153Radial†	24533.3	23352.3	5074.9 µg/L	5074.9 ppb	18:58:15
2	As 188.979†	1225.6	1198.0	507.75 µg/L	507.75 ppb	18:59:22
2	B 249.677†	33340.5	28846.3	482.59 µg/L	482.59 ppb	18:59:02
2	Ba 233.527†	112441.8	108777.0	497.33 µg/L	497.33 ppb	18:59:02
2	Be 313.107†	1592364.8	1538646.2	501.00 µg/L	501.00 ppb	18:59:02
2	Ca 317.933Radial†	89792.3	84737.0	4965.2 µg/L	4965.2 ppb	18:58:15
2	Cd 226.502†	73051.4	70651.1	487.59 µg/L	487.59 ppb	18:59:02
2	Co 228.616†	36781.7	35702.2	489.13 µg/L	489.13 ppb	18:59:02
2	Cr 267.716†	59502.2	57310.0	492.11 µg/L	492.11 ppb	18:59:02
2	Cu 324.752†	119947.4	113426.4	494.60 µg/L	494.60 ppb	18:59:02
2	Fe 238.204 Radial†	77968.6	74000.8	4919.8 µg/L	4919.8 ppb	18:58:15
2	K 766.490 Radial†	14058.0	11908.0	4898.2 µg/L	4898.2 ppb	18:58:15
2	Mg 279.077 IEC†	13036.1	12205.0	5039.9 µg/L	5039.9 ppb	18:58:15
2	Mn 257.610†	373427.3	360594.9	492.52 µg/L	492.52 ppb	18:59:02
2	Mo 202.031†	15910.1	15421.9	487.26 µg/L	487.26 ppb	18:59:22
2	Na 589.592 Radial†	69792.3	64647.2	9887.5 µg/L	9887.5 ppb	18:58:15
2	Ni 231.604†	39642.4	38329.5	490.28 µg/L	490.28 ppb	18:59:02
2	P 214.914†	10490.2	10052.4	2398.9 µg/L	2398.9 ppb	18:59:22
2	Pb 220.353†	8461.2	8059.8	489.79 µg/L	489.79 ppb	18:59:22

2	S 181.975 Axial†	1332.4	1192.1	969.89 µg/L	969.89 ppb	18:59:22
2	Sb 206.836†	3845.4	3627.4	490.36 µg/L	490.36 ppb	18:59:22
2	Se 196.026†	1281.0	1226.3	487 µg/L	487 ppb	18:59:22
2	SiO2†	51762.5	48422.0	5271.6 µg/L	5271.6 ppb	18:59:02
2	Si 251.611†	154651.7	148694.0	2448.9 µg/L	2448.9 ppb	18:59:02
2	Sn 189.927†	7107.0	6862.3	489.51 µg/L	489.51 ppb	18:59:22
2	Sr 421.552†	226773.0	215840.0	505.83 µg/L	505.83 ppb	18:58:13
2	Ti 334.940†	500715.6	482980.0	491.85 µg/L	491.85 ppb	18:59:02
2	Tl 190.801†	3643.2	3639.1	495.88 µg/L	495.88 ppb	18:59:22
2	U 409.014†	7329.7	7558.5	497.20 µg/L	497.20 ppb	18:59:02
2	V 292.402†	92631.5	89036.3	500.12 µg/L	500.12 ppb	18:59:02
2	Zn 213.857†	80666.5	77447.4	483.65 µg/L	483.65 ppb	18:59:02
3	Sc 361.383	1731636.7	1731636.7	103.52 %		18:59:25
3	Sc RADIAL	154205.4	154205.4	106 %		18:58:20
3	Y 371.029	1052626.8	1052626.8	102.94 %		18:59:25
3	Ag 328.068†	128532.9	121196.7	498.02 µg/L	498.02 ppb	18:59:25
3	Al 396.153Radial†	24950.8	23615.3	5132.4 µg/L	5132.4 ppb	18:58:20
3	As 188.979†	1233.7	1206.0	511.11 µg/L	511.11 ppb	18:59:45
3	B 249.677†	33475.9	28982.3	484.88 µg/L	484.88 ppb	18:59:25
3	Ba 233.527†	112293.7	108651.6	496.76 µg/L	496.76 ppb	18:59:25
3	Be 313.107†	1590952.1	1537532.1	500.63 µg/L	500.63 ppb	18:59:25
3	Ca 317.933Radial†	90838.5	85244.0	4994.9 µg/L	4994.9 ppb	18:58:20
3	Cd 226.502†	73036.3	70648.1	487.56 µg/L	487.56 ppb	18:59:25
3	Co 228.616†	36829.8	35754.4	489.84 µg/L	489.84 ppb	18:59:25
3	Cr 267.716†	59440.0	57259.2	491.68 µg/L	491.68 ppb	18:59:25
3	Cu 324.752†	119916.0	113414.9	494.56 µg/L	494.56 ppb	18:59:25
3	Fe 238.204 Radial†	78885.0	74448.4	4949.6 µg/L	4949.6 ppb	18:58:20
3	K 766.490 Radial†	14076.3	11849.9	4874.3 µg/L	4874.3 ppb	18:58:20
3	Mg 279.077 IEC†	13322.3	12405.5	5122.6 µg/L	5122.6 ppb	18:58:20
3	Mn 257.610†	373424.5	360651.0	492.59 µg/L	492.59 ppb	18:59:25
3	Mo 202.031†	15880.4	15395.8	486.44 µg/L	486.44 ppb	18:59:45
3	Na 589.592 Radial†	70305.8	64758.0	9904.5 µg/L	9904.5 ppb	18:58:20
3	Ni 231.604†	39803.4	38491.3	492.35 µg/L	492.35 ppb	18:59:25
3	P 214.914†	10482.3	10046.4	2397.5 µg/L	2397.5 ppb	18:59:45
3	Pb 220.353†	8408.9	8010.6	486.81 µg/L	486.81 ppb	18:59:45
3	S 181.975 Axial†	1326.3	1186.4	965.31 µg/L	965.31 ppb	18:59:45
3	Sb 206.836†	3839.9	3622.7	489.73 µg/L	489.73 ppb	18:59:45
3	Se 196.026†	1268.7	1214.6	483 µg/L	483 ppb	18:59:45
3	SiO2†	51614.7	48287.3	5257.0 µg/L	5257.0 ppb	18:59:25
3	Si 251.611†	154566.1	148635.7	2448.0 µg/L	2448.0 ppb	18:59:25
3	Sn 189.927†	7092.3	6849.2	488.58 µg/L	488.58 ppb	18:59:45
3	Sr 421.552†	224060.1	212058.6	496.97 µg/L	496.97 ppb	18:58:17
3	Ti 334.940†	500694.3	483038.2	491.90 µg/L	491.90 ppb	18:59:25
3	Tl 190.801†	3646.3	3642.7	496.35 µg/L	496.35 ppb	18:59:45
3	U 409.014†	7327.6	7557.6	497.15 µg/L	497.15 ppb	18:59:25
3	V 292.402†	92621.5	89041.2	500.13 µg/L	500.13 ppb	18:59:25
3	Zn 213.857†	80736.0	77527.2	484.14 µg/L	484.14 ppb	18:59:25

Mean Data: CCV

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1735242.1	103.73 %	0.359			0.35%
Sc RADIAL	154018.4	106 %	0.4			0.40%
Y 371.029	1054928.9	103.16 %	0.351			0.34%
Ag 328.068†	121239.6	498.20 µg/L	0.276	498.20 ppb	0.276	0.06%
QC value within limits for Ag 328.068 Recovery = 99.64%						
Al 396.153Radial†	23471.7	5101.0 µg/L	29.08	5101.0 ppb	29.08	0.57%
QC value within limits for Al 396.153Radial Recovery = 102.02%						
As 188.979†	1195.7	506.81 µg/L	4.846	506.81 ppb	4.846	0.96%
QC value within limits for As 188.979 Recovery = 101.36%						
B 249.677†	28895.0	483.41 µg/L	1.273	483.41 ppb	1.273	0.26%
QC value within limits for B 249.677 Recovery = 96.68%						
Ba 233.527†	108741.2	497.17 µg/L	0.357	497.17 ppb	0.357	0.07%
QC value within limits for Ba 233.527 Recovery = 99.43%						
Be 313.107†	1539239.2	501.19 µg/L	0.673	501.19 ppb	0.673	0.13%
QC value within limits for Be 313.107 Recovery = 100.24%						
Ca 317.933Radial†	84831.1	4970.7 µg/L	21.96	4970.7 ppb	21.96	0.44%
QC value within limits for Ca 317.933Radial Recovery = 99.41%						
Cd 226.502†	70679.3	487.78 µg/L	0.358	487.78 ppb	0.358	0.07%
QC value within limits for Cd 226.502 Recovery = 97.56%						

Co 228.616†	35756.6	489.87 µg/L	0.760	489.87 ppb	0.760	0.16%
QC value within limits for Co 228.616 Recovery = 97.97%						
Cr 267.716†	57335.3	492.33 µg/L	0.783	492.33 ppb	0.783	0.16%
QC value within limits for Cr 267.716 Recovery = 98.47%						
Cu 324.752†	113519.3	495.01 µg/L	0.740	495.01 ppb	0.740	0.15%
QC value within limits for Cu 324.752 Recovery = 99.00%						
Fe 238.204 Radial†	74032.1	4921.9 µg/L	26.70	4921.9 ppb	26.70	0.54%
QC value within limits for Fe 238.204 Radial Recovery = 98.44%						
K 766.490 Radial†	11891.9	4891.6 µg/L	15.12	4891.6 ppb	15.12	0.31%
QC value within limits for K 766.490 Radial Recovery = 97.83%						
Mg 279.077 IEC†	12287.8	5074.1 µg/L	43.14	5074.1 ppb	43.14	0.85%
QC value within limits for Mg 279.077 IEC Recovery = 101.48%						
Mn 257.610†	360776.1	492.77 µg/L	0.365	492.77 ppb	0.365	0.07%
QC value within limits for Mn 257.610 Recovery = 98.55%						
Mo 202.031†	15386.1	486.13 µg/L	1.313	486.13 ppb	1.313	0.27%
QC value within limits for Mo 202.031 Recovery = 97.23%						
Na 589.592 Radial†	64626.7	9884.4 µg/L	21.84	9884.4 ppb	21.84	0.22%
QC value within limits for Na 589.592 Radial Recovery = 98.84%						
Ni 231.604†	38419.1	491.43 µg/L	1.053	491.43 ppb	1.053	0.21%
QC value within limits for Ni 231.604 Recovery = 98.29%						
P 214.914†	10037.5	2395.4 µg/L	4.95	2395.4 ppb	4.95	0.21%
QC value within limits for P 214.914 Recovery = 95.81%						
Pb 220.353†	8019.5	487.34 µg/L	2.227	487.34 ppb	2.227	0.46%
QC value within limits for Pb 220.353 Recovery = 97.47%						
S 181.975 Axial†	1183.1	962.65 µg/L	8.881	962.65 ppb	8.881	0.92%
QC value within limits for S 181.975 Axial Recovery = 96.26%						
Sb 206.836†	3622.2	489.63 µg/L	0.781	489.63 ppb	0.781	0.16%
QC value within limits for Sb 206.836 Recovery = 97.93%						
Se 196.026†	1216.4	483 µg/L	3.6	483 ppb	3.6	0.75%
QC value within limits for Se 196.026 Recovery = 96.66%						
SiO2†	48320.2	5260.6 µg/L	9.78	5260.6 ppb	9.78	0.19%
QC value within limits for SiO2 Recovery = 98.37%						
Si 251.611†	148753.7	2449.9 µg/L	2.62	2449.9 ppb	2.62	0.11%
QC value within limits for Si 251.611 Recovery = 98.00%						
Sn 189.927†	6838.6	487.83 µg/L	2.157	487.83 ppb	2.157	0.44%
QC value within limits for Sn 189.927 Recovery = 97.57%						
Sr 421.552†	213804.8	501.06 µg/L	4.470	501.06 ppb	4.470	0.89%
QC value within limits for Sr 421.552 Recovery = 100.21%						
Ti 334.940†	483487.2	492.36 µg/L	0.845	492.36 ppb	0.845	0.17%
QC value within limits for Ti 334.940 Recovery = 98.47%						
Tl 190.801†	3628.3	494.42 µg/L	2.943	494.42 ppb	2.943	0.60%
QC value within limits for Tl 190.801 Recovery = 98.88%						
U 409.014†	7564.0	497.54 µg/L	0.636	497.54 ppb	0.636	0.13%
QC value within limits for U 409.014 Recovery = 99.51%						
V 292.402†	89023.2	500.03 µg/L	0.157	500.03 ppb	0.157	0.03%
QC value within limits for V 292.402 Recovery = 100.01%						
Zn 213.857†	77506.0	484.01 µg/L	0.318	484.01 ppb	0.318	0.07%
QC value within limits for Zn 213.857 Recovery = 96.80%						
All analyte(s) passed QC.						

Sequence No.: 16

Sample ID: CCB

Analyst:

Logged In Analyst (Original) : optima4

Initial Sample Wt:

Dilution:

Autosampler Location: 8

Date Collected: 3/29/2010 18:59:54

Data Type: Reprocessed on 3/29/2010 19:14:44

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCB

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc 361.383	1743930.9	1743930.9	104.25 %		19:01:45
1	Sc RADIAL	157207.9	157207.9	108 %		19:00:23
1	Y 371.029	1072817.8	1072817.8	104.91 %		19:01:45
1	Ag 328.068†	2785.5	-295.2	-1.1824 µg/L	-1.1824 ppb	19:01:47
1	Al 396.153Radial†	-35.9	-1.4	-0.3269 µg/L	-0.3269 ppb	19:00:43
1	As 188.979†	-9.7	4.9	2.0592 µg/L	2.0592 ppb	19:02:07
1	B 249.677†	3169.2	-315.8	-5.3028 µg/L	-5.3028 ppb	19:02:07
1	Ba 233.527†	-172.8	9.3	0.0423 µg/L	0.0423 ppb	19:02:07
1	Be 313.107†	-580.2	103.6	0.0392 µg/L	0.0392 ppb	19:01:47
1	Ca 317.933Radial†	703.1	35.6	2.0888 µg/L	2.0888 ppb	19:00:43
1	Cd 226.502†	-117.2	-18.0	-0.1248 µg/L	-0.1248 ppb	19:02:07
1	Co 228.616†	-175.0	8.7	0.1195 µg/L	0.1195 ppb	19:02:07
1	Cr 267.716†	174.7	7.4	0.0489 µg/L	0.0489 ppb	19:02:07
1	Cu 324.752†	2833.3	292.9	1.2883 µg/L	1.2883 ppb	19:01:47
1	Fe 238.204 Radial†	147.5	23.5	1.5605 µg/L	1.5605 ppb	19:00:43
1	K 766.490 Radial†	1652.9	77.5	31.907 µg/L	31.907 ppb	19:00:23
1	Mg 279.077 IEC†	179.9	-19.9	-8.1726 µg/L	-8.1726 ppb	19:00:43
1	Mn 257.610†	174.5	87.4	0.1197 µg/L	0.1197 ppb	19:02:07
1	Mo 202.031†	-38.4	18.4	0.5797 µg/L	0.5797 ppb	19:02:07
1	Na 589.592 Radial†	1931.7	96.3	14.699 µg/L	14.699 ppb	19:00:23
1	Ni 231.604†	-49.3	-6.4	-0.0822 µg/L	-0.0822 ppb	19:02:07
1	P 214.914†	78.3	-4.5	-1.0824 µg/L	-1.0824 ppb	19:02:07
1	Pb 220.353†	116.5	-0.7	-0.0551 µg/L	-0.0551 ppb	19:02:07
1	S 181.975 Axial†	92.5	-6.1	-4.9234 µg/L	-4.9234 ppb	19:02:07
1	Sb 206.836†	87.4	-2.8	-0.3729 µg/L	-0.3729 ppb	19:02:07
1	Se 196.026†	21.5	9.7	3.85 µg/L	3.85 ppb	19:02:07
1	SiO2†	1662.9	22.2	2.3983 µg/L	2.3983 ppb	19:02:07
1	Si 251.611†	781.9	73.6	1.2037 µg/L	1.2037 ppb	19:02:07
1	Sn 189.927†	15.0	12.4	0.8828 µg/L	0.8828 ppb	19:02:07
1	Sr 421.552†	-145.8	142.8	0.3347 µg/L	0.3347 ppb	19:00:23
1	Ti 334.940†	822.4	152.5	0.1487 µg/L	0.1487 ppb	19:01:47
1	Tl 190.801†	-112.5	12.4	1.6651 µg/L	1.6651 ppb	19:02:07
1	U 409.014†	-191.3	295.6	18.231 µg/L	18.231 ppb	19:01:47
1	V 292.402†	340.4	-105.3	-0.5658 µg/L	-0.5658 ppb	19:01:47
1	Zn 213.857†	528.4	42.4	0.2666 µg/L	0.2666 ppb	19:02:07
2	Sc 361.383	1749880.6	1749880.6	104.61 %		19:02:09
2	Sc RADIAL	154607.9	154607.9	106 %		19:00:45
2	Y 371.029	1075429.4	1075429.4	105.17 %		19:02:09
2	Ag 328.068†	2854.9	-238.0	-0.9266 µg/L	-0.9266 ppb	19:02:11
2	Al 396.153Radial†	-53.8	-18.9	-4.1894 µg/L	-4.1894 ppb	19:01:05
2	As 188.979†	-8.5	6.1	2.5641 µg/L	2.5641 ppb	19:02:31
2	B 249.677†	3184.7	-311.3	-5.2277 µg/L	-5.2277 ppb	19:02:31
2	Ba 233.527†	-166.1	16.2	0.0743 µg/L	0.0743 ppb	19:02:31
2	Be 313.107†	-429.5	249.5	0.0921 µg/L	0.0921 ppb	19:02:11
2	Ca 317.933Radial†	674.2	19.4	1.1395 µg/L	1.1395 ppb	19:01:05
2	Cd 226.502†	-92.3	6.1	0.0422 µg/L	0.0422 ppb	19:02:31
2	Co 228.616†	-147.4	35.7	0.4889 µg/L	0.4889 ppb	19:02:31
2	Cr 267.716†	146.6	-20.1	-0.2010 µg/L	-0.2010 ppb	19:02:31
2	Cu 324.752†	2740.1	194.5	0.8753 µg/L	0.8753 ppb	19:02:11
2	Fe 238.204 Radial†	152.9	30.9	2.0532 µg/L	2.0532 ppb	19:01:05
2	K 766.490 Radial†	1696.1	144.0	59.261 µg/L	59.261 ppb	19:00:45
2	Mg 279.077 IEC†	164.9	-31.2	-12.828 µg/L	-12.828 ppb	19:01:05
2	Mn 257.610†	159.3	72.2	0.0992 µg/L	0.0992 ppb	19:02:31
2	Mo 202.031†	-10.4	45.2	1.4272 µg/L	1.4272 ppb	19:02:31
2	Na 589.592 Radial†	1913.7	109.4	16.687 µg/L	16.687 ppb	19:00:45
2	Ni 231.604†	-34.9	7.5	0.0960 µg/L	0.0960 ppb	19:02:31
2	P 214.914†	88.9	5.5	1.2769 µg/L	1.2769 ppb	19:02:31
2	Pb 220.353†	116.9	-0.7	-0.0641 µg/L	-0.0641 ppb	19:02:31

2	S 181.975 Axial†	98.1	-1.0	-0.8273 µg/L	-0.8273 ppb	19:02:31
2	Sb 206.836†	79.8	-10.4	-1.3806 µg/L	-1.3806 ppb	19:02:31
2	Se 196.026†	23.1	11.2	4.46 µg/L	4.46 ppb	19:02:31
2	SiO2†	1662.3	16.2	1.7388 µg/L	1.7388 ppb	19:02:31
2	Si 251.611†	771.7	61.4	0.9975 µg/L	0.9975 ppb	19:02:31
2	Sn 189.927†	-2.4	-4.3	-0.3060 µg/L	-0.3060 ppb	19:02:31
2	Sr 421.552†	-168.4	119.2	0.2795 µg/L	0.2795 ppb	19:00:45
2	Ti 334.940†	843.2	169.7	0.1595 µg/L	0.1595 ppb	19:02:11
2	Tl 190.801†	-115.5	9.9	1.3206 µg/L	1.3206 ppb	19:02:31
2	U 409.014†	109.4	583.7	36.043 µg/L	36.043 ppb	19:02:11
2	V 292.402†	368.0	-80.0	-0.4063 µg/L	-0.4063 ppb	19:02:11
2	Zn 213.857†	532.3	44.4	0.2783 µg/L	0.2783 ppb	19:02:31
3	Sc 361.383	1734424.8	1734424.8	103.69 %		19:02:33
3	Sc RADIAL	152171.1	152171.1	104 %		19:01:07
3	Y 371.029	1067156.7	1067156.7	104.36 %		19:02:33
3	Ag 328.068†	2902.9	-167.4	-0.6806 µg/L	-0.6806 ppb	19:02:36
3	Al 396.153Radial†	-58.9	-24.5	-5.3555 µg/L	-5.3555 ppb	19:01:27
3	As 188.979†	-18.7	-3.8	-1.5762 µg/L	-1.5762 ppb	19:02:56
3	B 249.677†	3166.5	-301.7	-5.0666 µg/L	-5.0666 ppb	19:02:56
3	Ba 233.527†	-187.7	-6.0	-0.0277 µg/L	-0.0277 ppb	19:02:56
3	Be 313.107†	-333.0	339.0	0.1115 µg/L	0.1115 ppb	19:02:36
3	Ca 317.933Radial†	709.2	63.1	3.6954 µg/L	3.6954 ppb	19:01:27
3	Cd 226.502†	-99.5	-1.5	-0.0105 µg/L	-0.0105 ppb	19:02:56
3	Co 228.616†	-170.8	11.9	0.1624 µg/L	0.1624 ppb	19:02:56
3	Cr 267.716†	184.7	17.9	0.1506 µg/L	0.1506 ppb	19:02:56
3	Cu 324.752†	2715.6	194.2	0.8472 µg/L	0.8472 ppb	19:02:36
3	Fe 238.204 Radial†	137.1	18.1	1.2007 µg/L	1.2007 ppb	19:01:27
3	K 766.490 Radial†	1528.8	9.4	3.8507 µg/L	3.8507 ppb	19:01:07
3	Mg 279.077 IEC†	173.3	-20.7	-8.5238 µg/L	-8.5238 ppb	19:01:27
3	Mn 257.610†	141.1	56.1	0.0769 µg/L	0.0769 ppb	19:02:56
3	Mo 202.031†	-52.8	4.2	0.1336 µg/L	0.1336 ppb	19:02:56
3	Na 589.592 Radial†	1839.9	67.6	10.341 µg/L	10.341 ppb	19:01:07
3	Ni 231.604†	-39.3	3.0	0.0386 µg/L	0.0386 ppb	19:02:56
3	P 214.914†	57.3	-24.3	-5.8246 µg/L	-5.8246 ppb	19:02:56
3	Pb 220.353†	120.4	3.6	0.2179 µg/L	0.2179 ppb	19:02:56
3	S 181.975 Axial†	88.1	-9.8	-7.9574 µg/L	-7.9574 ppb	19:02:56
3	Sb 206.836†	87.1	-2.6	-0.3549 µg/L	-0.3549 ppb	19:02:56
3	Se 196.026†	3.8	-7.2	-2.85 µg/L	-2.85 ppb	19:02:56
3	SiO2†	1649.9	18.4	1.9980 µg/L	1.9980 ppb	19:02:56
3	Si 251.611†	767.7	64.1	1.0530 µg/L	1.0530 ppb	19:02:56
3	Sn 189.927†	11.8	9.4	0.6667 µg/L	0.6667 ppb	19:02:56
3	Sr 421.552†	-198.5	87.9	0.2060 µg/L	0.2060 ppb	19:01:07
3	Ti 334.940†	650.8	-8.7	-0.0097 µg/L	-0.0097 ppb	19:02:36
3	Tl 190.801†	-110.3	13.9	1.8642 µg/L	1.8642 ppb	19:02:56
3	U 409.014†	-434.4	60.1	3.6852 µg/L	3.6852 ppb	19:02:36
3	V 292.402†	355.5	-88.9	-0.4890 µg/L	-0.4890 ppb	19:02:36
3	Zn 213.857†	538.0	54.5	0.3420 µg/L	0.3420 ppb	19:02:56

Mean Data: CCB

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1742745.4	104.18 %	0.466			0.45%
Sc RADIAL	154662.3	106 %	1.7			1.63%
Y 371.029	1071801.3	104.81 %	0.414			0.39%
Ag 328.068†	-233.5	-0.9298 µg/L	0.25091	-0.9298 ppb	0.25091	26.98%
QC value within limits for Ag 328.068 Recovery = Not calculated						
Al 396.153Radial†	-14.9	-3.2906 µg/L	2.63203	-3.2906 ppb	2.63203	79.99%
QC value within limits for Al 396.153Radial Recovery = Not calculated						
As 188.979†	2.4	1.0157 µg/L	2.25883	1.0157 ppb	2.25883	222.39%
QC value within limits for As 188.979 Recovery = Not calculated						
B 249.677†	-309.6	-5.1990 µg/L	0.12069	-5.1990 ppb	0.12069	2.32%
QC value within limits for B 249.677 Recovery = Not calculated						
Ba 233.527†	6.5	0.0297 µg/L	0.05216	0.0297 ppb	0.05216	175.89%
QC value within limits for Ba 233.527 Recovery = Not calculated						
Be 313.107†	230.7	0.0809 µg/L	0.03739	0.0809 ppb	0.03739	46.19%
QC value within limits for Be 313.107 Recovery = Not calculated						
Ca 317.933Radial†	39.4	2.3079 µg/L	1.29199	2.3079 ppb	1.29199	55.98%
QC value within limits for Ca 317.933Radial Recovery = Not calculated						
Cd 226.502†	-4.5	-0.0310 µg/L	0.08537	-0.0310 ppb	0.08537	275.14%
QC value within limits for Cd 226.502 Recovery = Not calculated						

Co 228.616†	18.8	0.2569 µg/L	0.20203	0.2569 ppb	0.20203	78.63%
QC value within limits for Co 228.616 Recovery = Not calculated						
Cr 267.716†	1.7	-0.0005 µg/L	0.18092	-0.0005 ppb	0.18092	>999.9%
QC value within limits for Cr 267.716 Recovery = Not calculated						
Cu 324.752†	227.2	1.0036 µg/L	0.24693	1.0036 ppb	0.24693	24.60%
QC value within limits for Cu 324.752 Recovery = Not calculated						
Fe 238.204 Radial†	24.1	1.6048 µg/L	0.42799	1.6048 ppb	0.42799	26.67%
QC value within limits for Fe 238.204 Radial Recovery = Not calculated						
K 766.490 Radial†	76.9	31.673 µg/L	27.7059	31.673 ppb	27.7059	87.48%
QC value within limits for K 766.490 Radial Recovery = Not calculated						
Mg 279.077 IEC†	-23.9	-9.8414 µg/L	2.59218	-9.8414 ppb	2.59218	26.34%
QC value within limits for Mg 279.077 IEC Recovery = Not calculated						
Mn 257.610†	71.9	0.0986 µg/L	0.02141	0.0986 ppb	0.02141	21.70%
QC value within limits for Mn 257.610 Recovery = Not calculated						
Mo 202.031†	22.6	0.7135 µg/L	0.65711	0.7135 ppb	0.65711	92.10%
QC value within limits for Mo 202.031 Recovery = Not calculated						
Na 589.592 Radial†	91.1	13.909 µg/L	3.2461	13.909 ppb	3.2461	23.34%
QC value within limits for Na 589.592 Radial Recovery = Not calculated						
Ni 231.604†	1.4	0.0175 µg/L	0.09096	0.0175 ppb	0.09096	520.03%
QC value within limits for Ni 231.604 Recovery = Not calculated						
P 214.914†	-7.8	-1.8767 µg/L	3.61681	-1.8767 ppb	3.61681	192.72%
QC value within limits for P 214.914 Recovery = Not calculated						
Pb 220.353†	0.8	0.0329 µg/L	0.16029	0.0329 ppb	0.16029	486.83%
QC value within limits for Pb 220.353 Recovery = Not calculated						
S 181.975 Axial†	-5.6	-4.5694 µg/L	3.57820	-4.5694 ppb	3.57820	78.31%
QC value within limits for S 181.975 Axial Recovery = Not calculated						
Sb 206.836†	-5.3	-0.7028 µg/L	0.58704	-0.7028 ppb	0.58704	83.53%
QC value within limits for Sb 206.836 Recovery = Not calculated						
Se 196.026†	4.6	1.82 µg/L	4.054	1.82 ppb	4.054	222.54%
QC value within limits for Se 196.026 Recovery = Not calculated						
SiO2†	19.0	2.0451 µg/L	0.33227	2.0451 ppb	0.33227	16.25%
QC value within limits for SiO2 Recovery = Not calculated						
Si 251.611†	66.3	1.0847 µg/L	0.10673	1.0847 ppb	0.10673	9.84%
QC value within limits for Si 251.611 Recovery = Not calculated						
Sn 189.927†	5.8	0.4145 µg/L	0.63329	0.4145 ppb	0.63329	152.78%
QC value within limits for Sn 189.927 Recovery = Not calculated						
Sr 421.552†	116.6	0.2734 µg/L	0.06458	0.2734 ppb	0.06458	23.62%
QC value within limits for Sr 421.552 Recovery = Not calculated						
Ti 334.940†	104.5	0.0995 µg/L	0.09469	0.0995 ppb	0.09469	95.16%
QC value within limits for Ti 334.940 Recovery = Not calculated						
Tl 190.801†	12.1	1.6167 µg/L	0.27502	1.6167 ppb	0.27502	17.01%
QC value within limits for Tl 190.801 Recovery = Not calculated						
U 409.014†	313.1	19.320 µg/L	16.2065	19.320 ppb	16.2065	83.89%
QC value within limits for U 409.014 Recovery = Not calculated						
V 292.402†	-91.4	-0.4870 µg/L	0.07980	-0.4870 ppb	0.07980	16.39%
QC value within limits for V 292.402 Recovery = Not calculated						
Zn 213.857†	47.1	0.2956 µg/L	0.04054	0.2956 ppb	0.04054	13.71%
QC value within limits for Zn 213.857 Recovery = Not calculated						
All analyte(s) passed QC.						

Sequence No.: 8

Sample ID: CCV

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 7

Date Collected: 3/29/2010 19:31:23

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCV

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	154889.6	154889.6	106 %		19:31:56
1	Al 396.153Radial†	25248.9	23791.6	5171.1 µg/L	5171.1 ppb	19:31:56
1	Ca 317.933Radial†	90787.7	84816.9	4969.9 µg/L	4969.9 ppb	19:31:56
1	Fe 238.204 Radial†	79020.5	74246.6	4936.2 µg/L	4936.2 ppb	19:31:56
1	K 766.490 Radial†	14072.9	11787.9	4848.7 µg/L	4848.7 ppb	19:31:56
1	Mg 279.077 IEC†	13305.1	12333.7	5092.8 µg/L	5092.8 ppb	19:31:56
1	Na 589.592 Radial†	70517.8	64663.9	9890.1 µg/L	9890.1 ppb	19:31:56
1	Sr 421.552†	229051.2	215819.7	505.79 µg/L	505.79 ppb	19:31:54
1	Sc 361.383	1743822.4	1743822.4	104.25 %		19:32:23
1	Y 371.029	1059163.2	1059163.2	103.58 %		19:32:23
1	Ag 328.068†	128580.1	120374.3	494.64 µg/L	494.64 ppb	19:32:23
1	As 188.979†	1249.3	1212.6	513.82 µg/L	513.82 ppb	19:32:43
1	B 249.677†	33313.2	28600.3	478.47 µg/L	478.47 ppb	19:32:23
1	Ba 233.527†	113123.6	108689.7	496.93 µg/L	496.93 ppb	19:32:23
1	Be 313.107†	1610699.9	1545735.8	503.30 µg/L	503.30 ppb	19:32:23
1	Cd 226.502†	72730.5	69861.7	482.13 µg/L	482.13 ppb	19:32:23
1	Co 228.616†	36860.0	35534.8	486.84 µg/L	486.84 ppb	19:32:23
1	Cr 267.716†	59413.7	56832.8	488.02 µg/L	488.02 ppb	19:32:23
1	Cu 324.752†	120074.9	112757.8	491.69 µg/L	491.69 ppb	19:32:23
1	Mn 257.610†	374470.1	359133.2	490.52 µg/L	490.52 ppb	19:32:23
1	Mo 202.031†	15834.2	15244.3	481.66 µg/L	481.66 ppb	19:32:43
1	Ni 231.604†	39808.6	38227.6	488.98 µg/L	488.98 ppb	19:32:23
1	P 214.914†	10378.9	9876.5	2356.8 µg/L	2356.8 ppb	19:32:43
1	Pb 220.353†	8316.1	7864.8	477.97 µg/L	477.97 ppb	19:32:43
1	S 181.975 Axial†	1303.7	1155.8	940.47 µg/L	940.47 ppb	19:32:43
1	Sb 206.836†	3839.6	3596.5	486.17 µg/L	486.17 ppb	19:32:43
1	Se 196.026†	1266.7	1204.2	478 µg/L	478 ppb	19:32:43
1	SiO2†	51618.1	47942.2	5219.4 µg/L	5219.4 ppb	19:32:23
1	Si 251.611†	154593.2	147618.3	2431.2 µg/L	2431.2 ppb	19:32:23
1	Sn 189.927†	7080.7	6790.2	484.38 µg/L	484.38 ppb	19:32:43
1	Ti 334.940†	502894.8	481769.2	490.61 µg/L	490.61 ppb	19:32:23
1	Tl 190.801†	3593.0	3566.9	486.15 µg/L	486.15 ppb	19:32:43
1	U 409.014†	7303.3	7484.9	492.46 µg/L	492.46 ppb	19:32:23
1	V 292.402†	92682.1	88474.1	496.92 µg/L	496.92 ppb	19:32:23
1	Zn 213.857†	80453.5	76711.2	479.02 µg/L	479.02 ppb	19:32:23
2	Sc RADIAL	155203.4	155203.4	106 %		19:32:01
2	Al 396.153Radial†	25234.3	23729.9	5157.5 µg/L	5157.5 ppb	19:32:01
2	Ca 317.933Radial†	90949.0	84795.6	4968.7 µg/L	4968.7 ppb	19:32:01
2	Fe 238.204 Radial†	79090.7	74162.2	4930.6 µg/L	4930.6 ppb	19:32:01
2	K 766.490 Radial†	13942.4	11638.6	4787.3 µg/L	4787.3 ppb	19:32:01
2	Mg 279.077 IEC†	13250.9	12257.5	5061.5 µg/L	5061.5 ppb	19:32:01
2	Na 589.592 Radial†	70292.0	64317.7	9837.2 µg/L	9837.2 ppb	19:32:01
2	Sr 421.552†	228066.3	214459.1	502.60 µg/L	502.60 ppb	19:31:59
2	Sc 361.383	1737215.7	1737215.7	103.85 %		19:32:47
2	Y 371.029	1054931.1	1054931.1	103.16 %		19:32:47
2	Ag 328.068†	128483.5	120750.5	496.17 µg/L	496.17 ppb	19:32:47
2	As 188.979†	1256.3	1223.9	518.55 µg/L	518.55 ppb	19:33:07
2	B 249.677†	33149.8	28564.4	477.87 µg/L	477.87 ppb	19:32:47
2	Ba 233.527†	112832.9	108822.5	497.54 µg/L	497.54 ppb	19:32:47
2	Be 313.107†	1606762.7	1547820.7	503.98 µg/L	503.98 ppb	19:32:47
2	Cd 226.502†	72368.9	69778.8	481.56 µg/L	481.56 ppb	19:32:47
2	Co 228.616†	36711.4	35526.2	486.72 µg/L	486.72 ppb	19:32:47
2	Cr 267.716†	59192.4	56836.4	488.05 µg/L	488.05 ppb	19:32:47
2	Cu 324.752†	119958.6	113083.9	493.10 µg/L	493.10 ppb	19:32:47
2	Mn 257.610†	372915.3	359002.2	490.34 µg/L	490.34 ppb	19:32:47
2	Mo 202.031†	15840.2	15307.8	483.66 µg/L	483.66 ppb	19:33:07
2	Ni 231.604†	39651.1	38221.1	488.89 µg/L	488.89 ppb	19:32:47
2	P 214.914†	10418.1	9952.1	2374.9 µg/L	2374.9 ppb	19:33:07
2	Pb 220.353†	8335.8	7914.1	480.97 µg/L	480.97 ppb	19:33:07

2	S 181.975 Axial†	1310.0	1166.6	949.21 µg/L	949.21 ppb	19:33:07
2	Sb 206.836†	3818.2	3589.9	485.30 µg/L	485.30 ppb	19:33:07
2	Se 196.026†	1256.0	1198.5	476 µg/L	476 ppb	19:33:07
2	SiO2†	51436.2	47955.4	5220.8 µg/L	5220.8 ppb	19:32:47
2	Si 251.611†	154237.0	147839.3	2434.9 µg/L	2434.9 ppb	19:32:47
2	Sn 189.927†	7075.7	6811.2	485.88 µg/L	485.88 ppb	19:33:07
2	Ti 334.940†	501670.2	482424.6	491.29 µg/L	491.29 ppb	19:32:47
2	Tl 190.801†	3598.0	3584.8	488.57 µg/L	488.57 ppb	19:33:07
2	U 409.014†	7114.9	7330.1	482.93 µg/L	482.93 ppb	19:32:47
2	V 292.402†	92447.3	88586.2	497.56 µg/L	497.56 ppb	19:32:47
2	Zn 213.857†	80237.4	76796.6	479.56 µg/L	479.56 ppb	19:32:47
3	Sc RADIAL	152343.2	152343.2	105 %		19:32:05
3	Al 396.153Radial†	24790.2	23749.9	5162.0 µg/L	5162.0 ppb	19:32:05
3	Ca 317.933Radial†	88711.7	84258.7	4937.2 µg/L	4937.2 ppb	19:32:05
3	Fe 238.204 Radial†	77301.6	73844.9	4909.5 µg/L	4909.5 ppb	19:32:05
3	K 766.490 Radial†	13851.3	11797.3	4852.6 µg/L	4852.6 ppb	19:32:05
3	Mg 279.077 IEC†	12897.2	12152.7	5018.2 µg/L	5018.2 ppb	19:32:05
3	Na 589.592 Radial†	69172.5	64486.0	9862.9 µg/L	9862.9 ppb	19:32:05
3	Sr 421.552†	226674.9	217149.0	508.90 µg/L	508.90 ppb	19:32:03
3	Sc 361.383	1739184.0	1739184.0	103.97 %		19:33:10
3	Y 371.029	1056341.4	1056341.4	103.30 %		19:33:10
3	Ag 328.068†	128938.9	121048.4	497.41 µg/L	497.41 ppb	19:33:10
3	As 188.979†	1242.3	1209.1	512.38 µg/L	512.38 ppb	19:33:30
3	B 249.677†	33322.5	28694.4	480.05 µg/L	480.05 ppb	19:33:10
3	Ba 233.527†	113432.0	109275.8	499.61 µg/L	499.61 ppb	19:33:10
3	Be 313.107†	1612377.9	1551470.5	505.17 µg/L	505.17 ppb	19:33:10
3	Cd 226.502†	72852.6	70165.2	484.23 µg/L	484.23 ppb	19:33:10
3	Co 228.616†	36901.2	35668.8	488.67 µg/L	488.67 ppb	19:33:10
3	Cr 267.716†	59397.9	56969.5	489.19 µg/L	489.19 ppb	19:33:10
3	Cu 324.752†	120225.9	113210.3	493.66 µg/L	493.66 ppb	19:33:10
3	Mn 257.610†	374839.5	360446.6	492.32 µg/L	492.32 ppb	19:33:10
3	Mo 202.031†	15729.4	15184.0	479.75 µg/L	479.75 ppb	19:33:30
3	Ni 231.604†	40031.5	38543.8	493.02 µg/L	493.02 ppb	19:33:10
3	P 214.914†	10307.1	9834.0	2346.7 µg/L	2346.7 ppb	19:33:30
3	Pb 220.353†	8288.5	7859.6	477.65 µg/L	477.65 ppb	19:33:30
3	S 181.975 Axial†	1283.8	1140.0	927.63 µg/L	927.63 ppb	19:33:30
3	Sb 206.836†	3807.3	3575.3	483.25 µg/L	483.25 ppb	19:33:30
3	Se 196.026†	1249.7	1191.1	473 µg/L	473 ppb	19:33:30
3	SiO2†	51607.6	48064.2	5232.9 µg/L	5232.9 ppb	19:33:10
3	Si 251.611†	155270.1	148664.8	2448.6 µg/L	2448.6 ppb	19:33:10
3	Sn 189.927†	7010.2	6740.5	480.86 µg/L	480.86 ppb	19:33:30
3	Ti 334.940†	504064.8	484181.1	493.08 µg/L	493.08 ppb	19:33:10
3	Tl 190.801†	3573.6	3557.4	484.91 µg/L	484.91 ppb	19:33:30
3	U 409.014†	7322.0	7521.5	494.86 µg/L	494.86 ppb	19:33:10
3	V 292.402†	92839.2	88862.3	499.06 µg/L	499.06 ppb	19:33:10
3	Zn 213.857†	80753.8	77205.9	482.11 µg/L	482.11 ppb	19:33:10

Mean Data: CCV

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1740074.0	104.02 %	0.203			0.19%
Sc RADIAL	154145.4	106 %	1.1			1.02%
Y 371.029	1056811.9	103.35 %	0.211			0.20%
Ag 328.068†	120724.4	496.07 µg/L	1.385	496.07 ppb	1.385	0.28%
QC value within limits for Ag 328.068 Recovery = 99.21%						
Al 396.153Radial†	23757.1	5163.5 µg/L	6.91	5163.5 ppb	6.91	0.13%
QC value within limits for Al 396.153Radial Recovery = 103.27%						
As 188.979†	1215.2	514.92 µg/L	3.230	514.92 ppb	3.230	0.63%
QC value within limits for As 188.979 Recovery = 102.98%						
B 249.677†	28619.7	478.80 µg/L	1.123	478.80 ppb	1.123	0.23%
QC value within limits for B 249.677 Recovery = 95.76%						
Ba 233.527†	108929.3	498.02 µg/L	1.404	498.02 ppb	1.404	0.28%
QC value within limits for Ba 233.527 Recovery = 99.60%						
Be 313.107†	1548342.3	504.15 µg/L	0.946	504.15 ppb	0.946	0.19%
QC value within limits for Be 313.107 Recovery = 100.83%						
Ca 317.933Radial†	84623.7	4958.6 µg/L	18.54	4958.6 ppb	18.54	0.37%
QC value within limits for Ca 317.933Radial Recovery = 99.17%						
Cd 226.502†	69935.2	482.64 µg/L	1.407	482.64 ppb	1.407	0.29%
QC value within limits for Cd 226.502 Recovery = 96.53%						
Co 228.616†	35576.6	487.41 µg/L	1.097	487.41 ppb	1.097	0.23%

QC value within limits for Co 228.616 Recovery = 97.48%							
Cr 267.716†	56879.6	488.42 µg/L	0.666	488.42 ppb	0.666	0.14%	
QC value within limits for Cr 267.716 Recovery = 97.68%							
Cu 324.752†	113017.4	492.82 µg/L	1.012	492.82 ppb	1.012	0.21%	
QC value within limits for Cu 324.752 Recovery = 98.56%							
Fe 238.204 Radial†	74084.6	4925.4 µg/L	14.08	4925.4 ppb	14.08	0.29%	
QC value within limits for Fe 238.204 Radial Recovery = 98.51%							
K 766.490 Radial†	11741.2	4829.6 µg/L	36.64	4829.6 ppb	36.64	0.76%	
QC value within limits for K 766.490 Radial Recovery = 96.59%							
Mg 279.077 IEC†	12248.0	5057.5 µg/L	37.48	5057.5 ppb	37.48	0.74%	
QC value within limits for Mg 279.077 IEC Recovery = 101.15%							
Mn 257.610†	359527.3	491.06 µg/L	1.093	491.06 ppb	1.093	0.22%	
QC value within limits for Mn 257.610 Recovery = 98.21%							
Mo 202.031†	15245.4	481.69 µg/L	1.954	481.69 ppb	1.954	0.41%	
QC value within limits for Mo 202.031 Recovery = 96.34%							
Na 589.592 Radial†	64489.2	9863.4 µg/L	26.47	9863.4 ppb	26.47	0.27%	
QC value within limits for Na 589.592 Radial Recovery = 98.63%							
Ni 231.604†	38330.9	490.30 µg/L	2.360	490.30 ppb	2.360	0.48%	
QC value within limits for Ni 231.604 Recovery = 98.06%							
P 214.914†	9887.5	2359.5 µg/L	14.32	2359.5 ppb	14.32	0.61%	
QC value within limits for P 214.914 Recovery = 94.38%							
Pb 220.353†	7879.5	478.86 µg/L	1.831	478.86 ppb	1.831	0.38%	
QC value within limits for Pb 220.353 Recovery = 95.77%							
S 181.975 Axial†	1154.1	939.11 µg/L	10.857	939.11 ppb	10.857	1.16%	
QC value within limits for S 181.975 Axial Recovery = 93.91%							
Sb 206.836†	3587.2	484.91 µg/L	1.496	484.91 ppb	1.496	0.31%	
QC value within limits for Sb 206.836 Recovery = 96.98%							
Se 196.026†	1197.9	476 µg/L	2.6	476 ppb	2.6	0.55%	
QC value within limits for Se 196.026 Recovery = 95.20%							
SiO2†	47987.3	5224.4 µg/L	7.40	5224.4 ppb	7.40	0.14%	
QC value within limits for SiO2 Recovery = 97.70%							
Si 251.611†	148040.8	2438.2 µg/L	9.16	2438.2 ppb	9.16	0.38%	
QC value within limits for Si 251.611 Recovery = 97.53%							
Sn 189.927†	6780.7	483.70 µg/L	2.578	483.70 ppb	2.578	0.53%	
QC value within limits for Sn 189.927 Recovery = 96.74%							
Sr 421.552†	215809.3	505.76 µg/L	3.152	505.76 ppb	3.152	0.62%	
QC value within limits for Sr 421.552 Recovery = 101.15%							
Ti 334.940†	482791.6	491.66 µg/L	1.273	491.66 ppb	1.273	0.26%	
QC value within limits for Ti 334.940 Recovery = 98.33%							
Tl 190.801†	3569.7	486.55 µg/L	1.860	486.55 ppb	1.860	0.38%	
QC value within limits for Tl 190.801 Recovery = 97.31%							
U 409.014†	7445.5	490.08 µg/L	6.310	490.08 ppb	6.310	1.29%	
QC value within limits for U 409.014 Recovery = 98.02%							
V 292.402†	88640.9	497.85 µg/L	1.100	497.85 ppb	1.100	0.22%	
QC value within limits for V 292.402 Recovery = 99.57%							
Zn 213.857†	76904.5	480.23 µg/L	1.651	480.23 ppb	1.651	0.34%	
QC value within limits for Zn 213.857 Recovery = 96.05%							
All analyte(s) passed QC.							

Sequence No.: 9

Sample ID: CCB

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 8

Date Collected: 3/29/2010 19:33:37

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCB

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	154440.8	154440.8	106 %		19:34:06
1	Al 396.153Radial†	-43.3	-9.0	-2.0043 µg/L	-2.0043 ppb	19:34:26
1	Ca 317.933Radial†	696.6	41.2	2.4138 µg/L	2.4138 ppb	19:34:26
1	Fe 238.204 Radial†	166.8	44.1	2.9352 µg/L	2.9352 ppb	19:34:26
1	K 766.490 Radial†	1613.3	67.6	27.814 µg/L	27.814 ppb	19:34:06
1	Mg 279.077 IEC†	157.8	-37.7	-15.541 µg/L	-15.541 ppb	19:34:26
1	Na 589.592 Radial†	1722.8	-68.9	-10.561 µg/L	-10.561 ppb	19:34:06
1	Sr 421.552†	-120.8	163.9	0.3842 µg/L	0.3842 ppb	19:34:06
1	Sc 361.383	1731581.1	1731581.1	103.52 %		19:35:14
1	Y 371.029	1065562.9	1065562.9	104.20 %		19:35:14
1	Ag 328.068†	3216.9	140.6	0.5847 µg/L	0.5847 ppb	19:35:16
1	As 188.979†	-11.7	2.9	1.2300 µg/L	1.2300 ppb	19:35:36
1	B 249.677†	3120.0	-341.7	-5.7362 µg/L	-5.7362 ppb	19:35:36
1	Ba 233.527†	-175.6	5.4	0.0247 µg/L	0.0247 ppb	19:35:36
1	Be 313.107†	-246.2	422.2	0.1424 µg/L	0.1424 ppb	19:35:16
1	Cd 226.502†	-69.1	27.7	0.1908 µg/L	0.1908 ppb	19:35:36
1	Co 228.616†	-181.3	1.5	0.0198 µg/L	0.0198 ppb	19:35:36
1	Cr 267.716†	175.8	9.6	0.0693 µg/L	0.0693 ppb	19:35:36
1	Cu 324.752†	2669.4	153.9	0.6825 µg/L	0.6825 ppb	19:35:16
1	Mn 257.610†	196.9	110.2	0.1512 µg/L	0.1512 ppb	19:35:36
1	Mo 202.031†	-29.9	26.3	0.8305 µg/L	0.8305 ppb	19:35:36
1	Ni 231.604†	-61.5	-18.5	-0.2372 µg/L	-0.2372 ppb	19:35:36
1	P 214.914†	55.3	-26.1	-6.2662 µg/L	-6.2662 ppb	19:35:36
1	Pb 220.353†	115.1	-1.2	-0.0837 µg/L	-0.0837 ppb	19:35:36
1	S 181.975 Axial†	87.6	-10.2	-8.2246 µg/L	-8.2246 ppb	19:35:36
1	Sb 206.836†	73.1	-16.1	-2.1571 µg/L	-2.1571 ppb	19:35:36
1	Se 196.026†	13.4	2.0	0.826 µg/L	0.826 ppb	19:35:36
1	SiO2†	1671.5	41.8	4.5433 µg/L	4.5433 ppb	19:35:36
1	Si 251.611†	796.8	93.3	1.5290 µg/L	1.5290 ppb	19:35:36
1	Sn 189.927†	8.8	6.4	0.4582 µg/L	0.4582 ppb	19:35:36
1	Ti 334.940†	627.3	-30.4	-0.0364 µg/L	-0.0364 ppb	19:35:16
1	Tl 190.801†	-118.4	5.9	0.7913 µg/L	0.7913 ppb	19:35:36
1	U 409.014†	-222.3	264.4	16.308 µg/L	16.308 ppb	19:35:16
1	V 292.402†	354.1	-89.7	-0.4781 µg/L	-0.4781 ppb	19:35:16
1	Zn 213.857†	527.0	44.7	0.2818 µg/L	0.2818 ppb	19:35:36
2	Sc RADIAL	154279.9	154279.9	106 %		19:34:28
2	Al 396.153Radial†	-70.9	-35.1	-7.7094 µg/L	-7.7094 ppb	19:34:48
2	Ca 317.933Radial†	709.7	54.3	3.1826 µg/L	3.1826 ppb	19:34:48
2	Fe 238.204 Radial†	178.3	55.2	3.6708 µg/L	3.6708 ppb	19:34:48
2	K 766.490 Radial†	1463.8	-72.1	-29.690 µg/L	-29.690 ppb	19:34:28
2	Mg 279.077 IEC†	161.8	-33.8	-13.912 µg/L	-13.912 ppb	19:34:48
2	Na 589.592 Radial†	1747.5	-43.7	-6.6675 µg/L	-6.6675 ppb	19:34:28
2	Sr 421.552†	-216.0	73.9	0.1732 µg/L	0.1732 ppb	19:34:28
2	Sc 361.383	1751103.4	1751103.4	104.68 %		19:35:38
2	Y 371.029	1076583.0	1076583.0	105.28 %		19:35:38
2	Ag 328.068†	2689.9	-397.5	-1.6314 µg/L	-1.6314 ppb	19:35:40
2	As 188.979†	-19.4	-4.3	-1.7955 µg/L	-1.7955 ppb	19:36:00
2	B 249.677†	3164.1	-333.1	-5.5927 µg/L	-5.5927 ppb	19:36:00
2	Ba 233.527†	-177.8	5.3	0.0236 µg/L	0.0236 ppb	19:36:00
2	Be 313.107†	-520.5	162.9	0.0516 µg/L	0.0516 ppb	19:35:40
2	Cd 226.502†	-104.5	-5.4	-0.0378 µg/L	-0.0378 ppb	19:36:00
2	Co 228.616†	-170.5	13.7	0.1872 µg/L	0.1872 ppb	19:36:00
2	Cr 267.716†	176.6	8.5	0.0762 µg/L	0.0762 ppb	19:36:00
2	Cu 324.752†	2448.1	-86.2	-0.3785 µg/L	-0.3785 ppb	19:35:40
2	Mn 257.610†	240.0	149.3	0.2045 µg/L	0.2045 ppb	19:36:00
2	Mo 202.031†	-29.0	27.5	0.8664 µg/L	0.8664 ppb	19:36:00
2	Ni 231.604†	-48.2	-5.1	-0.0655 µg/L	-0.0655 ppb	19:36:00
2	P 214.914†	58.0	-24.2	-5.7906 µg/L	-5.7906 ppb	19:36:00
2	Pb 220.353†	124.4	6.4	0.3918 µg/L	0.3918 ppb	19:36:00

2	S 181.975 Axial†	90.4	-8.5	-6.8756 µg/L	-6.8756 ppb	19:36:00
2	Sb 206.836†	78.1	-12.0	-1.6140 µg/L	-1.6140 ppb	19:36:00
2	Se 196.026†	15.0	3.5	1.36 µg/L	1.36 ppb	19:36:00
2	SiO2†	1656.1	9.2	0.9709 µg/L	0.9709 ppb	19:36:00
2	Si 251.611†	759.0	48.7	0.7903 µg/L	0.7903 ppb	19:36:00
2	Sn 189.927†	8.2	5.8	0.4148 µg/L	0.4148 ppb	19:36:00
2	Ti 334.940†	745.1	75.4	0.0800 µg/L	0.0800 ppb	19:35:40
2	Tl 190.801†	-111.6	13.7	1.8304 µg/L	1.8304 ppb	19:36:00
2	U 409.014†	-582.4	-77.2	-4.8304 µg/L	-4.8304 ppb	19:35:40
2	V 292.402†	254.3	-188.9	-1.0423 µg/L	-1.0423 ppb	19:35:40
2	Zn 213.857†	524.9	37.0	0.2333 µg/L	0.2333 ppb	19:36:00
3	Sc RADIAL	154300.7	154300.7	106 %		19:34:50
3	Al 396.153Radial†	-22.9	10.3	2.2225 µg/L	2.2225 ppb	19:35:10
3	Ca 317.933Radial†	702.8	47.7	2.7963 µg/L	2.7963 ppb	19:35:10
3	Fe 238.204 Radial†	157.6	35.6	2.3638 µg/L	2.3638 ppb	19:35:10
3	K 766.490 Radial†	1363.4	-167.1	-68.805 µg/L	-68.805 ppb	19:34:50
3	Mg 279.077 IEC†	165.1	-30.7	-12.669 µg/L	-12.669 ppb	19:35:10
3	Na 589.592 Radial†	1617.5	-166.8	-25.467 µg/L	-25.467 ppb	19:34:50
3	Sr 421.552†	-166.5	120.7	0.2829 µg/L	0.2829 ppb	19:34:50
3	Sc 361.383	1756722.7	1756722.7	105.02 %		19:36:02
3	Y 371.029	1079825.4	1079825.4	105.60 %		19:36:02
3	Ag 328.068†	3226.0	104.8	0.4137 µg/L	0.4137 ppb	19:36:04
3	As 188.979†	-24.9	-9.5	-3.9669 µg/L	-3.9669 ppb	19:36:25
3	B 249.677†	3162.1	-344.7	-5.7874 µg/L	-5.7874 ppb	19:36:25
3	Ba 233.527†	-158.1	24.5	0.1116 µg/L	0.1116 ppb	19:36:25
3	Be 313.107†	-509.5	174.9	0.0572 µg/L	0.0572 ppb	19:36:04
3	Cd 226.502†	-104.2	-4.8	-0.0337 µg/L	-0.0337 ppb	19:36:25
3	Co 228.616†	-161.9	22.4	0.3068 µg/L	0.3068 ppb	19:36:25
3	Cr 267.716†	163.5	-4.5	-0.0399 µg/L	-0.0399 ppb	19:36:25
3	Cu 324.752†	2579.5	31.3	0.1372 µg/L	0.1372 ppb	19:36:04
3	Mn 257.610†	210.9	120.8	0.1656 µg/L	0.1656 ppb	19:36:25
3	Mo 202.031†	-42.5	14.8	0.4652 µg/L	0.4652 ppb	19:36:25
3	Ni 231.604†	-54.2	-10.7	-0.1372 µg/L	-0.1372 ppb	19:36:25
3	P 214.914†	63.9	-18.7	-4.4865 µg/L	-4.4865 ppb	19:36:25
3	Pb 220.353†	88.7	-28.0	-1.6935 µg/L	-1.6935 ppb	19:36:25
3	S 181.975 Axial†	84.6	-14.3	-11.562 µg/L	-11.562 ppb	19:36:25
3	Sb 206.836†	89.1	-1.8	-0.2346 µg/L	-0.2346 ppb	19:36:25
3	Se 196.026†	11.7	0.2	0.100 µg/L	0.100 ppb	19:36:25
3	SiO2†	1684.0	30.6	3.3325 µg/L	3.3325 ppb	19:36:25
3	Si 251.611†	773.1	59.7	0.9802 µg/L	0.9802 ppb	19:36:25
3	Sn 189.927†	5.3	3.0	0.2161 µg/L	0.2161 ppb	19:36:25
3	Ti 334.940†	867.2	189.4	0.1939 µg/L	0.1939 ppb	19:36:04
3	Tl 190.801†	-113.0	12.7	1.7012 µg/L	1.7012 ppb	19:36:25
3	U 409.014†	-487.5	14.9	0.8641 µg/L	0.8641 ppb	19:36:04
3	V 292.402†	257.1	-187.1	-1.0329 µg/L	-1.0329 ppb	19:36:04
3	Zn 213.857†	501.2	12.8	0.0813 µg/L	0.0813 ppb	19:36:25

Mean Data: CCB

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1746469.1	104.41 %	0.789			0.76%
Sc RADIAL	154340.5	106 %	0.1			0.06%
Y 371.029	1073990.4	105.03 %	0.731			0.70%
Ag 328.068†	-50.7	-0.2110 µg/L	1.23303	-0.2110 ppb	1.23303	584.39%
QC value within limits for Ag 328.068 Recovery = Not calculated						
Al 396.153Radial†	-11.3	-2.4971 µg/L	4.98426	-2.4971 ppb	4.98426	199.60%
QC value within limits for Al 396.153Radial Recovery = Not calculated						
As 188.979†	-3.6	-1.5108 µg/L	2.61013	-1.5108 ppb	2.61013	172.77%
QC value within limits for As 188.979 Recovery = Not calculated						
B 249.677†	-339.8	-5.7054 µg/L	0.10093	-5.7054 ppb	0.10093	1.77%
QC value within limits for B 249.677 Recovery = Not calculated						
Ba 233.527†	11.7	0.0533 µg/L	0.05049	0.0533 ppb	0.05049	94.76%
QC value within limits for Ba 233.527 Recovery = Not calculated						
Be 313.107†	253.3	0.0837 µg/L	0.05087	0.0837 ppb	0.05087	60.76%
QC value within limits for Be 313.107 Recovery = Not calculated						
Ca 317.933Radial†	47.7	2.7975 µg/L	0.38440	2.7975 ppb	0.38440	13.74%
QC value within limits for Ca 317.933Radial Recovery = Not calculated						
Cd 226.502†	5.8	0.0397 µg/L	0.13082	0.0397 ppb	0.13082	329.26%
QC value within limits for Cd 226.502 Recovery = Not calculated						
Co 228.616†	12.5	0.1713 µg/L	0.14419	0.1713 ppb	0.14419	84.18%

QC value within limits for Co 228.616 Recovery = Not calculated						
Cr 267.716†	4.5	0.0352 µg/L	0.06512	0.0352 ppb	0.06512	185.02%
QC value within limits for Cr 267.716 Recovery = Not calculated						
Cu 324.752†	33.0	0.1470 µg/L	0.53058	0.1470 ppb	0.53058	360.82%
QC value within limits for Cu 324.752 Recovery = Not calculated						
Fe 238.204 Radial†	45.0	2.9899 µg/L	0.65521	2.9899 ppb	0.65521	21.91%
QC value within limits for Fe 238.204 Radial Recovery = Not calculated						
K 766.490 Radial†	-57.2	-23.560 µg/L	48.6004	-23.560 ppb	48.6004	206.28%
QC value within limits for K 766.490 Radial Recovery = Not calculated						
Mg 279.077 IEC†	-34.1	-14.041 µg/L	1.4406	-14.041 ppb	1.4406	10.26%
QC value within limits for Mg 279.077 IEC Recovery = Not calculated						
Mn 257.610†	126.8	0.1738 µg/L	0.02760	0.1738 ppb	0.02760	15.88%
QC value within limits for Mn 257.610 Recovery = Not calculated						
Mo 202.031†	22.8	0.7207 µg/L	0.22201	0.7207 ppb	0.22201	30.81%
QC value within limits for Mo 202.031 Recovery = Not calculated						
Na 589.592 Radial†	-93.1	-14.232 µg/L	9.9226	-14.232 ppb	9.9226	69.72%
QC value within limits for Na 589.592 Radial Recovery = Not calculated						
Ni 231.604†	-11.5	-0.1466 µg/L	0.08623	-0.1466 ppb	0.08623	58.80%
QC value within limits for Ni 231.604 Recovery = Not calculated						
P 214.914†	-23.0	-5.5144 µg/L	0.92145	-5.5144 ppb	0.92145	16.71%
QC value within limits for P 214.914 Recovery = Not calculated						
Pb 220.353†	-7.6	-0.4618 µg/L	1.09284	-0.4618 ppb	1.09284	236.66%
QC value within limits for Pb 220.353 Recovery = Not calculated						
S 181.975 Axial†	-11.0	-8.8875 µg/L	2.41268	-8.8875 ppb	2.41268	27.15%
QC value within limits for S 181.975 Axial Recovery = Not calculated						
Sb 206.836†	-10.0	-1.3353 µg/L	0.99108	-1.3353 ppb	0.99108	74.22%
QC value within limits for Sb 206.836 Recovery = Not calculated						
Se 196.026†	1.9	0.763 µg/L	0.6334	0.763 ppb	0.6334	83.06%
QC value within limits for Se 196.026 Recovery = Not calculated						
SiO2†	27.2	2.9489 µg/L	1.81680	2.9489 ppb	1.81680	61.61%
QC value within limits for SiO2 Recovery = Not calculated						
Si 251.611†	67.2	1.0998 µg/L	0.38363	1.0998 ppb	0.38363	34.88%
QC value within limits for Si 251.611 Recovery = Not calculated						
Sn 189.927†	5.1	0.3630 µg/L	0.12911	0.3630 ppb	0.12911	35.56%
QC value within limits for Sn 189.927 Recovery = Not calculated						
Sr 421.552†	119.5	0.2801 µg/L	0.10556	0.2801 ppb	0.10556	37.69%
QC value within limits for Sr 421.552 Recovery = Not calculated						
Ti 334.940†	78.1	0.0792 µg/L	0.11512	0.0792 ppb	0.11512	145.40%
QC value within limits for Ti 334.940 Recovery = Not calculated						
Tl 190.801†	10.8	1.4410 µg/L	0.56631	1.4410 ppb	0.56631	39.30%
QC value within limits for Tl 190.801 Recovery = Not calculated						
U 409.014†	67.4	4.1140 µg/L	10.93772	4.1140 ppb	10.93772	265.87%
QC value within limits for U 409.014 Recovery = Not calculated						
V 292.402†	-155.2	-0.8511 µg/L	0.32304	-0.8511 ppb	0.32304	37.96%
QC value within limits for V 292.402 Recovery = Not calculated						
Zn 213.857†	31.5	0.1988 µg/L	0.10458	0.1988 ppb	0.10458	52.60%
QC value within limits for Zn 213.857 Recovery = Not calculated						
All analyte(s) passed QC.						

Sequence No.: 18
 Sample ID: CCV
 Analyst:
 Initial Sample Wt:
 Dilution:

Autosampler Location: 7
 Date Collected: 3/29/2010 19:52:48
 Data Type: Original
 Initial Sample Vol:
 Sample Prep Vol:

Replicate Data: CCV

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	155882.7	155882.7	107 %		19:53:21
1	Al 396.153Radial†	25404.5	23785.7	5169.7 µg/L	5169.7 ppb	19:53:21
1	Ca 317.933Radial†	90923.1	84399.2	4945.4 µg/L	4945.4 ppb	19:53:21
1	Fe 238.204 Radial†	79031.3	73782.9	4905.3 µg/L	4905.3 ppb	19:53:21
1	K 766.490 Radial†	14120.7	11748.2	4832.4 µg/L	4832.4 ppb	19:53:21
1	Mg 279.077 IEC†	13276.7	12227.4	5049.1 µg/L	5049.1 ppb	19:53:21
1	Na 589.592 Radial†	70685.1	64397.5	9849.3 µg/L	9849.3 ppb	19:53:21
1	Sr 421.552†	229627.1	214985.0	503.83 µg/L	503.83 ppb	19:53:19
1	Sc 361.383	1753609.4	1753609.4	104.83 %		19:53:33
1	Y 371.029	1065335.0	1065335.0	104.18 %		19:53:33
1	Ag 328.068†	129859.6	120906.6	496.82 µg/L	496.82 ppb	19:53:33
1	As 188.979†	1259.2	1215.4	515.01 µg/L	515.01 ppb	19:53:54
1	B 249.677†	33439.0	28541.9	477.50 µg/L	477.50 ppb	19:53:33
1	Ba 233.527†	114213.7	109124.0	498.92 µg/L	498.92 ppb	19:53:33
1	Be 313.107†	1623855.4	1549661.7	504.58 µg/L	504.58 ppb	19:53:33
1	Cd 226.502†	73102.1	69826.8	481.89 µg/L	481.89 ppb	19:53:33
1	Co 228.616†	36982.2	35454.0	485.73 µg/L	485.73 ppb	19:53:33
1	Cr 267.716†	59867.3	56947.4	489.01 µg/L	489.01 ppb	19:53:33
1	Cu 324.752†	121039.4	113035.1	492.88 µg/L	492.88 ppb	19:53:33
1	Mn 257.610†	376767.1	359319.5	490.78 µg/L	490.78 ppb	19:53:33
1	Mo 202.031†	15963.8	15283.1	482.88 µg/L	482.88 ppb	19:53:54
1	Ni 231.604†	39977.6	38175.7	488.31 µg/L	488.31 ppb	19:53:33
1	P 214.914†	10457.3	9895.7	2361.5 µg/L	2361.5 ppb	19:53:54
1	Pb 220.353†	8391.8	7892.5	479.66 µg/L	479.66 ppb	19:53:54
1	S 181.975 Axial†	1293.9	1139.4	927.23 µg/L	927.23 ppb	19:53:54
1	Sb 206.836†	3874.2	3609.0	487.86 µg/L	487.86 ppb	19:53:54
1	Se 196.026†	1272.9	1203.3	478 µg/L	478 ppb	19:53:54
1	SiO2†	51967.3	47999.0	5225.6 µg/L	5225.6 ppb	19:53:33
1	Si 251.611†	156115.9	148243.1	2441.5 µg/L	2441.5 ppb	19:53:33
1	Sn 189.927†	7141.4	6810.1	485.80 µg/L	485.80 ppb	19:53:54
1	Ti 334.940†	507174.4	483159.2	492.04 µg/L	492.04 ppb	19:53:33
1	Tl 190.801†	3640.2	3592.7	489.65 µg/L	489.65 ppb	19:53:54
1	U 409.014†	7175.3	7323.6	482.62 µg/L	482.62 ppb	19:53:33
1	V 292.402†	93601.0	88854.5	499.04 µg/L	499.04 ppb	19:53:33
1	Zn 213.857†	81005.3	76806.8	479.63 µg/L	479.63 ppb	19:53:33
2	Sc RADIAL	156189.6	156189.6	107 %		19:53:25
2	Al 396.153Radial†	25453.6	23784.9	5169.5 µg/L	5169.5 ppb	19:53:25
2	Ca 317.933Radial†	91189.7	84480.9	4950.2 µg/L	4950.2 ppb	19:53:25
2	Fe 238.204 Radial†	79453.6	74031.8	4921.9 µg/L	4921.9 ppb	19:53:25
2	K 766.490 Radial†	14048.5	11654.9	4794.0 µg/L	4794.0 ppb	19:53:25
2	Mg 279.077 IEC†	13352.4	12273.6	5068.1 µg/L	5068.1 ppb	19:53:25
2	Na 589.592 Radial†	70950.0	64514.9	9867.3 µg/L	9867.3 ppb	19:53:25
2	Sr 421.552†	232352.0	217106.1	508.80 µg/L	508.80 ppb	19:53:23
2	Sc 361.383	1749571.1	1749571.1	104.59 %		19:53:57
2	Y 371.029	1062777.0	1062777.0	103.93 %		19:53:57
2	Ag 328.068†	129030.1	120399.3	494.76 µg/L	494.76 ppb	19:53:57
2	As 188.979†	1277.4	1235.6	523.42 µg/L	523.42 ppb	19:54:17
2	B 249.677†	33289.1	28472.2	476.33 µg/L	476.33 ppb	19:53:57
2	Ba 233.527†	113708.3	108892.2	497.86 µg/L	497.86 ppb	19:53:57
2	Be 313.107†	1621134.0	1550635.2	504.90 µg/L	504.90 ppb	19:53:57
2	Cd 226.502†	72772.0	69672.1	480.82 µg/L	480.82 ppb	19:53:57
2	Co 228.616†	36900.7	35457.5	485.78 µg/L	485.78 ppb	19:53:57
2	Cr 267.716†	59600.3	56824.0	487.94 µg/L	487.94 ppb	19:53:57
2	Cu 324.752†	120397.9	112688.2	491.39 µg/L	491.39 ppb	19:53:57
2	Mn 257.610†	375323.1	358768.5	490.02 µg/L	490.02 ppb	19:53:57
2	Mo 202.031†	15936.5	15292.2	483.17 µg/L	483.17 ppb	19:54:17
2	Ni 231.604†	39772.4	38067.5	486.93 µg/L	486.93 ppb	19:53:57
2	P 214.914†	10473.9	9934.6	2370.8 µg/L	2370.8 ppb	19:54:17
2	Pb 220.353†	8398.2	7917.1	481.14 µg/L	481.14 ppb	19:54:17

2	S 181.975 Axial†	1310.8	1158.5	942.63 µg/L	942.63 ppb	19:54:17
2	Sb 206.836†	3846.2	3590.8	485.41 µg/L	485.41 ppb	19:54:17
2	Se 196.026†	1265.1	1198.6	476 µg/L	476 ppb	19:54:17
2	SiO2†	51895.6	48044.8	5230.6 µg/L	5230.6 ppb	19:53:57
2	Si 251.611†	155321.7	147827.6	2434.7 µg/L	2434.7 ppb	19:53:57
2	Sn 189.927†	7131.0	6815.9	486.21 µg/L	486.21 ppb	19:54:17
2	Ti 334.940†	504709.9	481919.6	490.77 µg/L	490.77 ppb	19:53:57
2	Tl 190.801†	3621.3	3582.7	488.28 µg/L	488.28 ppb	19:54:17
2	U 409.014†	7284.6	7443.9	490.00 µg/L	490.00 ppb	19:53:57
2	V 292.402†	93209.2	88686.0	498.11 µg/L	498.11 ppb	19:53:57
2	Zn 213.857†	80533.7	76534.3	477.93 µg/L	477.93 ppb	19:53:57
3	Sc RADIAL	155078.4	155078.4	106 %		19:53:29
3	Al 396.153Radial†	25069.2	23593.8	5127.8 µg/L	5127.8 ppb	19:53:29
3	Ca 317.933Radial†	90380.5	84330.2	4941.4 µg/L	4941.4 ppb	19:53:29
3	Fe 238.204 Radial†	78812.3	73960.4	4917.1 µg/L	4917.1 ppb	19:53:29
3	K 766.490 Radial†	14162.7	11856.1	4876.9 µg/L	4876.9 ppb	19:53:29
3	Mg 279.077 IEC†	13255.0	12271.4	5067.2 µg/L	5067.2 ppb	19:53:29
3	Na 589.592 Radial†	70378.5	64452.3	9857.7 µg/L	9857.7 ppb	19:53:29
3	Sr 421.552†	229789.0	216250.9	506.80 µg/L	506.80 ppb	19:53:27
3	Sc 361.383	1754221.5	1754221.5	104.87 %		19:54:20
3	Y 371.029	1065517.6	1065517.6	104.20 %		19:54:20
3	Ag 328.068†	129249.8	120281.8	494.30 µg/L	494.30 ppb	19:54:20
3	As 188.979†	1278.2	1233.1	522.37 µg/L	522.37 ppb	19:54:40
3	B 249.677†	33485.8	28575.4	478.06 µg/L	478.06 ppb	19:54:20
3	Ba 233.527†	113649.5	108547.9	496.28 µg/L	496.28 ppb	19:54:20
3	Be 313.107†	1620552.1	1545971.4	503.38 µg/L	503.38 ppb	19:54:20
3	Cd 226.502†	72839.4	69552.0	479.99 µg/L	479.99 ppb	19:54:20
3	Co 228.616†	36967.6	35427.9	485.37 µg/L	485.37 ppb	19:54:20
3	Cr 267.716†	59675.2	56744.3	487.25 µg/L	487.25 ppb	19:54:20
3	Cu 324.752†	120775.4	112743.0	491.64 µg/L	491.64 ppb	19:54:20
3	Mn 257.610†	375706.0	358182.3	489.22 µg/L	489.22 ppb	19:54:20
3	Mo 202.031†	15964.1	15278.1	482.72 µg/L	482.72 ppb	19:54:40
3	Ni 231.604†	39857.9	38048.2	486.68 µg/L	486.68 ppb	19:54:20
3	P 214.914†	10507.5	9940.1	2372.1 µg/L	2372.1 ppb	19:54:40
3	Pb 220.353†	8449.2	7944.5	482.78 µg/L	482.78 ppb	19:54:40
3	S 181.975 Axial†	1329.7	1173.2	954.54 µg/L	954.54 ppb	19:54:40
3	Sb 206.836†	3845.9	3580.7	484.06 µg/L	484.06 ppb	19:54:40
3	Se 196.026†	1261.3	1191.8	474 µg/L	474 ppb	19:54:40
3	SiO2†	51759.5	47783.5	5202.0 µg/L	5202.0 ppb	19:54:20
3	Si 251.611†	155480.2	147585.0	2430.6 µg/L	2430.6 ppb	19:54:20
3	Sn 189.927†	7188.1	6852.4	488.80 µg/L	488.80 ppb	19:54:40
3	Ti 334.940†	505136.1	481046.7	489.87 µg/L	489.87 ppb	19:54:20
3	Tl 190.801†	3646.0	3597.0	490.19 µg/L	490.19 ppb	19:54:40
3	U 409.014†	7585.0	7711.9	506.54 µg/L	506.54 ppb	19:54:20
3	V 292.402†	93415.0	88646.0	497.89 µg/L	497.89 ppb	19:54:20
3	Zn 213.857†	80914.4	76693.2	478.93 µg/L	478.93 ppb	19:54:20

Mean Data: CCV

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1752467.3	104.76 %	0.151			0.14%
Sc RADIAL	155716.9	107 %	0.4			0.37%
Y 371.029	1064543.2	104.10 %	0.150			0.14%
Ag 328.068†	120529.2	495.29 µg/L	1.342	495.29 ppb	1.342	0.27%
QC value within limits for Ag 328.068 Recovery = 99.06%						
Al 396.153Radial†	23721.5	5155.7 µg/L	24.12	5155.7 ppb	24.12	0.47%
QC value within limits for Al 396.153Radial Recovery = 103.11%						
As 188.979†	1228.0	520.27 µg/L	4.583	520.27 ppb	4.583	0.88%
QC value within limits for As 188.979 Recovery = 104.05%						
B 249.677†	28529.8	477.29 µg/L	0.884	477.29 ppb	0.884	0.19%
QC value within limits for B 249.677 Recovery = 95.46%						
Ba 233.527†	108854.7	497.68 µg/L	1.325	497.68 ppb	1.325	0.27%
QC value within limits for Ba 233.527 Recovery = 99.54%						
Be 313.107†	1548756.1	504.29 µg/L	0.798	504.29 ppb	0.798	0.16%
QC value within limits for Be 313.107 Recovery = 100.86%						
Ca 317.933Radial†	84403.4	4945.7 µg/L	4.42	4945.7 ppb	4.42	0.09%
QC value within limits for Ca 317.933Radial Recovery = 98.91%						
Cd 226.502†	69683.6	480.90 µg/L	0.952	480.90 ppb	0.952	0.20%
QC value within limits for Cd 226.502 Recovery = 96.18%						
Co 228.616†	35446.5	485.63 µg/L	0.223	485.63 ppb	0.223	0.05%

QC value within limits for Co 228.616 Recovery = 97.13%							
Cr 267.716†	56838.6	488.07 µg/L	0.888	488.07 ppb	0.888	0.18%	
QC value within limits for Cr 267.716 Recovery = 97.61%							
Cu 324.752†	112822.1	491.97 µg/L	0.803	491.97 ppb	0.803	0.16%	
QC value within limits for Cu 324.752 Recovery = 98.39%							
Fe 238.204 Radial†	73925.1	4914.8 µg/L	8.52	4914.8 ppb	8.52	0.17%	
QC value within limits for Fe 238.204 Radial Recovery = 98.30%							
K 766.490 Radial†	11753.1	4834.4 µg/L	41.46	4834.4 ppb	41.46	0.86%	
QC value within limits for K 766.490 Radial Recovery = 96.69%							
Mg 279.077 IEC†	12257.5	5061.5 µg/L	10.75	5061.5 ppb	10.75	0.21%	
QC value within limits for Mg 279.077 IEC Recovery = 101.23%							
Mn 257.610†	358756.8	490.01 µg/L	0.777	490.01 ppb	0.777	0.16%	
QC value within limits for Mn 257.610 Recovery = 98.00%							
Mo 202.031†	15284.5	482.92 µg/L	0.226	482.92 ppb	0.226	0.05%	
QC value within limits for Mo 202.031 Recovery = 96.58%							
Na 589.592 Radial†	64454.9	9858.1 µg/L	9.01	9858.1 ppb	9.01	0.09%	
QC value within limits for Na 589.592 Radial Recovery = 98.58%							
Ni 231.604†	38097.1	487.31 µg/L	0.879	487.31 ppb	0.879	0.18%	
QC value within limits for Ni 231.604 Recovery = 97.46%							
P 214.914†	9923.5	2368.1 µg/L	5.81	2368.1 ppb	5.81	0.25%	
QC value within limits for P 214.914 Recovery = 94.72%							
Pb 220.353†	7918.0	481.20 µg/L	1.563	481.20 ppb	1.563	0.32%	
QC value within limits for Pb 220.353 Recovery = 96.24%							
S 181.975 Axial†	1157.0	941.47 µg/L	13.693	941.47 ppb	13.693	1.45%	
QC value within limits for S 181.975 Axial Recovery = 94.15%							
Sb 206.836†	3593.5	485.78 µg/L	1.923	485.78 ppb	1.923	0.40%	
QC value within limits for Sb 206.836 Recovery = 97.16%							
Se 196.026†	1197.9	476 µg/L	2.3	476 ppb	2.3	0.48%	
QC value within limits for Se 196.026 Recovery = 95.20%							
SiO2†	47942.4	5219.4 µg/L	15.27	5219.4 ppb	15.27	0.29%	
QC value within limits for SiO2 Recovery = 97.60%							
Si 251.611†	147885.2	2435.6 µg/L	5.51	2435.6 ppb	5.51	0.23%	
QC value within limits for Si 251.611 Recovery = 97.42%							
Sn 189.927†	6826.1	486.94 µg/L	1.623	486.94 ppb	1.623	0.33%	
QC value within limits for Sn 189.927 Recovery = 97.39%							
Sr 421.552†	216114.0	506.48 µg/L	2.501	506.48 ppb	2.501	0.49%	
QC value within limits for Sr 421.552 Recovery = 101.30%							
Ti 334.940†	482041.8	490.89 µg/L	1.088	490.89 ppb	1.088	0.22%	
QC value within limits for Ti 334.940 Recovery = 98.18%							
Tl 190.801†	3590.8	489.38 µg/L	0.983	489.38 ppb	0.983	0.20%	
QC value within limits for Tl 190.801 Recovery = 97.88%							
U 409.014†	7493.2	493.05 µg/L	12.247	493.05 ppb	12.247	2.48%	
QC value within limits for U 409.014 Recovery = 98.61%							
V 292.402†	88728.8	498.35 µg/L	0.611	498.35 ppb	0.611	0.12%	
QC value within limits for V 292.402 Recovery = 99.67%							
Zn 213.857†	76678.1	478.83 µg/L	0.858	478.83 ppb	0.858	0.18%	
QC value within limits for Zn 213.857 Recovery = 95.77%							
All analyte(s) passed QC.							

Sequence No.: 19

Sample ID: CCB

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 8

Date Collected: 3/29/2010 19:54:47

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCB

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	157224.0	157224.0	108 %		19:55:16
1	Al 396.153Radial†	-32.4	1.9	0.3819 µg/L	0.3819 ppb	19:55:36
1	Ca 317.933Radial†	709.9	41.9	2.4560 µg/L	2.4560 ppb	19:55:36
1	Fe 238.204 Radial†	168.7	43.1	2.8662 µg/L	2.8662 ppb	19:55:36
1	K 766.490 Radial†	1483.0	-80.2	-33.015 µg/L	-33.015 ppb	19:55:16
1	Mg 279.077 IEC†	179.6	-20.2	-8.3135 µg/L	-8.3135 ppb	19:55:36
1	Na 589.592 Radial†	1705.0	-114.1	-17.428 µg/L	-17.428 ppb	19:55:16
1	Sr 421.552†	-122.3	164.6	0.3859 µg/L	0.3859 ppb	19:55:16
1	Sc 361.383	1744373.3	1744373.3	104.28 %		19:56:24
1	Y 371.029	1071958.2	1071958.2	104.83 %		19:56:24
1	Ag 328.068†	3041.9	-50.0	-0.2039 µg/L	-0.2039 ppb	19:56:26
1	As 188.979†	-16.7	-1.8	-0.7391 µg/L	-0.7391 ppb	19:56:46
1	B 249.677†	3115.7	-367.9	-6.1751 µg/L	-6.1751 ppb	19:56:46
1	Ba 233.527†	-172.9	9.3	0.0420 µg/L	0.0420 ppb	19:56:46
1	Be 313.107†	-510.3	170.7	0.0584 µg/L	0.0584 ppb	19:56:26
1	Cd 226.502†	-91.2	6.9	0.0476 µg/L	0.0476 ppb	19:56:46
1	Co 228.616†	-200.7	-15.9	-0.2172 µg/L	-0.2172 ppb	19:56:46
1	Cr 267.716†	193.2	25.0	0.2074 µg/L	0.2074 ppb	19:56:46
1	Cu 324.752†	2573.6	43.1	0.1952 µg/L	0.1952 ppb	19:56:26
1	Mn 257.610†	146.1	60.1	0.0824 µg/L	0.0824 ppb	19:56:46
1	Mo 202.031†	-38.9	17.9	0.5656 µg/L	0.5656 ppb	19:56:46
1	Ni 231.604†	-15.8	25.7	0.3290 µg/L	0.3290 ppb	19:56:46
1	P 214.914†	40.8	-40.5	-9.7010 µg/L	-9.7010 ppb	19:56:46
1	Pb 220.353†	105.0	-11.7	-0.7153 µg/L	-0.7153 ppb	19:56:46
1	S 181.975 Axial†	80.4	-17.8	-14.383 µg/L	-14.383 ppb	19:56:46
1	Sb 206.836†	78.7	-11.2	-1.5082 µg/L	-1.5082 ppb	19:56:46
1	Se 196.026†	26.3	14.3	5.65 µg/L	5.65 ppb	19:56:46
1	SiO2†	1648.2	7.7	0.8224 µg/L	0.8224 ppb	19:56:46
1	Si 251.611†	791.8	83.0	1.3617 µg/L	1.3617 ppb	19:56:46
1	Sn 189.927†	7.8	5.5	0.3882 µg/L	0.3882 ppb	19:56:46
1	Ti 334.940†	798.2	129.1	0.1285 µg/L	0.1285 ppb	19:56:26
1	Tl 190.801†	-105.6	19.0	2.5510 µg/L	2.5510 ppb	19:56:46
1	U 409.014†	-340.6	152.4	9.3589 µg/L	9.3589 ppb	19:56:26
1	V 292.402†	251.4	-190.7	-1.0454 µg/L	-1.0454 ppb	19:56:26
1	Zn 213.857†	524.6	38.6	0.2408 µg/L	0.2408 ppb	19:56:46
2	Sc RADIAL	153604.9	153604.9	105 %		19:55:38
2	Al 396.153Radial†	-40.7	-6.7	-1.5003 µg/L	-1.5003 ppb	19:55:58
2	Ca 317.933Radial†	698.2	46.3	2.7145 µg/L	2.7145 ppb	19:55:58
2	Fe 238.204 Radial†	160.1	38.6	2.5686 µg/L	2.5686 ppb	19:55:58
2	K 766.490 Radial†	1640.2	101.4	41.741 µg/L	41.741 ppb	19:55:38
2	Mg 279.077 IEC†	170.0	-25.4	-10.448 µg/L	-10.448 ppb	19:55:58
2	Na 589.592 Radial†	1652.3	-126.9	-19.447 µg/L	-19.447 ppb	19:55:38
2	Sr 421.552†	-170.5	116.2	0.2723 µg/L	0.2723 ppb	19:55:38
2	Sc 361.383	1769862.2	1769862.2	105.80 %		19:56:48
2	Y 371.029	1086957.3	1086957.3	106.30 %		19:56:48
2	Ag 328.068†	3055.4	-79.2	-0.3279 µg/L	-0.3279 ppb	19:56:50
2	As 188.979†	-3.9	10.5	4.3943 µg/L	4.3943 ppb	19:57:10
2	B 249.677†	3116.6	-410.1	-6.8860 µg/L	-6.8860 ppb	19:57:10
2	Ba 233.527†	-159.5	24.3	0.1105 µg/L	0.1105 ppb	19:57:10
2	Be 313.107†	-578.9	112.9	0.0378 µg/L	0.0378 ppb	19:56:50
2	Cd 226.502†	-100.7	-0.8	-0.0060 µg/L	-0.0060 ppb	19:57:10
2	Co 228.616†	-154.1	30.9	0.4233 µg/L	0.4233 ppb	19:57:10
2	Cr 267.716†	158.7	-10.2	-0.0909 µg/L	-0.0909 ppb	19:57:10
2	Cu 324.752†	2676.8	105.1	0.4602 µg/L	0.4602 ppb	19:56:50
2	Mn 257.610†	145.1	57.2	0.0785 µg/L	0.0785 ppb	19:57:10
2	Mo 202.031†	-36.1	21.0	0.6639 µg/L	0.6639 ppb	19:57:10
2	Ni 231.604†	-68.7	-24.1	-0.3078 µg/L	-0.3078 ppb	19:57:10
2	P 214.914†	59.6	-23.2	-5.5807 µg/L	-5.5807 ppb	19:57:10
2	Pb 220.353†	97.2	-20.5	-1.2440 µg/L	-1.2440 ppb	19:57:10

2	S 181.975 Axial†	84.9	-14.6	-11.787 µg/L	-11.787 ppb	19:57:10
2	Sb 206.836†	96.3	4.4	0.6052 µg/L	0.6052 ppb	19:57:10
2	Se 196.026†	0.8	-10.2	-4.02 µg/L	-4.02 ppb	19:57:10
2	SiO2†	1672.2	7.6	0.8120 µg/L	0.8120 ppb	19:57:10
2	Si 251.611†	794.7	74.7	1.2254 µg/L	1.2254 ppb	19:57:10
2	Sn 189.927†	4.2	1.9	0.1385 µg/L	0.1385 ppb	19:57:10
2	Ti 334.940†	903.8	217.9	0.2217 µg/L	0.2217 ppb	19:56:50
2	Tl 190.801†	-111.2	15.2	2.0307 µg/L	2.0307 ppb	19:57:10
2	U 409.014†	-447.5	56.1	3.4153 µg/L	3.4153 ppb	19:56:50
2	V 292.402†	287.1	-160.5	-0.8820 µg/L	-0.8820 ppb	19:56:50
2	Zn 213.857†	515.3	22.6	0.1440 µg/L	0.1440 ppb	19:57:10
3	Sc RADIAL	153703.8	153703.8	105 %		19:56:00
3	Al 396.153Radial†	-49.3	-14.8	-3.2844 µg/L	-3.2844 ppb	19:56:20
3	Ca 317.933Radial†	710.1	57.2	3.3512 µg/L	3.3512 ppb	19:56:20
3	Fe 238.204 Radial†	142.7	22.1	1.4665 µg/L	1.4665 ppb	19:56:20
3	K 766.490 Radial†	1683.5	141.5	58.243 µg/L	58.243 ppb	19:56:00
3	Mg 279.077 IEC†	155.1	-39.6	-16.319 µg/L	-16.319 ppb	19:56:20
3	Na 589.592 Radial†	1574.2	-202.0	-30.955 µg/L	-30.955 ppb	19:56:00
3	Sr 421.552†	-284.4	8.3	0.0193 µg/L	0.0193 ppb	19:56:00
3	Sc 361.383	1752547.4	1752547.4	104.77 %		19:57:12
3	Y 371.029	1077428.7	1077428.7	105.36 %		19:57:12
3	Ag 328.068†	3055.4	-50.7	-0.2129 µg/L	-0.2129 ppb	19:57:14
3	As 188.979†	-12.7	2.2	0.9041 µg/L	0.9041 ppb	19:57:35
3	B 249.677†	3085.6	-410.5	-6.8921 µg/L	-6.8921 ppb	19:57:35
3	Ba 233.527†	-169.6	13.1	0.0597 µg/L	0.0597 ppb	19:57:35
3	Be 313.107†	-482.0	200.1	0.0664 µg/L	0.0664 ppb	19:57:14
3	Cd 226.502†	-116.9	-17.2	-0.1188 µg/L	-0.1188 ppb	19:57:35
3	Co 228.616†	-195.4	-9.9	-0.1357 µg/L	-0.1357 ppb	19:57:35
3	Cr 267.716†	143.5	-23.2	-0.2031 µg/L	-0.2031 ppb	19:57:35
3	Cu 324.752†	2562.2	20.7	0.0929 µg/L	0.0929 ppb	19:57:14
3	Mn 257.610†	158.6	71.4	0.0982 µg/L	0.0982 ppb	19:57:35
3	Mo 202.031†	-25.3	31.1	0.9808 µg/L	0.9808 ppb	19:57:35
3	Ni 231.604†	-42.1	0.8	0.0099 µg/L	0.0099 ppb	19:57:35
3	P 214.914†	71.3	-11.5	-2.7700 µg/L	-2.7700 ppb	19:57:35
3	Pb 220.353†	104.0	-13.2	-0.8002 µg/L	-0.8002 ppb	19:57:35
3	S 181.975 Axial†	83.8	-14.8	-11.977 µg/L	-11.977 ppb	19:57:35
3	Sb 206.836†	75.3	-14.7	-1.9710 µg/L	-1.9710 ppb	19:57:35
3	Se 196.026†	23.6	11.6	4.60 µg/L	4.60 ppb	19:57:35
3	SiO2†	1653.5	5.4	0.5590 µg/L	0.5590 ppb	19:57:35
3	Si 251.611†	763.9	52.8	0.8589 µg/L	0.8589 ppb	19:57:35
3	Sn 189.927†	2.7	0.5	0.0386 µg/L	0.0386 ppb	19:57:35
3	Ti 334.940†	894.4	217.4	0.2215 µg/L	0.2215 ppb	19:57:14
3	Tl 190.801†	-118.7	7.0	0.9364 µg/L	0.9364 ppb	19:57:35
3	U 409.014†	-431.7	67.1	4.0863 µg/L	4.0863 ppb	19:57:14
3	V 292.402†	259.2	-184.4	-1.0115 µg/L	-1.0115 ppb	19:57:14
3	Zn 213.857†	491.0	4.2	0.0263 µg/L	0.0263 ppb	19:57:35

Mean Data: CCB

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1755594.3	104.95 %	0.778			0.74%
Sc RADIAL	154844.2	106 %	1.4			1.33%
Y 371.029	1078781.4	105.50 %	0.742			0.70%
Ag 328.068†	-60.0	-0.2482 µg/L	0.06913	-0.2482 ppb	0.06913	27.85%
QC value within limits for Ag 328.068 Recovery = Not calculated						
Al 396.153Radial†	-6.6	-1.4676 µg/L	1.83335	-1.4676 ppb	1.83335	124.92%
QC value within limits for Al 396.153Radial Recovery = Not calculated						
As 188.979†	3.6	1.5198 µg/L	2.62149	1.5198 ppb	2.62149	172.49%
QC value within limits for As 188.979 Recovery = Not calculated						
B 249.677†	-396.2	-6.6511 µg/L	0.41221	-6.6511 ppb	0.41221	6.20%
QC value within limits for B 249.677 Recovery = Not calculated						
Ba 233.527†	15.6	0.0707 µg/L	0.03556	0.0707 ppb	0.03556	50.28%
QC value within limits for Ba 233.527 Recovery = Not calculated						
Be 313.107†	161.2	0.0542 µg/L	0.01474	0.0542 ppb	0.01474	27.20%
QC value within limits for Be 313.107 Recovery = Not calculated						
Ca 317.933Radial†	48.5	2.8406 µg/L	0.46071	2.8406 ppb	0.46071	16.22%
QC value within limits for Ca 317.933Radial Recovery = Not calculated						
Cd 226.502†	-3.7	-0.0257 µg/L	0.08491	-0.0257 ppb	0.08491	330.30%
QC value within limits for Cd 226.502 Recovery = Not calculated						
Co 228.616†	1.7	0.0235 µg/L	0.34867	0.0235 ppb	0.34867	>999.9%

QC value within limits for Co 228.616 Recovery = Not calculated						
Cr 267.716†	-2.8	-0.0289 µg/L	0.21215	-0.0289 ppb	0.21215	734.89%
QC value within limits for Cr 267.716 Recovery = Not calculated						
Cu 324.752†	56.3	0.2495 µg/L	0.18957	0.2495 ppb	0.18957	75.99%
QC value within limits for Cu 324.752 Recovery = Not calculated						
Fe 238.204 Radial†	34.6	2.3004 µg/L	0.73735	2.3004 ppb	0.73735	32.05%
QC value within limits for Fe 238.204 Radial Recovery = Not calculated						
K 766.490 Radial†	54.2	22.323 µg/L	48.6295	22.323 ppb	48.6295	217.84%
QC value within limits for K 766.490 Radial Recovery = Not calculated						
Mg 279.077 IEC†	-28.4	-11.693 µg/L	4.1454	-11.693 ppb	4.1454	35.45%
QC value within limits for Mg 279.077 IEC Recovery = Not calculated						
Mn 257.610†	62.9	0.0864 µg/L	0.01044	0.0864 ppb	0.01044	12.09%
QC value within limits for Mn 257.610 Recovery = Not calculated						
Mo 202.031†	23.4	0.7368 µg/L	0.21697	0.7368 ppb	0.21697	29.45%
QC value within limits for Mo 202.031 Recovery = Not calculated						
Na 589.592 Radial†	-147.6	-22.610 µg/L	7.2970	-22.610 ppb	7.2970	32.27%
QC value within limits for Na 589.592 Radial Recovery = Not calculated						
Ni 231.604†	0.8	0.0104 µg/L	0.31844	0.0104 ppb	0.31844	>999.9%
QC value within limits for Ni 231.604 Recovery = Not calculated						
P 214.914†	-25.1	-6.0172 µg/L	3.48607	-6.0172 ppb	3.48607	57.93%
QC value within limits for P 214.914 Recovery = Not calculated						
Pb 220.353†	-15.2	-0.9198 µg/L	0.28391	-0.9198 ppb	0.28391	30.87%
QC value within limits for Pb 220.353 Recovery = Not calculated						
S 181.975 Axial†	-15.7	-12.716 µg/L	1.4469	-12.716 ppb	1.4469	11.38%
QC value within limits for S 181.975 Axial Recovery = Not calculated						
Sb 206.836†	-7.2	-0.9580 µg/L	1.37341	-0.9580 ppb	1.37341	143.36%
QC value within limits for Sb 206.836 Recovery = Not calculated						
Se 196.026†	5.2	2.08 µg/L	5.305	2.08 ppb	5.305	255.01%
QC value within limits for Se 196.026 Recovery = Not calculated						
SiO2†	6.9	0.7311 µg/L	0.14916	0.7311 ppb	0.14916	20.40%
QC value within limits for SiO2 Recovery = Not calculated						
Si 251.611†	70.1	1.1487 µg/L	0.26000	1.1487 ppb	0.26000	22.64%
QC value within limits for Si 251.611 Recovery = Not calculated						
Sn 189.927†	2.6	0.1884 µg/L	0.18007	0.1884 ppb	0.18007	95.55%
QC value within limits for Sn 189.927 Recovery = Not calculated						
Sr 421.552†	96.4	0.2258 µg/L	0.18764	0.2258 ppb	0.18764	83.09%
QC value within limits for Sr 421.552 Recovery = Not calculated						
Ti 334.940†	188.1	0.1905 µg/L	0.05374	0.1905 ppb	0.05374	28.21%
QC value within limits for Ti 334.940 Recovery = Not calculated						
Tl 190.801†	13.7	1.8394 µg/L	0.82412	1.8394 ppb	0.82412	44.80%
QC value within limits for Tl 190.801 Recovery = Not calculated						
U 409.014†	91.9	5.6202 µg/L	3.25513	5.6202 ppb	3.25513	57.92%
QC value within limits for U 409.014 Recovery = Not calculated						
V 292.402†	-178.5	-0.9796 µg/L	0.08622	-0.9796 ppb	0.08622	8.80%
QC value within limits for V 292.402 Recovery = Not calculated						
Zn 213.857†	21.8	0.1370 µg/L	0.10743	0.1370 ppb	0.10743	78.42%
QC value within limits for Zn 213.857 Recovery = Not calculated						
All analyte(s) passed QC.						

Sequence No.: 28

Sample ID: CCV

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 7

Date Collected: 3/29/2010 20:14:40

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCV

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	158830.4	158830.4	109 %		20:15:13
1	Al 396.153Radial†	25834.9	23739.9	5159.6 µg/L	5159.6 ppb	20:15:13
1	Ca 317.933Radial†	92141.6	83939.6	4918.5 µg/L	4918.5 ppb	20:15:13
1	Fe 238.204 Radial†	80227.4	73509.2	4887.1 µg/L	4887.1 ppb	20:15:13
1	K 766.490 Radial†	14250.9	11622.7	4780.8 µg/L	4780.8 ppb	20:15:13
1	Mg 279.077 IEC†	13509.5	12210.6	5042.2 µg/L	5042.2 ppb	20:15:13
1	Na 589.592 Radial†	71473.6	63894.6	9772.4 µg/L	9772.4 ppb	20:15:13
1	Sr 421.552†	233067.3	214157.3	501.89 µg/L	501.89 ppb	20:15:11
1	Sc 361.383	1758890.2	1758890.2	105.15 %		20:15:40
1	Y 371.029	1068006.2	1068006.2	104.44 %		20:15:40
1	Ag 328.068†	130795.7	121424.9	498.97 µg/L	498.97 ppb	20:15:40
1	As 188.979†	1305.1	1255.5	531.78 µg/L	531.78 ppb	20:16:00
1	B 249.677†	33757.2	28748.7	480.95 µg/L	480.95 ppb	20:15:40
1	Ba 233.527†	115387.0	109912.7	502.52 µg/L	502.52 ppb	20:15:40
1	Be 313.107†	1647211.3	1567223.6	510.30 µg/L	510.30 ppb	20:15:40
1	Cd 226.502†	73776.2	70258.5	484.88 µg/L	484.88 ppb	20:15:40
1	Co 228.616†	37405.4	35750.6	489.80 µg/L	489.80 ppb	20:15:40
1	Cr 267.716†	60425.3	57306.6	492.09 µg/L	492.09 ppb	20:15:40
1	Cu 324.752†	122063.0	113661.9	495.62 µg/L	495.62 ppb	20:15:40
1	Mn 257.610†	380412.8	361707.7	494.04 µg/L	494.04 ppb	20:15:40
1	Mo 202.031†	16080.3	15348.2	484.94 µg/L	484.94 ppb	20:16:00
1	Ni 231.604†	40320.7	38387.5	491.02 µg/L	491.02 ppb	20:15:40
1	P 214.914†	10614.3	10015.1	2390.0 µg/L	2390.0 ppb	20:16:00
1	Pb 220.353†	8478.6	7951.1	483.21 µg/L	483.21 ppb	20:16:00
1	S 181.975 Axial†	1339.7	1179.2	959.49 µg/L	959.49 ppb	20:16:00
1	Sb 206.836†	3893.5	3616.2	488.83 µg/L	488.83 ppb	20:16:00
1	Se 196.026†	1283.0	1209.3	480 µg/L	480 ppb	20:16:00
1	SiO2†	52444.4	48303.9	5258.8 µg/L	5258.8 ppb	20:15:40
1	Si 251.611†	157396.1	149013.5	2454.2 µg/L	2454.2 ppb	20:15:40
1	Sn 189.927†	7240.5	6884.0	491.06 µg/L	491.06 ppb	20:16:00
1	Ti 334.940†	511382.1	485708.4	494.63 µg/L	494.63 ppb	20:15:40
1	Tl 190.801†	3660.5	3601.6	490.88 µg/L	490.88 ppb	20:16:00
1	U 409.014†	7375.4	7493.4	493.30 µg/L	493.30 ppb	20:15:40
1	V 292.402†	94413.5	89359.2	501.88 µg/L	501.88 ppb	20:15:40
1	Zn 213.857†	81706.6	77241.8	482.36 µg/L	482.36 ppb	20:15:40
2	Sc RADIAL	157495.3	157495.3	108 %		20:15:18
2	Al 396.153Radial†	25706.5	23822.0	5177.5 µg/L	5177.5 ppb	20:15:18
2	Ca 317.933Radial†	91510.6	84072.4	4926.3 µg/L	4926.3 ppb	20:15:18
2	Fe 238.204 Radial†	79745.5	73687.3	4899.0 µg/L	4899.0 ppb	20:15:18
2	K 766.490 Radial†	14109.0	11602.1	4772.3 µg/L	4772.3 ppb	20:15:18
2	Mg 279.077 IEC†	13430.6	12242.7	5055.5 µg/L	5055.5 ppb	20:15:18
2	Na 589.592 Radial†	70962.0	63977.1	9785.1 µg/L	9785.1 ppb	20:15:18
2	Sr 421.552†	232192.9	215161.2	504.24 µg/L	504.24 ppb	20:15:16
2	Sc 361.383	1762035.0	1762035.0	105.34 %		20:16:04
2	Y 371.029	1068713.1	1068713.1	104.51 %		20:16:04
2	Ag 328.068†	130782.3	121190.1	498.00 µg/L	498.00 ppb	20:16:04
2	As 188.979†	1306.9	1255.0	531.56 µg/L	531.56 ppb	20:16:24
2	B 249.677†	33992.4	28914.7	483.74 µg/L	483.74 ppb	20:16:04
2	Ba 233.527†	115511.3	109834.8	502.16 µg/L	502.16 ppb	20:16:04
2	Be 313.107†	1645684.7	1562978.3	508.91 µg/L	508.91 ppb	20:16:04
2	Cd 226.502†	74022.3	70366.9	485.63 µg/L	485.63 ppb	20:16:04
2	Co 228.616†	37443.2	35723.0	489.42 µg/L	489.42 ppb	20:16:04
2	Cr 267.716†	60364.6	57146.4	490.71 µg/L	490.71 ppb	20:16:04
2	Cu 324.752†	122082.7	113473.4	494.80 µg/L	494.80 ppb	20:16:04
2	Mn 257.610†	380150.5	360813.0	492.82 µg/L	492.82 ppb	20:16:04
2	Mo 202.031†	16156.3	15393.1	486.35 µg/L	486.35 ppb	20:16:24
2	Ni 231.604†	40290.4	38290.3	489.78 µg/L	489.78 ppb	20:16:04
2	P 214.914†	10621.1	10003.5	2387.2 µg/L	2387.2 ppb	20:16:24
2	Pb 220.353†	8535.7	7990.8	485.62 µg/L	485.62 ppb	20:16:24

2	S 181.975 Axial†	1326.2	1164.2	947.33 µg/L	947.33 ppb	20:16:24
2	Sb 206.836†	3900.6	3616.4	488.88 µg/L	488.88 ppb	20:16:24
2	Se 196.026†	1284.8	1208.8	480 µg/L	480 ppb	20:16:24
2	SiO2†	52491.8	48259.9	5253.9 µg/L	5253.9 ppb	20:16:04
2	Si 251.611†	157382.7	148733.6	2449.6 µg/L	2449.6 ppb	20:16:04
2	Sn 189.927†	7227.9	6859.8	489.33 µg/L	489.33 ppb	20:16:24
2	Ti 334.940†	511020.6	484497.1	493.40 µg/L	493.40 ppb	20:16:04
2	Tl 190.801†	3689.6	3623.0	493.72 µg/L	493.72 ppb	20:16:24
2	U 409.014†	7356.3	7462.8	491.32 µg/L	491.32 ppb	20:16:04
2	V 292.402†	94327.3	89117.0	500.55 µg/L	500.55 ppb	20:16:04
2	Zn 213.857†	81870.2	77258.4	482.47 µg/L	482.47 ppb	20:16:04
3	Sc RADIAL	156537.6	156537.6	107 %		20:15:22
3	Al 396.153Radial†	25645.9	23911.1	5196.9 µg/L	5196.9 ppb	20:15:22
3	Ca 317.933Radial†	91188.8	84290.9	4939.1 µg/L	4939.1 ppb	20:15:22
3	Fe 238.204 Radial†	79529.7	73937.9	4915.6 µg/L	4915.6 ppb	20:15:22
3	K 766.490 Radial†	14092.0	11666.3	4798.7 µg/L	4798.7 ppb	20:15:22
3	Mg 279.077 IEC†	13237.8	12139.2	5012.8 µg/L	5012.8 ppb	20:15:22
3	Na 589.592 Radial†	70964.3	64381.0	9846.9 µg/L	9846.9 ppb	20:15:22
3	Sr 421.552†	233615.3	217800.3	510.43 µg/L	510.43 ppb	20:15:20
3	Sc 361.383	1760601.0	1760601.0	105.25 %		20:16:27
3	Y 371.029	1068160.3	1068160.3	104.46 %		20:16:27
3	Ag 328.068†	130523.2	121045.1	497.39 µg/L	497.39 ppb	20:16:27
3	As 188.979†	1312.2	1261.0	534.08 µg/L	534.08 ppb	20:16:47
3	B 249.677†	33684.6	28648.5	479.28 µg/L	479.28 ppb	20:16:27
3	Ba 233.527†	115155.8	109586.4	501.03 µg/L	501.03 ppb	20:16:27
3	Be 313.107†	1645527.7	1564101.6	509.28 µg/L	509.28 ppb	20:16:27
3	Cd 226.502†	73929.1	70335.6	485.41 µg/L	485.41 ppb	20:16:27
3	Co 228.616†	37338.0	35652.0	488.45 µg/L	488.45 ppb	20:16:27
3	Cr 267.716†	60447.8	57272.2	491.80 µg/L	491.80 ppb	20:16:27
3	Cu 324.752†	121740.8	113243.0	493.79 µg/L	493.79 ppb	20:16:27
3	Mn 257.610†	379672.2	360652.5	492.60 µg/L	492.60 ppb	20:16:27
3	Mo 202.031†	16168.3	15416.9	487.10 µg/L	487.10 ppb	20:16:47
3	Ni 231.604†	40268.9	38301.0	489.91 µg/L	489.91 ppb	20:16:27
3	P 214.914†	10675.3	10063.2	2401.6 µg/L	2401.6 ppb	20:16:47
3	Pb 220.353†	8520.4	7982.9	485.15 µg/L	485.15 ppb	20:16:47
3	S 181.975 Axial†	1321.3	1160.6	944.41 µg/L	944.41 ppb	20:16:47
3	Sb 206.836†	3929.7	3647.1	493.02 µg/L	493.02 ppb	20:16:47
3	Se 196.026†	1275.2	1200.7	477 µg/L	477 ppb	20:16:47
3	SiO2†	52357.5	48172.8	5244.4 µg/L	5244.4 ppb	20:16:27
3	Si 251.611†	157210.8	148692.0	2448.9 µg/L	2448.9 ppb	20:16:27
3	Sn 189.927†	7259.6	6895.4	491.87 µg/L	491.87 ppb	20:16:47
3	Ti 334.940†	509954.6	483879.4	492.77 µg/L	492.77 ppb	20:16:27
3	Tl 190.801†	3695.1	3631.0	494.80 µg/L	494.80 ppb	20:16:47
3	U 409.014†	7240.3	7358.2	484.82 µg/L	484.82 ppb	20:16:27
3	V 292.402†	94156.3	89027.6	500.06 µg/L	500.06 ppb	20:16:27
3	Zn 213.857†	81777.8	77234.0	482.31 µg/L	482.31 ppb	20:16:27

Mean Data: CCV

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1760508.7	105.24 %	0.094			0.09%
Sc RADIAL	157621.1	108 %	0.8			0.73%
Y 371.029	1068293.2	104.47 %	0.036			0.03%
Ag 328.068†	121220.0	498.12 µg/L	0.794	498.12 ppb	0.794	0.16%
QC value within limits for Ag 328.068 Recovery = 99.62%						
Al 396.153Radial†	23824.3	5178.0 µg/L	18.65	5178.0 ppb	18.65	0.36%
QC value within limits for Al 396.153Radial Recovery = 103.56%						
As 188.979†	1257.1	532.47 µg/L	1.398	532.47 ppb	1.398	0.26%
QC value within limits for As 188.979 Recovery = 106.49%						
B 249.677†	28770.7	481.32 µg/L	2.255	481.32 ppb	2.255	0.47%
QC value within limits for B 249.677 Recovery = 96.26%						
Ba 233.527†	109778.0	501.91 µg/L	0.779	501.91 ppb	0.779	0.16%
QC value within limits for Ba 233.527 Recovery = 100.38%						
Be 313.107†	1564767.8	509.50 µg/L	0.717	509.50 ppb	0.717	0.14%
QC value within limits for Be 313.107 Recovery = 101.90%						
Ca 317.933Radial†	84101.0	4928.0 µg/L	10.39	4928.0 ppb	10.39	0.21%
QC value within limits for Ca 317.933Radial Recovery = 98.56%						
Cd 226.502†	70320.3	485.30 µg/L	0.384	485.30 ppb	0.384	0.08%
QC value within limits for Cd 226.502 Recovery = 97.06%						
Co 228.616†	35708.6	489.22 µg/L	0.698	489.22 ppb	0.698	0.14%

QC value within limits for Co 228.616	Recovery = 97.84%			
Cr 267.716†	57241.7	491.53 µg/L	0.725	491.53 ppb
QC value within limits for Cr 267.716	Recovery = 98.31%			
Cu 324.752†	113459.4	494.74 µg/L	0.914	494.74 ppb
QC value within limits for Cu 324.752	Recovery = 98.95%			
Fe 238.204 Radial†	73711.5	4900.6 µg/L	14.32	4900.6 ppb
QC value within limits for Fe 238.204 Radial	Recovery = 98.01%			
K 766.490 Radial†	11630.4	4783.9 µg/L	13.48	4783.9 ppb
QC value within limits for K 766.490 Radial	Recovery = 95.68%			
Mg 279.077 IEC†	12197.5	5036.8 µg/L	21.85	5036.8 ppb
QC value within limits for Mg 279.077 IEC	Recovery = 100.74%			
Mn 257.610†	361057.7	493.15 µg/L	0.777	493.15 ppb
QC value within limits for Mn 257.610	Recovery = 98.63%			
Mo 202.031†	15386.1	486.13 µg/L	1.101	486.13 ppb
QC value within limits for Mo 202.031	Recovery = 97.23%			
Na 589.592 Radial†	64084.3	9801.5 µg/L	39.82	9801.5 ppb
QC value within limits for Na 589.592 Radial	Recovery = 98.01%			
Ni 231.604†	38326.3	490.24 µg/L	0.682	490.24 ppb
QC value within limits for Ni 231.604	Recovery = 98.05%			
P 214.914†	10027.2	2392.9 µg/L	7.59	2392.9 ppb
QC value within limits for P 214.914	Recovery = 95.72%			
Pb 220.353†	7974.9	484.66 µg/L	1.279	484.66 ppb
QC value within limits for Pb 220.353	Recovery = 96.93%			
S 181.975 Axial†	1168.0	950.41 µg/L	8.003	950.41 ppb
QC value within limits for S 181.975 Axial	Recovery = 95.04%			
Sb 206.836†	3626.6	490.24 µg/L	2.403	490.24 ppb
QC value within limits for Sb 206.836	Recovery = 98.05%			
Se 196.026†	1206.3	479 µg/L	1.9	479 ppb
QC value within limits for Se 196.026	Recovery = 95.86%			
SiO2†	48245.5	5252.4 µg/L	7.33	5252.4 ppb
QC value within limits for SiO2	Recovery = 98.22%			
Si 251.611†	148813.1	2450.9 µg/L	2.90	2450.9 ppb
QC value within limits for Si 251.611	Recovery = 98.04%			
Sn 189.927†	6879.7	490.75 µg/L	1.293	490.75 ppb
QC value within limits for Sn 189.927	Recovery = 98.15%			
Sr 421.552†	215706.3	505.52 µg/L	4.410	505.52 ppb
QC value within limits for Sr 421.552	Recovery = 101.10%			
Ti 334.940†	484695.0	493.60 µg/L	0.946	493.60 ppb
QC value within limits for Ti 334.940	Recovery = 98.72%			
Tl 190.801†	3618.5	493.13 µg/L	2.027	493.13 ppb
QC value within limits for Tl 190.801	Recovery = 98.63%			
U 409.014†	7438.1	489.81 µg/L	4.433	489.81 ppb
QC value within limits for U 409.014	Recovery = 97.96%			
V 292.402†	89167.9	500.83 µg/L	0.945	500.83 ppb
QC value within limits for V 292.402	Recovery = 100.17%			
Zn 213.857†	77244.7	482.38 µg/L	0.080	482.38 ppb
QC value within limits for Zn 213.857	Recovery = 96.48%			

All analyte(s) passed QC.

Sequence No.: 29

Sample ID: CCB

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 8

Date Collected: 3/29/2010 20:16:54

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCB

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	158157.7	158157.7	109 %		20:17:23
1	Al 396.153Radial†	-63.6	-26.8	-5.8638 µg/L	-5.8638 ppb	20:17:43
1	Ca 317.933Radial†	734.1	60.4	3.5365 µg/L	3.5365 ppb	20:17:43
1	Fe 238.204 Radial†	186.1	58.3	3.8728 µg/L	3.8728 ppb	20:17:43
1	K 766.490 Radial†	1649.8	65.4	26.926 µg/L	26.926 ppb	20:17:23
1	Mg 279.077 IEC†	176.6	-23.9	-9.8603 µg/L	-9.8603 ppb	20:17:43
1	Na 589.592 Radial†	1600.7	-219.6	-33.624 µg/L	-33.624 ppb	20:17:23
1	Sr 421.552†	-113.7	173.2	0.4058 µg/L	0.4058 ppb	20:17:23
1	Sc 361.383	1797162.4	1797162.4	107.44 %		20:18:45
1	Y 371.029	1101535.0	1101535.0	107.72 %		20:18:45
1	Ag 328.068†	3189.5	1.7	0.0181 µg/L	0.0181 ppb	20:18:47
1	As 188.979†	-18.7	-3.2	-1.3282 µg/L	-1.3282 ppb	20:19:07
1	B 249.677†	3164.5	-410.2	-6.8868 µg/L	-6.8868 ppb	20:19:07
1	Ba 233.527†	-166.3	20.3	0.0925 µg/L	0.0925 ppb	20:19:07
1	Be 313.107†	-796.9	-81.6	-0.0232 µg/L	-0.0232 ppb	20:18:47
1	Cd 226.502†	-88.5	12.1	0.0830 µg/L	0.0830 ppb	20:19:07
1	Co 228.616†	-182.6	6.7	0.0913 µg/L	0.0913 ppb	20:19:07
1	Cr 267.716†	146.8	-23.6	-0.2111 µg/L	-0.2111 ppb	20:19:07
1	Cu 324.752†	2533.1	-67.1	-0.2822 µg/L	-0.2822 ppb	20:18:47
1	Mn 257.610†	189.2	96.1	0.1316 µg/L	0.1316 ppb	20:19:07
1	Mo 202.031†	-43.6	14.6	0.4617 µg/L	0.4617 ppb	20:19:07
1	Ni 231.604†	-36.3	7.1	0.0912 µg/L	0.0912 ppb	20:19:07
1	P 214.914†	33.9	-48.0	-11.496 µg/L	-11.496 ppb	20:19:07
1	Pb 220.353†	106.6	-13.2	-0.8080 µg/L	-0.8080 ppb	20:19:07
1	S 181.975 Axial†	94.0	-7.3	-5.9118 µg/L	-5.9118 ppb	20:19:07
1	Sb 206.836†	77.5	-14.5	-1.9423 µg/L	-1.9423 ppb	20:19:07
1	Se 196.026†	26.1	13.3	5.29 µg/L	5.29 ppb	20:19:07
1	SiO2†	1703.2	12.4	1.3407 µg/L	1.3407 ppb	20:19:07
1	Si 251.611†	757.0	28.3	0.4592 µg/L	0.4592 ppb	20:19:07
1	Sn 189.927†	6.4	3.9	0.2796 µg/L	0.2796 ppb	20:19:07
1	Ti 334.940†	1092.2	380.2	0.3841 µg/L	0.3841 ppb	20:18:47
1	Tl 190.801†	-110.1	17.8	2.3981 µg/L	2.3981 ppb	20:19:07
1	U 409.014†	-322.2	179.2	11.064 µg/L	11.064 ppb	20:18:47
1	V 292.402†	429.3	-32.2	-0.1685 µg/L	-0.1685 ppb	20:18:47
1	Zn 213.857†	497.4	-1.5	-0.0099 µg/L	-0.0099 ppb	20:19:07
2	Sc RADIAL	155691.2	155691.2	107 %		20:17:45
2	Al 396.153Radial†	-30.3	3.5	0.7196 µg/L	0.7196 ppb	20:18:05
2	Ca 317.933Radial†	713.2	51.5	3.0148 µg/L	3.0148 ppb	20:18:05
2	Fe 238.204 Radial†	162.5	38.8	2.5826 µg/L	2.5826 ppb	20:18:05
2	K 766.490 Radial†	1523.5	-28.7	-11.809 µg/L	-11.809 ppb	20:17:45
2	Mg 279.077 IEC†	195.4	-3.7	-1.5189 µg/L	-1.5189 ppb	20:18:05
2	Na 589.592 Radial†	1538.6	-254.3	-38.906 µg/L	-38.906 ppb	20:17:45
2	Sr 421.552†	-172.2	116.8	0.2737 µg/L	0.2737 ppb	20:17:45
2	Sc 361.383	1776190.8	1776190.8	106.18 %		20:19:09
2	Y 371.029	1089581.5	1089581.5	106.55 %		20:19:09
2	Ag 328.068†	3209.2	55.3	0.2233 µg/L	0.2233 ppb	20:19:11
2	As 188.979†	-18.8	-3.4	-1.4319 µg/L	-1.4319 ppb	20:19:31
2	B 249.677†	3163.9	-376.0	-6.3128 µg/L	-6.3128 ppb	20:19:31
2	Ba 233.527†	-158.5	25.8	0.1177 µg/L	0.1177 ppb	20:19:31
2	Be 313.107†	-622.2	74.1	0.0253 µg/L	0.0253 ppb	20:19:11
2	Cd 226.502†	-71.9	26.7	0.1839 µg/L	0.1839 ppb	20:19:31
2	Co 228.616†	-183.6	3.7	0.0500 µg/L	0.0500 ppb	20:19:31
2	Cr 267.716†	166.1	-3.8	-0.0355 µg/L	-0.0355 ppb	20:19:31
2	Cu 324.752†	2626.6	48.8	0.2155 µg/L	0.2155 ppb	20:19:11
2	Mn 257.610†	203.0	111.2	0.1519 µg/L	0.1519 ppb	20:19:31
2	Mo 202.031†	-29.4	27.5	0.8686 µg/L	0.8686 ppb	20:19:31
2	Ni 231.604†	-58.1	-13.8	-0.1766 µg/L	-0.1766 ppb	20:19:31
2	P 214.914†	38.3	-43.5	-10.438 µg/L	-10.438 ppb	20:19:31
2	Pb 220.353†	142.1	21.4	1.2928 µg/L	1.2928 ppb	20:19:31

2	S 181.975 Axial†	84.7	-15.1	-12.191 µg/L	-12.191 ppb	20:19:31
2	Sb 206.836†	90.2	-1.7	-0.2231 µg/L	-0.2231 ppb	20:19:31
2	Se 196.026†	16.7	4.8	1.90 µg/L	1.90 ppb	20:19:31
2	SiO2†	1687.5	16.4	1.7745 µg/L	1.7745 ppb	20:19:31
2	Si 251.611†	744.1	24.4	0.3950 µg/L	0.3950 ppb	20:19:31
2	Sn 189.927†	-5.5	-7.2	-0.5152 µg/L	-0.5152 ppb	20:19:31
2	Ti 334.940†	590.2	-80.5	-0.0834 µg/L	-0.0834 ppb	20:19:11
2	Tl 190.801†	-116.1	11.0	1.4736 µg/L	1.4736 ppb	20:19:31
2	U 409.014†	-444.6	60.4	3.7028 µg/L	3.7028 ppb	20:19:11
2	V 292.402†	365.2	-87.9	-0.4766 µg/L	-0.4766 ppb	20:19:11
2	Zn 213.857†	508.8	14.8	0.0938 µg/L	0.0938 ppb	20:19:31
3	Sc RADIAL	155889.7	155889.7	107 %		20:18:07
3	Al 396.153Radial†	-21.6	11.7	2.4989 µg/L	2.4989 ppb	20:18:27
3	Ca 317.933Radial†	710.6	48.2	2.8268 µg/L	2.8268 ppb	20:18:27
3	Fe 238.204 Radial†	176.6	51.8	3.4464 µg/L	3.4464 ppb	20:18:27
3	K 766.490 Radial†	1522.8	-31.2	-12.835 µg/L	-12.835 ppb	20:18:07
3	Mg 279.077 IEC†	169.6	-28.1	-11.582 µg/L	-11.582 ppb	20:18:27
3	Na 589.592 Radial†	1514.3	-278.9	-42.658 µg/L	-42.658 ppb	20:18:07
3	Sr 421.552†	-115.2	170.3	0.3991 µg/L	0.3991 ppb	20:18:07
3	Sc 361.383	1775735.1	1775735.1	106.16 %		20:19:33
3	Y 371.029	1090212.1	1090212.1	106.61 %		20:19:33
3	Ag 328.068†	3310.5	151.5	0.6044 µg/L	0.6044 ppb	20:19:35
3	As 188.979†	-18.3	-3.0	-1.2478 µg/L	-1.2478 ppb	20:19:55
3	B 249.677†	3162.1	-376.9	-6.3290 µg/L	-6.3290 ppb	20:19:55
3	Ba 233.527†	-165.4	19.2	0.0872 µg/L	0.0872 ppb	20:19:55
3	Be 313.107†	-659.6	38.8	0.0140 µg/L	0.0140 ppb	20:19:35
3	Cd 226.502†	-97.0	3.1	0.0206 µg/L	0.0206 ppb	20:19:55
3	Co 228.616†	-161.6	24.4	0.3340 µg/L	0.3340 ppb	20:19:55
3	Cr 267.716†	177.4	6.9	0.0553 µg/L	0.0553 ppb	20:19:55
3	Cu 324.752†	2774.4	188.7	0.8244 µg/L	0.8244 ppb	20:19:35
3	Mn 257.610†	182.4	91.8	0.1259 µg/L	0.1259 ppb	20:19:55
3	Mo 202.031†	-25.4	31.3	0.9879 µg/L	0.9879 ppb	20:19:55
3	Ni 231.604†	-68.5	-23.6	-0.3019 µg/L	-0.3019 ppb	20:19:55
3	P 214.914†	51.6	-31.0	-7.4391 µg/L	-7.4391 ppb	20:19:55
3	Pb 220.353†	84.6	-32.7	-1.9844 µg/L	-1.9844 ppb	20:19:55
3	S 181.975 Axial†	85.3	-14.4	-11.697 µg/L	-11.697 ppb	20:19:55
3	Sb 206.836†	54.5	-35.3	-4.7507 µg/L	-4.7507 ppb	20:19:55
3	Se 196.026†	0.8	-10.1	-4.01 µg/L	-4.01 ppb	20:19:55
3	SiO2†	1675.1	5.1	0.5352 µg/L	0.5352 ppb	20:19:55
3	Si 251.611†	757.0	36.7	0.5978 µg/L	0.5978 ppb	20:19:55
3	Sn 189.927†	-6.1	-7.8	-0.5522 µg/L	-0.5522 ppb	20:19:55
3	Ti 334.940†	761.4	80.9	0.0816 µg/L	0.0816 ppb	20:19:35
3	Tl 190.801†	-108.3	18.3	2.4419 µg/L	2.4419 ppb	20:19:55
3	U 409.014†	-429.2	74.8	4.5456 µg/L	4.5456 ppb	20:19:35
3	V 292.402†	201.6	-241.9	-1.3288 µg/L	-1.3288 ppb	20:19:35
3	Zn 213.857†	514.6	20.3	0.1291 µg/L	0.1291 ppb	20:19:55

Mean Data: CCB

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1783029.4	106.59 %	0.732			0.69%
Sc RADIAL	156579.5	107 %	0.9			0.88%
Y 371.029	1093776.2	106.96 %	0.658			0.61%
Ag 328.068†	69.5	0.2819 µg/L	0.29754	0.2819 ppb	0.29754	105.55%
QC value within limits for Ag 328.068 Recovery = Not calculated						
Al 396.153Radial†	-3.9	-0.8818 µg/L	4.40531	-0.8818 ppb	4.40531	499.59%
QC value within limits for Al 396.153Radial Recovery = Not calculated						
As 188.979†	-3.2	-1.3360 µg/L	0.09228	-1.3360 ppb	0.09228	6.91%
QC value within limits for As 188.979 Recovery = Not calculated						
B 249.677†	-387.7	-6.5095 µg/L	0.32684	-6.5095 ppb	0.32684	5.02%
QC value within limits for B 249.677 Recovery = Not calculated						
Ba 233.527†	21.7	0.0991 µg/L	0.01628	0.0991 ppb	0.01628	16.43%
QC value within limits for Ba 233.527 Recovery = Not calculated						
Be 313.107†	10.4	0.0053 µg/L	0.02537	0.0053 ppb	0.02537	474.55%
QC value within limits for Be 313.107 Recovery = Not calculated						
Ca 317.933Radial†	53.3	3.1261 µg/L	0.36770	3.1261 ppb	0.36770	11.76%
QC value within limits for Ca 317.933Radial Recovery = Not calculated						
Cd 226.502†	13.9	0.0958 µg/L	0.08241	0.0958 ppb	0.08241	85.99%
QC value within limits for Cd 226.502 Recovery = Not calculated						
Co 228.616†	11.6	0.1584 µg/L	0.15343	0.1584 ppb	0.15343	96.85%

Cr 267.716†	QC value within limits for Co 228.616	Recovery = Not calculated			
	-6.8	-0.0638 µg/L	0.13543	-0.0638 ppb	0.13543 212.32%
Cu 324.752†	QC value within limits for Cr 267.716	Recovery = Not calculated			
	56.8	0.2526 µg/L	0.55423	0.2526 ppb	0.55423 219.45%
Fe 238.204 Radial†	QC value within limits for Cu 324.752	Recovery = Not calculated			
	49.6	3.3006 µg/L	0.65736	3.3006 ppb	0.65736 19.92%
K 766.490 Radial†	QC value within limits for Fe 238.204 Radial	Recovery = Not calculated			
	1.8	0.7609 µg/L	22.66551	0.7609 ppb	22.66551 >999.9%
Mg 279.077 IEC†	QC value within limits for K 766.490 Radial	Recovery = Not calculated			
	-18.6	-7.6537 µg/L	5.38218	-7.6537 ppb	5.38218 70.32%
Mn 257.610†	QC value within limits for Mg 279.077 IEC	Recovery = Not calculated			
	99.7	0.1365 µg/L	0.01367	0.1365 ppb	0.01367 10.02%
Mo 202.031†	QC value within limits for Mn 257.610	Recovery = Not calculated			
	24.5	0.7728 µg/L	0.27588	0.7728 ppb	0.27588 35.70%
Na 589.592 Radial†	QC value within limits for Mo 202.031	Recovery = Not calculated			
	-250.9	-38.396 µg/L	4.5384	-38.396 ppb	4.5384 11.82%
Ni 231.604†	QC value within limits for Na 589.592 Radial	Recovery = Not calculated			
	-10.1	-0.1291 µg/L	0.20080	-0.1291 ppb	0.20080 155.54%
P 214.914†	QC value within limits for Ni 231.604	Recovery = Not calculated			
	-40.8	-9.7910 µg/L	2.10426	-9.7910 ppb	2.10426 21.49%
Pb 220.353†	QC value within limits for P 214.914	Recovery = Not calculated			
	-8.2	-0.4998 µg/L	1.66019	-0.4998 ppb	1.66019 332.15%
S 181.975 Axial†	QC value within limits for Pb 220.353	Recovery = Not calculated			
	-12.3	-9.9332 µg/L	3.49134	-9.9332 ppb	3.49134 35.15%
Sb 206.836†	QC value within limits for S 181.975 Axial	Recovery = Not calculated			
	-17.2	-2.3053 µg/L	2.28550	-2.3053 ppb	2.28550 99.14%
Se 196.026†	QC value within limits for Sb 206.836	Recovery = Not calculated			
	2.7	1.06 µg/L	4.705	1.06 ppb	4.705 444.44%
SiO2†	QC value within limits for Se 196.026	Recovery = Not calculated			
	11.3	1.2168 µg/L	0.62889	1.2168 ppb	0.62889 51.68%
Si 251.611†	QC value within limits for SiO2	Recovery = Not calculated			
	29.8	0.4840 µg/L	0.10365	0.4840 ppb	0.10365 21.42%
Sn 189.927†	QC value within limits for Si 251.611	Recovery = Not calculated			
	-3.7	-0.2626 µg/L	0.46990	-0.2626 ppb	0.46990 178.94%
Sr 421.552†	QC value within limits for Sn 189.927	Recovery = Not calculated			
	153.4	0.3595 µg/L	0.07442	0.3595 ppb	0.07442 20.70%
Ti 334.940†	QC value within limits for Sr 421.552	Recovery = Not calculated			
	126.9	0.1275 µg/L	0.23711	0.1275 ppb	0.23711 186.03%
Tl 190.801†	QC value within limits for Ti 334.940	Recovery = Not calculated			
	15.7	2.1045 µg/L	0.54683	2.1045 ppb	0.54683 25.98%
U 409.014†	QC value within limits for Tl 190.801	Recovery = Not calculated			
	104.8	6.4375 µg/L	4.02889	6.4375 ppb	4.02889 62.58%
V 292.402†	QC value within limits for U 409.014	Recovery = Not calculated			
	-120.7	-0.6580 µg/L	0.60105	-0.6580 ppb	0.60105 91.35%
Zn 213.857†	QC value within limits for V 292.402	Recovery = Not calculated			
	11.2	0.0710 µg/L	0.07224	0.0710 ppb	0.07224 101.73%
	QC value within limits for Zn 213.857	Recovery = Not calculated			

All analyte(s) passed QC.

Sequence No.: 30

Sample ID: 1202056866|959109|1

Analyst: HSC

Initial Sample Wt:

Dilution:

Autosampler Location: 324

Date Collected: 3/29/2010 20:20:04

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: 1202056866|959109|1

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	157385.0	157385.0	108 %		20:20:36
1	Al 396.153Radial†	-8.0	24.5	5.2915 µg/L	5.2915 ppb	20:20:56
1	Ca 317.933Radial†	774.9	101.4	5.9420 µg/L	5.9420 ppb	20:20:56
1	Fe 238.204 Radial†	341.8	203.3	13.514 µg/L	13.514 ppb	20:20:56
1	K 766.490 Radial†	1553.3	-16.5	-6.7715 µg/L	-6.7715 ppb	20:20:36
1	Mg 279.077 IEC†	180.5	-19.5	-8.0285 µg/L	-8.0285 ppb	20:20:56
1	Na 589.592 Radial†	1691.6	-128.1	-19.598 µg/L	-19.598 ppb	20:20:36
1	Sr 421.552†	-265.1	32.4	0.0760 µg/L	0.0760 ppb	20:20:36
1	Sc 361.383	1783162.4	1783162.4	106.60 %		20:21:44
1	Y 371.029	1090137.4	1090137.4	106.61 %		20:21:44
1	Ag 328.068†	3204.3	38.9	0.1558 µg/L	0.1558 ppb	20:21:46
1	As 188.979†	-17.8	-2.5	-1.0360 µg/L	-1.0360 ppb	20:22:06
1	B 249.677†	3164.6	-387.0	-6.4973 µg/L	-6.4973 ppb	20:22:06
1	Ba 233.527†	-159.8	25.1	0.1140 µg/L	0.1140 ppb	20:22:06
1	Be 313.107†	-580.4	115.7	0.0421 µg/L	0.0421 ppb	20:21:46
1	Cd 226.502†	-94.8	5.4	0.0362 µg/L	0.0362 ppb	20:22:06
1	Co 228.616†	-176.8	10.8	0.1470 µg/L	0.1470 ppb	20:22:06
1	Cr 267.716†	187.9	16.0	0.1257 µg/L	0.1257 ppb	20:22:06
1	Cu 324.752†	2760.8	165.0	0.7312 µg/L	0.7312 ppb	20:21:46
1	Mn 257.610†	325.9	225.7	0.3088 µg/L	0.3088 ppb	20:22:06
1	Mo 202.031†	-21.1	35.5	1.1191 µg/L	1.1191 ppb	20:22:06
1	Ni 231.604†	-23.9	18.5	0.2370 µg/L	0.2370 ppb	20:22:06
1	P 214.914†	62.2	-21.2	-5.1165 µg/L	-5.1165 ppb	20:22:06
1	Pb 220.353†	101.0	-17.7	-1.0785 µg/L	-1.0785 ppb	20:22:06
1	S 181.975 Axial†	90.7	-9.7	-7.8623 µg/L	-7.8623 ppb	20:22:06
1	Sb 206.836†	91.1	-1.2	-0.1533 µg/L	-0.1533 ppb	20:22:06
1	Se 196.026†	12.9	1.2	0.488 µg/L	0.488 ppb	20:22:06
1	SiO2†	2242.9	531.2	58.039 µg/L	58.039 ppb	20:22:06
1	Si 251.611†	2337.2	1516.1	25.060 µg/L	25.060 ppb	20:21:46
1	Sn 189.927†	-11.2	-12.5	-0.8874 µg/L	-0.8874 ppb	20:22:06
1	Ti 334.940†	903.9	211.6	0.2105 µg/L	0.2105 ppb	20:21:46
1	Tl 190.801†	-117.8	9.8	1.3040 µg/L	1.3040 ppb	20:22:06
1	U 409.014†	-258.2	236.9	14.541 µg/L	14.541 ppb	20:21:46
1	V 292.402†	139.7	-300.8	-1.6489 µg/L	-1.6489 ppb	20:21:46
1	Zn 213.857†	738.3	228.2	1.4332 µg/L	1.4332 ppb	20:22:06
2	Sc RADIAL	155647.0	155647.0	107 %		20:20:58
2	Al 396.153Radial†	15.0	46.0	9.9857 µg/L	9.9857 ppb	20:21:18
2	Ca 317.933Radial†	761.3	96.7	5.6672 µg/L	5.6672 ppb	20:21:18
2	Fe 238.204 Radial†	356.1	220.2	14.640 µg/L	14.640 ppb	20:21:18
2	K 766.490 Radial†	1463.9	-84.1	-34.625 µg/L	-34.625 ppb	20:20:58
2	Mg 279.077 IEC†	178.0	-20.0	-8.2469 µg/L	-8.2469 ppb	20:21:18
2	Na 589.592 Radial†	1599.1	-197.2	-30.149 µg/L	-30.149 ppb	20:20:58
2	Sr 421.552†	-225.1	67.2	0.1574 µg/L	0.1574 ppb	20:20:58
2	Sc 361.383	1790615.6	1790615.6	107.04 %		20:22:08
2	Y 371.029	1094058.1	1094058.1	106.99 %		20:22:08
2	Ag 328.068†	2882.1	-274.6	-1.1165 µg/L	-1.1165 ppb	20:22:10
2	As 188.979†	-23.8	-8.0	-3.3419 µg/L	-3.3419 ppb	20:22:30
2	B 249.677†	3170.7	-393.7	-6.6092 µg/L	-6.6092 ppb	20:22:30
2	Ba 233.527†	-149.1	35.8	0.1633 µg/L	0.1633 ppb	20:22:30
2	Be 313.107†	-636.6	65.4	0.0225 µg/L	0.0225 ppb	20:22:10
2	Cd 226.502†	-106.9	-5.5	-0.0394 µg/L	-0.0394 ppb	20:22:30
2	Co 228.616†	-184.6	4.2	0.0566 µg/L	0.0566 ppb	20:22:30
2	Cr 267.716†	182.7	10.4	0.0865 µg/L	0.0865 ppb	20:22:30
2	Cu 324.752†	2788.4	180.0	0.7880 µg/L	0.7880 ppb	20:22:10
2	Mn 257.610†	293.6	194.3	0.2658 µg/L	0.2658 ppb	20:22:30
2	Mo 202.031†	-25.0	31.9	1.0065 µg/L	1.0065 ppb	20:22:30
2	Ni 231.604†	-50.4	-6.1	-0.0785 µg/L	-0.0785 ppb	20:22:30
2	P 214.914†	62.7	-21.0	-5.0455 µg/L	-5.0455 ppb	20:22:30
2	Pb 220.353†	93.3	-25.3	-1.5330 µg/L	-1.5330 ppb	20:22:30

2	S 181.975 Axial†	93.6	-7.4	-5.9985 µg/L	-5.9985 ppb	20:22:30
2	Sb 206.836†	96.5	3.5	0.4866 µg/L	0.4866 ppb	20:22:30
2	Se 196.026†	16.7	4.7	1.86 µg/L	1.86 ppb	20:22:30
2	SiO2†	2211.2	492.8	53.838 µg/L	53.838 ppb	20:22:30
2	Si 251.611†	2434.1	1597.5	26.401 µg/L	26.401 ppb	20:22:10
2	Sn 189.927†	3.9	1.6	0.1155 µg/L	0.1155 ppb	20:22:30
2	Ti 334.940†	941.0	242.7	0.2466 µg/L	0.2466 ppb	20:22:10
2	Tl 190.801†	-124.8	3.7	0.5008 µg/L	0.5008 ppb	20:22:30
2	U 409.014†	-441.6	66.6	4.0770 µg/L	4.0770 ppb	20:22:10
2	V 292.402†	348.4	-106.4	-0.5792 µg/L	-0.5792 ppb	20:22:10
2	Zn 213.857†	716.2	204.7	1.2870 µg/L	1.2870 ppb	20:22:30
3	Sc RADIAL	158974.7	158974.7	109 %		20:21:20
3	Al 396.153Radial†	-1.4	30.6	6.6425 µg/L	6.6425 ppb	20:21:40
3	Ca 317.933Radial†	783.6	102.3	5.9935 µg/L	5.9935 ppb	20:21:40
3	Fe 238.204 Radial†	319.3	179.5	11.934 µg/L	11.934 ppb	20:21:40
3	K 766.490 Radial†	1529.9	-52.3	-21.545 µg/L	-21.545 ppb	20:21:20
3	Mg 279.077 IEC†	194.1	-8.7	-3.5890 µg/L	-3.5890 ppb	20:21:40
3	Na 589.592 Radial†	1527.9	-293.9	-44.946 µg/L	-44.946 ppb	20:21:20
3	Sr 421.552†	-364.3	-56.0	-0.1313 µg/L	-0.1313 ppb	20:21:20
3	Sc 361.383	1783384.3	1783384.3	106.61 %		20:22:32
3	Y 371.029	1089400.3	1089400.3	106.53 %		20:22:32
3	Ag 328.068†	2929.4	-219.3	-0.8740 µg/L	-0.8740 ppb	20:22:34
3	As 188.979†	-11.8	3.2	1.3424 µg/L	1.3424 ppb	20:22:54
3	B 249.677†	3151.3	-399.8	-6.7127 µg/L	-6.7127 ppb	20:22:54
3	Ba 233.527†	-160.6	24.4	0.1114 µg/L	0.1114 ppb	20:22:54
3	Be 313.107†	-824.8	-113.5	-0.0328 µg/L	-0.0328 ppb	20:22:34
3	Cd 226.502†	-103.4	-2.6	-0.0190 µg/L	-0.0190 ppb	20:22:54
3	Co 228.616†	-185.0	3.0	0.0410 µg/L	0.0410 ppb	20:22:54
3	Cr 267.716†	190.4	18.4	0.1475 µg/L	0.1475 ppb	20:22:54
3	Cu 324.752†	2704.4	111.8	0.4992 µg/L	0.4992 ppb	20:22:34
3	Mn 257.610†	320.3	220.4	0.3013 µg/L	0.3013 ppb	20:22:54
3	Mo 202.031†	-34.7	22.7	0.7168 µg/L	0.7168 ppb	20:22:54
3	Ni 231.604†	-50.3	-6.2	-0.0797 µg/L	-0.0797 ppb	20:22:54
3	P 214.914†	55.7	-27.4	-6.5692 µg/L	-6.5692 ppb	20:22:54
3	Pb 220.353†	103.1	-15.7	-0.9620 µg/L	-0.9620 ppb	20:22:54
3	S 181.975 Axial†	93.9	-6.8	-5.4632 µg/L	-5.4632 ppb	20:22:54
3	Sb 206.836†	87.3	-4.8	-0.6378 µg/L	-0.6378 ppb	20:22:54
3	Se 196.026†	13.1	1.3	0.550 µg/L	0.550 ppb	20:22:54
3	SiO2†	2218.2	507.7	55.472 µg/L	55.472 ppb	20:22:54
3	Si 251.611†	2753.3	1906.2	31.507 µg/L	31.507 ppb	20:22:34
3	Sn 189.927†	6.0	3.6	0.2550 µg/L	0.2550 ppb	20:22:54
3	Ti 334.940†	833.5	145.5	0.1431 µg/L	0.1431 ppb	20:22:34
3	Tl 190.801†	-117.7	9.9	1.3317 µg/L	1.3317 ppb	20:22:54
3	U 409.014†	-273.0	223.0	13.778 µg/L	13.778 ppb	20:22:34
3	V 292.402†	449.7	-10.1	-0.0405 µg/L	-0.0405 ppb	20:22:34
3	Zn 213.857†	743.8	233.2	1.4674 µg/L	1.4674 ppb	20:22:54

Mean Data: 1202056866|959109|1

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1785720.7	106.75 %	0.254			0.24%
Sc RADIAL	157335.6	108 %	1.1			1.06%
Y 371.029	1091198.6	106.71 %	0.245			0.23%
Ag 328.068†	-151.7	-0.6116 µg/L	0.67552	-0.6116 ppb	0.67552	110.45%
Al 396.153Radial†	33.7	7.3066 µg/L	2.41656	7.3066 ppb	2.41656	33.07%
As 188.979†	-2.4	-1.0119 µg/L	2.34223	-1.0119 ppb	2.34223	231.48%
B 249.677†	-393.5	-6.6064 µg/L	0.10770	-6.6064 ppb	0.10770	1.63%
Ba 233.527†	28.4	0.1296 µg/L	0.02922	0.1296 ppb	0.02922	22.56%
Be 313.107†	22.5	0.0106 µg/L	0.03883	0.0106 ppb	0.03883	365.91%
Ca 317.933Radial†	100.1	5.8676 µg/L	0.17544	5.8676 ppb	0.17544	2.99%
Cd 226.502†	-0.9	-0.0074 µg/L	0.03912	-0.0074 ppb	0.03912	528.80%
Co 228.616†	6.0	0.0815 µg/L	0.05723	0.0815 ppb	0.05723	70.20%
Cr 267.716†	14.9	0.1199 µg/L	0.03092	0.1199 ppb	0.03092	25.79%
Cu 324.752†	152.3	0.6728 µg/L	0.15301	0.6728 ppb	0.15301	22.74%
Fe 238.204 Radial†	201.0	13.363 µg/L	1.3592	13.363 ppb	1.3592	10.17%
K 766.490 Radial†	-51.0	-20.981 µg/L	13.9354	-20.981 ppb	13.9354	66.42%
Mg 279.077 IEC†	-16.1	-6.6214 µg/L	2.62847	-6.6214 ppb	2.62847	39.70%
Mn 257.610†	213.5	0.2920 µg/L	0.02294	0.2920 ppb	0.02294	7.86%
Mo 202.031†	30.0	0.9475 µg/L	0.20755	0.9475 ppb	0.20755	21.91%
Na 589.592 Radial†	-206.4	-31.564 µg/L	12.7330	-31.564 ppb	12.7330	40.34%

Ni 231.604†	2.1	0.0262 µg/L	0.18248	0.0262 ppb	0.18248	695.36%
P 214.914†	-23.2	-5.5771 µg/L	0.85992	-5.5771 ppb	0.85992	15.42%
Pb 220.353†	-19.6	-1.1912 µg/L	0.30168	-1.1912 ppb	0.30168	25.33%
S 181.975 Axial†	-8.0	-6.4413 µg/L	1.25937	-6.4413 ppb	1.25937	19.55%
Sb 206.836†	-0.8	-0.1015 µg/L	0.56399	-0.1015 ppb	0.56399	555.80%
Se 196.026†	2.4	0.966 µg/L	0.7740	0.966 ppb	0.7740	80.16%
SiO2†	510.6	55.783 µg/L	2.1179	55.783 ppb	2.1179	3.80%
Si 251.611†	1673.3	27.656 µg/L	3.4020	27.656 ppb	3.4020	12.30%
Sn 189.927†	-2.4	-0.1723 µg/L	0.62320	-0.1723 ppb	0.62320	361.74%
Sr 421.552†	14.5	0.0340 µg/L	0.14885	0.0340 ppb	0.14885	437.55%
Ti 334.940†	199.9	0.2001 µg/L	0.05253	0.2001 ppb	0.05253	26.26%
Tl 190.801†	7.8	1.0455 µg/L	0.47191	1.0455 ppb	0.47191	45.14%
U 409.014†	175.5	10.799 µg/L	5.8338	10.799 ppb	5.8338	54.02%
V 292.402†	-139.1	-0.7562 µg/L	0.81870	-0.7562 ppb	0.81870	108.27%
Zn 213.857†	222.0	1.3959 µg/L	0.09583	1.3959 ppb	0.09583	6.87%

Sequence No.: 31
 Sample ID: 1202056867|959109|1
 Analyst: HSC
 Initial Sample Wt:
 Dilution:

Autosampler Location: 325
 Date Collected: 3/29/2010 20:23:02
 Data Type: Original
 Initial Sample Vol:
 Sample Prep Vol:

Replicate Data: 1202056867|959109|1

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	156746.7	156746.7	108 %		20:23:34
1	Al 396.153Radial†	25702.1	23931.5	5201.5 µg/L	5201.5 ppb	20:23:34
1	Ca 317.933Radial†	91602.9	84562.6	4955.0 µg/L	4955.0 ppb	20:23:34
1	Fe 238.204 Radial†	79597.0	73901.7	4913.2 µg/L	4913.2 ppb	20:23:34
1	K 766.490 Radial†	14133.9	11687.7	4808.3 µg/L	4808.3 ppb	20:23:34
1	Mg 279.077 IEC†	13534.4	12398.6	5119.7 µg/L	5119.7 ppb	20:23:34
1	Na 589.592 Radial†	36426.8	32177.5	4919.3 µg/L	4919.3 ppb	20:23:34
1	Sr 421.552†	234639.2	218462.1	511.98 µg/L	511.98 ppb	20:23:32
1	Sc 361.383	1745938.4	1745938.4	104.37 %		20:24:00
1	Y 371.029	1058622.0	1058622.0	103.52 %		20:24:00
1	Ag 328.068†	125737.6	117501.5	483.07 µg/L	483.07 ppb	20:24:00
1	As 188.979†	1319.3	1278.2	541.29 µg/L	541.29 ppb	20:24:20
1	B 249.677†	33274.0	28524.0	477.21 µg/L	477.21 ppb	20:24:00
1	Ba 233.527†	115985.8	111300.4	508.86 µg/L	508.86 ppb	20:24:00
1	Be 313.107†	1634178.2	1566357.7	510.02 µg/L	510.02 ppb	20:24:00
1	Cd 226.502†	72655.8	69705.5	481.06 µg/L	481.06 ppb	20:24:00
1	Co 228.616†	36589.5	35232.8	482.71 µg/L	482.71 ppb	20:24:00
1	Cr 267.716†	60048.3	57371.8	492.64 µg/L	492.64 ppb	20:24:00
1	Cu 324.752†	123069.2	115487.1	503.55 µg/L	503.55 ppb	20:24:00
1	Mn 257.610†	377960.3	362041.8	494.49 µg/L	494.49 ppb	20:24:00
1	Mo 202.031†	15960.8	15347.2	484.91 µg/L	484.91 ppb	20:24:20
1	Ni 231.604†	40582.2	38922.5	497.86 µg/L	497.86 ppb	20:24:00
1	P 214.914†	2194.5	2022.9	476.04 µg/L	476.04 ppb	20:24:20
1	Pb 220.353†	8527.2	8057.5	489.65 µg/L	489.65 ppb	20:24:20
1	S 181.975 Axial†	6385.9	6023.5	4884.2 µg/L	4884.2 ppb	20:24:20
1	Sb 206.836†	3920.5	3669.6	496.03 µg/L	496.03 ppb	20:24:20
1	Se 196.026†	1269.3	1205.2	479 µg/L	479 ppb	20:24:20
1	SiO2†	100911.8	95110.2	10375 µg/L	10375 ppb	20:24:00
1	Si 251.611†	305933.1	292436.5	4825.7 µg/L	4825.7 ppb	20:24:00
1	Sn 189.927†	7294.1	6986.4	498.33 µg/L	498.33 ppb	20:24:20
1	Ti 334.940†	504616.8	482834.4	491.70 µg/L	491.70 ppb	20:24:00
1	Tl 190.801†	3720.9	3685.2	502.13 µg/L	502.13 ppb	20:24:20
1	U 409.014†	7346.5	7517.8	494.93 µg/L	494.93 ppb	20:24:00
1	V 292.402†	94142.3	89765.5	504.14 µg/L	504.14 ppb	20:24:00
1	Zn 213.857†	80129.2	76307.0	476.42 µg/L	476.42 ppb	20:24:00
2	Sc RADIAL	156995.7	156995.7	108 %		20:23:38
2	Al 396.153Radial†	25711.0	23901.9	5195.0 µg/L	5195.0 ppb	20:23:38
2	Ca 317.933Radial†	91646.4	84468.0	4949.5 µg/L	4949.5 ppb	20:23:38
2	Fe 238.204 Radial†	79851.1	74020.2	4921.1 µg/L	4921.1 ppb	20:23:38
2	K 766.490 Radial†	14251.0	11775.6	4844.5 µg/L	4844.5 ppb	20:23:38
2	Mg 279.077 IEC†	13539.7	12383.6	5113.5 µg/L	5113.5 ppb	20:23:38
2	Na 589.592 Radial†	36521.1	32211.4	4924.4 µg/L	4924.4 ppb	20:23:38
2	Sr 421.552†	232493.8	216124.4	506.50 µg/L	506.50 ppb	20:23:36
2	Sc 361.383	1745031.8	1745031.8	104.32 %		20:24:23
2	Y 371.029	1058014.3	1058014.3	103.47 %		20:24:23
2	Ag 328.068†	125573.2	117406.5	482.71 µg/L	482.71 ppb	20:24:23
2	As 188.979†	1314.2	1274.0	539.52 µg/L	539.52 ppb	20:24:43
2	B 249.677†	33315.4	28580.3	478.16 µg/L	478.16 ppb	20:24:23
2	Ba 233.527†	115639.2	111026.0	507.61 µg/L	507.61 ppb	20:24:23
2	Be 313.107†	1628518.8	1561746.1	508.52 µg/L	508.52 ppb	20:24:23
2	Cd 226.502†	72273.4	69375.2	478.78 µg/L	478.78 ppb	20:24:23
2	Co 228.616†	36323.3	34995.9	479.47 µg/L	479.47 ppb	20:24:23
2	Cr 267.716†	59881.6	57241.8	491.51 µg/L	491.51 ppb	20:24:23
2	Cu 324.752†	122554.8	115055.3	501.70 µg/L	501.70 ppb	20:24:23
2	Mn 257.610†	376730.4	361051.0	493.14 µg/L	493.14 ppb	20:24:23
2	Mo 202.031†	15922.5	15318.4	484.00 µg/L	484.00 ppb	20:24:43
2	Ni 231.604†	40247.2	38621.5	494.01 µg/L	494.01 ppb	20:24:23
2	P 214.914†	2196.8	2026.3	476.84 µg/L	476.84 ppb	20:24:43
2	Pb 220.353†	8465.1	8002.2	486.27 µg/L	486.27 ppb	20:24:43

2	S 181.975 Axial†	6356.7	5998.6	4864.1 µg/L	4864.1 ppb	20:24:43
2	Sb 206.836†	3895.9	3647.9	493.11 µg/L	493.11 ppb	20:24:43
2	Se 196.026†	1254.0	1191.2	473 µg/L	473 ppb	20:24:43
2	SiO2†	100322.8	94595.9	10318 µg/L	10318 ppb	20:24:23
2	Si 251.611†	304957.5	291653.6	4812.7 µg/L	4812.7 ppb	20:24:23
2	Sn 189.927†	7261.2	6958.5	496.35 µg/L	496.35 ppb	20:24:43
2	Ti 334.940†	502978.4	481515.0	490.34 µg/L	490.34 ppb	20:24:23
2	Tl 190.801†	3664.0	3632.6	495.07 µg/L	495.07 ppb	20:24:43
2	U 409.014†	7772.1	7929.4	520.33 µg/L	520.33 ppb	20:24:23
2	V 292.402†	93997.2	89673.2	503.63 µg/L	503.63 ppb	20:24:23
2	Zn 213.857†	79919.0	76145.3	475.42 µg/L	475.42 ppb	20:24:23
3	Sc RADIAL	156164.6	156164.6	107 %		20:23:42
3	Al 396.153Radial†	25652.1	23973.9	5210.9 µg/L	5210.9 ppb	20:23:42
3	Ca 317.933Radial†	91471.8	84757.8	4966.4 µg/L	4966.4 ppb	20:23:42
3	Fe 238.204 Radial†	79270.8	73873.1	4911.3 µg/L	4911.3 ppb	20:23:42
3	K 766.490 Radial†	13996.5	11608.5	4775.7 µg/L	4775.7 ppb	20:23:42
3	Mg 279.077 IEC†	13392.7	12313.2	5084.4 µg/L	5084.4 ppb	20:23:42
3	Na 589.592 Radial†	36448.6	32324.1	4941.8 µg/L	4941.8 ppb	20:23:42
3	Sr 421.552†	233466.4	218180.9	511.32 µg/L	511.32 ppb	20:23:40
3	Sc 361.383	1768031.6	1768031.6	105.69 %		20:24:46
3	Y 371.029	1071355.4	1071355.4	104.77 %		20:24:46
3	Ag 328.068†	126891.9	117088.2	481.41 µg/L	481.41 ppb	20:24:46
3	As 188.979†	1324.5	1267.4	536.73 µg/L	536.73 ppb	20:25:06
3	B 249.677†	33845.0	28665.8	479.59 µg/L	479.59 ppb	20:24:46
3	Ba 233.527†	117533.1	111375.8	509.20 µg/L	509.20 ppb	20:24:46
3	Be 313.107†	1650050.4	1561809.9	508.54 µg/L	508.54 ppb	20:24:46
3	Cd 226.502†	73684.3	69808.8	481.77 µg/L	481.77 ppb	20:24:46
3	Co 228.616†	36917.5	35105.1	480.97 µg/L	480.97 ppb	20:24:46
3	Cr 267.716†	60599.7	57174.5	490.94 µg/L	490.94 ppb	20:24:46
3	Cu 324.752†	124098.7	114987.7	501.39 µg/L	501.39 ppb	20:24:46
3	Mn 257.610†	382440.2	361755.2	494.10 µg/L	494.10 ppb	20:24:46
3	Mo 202.031†	16010.5	15203.1	480.36 µg/L	480.36 ppb	20:25:06
3	Ni 231.604†	40962.8	38796.7	496.25 µg/L	496.25 ppb	20:24:46
3	P 214.914†	2197.9	1999.9	470.55 µg/L	470.55 ppb	20:25:06
3	Pb 220.353†	8533.5	7961.3	483.80 µg/L	483.80 ppb	20:25:06
3	S 181.975 Axial†	6377.7	5939.3	4816.0 µg/L	4816.0 ppb	20:25:06
3	Sb 206.836†	3923.2	3625.2	489.99 µg/L	489.99 ppb	20:25:06
3	Se 196.026†	1265.0	1185.9	471 µg/L	471 ppb	20:25:06
3	SiO2†	101815.4	94757.0	10336 µg/L	10336 ppb	20:24:46
3	Si 251.611†	309448.3	292099.7	4820.2 µg/L	4820.2 ppb	20:24:46
3	Sn 189.927†	7309.3	6913.5	493.15 µg/L	493.15 ppb	20:25:06
3	Ti 334.940†	510228.3	482102.2	490.95 µg/L	490.95 ppb	20:24:46
3	Tl 190.801†	3713.6	3633.9	495.23 µg/L	495.23 ppb	20:25:06
3	U 409.014†	7645.0	7712.2	506.95 µg/L	506.95 ppb	20:24:46
3	V 292.402†	95349.8	89780.8	504.18 µg/L	504.18 ppb	20:24:46
3	Zn 213.857†	81367.2	76519.0	477.76 µg/L	477.76 ppb	20:24:46

Mean Data: 1202056867|959109|1

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1753000.6	104.80 %	0.779			0.74%
Sc RADIAL	156635.7	107 %	0.3			0.27%
Y 371.029	1062663.9	103.92 %	0.737			0.71%
Ag 328.068†	117332.1	482.40 µg/L	0.874	482.40 ppb	0.874	0.18%
Al 396.153Radial†	23935.8	5202.5 µg/L	8.00	5202.5 ppb	8.00	0.15%
As 188.979†	1273.2	539.18 µg/L	2.300	539.18 ppb	2.300	0.43%
B 249.677†	28590.0	478.32 µg/L	1.202	478.32 ppb	1.202	0.25%
Ba 233.527†	111234.1	508.56 µg/L	0.841	508.56 ppb	0.841	0.17%
Be 313.107†	1563304.6	509.03 µg/L	0.857	509.03 ppb	0.857	0.17%
Ca 317.933Radial†	84596.2	4957.0 µg/L	8.66	4957.0 ppb	8.66	0.17%
Cd 226.502†	69629.8	480.54 µg/L	1.565	480.54 ppb	1.565	0.33%
Co 228.616†	35111.2	481.05 µg/L	1.625	481.05 ppb	1.625	0.34%
Cr 267.716†	57262.7	491.70 µg/L	0.867	491.70 ppb	0.867	0.18%
Cu 324.752†	115176.7	502.21 µg/L	1.171	502.21 ppb	1.171	0.23%
Fe 238.204 Radial†	73931.7	4915.2 µg/L	5.18	4915.2 ppb	5.18	0.11%
K 766.490 Radial†	11690.6	4809.5 µg/L	34.41	4809.5 ppb	34.41	0.72%
Mg 279.077 IEC†	12365.1	5105.9 µg/L	18.85	5105.9 ppb	18.85	0.37%
Mn 257.610†	361616.0	493.91 µg/L	0.697	493.91 ppb	0.697	0.14%
Mo 202.031†	15289.6	483.09 µg/L	2.408	483.09 ppb	2.408	0.50%
Na 589.592 Radial†	32237.7	4928.5 µg/L	11.77	4928.5 ppb	11.77	0.24%

Ni 231.604†	38780.3	496.04 µg/L	1.934	496.04 ppb	1.934	0.39%
P 214.914†	2016.4	474.48 µg/L	3.422	474.48 ppb	3.422	0.72%
Pb 220.353†	8007.0	486.57 µg/L	2.935	486.57 ppb	2.935	0.60%
S 181.975 Axial†	5987.1	4854.7 µg/L	35.06	4854.7 ppb	35.06	0.72%
Sb 206.836†	3647.6	493.05 µg/L	3.022	493.05 ppb	3.022	0.61%
Se 196.026†	1194.1	475 µg/L	3.9	475 ppb	3.9	0.83%
SiO2†	94821.0	10343 µg/L	28.7	10343 ppb	28.7	0.28%
Si 251.611†	292063.3	4819.5 µg/L	6.49	4819.5 ppb	6.49	0.13%
Sn 189.927†	6952.8	495.94 µg/L	2.618	495.94 ppb	2.618	0.53%
Sr 421.552†	217589.1	509.93 µg/L	2.991	509.93 ppb	2.991	0.59%
Ti 334.940†	482150.5	490.99 µg/L	0.679	490.99 ppb	0.679	0.14%
Tl 190.801†	3650.6	497.48 µg/L	4.031	497.48 ppb	4.031	0.81%
U 409.014†	7719.8	507.40 µg/L	12.704	507.40 ppb	12.704	2.50%
V 292.402†	89739.8	503.98 µg/L	0.306	503.98 ppb	0.306	0.06%
Zn 213.857†	76323.8	476.53 µg/L	1.174	476.53 ppb	1.174	0.25%

Sequence No.: 33

Sample ID: 1202056868|959109|1

Analyst: HSC

Initial Sample Wt:

Dilution:

Autosampler Location: 327

Date Collected: 3/29/2010 20:28:12

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: 1202056868|959109|1

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	155950.8	155950.8	107 %		20:28:42
1	Al 396.153Radial†	22.6	53.0	11.525 µg/L	11.525 ppb	20:29:02
1	Ca 317.933Radial†	1181.2	487.8	28.583 µg/L	28.583 ppb	20:29:02
1	Fe 238.204 Radial†	335.6	200.4	13.323 µg/L	13.323 ppb	20:29:02
1	K 766.490 Radial†	1555.3	-1.4	-0.6101 µg/L	-0.6101 ppb	20:28:42
1	Mg 279.077 IEC†	178.1	-20.2	-8.3346 µg/L	-8.3346 ppb	20:29:02
1	Na 589.592 Radial†	2483.6	626.5	95.859 µg/L	95.859 ppb	20:28:42
1	Sr 421.552†	-192.1	98.4	0.2305 µg/L	0.2305 ppb	20:28:42
1	Sc 361.383	1760747.3	1760747.3	105.26 %		20:29:50
1	Y 371.029	1075796.3	1075796.3	105.20 %		20:29:50
1	Ag 328.068†	2884.0	-227.1	-0.9321 µg/L	-0.9321 ppb	20:29:52
1	As 188.979†	-10.8	4.0	1.6623 µg/L	1.6623 ppb	20:30:12
1	B 249.677†	4706.0	1115.2	18.723 µg/L	18.723 ppb	20:29:52
1	Ba 233.527†	-139.7	42.3	0.1929 µg/L	0.1929 ppb	20:30:12
1	Be 313.107†	-886.0	-181.6	-0.0594 µg/L	-0.0594 ppb	20:29:52
1	Cd 226.502†	-127.9	-27.1	-0.1886 µg/L	-0.1886 ppb	20:30:12
1	Co 228.616†	-191.5	-5.3	-0.0729 µg/L	-0.0729 ppb	20:30:12
1	Cr 267.716†	197.1	27.0	0.2327 µg/L	0.2327 ppb	20:30:12
1	Cu 324.752†	2755.3	192.8	0.8389 µg/L	0.8389 ppb	20:29:52
1	Mn 257.610†	429.0	327.6	0.4479 µg/L	0.4479 ppb	20:30:12
1	Mo 202.031†	-30.3	26.4	0.8330 µg/L	0.8330 ppb	20:30:12
1	Ni 231.604†	-62.3	-18.3	-0.2340 µg/L	-0.2340 ppb	20:30:12
1	P 214.914†	50.0	-32.1	-7.7135 µg/L	-7.7135 ppb	20:30:12
1	Pb 220.353†	119.6	1.2	0.0781 µg/L	0.0781 ppb	20:30:12
1	S 181.975 Axial†	125.4	24.3	19.694 µg/L	19.694 ppb	20:30:12
1	Sb 206.836†	83.8	-7.1	-0.9481 µg/L	-0.9481 ppb	20:30:12
1	Se 196.026†	1.0	-10.0	-3.96 µg/L	-3.96 ppb	20:30:12
1	SiO2†	36457.7	33063.3	3613.8 µg/L	3613.8 ppb	20:29:52
1	Si 251.611†	107867.9	101802.1	1683.3 µg/L	1683.3 ppb	20:29:52
1	Sn 189.927†	-5.9	-7.6	-0.5392 µg/L	-0.5392 ppb	20:30:12
1	Ti 334.940†	1128.2	435.5	0.4458 µg/L	0.4458 ppb	20:29:52
1	Tl 190.801†	-115.9	10.2	1.3758 µg/L	1.3758 ppb	20:30:12
1	U 409.014†	-521.9	-16.8	-1.0757 µg/L	-1.0757 ppb	20:29:52
1	V 292.402†	322.5	-125.5	-0.6895 µg/L	-0.6895 ppb	20:29:52
1	Zn 213.857†	711.3	211.4	1.3302 µg/L	1.3302 ppb	20:30:12
2	Sc RADIAL	157839.8	157839.8	108 %		20:29:04
2	Al 396.153Radial†	-1.9	30.1	6.5287 µg/L	6.5287 ppb	20:29:24
2	Ca 317.933Radial†	1125.6	423.3	24.801 µg/L	24.801 ppb	20:29:24
2	Fe 238.204 Radial†	332.6	193.9	12.890 µg/L	12.890 ppb	20:29:24
2	K 766.490 Radial†	1665.0	82.5	33.929 µg/L	33.929 ppb	20:29:04
2	Mg 279.077 IEC†	184.7	-16.1	-6.6459 µg/L	-6.6459 ppb	20:29:24
2	Na 589.592 Radial†	2619.9	724.6	110.84 µg/L	110.84 ppb	20:29:04
2	Sr 421.552†	-262.9	35.2	0.0823 µg/L	0.0823 ppb	20:29:04
2	Sc 361.383	1790165.6	1790165.6	107.02 %		20:30:14
2	Y 371.029	1093133.4	1093133.4	106.90 %		20:30:14
2	Ag 328.068†	3063.1	-104.8	-0.4306 µg/L	-0.4306 ppb	20:30:16
2	As 188.979†	-5.9	8.7	3.6605 µg/L	3.6605 ppb	20:30:36
2	B 249.677†	4663.8	1002.3	16.827 µg/L	16.827 ppb	20:30:16
2	Ba 233.527†	-155.2	30.0	0.1370 µg/L	0.1370 ppb	20:30:36
2	Be 313.107†	-476.7	214.6	0.0699 µg/L	0.0699 ppb	20:30:16
2	Cd 226.502†	-100.6	0.4	0.0012 µg/L	0.0012 ppb	20:30:36
2	Co 228.616†	-194.5	-5.1	-0.0705 µg/L	-0.0705 ppb	20:30:36
2	Cr 267.716†	200.1	26.8	0.2302 µg/L	0.2302 ppb	20:30:36
2	Cu 324.752†	2797.6	189.3	0.8243 µg/L	0.8243 ppb	20:30:16
2	Mn 257.610†	414.4	307.2	0.4201 µg/L	0.4201 ppb	20:30:36
2	Mo 202.031†	-32.6	24.8	0.7823 µg/L	0.7823 ppb	20:30:36
2	Ni 231.604†	-56.6	-12.0	-0.1531 µg/L	-0.1531 ppb	20:30:36
2	P 214.914†	72.1	-12.2	-2.9498 µg/L	-2.9498 ppb	20:30:36
2	Pb 220.353†	73.7	-43.5	-2.6348 µg/L	-2.6348 ppb	20:30:36

2	S 181.975 Axial†	120.2	17.5	14.209 µg/L	14.209 ppb	20:30:36
2	Sb 206.836†	86.2	-6.1	-0.8153 µg/L	-0.8153 ppb	20:30:36
2	Se 196.026†	-2.6	-13.4	-5.28 µg/L	-5.28 ppb	20:30:36
2	SiO2†	37358.0	33335.4	3643.6 µg/L	3643.6 ppb	20:30:16
2	Si 251.611†	110459.1	102539.3	1695.5 µg/L	1695.5 ppb	20:30:16
2	Sn 189.927†	-6.4	-8.0	-0.5675 µg/L	-0.5675 ppb	20:30:36
2	Ti 334.940†	1109.1	400.0	0.4090 µg/L	0.4090 ppb	20:30:16
2	Tl 190.801†	-125.2	3.3	0.4435 µg/L	0.4435 ppb	20:30:36
2	U 409.014†	-512.9	-0.2	-0.0331 µg/L	-0.0331 ppb	20:30:16
2	V 292.402†	390.0	-67.4	-0.3674 µg/L	-0.3674 ppb	20:30:16
2	Zn 213.857†	717.3	205.9	1.2953 µg/L	1.2953 ppb	20:30:36
3	Sc RADIAL	155985.4	155985.4	107 %		20:29:26
3	Al 396.153Radial†	10.1	41.3	8.9851 µg/L	8.9851 ppb	20:29:46
3	Ca 317.933Radial†	1140.2	449.2	26.324 µg/L	26.324 ppb	20:29:46
3	Fe 238.204 Radial†	310.8	177.1	11.776 µg/L	11.776 ppb	20:29:46
3	K 766.490 Radial†	1637.4	75.0	30.843 µg/L	30.843 ppb	20:29:26
3	Mg 279.077 IEC†	175.5	-22.7	-9.3351 µg/L	-9.3351 ppb	20:29:46
3	Na 589.592 Radial†	2562.9	700.1	107.09 µg/L	107.09 ppb	20:29:26
3	Sr 421.552†	-258.0	36.9	0.0863 µg/L	0.0863 ppb	20:29:26
3	Sc 361.383	1808598.8	1808598.8	108.12 %		20:30:38
3	Y 371.029	1103697.9	1103697.9	107.93 %		20:30:38
3	Ag 328.068†	3080.6	-117.8	-0.4590 µg/L	-0.4590 ppb	20:30:40
3	As 188.979†	-19.0	-3.3	-1.3666 µg/L	-1.3666 ppb	20:31:00
3	B 249.677†	4718.9	1008.8	16.936 µg/L	16.936 ppb	20:30:40
3	Ba 233.527†	-152.9	33.6	0.1530 µg/L	0.1530 ppb	20:31:00
3	Be 313.107†	-540.5	160.2	0.0593 µg/L	0.0593 ppb	20:30:40
3	Cd 226.502†	-106.7	-4.3	-0.0307 µg/L	-0.0307 ppb	20:31:00
3	Co 228.616†	-176.5	13.3	0.1820 µg/L	0.1820 ppb	20:31:00
3	Cr 267.716†	239.4	61.2	0.5073 µg/L	0.5073 ppb	20:31:00
3	Cu 324.752†	2700.0	72.3	0.3355 µg/L	0.3355 ppb	20:30:40
3	Mn 257.610†	418.0	306.6	0.4193 µg/L	0.4193 ppb	20:31:00
3	Mo 202.031†	-39.8	18.4	0.5817 µg/L	0.5817 ppb	20:31:00
3	Ni 231.604†	-55.6	-10.6	-0.1350 µg/L	-0.1350 ppb	20:31:00
3	P 214.914†	57.1	-26.7	-6.4170 µg/L	-6.4170 ppb	20:31:00
3	Pb 220.353†	84.1	-34.6	-2.1127 µg/L	-2.1127 ppb	20:31:00
3	S 181.975 Axial†	119.9	16.1	13.026 µg/L	13.026 ppb	20:31:00
3	Sb 206.836†	83.5	-9.4	-1.2705 µg/L	-1.2705 ppb	20:31:00
3	Se 196.026†	34.2	20.7	8.23 µg/L	8.23 ppb	20:31:00
3	SiO2†	37261.4	32890.3	3594.9 µg/L	3594.9 ppb	20:30:40
3	Si 251.611†	110421.6	101452.6	1677.5 µg/L	1677.5 ppb	20:30:40
3	Sn 189.927†	1.0	-1.1	-0.0762 µg/L	-0.0762 ppb	20:31:00
3	Ti 334.940†	1055.6	340.0	0.3383 µg/L	0.3383 ppb	20:30:40
3	Tl 190.801†	-133.9	-3.6	-0.4826 µg/L	-0.4826 ppb	20:31:00
3	U 409.014†	-106.3	380.8	23.486 µg/L	23.486 ppb	20:30:40
3	V 292.402†	316.3	-139.2	-0.7505 µg/L	-0.7505 ppb	20:30:40
3	Zn 213.857†	713.0	195.0	1.2271 µg/L	1.2271 ppb	20:31:00

Mean Data: 1202056868|959109|1

Analyte	Mean Corrected Intensity	Conc. Units	Calib. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1786503.9	106.80 %		1.443			1.35%
Sc RADIAL	156592.0	107 %		0.7			0.69%
Y 371.029	1090875.9	106.68 %		1.378			1.29%
Ag 328.068†	-149.9	-0.6072 µg/L		0.28174	-0.6072 ppb	0.28174	46.40%
Al 396.153Radial†	41.4	9.0128 µg/L		2.49807	9.0128 ppb	2.49807	27.72%
As 188.979†	3.1	1.3187 µg/L		2.53109	1.3187 ppb	2.53109	191.93%
B 249.677†	1042.1	17.495 µg/L		1.0647	17.495 ppb	1.0647	6.09%
Ba 233.527†	35.3	0.1610 µg/L		0.02882	0.1610 ppb	0.02882	17.90%
Be 313.107†	64.4	0.0232 µg/L		0.07179	0.0232 ppb	0.07179	309.06%
Ca 317.933Radial†	453.4	26.569 µg/L		1.9028	26.569 ppb	1.9028	7.16%
Cd 226.502†	-10.3	-0.0727 µg/L		0.10161	-0.0727 ppb	0.10161	139.72%
Co 228.616†	1.0	0.0129 µg/L		0.14648	0.0129 ppb	0.14648	>999.9%
Cr 267.716†	38.3	0.3234 µg/L		0.15925	0.3234 ppb	0.15925	49.24%
Cu 324.752†	151.5	0.6662 µg/L		0.28654	0.6662 ppb	0.28654	43.01%
Fe 238.204 Radial†	190.5	12.663 µg/L		0.7981	12.663 ppb	0.7981	6.30%
K 766.490 Radial†	52.0	21.387 µg/L		19.1126	21.387 ppb	19.1126	89.36%
Mg 279.077 IEC†	-19.7	-8.1052 µg/L		1.35921	-8.1052 ppb	1.35921	16.77%
Mn 257.610†	313.8	0.4291 µg/L		0.01628	0.4291 ppb	0.01628	3.79%
Mo 202.031†	23.2	0.7323 µg/L		0.13290	0.7323 ppb	0.13290	18.15%
Na 589.592 Radial†	683.7	104.60 µg/L		7.797	104.60 ppb	7.797	7.45%

Ni 231.604†	-13.6	-0.1740 µg/L	0.05275	-0.1740 ppb	0.05275	30.31%
P 214.914†	-23.7	-5.6934 µg/L	2.46290	-5.6934 ppb	2.46290	43.26%
Pb 220.353†	-25.6	-1.5564 µg/L	1.43946	-1.5564 ppb	1.43946	92.48%
S 181.975 Axial†	19.3	15.643 µg/L	3.5579	15.643 ppb	3.5579	22.74%
Sb 206.836†	-7.5	-1.0113 µg/L	0.23412	-1.0113 ppb	0.23412	23.15%
Se 196.026†	-0.9	-0.337 µg/L	7.4460	-0.337 ppb	7.4460	>999.9%
SiO2†	33096.3	3617.4 µg/L	24.53	3617.4 ppb	24.53	0.68%
Si 251.611†	101931.3	1685.4 µg/L	9.17	1685.4 ppb	9.17	0.54%
Sn 189.927†	-5.6	-0.3943 µg/L	0.27586	-0.3943 ppb	0.27586	69.96%
Sr 421.552†	56.8	0.1330 µg/L	0.08445	0.1330 ppb	0.08445	63.48%
Ti 334.940†	391.8	0.3977 µg/L	0.05461	0.3977 ppb	0.05461	13.73%
Tl 190.801†	3.3	0.4456 µg/L	0.92922	0.4456 ppb	0.92922	208.53%
U 409.014†	121.3	7.4590 µg/L	13.88940	7.4590 ppb	13.88940	186.21%
V 292.402†	-110.7	-0.6025 µg/L	0.20584	-0.6025 ppb	0.20584	34.17%
Zn 213.857†	204.1	1.2842 µg/L	0.05246	1.2842 ppb	0.05246	4.08%

Sequence No.: 34

Sample ID: 1202056869|959109|1

Analyst: HSC

Initial Sample Wt:

Dilution:

Autosampler Location: 328

Date Collected: 3/29/2010 20:31:08

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: 1202056869|959109|1

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	155173.2	155173.2	106 %		20:31:40
1	Al 396.153Radial†	25444.3	23931.7	5202.0 µg/L	5202.0 ppb	20:31:40
1	Ca 317.933Radial†	90784.5	84657.6	4960.6 µg/L	4960.6 ppb	20:31:40
1	Fe 238.204 Radial†	78628.2	73742.1	4902.6 µg/L	4902.6 ppb	20:31:40
1	K 766.490 Radial†	14184.1	11868.1	4882.5 µg/L	4882.5 ppb	20:31:40
1	Mg 279.077 IEC†	13252.1	12261.1	5062.7 µg/L	5062.7 ppb	20:31:40
1	Na 589.592 Radial†	37067.5	33122.8	5063.9 µg/L	5063.9 ppb	20:31:40
1	Sr 421.552†	227630.8	214091.5	501.74 µg/L	501.74 ppb	20:31:38
1	Sc 361.383	1761502.0	1761502.0	105.30 %		20:31:53
1	Y 371.029	1067002.4	1067002.4	104.34 %		20:31:53
1	Ag 328.068†	125554.4	116263.1	477.99 µg/L	477.99 ppb	20:31:53
1	As 188.979†	1318.7	1266.5	536.32 µg/L	536.32 ppb	20:32:13
1	B 249.677†	34862.3	29750.6	497.82 µg/L	497.82 ppb	20:31:53
1	Ba 233.527†	116159.4	110483.5	505.12 µg/L	505.12 ppb	20:31:53
1	Be 313.107†	1635678.5	1553948.8	505.97 µg/L	505.97 ppb	20:31:53
1	Cd 226.502†	72484.2	68927.6	475.69 µg/L	475.69 ppb	20:31:53
1	Co 228.616†	36563.5	34898.4	478.13 µg/L	478.13 ppb	20:31:53
1	Cr 267.716†	60102.4	56914.7	488.72 µg/L	488.72 ppb	20:31:53
1	Cu 324.752†	122861.2	114247.7	498.16 µg/L	498.16 ppb	20:31:53
1	Mn 257.610†	377210.3	358130.0	489.15 µg/L	489.15 ppb	20:31:53
1	Mo 202.031†	15727.8	14990.8	473.65 µg/L	473.65 ppb	20:32:13
1	Ni 231.604†	40361.4	38369.3	490.79 µg/L	490.79 ppb	20:31:53
1	P 214.914†	2170.4	1981.5	466.20 µg/L	466.20 ppb	20:32:13
1	Pb 220.353†	8431.7	7894.5	479.75 µg/L	479.75 ppb	20:32:13
1	S 181.975 Axial†	6297.0	5885.0	4771.9 µg/L	4771.9 ppb	20:32:13
1	Sb 206.836†	3844.4	3564.1	481.68 µg/L	481.68 ppb	20:32:13
1	Se 196.026†	1245.3	1171.7	466 µg/L	466 ppb	20:32:13
1	SiO2†	137768.6	129256.3	14107 µg/L	14107 ppb	20:31:53
1	Si 251.611†	420279.6	398433.6	6578.5 µg/L	6578.5 ppb	20:31:53
1	Sn 189.927†	7190.0	6825.8	486.90 µg/L	486.90 ppb	20:32:13
1	Ti 334.940†	504113.7	478085.0	486.86 µg/L	486.86 ppb	20:31:53
1	Tl 190.801†	3635.9	3573.0	487.00 µg/L	487.00 ppb	20:32:13
1	U 409.014†	7293.2	7404.9	487.70 µg/L	487.70 ppb	20:31:53
1	V 292.402†	94226.2	89048.2	500.03 µg/L	500.03 ppb	20:31:53
1	Zn 213.857†	79872.0	75384.4	470.66 µg/L	470.66 ppb	20:31:53
2	Sc RADIAL	156899.2	156899.2	108 %		20:31:44
2	Al 396.153Radial†	25617.4	23829.6	5179.6 µg/L	5179.6 ppb	20:31:44
2	Ca 317.933Radial†	90933.3	83857.8	4913.7 µg/L	4913.7 ppb	20:31:44
2	Fe 238.204 Radial†	78908.7	73190.4	4865.9 µg/L	4865.9 ppb	20:31:44
2	K 766.490 Radial†	14241.7	11775.1	4844.3 µg/L	4844.3 ppb	20:31:44
2	Mg 279.077 IEC†	13381.3	12244.2	5055.9 µg/L	5055.9 ppb	20:31:44
2	Na 589.592 Radial†	37010.1	32686.4	4997.1 µg/L	4997.1 ppb	20:31:44
2	Sr 421.552†	231155.0	215013.4	503.90 µg/L	503.90 ppb	20:31:42
2	Sc 361.383	1755110.4	1755110.4	104.92 %		20:32:16
2	Y 371.029	1062740.2	1062740.2	103.93 %		20:32:16
2	Ag 328.068†	124228.5	115433.7	474.58 µg/L	474.58 ppb	20:32:16
2	As 188.979†	1305.9	1258.9	533.08 µg/L	533.08 ppb	20:32:36
2	B 249.677†	34397.7	29428.3	492.43 µg/L	492.43 ppb	20:32:16
2	Ba 233.527†	114769.6	109560.5	500.91 µg/L	500.91 ppb	20:32:16
2	Be 313.107†	1612974.7	1537966.8	500.78 µg/L	500.78 ppb	20:32:16
2	Cd 226.502†	71427.6	68171.1	470.46 µg/L	470.46 ppb	20:32:16
2	Co 228.616†	35967.1	34456.4	472.08 µg/L	472.08 ppb	20:32:16
2	Cr 267.716†	59284.8	56343.4	483.81 µg/L	483.81 ppb	20:32:16
2	Cu 324.752†	121545.6	113418.8	494.55 µg/L	494.55 ppb	20:32:16
2	Mn 257.610†	372734.9	355169.1	485.10 µg/L	485.10 ppb	20:32:16
2	Mo 202.031†	15763.3	15079.0	476.44 µg/L	476.44 ppb	20:32:36
2	Ni 231.604†	39797.0	37971.0	485.69 µg/L	485.69 ppb	20:32:16
2	P 214.914†	2160.1	1979.2	465.69 µg/L	465.69 ppb	20:32:36
2	Pb 220.353†	8415.6	7908.4	480.58 µg/L	480.58 ppb	20:32:36

2	S 181.975 Axial†	6313.6	5922.6	4802.4 µg/L	4802.4 ppb	20:32:36
2	Sb 206.836†	3883.0	3614.2	488.54 µg/L	488.54 ppb	20:32:36
2	Se 196.026†	1227.9	1159.4	461 µg/L	461 ppb	20:32:36
2	SiO2†	136216.4	128253.3	13998 µg/L	13998 ppb	20:32:16
2	Si 251.611†	414914.9	394774.0	6518.0 µg/L	6518.0 ppb	20:32:16
2	Sn 189.927†	7187.1	6848.0	488.46 µg/L	488.46 ppb	20:32:36
2	Ti 334.940†	497936.6	473941.0	482.63 µg/L	482.63 ppb	20:32:16
2	Tl 190.801†	3627.1	3577.2	487.50 µg/L	487.50 ppb	20:32:36
2	U 409.014†	7469.7	7598.4	499.35 µg/L	499.35 ppb	20:32:16
2	V 292.402†	92923.6	88132.5	494.98 µg/L	494.98 ppb	20:32:16
2	Zn 213.857†	78672.7	74517.6	465.24 µg/L	465.24 ppb	20:32:16
3	Sc RADIAL	154673.6	154673.6	106 %		20:31:48
3	Al 396.153Radial†	25364.6	23933.8	5202.4 µg/L	5202.4 ppb	20:31:48
3	Ca 317.933Radial†	89849.9	84052.4	4925.1 µg/L	4925.1 ppb	20:31:48
3	Fe 238.204 Radial†	77863.0	73259.7	4870.6 µg/L	4870.6 ppb	20:31:48
3	K 766.490 Radial†	14036.5	11772.1	4843.0 µg/L	4843.0 ppb	20:31:48
3	Mg 279.077 IEC†	13183.2	12236.3	5052.6 µg/L	5052.6 ppb	20:31:48
3	Na 589.592 Radial†	36715.1	32903.2	5030.3 µg/L	5030.3 ppb	20:31:48
3	Sr 421.552†	229351.6	216403.8	507.15 µg/L	507.15 ppb	20:31:46
3	Sc 361.383	1749797.0	1749797.0	104.60 %		20:32:39
3	Y 371.029	1059994.9	1059994.9	103.66 %		20:32:39
3	Ag 328.068†	123685.5	115274.1	473.97 µg/L	473.97 ppb	20:32:39
3	As 188.979†	1305.1	1261.8	534.33 µg/L	534.33 ppb	20:32:59
3	B 249.677†	34390.8	29521.3	493.98 µg/L	493.98 ppb	20:32:39
3	Ba 233.527†	114376.9	109517.3	500.71 µg/L	500.71 ppb	20:32:39
3	Be 313.107†	1610890.2	1540642.2	501.65 µg/L	501.65 ppb	20:32:39
3	Cd 226.502†	71427.6	68377.9	471.89 µg/L	471.89 ppb	20:32:39
3	Co 228.616†	35913.1	34508.9	472.80 µg/L	472.80 ppb	20:32:39
3	Cr 267.716†	59176.2	56411.2	484.38 µg/L	484.38 ppb	20:32:39
3	Cu 324.752†	121092.5	113337.3	494.21 µg/L	494.21 ppb	20:32:39
3	Mn 257.610†	371785.9	355340.7	485.34 µg/L	485.34 ppb	20:32:39
3	Mo 202.031†	15659.5	15025.5	474.75 µg/L	474.75 ppb	20:32:59
3	Ni 231.604†	39667.9	37962.7	485.59 µg/L	485.59 ppb	20:32:39
3	P 214.914†	2173.7	1998.5	470.31 µg/L	470.31 ppb	20:32:59
3	Pb 220.353†	8340.4	7860.8	477.69 µg/L	477.69 ppb	20:32:59
3	S 181.975 Axial†	6267.6	5896.9	4781.6 µg/L	4781.6 ppb	20:32:59
3	Sb 206.836†	3843.7	3587.8	484.95 µg/L	484.95 ppb	20:32:59
3	Se 196.026†	1216.1	1151.7	458 µg/L	458 ppb	20:32:59
3	SiO2†	135757.7	128209.1	13993 µg/L	13993 ppb	20:32:39
3	Si 251.611†	413665.6	394780.5	6518.1 µg/L	6518.1 ppb	20:32:39
3	Sn 189.927†	7131.3	6815.4	486.15 µg/L	486.15 ppb	20:32:59
3	Ti 334.940†	496950.9	474439.8	483.14 µg/L	483.14 ppb	20:32:39
3	Tl 190.801†	3586.0	3548.5	483.66 µg/L	483.66 ppb	20:32:59
3	U 409.014†	7658.5	7800.5	511.91 µg/L	511.91 ppb	20:32:39
3	V 292.402†	92890.1	88369.4	496.28 µg/L	496.28 ppb	20:32:39
3	Zn 213.857†	78647.3	74721.0	466.52 µg/L	466.52 ppb	20:32:39

Mean Data: 1202056869|959109|1

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1755469.8	104.94 %	0.350			0.33%
Sc RADIAL	155582.0	107 %	0.8			0.75%
Y 371.029	1063245.8	103.98 %	0.345			0.33%
Ag 328.068†	115657.0	475.52 µg/L	2.168	475.52 ppb	2.168	0.46%
Al 396.153Radial†	23898.4	5194.7 µg/L	13.07	5194.7 ppb	13.07	0.25%
As 188.979†	1262.4	534.58 µg/L	1.631	534.58 ppb	1.631	0.31%
B 249.677†	29566.8	494.74 µg/L	2.773	494.74 ppb	2.773	0.56%
Ba 233.527†	109853.8	502.25 µg/L	2.494	502.25 ppb	2.494	0.50%
Be 313.107†	1544185.9	502.80 µg/L	2.784	502.80 ppb	2.784	0.55%
Ca 317.933Radial†	84189.3	4933.1 µg/L	24.44	4933.1 ppb	24.44	0.50%
Cd 226.502†	68492.2	472.68 µg/L	2.699	472.68 ppb	2.699	0.57%
Co 228.616†	34621.2	474.34 µg/L	3.308	474.34 ppb	3.308	0.70%
Cr 267.716†	56556.5	485.64 µg/L	2.690	485.64 ppb	2.690	0.55%
Cu 324.752†	113668.0	495.64 µg/L	2.186	495.64 ppb	2.186	0.44%
Fe 238.204 Radial†	73397.4	4879.7 µg/L	19.98	4879.7 ppb	19.98	0.41%
K 766.490 Radial†	11805.1	4856.6 µg/L	22.46	4856.6 ppb	22.46	0.46%
Mg 279.077 IEC†	12247.2	5057.1 µg/L	5.18	5057.1 ppb	5.18	0.10%
Mn 257.610†	356213.3	486.53 µg/L	2.271	486.53 ppb	2.271	0.47%
Mo 202.031†	15031.8	474.95 µg/L	1.401	474.95 ppb	1.401	0.30%
Na 589.592 Radial†	32904.1	5030.4 µg/L	33.36	5030.4 ppb	33.36	0.66%

Ni 231.604†	38101.0	487.36 µg/L	2.973	487.36 ppb	2.973	0.61%
P 214.914†	1986.4	467.40 µg/L	2.533	467.40 ppb	2.533	0.54%
Pb 220.353†	7887.9	479.34 µg/L	1.490	479.34 ppb	1.490	0.31%
S 181.975 Axial†	5901.5	4785.3 µg/L	15.57	4785.3 ppb	15.57	0.33%
Sb 206.836†	3588.7	485.06 µg/L	3.434	485.06 ppb	3.434	0.71%
Se 196.026†	1160.9	461 µg/L	4.0	461 ppb	4.0	0.87%
SiO2†	128572.9	14033 µg/L	64.8	14033 ppb	64.8	0.46%
Si 251.611†	395996.0	6538.2 µg/L	34.92	6538.2 ppb	34.92	0.53%
Sn 189.927†	6829.7	487.17 µg/L	1.180	487.17 ppb	1.180	0.24%
Sr 421.552†	215169.6	504.26 µg/L	2.728	504.26 ppb	2.728	0.54%
Ti 334.940†	475488.6	484.21 µg/L	2.310	484.21 ppb	2.310	0.48%
Tl 190.801†	3566.2	486.05 µg/L	2.089	486.05 ppb	2.089	0.43%
U 409.014†	7601.2	499.65 µg/L	12.109	499.65 ppb	12.109	2.42%
V 292.402†	88516.7	497.10 µg/L	2.623	497.10 ppb	2.623	0.53%
Zn 213.857†	74874.3	467.47 µg/L	2.831	467.47 ppb	2.831	0.61%

Sequence No.: 35

Sample ID: 1202056870|959109|5

Analyst: HSC

Initial Sample Wt:

Dilution:

Autosampler Location: 329

Date Collected: 3/29/2010 20:33:07

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: 1202056870|959109|5

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	157991.8	157991.8	108 %		20:33:37
1	Al 396.153Radial†	-48.0	-12.4	-2.7357 µg/L	-2.7357 ppb	20:33:57
1	Ca 317.933Radial†	854.0	171.7	10.059 µg/L	10.059 ppb	20:33:57
1	Fe 238.204 Radial†	231.5	100.2	6.6647 µg/L	6.6647 ppb	20:33:57
1	K 766.490 Radial†	1603.1	23.9	9.8525 µg/L	9.8525 ppb	20:33:37
1	Mg 279.077 IEC†	172.2	-27.8	-11.444 µg/L	-11.444 ppb	20:33:57
1	Na 589.592 Radial†	1691.9	-133.8	-20.487 µg/L	-20.487 ppb	20:33:37
1	Sr 421.552†	-116.8	170.2	0.3988 µg/L	0.3988 ppb	20:33:37
1	Sc 361.383	1767023.5	1767023.5	105.63 %		20:34:45
1	Y 371.029	1081596.6	1081596.6	105.77 %		20:34:45
1	Ag 328.068†	3032.9	-95.9	-0.3816 µg/L	-0.3816 ppb	20:34:47
1	As 188.979†	-29.7	-13.9	-5.7879 µg/L	-5.7879 ppb	20:35:07
1	B 249.677†	3478.3	-62.9	-1.0574 µg/L	-1.0574 ppb	20:35:07
1	Ba 233.527†	-166.2	17.7	0.0806 µg/L	0.0806 ppb	20:35:07
1	Be 313.107†	-429.4	253.6	0.0870 µg/L	0.0870 ppb	20:34:47
1	Cd 226.502†	-108.6	-8.4	-0.0587 µg/L	-0.0587 ppb	20:35:07
1	Co 228.616†	-174.4	11.5	0.1572 µg/L	0.1572 ppb	20:35:07
1	Cr 267.716†	162.4	-6.5	-0.0677 µg/L	-0.0677 ppb	20:35:07
1	Cu 324.752†	2781.7	208.5	0.9194 µg/L	0.9194 ppb	20:34:47
1	Mn 257.610†	238.1	145.4	0.1992 µg/L	0.1992 ppb	20:35:07
1	Mo 202.031†	-40.1	17.2	0.5430 µg/L	0.5430 ppb	20:35:07
1	Ni 231.604†	-43.1	0.1	0.0010 µg/L	0.0010 ppb	20:35:07
1	P 214.914†	39.0	-42.7	-10.248 µg/L	-10.248 ppb	20:35:07
1	Pb 220.353†	86.2	-30.9	-1.8797 µg/L	-1.8797 ppb	20:35:07
1	S 181.975 Axial†	93.6	-6.2	-5.0374 µg/L	-5.0374 ppb	20:35:07
1	Sb 206.836†	75.3	-15.4	-2.0713 µg/L	-2.0713 ppb	20:35:07
1	Se 196.026†	16.5	4.7	1.89 µg/L	1.89 ppb	20:35:07
1	SiO2†	8989.0	6936.7	758.18 µg/L	758.18 ppb	20:34:47
1	Si 251.611†	22783.7	20892.1	345.45 µg/L	345.45 ppb	20:34:47
1	Sn 189.927†	-8.1	-9.7	-0.6886 µg/L	-0.6886 ppb	20:35:07
1	Ti 334.940†	944.5	257.7	0.2580 µg/L	0.2580 ppb	20:34:47
1	Tl 190.801†	-107.1	18.9	2.5327 µg/L	2.5327 ppb	20:35:07
1	U 409.014†	-252.8	239.8	14.768 µg/L	14.768 ppb	20:34:47
1	V 292.402†	289.1	-158.2	-0.8633 µg/L	-0.8633 ppb	20:34:47
1	Zn 213.857†	611.9	114.8	0.7213 µg/L	0.7213 ppb	20:35:07
2	Sc RADIAL	157710.0	157710.0	108 %		20:33:59
2	Al 396.153Radial†	-49.6	-14.0	-3.0882 µg/L	-3.0882 ppb	20:34:19
2	Ca 317.933Radial†	860.5	179.1	10.493 µg/L	10.493 ppb	20:34:19
2	Fe 238.204 Radial†	244.9	113.0	7.5133 µg/L	7.5133 ppb	20:34:19
2	K 766.490 Radial†	1460.2	-105.5	-43.423 µg/L	-43.423 ppb	20:33:59
2	Mg 279.077 IEC†	176.8	-23.3	-9.5962 µg/L	-9.5962 ppb	20:34:19
2	Na 589.592 Radial†	1698.8	-124.7	-19.037 µg/L	-19.037 ppb	20:33:59
2	Sr 421.552†	-173.6	117.5	0.2754 µg/L	0.2754 ppb	20:33:59
2	Sc 361.383	1789131.0	1789131.0	106.96 %		20:35:09
2	Y 371.029	1094714.6	1094714.6	107.05 %		20:35:09
2	Ag 328.068†	3142.7	-28.7	-0.1196 µg/L	-0.1196 ppb	20:35:11
2	As 188.979†	-9.5	5.4	2.2489 µg/L	2.2489 ppb	20:35:31
2	B 249.677†	3452.5	-127.7	-2.1455 µg/L	-2.1455 ppb	20:35:31
2	Ba 233.527†	-189.5	-2.1	-0.0103 µg/L	-0.0103 ppb	20:35:31
2	Be 313.107†	-451.5	238.0	0.0807 µg/L	0.0807 ppb	20:35:11
2	Cd 226.502†	-74.9	24.4	0.1679 µg/L	0.1679 ppb	20:35:31
2	Co 228.616†	-163.0	24.2	0.3314 µg/L	0.3314 ppb	20:35:31
2	Cr 267.716†	159.7	-10.9	-0.1026 µg/L	-0.1026 ppb	20:35:31
2	Cu 324.752†	2679.7	80.5	0.3599 µg/L	0.3599 ppb	20:35:11
2	Mn 257.610†	248.2	152.0	0.2081 µg/L	0.2081 ppb	20:35:31
2	Mo 202.031†	-31.2	26.0	0.8209 µg/L	0.8209 ppb	20:35:31
2	Ni 231.604†	-35.3	7.9	0.1009 µg/L	0.1009 ppb	20:35:31
2	P 214.914†	53.0	-30.0	-7.2103 µg/L	-7.2103 ppb	20:35:31
2	Pb 220.353†	94.9	-23.7	-1.4404 µg/L	-1.4404 ppb	20:35:31

2	S 181.975 Axial†	100.8	-0.6	-0.5005 µg/L	-0.5005 ppb	20:35:31
2	Sb 206.836†	95.7	2.9	0.3965 µg/L	0.3965 ppb	20:35:31
2	Se 196.026†	20.0	7.8	3.10 µg/L	3.10 ppb	20:35:31
2	SiO2†	8961.6	6805.9	743.88 µg/L	743.88 ppb	20:35:11
2	Si 251.611†	23204.1	21018.6	347.53 µg/L	347.53 ppb	20:35:11
2	Sn 189.927†	-8.6	-10.0	-0.7125 µg/L	-0.7125 ppb	20:35:31
2	Ti 334.940†	805.3	116.5	0.1155 µg/L	0.1155 ppb	20:35:11
2	Tl 190.801†	-109.4	18.0	2.4093 µg/L	2.4093 ppb	20:35:31
2	U 409.014†	-326.2	174.1	10.682 µg/L	10.682 ppb	20:35:11
2	V 292.402†	206.2	-239.1	-1.3121 µg/L	-1.3121 ppb	20:35:11
2	Zn 213.857†	662.0	154.5	0.9709 µg/L	0.9709 ppb	20:35:31
3	Sc RADIAL	156329.8	156329.8	107 %		20:34:21
3	Al 396.153Radial†	-21.1	12.2	2.6224 µg/L	2.6224 ppb	20:34:41
3	Ca 317.933Radial†	855.0	181.0	10.603 µg/L	10.603 ppb	20:34:41
3	Fe 238.204 Radial†	238.4	109.0	7.2477 µg/L	7.2477 ppb	20:34:41
3	K 766.490 Radial†	1444.2	-108.5	-44.654 µg/L	-44.654 ppb	20:34:21
3	Mg 279.077 IEC†	187.2	-12.1	-4.9847 µg/L	-4.9847 ppb	20:34:41
3	Na 589.592 Radial†	1681.5	-127.0	-19.393 µg/L	-19.393 ppb	20:34:21
3	Sr 421.552†	-337.2	-36.4	-0.0854 µg/L	-0.0854 ppb	20:34:21
3	Sc 361.383	1763307.4	1763307.4	105.41 %		20:35:33
3	Y 371.029	1079799.3	1079799.3	105.60 %		20:35:33
3	Ag 328.068†	3157.2	28.0	0.1284 µg/L	0.1284 ppb	20:35:35
3	As 188.979†	-16.8	-1.7	-0.7072 µg/L	-0.7072 ppb	20:35:55
3	B 249.677†	3408.0	-122.6	-2.0595 µg/L	-2.0595 ppb	20:35:55
3	Ba 233.527†	-156.9	26.2	0.1191 µg/L	0.1191 ppb	20:35:55
3	Be 313.107†	-635.8	56.9	0.0267 µg/L	0.0267 ppb	20:35:35
3	Cd 226.502†	-93.6	5.6	0.0379 µg/L	0.0379 ppb	20:35:55
3	Co 228.616†	-166.9	18.2	0.2495 µg/L	0.2495 ppb	20:35:55
3	Cr 267.716†	167.0	-1.8	-0.0372 µg/L	-0.0372 ppb	20:35:55
3	Cu 324.752†	2620.4	61.0	0.2883 µg/L	0.2883 ppb	20:35:35
3	Mn 257.610†	281.4	187.0	0.2557 µg/L	0.2557 ppb	20:35:55
3	Mo 202.031†	-22.1	34.3	1.0814 µg/L	1.0814 ppb	20:35:55
3	Ni 231.604†	-42.2	0.9	0.0114 µg/L	0.0114 ppb	20:35:55
3	P 214.914†	47.8	-34.2	-8.2133 µg/L	-8.2133 ppb	20:35:55
3	Pb 220.353†	93.6	-23.6	-1.4459 µg/L	-1.4459 ppb	20:35:55
3	S 181.975 Axial†	96.2	-3.5	-2.8511 µg/L	-2.8511 ppb	20:35:55
3	Sb 206.836†	70.1	-20.2	-2.7063 µg/L	-2.7063 ppb	20:35:55
3	Se 196.026†	12.6	1.0	0.428 µg/L	0.428 ppb	20:35:55
3	SiO2†	8819.2	6793.6	742.51 µg/L	742.51 ppb	20:35:35
3	Si 251.611†	22832.6	20983.9	346.95 µg/L	346.95 ppb	20:35:35
3	Sn 189.927†	9.7	7.2	0.5106 µg/L	0.5106 ppb	20:35:55
3	Ti 334.940†	1035.3	345.8	0.3423 µg/L	0.3423 ppb	20:35:35
3	Tl 190.801†	-115.5	10.8	1.4385 µg/L	1.4385 ppb	20:35:55
3	U 409.014†	-45.2	436.2	26.866 µg/L	26.866 ppb	20:35:35
3	V 292.402†	167.7	-272.7	-1.4852 µg/L	-1.4852 ppb	20:35:35
3	Zn 213.857†	617.9	121.8	0.7658 µg/L	0.7658 ppb	20:35:55

Mean Data: 1202056870|959109|5

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1773154.0	106.00 %	0.835			0.79%
Sc RADIAL	157343.9	108 %	0.6			0.57%
Y 371.029	1085370.2	106.14 %	0.796			0.75%
Ag 328.068†	-32.2	-0.1243 µg/L	0.25504	-0.1243 ppb	0.25504	205.20%
Al 396.153Radial†	-4.7	-1.0672 µg/L	3.20015	-1.0672 ppb	3.20015	299.87%
As 188.979†	-3.4	-1.4154 µg/L	4.06495	-1.4154 ppb	4.06495	287.20%
B 249.677†	-104.4	-1.7541 µg/L	0.60492	-1.7541 ppb	0.60492	34.49%
Ba 233.527†	14.0	0.0631 µg/L	0.06644	0.0631 ppb	0.06644	105.24%
Be 313.107†	182.9	0.0648 µg/L	0.03318	0.0648 ppb	0.03318	51.19%
Ca 317.933Radial†	177.2	10.385 µg/L	0.2880	10.385 ppb	0.2880	2.77%
Cd 226.502†	7.2	0.0490 µg/L	0.11369	0.0490 ppb	0.11369	231.87%
Co 228.616†	18.0	0.2460 µg/L	0.08710	0.2460 ppb	0.08710	35.41%
Cr 267.716†	-6.4	-0.0691 µg/L	0.03271	-0.0691 ppb	0.03271	47.32%
Cu 324.752†	116.7	0.5225 µg/L	0.34551	0.5225 ppb	0.34551	66.12%
Fe 238.204 Radial†	107.4	7.1419 µg/L	0.43409	7.1419 ppb	0.43409	6.08%
K 766.490 Radial†	-63.3	-26.075 µg/L	31.1201	-26.075 ppb	31.1201	119.35%
Mg 279.077 IEC†	-21.1	-8.6750 µg/L	3.32671	-8.6750 ppb	3.32671	38.35%
Mn 257.610†	161.5	0.2210 µg/L	0.03037	0.2210 ppb	0.03037	13.74%
Mo 202.031†	25.8	0.8151 µg/L	0.26928	0.8151 ppb	0.26928	33.04%
Na 589.592 Radial†	-128.5	-19.639 µg/L	0.7556	-19.639 ppb	0.7556	3.85%

Ni 231.604†	3.0	0.0378 µg/L	0.05491	0.0378 ppb	0.05491	145.35%
P 214.914†	-35.6	-8.5571 µg/L	1.54759	-8.5571 ppb	1.54759	18.09%
Pb 220.353†	-26.0	-1.5887 µg/L	0.25207	-1.5887 ppb	0.25207	15.87%
S 181.975 Axial†	-3.5	-2.7963 µg/L	2.26896	-2.7963 ppb	2.26896	81.14%
Sb 206.836†	-10.9	-1.4604 µg/L	1.63913	-1.4604 ppb	1.63913	112.24%
Se 196.026†	4.5	1.80 µg/L	1.336	1.80 ppb	1.336	74.10%
SiO2†	6845.4	748.19 µg/L	8.682	748.19 ppb	8.682	1.16%
Si 251.611†	20964.9	346.64 µg/L	1.077	346.64 ppb	1.077	0.31%
Sn 189.927†	-4.2	-0.2968 µg/L	0.69935	-0.2968 ppb	0.69935	235.59%
Sr 421.552†	83.8	0.1963 µg/L	0.25162	0.1963 ppb	0.25162	128.20%
Ti 334.940†	240.0	0.2386 µg/L	0.11463	0.2386 ppb	0.11463	48.04%
Tl 190.801†	15.9	2.1268 µg/L	0.59929	2.1268 ppb	0.59929	28.18%
U 409.014†	283.4	17.439 µg/L	8.4162	17.439 ppb	8.4162	48.26%
V 292.402†	-223.3	-1.2202 µg/L	0.32097	-1.2202 ppb	0.32097	26.31%
Zn 213.857†	130.4	0.8193 µg/L	0.13310	0.8193 ppb	0.13310	16.24%

Sequence No.: 37

Sample ID: CCV

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 7

Date Collected: 3/29/2010 20:39:13

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCV

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	158480.3	158480.3	109 %		20:39:46
1	Al 396.153Radial†	25899.3	23851.4	5184.2 µg/L	5184.2 ppb	20:39:46
1	Ca 317.933Radial†	91372.8	83419.3	4888.0 µg/L	4888.0 ppb	20:39:46
1	Fe 238.204 Radial†	79864.5	73338.0	4875.8 µg/L	4875.8 ppb	20:39:46
1	K 766.490 Radial†	13976.2	11398.9	4688.7 µg/L	4688.7 ppb	20:39:46
1	Mg 279.077 IEC†	13513.6	12241.7	5054.9 µg/L	5054.9 ppb	20:39:46
1	Na 589.592 Radial†	70984.5	63589.7	9725.9 µg/L	9725.9 ppb	20:39:46
1	Sr 421.552†	231158.4	212874.2	498.88 µg/L	498.88 ppb	20:39:44
1	Sc 361.383	1746203.9	1746203.9	104.39 %		20:40:13
1	Y 371.029	1060403.2	1060403.2	103.70 %		20:40:13
1	Ag 328.068†	129222.9	120821.9	496.49 µg/L	496.49 ppb	20:40:13
1	As 188.979†	1283.9	1244.1	526.99 µg/L	526.99 ppb	20:40:33
1	B 249.677†	33276.5	28521.6	477.15 µg/L	477.15 ppb	20:40:13
1	Ba 233.527†	114363.4	109729.4	501.68 µg/L	501.68 ppb	20:40:13
1	Be 313.107†	1632572.9	1564581.9	509.43 µg/L	509.43 ppb	20:40:13
1	Cd 226.502†	72628.8	69669.1	480.81 µg/L	480.81 ppb	20:40:13
1	Co 228.616†	36875.4	35501.3	486.39 µg/L	486.39 ppb	20:40:13
1	Cr 267.716†	59790.0	57115.6	490.45 µg/L	490.45 ppb	20:40:13
1	Cu 324.752†	120808.8	113303.8	494.05 µg/L	494.05 ppb	20:40:13
1	Mn 257.610†	375213.3	359355.3	490.82 µg/L	490.82 ppb	20:40:13
1	Mo 202.031†	15789.8	15181.1	479.66 µg/L	479.66 ppb	20:40:33
1	Ni 231.604†	39738.4	38108.3	487.45 µg/L	487.45 ppb	20:40:13
1	P 214.914†	10363.4	9848.0	2350.1 µg/L	2350.1 ppb	20:40:33
1	Pb 220.353†	8305.0	7843.4	476.67 µg/L	476.67 ppb	20:40:33
1	S 181.975 Axial†	1299.5	1150.0	935.75 µg/L	935.75 ppb	20:40:33
1	Sb 206.836†	3827.9	3580.3	483.91 µg/L	483.91 ppb	20:40:33
1	Se 196.026†	1246.7	1183.4	470 µg/L	470 ppb	20:40:33
1	SiO2†	51835.7	48083.1	5234.9 µg/L	5234.9 ppb	20:40:13
1	Si 251.611†	155248.2	148043.5	2438.3 µg/L	2438.3 ppb	20:40:13
1	Sn 189.927†	7083.7	6783.8	483.93 µg/L	483.93 ppb	20:40:33
1	Ti 334.940†	505298.5	483413.9	492.29 µg/L	492.29 ppb	20:40:13
1	Tl 190.801†	3587.5	3556.9	484.85 µg/L	484.85 ppb	20:40:33
1	U 409.014†	7184.1	7361.1	484.98 µg/L	484.98 ppb	20:40:13
1	V 292.402†	93312.1	88956.4	499.59 µg/L	499.59 ppb	20:40:13
1	Zn 213.857†	80758.5	76898.2	480.22 µg/L	480.22 ppb	20:40:13
2	Sc RADIAL	157839.6	157839.6	108 %		20:39:50
2	Al 396.153Radial†	25654.3	23721.9	5156.0 µg/L	5156.0 ppb	20:39:50
2	Ca 317.933Radial†	90857.8	83284.8	4880.1 µg/L	4880.1 ppb	20:39:50
2	Fe 238.204 Radial†	79351.6	73162.6	4864.1 µg/L	4864.1 ppb	20:39:50
2	K 766.490 Radial†	14108.1	11572.9	4760.3 µg/L	4760.3 ppb	20:39:50
2	Mg 279.077 IEC†	13317.1	12110.8	5000.9 µg/L	5000.9 ppb	20:39:50
2	Na 589.592 Radial†	70889.1	63766.6	9752.9 µg/L	9752.9 ppb	20:39:50
2	Sr 421.552†	232019.8	214532.6	502.77 µg/L	502.77 ppb	20:39:48
2	Sc 361.383	1748401.5	1748401.5	104.52 %		20:40:36
2	Y 371.029	1060574.0	1060574.0	103.72 %		20:40:36
2	Ag 328.068†	128320.4	119802.8	492.33 µg/L	492.33 ppb	20:40:36
2	As 188.979†	1300.9	1258.8	533.09 µg/L	533.09 ppb	20:40:56
2	B 249.677†	33199.5	28407.7	475.25 µg/L	475.25 ppb	20:40:36
2	Ba 233.527†	113312.8	108586.5	496.46 µg/L	496.46 ppb	20:40:36
2	Be 313.107†	1626044.8	1556370.4	506.76 µg/L	506.76 ppb	20:40:36
2	Cd 226.502†	71814.6	68802.6	474.82 µg/L	474.82 ppb	20:40:36
2	Co 228.616†	36702.1	35291.2	483.50 µg/L	483.50 ppb	20:40:36
2	Cr 267.716†	59191.4	56470.8	484.90 µg/L	484.90 ppb	20:40:36
2	Cu 324.752†	120253.9	112627.4	491.11 µg/L	491.11 ppb	20:40:36
2	Mn 257.610†	372516.4	356323.3	486.68 µg/L	486.68 ppb	20:40:36
2	Mo 202.031†	15750.8	15124.7	477.88 µg/L	477.88 ppb	20:40:56
2	Ni 231.604†	39612.3	37939.8	485.29 µg/L	485.29 ppb	20:40:36
2	P 214.914†	10343.5	9816.5	2342.6 µg/L	2342.6 ppb	20:40:56
2	Pb 220.353†	8312.4	7840.4	476.48 µg/L	476.48 ppb	20:40:56

2	S 181.975 Axial†	1287.8	1137.3	925.44 µg/L	925.44 ppb	20:40:56
2	Sb 206.836†	3843.7	3590.8	485.39 µg/L	485.39 ppb	20:40:56
2	Se 196.026†	1243.8	1179.1	469 µg/L	469 ppb	20:40:56
2	SiO2†	51279.8	47488.8	5170.0 µg/L	5170.0 ppb	20:40:36
2	Si 251.611†	154265.1	146916.0	2419.7 µg/L	2419.7 ppb	20:40:36
2	Sn 189.927†	7111.0	6801.4	485.17 µg/L	485.17 ppb	20:40:56
2	Ti 334.940†	501677.3	479340.9	488.14 µg/L	488.14 ppb	20:40:36
2	Tl 190.801†	3591.8	3556.8	484.78 µg/L	484.78 ppb	20:40:56
2	U 409.014†	7373.9	7534.0	495.49 µg/L	495.49 ppb	20:40:36
2	V 292.402†	92934.7	88483.0	496.93 µg/L	496.93 ppb	20:40:36
2	Zn 213.857†	80169.9	76237.8	476.08 µg/L	476.08 ppb	20:40:36
3	Sc RADIAL	156089.6	156089.6	107 %		20:39:54
3	Al 396.153Radial†	25631.8	23966.5	5209.3 µg/L	5209.3 ppb	20:39:54
3	Ca 317.933Radial†	90218.0	83628.1	4900.2 µg/L	4900.2 ppb	20:39:54
3	Fe 238.204 Radial†	78756.2	73428.1	4881.8 µg/L	4881.8 ppb	20:39:54
3	K 766.490 Radial†	13885.5	11511.0	4734.8 µg/L	4734.8 ppb	20:39:54
3	Mg 279.077 IEC†	13155.9	12098.2	4995.8 µg/L	4995.8 ppb	20:39:54
3	Na 589.592 Radial†	70406.1	64049.4	9796.2 µg/L	9796.2 ppb	20:39:54
3	Sr 421.552†	227678.4	212880.7	498.90 µg/L	498.90 ppb	20:39:52
3	Sc 361.383	1750051.7	1750051.7	104.62 %		20:40:59
3	Y 371.029	1061656.2	1061656.2	103.82 %		20:40:59
3	Ag 328.068†	129101.5	120433.7	494.92 µg/L	494.92 ppb	20:40:59
3	As 188.979†	1318.4	1274.5	539.66 µg/L	539.66 ppb	20:41:19
3	B 249.677†	33442.7	28610.3	478.64 µg/L	478.64 ppb	20:40:59
3	Ba 233.527†	114533.5	109651.1	501.32 µg/L	501.32 ppb	20:40:59
3	Be 313.107†	1637681.6	1566026.4	509.91 µg/L	509.91 ppb	20:40:59
3	Cd 226.502†	72370.3	69269.0	478.04 µg/L	478.04 ppb	20:40:59
3	Co 228.616†	36966.6	35510.9	486.52 µg/L	486.52 ppb	20:40:59
3	Cr 267.716†	59644.0	56850.1	488.16 µg/L	488.16 ppb	20:40:59
3	Cu 324.752†	121321.2	113539.1	495.08 µg/L	495.08 ppb	20:40:59
3	Mn 257.610†	375810.6	359135.9	490.53 µg/L	490.53 ppb	20:40:59
3	Mo 202.031†	15874.8	15229.0	481.17 µg/L	481.17 ppb	20:41:19
3	Ni 231.604†	39836.0	38117.9	487.57 µg/L	487.57 ppb	20:40:59
3	P 214.914†	10423.7	9883.8	2358.6 µg/L	2358.6 ppb	20:41:19
3	Pb 220.353†	8358.7	7877.1	478.72 µg/L	478.72 ppb	20:41:19
3	S 181.975 Axial†	1303.9	1151.5	936.96 µg/L	936.96 ppb	20:41:19
3	Sb 206.836†	3860.5	3603.4	487.09 µg/L	487.09 ppb	20:41:19
3	Se 196.026†	1260.6	1194.1	474 µg/L	474 ppb	20:41:19
3	SiO2†	51807.0	47946.5	5219.9 µg/L	5219.9 ppb	20:40:59
3	Si 251.611†	155533.5	147989.2	2437.4 µg/L	2437.4 ppb	20:40:59
3	Sn 189.927†	7141.0	6823.7	486.76 µg/L	486.76 ppb	20:41:19
3	Ti 334.940†	505758.7	482789.5	491.66 µg/L	491.66 ppb	20:40:59
3	Tl 190.801†	3621.3	3581.7	488.18 µg/L	488.18 ppb	20:41:19
3	U 409.014†	7328.7	7484.2	492.60 µg/L	492.60 ppb	20:40:59
3	V 292.402†	93571.4	89007.7	499.88 µg/L	499.88 ppb	20:40:59
3	Zn 213.857†	80716.3	76687.7	478.89 µg/L	478.89 ppb	20:40:59

Mean Data: CCV

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1748219.0	104.51 %	0.115			0.11%
Sc RADIAL	157469.8	108 %	0.8			0.79%
Y 371.029	1060877.8	103.75 %	0.066			0.06%
Ag 328.068†	120352.8	494.58 µg/L	2.097	494.58 ppb	2.097	0.42%
QC value within limits for Ag 328.068 Recovery = 98.92%						
Al 396.153Radial†	23846.6	5183.2 µg/L	26.63	5183.2 ppb	26.63	0.51%
QC value within limits for Al 396.153Radial Recovery = 103.66%						
As 188.979†	1259.1	533.25 µg/L	6.336	533.25 ppb	6.336	1.19%
QC value within limits for As 188.979 Recovery = 106.65%						
B 249.677†	28513.2	477.02 µg/L	1.699	477.02 ppb	1.699	0.36%
QC value within limits for B 249.677 Recovery = 95.40%						
Ba 233.527†	109322.4	499.82 µg/L	2.918	499.82 ppb	2.918	0.58%
QC value within limits for Ba 233.527 Recovery = 99.96%						
Be 313.107†	1562326.2	508.70 µg/L	1.694	508.70 ppb	1.694	0.33%
QC value within limits for Be 313.107 Recovery = 101.74%						
Ca 317.933Radial†	83444.1	4889.5 µg/L	10.13	4889.5 ppb	10.13	0.21%
QC value within limits for Ca 317.933Radial Recovery = 97.79%						
Cd 226.502†	69246.9	477.89 µg/L	2.994	477.89 ppb	2.994	0.63%
QC value within limits for Cd 226.502 Recovery = 95.58%						
Co 228.616†	35434.5	485.47 µg/L	1.703	485.47 ppb	1.703	0.35%

QC value within limits for Co 228.616 Recovery = 97.09%							
Cr 267.716†	56812.2	487.84 µg/L	2.787	487.84 ppb	2.787	0.57%	
QC value within limits for Cr 267.716 Recovery = 97.57%							
Cu 324.752†	113156.8	493.41 µg/L	2.057	493.41 ppb	2.057	0.42%	
QC value within limits for Cu 324.752 Recovery = 98.68%							
Fe 238.204 Radial†	73309.6	4873.9 µg/L	8.98	4873.9 ppb	8.98	0.18%	
QC value within limits for Fe 238.204 Radial Recovery = 97.48%							
K 766.490 Radial†	11494.3	4727.9 µg/L	36.31	4727.9 ppb	36.31	0.77%	
QC value within limits for K 766.490 Radial Recovery = 94.56%							
Mg 279.077 IEC†	12150.2	5017.2 µg/L	32.78	5017.2 ppb	32.78	0.65%	
QC value within limits for Mg 279.077 IEC Recovery = 100.34%							
Mn 257.610†	358271.5	489.35 µg/L	2.310	489.35 ppb	2.310	0.47%	
QC value within limits for Mn 257.610 Recovery = 97.87%							
Mo 202.031†	15178.3	479.57 µg/L	1.650	479.57 ppb	1.650	0.34%	
QC value within limits for Mo 202.031 Recovery = 95.91%							
Na 589.592 Radial†	63801.9	9758.3 µg/L	35.47	9758.3 ppb	35.47	0.36%	
QC value within limits for Na 589.592 Radial Recovery = 97.58%							
Ni 231.604†	38055.3	486.77 µg/L	1.281	486.77 ppb	1.281	0.26%	
QC value within limits for Ni 231.604 Recovery = 97.35%							
P 214.914†	9849.4	2350.4 µg/L	8.04	2350.4 ppb	8.04	0.34%	
QC value within limits for P 214.914 Recovery = 94.02%							
Pb 220.353†	7853.6	477.29 µg/L	1.242	477.29 ppb	1.242	0.26%	
QC value within limits for Pb 220.353 Recovery = 95.46%							
S 181.975 Axial†	1146.3	932.72 µg/L	6.328	932.72 ppb	6.328	0.68%	
QC value within limits for S 181.975 Axial Recovery = 93.27%							
Sb 206.836†	3591.5	485.47 µg/L	1.590	485.47 ppb	1.590	0.33%	
QC value within limits for Sb 206.836 Recovery = 97.09%							
Se 196.026†	1185.5	471 µg/L	3.0	471 ppb	3.0	0.65%	
QC value within limits for Se 196.026 Recovery = 94.21%							
SiO2†	47839.5	5208.2 µg/L	33.99	5208.2 ppb	33.99	0.65%	
QC value within limits for SiO2 Recovery = 97.40%							
Si 251.611†	147649.6	2431.8 µg/L	10.49	2431.8 ppb	10.49	0.43%	
QC value within limits for Si 251.611 Recovery = 97.27%							
Sn 189.927†	6803.0	485.29 µg/L	1.421	485.29 ppb	1.421	0.29%	
QC value within limits for Sn 189.927 Recovery = 97.06%							
Sr 421.552†	213429.2	500.18 µg/L	2.240	500.18 ppb	2.240	0.45%	
QC value within limits for Sr 421.552 Recovery = 100.04%							
Ti 334.940†	481848.1	490.70 µg/L	2.236	490.70 ppb	2.236	0.46%	
QC value within limits for Ti 334.940 Recovery = 98.14%							
Tl 190.801†	3565.2	485.94 µg/L	1.942	485.94 ppb	1.942	0.40%	
QC value within limits for Tl 190.801 Recovery = 97.19%							
U 409.014†	7459.8	491.02 µg/L	5.432	491.02 ppb	5.432	1.11%	
QC value within limits for U 409.014 Recovery = 98.20%							
V 292.402†	88815.7	498.80 µg/L	1.625	498.80 ppb	1.625	0.33%	
QC value within limits for V 292.402 Recovery = 99.76%							
Zn 213.857†	76607.9	478.40 µg/L	2.115	478.40 ppb	2.115	0.44%	
QC value within limits for Zn 213.857 Recovery = 95.68%							
All analyte(s) passed QC.							

Sequence No.: 38

Sample ID: CCB

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 8

Date Collected: 3/29/2010 20:41:27

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCB

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	159642.2	159642.2	110 %		20:41:56
1	Al 396.153Radial†	-31.9	2.8	0.5753 µg/L	0.5753 ppb	20:42:16
1	Ca 317.933Radial†	722.9	43.8	2.5682 µg/L	2.5682 ppb	20:42:16
1	Fe 238.204 Radial†	156.5	29.6	1.9698 µg/L	1.9698 ppb	20:42:16
1	K 766.490 Radial†	1376.5	-198.2	-81.588 µg/L	-81.588 ppb	20:41:56
1	Mg 279.077 IEC†	160.5	-40.1	-16.536 µg/L	-16.536 ppb	20:42:16
1	Na 589.592 Radial†	1426.6	-392.2	-59.938 µg/L	-59.938 ppb	20:41:56
1	Sr 421.552†	-236.3	62.2	0.1458 µg/L	0.1458 ppb	20:41:56
1	Sc 361.383	1761363.3	1761363.3	105.30 %		20:43:04
1	Y 371.029	1082249.7	1082249.7	105.84 %		20:43:04
1	Ag 328.068†	2961.0	-154.9	-0.6438 µg/L	-0.6438 ppb	20:43:06
1	As 188.979†	-17.6	-2.5	-1.0426 µg/L	-1.0426 ppb	20:43:26
1	B 249.677†	3116.7	-395.7	-6.6440 µg/L	-6.6440 ppb	20:43:26
1	Ba 233.527†	-177.6	6.4	0.0281 µg/L	0.0281 ppb	20:43:26
1	Be 313.107†	-787.6	-87.9	-0.0270 µg/L	-0.0270 ppb	20:43:06
1	Cd 226.502†	-97.6	1.7	0.0116 µg/L	0.0116 ppb	20:43:26
1	Co 228.616†	-177.8	7.8	0.1062 µg/L	0.1062 ppb	20:43:26
1	Cr 267.716†	140.3	-27.0	-0.2369 µg/L	-0.2369 ppb	20:43:26
1	Cu 324.752†	2779.8	215.1	0.9395 µg/L	0.9395 ppb	20:43:06
1	Mn 257.610†	177.4	88.5	0.1216 µg/L	0.1216 ppb	20:43:26
1	Mo 202.031†	-33.7	23.2	0.7311 µg/L	0.7311 ppb	20:43:26
1	Ni 231.604†	-52.7	-9.1	-0.1163 µg/L	-0.1163 ppb	20:43:26
1	P 214.914†	64.5	-18.3	-4.4052 µg/L	-4.4052 ppb	20:43:26
1	Pb 220.353†	118.6	0.2	0.0090 µg/L	0.0090 ppb	20:43:26
1	S 181.975 Axial†	91.5	-7.9	-6.4221 µg/L	-6.4221 ppb	20:43:26
1	Sb 206.836†	85.6	-5.4	-0.7134 µg/L	-0.7134 ppb	20:43:26
1	Se 196.026†	17.8	6.0	2.38 µg/L	2.38 ppb	20:43:26
1	SiO2†	1758.9	97.6	10.643 µg/L	10.643 ppb	20:43:26
1	Si 251.611†	831.5	113.3	1.8631 µg/L	1.8631 ppb	20:43:26
1	Sn 189.927†	4.0	1.8	0.1284 µg/L	0.1284 ppb	20:43:26
1	Ti 334.940†	1053.8	364.4	0.3709 µg/L	0.3709 ppb	20:43:06
1	Tl 190.801†	-105.5	20.1	2.6847 µg/L	2.6847 ppb	20:43:26
1	U 409.014†	-413.2	86.7	5.2550 µg/L	5.2550 ppb	20:43:06
1	V 292.402†	111.6	-325.8	-1.7979 µg/L	-1.7979 ppb	20:43:06
1	Zn 213.857†	508.2	18.2	0.1146 µg/L	0.1146 ppb	20:43:26
2	Sc RADIAL	156186.9	156186.9	107 %		20:42:18
2	Al 396.153Radial†	-15.2	17.7	3.8291 µg/L	3.8291 ppb	20:42:38
2	Ca 317.933Radial†	693.6	31.0	1.8191 µg/L	1.8191 ppb	20:42:38
2	Fe 238.204 Radial†	162.9	38.7	2.5747 µg/L	2.5747 ppb	20:42:38
2	K 766.490 Radial†	1472.5	-80.8	-33.270 µg/L	-33.270 ppb	20:42:18
2	Mg 279.077 IEC†	190.1	-9.2	-3.7954 µg/L	-3.7954 ppb	20:42:38
2	Na 589.592 Radial†	1486.0	-308.0	-47.099 µg/L	-47.099 ppb	20:42:18
2	Sr 421.552†	-366.4	-64.0	-0.1499 µg/L	-0.1499 ppb	20:42:18
2	Sc 361.383	1768341.2	1768341.2	105.71 %		20:43:28
2	Y 371.029	1086167.8	1086167.8	106.22 %		20:43:28
2	Ag 328.068†	2860.7	-260.9	-1.0681 µg/L	-1.0681 ppb	20:43:30
2	As 188.979†	-12.8	2.1	0.8941 µg/L	0.8941 ppb	20:43:50
2	B 249.677†	3095.0	-428.0	-7.1869 µg/L	-7.1869 ppb	20:43:50
2	Ba 233.527†	-192.4	-6.9	-0.0315 µg/L	-0.0315 ppb	20:43:50
2	Be 313.107†	-460.5	224.5	0.0719 µg/L	0.0719 ppb	20:43:30
2	Cd 226.502†	-94.7	4.9	0.0334 µg/L	0.0334 ppb	20:43:50
2	Co 228.616†	-140.7	43.5	0.5958 µg/L	0.5958 ppb	20:43:50
2	Cr 267.716†	149.4	-18.9	-0.1596 µg/L	-0.1596 ppb	20:43:50
2	Cu 324.752†	2666.0	97.1	0.4194 µg/L	0.4194 ppb	20:43:30
2	Mn 257.610†	165.4	76.4	0.1046 µg/L	0.1046 ppb	20:43:50
2	Mo 202.031†	-30.4	26.4	0.8348 µg/L	0.8348 ppb	20:43:50
2	Ni 231.604†	-24.5	17.7	0.2263 µg/L	0.2263 ppb	20:43:50
2	P 214.914†	45.9	-36.2	-8.6751 µg/L	-8.6751 ppb	20:43:50
2	Pb 220.353†	89.4	-27.9	-1.6824 µg/L	-1.6824 ppb	20:43:50

2	S 181.975 Axial†	94.2	-5.7	-4.6425 µg/L	-4.6425 ppb	20:43:50
2	Sb 206.836†	72.8	-17.8	-2.3809 µg/L	-2.3809 ppb	20:43:50
2	Se 196.026†	8.4	-3.0	-1.17 µg/L	-1.17 ppb	20:43:50
2	SiO2†	1693.5	29.1	3.1523 µg/L	3.1523 ppb	20:43:50
2	Si 251.611†	804.4	84.5	1.3841 µg/L	1.3841 ppb	20:43:50
2	Sn 189.927†	8.2	5.7	0.4069 µg/L	0.4069 ppb	20:43:50
2	Ti 334.940†	839.4	157.7	0.1627 µg/L	0.1627 ppb	20:43:30
2	Tl 190.801†	-101.0	24.8	3.3258 µg/L	3.3258 ppb	20:43:50
2	U 409.014†	-571.5	-61.5	-3.8245 µg/L	-3.8245 ppb	20:43:30
2	V 292.402†	384.6	-68.0	-0.3725 µg/L	-0.3725 ppb	20:43:30
2	Zn 213.857†	520.5	28.0	0.1740 µg/L	0.1740 ppb	20:43:50
3	Sc RADIAL	157025.4	157025.4	108 %		20:42:40
3	Al 396.153Radial†	-41.8	-6.9	-1.5626 µg/L	-1.5626 ppb	20:43:00
3	Ca 317.933Radial†	735.1	66.2	3.8771 µg/L	3.8771 ppb	20:43:00
3	Fe 238.204 Radial†	156.0	31.5	2.0942 µg/L	2.0942 ppb	20:43:00
3	K 766.490 Radial†	1504.7	-58.3	-23.989 µg/L	-23.989 ppb	20:42:40
3	Mg 279.077 IEC†	175.7	-23.6	-9.6897 µg/L	-9.6897 ppb	20:43:00
3	Na 589.592 Radial†	1490.0	-311.7	-47.668 µg/L	-47.668 ppb	20:42:40
3	Sr 421.552†	-200.3	92.1	0.2158 µg/L	0.2158 ppb	20:42:40
3	Sc 361.383	1802169.8	1802169.8	107.74 %		20:43:52
3	Y 371.029	1105477.1	1105477.1	108.11 %		20:43:52
3	Ag 328.068†	2995.0	-187.1	-0.7466 µg/L	-0.7466 ppb	20:43:54
3	As 188.979†	-15.0	0.3	0.1424 µg/L	0.1424 ppb	20:44:15
3	B 249.677†	3108.4	-470.5	-7.8995 µg/L	-7.8995 ppb	20:44:15
3	Ba 233.527†	-173.6	13.9	0.0633 µg/L	0.0633 ppb	20:44:15
3	Be 313.107†	-686.3	23.1	0.0136 µg/L	0.0136 ppb	20:43:54
3	Cd 226.502†	-87.9	12.8	0.0881 µg/L	0.0881 ppb	20:44:15
3	Co 228.616†	-169.8	19.0	0.2599 µg/L	0.2599 ppb	20:44:15
3	Cr 267.716†	170.2	-2.2	-0.0351 µg/L	-0.0351 ppb	20:44:15
3	Cu 324.752†	2724.0	103.6	0.4670 µg/L	0.4670 ppb	20:43:54
3	Mn 257.610†	180.6	87.6	0.1201 µg/L	0.1201 ppb	20:44:15
3	Mo 202.031†	-18.7	37.8	1.1943 µg/L	1.1943 ppb	20:44:15
3	Ni 231.604†	-67.6	-21.8	-0.2790 µg/L	-0.2790 ppb	20:44:15
3	P 214.914†	48.5	-34.6	-8.3057 µg/L	-8.3057 ppb	20:44:15
3	Pb 220.353†	111.7	-8.7	-0.5419 µg/L	-0.5419 ppb	20:44:15
3	S 181.975 Axial†	82.0	-18.7	-15.128 µg/L	-15.128 ppb	20:44:15
3	Sb 206.836†	86.7	-6.1	-0.8115 µg/L	-0.8115 ppb	20:44:15
3	Se 196.026†	20.9	8.5	3.37 µg/L	3.37 ppb	20:44:15
3	SiO2†	1699.8	4.9	0.5106 µg/L	0.5106 ppb	20:44:15
3	Si 251.611†	817.9	82.8	1.3569 µg/L	1.3569 ppb	20:44:15
3	Sn 189.927†	-7.0	-8.5	-0.6027 µg/L	-0.6027 ppb	20:44:15
3	Ti 334.940†	578.4	-99.5	-0.1088 µg/L	-0.1088 ppb	20:43:54
3	Tl 190.801†	-115.5	13.1	1.7476 µg/L	1.7476 ppb	20:44:15
3	U 409.014†	-166.7	324.4	19.989 µg/L	19.989 ppb	20:43:54
3	V 292.402†	270.2	-181.0	-0.9785 µg/L	-0.9785 ppb	20:43:54
3	Zn 213.857†	519.3	17.6	0.1119 µg/L	0.1119 ppb	20:44:15

Mean Data: CCB

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1777291.5	106.25 %	1.305			1.23%
Sc RADIAL	157618.2	108 %	1.2			1.14%
Y 371.029	1091298.2	106.72 %	1.216			1.14%
Ag 328.068†	-201.0	-0.8195 µg/L	0.22133	-0.8195 ppb	0.22133	27.01%
QC value within limits for Ag 328.068 Recovery = Not calculated						
Al 396.153Radial†	4.5	0.9472 µg/L	2.71501	0.9472 ppb	2.71501	286.62%
QC value within limits for Al 396.153Radial Recovery = Not calculated						
As 188.979†	-0.0	-0.0020 µg/L	0.97639	-0.0020 ppb	0.97639	>999.9%
QC value within limits for As 188.979 Recovery = Not calculated						
B 249.677†	-431.4	-7.2435 µg/L	0.62967	-7.2435 ppb	0.62967	8.69%
QC value within limits for B 249.677 Recovery = Not calculated						
Ba 233.527†	4.5	0.0200 µg/L	0.04797	0.0200 ppb	0.04797	240.04%
QC value within limits for Ba 233.527 Recovery = Not calculated						
Be 313.107†	53.2	0.0195 µg/L	0.04972	0.0195 ppb	0.04972	254.94%
QC value within limits for Be 313.107 Recovery = Not calculated						
Ca 317.933Radial†	47.0	2.7548 µg/L	1.04159	2.7548 ppb	1.04159	37.81%
QC value within limits for Ca 317.933Radial Recovery = Not calculated						
Cd 226.502†	6.5	0.0444 µg/L	0.03942	0.0444 ppb	0.03942	88.81%
QC value within limits for Cd 226.502 Recovery = Not calculated						
Co 228.616†	23.4	0.3206 µg/L	0.25038	0.3206 ppb	0.25038	78.09%

QC value within limits for Co 228.616 Recovery = Not calculated							
Cr 267.716†	-16.1	-0.1439 µg/L	0.10181	-0.1439 ppb	0.10181	70.75%	
QC value within limits for Cr 267.716 Recovery = Not calculated							
Cu 324.752†	138.6	0.6086 µg/L	0.28751	0.6086 ppb	0.28751	47.24%	
QC value within limits for Cu 324.752 Recovery = Not calculated							
Fe 238.204 Radial†	33.3	2.2129 µg/L	0.31946	2.2129 ppb	0.31946	14.44%	
QC value within limits for Fe 238.204 Radial Recovery = Not calculated							
K 766.490 Radial†	-112.4	-46.282 µg/L	30.9255	-46.282 ppb	30.9255	66.82%	
QC value within limits for K 766.490 Radial Recovery = Not calculated							
Mg 279.077 IEC†	-24.3	-10.007 µg/L	6.3764	-10.007 ppb	6.3764	63.72%	
QC value within limits for Mg 279.077 IEC Recovery = Not calculated							
Mn 257.610†	84.2	0.1154 µg/L	0.00942	0.1154 ppb	0.00942	8.16%	
QC value within limits for Mn 257.610 Recovery = Not calculated							
Mo 202.031†	29.2	0.9200 µg/L	0.24309	0.9200 ppb	0.24309	26.42%	
QC value within limits for Mo 202.031 Recovery = Not calculated							
Na 589.592 Radial†	-337.3	-51.568 µg/L	7.2542	-51.568 ppb	7.2542	14.07%	
QC value within limits for Na 589.592 Radial Recovery = Not calculated							
Ni 231.604†	-4.4	-0.0563 µg/L	0.25791	-0.0563 ppb	0.25791	457.85%	
QC value within limits for Ni 231.604 Recovery = Not calculated							
P 214.914†	-29.7	-7.1287 µg/L	2.36584	-7.1287 ppb	2.36584	33.19%	
QC value within limits for P 214.914 Recovery = Not calculated							
Pb 220.353†	-12.1	-0.7384 µg/L	0.86263	-0.7384 ppb	0.86263	116.82%	
QC value within limits for Pb 220.353 Recovery = Not calculated							
S 181.975 Axial†	-10.8	-8.7308 µg/L	5.61093	-8.7308 ppb	5.61093	64.27%	
QC value within limits for S 181.975 Axial Recovery = Not calculated							
Sb 206.836†	-9.7	-1.3019 µg/L	0.93572	-1.3019 ppb	0.93572	71.87%	
QC value within limits for Sb 206.836 Recovery = Not calculated							
Se 196.026†	3.8	1.53 µg/L	2.391	1.53 ppb	2.391	156.61%	
QC value within limits for Se 196.026 Recovery = Not calculated							
SiO2†	43.9	4.7687 µg/L	5.25620	4.7687 ppb	5.25620	110.22%	
QC value within limits for SiO2 Recovery = Not calculated							
Si 251.611†	93.5	1.5347 µg/L	0.28470	1.5347 ppb	0.28470	18.55%	
QC value within limits for Si 251.611 Recovery = Not calculated							
Sn 189.927†	-0.3	-0.0225 µg/L	0.52147	-0.0225 ppb	0.52147	>999.9%	
QC value within limits for Sn 189.927 Recovery = Not calculated							
Sr 421.552†	30.1	0.0706 µg/L	0.19411	0.0706 ppb	0.19411	275.10%	
QC value within limits for Sr 421.552 Recovery = Not calculated							
Ti 334.940†	140.8	0.1416 µg/L	0.24052	0.1416 ppb	0.24052	169.85%	
QC value within limits for Ti 334.940 Recovery = Not calculated							
Tl 190.801†	19.3	2.5860 µg/L	0.79369	2.5860 ppb	0.79369	30.69%	
QC value within limits for Tl 190.801 Recovery = Not calculated							
U 409.014†	116.5	7.1397 µg/L	12.01791	7.1397 ppb	12.01791	168.33%	
QC value within limits for U 409.014 Recovery = Not calculated							
V 292.402†	-191.6	-1.0496 µg/L	0.71539	-1.0496 ppb	0.71539	68.16%	
QC value within limits for V 292.402 Recovery = Not calculated							
Zn 213.857†	21.3	0.1335 µg/L	0.03514	0.1335 ppb	0.03514	26.32%	
QC value within limits for Zn 213.857 Recovery = Not calculated							
All analyte(s) passed QC.							

Sequence No.: 39

Sample ID: 248117001|959109|1

Analyst: HSC

Initial Sample Wt:

Dilution:

Autosampler Location: 331

Date Collected: 3/29/2010 20:44:22

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: 248117001|959109|1

Repl#	Analyte	Net Intensity	Corrected Intensity	Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	160370.5	160370.5	110 %		20:44:53
1	Al 396.153Radial†	30.3	59.4	12.935 µg/L	12.935 ppb	20:45:13
1	Ca 317.933Radial†	1649.9	883.3	51.758 µg/L	51.758 ppb	20:45:13
1	Fe 238.204 Radial†	454.1	299.4	19.906 µg/L	19.906 ppb	20:45:13
1	K 766.490 Radial†	2384.3	712.0	293.08 µg/L	293.08 ppb	20:44:53
1	Mg 279.077 IEC†	208.4	2.7	1.1103 µg/L	1.1103 ppb	20:45:13
1	Na 589.592 Radial†	2868.2	912.0	139.29 µg/L	139.29 ppb	20:44:53
1	Sr 421.552†	-88.4	197.6	0.4627 µg/L	0.4627 ppb	20:44:53
1	Sc 361.383	1781146.3	1781146.3	106.48 %		20:46:01
1	Y 371.029	1087914.8	1087914.8	106.39 %		20:46:01
1	Ag 328.068†	3093.1	-62.2	-0.2418 µg/L	-0.2418 ppb	20:46:03
1	As 188.979†	-13.2	1.8	0.7676 µg/L	0.7676 ppb	20:46:23
1	B 249.677†	4744.3	1099.9	18.467 µg/L	18.467 ppb	20:46:03
1	Ba 233.527†	-95.0	85.8	0.3919 µg/L	0.3919 ppb	20:46:23
1	Be 313.107†	-550.5	143.1	0.0507 µg/L	0.0507 ppb	20:46:03
1	Cd 226.502†	-93.7	6.4	0.0421 µg/L	0.0421 ppb	20:46:23
1	Co 228.616†	-186.5	1.5	0.0193 µg/L	0.0193 ppb	20:46:23
1	Cr 267.716†	239.3	64.5	0.5439 µg/L	0.5439 ppb	20:46:23
1	Cu 324.752†	4113.8	1438.7	6.2680 µg/L	6.2680 ppb	20:46:03
1	Mn 257.610†	582.1	466.7	0.6377 µg/L	0.6377 ppb	20:46:23
1	Mo 202.031†	-37.3	20.2	0.6388 µg/L	0.6388 ppb	20:46:23
1	Ni 231.604†	-33.7	9.3	0.1185 µg/L	0.1185 ppb	20:46:23
1	P 214.914†	67.7	-16.0	-3.9172 µg/L	-3.9172 ppb	20:46:23
1	Pb 220.353†	83.6	-33.9	-2.0652 µg/L	-2.0652 ppb	20:46:23
1	S 181.975 Axial†	147.2	43.4	35.204 µg/L	35.204 ppb	20:46:23
1	Sb 206.836†	88.7	-3.4	-0.4537 µg/L	-0.4537 ppb	20:46:23
1	Se 196.026†	19.5	7.4	2.96 µg/L	2.96 ppb	20:46:23
1	SiO2†	43145.4	38947.4	4257.0 µg/L	4257.0 ppb	20:46:03
1	Si 251.611†	128490.0	119995.8	1984.1 µg/L	1984.1 ppb	20:46:03
1	Sn 189.927†	-5.0	-6.7	-0.4744 µg/L	-0.4744 ppb	20:46:23
1	Ti 334.940†	974.7	279.0	0.2800 µg/L	0.2800 ppb	20:46:03
1	Tl 190.801†	-122.5	5.2	0.7051 µg/L	0.7051 ppb	20:46:23
1	U 409.014†	-277.2	218.7	13.495 µg/L	13.495 ppb	20:46:03
1	V 292.402†	384.8	-70.4	-0.3760 µg/L	-0.3760 ppb	20:46:03
1	Zn 213.857†	1542.8	984.5	6.1897 µg/L	6.1897 ppb	20:46:23
2	Sc RADIAL	155891.5	155891.5	107 %		20:45:15
2	Al 396.153Radial†	33.8	63.5	13.829 µg/L	13.829 ppb	20:45:35
2	Ca 317.933Radial†	1656.2	932.3	54.630 µg/L	54.630 ppb	20:45:35
2	Fe 238.204 Radial†	468.7	325.0	21.604 µg/L	21.604 ppb	20:45:35
2	K 766.490 Radial†	2287.1	683.4	281.31 µg/L	281.31 ppb	20:45:15
2	Mg 279.077 IEC†	215.1	14.4	5.9353 µg/L	5.9353 ppb	20:45:35
2	Na 589.592 Radial†	2827.3	948.8	144.92 µg/L	144.92 ppb	20:45:15
2	Sr 421.552†	-143.4	143.9	0.3369 µg/L	0.3369 ppb	20:45:15
2	Sc 361.383	1798822.3	1798822.3	107.54 %		20:46:25
2	Y 371.029	1097841.5	1097841.5	107.36 %		20:46:25
2	Ag 328.068†	2975.9	-199.6	-0.8053 µg/L	-0.8053 ppb	20:46:27
2	As 188.979†	-15.6	-0.3	-0.0933 µg/L	-0.0933 ppb	20:46:47
2	B 249.677†	4776.2	1085.9	18.229 µg/L	18.229 ppb	20:46:27
2	Ba 233.527†	-94.2	87.4	0.3993 µg/L	0.3993 ppb	20:46:47
2	Be 313.107†	-539.1	158.8	0.0534 µg/L	0.0534 ppb	20:46:27
2	Cd 226.502†	-75.4	24.3	0.1655 µg/L	0.1655 ppb	20:46:47
2	Co 228.616†	-163.2	24.8	0.3394 µg/L	0.3394 ppb	20:46:47
2	Cr 267.716†	245.1	67.7	0.5774 µg/L	0.5774 ppb	20:46:47
2	Cu 324.752†	4294.2	1568.5	6.8264 µg/L	6.8264 ppb	20:46:27
2	Mn 257.610†	594.7	473.0	0.6461 µg/L	0.6461 ppb	20:46:47
2	Mo 202.031†	-36.6	21.2	0.6707 µg/L	0.6707 ppb	20:46:47
2	Ni 231.604†	-7.1	34.3	0.4393 µg/L	0.4393 ppb	20:46:47
2	P 214.914†	49.9	-33.2	-8.0477 µg/L	-8.0477 ppb	20:46:47
2	Pb 220.353†	89.5	-29.2	-1.7704 µg/L	-1.7704 ppb	20:46:47

2	S 181.975 Axial†	142.7	37.9	30.706 µg/L	30.706 ppb	20:46:47
2	Sb 206.836†	78.5	-13.6	-1.8344 µg/L	-1.8344 ppb	20:46:47
2	Se 196.026†	14.8	2.8	1.13 µg/L	1.13 ppb	20:46:47
2	SiO2†	42780.1	38209.5	4176.3 µg/L	4176.3 ppb	20:46:27
2	Si 251.611†	126994.7	117419.5	1941.5 µg/L	1941.5 ppb	20:46:27
2	Sn 189.927†	-0.3	-2.3	-0.1614 µg/L	-0.1614 ppb	20:46:47
2	Ti 334.940†	1060.2	349.6	0.3549 µg/L	0.3549 ppb	20:46:27
2	Tl 190.801†	-118.2	10.4	1.4005 µg/L	1.4005 ppb	20:46:47
2	U 409.014†	-414.6	93.6	5.7787 µg/L	5.7787 ppb	20:46:27
2	V 292.402†	453.1	-10.4	-0.0484 µg/L	-0.0484 ppb	20:46:27
2	Zn 213.857†	1560.7	986.9	6.2023 µg/L	6.2023 ppb	20:46:47
3	Sc RADIAL	158745.6	158745.6	109 %		20:45:37
3	Al 396.153Radial†	61.3	88.2	19.216 µg/L	19.216 ppb	20:45:57
3	Ca 317.933Radial†	1649.6	898.4	52.642 µg/L	52.642 ppb	20:45:57
3	Fe 238.204 Radial†	476.7	324.4	21.568 µg/L	21.568 ppb	20:45:57
3	K 766.490 Radial†	2393.6	742.7	305.72 µg/L	305.72 ppb	20:45:37
3	Mg 279.077 IEC†	215.1	10.8	4.4549 µg/L	4.4549 ppb	20:45:57
3	Na 589.592 Radial†	2824.4	898.5	137.21 µg/L	137.21 ppb	20:45:37
3	Sr 421.552†	-232.8	64.3	0.1502 µg/L	0.1502 ppb	20:45:37
3	Sc 361.383	1759292.6	1759292.6	105.17 %		20:46:50
3	Y 371.029	1073507.0	1073507.0	104.98 %		20:46:50
3	Ag 328.068†	2936.0	-175.4	-0.7021 µg/L	-0.7021 ppb	20:46:52
3	As 188.979†	-13.0	1.9	0.8023 µg/L	0.8023 ppb	20:47:12
3	B 249.677†	4630.3	1046.9	17.575 µg/L	17.575 ppb	20:46:52
3	Ba 233.527†	-101.6	78.5	0.3588 µg/L	0.3588 ppb	20:47:12
3	Be 313.107†	-664.7	28.1	0.0110 µg/L	0.0110 ppb	20:46:52
3	Cd 226.502†	-104.6	-5.1	-0.0371 µg/L	-0.0371 ppb	20:47:12
3	Co 228.616†	-165.1	19.6	0.2674 µg/L	0.2674 ppb	20:47:12
3	Cr 267.716†	205.7	35.3	0.2992 µg/L	0.2992 ppb	20:47:12
3	Cu 324.752†	4151.5	1522.5	6.6270 µg/L	6.6270 ppb	20:46:52
3	Mn 257.610†	552.3	445.1	0.6080 µg/L	0.6080 ppb	20:47:12
3	Mo 202.031†	-31.5	25.2	0.7974 µg/L	0.7974 ppb	20:47:12
3	Ni 231.604†	-2.9	38.2	0.4886 µg/L	0.4886 ppb	20:47:12
3	P 214.914†	51.0	-31.1	-7.5361 µg/L	-7.5361 ppb	20:47:12
3	Pb 220.353†	88.4	-28.4	-1.7200 µg/L	-1.7200 ppb	20:47:12
3	S 181.975 Axial†	149.2	47.0	38.101 µg/L	38.101 ppb	20:47:12
3	Sb 206.836†	89.1	-2.0	-0.2586 µg/L	-0.2586 ppb	20:47:12
3	Se 196.026†	18.2	6.4	2.56 µg/L	2.56 ppb	20:47:12
3	SiO2†	41466.8	37854.7	4137.5 µg/L	4137.5 ppb	20:46:52
3	Si 251.611†	123095.2	116365.2	1924.1 µg/L	1924.1 ppb	20:46:52
3	Sn 189.927†	-8.5	-10.1	-0.7163 µg/L	-0.7163 ppb	20:47:12
3	Ti 334.940†	2070.1	1332.0	1.3565 µg/L	1.3565 ppb	20:46:52
3	Tl 190.801†	-128.4	-1.8	-0.2214 µg/L	-0.2214 ppb	20:47:12
3	U 409.014†	-397.0	101.6	6.2948 µg/L	6.2948 ppb	20:46:52
3	V 292.402†	510.7	53.8	0.3075 µg/L	0.3075 ppb	20:46:52
3	Zn 213.857†	1508.9	970.3	6.0982 µg/L	6.0982 ppb	20:47:12

Mean Data: 248117001|959109|1

Analyte	Mean Corrected Intensity	Conc. Units	Calib. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1779753.7	106.40 %		1.184			1.11%
Sc RADIAL	158335.8	109 %		1.6			1.43%
Y 371.029	1086421.1	106.24 %		1.197			1.13%
Ag 328.068†	-145.7	-0.5831 µg/L		0.30002	-0.5831 ppb	0.30002	51.45%
Al 396.153Radial†	70.4	15.327 µg/L		3.3979	15.327 ppb	3.3979	22.17%
As 188.979†	1.2	0.4922 µg/L		0.50735	0.4922 ppb	0.50735	103.08%
B 249.677†	1077.6	18.090 µg/L		0.4619	18.090 ppb	0.4619	2.55%
Ba 233.527†	83.9	0.3833 µg/L		0.02157	0.3833 ppb	0.02157	5.63%
Be 313.107†	110.0	0.0384 µg/L		0.02373	0.0384 ppb	0.02373	61.81%
Ca 317.933Radial†	904.7	53.010 µg/L		1.4711	53.010 ppb	1.4711	2.78%
Cd 226.502†	8.5	0.0569 µg/L		0.10210	0.0569 ppb	0.10210	179.54%
Co 228.616†	15.3	0.2087 µg/L		0.16793	0.2087 ppb	0.16793	80.46%
Cr 267.716†	55.8	0.4735 µg/L		0.15190	0.4735 ppb	0.15190	32.08%
Cu 324.752†	1509.9	6.5738 µg/L		0.28300	6.5738 ppb	0.28300	4.30%
Fe 238.204 Radial†	316.3	21.026 µg/L		0.9700	21.026 ppb	0.9700	4.61%
K 766.490 Radial†	712.7	293.37 µg/L		12.209	293.37 ppb	12.209	4.16%
Mg 279.077 IEC†	9.3	3.8335 µg/L		2.47182	3.8335 ppb	2.47182	64.48%
Mn 257.610†	461.6	0.6306 µg/L		0.02000	0.6306 ppb	0.02000	3.17%
Mo 202.031†	22.2	0.7023 µg/L		0.08388	0.7023 ppb	0.08388	11.94%
Na 589.592 Radial†	919.8	140.48 µg/L		3.989	140.48 ppb	3.989	2.84%

Ni 231.604†	27.3	0.3488 µg/L	0.20095	0.3488 ppb	0.20095	57.61%
P 214.914†	-26.8	-6.5003 µg/L	2.25166	-6.5003 ppb	2.25166	34.64%
Pb 220.353†	-30.5	-1.8519 µg/L	0.18649	-1.8519 ppb	0.18649	10.07%
S 181.975 Axial†	42.8	34.671 µg/L	3.7263	34.671 ppb	3.7263	10.75%
Sb 206.836†	-6.3	-0.8489 µg/L	0.85901	-0.8489 ppb	0.85901	101.19%
Se 196.026†	5.6	2.22 µg/L	0.959	2.22 ppb	0.959	43.26%
SiO2†	38337.2	4190.3 µg/L	60.93	4190.3 ppb	60.93	1.45%
Si 251.611†	117926.8	1949.9 µg/L	30.88	1949.9 ppb	30.88	1.58%
Sn 189.927†	-6.4	-0.4507 µg/L	0.27824	-0.4507 ppb	0.27824	61.74%
Sr 421.552†	135.3	0.3166 µg/L	0.15725	0.3166 ppb	0.15725	49.67%
Ti 334.940†	653.5	0.6638 µg/L	0.60108	0.6638 ppb	0.60108	90.55%
Tl 190.801†	4.6	0.6281 µg/L	0.81367	0.6281 ppb	0.81367	129.55%
U 409.014†	138.0	8.5230 µg/L	4.31400	8.5230 ppb	4.31400	50.62%
V 292.402†	-9.0	-0.0390 µg/L	0.34184	-0.0390 ppb	0.34184	876.84%
Zn 213.857†	980.6	6.1634 µg/L	0.05682	6.1634 ppb	0.05682	0.92%

Sequence No.: 46

Sample ID: CCV

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 7

Date Collected: 3/29/2010 21:03:21

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCV

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	154851.7	154851.7	106 %		21:03:53
1	Al 396.153Radial†	25485.8	24020.4	5220.8 µg/L	5220.8 ppb	21:03:53
1	Ca 317.933Radial†	90010.8	84106.5	4928.3 µg/L	4928.3 ppb	21:03:53
1	Fe 238.204 Radial†	78533.5	73806.4	4906.9 µg/L	4906.9 ppb	21:03:53
1	K 766.490 Radial†	13939.7	11665.7	4798.5 µg/L	4798.5 ppb	21:03:53
1	Mg 279.077 IEC†	13229.3	12265.4	5064.8 µg/L	5064.8 ppb	21:03:53
1	Na 589.592 Radial†	69846.3	64048.1	9795.9 µg/L	9795.9 ppb	21:03:53
1	Sr 421.552†	228674.2	215517.6	505.08 µg/L	505.08 ppb	21:03:51
1	Sc 361.383	1713248.9	1713248.9	102.42 %		21:04:06
1	Y 371.029	1039105.6	1039105.6	101.62 %		21:04:06
1	Ag 328.068†	126578.4	120621.1	495.66 µg/L	495.66 ppb	21:04:06
1	As 188.979†	1286.8	1270.6	538.07 µg/L	538.07 ppb	21:04:26
1	B 249.677†	32552.7	28428.0	475.59 µg/L	475.59 ppb	21:04:06
1	Ba 233.527†	111768.2	109302.8	499.73 µg/L	499.73 ppb	21:04:06
1	Be 313.107†	1595894.5	1558852.6	507.57 µg/L	507.57 ppb	21:04:06
1	Cd 226.502†	71067.7	69483.2	479.52 µg/L	479.52 ppb	21:04:06
1	Co 228.616†	36010.7	35336.6	484.13 µg/L	484.13 ppb	21:04:06
1	Cr 267.716†	58430.3	56889.7	488.51 µg/L	488.51 ppb	21:04:06
1	Cu 324.752†	118439.2	113216.3	493.68 µg/L	493.68 ppb	21:04:06
1	Mn 257.610†	368025.4	359251.0	490.68 µg/L	490.68 ppb	21:04:06
1	Mo 202.031†	15706.6	15390.8	486.28 µg/L	486.28 ppb	21:04:26
1	Ni 231.604†	38854.0	37977.0	485.77 µg/L	485.77 ppb	21:04:06
1	P 214.914†	10314.2	9990.9	2384.3 µg/L	2384.3 ppb	21:04:26
1	Pb 220.353†	8262.0	7954.4	483.41 µg/L	483.41 ppb	21:04:26
1	S 181.975 Axial†	1274.3	1149.4	935.31 µg/L	935.31 ppb	21:04:26
1	Sb 206.836†	3786.5	3610.4	488.11 µg/L	488.11 ppb	21:04:26
1	Se 196.026†	1247.6	1207.2	480 µg/L	480 ppb	21:04:26
1	SiO2†	50572.1	47804.5	5204.1 µg/L	5204.1 ppb	21:04:06
1	Si 251.611†	152175.1	147903.7	2435.8 µg/L	2435.8 ppb	21:04:06
1	Sn 189.927†	7069.4	6900.4	492.22 µg/L	492.22 ppb	21:04:26
1	Ti 334.940†	495105.0	482772.1	491.64 µg/L	491.64 ppb	21:04:06
1	Tl 190.801†	3560.4	3596.6	490.17 µg/L	490.17 ppb	21:04:26
1	U 409.014†	7150.7	7460.8	491.07 µg/L	491.07 ppb	21:04:06
1	V 292.402†	91336.8	88747.2	498.49 µg/L	498.49 ppb	21:04:06
1	Zn 213.857†	78849.4	76522.2	477.86 µg/L	477.86 ppb	21:04:06
2	Sc RADIAL	153431.3	153431.3	105 %		21:03:57
2	Al 396.153Radial†	25174.7	23947.0	5204.9 µg/L	5204.9 ppb	21:03:57
2	Ca 317.933Radial†	89019.4	83949.0	4919.1 µg/L	4919.1 ppb	21:03:57
2	Fe 238.204 Radial†	77673.0	73673.3	4898.1 µg/L	4898.1 ppb	21:03:57
2	K 766.490 Radial†	13736.1	11593.9	4768.9 µg/L	4768.9 ppb	21:03:57
2	Mg 279.077 IEC†	13051.1	12211.4	5042.5 µg/L	5042.5 ppb	21:03:57
2	Na 589.592 Radial†	69569.0	64393.3	9848.8 µg/L	9848.8 ppb	21:03:57
2	Sr 421.552†	230380.7	219131.5	513.55 µg/L	513.55 ppb	21:03:55
2	Sc 361.383	1723240.0	1723240.0	103.02 %		21:04:29
2	Y 371.029	1044358.9	1044358.9	102.13 %		21:04:29
2	Ag 328.068†	127680.9	120974.7	497.13 µg/L	497.13 ppb	21:04:29
2	As 188.979†	1279.6	1256.3	532.10 µg/L	532.10 ppb	21:04:49
2	B 249.677†	32914.0	28594.4	478.37 µg/L	478.37 ppb	21:04:29
2	Ba 233.527†	112872.1	109741.6	501.74 µg/L	501.74 ppb	21:04:29
2	Be 313.107†	1612082.1	1565532.0	509.75 µg/L	509.75 ppb	21:04:29
2	Cd 226.502†	71525.6	69525.3	479.81 µg/L	479.81 ppb	21:04:29
2	Co 228.616†	36504.1	35611.7	487.90 µg/L	487.90 ppb	21:04:29
2	Cr 267.716†	58865.9	56981.8	489.29 µg/L	489.29 ppb	21:04:29
2	Cu 324.752†	119296.1	113377.7	494.39 µg/L	494.39 ppb	21:04:29
2	Mn 257.610†	370507.0	359576.6	491.13 µg/L	491.13 ppb	21:04:29
2	Mo 202.031†	15700.9	15296.3	483.30 µg/L	483.30 ppb	21:04:49
2	Ni 231.604†	39299.1	38189.1	488.48 µg/L	488.48 ppb	21:04:29
2	P 214.914†	10271.7	9891.3	2360.4 µg/L	2360.4 ppb	21:04:49
2	Pb 220.353†	8221.9	7868.7	478.21 µg/L	478.21 ppb	21:04:49

2	S 181.975 Axial†	1283.0	1150.6	936.30 µg/L	936.30 ppb	21:04:49
2	Sb 206.836†	3813.2	3614.9	488.65 µg/L	488.65 ppb	21:04:49
2	Se 196.026†	1244.9	1197.5	476 µg/L	476 ppb	21:04:49
2	SiO2†	51026.3	47959.1	5221.2 µg/L	5221.2 ppb	21:04:29
2	Si 251.611†	153367.0	148199.2	2440.8 µg/L	2440.8 ppb	21:04:29
2	Sn 189.927†	7028.6	6820.7	486.55 µg/L	486.55 ppb	21:04:49
2	Ti 334.940†	498901.8	483655.0	492.54 µg/L	492.54 ppb	21:04:29
2	Tl 190.801†	3590.9	3606.0	491.45 µg/L	491.45 ppb	21:04:49
2	U 409.014†	7310.8	7575.8	498.29 µg/L	498.29 ppb	21:04:29
2	V 292.402†	92221.6	89089.0	500.36 µg/L	500.36 ppb	21:04:29
2	Zn 213.857†	79595.3	76799.9	479.59 µg/L	479.59 ppb	21:04:29
3	Sc RADIAL	153860.9	153860.9	106 %		21:04:01
3	Al 396.153Radial†	25294.4	23993.6	5215.1 µg/L	5215.1 ppb	21:04:01
3	Ca 317.933Radial†	89754.2	84409.0	4946.0 µg/L	4946.0 ppb	21:04:01
3	Fe 238.204 Radial†	78247.7	74011.6	4920.6 µg/L	4920.6 ppb	21:04:01
3	K 766.490 Radial†	13894.4	11707.3	4815.6 µg/L	4815.6 ppb	21:04:01
3	Mg 279.077 IEC†	13234.5	12350.5	5099.8 µg/L	5099.8 ppb	21:04:01
3	Na 589.592 Radial†	69626.7	64263.4	9828.8 µg/L	9828.8 ppb	21:04:01
3	Sr 421.552†	228028.2	216291.8	506.89 µg/L	506.89 ppb	21:03:59
3	Sc 361.383	1732745.4	1732745.4	103.59 %		21:04:52
3	Y 371.029	1050125.7	1050125.7	102.69 %		21:04:52
3	Ag 328.068†	127692.6	120306.0	494.38 µg/L	494.38 ppb	21:04:52
3	As 188.979†	1285.3	1255.0	531.54 µg/L	531.54 ppb	21:05:12
3	B 249.677†	33066.4	28566.3	477.91 µg/L	477.91 ppb	21:04:52
3	Ba 233.527†	113084.6	109345.8	499.93 µg/L	499.93 ppb	21:04:52
3	Be 313.107†	1614930.2	1559697.0	507.85 µg/L	507.85 ppb	21:04:52
3	Cd 226.502†	71595.2	69211.7	477.64 µg/L	477.64 ppb	21:04:52
3	Co 228.616†	36541.6	35453.5	485.73 µg/L	485.73 ppb	21:04:52
3	Cr 267.716†	58957.8	56757.0	487.36 µg/L	487.36 ppb	21:04:52
3	Cu 324.752†	119675.9	113109.0	493.23 µg/L	493.23 ppb	21:04:52
3	Mn 257.610†	371477.0	358540.1	489.71 µg/L	489.71 ppb	21:04:52
3	Mo 202.031†	15758.3	15268.1	482.41 µg/L	482.41 ppb	21:05:12
3	Ni 231.604†	39365.4	38043.9	486.63 µg/L	486.63 ppb	21:04:52
3	P 214.914†	10350.1	9912.3	2365.5 µg/L	2365.5 ppb	21:05:12
3	Pb 220.353†	8278.4	7879.4	478.85 µg/L	478.85 ppb	21:05:12
3	S 181.975 Axial†	1296.2	1156.5	941.02 µg/L	941.02 ppb	21:05:12
3	Sb 206.836†	3820.2	3601.3	486.84 µg/L	486.84 ppb	21:05:12
3	Se 196.026†	1245.9	1191.9	474 µg/L	474 ppb	21:05:12
3	SiO2†	51139.5	47796.6	5203.5 µg/L	5203.5 ppb	21:04:52
3	Si 251.611†	153580.9	147589.1	2430.7 µg/L	2430.7 ppb	21:04:52
3	Sn 189.927†	7084.4	6837.2	487.72 µg/L	487.72 ppb	21:05:12
3	Ti 334.940†	499459.5	481536.7	490.37 µg/L	490.37 ppb	21:04:52
3	Tl 190.801†	3572.9	3569.5	486.51 µg/L	486.51 ppb	21:05:12
3	U 409.014†	7416.3	7638.8	501.99 µg/L	501.99 ppb	21:04:52
3	V 292.402†	92167.5	88545.7	497.33 µg/L	497.33 ppb	21:04:52
3	Zn 213.857†	79634.5	76413.9	477.17 µg/L	477.17 ppb	21:04:52

Mean Data: CCV

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1723078.1	103.01 %	0.583			0.57%
Sc RADIAL	154048.0	106 %	0.5			0.47%
Y 371.029	1044530.0	102.15 %	0.539			0.53%
Ag 328.068†	120633.9	495.73 µg/L	1.374	495.73 ppb	1.374	0.28%
QC value within limits for Ag 328.068 Recovery = 99.15%						
Al 396.153Radial†	23987.0	5213.6 µg/L	8.05	5213.6 ppb	8.05	0.15%
QC value within limits for Al 396.153Radial Recovery = 104.27%						
As 188.979†	1260.7	533.90 µg/L	3.620	533.90 ppb	3.620	0.68%
QC value within limits for As 188.979 Recovery = 106.78%						
B 249.677†	28529.6	477.29 µg/L	1.490	477.29 ppb	1.490	0.31%
QC value within limits for B 249.677 Recovery = 95.46%						
Ba 233.527†	109463.4	500.47 µg/L	1.106	500.47 ppb	1.106	0.22%
QC value within limits for Ba 233.527 Recovery = 100.09%						
Be 313.107†	1561360.5	508.39 µg/L	1.184	508.39 ppb	1.184	0.23%
QC value within limits for Be 313.107 Recovery = 101.68%						
Ca 317.933Radial†	84154.8	4931.1 µg/L	13.70	4931.1 ppb	13.70	0.28%
QC value within limits for Ca 317.933Radial Recovery = 98.62%						
Cd 226.502†	69406.7	478.99 µg/L	1.177	478.99 ppb	1.177	0.25%
QC value within limits for Cd 226.502 Recovery = 95.80%						
Co 228.616†	35467.2	485.92 µg/L	1.892	485.92 ppb	1.892	0.39%

QC value within limits for Co 228.616 Recovery = 97.18%							
Cr 267.716†	56876.2	488.38 µg/L	0.973	488.38 ppb	0.973	0.20%	
QC value within limits for Cr 267.716 Recovery = 97.68%							
Cu 324.752†	113234.3	493.76 µg/L	0.585	493.76 ppb	0.585	0.12%	
QC value within limits for Cu 324.752 Recovery = 98.75%							
Fe 238.204 Radial†	73830.5	4908.5 µg/L	11.33	4908.5 ppb	11.33	0.23%	
QC value within limits for Fe 238.204 Radial Recovery = 98.17%							
K 766.490 Radial†	11655.6	4794.3 µg/L	23.63	4794.3 ppb	23.63	0.49%	
QC value within limits for K 766.490 Radial Recovery = 95.89%							
Mg 279.077 IEC†	12275.8	5069.1 µg/L	28.89	5069.1 ppb	28.89	0.57%	
QC value within limits for Mg 279.077 IEC Recovery = 101.38%							
Mn 257.610†	359122.6	490.51 µg/L	0.726	490.51 ppb	0.726	0.15%	
QC value within limits for Mn 257.610 Recovery = 98.10%							
Mo 202.031†	15318.4	483.99 µg/L	2.029	483.99 ppb	2.029	0.42%	
QC value within limits for Mo 202.031 Recovery = 96.80%							
Na 589.592 Radial†	64235.0	9824.5 µg/L	26.69	9824.5 ppb	26.69	0.27%	
QC value within limits for Na 589.592 Radial Recovery = 98.25%							
Ni 231.604†	38070.0	486.96 µg/L	1.387	486.96 ppb	1.387	0.28%	
QC value within limits for Ni 231.604 Recovery = 97.39%							
P 214.914†	9931.5	2370.0 µg/L	12.59	2370.0 ppb	12.59	0.53%	
QC value within limits for P 214.914 Recovery = 94.80%							
Pb 220.353†	7900.8	480.16 µg/L	2.839	480.16 ppb	2.839	0.59%	
QC value within limits for Pb 220.353 Recovery = 96.03%							
S 181.975 Axial†	1152.2	937.54 µg/L	3.050	937.54 ppb	3.050	0.33%	
QC value within limits for S 181.975 Axial Recovery = 93.75%							
Sb 206.836†	3608.9	487.87 µg/L	0.930	487.87 ppb	0.930	0.19%	
QC value within limits for Sb 206.836 Recovery = 97.57%							
Se 196.026†	1198.9	476 µg/L	3.1	476 ppb	3.1	0.64%	
QC value within limits for Se 196.026 Recovery = 95.27%							
SiO2†	47853.4	5209.6 µg/L	10.06	5209.6 ppb	10.06	0.19%	
QC value within limits for SiO2 Recovery = 97.42%							
Si 251.611†	147897.3	2435.8 µg/L	5.04	2435.8 ppb	5.04	0.21%	
QC value within limits for Si 251.611 Recovery = 97.43%							
Sn 189.927†	6852.8	488.83 µg/L	2.990	488.83 ppb	2.990	0.61%	
QC value within limits for Sn 189.927 Recovery = 97.77%							
Sr 421.552†	216980.3	508.51 µg/L	4.460	508.51 ppb	4.460	0.88%	
QC value within limits for Sr 421.552 Recovery = 101.70%							
Ti 334.940†	482654.6	491.52 µg/L	1.088	491.52 ppb	1.088	0.22%	
QC value within limits for Ti 334.940 Recovery = 98.30%							
Tl 190.801†	3590.7	489.37 µg/L	2.564	489.37 ppb	2.564	0.52%	
QC value within limits for Tl 190.801 Recovery = 97.87%							
U 409.014†	7558.5	497.12 µg/L	5.554	497.12 ppb	5.554	1.12%	
QC value within limits for U 409.014 Recovery = 99.42%							
V 292.402†	88794.0	498.73 µg/L	1.529	498.73 ppb	1.529	0.31%	
QC value within limits for V 292.402 Recovery = 99.75%							
Zn 213.857†	76578.7	478.21 µg/L	1.247	478.21 ppb	1.247	0.26%	
QC value within limits for Zn 213.857 Recovery = 95.64%							

All analyte(s) passed QC.

Sequence No.: 47

Sample ID: CCB

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 8

Date Collected: 3/29/2010 21:05:20

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCB

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	154996.4	154996.4	106 %		21:05:49
1	Al 396.153Radial†	-63.3	-27.7	-6.1097 µg/L	-6.1097 ppb	21:06:09
1	Ca 317.933Radial†	693.4	35.9	2.1034 µg/L	2.1034 ppb	21:06:09
1	Fe 238.204 Radial†	151.1	28.8	1.9138 µg/L	1.9138 ppb	21:06:09
1	K 766.490 Radial†	1597.5	47.3	19.463 µg/L	19.463 ppb	21:05:49
1	Mg 279.077 IEC†	208.9	9.8	4.0702 µg/L	4.0702 ppb	21:06:09
1	Na 589.592 Radial†	1678.5	-116.3	-17.818 µg/L	-17.818 ppb	21:05:49
1	Sr 421.552†	-227.7	63.9	0.1497 µg/L	0.1497 ppb	21:05:49
1	Sc 361.383	1725992.9	1725992.9	103.18 %		21:06:57
1	Y 371.029	1059747.2	1059747.2	103.63 %		21:06:57
1	Ag 328.068†	3051.7	-9.4	-0.0382 µg/L	-0.0382 ppb	21:06:59
1	As 188.979†	-12.6	2.0	0.8526 µg/L	0.8526 ppb	21:07:19
1	B 249.677†	3056.4	-393.5	-6.6077 µg/L	-6.6077 ppb	21:07:19
1	Ba 233.527†	-168.8	11.5	0.0524 µg/L	0.0524 ppb	21:07:19
1	Be 313.107†	-508.1	167.7	0.0571 µg/L	0.0571 ppb	21:06:59
1	Cd 226.502†	-60.4	35.9	0.2479 µg/L	0.2479 ppb	21:07:19
1	Co 228.616†	-169.8	12.0	0.1644 µg/L	0.1644 ppb	21:07:19
1	Cr 267.716†	146.1	-18.7	-0.1673 µg/L	-0.1673 ppb	21:07:19
1	Cu 324.752†	2666.8	159.7	0.7014 µg/L	0.7014 ppb	21:06:59
1	Mn 257.610†	177.8	92.3	0.1259 µg/L	0.1259 ppb	21:07:19
1	Mo 202.031†	-5.1	50.3	1.5872 µg/L	1.5872 ppb	21:07:19
1	Ni 231.604†	-16.9	24.5	0.3133 µg/L	0.3133 ppb	21:07:19
1	P 214.914†	22.6	-57.6	-13.826 µg/L	-13.826 ppb	21:07:19
1	Pb 220.353†	90.0	-25.2	-1.5281 µg/L	-1.5281 ppb	21:07:19
1	S 181.975 Axial†	71.1	-25.9	-21.007 µg/L	-21.007 ppb	21:07:19
1	Sb 206.836†	85.9	-3.3	-0.4268 µg/L	-0.4268 ppb	21:07:19
1	Se 196.026†	19.1	7.6	3.00 µg/L	3.00 ppb	21:07:19
1	SiO2†	1671.8	47.4	5.1244 µg/L	5.1244 ppb	21:07:19
1	Si 251.611†	772.8	72.6	1.1761 µg/L	1.1761 ppb	21:07:19
1	Sn 189.927†	9.7	7.4	0.5233 µg/L	0.5233 ppb	21:07:19
1	Ti 334.940†	780.1	119.7	0.1184 µg/L	0.1184 ppb	21:06:59
1	Tl 190.801†	-117.8	6.2	0.8248 µg/L	0.8248 ppb	21:07:19
1	U 409.014†	-356.1	134.0	8.2316 µg/L	8.2316 ppb	21:06:59
1	V 292.402†	287.8	-152.9	-0.8274 µg/L	-0.8274 ppb	21:06:59
1	Zn 213.857†	507.5	27.4	0.1698 µg/L	0.1698 ppb	21:07:19
2	Sc RADIAL	152412.0	152412.0	105 %		21:06:11
2	Al 396.153Radial†	-24.5	8.4	1.8014 µg/L	1.8014 ppb	21:06:31
2	Ca 317.933Radial†	694.0	47.5	2.7825 µg/L	2.7825 ppb	21:06:31
2	Fe 238.204 Radial†	146.8	27.1	1.7992 µg/L	1.7992 ppb	21:06:31
2	K 766.490 Radial†	1385.9	-129.6	-53.361 µg/L	-53.361 ppb	21:06:11
2	Mg 279.077 IEC†	168.1	-25.9	-10.680 µg/L	-10.680 ppb	21:06:31
2	Na 589.592 Radial†	1601.9	-162.8	-24.860 µg/L	-24.860 ppb	21:06:11
2	Sr 421.552†	-193.2	93.2	0.2184 µg/L	0.2184 ppb	21:06:11
2	Sc 361.383	1730228.9	1730228.9	103.43 %		21:07:21
2	Y 371.029	1062056.7	1062056.7	103.86 %		21:07:21
2	Ag 328.068†	3294.6	218.2	0.8697 µg/L	0.8697 ppb	21:07:23
2	As 188.979†	-7.8	6.7	2.7923 µg/L	2.7923 ppb	21:07:43
2	B 249.677†	3121.5	-337.9	-5.6726 µg/L	-5.6726 ppb	21:07:43
2	Ba 233.527†	-196.4	-14.9	-0.0686 µg/L	-0.0686 ppb	21:07:43
2	Be 313.107†	-630.3	50.7	0.0170 µg/L	0.0170 ppb	21:07:23
2	Cd 226.502†	-85.2	12.1	0.0830 µg/L	0.0830 ppb	21:07:43
2	Co 228.616†	-178.5	4.0	0.0551 µg/L	0.0551 ppb	21:07:43
2	Cr 267.716†	146.8	-18.3	-0.1593 µg/L	-0.1593 ppb	21:07:43
2	Cu 324.752†	2640.7	128.1	0.5583 µg/L	0.5583 ppb	21:07:23
2	Mn 257.610†	136.5	52.0	0.0714 µg/L	0.0714 ppb	21:07:43
2	Mo 202.031†	-31.2	25.1	0.7914 µg/L	0.7914 ppb	21:07:43
2	Ni 231.604†	-64.5	-21.4	-0.2741 µg/L	-0.2741 ppb	21:07:43
2	P 214.914†	43.5	-37.5	-8.9955 µg/L	-8.9955 ppb	21:07:43
2	Pb 220.353†	100.4	-15.4	-0.9295 µg/L	-0.9295 ppb	21:07:43

2	S 181.975 Axial†	84.3	-13.3	-10.766 µg/L	-10.766 ppb	21:07:43
2	Sb 206.836†	56.9	-31.6	-4.2573 µg/L	-4.2573 ppb	21:07:43
2	Se 196.026†	21.3	9.7	3.82 µg/L	3.82 ppb	21:07:43
2	SiO2†	1625.1	-1.7	-0.2117 µg/L	-0.2117 ppb	21:07:43
2	Si 251.611†	795.8	92.9	1.5262 µg/L	1.5262 ppb	21:07:43
2	Sn 189.927†	2.5	0.4	0.0269 µg/L	0.0269 ppb	21:07:43
2	Ti 334.940†	1026.5	356.1	0.3635 µg/L	0.3635 ppb	21:07:23
2	Tl 190.801†	-125.8	-1.3	-0.1808 µg/L	-0.1808 ppb	21:07:43
2	U 409.014†	-469.0	25.7	1.5015 µg/L	1.5015 ppb	21:07:23
2	V 292.402†	173.5	-264.1	-1.4569 µg/L	-1.4569 ppb	21:07:23
2	Zn 213.857†	498.1	17.1	0.1092 µg/L	0.1092 ppb	21:07:43
3	Sc RADIAL	153579.1	153579.1	105 %		21:06:33
3	Al 396.153Radial†	-58.8	-23.9	-5.2607 µg/L	-5.2607 ppb	21:06:53
3	Ca 317.933Radial†	673.1	22.6	1.3237 µg/L	1.3237 ppb	21:06:53
3	Fe 238.204 Radial†	131.8	11.8	0.7823 µg/L	0.7823 ppb	21:06:53
3	K 766.490 Radial†	1453.7	-75.3	-31.005 µg/L	-31.005 ppb	21:06:33
3	Mg 279.077 IEC†	180.2	-15.7	-6.4370 µg/L	-6.4370 ppb	21:06:53
3	Na 589.592 Radial†	1585.7	-189.9	-29.024 µg/L	-29.024 ppb	21:06:33
3	Sr 421.552†	-259.8	31.4	0.0737 µg/L	0.0737 ppb	21:06:33
3	Sc 361.383	1727714.6	1727714.6	103.28 %		21:07:45
3	Y 371.029	1060914.8	1060914.8	103.75 %		21:07:45
3	Ag 328.068†	3064.7	0.2	-0.0004 µg/L	-0.0004 ppb	21:07:47
3	As 188.979†	-17.3	-2.5	-1.0488 µg/L	-1.0488 ppb	21:08:08
3	B 249.677†	3076.5	-377.0	-6.3309 µg/L	-6.3309 ppb	21:08:08
3	Ba 233.527†	-187.7	-6.7	-0.0307 µg/L	-0.0307 ppb	21:08:08
3	Be 313.107†	-530.7	146.3	0.0497 µg/L	0.0497 ppb	21:07:47
3	Cd 226.502†	-118.4	-20.2	-0.1396 µg/L	-0.1396 ppb	21:08:08
3	Co 228.616†	-159.8	21.9	0.3001 µg/L	0.3001 ppb	21:08:08
3	Cr 267.716†	166.1	0.6	-0.0009 µg/L	-0.0009 ppb	21:08:08
3	Cu 324.752†	2799.8	285.9	1.2487 µg/L	1.2487 ppb	21:07:47
3	Mn 257.610†	156.9	71.9	0.0985 µg/L	0.0985 ppb	21:08:08
3	Mo 202.031†	-29.4	26.7	0.8435 µg/L	0.8435 ppb	21:08:08
3	Ni 231.604†	-49.4	-6.9	-0.0885 µg/L	-0.0885 ppb	21:08:08
3	P 214.914†	34.7	-45.9	-11.027 µg/L	-11.027 ppb	21:08:08
3	Pb 220.353†	99.2	-16.4	-0.9975 µg/L	-0.9975 ppb	21:08:08
3	S 181.975 Axial†	91.1	-6.6	-5.3466 µg/L	-5.3466 ppb	21:08:08
3	Sb 206.836†	84.8	-4.6	-0.6054 µg/L	-0.6054 ppb	21:08:08
3	Se 196.026†	15.6	4.2	1.65 µg/L	1.65 ppb	21:08:08
3	SiO2†	1696.3	69.5	7.5803 µg/L	7.5803 ppb	21:08:08
3	Si 251.611†	783.8	82.5	1.3544 µg/L	1.3544 ppb	21:08:08
3	Sn 189.927†	-1.7	-3.7	-0.2629 µg/L	-0.2629 ppb	21:08:08
3	Ti 334.940†	938.9	272.7	0.2758 µg/L	0.2758 ppb	21:07:47
3	Tl 190.801†	-117.7	6.3	0.8448 µg/L	0.8448 ppb	21:08:08
3	U 409.014†	-379.0	112.2	6.8863 µg/L	6.8863 ppb	21:07:47
3	V 292.402†	296.9	-144.3	-0.7876 µg/L	-0.7876 ppb	21:07:47
3	Zn 213.857†	483.2	3.5	0.0213 µg/L	0.0213 ppb	21:08:08

Mean Data: CCB

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1727978.8	103.30 %	0.127			0.12%
Sc RADIAL	153662.5	105 %	0.9			0.84%
Y 371.029	1060906.2	103.75 %	0.113			0.11%
Ag 328.068†	69.6	0.2771 µg/L	0.51363	0.2771 ppb	0.51363	185.39%
QC value within limits for Ag 328.068 Recovery = Not calculated						
Al 396.153Radial†	-14.4	-3.1897 µg/L	4.34321	-3.1897 ppb	4.34321	136.17%
QC value within limits for Al 396.153Radial Recovery = Not calculated						
As 188.979†	2.1	0.8654 µg/L	1.92055	0.8654 ppb	1.92055	221.93%
QC value within limits for As 188.979 Recovery = Not calculated						
B 249.677†	-369.5	-6.2037 µg/L	0.48034	-6.2037 ppb	0.48034	7.74%
QC value within limits for B 249.677 Recovery = Not calculated						
Ba 233.527†	-3.3	-0.0156 µg/L	0.06185	-0.0156 ppb	0.06185	395.65%
QC value within limits for Ba 233.527 Recovery = Not calculated						
Be 313.107†	121.6	0.0413 µg/L	0.02134	0.0413 ppb	0.02134	51.70%
QC value within limits for Be 313.107 Recovery = Not calculated						
Ca 317.933Radial†	35.3	2.0699 µg/L	0.72997	2.0699 ppb	0.72997	35.27%
QC value within limits for Ca 317.933Radial Recovery = Not calculated						
Cd 226.502†	9.3	0.0638 µg/L	0.19446	0.0638 ppb	0.19446	304.95%
QC value within limits for Cd 226.502 Recovery = Not calculated						
Co 228.616†	12.7	0.1732 µg/L	0.12276	0.1732 ppb	0.12276	70.87%

QC value within limits for Co 228.616 Recovery = Not calculated							
Cr 267.716†	-12.2	-0.1092 µg/L	0.09382	-0.1092 ppb	0.09382	85.93%	
QC value within limits for Cr 267.716 Recovery = Not calculated							
Cu 324.752†	191.2	0.8362 µg/L	0.36438	0.8362 ppb	0.36438	43.58%	
QC value within limits for Cu 324.752 Recovery = Not calculated							
Fe 238.204 Radial†	22.5	1.4984 µg/L	0.62279	1.4984 ppb	0.62279	41.56%	
QC value within limits for Fe 238.204 Radial Recovery = Not calculated							
K 766.490 Radial†	-52.6	-21.634 µg/L	37.3056	-21.634 ppb	37.3056	172.44%	
QC value within limits for K 766.490 Radial Recovery = Not calculated							
Mg 279.077 IEC†	-10.6	-4.3490 µg/L	7.59366	-4.3490 ppb	7.59366	174.61%	
QC value within limits for Mg 279.077 IEC Recovery = Not calculated							
Mn 257.610†	72.1	0.0986 µg/L	0.02726	0.0986 ppb	0.02726	27.63%	
QC value within limits for Mn 257.610 Recovery = Not calculated							
Mo 202.031†	34.0	1.0741 µg/L	0.44518	1.0741 ppb	0.44518	41.45%	
QC value within limits for Mo 202.031 Recovery = Not calculated							
Na 589.592 Radial†	-156.3	-23.901 µg/L	5.6641	-23.901 ppb	5.6641	23.70%	
QC value within limits for Na 589.592 Radial Recovery = Not calculated							
Ni 231.604†	-1.3	-0.0164 µg/L	0.30026	-0.0164 ppb	0.30026	>999.9%	
QC value within limits for Ni 231.604 Recovery = Not calculated							
P 214.914†	-47.0	-11.283 µg/L	2.4255	-11.283 ppb	2.4255	21.50%	
QC value within limits for P 214.914 Recovery = Not calculated							
Pb 220.353†	-19.0	-1.1517 µg/L	0.32775	-1.1517 ppb	0.32775	28.46%	
QC value within limits for Pb 220.353 Recovery = Not calculated							
S 181.975 Axial†	-15.3	-12.373 µg/L	7.9530	-12.373 ppb	7.9530	64.28%	
QC value within limits for S 181.975 Axial Recovery = Not calculated							
Sb 206.836†	-13.2	-1.7632 µg/L	2.16182	-1.7632 ppb	2.16182	122.61%	
QC value within limits for Sb 206.836 Recovery = Not calculated							
Se 196.026†	7.1	2.83 µg/L	1.094	2.83 ppb	1.094	38.72%	
QC value within limits for Se 196.026 Recovery = Not calculated							
SiO2†	38.4	4.1643 µg/L	3.98373	4.1643 ppb	3.98373	95.66%	
QC value within limits for SiO2 Recovery = Not calculated							
Si 251.611†	82.7	1.3522 µg/L	0.17505	1.3522 ppb	0.17505	12.95%	
QC value within limits for Si 251.611 Recovery = Not calculated							
Sn 189.927†	1.3	0.0958 µg/L	0.39756	0.0958 ppb	0.39756	415.11%	
QC value within limits for Sn 189.927 Recovery = Not calculated							
Sr 421.552†	62.8	0.1473 µg/L	0.07240	0.1473 ppb	0.07240	49.16%	
QC value within limits for Sr 421.552 Recovery = Not calculated							
Ti 334.940†	249.5	0.2525 µg/L	0.12417	0.2525 ppb	0.12417	49.17%	
QC value within limits for Ti 334.940 Recovery = Not calculated							
Tl 190.801†	3.7	0.4963 µg/L	0.58643	0.4963 ppb	0.58643	118.16%	
QC value within limits for Tl 190.801 Recovery = Not calculated							
U 409.014†	90.6	5.5398 µg/L	3.56137	5.5398 ppb	3.56137	64.29%	
QC value within limits for U 409.014 Recovery = Not calculated							
V 292.402†	-187.1	-1.0240 µg/L	0.37548	-1.0240 ppb	0.37548	36.67%	
QC value within limits for V 292.402 Recovery = Not calculated							
Zn 213.857†	16.0	0.1001 µg/L	0.07465	0.1001 ppb	0.07465	74.57%	
QC value within limits for Zn 213.857 Recovery = Not calculated							
All analyte(s) passed QC.							

Daily Performance Report

Sample ID: Sample

Sample Date/Time: Sunday, April 11, 2010 14:25:07

Sample Description:

Method File: C:\elandata\Method\Daily2.mth

Dataset File: c:\elandata\Dataset\100125\Sample.718

Tuning File: c:\elandata\Tuning\default2.tun

Optimization File: c:\elandata\Optimize\default.dac

Dual Detector Mode: Pulse

Acq. Dead Time(ns): 35

Current Dead Time (ns): 35

Summary

Analyte	Mass	Meas. Intens. Mean	Net Intens. Mean	Net Intens. SD	Net Intens. RSD
Be	9.0	1476.9	1476.876	69.851	4.7
Mg	24.0	20563.4	20563.391	243.887	1.2
Co	58.9	60201.8	60201.792	593.479	1.0
Rh	102.9	118302.4	118302.431	575.695	0.5
In	114.9	144990.3	144990.303	1225.130	0.8
Pb	208.0	62594.6	62594.639	440.991	0.7
[> Ba	137.9	132866.7	132866.686	904.406	0.7
[Ba++	69.0	2162.0	0.016	0.001	4.8
[> Ce	139.9	160176.6	160176.628	1412.329	0.9
[CeO	155.9	3192.0	0.020	0.000	1.4
Bkgd	220.0	7.3	7.300	1.789	24.5

Current Optimization File Data

Current Value	Description
0.88	Nebulizer Gas Flow
4.25	Lens Voltage
1000.00	ICP RF Power
-1750.00	Analog Stage Voltage
1100.00	Pulse Stage Voltage
50.00	Discriminator Threshold
-2.00	AC Rod Offset

Current Autolens Data

Analyte	Mass	Num of Pts	DAC Value	Maximum Intensity
Be	9	13	5.5	1447.7
Co	59	13	6.0	52914.8
In	115	13	6.8	126833.9

ICPMS #4 TUNING REPORT

File Name: 100411.tun
File Path: C:\elandata\Tuning

Analyte	Exact Mass	Meas. Mass	Mass DAC	Res. DAC	Meas Peak W
He	3.0	3.0	602	2085	0.624
Be	9.0	9.0	2054	2075	0.628
Mg	24.0	24.0	5659	2110	0.557
Mg	25.0	25.0	5959	2125	0.584
Mg	26.0	26.0	6140	2110	0.602
Co	58.9	58.9	14170	2165	0.603
Rh	102.9	102.9	24875	2255	0.608
In	114.9	114.8	27768	2285	0.615
Ce	139.9	139.9	33849	2320	0.631
Pb	206.0	206.0	49939	2485	0.628
Pb	207.0	207.0	50101	2400	0.596
Pb	208.0	208.0	50448	2480	0.675
U	238.1	238.0	57686	2500	0.623

ICPMS#4 - Summary Report

Sample ID: Blank
 Sample Date/Time: Monday, April 12, 2010 02:43:35
 Sample Type:
 Sample Description:
 Number of Replicates: 3
 Batch ID:
 Method File: c:\elandata\Method\6020.mth
 Dataset File: c:\elandata\Dataset\100408\Blank.550

Concentration Results

Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Li 7		ug/L		30	
Be 9		ug/L		6	
B 11		ug/L		106	
Na 23		ug/L		11005	
Mg 24		ug/L		667	
Al 27		ug/L		667	
P 31		ug/L		2927	
K 39		ug/L		381369	
Ca 43		ug/L		201	
> Sc 45		ug/L		644697	
Ti 47		ug/L		173	
V 51		ug/L		20411	
Cr 52		ug/L		-11274	
Cr 53		ug/L		126123	
Mn 55		ug/L		733	
Fe 57		ug/L		5468	
Co 59		ug/L		148	
Ni 60		ug/L		69	
Cu 63		ug/L		2622	
Cu 65		ug/L		1333	
Zn 66		ug/L		1259	
Zn 67		ug/L		7250	
Zn 68		ug/L		1418	
> Ge 74		ug/L		260111	
As 75		ug/L		74	
Se 77		ug/L		5357	
Se 82		ug/L		30	
Kr 83		ug/L		58	
Sr 88		ug/L		181	
Y 89		ug/L		25	
Zr 90		ug/L		545	
Mo 98		ug/L		492	
Ag 107		ug/L		176	
Cd 111		ug/L		22	
Cd 114		ug/L		34	
> In 115		ug/L		163380	
Sn 120		ug/L		1034	
Sb 121		ug/L		688	
Sb 123		ug/L		540	
Ba 135		ug/L		22	
Ba 137		ug/L		31	
Ho 165		ug/L		10	
> Lu 175		ug/L		193728	
Tl 205		ug/L		1200	
Pb 208		ug/L		4306	
Th 232		ug/L		1376	
U 238		ug/L		597	

Sample ID: Blank
 Report Date/Time: Monday, April 12, 2010 02:46:20
 Page 1

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Li	7Linear Thru Zero	1.0000
Be	9Linear Thru Zero	1.0000
B	11Linear Thru Zero	1.0000
Na	23Linear Thru Zero	1.0000
Mg	24Linear Thru Zero	0.9999
Al	27Linear Thru Zero	1.0000
P	31Linear Thru Zero	1.0000
K	39Linear Thru Zero	1.0000
Ca	43Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ti	47Linear Thru Zero	1.0000
V	51Linear Thru Zero	1.0000
Cr	52Linear Thru Zero	1.0000
Cr	53Linear Thru Zero	
Mn	55Linear Thru Zero	1.0000
Fe	57Linear Thru Zero	1.0000
Co	59Linear Thru Zero	1.0000
Ni	60Linear Thru Zero	1.0000
Cu	63Linear Thru Zero	
Cu	65Linear Thru Zero	1.0000
Zn	66Linear Thru Zero	1.0000
Zn	67Linear Thru Zero	
Zn	68Linear Thru Zero	
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	0.9998
Kr	83Linear Thru Zero	
Sr	88Linear Thru Zero	1.0000
Y	89Linear Thru Zero	
Zr	90Linear Thru Zero	1.0000
Mo	98Linear Thru Zero	1.0000
Ag	107Linear Thru Zero	1.0000
Cd	111Linear Thru Zero	1.0000
Cd	114Linear Thru Zero	
In	115Linear Thru Zero	
Sn	120Linear Thru Zero	1.0000
Sb	121Linear Thru Zero	0.9998
Sb	123Linear Thru Zero	
Ba	135Linear Thru Zero	
Ba	137Linear Thru Zero	1.0000
Ho	165Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000
Pb	208Linear Thru Zero	1.0000
Th	232Linear Thru Zero	1.0000
U	238Linear Thru Zero	1.0000

Sample ID: Blank

Report Date/Time: Monday, April 12, 2010 02:46:20

Page 2

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Diff	Dup. Rel. % Diff
Li	7					
Be	9					
B	11					
Na	23					
Mg	24					
Al	27					
P	31					
K	39					
Ca	43					
> Sc	45					
Ti	47					
V	51					
Cr	52					
Cr	53					
Mn	55					
Fe	57					
Co	59					
Ni	60					
Cu	63					
Cu	65					
Zn	66					
Zn	67					
Zn	68					
> Ge	74					
As	75					
Se	77					
Se	82					
Kr	83					
Sr	88					
Y	89					
Zr	90					
Mo	98					
Ag	107					
Cd	111					
Cd	114					
> In	115					
Sn	120					
Sb	121					
Sb	123					
Ba	135					
Ba	137					
Ho	165					
> Lu	175					
Tl	205					
Pb	208					
Th	232					
U	238					

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message

QC Action

QC Action Line: No QC out of limits detected

ICPMS#4 - Summary Report

Sample ID: Standard 1

Sample Date/Time: Monday, April 12, 2010 02:49:43

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\6020.mth

Dataset File: c:\elandata\Dataset\100408\Standard 1.551

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Li	7	10.000	ug/L	3.051	5935	0.009
Be	9	10.000	ug/L	4.857	1595	0.002
B	11	20.000	ug/L	1.032	2923	0.004
Na	23	1000.000	ug/L	1.999	1740656	2.642
Mg	24	1000.000	ug/L	8.623	1174149	1.795
Al	27	1000.000	ug/L	3.071	1820390	2.781
P	31	1000.000	ug/L	3.608	101079	0.150
K	39	1000.000	ug/L	1.998	3185175	4.275
Ca	43	1000.000	ug/L	4.116	6423	0.010
Sc	45		ug/L		654559	654559.347
Ti	47	10.000	ug/L	4.296	3283	0.005
V	51	10.000	ug/L	12.650	56767	0.055
Cr	52	10.000	ug/L	3.946	19505	0.047
Cr	53		ug/L		128000	-0.000
Mn	55	10.000	ug/L	2.286	52707	0.079
Fe	57	1000.000	ug/L	2.969	111440	0.162
Co	59	10.000	ug/L	1.793	40361	0.061
Ni	60	10.000	ug/L	1.788	8627	0.013
Cu	63		ug/L		22243	0.030
Cu	65	10.000	ug/L	2.163	10815	0.014
Zn	66	10.000	ug/L	2.423	6694	0.021
Zn	67		ug/L		8080	0.003
Zn	68		ug/L		5377	0.015
Ge	74		ug/L		261149	261148.613
As	75	10.000	ug/L	8.084	6208	0.023
Se	77		ug/L		5552	0.001
Se	82	10.000	ug/L	8.766	527	0.002
Kr	83		ug/L		47	-0.000
Sr	88	10.000	ug/L	1.355	90477	0.544
Y	89		ug/L		27	0.000
Zr	90	10.000	ug/L	2.578	48629	0.289
Mo	98	10.000	ug/L	1.619	21857	0.129
Ag	107	10.000	ug/L	1.159	34952	0.209
Cd	111	10.000	ug/L	2.337	8067	0.048
Cd	114		ug/L		18844	0.113
In	115		ug/L		166132	166132.045
Sn	120	10.000	ug/L	2.971	36935	0.216
Sb	121	10.000	ug/L	14.028	20495	0.119
Sb	123		ug/L		15889	0.092
Ba	135		ug/L		8654	0.044
Ba	137	10.000	ug/L	1.519	14860	0.076
Ho	165		ug/L		8	-0.000
Lu	175		ug/L		194979	194978.643
Tl	205	10.000	ug/L	2.570	54419	0.273
Pb	208	10.000	ug/L	1.852	108675	0.535
Th	232	10.000	ug/L	5.297	98720	0.499
U	238	10.000	ug/L	2.487	102344	0.522

Sample ID: Standard 1

Report Date/Time: Monday, April 12, 2010 02:52:26

Page 1

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Li	7Linear Thru Zero	1.0000
Be	9Linear Thru Zero	1.0000
B	11Linear Thru Zero	1.0000
Na	23Linear Thru Zero	1.0000
Mg	24Linear Thru Zero	1.0000
Al	27Linear Thru Zero	1.0000
P	31Linear Thru Zero	1.0000
K	39Linear Thru Zero	1.0000
Ca	43Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ti	47Linear Thru Zero	1.0000
V	51Linear Thru Zero	1.0000
Cr	52Linear Thru Zero	1.0000
Cr	53Linear Thru Zero	
Mn	55Linear Thru Zero	1.0000
Fe	57Linear Thru Zero	1.0000
Co	59Linear Thru Zero	1.0000
Ni	60Linear Thru Zero	1.0000
Cu	63Linear Thru Zero	
Cu	65Linear Thru Zero	1.0000
Zn	66Linear Thru Zero	1.0000
Zn	67Linear Thru Zero	
Zn	68Linear Thru Zero	
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	1.0000
Kr	83Linear Thru Zero	
Sr	88Linear Thru Zero	1.0000
Y	89Linear Thru Zero	
Zr	90Linear Thru Zero	1.0000
Mo	98Linear Thru Zero	1.0000
Ag	107Linear Thru Zero	1.0000
Cd	111Linear Thru Zero	1.0000
Cd	114Linear Thru Zero	
In	115Linear Thru Zero	
Sn	120Linear Thru Zero	1.0000
Sb	121Linear Thru Zero	1.0000
Sb	123Linear Thru Zero	
Ba	135Linear Thru Zero	
Ba	137Linear Thru Zero	1.0000
Ho	165Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000
Pb	208Linear Thru Zero	1.0000
Th	232Linear Thru Zero	1.0000
U	238Linear Thru Zero	1.0000

Sample ID: Standard 1

Report Date/Time: Monday, April 12, 2010 02:52:26

Page 2

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Diff	Dup. Ret. % Diff
Li	7					
Be	9					
B	11					
Na	23					
Mg	24					
Al	27					
P	31					
K	39					
Ca	43					
> Sc	45					
Ti	47					
V	51					
Cr	52					
Cr	53					
Mn	55					
Fe	57					
Co	59					
Ni	60					
Cu	63					
Cu	65					
Zn	66					
Zn	67					
Zn	68					
> Ge	74					
As	75					
Se	77					
Se	82					
Kr	83					
Sr	88					
Y	89					
Zr	90					
Mo	98					
Ag	107					
Cd	111					
Cd	114					
> In	115					
Sn	120					
Sb	121					
Sb	123					
Ba	135					
Ba	137					
Ho	165					
> Lu	175					
Tl	205					
Pb	208					
Th	232					
U	238					

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: Standard 1

Report Date/Time: Monday, April 12, 2010 02:52:26

Page 3

ICPMS#4 - Summary Report

Sample ID: Standard 2

Sample Date/Time: Monday, April 12, 2010 02:55:49

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\6020.mth

Dataset File: c:\elandata\Dataset\100408\Standard 2.552

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Li	7	100.043	ug/L	0.439	60123	0.094
Be	9	100.016	ug/L	1.767	15735	0.025
B	11	199.993	ug/L	2.069	27415	0.043
Na	23	9998.559	ug/L	6.984	16606589	26.045
Mg	24	10004.944	ug/L	7.452	12030390	18.889
Al	27	9994.146	ug/L	1.375	16728759	26.256
P	31	10002.874	ug/L	2.950	986658	1.544
K	39	10006.213	ug/L	7.965	29441031	45.615
Ca	43	10001.291	ug/L	1.812	61554	0.096
> Sc	45		ug/L		637156	637156.287
Ti	47	100.044	ug/L	2.048	31837	0.050
V	51	100.133	ug/L	3.174	425762	0.637
Cr	52	100.017	ug/L	2.105	295563	0.481
Cr	53		ug/L		135025	0.016
Mn	55	100.009	ug/L	0.471	511300	0.801
Fe	57	10000.551	ug/L	0.519	1042145	1.627
Co	59	100.006	ug/L	1.581	393820	0.618
Ni	60	100.008	ug/L	1.618	84080	0.132
Cu	63		ug/L		195407	0.303
Cu	65	100.012	ug/L	1.779	94538	0.146
Zn	66	100.038	ug/L	2.481	56600	0.216
Zn	67		ug/L		14629	0.029
Zn	68		ug/L		40772	0.154
> Ge	74		ug/L		256004	256003.543
As	75	100.077	ug/L	0.819	65273	0.255
Se	77		ug/L		8097	0.011
Se	82	100.192	ug/L	4.627	6065	0.024
Kr	83		ug/L		51	-0.000
Sr	88	100.039	ug/L	0.725	904536	5.660
Y	89		ug/L		111	0.001
Zr	90	100.062	ug/L	1.418	493543	3.086
Mo	98	100.050	ug/L	2.085	216739	1.354
Ag	107	100.018	ug/L	1.016	340746	2.132
Cd	111	100.046	ug/L	1.329	81144	0.508
Cd	114		ug/L		190957	1.195
> In	115		ug/L		159787	159786.951
Sn	120	100.038	ug/L	2.506	359769	2.245
Sb	121	100.233	ug/L	9.698	249424	1.557
Sb	123		ug/L		191456	1.195
Ba	135		ug/L		86191	0.451
Ba	137	100.034	ug/L	1.151	150414	0.787
Ho	165		ug/L		12	0.000
> Lu	175		ug/L		190991	190990.522
Tl	205	100.015	ug/L	1.434	530708	2.772
Pb	208	100.000	ug/L	1.919	1026701	5.354
Th	232	100.079	ug/L	0.786	1037671	5.426
U	238	100.010	ug/L	1.602	1007913	5.275

Sample ID: Standard 2

Report Date/Time: Monday, April 12, 2010 02:58:32

Page 1

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Li	7Linear Thru Zero	1.0000
Be	9Linear Thru Zero	1.0000
B	11Linear Thru Zero	1.0000
Na	23Linear Thru Zero	1.0000
Mg	24Linear Thru Zero	1.0000
Al	27Linear Thru Zero	1.0000
P	31Linear Thru Zero	1.0000
K	39Linear Thru Zero	1.0000
Ca	43Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ti	47Linear Thru Zero	1.0000
V	51Linear Thru Zero	0.9999
Cr	52Linear Thru Zero	1.0000
Cr	53Linear Thru Zero	
Mn	55Linear Thru Zero	1.0000
Fe	57Linear Thru Zero	1.0000
Co	59Linear Thru Zero	1.0000
Ni	60Linear Thru Zero	1.0000
Cu	63Linear Thru Zero	
Cu	65Linear Thru Zero	1.0000
Zn	66Linear Thru Zero	1.0000
Zn	67Linear Thru Zero	
Zn	68Linear Thru Zero	
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	0.9998
Kr	83Linear Thru Zero	
Sr	88Linear Thru Zero	1.0000
Y	89Linear Thru Zero	
Zr	90Linear Thru Zero	1.0000
Mo	98Linear Thru Zero	1.0000
Ag	107Linear Thru Zero	1.0000
Cd	111Linear Thru Zero	1.0000
Cd	114Linear Thru Zero	
In	115Linear Thru Zero	
Sn	120Linear Thru Zero	1.0000
Sb	121Linear Thru Zero	0.9997
Sb	123Linear Thru Zero	
Ba	135Linear Thru Zero	
Ba	137Linear Thru Zero	1.0000
Ho	165Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000
Pb	208Linear Thru Zero	1.0000
Th	232Linear Thru Zero	1.0000
U	238Linear Thru Zero	1.0000

Sample ID: Standard 2

Report Date/Time: Monday, April 12, 2010 02:58:32

Page 2

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Diff	Dup. Rel. % Diff
Li	7					
Be	9					
B	11					
Na	23					
Mg	24					
Al	27					
P	31					
K	39					
Ca	43					
> Sc	45					
Ti	47					
V	51					
Cr	52					
Cr	53					
Mn	55					
Fe	57					
Co	59					
Ni	60					
Cu	63					
Cu	65					
Zn	66					
Zn	67					
Zn	68					
> Ge	74					
As	75					
Se	77					
Se	82					
Kr	83					
Sr	88					
Y	89					
Zr	90					
Mo	98					
Ag	107					
Cd	111					
Cd	114					
> In	115					
Sn	120					
Sb	121					
Sb	123					
Ba	135					
Ba	137					
Ho	165					
> Lu	175					
Tl	205					
Pb	208					
Th	232					
U	238					

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: Standard 2

Report Date/Time: Monday, April 12, 2010 02:58:32

Page 3

ICPMS#4 - Summary Report

Sample ID: QC Std 1

Sample Date/Time: Monday, April 12, 2010 03:01:55

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\6020.mth

Dataset File: c:\elandata\Dataset\100408\QC Std 1.553

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Li	7	52.295	ug/L	1.620	31254	0.049
Be	9	51.774	ug/L	1.574	8100	0.013
B	11	104.630	ug/L	4.252	14304	0.022
Na	23	5284.399	ug/L	1.908	8728570	13.765
Mg	24	5032.256	ug/L	2.318	6019199	9.500
Al	27	5458.305	ug/L	5.797	9080269	14.340
P	31	5042.371	ug/L	1.568	495924	0.778
K	39	4840.904	ug/L	7.678	14347844	22.068
Ca	43	4938.767	ug/L	0.125	30322	0.048
Sc	45		ug/L		633444	633444.181
Ti	47	50.496	ug/L	0.981	16061	0.025
V	51	52.167	ug/L	3.233	230100	0.332
Cr	52	52.279	ug/L	1.755	148300	0.252
Cr	53		ug/L		118451	-0.009
Mn	55	53.290	ug/L	1.211	271172	0.427
Fe	57	5007.240	ug/L	2.835	521311	0.815
Co	59	51.068	ug/L	2.686	199962	0.316
Ni	60	53.284	ug/L	1.085	44568	0.070
Cu	63		ug/L		103227	0.159
Cu	65	51.977	ug/L	1.526	49475	0.076
Zn	66	50.976	ug/L	1.360	29850	0.110
Zn	67		ug/L		10442	0.012
Zn	68		ug/L		22024	0.079
Ge	74		ug/L		259504	259503.868
As	75	51.099	ug/L	1.198	33820	0.130
Se	77		ug/L		6231	0.003
Se	82	52.015	ug/L	5.531	3207	0.012
Kr	83		ug/L		56	-0.000
Sr	88	50.999	ug/L	0.504	466334	2.885
Y	89		ug/L		39	0.000
Zr	90	49.508	ug/L	2.996	247116	1.527
Mo	98	50.341	ug/L	2.496	110503	0.681
Ag	107	51.627	ug/L	2.782	177887	1.100
Cd	111	51.230	ug/L	2.371	42017	0.260
Cd	114		ug/L		98373	0.609
In	115		ug/L		161562	161562.371
Sn	120	50.250	ug/L	2.579	183203	1.128
Sb	121	62.455	ug/L	3.564	157343	0.970
Sb	123		ug/L		121103	0.746
Ba	135		ug/L		43786	0.227
Ba	137	49.487	ug/L	1.900	75116	0.390
Ho	165		ug/L		15	0.000
Lu	175		ug/L		192786	192785.530
Tl	205	49.958	ug/L	1.568	268133	1.385
Pb	208	51.312	ug/L	2.257	533798	2.747
Th	232	50.861	ug/L	1.455	532958	2.758
U	238	53.818	ug/L	2.203	547709	2.838

Sample ID: QC Std 1

Report Date/Time: Monday, April 12, 2010 03:04:38

Page 1

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Li	7Linear Thru Zero	1.0000
Be	9Linear Thru Zero	1.0000
B	11Linear Thru Zero	1.0000
Na	23Linear Thru Zero	1.0000
Mg	24Linear Thru Zero	1.0000
Al	27Linear Thru Zero	1.0000
P	31Linear Thru Zero	1.0000
K	39Linear Thru Zero	1.0000
Ca	43Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ti	47Linear Thru Zero	1.0000
V	51Linear Thru Zero	0.9999
Cr	52Linear Thru Zero	1.0000
Cr	53Linear Thru Zero	
Mn	55Linear Thru Zero	1.0000
Fe	57Linear Thru Zero	1.0000
Co	59Linear Thru Zero	1.0000
Ni	60Linear Thru Zero	1.0000
Cu	63Linear Thru Zero	
Cu	65Linear Thru Zero	1.0000
Zn	66Linear Thru Zero	1.0000
Zn	67Linear Thru Zero	
Zn	68Linear Thru Zero	
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	0.9998
Kr	83Linear Thru Zero	
Sr	88Linear Thru Zero	1.0000
Y	89Linear Thru Zero	
Zr	90Linear Thru Zero	1.0000
Mo	98Linear Thru Zero	1.0000
Ag	107Linear Thru Zero	1.0000
Cd	111Linear Thru Zero	1.0000
Cd	114Linear Thru Zero	
In	115Linear Thru Zero	
Sn	120Linear Thru Zero	1.0000
Sb	121Linear Thru Zero	0.9997
Sb	123Linear Thru Zero	
Ba	135Linear Thru Zero	
Ba	137Linear Thru Zero	1.0000
Ho	165Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000
Pb	208Linear Thru Zero	1.0000
Th	232Linear Thru Zero	1.0000
U	238Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Diff	Dup. Rel. % Diff
Li	7	104.590				
Be	9	103.549				
B	11	104.630				
Na	23	105.688				
Mg	24	100.645				
Al	27	108.085				
P	31	100.847				
K	39	96.818				
Ca	43	98.775				
> Sc	45		98.3			
Ti	47	100.991				
V	51	104.333				
Cr	52	104.558				
Cr	53					
Mn	55	106.580				
Fe	57	100.145				
Co	59	102.135				
Ni	60	106.568				
Cu	63					
Cu	65	103.953				
Zn	66	101.952				
Zn	67					
Zn	68					
> Ge	74		99.8			
As	75	102.199				
Se	77					
Se	82	104.030				
Kr	83					
Sr	88	101.997				
Y	89					
Zr	90	99.015				
Mo	98	100.683				
Ag	107	103.254				
Cd	111	102.461				
Cd	114					
> In	115		98.9			
Sn	120	100.500				
Sb	121	124.909				
Sb	123					
Ba	135					
Ba	137	98.975				
Ho	165					
> Lu	175		99.5			
Tl	205	99.915				
Pb	208	102.623				
Th	232	101.722				
U	238	107.636				

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message
 QC Std 1 Sb 121ICV is out of limits (+/- 10%)

QC Action

QC Action Line: Continue

ICPMS#4 - Summary Report

Sample ID: QC Std 2

Sample Date/Time: Monday, April 12, 2010 03:08:04

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\6020.mth

Dataset File: c:\elandata\Dataset\100408\QC Std 2.554

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Li	7	0.030	ug/L	9.690	48	0.000
Be	9	0.013	ug/L	29.920	8	0.000
B	11	1.862	ug/L	15.533	362	0.000
Na	23	-1.575	ug/L	79.664	8336	-0.004
Mg	24	1.650	ug/L	29.230	2667	0.003
Al	27	2.571	ug/L	80.004	5001	0.007
P	31	6.300	ug/L	13.671	3545	0.001
K	39	-4.920	ug/L	149.211	365972	-0.022
Ca	43	1.480	ug/L	96.252	209	0.000
Sc	45		ug/L		643091	643091.349
Ti	47	0.043	ug/L	212.623	186	0.000
V	51	-1.289	ug/L	31.094	15092	-0.008
Cr	52	0.008	ug/L	482.794	-11219	0.000
Cr	53		ug/L		122896	-0.005
Mn	55	-0.001	ug/L	496.489	724	-0.000
Fe	57	2.296	ug/L	85.205	5695	0.000
Co	59	0.008	ug/L	32.969	179	0.000
Ni	60	0.012	ug/L	117.899	80	0.000
Cu	63		ug/L		2753	0.000
Cu	65	-0.063	ug/L	153.288	1271	-0.000
Zn	66	-0.055	ug/L	37.738	1230	-0.000
Zn	67		ug/L		7100	-0.001
Zn	68		ug/L		1455	0.000
Ge	74		ug/L		260464	260464.089
As	75	0.142	ug/L	195.892	167	0.000
Se	77		ug/L		5206	-0.001
Se	82	1.677	ug/L	19.930	133	0.000
Kr	83		ug/L		52	-0.000
Sr	88	0.010	ug/L	42.279	273	0.001
Y	89		ug/L		21	-0.000
Zr	90	0.234	ug/L	15.682	1714	0.007
Mo	98	0.505	ug/L	12.312	1599	0.007
Ag	107	0.068	ug/L	16.945	412	0.001
Cd	111	0.002	ug/L	813.349	23	0.000
Cd	114		ug/L		79	0.000
In	115		ug/L		162474	162473.993
Sn	120	0.143	ug/L	9.388	1549	0.003
Sb	121	2.377	ug/L	15.275	6684	0.037
Sb	123		ug/L		5197	0.029
Ba	135		ug/L		29	0.000
Ba	137	0.013	ug/L	39.855	50	0.000
Ho	165		ug/L		8	-0.000
Lu	175		ug/L		193703	193703.050
Tl	205	0.252	ug/L	31.990	2554	0.007
Pb	208	0.014	ug/L	65.656	4455	0.001
Th	232	0.382	ug/L	23.171	5390	0.021
U	238	0.022	ug/L	58.185	824	0.001

Sample ID: QC Std 2

Report Date/Time: Monday, April 12, 2010 03:10:49

Page 1

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Li	7Linear Thru Zero	1.0000
Be	9Linear Thru Zero	1.0000
B	11Linear Thru Zero	1.0000
Na	23Linear Thru Zero	1.0000
Mg	24Linear Thru Zero	1.0000
Al	27Linear Thru Zero	1.0000
P	31Linear Thru Zero	1.0000
K	39Linear Thru Zero	1.0000
Ca	43Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ti	47Linear Thru Zero	1.0000
V	51Linear Thru Zero	0.9999
Cr	52Linear Thru Zero	1.0000
Cr	53Linear Thru Zero	
Mn	55Linear Thru Zero	1.0000
Fe	57Linear Thru Zero	1.0000
Co	59Linear Thru Zero	1.0000
Ni	60Linear Thru Zero	1.0000
Cu	63Linear Thru Zero	
Cu	65Linear Thru Zero	1.0000
Zn	66Linear Thru Zero	1.0000
Zn	67Linear Thru Zero	
Zn	68Linear Thru Zero	
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	0.9998
Kr	83Linear Thru Zero	
Sr	88Linear Thru Zero	1.0000
Y	89Linear Thru Zero	
Zr	90Linear Thru Zero	1.0000
Mo	98Linear Thru Zero	1.0000
Ag	107Linear Thru Zero	1.0000
Cd	111Linear Thru Zero	1.0000
Cd	114Linear Thru Zero	
In	115Linear Thru Zero	
Sn	120Linear Thru Zero	1.0000
Sb	121Linear Thru Zero	0.9997
Sb	123Linear Thru Zero	
Ba	135Linear Thru Zero	
Ba	137Linear Thru Zero	1.0000
Ho	165Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000
Pb	208Linear Thru Zero	1.0000
Th	232Linear Thru Zero	1.0000
U	238Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Diff	Dup. Rel. % Diff
Li	7					
Be	9					
B	11					
Na	23					
Mg	24					
Al	27					
P	31					
K	39					
Ca	43					
> Sc	45		99.8			
Ti	47					
V	51					
Cr	52					
Cr	53					
Mn	55					
Fe	57					
Co	59					
Ni	60					
Cu	63					
Cu	65					
Zn	66					
Zn	67					
Zn	68					
> Ge	74		100.1			
As	75					
Se	77					
Se	82					
Kr	83					
Sr	88					
Y	89					
Zr	90					
Mo	98					
Ag	107					
Cd	111					
Cd	114					
> In	115		99.4			
Sn	120					
Sb	121					
Sb	123					
Ba	135					
Ba	137					
Ho	165					
> Lu	175		100.0			
Tl	205					
Pb	208					
Th	232					
U	238					

QC Out Of Limits

Measurement Type	Analyte	MassOut of Limits Message
QC Std 2	Mo	98ICB is out of limits (+/- PQL)

QC Action

QC Action Line: Continue

Sample ID: QC Std 2
 Report Date/Time: Monday, April 12, 2010 03:10:49
 Page 3

ICPMS#4 - Summary Report

Sample ID: QC Std 3

Sample Date/Time: Monday, April 12, 2010 03:14:14

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\6020.mth

Dataset File: c:\elandata\Dataset\100408\QC Std 3.555

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Li	7	12.092	ug/L	3.179	7134	0.011
Be	9	0.545	ug/L	10.831	89	0.000
B	11	17.874	ug/L	0.561	2490	0.004
Na	23	324.310	ug/L	14.215	537027	0.845
Mg	24	17.318	ug/L	17.973	21016	0.033
Al	27	35.927	ug/L	13.072	59458	0.094
P	31	54.701	ug/L	4.501	8094	0.008
K	39	351.702	ug/L	7.260	1367941	1.603
Ca	43	237.508	ug/L	3.197	1619	0.002
> Sc	45		ug/L		623258	623258.014
Ti	47	9.676	ug/L	2.209	3163	0.005
V	51	10.385	ug/L	4.501	60883	0.066
Cr	52	12.481	ug/L	0.723	26545	0.060
Cr	53		ug/L		104248	-0.028
Mn	55	6.177	ug/L	1.561	31559	0.049
Fe	57	117.906	ug/L	1.785	17243	0.019
Co	59	1.190	ug/L	2.162	4724	0.007
Ni	60	2.424	ug/L	2.223	2059	0.003
Cu	63		ug/L		4310	0.003
Cu	65	0.920	ug/L	13.308	2128	0.001
Zn	66	13.387	ug/L	0.745	8577	0.029
Zn	67		ug/L		6860	-0.001
Zn	68		ug/L		6551	0.020
> Ge	74		ug/L		253903	253902.525
As	75	5.344	ug/L	14.596	3530	0.014
Se	77		ug/L		4054	-0.005
Se	82	4.843	ug/L	14.657	319	0.001
Kr	83		ug/L		47	-0.000
Sr	88	11.935	ug/L	0.956	107622	0.675
Y	89		ug/L		19	-0.000
Zr	90	2.138	ug/L	3.509	11021	0.066
Mo	98	0.648	ug/L	3.093	1874	0.009
Ag	107	1.058	ug/L	3.086	3758	0.023
Cd	111	1.190	ug/L	4.891	983	0.006
Cd	114		ug/L		2316	0.014
> In	115		ug/L		159116	159116.444
Sn	120	5.660	ug/L	0.405	21221	0.127
Sb	121	2.646	ug/L	7.952	7208	0.041
Sb	123		ug/L		5584	0.032
Ba	135		ug/L		1967	0.010
Ba	137	2.325	ug/L	1.416	3453	0.018
Ho	165		ug/L		9	-0.000
> Lu	175		ug/L		187029	187029.060
Tl	205	1.143	ug/L	2.392	7085	0.032
Pb	208	2.316	ug/L	1.549	27345	0.124
Th	232	1.141	ug/L	2.913	12905	0.062
U	238	0.290	ug/L	2.865	3435	0.015

Sample ID: QC Std 3

Report Date/Time: Monday, April 12, 2010 03:16:57

Page 1

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Li	7Linear Thru Zero	1.0000
Be	9Linear Thru Zero	1.0000
B	11Linear Thru Zero	1.0000
Na	23Linear Thru Zero	1.0000
Mg	24Linear Thru Zero	1.0000
Al	27Linear Thru Zero	1.0000
P	31Linear Thru Zero	1.0000
K	39Linear Thru Zero	1.0000
Ca	43Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ti	47Linear Thru Zero	1.0000
V	51Linear Thru Zero	0.9999
Cr	52Linear Thru Zero	1.0000
Cr	53Linear Thru Zero	
Mn	55Linear Thru Zero	1.0000
Fe	57Linear Thru Zero	1.0000
Co	59Linear Thru Zero	1.0000
Ni	60Linear Thru Zero	1.0000
Cu	63Linear Thru Zero	
Cu	65Linear Thru Zero	1.0000
Zn	66Linear Thru Zero	1.0000
Zn	67Linear Thru Zero	
Zn	68Linear Thru Zero	
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	0.9998
Kr	83Linear Thru Zero	
Sr	88Linear Thru Zero	1.0000
Y	89Linear Thru Zero	
Zr	90Linear Thru Zero	1.0000
Mo	98Linear Thru Zero	1.0000
Ag	107Linear Thru Zero	1.0000
Cd	111Linear Thru Zero	1.0000
Cd	114Linear Thru Zero	
In	115Linear Thru Zero	
Sn	120Linear Thru Zero	1.0000
Sb	121Linear Thru Zero	0.9997
Sb	123Linear Thru Zero	
Ba	135Linear Thru Zero	
Ba	137Linear Thru Zero	1.0000
Ho	165Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000
Pb	208Linear Thru Zero	1.0000
Th	232Linear Thru Zero	1.0000
U	238Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Diff	Dup. Rel. % Diff
Li	7	120.918				
Be	9	108.989				
B	11	119.160				
Na	23	129.724				
Mg	24	115.455				
Al	27	119.757				
P	31	109.402				
K	39	117.234				
Ca	43	118.754				
> Sc	45		96.7			
Ti	47	96.756				
V	51	103.849				
Cr	52	124.814				
Cr	53					
Mn	55	123.546				
Fe	57	117.906				
Co	59	118.979				
Ni	60	121.205				
Cu	63					
L Cu	65	91.982				
Zn	66	133.866				
Zn	67					
Zn	68					
> Ge	74		97.6			
As	75	106.888				
Se	77					
Se	82	96.865				
Kr	83					
Sr	88	119.347				
Y	89					
Zr	90	106.915				
Mo	98	129.619				
Ag	107	105.774				
Cd	111	119.030				
Cd	114					
> In	115		97.4			
Sn	120	113.206				
Sb	121	88.208				
L Sb	123					
Ba	135					
Ba	137	116.245				
Ho	165					
> Lu	175		96.5			
Tl	205	114.348				
Pb	208	115.800				
Th	232	114.134				
L U	238	144.898				

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
QC Std 3	Zn	66	CRDL is out of limits
QC Std 3	U	238	CRDL is out of limits

QC Action

QC Action Line: Continue

Sample ID: QC Std 3

Report Date/Time: Monday, April 12, 2010 03:16:57

Page 3

ICPMS#4 - Summary Report

Sample ID: QC Std 4

Sample Date/Time: Monday, April 12, 2010 03:20:21

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\6020.mth

Dataset File: c:\elandata\Dataset\100408\QC Std 4.556

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Li	7	0.104	ug/L	43.708	92	0.000
Be	9	0.135	ug/L	19.636	27	0.000
B	11	1.106	ug/L	15.745	256	0.000
Na	23	96448.705	ug/L	4.239	160325276	251.232
Mg	24	93854.896	ug/L	2.143	113091539	177.190
Al	27	92569.880	ug/L	2.132	155212821	243.196
P	31	89883.826	ug/L	3.067	8857623	13.877
K	39	92229.964	ug/L	2.230	268695995	420.444
Ca	43	94558.095	ug/L	3.448	581225	0.911
> Sc	45		ug/L		638350	638349.584
Ti	47	1564.928	ug/L	1.470	496414	0.778
V	51	-1.084	ug/L	117.800	15753	-0.007
Cr	52	2.343	ug/L	0.348	-3962	0.011
Cr	53		ug/L		116150	-0.014
Mn	55	5.810	ug/L	1.855	30437	0.047
Fe	57	96382.179	ug/L	3.090	10012270	15.682
Co	59	0.221	ug/L	5.806	1017	0.001
Ni	60	3.297	ug/L	5.866	2841	0.004
Cu	63		ug/L		8204	0.009
Cu	65	3.191	ug/L	5.911	4298	0.005
Zn	66	5.452	ug/L	2.046	4245	0.012
Zn	67		ug/L		8283	0.005
Zn	68		ug/L		2553	0.005
> Ge	74		ug/L		255306	255305.878
As	75	0.972	ug/L	82.383	702	0.002
Se	77		ug/L		6317	0.004
Se	82	0.600	ug/L	102.228	66	0.000
Kr	83		ug/L		147	0.000
Sr	88	2.893	ug/L	2.580	25999	0.164
Y	89		ug/L		257	0.001
Zr	90	0.867	ug/L	40.756	4753	0.027
Mo	98	2048.514	ug/L	1.785	4373026	27.713
Ag	107	0.106	ug/L	6.000	528	0.002
Cd	111	0.235	ug/L	75.167	209	0.001
Cd	114		ug/L		4885	0.031
> In	115		ug/L		157776	157776.284
Sn	120	1.185	ug/L	3.018	5192	0.027
Sb	121	1.543	ug/L	25.456	4449	0.024
Sb	123		ug/L		3493	0.019
Ba	135		ug/L		664	0.003
Ba	137	0.686	ug/L	5.219	1080	0.005
Ho	165		ug/L		3895	0.020
> Lu	175		ug/L		194389	194388.596
Tl	205	-0.037	ug/L	20.758	1004	-0.001
Pb	208	0.207	ug/L	4.496	6476	0.011
Th	232	0.390	ug/L	37.137	5482	0.021
U	238	-0.024	ug/L	106.922	356	-0.001

Sample ID: QC Std 4

Report Date/Time: Monday, April 12, 2010 03:23:05

Page 1

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Li	7Linear Thru Zero	1.0000
Be	9Linear Thru Zero	1.0000
B	11Linear Thru Zero	1.0000
Na	23Linear Thru Zero	1.0000
Mg	24Linear Thru Zero	1.0000
Al	27Linear Thru Zero	1.0000
P	31Linear Thru Zero	1.0000
K	39Linear Thru Zero	1.0000
Ca	43Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ti	47Linear Thru Zero	1.0000
V	51Linear Thru Zero	0.9999
Cr	52Linear Thru Zero	1.0000
Cr	53Linear Thru Zero	
Mn	55Linear Thru Zero	1.0000
Fe	57Linear Thru Zero	1.0000
Co	59Linear Thru Zero	1.0000
Ni	60Linear Thru Zero	1.0000
Cu	63Linear Thru Zero	
Cu	65Linear Thru Zero	1.0000
Zn	66Linear Thru Zero	1.0000
Zn	67Linear Thru Zero	
Zn	68Linear Thru Zero	
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	0.9998
Kr	83Linear Thru Zero	
Sr	88Linear Thru Zero	1.0000
Y	89Linear Thru Zero	
Zr	90Linear Thru Zero	1.0000
Mo	98Linear Thru Zero	1.0000
Ag	107Linear Thru Zero	1.0000
Cd	111Linear Thru Zero	1.0000
Cd	114Linear Thru Zero	
In	115Linear Thru Zero	
Sn	120Linear Thru Zero	1.0000
Sb	121Linear Thru Zero	0.9997
Sb	123Linear Thru Zero	
Ba	135Linear Thru Zero	
Ba	137Linear Thru Zero	1.0000
Ho	165Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000
Pb	208Linear Thru Zero	1.0000
Th	232Linear Thru Zero	1.0000
U	238Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Diff	Dup. Rel. % Diff
Li	7					
Be	9					
B	11					
Na	23	96.449				
Mg	24	93.855				
Al	27	92.570				
P	31	89.884				
K	39	92.230				
Ca	43	94.558				
> Sc	45		99.0			
Ti	47	78.246				
V	51					
Cr	52	71.012				
Cr	53					
Mn	55	100.174				
Fe	57	96.382				
Co	59	94.057				
Ni	60	99.597				
Cu	63					
Cu	65	95.541				
Zn	66	145.012				
Zn	67					
Zn	68					
> Ge	74		98.2			
As	75					
Se	77					
Se	82					
Kr	83					
Sr	88	97.750				
Y	89					
Zr	90					
Mo	98	102.426				
Ag	107					
Cd	111	52.946				
Cd	114					
> In	115		96.6			
Sn	120					
Sb	121					
Sb	123					
Ba	135					
Ba	137	85.906				
Ho	165					
> Lu	175		100.3			
Tl	205					
Pb	208	109.531				
Th	232					
U	238					

QC Out Of Limits

Measurement Type	Analyte	MassOut of Limits Message
QC Std 4	Ti	47ICSA is out of limits

QC Action

QC Action Line: Continue

ICPMS#4 - Summary Report

Sample ID: QC Std 5

Sample Date/Time: Monday, April 12, 2010 03:26:29

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\6020.mth

Dataset File: c:\elandata\Dataset\100408\QC Std 5.557

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Li	7	17.926	ug/L	0.270	10900	0.017
Be	9	17.899	ug/L	1.814	2847	0.004
B	11	17.969	ug/L	2.873	2582	0.004
Na	23	99229.137	ug/L	1.560	166286490	258.475
Mg	24	91729.458	ug/L	2.978	111383208	173.178
Al	27	90157.485	ug/L	4.608	152298026	236.858
P	31	90232.131	ug/L	1.578	8962661	13.930
K	39	100068.116	ug/L	5.956	293664971	456.176
Ca	43	94672.344	ug/L	1.747	586606	0.912
> Sc	45		ug/L		643236	643235.606
Ti	47	1597.247	ug/L	2.850	510537	0.794
V	51	18.667	ug/L	6.453	96664	0.119
Cr	52	21.852	ug/L	3.906	56392	0.105
Cr	53		ug/L		125355	-0.001
Mn	55	25.389	ug/L	0.905	131579	0.203
Fe	57	97420.346	ug/L	1.310	10200950	15.851
Co	59	19.164	ug/L	2.849	76290	0.118
Ni	60	22.085	ug/L	1.833	18797	0.029
Cu	63		ug/L		44508	0.065
Cu	65	21.985	ug/L	1.043	22019	0.032
Zn	66	22.617	ug/L	2.452	13997	0.049
Zn	67		ug/L		10070	0.011
Zn	68		ug/L		9469	0.031
> Ge	74		ug/L		260493	260493.142
As	75	19.783	ug/L	6.566	13191	0.050
Se	77		ug/L		7667	0.009
Se	82	20.733	ug/L	4.100	1301	0.005
Kr	83		ug/L		143	0.000
Sr	88	23.013	ug/L	1.357	211807	1.302
Y	89		ug/L		273	0.002
Zr	90	20.009	ug/L	3.040	100805	0.617
Mo	98	2044.049	ug/L	4.536	4493389	27.653
Ag	107	18.872	ug/L	2.287	65541	0.402
Cd	111	18.952	ug/L	4.475	15648	0.096
Cd	114		ug/L		40425	0.249
> In	115		ug/L		162558	162558.022
Sn	120	19.777	ug/L	2.159	73169	0.444
Sb	121	21.342	ug/L	6.872	54535	0.331
Sb	123		ug/L		42004	0.255
Ba	135		ug/L		17393	0.089
Ba	137	19.595	ug/L	1.396	30272	0.154
Ho	165		ug/L		4037	0.021
> Lu	175		ug/L		196073	196073.033
Tl	205	17.701	ug/L	0.937	97424	0.491
Pb	208	18.513	ug/L	0.697	198700	0.991
Th	232	19.059	ug/L	0.712	204004	1.033
U	238	19.999	ug/L	1.272	207403	1.055

Sample ID: QC Std 5

Report Date/Time: Monday, April 12, 2010 03:29:13

Page 1

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Li	7Linear Thru Zero	1.0000
Be	9Linear Thru Zero	1.0000
B	11Linear Thru Zero	1.0000
Na	23Linear Thru Zero	1.0000
Mg	24Linear Thru Zero	1.0000
Al	27Linear Thru Zero	1.0000
P	31Linear Thru Zero	1.0000
K	39Linear Thru Zero	1.0000
Ca	43Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ti	47Linear Thru Zero	1.0000
V	51Linear Thru Zero	0.9999
Cr	52Linear Thru Zero	1.0000
Cr	53Linear Thru Zero	
Mn	55Linear Thru Zero	1.0000
Fe	57Linear Thru Zero	1.0000
Co	59Linear Thru Zero	1.0000
Ni	60Linear Thru Zero	1.0000
Cu	63Linear Thru Zero	
Cu	65Linear Thru Zero	1.0000
Zn	66Linear Thru Zero	1.0000
Zn	67Linear Thru Zero	
Zn	68Linear Thru Zero	
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	0.9998
Kr	83Linear Thru Zero	
Sr	88Linear Thru Zero	1.0000
Y	89Linear Thru Zero	
Zr	90Linear Thru Zero	1.0000
Mo	98Linear Thru Zero	1.0000
Ag	107Linear Thru Zero	1.0000
Cd	111Linear Thru Zero	1.0000
Cd	114Linear Thru Zero	
In	115Linear Thru Zero	
Sn	120Linear Thru Zero	1.0000
Sb	121Linear Thru Zero	0.9997
Sb	123Linear Thru Zero	
Ba	135Linear Thru Zero	
Ba	137Linear Thru Zero	1.0000
Ho	165Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000
Pb	208Linear Thru Zero	1.0000
Th	232Linear Thru Zero	1.0000
U	238Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Diff	Dup. Rel. % Diff
Li	7	89.631				
Be	9	89.497				
B	11	89.847				
Na	23	99.229				
Mg	24	91.729				
Al	27	90.157				
P	31	90.232				
K	39	100.068				
Ca	43	94.672				
> Sc	45		99.8			
Ti	47	79.862				
V	51	93.335				
Cr	52	93.785				
Cr	53					
Mn	55	98.407				
Fe	57	97.420				
Co	59	94.706				
Ni	60	94.744				
Cu	63					
Cu	65	94.195				
Zn	66	95.189				
Zn	67					
Zn	68					
> Ge	74		100.1			
As	75	98.914				
Se	77					
Se	82	103.665				
Kr	83					
Sr	88	100.232				
Y	89					
Zr	90	100.046				
Mo	98	102.202				
Ag	107	94.361				
Cd	111	92.703				
Cd	114					
> In	115		99.5			
Sn	120	98.884				
Sb	121	106.710				
Sb	123					
Ba	135					
Ba	137	94.214				
Ho	165					
> Lu	175		101.2			
Tl	205	88.504				
Pb	208	91.698				
Th	232	95.296				
U	238	99.993				

QC Out Of Limits

Measurement Type	Analyte	MassOut of Limits Message
QC Std 5	Ti	47IC5AB is out of limits

QC Action

QC Action Line: Continue

ICPMS#4 - Summary Report

Sample ID: QC Std 6

Sample Date/Time: Monday, April 12, 2010 03:32:38

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\6020.mth

Dataset File: c:\elandata\Dataset\100408\QC Std 6.558

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Li	7	49.592	ug/L	1.555	30626	0.047
Be	9	49.022	ug/L	3.029	7924	0.012
B	11	98.787	ug/L	3.018	13962	0.021
Na	23	5255.300	ug/L	3.106	8971235	13.689
Mg	24	5073.394	ug/L	4.907	6267441	9.578
Al	27	5051.226	ug/L	2.011	8684608	13.270
P	31	4917.974	ug/L	1.255	499825	0.759
K	39	4861.454	ug/L	1.967	14889382	22.162
Ca	43	4848.567	ug/L	1.604	30757	0.047
> Sc	45		ug/L		654444	654443.829
Ti	47	52.142	ug/L	2.541	17127	0.026
V	51	50.453	ug/L	4.440	230632	0.321
Cr	52	52.131	ug/L	0.590	152781	0.251
Cr	53		ug/L		121797	-0.009
Mn	55	52.888	ug/L	1.546	278063	0.424
Fe	57	5088.821	ug/L	2.129	547355	0.828
Co	59	51.613	ug/L	1.504	208834	0.319
Ni	60	53.706	ug/L	0.959	46411	0.071
Cu	63		ug/L		109089	0.163
Cu	65	53.858	ug/L	1.179	52919	0.079
Zn	66	51.795	ug/L	2.776	31630	0.112
Zn	67		ug/L		10913	0.012
Zn	68		ug/L		23355	0.081
> Ge	74		ug/L		270833	270832.765
As	75	50.293	ug/L	0.456	34740	0.128
Se	77		ug/L		6844	0.005
Se	82	49.302	ug/L	2.574	3173	0.012
Kr	83		ug/L		53	-0.000
Sr	88	50.962	ug/L	1.769	479052	2.883
Y	89		ug/L		42	0.000
Zr	90	49.253	ug/L	2.767	252772	1.519
Mo	98	52.057	ug/L	3.849	117441	0.704
Ag	107	51.732	ug/L	0.923	183305	1.102
Cd	111	50.831	ug/L	2.368	42864	0.258
Cd	114		ug/L		100731	0.606
> In	115		ug/L		166118	166118.400
Sn	120	49.632	ug/L	1.852	186070	1.114
Sb	121	57.383	ug/L	4.521	148680	0.891
Sb	123		ug/L		114475	0.686
Ba	135		ug/L		44954	0.232
Ba	137	50.492	ug/L	1.834	76960	0.397
Ho	165		ug/L		14	0.000
> Lu	175		ug/L		193577	193577.415
Tl	205	50.309	ug/L	1.524	271126	1.395
Pb	208	51.343	ug/L	1.547	536368	2.749
Th	232	50.726	ug/L	1.060	533760	2.750
U	238	54.028	ug/L	1.100	552171	2.849

Sample ID: QC Std 6

Report Date/Time: Monday, April 12, 2010 03:35:22

Page 1

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Li	7Linear Thru Zero	1.0000
Be	9Linear Thru Zero	1.0000
B	11Linear Thru Zero	1.0000
Na	23Linear Thru Zero	1.0000
Mg	24Linear Thru Zero	1.0000
Al	27Linear Thru Zero	1.0000
P	31Linear Thru Zero	1.0000
K	39Linear Thru Zero	1.0000
Ca	43Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ti	47Linear Thru Zero	1.0000
V	51Linear Thru Zero	0.9999
Cr	52Linear Thru Zero	1.0000
Cr	53Linear Thru Zero	
Mn	55Linear Thru Zero	1.0000
Fe	57Linear Thru Zero	1.0000
Co	59Linear Thru Zero	1.0000
Ni	60Linear Thru Zero	1.0000
Cu	63Linear Thru Zero	
Cu	65Linear Thru Zero	1.0000
Zn	66Linear Thru Zero	1.0000
Zn	67Linear Thru Zero	
Zn	68Linear Thru Zero	
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	0.9998
Kr	83Linear Thru Zero	
Sr	88Linear Thru Zero	1.0000
Y	89Linear Thru Zero	
Zr	90Linear Thru Zero	1.0000
Mo	98Linear Thru Zero	1.0000
Ag	107Linear Thru Zero	1.0000
Cd	111Linear Thru Zero	1.0000
Cd	114Linear Thru Zero	
In	115Linear Thru Zero	
Sn	120Linear Thru Zero	1.0000
Sb	121Linear Thru Zero	0.9997
Sb	123Linear Thru Zero	
Ba	135Linear Thru Zero	
Ba	137Linear Thru Zero	1.0000
Ho	165Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000
Pb	208Linear Thru Zero	1.0000
Th	232Linear Thru Zero	1.0000
U	238Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Diff	Dup. Rel. % Diff
Li	7	99.185				
Be	9	98.044				
B	11	98.787				
Na	23	105.106				
Mg	24	101.468				
Al	27	100.024				
P	31	98.359				
K	39	97.229				
Ca	43	96.971				
> Sc	45		101.5			
Ti	47	104.284				
V	51	100.907				
Cr	52	104.262				
Cr	53					
Mn	55	105.776				
Fe	57	101.776				
Co	59	103.227				
Ni	60	107.412				
Cu	63					
Cu	65	107.716				
Zn	66	103.590				
Zn	67					
Zn	68					
> Ge	74		104.1			
As	75	100.585				
Se	77					
Se	82	98.604				
Kr	83					
Sr	88	101.924				
Y	89					
Zr	90	98.506				
Mo	98	104.115				
Ag	107	103.463				
Cd	111	101.662				
Cd	114					
> In	115		101.7			
Sn	120	99.265				
Sb	121	114.766				
Sb	123					
Ba	135					
Ba	137	100.985				
Ho	165					
> Lu	175		99.9			
Tl	205	100.617				
Pb	208	102.686				
Th	232	101.453				
U	238	108.056				

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message
 QC Std 6 Sb 121CCV is out of limits (+/- 10%)

QC Action

QC Action Line: Continue

ICPMS#4 - Summary Report

Sample ID: QC Std 7

Sample Date/Time: Monday, April 12, 2010 03:38:48

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\6020.mth

Dataset File: c:\elandata\Dataset\100408\QC Std 7.559

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Li	7	0.061	ug/L	9.246	68	0.000
Be	9	0.015	ug/L	95.491	8	0.000
B	11	1.025	ug/L	31.807	255	0.000
Na	23	4.830	ug/L	34.168	19680	0.013
Mg	24	3.971	ug/L	94.869	5668	0.007
Al	27	4.002	ug/L	35.500	7669	0.011
P	31	7.560	ug/L	27.925	3786	0.001
K	39	-3.637	ug/L	156.122	381367	-0.017
Ca	43	9.657	ug/L	71.987	268	0.000
Sc	45		ug/L		663073	663072.553
Ti	47	0.584	ug/L	6.487	370	0.000
V	51	-1.081	ug/L	164.553	16380	-0.007
Cr	52	0.242	ug/L	42.570	-10822	0.001
Cr	53		ug/L		123785	-0.009
Mn	55	0.001	ug/L	333.696	761	0.000
Fe	57	6.068	ug/L	23.706	6279	0.001
Co	59	0.008	ug/L	91.430	186	0.000
Ni	60	0.007	ug/L	202.126	77	0.000
Cu	63		ug/L		2695	-0.000
Cu	65	-0.028	ug/L	99.092	1344	-0.000
Zn	66	-0.410	ug/L	23.152	1059	-0.001
Zn	67		ug/L		7077	-0.001
Zn	68		ug/L		1239	-0.001
Ge	74		ug/L		267568	267567.613
As	75	1.207	ug/L	49.169	899	0.003
Se	77		ug/L		5882	0.001
Se	82	0.805	ug/L	41.251	82	0.000
Kr	83		ug/L		58	-0.000
Sr	88	0.009	ug/L	25.050	263	0.000
Y	89		ug/L		19	-0.000
Zr	90	0.134	ug/L	20.539	1222	0.004
Mo	98	0.646	ug/L	11.800	1925	0.009
Ag	107	0.043	ug/L	27.991	327	0.001
Cd	111	-0.006	ug/L	114.590	17	-0.000
Cd	114		ug/L		56	0.000
In	115		ug/L		164037	164036.764
Sn	120	0.097	ug/L	8.909	1393	0.002
Sb	121	1.242	ug/L	18.014	3850	0.019
Sb	123		ug/L		3075	0.015
Ba	135		ug/L		32	0.000
Ba	137	0.010	ug/L	85.996	47	0.000
Ho	165		ug/L		10	-0.000
Lu	175		ug/L		196361	196360.616
Tl	205	0.124	ug/L	26.657	1893	0.003
Pb	208	0.034	ug/L	22.706	4727	0.002
Th	232	0.203	ug/L	26.757	3559	0.011
U	238	0.033	ug/L	44.914	948	0.002

Sample ID: QC Std 7

Report Date/Time: Monday, April 12, 2010 03:41:33

Page 1

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Li	7Linear Thru Zero	1.0000
Be	9Linear Thru Zero	1.0000
B	11Linear Thru Zero	1.0000
Na	23Linear Thru Zero	1.0000
Mg	24Linear Thru Zero	1.0000
Al	27Linear Thru Zero	1.0000
P	31Linear Thru Zero	1.0000
K	39Linear Thru Zero	1.0000
Ca	43Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ti	47Linear Thru Zero	1.0000
V	51Linear Thru Zero	0.9999
Cr	52Linear Thru Zero	1.0000
Cr	53Linear Thru Zero	
Mn	55Linear Thru Zero	1.0000
Fe	57Linear Thru Zero	1.0000
Co	59Linear Thru Zero	1.0000
Ni	60Linear Thru Zero	1.0000
Cu	63Linear Thru Zero	
Cu	65Linear Thru Zero	1.0000
Zn	66Linear Thru Zero	1.0000
Zn	67Linear Thru Zero	
Zn	68Linear Thru Zero	
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	0.9998
Kr	83Linear Thru Zero	
Sr	88Linear Thru Zero	1.0000
Y	89Linear Thru Zero	
Zr	90Linear Thru Zero	1.0000
Mo	98Linear Thru Zero	1.0000
Ag	107Linear Thru Zero	1.0000
Cd	111Linear Thru Zero	1.0000
Cd	114Linear Thru Zero	
In	115Linear Thru Zero	
Sn	120Linear Thru Zero	1.0000
Sb	121Linear Thru Zero	0.9997
Sb	123Linear Thru Zero	
Ba	135Linear Thru Zero	
Ba	137Linear Thru Zero	1.0000
Ho	165Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000
Pb	208Linear Thru Zero	1.0000
Th	232Linear Thru Zero	1.0000
U	238Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Diff	Dup. Rel. % Diff
Li	7					
Be	9					
B	11					
Na	23					
Mg	24					
Al	27					
P	31					
K	39					
Ca	43					
> Sc	45		102.9			
Ti	47					
V	51					
Cr	52					
Cr	53					
Mn	55					
Fe	57					
Co	59					
Ni	60					
Cu	63					
Cu	65					
Zn	66					
Zn	67					
Zn	68					
> Ge	74		102.9			
As	75					
Se	77					
Se	82					
Kr	83					
Sr	88					
Y	89					
Zr	90					
Mo	98					
Ag	107					
Cd	111					
Cd	114					
> In	115		100.4			
Sn	120					
Sb	121					
Sb	123					
Ba	135					
Ba	137					
Ho	165					
> Lu	175		101.4			
Tl	205					
Pb	208					
Th	232					
U	238					

QC Out Of Limits

Measurement Type	Analyte	MassOut of Limits Message
QC Std 7	Mo	98CCB is out of limits (+/- PQL)

QC Action

QC Action Line: Continue

ICPMS#4 - Summary Report

Sample ID: QC Std 10

Sample Date/Time: Monday, April 12, 2010 03:44:57

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\6020.mth

Dataset File: c:\elandata\Dataset\100408\QC Std 10.560

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Li	7	927.313	ug/L	1.278	557826	0.874
Be	9	922.146	ug/L	1.775	145235	0.228
B	11	0.474	ug/L	11.019	169	0.000
Na	23	51598.467	ug/L	5.107	85810104	134.405
Mg	24	46808.744	ug/L	6.066	56374936	88.371
Al	27	48162.212	ug/L	6.150	80703380	126.530
P	31	23434.550	ug/L	2.523	2311066	3.618
K	39	47071.099	ug/L	3.449	137329368	214.581
Ca	43	48493.935	ug/L	1.746	298119	0.467
> Sc	45		ug/L		638102	638101.544
Ti	47	36.866	ug/L	0.561	11859	0.018
V	51	972.502	ug/L	2.292	3965163	6.183
Cr	52	956.697	ug/L	1.815	2926937	4.605
Cr	53		ug/L		469482	0.540
Mn	55	953.528	ug/L	1.124	4875974	7.640
Fe	57	48463.500	ug/L	1.786	5036258	7.885
Co	59	932.764	ug/L	2.441	3677005	5.763
Ni	60	926.039	ug/L	2.526	779053	1.221
Cu	63		ug/L		1762631	2.758
Cu	65	919.747	ug/L	0.637	859933	1.346
Zn	66	2150.083	ug/L	2.282	1196250	4.648
Zn	67		ug/L		197960	0.742
Zn	68		ug/L		860229	3.340
> Ge	74		ug/L		257165	257165.003
As	75	928.629	ug/L	0.652	607780	2.363
Se	77		ug/L		27289	0.086
Se	82	487.321	ug/L	0.379	29518	0.115
Kr	83		ug/L		85	0.000
Sr	88	974.371	ug/L	3.140	8749776	55.127
Y	89		ug/L		263	0.002
Zr	90	491.383	ug/L	2.706	2405499	15.152
Mo	98	1000.086	ug/L	3.082	2147875	13.530
Ag	107	245.837	ug/L	0.361	831778	5.239
Cd	111	948.438	ug/L	1.211	763975	4.813
Cd	114		ug/L		1749824	11.024
> In	115		ug/L		158729	158728.630
Sn	120	966.554	ug/L	2.314	3444352	21.694
Sb	121	311.858	ug/L	1.357	769423	4.843
Sb	123		ug/L		596219	3.753
Ba	135		ug/L		831661	4.167
Ba	137	912.568	ug/L	1.544	1433706	7.183
Ho	165		ug/L		96	0.000
> Lu	175		ug/L		199577	199577.070
Tl	205	453.029	ug/L	0.758	2507600	12.558
Pb	208	4655.006	ug/L	1.594	49745449	249.227
Th	232	2358.733	ug/L	1.733	25525609	127.888
U	238	4997.893	ug/L	1.507	52606827	263.595

Sample ID: QC Std 10

Report Date/Time: Monday, April 12, 2010 03:47:39

Page 1

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Li	7Linear Thru Zero	1.0000
Be	9Linear Thru Zero	1.0000
B	11Linear Thru Zero	1.0000
Na	23Linear Thru Zero	1.0000
Mg	24Linear Thru Zero	1.0000
Al	27Linear Thru Zero	1.0000
P	31Linear Thru Zero	1.0000
K	39Linear Thru Zero	1.0000
Ca	43Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ti	47Linear Thru Zero	1.0000
V	51Linear Thru Zero	0.9999
Cr	52Linear Thru Zero	1.0000
Cr	53Linear Thru Zero	
Mn	55Linear Thru Zero	1.0000
Fe	57Linear Thru Zero	1.0000
Co	59Linear Thru Zero	1.0000
Ni	60Linear Thru Zero	1.0000
Cu	63Linear Thru Zero	
Cu	65Linear Thru Zero	1.0000
Zn	66Linear Thru Zero	1.0000
Zn	67Linear Thru Zero	
Zn	68Linear Thru Zero	
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	0.9998
Kr	83Linear Thru Zero	
Sr	88Linear Thru Zero	1.0000
Y	89Linear Thru Zero	
Zr	90Linear Thru Zero	1.0000
Mo	98Linear Thru Zero	1.0000
Ag	107Linear Thru Zero	1.0000
Cd	111Linear Thru Zero	1.0000
Cd	114Linear Thru Zero	
In	115Linear Thru Zero	
Sn	120Linear Thru Zero	1.0000
Sb	121Linear Thru Zero	0.9997
Sb	123Linear Thru Zero	
Ba	135Linear Thru Zero	
Ba	137Linear Thru Zero	1.0000
Ho	165Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000
Pb	208Linear Thru Zero	1.0000
Th	232Linear Thru Zero	1.0000
U	238Linear Thru Zero	1.0000

Sample ID: QC Std 10

Report Date/Time: Monday, April 12, 2010 03:47:39

Page 2

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Diff	Dup. Rel. % Diff
Li	7	92.731				
Be	9	92.215				
B	11					
Na	23	103.197				
Mg	24	93.617				
Al	27	96.324				
P	31	93.738				
K	39	94.142				
Ca	43	96.988				
Sc	45		99.0			
Ti	47					
V	51	97.250				
Cr	52	95.670				
Cr	53					
Mn	55	95.353				
Fe	57	96.927				
Co	59	93.276				
Ni	60	92.604				
Cu	63					
Cu	65	91.975				
Zn	66	86.003				
Zn	67					
Zn	68					
Ge	74		98.9			
As	75	92.863				
Se	77					
Se	82	97.464				
Kr	83					
Sr	88	97.437				
Y	89					
Zr	90	98.277				
Mo	98	100.009				
Ag	107	98.335				
Cd	111	94.844				
Cd	114					
In	115		97.2			
Sn	120	96.655				
Sb	121	124.743				
Sb	123					
Ba	135					
Ba	137	91.257				
Ho	165					
Lu	175		103.0			
Tl	205	90.606				
Pb	208	93.100				
Th	232	94.349				
U	238	99.958				

QC Out Of Limits

Measurement Type	Analyte	Mass Out of Limits Message
QC Std 10	Zn	66LRS is out of limits (+/- 10%)
QC Std 10	Sb	121LRS is out of limits (+/- 10%)

QC Action

QC Action Line: Continue

Sample ID: QC Std 10
Report Date/Time: Monday, April 12, 2010 03:47:39
Page 3

ICPMS#4 - Summary Report

Sample ID: QC Std 11

Sample Date/Time: Monday, April 12, 2010 03:51:03

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\6020.mth

Dataset File: c:\elandata\Dataset\100408\QC Std 11.561

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Li	7	50.281	ug/L	0.388	31325	0.047
Be	9	49.923	ug/L	1.133	8142	0.012
B	11	99.071	ug/L	1.624	14127	0.021
Na	23	5262.825	ug/L	1.901	9061927	13.709
Mg	24	5479.521	ug/L	9.688	6830656	10.345
Al	27	4937.453	ug/L	2.473	8565056	12.971
P	31	4902.983	ug/L	1.219	502697	0.757
K	39	5110.624	ug/L	1.108	15771565	23.298
Ca	43	4971.923	ug/L	0.396	31813	0.048
> Sc	45		ug/L		660190	660190.110
Ti	47	50.088	ug/L	1.730	16606	0.025
V	51	51.249	ug/L	3.664	236055	0.326
Cr	52	53.142	ug/L	1.690	157338	0.256
Cr	53		ug/L		120832	-0.013
Mn	55	53.603	ug/L	1.917	284333	0.430
Fe	57	5012.467	ug/L	1.000	544027	0.816
Co	59	51.398	ug/L	1.452	209797	0.318
Ni	60	53.972	ug/L	2.027	47049	0.071
Cu	63		ug/L		109472	0.162
Cu	65	53.257	ug/L	0.502	52806	0.078
Zn	66	51.496	ug/L	2.455	31544	0.111
Zn	67		ug/L		10903	0.012
Zn	68		ug/L		23267	0.080
> Ge	74		ug/L		271556	271556.081
As	75	52.836	ug/L	0.892	36592	0.134
Se	77		ug/L		6719	0.004
Se	82	54.296	ug/L	4.039	3501	0.013
Kr	83		ug/L		53	-0.000
Sr	88	51.716	ug/L	1.399	488312	2.926
Y	89		ug/L		44	0.000
Zr	90	52.085	ug/L	4.805	268373	1.606
Mo	98	52.431	ug/L	3.757	118790	0.709
Ag	107	51.756	ug/L	1.435	184183	1.103
Cd	111	52.082	ug/L	2.664	44109	0.264
Cd	114		ug/L		103281	0.619
> In	115		ug/L		166853	166853.012
Sn	120	51.674	ug/L	2.448	194511	1.160
Sb	121	57.659	ug/L	4.589	150048	0.895
Sb	123		ug/L		115405	0.688
Ba	135		ug/L		45547	0.229
Ba	137	50.585	ug/L	1.753	79109	0.398
Ho	165		ug/L		9	-0.000
> Lu	175		ug/L		198599	198598.574
Tl	205	50.834	ug/L	1.645	281077	1.409
Pb	208	52.404	ug/L	1.413	561624	2.806
Th	232	54.371	ug/L	1.202	586846	2.948
U	238	54.322	ug/L	1.641	569608	2.865

Sample ID: QC Std 11

Report Date/Time: Monday, April 12, 2010 03:53:46

Page 1

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Li	7Linear Thru Zero	1.0000
Be	9Linear Thru Zero	1.0000
B	11Linear Thru Zero	1.0000
Na	23Linear Thru Zero	1.0000
Mg	24Linear Thru Zero	1.0000
Al	27Linear Thru Zero	1.0000
P	31Linear Thru Zero	1.0000
K	39Linear Thru Zero	1.0000
Ca	43Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ti	47Linear Thru Zero	1.0000
V	51Linear Thru Zero	0.9999
Cr	52Linear Thru Zero	1.0000
Cr	53Linear Thru Zero	
Mn	55Linear Thru Zero	1.0000
Fe	57Linear Thru Zero	1.0000
Co	59Linear Thru Zero	1.0000
Ni	60Linear Thru Zero	1.0000
Cu	63Linear Thru Zero	
Cu	65Linear Thru Zero	1.0000
Zn	66Linear Thru Zero	1.0000
Zn	67Linear Thru Zero	
Zn	68Linear Thru Zero	
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	0.9998
Kr	83Linear Thru Zero	
Sr	88Linear Thru Zero	1.0000
Y	89Linear Thru Zero	
Zr	90Linear Thru Zero	1.0000
Mo	98Linear Thru Zero	1.0000
Ag	107Linear Thru Zero	1.0000
Cd	111Linear Thru Zero	1.0000
Cd	114Linear Thru Zero	
In	115Linear Thru Zero	
Sn	120Linear Thru Zero	1.0000
Sb	121Linear Thru Zero	0.9997
Sb	123Linear Thru Zero	
Ba	135Linear Thru Zero	
Ba	137Linear Thru Zero	1.0000
Ho	165Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000
Pb	208Linear Thru Zero	1.0000
Th	232Linear Thru Zero	1.0000
U	238Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Diff	Dup. Rel. % Diff
Li	7	100.562				
Be	9	99.845				
B	11	99.071				
Na	23	105.257				
Mg	24	109.590				
Al	27	97.771				
P	31	98.060				
K	39	102.212				
Ca	43	99.438				
> Sc	45		102.4			
Ti	47	100.175				
V	51	102.498				
Cr	52	106.284				
Cr	53					
Mn	55	107.206				
Fe	57	100.249				
Co	59	102.796				
Ni	60	107.945				
Cu	63					
Cu	65	106.513				
Zn	66	102.992				
Zn	67					
Zn	68					
> Ge	74		104.4			
As	75	105.672				
Se	77					
Se	82	108.592				
Kr	83					
Sr	88	103.433				
Y	89					
Zr	90	104.169				
Mo	98	104.862				
Ag	107	103.513				
Cd	111	104.165				
Cd	114					
> In	115		102.1			
Sn	120	103.349				
Sb	121	115.317				
Sb	123					
Ba	135					
Ba	137	101.170				
Ho	165					
> Lu	175		102.5			
Tl	205	101.668				
Pb	208	104.808				
Th	232	108.741				
U	238	108.645				

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message
 QC Std 11 Sb 121CCV is out of limits (+/- 10%)

QC Action

QC Action Line: Continue

ICPMS#4 - Summary Report

Sample ID: QC Std 12

Sample Date/Time: Monday, April 12, 2010 03:57:12

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\6020.mth

Dataset File: c:\elandata\Dataset\100408\QC Std 12.562

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Li	7	0.106	ug/L	30.845	100	0.000
Be	9	0.018	ug/L	64.210	9	0.000
B	11	1.041	ug/L	15.698	265	0.000
Na	23	4.686	ug/L	75.280	20015	0.012
Mg	24	4.353	ug/L	19.683	6335	0.008
Al	27	3.889	ug/L	60.477	7669	0.010
P	31	2.577	ug/L	69.782	3377	0.000
K	39	0.880	ug/L	633.113	407402	0.004
Ca	43	7.240	ug/L	24.333	261	0.000
Sc	45		ug/L		684008	684008.183
Ti	47	0.160	ug/L	19.632	238	0.000
V	51	-1.276	ug/L	110.481	16065	-0.008
Cr	52	0.442	ug/L	11.535	-10504	0.002
Cr	53		ug/L		124787	-0.013
Mn	55	0.026	ug/L	26.601	919	0.000
Fe	57	1.571	ug/L	154.676	5975	0.000
Co	59	0.040	ug/L	20.317	326	0.000
Ni	60	0.039	ug/L	29.603	109	0.000
Cu	63		ug/L		2799	0.000
Cu	65	-0.092	ug/L	88.529	1323	-0.000
Zn	66	-0.280	ug/L	14.627	1182	-0.001
Zn	67		ug/L		7551	-0.001
Zn	68		ug/L		1443	-0.000
Ge	74		ug/L		279215	279215.269
As	75	0.576	ug/L	42.343	490	0.001
Se	77		ug/L		5750	-0.000
Se	82	2.231	ug/L	10.212	179	0.001
Kr	83		ug/L		61	-0.000
Sr	88	0.040	ug/L	10.674	572	0.002
Y	89		ug/L		21	-0.000
Zr	90	0.409	ug/L	16.051	2729	0.013
Mo	98	0.888	ug/L	7.891	2572	0.012
Ag	107	0.111	ug/L	20.059	588	0.002
Cd	111	0.053	ug/L	11.616	69	0.000
Cd	114		ug/L		172	0.001
In	115		ug/L		171192	171191.715
Sn	120	0.414	ug/L	7.981	2675	0.009
Sb	121	1.154	ug/L	19.713	3786	0.018
Sb	123		ug/L		2909	0.014
Ba	135		ug/L		75	0.000
Ba	137	0.032	ug/L	22.477	81	0.000
Ho	165		ug/L		8	-0.000
Lu	175		ug/L		198223	198222.584
Tl	205	0.597	ug/L	15.075	4505	0.017
Pb	208	0.341	ug/L	7.117	8020	0.018
Th	232	0.835	ug/L	13.697	10368	0.045
U	238	0.251	ug/L	13.116	3230	0.013

Sample ID: QC Std 12

Report Date/Time: Monday, April 12, 2010 03:59:57

Page 1

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Li	7Linear Thru Zero	1.0000
Be	9Linear Thru Zero	1.0000
B	11Linear Thru Zero	1.0000
Na	23Linear Thru Zero	1.0000
Mg	24Linear Thru Zero	1.0000
Al	27Linear Thru Zero	1.0000
P	31Linear Thru Zero	1.0000
K	39Linear Thru Zero	1.0000
Ca	43Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ti	47Linear Thru Zero	1.0000
V	51Linear Thru Zero	0.9999
Cr	52Linear Thru Zero	1.0000
Cr	53Linear Thru Zero	
Mn	55Linear Thru Zero	1.0000
Fe	57Linear Thru Zero	1.0000
Co	59Linear Thru Zero	1.0000
Ni	60Linear Thru Zero	1.0000
Cu	63Linear Thru Zero	
Cu	65Linear Thru Zero	1.0000
Zn	66Linear Thru Zero	1.0000
Zn	67Linear Thru Zero	
Zn	68Linear Thru Zero	
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	0.9998
Kr	83Linear Thru Zero	
Sr	88Linear Thru Zero	1.0000
Y	89Linear Thru Zero	
Zr	90Linear Thru Zero	1.0000
Mo	98Linear Thru Zero	1.0000
Ag	107Linear Thru Zero	1.0000
Cd	111Linear Thru Zero	1.0000
Cd	114Linear Thru Zero	
In	115Linear Thru Zero	
Sn	120Linear Thru Zero	1.0000
Sb	121Linear Thru Zero	0.9997
Sb	123Linear Thru Zero	
Ba	135Linear Thru Zero	
Ba	137Linear Thru Zero	1.0000
Ho	165Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000
Pb	208Linear Thru Zero	1.0000
Th	232Linear Thru Zero	1.0000
U	238Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Diff	Dup. Rel. % Diff
Li	7					
Be	9					
B	11					
Na	23					
Mg	24					
Al	27					
P	31					
K	39					
Ca	43					
> Sc	45		106.1			
Ti	47					
V	51					
Cr	52					
Cr	53					
Mn	55					
Fe	57					
Co	59					
Ni	60					
Cu	63					
Cu	65					
Zn	66					
Zn	67					
Zn	68					
> Ge	74		107.3			
As	75					
Se	77					
Se	82					
Kr	83					
Sr	88					
Y	89					
Zr	90					
Mo	98					
Ag	107					
Cd	111					
Cd	114					
> In	115		104.8			
Sn	120					
Sb	121					
Sb	123					
Ba	135					
Ba	137					
Ho	165					
> Lu	175		102.3			
Tl	205					
Pb	208					
Th	232					
U	238					

QC Out Of Limits

Measurement Type	Analyte	MassOut of Limits Message
QC Std 12	Mo	98CCB is out of limits (+/- PQL)
QC Std 12	U	238CCB is out of limits (+/- PQL)

QC Action

QC Action Line: Continue

Sample ID: QC Std 12

Report Date/Time: Monday, April 12, 2010 03:59:57

Page 3

ICPMS#4 - Summary Report

Sample ID: 1202056872

Sample Date/Time: Monday, April 12, 2010 04:03:24

Sample Type:

Sample Description: LANL 6020 MB

Number of Replicates: 3

Batch ID: 959112|1|bcd1

Method File: c:\elandata\Method\6020.mth

Dataset File: c:\elandata\Dataset\100408\1202056872.563

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Li	7	0.144	ug/L	12.170	127	0.000
Be	9	0.024	ug/L	47.465	10	0.000
B	11	0.646	ug/L	11.407	212	0.000
Na	23	12.449	ug/L	9.262	34709	0.032
Mg	24	1.980	ug/L	60.334	3334	0.004
Al	27	3.940	ug/L	46.843	8003	0.010
P	31	2.807	ug/L	94.310	3482	0.000
K	39	4.906	ug/L	124.806	429703	0.022
Ca	43	42.570	ug/L	9.692	505	0.000
> Sc	45		ug/L		700502	700502.234
Ti	47	0.659	ug/L	10.251	417	0.000
V	51	-0.627	ug/L	395.800	19170	-0.004
Cr	52	-5.241	ug/L	10.083	-29897	-0.025
Cr	53		ug/L		345927	0.299
Mn	55	0.242	ug/L	5.101	2155	0.002
Fe	57	12.836	ug/L	10.541	7406	0.002
Co	59	0.008	ug/L	65.912	194	0.000
Ni	60	0.029	ug/L	51.539	102	0.000
Cu	63		ug/L		4478	0.002
Cu	65	0.689	ug/L	19.996	2152	0.001
Zn	66	3.968	ug/L	27.214	3880	0.009
Zn	67		ug/L		30421	0.077
Zn	68		ug/L		4296	0.009
> Ge	74		ug/L		289438	289438.482
As	75	0.201	ug/L	625.115	237	0.001
Se	77		ug/L		19595	0.047
Se	82	1.361	ug/L	31.244	126	0.000
Kr	83		ug/L		64	-0.000
Sr	88	0.038	ug/L	20.272	578	0.002
Y	89		ug/L		33	0.000
Zr	90	0.402	ug/L	15.740	2782	0.012
Mo	98	0.595	ug/L	4.559	1954	0.008
Ag	107	0.047	ug/L	22.882	369	0.001
Cd	111	0.026	ug/L	15.146	47	0.000
Cd	114		ug/L		119	0.000
> In	115		ug/L		176710	176709.743
Sn	120	1.278	ug/L	8.215	6187	0.029
Sb	121	0.728	ug/L	24.379	2744	0.011
Sb	123		ug/L		2109	0.009
Ba	135		ug/L		69	0.000
Ba	137	0.044	ug/L	14.291	102	0.000
Ho	165		ug/L		9	-0.000
> Lu	175		ug/L		199834	199833.745
Tl	205	0.338	ug/L	17.899	3105	0.009
Pb	208	1.110	ug/L	5.047	16318	0.059
Th	232	0.592	ug/L	14.269	7823	0.032
U	238	0.095	ug/L	10.877	1611	0.005

Sample ID: 1202056872

Report Date/Time: Monday, April 12, 2010 04:06:11

Page 1

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Li	7Linear Thru Zero	1.0000
Be	9Linear Thru Zero	1.0000
B	11Linear Thru Zero	1.0000
Na	23Linear Thru Zero	1.0000
Mg	24Linear Thru Zero	1.0000
Al	27Linear Thru Zero	1.0000
P	31Linear Thru Zero	1.0000
K	39Linear Thru Zero	1.0000
Ca	43Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ti	47Linear Thru Zero	1.0000
V	51Linear Thru Zero	0.9999
Cr	52Linear Thru Zero	1.0000
Cr	53Linear Thru Zero	
Mn	55Linear Thru Zero	1.0000
Fe	57Linear Thru Zero	1.0000
Co	59Linear Thru Zero	1.0000
Ni	60Linear Thru Zero	1.0000
Cu	63Linear Thru Zero	
Cu	65Linear Thru Zero	1.0000
Zn	66Linear Thru Zero	1.0000
Zn	67Linear Thru Zero	
Zn	68Linear Thru Zero	
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	0.9998
Kr	83Linear Thru Zero	
Sr	88Linear Thru Zero	1.0000
Y	89Linear Thru Zero	
Zr	90Linear Thru Zero	1.0000
Mo	98Linear Thru Zero	1.0000
Ag	107Linear Thru Zero	1.0000
Cd	111Linear Thru Zero	1.0000
Cd	114Linear Thru Zero	
In	115Linear Thru Zero	
Sn	120Linear Thru Zero	1.0000
Sb	121Linear Thru Zero	0.9997
Sb	123Linear Thru Zero	
Ba	135Linear Thru Zero	
Ba	137Linear Thru Zero	1.0000
Ho	165Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000
Pb	208Linear Thru Zero	1.0000
Th	232Linear Thru Zero	1.0000
U	238Linear Thru Zero	1.0000

Sample ID: 1202056872

Report Date/Time: Monday, April 12, 2010 04:06:11

Page 2

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Diff	Dup. Rel. % Diff
Li	7					
Be	9					
B	11					
Na	23					
Mg	24					
Al	27					
P	31					
K	39					
Ca	43					
> Sc	45			108.7		
Ti	47					
V	51					
Cr	52					
Cr	53					
Mn	55					
Fe	57					
Co	59					
Ni	60					
Cu	63					
Cu	65					
Zn	66					
Zn	67					
Zn	68					
> Ge	74			111.3		
As	75					
Se	77					
Se	82					
Kr	83					
Sr	88					
Y	89					
Zr	90					
Mo	98					
Ag	107					
Cd	111					
Cd	114					
> In	115			108.2		
Sn	120					
Sb	121					
Sb	123					
Ba	135					
Ba	137					
Ho	165					
> Lu	175			103.2		
Tl	205					
Pb	208					
Th	232					
U	238					

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: 1202056872

Report Date/Time: Monday, April 12, 2010 04:06:11

Page 3

ICPMS#4 - Summary Report

Sample ID: 1202056873

Sample Date/Time: Monday, April 12, 2010 04:09:38

Sample Type:

Sample Description: LANL 6020 LCS

Number of Replicates: 3

Batch ID: 959112|1|bcd1

Method File: c:\elandata\Method\6020.mth

Dataset File: c:\elandata\Dataset\100408\1202056873.564

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Li	7	47.437	ug/L	0.939	31120	0.045
Be	9	48.562	ug/L	2.265	8339	0.012
B	11	103.534	ug/L	1.014	15540	0.022
Na	23	1968.041	ug/L	4.852	3576238	5.126
Mg	24	1911.396	ug/L	6.957	2509112	3.609
Al	27	1926.582	ug/L	6.333	3518248	5.061
P	31	1868.379	ug/L	0.129	203673	0.288
K	39	1998.747	ug/L	2.059	6745933	9.112
Ca	43	2046.946	ug/L	2.403	13917	0.020
> Sc	45		ug/L		695164	695164.170
Ti	47	45.898	ug/L	2.479	16039	0.023
V	51	50.993	ug/L	3.710	247360	0.324
Cr	52	46.568	ug/L	0.888	143662	0.224
Cr	53		ug/L		374813	0.344
Mn	55	53.782	ug/L	1.889	300344	0.431
Fe	57	2121.865	ug/L	1.423	245883	0.345
Co	59	53.070	ug/L	0.130	228101	0.328
Ni	60	53.825	ug/L	1.194	49408	0.071
Cu	63		ug/L		118286	0.166
Cu	65	54.375	ug/L	1.626	56737	0.080
Zn	66	48.706	ug/L	3.022	32004	0.105
Zn	67		ug/L		36860	0.099
Zn	68		ug/L		24546	0.079
> Ge	74		ug/L		290647	290646.962
As	75	50.602	ug/L	8.493	37502	0.129
Se	77		ug/L		22061	0.055
Se	82	48.832	ug/L	1.900	3374	0.011
Kr	83		ug/L		77	0.000
Sr	88	49.778	ug/L	2.151	504519	2.816
Y	89		ug/L		54	0.000
Zr	90	48.628	ug/L	1.705	269097	1.500
Mo	98	50.242	ug/L	1.086	122252	0.680
Ag	107	51.337	ug/L	1.035	196116	1.094
Cd	111	48.182	ug/L	1.577	43813	0.245
Cd	114		ug/L		102944	0.575
> In	115		ug/L		179071	179071.035
Sn	120	49.003	ug/L	1.390	198077	1.100
Sb	121	59.775	ug/L	0.767	166990	0.928
Sb	123		ug/L		128408	0.714
Ba	135		ug/L		45678	0.224
Ba	137	49.095	ug/L	0.294	78890	0.386
Ho	165		ug/L		17	0.000
> Lu	175		ug/L		204056	204056.313
Tl	205	47.789	ug/L	0.506	271579	1.325
Pb	208	52.187	ug/L	1.590	574669	2.794
Th	232	51.609	ug/L	1.924	572492	2.798
U	238	54.936	ug/L	2.300	591709	2.897

Sample ID: 1202056873

Report Date/Time: Monday, April 12, 2010 04:12:25

Page 1

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Li	7Linear Thru Zero	1.0000
Be	9Linear Thru Zero	1.0000
B	11Linear Thru Zero	1.0000
Na	23Linear Thru Zero	1.0000
Mg	24Linear Thru Zero	1.0000
Al	27Linear Thru Zero	1.0000
P	31Linear Thru Zero	1.0000
K	39Linear Thru Zero	1.0000
Ca	43Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ti	47Linear Thru Zero	1.0000
V	51Linear Thru Zero	0.9999
Cr	52Linear Thru Zero	1.0000
Cr	53Linear Thru Zero	
Mn	55Linear Thru Zero	1.0000
Fe	57Linear Thru Zero	1.0000
Co	59Linear Thru Zero	1.0000
Ni	60Linear Thru Zero	1.0000
Cu	63Linear Thru Zero	
Cu	65Linear Thru Zero	1.0000
Zn	66Linear Thru Zero	1.0000
Zn	67Linear Thru Zero	
Zn	68Linear Thru Zero	
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	0.9998
Kr	83Linear Thru Zero	
Sr	88Linear Thru Zero	1.0000
Y	89Linear Thru Zero	
Zr	90Linear Thru Zero	1.0000
Mo	98Linear Thru Zero	1.0000
Ag	107Linear Thru Zero	1.0000
Cd	111Linear Thru Zero	1.0000
Cd	114Linear Thru Zero	
In	115Linear Thru Zero	
Sn	120Linear Thru Zero	1.0000
Sb	121Linear Thru Zero	0.9997
Sb	123Linear Thru Zero	
Ba	135Linear Thru Zero	
Ba	137Linear Thru Zero	1.0000
Ho	165Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000
Pb	208Linear Thru Zero	1.0000
Th	232Linear Thru Zero	1.0000
U	238Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Diff	Dup. Rel. % Diff
Li	7					
Be	9					
B	11					
Na	23					
Mg	24					
Al	27					
P	31					
K	39					
Ca	43					
> Sc	45		107.8			
Ti	47					
V	51					
Cr	52					
Cr	53					
Mn	55					
Fe	57					
Co	59					
Ni	60					
Cu	63					
Cu	65					
Zn	66					
Zn	67					
Zn	68					
> Ge	74		111.7			
As	75					
Se	77					
Se	82					
Kr	83					
Sr	88					
Y	89					
Zr	90					
Mo	98					
Ag	107					
Cd	111					
Cd	114					
> In	115		109.6			
Sn	120					
Sb	121					
Sb	123					
Ba	135					
Ba	137					
Ho	165					
> Lu	175		105.3			
Tl	205					
Pb	208					
Th	232					
U	238					

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: 1202056873

Report Date/Time: Monday, April 12, 2010 04:12:25

Page 3

ICPMS#4 - Summary Report

Sample ID: 248117001

Sample Date/Time: Monday, April 12, 2010 04:22:06

Sample Type:

Sample Description: LANL 6020

Number of Replicates: 3

Batch ID: 959112|1|bcd1

Method File: c:\elandata\Method\6020.mth

Dataset File: c:\elandata\Dataset\100408\248117001.566

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Li	7	0.383	ug/L	12.846	292	0.000
Be	9	-0.011	ug/L	162.331	4	-0.000
B	11	27.397	ug/L	4.825	4337	0.006
Na	23	187.850	ug/L	10.750	363590	0.489
Mg	24	9.244	ug/L	36.448	13340	0.017
Al	27	14.980	ug/L	12.568	29030	0.039
P	31	8.641	ug/L	24.199	4221	0.001
K	39	298.340	ug/L	6.876	1402301	1.360
Ca	43	93.835	ug/L	7.336	873	0.001
> Sc	45		ug/L		719040	719040.027
Ti	47	0.957	ug/L	5.215	534	0.000
V	51	-0.931	ug/L	296.883	18374	-0.006
Cr	52	-3.547	ug/L	12.849	-24834	-0.017
Cr	53		ug/L		406795	0.370
Mn	55	0.651	ug/L	5.327	4563	0.005
Fe	57	25.813	ug/L	11.046	9114	0.004
Co	59	0.014	ug/L	10.911	228	0.000
Ni	60	0.141	ug/L	6.097	211	0.000
Cu	63		ug/L		20446	0.024
Cu	65	7.915	ug/L	4.445	9808	0.012
Zn	66	6.643	ug/L	3.513	5796	0.014
Zn	67		ug/L		34522	0.087
Zn	68		ug/L		5854	0.014
> Ge	74		ug/L		301835	301834.851
As	75	-1.229	ug/L	234.841	-845	-0.003
Se	77		ug/L		27043	0.069
Se	82	0.546	ug/L	31.830	74	0.000
Kr	83		ug/L		63	-0.000
Sr	88	0.193	ug/L	2.881	2138	0.011
Y	89		ug/L		263	0.001
Zr	90	0.159	ug/L	7.590	1464	0.005
Mo	98	0.190	ug/L	14.144	992	0.003
Ag	107	0.013	ug/L	19.888	241	0.000
Cd	111	0.012	ug/L	81.728	34	0.000
Cd	114		ug/L		63	0.000
> In	115		ug/L		177669	177669.407
Sn	120	0.713	ug/L	2.159	3968	0.016
Sb	121	0.149	ug/L	12.682	1161	0.002
Sb	123		ug/L		904	0.002
Ba	135		ug/L		297	0.001
Ba	137	0.318	ug/L	7.557	534	0.002
Ho	165		ug/L		15	0.000
> Lu	175		ug/L		201083	201082.863
Tl	205	0.193	ug/L	25.493	2318	0.005
Pb	208	0.866	ug/L	7.674	13788	0.046
Th	232	0.220	ug/L	14.727	3822	0.012
U	238	0.002	ug/L	1081.361	645	0.000

Sample ID: 248117001

Report Date/Time: Monday, April 12, 2010 04:24:52

Page 1

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Li	7Linear Thru Zero	1.0000
Be	9Linear Thru Zero	1.0000
B	11Linear Thru Zero	1.0000
Na	23Linear Thru Zero	1.0000
Mg	24Linear Thru Zero	1.0000
Al	27Linear Thru Zero	1.0000
P	31Linear Thru Zero	1.0000
K	39Linear Thru Zero	1.0000
Ca	43Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ti	47Linear Thru Zero	1.0000
V	51Linear Thru Zero	0.9999
Cr	52Linear Thru Zero	1.0000
Cr	53Linear Thru Zero	
Mn	55Linear Thru Zero	1.0000
Fe	57Linear Thru Zero	1.0000
Co	59Linear Thru Zero	1.0000
Ni	60Linear Thru Zero	1.0000
Cu	63Linear Thru Zero	
Cu	65Linear Thru Zero	1.0000
Zn	66Linear Thru Zero	1.0000
Zn	67Linear Thru Zero	
Zn	68Linear Thru Zero	
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	0.9998
Kr	83Linear Thru Zero	
Sr	88Linear Thru Zero	1.0000
Y	89Linear Thru Zero	
Zr	90Linear Thru Zero	1.0000
Mo	98Linear Thru Zero	1.0000
Ag	107Linear Thru Zero	1.0000
Cd	111Linear Thru Zero	1.0000
Cd	114Linear Thru Zero	
In	115Linear Thru Zero	
Sn	120Linear Thru Zero	1.0000
Sb	121Linear Thru Zero	0.9997
Sb	123Linear Thru Zero	
Ba	135Linear Thru Zero	
Ba	137Linear Thru Zero	1.0000
Ho	165Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000
Pb	208Linear Thru Zero	1.0000
Th	232Linear Thru Zero	1.0000
U	238Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Diff	Dup. Rel. % Diff
Li	7					
Be	9					
B	11					
Na	23					
Mg	24					
Al	27					
P	31					
K	39					
Ca	43					
> Sc	45		111.5			
Ti	47					
V	51					
Cr	52					
Cr	53					
Mn	55					
Fe	57					
Co	59					
Ni	60					
Cu	63					
Cu	65					
Zn	66					
Zn	67					
Zn	68					
> Ge	74		116.0			
As	75					
Se	77					
Se	82					
Kr	83					
Sr	88					
Y	89					
Zr	90					
Mo	98					
Ag	107					
Cd	111					
Cd	114					
> In	115		108.7			
Sn	120					
Sb	121					
Sb	123					
Ba	135					
Ba	137					
Ho	165					
> Lu	175		103.8			
Tl	205					
Pb	208					
Th	232					
U	238					

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: 248117001

Report Date/Time: Monday, April 12, 2010 04:24:52

Page 3

ICPMS#4 - Summary Report

Sample ID: QC Std 6

Sample Date/Time: Monday, April 12, 2010 05:05:40

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\6020.mth

Dataset File: c:\elandata\Dataset\100408\QC Std 6.573

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Li	7	49.807	ug/L	0.772	30576	0.047
Be	9	49.214	ug/L	3.101	7907	0.012
B	11	100.083	ug/L	0.214	14062	0.021
Na	23	5216.555	ug/L	3.695	8851128	13.588
Mg	24	5018.461	ug/L	2.745	6163339	9.474
Al	27	4977.080	ug/L	2.341	8508127	13.076
P	31	4827.331	ug/L	1.539	487750	0.745
K	39	4923.194	ug/L	3.536	14982550	22.443
Ca	43	4807.632	ug/L	2.311	30315	0.046
> Sc	45		ug/L		650556	650555.880
Ti	47	48.828	ug/L	2.560	15954	0.024
V	51	50.823	ug/L	5.859	230743	0.323
Cr	52	51.102	ug/L	2.324	148619	0.246
Cr	53		ug/L		133243	0.009
Mn	55	51.807	ug/L	2.184	270763	0.415
Fe	57	4922.337	ug/L	3.660	526405	0.801
Co	59	50.163	ug/L	2.546	201740	0.310
Ni	60	52.646	ug/L	2.991	45219	0.069
Cu	63		ug/L		106822	0.160
Cu	65	52.665	ug/L	1.370	51467	0.077
Zn	66	51.158	ug/L	0.703	30435	0.111
Zn	67		ug/L		11640	0.016
Zn	68		ug/L		22331	0.079
> Ge	74		ug/L		263670	263669.826
As	75	49.662	ug/L	1.381	33396	0.126
Se	77		ug/L		6861	0.005
Se	82	45.092	ug/L	6.433	2828	0.011
Kr	83		ug/L		56	-0.000
Sr	88	50.459	ug/L	1.655	465513	2.855
Y	89		ug/L		55	0.000
Zr	90	48.396	ug/L	3.484	243744	1.492
Mo	98	48.849	ug/L	2.834	108195	0.661
Ag	107	51.342	ug/L	2.178	178514	1.094
Cd	111	50.418	ug/L	1.882	41725	0.256
Cd	114		ug/L		97125	0.596
> In	115		ug/L		163029	163028.776
Sn	120	49.522	ug/L	3.255	182181	1.112
Sb	121	54.526	ug/L	4.869	138667	0.847
Sb	123		ug/L		107791	0.658
Ba	135		ug/L		43763	0.225
Ba	137	49.324	ug/L	1.487	75408	0.388
Ho	165		ug/L		13	0.000
> Lu	175		ug/L		194149	194149.341
Tl	205	48.008	ug/L	1.285	259566	1.331
Pb	208	50.697	ug/L	0.790	531286	2.714
Th	232	49.529	ug/L	2.342	522761	2.685
U	238	53.530	ug/L	1.177	548709	2.823

Sample ID: QC Std 6

Report Date/Time: Monday, April 12, 2010 05:08:24

Page 1

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Li	7Linear Thru Zero	1.0000
Be	9Linear Thru Zero	1.0000
B	11Linear Thru Zero	1.0000
Na	23Linear Thru Zero	1.0000
Mg	24Linear Thru Zero	1.0000
Al	27Linear Thru Zero	1.0000
P	31Linear Thru Zero	1.0000
K	39Linear Thru Zero	1.0000
Ca	43Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ti	47Linear Thru Zero	1.0000
V	51Linear Thru Zero	0.9999
Cr	52Linear Thru Zero	1.0000
Cr	53Linear Thru Zero	
Mn	55Linear Thru Zero	1.0000
Fe	57Linear Thru Zero	1.0000
Co	59Linear Thru Zero	1.0000
Ni	60Linear Thru Zero	1.0000
Cu	63Linear Thru Zero	
Cu	65Linear Thru Zero	1.0000
Zn	66Linear Thru Zero	1.0000
Zn	67Linear Thru Zero	
Zn	68Linear Thru Zero	
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	0.9998
Kr	83Linear Thru Zero	
Sr	88Linear Thru Zero	1.0000
Y	89Linear Thru Zero	
Zr	90Linear Thru Zero	1.0000
Mo	98Linear Thru Zero	1.0000
Ag	107Linear Thru Zero	1.0000
Cd	111Linear Thru Zero	1.0000
Cd	114Linear Thru Zero	
In	115Linear Thru Zero	
Sn	120Linear Thru Zero	1.0000
Sb	121Linear Thru Zero	0.9997
Sb	123Linear Thru Zero	
Ba	135Linear Thru Zero	
Ba	137Linear Thru Zero	1.0000
Ho	165Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000
Pb	208Linear Thru Zero	1.0000
Th	232Linear Thru Zero	1.0000
U	238Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Diff	Dup. Rel. % Diff
Li	7	99.613				
Be	9	98.428				
B	11	100.083				
Na	23	104.331				
Mg	24	100.369				
Al	27	98.556				
P	31	96.547				
K	39	98.464				
Ca	43	96.153				
Sc	45		100.9			
Ti	47	97.656				
V	51	101.647				
Cr	52	102.204				
Cr	53					
Mn	55	103.614				
Fe	57	98.447				
Co	59	100.325				
Ni	60	105.292				
Cu	63					
Cu	65	105.330				
Zn	66	102.316				
Zn	67					
Zn	68					
Ge	74		101.4			
As	75	99.324				
Se	77					
Se	82	90.184				
Kr	83					
Sr	88	100.918				
Y	89					
Zr	90	96.793				
Mo	98	97.699				
Ag	107	102.684				
Cd	111	100.836				
Cd	114					
In	115		99.8			
Sn	120	99.044				
Sb	121	109.053				
Sb	123					
Ba	135					
Ba	137	98.648				
Ho	165					
Lu	175		100.2			
Tl	205	96.015				
Pb	208	101.395				
Th	232	99.058				
U	238	107.061				

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 6

Report Date/Time: Monday, April 12, 2010 05:08:24

Page 3

ICPMS#4 - Summary Report

Sample ID: QC Std 7

Sample Date/Time: Monday, April 12, 2010 05:11:50

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\6020.mth

Dataset File: c:\elandata\Dataset\100408\QC Std 7.574

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Li	7	0.015	ug/L	73.906	37	0.000
Be	9	0.018	ug/L	71.383	8	0.000
B	11	1.113	ug/L	31.283	251	0.000
Na	23	3.520	ug/L	64.005	16343	0.009
Mg	24	0.861	ug/L	111.528	1667	0.002
Al	27	0.626	ug/L	113.629	1667	0.002
P	31	5.295	ug/L	64.947	3340	0.001
K	39	-3.257	ug/L	243.352	359823	-0.015
Ca	43	7.954	ug/L	74.235	242	0.000
> Sc	45		ug/L		623723	623722.517
Ti	47	0.070	ug/L	49.820	189	0.000
V	51	-0.577	ug/L	131.908	17449	-0.004
Cr	52	-0.119	ug/L	72.616	-11263	-0.001
Cr	53		ug/L		128536	0.010
Mn	55	0.016	ug/L	82.483	789	0.000
Fe	57	2.040	ug/L	47.616	5497	0.000
Co	59	0.005	ug/L	49.639	164	0.000
Ni	60	0.021	ug/L	28.689	84	0.000
Cu	63		ug/L		2312	-0.000
Cu	65	-0.252	ug/L	46.900	1059	-0.000
Zn	66	-0.566	ug/L	4.153	932	-0.001
Zn	67		ug/L		7738	0.002
Zn	68		ug/L		1250	-0.001
> Ge	74		ug/L		257660	257659.924
As	75	0.952	ug/L	86.590	696	0.002
Se	77		ug/L		5918	0.002
Se	82	1.496	ug/L	14.573	121	0.000
Kr	83		ug/L		56	-0.000
Sr	88	0.010	ug/L	50.491	261	0.001
Y	89		ug/L		17	-0.000
Zr	90	0.335	ug/L	17.985	2139	0.010
Mo	98	0.412	ug/L	19.540	1345	0.006
Ag	107	0.042	ug/L	28.426	311	0.001
Cd	111	0.000	ug/L	2482.021	21	0.000
Cd	114		ug/L		63	0.000
> In	115		ug/L		156899	156899.262
Sn	120	0.122	ug/L	27.708	1422	0.003
Sb	121	1.255	ug/L	26.378	3712	0.019
Sb	123		ug/L		2867	0.015
Ba	135		ug/L		31	0.000
Ba	137	0.011	ug/L	16.822	46	0.000
Ho	165		ug/L		7	-0.000
> Lu	175		ug/L		189202	189202.061
Tl	205	0.370	ug/L	20.545	3110	0.010
Pb	208	0.019	ug/L	56.827	4400	0.001
Th	232	0.441	ug/L	25.314	5866	0.024
U	238	0.044	ug/L	53.866	1024	0.002

Sample ID: QC Std 7

Report Date/Time: Monday, April 12, 2010 05:14:35

Page 1

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Li	7Linear Thru Zero	1.0000
Be	9Linear Thru Zero	1.0000
B	11Linear Thru Zero	1.0000
Na	23Linear Thru Zero	1.0000
Mg	24Linear Thru Zero	1.0000
Al	27Linear Thru Zero	1.0000
P	31Linear Thru Zero	1.0000
K	39Linear Thru Zero	1.0000
Ca	43Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ti	47Linear Thru Zero	1.0000
V	51Linear Thru Zero	0.9999
Cr	52Linear Thru Zero	1.0000
Cr	53Linear Thru Zero	
Mn	55Linear Thru Zero	1.0000
Fe	57Linear Thru Zero	1.0000
Co	59Linear Thru Zero	1.0000
Ni	60Linear Thru Zero	1.0000
Cu	63Linear Thru Zero	
Cu	65Linear Thru Zero	1.0000
Zn	66Linear Thru Zero	1.0000
Zn	67Linear Thru Zero	
Zn	68Linear Thru Zero	
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	0.9998
Kr	83Linear Thru Zero	
Sr	88Linear Thru Zero	1.0000
Y	89Linear Thru Zero	
Zr	90Linear Thru Zero	1.0000
Mo	98Linear Thru Zero	1.0000
Ag	107Linear Thru Zero	1.0000
Cd	111Linear Thru Zero	1.0000
Cd	114Linear Thru Zero	
In	115Linear Thru Zero	
Sn	120Linear Thru Zero	1.0000
Sb	121Linear Thru Zero	0.9997
Sb	123Linear Thru Zero	
Ba	135Linear Thru Zero	
Ba	137Linear Thru Zero	1.0000
Ho	165Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000
Pb	208Linear Thru Zero	1.0000
Th	232Linear Thru Zero	1.0000
U	238Linear Thru Zero	1.0000

Sample ID: QC Std 7

Report Date/Time: Monday, April 12, 2010 05:14:35

Page 2

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Diff	Dup. Rel. % Diff
Li	7					
Be	9					
B	11					
Na	23					
Mg	24					
Al	27					
P	31					
K	39					
Ca	43					
> Sc	45			96.7		
Ti	47					
V	51					
Cr	52					
Cr	53					
Mn	55					
Fe	57					
Co	59					
Ni	60					
Cu	63					
Cu	65					
Zn	66					
Zn	67					
Zn	68					
> Ge	74			99.1		
As	75					
Se	77					
Se	82					
Kr	83					
Sr	88					
Y	89					
Zr	90					
Mo	98					
Ag	107					
Cd	111					
Cd	114					
> In	115			96.0		
Sn	120					
Sb	121					
Sb	123					
Ba	135					
Ba	137					
Ho	165					
> Lu	175			97.7		
Tl	205					
Pb	208					
Th	232					
U	238					

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 7

Report Date/Time: Monday, April 12, 2010 05:14:35

Page 3

ICPMS#4 - Summary Report

Sample ID: 1202056874

Sample Date/Time: Monday, April 12, 2010 05:24:14

Sample Type:

Sample Description: LANL 6020 DUP

Number of Replicates: 3

Batch ID: 959112|1|bcd1

Method File: c:\elandata\Method\6020.mth

Dataset File: c:\elandata\Dataset\100408\1202056874.576

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Li	7	0.163	ug/L	9.060	131	0.000
Be	9	-0.011	ug/L	60.124	4	-0.000
B	11	29.717	ug/L	0.980	4273	0.006
Na	23	143.901	ug/L	1.645	256278	0.375
Mg	24	5.947	ug/L	25.291	8002	0.011
Al	27	11.674	ug/L	28.940	20682	0.031
P	31	1.213	ug/L	210.233	3090	0.000
K	39	69.529	ug/L	19.840	594503	0.317
Ca	43	65.872	ug/L	6.895	619	0.001
> Sc	45		ug/L		654020	654020.219
Ti	47	0.771	ug/L	3.964	426	0.000
V	51	-0.394	ug/L	955.459	19099	-0.003
Cr	52	-5.611	ug/L	6.633	-29091	-0.027
Cr	53		ug/L		388344	0.398
Mn	55	0.490	ug/L	3.536	3310	0.004
Fe	57	13.263	ug/L	4.708	6959	0.002
Co	59	-0.002	ug/L	209.194	142	-0.000
Ni	60	0.048	ug/L	26.985	112	0.000
Cu	63		ug/L		3841	0.002
Cu	65	0.553	ug/L	5.320	1881	0.001
Zn	66	1.340	ug/L	11.538	2120	0.003
Zn	67		ug/L		31279	0.086
Zn	68		ug/L		3096	0.006
> Ge	74		ug/L		273976	273976.097
As	75	-0.257	ug/L	600.100	-99	-0.001
Se	77		ug/L		25431	0.072
Se	82	-0.011	ug/L	627.991	31	-0.000
Kr	83		ug/L		63	0.000
Sr	88	0.094	ug/L	7.249	1052	0.005
Y	89		ug/L		148	0.001
Zr	90	0.055	ug/L	19.588	822	0.002
Mo	98	0.012	ug/L	120.393	521	0.000
Ag	107	-0.004	ug/L	33.326	161	-0.000
Cd	111	-0.008	ug/L	62.280	15	-0.000
Cd	114		ug/L		23	-0.000
> In	115		ug/L		163784	163784.255
Sn	120	0.370	ug/L	7.424	2397	0.008
Sb	121	0.071	ug/L	24.527	871	0.001
Sb	123		ug/L		672	0.001
Ba	135		ug/L		207	0.001
Ba	137	0.209	ug/L	3.397	345	0.002
Ho	165		ug/L		11	0.000
> Lu	175		ug/L		191276	191276.071
Tl	205	-0.042	ug/L	21.813	960	-0.001
Pb	208	0.631	ug/L	10.302	10704	0.034
Th	232	-0.010	ug/L	78.092	1254	-0.001
U	238	-0.037	ug/L	22.681	217	-0.002

Sample ID: 1202056874

Report Date/Time: Monday, April 12, 2010 05:27:00

Page 1

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Li	7Linear Thru Zero	1.0000
Be	9Linear Thru Zero	1.0000
B	11Linear Thru Zero	1.0000
Na	23Linear Thru Zero	1.0000
Mg	24Linear Thru Zero	1.0000
Al	27Linear Thru Zero	1.0000
P	31Linear Thru Zero	1.0000
K	39Linear Thru Zero	1.0000
Ca	43Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ti	47Linear Thru Zero	1.0000
V	51Linear Thru Zero	0.9999
Cr	52Linear Thru Zero	1.0000
Cr	53Linear Thru Zero	
Mn	55Linear Thru Zero	1.0000
Fe	57Linear Thru Zero	1.0000
Co	59Linear Thru Zero	1.0000
Ni	60Linear Thru Zero	1.0000
Cu	63Linear Thru Zero	
Cu	65Linear Thru Zero	1.0000
Zn	66Linear Thru Zero	1.0000
Zn	67Linear Thru Zero	
Zn	68Linear Thru Zero	
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	0.9998
Kr	83Linear Thru Zero	
Sr	88Linear Thru Zero	1.0000
Y	89Linear Thru Zero	
Zr	90Linear Thru Zero	1.0000
Mo	98Linear Thru Zero	1.0000
Ag	107Linear Thru Zero	1.0000
Cd	111Linear Thru Zero	1.0000
Cd	114Linear Thru Zero	
In	115Linear Thru Zero	
Sn	120Linear Thru Zero	1.0000
Sb	121Linear Thru Zero	0.9997
Sb	123Linear Thru Zero	
Ba	135Linear Thru Zero	
Ba	137Linear Thru Zero	1.0000
Ho	165Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000
Pb	208Linear Thru Zero	1.0000
Th	232Linear Thru Zero	1.0000
U	238Linear Thru Zero	1.0000

Sample ID: 1202056874

Report Date/Time: Monday, April 12, 2010 05:27:00

Page 2

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Diff	Dup. Rel. % Diff
Li	7					
Be	9					
B	11					
Na	23					
Mg	24					
Al	27					
P	31					
K	39					
Ca	43					
Sc	45		101.4			
Ti	47					
V	51					
Cr	52					
Cr	53					
Mn	55					
Fe	57					
Co	59					
Ni	60					
Cu	63					
Cu	65					
Zn	66					
Zn	67					
Zn	68					
Ge	74		105.3			
As	75					
Se	77					
Se	82					
Kr	83					
Sr	88					
Y	89					
Zr	90					
Mo	98					
Ag	107					
Cd	111					
Cd	114					
In	115		100.2			
Sn	120					
Sb	121					
Sb	123					
Ba	135					
Ba	137					
Ho	165					
Lu	175		98.7			
Tl	205					
Pb	208					
Th	232					
U	238					

QC Out Of Limits

Measurement Type Analyte

Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: 1202056874

Report Date/Time: Monday, April 12, 2010 05:27:00

Page 3

ICPMS#4 - Summary Report

Sample ID: 1202056875

Sample Date/Time: Monday, April 12, 2010 05:30:27

Sample Type:

Sample Description: LANL 6020 MS

Number of Replicates: 3

Batch ID: 959112|1|bcd1

Method File: c:\elandata\Method\6020.mth

Dataset File: c:\elandata\Dataset\100408\1202056875.577

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Li	7	46.576	ug/L	2.348	29450	0.044
Be	9	48.583	ug/L	2.698	8040	0.012
B	11	129.597	ug/L	2.850	18717	0.028
Na	23	2050.399	ug/L	7.388	3588494	5.341
Mg	24	1859.937	ug/L	14.140	2353582	3.511
Al	27	1813.940	ug/L	7.969	3190903	4.766
P	31	1764.429	ug/L	1.812	185542	0.272
K	39	2029.296	ug/L	10.589	6588712	9.251
Ca	43	2041.905	ug/L	2.550	13383	0.020
> Sc	45		ug/L		670115	670115.239
Ti	47	45.960	ug/L	2.185	15477	0.023
V	51	50.488	ug/L	7.017	236143	0.321
Cr	52	46.128	ug/L	2.249	137027	0.222
Cr	53		ug/L		382213	0.375
Mn	55	51.922	ug/L	0.689	279535	0.416
Fe	57	2051.668	ug/L	3.789	229276	0.334
Co	59	50.261	ug/L	3.219	208170	0.311
Ni	60	52.295	ug/L	3.408	46258	0.069
Cu	63		ug/L		111270	0.162
Cu	65	53.613	ug/L	1.694	53945	0.078
Zn	66	47.285	ug/L	1.235	29971	0.102
Zn	67		ug/L		35550	0.099
Zn	68		ug/L		23294	0.078
> Ge	74		ug/L		279946	279945.776
As	75	76.038	ug/L	2.875	54253	0.194
Se	77		ug/L		22447	0.060
Se	82	18.808	ug/L	4.559	1272	0.004
Kr	83		ug/L		79	0.000
Sr	88	50.646	ug/L	1.864	475658	2.865
Y	89		ug/L		191	0.001
Zr	90	50.773	ug/L	0.530	260384	1.566
Mo	98	50.124	ug/L	1.962	113022	0.678
Ag	107	52.083	ug/L	1.476	184371	1.110
Cd	111	9.941	ug/L	2.766	8393	0.050
Cd	114		ug/L		19535	0.118
> In	115		ug/L		165966	165965.636
Sn	120	49.470	ug/L	0.315	185334	1.110
Sb	121	245.922	ug/L	0.959	634519	3.819
Sb	123		ug/L		484668	2.917
Ba	135		ug/L		43546	0.223
Ba	137	49.305	ug/L	1.289	75732	0.388
Ho	165		ug/L		103	0.000
> Lu	175		ug/L		195069	195069.184
Tl	205	84.356	ug/L	4.255	457429	2.338
Pb	208	41.487	ug/L	1.425	437598	2.221
Th	232	51.956	ug/L	2.455	550955	2.817
U	238	54.665	ug/L	0.886	562992	2.883

Sample ID: 1202056875

Report Date/Time: Monday, April 12, 2010 05:33:14

Page 1

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Li	7Linear Thru Zero	1.0000
Be	9Linear Thru Zero	1.0000
B	11Linear Thru Zero	1.0000
Na	23Linear Thru Zero	1.0000
Mg	24Linear Thru Zero	1.0000
Al	27Linear Thru Zero	1.0000
P	31Linear Thru Zero	1.0000
K	39Linear Thru Zero	1.0000
Ca	43Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ti	47Linear Thru Zero	1.0000
V	51Linear Thru Zero	0.9999
Cr	52Linear Thru Zero	1.0000
Cr	53Linear Thru Zero	
Mn	55Linear Thru Zero	1.0000
Fe	57Linear Thru Zero	1.0000
Co	59Linear Thru Zero	1.0000
Ni	60Linear Thru Zero	1.0000
Cu	63Linear Thru Zero	
Cu	65Linear Thru Zero	1.0000
Zn	66Linear Thru Zero	1.0000
Zn	67Linear Thru Zero	
Zn	68Linear Thru Zero	
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	0.9998
Kr	83Linear Thru Zero	
Sr	88Linear Thru Zero	1.0000
Y	89Linear Thru Zero	
Zr	90Linear Thru Zero	1.0000
Mo	98Linear Thru Zero	1.0000
Ag	107Linear Thru Zero	1.0000
Cd	111Linear Thru Zero	1.0000
Cd	114Linear Thru Zero	
In	115Linear Thru Zero	
Sn	120Linear Thru Zero	1.0000
Sb	121Linear Thru Zero	0.9997
Sb	123Linear Thru Zero	
Ba	135Linear Thru Zero	
Ba	137Linear Thru Zero	1.0000
Ho	165Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000
Pb	208Linear Thru Zero	1.0000
Th	232Linear Thru Zero	1.0000
U	238Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Diff	Dup. Rel. % Diff
Li	7					
Be	9					
B	11					
Na	23					
Mg	24					
Al	27					
P	31					
K	39					
Ca	43					
> Sc	45			103.9		
Ti	47					
V	51					
Cr	52					
Cr	53					
Mn	55					
Fe	57					
Co	59					
Ni	60					
Cu	63					
Cu	65					
Zn	66					
Zn	67					
Zn	68					
> Ge	74			107.6		
As	75					
Se	77					
Se	82					
Kr	83					
Sr	88					
Y	89					
Zr	90					
Mo	98					
Ag	107					
Cd	111					
Cd	114					
> In	115			101.6		
Sn	120					
Sb	121					
Sb	123					
Ba	135					
Ba	137					
Ho	165					
> Lu	175			100.7		
Tl	205					
Pb	208					
Th	232					
U	238					

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: 1202056875

Report Date/Time: Monday, April 12, 2010 05:33:14

Page 3

ICPMS#4 - Summary Report

Sample ID: 1202056876

Sample Date/Time: Monday, April 12, 2010 05:36:41

Sample Type:

Sample Description: LANL 6020 SDILT

Number of Replicates: 3

Batch ID: 959112|5|bcd1

Method File: c:\elandata\Method\6020.mth

Dataset File: c:\elandata\Dataset\100408\1202056876.578

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Li	7	0.057	ug/L	13.763	64	0.000
Be	9	0.019	ug/L	135.259	9	0.000
B	11	4.705	ug/L	6.437	750	0.001
Na	23	20.084	ug/L	27.915	44404	0.052
Mg	24	2.759	ug/L	28.811	4001	0.005
Al	27	2.779	ug/L	11.564	5334	0.007
P	31	1.873	ug/L	59.405	3090	0.000
K	39	2.018	ug/L	156.933	384442	0.009
Ca	43	23.514	ug/L	12.351	344	0.000
Sc	45		ug/L		639817	639817.135
Ti	47	0.233	ug/L	8.448	245	0.000
V	51	-0.158	ug/L	452.055	19635	-0.001
Cr	52	-0.930	ug/L	15.590	-14050	-0.004
Cr	53		ug/L		194517	0.108
Mn	55	0.130	ug/L	7.403	1396	0.001
Fe	57	1.343	ug/L	100.892	5566	0.000
Co	59	0.026	ug/L	5.274	250	0.000
Ni	60	0.030	ug/L	11.981	94	0.000
Cu	63		ug/L		2285	-0.000
Cu	65	-0.255	ug/L	7.267	1084	-0.000
Zn	66	-0.144	ug/L	111.964	1186	-0.000
Zn	67		ug/L		11711	0.017
Zn	68		ug/L		1589	0.001
Ge	74		ug/L		261765	261764.795
As	75	0.901	ug/L	40.481	676	0.002
Se	77		ug/L		11146	0.022
Se	82	0.418	ug/L	83.108	57	0.000
Kr	83		ug/L		51	-0.000
Sr	88	0.043	ug/L	9.811	573	0.002
Y	89		ug/L		41	0.000
Zr	90	0.034	ug/L	35.882	706	0.001
Mo	98	0.054	ug/L	17.545	603	0.001
Ag	107	0.032	ug/L	10.191	283	0.001
Cd	111	-0.006	ug/L	134.627	17	-0.000
Cd	114		ug/L		30	-0.000
In	115		ug/L		161127	161127.437
Sn	120	0.203	ug/L	19.640	1755	0.005
Sb	121	0.059	ug/L	53.057	827	0.001
Sb	123		ug/L		649	0.001
Ba	135		ug/L		81	0.000
Ba	137	0.075	ug/L	8.815	143	0.001
Ho	165		ug/L		9	-0.000
Lu	175		ug/L		192513	192513.157
Tl	205	2.680	ug/L	12.956	15509	0.074
Pb	208	0.081	ug/L	6.472	5116	0.004
Th	232	0.281	ug/L	18.226	4304	0.015
U	238	0.012	ug/L	190.932	715	0.001

Sample ID: 1202056876

Report Date/Time: Monday, April 12, 2010 05:39:28

Page 1

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Li	7Linear Thru Zero	1.0000
Be	9Linear Thru Zero	1.0000
B	11Linear Thru Zero	1.0000
Na	23Linear Thru Zero	1.0000
Mg	24Linear Thru Zero	1.0000
Al	27Linear Thru Zero	1.0000
P	31Linear Thru Zero	1.0000
K	39Linear Thru Zero	1.0000
Ca	43Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ti	47Linear Thru Zero	1.0000
V	51Linear Thru Zero	0.9999
Cr	52Linear Thru Zero	1.0000
Cr	53Linear Thru Zero	
Mn	55Linear Thru Zero	1.0000
Fe	57Linear Thru Zero	1.0000
Co	59Linear Thru Zero	1.0000
Ni	60Linear Thru Zero	1.0000
Cu	63Linear Thru Zero	
Cu	65Linear Thru Zero	1.0000
Zn	66Linear Thru Zero	1.0000
Zn	67Linear Thru Zero	
Zn	68Linear Thru Zero	
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	0.9998
Kr	83Linear Thru Zero	
Sr	88Linear Thru Zero	1.0000
Y	89Linear Thru Zero	
Zr	90Linear Thru Zero	1.0000
Mo	98Linear Thru Zero	1.0000
Ag	107Linear Thru Zero	1.0000
Cd	111Linear Thru Zero	1.0000
Cd	114Linear Thru Zero	
In	115Linear Thru Zero	
Sn	120Linear Thru Zero	1.0000
Sb	121Linear Thru Zero	0.9997
Sb	123Linear Thru Zero	
Ba	135Linear Thru Zero	
Ba	137Linear Thru Zero	1.0000
Ho	165Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000
Pb	208Linear Thru Zero	1.0000
Th	232Linear Thru Zero	1.0000
U	238Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Diff	Dup. Rel. % Diff
Li	7					
Be	9					
B	11					
Na	23					
Mg	24					
Al	27					
P	31					
K	39					
Ca	43					
> Sc	45		99.2			
Ti	47					
V	51					
Cr	52					
Cr	53					
Mn	55					
Fe	57					
Co	59					
Ni	60					
Cu	63					
Cu	65					
Zn	66					
Zn	67					
Zn	68					
> Ge	74		100.6			
As	75					
Se	77					
Se	82					
Kr	83					
Sr	88					
Y	89					
Zr	90					
Mo	98					
Ag	107					
Cd	111					
Cd	114					
> In	115		98.6			
Sn	120					
Sb	121					
Sb	123					
Ba	135					
Ba	137					
Ho	165					
> Lu	175		99.4			
Tl	205					
Pb	208					
Th	232					
U	238					

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: 1202056876

Report Date/Time: Monday, April 12, 2010 05:39:28

Page 3

ICPMS#4 - Summary Report

Sample ID: QC Std 6

Sample Date/Time: Monday, April 12, 2010 05:42:53

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\6020.mth

Dataset File: c:\elandata\Dataset\100408\QC Std 6.579

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Li	7	51.720	ug/L	1.757	30736	0.049
Be	9	50.903	ug/L	1.715	7919	0.013
B	11	99.402	ug/L	1.099	13523	0.021
Na	23	5683.830	ug/L	6.494	9331555	14.805
Mg	24	4766.103	ug/L	2.714	5666856	8.998
Al	27	5113.478	ug/L	3.764	8459736	13.434
P	31	4864.794	ug/L	0.505	475881	0.751
K	39	4925.418	ug/L	5.634	14519623	22.453
Ca	43	4849.215	ug/L	1.453	29609	0.047
> Sc	45		ug/L		629840	629839.788
Ti	47	49.411	ug/L	2.449	15628	0.025
V	51	51.095	ug/L	3.366	224538	0.325
Cr	52	51.563	ug/L	1.471	145299	0.248
Cr	53		ug/L		125730	0.004
Mn	55	52.023	ug/L	1.914	263235	0.417
Fe	57	4909.381	ug/L	1.235	508424	0.799
Co	59	50.172	ug/L	2.477	195373	0.310
Ni	60	52.152	ug/L	1.643	43377	0.069
Cu	63		ug/L		103339	0.160
Cu	65	52.900	ug/L	1.535	50044	0.077
Zn	66	51.383	ug/L	3.220	29731	0.111
Zn	67		ug/L		10948	0.015
Zn	68		ug/L		21826	0.080
> Ge	74		ug/L		256530	256530.478
As	75	50.277	ug/L	3.169	32898	0.128
Se	77		ug/L		6659	0.005
Se	82	46.676	ug/L	0.991	2848	0.011
Kr	83		ug/L		52	-0.000
Sr	88	50.513	ug/L	1.869	455731	2.858
Y	89		ug/L		37	0.000
Zr	90	47.917	ug/L	1.419	236065	1.478
Mo	98	48.577	ug/L	1.226	105249	0.657
Ag	107	50.757	ug/L	2.517	172589	1.082
Cd	111	50.014	ug/L	1.181	40483	0.254
Cd	114		ug/L		95085	0.596
> In	115		ug/L		159427	159426.925
Sn	120	48.990	ug/L	1.789	176290	1.100
Sb	121	54.951	ug/L	2.862	136753	0.853
Sb	123		ug/L		104461	0.652
Ba	135		ug/L		42677	0.221
Ba	137	48.751	ug/L	2.080	73940	0.384
Ho	165		ug/L		14	0.000
> Lu	175		ug/L		192615	192614.780
Tl	205	48.237	ug/L	0.359	258748	1.337
Pb	208	50.379	ug/L	1.700	523786	2.697
Th	232	49.973	ug/L	2.542	523249	2.709
U	238	53.198	ug/L	1.145	541011	2.806

Sample ID: QC Std 6

Report Date/Time: Monday, April 12, 2010 05:45:37

Page 1

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Li	7Linear Thru Zero	1.0000
Be	9Linear Thru Zero	1.0000
B	11Linear Thru Zero	1.0000
Na	23Linear Thru Zero	1.0000
Mg	24Linear Thru Zero	1.0000
Al	27Linear Thru Zero	1.0000
P	31Linear Thru Zero	1.0000
K	39Linear Thru Zero	1.0000
Ca	43Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ti	47Linear Thru Zero	1.0000
V	51Linear Thru Zero	0.9999
Cr	52Linear Thru Zero	1.0000
Cr	53Linear Thru Zero	
Mn	55Linear Thru Zero	1.0000
Fe	57Linear Thru Zero	1.0000
Co	59Linear Thru Zero	1.0000
Ni	60Linear Thru Zero	1.0000
Cu	63Linear Thru Zero	
Cu	65Linear Thru Zero	1.0000
Zn	66Linear Thru Zero	1.0000
Zn	67Linear Thru Zero	
Zn	68Linear Thru Zero	
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	0.9998
Kr	83Linear Thru Zero	
Sr	88Linear Thru Zero	1.0000
Y	89Linear Thru Zero	
Zr	90Linear Thru Zero	1.0000
Mo	98Linear Thru Zero	1.0000
Ag	107Linear Thru Zero	1.0000
Cd	111Linear Thru Zero	1.0000
Cd	114Linear Thru Zero	
In	115Linear Thru Zero	
Sn	120Linear Thru Zero	1.0000
Sb	121Linear Thru Zero	0.9997
Sb	123Linear Thru Zero	
Ba	135Linear Thru Zero	
Ba	137Linear Thru Zero	1.0000
Ho	165Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000
Pb	208Linear Thru Zero	1.0000
Th	232Linear Thru Zero	1.0000
U	238Linear Thru Zero	1.0000

QC Calculated Values

	Analyte	Mass	QC Std	% Recovery	Int Std	% Recovery	Spike	% Recovery	Dilution	% Diff	Dup. Rel.	% Diff
[Li	7		103.439								
	Be	9		101.806								
	B	11		99.402								
	Na	23		113.677								
	Mg	24		95.322								
	Al	27		101.257								
	P	31		97.296								
	K	39		98.508								
	Ca	43		96.984								
>	Sc	45						97.7				
	Ti	47		98.823								
	V	51		102.189								
	Cr	52		103.126								
	Cr	53										
	Mn	55		104.047								
	Fe	57		98.188								
	Co	59		100.345								
	Ni	60		104.304								
	Cu	63										
	Cu	65		105.800								
	Zn	66		102.766								
	Zn	67										
	Zn	68										
>	Ge	74						98.6				
	As	75		100.554								
	Se	77										
	Se	82		93.352								
	Kr	83										
	Sr	88		101.027								
	Y	89										
	Zr	90		95.834								
	Mo	98		97.154								
	Ag	107		101.515								
	Cd	111		100.029								
	Cd	114										
>	In	115						97.6				
	Sn	120		97.981								
	Sb	121		109.902								
	Sb	123										
	Ba	135										
	Ba	137		97.503								
	Ho	165										
>	Lu	175						99.4				
	Tl	205		96.474								
	Pb	208		100.759								
	Th	232		99.946								
	U	238		106.397								

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message
 QC Std 6 Na 23CCV is out of limits (+/- 10%)

QC Action

QC Action Line: Continue

ICPMS#4 - Summary Report

Sample ID: QC Std 7

Sample Date/Time: Monday, April 12, 2010 05:49:03

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\6020.mth

Dataset File: c:\elandata\Dataset\100408\QC Std 7.580

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Li	7	0.016	ug/L	70.693	38	0.000
Be	9	0.016	ug/L	107.694	8	0.000
B	11	1.302	ug/L	16.447	278	0.000
Na	23	-0.431	ug/L	1267.292	10005	-0.001
Mg	24	1.700	ug/L	57.325	2667	0.003
Al	27	1.222	ug/L	57.324	2667	0.003
P	31	2.174	ug/L	38.795	3064	0.000
K	39	-5.483	ug/L	94.620	356054	-0.025
Ca	43	11.857	ug/L	31.531	267	0.000
Sc	45		ug/L		628463	628462.563
Ti	47	0.088	ug/L	154.404	196	0.000
V	51	-0.482	ug/L	144.274	17973	-0.003
Cr	52	0.109	ug/L	19.617	-10659	0.001
Cr	53		ug/L		123875	0.001
Mn	55	0.006	ug/L	174.065	744	0.000
Fe	57	1.135	ug/L	163.202	5446	0.000
Co	59	0.009	ug/L	30.186	179	0.000
Ni	60	0.019	ug/L	112.743	83	0.000
Cu	63		ug/L		1909	-0.001
Cu	65	-0.345	ug/L	11.503	982	-0.001
Zn	66	-0.748	ug/L	3.421	821	-0.002
Zn	67		ug/L		7288	0.001
Zn	68		ug/L		1137	-0.001
Ge	74		ug/L		254718	254717.757
As	75	0.131	ug/L	370.804	156	0.000
Se	77		ug/L		5725	0.002
Se	82	1.372	ug/L	21.012	112	0.000
Kr	83		ug/L		51	-0.000
Sr	88	0.009	ug/L	43.594	259	0.001
Y	89		ug/L		21	-0.000
Zr	90	0.233	ug/L	17.927	1684	0.007
Mo	98	0.339	ug/L	15.313	1216	0.005
Ag	107	0.041	ug/L	15.479	311	0.001
Cd	111	0.005	ug/L	249.476	25	0.000
Cd	114		ug/L		68	0.000
In	115		ug/L		159918	159918.394
Sn	120	0.084	ug/L	10.297	1313	0.002
Sb	121	1.242	ug/L	24.611	3759	0.019
Sb	123		ug/L		2966	0.015
Ba	135		ug/L		30	0.000
Ba	137	0.015	ug/L	38.536	53	0.000
Ho	165		ug/L		12	0.000
Lu	175		ug/L		190007	190007.488
Tl	205	1.121	ug/L	9.930	7077	0.031
Pb	208	-0.016	ug/L	36.498	4057	-0.001
Th	232	0.429	ug/L	24.961	5764	0.023
U	238	0.019	ug/L	63.535	775	0.001

Sample ID: QC Std 7

Report Date/Time: Monday, April 12, 2010 05:51:48

Page 1

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Li	7Linear Thru Zero	1.0000
Be	9Linear Thru Zero	1.0000
B	11Linear Thru Zero	1.0000
Na	23Linear Thru Zero	1.0000
Mg	24Linear Thru Zero	1.0000
Al	27Linear Thru Zero	1.0000
P	31Linear Thru Zero	1.0000
K	39Linear Thru Zero	1.0000
Ca	43Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ti	47Linear Thru Zero	1.0000
V	51Linear Thru Zero	0.9999
Cr	52Linear Thru Zero	1.0000
Cr	53Linear Thru Zero	
Mn	55Linear Thru Zero	1.0000
Fe	57Linear Thru Zero	1.0000
Co	59Linear Thru Zero	1.0000
Ni	60Linear Thru Zero	1.0000
Cu	63Linear Thru Zero	
Cu	65Linear Thru Zero	1.0000
Zn	66Linear Thru Zero	1.0000
Zn	67Linear Thru Zero	
Zn	68Linear Thru Zero	
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	0.9998
Kr	83Linear Thru Zero	
Sr	88Linear Thru Zero	1.0000
Y	89Linear Thru Zero	
Zr	90Linear Thru Zero	1.0000
Mo	98Linear Thru Zero	1.0000
Ag	107Linear Thru Zero	1.0000
Cd	111Linear Thru Zero	1.0000
Cd	114Linear Thru Zero	
In	115Linear Thru Zero	
Sn	120Linear Thru Zero	1.0000
Sb	121Linear Thru Zero	0.9997
Sb	123Linear Thru Zero	
Ba	135Linear Thru Zero	
Ba	137Linear Thru Zero	1.0000
Ho	165Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000
Pb	208Linear Thru Zero	1.0000
Th	232Linear Thru Zero	1.0000
U	238Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Diff	Dup. Rel. % Diff
Li	7					
Be	9					
B	11					
Na	23					
Mg	24					
Al	27					
P	31					
K	39					
Ca	43					
> Sc	45		97.5			
Ti	47					
V	51					
Cr	52					
Cr	53					
Mn	55					
Fe	57					
Co	59					
Ni	60					
Cu	63					
Cu	65					
Zn	66					
Zn	67					
Zn	68					
> Ge	74		97.9			
As	75					
Se	77					
Se	82					
Kr	83					
Sr	88					
Y	89					
Zr	90					
Mo	98					
Ag	107					
Cd	111					
Cd	114					
> In	115		97.9			
Sn	120					
Sb	121					
Sb	123					
Ba	135					
Ba	137					
Ho	165					
> Lu	175		98.1			
Tl	205					
Pb	208					
Th	232					
U	238					

QC Out Of Limits

Measurement Type	Analyte	MassOut of Limits Message
QC Std 7	Ti	205CCB is out of limits (+/- PQL)

QC Action

QC Action Line: Continue

Sample ID: QC Std 7
Report Date/Time: Monday, April 12, 2010 05:51:48
Page 3

ICPMS #5 Daily Performance Report

Sample ID: Sample

Sample Date/Time: Tuesday, April 13, 2010 11:33:12

Sample Description:

Method File: c:\elandata\Method\Daily2.mth

Dataset File: c:\elandata\Dataset\default\Sample.1054

Tuning File: c:\elandata\Tuning\default2.tun

Optimization File: c:\elandata\Optimize\default.dac

Dual Detector Mode: Pulse

Acq. Dead Time(ns): 35

Current Dead Time (ns): 35

Number of Replicates: 5

Summary

Analyte	Mass	Meas. Intens.	Mean	Net Intens.	Mean	Net Intens.	SD	Net Intens.	RSD
Be	9.0		1541.9		1541.883		43.705		2.8
Mg	24.0		38738.9		38738.859		434.290		1.1
Co	58.9		63185.8		63185.831		373.250		0.6
Rh	102.9		123622.6		123622.601		766.014		0.6
In	114.9		178721.4		178721.441		1254.626		0.7
Pb	208.0		214246.1		214246.105		2038.893		1.0
[> Ba	137.9		169586.4		169586.427		957.403		0.6
[Ba++	69.0		1987.6		0.012		0.000		2.3
[> Ce	139.9		205613.0		205612.974		1509.978		0.7
[CeO	155.9		4192.2		0.020		0.000		2.1
Bkgd	220.0		19.8		19.800		2.564		13.0

Current Optimization File Data

Current Value	Description
0.86	Nebulizer Gas Flow
6.75	Lens Voltage
1450.00	ICP RF Power
-1812.50	Analog Stage Voltage
1300.00	Pulse Stage Voltage
200.00	Discriminator Threshold
-6.00	AC Rod Offset

Current Autolens Data

Analyte	Mass	Num of Pts	DAC Value	Maximum Intensity
Be	9	21	7.0	3372.1
Co	59	21	7.8	60333.1
In	115	21	9.5	172853.8

ICPMS #5 Instrument Tuning Report

File Name: 100413.tun
File Path: C:\elandata\Tuning

Analyte	Exact Mass	Meas. Mass	Mass DAC	Res. DAC	Meas. Pk. Width
He	3.0	3.0	606	2072	0.540
Be	9.0	9.0	2061	2088	0.543
Mg	24.0	24.0	5699	2085	0.562
Mg	25.0	25.0	5939	2085	0.540
Mg	26.0	26.0	6187	2100	0.545
Co	58.9	59.0	14193	2125	0.528
Rh	102.9	102.9	24880	2180	0.530
In	114.9	114.9	27796	2200	0.535
Ce	139.9	139.9	33878	2220	0.547
Pb	206.0	206.0	49948	2305	0.522
Pb	207.0	207.0	50171	2240	0.593
Pb	208.0	208.0	50451	2280	0.636
U	238.1	238.0	57731	2295	0.641

ICPMS#5 - Summary Report

Sample ID: Blank
Sample Date/Time: Tuesday, April 13, 2010 11:45:01
Sample Type:
Sample Description:
Number of Replicates: 3
Batch ID:
Method File: c:\elandata\Method\sb and u.mth
Dataset File: C:\elandata\Dataset\100413\Blank.001

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	In	115		ug/L		185761	
	Sn	120		ug/L		601	
	Sb	121		ug/L		81	
	Sb	123		ug/L		67	
[>	Lu	175		ug/L		392643	
	U	238		ug/L		76	

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
In	115	Simple Linear	
Sn	120	Simple Linear	
Sb	121	Simple Linear	
Sb	123	Simple Linear	
Lu	175	Simple Linear	
U	238	Simple Linear	

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[>	In	115						
	Sn	120						
	Sb	121						
	Sb	123						
[>	Lu	175						
	U	238						

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

ICPMS#5 - Summary Report

Sample ID: Standard 1

Sample Date/Time: Tuesday, April 13, 2010 11:47:29

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\sb and u.mth

Dataset File: C:\elandata\Dataset\100413\Standard 1.002

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	In	115		ug/L		182036	182035.964
	Sn	120	10.000	ug/L	2.014	53910	0.293
	Sb	121	10.000	ug/L	2.863	41462	0.227
	Sb	123		ug/L		32322	0.177
[>	Lu	175		ug/L		382362	382362.256
	U	238	10.000	ug/L	3.365	459323	1.201

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
In	115	Linear Thru Zero	
Sn	120	Linear Thru Zero	1.0000
Sb	121	Linear Thru Zero	1.0000
Sb	123	Linear Thru Zero	
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	1.0000

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[>	In	115						
	Sn	120						
	Sb	121						
	Sb	123						
[>	Lu	175						
	U	238						

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: Standard 1

Report Date/Time: Tuesday, April 13, 2010 11:47:57

Page 1

ICPMS#5 - Summary Report

Sample ID: Standard 2

Sample Date/Time: Tuesday, April 13, 2010 11:49:55

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\sb and u.mth

Dataset File: C:\elandata\Dataset\100413\Standard 2.003

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	In	115		ug/L		184236	184236.210
	Sn	120	99.964	ug/L	2.074	521119	2.826
	Sb	121	100.049	ug/L	1.558	440889	2.393
	Sb	123		ug/L		342818	1.861
[>	Lu	175		ug/L		399772	399771.738
	U	238	99.900	ug/L	1.081	4361704	10.910

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
In	115	Linear Thru Zero	
Sn	120	Linear Thru Zero	1.0000
Sb	121	Linear Thru Zero	1.0000
Sb	123	Linear Thru Zero	
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	0.9999

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[>	In	115						
	Sn	120						
	Sb	121						
	Sb	123						
[>	Lu	175						
	U	238						

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: Standard 2

Report Date/Time: Tuesday, April 13, 2010 11:50:23

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 1

Sample Date/Time: Tuesday, April 13, 2010 11:52:21

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\sb and u.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 1.004

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	In	115		ug/L		184783	184782.938
	Sn	120	50.255	ug/L	2.353	263015	1.421
	Sb	121	53.137	ug/L	3.381	234778	1.271
	Sb	123		ug/L		182858	0.989
[>	Lu	175		ug/L		396367	396366.712
	U	238	51.729	ug/L	1.463	2238990	5.649

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
In	115	Linear Thru Zero	
Sn	120	Linear Thru Zero	1.0000
Sb	121	Linear Thru Zero	1.0000
Sb	123	Linear Thru Zero	
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	0.9999

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[>	In	115			99.5			
	Sn	120	100.511					
	Sb	121	106.273					
	Sb	123						
[>	Lu	175			100.9			
	U	238	103.458					

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 1

Report Date/Time: Tuesday, April 13, 2010 11:52:49

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 2

Sample Date/Time: Tuesday, April 13, 2010 11:54:49

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\sb and u.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 2.005

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[> In	115		ug/L		186749	186749.324
Sn	120	-0.014	ug/L	83.102	532	-0.000
Sb	121	0.344	ug/L	3.857	1616	0.008
Sb	123		ug/L		1273	0.006
[> Lu	175		ug/L		394533	394532.622
U	238	0.005	ug/L	10.622	275	0.001

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
In	115	Linear Thru Zero	
Sn	120	Linear Thru Zero	1.0000
Sb	121	Linear Thru Zero	1.0000
Sb	123	Linear Thru Zero	
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	0.9999

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel. % Difference
[> In	115		100.5			
Sn	120					
Sb	121					
Sb	123					
[> Lu	175		100.5			
U	238					

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message

QC Action

QC Action Line: No QC out of limits detected

ICPMS#5 - Summary Report

Sample ID: QC Std 3

Sample Date/Time: Tuesday, April 13, 2010 11:57:18

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\sb and u.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 3.006

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	In	115		ug/L		187234	187233.558
	Sn	120	5.598	ug/L	2.621	30227	0.158
	Sb	121	2.944	ug/L	1.367	13265	0.070
	Sb	123		ug/L		10433	0.055
[>	Lu	175		ug/L		396608	396607.555
	U	238	0.301	ug/L	2.546	13096	0.033

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
In	115	Linear Thru Zero	
Sn	120	Linear Thru Zero	1.0000
Sb	121	Linear Thru Zero	1.0000
Sb	123	Linear Thru Zero	
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	0.9999

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[>	In	115		100.8				
	Sn	120	111.957					
	Sb	121	98.142					
	Sb	123						
[>	Lu	175		101.0				
	U	238	150.304					

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
QC Std 3	U	238	CRDL is out of limits

QC Action

QC Action Line: Continue

Sample ID: QC Std 3

Report Date/Time: Tuesday, April 13, 2010 11:57:47

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 4

Sample Date/Time: Tuesday, April 13, 2010 11:59:45

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\sb and u.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 4.007

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	In	115		ug/L		163099	163099.298
	Sn	120	0.204	ug/L	2.717	1469	0.006
	Sb	121	0.265	ug/L	3.152	1103	0.006
	Sb	123		ug/L		895	0.005
[>	Lu	175		ug/L		355401	355400.625
	U	238	0.002	ug/L	19.302	147	0.000

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
In	115	Linear Thru Zero	
Sn	120	Linear Thru Zero	1.0000
Sb	121	Linear Thru Zero	1.0000
Sb	123	Linear Thru Zero	
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	0.9999

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[>	In	115			87.8			
	Sn	120						
	Sb	121						
	Sb	123						
[>	Lu	175			90.5			
	U	238						

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 4

Report Date/Time: Tuesday, April 13, 2010 12:00:14

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 5

Sample Date/Time: Tuesday, April 13, 2010 12:02:12

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\sb and u.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 5.008

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	In	115		ug/L		164246	164245.716
	Sn	120	20.117	ug/L	2.678	93906	0.569
	Sb	121	20.261	ug/L	2.170	79645	0.485
	Sb	123		ug/L		62352	0.379
[>	Lu	175		ug/L		356670	356669.933
	U	238	21.125	ug/L	0.769	822958	2.307

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
In	115	Linear Thru Zero	
Sn	120	Linear Thru Zero	1.0000
Sb	121	Linear Thru Zero	1.0000
Sb	123	Linear Thru Zero	
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	0.9999

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[>	In	115			88.4			
	Sn	120	100.587					
	Sb	121	101.307					
	Sb	123						
[>	Lu	175			90.8			
	U	238	105.631					

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 5

Report Date/Time: Tuesday, April 13, 2010 12:02:42

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 6

Sample Date/Time: Tuesday, April 13, 2010 12:04:40

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\sb and u.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 6.009

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	In	115		ug/L		180800	180799.988
	Sn	120	49.813	ug/L	3.483	255017	1.408
	Sb	121	52.557	ug/L	3.494	227209	1.257
	Sb	123		ug/L		178584	0.988
[>	Lu	175		ug/L		384201	384200.999
	U	238	52.168	ug/L	0.479	2188900	5.697

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
In	115	Linear Thru Zero	
Sn	120	Linear Thru Zero	1.0000
Sb	121	Linear Thru Zero	1.0000
Sb	123	Linear Thru Zero	
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	0.9999

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[>	In	115		97.3				
	Sn	120	99.627					
	Sb	121	105.114					
	Sb	123						
[>	Lu	175		97.8				
	U	238	104.336					

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 6

Report Date/Time: Tuesday, April 13, 2010 12:05:10

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 7

Sample Date/Time: Tuesday, April 13, 2010 12:07:10

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\sb and u.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 7.010

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	In	115		ug/L		178005	178004.541
	Sn	120	-0.027	ug/L	23.813	442	-0.001
	Sb	121	0.191	ug/L	2.212	892	0.005
	Sb	123		ug/L		687	0.004
[>	Lu	175		ug/L		382061	382060.614
	U	238	0.003	ug/L	10.893	210	0.000

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
In	115	Linear Thru Zero	
Sn	120	Linear Thru Zero	1.0000
Sb	121	Linear Thru Zero	1.0000
Sb	123	Linear Thru Zero	
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	0.9999

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[>	In	115		95.8			
	Sn	120					
	Sb	121					
	Sb	123					
[>	Lu	175		97.3			
	U	238					

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 7

Report Date/Time: Tuesday, April 13, 2010 12:07:40

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 8

Sample Date/Time: Tuesday, April 13, 2010 12:31:44

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\sb and u.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 8.020

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	In	115		ug/L		179880	179879.590
	Sn	120	50.183	ug/L	0.622	255755	1.419
	Sb	121	52.882	ug/L	0.671	227587	1.265
	Sb	123		ug/L		177328	0.985
[>	Lu	175		ug/L		385933	385933.317
	U	238	51.782	ug/L	2.522	2181888	5.655

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
In	115	Linear Thru Zero	
Sn	120	Linear Thru Zero	1.0000
Sb	121	Linear Thru Zero	1.0000
Sb	123	Linear Thru Zero	
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	0.9999

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Di	Duplicate Rel.	% Difference
[>	In	115		96.8				
	Sn	120	100.367					
	Sb	121	105.764					
	Sb	123						
[>	Lu	175		98.3				
	U	238	103.564					

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 8

Report Date/Time: Tuesday, April 13, 2010 12:32:13

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 9

Sample Date/Time: Tuesday, April 13, 2010 12:34:13

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\sb and u.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 9.021

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[> In	115		ug/L		180084	180084.005
Sn	120	-0.039	ug/L	7.068	383	-0.001
Sb	121	0.142	ug/L	4.782	688	0.003
Sb	123		ug/L		548	0.003
[> Lu	175		ug/L		382471	382471.262
U	238	0.004	ug/L	7.628	243	0.000

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
In	115	Linear Thru Zero	
Sn	120	Linear Thru Zero	1.0000
Sb	121	Linear Thru Zero	1.0000
Sb	123	Linear Thru Zero	
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	0.9999

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[> In	115		96.9				
Sn	120						
Sb	121						
Sb	123						
[> Lu	175		97.4				
U	238						

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 9

Report Date/Time: Tuesday, April 13, 2010 12:34:43

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 8

Sample Date/Time: Tuesday, April 13, 2010 12:53:55

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\sb and u.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 8.029

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	In	115		ug/L		179439	179438.954
	Sn	120	49.856	ug/L	1.546	253434	1.409
	Sb	121	52.280	ug/L	2.701	224406	1.250
	Sb	123		ug/L		175814	0.980
[>	Lu	175		ug/L		380571	380570.868
	U	238	51.864	ug/L	1.091	2155752	5.664

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
In	115	Linear Thru Zero	
Sn	120	Linear Thru Zero	1.0000
Sb	121	Linear Thru Zero	1.0000
Sb	123	Linear Thru Zero	
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	0.9999

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[>	In	115		96.6				
	Sn	120	99.711					
	Sb	121	104.560					
	Sb	123						
[>	Lu	175		96.9				
	U	238	103.728					

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 8

Report Date/Time: Tuesday, April 13, 2010 12:54:24

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 9

Sample Date/Time: Tuesday, April 13, 2010 12:56:24

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\sb and u.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 9.030

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	In	115		ug/L		178375	178374.506
	Sn	120	-0.037	ug/L	13.537	393	-0.001
	Sb	121	0.145	ug/L	3.498	696	0.003
	Sb	123		ug/L		550	0.003
[>	Lu	175		ug/L		376824	376824.203
	U	238	0.004	ug/L	28.193	240	0.000

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
In	115	Linear Thru Zero	
Sn	120	Linear Thru Zero	1.0000
Sb	121	Linear Thru Zero	1.0000
Sb	123	Linear Thru Zero	
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	0.9999

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[>	In	115		96.0				
	Sn	120						
	Sb	121						
	Sb	123						
[>	Lu	175		96.0				
	U	238						

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 9

Report Date/Time: Tuesday, April 13, 2010 12:56:55

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 8

Sample Date/Time: Tuesday, April 13, 2010 13:21:54

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\sb and u.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 8.039

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[> In	115		ug/L		181343	181343.112
Sn	120	49.625	ug/L	1.270	254948	1.403
Sb	121	51.369	ug/L	0.964	222861	1.229
Sb	123		ug/L		175048	0.965
[> Lu	175		ug/L		380870	380870.172
U	238	51.061	ug/L	0.982	2123878	5.576

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
In	115	Linear Thru Zero	
Sn	120	Linear Thru Zero	1.0000
Sb	121	Linear Thru Zero	1.0000
Sb	123	Linear Thru Zero	
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	0.9999

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[> In	115			97.6		
Sn	120	99.251				
Sb	121	102.737				
Sb	123					
[> Lu	175			97.0		
U	238	102.121				

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 8

Report Date/Time: Tuesday, April 13, 2010 13:22:24

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 9

Sample Date/Time: Tuesday, April 13, 2010 13:24:23

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\sb and u.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 9.040

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	In	115		ug/L		182593	182593.360
	Sn	120	-0.048	ug/L	9.118	341	-0.001
	Sb	121	0.142	ug/L	3.687	700	0.003
	Sb	123		ug/L		534	0.003
[>	Lu	175		ug/L		384056	384055.625
	U	238	0.004	ug/L	3.626	253	0.000

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
In	115	Linear Thru Zero	
Sn	120	Linear Thru Zero	1.0000
Sb	121	Linear Thru Zero	1.0000
Sb	123	Linear Thru Zero	
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	0.9999

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[>	In	115			98.3		
	Sn	120					
	Sb	121					
	Sb	123					
[>	Lu	175			97.8		
	U	238					

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 9

Report Date/Time: Tuesday, April 13, 2010 13:24:54

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 8

Sample Date/Time: Tuesday, April 13, 2010 13:36:45

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\sb and u.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 8.045

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	In	115		ug/L		169071	169071.440
	Sn	120	49.887	ug/L	2.022	238915	1.410
	Sb	121	52.708	ug/L	3.274	213128	1.261
	Sb	123		ug/L		164071	0.970
[>	Lu	175		ug/L		364393	364393.398
	U	238	49.365	ug/L	2.181	1964182	5.391

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
In	115	Linear Thru Zero	
Sn	120	Linear Thru Zero	1.0000
Sb	121	Linear Thru Zero	1.0000
Sb	123	Linear Thru Zero	
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	0.9999

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[>	In	115		91.0				
	Sn	120	99.775					
	Sb	121	105.416					
	Sb	123						
[>	Lu	175		92.8				
	U	238	98.730					

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 8

Report Date/Time: Tuesday, April 13, 2010 13:37:15

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 9

Sample Date/Time: Tuesday, April 13, 2010 13:39:15

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\sb and u.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 9.046

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	In	115		ug/L		179196	179196.267
	Sn	120	-0.042	ug/L	10.523	368	-0.001
	Sb	121	0.141	ug/L	7.956	681	0.003
	Sb	123		ug/L		547	0.003
[>	Lu	175		ug/L		383407	383407.402
	U	238	0.006	ug/L	16.687	322	0.001

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
In	115	Linear Thru Zero	
Sn	120	Linear Thru Zero	1.0000
Sb	121	Linear Thru Zero	1.0000
Sb	123	Linear Thru Zero	
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	0.9999

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[>	In	115			96.5			
	Sn	120						
	Sb	121						
	Sb	123						
[>	Lu	175			97.6			
	U	238						

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 9

Report Date/Time: Tuesday, April 13, 2010 13:39:45

Page 1

ICPMS#5 - Summary Report

Sample ID: 1202056872

Sample Date/Time: Tuesday, April 13, 2010 13:41:44

Sample Type:

Sample Description: LANL 6020 MB

Number of Replicates: 3

Batch ID: 959112|1|prb

Method File: c:\elandata\Method\sb and u.mth

Dataset File: C:\elandata\Dataset\100413\1202056872.047

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[> In	115		ug/L		183873	183872.913
Sn	120	0.022	ug/L	42.356	708	0.001
Sb	121	0.108	ug/L	1.614	556	0.003
Sb	123		ug/L		434	0.002
[> Lu	175		ug/L		375289	375288.864
U	238	0.028	ug/L	4.765	1211	0.003

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
In	115	Linear Thru Zero	
Sn	120	Linear Thru Zero	1.0000
Sb	121	Linear Thru Zero	1.0000
Sb	123	Linear Thru Zero	
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	0.9999

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[> In	115		99.0				
Sn	120						
Sb	121						
Sb	123						
[> Lu	175		95.6				
U	238						

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: 1202056872

Report Date/Time: Tuesday, April 13, 2010 13:42:13

Page 1

ICPMS#5 - Summary Report

Sample ID: 1202056873

Sample Date/Time: Tuesday, April 13, 2010 13:44:12

Sample Type:

Sample Description: LANL 6020 LCS

Number of Replicates: 3

Batch ID: 959112|1|prb

Method File: c:\elandata\Method\sb and u.mth

Dataset File: C:\elandata\Dataset\100413\1202056873.048

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	In 115		ug/L		185224	185224.369
	Sn 120	52.005	ug/L	2.009	272834	1.470
	Sb 121	55.050	ug/L	1.670	243921	1.317
	Sb 123		ug/L		189522	1.023
[>	Lu 175		ug/L		394091	394090.713
	U 238	49.007	ug/L	0.427	2109270	5.352

Calibration

Analyte	MassCurve Type	Correlation Coefficient
In	115Linear Thru Zero	
Sn	120Linear Thru Zero	1.0000
Sb	121Linear Thru Zero	1.0000
Sb	123Linear Thru Zero	
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	0.9999

QC Calculated Values

Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[> In 115			99.7			
Sn 120						
Sb 121						
Sb 123						
[> Lu 175		100.4				
U 238						

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: 1202056873

Report Date/Time: Tuesday, April 13, 2010 13:44:42

Page 1

ICPMS#5 - Summary Report

Sample ID: 248117001

Sample Date/Time: Tuesday, April 13, 2010 13:49:09

Sample Type:

Sample Description: LANL 6020

Number of Replicates: 3

Batch ID: 959112|1|prb

Method File: c:\elandata\Method\sb and u.mth

Dataset File: C:\elandata\Dataset\100413\248117001.050

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	In	115		ug/L		190547	190547.456
	Sn	120	0.040	ug/L	21.676	833	0.001
	Sb	121	0.035	ug/L	9.798	240	0.001
	Sb	123		ug/L		196	0.001
[>	Lu	175		ug/L		394576	394575.851
	U	238	0.008	ug/L	7.421	417	0.001

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
In	115	Linear Thru Zero	
Sn	120	Linear Thru Zero	1.0000
Sb	121	Linear Thru Zero	1.0000
Sb	123	Linear Thru Zero	
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	0.9999

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[>	In	115		102.6				
	Sn	120						
	Sb	121						
	Sb	123						
[>	Lu	175		100.5				
	U	238						

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: 248117001

Report Date/Time: Tuesday, April 13, 2010 13:49:38

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 8

Sample Date/Time: Tuesday, April 13, 2010 13:59:03

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\sb and u.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 8.054

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[> In	115		ug/L		178367	178366.510
Sn	120	49.196	ug/L	3.624	248523	1.391
Sb	121	52.090	ug/L	3.068	222216	1.246
Sb	123		ug/L		172734	0.968
[> Lu	175		ug/L		382366	382366.019
U	238	50.712	ug/L	2.659	2117499	5.538

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
In	115	Linear Thru Zero	
Sn	120	Linear Thru Zero	1.0000
Sb	121	Linear Thru Zero	1.0000
Sb	123	Linear Thru Zero	
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	0.9999

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[> In	115		96.0				
Sn	120	98.392					
Sb	121	104.180					
Sb	123						
[> Lu	175		97.4				
U	238	101.425					

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 8

Report Date/Time: Tuesday, April 13, 2010 13:59:32

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 9

Sample Date/Time: Tuesday, April 13, 2010 14:01:32

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\sb and u.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 9.055

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	In	115		ug/L		174808	174808.186
	Sn	120	-0.044	ug/L	6.363	351	-0.001
	Sb	121	0.149	ug/L	10.566	697	0.004
	Sb	123		ug/L		526	0.003
[>	Lu	175		ug/L		371771	371770.735
	U	238	0.005	ug/L	17.914	269	0.001

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
In	115	Linear Thru Zero	
Sn	120	Linear Thru Zero	1.0000
Sb	121	Linear Thru Zero	1.0000
Sb	123	Linear Thru Zero	
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	0.9999

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[>	In	115		94.1				
	Sn	120						
	Sb	121						
	Sb	123						
[>	Lu	175		94.7				
	U	238						

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 9

Report Date/Time: Tuesday, April 13, 2010 14:02:02

Page 1

ICPMS#5 - Summary Report

Sample ID: 1202056874

Sample Date/Time: Tuesday, April 13, 2010 14:13:56

Sample Type:

Sample Description: LANL 6020 DUP

Number of Replicates: 3

Batch ID: 959112|1|prb

Method File: c:\elandata\Method\sb and u.mth

Dataset File: C:\elandata\Dataset\100413\1202056874.060

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	In	115		ug/L		183511	183510.515
	Sn	120	0.010	ug/L	32.678	647	0.000
	Sb	121	0.017	ug/L	23.197	153	0.000
	Sb	123		ug/L		126	0.000
[>	Lu	175		ug/L		379926	379925.971
	U	238	0.004	ug/L	4.595	245	0.000

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
In	115	Linear Thru Zero	
Sn	120	Linear Thru Zero	1.0000
Sb	121	Linear Thru Zero	1.0000
Sb	123	Linear Thru Zero	
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	0.9999

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[>	In	115		98.8				
	Sn	120						
	Sb	121						
	Sb	123						
[>	Lu	175		96.8				
	U	238						

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: 1202056874

Report Date/Time: Tuesday, April 13, 2010 14:14:26

Page 1

ICPMS#5 - Summary Report

Sample ID: 1202056875

Sample Date/Time: Tuesday, April 13, 2010 14:16:25

Sample Type:

Sample Description: LANL 6020 MS

Number of Replicates: 3

Batch ID: 959112|1|prb

Method File: c:\elandata\Method\sb and u.mth

Dataset File: C:\elandata\Dataset\100413\1202056875.061

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	In	115		ug/L		184504	184503.801
	Sn	120	50.095	ug/L	2.882	261787	1.416
	Sb	121	206.325	ug/L	1.949	910385	4.935
	Sb	123		ug/L		727167	3.941
[>	Lu	175		ug/L		378759	378758.586
	U	238	46.688	ug/L	3.219	1931244	5.099

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
In	115	Linear Thru Zero	
Sn	120	Linear Thru Zero	1.0000
Sb	121	Linear Thru Zero	1.0000
Sb	123	Linear Thru Zero	
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	0.9999

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[>	In	115		99.3				
	Sn	120						
	Sb	121						
	Sb	123						
[>	Lu	175		96.5				
	U	238						

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: 1202056875

Report Date/Time: Tuesday, April 13, 2010 14:16:55

Page 1

ICPMS#5 - Summary Report

Sample ID: 1202056876

Sample Date/Time: Tuesday, April 13, 2010 14:18:54

Sample Type:

Sample Description: LANL 6020 SDILT

Number of Replicates: 3

Batch ID: 959112|5|prb

Method File: c:\elandata\Method\sb and u.mth

Dataset File: C:\elandata\Dataset\100413\1202056876.062

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	In	115		ug/L		172777	172777.165
	Sn	120	0.108	ug/L	4.382	1087	0.003
	Sb	121	0.133	ug/L	3.068	624	0.003
	Sb	123		ug/L		511	0.003
[>	Lu	175		ug/L		362453	362453.458
	U	238	0.029	ug/L	2.132	1225	0.003

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
In	115	Linear Thru Zero	
Sn	120	Linear Thru Zero	1.0000
Sb	121	Linear Thru Zero	1.0000
Sb	123	Linear Thru Zero	
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	0.9999

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[>	In	115		93.0				
	Sn	120						
	Sb	121						
	Sb	123						
[>	Lu	175		92.3				
	U	238						

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: 1202056876

Report Date/Time: Tuesday, April 13, 2010 14:19:24

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 6

Sample Date/Time: Tuesday, April 13, 2010 14:21:23

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\sb and u.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 6.063

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[> In	115		ug/L		176533	176532.965
Sn	120	49.140	ug/L	2.871	245656	1.389
Sb	121	51.039	ug/L	2.469	215473	1.221
Sb	123		ug/L		169003	0.958
[> Lu	175		ug/L		378342	378341.641
U	238	49.947	ug/L	1.379	2064193	5.455

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
In	115	Linear Thru Zero	
Sn	120	Linear Thru Zero	1.0000
Sb	121	Linear Thru Zero	1.0000
Sb	123	Linear Thru Zero	
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	0.9999

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel. % Difference
[> In	115		95.0			
Sn	120	98.280				
Sb	121	102.078				
Sb	123					
[> Lu	175		96.4			
U	238	99.895				

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 6

Report Date/Time: Tuesday, April 13, 2010 14:21:52

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 7

Sample Date/Time: Tuesday, April 13, 2010 14:23:52

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\sb and u.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 7.064

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	In	115		ug/L		170706	170705.939
	Sn	120	-0.042	ug/L	12.514	352	-0.001
	Sb	121	0.155	ug/L	2.783	706	0.004
	Sb	123		ug/L		561	0.003
[>	Lu	175		ug/L		367949	367949.069
	U	238	0.006	ug/L	12.517	315	0.001

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
In	115	Linear Thru Zero	
Sn	120	Linear Thru Zero	1.0000
Sb	121	Linear Thru Zero	1.0000
Sb	123	Linear Thru Zero	
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	0.9999

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[>	In	115		91.9				
	Sn	120						
	Sb	121						
	Sb	123						
[>	Lu	175		93.7				
	U	238						

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 7

Report Date/Time: Tuesday, April 13, 2010 14:24:23

Page 1

ICPMS#5 - Summary Report

Sample ID: Blank

Sample Date/Time: Tuesday, April 13, 2010 15:12:52

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\lu only.mth

Dataset File: C:\elandata\Dataset\100413\Blank.090

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[> Lu	175		ug/L		350450	
[U	238		ug/L		325	

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Di	Duplicate Rel. % Difference
[> Lu	175					
[U	238					

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

Sample ID: Blank

Report Date/Time: Tuesday, April 13, 2010 15:13:04

Page 1

ICPMS#5 - Summary Report

Sample ID: Standard 1

Sample Date/Time: Tuesday, April 13, 2010 15:14:32

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\lu only.mth

Dataset File: C:\elandata\Dataset\100413\Standard 1.091

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175		ug/L		357385	357385.496
[U	238	10.000	ug/L	1.263	423309	1.183

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	1.0000

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Di	Duplicate Rel. % Difference
[>	Lu	175					
[U	238					

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

Sample ID: Standard 1

Report Date/Time: Tuesday, April 13, 2010 15:14:41

Page 1

ICPMS#5 - Summary Report

Sample ID: Standard 2

Sample Date/Time: Tuesday, April 13, 2010 15:16:09

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\lu only.mth

Dataset File: C:\elandata\Dataset\100413\Standard 2.092

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175		ug/L		346400	346400.487
[U	238	99.956	ug/L	0.528	3924964	11.330

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	1.0000

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Di	Duplicate Rel. % Difference
[>	Lu	175					
[U	238					

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

Sample ID: Standard 2

Report Date/Time: Tuesday, April 13, 2010 15:16:18

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 1

Sample Date/Time: Tuesday, April 13, 2010 15:17:46

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\lu only.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 1.093

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175		ug/L		349311	349311.125
[U	238	49.627	ug/L	0.746	1965252	5.625

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	1.0000

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[>	Lu	175			99.7			
[U	238	99.254					

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 1

Report Date/Time: Tuesday, April 13, 2010 15:17:56

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 2

Sample Date/Time: Tuesday, April 13, 2010 15:19:26

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\lu only.mth

Dataset File: C:\elandata\Dataset\100413\QC-Std 2.094

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175		ug/L		350872	350872.277
[U	238	0.012	ug/L	5.508	815	0.001

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	1.0000

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[>	Lu	175		100.1				
[U	238						

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 2

Report Date/Time: Tuesday, April 13, 2010 15:19:38

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 3

Sample Date/Time: Tuesday, April 13, 2010 15:21:07

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\only.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 3.095

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[> Lu	175		ug/L		341237	341237.117
[U	238	0.216	ug/L	1.954	8686	0.025

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[> Lu	175			97.4		
[U	238	108.183				

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#5 - Summary Report

Sample ID: QC Std 4

Sample Date/Time: Tuesday, April 13, 2010 15:22:46

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\only.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 4.096

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175		ug/L		321479	321479.366
[U	238	-0.002	ug/L	2.476	214	-0.000

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	1.0000

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[>	Lu	175			91.7			
[U	238						

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 4

Report Date/Time: Tuesday, April 13, 2010 15:22:56

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 5

Sample Date/Time: Tuesday, April 13, 2010 15:24:25

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\only.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 5.097

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175		ug/L		323412	323411.634
[U	238	20.986	ug/L	1.639	769564	2.379

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	1.0000

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[>	Lu	175			92.3		
[U	238	104.932				

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 5

Report Date/Time: Tuesday, April 13, 2010 15:24:35

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 6

Sample Date/Time: Tuesday, April 13, 2010 15:26:04

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\only.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 6.098

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175	ug/L		344845	344845.355
[U	238	ug/L	1.762	1927882	5.589

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	1.0000

QC Calculated Values

	Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Di	Duplicate Rel.	% Difference
[>	Lu	175		98.4			
[U	238	98.617				

QC Out Of Limits

Measurement Type	Analyte	MassOut of Limits Message
------------------	---------	---------------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#5 - Summary Report

Sample ID: QC Std 7

Sample Date/Time: Tuesday, April 13, 2010 15:27:45

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\lu only.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 7.099

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175		ug/L		345974	345974.197
[U	238	0.010	ug/L	12.917	706	0.001

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	1.0000

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Di	Duplicate Rel. % Difference
[>	Lu	175			98.7		
[U	238					

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 7

Report Date/Time: Tuesday, April 13, 2010 15:27:57

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 8

Sample Date/Time: Tuesday, April 13, 2010 15:44:13

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\lu only.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 8.109

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175		ug/L		341777	341777.190
[U	238	50.362	ug/L	1.286	1951226	5.709

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	1.0000

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[>	Lu	175			97.5			
[U	238	100.723					

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 8

Report Date/Time: Tuesday, April 13, 2010 15:44:24

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 9

Sample Date/Time: Tuesday, April 13, 2010 15:45:54

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\lu only.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 9.110

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[> Lu	175		ug/L		349790	349789.814
[U	238	0.009	ug/L	2.899	693	0.001

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel. % Difference
[> Lu	175			99.8		
[U	238					

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#5 - Summary Report

Sample ID: QC Std 8

Sample Date/Time: Tuesday, April 13, 2010 15:59:07

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\only.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 8.118

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175		ug/L		351399	351399.441
[U	238	48.797	ug/L	2.328	1943686	5.531

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	1.0000

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Di	Duplicate Rel. % Difference
[>	Lu	175			100.3		
[U	238	97.594				

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 8

Report Date/Time: Tuesday, April 13, 2010 15:59:18

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 9

Sample Date/Time: Tuesday, April 13, 2010 16:00:48

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\only.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 9.119

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175		ug/L		348712	348712.118
[U	238	0.009	ug/L	8.140	686	0.001

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	1.0000

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[>	Lu	175			99.5			
[U	238						

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 9

Report Date/Time: Tuesday, April 13, 2010 16:01:00

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 8

Sample Date/Time: Tuesday, April 13, 2010 16:14:04

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\only.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 8.127

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175		ug/L		343618	343618.256
[U	238	50.399	ug/L	1.318	1963281	5.713

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	1.0000

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Di	Duplicate Rel.	% Difference
[>	Lu	175			98.1			
[U	238	100.798					

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 8

Report Date/Time: Tuesday, April 13, 2010 16:14:15

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 9

Sample Date/Time: Tuesday, April 13, 2010 16:15:45

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\lu only.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 9.128

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175		ug/L		351588	351587.835
[U	238	0.011	ug/L	7.475	771	0.001

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	1.0000

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel. % Difference
[>	Lu	175			100.3		
[U	238					

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 9

Report Date/Time: Tuesday, April 13, 2010 16:15:57

Page 1

ICPMS#5 - Summary Report

Sample ID: 1202056872

Sample Date/Time: Tuesday, April 13, 2010 16:17:26

Sample Type:

Sample Description: LANL 6020 MB

Number of Replicates: 3

Batch ID: 959112|1|prb

Method File: c:\elandata\Method\only.mth

Dataset File: C:\elandata\Dataset\100413\1202056872.129

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175	ug/L		360749	360749.021
[U	238	ug/L	1.128	1318	0.003

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	1.0000

QC Calculated Values

	Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel. % Difference
[>	Lu	175		102.9		
[U	238				

QC Out Of Limits

Measurement Type	Analyte	MassOut of Limits Message
------------------	---------	---------------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#5 - Summary Report

Sample ID: 1202056873

Sample Date/Time: Tuesday, April 13, 2010 16:19:05

Sample Type:

Sample Description: LANL 6020 LCS

Number of Replicates: 3

Batch ID: 959112|1|prb

Method File: c:\elandata\Method\lu only.mth

Dataset File: C:\elandata\Dataset\100413\1202056873.130

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175		ug/L		375936	375936.462
[U	238	44.852	ug/L	1.326	1911724	5.084

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	1.0000

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Di	Duplicate Rel. % Difference
[>	Lu	175		107.3			
[U	238					

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#5 - Summary Report

Sample ID: 248117001

Sample Date/Time: Tuesday, April 13, 2010 16:22:25

Sample Type:

Sample Description: LANL 6020

Number of Replicates: 3

Batch ID: 959112|1|prb

Method File: c:\elandata\Method\lu only.mth

Dataset File: C:\elandata\Dataset\100413\248117001.132

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175		ug/L		370536	370536.111
[U	238	0.005	ug/L	11.164	569	0.001

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	1.0000

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel. % Difference
[>	Lu	175			105.7		
[U	238					

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

Sample ID: 248117001

Report Date/Time: Tuesday, April 13, 2010 16:22:35

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 8

Sample Date/Time: Tuesday, April 13, 2010 16:29:04

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\lu only.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 8.136

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[> Lu	175		ug/L		347316	347316.293
[U	238	49.452	ug/L	1.572	1947017	5.605

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[> Lu	175			99.1			
[U	238						

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 8

Report Date/Time: Tuesday, April 13, 2010 16:29:15

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 9

Sample Date/Time: Tuesday, April 13, 2010 16:30:45

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\only.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 9.137

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175		ug/L		346483	346483.244
[U	238	0.010	ug/L	6.689	699	0.001

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	1.0000

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[>	Lu	175			98.9			
[U	238						

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 9

Report Date/Time: Tuesday, April 13, 2010 16:30:57

Page 1

ICPMS#5 - Summary Report

Sample ID: 1202056874

Sample Date/Time: Tuesday, April 13, 2010 16:39:06

Sample Type:

Sample Description: LANL 6020 DUP

Number of Replicates: 3

Batch ID: 959112|1|prb

Method File: c:\elandata\Method\lu only.mth

Dataset File: C:\elandata\Dataset\100413\1202056874.142

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175		ug/L		365467	365466.732
[U	238	-0.002	ug/L	15.135	237	-0.000

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	1.0000

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Di	Duplicate Rel. % Difference
[>	Lu	175			104.3		
[U	238					

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

Sample ID: 1202056874

Report Date/Time: Tuesday, April 13, 2010 16:39:17

Page 1

ICPMS#5 - Summary Report

Sample ID: 1202056875

Sample Date/Time: Tuesday, April 13, 2010 16:40:47

Sample Type:

Sample Description: LANL 6020 MS

Number of Replicates: 3

Batch ID: 959112|1|prb

Method File: c:\elandata\Method\only.mth

Dataset File: C:\elandata\Dataset\100413\1202056875.143

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175		ug/L		371431	371431.303
[U	238	45.210	ug/L	1.440	1903928	5.125

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	1.0000

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Di	Duplicate Rel. % Difference
[>	Lu	175			106.0		
[U	238					

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#5 - Summary Report

Sample ID: 1202056876

Sample Date/Time: Tuesday, April 13, 2010 16:42:27

Sample Type:

Sample Description: LANL 6020 SDILT

Number of Replicates: 3

Batch ID: 959112|5|prb

Method File: c:\elandata\Method\lu only.mth

Dataset File: C:\elandata\Dataset\100413\1202056876.144

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175		ug/L		353171	353171.163
[U	238	0.032	ug/L	0.569	1622	0.004

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	1.0000

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Di	Duplicate Rel. % Difference
[>	Lu	175			100.8		
[U	238					

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#5 - Summary Report

Sample ID: QC Std 6

Sample Date/Time: Tuesday, April 13, 2010 16:44:07

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\only.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 6.145

Concentration Results

	Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175		ug/L		351138	351137.585
[U	238	48.819	ug/L	1.491	1943227	5.534

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	1.0000

QC Calculated Values

	Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[>	Lu	175			100.2		
[U	238	97.638				

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 6

Report Date/Time: Tuesday, April 13, 2010 16:44:18

Page 1

ICPMS#5 - Summary Report

Sample ID: QC Std 7

Sample Date/Time: Tuesday, April 13, 2010 16:45:48

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\only.mth

Dataset File: C:\elandata\Dataset\100413\QC Std 7.146

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175	ug/L		352560	352559.902
[U	238	ug/L	14.005	774	0.001

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	1.0000

QC Calculated Values

	Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Di	Duplicate Rel. % Difference
[>	Lu	175		100.6		
[U	238				

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 7

Report Date/Time: Tuesday, April 13, 2010 16:46:00

Page 1

=====
Analysis BegunLogged In Analyst: Administrator
Spectrometer Model: FIMS-100, S/N B050-9550Technique: AA FIMS-MHS
Autosampler Model: S10

Sample Information File: C:\data-AA\Administrator\Sample Information\030210W1.SIF

Batch ID:

Results Data Set: 030210W3

Results Library: C:\data-AA\Administrator\Results\Results.mdb

=====
Sequence No.: 1
Sample ID: Calib Blank
Analyst:Autosampler Location: 1
Date Collected: 3/2/2010 08:26:33
Data Type: Original-----
Replicate Data: Calib Blank

Repl #	SampleConc ug/L	StdConc ug/L	BlkCorr Signal	Peak Area	Peak Height	Time	Peak Stored
1		[0.00]	0.0006	0.0027	0.0006	08:27:33	Yes
2		[0.00]	0.0006	0.0025	0.0006	08:28:08	Yes
Mean:		[0.00]	0.0006				
SD:		0.00	0.0000				
%RSD:		0.00	8.04				

Auto-zero performed.

=====
Sequence No.: 2
Sample ID: S0.2
Analyst:Autosampler Location: 2
Date Collected: 3/2/2010 08:28:26
Data Type: Original-----
Replicate Data: S0.2

Repl #	SampleConc ug/L	StdConc ug/L	BlkCorr Signal	Peak Area	Peak Height	Time	Peak Stored
1		[0.2]	0.0021	0.0131	0.0027	08:29:27	Yes
2		[0.2]	0.0021	0.0122	0.0028	08:30:02	Yes
Mean:		[0.2]	0.0021				
SD:		0.0	0.0000				
%RSD:		0.0	0.35				

Standard number 1 applied. [0.2]

Correlation Coef.: 1.000000 Slope: 0.01068 Intercept: 0.00000

=====
Sequence No.: 3
Sample ID: S0.5
Analyst:Autosampler Location: 3
Date Collected: 3/2/2010 08:30:21
Data Type: Original-----
Replicate Data: S0.5

Repl #	SampleConc ug/L	StdConc ug/L	BlkCorr Signal	Peak Area	Peak Height	Time	Peak Stored
1		[0.5]	0.0054	0.0299	0.0060	08:31:22	Yes
2		[0.5]	0.0055	0.0282	0.0061	08:31:57	Yes
Mean:		[0.5]	0.0055				
SD:		0.0	0.0001				
%RSD:		0.0	1.42				

Standard number 2 applied. [0.5]

Correlation Coef.: 0.999936 Slope: 0.01097 Intercept: -0.00002

=====
Sequence No.: 4
Sample ID: S2.0
Analyst:Autosampler Location: 4
Date Collected: 3/2/2010 08:32:17
Data Type: Original-----
Replicate Data: S2.0

Repl #	SampleConc ug/L	StdConc ug/L	BlkCorr Signal	Peak Area	Peak Height	Time	Peak Stored
-----------	--------------------	-----------------	-------------------	--------------	----------------	------	----------------

1	[2.0]	0.0209	0.1041	0.0215	08:33:18	Yes
2	[2.0]	0.0206	0.1004	0.0212	08:33:53	Yes
Mean:	[2.0]	0.0207				
SD:	0.0	0.0002				
%RSD:	0.0	0.90				
Standard number 3 applied. [2.0]						
Correlation Coef.: 0.999896 Slope: 0.01034 Intercept: 0.00011						

Sequence No.: 5 Autosampler Location: 5
 Sample ID: S5.0 Date Collected: 3/2/2010 08:34:13
 Analyst: Data Type: Original


Replicate Data: S5.0

Repl #	SampleConc ug/L	StdConc ug/L	BlkCorr Signal	Peak Area	Peak Height	Time	Peak Stored
1	[5.0]	0.0520	0.2558	0.0526	08:35:15	Yes	
2	[5.0]	0.0500	0.2379	0.0506	08:35:49	Yes	
Mean:	[5.0]	0.0510					
SD:	0.0	0.0014					
%RSD:	0.0	2.77					
Standard number 4 applied. [5.0]							
Correlation Coef.: 0.999965 Slope: 0.01018 Intercept: 0.00020							

Sequence No.: 6 Autosampler Location: 6
 Sample ID: S10.0 Date Collected: 3/2/2010 08:36:10
 Analyst: Data Type: Original

Replicate Data: S10.0

Repl #	SampleConc ug/L	StdConc ug/L	BlkCorr Signal	Peak Area	Peak Height	Time	Peak Stored
1	[10.0]	0.1058	0.5210	0.1064	08:37:10	Yes	
2	[10.0]	0.1077	0.5459	0.1083	08:37:45	Yes	
Mean:	[10.0]	0.1068					
SD:	0.0	0.0014					
%RSD:	0.0	1.27					
Standard number 5 applied. [10.0]							
Correlation Coef.: 0.999746 Slope: 0.01062 Intercept: -0.00030							

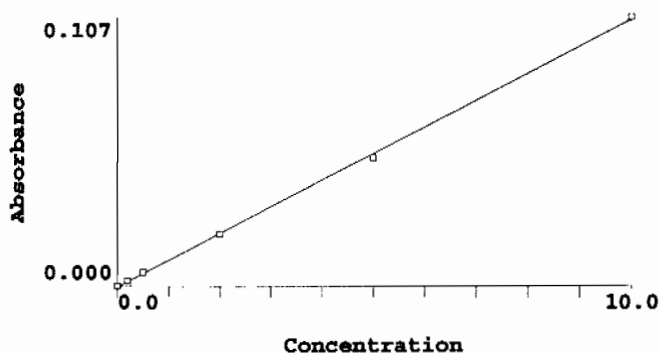

Calibration data for Hg 253.7

Equation: Linear, Calculated Intercept

ID	Mean Signal (Abs)	Entered Conc. ug/L	Calculated Conc. ug/L	Standard Deviation	%RSD
Calib Blank	0.0000	0	0.028	0.00	8.0
S0.2	0.0021	0.2	0.229	0.00	0.4
S0.5	0.0055	0.5	0.544	0.00	1.4
S2.0	0.0207	2.0	1.982	0.00	0.9
S5.0	0.0510	5.0	4.832	0.00	2.8
S10.0	0.1068	10.0	10.085	0.00	1.3
Correlation Coef.: 0.999746 Slope: 0.01062 Intercept: -0.00030					

Sequence No.: 7
Sample ID: ICV
Analyst:

Autosampler Location: 9
Date Collected: 3/2/2010 08:38:04
Data Type: Original

Replicate Data: ICV

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	5.221	5.221	0.0551	0.2819	0.0557	08:39:05	Yes
2	5.176	5.176	0.0547	0.2755	0.0553	08:39:40	Yes
Mean:	5.199	5.199	0.0549				
SD:	0.032	0.032	0.0003				
%RSD:	0.612	0.612	0.61				

QC value within limits for Hg 253.7 Recovery = 103.98%
All analyte(s) passed QC.

Sequence No.: 8
Sample ID: ICB
Analyst:

Autosampler Location: 10
Date Collected: 3/2/2010 08:40:00
Data Type: Original

Replicate Data: ICB

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.031	0.031	0.0000	0.0024	0.0006	08:41:01	Yes
2	0.039	0.039	0.0001	0.0036	0.0007	08:41:36	Yes
Mean:	0.035	0.035	0.0001				
SD:	0.006	0.006	0.0001				
%RSD:	15.89	15.89	82.13				

QC value within limits for Hg 253.7 Recovery = Not calculated
All analyte(s) passed QC.

Sequence No.: 9
Sample ID: CRDL
Analyst:

Autosampler Location: 11
Date Collected: 3/2/2010 08:41:56
Data Type: Original

Replicate Data: CRDL

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.234	0.234	0.0022	0.0142	0.0028	08:42:57	Yes
2	0.245	0.245	0.0023	0.0156	0.0029	08:43:32	Yes
Mean:	0.240	0.240	0.0022				
SD:	0.008	0.008	0.0001				
%RSD:	3.187	3.187	3.61				

QC value within limits for Hg 253.7 Recovery = 119.76%
All analyte(s) passed QC.

Sequence No.: 10
Sample ID: CCV
Analyst:

Autosampler Location: 7
Date Collected: 3/2/2010 08:43:52
Data Type: Original

Replicate Data: CCV

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	5.182	5.182	0.0547	0.2774	0.0553	08:44:52	Yes
2	5.128	5.128	0.0542	0.2734	0.0548	08:45:27	Yes
Mean:	5.155	5.155	0.0544				
SD:	0.038	0.038	0.0004				
%RSD:	0.738	0.738	0.74				

QC value within limits for Hg 253.7 Recovery = 103.11%
All analyte(s) passed QC.

Sequence No.: 11
Sample ID: CCB
Analyst:

Autosampler Location: 8
Date Collected: 3/2/2010 08:45:46
Data Type: Original

Replicate Data: CCB

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.012	0.012	-0.0002	-0.0000	0.0004	08:46:47	Yes
2	0.012	0.012	-0.0002	-0.0001	0.0004	08:47:22	Yes
Mean:	0.012	0.012	-0.0002				
SD:	0.000	0.000	0.0000				
%RSD:	0.848	0.848	0.63				

QC value within limits for Hg 253.7 Recovery = Not calculated
All analyte(s) passed QC.

Sequence No.: 12

Sample ID: 1202055823|958575|1

Analyst: JXL

Autosampler Location: 12

Date Collected: 3/2/2010 08:47:41

Data Type: Original

Replicate Data: 1202055823|958575|1

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.012	0.012	-0.0002	-0.0000	0.0004	08:48:43	Yes
2	0.016	0.016	-0.0001	0.0004	0.0005	08:49:17	Yes
Mean:	0.014	0.014	-0.0001				
SD:	0.003	0.003	0.0000				
%RSD:	18.17	18.17	19.03				

Sequence No.: 13

Sample ID: 1202055824|958575|1

Analyst: JXL

Autosampler Location: 13

Date Collected: 3/2/2010 08:49:38

Data Type: Original

Replicate Data: 1202055824|958575|1

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	2.127	2.127	0.0223	0.1129	0.0229	08:50:40	Yes
2	2.104	2.104	0.0220	0.1110	0.0227	08:51:14	Yes
Mean:	2.116	2.116	0.0222				
SD:	0.016	0.016	0.0002				
%RSD:	0.778	0.778	0.79				

Sequence No.: 14

Sample ID: 247037001|958575|1

Analyst: JXL

Autosampler Location: 14

Date Collected: 3/2/2010 08:51:35

Data Type: Original

Replicate Data: 247037001|958575|1

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.028	0.028	-0.0000	0.0025	0.0006	08:52:35	Yes
2	0.045	0.045	0.0002	0.0048	0.0008	08:53:11	Yes
Mean:	0.037	0.037	0.0001				
SD:	0.012	0.012	0.0001				
%RSD:	34.19	34.19	145.41				

Sequence No.: 15

Sample ID: 1202055825|958575|1

Analyst: JXL

Autosampler Location: 15

Date Collected: 3/2/2010 08:53:30

Data Type: Original

Replicate Data: 1202055825|958575|1

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.019	0.019	-0.0001	0.0021	0.0005	08:54:30	Yes
2	0.028	0.028	-0.0000	0.0030	0.0006	08:55:05	Yes
Mean:	0.024	0.024	-0.0000				
SD:	0.006	0.006	0.0001				

1	0.032	0.032	0.0000	0.0035	0.0007	09:04:04	Yes
2	0.032	0.032	0.0000	0.0030	0.0007	09:04:39	Yes
Mean:	0.032	0.032	0.0000				
SD:	0.000	0.000	0.0000				
%RSD:	0.786	0.786	6.22				

Sequence No.: 21

Autosampler Location: 21

Sample ID: 247042004|958575|1

Date Collected: 3/2/2010 09:04:58

Analyst: JXL

Data Type: Original

Replicate Data: 247042004|958575|1

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.028	0.028	0.0000	0.0031	0.0006	09:05:59	Yes
2	0.030	0.030	0.0000	0.0036	0.0006	09:06:34	Yes
Mean:	0.029	0.029	0.0000				
SD:	0.001	0.001	0.0000				
%RSD:	4.826	4.826	93.90				

Sequence No.: 22

Autosampler Location: 7

Sample ID: CCV

Date Collected: 3/2/2010 09:06:54

Analyst:

Data Type: Original

Replicate Data: CCV

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	5.128	5.128	0.0541	0.2768	0.0548	09:07:54	Yes
2	5.127	5.127	0.0541	0.2755	0.0547	09:08:29	Yes
Mean:	5.128	5.128	0.0541				
SD:	0.001	0.001	0.0000				
%RSD:	0.015	0.015	0.02				

QC value within limits for Hg 253.7 Recovery = 102.55%
All analyte(s) passed QC.

Sequence No.: 23

Autosampler Location: 8

Sample ID: CCB

Date Collected: 3/2/2010 09:08:48

Analyst:

Data Type: Original

Replicate Data: CCB

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.032	0.032	0.0000	0.0035	0.0007	09:09:49	Yes
2	0.037	0.037	0.0001	0.0040	0.0007	09:10:24	Yes
Mean:	0.035	0.035	0.0001				
SD:	0.004	0.004	0.0000				
%RSD:	10.44	10.44	53.94				

QC value within limits for Hg 253.7 Recovery = Not calculated
All analyte(s) passed QC.

Sequence No.: 24

Autosampler Location: 22

Sample ID: 247042005|958575|1

Date Collected: 3/2/2010 09:10:43

Analyst: JXL

Data Type: Original

Replicate Data: 247042005|958575|1

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.029	0.029	0.0000	0.0033	0.0006	09:11:44	Yes
2	0.033	0.033	0.0001	0.0036	0.0007	09:12:19	Yes
Mean:	0.031	0.031	0.0000				
SD:	0.003	0.003	0.0000				
%RSD:	8.235	8.235	83.29				

SD: 0.003 0.003 0.0000
%RSD: 9.252 9.252 154.88

Sequence No.: 30
Sample ID: 1202055830|958578|1
Analyst: JXL

Autosampler Location: 28
Date Collected: 3/2/2010 09:22:19
Data Type: Original

Replicate Data: 1202055830|958578|1

Repl #	SampleConc ug/L	StdConc ug/L	BlkCorr Signal	Peak Area	Peak Height	Time	Peak Stored
1	0.029	0.029	0.0000	0.0034	0.0006	09:23:19	Yes
2	0.026	0.026	-0.0000	0.0025	0.0006	09:23:54	Yes
Mean:	0.027	0.027	-0.0000				
SD:	0.002	0.002	0.0000				
%RSD:	7.825	7.825	359.08				

Sequence No.: 31
Sample ID: 1202055831|958578|1
Analyst: JXL

Autosampler Location: 29
Date Collected: 3/2/2010 09:24:13
Data Type: Original

Replicate Data: 1202055831|958578|1

Repl #	SampleConc ug/L	StdConc ug/L	BlkCorr Signal	Peak Area	Peak Height	Time	Peak Stored
1	2.105	2.105	0.0221	0.1147	0.0227	09:25:14	Yes
2	2.105	2.105	0.0221	0.1146	0.0227	09:25:49	Yes
Mean:	2.105	2.105	0.0221				
SD:	0.000	0.000	0.0000				
%RSD:	0.010	0.010	0.01				

Sequence No.: 32
Sample ID: 1202055832|958278|5
Analyst: JXL

Autosampler Location: 30
Date Collected: 3/2/2010 09:26:08
Data Type: Original

Replicate Data: 1202055832|958278|5

Repl #	SampleConc ug/L	StdConc ug/L	BlkCorr Signal	Peak Area	Peak Height	Time	Peak Stored
1	0.026	0.026	-0.0000	0.0028	0.0006	09:27:08	Yes
2	0.025	0.025	-0.0000	0.0026	0.0006	09:27:43	Yes
Mean:	0.025	0.025	-0.0000				
SD:	0.001	0.001	0.0000				
%RSD:	3.125	3.125	27.93				

Sequence No.: 33
Sample ID: 247036002|958578|1
Analyst: JXL

Autosampler Location: 31
Date Collected: 3/2/2010 09:28:02
Data Type: Original

Replicate Data: 247036002|958578|1

Repl #	SampleConc ug/L	StdConc ug/L	BlkCorr Signal	Peak Area	Peak Height	Time	Peak Stored
1	0.023	0.023	-0.0001	0.0026	0.0006	09:29:03	Yes
2	0.029	0.029	0.0000	0.0031	0.0006	09:29:38	Yes
Mean:	0.026	0.026	-0.0000				
SD:	0.004	0.004	0.0000				
%RSD:	16.58	16.58	246.20				

Sequence No.: 34
Sample ID: CCV
Analyst:

Autosampler Location: 7
Date Collected: 3/2/2010 09:29:57
Data Type: Original

Replicate Data: CCV

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
------	------------	---------	---------	------	------	------	------

#	ug/L	ug/L	Signal	Area	Height		Stored
1	5.092	5.092	0.0538	0.2718	0.0544	09:30:58	Yes
2	5.019	5.019	0.0530	0.2655	0.0536	09:31:32	Yes
Mean:	5.056	5.056	0.0534				
SD:	0.051	0.051	0.0005				
%RSD:	1.013	1.013	1.02				

QC value within limits for Hg 253.7 Recovery = 101.11%
All analyte(s) passed QC.

Sequence No.: 35

Sample ID: CCB

Analyst:

Autosampler Location: 8

Date Collected: 3/2/2010 09:31:51

Data Type: Original

Replicate Data: CCB

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.048	0.048	0.0002	0.0039	0.0008	09:32:52	Yes
2	0.033	0.033	0.0001	0.0029	0.0007	09:33:27	Yes
Mean:	0.040	0.040	0.0001				
SD:	0.010	0.010	0.0001				
%RSD:	25.10	25.10	81.63				

QC value within limits for Hg 253.7 Recovery = Not calculated
All analyte(s) passed QC.

Sequence No.: 36

Sample ID: 247036003|958578|1

Analyst: JXL

Autosampler Location: 32

Date Collected: 3/2/2010 09:33:47

Data Type: Original

Replicate Data: 247036003|958578|1

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.026	0.026	-0.0000	0.0027	0.0006	09:34:48	Yes
2	0.029	0.029	0.0000	0.0030	0.0006	09:35:23	Yes
Mean:	0.028	0.028	-0.0000				
SD:	0.002	0.002	0.0000				
%RSD:	8.511	8.511	602.34				

Sequence No.: 37

Sample ID: 247036004|958578|1

Analyst: JXL

Autosampler Location: 33

Date Collected: 3/2/2010 09:35:42

Data Type: Original

Replicate Data: 247036004|958578|1

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.023	0.023	-0.0000	0.0024	0.0006	09:36:43	Yes
2	0.037	0.037	0.0001	0.0036	0.0007	09:37:18	Yes
Mean:	0.030	0.030	0.0000				
SD:	0.009	0.009	0.0001				
%RSD:	31.23	31.23	437.06				

Sequence No.: 38

Sample ID: 247036005|958578|1

Analyst: JXL

Autosampler Location: 34

Date Collected: 3/2/2010 09:37:38

Data Type: Original

Replicate Data: 247036005|958578|1

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.027	0.027	-0.0000	0.0029	0.0006	09:38:39	Yes
2	0.025	0.025	-0.0000	0.0028	0.0006	09:39:14	Yes
Mean:	0.026	0.026	-0.0000				
SD:	0.001	0.001	0.0000				
%RSD:	4.570	4.570	52.14				

Mean: 0.029 0.029 0.0000
SD: 0.004 0.004 0.0000
%RSD: 15.71 15.71 746.11

Sequence No.: 44

Sample ID: 1202055833|958581|1

Analyst: JXL

Autosampler Location: 40

Date Collected: 3/2/2010 09:49:16

Data Type: Original

Replicate Data: 1202055833|958581|1

Repl #	SampleConc ug/L	StdConc ug/L	BlkCorr Signal	Peak Area	Peak Height	Time	Peak Stored
1	0.021	0.021	-0.0001	0.0024	0.0005	09:50:17	Yes
2	0.029	0.029	0.0000	0.0030	0.0006	09:50:51	Yes
Mean:	0.025	0.025	-0.0000				
SD:	0.005	0.005	0.0001				
%RSD:	21.51	21.51	171.71				

Sequence No.: 45

Sample ID: 1202055834|958581|1

Analyst: JXL

Autosampler Location: 41

Date Collected: 3/2/2010 09:51:11

Data Type: Original

Replicate Data: 1202055834|958581|1

Repl #	SampleConc ug/L	StdConc ug/L	BlkCorr Signal	Peak Area	Peak Height	Time	Peak Stored
1	2.186	2.186	0.0229	0.1196	0.0235	09:52:12	Yes
2	2.183	2.183	0.0229	0.1194	0.0235	09:52:47	Yes
Mean:	2.184	2.184	0.0229				
SD:	0.003	0.003	0.0000				
%RSD:	0.123	0.123	0.12				

Sequence No.: 46

Sample ID: CCV

Analyst:

Autosampler Location: 7

Date Collected: 3/2/2010 09:53:06

Data Type: Original

Replicate Data: CCV

Repl #	SampleConc ug/L	StdConc ug/L	BlkCorr Signal	Peak Area	Peak Height	Time	Peak Stored
1	5.016	5.016	0.0530	0.2735	0.0536	09:54:06	Yes
2	5.018	5.018	0.0530	0.2717	0.0536	09:54:41	Yes
Mean:	5.017	5.017	0.0530				
SD:	0.001	0.001	0.0000				
%RSD:	0.023	0.023	0.02				

QC value within limits for Hg 253.7 Recovery = 100.34%
All analyte(s) passed QC.

Sequence No.: 47

Sample ID: CCB

Analyst:

Autosampler Location: 8

Date Collected: 3/2/2010 09:55:00

Data Type: Original

Replicate Data: CCB

Repl #	SampleConc ug/L	StdConc ug/L	BlkCorr Signal	Peak Area	Peak Height	Time	Peak Stored
1	0.035	0.035	0.0001	0.0033	0.0007	09:56:01	Yes
2	0.032	0.032	0.0000	0.0031	0.0007	09:56:36	Yes
Mean:	0.034	0.034	0.0001				
SD:	0.002	0.002	0.0000				
%RSD:	5.467	5.467	32.35				

QC value within limits for Hg 253.7 Recovery = Not calculated
All analyte(s) passed QC.

Sequence No.: 48

Sample ID: 247817001|958581|1

Autosampler Location: 42

Date Collected: 3/2/2010 09:56:55

2	0.038	0.038	0.0001	0.0037	0.0007	10:15:55	Yes
Mean:	0.037	0.037	0.0001				
SD:	0.001	0.001	0.0000				
%RSD:	4.045	4.045	16.44				

Sequence No.: 58

Sample ID: CCV

Analyst:

Autosampler Location: 7

Date Collected: 3/2/2010 10:16:14

Data Type: Original

Replicate Data: CCV

Repl #	SampleConc ug/L	StdConc ug/L	BlkCorr Signal	Peak Area	Peak Height	Time	Peak Stored
1	5.001	5.001	0.0528	0.2739	0.0534	10:17:15	Yes
2	4.992	4.992	0.0527	0.2715	0.0533	10:17:50	Yes
Mean:	4.997	4.997	0.0528				
SD:	0.006	0.006	0.0001				
%RSD:	0.126	0.126	0.13				

QC value within limits for Hg 253.7 Recovery = 99.93%
All analyte(s) passed QC.

Sequence No.: 59

Sample ID: CCB

Analyst:

Autosampler Location: 8

Date Collected: 3/2/2010 10:18:09

Data Type: Original

Replicate Data: CCB

Repl #	SampleConc ug/L	StdConc ug/L	BlkCorr Signal	Peak Area	Peak Height	Time	Peak Stored
1	0.031	0.031	0.0000	0.0030	0.0006	10:19:09	Yes
2	0.033	0.033	0.0001	0.0032	0.0007	10:19:45	Yes
Mean:	0.032	0.032	0.0000				
SD:	0.002	0.002	0.0000				
%RSD:	5.084	5.084	37.73				

QC value within limits for Hg 253.7 Recovery = Not calculated
All analyte(s) passed QC.

Sequence No.: 60

Sample ID: 1202055843|958587|1

Analyst: JXL

Autosampler Location: 52

Date Collected: 3/2/2010 10:20:04

Data Type: Original

Replicate Data: 1202055843|958587|1

Repl #	SampleConc ug/L	StdConc ug/L	BlkCorr Signal	Peak Area	Peak Height	Time	Peak Stored
1	0.028	0.028	-0.0000	0.0029	0.0006	10:21:05	Yes
2	0.032	0.032	0.0000	0.0035	0.0007	10:21:41	Yes
Mean:	0.030	0.030	0.0000				
SD:	0.003	0.003	0.0000				
%RSD:	11.19	11.19	167.05				

Sequence No.: 61

Sample ID: 1202055844|958587|1

Analyst: JXL

Autosampler Location: 53

Date Collected: 3/2/2010 10:22:00

Data Type: Original

Replicate Data: 1202055844|958587|1

Repl #	SampleConc ug/L	StdConc ug/L	BlkCorr Signal	Peak Area	Peak Height	Time	Peak Stored
1	2.176	2.176	0.0228	0.1196	0.0234	10:23:01	Yes
2	2.169	2.169	0.0227	0.1186	0.0233	10:23:36	Yes
Mean:	2.173	2.173	0.0228				
SD:	0.005	0.005	0.0001				
%RSD:	0.228	0.228	0.23				

Sequence No.: 62

Autosampler Location: 54

%RSD: 3.709 3.709 11.51

Sequence No.: 67

Sample ID: 248044003|958587|1

Analyst: JXL

Autosampler Location: 59

Date Collected: 3/2/2010 10:33:34

Data Type: Original

Replicate Data: 248044003|958587|1

Repl	SampleConc	StndConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.037	0.037	0.0001	0.0035	0.0007	10:34:36	Yes
2	0.042	0.042	0.0001	0.0036	0.0008	10:35:11	Yes
Mean:	0.039	0.039	0.0001				
SD:	0.003	0.003	0.0000				
%RSD:	8.563	8.563	29.80				

Sequence No.: 68

Sample ID: 248044004|958587|1

Analyst: JXL

Autosampler Location: 60

Date Collected: 3/2/2010 10:35:31

Data Type: Original

Replicate Data: 248044004|958587|1

Repl	SampleConc	StndConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.037	0.037	0.0001	0.0035	0.0007	10:36:32	Yes
2	0.037	0.037	0.0001	0.0031	0.0007	10:37:07	Yes
Mean:	0.037	0.037	0.0001				
SD:	0.000	0.000	0.0000				
%RSD:	0.860	0.860	3.53				

Sequence No.: 69

Sample ID: 248044005|958587|1

Analyst: JXL

Autosampler Location: 61

Date Collected: 3/2/2010 10:37:27

Data Type: Original

Replicate Data: 248044005|958587|1

Repl	SampleConc	StndConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.026	0.026	-0.0000	0.0028	0.0006	10:38:29	Yes
2	0.029	0.029	0.0000	0.0030	0.0006	10:39:04	Yes
Mean:	0.027	0.027	-0.0000				
SD:	0.002	0.002	0.0000				
%RSD:	7.669	7.669	260.52				

Sequence No.: 70

Sample ID: CCV

Analyst:

Autosampler Location: 7

Date Collected: 3/2/2010 10:39:24

Data Type: Original

Replicate Data: CCV

Repl	SampleConc	StndConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	5.079	5.079	0.0536	0.2761	0.0542	10:40:25	Yes
2	5.044	5.044	0.0533	0.2727	0.0539	10:41:00	Yes
Mean:	5.061	5.061	0.0534				
SD:	0.025	0.025	0.0003				
%RSD:	0.487	0.487	0.49				

QC value within limits for Hg 253.7 Recovery = 101.22%

All analyte(s) passed QC.

Sequence No.: 71

Sample ID: CCB

Analyst:

Autosampler Location: 8

Date Collected: 3/2/2010 10:41:19

Data Type: Original

Replicate Data: CCB

Repl #	SampleConc ug/L	StdConc ug/L	BlkCorr Signal	Peak Area	Peak Height	Time	Peak Stored
1	0.032	0.032	0.0000	0.0028	0.0006	10:42:20	Yes
2	0.037	0.037	0.0001	0.0037	0.0007	10:42:55	Yes
Mean:	0.034	0.034	0.0001				
SD:	0.004	0.004	0.0000				
%RSD:	10.27	10.27	56.74				

QC value within limits for Hg 253.7 Recovery = Not calculated
All analyte(s) passed QC.

Sequence No.: 72

Autosampler Location: 62

Sample ID: 248044006|958587|1

Date Collected: 3/2/2010 10:43:14

Analyst: JXL

Data Type: Original

Replicate Data: 248044006|958587|1

Repl #	SampleConc ug/L	StdConc ug/L	BlkCorr Signal	Peak Area	Peak Height	Time	Peak Stored
1	0.035	0.035	0.0001	0.0032	0.0007	10:44:16	Yes
2	0.041	0.041	0.0001	0.0037	0.0007	10:44:51	Yes
Mean:	0.038	0.038	0.0001				
SD:	0.004	0.004	0.0000				
%RSD:	10.62	10.62	40.88				

Sequence No.: 73

Autosampler Location: 63

Sample ID: 248127002|958587|1

Date Collected: 3/2/2010 10:45:11

Analyst: JXL

Data Type: Original

Replicate Data: 248127002|958587|1

Repl #	SampleConc ug/L	StdConc ug/L	BlkCorr Signal	Peak Area	Peak Height	Time	Peak Stored
1	0.049	0.049	0.0002	0.0042	0.0008	10:46:12	Yes
2	0.049	0.049	0.0002	0.0038	0.0008	10:46:47	Yes
Mean:	0.049	0.049	0.0002				
SD:	0.000	0.000	0.0000				
%RSD:	0.072	0.072	0.17				

Sequence No.: 74

Autosampler Location: 64

Sample ID: 248168006|958587|1

Date Collected: 3/2/2010 10:47:07

Analyst: JXL

Data Type: Original

Replicate Data: 248168006|958587|1

Repl #	SampleConc ug/L	StdConc ug/L	BlkCorr Signal	Peak Area	Peak Height	Time	Peak Stored
1	0.032	0.032	0.0000	0.0032	0.0006	10:48:08	Yes
2	0.039	0.039	0.0001	0.0038	0.0007	10:48:43	Yes
Mean:	0.035	0.035	0.0001				
SD:	0.005	0.005	0.0001				
%RSD:	15.15	15.15	72.49				

Sequence No.: 75

Autosampler Location: 65

Sample ID: 248169004|958587|1

Date Collected: 3/2/2010 10:49:03

Analyst: JXL

Data Type: Original

Replicate Data: 248169004|958587|1

Repl #	SampleConc ug/L	StdConc ug/L	BlkCorr Signal	Peak Area	Peak Height	Time	Peak Stored
1	0.039	0.039	0.0001	0.0037	0.0007	10:50:04	Yes
2	0.041	0.041	0.0001	0.0036	0.0008	10:50:39	Yes
Mean:	0.040	0.040	0.0001				
SD:	0.001	0.001	0.0000				
%RSD:	3.561	3.561	11.62				

Replicate Data: 1202055863|958593|1

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	26.95	26.95	0.2859	1.4918	0.2865	10:59:45	Yes
Sample concentration is greater than that of the highest standard.							
2	26.74	26.74	0.2836	1.4832	0.2842	11:00:20	Yes
Sample concentration is greater than that of the highest standard.							
Mean:	26.85	26.85	0.2847				
SD:	0.150	0.150	0.0016				
%RSD:	0.559	0.559	0.56				

Sample concentration is greater than that of the highest standard.

Sequence No.: 81

Autosampler Location: 71

Sample ID: 1202055864|958593|5

Date Collected: 3/2/2010 11:00:40

Analyst: JXL

Data Type: Original

Replicate Data: 1202055864|958593|5

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	5.495	5.495	0.0580	0.2982	0.0586	11:01:41	Yes
2	5.466	5.466	0.0577	0.2966	0.0583	11:02:16	Yes
Mean:	5.480	5.480	0.0579				
SD:	0.020	0.020	0.0002				
%RSD:	0.371	0.371	0.37				

Sequence No.: 82

Autosampler Location: 7

Sample ID: CCV

Date Collected: 3/2/2010 11:02:36

Analyst:

Data Type: Original

Replicate Data: CCV

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	5.006	5.006	0.0528	0.2714	0.0535	11:03:37	Yes
2	5.022	5.022	0.0530	0.2712	0.0536	11:04:12	Yes
Mean:	5.014	5.014	0.0529				
SD:	0.011	0.011	0.0001				
%RSD:	0.227	0.227	0.23				

QC value within limits for Hg 253.7 Recovery = 100.27%
All analyte(s) passed QC.

Sequence No.: 83

Autosampler Location: 8

Sample ID: CCB

Date Collected: 3/2/2010 11:04:31

Analyst:

Data Type: Original

Replicate Data: CCB

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.033	0.033	0.0001	0.0031	0.0007	11:05:31	Yes
2	0.048	0.048	0.0002	0.0040	0.0008	11:06:06	Yes
Mean:	0.040	0.040	0.0001				
SD:	0.010	0.010	0.0001				
%RSD:	26.02	26.02	85.60				

QC value within limits for Hg 253.7 Recovery = Not calculated
All analyte(s) passed QC.

Sequence No.: 84

Autosampler Location: 72

Sample ID: 247958002|958593|1

Date Collected: 3/2/2010 11:06:25

Analyst: JXL

Data Type: Original

Replicate Data: 247958002|958593|1

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.063	0.063	0.0004	0.0052	0.0010	11:07:27	Yes

2	0.068	0.068	0.0004	0.0049	0.0010	11:08:02	Yes
Mean:	0.066	0.066	0.0004				
SD:	0.004	0.004	0.0000				
%RSD:	5.695	5.695	9.90				

Sequence No.: 85

Sample ID: 247958003|958593|1

Analyst: JXL

Autosampler Location: 73

Date Collected: 3/2/2010 11:08:22

Data Type: Original

Replicate Data: 247958003|958593|1

Repl	SampleConc	StndConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	14.14	14.14	0.1498	0.7668	0.1504	11:09:24	Yes
Sample concentration is greater than that of the highest standard.							
2	14.18	14.18	0.1503	0.7699	0.1509	11:09:59	Yes
Sample concentration is greater than that of the highest standard.							
Mean:	14.16	14.16	0.1501				
SD:	0.029	0.029	0.0003				
%RSD:	0.202	0.202	0.20				
Sample concentration is greater than that of the highest standard.							

Sequence No.: 86

Sample ID: 247958004|958593|1

Analyst: JXL

Autosampler Location: 74

Date Collected: 3/2/2010 11:10:19

Data Type: Original

Replicate Data: 247958004|958593|1

Repl	SampleConc	StndConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.261	0.261	0.0025	0.0153	0.0031	11:11:21	Yes
2	0.275	0.275	0.0026	0.0162	0.0032	11:11:56	Yes
Mean:	0.268	0.268	0.0026				
SD:	0.010	0.010	0.0001				
%RSD:	3.710	3.710	4.14				

Sequence No.: 87

Sample ID: 247958005|958593|1

Analyst: JXL

Autosampler Location: 75

Date Collected: 3/2/2010 11:12:16

Data Type: Original

Replicate Data: 247958005|958593|1

Repl	SampleConc	StndConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.159	0.159	0.0014	0.0102	0.0020	11:13:17	Yes
2	0.170	0.170	0.0015	0.0105	0.0021	11:13:52	Yes
Mean:	0.165	0.165	0.0015				
SD:	0.007	0.007	0.0001				
%RSD:	4.420	4.420	5.32				

Sequence No.: 88

Sample ID: 1202056573|958951|1

Analyst: JXL

Autosampler Location: 76

Date Collected: 3/2/2010 11:14:12

Data Type: Original

Replicate Data: 1202056573|958951|1

Repl	SampleConc	StndConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.033	0.033	0.0000	0.0033	0.0007	11:15:13	Yes
2	0.046	0.046	0.0002	0.0042	0.0008	11:15:48	Yes
Mean:	0.040	0.040	0.0001				
SD:	0.010	0.010	0.0001				
%RSD:	24.87	24.87	84.85				

Sequence No.: 89

Sample ID: 1202056574|958951|1

Autosampler Location: 77

Date Collected: 3/2/2010 11:16:08

Analyst: JXL

Data Type: Original

Replicate Data: 1202056574|958951|1

Repl	SampleConc	StndConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	2.200	2.200	0.0231	0.1197	0.0237	11:17:10	Yes
2	2.209	2.209	0.0232	0.1196	0.0238	11:17:45	Yes
Mean:	2.205	2.205	0.0231				
SD:	0.006	0.006	0.0001				
%RSD:	0.267	0.267	0.27				

Sequence No.: 90

Autosampler Location: 78

Sample ID: 247997001|958951|1

Date Collected: 3/2/2010 11:18:05

Analyst: JXL

Data Type: Original

Replicate Data: 247997001|958951|1

Repl	SampleConc	StndConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.033	0.033	0.0001	0.0032	0.0007	11:19:06	Yes
2	0.041	0.041	0.0001	0.0035	0.0007	11:19:41	Yes
Mean:	0.037	0.037	0.0001				
SD:	0.006	0.006	0.0001				
%RSD:	15.81	15.81	65.70				

Sequence No.: 91

Autosampler Location: 79

Sample ID: 248001001|958951|1

Date Collected: 3/2/2010 11:20:01

Analyst: JXL

Data Type: Original

Replicate Data: 248001001|958951|1

Repl	SampleConc	StndConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.033	0.033	0.0001	0.0032	0.0007	11:21:03	Yes
2	0.041	0.041	0.0001	0.0038	0.0008	11:21:38	Yes
Mean:	0.037	0.037	0.0001				
SD:	0.006	0.006	0.0001				
%RSD:	15.33	15.33	60.50				

Sequence No.: 92

Autosampler Location: 80

Sample ID: 248010001|958951|1

Date Collected: 3/2/2010 11:21:58

Analyst: JXL

Data Type: Original

Replicate Data: 248010001|958951|1

Repl	SampleConc	StndConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.034	0.034	0.0001	0.0037	0.0007	11:22:59	Yes
2	0.035	0.035	0.0001	0.0034	0.0007	11:23:34	Yes
Mean:	0.035	0.035	0.0001				
SD:	0.001	0.001	0.0000				
%RSD:	3.747	3.747	19.55				

Sequence No.: 93

Autosampler Location: 81

Sample ID: 248010002|958951|1

Date Collected: 3/2/2010 11:23:54

Analyst: JXL

Data Type: Original

Replicate Data: 248010002|958951|1

Repl	SampleConc	StndConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.039	0.039	0.0001	0.0041	0.0007	11:24:55	Yes
2	0.036	0.036	0.0001	0.0033	0.0007	11:25:30	Yes
Mean:	0.038	0.038	0.0001				
SD:	0.002	0.002	0.0000				
%RSD:	5.841	5.841	22.77				

Sequence No.: 94
Sample ID: CCV
Analyst:

Autosampler Location: 7
Date Collected: 3/2/2010 11:25:50
Data Type: Original

Replicate Data: CCV

Repl #	SampleConc ug/L	StndConc ug/L	BlkCorr Signal	Peak Area	Peak Height	Time	Peak Stored
1	5.218	5.218	0.0551	0.2817	0.0557	11:26:50	Yes
2	5.211	5.211	0.0550	0.2791	0.0556	11:27:25	Yes
Mean:	5.214	5.214	0.0551				
SD:	0.005	0.005	0.0001				
%RSD:	0.095	0.095	0.10				

QC value within limits for Hg 253.7 Recovery = 104.29%
All analyte(s) passed QC.

Sequence No.: 95
Sample ID: CCB
Analyst:

Autosampler Location: 8
Date Collected: 3/2/2010 11:27:44
Data Type: Original

Replicate Data: CCB

Repl #	SampleConc ug/L	StndConc ug/L	BlkCorr Signal	Peak Area	Peak Height	Time	Peak Stored
1	0.029	0.029	0.0000	0.0027	0.0006	11:28:45	Yes
2	0.038	0.038	0.0001	0.0032	0.0007	11:29:20	Yes
Mean:	0.033	0.033	0.0001				
SD:	0.006	0.006	0.0001				
%RSD:	19.42	19.42	124.89				

QC value within limits for Hg 253.7 Recovery = Not calculated
All analyte(s) passed QC.

Sequence No.: 96
Sample ID: 248026001|958951|1
Analyst: JXL

Autosampler Location: 82
Date Collected: 3/2/2010 11:29:40
Data Type: Original

Replicate Data: 248026001|958951|1

Repl #	SampleConc ug/L	StndConc ug/L	BlkCorr Signal	Peak Area	Peak Height	Time	Peak Stored
1	0.036	0.036	0.0001	0.0035	0.0007	11:30:41	Yes
2	0.037	0.037	0.0001	0.0031	0.0007	11:31:16	Yes
Mean:	0.036	0.036	0.0001				
SD:	0.001	0.001	0.0000				
%RSD:	1.939	1.939	8.63				

Sequence No.: 97
Sample ID: 248032001|958951|1
Analyst: JXL

Autosampler Location: 83
Date Collected: 3/2/2010 11:31:36
Data Type: Original

Replicate Data: 248032001|958951|1

Repl #	SampleConc ug/L	StndConc ug/L	BlkCorr Signal	Peak Area	Peak Height	Time	Peak Stored
1	0.028	0.028	-0.0000	0.0029	0.0006	11:32:37	Yes
2	0.031	0.031	0.0000	0.0032	0.0006	11:33:12	Yes
Mean:	0.030	0.030	0.0000				
SD:	0.003	0.003	0.0000				
%RSD:	8.573	8.573	152.05				

Sequence No.: 98
Sample ID: 248034001|958951|1
Analyst: JXL

Autosampler Location: 84
Date Collected: 3/2/2010 11:33:32
Data Type: Original

Sample ID: 248046002|958951|1
Analyst: JXL

Date Collected: 3/2/2010 11:43:16
Data Type: Original

Replicate Data: 248046002|958951|1

Repl	SampleConc	StndConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.025	0.025	-0.0000	0.0028	0.0006	11:44:17	Yes
2	0.031	0.031	0.0000	0.0032	0.0006	11:44:52	Yes
Mean:	0.028	0.028	-0.0000				
SD:	0.004	0.004	0.0000				
%RSD:	15.25	15.25	>999.9%				

Sequence No.: 104

Autosampler Location: 90

Sample ID: 248053001|958951|1

Date Collected: 3/2/2010 11:45:12

Analyst: JXL

Data Type: Original

Replicate Data: 248053001|958951|1

Repl	SampleConc	StndConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.028	0.028	0.0000	0.0030	0.0006	11:46:14	Yes
2	0.031	0.031	0.0000	0.0030	0.0006	11:46:49	Yes
Mean:	0.029	0.029	0.0000				
SD:	0.002	0.002	0.0000				
%RSD:	5.471	5.471	107.18				

Sequence No.: 105

Autosampler Location: 91

Sample ID: 248053002|958951|1

Date Collected: 3/2/2010 11:47:10

Analyst: JXL

Data Type: Original

Replicate Data: 248053002|958951|1

Repl	SampleConc	StndConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.026	0.026	-0.0000	0.0027	0.0006	11:48:11	Yes
2	0.028	0.028	0.0000	0.0029	0.0006	11:48:46	Yes
Mean:	0.027	0.027	-0.0000				
SD:	0.002	0.002	0.0000				
%RSD:	5.952	5.952	162.46				

Sequence No.: 106

Autosampler Location: 7

Sample ID: CCV

Date Collected: 3/2/2010 11:49:06

Analyst:

Data Type: Original

Replicate Data: CCV

Repl	SampleConc	StndConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	4.948	4.948	0.0522	0.2686	0.0529	11:50:06	Yes
2	4.918	4.918	0.0519	0.2653	0.0525	11:50:41	Yes
Mean:	4.933	4.933	0.0521				
SD:	0.021	0.021	0.0002				
%RSD:	0.435	0.435	0.44				

QC value within limits for Hg 253.7 Recovery = 98.67%
All analyte(s) passed QC.

Sequence No.: 107

Autosampler Location: 8

Sample ID: CCB

Date Collected: 3/2/2010 11:51:00

Analyst:

Data Type: Original

Replicate Data: CCB

Repl	SampleConc	StndConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.024	0.024	-0.0000	0.0025	0.0006	11:52:01	Yes
2	0.032	0.032	0.0000	0.0029	0.0007	11:52:36	Yes

Mean: 0.028 0.028 -0.0000
SD: 0.006 0.006 0.0001
%RSD: 20.56 20.56 >999.9%

QC value within limits for Hg 253.7 Recovery = Not calculated
All analyte(s) passed QC.

Sequence No.: 108

Sample ID: 248053003|958951|1

Analyst: JXL

Autosampler Location: 92

Date Collected: 3/2/2010 11:52:55

Data Type: Original

Replicate Data: 248053003|958951|1

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.030	0.030	0.0000	0.0032	0.0006	11:53:57	Yes
2	0.035	0.035	0.0001	0.0036	0.0007	11:54:31	Yes
Mean:	0.032	0.032	0.0000				
SD:	0.004	0.004	0.0000				
%RSD:	11.99	11.99	88.45				

Sequence No.: 109

Sample ID: 248108001|958951|1

Analyst: JXL

Autosampler Location: 93

Date Collected: 3/2/2010 11:54:52

Data Type: Original

Replicate Data: 248108001|958951|1

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.026	0.026	-0.0000	0.0030	0.0006	11:55:53	Yes
2	0.030	0.030	0.0000	0.0033	0.0006	11:56:28	Yes
Mean:	0.028	0.028	0.0000				
SD:	0.003	0.003	0.0000				
%RSD:	9.111	9.111	>999.9%				

Sequence No.: 110

Sample ID: 248117001|958951|1

Analyst: JXL

Autosampler Location: 94

Date Collected: 3/2/2010 11:56:48

Data Type: Original

Replicate Data: 248117001|958951|1

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.023	0.023	-0.0000	0.0025	0.0006	11:57:50	Yes
2	0.031	0.031	0.0000	0.0032	0.0006	11:58:25	Yes
Mean:	0.027	0.027	-0.0000				
SD:	0.005	0.005	0.0001				
%RSD:	19.43	19.43	681.10				

Sequence No.: 111

Sample ID: 248145001|958951|1

Analyst: JXL

Autosampler Location: 95

Date Collected: 3/2/2010 11:58:45

Data Type: Original

Replicate Data: 248145001|958951|1

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.029	0.029	0.0000	0.0032	0.0006	11:59:46	Yes
2	0.027	0.027	-0.0000	0.0029	0.0006	12:00:21	Yes
Mean:	0.028	0.028	0.0000				
SD:	0.001	0.001	0.0000				
%RSD:	4.334	4.334	287.89				

Sequence No.: 112

Sample ID: 1202056575|958951|1

Analyst: JXL

Autosampler Location: 96

Date Collected: 3/2/2010 12:00:41

Data Type: Original

Replicate Data: 1202056575|958951|1

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.024	0.024	-0.0000	0.0028	0.0006	12:01:43	Yes
2	0.032	0.032	0.0000	0.0030	0.0007	12:02:19	Yes
Mean:	0.028	0.028	-0.0000				
SD:	0.006	0.006	0.0001				
%RSD:	20.52	20.52	>999.9%				

=====

Sequence No.: 113
Sample ID: 1202056576|958951|1
Analyst: JXLAutosampler Location: 97
Date Collected: 3/2/2010 12:02:39
Data Type: Original-----
Replicate Data: 1202056576|958951|1

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	2.290	2.290	0.0240	0.1266	0.0246	12:03:41	Yes
2	2.255	2.255	0.0236	0.1250	0.0243	12:04:16	Yes
Mean:	2.273	2.273	0.0238				
SD:	0.024	0.024	0.0003				
%RSD:	1.063	1.063	1.08				

=====

Sequence No.: 114
Sample ID: 1202056577|958951|5
Analyst: JXLAutosampler Location: 98
Date Collected: 3/2/2010 12:04:36
Data Type: Original-----
Replicate Data: 1202056577|958951|5

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.030	0.030	0.0000	0.0032	0.0006	12:05:38	Yes
2	0.032	0.032	0.0000	0.0031	0.0006	12:06:13	Yes
Mean:	0.031	0.031	0.0000				
SD:	0.001	0.001	0.0000				
%RSD:	4.606	4.606	53.00				

=====

Sequence No.: 115
Sample ID: 1202056608|958969|1
Analyst: JXLAutosampler Location: 99
Date Collected: 3/2/2010 12:06:33
Data Type: Original-----
Replicate Data: 1202056608|958969|1

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.025	0.025	-0.0000	0.0030	0.0006	12:07:35	Yes
2	0.023	0.023	-0.0000	0.0027	0.0006	12:08:10	Yes
Mean:	0.024	0.024	-0.0000				
SD:	0.001	0.001	0.0000				
%RSD:	4.800	4.800	32.24				

=====

Sequence No.: 116
Sample ID: 1202056609|958969|1
Analyst: JXLAutosampler Location: 100
Date Collected: 3/2/2010 12:08:30
Data Type: Original-----
Replicate Data: 1202056609|958969|1

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	2.265	2.265	0.0237	0.1245	0.0244	12:09:32	Yes
2	2.262	2.262	0.0237	0.1229	0.0243	12:10:08	Yes
Mean:	2.263	2.263	0.0237				
SD:	0.002	0.002	0.0000				
%RSD:	0.077	0.077	0.08				

Sequence No.: 117

Sample ID: 248162001|958969|1

Analyst: JXL

Autosampler Location: 101

Date Collected: 3/2/2010 12:10:28

Data Type: Original

Replicate Data: 248162001|958969|1

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.027	0.027	-0.0000	0.0030	0.0006	12:11:30	Yes
2	0.030	0.030	0.0000	0.0030	0.0006	12:12:05	Yes
Mean:	0.028	0.028	0.0000				
SD:	0.002	0.002	0.0000				
%RSD:	5.485	5.485	294.70				

=====

Sequence No.: 118

Sample ID: CCV

Analyst:

Autosampler Location: 7

Date Collected: 3/2/2010 12:12:25

Data Type: Original

Replicate Data: CCV

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	5.004	5.004	0.0528	0.2717	0.0534	12:13:26	Yes
2	5.010	5.010	0.0529	0.2692	0.0535	12:14:01	Yes
Mean:	5.007	5.007	0.0529				
SD:	0.004	0.004	0.0000				
%RSD:	0.080	0.080	0.08				

QC value within limits for Hg 253.7 Recovery = 100.14%

All analyte(s) passed QC.

=====

Sequence No.: 119

Sample ID: CCB

Analyst:

Autosampler Location: 8

Date Collected: 3/2/2010 12:14:20

Data Type: Original

Replicate Data: CCB

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.030	0.030	0.0000	0.0031	0.0006	12:15:21	Yes
2	0.038	0.038	0.0001	0.0035	0.0007	12:15:56	Yes
Mean:	0.034	0.034	0.0001				
SD:	0.005	0.005	0.0001				
%RSD:	15.64	15.64	89.85				

QC value within limits for Hg 253.7 Recovery = Not calculated

All analyte(s) passed QC.

=====

Sequence No.: 120

Sample ID: 248162002|958969|1

Analyst: JXL

Autosampler Location: 102

Date Collected: 3/2/2010 12:16:15

Data Type: Original

Replicate Data: 248162002|958969|1

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
#	ug/L	ug/L	Signal	Area	Height		Stored
1	0.024	0.024	-0.0000	0.0026	0.0006	12:17:17	Yes
2	0.032	0.032	0.0000	0.0031	0.0006	12:17:52	Yes
Mean:	0.028	0.028	-0.0000				
SD:	0.005	0.005	0.0001				
%RSD:	18.16	18.16	>999.9%				

=====

Sequence No.: 121

Sample ID: 248162003|958969|1

Analyst: JXL

Autosampler Location: 103

Date Collected: 3/2/2010 12:18:12

Data Type: Original

Replicate Data: 248162003|958969|1

Repl	SampleConc	StdConc	BlkCorr	Peak	Peak	Time	Peak
------	------------	---------	---------	------	------	------	------

Miscellaneous

Prep Logbook

Acid Digestion of Total Recoverable or Dissolved Metals in Surface and Groundwater Samples for Analysis by ICP or ICP-MS

Batch ID: 959108.0
 Analyst: Francena Armstrong
 Method: SW846 3005A
 Lab SOP: GL-MA-E-006 REV# 9
 Instrument: Sartorius Balance B-001

Type	Sample Id	Description	Serial Number	Spike Amount	Spike Units
LCS	1202056867	Metals Spike Mix I	U1100205-01	.25	mL
LCS	1202056867	Metals Spike Mix II	U1100205-06	.25	mL
MS	1202056869	Metals Spike Mix I	U1100205-01	.25	mL
MS	1202056869	Metals Spike Mix II	U1100205-06	.25	mL

Sample ID	Run Date	Matrix	Initial Volume (mL)	Final Volume (mL)	Prep Factor (mL/mL)	pH Check
1202056866 MB	04-MAR-2010 14:00:00	Water	50	50	1	<2
1202056867 LCS	04-MAR-2010 14:00:00	Water	50	50	1	<2
248108001	04-MAR-2010 14:00:00	Water	50	50	1	<2
248117001	04-MAR-2010 14:00:00	Water	50	50	1	<2
248162001	04-MAR-2010 14:00:00	Water	50	50	1	<2
248162002	04-MAR-2010 14:00:00	Water	50	50	1	<2
248162003	04-MAR-2010 14:00:00	Water	50	50	1	<2
248162004	04-MAR-2010 14:00:00	Water	50	50	1	<2
248172001	04-MAR-2010 14:00:00	Water	50	50	1	<2
248173001	04-MAR-2010 14:00:00	Water	50	50	1	<2
248199001	04-MAR-2010 14:00:00	Water	50	50	1	<2
1202056868 DUP (248199001)	04-MAR-2010 14:00:00	Water	50	50	1	<2
1202056869 MS (248199001)	04-MAR-2010 14:00:00	Water	50	50	1	<2
1202056870 SDI.T (248199001)	04-MAR-2010 14:00:00	Water	50	50	1	<2

Reagent/Solvent Lot ID	Description	Amount	Comments:
1277916	HYDROCHLORIC ACID	2.5 mL	
1277919	Nitric Acid CONC.	1 mL	

Prep Logbook

Acid Digestion of Total Recoverable or Dissolved Metals in Surface and Groundwater Samples for Analysis by ICP or ICP-MS

Batch ID: 959110.0
 Analyst: Francena Armstrong
 Method: SW846 3005A
 Lab SOP: GL-MA-E-006 REV# 9
 Instrument: Sartorius Balance B-001

Verified by: _____
 Type: LCS
 Sample Id: 1202056873
 Description: ICP-MS SPIKE FOR ALL CLIENTS EXCEPT DOE CLIENTS (Solution A). MS SPIKE FOR ALL CLIENTS EXCEPT DOE CLIENTS (Solution B).
 Serial Number: U1100205-A
 Spike Amount: .5 mL
 Type: LCS
 Sample Id: 1202056873
 Description: ICP-MS SPIKE FOR ALL CLIENTS EXCEPT DOE CLIENTS (Solution A). MS SPIKE FOR ALL CLIENTS EXCEPT DOE CLIENTS (Solution B).
 Serial Number: U1100205-B
 Spike Amount: .5 mL
 Type: MS
 Sample Id: 1202056875
 Description: ICP-MS DOE Liquid Spike Solution A
 Serial Number: U1090930-A
 Spike Amount: .5 mL
 Type: MS
 Sample Id: 1202056875
 Description: ICP-MS DOE Liquid Spike Solution B
 Serial Number: U1090930-B
 Spike Amount: .5 mL

Sample ID	Run Date	Matrix	Initial Volume (mL)	Final Volume (mL)	Prep Factor (mL/mL)	pH Check
1202056872 MB	04-MAR-2010 14:00:00	Water	50	50	1	<2
1202056873 LCS	04-MAR-2010 14:00:00	Water	50	50	1	<2
248108001	04-MAR-2010 14:00:00	Water	50	50	1	<2
248117001	04-MAR-2010 14:00:00	Water	50	50	1	<2
248162001	04-MAR-2010 14:00:00	Water	50	50	1	<2
248162002	04-MAR-2010 14:00:00	Water	50	50	1	<2
248162003	04-MAR-2010 14:00:00	Water	50	50	1	<2
248162004	04-MAR-2010 14:00:00	Water	50	50	1	<2
248172001	04-MAR-2010 14:00:00	Water	50	50	1	<2
248173001	04-MAR-2010 14:00:00	Water	50	50	1	<2
248199001	04-MAR-2010 14:00:00	Water	50	50	1	<2
1202056874 DUP (248199001)	04-MAR-2010 14:00:00	Water	50	50	1	<2
1202056875 MS (248199001)	04-MAR-2010 14:00:00	Water	50	50	1	<2
1202056876 SDILT (248199001)	04-MAR-2010 14:00:00	Water	50	50	1	<2

Reagent/Solvent Lot ID	Description	Amount	Comments:
1277916	HYDROCHLORIC ACID	2.5 mL	
1277919	Nitric Acid CONC.	1 mL	

Prep Logbook

Mercury Analysis Using the Perkin Elmer Automated Mercury Analyzer

Batch ID: 958949.0
Analyst: Tara Griffin
Method: SW846 7470A Prep
Lab SOP: GL-MA-E-010 REV# 23
Instrument: No analytical instrument

Verified by: _____

Type	Sample Id	Description	Serial Number	Spike Amount	Spike Units
LCS	1202056574	Mercury working intermediate standard for LCS/MS	WHG100301-13	.2	mL
MS	1202056576	Mercury working intermediate standard for LCS/MS	WHG100301-13	.2	mL

Sample ID	Run Date	Matrix	Initial Volume (mL)	Final Volume (mL)	Prep Factor (mL/mL)	pH Check
1202056573 MB	01-MAR-2010 12:20:00	Water	20	20	1	<2
1202056574 LCS	01-MAR-2010 12:20:00	Water	20	20	1	<2
247997001	01-MAR-2010 12:20:00	Water	20	20	1	<2
248001001	01-MAR-2010 12:20:00	Water	20	20	1	<2
248010001	01-MAR-2010 12:20:00	Water	20	20	1	<2
248010002	01-MAR-2010 12:20:00	Water	20	20	1	<2
248032001	01-MAR-2010 12:20:00	Water	20	20	1	<2
248034001	01-MAR-2010 12:20:00	Water	20	20	1	<2
248038001	01-MAR-2010 12:20:00	Water	20	20	1	<2
248038002	01-MAR-2010 12:20:00	Water	20	20	1	<2
248039001	01-MAR-2010 12:20:00	Water	20	20	1	<2
248046001	01-MAR-2010 12:20:00	Water	20	20	1	<2
248046002	01-MAR-2010 12:20:00	Water	20	20	1	<2
248053001	01-MAR-2010 12:20:00	Water	20	20	1	<2
248053002	01-MAR-2010 12:20:00	Water	20	20	1	<2
248053003	01-MAR-2010 12:20:00	Water	20	20	1	<2
248108001	01-MAR-2010 12:20:00	Water	20	20	1	<2
248117001	01-MAR-2010 12:20:00	Water	20	20	1	<2
248145001	01-MAR-2010 12:20:00	Water	20	20	1	<2
1202056575 DUP (248145001)	01-MAR-2010 12:20:00	Water	20	20	1	<2
1202056576 MS (248145001)	01-MAR-2010 12:20:00	Water	20	20	1	<2
1202056577 SDILT (248145001)	01-MAR-2010 12:20:00	Water	20	20	1	<2

Reagent/Solvent Lot ID	Description	Amount	Comments:
1176183	Sulfuric Acid, Concentrated	1 mL	Digestion Start Date: 01-MAR-10 12:20
1255532-C	Hg reducing agent	1 mL	Digestion End Date: 01-MAR-10 14:20
1274391-1	NITRIC ACID	.5 mL	

Analytical Logbook version 1 11-04-2002

GEL Laboratories LLC

Standard Logbook

Serial ID: UHG1167639-01 **Opened:** 13-AUG-09 **Amount :** 125 mL
Name: MHGSTOCK1 **Received:** 13-AUG-09 **Catalog Number :** PLHG4-2Y
Type: Source Material **Expires:** 13-AUG-10 **Lot Number :** 15-37HG
Employee: Bryan Davis **Solvent :** 10% HNO3
Supplier: Spex
Description: Mercury Source Standard #1 1,000 mg/L
Comments: None

Analyte	Concentration	Analyte	Concentration
Mercury	1000 mg/L		

Serial ID: UHG1167641-02 **Opened:** 13-AUG-09 **Amount :** 100 mL
Name: MHGSTOCK2 **Received:** 13-AUG-09 **Catalog Number :** AHG1KN-100
Type: Source Material **Expires:** 13-AUG-10 **Lot Number :** 4905530
Employee: Bryan Davis **Solvent :** 3% HNO3
Supplier: Ricca Chemical Company
Description: Mercury Source Standard #2 1,000 mg/L
Comments: None

Analyte	Concentration	Analyte	Concentration
Mercury	999.7 mg/L		

Serial ID: UI090421-40 **Opened:** 09-OCT-09 **Amount :** 250 mL
Name: TRACE ICP Na-1000SOUR **Received:** 21-APR-09 **Catalog Number :** HP100052-1
Type: Source Material **Expires:** 09-OCT-10 **Lot Number :** 0830227
Employee: Helen Camello **Solvent :** 1%HNO3
Supplier: ENVIRONMENTAL EXPRESS
Description: Sodium 1000 +/- 3 ug/mL in 1% HNO3
Comments: None

Analyte	Concentration	Analyte	Concentration
Sodium	1000 ug/mL		

Serial ID: UI090422-40 **Opened:** 04-MAY-09 **Amount :** 500 mL
Name: TRACE ICP ICSA SOLN A **Received:** 22-APR-09 **Catalog Number :** 160005-01-03
Type: Source Material **Expires:** 04-MAY-10 **Lot Number :** 1013357
Employee: Helen Camello **Solvent :** 5%HNO3
Supplier: o2si
Description: TRACE ICP ICSA SOLN A mg/L +/- 0.5% IN 5% HNO3
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	5000 mg/L	Calcium	5000 mg/L
Iron	2000 mg/L	Magnesium	5000 mg/L

Standard Logbook

Serial ID: UI090612-02 **Opened:** 12-JUN-09 **Catalog Number :** 060074-06-01
Name: ICPMS Tungsten - 10mg/L **Received:** 12-JUN-09 **Lot Number :** 1016377
Type: Source Material **Expires:** 12-JUN-10 **Solvent :** 2% HNO3
Employee: Paul Boyd
Supplier: O2SI
Description: ICPMS Tungsten standard SPIKE - 10mg/L
Comments: None

Analyte	Concentration	Analyte	Concentration
Tungsten	10 mg/L		

Serial ID: UI090701-09 **Opened:** 01-JUL-09 **Amount :** 250 mL
Name: ICP-MS CRDL Master #1 **Received:** 01-JUL-09 **Catalog Number :** 160044-09-02
Type: Source Material **Expires:** 01-JUL-10 **Lot Number :** 1016477
Employee: Paul Boyd **Solvent :** +/- 0.5% IN 2% HNO3
Supplier: O2SI
Description: ICPMS CRDL Master Soln #1
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	15 mg/L	Arsenic	5 mg/L
Barium	2 mg/L	Beryllium	.5 mg/L
Boron	15 mg/L	Cadmium	1 mg/L
Calcium	100 mg/L	Chromium	3 mg/L
Cobalt	1 mg/L	Copper	1 mg/L
Iron	25 mg/L	Lead	2 mg/L
Lithium	10 mg/L	Magnesium	15 mg/L
Manganese	5 mg/L	Nickel	2 mg/L
Phosphorous	50 mg/L	Potassium	300 mg/L
Selenium	5 mg/L	Sodium	250 mg/L
Strontium	10 mg/L	Thallium	1 mg/L
Thorium	1 mg/L	Uranium	.2 mg/L
Vanadium	10 mg/L	Zinc	10 mg/L

Serial ID: UI090701-10 **Opened:** 01-JUL-09 **Amount :** 250 mL
Name: ICP-MS CRDL Master #2 **Received:** 01-JUL-09 **Catalog Number :** 160044-08-02
Type: Source Material **Expires:** 01-JUL-10 **Lot Number :** 1016476
Employee: Paul Boyd **Solvent :** +/- 0.5% IN 2% HNO3
Supplier: O2SI
Description: ICPMS CRDL Soln #2
Comments: None

Analyte	Concentration	Analyte	Concentration
Antimony	2 mg/L	Molybdenum	.5 mg/L
Silver	1 mg/L	Tin	2 mg/L
Titanium	10 mg/L	Tungsten	5 mg/L

Standard Logbook

Analyte	Concentration	Analyte	Concentration
Zirconium	2 mg/L		

Serial ID: UI090701-40 **Opened:** 01-JUL-09 **Amount :** 500 mL
Name: TRACE ICP Stock PQL St **Received:** 30-JUN-09 **Catalog Number :** 160543-01-03
Type: Source Material **Expires:** 01-JUL-10 **Lot Number :** 1016475
Employee: Helen Camello **Solvent :** +/-0.5%in2%HNO3+TrHF
Supplier: 02si
Description: TRACE ICP Stock PQL Standard
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	100 mg/L	Antimony	5 mg/L
Arsenic	15 mg/L	Barium	2.5 mg/L
Beryllium	2.5 mg/L	Boron	25 mg/L
Cadmium	2.5 mg/L	Calcium	100 mg/L
Chromium	2.5 mg/L	Cobalt	2.5 mg/L
Copper	5 mg/L	Iron	50 mg/L
Lead	5 mg/L	Magnesium	150 mg/L
Manganese	5 mg/L	Molybdenum	5 mg/L
Nickel	2.5 mg/L	Phosphorous	75 mg/L
Potassium	75 mg/L	Selenium	15 mg/L
Silicon	50 mg/L	Silver	2.5 mg/L
Sodium	150 mg/L	Strontium	2.5 mg/L
Sulfur	50 mg/L	Thallium	10 mg/L
Tin	5 mg/L	Titanium	2.5 mg/L
Uranium	25 mg/L	Vanadium	2.5 mg/L
Zinc	5 mg/L		

Serial ID: UI090925-40 **Opened:** 23-OCT-09 **Amount :** 500 mL
Name: SECOND SOURCE STD -1 **Received:** 25-SEP-09 **Catalog Number :** SGELMX38-500N
Type: Source Material **Expires:** 30-SEP-10 **Lot Number :** 4909129
Employee: Helen Camello **Solvent :** 5%HNO3
Supplier: SPECTRO PURE
Description: SECOND SOURCE STD #1A 5%HNO3
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	1000 mg/L	Arsenic	100 mg/L
Barium	100 mg/L	Boron	100 mg/L
Cadmium	100 mg/L	Calcium	1000 mg/L
Chromium	100 mg/L	Cobalt	100 mg/L
Copper	100 mg/L	Iron	1000 mg/L
Lead	100 mg/L	Phosphorous	500 mg/L
Potassium	500 mg/L	Selenium	500 mg/L
Sodium	500 mg/L	Strontium	100 mg/L

Standard Logbook

Serial ID: UI090925-41 **Opened:** 23-OCT-09 **Amount :** 500 mL
Name: SECOND SOURCE STD -1 **Received:** 25-SEP-09 **Catalog Number :** SGELMX39-500B
Type: Source Material **Expires:** 30-SEP-10 **Lot Number :** 4909130
Employee: Helen Camello **Solvent :** 5%HNO3,TR,HF
Supplier: SPECTRO PURE
Description: SECOND SOURCE STD #1B
Comments: None

Analyte	Concentration	Analyte	Concentration
Antimony	100 mg/L	Beryllium	50 mg/L
Magnesium	1000 mg/L	Manganese	100 mg/L
Molybdenum	100 mg/L	Nickel	100 mg/L
Silver	50 mg/L	Sulfur	500 mg/L
Thallium	100 mg/L	Tin	100 mg/L
Titanium	100 mg/L	Uranium	100 mg/L
Vanadium	100 mg/L	Zinc	100 mg/L

Serial ID: UI090930-A **Opened:** 30-SEP-09 **Catalog Number :** 160067-02
Name: ICP-MS DOE Liquid SPIKE **Received:** 28-SEP-09 **Lot Number :** 1017141
Type: Source Material **Expires:** 30-SEP-10
Employee: Francena Armstrong **Verified:** 21-NOV-08
Supplier: O2Si
Description: ICP-MS DOE liquid Spike Solution A
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	200 mg/L	Arsenic	8 mg/L
Barium	5 mg/L	Beryllium	5 mg/L
Boron	10 mg/L	Cadmium	1 mg/L
Calcium	200 mg/L	Chromium	5 mg/L
Cobalt	5 mg/L	Copper	5 mg/L
Iron	200 mg/L	Lead	4 mg/L
Lithium	5 mg/L	Magnesium	200 mg/L
Manganese	5 mg/L	Nickel	5 mg/L
Phosphorus, Total as P	200 mg/L	Potassium	200 mg/L
Selenium	2 mg/L	Silicon	200 mg/L
Sodium	200 mg/L	Strontium	5 mg/L
Thallium	10 mg/L	Thorium	5 mg/L
Total Uranium	5 mg/L	Uranium	5 mg/L
Uranium-235	.0364 mg/L	Uranium-238	4.96 mg/L
Vanadium	5 mg/L	Zinc	5 mg/L

Standard Logbook

Serial ID: UI090930-B **Opened:** 30-SEP-09 **Catalog Number :** 160067-02
Name: ICP-MS DOE Liquid SPIKE **Received:** 28-SEP-09 **Lot Number :** 1017141
Type: Source Material **Expires:** 30-SEP-10
Employee: Francena Armstrong **Verified:** 21-NOV-08
Supplier: O2Si
Description: ICP-MS DOE Liquid Spike Solution B
Comments: None

Analyte	Concentration	Analyte	Concentration
Antimony	20 mg/L	Molybdenum	5 mg/L
Silver	5 mg/L	Tin	5 mg/L
Titanium	5 mg/L	Zirconium	5 mg/L

Serial ID: UI091015-42 **Opened:** 28-OCT-09 **Amount :** 500 mL
Name: SI 1000mg/L **Received:** 15-OCT-09 **Catalog Number :** 060014-02-03
Type: Source Material **Expires:** 28-OCT-10 **Lot Number :** 1017581
Employee: Helen Camello **Solvent :** 0.3%H2O(NH4)2SiF6
Supplier: o2si
Description: Silicon 1000mg/L+/-0.3%in H2O(NH4)2SiF6
Comments: None

Analyte	Concentration	Analyte	Concentration
Silica	2139 mg/L	Silicon	1000 mg/L

Serial ID: UI091102-40 **Opened:** 16-NOV-09 **Amount :** 500 mL
Name: TRACE CALSTD#1A SOUF **Received:** 02-NOV-09 **Catalog Number :** HP2270-1-500
Type: Source Material **Expires:** 31-OCT-10 **Lot Number :** 0930215
Employee: Helen Camello **Solvent :** HNO3
Supplier: Environmental Express
Description: Trace Calibration Std #1A
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	2000 mg/L	Arsenic	200 mg/L
Barium	200 mg/L	Beryllium	200 mg/L
Boron	200 mg/L	Cadmium	200 mg/L
Calcium	2000 mg/L	Chromium	200 mg/L
Cobalt	200 mg/L	Copper	200 mg/L
Iron	2000 mg/L	Lead	200 mg/L
Magnesium	2000 mg/L	Manganese	200 mg/L
Nickel	200 mg/L	Phosphorous	1000 mg/L
Potassium	2000 mg/L	Selenium	200 mg/L
Sodium	2000 mg/L	Strontium	200 mg/L
Thallium	200 mg/L	Uranium	200 mg/L
Vanadium	200 mg/L	Zinc	200 mg/L

Standard Logbook

Serial ID: UI091102-41 **Opened:** 16-NOV-09 **Amount :** 500 mL
Name: TRACE CALSTD#1B SOUF **Received:** 02-NOV-09 **Catalog Number :** HP2270-2-500
Type: Source Material **Expires:** 31-OCT-10 **Lot Number :** 0930216
Employee: Helen Camello **Solvent :** HNO3
Supplier: Environmental Express
Description: Trace Calibration Standard #1B
Comments: None

Analyte	Concentration	Analyte	Concentration
Antimony	200 mg/L	Molybdenum	200 mg/L
Silver	200 mg/L	Sulfur	400 mg/L
Tin	200 mg/L	Titanium	200 mg/L

Serial ID: UI091102-42 **Opened:** 17-NOV-09 **Amount :** 200 mL
Name: SILICON **Received:** 02-NOV-09 **Catalog Number :** HP100050-4F
Type: Source Material **Expires:** 17-NOV-10 **Lot Number :** 0921924
Employee: Helen Camello **Solvent :** H2O/tr HF
Supplier: ENVIRONMENTAL EXPRESS
Description: SILICON 1000mg/L H2O/tr HF
Comments: None

Analyte	Concentration	Analyte	Concentration
Silica	2139 mg/L	Silicon	1000 mg/L

Serial ID: UI100205-01 **Opened:** 05-FEB-10 **Lot Number :** 1018514
Name: METALSPIKE-1 **Received:** 05-FEB-10
Type: Source Material **Expires:** 05-FEB-11
Employee: Francena Armstrong
Supplier: OS2I
Description: Metals Spike Mix I
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	1000 ug/mL	Arsenic	100 ug/mL
Barium	100 ug/mL	Beryllium	100 ug/mL
Boron	100 ug/mL	Cadmium	100 ug/mL
Calcium	1000 ug/mL	Cobalt	100 ug/mL
Iron	1000 ug/mL	Lead	100 ug/mL
Magnesium	1000 ug/mL	Phosphorous	100 ug/mL
Potassium	1000 ug/mL	Silver	100 ug/mL
Sodium	1000 ug/mL	Strontium	100 ug/mL

Standard Logbook

Serial ID: UI100205-06 **Opened:** 05-FEB-10 **Lot Number :** 1018515
Name: METALSPIKE-2 **Received:** 05-FEB-10
Type: Source Material **Expires:** 05-FEB-11
Employee: Francena Armstrong
Supplier: OS2I
Description: Metals Spike Mix II
Comments: None

Analyte	Concentration	Analyte	Concentration
Antimony	100 ug/mL	Chromium	100 ug/mL
Copper	100 ug/mL	Manganese	100 ug/mL
Molybdenum	100 ug/mL	Nickel	100 ug/mL
Selenium	100 ug/mL	Silica	2141 ug/mL
Silicon	1000 ug/mL	Sulfur	1000 ug/mL
Thallium	100 ug/mL	Tin	100 ug/mL
Titanium	100 ug/mL	Uranium	100 ug/mL
Uranium-235	.72 ug/mL	Uranium-238	99.28 ug/mL
Vanadium	100 ug/mL	Zinc	100 ug/mL

Serial ID: UI100205-A **Opened:** 05-FEB-10 **Catalog Number :** 160067-05
Name: ICP-MS ALL OTHER SPIKE **Received:** 05-FEB-10 **Lot Number :** 1018516
Type: Source Material **Expires:** 05-FEB-11
Employee: Francena Armstrong
Supplier: O2si
Description: ICP-MS SPIKE FOR ALL CLIENTS EXCEPT DOE CLIENTS (Solution A).
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	200 mg/L	Arsenic	5 mg/L
Barium	5 mg/L	Beryllium	5 mg/L
Bismuth	5 mg/L	Boron	10 mg/L
Cadmium	5 mg/L	Calcium	200 mg/L
Cesium	5 mg/L	Chromium	5 mg/L
Cobalt	5 mg/L	Copper	5 mg/L
Iron	200 mg/L	Lead	5 mg/L
Lithium	5 mg/L	Magnesium	200 mg/L
Manganese	5 mg/L	Nickel	5 mg/L
Phosphorous	200 mg/L	Potassium	200 mg/L
Selenium	5 mg/L	Sodium	200 mg/L
Strontium	5 mg/L	Thallium	5 mg/L
Thorium	5 mg/L	Uranium	5 mg/L
Uranium-235	.036 mg/L	Uranium-238	4.964 mg/L
Vanadium	5 mg/L	Zinc	5 mg/L

Standard Logbook

Serial ID: UI100205-B **Opened:** 05-FEB-10 **Catalog Number :** 160067-05
Name: ICP-MS ALL OTHER SPIKE **Received:** 05-FEB-10 **Lot Number :** 1018516
Type: Source Material **Expires:** 05-FEB-11
Employee: Francena Armstrong
Supplier: O2si
Description: MS SPIKE FOR ALL CLIENTS EXCEPT DOE CLIENTS (Solution B).
Comments: None

Analyte	Concentration	Analyte	Concentration
Antimony	5 mg/L	Molybdenum	5 mg/L
Silver	5 mg/L	Tin	5 mg/L
Titanium	5 mg/L	Zirconium	5 mg/L

Serial ID: UI100310-48 **Opened:** 19-MAR-10 **Amount :** 1000 mL
Name: Trace ICP ICSA **Received:** 12-MAR-10 **Catalog Number :** 160005-02
Type: Source Material **Expires:** 19-MAR-11 **Lot Number :** 1019141
Employee: Helen Camello **Solvent :** 3% HCl + 1% HNO3
Supplier: o2si
Description: Trace ICP Interferent Check Standard A
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	500000 UG/L	Calcium	500000 UG/L
Iron	200000 UG/L	Magnesium	500000 UG/L

Serial ID: UI100310-49.11 **Opened:** 29-MAR-10 **Amount :** 100 ml
Name: Trace ICP ICSAB **Received:** 12-MAR-10 **Catalog Number :** 160066-04
Type: Source Material **Expires:** 30-MAR-10 **Lot Number :** 1019142
Employee: Helen Camello **Solvent :** 3% HCl + 1% HNO3
Supplier: o2si
Description: Trace ICP Inteferent Check Standard AB
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	500000 ug/L	Antimony	500 ug/L
Arsenic	500 ug/L	Barium	500 ug/L
Beryllium	250 ug/L	Boron	500 ug/L
Cadmium	500 ug/L	Calcium	500000 ug/L
Chromium	500 ug/L	Cobalt	500 ug/L
Copper	500 ug/L	Iron	200000 ug/L
Lead	500 ug/L	Magnesium	500000 ug/L
Manganese	500 ug/L	Molybdenum	500 ug/L
Nickel	500 ug/L	Phosphorous	2500 ug/L
Potassium	5000 ug/L	Selenium	2500 ug/L
Silica	10696.5 ug/L	Silicon	5000 ug/L
Silver	250 ug/L	Sodium	5000 ug/L

Standard Logbook

Analyte	Concentration	Analyte	Concentration
Strontium	500 ug/L	Sulfur	2500 ug/L
Thallium	500 ug/L	Tin	500 ug/L
Titanium	500 ug/L	Uranium	500 ug/L
Vanadium	500 ug/L	Zinc	500 ug/L

Serial ID: UI100317-06 **Opened:** 17-MAR-10 **Amount :** 250 mL
Name: ICP-MS ICV/CCV Master A **Received:** 17-MAR-10 **Catalog Number :** 160055-01
Type: Source Material **Expires:** 17-MAR-11 **Lot Number :** 1019161
Employee: Paul Boyd **Solvent :** +/- 0.5% in 5% HNO3 100 cm2
Supplier: 02SI
Description: ICPMS ICV/CCV SOLN A - 10ppm
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	2020 mg/L	Calcium	2000 mg/L
Iron	2000 mg/L	Magnesium	2000 mg/L
Phosphorous	2000 mg/L	Potassium	2000 mg/L
Sodium	2000 mg/L		

Serial ID: UI100317-07 **Opened:** 17-MAR-10 **Amount :** 250 mL
Name: ICP-MS ICV/CCV Master B **Received:** 17-MAR-10 **Catalog Number :** 160054-02
Type: Source Material **Expires:** 17-MAR-11 **Lot Number :** 1019162
Employee: Paul Boyd **Solvent :** +/- 0.5% in 5% HNO3 100 cm2
Supplier: 02SI
Description: ICPMS ICV/CCV Soln B - 10ppm
Comments: None

Analyte	Concentration	Analyte	Concentration
Arsenic	20 mg/L	Barium	20 mg/L
Beryllium	20 mg/L	Boron	40 mg/L
Cadmium	20 mg/L	Chromium	20 mg/L
Cobalt	20 mg/L	Copper	20 mg/L
Lead	20 mg/L	Lithium	20 mg/L
Manganese	20 mg/L	Nickel	20 mg/L
Selenium	20 mg/L	Strontium	20 mg/L
Thallium	20 mg/L	Thorium	20 mg/L
Uranium	20 mg/L	Vanadium	20 mg/L
Zinc	20 mg/L		

Serial ID: UI100317-08 **Opened:** 17-MAR-10 **Amount :** 250 mL
Name: ICP-MS ICV/CCV Master C **Received:** 17-MAR-10 **Catalog Number :** 160054-03
Type: Source Material **Expires:** 17-MAR-11 **Lot Number :** 1019163
Employee: Paul Boyd **Solvent :** +/- 0.5% in 5% HNO3 100 cm2
Supplier: 02SI

Standard Logbook

Description: ICPMS ICV/CCV Soln C - 10ppm

Comments: None

Analyte	Concentration	Analyte	Concentration
Antimony	20 mg/L	Molybdenum	20 mg/L
Silver	20 mg/L	Tin	20 mg/L
Titanium	20 mg/L	Tungsten	20 mg/L
Zirconium	20 mg/L		

Serial ID: UI100318-11 **Opened:** 18-MAR-10 **Amount :** 1000 mL
Name: ICP-MS ICSA Master A **Received:** 18-MAR-10 **Catalog Number :** 160013-01-01L
Type: Source Material **Expires:** 15-APR-10 **Lot Number :** 1018321
Employee: Paul Boyd **Solvent :** 2% HNO3
Supplier: 02SI
Description: ICP-MS ICSA Master A
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	1000 mg/L	Calcium	1000 mg/L
Carbon	2000 mg/L	Chloride	10000 mg/L
Iron	1000 mg/L	Magnesium	1000 mg/L
Molybdenum	20 mg/L	Phosphorous	1000 mg/L
Potassium	1000 mg/L	Sodium	1000 mg/L
Sulfur	1000 mg/L	Titanium	20 mg/L

Serial ID: UI100325-40 **Opened:** 25-MAR-10 **Amount :** 500 mL
Name: ICP HIGH RANGE STD-A **Received:** 25-MAR-10 **Catalog Number :** 160211-05-03
Type: Source Material **Expires:** 25-MAR-11 **Lot Number :** 1019348
Employee: Helen Camello **Solvent :** +/-0.5%in2%HNO3
Supplier: 02SI
Description: ICP HIGH RANGE STD SOLUTION A
Comments: None

Analyte	Concentration	Analyte	Concentration
Antimony	10000 ug/L	Arsenic	10000 ug/L
Barium	15000 ug/L	Beryllium	3000 ug/L
Boron	5000 ug/L	Cadmium	10000 ug/L
Chromium	25000 ug/L	Cobalt	10000 ug/L
Copper	20000 ug/L	Lead	25000 ug/L
Manganese	10000 ug/L	Molybdenum	10000 ug/L
Nickel	10000 ug/L	Phosphorous	15000 ug/L
Potassium	300000 ug/L	Selenium	10000 ug/L
Silica	107000 ug/L	Silicon	50000 ug/L
Silver	1000 ug/L	Strontium	10000 ug/L
Sulfur	50000 ug/L	Thallium	10000 ug/L
Tin	10000 ug/L	Titanium	10000 ug/L

Standard Logbook

Analyte	Concentration	Analyte	Concentration
Vanadium	10000 ug/L	Zinc	15000 ug/L

Serial ID: UI100325-41 **Opened:** 25-MAR-10 **Amount :** 500 mL
Name: ICP HIGH RANGE STD B **Received:** 25-MAR-10 **Catalog Number :** 160211-05-03
Type: Source Material **Expires:** 25-MAR-11 **Lot Number :** 1019348
Employee: Helen Camello **Solvent :** +/-0.5%in2%HNO3
Supplier: 02SI
Description: ICP HIGH RANGE STD SOLUTION B
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	500000 ug/L	Calcium	500000 ug/L
Iron	500000 ug/L	Magnesium	500000 ug/L
Sodium	500000 ug/L	Uranium	15000 ug/L

Serial ID: UI100405-12 **Opened:** 05-APR-10 **Amount :** 250 mL
Name: ICP-MS ICSAB Master B **Received:** 05-APR-10 **Catalog Number :** 160033-02
Type: Source Material **Expires:** 05-APR-11 **Lot Number :** 1019466
Employee: Paul Boyd **Solvent :** +/- 0.5% in 2% HNO3
Supplier: 02SI
Description: ICPMS ICSAB Master B
Comments: None

Analyte	Concentration	Analyte	Concentration
Arsenic	2 mg/L	Barium	2 mg/L
Beryllium	2 mg/L	Boron	2 mg/L
Cadmium	2 mg/L	Chromium	2 mg/L
Cobalt	2 mg/L	Copper	2 mg/L
Lead	2 mg/L	Lithium	2 mg/L
Manganese	2 mg/L	Nickel	2 mg/L
Selenium	2 mg/L	Strontium	2 mg/L
Thallium	2 mg/L	Thorium	2 mg/L
Uranium	2 mg/L	Vanadium	2 mg/L
Zinc	2 mg/L		

Serial ID: UI100405-13 **Opened:** 05-APR-10 **Amount :** 250 mL
Name: ICP-MS ICSAB Master C **Received:** 05-APR-10 **Catalog Number :** 160033-03
Type: Source Material **Expires:** 05-APR-11 **Lot Number :** 1019467
Employee: Paul Boyd **Solvent :** +/- 0.5% in 2% HNO3
Supplier: 02SI
Description: ICPMS ICSAB Master C
Comments: None

Analyte	Concentration	Analyte	Concentration
---------	---------------	---------	---------------

Standard Logbook

Analyte	Concentration	Analyte	Concentration
Antimony	2 mg/L	Silver	2 mg/L
Tin	2 mg/L	Tungsten	2 mg/L
Zirconium	2 mg/L		

Serial ID: UI100405-60 **Opened:** 05-APR-10 **Amount :** .5 mL
Name: ICPMS High Range Standard **Received:** 05-APR-10 **Catalog Number :** 160212-02-01
Type: Source Material **Expires:** 05-APR-11 **Lot Number :** 1019464
Employee: Paul Boyd **Solvent :** 2%HNO3 + Tr HF
Supplier: O2SI
Description: Linear Range Standard A
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	5000 mg/L	Arsenic	100 mg/L
Barium	250 mg/L	Beryllium	100 mg/L
Cadmium	100 mg/L	Calcium	5000 mg/L
Chromium	100 mg/L	Cobalt	100 mg/L
Copper	100 mg/L	Iron	5000 mg/L
Lead	500 mg/L	Lithium	100 mg/L
Magnesium	5000 mg/L	Manganese	100 mg/L
Nickel	100 mg/L	Phosphorous	2500 mg/L
Potassium	5000 mg/L	Selenium	50 mg/L
Sodium	5000 mg/L	Strontium	100 mg/L
Thallium	50 mg/L	Thorium	250 mg/L
Uranium	500 mg/L	Vanadium	100 mg/L
Zinc	250 mg/L		

Serial ID: UI100405-61 **Opened:** 05-APR-10 **Amount :** .5 mL
Name: ICPMS High Range Standard **Received:** 05-APR-10 **Catalog Number :** 160212-02-01
Type: Source Material **Expires:** 05-APR-11 **Lot Number :** 1019464
Employee: Paul Boyd **Solvent :** 2%HNO3 + Tr HF
Supplier: O2SI
Description: Linear Range Standard B
Comments: None

Analyte	Concentration	Analyte	Concentration
Antimony	25 mg/L	Molybdenum	100 mg/L
Silver	25 mg/L	Tin	100 mg/L
Tungsten	100 mg/L	Zirconium	50 mg/L

Standard Logbook

Serial ID: UMS100226-01 **Opened:** 26-FEB-10 **Amount :** 250 mL
Name: ICPMSCaSPIKEB **Received:** 26-FEB-10 **Catalog Number :** ZGEL-100-250
Type: Source Material **Expires:** 26-FEB-11 **Lot Number :** 21-104JB
Employee: Paul Boyd
Supplier: SPEX
Description: ICPMS Calibration Standard Solution B
Comments: None

Analyte	Concentration	Analyte	Concentration
Arsenic	10 mg/L	Barium	10 mg/L
Beryllium	10 mg/L	Boron	20 mg/L
Cadmium	10 mg/L	Chromium	10 mg/L
Cobalt	10 mg/L	Copper	10 mg/L
Lead	10 mg/L	Lithium	10 mg/L
Manganese	10 mg/L	Nickel	10 mg/L
Selenium	10 mg/L	Silver	10 mg/L
Strontium	10 mg/L	Thallium	10 mg/L
Thorium	10 mg/L	Uranium	10 mg/L
Vanadium	10 mg/L	Zinc	10 mg/L

Serial ID: UMS100226-02 **Opened:** 26-FEB-10 **Catalog Number :** ZGEL-102-250
Name: ICPMSCaSPIKEA **Received:** 26-FEB-10 **Lot Number :** 21-103JB
Type: Source Material **Expires:** 26-FEB-11
Employee: Paul Boyd
Supplier: SPEX
Description: ICPMS Calibration Standard Solution A
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	1000 mg/L	Calcium	1000 mg/L
Iron	1000 mg/L	Magnesium	1000 mg/L
Phosphorous	1000 mg/L	Potassium	1000 mg/L
Sodium	1000 mg/L		

Serial ID: UMS100226-03 **Opened:** 26-FEB-10 **Amount :** 250 ml
Name: ICPMSCaSPIKEC **Received:** 26-FEB-10 **Catalog Number :** ZGEL-101-250
Type: Source Material **Expires:** 26-FEB-11 **Lot Number :** 21-102JB
Employee: Paul Boyd
Supplier: SPEX
Description: ICPMS Calibration Standard Solution C
Comments: None

Analyte	Concentration	Analyte	Concentration
Antimony	10 mg/L	Molybdenum	10 mg/L
Tin	10 mg/L	Titanium	10 mg/L
Zirconium	10 mg/L		

Standard Logbook

Serial ID: IHG100301-01 **Opened:** 01-MAR-10 **Instrument Id :** Mercury
Name: MHGINTER1 **Received:** 01-MAR-10 **Pipet Id :** Minou1
Type: Intermediate **Expires:** 02-MAR-10 **Solvent :** 1mL HNO3 + Typel H2O
Employee: Tara Griffin
Supplier: GEL
Description: Mercury Intermediate 1st Source 200 ug/L
Comments: Prepare fresh daily

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UHG1167639-01	Mercury	1000 mg/L	.05 mL	250 mL	200 ug/L

Serial ID: IHG100301-02 **Opened:** 01-MAR-10 **Pipet Id :** Minou1
Name: MHGINTER2 **Received:** 01-MAR-10 **Solvent :** 2% HNO3-1274391
Type: Intermediate **Expires:** 02-MAR-10
Employee: Tara Griffin
Supplier: GEL
Description: Mercury Intermediate 2nd Source 200 ug/L
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UHG1167641-02	Mercury	999.7 mg/L	.05 mL	250 mL	200 ug/L

Serial ID: WHG100301-01a **Opened:** 01-MAR-10 **Pipet Id :** Hg1289245
Name: MHGWORKCAL0.2CRA **Received:** 01-MAR-10 **Solvent :** 2% HNO3-1274391
Type: Working **Expires:** 08-MAR-10
Employee: Tara Griffin
Supplier: GEL
Description: Mercury Working 1st Source CAL 0.2/CRA
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
IHG100301-01	Mercury	200 ug/L	20 uL	20 mL	.2 ug/L

Serial ID: WHG100301-02 **Opened:** 01-MAR-10 **Pipet Id :** Hg1289245
Name: MHGWORKCAL0.5 **Received:** 01-MAR-10 **Solvent :** 2% HNO3-1274391
Type: Working **Expires:** 08-MAR-10
Employee: Tara Griffin
Supplier: GEL
Description: Mercury Working 1st Source CAL 0.5
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
IHG100301-01	Mercury	200 ug/L	50 uL	20 mL	.5 ug/L

Standard Logbook

Serial ID: WHG100301-03 **Opened:** 01-MAR-10 **Pipet Id :** Hg1289245
Name: MHGWORKCAL2.0 **Received:** 01-MAR-10 **Solvent :** 2% HNO3-1274391
Type: Working **Expires:** 08-MAR-10
Employee: Tara Griffin **Verified:** 20-JUL-07
Supplier: GEL
Description: Mercury Working 1st Source CAL 2.0
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
IHG100301-01	Mercury	200 ug/L	200 uL	20 mL	2 ug/L

Serial ID: WHG100301-04 **Opened:** 01-MAR-10 **Pipet Id :** Hg1289245
Name: MHGWORKCAL5.0CCV **Received:** 01-MAR-10 **Solvent :** 2% HNO3-1274391
Type: Working **Expires:** 08-MAR-10
Employee: Tara Griffin **Verified:** 20-JUL-07
Supplier: GEL
Description: Mercury Working 1st Source CAL 5.0/CCV
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
IHG100301-01	Mercury	200 ug/L	500 uL	20 mL	5 ug/L

Serial ID: WHG100301-05 **Opened:** 01-MAR-10 **Pipet Id :** Hg1289245
Name: MHGWORKCAL10.0 **Received:** 01-MAR-10 **Solvent :** 2% HNO3-1274391
Type: Working **Expires:** 08-MAR-10
Employee: Tara Griffin **Verified:** 20-JUL-07
Supplier: GEL
Description: Mercury Working 1st Source CAL 10.0
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
IHG100301-01	Mercury	200 ug/L	1 mL	20 mL	10 ug/L

Serial ID: WHG100301-06 **Opened:** 01-MAR-10 **Pipet Id :** Hg1289245
Name: MHGWORK5.0ICV **Received:** 01-MAR-10 **Solvent :** 2% HNO3-1274391
Type: Working **Expires:** 08-MAR-10
Employee: Tara Griffin
Supplier: GEL
Description: Mercury Working 2nd Source 5.0/ICV
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
IHG100301-02	Mercury	200 ug/L	500 uL	20 mL	5 ug/L

Standard Logbook

Serial ID: WHG100301-13 **Opened:** 01-MAR-10 **Pipet Id :** Hg1289245
Name: MHGLIQLCSMSSPIKE **Received:** 01-MAR-10 **Solvent :** 2% HNO3-1274391
Type: Working **Expires:** 08-MAR-10
Employee: Tara Griffin **Verified:** 20-JUL-07
Supplier: GEL
Description: Mercury working intermediate standard for LCS/MS
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UHG1167639-01	Mercury	1000 mg/L	.05 mL	250 mL	200 ug/L

Serial ID: WI100329-42 **Opened:** 29-MAR-10 **Balance Id :** 216
Name: TRACE ICP 0.1 PPM STD. **Received:** 02-NOV-09 **Pipet Id :** 3581809
Type: Working **Expires:** 30-MAR-10 **Solvent :** 3%HCL and 1%HNO3 -1293083
Employee: Helen Camello
Supplier: GEL
Description: TRACE ICP 0.1 PPM CALIBRATION STD.
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
WI100329-44	Aluminum	10000 ug/L	10 mL	100 mL	1000 ug/L
WI100329-44	Antimony	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Arsenic	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Barium	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Beryllium	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Boron	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Cadmium	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Calcium	10000 ug/L	10 mL	100 mL	1000 ug/L
WI100329-44	Chromium	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Cobalt	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Copper	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Iron	10000 ug/L	10 mL	100 mL	1000 ug/L
WI100329-44	Lead	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Magnesium	10000 ug/L	10 mL	100 mL	1000 ug/L
WI100329-44	Manganese	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Molybdenum	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Nickel	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Phosphorous	5000 ug/L	10 mL	100 mL	500 ug/L
WI100329-44	Potassium	10000 ug/L	10 mL	100 mL	1000 ug/L
WI100329-44	Selenium	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Silica	10698 ug/L	10 mL	100 mL	1069 ug/L
WI100329-44	Silicon	5000 ug/L	10 mL	100 mL	500 ug/L
WI100329-44	Silver	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Sodium	10000 ug/L	10 mL	100 mL	1000 ug/L
WI100329-44	Strontium	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Sulfur	2000 ug/L	10 mL	100 mL	200 ug/L
WI100329-44	Thallium	1000 ug/L	10 mL	100 mL	100 ug/L

Standard Logbook

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
WI100329-44	Tin	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Titanium	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Uranium	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Vanadium	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Zinc	1000 ug/L	10 mL	100 mL	100 ug/L

Serial ID: WI100329-43 **Opened:** 29-MAR-10 **Balance Id :** 216
Name: TRACE ICP 0.5/CCV STD. **Received:** 02-NOV-09 **Pipet Id :** 3581809
Type: Working **Expires:** 30-MAR-10 **Solvent :** 3%HCL and 1%HNO3 -1293083
Employee: Helen Camello
Supplier: GEL
Description: TRACE ICP 0.5/CCV CALIBRATION STD.
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI090421-40	Sodium	1000 ug/mL	5 mL	1000 mL	5000 UG/L
UI091015-42	Silica	2139 mg/L	2.5 mL	1000 mL	5348.25 UG/L
UI091015-42	Silicon	1000 mg/L	2.5 mL	1000 mL	2500 UG/L
UI091102-40	Aluminum	2000 mg/L	2.5 mL	1000 mL	5000 UG/L
UI091102-40	Arsenic	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Barium	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Beryllium	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Boron	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Cadmium	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Calcium	2000 mg/L	2.5 mL	1000 mL	5000 UG/L
UI091102-40	Chromium	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Cobalt	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Copper	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Iron	2000 mg/L	2.5 mL	1000 mL	5000 UG/L
UI091102-40	Lead	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Magnesium	2000 mg/L	2.5 mL	1000 mL	5000 UG/L
UI091102-40	Manganese	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Nickel	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Phosphorous	1000 mg/L	2.5 mL	1000 mL	2500 UG/L
UI091102-40	Potassium	2000 mg/L	2.5 mL	1000 mL	5000 UG/L
UI091102-40	Selenium	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Sodium	2000 mg/L	2.5 mL	1000 mL	5000 UG/L
UI091102-40	Strontium	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Thallium	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Uranium	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Vanadium	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Zinc	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-41	Antimony	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-41	Molybdenum	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-41	Silver	200 mg/L	2.5 mL	1000 mL	500 UG/L

Standard Logbook

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI091102-41	Sulfur	400 mg/L	2.5 mL	1000 mL	1000 UG/L
UI091102-41	Tin	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-41	Titanium	200 mg/L	2.5 mL	1000 mL	500 UG/L

Serial ID: WI100329-44 **Opened:** 29-MAR-10 **Balance Id :** 216
Name: TRACE ICP SCAL 1.0 **Received:** 02-NOV-09 **Pipet Id :** 3581809
Type: Working **Expires:** 30-MAR-10 **Solvent :** 3%HCL and 1 %HNO3-1293083
Employee: Helen Camello
Supplier: o2si
Description: Trace ICP Calibration Standard 1.0ppm
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI091015-42	Silica	2139 mg/L	2.5 mL	500 mL	10698 ug/L
UI091015-42	Silicon	1000 mg/L	2.5 mL	500 mL	5000 ug/L
UI091102-40	Aluminum	2000 mg/L	2.5 mL	500 mL	10000 ug/L
UI091102-40	Arsenic	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Barium	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Beryllium	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Boron	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Cadmium	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Calcium	2000 mg/L	2.5 mL	500 mL	10000 ug/L
UI091102-40	Chromium	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Cobalt	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Copper	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Iron	2000 mg/L	2.5 mL	500 mL	10000 ug/L
UI091102-40	Lead	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Magnesium	2000 mg/L	2.5 mL	500 mL	10000 ug/L
UI091102-40	Manganese	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Nickel	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Phosphorous	1000 mg/L	2.5 mL	500 mL	5000 ug/L
UI091102-40	Potassium	2000 mg/L	2.5 mL	500 mL	10000 ug/L
UI091102-40	Selenium	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Sodium	2000 mg/L	2.5 mL	500 mL	10000 ug/L
UI091102-40	Strontium	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Thallium	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Uranium	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Vanadium	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Zinc	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-41	Antimony	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-41	Molybdenum	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-41	Silver	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-41	Sulfur	400 mg/L	2.5 mL	500 mL	2000 ug/L
UI091102-41	Tin	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-41	Titanium	200 mg/L	2.5 mL	500 mL	1000 ug/L

Standard Logbook

Serial ID: WI100329-45 **Opened:** 29-MAR-10 **Balance Id :** 216
Name: TRACE ICP S-10 STD **Received:** 22-APR-09 **Pipet Id :** 3581809
Type: Working **Expires:** 30-MAR-10 **Solvent :** 3%HCL and 1%HNO3 -1293083
Employee: Helen Camello
Supplier: GEL
Description: TRACE ICP S-10 CALIBRATION STD.
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI090421-40	Sodium	1000 ug/mL	10 mL	500 mL	20000 UG/L
UI090422-40	Aluminum	5000 mg/L	5 mL	500 mL	50000 UG/L
UI090422-40	Calcium	5000 mg/L	5 mL	500 mL	50000 UG/L
UI090422-40	Iron	2000 mg/L	5 mL	500 mL	20000 UG/L
UI090422-40	Magnesium	5000 mg/L	5 mL	500 mL	50000 UG/L

Serial ID: WI100329-46 **Opened:** 29-MAR-10 **Balance Id :** 216
Name: ICP TRACE ICV **Received:** 25-SEP-09 **Pipet Id :** 3581809
Type: Working **Expires:** 30-MAR-10 **Solvent :** 3%HCL AND 1%HNO3-1293083
Employee: Helen Camello
Supplier: GEL
Description: Initial Calibration Verification ICP Trace Metals
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI090925-40	Aluminum	1000 mg/L	2.5 mL	500 mL	5000 ug/L
UI090925-40	Arsenic	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-40	Barium	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-40	Boron	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-40	Cadmium	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-40	Calcium	1000 mg/L	2.5 mL	500 mL	5000 ug/L
UI090925-40	Chromium	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-40	Cobalt	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-40	Copper	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-40	Iron	1000 mg/L	2.5 mL	500 mL	5000 ug/L
UI090925-40	Lead	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-40	Phosphorous	500 mg/L	2.5 mL	500 mL	2500 ug/L
UI090925-40	Potassium	500 mg/L	2.5 mL	500 mL	2500 ug/L
UI090925-40	Selenium	500 mg/L	2.5 mL	500 mL	2500 ug/L
UI090925-40	Sodium	500 mg/L	2.5 mL	500 mL	2500 ug/L
UI090925-40	Strontium	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-41	Antimony	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-41	Beryllium	50 mg/L	2.5 mL	500 mL	250 ug/L
UI090925-41	Magnesium	1000 mg/L	2.5 mL	500 mL	5000 ug/L
UI090925-41	Manganese	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-41	Molybdenum	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-41	Nickel	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-41	Silver	50 mg/L	2.5 mL	500 mL	250 ug/L

Standard Logbook

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI090925-41	Sulfur	500 mg/L	2.5 mL	500 mL	2500 ug/L
UI090925-41	Thallium	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-41	Tin	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-41	Titanium	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-41	Uranium	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-41	Vanadium	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-41	Zinc	100 mg/L	2.5 mL	500 mL	500 ug/L
UI091102-42	Silica	2139 mg/L	2.5 mL	500 mL	10695 ug/L
UI091102-42	Silicon	1000 mg/L	2.5 mL	500 mL	5000 ug/L

Serial ID: WI100329-47 **Opened:** 29-MAR-10 **Balance Id :** 216
Name: PQL Working Standard **Received:** 30-JUN-09 **Pipet Id :** 3581809
Type: Working **Expires:** 30-MAR-10 **Solvent :** 3%HCL &1%HNO3-1293083
Employee: Helen Camello
Supplier: 02si
Description: PQL Working Standard
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI090701-40	Aluminum	100 mg/L	2 mL	1000 mL	200 ug/L
UI090701-40	Antimony	5 mg/L	2 mL	1000 mL	10 ug/L
UI090701-40	Arsenic	15 mg/L	2 mL	1000 mL	15 ug/L
UI090701-40	Barium	2.5 mg/L	2 mL	1000 mL	5 ug/L
UI090701-40	Beryllium	2.5 mg/L	2 mL	1000 mL	5 ug/L
UI090701-40	Boron	25 mg/L	2 mL	1000 mL	50 ug/L
UI090701-40	Cadmium	2.5 mg/L	2 mL	1000 mL	5 ug/L
UI090701-40	Calcium	100 mg/L	2 mL	1000 mL	100 ug/L
UI090701-40	Chromium	2.5 mg/L	2 mL	1000 mL	5 ug/L
UI090701-40	Cobalt	2.5 mg/L	2 mL	1000 mL	5 ug/L
UI090701-40	Copper	5 mg/L	2 mL	1000 mL	10 ug/L
UI090701-40	Iron	50 mg/L	2 mL	1000 mL	100 ug/L
UI090701-40	Lead	5 mg/L	2 mL	1000 mL	10 ug/L
UI090701-40	Magnesium	150 mg/L	2 mL	1000 mL	300 ug/L
UI090701-40	Manganese	5 mg/L	2 mL	1000 mL	10 ug/L
UI090701-40	Molybdenum	5 mg/L	2 mL	1000 mL	10 ug/L
UI090701-40	Nickel	2.5 mg/L	2 mL	1000 mL	5 ug/L
UI090701-40	Phosphorous	75 mg/L	2 mL	1000 mL	150 ug/L
UI090701-40	Potassium	75 mg/L	2 mL	1000 mL	150 ug/L
UI090701-40	Selenium	15 mg/L	2 mL	1000 mL	15 ug/L
UI090701-40	Silicon	50 mg/L	2 mL	1000 mL	100 ug/L
UI090701-40	Silver	2.5 mg/L	2 mL	1000 mL	5 ug/L
UI090701-40	Sodium	150 mg/L	2 mL	1000 mL	150 ug/L
UI090701-40	Strontium	2.5 mg/L	2 mL	1000 mL	5 ug/L
UI090701-40	Sulfur	50 mg/L	2 mL	1000 mL	100 ug/L
UI090701-40	Thallium	10 mg/L	2 mL	1000 mL	20 ug/L

Standard Logbook

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI090701-40	Tin	5 mg/L	2 mL	1000 mL	10 ug/L
UI090701-40	Titanium	2.5 mg/L	2 mL	1000 mL	5 ug/L
UI090701-40	Uranium	25 mg/L	2 mL	1000 mL	50 ug/L
UI090701-40	Vanadium	2.5 mg/L	2 mL	1000 mL	5 ug/L
UI090701-40	Zinc	5 mg/L	2 mL	1000 mL	10 ug/L

Serial ID: WMS100411-04 Opened: 11-APR-10 Amount : 50 mL
 Name: ICPMS Cal Standard 100 Received: 11-APR-10 Balance Id : 4025216
 Type: Working Expires: 12-APR-10 Pipet Id : 3541598
 Employee: Paul Boyd Solvent : 2%HNO3/1%HCl-1296562
 Supplier: GEL
 Description: ICPMS Calibration Standard (100 ppb)
 Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI090612-02	Tungsten	10 mg/L	.5 mL	50 mL	100 ug/L
UMS100226-01	Arsenic	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Barium	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Beryllium	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Boron	20 mg/L	.5 mL	50 mL	200 ug/l
UMS100226-01	Cadmium	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Chromium	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Cobalt	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Copper	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Lead	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Lithium	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Manganese	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Nickel	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Selenium	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Silver	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Strontium	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Thallium	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Thorium	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Uranium	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Vanadium	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Zinc	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-02	Aluminum	1000 mg/L	.5 mL	50 mL	10000 ug/l
UMS100226-02	Calcium	1000 mg/L	.5 mL	50 mL	10000 ug/l
UMS100226-02	Iron	1000 mg/L	.5 mL	50 mL	10000 ug/l
UMS100226-02	Magnesium	1000 mg/L	.5 mL	50 mL	10000 ug/l
UMS100226-02	Phosphorous	1000 mg/L	.5 mL	50 mL	10000 ug/l
UMS100226-02	Potassium	1000 mg/L	.5 mL	50 mL	10000 ug/l
UMS100226-02	Sodium	1000 mg/L	.5 mL	50 mL	10000 ug/l
UMS100226-03	Antimony	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-03	Molybdenum	10 mg/L	.5 mL	50 mL	100 ug/l

Standard Logbook

Parent Material	Analyte	Parent Conc.	Alliquot	Final Vol.	Final Conc.
UMS100226-03	Tin	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-03	Titanium	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-03	Zirconium	10 mg/L	.5 mL	50 mL	100 ug/l

Serial ID: WMS100411-04A **Opened:** 11-APR-10 **Balance Id :** 4025216
Name: ICPMS Cal Standard 10 **Received:** 11-APR-10 **Pipet Id :** 3541598
Type: Working **Expires:** 12-APR-10 **Solvent :** 2%HNO3/1%HCl - 1296562
Employee: Paul Boyd
Supplier: GEL
Description: ICPMS Calibration Standard (10 ppb)
Comments: None

Parent Material	Analyte	Parent Conc.	Alliquot	Final Vol.	Final Conc.
WMS100411-04	Aluminum	10000 ug/l	5 mL	50 mL	1000 ug/l
WMS100411-04	Antimony	100 ug/l	5 mL	50 mL	10 ug/l
WMS100411-04	Arsenic	100 ug/l	5 mL	50 mL	10 ug/l
WMS100411-04	Barium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100411-04	Beryllium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100411-04	Boron	200 ug/l	5 mL	50 mL	20 ug/l
WMS100411-04	Cadmium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100411-04	Calcium	10000 ug/l	5 mL	50 mL	1000 ug/l
WMS100411-04	Chromium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100411-04	Cobalt	100 ug/l	5 mL	50 mL	10 ug/l
WMS100411-04	Copper	100 ug/l	5 mL	50 mL	10 ug/l
WMS100411-04	Iron	10000 ug/l	5 mL	50 mL	1000 ug/l
WMS100411-04	Lead	100 ug/l	5 mL	50 mL	10 ug/l
WMS100411-04	Lithium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100411-04	Magnesium	10000 ug/l	5 mL	50 mL	1000 ug/l
WMS100411-04	Manganese	100 ug/l	5 mL	50 mL	10 ug/l
WMS100411-04	Molybdenum	100 ug/l	5 mL	50 mL	10 ug/l
WMS100411-04	Nickel	100 ug/l	5 mL	50 mL	10 ug/l
WMS100411-04	Phosphorous	10000 ug/l	5 mL	50 mL	1000 ug/l
WMS100411-04	Potassium	10000 ug/l	5 mL	50 mL	1000 ug/l
WMS100411-04	Selenium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100411-04	Silver	100 ug/l	5 mL	50 mL	10 ug/l
WMS100411-04	Sodium	10000 ug/l	5 mL	50 mL	1000 ug/l
WMS100411-04	Strontium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100411-04	Thallium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100411-04	Thorium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100411-04	Tin	100 ug/l	5 mL	50 mL	10 ug/l
WMS100411-04	Titanium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100411-04	Tungsten	100 ug/L	5 mL	50 mL	10 ug/L
WMS100411-04	Uranium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100411-04	Vanadium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100411-04	Zinc	100 ug/l	5 mL	50 mL	10 ug/l

Standard Logbook

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
WMS100411-04	Zirconium	100 ug/l	5 mL	50 mL	10 ug/l

Serial ID: WMS100411-05 **Opened:** 11-APR-10 **Balance Id :** 40245216
Name: ICPMS ICV **Received:** 11-APR-10 **Pipet Id :** 3541598
Type: Working **Expires:** 12-APR-10 **Solvent :** 2%HNO3/1%HCl - 1296562
Employee: Paul Boyd
Supplier: GEL
Description: ICPMS ICV
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI100317-06	Aluminum	2020 mg/L	.125 mL	50 mL	5050 ug/L
UI100317-06	Calcium	2000 mg/L	.125 mL	50 mL	5000 ug/L
UI100317-06	Iron	2000 mg/L	.125 mL	50 mL	5000 ug/L
UI100317-06	Magnesium	2000 mg/L	.125 mL	50 mL	5000 ug/L
UI100317-06	Phosphorous	2000 mg/L	.125 mL	50 mL	5000 ug/L
UI100317-06	Potassium	2000 mg/L	.125 mL	50 mL	5000 ug/L
UI100317-06	Sodium	2000 mg/L	.125 mL	50 mL	5000 ug/L
UI100317-07	Arsenic	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Barium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Beryllium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Boron	40 mg/L	.125 mL	50 mL	100 ug/L
UI100317-07	Cadmium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Chromium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Cobalt	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Copper	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Lead	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Lithium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Manganese	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Nickel	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Selenium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Strontium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Thallium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Thorium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Uranium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Vanadium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Zinc	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-08	Antimony	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-08	Molybdenum	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-08	Silver	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-08	Tin	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-08	Titanium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-08	Tungsten	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-08	Zirconium	20 mg/L	.125 mL	50 mL	50 ug/L

Standard Logbook

Serial ID: WMS100411-06 **Opened:** 11-APR-10 **Balance Id :** 40245216
Name: ICPMS CRDL **Received:** 11-APR-10 **Pipet Id :** 3820544
Type: Working **Expires:** 12-APR-10 **Solvent :** 2%HNO3/1%HCl - 1296562
Employee: Paul Boyd
Supplier: GEL
Description: ICPMS CRDL
Comments: None

Parent Material	Analyte	Parent Conc.	Allquot	Final Vol.	Final Conc.
UI090701-09	Aluminum	15 mg/L	.05 mL	50 mL	15 ug/L
UI090701-09	Arsenic	5 mg/L	.05 mL	50 mL	5 ug/L
UI090701-09	Barium	2 mg/L	.05 mL	50 mL	2 ug/L
UI090701-09	Beryllium	.5 mg/L	.05 mL	50 mL	.5 ug/L
UI090701-09	Boron	15 mg/L	.05 mL	50 mL	15 ug/L
UI090701-09	Cadmium	1 mg/L	.05 mL	50 mL	1 ug/L
UI090701-09	Calcium	100 mg/L	.05 mL	50 mL	100 ug/L
UI090701-09	Chromium	3 mg/L	.05 mL	50 mL	3 ug/L
UI090701-09	Cobalt	1 mg/L	.05 mL	50 mL	1 ug/L
UI090701-09	Copper	1 mg/L	.05 mL	50 mL	1 ug/L
UI090701-09	Iron	25 mg/L	.05 mL	50 mL	25 ug/L
UI090701-09	Lead	2 mg/L	.05 mL	50 mL	2 ug/L
UI090701-09	Lithium	10 mg/L	.05 mL	50 mL	10 ug/L
UI090701-09	Magnesium	15 mg/L	.05 mL	50 mL	15 ug/L
UI090701-09	Manganese	5 mg/L	.05 mL	50 mL	5 ug/L
UI090701-09	Nickel	2 mg/L	.05 mL	50 mL	2 ug/L
UI090701-09	Phosphorous	50 mg/L	.05 mL	50 mL	50 ug/L
UI090701-09	Potassium	300 mg/L	.05 mL	50 mL	300 ug/L
UI090701-09	Selenium	5 mg/L	.05 mL	50 mL	5 ug/L
UI090701-09	Sodium	250 mg/L	.05 mL	50 mL	250 ug/L
UI090701-09	Strontium	10 mg/L	.05 mL	50 mL	10 ug/L
UI090701-09	Thallium	1 mg/L	.05 mL	50 mL	1 ug/L
UI090701-09	Thorium	1 mg/L	.05 mL	50 mL	1 ug/L
UI090701-09	Uranium	.2 mg/L	.05 mL	50 mL	.2 ug/L
UI090701-09	Vanadium	10 mg/L	.05 mL	50 mL	10 ug/L
UI090701-09	Zinc	10 mg/L	.05 mL	50 mL	10 ug/L
UI090701-10	Antimony	2 mg/L	.05 mL	50 mL	2 ug/L
UI090701-10	Molybdenum	.5 mg/L	.05 mL	50 mL	.5 ug/L
UI090701-10	Silver	1 mg/L	.05 mL	50 mL	1 ug/L
UI090701-10	Tin	2 mg/L	.05 mL	50 mL	5 ug/L
UI090701-10	Titanium	10 mg/L	.05 mL	50 mL	10 ug/L
UI090701-10	Tungsten	5 mg/L	.05 mL	50 mL	5 ug/L
UI090701-10	Zirconium	2 mg/L	.05 mL	50 mL	2 ug/L

Standard Logbook

Serial ID: WMS100411-07 **Opened:** 11-APR-10 **Balance Id :** 40245216
Name: ICPMS ICSA **Received:** 11-APR-10 **Lot Number :** 1010773
Type: Working **Expires:** 12-APR-10 **Pipet Id :** 3541598
Employee: Paul Boyd **Solvent :** 2%HNO3/1%HCl - 1296562
Supplier: GEL
Description: ICPMS ICSA
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI100318-11	Aluminum	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Calcium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Chloride	10000 mg/L	5 mL	50 mL	1000000 ug/L
UI100318-11	Iron	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Magnesium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Molybdenum	20 mg/L	5 mL	50 mL	2000 ug/L
UI100318-11	Phosphorous	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Potassium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Sodium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Sulfur	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Titanium	20 mg/L	5 mL	50 mL	2000 ug/L

Serial ID: WMS100411-08 **Opened:** 11-APR-10 **Balance Id :** 40245216
Name: ICPMS ICSAB **Received:** 11-APR-10 **Pipet Id :** 1758088
Type: Working **Expires:** 12-APR-10 **Solvent :** 2%HNO3/1%HCl - 1296562
Employee: Paul Boyd
Supplier: GEL
Description: ICPMS ICSAB
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI100318-11	Aluminum	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Calcium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Chloride	10000 mg/L	5 mL	50 mL	1000000 ug/L
UI100318-11	Iron	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Magnesium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Molybdenum	20 mg/L	5 mL	50 mL	2000 ug/L
UI100318-11	Phosphorous	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Potassium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Sodium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Sulfur	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Titanium	20 mg/L	5 mL	50 mL	2000 ug/L
UI100405-12	Arsenic	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-12	Barium	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-12	Beryllium	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-12	Boron	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-12	Cadmium	2 mg/L	.5 mL	50 mL	20.2 ug/L
UI100405-12	Chromium	2 mg/L	.5 mL	50 mL	22.2 ug/L

Standard Logbook

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI100405-12	Cobalt	2 mg/L	.5 mL	50 mL	20.4 ug/L
UI100405-12	Copper	2 mg/L	.5 mL	50 mL	23.4 ug/L
UI100405-12	Lead	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-12	Lithium	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-12	Manganese	2 mg/L	.5 mL	50 mL	22.7 ug/L
UI100405-12	Nickel	2 mg/L	.5 mL	50 mL	22.4 ug/L
UI100405-12	Selenium	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-12	Strontium	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-12	Thallium	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-12	Thorium	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-12	Uranium	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-12	Vanadium	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-12	Zinc	2 mg/L	.5 mL	50 mL	27 ug/L
UI100405-13	Antimony	2 mg/L	.5 mL	50 mL	20.5 ug/L
UI100405-13	Silver	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-13	Tin	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-13	Tungsten	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-13	Zirconium	2 mg/L	.5 mL	50 mL	20 ug/L

Serial ID: WMS100411-70 **Opened:** 11-APR-10 **Balance Id :** 40245216
Name: ICPMS LINEAR RANGE ST **Received:** 11-APR-10 **Pipet Id :** 1758088
Type: Working **Expires:** 12-APR-10 **Solvent :** 2%HNO3/1%HCl - 1296562
Employee: Paul Boyd
Supplier: 02SI
Description: ICPMS LINEAR RANGE STANDARD
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI100405-60	Aluminum	5000 mg/L	.5 mL	50 mL	50000 ug/L
UI100405-60	Arsenic	100 mg/L	.5 mL	50 mL	1000 ug/L
UI100405-60	Barium	250 mg/L	.5 mL	50 mL	2500 ug/L
UI100405-60	Beryllium	100 mg/L	.5 mL	50 mL	1000 ug/L
UI100405-60	Cadmium	100 mg/L	.5 mL	50 mL	1000 ug/L
UI100405-60	Calcium	5000 mg/L	.5 mL	50 mL	50000 ug/L
UI100405-60	Chromium	100 mg/L	.5 mL	50 mL	1000 ug/L
UI100405-60	Cobalt	100 mg/L	.5 mL	50 mL	1000 ug/L
UI100405-60	Copper	100 mg/L	.5 mL	50 mL	1000 ug/L
UI100405-60	Iron	5000 mg/L	.5 mL	50 mL	50000 ug/L
UI100405-60	Lead	500 mg/L	.5 mL	50 mL	5000 ug/L
UI100405-60	Lithium	100 mg/L	.5 mL	50 mL	1000 ug/L
UI100405-60	Magnesium	5000 mg/L	.5 mL	50 mL	50000 ug/L
UI100405-60	Manganese	100 mg/L	.5 mL	50 mL	1000 ug/L
UI100405-60	Nickel	100 mg/L	.5 mL	50 mL	1000 ug/L
UI100405-60	Phosphorous	2500 mg/L	.5 mL	50 mL	25000 ug/L
UI100405-60	Potassium	5000 mg/L	.5 mL	50 mL	50000 ug/L

Standard Logbook

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI100405-60	Selenium	50 mg/L	.5 mL	50 mL	500 ug/L
UI100405-60	Sodium	5000 mg/L	.5 mL	50 mL	50000 ug/L
UI100405-60	Strontium	100 mg/L	.5 mL	50 mL	1000 ug/L
UI100405-60	Thallium	50 mg/L	.5 mL	50 mL	500 ug/L
UI100405-60	Thorium	250 mg/L	.5 mL	50 mL	2500 ug/L
UI100405-60	Uranium	500 mg/L	.5 mL	50 mL	5000 ug/L
UI100405-60	Vanadium	100 mg/L	.5 mL	50 mL	1000 ug/L
UI100405-60	Zinc	250 mg/L	.5 mL	50 mL	2500 ug/L
UI100405-61	Antimony	25 mg/L	.5 mL	50 mL	250 ug/L
UI100405-61	Molybdenum	100 mg/L	.5 mL	50 mL	1000 ug/L
UI100405-61	Silver	25 mg/L	.5 mL	50 mL	250 ug/L
UI100405-61	Tin	100 mg/L	.5 mL	50 mL	1000 ug/L
UI100405-61	Tungsten	100 mg/L	.5 mL	50 mL	1000 ug/L
UI100405-61	Zirconium	50 mg/L	.5 mL	50 mL	500 ug/L

Serial ID: WMS100413-04 **Opened:** 13-APR-10 **Amount :** 50 mL
Name: ICPMS Cal Standard 100 **Received:** 13-APR-10 **Balance Id :** 4025216
Type: Working **Expires:** 14-APR-10 **Pipet Id :** 3541598
Employee: Paul Boyd **Solvent :** 2%HNO3/1%HCl-1300209
Supplier: GEL
Description: ICPMS Calibration Standard (100 ppb)
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI090612-02	Tungsten	10 mg/L	.5 mL	50 mL	100 ug/L
UMS100226-01	Arsenic	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Barium	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Beryllium	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Boron	20 mg/L	.5 mL	50 mL	200 ug/l
UMS100226-01	Cadmium	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Chromium	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Cobalt	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Copper	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Lead	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Lithium	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Manganese	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Nickel	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Selenium	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Silver	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Strontium	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Thallium	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Thorium	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Uranium	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Vanadium	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-01	Zinc	10 mg/L	.5 mL	50 mL	100 ug/l

Standard Logbook

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UMS100226-02	Aluminum	1000 mg/L	.5 mL	50 mL	10000 ug/l
UMS100226-02	Calcium	1000 mg/L	.5 mL	50 mL	10000 ug/l
UMS100226-02	Iron	1000 mg/L	.5 mL	50 mL	10000 ug/l
UMS100226-02	Magnesium	1000 mg/L	.5 mL	50 mL	10000 ug/l
UMS100226-02	Phosphorous	1000 mg/L	.5 mL	50 mL	10000 ug/l
UMS100226-02	Potassium	1000 mg/L	.5 mL	50 mL	10000 ug/l
UMS100226-02	Sodium	1000 mg/L	.5 mL	50 mL	10000 ug/l
UMS100226-03	Antimony	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-03	Molybdenum	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-03	Tin	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-03	Titanium	10 mg/L	.5 mL	50 mL	100 ug/l
UMS100226-03	Zirconium	10 mg/L	.5 mL	50 mL	100 ug/l

Serial ID: WMS100413-04A **Opened:** 13-APR-10 **Balance Id :** 4025216
Name: ICPMS Cal Standard 10 **Received:** 13-APR-10 **Pipet Id :** 3541598
Type: Working **Expires:** 14-APR-10 **Solvent :** 2%HNO3/1%HCl - 1300209
Employee: Paul Boyd
Supplier: GEL
Description: ICPMS Calibration Standard (10 ppb)
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
WMS100413-04	Aluminum	10000 ug/l	5 mL	50 mL	1000 ug/l
WMS100413-04	Antimony	100 ug/l	5 mL	50 mL	10 ug/l
WMS100413-04	Arsenic	100 ug/l	5 mL	50 mL	10 ug/l
WMS100413-04	Barium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100413-04	Beryllium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100413-04	Boron	200 ug/l	5 mL	50 mL	20 ug/l
WMS100413-04	Cadmium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100413-04	Calcium	10000 ug/l	5 mL	50 mL	1000 ug/l
WMS100413-04	Chromium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100413-04	Cobalt	100 ug/l	5 mL	50 mL	10 ug/l
WMS100413-04	Copper	100 ug/l	5 mL	50 mL	10 ug/l
WMS100413-04	Iron	10000 ug/l	5 mL	50 mL	1000 ug/l
WMS100413-04	Lead	100 ug/l	5 mL	50 mL	10 ug/l
WMS100413-04	Lithium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100413-04	Magnesium	10000 ug/l	5 mL	50 mL	1000 ug/l
WMS100413-04	Manganese	100 ug/l	5 mL	50 mL	10 ug/l
WMS100413-04	Molybdenum	100 ug/l	5 mL	50 mL	10 ug/l
WMS100413-04	Nickel	100 ug/l	5 mL	50 mL	10 ug/l
WMS100413-04	Phosphorous	10000 ug/l	5 mL	50 mL	1000 ug/l
WMS100413-04	Potassium	10000 ug/l	5 mL	50 mL	1000 ug/l
WMS100413-04	Selenium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100413-04	Silver	100 ug/l	5 mL	50 mL	10 ug/l
WMS100413-04	Sodium	10000 ug/l	5 mL	50 mL	1000 ug/l

Standard Logbook

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
WMS100413-04	Strontium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100413-04	Thallium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100413-04	Thorium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100413-04	Tin	100 ug/l	5 mL	50 mL	10 ug/l
WMS100413-04	Titanium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100413-04	Tungsten	100 ug/L	5 mL	50 mL	10 ug/L
WMS100413-04	Uranium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100413-04	Vanadium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100413-04	Zinc	100 ug/l	5 mL	50 mL	10 ug/l
WMS100413-04	Zirconium	100 ug/l	5 mL	50 mL	10 ug/l

Serial ID: WMS100413-05 **Opened:** 13-APR-10 **Balance Id :** 40245216
Name: ICPMS ICV **Received:** 13-APR-10 **Pipet Id :** 3541598
Type: Working **Expires:** 14-APR-10 **Solvent :** 2%HNO3/1%HCl - 1300209
Employee: Paul Boyd
Supplier: GEL
Description: ICPMS ICV
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI100317-06	Aluminum	2020 mg/L	.125 mL	50 mL	5050 ug/L
UI100317-06	Calcium	2000 mg/L	.125 mL	50 mL	5000 ug/L
UI100317-06	Iron	2000 mg/L	.125 mL	50 mL	5000 ug/L
UI100317-06	Magnesium	2000 mg/L	.125 mL	50 mL	5000 ug/L
UI100317-06	Phosphorous	2000 mg/L	.125 mL	50 mL	5000 ug/L
UI100317-06	Potassium	2000 mg/L	.125 mL	50 mL	5000 ug/L
UI100317-06	Sodium	2000 mg/L	.125 mL	50 mL	5000 ug/L
UI100317-07	Arsenic	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Barium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Beryllium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Boron	40 mg/L	.125 mL	50 mL	100 ug/L
UI100317-07	Cadmium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Chromium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Cobalt	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Copper	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Lead	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Lithium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Manganese	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Nickel	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Selenium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Strontium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Thallium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Thorium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Uranium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Vanadium	20 mg/L	.125 mL	50 mL	50 ug/L

Standard Logbook

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI100317-07	Zinc	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-08	Antimony	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-08	Molybdenum	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-08	Silver	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-08	Tin	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-08	Titanium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-08	Tungsten	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-08	Zirconium	20 mg/L	.125 mL	50 mL	50 ug/L

Serial ID: WMS100413-06 **Opened:** 13-APR-10 **Balance Id :** 40245216
Name: ICPMS CRDL **Received:** 13-APR-10 **Pipet Id :** 3820544
Type: Working **Expires:** 14-APR-10 **Solvent :** 2%HNO3/1%HCl - 1300209
Employee: Paul Boyd
Supplier: GEL
Description: ICPMS CRDL
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI090701-09	Aluminum	15 mg/L	.05 mL	50 mL	15 ug/L
UI090701-09	Arsenic	5 mg/L	.05 mL	50 mL	5 ug/L
UI090701-09	Barium	2 mg/L	.05 mL	50 mL	2 ug/L
UI090701-09	Beryllium	.5 mg/L	.05 mL	50 mL	.5 ug/L
UI090701-09	Boron	15 mg/L	.05 mL	50 mL	15 ug/L
UI090701-09	Cadmium	1 mg/L	.05 mL	50 mL	1 ug/L
UI090701-09	Calcium	100 mg/L	.05 mL	50 mL	100 ug/L
UI090701-09	Chromium	3 mg/L	.05 mL	50 mL	3 ug/L
UI090701-09	Cobalt	1 mg/L	.05 mL	50 mL	1 ug/L
UI090701-09	Copper	1 mg/L	.05 mL	50 mL	1 ug/L
UI090701-09	Iron	25 mg/L	.05 mL	50 mL	25 ug/L
UI090701-09	Lead	2 mg/L	.05 mL	50 mL	2 ug/L
UI090701-09	Lithium	10 mg/L	.05 mL	50 mL	10 ug/L
UI090701-09	Magnesium	15 mg/L	.05 mL	50 mL	15 ug/L
UI090701-09	Manganese	5 mg/L	.05 mL	50 mL	5 ug/L
UI090701-09	Nickel	2 mg/L	.05 mL	50 mL	2 ug/L
UI090701-09	Phosphorous	50 mg/L	.05 mL	50 mL	50 ug/L
UI090701-09	Potassium	300 mg/L	.05 mL	50 mL	300 ug/L
UI090701-09	Selenium	5 mg/L	.05 mL	50 mL	5 ug/L
UI090701-09	Sodium	250 mg/L	.05 mL	50 mL	250 ug/L
UI090701-09	Strontium	10 mg/L	.05 mL	50 mL	10 ug/L
UI090701-09	Thallium	1 mg/L	.05 mL	50 mL	1 ug/L
UI090701-09	Thorium	1 mg/L	.05 mL	50 mL	1 ug/L
UI090701-09	Uranium	.2 mg/L	.05 mL	50 mL	.2 ug/L
UI090701-09	Vanadium	10 mg/L	.05 mL	50 mL	10 ug/L
UI090701-09	Zinc	10 mg/L	.05 mL	50 mL	10 ug/L
UI090701-10	Antimony	2 mg/L	.05 mL	50 mL	2 ug/L

Standard Logbook

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI090701-10	Molybdenum	.5 mg/L	.05 mL	50 mL	.5 ug/L
UI090701-10	Silver	1 mg/L	.05 mL	50 mL	1 ug/L
UI090701-10	Tin	2 mg/L	.05 mL	50 mL	5 ug/L
UI090701-10	Titanium	10 mg/L	.05 mL	50 mL	10 ug/L
UI090701-10	Tungsten	5 mg/L	.05 mL	50 mL	5 ug/L
UI090701-10	Zirconium	2 mg/L	.05 mL	50 mL	2 ug/L

Serial ID: WMS100413-07 **Opened:** 13-APR-10 **Balance Id :** 40245216
Name: ICPMS ICSA **Received:** 13-APR-10 **Lot Number :** 1010773
Type: Working **Expires:** 14-APR-10 **Pipet Id :** 3541598
Employee: Paul Boyd **Solvent :** 2%HNO3/1%HCl - 1300209
Supplier: GEL
Description: ICPMS ICSA
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI100318-11	Aluminum	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Calcium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Chloride	10000 mg/L	5 mL	50 mL	1000000 ug/L
UI100318-11	Iron	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Magnesium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Molybdenum	20 mg/L	5 mL	50 mL	2000 ug/L
UI100318-11	Phosphorous	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Potassium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Sodium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Sulfur	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Titanium	20 mg/L	5 mL	50 mL	2000 ug/L

Serial ID: WMS100413-08 **Opened:** 13-APR-10 **Balance Id :** 40245216
Name: ICPMS ICSAB **Received:** 13-APR-10 **Pipet Id :** 1758088
Type: Working **Expires:** 14-APR-10 **Solvent :** 2%HNO3/1%HCl - 1300209
Employee: Paul Boyd
Supplier: GEL
Description: ICPMS ICSAB
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI100318-11	Aluminum	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Calcium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Chloride	10000 mg/L	5 mL	50 mL	1000000 ug/L
UI100318-11	Iron	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Magnesium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Molybdenum	20 mg/L	5 mL	50 mL	2000 ug/L
UI100318-11	Phosphorous	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Potassium	1000 mg/L	5 mL	50 mL	100000 ug/L

Standard Logbook

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI100318-11	Sodium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Sulfur	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Titanium	20 mg/L	5 mL	50 mL	2000 ug/L
UI100405-12	Arsenic	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-12	Barium	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-12	Beryllium	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-12	Boron	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-12	Cadmium	2 mg/L	.5 mL	50 mL	20.2 ug/L
UI100405-12	Chromium	2 mg/L	.5 mL	50 mL	22.2 ug/L
UI100405-12	Cobalt	2 mg/L	.5 mL	50 mL	20.4 ug/L
UI100405-12	Copper	2 mg/L	.5 mL	50 mL	23.4 ug/L
UI100405-12	Lead	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-12	Lithium	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-12	Manganese	2 mg/L	.5 mL	50 mL	22.7 ug/L
UI100405-12	Nickel	2 mg/L	.5 mL	50 mL	22.4 ug/L
UI100405-12	Selenium	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-12	Strontium	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-12	Thallium	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-12	Thorium	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-12	Uranium	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-12	Vanadium	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-12	Zinc	2 mg/L	.5 mL	50 mL	27 ug/L
UI100405-13	Antimony	2 mg/L	.5 mL	50 mL	20.5 ug/L
UI100405-13	Silver	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-13	Tin	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-13	Tungsten	2 mg/L	.5 mL	50 mL	20 ug/L
UI100405-13	Zirconium	2 mg/L	.5 mL	50 mL	20 ug/L

Serial ID: 1156689-A **Opened:** 20-JUL-09 **Lot Number :** 41226920
Name: B-KMnO4(VWR)-MER **Received:** 20-JUL-09
Type: Reagent/Solvent **Expires:** 20-JUL-10
Employee: Tara Griffin **Verified:** 07-AUG-07
Supplier: VWR
Description: Potassium Permanganate
Comments: None

Serial ID: 1176183 **Opened:** 24-AUG-09 **Lot Number :** H20001
Name: B-H2SO4-MER **Received:** 24-AUG-09
Type: Reagent/Solvent **Expires:** 24-AUG-10
Employee: Tara Griffin
Supplier: Mallinckrodt
Description: Sulfuric Acid, Concentrated
Comments: None

Standard Logbook

Serial ID: 1215906 Opened: 06-NOV-09 Lot Number : H44465
Name: B-K2S2O8S-MER Received: 06-NOV-09
Type: Reagent/Solvent Expires: 06-NOV-10
Employee: Tara Griffin
Supplier: J.T BAKER
Description: Potassium Persulfate Concentrate
Comments: None

Serial ID: 1228372-A Opened: 12-NOV-09 Lot Number : 49215936
Name: B-NH2OH.HCl-MER Received: 12-NOV-09
Type: Reagent/Solvent Expires: 12-NOV-10
Employee: Tara Griffin
Supplier: Fisher Scientific
Description: Hydroxylamine Hydrochloride
Comments: None

Serial ID: 1255532-C Opened: 15-JAN-10 Balance Id : BAL-002
Name: B-NaCl.NH2OH.HCl-MER Received: 15-JAN-10
Type: Reagent/Solvent Expires: 15-JUL-10
Employee: Tara Griffin
Supplier: GEL
Description: Hg reducing agent
Comments: None

Parent Material	Analyte	Parent Conc.	Allquot	Final Vol.	Final Conc.
1228372-A	B-NH2OH.HCl-MER	N/A	120 g	1000 mL	N/A

Serial ID: 1274391-1 Opened: 24-FEB-10 Instrument Id : MERCURY
Name: B-HNO3-MER Received: 24-FEB-10 Lot Number : H44025
Type: Reagent/Solvent Expires: 24-FEB-11
Employee: Tara Griffin
Supplier: Mallinckrodt Chemicals
Description: NITRIC ACID
Comments: None

Serial ID: 1274397-C Opened: 24-FEB-10 Balance Id : BAL-002
Name: B-KMnO4-MER Received: 24-FEB-10
Type: Reagent/Solvent Expires: 20-JUL-10
Employee: Tara Griffin
Supplier: GEL
Description: 5% KMnO4 solution
Comments: None

Standard Logbook

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
1156689-A	B-KMnO4(VWR)-MER	Crystals	50 g	1000 mL	3%

Serial ID: 1276435-C Opened: 28-FEB-10 Balance Id : BAL-002
 Name: B-K2S2O8-MER Received: 28-FEB-10
 Type: Reagent/Solvent Expires: 28-AUG-10
 Employee: Tara Griffin
 Supplier: GEL
 Description: 5% Potassium Persulfate
 Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
1215906	B-K2S2O8S-MER	N/A	50 g	1000 mL	N/A

Serial ID: 1277916 Opened: 02-MAR-10 Lot Number : J02039
 Name: I-HCL Received: 02-MAR-10 Preservative_Id : 5 none
 Type: Reagent/Solvent Expires: 02-MAR-11
 Employee: Francena Armstrong
 Supplier: J.T. BAKER
 Description: HYDROCHLORIC ACID
 Comments: None

Serial ID: 1277919 Opened: 02-MAR-10 Lot Number : J 04043 L
 Name: I-HNO3 Received: 02-MAR-10
 Type: Reagent/Solvent Expires: 02-MAR-11
 Employee: Francena Armstrong
 Supplier: BAKER
 Description: Nitric Acid CONC.
 Comments: None

Serial ID: 1291278 Opened: 25-MAR-10 Lot Number : J 08035 L
 Name: I-HNO3 Received: 25-MAR-10
 Type: Reagent/Solvent Expires: 25-MAR-11
 Employee: Anthony Green
 Supplier: BAKER
 Description: Nitric Acid CONC.
 Comments: None

Serial ID: 1293083 Opened: 29-MAR-10 Amount : 20 L
 Name: B-ICP-RINSE SOLN Received: 29-MAR-10 Lot Number : H04040+G34050
 Type: Reagent/Solvent Expires: 04-APR-10 Solvent : 3%HCL+1%HNO3
 Employee: Helen Camello
 Supplier: GEL

Standard Logbook

Description: 3%HCL+1%HNO3 RINSE SOLN.

Comments: None

Serial ID: 1296562 **Opened:** 05-APR-10 **Solvent :** Type I Water

Name: B-2%HNO3/1%HCL-ICPMS **Received:** 05-APR-10

Type: Reagent/Solvent **Expires:** 12-APR-10

Employee: Paul Boyd

Supplier: GEL

Description: 2%HNO3/1%HCL Solution (Type I Water)

Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
1277916	I-HCL	36.5-38.0	90 mL	9 l	N/A
1291278	I-HNO3	69.0-70.0	180 mL	9 l	N/A

Serial ID: 1300209 **Opened:** 12-APR-10 **Solvent :** Type I Water

Name: B-2%HNO3/1%HCL-ICPMS **Received:** 12-APR-10

Type: Reagent/Solvent **Expires:** 19-APR-10

Employee: Paul Boyd

Supplier: GEL

Description: 2%HNO3/1%HCL Solution (Type I Water)

Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
1277916	I-HCL	36.5-38.0	90 mL	9 l	N/A
1291278	I-HNO3	69.0-70.0	180 mL	9 l	N/A

Metals Analysis

Case Narrative

**Metals Fractional Narrative
Los Alamos National Laboratory (LANL)
SDG 10-2093-1**

Sample Analysis

Sample ID	Client ID
248118001	RE36-10-8448
248118002	RE36-10-8456
248118003	RE36-10-8451
248118004	RE36-10-8450
248118005	RE36-10-8449
248118006	RE36-10-8453
248118007	RE36-10-8452
1202056877	Method Blank (MB) ICP
1202056882	Laboratory Control Sample (LCS)
1202056879	248110001(RE15-10-8404L) Serial Dilution (SD)
1202056878	248110001(RE15-10-8404D) Sample Duplicate (DUP)
1202056880	248110001(RE15-10-8404S) Matrix Spike (MS)
1202056881	248110001(RE15-10-8404SD) Matrix Spike Duplicate (MSD)
1202056883	Method Blank (MB) ICP-MS
1202056888	Laboratory Control Sample (LCS)
1202056885	248110001(RE15-10-8404L) Serial Dilution (SD)
1202056884	248110001(RE15-10-8404D) Sample Duplicate (DUP)
1202056886	248110001(RE15-10-8404S) Matrix Spike (MS)
1202056887	248110001(RE15-10-8404SD) Matrix Spike Duplicate (MSD)

1202056179	Method Blank (MB) CVAA
1202056180	Laboratory Control Sample (LCS)
1202056183	248068001(RE11-10-1786L) Serial Dilution (SD)
1202056181	248068001(RE11-10-1786D) Sample Duplicate (DUP)
1202056182	248068001(RE11-10-1786S) Matrix Spike (MS)
1202056184	248068001(RE11-10-1786SD) Matrix Spike Duplicate (MSD)

The samples in this SDG were analyzed on a "dry weight" basis.

Method/Analysis Information

Analytical Batch:	959114, 959116 and 958757
Prep Batch :	959113, 959115 and 958755
Standard Operating Procedures:	GL-MA-E-013 REV# 20, GL-MA-E-009 REV# 19, GL-MA-E-014 REV# 21 and GL-MA-E-010 REV# 23
Analytical Method:	SW846 3050B/6010B, SW846 3050B/6020 and SW846 7471A
Prep Method :	SW846 3050B and SW846 7471A Prep

Preparation/Analytical Method Verification

The SOP stated above has been prepared based on technical research and testing conducted by GEL Laboratories, LLC. and with guidance from the regulatory documents listed in this "Method/Analysis Information" section.

System Configuration

The Metals analysis-ICP was performed on a P E 7300 Optima radial/axial-viewing inductively coupled plasma atomic emission spectrometer. The instrument is equipped with a Burgener nebulizer, cyclonic spray chamber, and yttrium or scandium internal standard. Operating conditions for the ICP are set at a power level of 1500 watts. The instrument has a peristaltic pump flow rate of 1.4L/min, argon gas flows of 15 L/min and 0.2 L/min for the torch and auxiliary gases, and a flow setting of 0.65L/min for the nebulizer.

The Metals analysis - ICPMS was performed on a Perkin Elmer ELAN 9000 inductively coupled plasma mass spectrometer (ICP-MS). The instrument is equipped with a cross-flow nebulizer, quadrupole mass spectrometer, and dual mode electron multiplier detector. Internal standards of scandium, germanium, indium, tantalum, and/or lutetium were utilized to cover the mass spectrum. Operating conditions are set at 1400W power and combined argon pressures of 360+/- 7 kPa for the plasma and auxiliary gases, and 0.85 L/min carrier gas flow, and an initial lens

voltage of 5.2.

The Metals analysis-Mercury was performed on a Perkin-Elmer Flow Injection Mercury System (FIMS-100) automated mercury analyzer. The instrument consists of a cold vapor atomic absorption spectrometer set to detect mercury at a wavelength of 253.7 nm. Sample introduction through the flow injection system is performed via a peristaltic pump at 9 mL/min and nitrogen carrier gas rate of 80 mL/min.

Calibration Information

Instrument Calibration

All initial calibration requirements have been met for this sample delivery group (SDG).

CRDL Requirements

All CRDL standard(s) met the referenced advisory control limits.

ICSA/ICSAB Statement

All interference check samples (ICSA and ICSAB) associated with this SDG met the established acceptance criteria.

Continuing Calibration Blank (CCB) Requirements

All continuing calibration blanks (CCB) bracketing this batch met the established acceptance criteria.

Continuing Calibration Verification (CCV) Requirements

All continuing calibration verifications (CCV) bracketing this SDG met the acceptance criteria.

Quality Control (QC) Information

Method Blank (MB) Statement

The method blank analyzed with this SDG met the acceptance criteria.

Laboratory Control Sample (LCS) Recovery

The laboratory control sample (LCS) met the recommended acceptance criteria for percent recovery (%R) for all elements of interest, with the exception of antimony. Silver and/or antimony did not meet the recovery acceptance criteria for the LCS. Per the DOE-AL statement of work, page forty, silver and antimony are exempt from the re-digestion requirement for LCS failures.

Quality Control (QC) Sample Statement

The following samples were selected as the quality control (QC) samples for this SDG: 248110001 (RE15-10-8404) and 248068001 (RE11-10-1786).

Matrix Spike (MS) Recovery Statement

The percent recoveries (%R) obtained from the MS analyses are evaluated when the sample concentration is less than four times (4X) the spike concentration added. The MS met the recommended quality control acceptance criteria for percent recoveries for all applicable analytes with the exceptions of antimony, potassium and selenium, as indicated by the "N" qualifiers.

Matrix Spike Duplicate (MSD) Recovery Statement

The percent recovery (%R) obtained from the MSD analyses are evaluated when the sample concentration is less than four times (4X) the spike concentration added. The MSD met the recommended quality control acceptance criteria for percent recoveries for all applicable analytes with the exceptions of antimony, potassium and selenium, as indicated by the "N" qualifiers.

MS/MSD Relative Percent Difference (RPD) Statement

The RPD(s) between the MS and MSD met the acceptance limits.

Duplicate Relative Percent Difference (RPD) Statement

The relative percent difference (RPD) obtained from the designated sample duplicate (DUP) is evaluated based on acceptance criteria of 20% when the sample is 5X the contract required detection limit (RL). In cases where either the sample or duplicate value is less than 5X the contract required detection limit (RL), a control of +/-RL is used to evaluate the DUP results. All applicable analytes met these requirements with the exception of manganese, as indicated by the "*" qualifier.

Serial Dilution % Difference Statement

The serial dilution is used to assess matrix suppression or enhancement. Raw element concentrations that are 25X the IDL/MDL for CVAA, 50X the IDL/MDL for ICP, and 100X the IDL/MDL for ICP-MS analyses are applicable for serial dilution assessment. All applicable analytes met the acceptance criteria of less than 10% difference (%D).

Technical Information**Holding Time Specifications**

GEL assigns holding times based on the associated methodology, which assigns the date and time from sample collection of sample receipt. Those holding times expressed in hours are calculated in the AlphaLIMS system. Those holding times expressed as days expire at midnight on the day of expiration. All samples in this SDG met the specified holding time.

Sample Dilutions

Dilutions are performed to minimize matrix interferences resulting from elevated mineral element concentrations present in solid samples and/or to bring over range target analyte concentrations into the linear calibration range of the instrument. The samples in this SDG were diluted the standard 2x for solids on the ICPMS.

Preparation Information

The samples in this SDG were prepared exactly according to the cited SOP.

Miscellaneous Information

Electronic Packaging Comment

This data package was generated using an electronic data processing program referred to as virtual packaging. In an effort to increase quality and efficiency, the laboratory has developed systems to generate all data packages electronically. The following change from traditional packages should be noted:

Analyst/peer reviewer initials and dates are not present on the electronic data files. Presently, all initials and dates are present on the original raw data. These hard copies are temporarily stored in the laboratory. The data validator will always sign and date the case narrative. Data that are not generated electronically, such as hand written pages, will be scanned and inserted into the electronic package.

Data Exception (DER) Documentation

Data exception reports are generated to document any procedural anomalies that may deviate from referenced SOP or contractual documents. The following DERs were generated for this SDG: 810028 and 811428. A copy of each DER is included in the Miscellaneous Data section of this package.

Additional Comments

Additional comments were not required for this SDG.

Certification Statement

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless otherwise noted in the analytical case narrative.

Review Validation:

GEL requires all analytical data to be verified by a qualified data validator. In addition, all data designated for CLP or CLP-like packaging will receive a third level validation upon completion of the data package.

The following data validator verified the information presented in this case narrative:

Reviewer: Kristen Farson Date: 3/31/10

Sample Data Summary

METALS
-1-
INORGANICS ANALYSIS DATA PACKAGE

SDG No: 10-2093-1

CONTRACT: LANL01004

METHOD TYPE: SW846

SAMPLE ID: 248118001

BASIS: Dry Weight

DATE COLLECTED 22-FEB-10

CLIENT ID: RE36-10-8448

LEVEL: Low

DATE RECEIVED 26-FEB-10

MATRIX: SOIL

%SOLIDS: 97.3

CAS No.	Analyte	Result	Units	Qual	MDL	PQL	CRDL	DF	M*	Analyst	Run Date	Analytical Run	Analytical Batch
7429-90-5	Aluminum	1730000	ug/Kg		6900	20300	20300	1	P	HSC	03/29/10 23:24	032910C-1	959114
7440-36-0	Antimony	1020	ug/Kg	U	335	1020	1020	1	P	HSC	03/29/10 23:24	032910C-1	959114
7440-38-2	Arsenic	0.665	mg/kg	J	0.194	0.969	0.969	2	MS	RMJ	03/24/10 17:51	100323-2	959116
7440-39-3	Barium	20400	ug/Kg		102	508	508	1	P	HSC	03/29/10 23:24	032910C-1	959114
7440-41-7	Beryllium	0.512	mg/kg		0.0194	0.0969	0.0969	2	MS	RMJ	03/24/10 17:51	100323-2	959116
7440-43-9	Cadmium	508	ug/Kg	U	102	508	508	1	P	HSC	03/29/10 23:24	032910C-1	959114
7440-70-2	Calcium	347000	ug/Kg		8120	25400	25400	1	P	HSC	03/29/10 23:24	032910C-1	959114
7440-47-3	Chromium	2230	ug/Kg		152	508	508	1	P	HSC	03/29/10 23:24	032910C-1	959114
7440-48-4	Cobalt	657	ug/Kg		152	508	508	1	P	HSC	03/29/10 23:24	032910C-1	959114
7440-50-8	Copper	2180	ug/Kg		305	1020	1020	1	P	HSC	03/29/10 23:24	032910C-1	959114
7439-89-6	Iron	7330000	ug/Kg		8120	25400	25400	1	P	HSC	03/29/10 23:24	032910C-1	959114
7439-92-1	Lead	3720	ug/Kg		254	1020	1020	1	P	HSC	03/29/10 23:24	032910C-1	959114
7439-95-4	Magnesium	265000	ug/Kg		8630	30500	30500	1	P	HSC	03/29/10 23:24	032910C-1	959114
7439-96-5	Manganese	399000	ug/Kg		203	1020	1020	1	P	HSC	03/29/10 23:24	032910C-1	959114
7439-97-6	Mercury	11	ug/kg	U	3.76	11	11	1	AV	JXL1	03/10/10 13:22	031010S1-4	958757
7440-02-0	Nickel	1.87	mg/kg		0.0969	0.388	0.388	2	MS	RMJ	03/24/10 17:51	100323-2	959116
7440-09-7	Potassium	364000	ug/Kg		6500	25400	25400	1	P	HSC	03/29/10 23:24	032910C-1	959114
7782-49-2	Selenium	0.969	mg/kg	U	0.485	0.969	0.969	2	MS	RMJ	03/24/10 17:51	100323-2	959116
7440-22-4	Silver	508	ug/Kg	U	102	508	508	1	P	HSC	03/29/10 23:24	032910C-1	959114
7440-23-5	Sodium	218000	ug/Kg		7110	25400	25400	1	P	HSC	03/29/10 23:24	032910C-1	959114
7440-28-0	Thallium	0.194	mg/kg	U	0.0582	0.194	0.194	2	MS	RMJ	03/24/10 17:51	100323-2	959116
7440-61-1	Uranium	0.613	mg/kg		0.0128	0.0388	0.0388	2	MS	RMJ	03/26/10 01:27	100325-3	959116
7440-62-2	Vanadium	3630	ug/Kg		102	508	508	1	P	HSC	03/29/10 23:24	032910C-1	959114
7440-66-6	Zinc	46600	ug/Kg		335	1020	1020	1	P	HSC	03/29/10 23:24	032910C-1	959114

Prep Information:

Analytical Batch	Prep Batch	Prep Method	Initial wt./vol.	Units	Final wt./vol.	Units	Date	Analyst
958757	958755	SW846 7471A Prep	0.558	g	30	mL	03/10/10	LXH2
959114	959113	SW846 3050B	0.506	g	50	mL	03/09/10	AXG2
959116	959115	SW846 3050B	0.53	g	50	mL	03/03/10	BXA1

METALS
-1-
INORGANICS ANALYSIS DATA PACKAGE

SDG No: 10-2093-1

CONTRACT: LANL01004

METHOD TYPE: SW846

SAMPLE ID: 248118002

BASIS: Dry Weight

DATE COLLECTED 22-FEB-10

CLIENT ID: RE36-10-8456

LEVEL: Low

DATE RECEIVED 26-FEB-10

MATRIX: SOIL

%SOLIDS: 97.2

CAS No.	Analyte	Result	Units	Qual	MDL	PQL	CRDL	DF	M*	Analyst	Run Date	Analytical Run	Analytical Batch
7429-90-5	Aluminum	1820000	ug/Kg		6710	19700	19700	1	P	HSC	03/29/10 23:26	032910C-1	959114
7440-36-0	Antimony	987	ug/Kg	U	326	987	987	1	P	HSC	03/29/10 23:26	032910C-1	959114
7440-38-2	Arsenic	0.761	mg/kg	J	0.176	0.879	0.879	2	MS	RMJ	03/24/10 17:55	100323-2	959116
7440-39-3	Barium	21800	ug/Kg		98.7	494	494	1	P	HSC	03/29/10 23:26	032910C-1	959114
7440-41-7	Beryllium	0.485	mg/kg		0.0176	0.0879	0.0879	2	MS	RMJ	03/24/10 17:55	100323-2	959116
7440-43-9	Cadmium	494	ug/Kg	U	98.7	494	494	1	P	HSC	03/29/10 23:26	032910C-1	959114
7440-70-2	Calcium	396000	ug/Kg		7900	24700	24700	1	P	HSC	03/29/10 23:26	032910C-1	959114
7440-47-3	Chromium	2740	ug/Kg		148	494	494	1	P	HSC	03/29/10 23:26	032910C-1	959114
7440-48-4	Cobalt	740	ug/Kg		148	494	494	1	P	HSC	03/29/10 23:26	032910C-1	959114
7440-50-8	Copper	2120	ug/Kg		296	987	987	1	P	HSC	03/29/10 23:26	032910C-1	959114
7439-89-6	Iron	6920000	ug/Kg		7900	24700	24700	1	P	HSC	03/29/10 23:26	032910C-1	959114
7439-92-1	Lead	3560	ug/Kg		247	987	987	1	P	HSC	03/29/10 23:26	032910C-1	959114
7439-95-4	Magnesium	295000	ug/Kg		8390	29600	29600	1	P	HSC	03/29/10 23:26	032910C-1	959114
7439-96-5	Manganese	389000	ug/Kg		197	987	987	1	P	HSC	03/29/10 23:26	032910C-1	959114
7439-97-6	Mercury	11.3	ug/kg	U	3.85	11.3	11.3	1	AV	JXL1	03/10/10 13:24	031010S1-4	958757
7440-02-0	Nickel	1.85	mg/kg		0.0879	0.352	0.352	2	MS	RMJ	03/24/10 17:55	100323-2	959116
7440-09-7	Potassium	366000	ug/Kg		6320	24700	24700	1	P	HSC	03/29/10 23:26	032910C-1	959114
7782-49-2	Selenium	0.879	mg/kg	U	0.44	0.879	0.879	2	MS	RMJ	03/24/10 17:55	100323-2	959116
7440-22-4	Silver	494	ug/Kg	U	98.7	494	494	1	P	HSC	03/29/10 23:26	032910C-1	959114
7440-23-5	Sodium	209000	ug/Kg		6910	24700	24700	1	P	HSC	03/29/10 23:26	032910C-1	959114
7440-28-0	Thallium	0.176	mg/kg	U	0.0528	0.176	0.176	2	MS	RMJ	03/24/10 17:55	100323-2	959116
7440-61-1	Uranium	0.595	mg/kg		0.0116	0.0352	0.0352	2	MS	RMJ	03/26/10 01:30	100325-3	959116
7440-62-2	Vanadium	3650	ug/Kg		98.7	494	494	1	P	HSC	03/29/10 23:26	032910C-1	959114
7440-66-6	Zinc	43600	ug/Kg		326	987	987	1	P	HSC	03/29/10 23:26	032910C-1	959114

Prep Information:

Analytical Batch	Prep Batch	Prep Method	Initial wt./vol.	Units	Final wt./vol.	Units	Date	Analyst
958757	958755	SW846 7471A Prep	0.545	g	30	mL	03/10/10	LXH2
959114	959113	SW846 3050B	0.521	g	50	mL	03/09/10	AXG2
959116	959115	SW846 3050B	0.585	g	50	mL	03/03/10	BXA1

METALS
-1-
INORGANICS ANALYSIS DATA PACKAGE

SDG No: 10-2093-1

CONTRACT: LANL01004

METHOD TYPE: SW846

SAMPLE ID: 248118003

BASIS: Dry Weight

DATE COLLECTED 22-FEB-10

CLIENT ID: RE36-10-8451

LEVEL: Low

DATE RECEIVED 26-FEB-10

MATRIX: SOIL

%SOLIDS: 97

CAS No.	Analyte	Result	Units	Qual	MDL	PQL	CRDL	DF	M*	Analyst	Run Date	Analytical Run	Analytical Batch
7429-90-5	Aluminum	2450000	ug/Kg		6870	20200	20200	1	P	HSC	03/29/10 23:28	032910C-1	959114
7440-36-0	Antimony	1010	ug/Kg	U	334	1010	1010	1	P	HSC	03/29/10 23:28	032910C-1	959114
7440-38-2	Arsenic	0.644	mg/kg	J	0.2	0.999	0.999	2	MS	RMJ	03/24/10 17:59	100323-2	959116
7440-39-3	Barium	28800	ug/Kg		101	505	505	1	P	HSC	03/29/10 23:28	032910C-1	959114
7440-41-7	Beryllium	0.632	mg/kg		0.02	0.0999	0.0999	2	MS	RMJ	03/24/10 17:59	100323-2	959116
7440-43-9	Cadmium	505	ug/Kg	U	101	505	505	1	P	HSC	03/29/10 23:28	032910C-1	959114
7440-70-2	Calcium	575000	ug/Kg		8090	25300	25300	1	P	HSC	03/29/10 23:28	032910C-1	959114
7440-47-3	Chromium	3440	ug/Kg		152	505	505	1	P	HSC	03/29/10 23:28	032910C-1	959114
7440-48-4	Cobalt	1130	ug/Kg		152	505	505	1	P	HSC	03/29/10 23:28	032910C-1	959114
7440-50-8	Copper	2750	ug/Kg		303	1010	1010	1	P	HSC	03/29/10 23:28	032910C-1	959114
7439-89-6	Iron	7320000	ug/Kg		8090	25300	25300	1	P	HSC	03/29/10 23:28	032910C-1	959114
7439-92-1	Lead	6400	ug/Kg		253	1010	1010	1	P	HSC	03/29/10 23:28	032910C-1	959114
7439-95-4	Magnesium	461000	ug/Kg		8590	30300	30300	1	P	HSC	03/29/10 23:28	032910C-1	959114
7439-96-5	Manganese	362000	ug/Kg		202	1010	1010	1	P	HSC	03/29/10 23:28	032910C-1	959114
7439-97-6	Mercury	10.5	ug/kg	U	3.58	10.5	10.5	1	AV	JXL1	03/10/10 13:26	031010S1-4	958757
7440-02-0	Nickel	1.59	mg/kg		0.0999	0.4	0.4	2	MS	RMJ	03/24/10 17:59	100323-2	959116
7440-09-7	Potassium	479000	ug/Kg		6470	25300	25300	1	P	HSC	03/29/10 23:28	032910C-1	959114
7782-49-2	Selenium	0.999	mg/kg	U	0.5	0.999	0.999	2	MS	RMJ	03/24/10 17:59	100323-2	959116
7440-22-4	Silver	505	ug/Kg	U	101	505	505	1	P	HSC	03/29/10 23:28	032910C-1	959114
7440-23-5	Sodium	224000	ug/Kg		7080	25300	25300	1	P	HSC	03/29/10 23:28	032910C-1	959114
7440-28-0	Thallium	0.20	mg/kg	U	0.0599	0.2	0.2	2	MS	RMJ	03/24/10 17:59	100323-2	959116
7440-61-1	Uranium	0.587	mg/kg		0.0132	0.04	0.04	2	MS	RMJ	03/26/10 01:33	100325-3	959116
7440-62-2	Vanadium	4120	ug/Kg		101	505	505	1	P	HSC	03/29/10 23:28	032910C-1	959114
7440-66-6	Zinc	38700	ug/Kg		334	1010	1010	1	P	HSC	03/29/10 23:28	032910C-1	959114

Prep Information:

Analytical Batch	Prep Batch	Prep Method	Initial wt./vol.	Units	Final wt./vol.	Units	Date	Analyst
958757	958755	SW846 7471A Prep	0.588	g	30	mL	03/10/10	LXH2
959114	959113	SW846 3050B	0.51	g	50	mL	03/09/10	AXG2
959116	959115	SW846 3050B	0.516	g	50	mL	03/03/10	BXA1

METALS
-1-
INORGANICS ANALYSIS DATA PACKAGE

SDG No: 10-2093-1

CONTRACT: LANL01004

METHOD TYPE: SW846

SAMPLE ID: 248118004

BASIS: Dry Weight

DATE COLLECTED 22-FEB-10

CLIENT ID: RE36-10-8450

LEVEL: Low

DATE RECEIVED 26-FEB-10

MATRIX: SOIL

%SOLIDS: 85

CAS No.	Analyte	Result	Units	Qual	MDL	PQL	CRDL	DF	M*	Analyst	Run Date	Analytical Run	Analytical Batch
7429-90-5	Aluminum	13800000	ug/Kg		7250	21300	21300	1	P	HSC	03/29/10 23:30	032910C-1	959114
7440-36-0	Antimony	1070	ug/Kg	U	352	1070	1070	1	P	HSC	03/29/10 23:30	032910C-1	959114
7440-38-2	Arsenic	2.07	mg/kg		0.205	1.02	1.02	2	MS	RMJ	03/24/10 18:03	100323-2	959116
7440-39-3	Barium	82200	ug/Kg		107	533	533	1	P	HSC	03/29/10 23:30	032910C-1	959114
7440-41-7	Beryllium	2.69	mg/kg		0.0205	0.102	0.102	2	MS	RMJ	03/24/10 18:03	100323-2	959116
7440-43-9	Cadmium	533	ug/Kg	U	107	533	533	1	P	HSC	03/29/10 23:30	032910C-1	959114
7440-70-2	Calcium	47000000	ug/Kg		8530	26700	26700	1	P	HSC	03/29/10 23:30	032910C-1	959114
7440-47-3	Chromium	9640	ug/Kg		160	533	533	1	P	HSC	03/29/10 23:30	032910C-1	959114
7440-48-4	Cobalt	2440	ug/Kg		160	533	533	1	P	HSC	03/29/10 23:30	032910C-1	959114
7440-50-8	Copper	9920	ug/Kg		320	1070	1070	1	P	HSC	03/29/10 23:30	032910C-1	959114
7439-89-6	Iron	12700000	ug/Kg		8530	26700	26700	1	P	HSC	03/29/10 23:30	032910C-1	959114
7439-92-1	Lead	13000	ug/Kg		267	1070	1070	1	P	HSC	03/29/10 23:30	032910C-1	959114
7439-95-4	Magnesium	3080000	ug/Kg		9070	32000	32000	1	P	HSC	03/29/10 23:30	032910C-1	959114
7439-96-5	Manganese	402000	ug/Kg		213	1070	1070	1	P	HSC	03/29/10 23:30	032910C-1	959114
7439-97-6	Mercury	56.1	ug/kg		4	11.8	11.8	1	AV	JXL1	03/10/10 13:28	031010S1-4	958757
7440-02-0	Nickel	10.6	mg/kg		0.102	0.41	0.41	2	MS	RMJ	03/24/10 18:03	100323-2	959116
7440-09-7	Potassium	1920000	ug/Kg		6830	26700	26700	1	P	HSC	03/29/10 23:30	032910C-1	959114
7782-49-2	Selenium	1.02	mg/kg	U	0.512	1.02	1.02	2	MS	RMJ	03/24/10 18:03	100323-2	959116
7440-22-4	Silver	533	ug/Kg	U	107	533	533	1	P	HSC	03/29/10 23:30	032910C-1	959114
7440-23-5	Sodium	155000	ug/Kg		7470	26700	26700	1	P	HSC	03/29/10 23:30	032910C-1	959114
7440-28-0	Thallium	0.152	mg/kg	J	0.0614	0.205	0.205	2	MS	RMJ	03/24/10 18:03	100323-2	959116
7440-61-1	Uranium	1.37	mg/kg		0.0135	0.041	0.041	2	MS	RMJ	03/26/10 01:42	100325-3	959116
7440-62-2	Vanadium	16200	ug/Kg		107	533	533	1	P	HSC	03/29/10 23:30	032910C-1	959114
7440-66-6	Zinc	49600	ug/Kg		352	1070	1070	1	P	HSC	03/29/10 23:30	032910C-1	959114

Prep Information:

Analytical Batch	Prep Batch	Prep Method	Initial wt./vol.	Units	Final wt./vol.	Units	Date	Analyst
958757	958755	SW846 7471A Prep	0.599	g	30	mL	03/10/10	LXH2
959114	959113	SW846 3050B	0.551	g	50	mL	03/09/10	AXG2
959116	959115	SW846 3050B	0.574	g	50	mL	03/03/10	BXA1

METALS
-1-
INORGANICS ANALYSIS DATA PACKAGE

SDG No: 10-2093-1

CONTRACT: LANL01004

METHOD TYPE: SW846

SAMPLE ID: 248118005

BASIS: Dry Weight

DATE COLLECTED 22-FEB-10

CLIENT ID: RE36-10-8449

LEVEL: Low

DATE RECEIVED 26-FEB-10

MATRIX: SOIL

%SOLIDS: 98.2

CAS No.	Analyte	Result	Units	Qual	MDL	PQL	CRDL	DF	M*	Analyst	Run Date	Analytical Run	Analytical Batch
7429-90-5	Aluminum	1410000	ug/Kg		5830	17100	17100	1	P	HSC	03/29/10 23:32	032910C-1	959114
7440-36-0	Antimony	857	ug/Kg	U	283	857	857	1	P	HSC	03/29/10 23:32	032910C-1	959114
7440-38-2	Arsenic	0.533	mg/kg	J	0.177	0.884	0.884	2	MS	RMJ	03/24/10 18:07	100323-2	959116
7440-39-3	Barium	28200	ug/Kg		85.7	428	428	1	P	HSC	03/29/10 23:32	032910C-1	959114
7440-41-7	Beryllium	0.493	mg/kg		0.0177	0.0884	0.0884	2	MS	RMJ	03/24/10 18:07	100323-2	959116
7440-43-9	Cadmium	428	ug/Kg	U	85.7	428	428	1	P	HSC	03/29/10 23:32	032910C-1	959114
7440-70-2	Calcium	256000	ug/Kg		6850	21400	21400	1	P	HSC	03/29/10 23:32	032910C-1	959114
7440-47-3	Chromium	2240	ug/Kg		129	428	428	1	P	HSC	03/29/10 23:32	032910C-1	959114
7440-48-4	Cobalt	612	ug/Kg		129	428	428	1	P	HSC	03/29/10 23:32	032910C-1	959114
7440-50-8	Copper	2400	ug/Kg		257	857	857	1	P	HSC	03/29/10 23:32	032910C-1	959114
7439-89-6	Iron	6440000	ug/Kg		6850	21400	21400	1	P	HSC	03/29/10 23:32	032910C-1	959114
7439-92-1	Lead	6970	ug/Kg		214	857	857	1	P	HSC	03/29/10 23:32	032910C-1	959114
7439-95-4	Magnesium	160000	ug/Kg		7280	25700	25700	1	P	HSC	03/29/10 23:32	032910C-1	959114
7439-96-5	Manganese	497000	ug/Kg		171	857	857	1	P	HSC	03/29/10 23:32	032910C-1	959114
7439-97-6	Mercury	11.4	ug/kg	U	3.88	11.4	11.4	1	AV	JXL1	03/10/10 13:34	031010S1-4	958757
7440-02-0	Nickel	1.72	mg/kg		0.0884	0.353	0.353	2	MS	RMJ	03/24/10 18:07	100323-2	959116
7440-09-7	Potassium	438000	ug/Kg		5480	21400	21400	1	P	HSC	03/29/10 23:32	032910C-1	959114
7782-49-2	Selenium	0.884	mg/kg	U	0.442	0.884	0.884	2	MS	RMJ	03/24/10 18:07	100323-2	959116
7440-22-4	Silver	428	ug/Kg	U	85.7	428	428	1	P	HSC	03/29/10 23:32	032910C-1	959114
7440-23-5	Sodium	332000	ug/Kg		6000	21400	21400	1	P	HSC	03/29/10 23:32	032910C-1	959114
7440-28-0	Thallium	0.177	mg/kg	U	0.053	0.177	0.177	2	MS	RMJ	03/24/10 18:07	100323-2	959116
7440-61-1	Uranium	0.687	mg/kg		0.0117	0.0353	0.0353	2	MS	RMJ	03/26/10 01:45	100325-3	959116
7440-62-2	Vanadium	2750	ug/Kg		85.7	428	428	1	P	HSC	03/29/10 23:32	032910C-1	959114
7440-66-6	Zinc	47000	ug/Kg		283	857	857	1	P	HSC	03/29/10 23:32	032910C-1	959114

Prep Information:

Analytical Batch	Prep Batch	Prep Method	Initial wt./vol.	Units	Final wt./vol.	Units	Date	Analyst
958757	958755	SW846 7471A Prep	0.535	g	30	mL	03/10/10	LXH2
959114	959113	SW846 3050B	0.594	g	50	mL	03/09/10	AXG2
959116	959115	SW846 3050B	0.576	g	50	mL	03/03/10	BXA1

METALS
-1-
INORGANICS ANALYSIS DATA PACKAGE

SDG No: 10-2093-1

CONTRACT: LANL01004

METHOD TYPE: SW846

SAMPLE ID: 248118006

BASIS: Dry Weight

DATE COLLECTED 22-FEB-10

CLIENT ID: RE36-10-8453

LEVEL: Low

DATE RECEIVED 26-FEB-10

MATRIX: SOIL

%SOLIDS: 95.7

CAS No.	Analyte	Result	Units	Qual	MDL	PQL	CRDL	DF	M*	Analyst	Run Date	Analytical Run	Analytical Batch
7429-90-5	Aluminum	3570000	ug/Kg		6780	19900	19900	1	P	HSC	03/29/10 23:34	032910C-1	959114
7440-36-0	Antimony	997	ug/Kg	U	329	997	997	1	P	HSC	03/29/10 23:34	032910C-1	959114
7440-38-2	Arsenic	0.850	mg/kg	J	0.204	1.02	1.02	2	MS	RMJ	03/24/10 18:11	100323-2	959116
7440-39-3	Barium	63700	ug/Kg		99.7	498	498	1	P	HSC	03/29/10 23:34	032910C-1	959114
7440-41-7	Beryllium	0.678	mg/kg		0.0204	0.102	0.102	2	MS	RMJ	03/24/10 18:11	100323-2	959116
7440-43-9	Cadmium	498	ug/Kg	U	99.7	498	498	1	P	HSC	03/29/10 23:34	032910C-1	959114
7440-70-2	Calcium	775000	ug/Kg		7970	24900	24900	1	P	HSC	03/29/10 23:34	032910C-1	959114
7440-47-3	Chromium	8380	ug/Kg		150	498	498	1	P	HSC	03/29/10 23:34	032910C-1	959114
7440-48-4	Cobalt	916	ug/Kg		150	498	498	1	P	HSC	03/29/10 23:34	032910C-1	959114
7440-50-8	Copper	3930	ug/Kg		299	997	997	1	P	HSC	03/29/10 23:34	032910C-1	959114
7439-89-6	Iron	10000000	ug/Kg		7970	24900	24900	1	P	HSC	03/29/10 23:34	032910C-1	959114
7439-92-1	Lead	5490	ug/Kg		249	997	997	1	P	HSC	03/29/10 23:34	032910C-1	959114
7439-95-4	Magnesium	766000	ug/Kg		8470	29900	29900	1	P	HSC	03/29/10 23:34	032910C-1	959114
7439-96-5	Manganese	359000	ug/Kg		199	997	997	1	P	HSC	03/29/10 23:34	032910C-1	959114
7439-97-6	Mercury	11.1	ug/kg	U	3.79	11.1	11.1	1	AV	JXLI	03/10/10 13:36	031010S1-4	958757
7440-02-0	Nickel	2.99	mg/kg		0.102	0.408	0.408	2	MS	RMJ	03/24/10 18:11	100323-2	959116
7440-09-7	Potassium	601000	ug/Kg		6380	24900	24900	1	P	HSC	03/29/10 23:34	032910C-1	959114
7782-49-2	Selenium	1.02	mg/kg	U	0.51	1.02	1.02	2	MS	RMJ	03/24/10 18:11	100323-2	959116
7440-22-4	Silver	498	ug/Kg	U	99.7	498	498	1	P	HSC	03/29/10 23:34	032910C-1	959114
7440-23-5	Sodium	358000	ug/Kg		6980	24900	24900	1	P	HSC	03/29/10 23:34	032910C-1	959114
7440-28-0	Thallium	0.204	mg/kg	U	0.0612	0.204	0.204	2	MS	RMJ	03/24/10 18:11	100323-2	959116
7440-61-1	Uranium	0.678	mg/kg		0.0135	0.0408	0.0408	2	MS	RMJ	03/26/10 01:48	100325-3	959116
7440-62-2	Vanadium	7320	ug/Kg		99.7	498	498	1	P	HSC	03/29/10 23:34	032910C-1	959114
7440-66-6	Zinc	50500	ug/Kg		329	997	997	1	P	HSC	03/29/10 23:34	032910C-1	959114

Prep Information:

Analytical Batch	Prep Batch	Prep Method	Initial wt./vol.	Units	Final wt./vol.	Units	Date	Analyst
958757	958755	SW846 7471A Prep	0.563	g	30	mL	03/10/10	LXH2
959114	959113	SW846 3050B	0.524	g	50	mL	03/09/10	AXG2
959116	959115	SW846 3050B	0.512	g	50	mL	03/03/10	BXA1

METALS
-1-
INORGANICS ANALYSIS DATA PACKAGE

SDG No: 10-2093-1

CONTRACT: LANL01004

METHOD TYPE: SW846

SAMPLE ID: 248118007

BASIS: Dry Weight

DATE COLLECTED 22-FEB-10

CLIENT ID: RE36-10-8452

LEVEL: Low

DATE RECEIVED 26-FEB-10

MATRIX: SOIL

%SOLIDS: 92.9

CAS No.	Analyte	Result	Units	Qual	MDL	PQL	CRDL	DF	M*	Analyst	Run Date	Analytical Run	Analytical Batch
7429-90-5	Aluminum	6940000	ug/Kg		6210	18300	18300	1	P	HSC	03/29/10 23:36	032910C-1	959114
7440-36-0	Antimony	913	ug/Kg	U	301	913	913	1	P	HSC	03/29/10 23:36	032910C-1	959114
7440-38-2	Arsenic	1.71	mg/kg		0.184	0.922	0.922	2	MS	RMJ	03/24/10 18:15	100323-2	959116
7440-39-3	Barium	84600	ug/Kg		91.3	456	456	1	P	HSC	03/29/10 23:36	032910C-1	959114
7440-41-7	Beryllium	0.863	mg/kg		0.0184	0.0922	0.0922	2	MS	RMJ	03/24/10 18:15	100323-2	959116
7440-43-9	Cadmium	456	ug/Kg	U	91.3	456	456	1	P	HSC	03/29/10 23:36	032910C-1	959114
7440-70-2	Calcium	1570000	ug/Kg		7300	22800	22800	1	P	HSC	03/29/10 23:36	032910C-1	959114
7440-47-3	Chromium	6860	ug/Kg		137	456	456	1	P	HSC	03/29/10 23:36	032910C-1	959114
7440-48-4	Cobalt	4200	ug/Kg		137	456	456	1	P	HSC	03/29/10 23:36	032910C-1	959114
7440-50-8	Copper	5980	ug/Kg		274	913	913	1	P	HSC	03/29/10 23:36	032910C-1	959114
7439-89-6	Iron	11100000	ug/Kg		7300	22800	22800	1	P	HSC	03/29/10 23:36	032910C-1	959114
7439-92-1	Lead	9290	ug/Kg		228	913	913	1	P	HSC	03/29/10 23:36	032910C-1	959114
7439-95-4	Magnesium	1730000	ug/Kg		7760	27400	27400	1	P	HSC	03/29/10 23:36	032910C-1	959114
7439-96-5	Manganese	359000	ug/Kg		183	913	913	1	P	HSC	03/29/10 23:36	032910C-1	959114
7439-97-6	Mercury	11.7	ug/kg	U	3.97	11.7	11.7	1	AV	JXL1	03/10/10 13:38	031010S1-4	958757
7440-02-0	Nickel	6.82	mg/kg		0.0922	0.369	0.369	2	MS	RMJ	03/24/10 18:15	100323-2	959116
7440-09-7	Potassium	1510000	ug/Kg		5840	22800	22800	1	P	HSC	03/29/10 23:36	032910C-1	959114
7782-49-2	Selenium	0.922	mg/kg	U	0.461	0.922	0.922	2	MS	RMJ	03/24/10 18:15	100323-2	959116
7440-22-4	Silver	456	ug/Kg	U	91.3	456	456	1	P	HSC	03/29/10 23:36	032910C-1	959114
7440-23-5	Sodium	452000	ug/Kg		6390	22800	22800	1	P	HSC	03/29/10 23:36	032910C-1	959114
7440-28-0	Thallium	0.124	mg/kg	J	0.0553	0.184	0.184	2	MS	RMJ	03/24/10 18:15	100323-2	959116
7440-61-1	Uranium	0.688	mg/kg		0.0122	0.0369	0.0369	2	MS	RMJ	03/26/10 01:51	100325-3	959116
7440-62-2	Vanadium	15700	ug/Kg		91.3	456	456	1	P	HSC	03/29/10 23:36	032910C-1	959114
7440-66-6	Zinc	33400	ug/Kg		301	913	913	1	P	HSC	03/29/10 23:36	032910C-1	959114

Prep Information:

Analytical Batch	Prep Batch	Prep Method	Initial wt./vol.	Units	Final wt./vol.	Units	Date	Analyst
958757	958755	SW846 7471A Prep	0.554	g	30	mL	03/10/10	LXH2
959114	959113	SW846 3050B	0.59	g	50	mL	03/09/10	AXG2
959116	959115	SW846 3050B	0.584	g	50	mL	03/03/10	BXA1

Quality Control Summary

METALS
-2a-
Initial and Continuing Calibration Verification

SDG No: 10-2093-1

Contract: LANL01004

Lab Code: GEL

Initial Calibration Source: Solutions Plus

Continuing Calibration Source: O2Si

Instrument ID: ICPMS6,MER536,OPTIMA4

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>True Value</u>	<u>Units</u>	<u>% Recovery</u>	<u>Acceptance Window (%R)</u>	<u>M</u>	<u>Analysis Date/Time</u>	<u>Run Number</u>
ICV01										
	Mercury	5.29	ug/L	5	ug/L	105.8	90.0 – 110.0	AV	10-MAR-10 11:37	031010S1-4
	Arsenic	51.4	ug/L	50	ug/L	102.8	90.0 – 110.0	MS	24-MAR-10 16:10	100323-2
	Beryllium	50.6	ug/L	50	ug/L	101.2	90.0 – 110.0	MS	24-MAR-10 16:10	100323-2
	Nickel	51.5	ug/L	50	ug/L	103	90.0 – 110.0	MS	24-MAR-10 16:10	100323-2
	Selenium	51.9	ug/L	50	ug/L	103.8	90.0 – 110.0	MS	24-MAR-10 16:10	100323-2
	Thallium	50.4	ug/L	50	ug/L	100.8	90.0 – 110.0	MS	24-MAR-10 16:10	100323-2
	Uranium	54.1	ug/L	50	ug/L	108.2	90.0 – 110.0	MS	25-MAR-10 23:48	100325-3
	Aluminum	5140	ug/L	5000	ug/L	102.7	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Antimony	491	ug/L	500	ug/L	98.2	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Barium	508	ug/L	500	ug/L	101.6	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Cadmium	497	ug/L	500	ug/L	99.5	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Calcium	5000	ug/L	5000	ug/L	100	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Chromium	488	ug/L	500	ug/L	97.6	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Cobalt	506	ug/L	500	ug/L	101.3	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Copper	510	ug/L	500	ug/L	102	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Iron	5010	ug/L	5000	ug/L	100.3	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Lead	499	ug/L	500	ug/L	99.8	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Magnesium	5200	ug/L	5000	ug/L	103.9	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Manganese	506	ug/L	500	ug/L	101.2	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Potassium	2470	ug/L	2500	ug/L	98.7	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Silver	257	ug/L	250	ug/L	102.8	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Sodium	2460	ug/L	2500	ug/L	98.5	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Vanadium	505	ug/L	500	ug/L	100.9	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
	Zinc	497	ug/L	500	ug/L	99.4	90.0 – 110.0	P	29-MAR-10 18:35	032910C-1
CCV01										
	Mercury	5.16	ug/L	5	ug/L	103.3	80.0 – 120.0	AV	10-MAR-10 11:43	031010S1-4
	Arsenic	50.4	ug/L	50	ug/L	100.8	90.0 – 110.0	MS	24-MAR-10 16:30	100323-2
	Beryllium	49.4	ug/L	50	ug/L	98.7	90.0 – 110.0	MS	24-MAR-10 16:30	100323-2
	Nickel	51.3	ug/L	50	ug/L	102.6	90.0 – 110.0	MS	24-MAR-10 16:30	100323-2
	Selenium	51.9	ug/L	50	ug/L	103.8	90.0 – 110.0	MS	24-MAR-10 16:30	100323-2

METALS
-2a-
Initial and Continuing Calibration Verification

SDG No: 10-2093-1

Contract: LANL01004

Lab Code: GEL

Initial Calibration Source: Solutions Plus

Continuing Calibration Source: O2Si

Instrument ID: ICPMS6.MER536.OPTIMA4

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>True Value</u>	<u>Units</u>	<u>% Recovery</u>	<u>Acceptance Window (%R)</u>	<u>M</u>	<u>Analysis Date/Time</u>	<u>Run Number</u>
	Thallium	50.1	ug/L	50	ug/L	100.1	90.0 – 110.0	MS	24-MAR-10 16:30	100323-2
	Uranium	53.8	ug/L	50	ug/L	107.6	90.0 – 110.0	MS	26-MAR-10 00:04	100325-3
	Aluminum	5090	ug/L	5000	ug/L	101.7	90.0 – 110.0	P	29-MAR-10 18:49	032910C-1
	Antimony	490	ug/L	500	ug/L	98.1	90.0 – 110.0	P	29-MAR-10 18:49	032910C-1
	Barium	498	ug/L	500	ug/L	99.6	90.0 – 110.0	P	29-MAR-10 18:49	032910C-1
	Cadmium	489	ug/L	500	ug/L	97.8	90.0 – 110.0	P	29-MAR-10 18:49	032910C-1
	Calcium	4990	ug/L	5000	ug/L	99.8	90.0 – 110.0	P	29-MAR-10 18:49	032910C-1
	Chromium	493	ug/L	500	ug/L	98.6	90.0 – 110.0	P	29-MAR-10 18:49	032910C-1
	Cobalt	491	ug/L	500	ug/L	98.2	90.0 – 110.0	P	29-MAR-10 18:49	032910C-1
	Copper	496	ug/L	500	ug/L	99.3	90.0 – 110.0	P	29-MAR-10 18:49	032910C-1
	Iron	4940	ug/L	5000	ug/L	98.8	90.0 – 110.0	P	29-MAR-10 18:49	032910C-1
	Lead	494	ug/L	500	ug/L	98.8	90.0 – 110.0	P	29-MAR-10 18:49	032910C-1
	Magnesium	5080	ug/L	5000	ug/L	101.5	90.0 – 110.0	P	29-MAR-10 18:49	032910C-1
	Manganesec	494	ug/L	500	ug/L	98.7	90.0 – 110.0	P	29-MAR-10 18:49	032910C-1
	Potassium	5440	ug/L	5000	ug/L	108.7	90.0 – 110.0	P	29-MAR-10 18:49	032910C-1
	Silver	498	ug/L	500	ug/L	99.6	90.0 – 110.0	P	29-MAR-10 18:49	032910C-1
	Sodium	10000	ug/L	10000	ug/L	100	90.0 – 110.0	P	29-MAR-10 18:49	032910C-1
	Vanadium	499	ug/L	500	ug/L	99.8	90.0 – 110.0	P	29-MAR-10 18:49	032910C-1
	Zinc	488	ug/L	500	ug/L	97.7	90.0 – 110.0	P	29-MAR-10 18:49	032910C-1
CCV02	Mercury	5.15	ug/L	5	ug/L	103	80.0 – 120.0	AV	10-MAR-10 12:06	031010S1-4
	Arsenic	50.2	ug/L	50	ug/L	100.3	90.0 – 110.0	MS	24-MAR-10 16:47	100323-2
	Beryllium	49.7	ug/L	50	ug/L	99.5	90.0 – 110.0	MS	24-MAR-10 16:47	100323-2
	Nickel	51.8	ug/L	50	ug/L	103.6	90.0 – 110.0	MS	24-MAR-10 16:47	100323-2
	Selenium	51.9	ug/L	50	ug/L	103.9	90.0 – 110.0	MS	24-MAR-10 16:47	100323-2
	Thallium	50.8	ug/L	50	ug/L	101.5	90.0 – 110.0	MS	24-MAR-10 16:47	100323-2
	Uranium	54	ug/L	50	ug/L	108.1	90.0 – 110.0	MS	26-MAR-10 00:32	100325-3
	Aluminum	5100	ug/L	5000	ug/L	102	90.0 – 110.0	P	29-MAR-10 18:57	032910C-1
	Antimony	490	ug/L	500	ug/L	97.9	90.0 – 110.0	P	29-MAR-10 18:57	032910C-1
	Barium	497	ug/L	500	ug/L	99.4	90.0 – 110.0	P	29-MAR-10 18:57	032910C-1

METALS
-2a-
Initial and Continuing Calibration Verification

SDG No: 10-2093-1

Contract: LANL01004

Lab Code: GEL

Initial Calibration Source: Solutions Plus

Continuing Calibration Source: O2Si

Instrument ID: ICPMS6,MER536,OPTIMA4

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>True Value</u>	<u>Units</u>	<u>% Recovery</u>	<u>Acceptance Window (%R)</u>	<u>M</u>	<u>Analysis Date/Time</u>	<u>Run Number</u>
	Cadmium	488	ug/L	500	ug/L	97.6	90.0 – 110.0	P	29-MAR-10 18:57	032910C-1
	Calcium	4970	ug/L	5000	ug/L	99.4	90.0 – 110.0	P	29-MAR-10 18:57	032910C-1
	Chromium	492	ug/L	500	ug/L	98.5	90.0 – 110.0	P	29-MAR-10 18:57	032910C-1
	Cobalt	490	ug/L	500	ug/L	98	90.0 – 110.0	P	29-MAR-10 18:57	032910C-1
	Copper	495	ug/L	500	ug/L	99	90.0 – 110.0	P	29-MAR-10 18:57	032910C-1
	Iron	4920	ug/L	5000	ug/L	98.4	90.0 – 110.0	P	29-MAR-10 18:57	032910C-1
	Lead	487	ug/L	500	ug/L	97.5	90.0 – 110.0	P	29-MAR-10 18:57	032910C-1
	Magnesium	5070	ug/L	5000	ug/L	101.5	90.0 – 110.0	P	29-MAR-10 18:57	032910C-1
	Manganese	493	ug/L	500	ug/L	98.6	90.0 – 110.0	P	29-MAR-10 18:57	032910C-1
	Potassium	4890	ug/L	5000	ug/L	97.8	90.0 – 110.0	P	29-MAR-10 18:57	032910C-1
	Silver	498	ug/L	500	ug/L	99.6	90.0 – 110.0	P	29-MAR-10 18:57	032910C-1
	Sodium	9880	ug/L	10000	ug/L	98.8	90.0 – 110.0	P	29-MAR-10 18:57	032910C-1
	Vanadium	500	ug/L	500	ug/L	100	90.0 – 110.0	P	29-MAR-10 18:57	032910C-1
	Zinc	484	ug/L	500	ug/L	96.8	90.0 – 110.0	P	29-MAR-10 18:57	032910C-1
CCV03										
	Mercury	3.21	ug/L	5	ug/L	64.1	80.0 – 120.0	AV	10-MAR-10 12:31	031010S1-4
	Arsenic	51.8	ug/L	50	ug/L	103.5	90.0 – 110.0	MS	24-MAR-10 17:27	100323-2
	Beryllium	52.5	ug/L	50	ug/L	105	90.0 – 110.0	MS	24-MAR-10 17:27	100323-2
	Nickel	51.5	ug/L	50	ug/L	102.9	90.0 – 110.0	MS	24-MAR-10 17:27	100323-2
	Selenium	52.6	ug/L	50	ug/L	105.1	90.0 – 110.0	MS	24-MAR-10 17:27	100323-2
	Thallium	50.5	ug/L	50	ug/L	101.1	90.0 – 110.0	MS	24-MAR-10 17:27	100323-2
	Uranium	53.8	ug/L	50	ug/L	107.7	90.0 – 110.0	MS	26-MAR-10 01:02	100325-3
	Aluminum	5160	ug/L	5000	ug/L	103.3	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Antimony	485	ug/L	500	ug/L	97	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Barium	498	ug/L	500	ug/L	99.6	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Cadmium	483	ug/L	500	ug/L	96.5	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Calcium	4960	ug/L	5000	ug/L	99.2	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Chromium	488	ug/L	500	ug/L	97.7	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Cobalt	487	ug/L	500	ug/L	97.5	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Copper	493	ug/L	500	ug/L	98.6	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1

METALS
-2a-
Initial and Continuing Calibration Verification

SDG No: 10-2093-1

Contract: LANL01004

Lab Code: GEL

Initial Calibration Source: Solutions Plus

Continuing Calibration Source: O2Si

Instrument ID: ICPMS6,MER536,OPTIMA4

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>True Value</u>	<u>Units</u>	<u>% Recovery</u>	<u>Acceptance Window (%R)</u>	<u>M</u>	<u>Analysis Date/Time</u>	<u>Run Number</u>
	Iron	4930	ug/L	5000	ug/L	98.5	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Lead	479	ug/L	500	ug/L	95.8	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Magnesium	5060	ug/L	5000	ug/L	101.2	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Manganese	491	ug/L	500	ug/L	98.2	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Potassium	4830	ug/L	5000	ug/L	96.6	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Silver	496	ug/L	500	ug/L	99.2	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Sodium	9860	ug/L	10000	ug/L	98.6	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Vanadium	498	ug/L	500	ug/L	99.6	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
	Zinc	480	ug/L	500	ug/L	96.1	90.0 – 110.0	P	29-MAR-10 19:31	032910C-1
CCV04										
	Mercury	3.92	ug/L	5	ug/L	78.5	80.0 – 120.0	AV	10-MAR-10 12:54	031010S1-4
	Arsenic	50.3	ug/L	50	ug/L	100.5	90.0 – 110.0	MS	24-MAR-10 18:19	100323-2
	Beryllium	53.1	ug/L	50	ug/L	106.2	90.0 – 110.0	MS	24-MAR-10 18:19	100323-2
	Nickel	51.9	ug/L	50	ug/L	103.8	90.0 – 110.0	MS	24-MAR-10 18:19	100323-2
	Selenium	51.2	ug/L	50	ug/L	102.4	90.0 – 110.0	MS	24-MAR-10 18:19	100323-2
	Thallium	51	ug/L	50	ug/L	102	90.0 – 110.0	MS	24-MAR-10 18:19	100323-2
	Uranium	53.6	ug/L	50	ug/L	107.2	90.0 – 110.0	MS	26-MAR-10 01:36	100325-3
	Aluminum	5160	ug/L	5000	ug/L	103.1	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Antimony	486	ug/L	500	ug/L	97.2	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Barium	498	ug/L	500	ug/L	99.5	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Cadmium	481	ug/L	500	ug/L	96.2	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Calcium	4950	ug/L	5000	ug/L	98.9	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Chromium	488	ug/L	500	ug/L	97.6	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Cobalt	486	ug/L	500	ug/L	97.1	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Copper	492	ug/L	500	ug/L	98.4	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Iron	4910	ug/L	5000	ug/L	98.3	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Lead	481	ug/L	500	ug/L	96.2	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Magnesium	5060	ug/L	5000	ug/L	101.2	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Manganese	490	ug/L	500	ug/L	98	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Potassium	4830	ug/L	5000	ug/L	96.7	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1

METALS

-2a-

Initial and Continuing Calibration Verification

SDG No: 10-2093-1

Contract: LANL01004

Lab Code: GEL

Initial Calibration Source: Solutions Plus

Continuing Calibration Source: O2Si

Instrument ID: ICPMS6,MER536,OPTIMA4

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>True Value</u>	<u>Units</u>	<u>% Recovery</u>	<u>Acceptance Window (%R)</u>	<u>M</u>	<u>Analysis Date/Time</u>	<u>Run Number</u>
	Silver	495	ug/L	500	ug/L	99.1	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Sodium	9860	ug/L	10000	ug/L	98.6	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Vanadium	498	ug/L	500	ug/L	99.7	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
	Zinc	479	ug/L	500	ug/L	95.8	90.0 – 110.0	P	29-MAR-10 19:52	032910C-1
CCV05										
	Mercury	4.95	ug/L	5	ug/L	99	80.0 – 120.0	AV	10-MAR-10 13:06	031010S1-4
	Uranium	53.8	ug/L	50	ug/L	107.6	90.0 – 110.0	MS	26-MAR-10 01:54	100325-3
	Aluminum	5180	ug/L	5000	ug/L	103.6	90.0 – 110.0	P	29-MAR-10 20:14	032910C-1
	Antimony	490	ug/L	500	ug/L	98.1	90.0 – 110.0	P	29-MAR-10 20:14	032910C-1
	Barium	502	ug/L	500	ug/L	100.4	90.0 – 110.0	P	29-MAR-10 20:14	032910C-1
	Cadmium	485	ug/L	500	ug/L	97.1	90.0 – 110.0	P	29-MAR-10 20:14	032910C-1
	Calcium	4930	ug/L	5000	ug/L	98.6	90.0 – 110.0	P	29-MAR-10 20:14	032910C-1
	Chromium	492	ug/L	500	ug/L	98.3	90.0 – 110.0	P	29-MAR-10 20:14	032910C-1
	Cobalt	489	ug/L	500	ug/L	97.8	90.0 – 110.0	P	29-MAR-10 20:14	032910C-1
	Copper	495	ug/L	500	ug/L	99	90.0 – 110.0	P	29-MAR-10 20:14	032910C-1
	Iron	4900	ug/L	5000	ug/L	98	90.0 – 110.0	P	29-MAR-10 20:14	032910C-1
	Lead	485	ug/L	500	ug/L	96.9	90.0 – 110.0	P	29-MAR-10 20:14	032910C-1
	Magnesium	5040	ug/L	5000	ug/L	100.7	90.0 – 110.0	P	29-MAR-10 20:14	032910C-1
	Manganese	493	ug/L	500	ug/L	98.6	90.0 – 110.0	P	29-MAR-10 20:14	032910C-1
	Potassium	4780	ug/L	5000	ug/L	95.7	90.0 – 110.0	P	29-MAR-10 20:14	032910C-1
	Silver	498	ug/L	500	ug/L	99.6	90.0 – 110.0	P	29-MAR-10 20:14	032910C-1
	Sodium	9800	ug/L	10000	ug/L	98	90.0 – 110.0	P	29-MAR-10 20:14	032910C-1
	Vanadium	501	ug/L	500	ug/L	100.2	90.0 – 110.0	P	29-MAR-10 20:14	032910C-1
	Zinc	482	ug/L	500	ug/L	96.5	90.0 – 110.0	P	29-MAR-10 20:14	032910C-1
CCV06										
	Mercury	4.94	ug/L	5	ug/L	98.8	80.0 – 120.0	AV	10-MAR-10 13:30	031010S1-4
	Aluminum	5180	ug/L	5000	ug/L	103.7	90.0 – 110.0	P	29-MAR-10 20:39	032910C-1
	Antimony	485	ug/L	500	ug/L	97.1	90.0 – 110.0	P	29-MAR-10 20:39	032910C-1
	Barium	500	ug/L	500	ug/L	100	90.0 – 110.0	P	29-MAR-10 20:39	032910C-1
	Cadmium	478	ug/L	500	ug/L	95.6	90.0 – 110.0	P	29-MAR-10 20:39	032910C-1

METALS

-2a-

Initial and Continuing Calibration Verification

SDG No: 10-2093-1

Contract: LANL01004

Lab Code: GEL

Initial Calibration Source: Solutions Plus

Continuing Calibration Source: O2Si

Instrument ID: ICPMS6,MER536,OPTIMA4

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>True Value</u>	<u>Units</u>	<u>% Recovery</u>	<u>Acceptance Window (%R)</u>	<u>M</u>	<u>Analysis Date/Time</u>	<u>Run Number</u>
	Calcium	4890	ug/L	5000	ug/L	97.8	90.0 - 110.0	P	29-MAR-10 20:39	032910C-1
	Chromium	488	ug/L	500	ug/L	97.6	90.0 - 110.0	P	29-MAR-10 20:39	032910C-1
	Cobalt	485	ug/L	500	ug/L	97.1	90.0 - 110.0	P	29-MAR-10 20:39	032910C-1
	Copper	493	ug/L	500	ug/L	98.7	90.0 - 110.0	P	29-MAR-10 20:39	032910C-1
	Iron	4870	ug/L	5000	ug/L	97.5	90.0 - 110.0	P	29-MAR-10 20:39	032910C-1
	Lead	477	ug/L	500	ug/L	95.5	90.0 - 110.0	P	29-MAR-10 20:39	032910C-1
	Magnesium	5020	ug/L	5000	ug/L	100.3	90.0 - 110.0	P	29-MAR-10 20:39	032910C-1
	Manganese	489	ug/L	500	ug/L	97.9	90.0 - 110.0	P	29-MAR-10 20:39	032910C-1
	Potassium	4730	ug/L	5000	ug/L	94.6	90.0 - 110.0	P	29-MAR-10 20:39	032910C-1
	Silver	495	ug/L	500	ug/L	98.9	90.0 - 110.0	P	29-MAR-10 20:39	032910C-1
	Sodium	9760	ug/L	10000	ug/L	97.6	90.0 - 110.0	P	29-MAR-10 20:39	032910C-1
	Vanadium	499	ug/L	500	ug/L	99.8	90.0 - 110.0	P	29-MAR-10 20:39	032910C-1
	Zinc	478	ug/L	500	ug/L	95.7	90.0 - 110.0	P	29-MAR-10 20:39	032910C-1
CCV07	Mercury	4.95	ug/L	5	ug/L	99.1	80.0 - 120.0	AV	10-MAR-10 13:53	031010S1-4
	Aluminum	5210	ug/L	5000	ug/L	104.3	90.0 - 110.0	P	29-MAR-10 21:03	032910C-1
	Antimony	488	ug/L	500	ug/L	97.6	90.0 - 110.0	P	29-MAR-10 21:03	032910C-1
	Barium	500	ug/L	500	ug/L	100.1	90.0 - 110.0	P	29-MAR-10 21:03	032910C-1
	Cadmium	479	ug/L	500	ug/L	95.8	90.0 - 110.0	P	29-MAR-10 21:03	032910C-1
	Calcium	4930	ug/L	5000	ug/L	98.6	90.0 - 110.0	P	29-MAR-10 21:03	032910C-1
	Chromium	488	ug/L	500	ug/L	97.7	90.0 - 110.0	P	29-MAR-10 21:03	032910C-1
	Cobalt	486	ug/L	500	ug/L	97.2	90.0 - 110.0	P	29-MAR-10 21:03	032910C-1
	Copper	494	ug/L	500	ug/L	98.8	90.0 - 110.0	P	29-MAR-10 21:03	032910C-1
	Iron	4910	ug/L	5000	ug/L	98.2	90.0 - 110.0	P	29-MAR-10 21:03	032910C-1
	Lead	480	ug/L	500	ug/L	96	90.0 - 110.0	P	29-MAR-10 21:03	032910C-1
	Magnesium	5070	ug/L	5000	ug/L	101.4	90.0 - 110.0	P	29-MAR-10 21:03	032910C-1
	Manganese	491	ug/L	500	ug/L	98.1	90.0 - 110.0	P	29-MAR-10 21:03	032910C-1
	Potassium	4790	ug/L	5000	ug/L	95.9	90.0 - 110.0	P	29-MAR-10 21:03	032910C-1
	Silver	496	ug/L	500	ug/L	99.2	90.0 - 110.0	P	29-MAR-10 21:03	032910C-1
	Sodium	9820	ug/L	10000	ug/L	98.3	90.0 - 110.0	P	29-MAR-10 21:03	032910C-1

METALS
-2a-
Initial and Continuing Calibration Verification

SDG No: 10-2093-1

Contract: LANL01004

Lab Code: GEL

Initial Calibration Source: Solutions Plus

Continuing Calibration Source: O2Si

Instrument ID: ICPMS6,MER536,OPTIMA4

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>True Value</u>	<u>Units</u>	<u>% Recovery</u>	<u>Acceptance Window (%R)</u>	<u>M</u>	<u>Analysis Date/Time</u>	<u>Run Number</u>
	Vanadium	499	ug/L	500	ug/L	99.8	90.0 – 110.0	P	29-MAR-10 21:03	032910C-1
	Zinc	478	ug/L	500	ug/L	95.6	90.0 – 110.0	P	29-MAR-10 21:03	032910C-1
CCV08										
	Aluminum	5260	ug/L	5000	ug/L	105.2	90.0 – 110.0	P	29-MAR-10 21:21	032910C-1
	Antimony	490	ug/L	500	ug/L	98	90.0 – 110.0	P	29-MAR-10 21:21	032910C-1
	Barium	503	ug/L	500	ug/L	100.6	90.0 – 110.0	P	29-MAR-10 21:21	032910C-1
	Cadmium	481	ug/L	500	ug/L	96.2	90.0 – 110.0	P	29-MAR-10 21:21	032910C-1
	Calcium	4940	ug/L	5000	ug/L	98.8	90.0 – 110.0	P	29-MAR-10 21:21	032910C-1
	Chromium	490	ug/L	500	ug/L	98.1	90.0 – 110.0	P	29-MAR-10 21:21	032910C-1
	Cobalt	488	ug/L	500	ug/L	97.7	90.0 – 110.0	P	29-MAR-10 21:21	032910C-1
	Copper	494	ug/L	500	ug/L	98.9	90.0 – 110.0	P	29-MAR-10 21:21	032910C-1
	Iron	4930	ug/L	5000	ug/L	98.6	90.0 – 110.0	P	29-MAR-10 21:21	032910C-1
	Lead	479	ug/L	500	ug/L	95.8	90.0 – 110.0	P	29-MAR-10 21:21	032910C-1
	Magnesium	5090	ug/L	5000	ug/L	101.7	90.0 – 110.0	P	29-MAR-10 21:21	032910C-1
	Manganese	492	ug/L	500	ug/L	98.4	90.0 – 110.0	P	29-MAR-10 21:21	032910C-1
	Potassium	4820	ug/L	5000	ug/L	96.5	90.0 – 110.0	P	29-MAR-10 21:21	032910C-1
	Silver	496	ug/L	500	ug/L	99.2	90.0 – 110.0	P	29-MAR-10 21:21	032910C-1
	Sodium	9850	ug/L	10000	ug/L	98.5	90.0 – 110.0	P	29-MAR-10 21:21	032910C-1
	Vanadium	501	ug/L	500	ug/L	100.2	90.0 – 110.0	P	29-MAR-10 21:21	032910C-1
	Zinc	480	ug/L	500	ug/L	96.1	90.0 – 110.0	P	29-MAR-10 21:21	032910C-1
CCV09										
	Aluminum	5260	ug/L	5000	ug/L	105.1	90.0 – 110.0	P	29-MAR-10 21:41	032910C-1
	Antimony	488	ug/L	500	ug/L	97.7	90.0 – 110.0	P	29-MAR-10 21:41	032910C-1
	Barium	501	ug/L	500	ug/L	100.2	90.0 – 110.0	P	29-MAR-10 21:41	032910C-1
	Cadmium	480	ug/L	500	ug/L	96.1	90.0 – 110.0	P	29-MAR-10 21:41	032910C-1
	Calcium	4940	ug/L	5000	ug/L	98.8	90.0 – 110.0	P	29-MAR-10 21:41	032910C-1
	Chromium	488	ug/L	500	ug/L	97.7	90.0 – 110.0	P	29-MAR-10 21:41	032910C-1
	Cobalt	486	ug/L	500	ug/L	97.2	90.0 – 110.0	P	29-MAR-10 21:41	032910C-1
	Copper	493	ug/L	500	ug/L	98.6	90.0 – 110.0	P	29-MAR-10 21:41	032910C-1
	Iron	4940	ug/L	5000	ug/L	98.7	90.0 – 110.0	P	29-MAR-10 21:41	032910C-1

SW846

METALS
-2a-
Initial and Continuing Calibration Verification

SDG No: 10-2093-1

Contract: LANL01004

Lab Code: GEL

Initial Calibration Source: Solutions Plus

Continuing Calibration Source: O2Si

Instrument ID: ICPMS6,MER536,OPTIMA4

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>True Value</u>	<u>Units</u>	<u>% Recovery</u>	<u>Acceptance Window (%R)</u>	<u>M</u>	<u>Analysis Date/Time</u>	<u>Run Number</u>
	Lead	480	ug/L	500	ug/L	96	90.0 – 110.0	P	29-MAR-10 21:41	032910C-1
	Magnesium	5080	ug/L	5000	ug/L	101.6	90.0 – 110.0	P	29-MAR-10 21:41	032910C-1
	Manganese	490	ug/L	500	ug/L	98	90.0 – 110.0	P	29-MAR-10 21:41	032910C-1
	Potassium	4830	ug/L	5000	ug/L	96.5	90.0 – 110.0	P	29-MAR-10 21:41	032910C-1
	Silver	494	ug/L	500	ug/L	98.8	90.0 – 110.0	P	29-MAR-10 21:41	032910C-1
	Sodium	9870	ug/L	10000	ug/L	98.7	90.0 – 110.0	P	29-MAR-10 21:41	032910C-1
	Vanadium	500	ug/L	500	ug/L	99.9	90.0 – 110.0	P	29-MAR-10 21:41	032910C-1
	Zinc	479	ug/L	500	ug/L	95.7	90.0 – 110.0	P	29-MAR-10 21:41	032910C-1
CCV10	Aluminum	5280	ug/L	5000	ug/L	105.6	90.0 – 110.0	P	29-MAR-10 22:01	032910C-1
	Antimony	487	ug/L	500	ug/L	97.4	90.0 – 110.0	P	29-MAR-10 22:01	032910C-1
	Barium	503	ug/L	500	ug/L	100.6	90.0 – 110.0	P	29-MAR-10 22:01	032910C-1
	Cadmium	482	ug/L	500	ug/L	96.4	90.0 – 110.0	P	29-MAR-10 22:01	032910C-1
	Calcium	4950	ug/L	5000	ug/L	99	90.0 – 110.0	P	29-MAR-10 22:01	032910C-1
	Chromium	489	ug/L	500	ug/L	97.8	90.0 – 110.0	P	29-MAR-10 22:01	032910C-1
	Cobalt	488	ug/L	500	ug/L	97.7	90.0 – 110.0	P	29-MAR-10 22:01	032910C-1
	Copper	496	ug/L	500	ug/L	99.3	90.0 – 110.0	P	29-MAR-10 22:01	032910C-1
	Iron	4940	ug/L	5000	ug/L	98.9	90.0 – 110.0	P	29-MAR-10 22:01	032910C-1
	Lead	480	ug/L	500	ug/L	96	90.0 – 110.0	P	29-MAR-10 22:01	032910C-1
	Magnesium	5110	ug/L	5000	ug/L	102.2	90.0 – 110.0	P	29-MAR-10 22:01	032910C-1
	Manganese	492	ug/L	500	ug/L	98.3	90.0 – 110.0	P	29-MAR-10 22:01	032910C-1
	Potassium	4900	ug/L	5000	ug/L	98	90.0 – 110.0	P	29-MAR-10 22:01	032910C-1
	Silver	494	ug/L	500	ug/L	98.9	90.0 – 110.0	P	29-MAR-10 22:01	032910C-1
	Sodium	9910	ug/L	10000	ug/L	99.1	90.0 – 110.0	P	29-MAR-10 22:01	032910C-1
	Vanadium	500	ug/L	500	ug/L	99.9	90.0 – 110.0	P	29-MAR-10 22:01	032910C-1
	Zinc	482	ug/L	500	ug/L	96.5	90.0 – 110.0	P	29-MAR-10 22:01	032910C-1
CCV11	Aluminum	5250	ug/L	5000	ug/L	104.9	90.0 – 110.0	P	29-MAR-10 22:19	032910C-1
	Antimony	495	ug/L	500	ug/L	98.9	90.0 – 110.0	P	29-MAR-10 22:19	032910C-1
	Barium	505	ug/L	500	ug/L	101	90.0 – 110.0	P	29-MAR-10 22:19	032910C-1

METALS
-2a-
Initial and Continuing Calibration Verification

SDG No: 10-2093-1

Contract: LANL01004

Lab Code: GEL

Initial Calibration Source: Solutions Plus

Continuing Calibration Source: O2Si

Instrument ID: ICPMS6,MER536,OPTIMA4

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>True Value</u>	<u>Units</u>	<u>% Recovery</u>	<u>Acceptance Window (%R)</u>	<u>M</u>	<u>Analysis Date/Time</u>	<u>Run Number</u>
	Cadmium	482	ug/L	500	ug/L	96.4	90.0 – 110.0	P	29-MAR-10 22:19	032910C-1
	Calcium	4950	ug/L	5000	ug/L	99	90.0 – 110.0	P	29-MAR-10 22:19	032910C-1
	Chromium	491	ug/L	500	ug/L	98.3	90.0 – 110.0	P	29-MAR-10 22:19	032910C-1
	Cobalt	489	ug/L	500	ug/L	97.8	90.0 – 110.0	P	29-MAR-10 22:19	032910C-1
	Copper	496	ug/L	500	ug/L	99.3	90.0 – 110.0	P	29-MAR-10 22:19	032910C-1
	Iron	4940	ug/L	5000	ug/L	98.8	90.0 – 110.0	P	29-MAR-10 22:19	032910C-1
	Lead	487	ug/L	500	ug/L	97.4	90.0 – 110.0	P	29-MAR-10 22:19	032910C-1
	Magnesium	5120	ug/L	5000	ug/L	102.3	90.0 – 110.0	P	29-MAR-10 22:19	032910C-1
	Manganese	493	ug/L	500	ug/L	98.6	90.0 – 110.0	P	29-MAR-10 22:19	032910C-1
	Potassium	4850	ug/L	5000	ug/L	96.9	90.0 – 110.0	P	29-MAR-10 22:19	032910C-1
	Silver	497	ug/L	500	ug/L	99.4	90.0 – 110.0	P	29-MAR-10 22:19	032910C-1
	Sodium	9930	ug/L	10000	ug/L	99.3	90.0 – 110.0	P	29-MAR-10 22:19	032910C-1
	Vanadium	502	ug/L	500	ug/L	100.4	90.0 – 110.0	P	29-MAR-10 22:19	032910C-1
	Zinc	481	ug/L	500	ug/L	96.3	90.0 – 110.0	P	29-MAR-10 22:19	032910C-1
CCV12	Aluminum	5270	ug/L	5000	ug/L	105.5	90.0 – 110.0	P	29-MAR-10 22:42	032910C-1
	Antimony	490	ug/L	500	ug/L	97.9	90.0 – 110.0	P	29-MAR-10 22:42	032910C-1
	Barium	505	ug/L	500	ug/L	101	90.0 – 110.0	P	29-MAR-10 22:42	032910C-1
	Cadmium	482	ug/L	500	ug/L	96.4	90.0 – 110.0	P	29-MAR-10 22:42	032910C-1
	Calcium	4940	ug/L	5000	ug/L	98.8	90.0 – 110.0	P	29-MAR-10 22:42	032910C-1
	Chromium	490	ug/L	500	ug/L	98.1	90.0 – 110.0	P	29-MAR-10 22:42	032910C-1
	Cobalt	488	ug/L	500	ug/L	97.5	90.0 – 110.0	P	29-MAR-10 22:42	032910C-1
	Copper	497	ug/L	500	ug/L	99.4	90.0 – 110.0	P	29-MAR-10 22:42	032910C-1
	Iron	4940	ug/L	5000	ug/L	98.9	90.0 – 110.0	P	29-MAR-10 22:42	032910C-1
	Lead	480	ug/L	500	ug/L	96	90.0 – 110.0	P	29-MAR-10 22:42	032910C-1
	Magnesium	5120	ug/L	5000	ug/L	102.4	90.0 – 110.0	P	29-MAR-10 22:42	032910C-1
	Manganese	493	ug/L	500	ug/L	98.6	90.0 – 110.0	P	29-MAR-10 22:42	032910C-1
	Potassium	4860	ug/L	5000	ug/L	97.2	90.0 – 110.0	P	29-MAR-10 22:42	032910C-1
	Silver	497	ug/L	500	ug/L	99.3	90.0 – 110.0	P	29-MAR-10 22:42	032910C-1
	Sodium	9910	ug/L	10000	ug/L	99.1	90.0 – 110.0	P	29-MAR-10 22:42	032910C-1

METALS
-2a-
Initial and Continuing Calibration Verification

SDG No: 10-2093-1

Contract: LANL01004

Lab Code: GEL

Initial Calibration Source: Solutions Plus

Continuing Calibration Source: O2Si

Instrument ID: ICPMS6,MER536,OPTIMA4

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>True Value</u>	<u>Units</u>	<u>% Recovery</u>	<u>Acceptance Window (%R)</u>	<u>M</u>	<u>Analysis Date/Time</u>	<u>Run Number</u>
	Vanadium	502	ug/L	500	ug/L	100.5	90.0 - 110.0	P	29-MAR-10 22:42	032910C-1
	Zinc	481	ug/L	500	ug/L	96.2	90.0 - 110.0	P	29-MAR-10 22:42	032910C-1
CCV13										
	Aluminum	5270	ug/L	5000	ug/L	105.4	90.0 - 110.0	P	29-MAR-10 22:59	032910C-1
	Antimony	496	ug/L	500	ug/L	99.2	90.0 - 110.0	P	29-MAR-10 22:59	032910C-1
	Barium	507	ug/L	500	ug/L	101.4	90.0 - 110.0	P	29-MAR-10 22:59	032910C-1
	Cadmium	486	ug/L	500	ug/L	97.3	90.0 - 110.0	P	29-MAR-10 22:59	032910C-1
	Calcium	4960	ug/L	5000	ug/L	99.2	90.0 - 110.0	P	29-MAR-10 22:59	032910C-1
	Chromium	493	ug/L	500	ug/L	98.7	90.0 - 110.0	P	29-MAR-10 22:59	032910C-1
	Cobalt	491	ug/L	500	ug/L	98.2	90.0 - 110.0	P	29-MAR-10 22:59	032910C-1
	Copper	498	ug/L	500	ug/L	99.6	90.0 - 110.0	P	29-MAR-10 22:59	032910C-1
	Iron	4970	ug/L	5000	ug/L	99.5	90.0 - 110.0	P	29-MAR-10 22:59	032910C-1
	Lead	487	ug/L	500	ug/L	97.4	90.0 - 110.0	P	29-MAR-10 22:59	032910C-1
	Magnesium	5160	ug/L	5000	ug/L	103.2	90.0 - 110.0	P	29-MAR-10 22:59	032910C-1
	Manganese	495	ug/L	500	ug/L	99	90.0 - 110.0	P	29-MAR-10 22:59	032910C-1
	Potassium	4920	ug/L	5000	ug/L	98.4	90.0 - 110.0	P	29-MAR-10 22:59	032910C-1
	Silver	499	ug/L	500	ug/L	99.9	90.0 - 110.0	P	29-MAR-10 22:59	032910C-1
	Sodium	9930	ug/L	10000	ug/L	99.3	90.0 - 110.0	P	29-MAR-10 22:59	032910C-1
	Vanadium	504	ug/L	500	ug/L	100.9	90.0 - 110.0	P	29-MAR-10 22:59	032910C-1
	Zinc	485	ug/L	500	ug/L	97	90.0 - 110.0	P	29-MAR-10 22:59	032910C-1
CCV14										
	Aluminum	5300	ug/L	5000	ug/L	106	90.0 - 110.0	P	29-MAR-10 23:19	032910C-1
	Antimony	493	ug/L	500	ug/L	98.6	90.0 - 110.0	P	29-MAR-10 23:19	032910C-1
	Barium	505	ug/L	500	ug/L	101	90.0 - 110.0	P	29-MAR-10 23:19	032910C-1
	Cadmium	482	ug/L	500	ug/L	96.4	90.0 - 110.0	P	29-MAR-10 23:19	032910C-1
	Calcium	4980	ug/L	5000	ug/L	99.5	90.0 - 110.0	P	29-MAR-10 23:19	032910C-1
	Chromium	491	ug/L	500	ug/L	98.2	90.0 - 110.0	P	29-MAR-10 23:19	032910C-1
	Cobalt	489	ug/L	500	ug/L	97.8	90.0 - 110.0	P	29-MAR-10 23:19	032910C-1
	Copper	496	ug/L	500	ug/L	99.2	90.0 - 110.0	P	29-MAR-10 23:19	032910C-1
	Iron	4970	ug/L	5000	ug/L	99.4	90.0 - 110.0	P	29-MAR-10 23:19	032910C-1

METALS

-2a-

Initial and Continuing Calibration Verification

SDG No: 10-2093-1

Contract: LANL01004

Lab Code: GEL

Initial Calibration Source: Solutions Plus

Continuing Calibration Source: O2Si

Instrument ID: ICPMS6,MER536,OPTIMA4

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>True Value</u>	<u>Units</u>	<u>% Recovery</u>	<u>Acceptance Window (%R)</u>	<u>M</u>	<u>Analysis Date/Time</u>	<u>Run Number</u>
	Lead	483	ug/L	500	ug/L	96.6	90.0 – 110.0	P	29-MAR-10 23:19	032910C-1
	Magnesium	5130	ug/L	5000	ug/L	102.7	90.0 – 110.0	P	29-MAR-10 23:19	032910C-1
	Manganese	493	ug/L	500	ug/L	98.6	90.0 – 110.0	P	29-MAR-10 23:19	032910C-1
	Potassium	4970	ug/L	5000	ug/L	99.4	90.0 – 110.0	P	29-MAR-10 23:19	032910C-1
	Silver	496	ug/L	500	ug/L	99.2	90.0 – 110.0	P	29-MAR-10 23:19	032910C-1
	Sodium	9950	ug/L	10000	ug/L	99.5	90.0 – 110.0	P	29-MAR-10 23:19	032910C-1
	Vanadium	502	ug/L	500	ug/L	100.5	90.0 – 110.0	P	29-MAR-10 23:19	032910C-1
	Zinc	482	ug/L	500	ug/L	96.5	90.0 – 110.0	P	29-MAR-10 23:19	032910C-1
CCV15	Aluminum	5280	ug/L	5000	ug/L	105.6	90.0 – 110.0	P	29-MAR-10 23:38	032910C-1
	Antimony	490	ug/L	500	ug/L	98	90.0 – 110.0	P	29-MAR-10 23:38	032910C-1
	Barium	505	ug/L	500	ug/L	101.1	90.0 – 110.0	P	29-MAR-10 23:38	032910C-1
	Cadmium	483	ug/L	500	ug/L	96.7	90.0 – 110.0	P	29-MAR-10 23:38	032910C-1
	Calcium	4930	ug/L	5000	ug/L	98.5	90.0 – 110.0	P	29-MAR-10 23:38	032910C-1
	Chromium	491	ug/L	500	ug/L	98.1	90.0 – 110.0	P	29-MAR-10 23:38	032910C-1
	Cobalt	490	ug/L	500	ug/L	98	90.0 – 110.0	P	29-MAR-10 23:38	032910C-1
	Copper	495	ug/L	500	ug/L	99.1	90.0 – 110.0	P	29-MAR-10 23:38	032910C-1
	Iron	4950	ug/L	5000	ug/L	98.9	90.0 – 110.0	P	29-MAR-10 23:38	032910C-1
	Lead	481	ug/L	500	ug/L	96.2	90.0 – 110.0	P	29-MAR-10 23:38	032910C-1
	Magnesium	5080	ug/L	5000	ug/L	101.7	90.0 – 110.0	P	29-MAR-10 23:38	032910C-1
	Manganese	493	ug/L	500	ug/L	98.7	90.0 – 110.0	P	29-MAR-10 23:38	032910C-1
	Potassium	4890	ug/L	5000	ug/L	97.8	90.0 – 110.0	P	29-MAR-10 23:38	032910C-1
	Silver	497	ug/L	500	ug/L	99.5	90.0 – 110.0	P	29-MAR-10 23:38	032910C-1
	Sodium	9880	ug/L	10000	ug/L	98.8	90.0 – 110.0	P	29-MAR-10 23:38	032910C-1
	Vanadium	503	ug/L	500	ug/L	100.6	90.0 – 110.0	P	29-MAR-10 23:38	032910C-1
	Zinc	482	ug/L	500	ug/L	96.4	90.0 – 110.0	P	29-MAR-10 23:38	032910C-1

METALS
-2b-
CRDL Standard for AA & ICP

SDG No: 10-2093-1

Contract: LANL01004

Lab Code: GEL

AA CRDL Standard Source: SPEX

ICP CRDL Standard Source Solutions Plus

Instrument ID: ICPMS6,MER536,OPTIMA4

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>True Value</u>	<u>Units</u>	<u>% Recovery</u>	<u>Advisory Limits (%R)</u>	<u>M</u>	<u>Analysis Date/Time</u>	<u>Run Number</u>
CRDL01										
	Mercury	.21	ug/L	.2	ug/L	105.2	70.0 – 130.0	AV	10-MAR-10 11:41	031010S1-4
	Nickel	2.3	ug/L	2	ug/L	114.8	70.0 – 130.0	MS	24-MAR-10 16:18	100323-2
	Thallium	1.16	ug/L	1	ug/L	115.9	70.0 – 130.0	MS	24-MAR-10 16:18	100323-2
	Arsenic	5.68	ug/L	5	ug/L	113.6	70.0 – 130.0	MS	24-MAR-10 16:18	100323-2
	Beryllium	.591	ug/L	.5	ug/L	118.2	70.0 – 130.0	MS	24-MAR-10 16:18	100323-2
	Selenium	5.47	ug/L	5	ug/L	109.5	70.0 – 130.0	MS	24-MAR-10 16:18	100323-2
	Uranium	.218	ug/L	.2	ug/L	109	70.0 – 130.0	MS	25-MAR-10 23:55	100325-3
PQL01										
	Aluminum	201	ug/L	200	ug/L	100.4	70.0 – 130.0	P	29-MAR-10 18:40	032910C-1
	Iron	103	ug/L	100	ug/L	103.4	70.0 – 130.0	P	29-MAR-10 18:40	032910C-1
	Lead	9.72	ug/L	10	ug/L	97.2	70.0 – 130.0	P	29-MAR-10 18:40	032910C-1
	Magnesium	303	ug/L	300	ug/L	101.1	70.0 – 130.0	P	29-MAR-10 18:40	032910C-1
	Manganese	10.3	ug/L	10	ug/L	103.4	70.0 – 130.0	P	29-MAR-10 18:40	032910C-1
	Potassium	170	ug/L	150	ug/L	113.4	70.0 – 130.0	P	29-MAR-10 18:40	032910C-1
	Silver	4.62	ug/L	5	ug/L	92.4	70.0 – 130.0	P	29-MAR-10 18:40	032910C-1
	Sodium	260	ug/L	300	ug/L	86.8	70.0 – 130.0	P	29-MAR-10 18:40	032910C-1
	Antimony	8.94	ug/L	10	ug/L	89.4	70.0 – 130.0	P	29-MAR-10 18:40	032910C-1
	Barium	5.16	ug/L	5	ug/L	103.1	70.0 – 130.0	P	29-MAR-10 18:40	032910C-1
	Cadmium	4.98	ug/L	5	ug/L	99.6	70.0 – 130.0	P	29-MAR-10 18:40	032910C-1
	Chromium	4.84	ug/L	5	ug/L	96.8	70.0 – 130.0	P	29-MAR-10 18:40	032910C-1
	Cobalt	5.14	ug/L	5	ug/L	102.7	70.0 – 130.0	P	29-MAR-10 18:40	032910C-1
	Copper	10.1	ug/L	10	ug/L	101.4	70.0 – 130.0	P	29-MAR-10 18:40	032910C-1
	Vanadium	4.53	ug/L	5	ug/L	90.6	70.0 – 130.0	P	29-MAR-10 18:40	032910C-1
	Zinc	9.92	ug/L	10	ug/L	99.2	70.0 – 130.0	P	29-MAR-10 18:40	032910C-1
	Calcium	204	ug/L	200	ug/L	101.8	70.0 – 130.0	P	29-MAR-10 18:40	032910C-1

Metals
-3a-
Initial and Continuing Calibration Blank Summary

SDG No.: 10-2093-1

Contract: LANL01004

Lab Code: GEL

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u> <u>ug/L</u>	<u>Acceptance</u>	<u>Conc</u> <u>Qual</u>	<u>MDL</u>	<u>RDL</u>	<u>Matrix</u>	<u>M</u>	<u>Analysis</u> <u>Date/Time</u>	<u>Run</u>
ICB01	Mercury	-0.095	+/-2	J	0.068	0.2	SOL	AV	10-MAR-10 11:39	031010S1-4
	Arsenic	1.0	+/-5	U	1.0	5.0	SOL	MS	24-MAR-10 16:14	100323-2
	Beryllium	0.1	+/-5	U	0.1	0.5	SOL	MS	24-MAR-10 16:14	100323-2
	Nickel	0.5	+/-2	U	0.5	2.0	SOL	MS	24-MAR-10 16:14	100323-2
	Selenium	2.5	+/-5	U	2.5	5.0	SOL	MS	24-MAR-10 16:14	100323-2
	Thallium	0.3	+/-1	U	0.3	1.0	SOL	MS	24-MAR-10 16:14	100323-2
	Uranium	0.066	+/-2	U	0.066	0.2	SOL	MS	25-MAR-10 23:52	100325-3
	Aluminum	68.0	+/-200	U	68.0	200	SOL	P	29-MAR-10 18:37	032910C-1
	Antimony	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 18:37	032910C-1
	Barium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 18:37	032910C-1
	Cadmium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 18:37	032910C-1
	Calcium	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 18:37	032910C-1
	Chromium	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 18:37	032910C-1
	Cobalt	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 18:37	032910C-1
	Copper	3.0	+/-10	U	3.0	10.0	SOL	P	29-MAR-10 18:37	032910C-1
	Iron	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 18:37	032910C-1
	Lead	2.5	+/-10	U	2.5	10.0	SOL	P	29-MAR-10 18:37	032910C-1
	Magnesium	85.0	+/-300	U	85.0	300	SOL	P	29-MAR-10 18:37	032910C-1
	Manganese	2.0	+/-10	U	2.0	10.0	SOL	P	29-MAR-10 18:37	032910C-1
	Potassium	64.0	+/-250	U	64.0	250	SOL	P	29-MAR-10 18:37	032910C-1
	Silver	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 18:37	032910C-1
	Sodium	70.0	+/-250	U	70.0	250	SOL	P	29-MAR-10 18:37	032910C-1
	Vanadium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 18:37	032910C-1
	Zinc	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 18:37	032910C-1
CCB01	Mercury	0.068	+/-2	U	0.068	0.2	SOL	AV	10-MAR-10 11:45	031010S1-4
	Arsenic	1.0	+/-5	U	1.0	5.0	SOL	MS	24-MAR-10 16:34	100323-2
	Beryllium	0.1	+/-5	U	0.1	0.5	SOL	MS	24-MAR-10 16:34	100323-2
	Nickel	0.5	+/-2	U	0.5	2.0	SOL	MS	24-MAR-10 16:34	100323-2
	Selenium	2.5	+/-5	U	2.5	5.0	SOL	MS	24-MAR-10 16:34	100323-2
	Thallium	0.3	+/-1	U	0.3	1.0	SOL	MS	24-MAR-10 16:34	100323-2

Metals
-3a-
Initial and Continuing Calibration Blank Summary

SDG No.: 10-2093-1

Contract: LANL01004

Lab Code: GEL

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u> <u>ug/L</u>	<u>Acceptance</u>	<u>Conc</u> <u>Qual</u>	<u>MDL</u>	<u>RDL</u>	<u>Matrix</u>	<u>M</u>	<u>Analysis</u> <u>Date/Time</u>	<u>Run</u>
	Uranium	0.066	+/-2	U	0.066	0.2	SOL	MS	26-MAR-10 00:07	100325-3
	Aluminum	68.0	+/-200	U	68.0	200	SOL	P	29-MAR-10 18:51	032910C-1
	Antimony	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 18:51	032910C-1
	Barium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 18:51	032910C-1
	Cadmium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 18:51	032910C-1
	Calcium	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 18:51	032910C-1
	Chromium	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 18:51	032910C-1
	Cobalt	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 18:51	032910C-1
	Copper	3.0	+/-10	U	3.0	10.0	SOL	P	29-MAR-10 18:51	032910C-1
	Iron	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 18:51	032910C-1
	Lead	2.5	+/-10	U	2.5	10.0	SOL	P	29-MAR-10 18:51	032910C-1
	Magnesium	85.0	+/-300	U	85.0	300	SOL	P	29-MAR-10 18:51	032910C-1
	Manganese	2.0	+/-10	U	2.0	10.0	SOL	P	29-MAR-10 18:51	032910C-1
	Potassium	152.39	+/-250	J	64.0	250	SOL	P	29-MAR-10 18:51	032910C-1
	Silver	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 18:51	032910C-1
	Sodium	70.0	+/-250	U	70.0	250	SOL	P	29-MAR-10 18:51	032910C-1
	Vanadium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 18:51	032910C-1
	Zinc	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 18:51	032910C-1
CCB02										
	Mercury	0.068	+/-2	U	0.068	0.2	SOL	AV	10-MAR-10 12:09	031010S1-4
	Arsenic	1.0	+/-5	U	1.0	5.0	SOL	MS	24-MAR-10 16:51	100323-2
	Beryllium	0.1	+/-5	U	0.1	0.5	SOL	MS	24-MAR-10 16:51	100323-2
	Nickel	0.5	+/-2	U	0.5	2.0	SOL	MS	24-MAR-10 16:51	100323-2
	Selenium	2.5	+/-5	U	2.5	5.0	SOL	MS	24-MAR-10 16:51	100323-2
	Thallium	0.3	+/-1	U	0.3	1.0	SOL	MS	24-MAR-10 16:51	100323-2
	Uranium	0.066	+/-2	U	0.066	0.2	SOL	MS	26-MAR-10 00:35	100325-3
	Aluminum	68.0	+/-200	U	68.0	200	SOL	P	29-MAR-10 18:59	032910C-1
	Antimony	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 18:59	032910C-1
	Barium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 18:59	032910C-1
	Cadmium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 18:59	032910C-1
	Calcium	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 18:59	032910C-1

SW846

Metals
-3a-
Initial and Continuing Calibration Blank Summary

SDG No.: 10-2093-1

Contract: LANL01004

Lab Code: GEL

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u> <u>ug/L</u>	<u>Acceptance</u>	<u>Conc</u> <u>Qual</u>	<u>MDL</u>	<u>RDL</u>	<u>Matrix</u>	<u>M</u>	<u>Analysis</u> <u>Date/Time</u>	<u>Run</u>
	Chromium	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 18:59	032910C-1
	Cobalt	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 18:59	032910C-1
	Copper	3.0	+/-10	U	3.0	10.0	SOL	P	29-MAR-10 18:59	032910C-1
	Iron	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 18:59	032910C-1
	Lead	2.5	+/-10	U	2.5	10.0	SOL	P	29-MAR-10 18:59	032910C-1
	Magnesium	85.0	+/-300	U	85.0	300	SOL	P	29-MAR-10 18:59	032910C-1
	Manganese	2.0	+/-10	U	2.0	10.0	SOL	P	29-MAR-10 18:59	032910C-1
	Potassium	64.0	+/-250	U	64.0	250	SOL	P	29-MAR-10 18:59	032910C-1
	Silver	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 18:59	032910C-1
	Sodium	70.0	+/-250	U	70.0	250	SOL	P	29-MAR-10 18:59	032910C-1
	Vanadium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 18:59	032910C-1
	Zinc	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 18:59	032910C-1
CCB03	Mercury	-0.14	+/-2	J	0.068	0.2	SOL	AV	10-MAR-10 12:33	031010S1-4
	Arsenic	1.0	+/-5	U	1.0	5.0	SOL	MS	24-MAR-10 17:31	100323-2
	Beryllium	0.1	+/-5	U	0.1	0.5	SOL	MS	24-MAR-10 17:31	100323-2
	Nickel	0.5	+/-2	U	0.5	2.0	SOL	MS	24-MAR-10 17:31	100323-2
	Selenium	2.5	+/-5	U	2.5	5.0	SOL	MS	24-MAR-10 17:31	100323-2
	Thallium	0.3	+/-1	U	0.3	1.0	SOL	MS	24-MAR-10 17:31	100323-2
	Uranium	0.066	+/-2	U	0.066	0.2	SOL	MS	26-MAR-10 01:05	100325-3
	Aluminum	68.0	+/-200	U	68.0	200	SOL	P	29-MAR-10 19:33	032910C-1
	Antimony	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 19:33	032910C-1
	Barium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 19:33	032910C-1
	Cadmium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 19:33	032910C-1
	Calcium	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 19:33	032910C-1
	Chromium	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 19:33	032910C-1
	Cobalt	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 19:33	032910C-1
	Copper	3.0	+/-10	U	3.0	10.0	SOL	P	29-MAR-10 19:33	032910C-1
	Iron	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 19:33	032910C-1
	Lead	2.5	+/-10	U	2.5	10.0	SOL	P	29-MAR-10 19:33	032910C-1
	Magnesium	85.0	+/-300	U	85.0	300	SOL	P	29-MAR-10 19:33	032910C-1

SW846

Metals
-3a-
Initial and Continuing Calibration Blank Summary

SDG No.: 10-2093-1

Contract: LANL01004

Lab Code: GEL

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u> <u>ug/L</u>	<u>Acceptance</u>	<u>Conc</u> <u>Qual</u>	<u>MDL</u>	<u>RDL</u>	<u>Matrix</u>	<u>M</u>	<u>Analysis</u> <u>Date/Time</u>	<u>Run</u>
	Manganese	2.0	+/-10	U	2.0	10.0	SOL	P	29-MAR-10 19:33	032910C-1
	Potassium	64.0	+/-250	U	64.0	250	SOL	P	29-MAR-10 19:33	032910C-1
	Silver	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 19:33	032910C-1
	Sodium	70.0	+/-250	U	70.0	250	SOL	P	29-MAR-10 19:33	032910C-1
	Vanadium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 19:33	032910C-1
	Zinc	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 19:33	032910C-1
CCB04	Mercury	-0.109	+/-2	J	0.068	0.2	SOL	AV	10-MAR-10 12:56	031010S1-4
	Arsenic	1.0	+/-5	U	1.0	5.0	SOL	MS	24-MAR-10 18:23	100323-2
	Beryllium	0.1	+/-5	U	0.1	0.5	SOL	MS	24-MAR-10 18:23	100323-2
	Nickel	0.5	+/-2	U	0.5	2.0	SOL	MS	24-MAR-10 18:23	100323-2
	Selenium	2.5	+/-5	U	2.5	5.0	SOL	MS	24-MAR-10 18:23	100323-2
	Thallium	0.3	+/-1	U	0.3	1.0	SOL	MS	24-MAR-10 18:23	100323-2
	Uranium	0.066	+/-2	U	0.066	0.2	SOL	MS	26-MAR-10 01:39	100325-3
	Aluminum	68.0	+/-200	U	68.0	200	SOL	P	29-MAR-10 19:54	032910C-1
	Antimony	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 19:54	032910C-1
	Barium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 19:54	032910C-1
	Cadmium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 19:54	032910C-1
	Calcium	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 19:54	032910C-1
	Chromium	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 19:54	032910C-1
	Cobalt	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 19:54	032910C-1
	Copper	3.0	+/-10	U	3.0	10.0	SOL	P	29-MAR-10 19:54	032910C-1
	Iron	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 19:54	032910C-1
	Lead	2.5	+/-10	U	2.5	10.0	SOL	P	29-MAR-10 19:54	032910C-1
	Magnesium	85.0	+/-300	U	85.0	300	SOL	P	29-MAR-10 19:54	032910C-1
	Manganese	2.0	+/-10	U	2.0	10.0	SOL	P	29-MAR-10 19:54	032910C-1
	Potassium	64.0	+/-250	U	64.0	250	SOL	P	29-MAR-10 19:54	032910C-1
	Silver	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 19:54	032910C-1
	Sodium	70.0	+/-250	U	70.0	250	SOL	P	29-MAR-10 19:54	032910C-1
	Vanadium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 19:54	032910C-1
	Zinc	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 19:54	032910C-1

SW846

Metals
-3a-
Initial and Continuing Calibration Blank Summary

SDG No.: 10-2093-1

Contract: LANL01004

Lab Code: GEL

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u> <u>ug/L</u>	<u>Acceptance</u>	<u>Conc</u> <u>Qual</u>	<u>MDL</u>	<u>RDL</u>	<u>Matrix</u>	<u>M</u>	<u>Analysis</u> <u>Date/Time</u>	<u>Run</u>
CCB05	Mercury	-0.086	+/-2	J	0.068	0.2	SOL	AV	10-MAR-10 13:08	031010S1-4
	Uranium	0.066	+/-2	U	0.066	0.2	SOL	MS	26-MAR-10 01:58	100325-3
	Aluminum	68.0	+/-200	U	68.0	200	SOL	P	29-MAR-10 20:16	032910C-1
	Antimony	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 20:16	032910C-1
	Barium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 20:16	032910C-1
	Cadmium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 20:16	032910C-1
	Calcium	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 20:16	032910C-1
	Chromium	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 20:16	032910C-1
	Cobalt	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 20:16	032910C-1
	Copper	3.0	+/-10	U	3.0	10.0	SOL	P	29-MAR-10 20:16	032910C-1
	Iron	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 20:16	032910C-1
	Lead	2.5	+/-10	U	2.5	10.0	SOL	P	29-MAR-10 20:16	032910C-1
	Magnesium	85.0	+/-300	U	85.0	300	SOL	P	29-MAR-10 20:16	032910C-1
	Manganese	2.0	+/-10	U	2.0	10.0	SOL	P	29-MAR-10 20:16	032910C-1
	Potassium	64.0	+/-250	U	64.0	250	SOL	P	29-MAR-10 20:16	032910C-1
	Silver	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 20:16	032910C-1
	Sodium	70.0	+/-250	U	70.0	250	SOL	P	29-MAR-10 20:16	032910C-1
	Vanadium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 20:16	032910C-1
	Zinc	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 20:16	032910C-1
CCB06	Mercury	0.068	+/-2	U	0.068	0.2	SOL	AV	10-MAR-10 13:32	031010S1-4
	Aluminum	68.0	+/-200	U	68.0	200	SOL	P	29-MAR-10 20:41	032910C-1
	Antimony	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 20:41	032910C-1
	Barium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 20:41	032910C-1
	Cadmium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 20:41	032910C-1
	Calcium	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 20:41	032910C-1
	Chromium	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 20:41	032910C-1
	Cobalt	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 20:41	032910C-1
	Copper	3.0	+/-10	U	3.0	10.0	SOL	P	29-MAR-10 20:41	032910C-1
	Iron	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 20:41	032910C-1
	Lead	2.5	+/-10	U	2.5	10.0	SOL	P	29-MAR-10 20:41	032910C-1

SW846

Metals
-3a-
Initial and Continuing Calibration Blank Summary

SDG No.: 10-2093-1

Contract: LANL01004

Lab Code: GEL

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u> <u>ug/L</u>	<u>Acceptance</u>	<u>Conc</u> <u>Qual</u>	<u>MDL</u>	<u>RDL</u>	<u>Matrix</u>	<u>M</u>	<u>Analysis</u> <u>Date/Time</u>	<u>Run</u>
	Magnesium	85.0	+/-300	U	85.0	300	SOL	P	29-MAR-10 20:41	032910C-1
	Manganese	2.0	+/-10	U	2.0	10.0	SOL	P	29-MAR-10 20:41	032910C-1
	Potassium	64.0	+/-250	U	64.0	250	SOL	P	29-MAR-10 20:41	032910C-1
	Silver	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 20:41	032910C-1
	Sodium	70.0	+/-250	U	70.0	250	SOL	P	29-MAR-10 20:41	032910C-1
	Vanadium	-1.05	+/-5	J	1.0	5.0	SOL	P	29-MAR-10 20:41	032910C-1
	Zinc	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 20:41	032910C-1
CCB07	Mercury	-0.082	+/-2	J	0.068	0.2	SOL	AV	10-MAR-10 13:55	031010S1-4
	Aluminum	68.0	+/-200	U	68.0	200	SOL	P	29-MAR-10 21:05	032910C-1
	Antimony	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 21:05	032910C-1
	Barium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 21:05	032910C-1
	Cadmium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 21:05	032910C-1
	Calcium	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 21:05	032910C-1
	Chromium	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 21:05	032910C-1
	Cobalt	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 21:05	032910C-1
	Copper	3.0	+/-10	U	3.0	10.0	SOL	P	29-MAR-10 21:05	032910C-1
	Iron	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 21:05	032910C-1
	Lead	2.5	+/-10	U	2.5	10.0	SOL	P	29-MAR-10 21:05	032910C-1
	Magnesium	85.0	+/-300	U	85.0	300	SOL	P	29-MAR-10 21:05	032910C-1
	Manganese	2.0	+/-10	U	2.0	10.0	SOL	P	29-MAR-10 21:05	032910C-1
	Potassium	64.0	+/-250	U	64.0	250	SOL	P	29-MAR-10 21:05	032910C-1
	Silver	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 21:05	032910C-1
	Sodium	70.0	+/-250	U	70.0	250	SOL	P	29-MAR-10 21:05	032910C-1
	Vanadium	-1.02	+/-5	J	1.0	5.0	SOL	P	29-MAR-10 21:05	032910C-1
	Zinc	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 21:05	032910C-1
CCB08	Aluminum	68.0	+/-200	U	68.0	200	SOL	P	29-MAR-10 21:23	032910C-1
	Antimony	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 21:23	032910C-1
	Barium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 21:23	032910C-1
	Cadmium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 21:23	032910C-1

Metals
-3a-
Initial and Continuing Calibration Blank Summary

SDG No.: 10-2093-1

Contract: LANL01004

Lab Code: GEL

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u> <u>ng/L</u>	<u>Acceptance</u>	<u>Conc</u> <u>Qual</u>	<u>MDL</u>	<u>RDL</u>	<u>Matrix</u>	<u>M</u>	<u>Analysis</u> <u>Date/Time</u>	<u>Run</u>
	Calcium	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 21:23	032910C-1
	Chromium	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 21:23	032910C-1
	Cobalt	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 21:23	032910C-1
	Copper	3.0	+/-10	U	3.0	10.0	SOL	P	29-MAR-10 21:23	032910C-1
	Iron	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 21:23	032910C-1
	Lead	2.5	+/-10	U	2.5	10.0	SOL	P	29-MAR-10 21:23	032910C-1
	Magnesium	85.0	+/-300	U	85.0	300	SOL	P	29-MAR-10 21:23	032910C-1
	Manganese	2.0	+/-10	U	2.0	10.0	SOL	P	29-MAR-10 21:23	032910C-1
	Potassium	64.0	+/-250	U	64.0	250	SOL	P	29-MAR-10 21:23	032910C-1
	Silver	1.24	+/-5	J	1.0	5.0	SOL	P	29-MAR-10 21:23	032910C-1
	Sodium	70.0	+/-250	U	70.0	250	SOL	P	29-MAR-10 21:23	032910C-1
	Vanadium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 21:23	032910C-1
	Zinc	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 21:23	032910C-1
CCB09	Aluminum	68.0	+/-200	U	68.0	200	SOL	P	29-MAR-10 21:43	032910C-1
	Antimony	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 21:43	032910C-1
	Barium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 21:43	032910C-1
	Cadmium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 21:43	032910C-1
	Calcium	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 21:43	032910C-1
	Chromium	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 21:43	032910C-1
	Cobalt	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 21:43	032910C-1
	Copper	3.0	+/-10	U	3.0	10.0	SOL	P	29-MAR-10 21:43	032910C-1
	Iron	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 21:43	032910C-1
	Lead	2.5	+/-10	U	2.5	10.0	SOL	P	29-MAR-10 21:43	032910C-1
	Magnesium	85.0	+/-300	U	85.0	300	SOL	P	29-MAR-10 21:43	032910C-1
	Manganese	2.0	+/-10	U	2.0	10.0	SOL	P	29-MAR-10 21:43	032910C-1
	Potassium	64.0	+/-250	U	64.0	250	SOL	P	29-MAR-10 21:43	032910C-1
	Silver	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 21:43	032910C-1
	Sodium	70.0	+/-250	U	70.0	250	SOL	P	29-MAR-10 21:43	032910C-1
	Vanadium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 21:43	032910C-1
	Zinc	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 21:43	032910C-1

SW846

Metals
-3a-
Initial and Continuing Calibration Blank Summary

SDG No.: 10-2093-1

Contract: LANL01004

Lab Code: GEL

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u> <u>ug/L</u>	<u>Acceptance</u>	<u>Conc</u> <u>Qual</u>	<u>MDL</u>	<u>RDL</u>	<u>Matrix</u>	<u>M</u>	<u>Analysis</u> <u>Date/Time</u>	<u>Run</u>
CCB10	Aluminum	68.0	+/-200	U	68.0	200	SOL	P	29-MAR-10 22:03	032910C-1
	Antimony	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 22:03	032910C-1
	Barium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 22:03	032910C-1
	Cadmium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 22:03	032910C-1
	Calcium	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 22:03	032910C-1
	Chromium	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 22:03	032910C-1
	Cobalt	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 22:03	032910C-1
	Copper	3.0	+/-10	U	3.0	10.0	SOL	P	29-MAR-10 22:03	032910C-1
	Iron	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 22:03	032910C-1
	Lead	2.5	+/-10	U	2.5	10.0	SOL	P	29-MAR-10 22:03	032910C-1
	Magnesium	85.0	+/-300	U	85.0	300	SOL	P	29-MAR-10 22:03	032910C-1
	Manganese	2.0	+/-10	U	2.0	10.0	SOL	P	29-MAR-10 22:03	032910C-1
	Potassium	64.0	+/-250	U	64.0	250	SOL	P	29-MAR-10 22:03	032910C-1
	Silver	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 22:03	032910C-1
	Sodium	70.0	+/-250	U	70.0	250	SOL	P	29-MAR-10 22:03	032910C-1
	Vanadium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 22:03	032910C-1
	Zinc	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 22:03	032910C-1
CCB11	Aluminum	68.0	+/-200	U	68.0	200	SOL	P	29-MAR-10 22:21	032910C-1
	Antimony	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 22:21	032910C-1
	Barium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 22:21	032910C-1
	Cadmium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 22:21	032910C-1
	Calcium	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 22:21	032910C-1
	Chromium	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 22:21	032910C-1
	Cobalt	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 22:21	032910C-1
	Copper	3.0	+/-10	U	3.0	10.0	SOL	P	29-MAR-10 22:21	032910C-1
	Iron	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 22:21	032910C-1
	Lead	2.5	+/-10	U	2.5	10.0	SOL	P	29-MAR-10 22:21	032910C-1
	Magnesium	85.0	+/-300	U	85.0	300	SOL	P	29-MAR-10 22:21	032910C-1
	Manganese	2.0	+/-10	U	2.0	10.0	SOL	P	29-MAR-10 22:21	032910C-1
	Potassium	64.0	+/-250	U	64.0	250	SOL	P	29-MAR-10 22:21	032910C-1

Metals
-3a-
Initial and Continuing Calibration Blank Summary

SDG No.: 10-2093-1

Contract: LANL01004

Lab Code: GEL

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u> <u>ng/L</u>	<u>Acceptance</u>	<u>Conc</u> <u>Qual</u>	<u>MDL</u>	<u>RDL</u>	<u>Matrix</u>	<u>M</u>	<u>Analysis</u> <u>Date/Time</u>	<u>Run</u>
	Silver	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 22:21	032910C-1
	Sodium	70.0	+/-250	U	70.0	250	SOL	P	29-MAR-10 22:21	032910C-1
	Vanadium	-1.16	+/-5	J	1.0	5.0	SOL	P	29-MAR-10 22:21	032910C-1
	Zinc	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 22:21	032910C-1
CCB12										
	Aluminum	68.0	+/-200	U	68.0	200	SOL	P	29-MAR-10 22:44	032910C-1
	Antimony	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 22:44	032910C-1
	Barium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 22:44	032910C-1
	Cadmium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 22:44	032910C-1
	Calcium	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 22:44	032910C-1
	Chromium	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 22:44	032910C-1
	Cobalt	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 22:44	032910C-1
	Copper	3.0	+/-10	U	3.0	10.0	SOL	P	29-MAR-10 22:44	032910C-1
	Iron	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 22:44	032910C-1
	Lead	2.5	+/-10	U	2.5	10.0	SOL	P	29-MAR-10 22:44	032910C-1
	Magnesium	85.0	+/-300	U	85.0	300	SOL	P	29-MAR-10 22:44	032910C-1
	Manganese	2.0	+/-10	U	2.0	10.0	SOL	P	29-MAR-10 22:44	032910C-1
	Potassium	64.0	+/-250	U	64.0	250	SOL	P	29-MAR-10 22:44	032910C-1
	Silver	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 22:44	032910C-1
	Sodium	70.0	+/-250	U	70.0	250	SOL	P	29-MAR-10 22:44	032910C-1
	Vanadium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 22:44	032910C-1
	Zinc	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 22:44	032910C-1
CCB13										
	Aluminum	68.0	+/-200	U	68.0	200	SOL	P	29-MAR-10 23:01	032910C-1
	Antimony	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 23:01	032910C-1
	Barium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 23:01	032910C-1
	Cadmium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 23:01	032910C-1
	Calcium	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 23:01	032910C-1
	Chromium	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 23:01	032910C-1
	Cobalt	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 23:01	032910C-1
	Copper	3.0	+/-10	U	3.0	10.0	SOL	P	29-MAR-10 23:01	032910C-1

Metals
-3a-
Initial and Continuing Calibration Blank Summary

SDG No.: 10-2093-1

Contract: LANL01004

Lab Code: GEL

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u> <u>ug/L</u>	<u>Acceptance</u>	<u>Conc</u> <u>Qual</u>	<u>MDL</u>	<u>RDL</u>	<u>Matrix</u>	<u>M</u>	<u>Analysis</u> <u>Date/Time</u>	<u>Run</u>
	Iron	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 23:01	032910C-1
	Lead	2.5	+/-10	U	2.5	10.0	SOL	P	29-MAR-10 23:01	032910C-1
	Magnesium	85.0	+/-300	U	85.0	300	SOL	P	29-MAR-10 23:01	032910C-1
	Manganese	2.0	+/-10	U	2.0	10.0	SOL	P	29-MAR-10 23:01	032910C-1
	Potassium	64.0	+/-250	U	64.0	250	SOL	P	29-MAR-10 23:01	032910C-1
	Silver	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 23:01	032910C-1
	Sodium	70.0	+/-250	U	70.0	250	SOL	P	29-MAR-10 23:01	032910C-1
	Vanadium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 23:01	032910C-1
	Zinc	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 23:01	032910C-1
CCB14	Aluminum	68.0	+/-200	U	68.0	200	SOL	P	29-MAR-10 23:21	032910C-1
	Antimony	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 23:21	032910C-1
	Barium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 23:21	032910C-1
	Cadmium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 23:21	032910C-1
	Calcium	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 23:21	032910C-1
	Chromium	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 23:21	032910C-1
	Cobalt	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 23:21	032910C-1
	Copper	3.0	+/-10	U	3.0	10.0	SOL	P	29-MAR-10 23:21	032910C-1
	Iron	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 23:21	032910C-1
	Lead	2.5	+/-10	U	2.5	10.0	SOL	P	29-MAR-10 23:21	032910C-1
	Magnesium	85.0	+/-300	U	85.0	300	SOL	P	29-MAR-10 23:21	032910C-1
	Manganese	2.0	+/-10	U	2.0	10.0	SOL	P	29-MAR-10 23:21	032910C-1
	Potassium	64.0	+/-250	U	64.0	250	SOL	P	29-MAR-10 23:21	032910C-1
	Silver	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 23:21	032910C-1
	Sodium	70.0	+/-250	U	70.0	250	SOL	P	29-MAR-10 23:21	032910C-1
	Vanadium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 23:21	032910C-1
	Zinc	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 23:21	032910C-1
CCB15	Aluminum	68.0	+/-200	U	68.0	200	SOL	P	29-MAR-10 23:41	032910C-1
	Antimony	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 23:41	032910C-1
	Barium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 23:41	032910C-1

Metals
-3a-
Initial and Continuing Calibration Blank Summary

SDG No.: 10-2093-1

Contract: LANL01004

Lab Code: GEL

<u>Sample ID</u>	<u>Analyte</u>	<u>Result ng/L</u>	<u>Acceptance</u>	<u>Conc Qual</u>	<u>MDL</u>	<u>RDL</u>	<u>Matrix</u>	<u>M</u>	<u>Analysis Date/Time</u>	<u>Run</u>
	Cadmium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 23:41	032910C-1
	Calcium	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 23:41	032910C-1
	Chromium	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 23:41	032910C-1
	Cobalt	1.5	+/-5	U	1.5	5.0	SOL	P	29-MAR-10 23:41	032910C-1
	Copper	3.0	+/-10	U	3.0	10.0	SOL	P	29-MAR-10 23:41	032910C-1
	Iron	80.0	+/-250	U	80.0	250	SOL	P	29-MAR-10 23:41	032910C-1
	Lead	-2.63	+/-10	J	2.5	10.0	SOL	P	29-MAR-10 23:41	032910C-1
	Magnesium	85.0	+/-300	U	85.0	300	SOL	P	29-MAR-10 23:41	032910C-1
	Manganese	2.0	+/-10	U	2.0	10.0	SOL	P	29-MAR-10 23:41	032910C-1
	Potassium	64.0	+/-250	U	64.0	250	SOL	P	29-MAR-10 23:41	032910C-1
	Silver	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 23:41	032910C-1
	Sodium	70.0	+/-250	U	70.0	250	SOL	P	29-MAR-10 23:41	032910C-1
	Vanadium	1.0	+/-5	U	1.0	5.0	SOL	P	29-MAR-10 23:41	032910C-1
	Zinc	3.3	+/-10	U	3.3	10.0	SOL	P	29-MAR-10 23:41	032910C-1

METALS
-3b-
PREPARATION BLANK SUMMARY

SDG NO. 10-2093-1

Contract: LANL01004

Matrix: SOIL

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>Acceptance Window</u>	<u>Conc Qual</u>	<u>M</u>	<u>MDL</u>	<u>RDL</u>
1202056179	Mercury	-3.78	ug/kg	+/-11	J	AV	3.73	11
1202056877	Aluminum	7160	ug/Kg	+/-18200	J	P	6190	18200
	Antimony	301	ug/Kg	+/-911	U	P	301	911
	Barium	165	ug/Kg	+/-455	J	P	91.1	455
	Cadmium	91.1	ug/Kg	+/-455	U	P	91.1	455
	Calcium	7290	ug/Kg	+/-22800	U	P	7290	22800
	Chromium	137	ug/Kg	+/-455	U	P	137	455
	Cobalt	137	ug/Kg	+/-455	U	P	137	455
	Copper	273	ug/Kg	+/-911	U	P	273	911
	Iron	14000	ug/Kg	+/-22800	J	P	7290	22800
	Lead	228	ug/Kg	+/-911	U	P	228	911
	Magnesium	7740	ug/Kg	+/-27300	U	P	7740	27300
	Manganese	292	ug/Kg	+/-911	J	P	182	911
	Potassium	5830	ug/Kg	+/-22800	U	P	5830	22800
	Silver	91.1	ug/Kg	+/-455	U	P	91.1	455
	Sodium	6380	ug/Kg	+/-22800	U	P	6380	22800
	Vanadium	91.1	ug/Kg	+/-455	U	P	91.1	455
	Zinc	301	ug/Kg	+/-911	U	P	301	911
1202056883	Arsenic	0.192	mg/kg	+/-0.96	U	MS	0.192	0.96
	Beryllium	0.0192	mg/kg	+/-0.096	U	MS	0.0192	0.096
	Nickel	0.096	mg/kg	+/-0.384	U	MS	0.096	0.384
	Selenium	0.48	mg/kg	+/-0.96	U	MS	0.48	0.96
	Thallium	0.0576	mg/kg	+/-0.192	U	MS	0.0576	0.192
	Uranium	0.0127	mg/kg	+/-0.0384	U	MS	0.0127	0.0384

METALS

-4-

Interference Check Sample

SDG No: 10-2093-1

Contract: LANL01004

Lab Code: GEL

ICS: O2Si

Instrument: OPTIMA4

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>True Value</u>	<u>Units</u>	<u>% Recovery</u>	<u>Acceptance Window (%R)</u>	<u>Analysis Date/Time</u>	<u>Run Number</u>
ICSA01									
	Aluminum	511000	ug/L	500000	ug/L	102	80.0 – 120.0	29-MAR-10 18:43	032910C-1
	Antimony	-0.864	ug/L					29-MAR-10 18:43	032910C-1
	Barium	0.49	ug/L					29-MAR-10 18:43	032910C-1
	Cadmium	-2.27	ug/L					29-MAR-10 18:43	032910C-1
	Calcium	479000	ug/L	500000	ug/L	95.7	80.0 – 120.0	29-MAR-10 18:43	032910C-1
	Chromium	1.9	ug/L					29-MAR-10 18:43	032910C-1
	Cobalt	-6.27	ug/L					29-MAR-10 18:43	032910C-1
	Copper	-2.45	ug/L					29-MAR-10 18:43	032910C-1
	Iron	189000	ug/L	200000	ug/L	94.6	80.0 – 120.0	29-MAR-10 18:43	032910C-1
	Lead	0.983	ug/L					29-MAR-10 18:43	032910C-1
	Magnesium	481000	ug/L	500000	ug/L	96.2	80.0 – 120.0	29-MAR-10 18:43	032910C-1
	Manganese	2.08	ug/L					29-MAR-10 18:43	032910C-1
	Potassium	-157.0	ug/L					29-MAR-10 18:43	032910C-1
	Silver	0.683	ug/L					29-MAR-10 18:43	032910C-1
	Sodium	12.5	ug/L					29-MAR-10 18:43	032910C-1
	Vanadium	1.57	ug/L					29-MAR-10 18:43	032910C-1
	Zinc	7.6	ug/L					29-MAR-10 18:43	032910C-1
ICSAB01									
	Aluminum	520000	ug/L	500000	ug/L	104	80.0 – 120.0	29-MAR-10 18:45	032910C-1
	Antimony	502	ug/L	500	ug/L	100	80.0 – 120.0	29-MAR-10 18:45	032910C-1
	Barium	500	ug/L	500	ug/L	100	80.0 – 120.0	29-MAR-10 18:45	032910C-1
	Cadmium	467	ug/L	500	ug/L	93.3	80.0 – 120.0	29-MAR-10 18:45	032910C-1
	Calcium	487000	ug/L	500000	ug/L	97.4	80.0 – 120.0	29-MAR-10 18:45	032910C-1
	Chromium	485	ug/L	500	ug/L	96.9	80.0 – 120.0	29-MAR-10 18:45	032910C-1
	Cobalt	437	ug/L	500	ug/L	87.5	80.0 – 120.0	29-MAR-10 18:45	032910C-1
	Copper	537	ug/L	500	ug/L	107	80.0 – 120.0	29-MAR-10 18:45	032910C-1
	Iron	191000	ug/L	200000	ug/L	95.3	80.0 – 120.0	29-MAR-10 18:45	032910C-1
	Lead	459	ug/L	500	ug/L	91.7	80.0 – 120.0	29-MAR-10 18:45	032910C-1
	Magnesium	483000	ug/L	500000	ug/L	96.6	80.0 – 120.0	29-MAR-10 18:45	032910C-1

METALS

-4-

Interference Check Sample

SDG No: 10-2093-1

Contract: LANL01004

Lab Code: GEL

ICS:

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>True Value</u>	<u>Units</u>	<u>% Recovery</u>	<u>Acceptance Window (%R)</u>	<u>Analysis Date/Time</u>	<u>Run Number</u>
	Manganese	478	ug/L	500	ug/L	95.7	80.0 - 120.0	29-MAR-10 18:45	032910C-1
	Potassium	5450	ug/L	5000	ug/L	109	80.0 - 120.0	29-MAR-10 18:45	032910C-1
	Silver	271	ug/L	250	ug/L	108	80.0 - 120.0	29-MAR-10 18:45	032910C-1
	Sodium	5320	ug/L	5000	ug/L	106	80.0 - 120.0	29-MAR-10 18:45	032910C-1
	Vanadium	517	ug/L	500	ug/L	103	80.0 - 120.0	29-MAR-10 18:45	032910C-1
	Zinc	484	ug/L	500	ug/L	96.8	80.0 - 120.0	29-MAR-10 18:45	032910C-1

METALS

-4-

Interference Check Sample

SDG No: 10-2093-1

Contract: LANL01004

Lab Code: GEL

ICS: O2Si

Instrument: ICPMS6

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>True Value</u>	<u>Units</u>	<u>% Recovery</u>	<u>Acceptance Window (%R)</u>	<u>Analysis Date/Time</u>	<u>Run Number</u>
ICSA01									
	Arsenic	0.011	ug/L					24-MAR-10 16:22	100323-2
	Beryllium	0.103	ug/L					24-MAR-10 16:22	100323-2
	Nickel	2.45	ug/L					24-MAR-10 16:22	100323-2
	Selenium	-1.62	ug/L					24-MAR-10 16:22	100323-2
	Thallium	0.022	ug/L					24-MAR-10 16:22	100323-2
ICSAB01									
	Arsenic	21.8	ug/L	20	ug/L	109	80.0 - 120.0	24-MAR-10 16:26	100323-2
	Beryllium	20.0	ug/L	20	ug/L	100	80.0 - 120.0	24-MAR-10 16:26	100323-2
	Nickel	22.1	ug/L	23.31	ug/L	94.8	80.0 - 120.0	24-MAR-10 16:26	100323-2
	Selenium	20.0	ug/L	20	ug/L	100	80.0 - 120.0	24-MAR-10 16:26	100323-2
	Thallium	19.7	ug/L	20	ug/L	98.4	80.0 - 120.0	24-MAR-10 16:26	100323-2

METALS

-4-

Interference Check Sample

SDG No: 10-2093-1

Contract: LANL01004

Lab Code: GEL

ICS: O2Si

Instrument: ICPMS6

<u>Sample ID</u>	<u>Analyte</u>	<u>Result</u>	<u>Units</u>	<u>True Value</u>	<u>Units</u>	<u>% Recovery</u>	<u>Acceptance Window (%R)</u>	<u>Analysis Date/Time</u>	<u>Run Number</u>
ICSA01	Uranium	0.005	ug/L					25-MAR-10 23:58	100325-3
ICSAB01	Uranium	21.8	ug/L	20	ug/L	109	80.0 - 120.0	26-MAR-10 00:01	100325-3

METALS

-5a-

Matrix Spike Summary

SDG NO. 10-2093-1 Client ID RE11-10-1786S

Contract: LANL01004 Level: Low

Matrix: SOIL % Solids: 93.2

Sample ID: 248068001 Spike ID: 1202056182

Analyte	Units	Acceptance Limit	Spiked Result	C	Sample Result	C	Spike Added	% Recovery	Qual	M
Mercury	ug/kg	75-125	133		3.96	U	127	103		AV

METALS

-5a-

Matrix Spike Duplicate Summary

SDG NO.	10-2093-1	Client ID	RE11-10-1786SD
---------	-----------	-----------	----------------

Contract:	LANL01004	Level:	Low
-----------	-----------	--------	-----

Matrix:	SOIL	% Solids:	93.2
---------	------	-----------	------

Sample ID:	248068001	Spike ID:	1202056184
------------	-----------	-----------	------------

<u>Analyte</u>	<u>Units</u>	<u>Acceptance Limit</u>	<u>Spiked Result</u>	<u>C</u>	<u>Sample Result</u>	<u>C</u>	<u>Spike Added</u>	<u>% Recovery</u>	<u>Qual</u>	<u>M</u>
Mercury	ug/kg	75-125	129		3.96	U	122	105		AV

METALS

-5a-

Matrix Spike Summary

SDG NO. 10-2093-1 Client ID RE15-10-8404S

Contract: LANL01004 Level: Low

Matrix: SOIL % Solids: 90.6

Sample ID: 248110001 Spike ID: 1202056880

Analyte	Units	Acceptance Limit	Spiked Result	C	Sample Result	C	Spike Added	% Recovery	Qual	M
Aluminum	ug/Kg		19200000		11200000		538000	1480	N/A	P
Antimony	ug/Kg	75-125	32100		342	U	53800	59.7	N	P
Barium	ug/Kg	75-125	219000		167000		53800	96.8		P
Cadmium	ug/Kg	75-125	45400		104	U	53800	84.4		P
Calcium	ug/Kg		3970000		3220000		538000	139	N/A	P
Chromium	ug/Kg	75-125	63800		9850		53800	100		P
Cobalt	ug/Kg	75-125	49700		5200		53800	82.7		P
Copper	ug/Kg	75-125	63400		6500		53800	106		P
Iron	ug/Kg		16700000		14500000		538000	410	N/A	P
Lead	ug/Kg	75-125	54100		9820		53800	82.3		P
Magnesium	ug/Kg		3070000		2240000		538000	153	N/A	P
Manganese	ug/Kg		318000		300000		53800	32.4	N/A	P
Potassium	ug/Kg	75-125	2530000		1790000		538000	139	N	P
Silver	ug/Kg	75-125	46900		104	U	53800	87.2		P
Sodium	ug/Kg	75-125	1050000		546000		538000	93.5		P
Vanadium	ug/Kg	75-125	76600		21500		53800	103		P
Zinc	ug/Kg	75-125	85700		29900		53800	104		P

METALS

-5a-

Matrix Spike Duplicate Summary

SDG NO. 10-2093-1 Client ID RE15-10-8404SD

Contract: LANL01004 Level: Low

Matrix: SOIL % Solids: 90.6

Sample ID: 248110001 Spike ID: 1202056881

Analyte	Units	Acceptance Limit	Spiked Result	C	Sample Result	C	Spike Added	% Recovery	Qual	M
Aluminum	ug/Kg		19800000		11200000		531000	1620	N/A	P
Antimony	ug/Kg	75-125	31900		342	U	53100	60	N	P
Barium	ug/Kg	75-125	216000		167000		53100	93		P
Cadmium	ug/Kg	75-125	45500		104	U	53100	85.7		P
Calcium	ug/Kg		3770000		3220000		531000	103	N/A	P
Chromium	ug/Kg	75-125	62800		9850		53100	99.8		P
Cobalt	ug/Kg	75-125	50700		5200		53100	85.6		P
Copper	ug/Kg	75-125	63100		6500		53100	107		P
Iron	ug/Kg		15500000		14500000		531000	193	N/A	P
Lead	ug/Kg	75-125	55600		9820		53100	86.3		P
Magnesium	ug/Kg		3050000		2240000		531000	152	N/A	P
Manganese	ug/Kg		340000		300000		53100	74.5	N/A	P
Potassium	ug/Kg	75-125	2510000		1790000		531000	136	N	P
Silver	ug/Kg	75-125	47200		104	U	53100	88.8		P
Sodium	ug/Kg	75-125	1070000		546000		531000	98.1		P
Vanadium	ug/Kg	75-125	75200		21500		53100	101		P
Zinc	ug/Kg	75-125	82400		29900		53100	98.8		P

METALS

-5a-

Matrix Spike Summary

SDG NO. 10-2093-1 Client ID RE15-10-8404S

Contract: LANL01004 Level: Low

Matrix: SOIL % Solids: 90.6

Sample ID: 248110001 Spike ID: 1202056886

Analyte	Units	Acceptance Limit	Spiked Result	C	Sample Result	C	Spike Added	% Recovery	Qual	M
Arsenic	mg/kg	75-125	9.63		1.74		8.4	93.9		MS
Beryllium	mg/kg	75-125	6.25		1.02		5.25	99.6		MS
Nickel	mg/kg	75-125	12.8		7.48		5.25	101		MS
Selenium	mg/kg	75-125	1.56		0.517	U	2.1	70.3	N	MS
Thallium	mg/kg	75-125	9.75		0.185	J	10.5	91.1		MS
Uranium	mg/kg	75-125	9.6		4.07		5.25	105		MS

METALS

-5a-

Matrix Spike Duplicate Summary

SDG NO. 10-2093-1 Client ID RE15-10-8404SD

Contract: LANL01004 Level: Low

Matrix: SOIL % Solids: 90.6

Sample ID: 248110001 Spike ID: 1202056887

Analyte	Units	Acceptance Limit	Spiked Result	C	Sample Result	C	Spike Added	% Recovery	Qual	M
Arsenic	mg/kg	75-125	9.76		1.74		8.8	91.1		MS
Beryllium	mg/kg	75-125	6.25		1.02		5.5	95.1		MS
Nickel	mg/kg	75-125	12.7		7.48		5.5	95.7		MS
Selenium	mg/kg	75-125	1.58		0.517	U	2.2	67.8	N	MS
Thallium	mg/kg	75-125	9.99		0.185	J	11	89.2		MS
Uranium	mg/kg	75-125	9.64		4.07		5.5	101		MS

Metals
-6-
Duplicate Sample Summary

SDG No.: 10-2093-1

Contract: LANL01004

Lab Code: GEL

Matrix: SOLID

Level: Low

Client ID: RE11-10-1786D

Sample ID: 248068001

Duplicate ID: 1202056181

Percent Solids for Dup: 93.2

Analyte	Units	Acceptance Limit	Sample Result	C	Duplicate Result	C	RPD	Qual	M
Mercury	ug/kg		3.96 U		3.74 U				AV

Metals
-6-
Duplicate Sample Summary

SDG No.: 10-2093-1

Contract: LANL01004

Lab Code: GEL

Matrix: SOLID

Level: Low

Client ID: RE11-10-1786SD

Sample ID: 1202056182

Duplicate ID: 1202056184

Percent Solids for Dup: 93.2

Analyte	Units	Acceptance Limit	Sample Result	C	Duplicate Result	C	RPD	Qual	M
Mercury	ug/kg	+/-20	133		129		2.71		AV

Metals
-6-
Duplicate Sample Summary

SDG No.: 10-2093-1

Contract: LANL01004

Lab Code: GEL

Matrix: SOLID

Level: Low

Client ID: RE15-10-8404D

Sample ID: 248110001

Duplicate ID: 1202056878

Percent Solids for Dup: 90.6

Analyte	Units	Acceptance Limit	Sample Result	C	Duplicate Result	C	RPD	Qual	M
Aluminum	ug/Kg	+/-20%	11200000		11400000		1.7		P
Antimony	ug/Kg		342 U		346 U				P
Barium	ug/Kg	+/-20%	167000		151000		9.81		P
Cadmium	ug/Kg		104 U		105 U				P
Calcium	ug/Kg	+/-20%	3220000		3010000		6.62		P
Chromium	ug/Kg	+/-20%	9850		9720		1.34		P
Cobalt	ug/Kg	+/-20%	5200		4320		18.7		P
Copper	ug/Kg	+/-20%	6500		6300		3.16		P
Iron	ug/Kg	+/-20%	14500000		13900000		3.79		P
Lead	ug/Kg	+/-20%	9820		8510		14.3		P
Magnesium	ug/Kg	+/-20%	2240000		2050000		9.21		P
Manganese	ug/Kg	+/-20%	300000		245000		20.1	*	P
Potassium	ug/Kg	+/-20%	1790000		1650000		8.3		P
Silver	ug/Kg		104 U		105 U				P
Sodium	ug/Kg	+/-20%	546000		525000		4.04		P
Vanadium	ug/Kg	+/-20%	21500		21700		1.13		P
Zinc	ug/Kg	+/-20%	29900		29600		1.04		P

Metals
-6-
Duplicate Sample Summary

SDG No.: 10-2093-1

Contract: LANL01004

Lab Code: GEL

Matrix: SOLID

Level: Low

Client ID: RE15-10-8404SD

Sample ID: 1202056880

Duplicate ID: 1202056881

Percent Solids for Dup: 90.6

Analyte	Units	Acceptance Limit	Sample Result	C	Duplicate Result	C	RPD	Qual	M
Aluminum	ug/Kg	+/-20	19200000		19800000		3.04		P
Antimony	ug/Kg	+/-20	32100		31900		.884		P
Barium	ug/Kg	+/-20	219000		216000		1.25		P
Cadmium	ug/Kg	+/-20	45400		45500		.262		P
Calcium	ug/Kg	+/-20	3970000		3770000		5.2		P
Chromium	ug/Kg	+/-20	63800		62800		1.58		P
Cobalt	ug/Kg	+/-20	49700		50700		1.91		P
Copper	ug/Kg	+/-20	63400		63100		.51		P
Iron	ug/Kg	+/-20	16700000		15500000		7.32		P
Lead	ug/Kg	+/-20	54100		55600		2.71		P
Magnesium	ug/Kg	+/-20	3070000		3050000		.489		P
Manganese	ug/Kg	+/-20	318000		340000		6.72		P
Potassium	ug/Kg	+/-20	2530000		2510000		1.04		P
Silver	ug/Kg	+/-20	46900		47200		.435		P
Sodium	ug/Kg	+/-20	1050000		1070000		1.67		P
Vanadium	ug/Kg	+/-20	76600		75200		1.92		P
Zinc	ug/Kg	+/-20	85700		82400		3.98		P

Metals

-6-

Duplicate Sample Summary

SDG No.: 10-2093-1

Contract: LANL01004

Lab Code: GEL

Matrix: SOLID

Level: Low

Client ID: RE15-10-8404D

Sample ID: 248110001

Duplicate ID: 1202056884

Percent Solids for Dup: 90.6

Analyte	Units	Acceptance Limit	Sample Result	C	Duplicate Result	C	RPD	Qual	M
Arsenic	mg/kg	+/- .993	1.74		1.89		8.07		MS
Beryllium	mg/kg	+/-20%	1.02		1.02		.0288		MS
Nickel	mg/kg	+/-20%	7.48		7.58		1.33		MS
Selenium	mg/kg		0.517 U		0.497 U				MS
Thallium	mg/kg	+/- .199	0.185 J		0.183 J		1.39		MS
Uranium	mg/kg	+/-20%	4.07		4.82		17		MS

Metals

-6-

Duplicate Sample Summary

SDG No.: 10-2093-1

Contract: LANL01004

Lab Code: GEL

Matrix: SOLID

Level: Low

Client ID: RE15-10-8404SD

Sample ID: 1202056886

Duplicate ID: 1202056887

Percent Solids for Dup: 90.6

Analyte	Units	Acceptance Limit	Sample Result	C	Duplicate Result	C	RPD	Qual	M
Arsenic	mg/kg	+/-20	9.63		9.76		1.35		MS
Beryllium	mg/kg	+/-20	6.25		6.25		.108		MS
Nickel	mg/kg	+/-20	12.8		12.7		.414		MS
Selenium	mg/kg	+/-20	1.56		1.58		.868		MS
Thallium	mg/kg	+/-20	9.75		9.99		2.46		MS
Uranium	mg/kg	+/-20	9.6		9.64		.412		MS

METALS

-7-

Laboratory Control Sample Summary

SDG NO. 10-2093-1

Contract: LANL01004

Aqueous LCS Source:

Solid LCS Source: ERA

<u>Sample ID</u>	<u>Analyte</u>	<u>Units</u>	<u>True Value</u>	<u>Result</u>	<u>C</u>	<u>% Recovery</u>	<u>Acceptance Limit</u>	<u>M</u>
1202056180	Mercury	ug/kg	5150	5250		102	71.6-128.3	AV

METALS

-7-

Laboratory Control Sample Summary

SDG NO. 10-2093-1

Contract: LANL01004

Aqueous LCS Source:

Solid LCS Source: ERA

<u>Sample ID</u>	<u>Analyte</u>	<u>Units</u>	<u>True Value</u>	<u>Result</u>	<u>C</u>	<u>% Recovery</u>	<u>Acceptance Limit</u>	<u>M</u>
1202056882								
	Aluminum	ug/Kg	10500000	9340000		88.9	56-144	P
	Antimony	ug/Kg	173000	109000		63.2	71-130	P
	Barium	ug/Kg	198000	194000		98	80-120	P
	Cadmium	ug/Kg	60700	59800		98.5	81-120	P
	Calcium	ug/Kg	9870000	9710000		98.3	83-117	P
	Chromium	ug/Kg	236000	241000		102	80-120	P
	Cobalt	ug/Kg	91200	92200		101	81-120	P
	Copper	ug/Kg	174000	187000		108	81-118	P
	Iron	ug/Kg	18000000	18100000		101	51-149	P
	Lead	ug/Kg	86000	81800		95.1	79-121	P
	Magnesium	ug/Kg	4000000	3800000		94.9	79-122	P
	Manganese	ug/Kg	558000	530000		95.1	81-119	P
	Potassium	ug/Kg	4300000	4000000		93.1	74-127	P
	Silver	ug/Kg	30100	30600		102	66-134	P
	Sodium	ug/Kg	1020000	1030000		101	74-127	P
	Vanadium	ug/Kg	115000	122000		106	79-121	P
	Zinc	ug/Kg	594000	591000		99.5	80-121	P

METALS

-7-

Laboratory Control Sample Summary

SDG NO. 10-2093-1

Contract: LANL01004

Aqueous LCS Source:

Solid LCS Source: ERA

<u>Sample ID</u>	<u>Analyte</u>	<u>Units</u>	<u>True Value</u>	<u>Result</u>	<u>C</u>	<u>% Recovery</u>	<u>Acceptance Limit</u>	<u>M</u>
1202056888								
	Arsenic	mg/kg	104	115		111	78-123	MS
	Beryllium	mg/kg	77.6	83.4		107	84-116	MS
	Nickel	mg/kg	134	148		111	78-123	MS
	Selenium	mg/kg	286	312		109	77-123	MS
	Thallium	mg/kg	121	128		106	78-122	MS
	Uranium	mg/kg	2.13	2.13		100	73-127	MS

METALS

-9-

Serial Dilution Sample Summary

SDG NO. 10-2093-1 **Client ID** RE11-10-1786L

Contract: LANL01004**Matrix:** SOLID **Level:** Low**Sample ID:** 248068001 **Serial Dilution ID:** 1202056183

<u>Analyte</u>	<u>Initial Value ug/L</u>	<u>C</u>	<u>Serial Value ug/L</u>	<u>C</u>	<u>% Difference</u>	<u>Qual</u>	<u>Acceptance Limit</u>	<u>M</u>
Mercury	.068	U	.34	U				AV

METALS

-9-

Serial Dilution Sample Summary

SDG NO. 10-2093-1 Client ID RE15-10-8404L

Contract: LANL01004

Matrix: SOLID Level: Low

Sample ID: 248110001 Serial Dilution ID: 1202056879

Analyte	Initial Value ug/L	C	Serial Value ug/L	C	% Difference	Qual	Acceptance Limit	M
Aluminum	108000		112000		3.24		10	P
Antimony	3.3	U	16.5	U				P
Barium	1610		1650		2.48		10	P
Cadmium	1	U	5	U				P
Calcium	31100		31700		1.77		10	P
Chromium	95.1		97		2		10	P
Cobalt	50.2		51.5		2.59			P
Copper	62.8		65.5		4.3			P
Iron	140000		145000		3.21		10	P
Lead	94.8		91.5		3.48			P
Magnesium	21700		22300		2.76		10	P
Manganese	2900		2980		2.59		10	P
Potassium	17300		17400		.578		10	P
Silver	1	U	5	U				P
Sodium	5270		5350		1.52		10	P
Vanadium	207		204		1.69		10	P
Zinc	288		293		1.56		10	P

METALS

-9-

Serial Dilution Sample Summary

SDG NO. 10-2093-1 Client ID RE15-10-8404L

Contract: LANL01004

Matrix: SOLID Level: Low

Sample ID: 248110001 Serial Dilution ID: 1202056885

Analyte	Initial Value ug/L	C	Serial Value ug/L	C	% Difference	Qual	Acceptance Limit	M
Arsenic	8.42		10.5	J	24.1			MS
Beryllium	4.94		5.2		5.26			MS
Nickel	36.2		39.8		9.81			MS
Selenium	2.5	U	12.5	U				MS
Thallium	.896	J	1.55	J	72.4			MS
Uranium	19.7		20		1.52		10	MS

METALS
-13-
SAMPLE PREPARATION SUMMARY

SDG No: 10-2093-1

Method Type: P

Contract: LANL01004

Lab Code: GEL

<u>Sample ID</u>	<u>Client ID</u>	<u>Sample Type</u>	<u>Matrix</u>	<u>Prep Date</u>	<u>Initial Sample Size</u>	<u>Final Sample Volume</u>	<u>Percent Solids</u>
Batch Number 959113							
1202056877	MB for batch 959113	MB	S	09-MAR-10	.549g	50mL	
1202056882	LCS for batch 959113	LCS	S	09-MAR-10	.548g	50mL	
1202056880	RE15-10-8404S	MS	S	09-MAR-10	.513g	50mL	
1202056881	RE15-10-8404SD	MSD	S	09-MAR-10	.52g	50mL	
1202056878	RE15-10-8404D	DUP	S	09-MAR-10	.527g	50mL	
248118001	RE36-10-8448	SAMPLE	S	09-MAR-10	.506g	50mL	
248118002	RE36-10-8456	SAMPLE	S	09-MAR-10	.521g	50mL	
248118003	RE36-10-8451	SAMPLE	S	09-MAR-10	.51g	50mL	
248118004	RE36-10-8450	SAMPLE	S	09-MAR-10	.551g	50mL	
248118005	RE36-10-8449	SAMPLE	S	09-MAR-10	.594g	50mL	
248118006	RE36-10-8453	SAMPLE	S	09-MAR-10	.524g	50mL	
248118007	RE36-10-8452	SAMPLE	S	09-MAR-10	.59g	50mL	

SW846

METALS
-13-
SAMPLE PREPARATION SUMMARY

SDG No: 10-2093-1

Method Type: MS

Contract: LANL01004

Lab Code: GEL

<u>Sample ID</u>	<u>Client ID</u>	<u>Sample Type</u>	<u>Matrix</u>	<u>Prep Date</u>	<u>Initial Sample Size</u>	<u>Final Sample Volume</u>	<u>Percent Solids</u>
Batch Number 959115							
1202056883	MB for batch 959115	MB	S	03-MAR-10	.521g	50mL	
1202056888	LCS for batch 959115	LCS	S	03-MAR-10	.578g	50mL	
1202056886	RE15-10-8404S	MS	S	03-MAR-10	.526g	50mL	
1202056887	RE15-10-8404SD	MSD	S	03-MAR-10	.502g	50mL	
1202056884	RE15-10-8404D	DUP	S	03-MAR-10	.556g	50mL	
248118001	RE36-10-8448	SAMPLE	S	03-MAR-10	.53g	50mL	
248118002	RE36-10-8456	SAMPLE	S	03-MAR-10	.585g	50mL	
248118003	RE36-10-8451	SAMPLE	S	03-MAR-10	.516g	50mL	
248118004	RE36-10-8450	SAMPLE	S	03-MAR-10	.574g	50mL	
248118005	RE36-10-8449	SAMPLE	S	03-MAR-10	.576g	50mL	
248118006	RE36-10-8453	SAMPLE	S	03-MAR-10	.512g	50mL	
248118007	RE36-10-8452	SAMPLE	S	03-MAR-10	.584g	50mL	

SW846

METALS
-13-
SAMPLE PREPARATION SUMMARY

SDG No: 10-2093-1

Method Type: AV

Contract: LANL01004

Lab Code: GEL

<u>Sample ID</u>	<u>Client ID</u>	<u>Sample Type</u>	<u>Matrix</u>	<u>Prep Date</u>	<u>Initial Sample Size</u>	<u>Final Sample Volume</u>	<u>Percent Solids</u>
Batch Number 958755							
1202056179	MB for batch 958755	MB	S	10-MAR-10	.547g	30mL	
1202056180	LCS for batch 958755	LCS	S	10-MAR-10	.209g	30mL	
1202056182	RE11-10-1786S	MS	S	10-MAR-10	.505g	30mL	
1202056184	RE11-10-1786SD	MSD	S	10-MAR-10	.528g	30mL	
1202056181	RE11-10-1786D	DUP	S	10-MAR-10	.585g	30mL	
248118001	RE36-10-8448	SAMPLE	S	10-MAR-10	.558g	30mL	
248118002	RE36-10-8456	SAMPLE	S	10-MAR-10	.545g	30mL	
248118003	RE36-10-8451	SAMPLE	S	10-MAR-10	.588g	30mL	
248118004	RE36-10-8450	SAMPLE	S	10-MAR-10	.599g	30mL	
248118005	RE36-10-8449	SAMPLE	S	10-MAR-10	.535g	30mL	
248118006	RE36-10-8453	SAMPLE	S	10-MAR-10	.563g	30mL	
248118007	RE36-10-8452	SAMPLE	S	10-MAR-10	.554g	30mL	

SW846

Metals
-14-
Analysis Run Log

Contract: LANL01004

Lab Code: GEL

Inst Name: ICPMS6

Start Date: 24-MAR-10

End Date: 24-MAR-10

Client Sdg: 10-2093-1

Method MS

Data File: 100323-2

Samp No.	D/F	Run Time	Al	Sb	As	Ba	Be	Cd	Ca	Cr	Co	Cu	Fe	Pb	Mg	Mn	Hg	Ni	K	Se	Ag	Na	Tl	U	V	Zn
S0.0	1	15:58			X		X											X	X			X				
S10	1	16:02			X		X											X	X			X				
S100	1	16:06			X		X											X	X			X				
ICV01	1	16:10			X		X											X	X			X				
ICB01	1	16:14			X		X											X	X			X				
CRDL01	1	16:18			X		X											X	X			X				
ICSA01	1	16:22			X		X											X	X			X				
ICSAB01	1	16:26			X		X											X	X			X				
CCV01	1	16:30			X		X											X	X			X				
CCB01	1	16:34			X		X											X	X			X				
1202056883	2	16:39			X		X											X	X			X				
1202056888	40	16:43			X		X											X	X			X				
CCV02	1	16:47			X		X											X	X			X				
CCB02	1	16:51			X		X											X	X			X				
ZZZZZZ	2	16:55																								
1202056884	2	16:59			X		X											X	X			X				
1202056886	2	17:03			X		X											X	X			X				
1202056887	2	17:07			X		X											X	X			X				
1202056885	10	17:11			X		X											X	X			X				
ZZZZZZ	2	17:15																								
ZZZZZZ	2	17:19																								
ZZZZZZ	2	17:23																								
CCV03	1	17:27			X		X											X	X			X				
CCB03	1	17:31			X		X											X	X			X				
ZZZZZZ	2	17:35																								
ZZZZZZ	2	17:39																								
ZZZZZZ	2	17:43																								
ZZZZZZ	2	17:47																								
248118001	2	17:51			X		X											X	X			X				
248118002	2	17:55			X		X											X	X			X				
248118003	2	17:59			X		X											X	X			X				
248118004	2	18:03			X		X											X	X			X				
248118005	2	18:07			X		X											X	X			X				
248118006	2	18:11			X		X											X	X			X				
248118007	2	18:15			X		X											X	X			X				
CCV04	1	18:19			X		X											X	X			X				
CCB04	1	18:23			X		X											X	X			X				

Metals
-14-
Analysis Run Log

Contract: LANL01004

Lab Code: GEL

Inst Name: ICPMS6

Start Date: 25-MAR-10

End Date: 26-MAR-10

Client Sdg: 10-2093-1

Method MS

Data File: 100325-3

Samp No.	D/F	Run Time	Al	Sb	As	Ba	Be	Cd	Ca	Cr	Co	Cu	Fe	Pb	Mg	Mn	Hg	Ni	K	Se	Ag	Na	Tl	U	V	Zn
S0.0	1	23:39																						X		
S10	1	23:42																						X		
S100	1	23:45																						X		
ICV01	1	23:48																						X		
ICB01	1	23:52																						X		
CRDL01	1	23:55																						X		
ICSA01	1	23:58																						X		
ICSAB01	1	00:01																						X		
CCV01	1	00:04																						X		
CCB01	1	00:07																						X		
ZZZZZZ	2	00:10																								
ZZZZZZ	2	00:13																								
ZZZZZZ	2	00:16																								
ZZZZZZ	2	00:19																								
ZZZZZZ	2	00:22																								
ZZZZZZ	2	00:25																								
ZZZZZZ	2	00:28																								
CCV02	1	00:32																						X		
CCB02	1	00:35																						X		
1202056883	2	00:38																						X		
1202056888	40	00:41																						X		
ZZZZZZ	2	00:44																								
1202056884	2	00:47																						X		
1202056886	2	00:50																						X		
1202056887	2	00:53																						X		
1202056885	10	00:56																						X		
ZZZZZZ	2	00:59																								
CCV03	1	01:02																						X		
CCB03	1	01:05																						X		
ZZZZZZ	2	01:08																								
ZZZZZZ	2	01:11																								
ZZZZZZ	2	01:15																								
ZZZZZZ	2	01:18																								
ZZZZZZ	2	01:21																								
ZZZZZZ	2	01:24																								
248118001	2	01:27																						X		
248118002	2	01:30																						X		
248118003	2	01:33																						X		
CCV04	1	01:36																						X		
CCB04	1	01:39																						X		

[illegible]

Metals
-14-
Analysis Run Log

Contract: LANL01004

Lab Code: GEL

Inst Name: OPTIMA4

Start Date: 29-MAR-10

Client Sdg: 10-2093-1

Method P

Data File: 032910C-1

End Date: 29-MAR-10

Samp No.	D/F	Run Time	Al	Sb	As	Ba	Be	Cd	Ca	Cr	Co	Cu	Fe	Pb	Mg	Mn	Hg	Ni	K	Se	Ag	Na	Ti	U	V	Zn
S0.0	1	18:25	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
S0.1	1	18:28		X		X		X		X	X	X		X		X			X		X				X	X
S0.5	1	18:30	X	X		X		X	X	X	X	X		X	X	X			X		X				X	X
SCAL	1	18:32	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
S10	1	18:34	X						X				X		X							X				
ICV01	1	18:35	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
ICB01	1	18:37	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
PQL01	1	18:40	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
ICSA01	1	18:43	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
ICSAB01	1	18:45	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
LR01	1	18:46	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
LR02	1	18:48	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
CCV01	1	18:49	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
CCB01	1	18:51	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
CCV02	1	18:57	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
CCB02	1	18:59	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
ZZZZZZ	1	19:17																								
ZZZZZZ	1	19:20																								
ZZZZZZ	1	19:21																								
ZZZZZZ	1	19:23																								
ZZZZZZ	1	19:25																								
ZZZZZZ	1	19:26																								
ZZZZZZ	5	19:29																								
CCV03	1	19:31	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
CCB03	1	19:33	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
ZZZZZZ	1	19:36																								
ZZZZZZ	1	19:38																								
ZZZZZZ	1	19:40																								
ZZZZZZ	1	19:42																								
ZZZZZZ	1	19:44																								
ZZZZZZ	1	19:46																								
ZZZZZZ	1	19:48																								
ZZZZZZ	1	19:50																								
CCV04	1	19:52	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
CCB04	1	19:54	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
ZZZZZZ	1	19:57																								
ZZZZZZ	1	19:59																								
ZZZZZZ	1	20:02																								
ZZZZZZ	1	20:04																								
ZZZZZZ	1	20:06																								

Samp No.	D/F	Run Time																								
ZZZZZZ	1	20:08																								
ZZZZZZ	1	20:10																								
ZZZZZZ	1	20:12																								
CCV05	1	20:14	X	X		X		X	X	X	X	X	X	X	X		X		X	X		X	X			
CCB05	1	20:16	X	X		X		X	X	X	X	X	X	X	X		X		X	X		X	X			
ZZZZZZ	1	20:20																								
ZZZZZZ	1	20:23																								
ZZZZZZ	1	20:25																								
ZZZZZZ	1	20:28																								
ZZZZZZ	1	20:31																								
ZZZZZZ	5	20:33																								
ZZZZZZ	1	20:36																								
CCV06	1	20:39	X	X		X		X	X	X	X	X	X	X	X		X		X	X		X	X			
CCB06	1	20:41	X	X		X		X	X	X	X	X	X	X	X		X		X	X		X	X			
ZZZZZZ	1	20:44																								
ZZZZZZ	1	20:47																								
ZZZZZZ	1	20:50																								
ZZZZZZ	1	20:52																								
ZZZZZZ	1	20:55																								
ZZZZZZ	1	20:57																								
ZZZZZZ	1	21:00																								
CCV07	1	21:03	X	X		X		X	X	X	X	X	X	X	X		X		X	X		X	X			
CCB07	1	21:05	X	X		X		X	X	X	X	X	X	X	X		X		X	X		X	X			
ZZZZZZ	1	21:08																								
ZZZZZZ	1	21:11																								
ZZZZZZ	1	21:12																								
ZZZZZZ	1	21:14																								
ZZZZZZ	1	21:16																								
ZZZZZZ	1	21:18																								
ZZZZZZ	5	21:19																								
CCV08	1	21:21	X	X		X		X	X	X	X	X	X	X	X		X		X	X		X	X			
CCB08	1	21:23	X	X		X		X	X	X	X	X	X	X	X		X		X	X		X	X			
ZZZZZZ	1	21:26																								
ZZZZZZ	1	21:28																								
ZZZZZZ	1	21:30																								
ZZZZZZ	1	21:32																								
ZZZZZZ	1	21:34																								
ZZZZZZ	1	21:37																								
ZZZZZZ	1	21:39																								
CCV09	1	21:41	X	X		X		X	X	X	X	X	X	X	X		X		X	X		X	X			

Metals
-14-
Analysis Run Log

Samp No.	D/F	Run Time	Al	Sb	As	Ba	Be	Cd	Ca	Cr	Co	Cu	Fe	Pb	Mg	Mn	Hg	Ni	K	Se	Ag	Na	Tl	U	V	Zn
CCB09	1	21:43	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
ZZZZZZ	1	21:46																								
ZZZZZZ	1	21:48																								
ZZZZZZ	1	21:50																								
ZZZZZZ	1	21:52																								
ZZZZZZ	1	21:54																								
ZZZZZZ	1	21:56																								
ZZZZZZ	1	21:58																								
CCV10	1	22:01	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
CCB10	1	22:03	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
ZZZZZZ	1	22:06																								
ZZZZZZ	1	22:08																								
ZZZZZZ	1	22:10																								
ZZZZZZ	1	22:13																								
ZZZZZZ	1	22:15																								
ZZZZZZ	5	22:17																								
CCV11	1	22:19	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
CCB11	1	22:21	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
ZZZZZZ	1	22:24																								
ZZZZZZ	1	22:27																								
ZZZZZZ	1	22:29																								
ZZZZZZ	1	22:31																								
ZZZZZZ	1	22:34																								
ZZZZZZ	1	22:36																								
ZZZZZZ	1	22:39																								
CCV12	1	22:42	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
CCB12	1	22:44	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
1202056877	1	22:47	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
1202056882	1	22:49	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
ZZZZZZ	1	22:50																								
1202056878	1	22:52	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
1202056880	1	22:55	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
1202056881	1	22:56	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
1202056879	5	22:57	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
CCV13	1	22:59	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
CCB13	1	23:01	X	X		X		X	X	X	X	X	X	X	X	X			X		X	X			X	X
ZZZZZZ	1	23:04																								
ZZZZZZ	1	23:06																								
ZZZZZZ	1	23:08																								
ZZZZZZ	1	23:11																								

Metals
-14-
Analysis Run Log

[illegible]

Metals
-14-
Analysis Run Log

Contract: LANL01004

Lab Code: GEL

Inst Name: MER536

Start Date: 10-MAR-10

End Date: 10-MAR-10

Client Sdg: 10-2093-1

Method: AV

Data File: 031010S1-4

Samp No.	D/F	Run Time	Al	Sb	As	Ba	Be	Cd	Ca	Cr	Co	Cu	Fe	Pb	Mg	Mn	Hg	Ni	K	Se	Ag	Na	Ti	U	V	Zn
S0.0	1	11:25															X									
S0.2	1	11:27															X									
S0.5	1	11:29															X									
S2.0	1	11:31															X									
S5.0	1	11:33															X									
S10	1	11:35															X									
ICV01	1	11:37															X									
ICB01	1	11:39															X									
CRDL01	1	11:41															X									
CCV01	1	11:43															X									
CCB01	1	11:45															X									
1202056179	1	11:47															X									
1202056180	10	11:49															X									
ZZZZZZ	1	11:51																								
1202056181	1	11:53															X									
1202056182	1	11:55															X									
1202056184	1	11:57															X									
1202056183	5	11:59															X									
ZZZZZZ	1	12:01																								
ZZZZZZ	1	12:03																								
ZZZZZZ	1	12:04																								
CCV02	1	12:06															X									
CCB02	1	12:09															X									
ZZZZZZ	1	12:11																								
ZZZZZZ	1	12:12																								
ZZZZZZ	1	12:14																								
ZZZZZZ	1	12:16																								
ZZZZZZ	1	12:18																								
ZZZZZZ	1	12:20																								
ZZZZZZ	1	12:22																								
ZZZZZZ	1	12:24																								
ZZZZZZ	1	12:26																								
ZZZZZZ	1	12:28																								
CCV03	1	12:31															X									
CCB03	1	12:33															X									
ZZZZZZ	1	12:35																								
ZZZZZZ	1	12:36																								
ZZZZZZ	1	12:38																								
ZZZZZZ	1	12:40																								
ZZZZZZ	10	12:42																								

Metals
-14-
Analysis Run Log

Samp No.	D/F	Run Time
ZZZZZZ	1	12:44
ZZZZZZ	1	12:46
ZZZZZZ	1	12:48
ZZZZZZ	1	12:50
ZZZZZZ	5	12:52
CCV04	1	12:54
CCB04	1	12:56
ZZZZZZ	1	12:58
ZZZZZZ	1	13:00
CCV05	1	13:06
CCB05	1	13:08
ZZZZZZ	1	13:10
ZZZZZZ	1	13:12
ZZZZZZ	1	13:14
ZZZZZZ	1	13:16
ZZZZZZ	1	13:18
ZZZZZZ	1	13:20
248118001	1	13:22
248118002	1	13:24
248118003	1	13:26
248118004	1	13:28
CCV06	1	13:30
CCB06	1	13:32
248118005	1	13:34
248118006	1	13:36
248118007	1	13:38
ZZZZZZ	1	13:40
ZZZZZZ	10	13:41
ZZZZZZ	1	13:43
ZZZZZZ	1	13:45
ZZZZZZ	1	13:47
ZZZZZZ	1	13:49
ZZZZZZ	5	13:51
CCV07	1	13:53
CCB07	1	13:55

Standards

METALS
-10-
Instrument Detection Limits

SDG NO. 10-2093-1

Contract: LANL01004

Lab Code: GEL

MDL Effective Date: 01-JUL-09

ICP/MS	<u>Analyte</u>	<u>Wavelength</u>	<u>MDL</u>	<u>RDL</u>
		<u>(nm)</u>	<u>ug/L</u>	<u>ug/L</u>
SOLID	Aluminum		15.0	50
	Antimony		0.5	3
	Arsenic		1.0	5
	Barium		0.5	2
	Beryllium		0.1	.5
	Cadmium		0.1	1
	Calcium		33.0	100
	Chromium		1.0	3
	Cobalt		0.3	1
	Copper		0.33	1
	Iron		25.0	100
	Lead		0.5	2
	Magnesium		7.5	25
	Manganese		1.0	5
	Nickel		0.5	2
	Potassium		80.0	300
	Selenium		2.5	5
	Silver		0.2	1
	Sodium		80.0	250
	Thallium		0.3	1
	Uranium		0.066	.2
	Vanadium		2.0	10
	Zinc		2.0	10

METALS
-10-
Instrument Detection Limits

SDG NO. 10-2093-1

Contract: LANL01004

Lab Code: GEL

MDL Effective Date: 15-JUN-09

	<u>Analyte</u>	<u>Wavelength</u> <u>(nm)</u>	<u>MDL</u> <u>ug/L</u>	<u>RDL</u> <u>ug/L</u>
MERCURY				
SOLID	Mercury		0.068	.2

METALS
-10-
Instrument Detection Limits

SDG NO. 10-2093-1

Contract: LANL01004

Lab Code: GEL

MDL Effective Date: 01-JUL-09

ICP	<u>Analyte</u>	<u>Wavelength</u>	<u>MDL</u>	<u>RDL</u>
		<u>(nm)</u>	<u>ug/L</u>	<u>ug/L</u>
SOLID	Aluminum	396.153	68.0	200
	Antimony	206.836	3.3	10
	Arsenic	188.979	5.0	30
	Barium	233.527	1.0	5
	Beryllium	313.107	1.0	5
	Cadmium	226.502	1.0	5
	Calcium	317.933	80.0	250
	Chromium	267.716	1.5	5
	Cobalt	228.616	1.5	5
	Copper	324.752	3.0	10
	Iron	238.204	80.0	250
	Lead	220.353	2.5	10
	Magnesium	279.077	85.0	300
	Manganese	257.61	2.0	10
	Nickel	231.604	1.5	5
	Potassium	766.49	64.0	250
	Selenium	196.026	5.0	30
	Silver	328.068	1.0	5
	Sodium	589.592	70.0	250
	Thallium	190.801	5.0	20
	Uranium	409.014	10.0	50
	Vanadium	292.402	1.0	5
	Zinc	213.857	3.3	10

METALS
-11-
Interelement Correction Factors

Lab Code: GEL

GEL Job No: 10-2093-1

Contract: LANL01004

Instrument: OPTIMA4

Effective Dates: 25-MAR-10

Interelement Correction Factors (apparent ppb analyte/ppm interferent)

Parmname	Wavelength	Aluminum	Antimony	Arsenic	Barium	Beryllium
Aluminum	396.153	0.00000	0.00000	0.00000	0.00000	0.00000
Antimony	206.836	0.00676	0.00000	0.00000	0.00000	0.00000
Arsenic	188.979	0.00000	0.00000	0.00000	0.00000	0.00000
Barium	233.527	0.00000	0.00000	0.00000	0.00000	0.00000
Beryllium	313.107	0.00000	0.00000	0.00000	0.00000	0.00000
Boron	249.677	0.00000	0.00000	0.00000	0.00000	0.00000
Cadmium	226.502	0.00000	0.00000	0.00000	0.00000	0.00000
Chromium	267.716	0.00000	0.00000	0.00000	0.00000	0.00000
Cobalt	228.616	0.00000	0.00000	0.00000	-0.98369	0.00000
Copper	324.752	0.00000	0.00000	0.00000	0.00000	0.00000
Lead	220.353	-0.06206	0.00000	0.00000	0.00000	0.00000
Magnesium	279.077	0.00000	0.00000	0.00000	0.00000	0.00000
Manganese	257.61	0.00000	0.00000	0.00000	0.00000	0.00000
Molybdenum	202.031	0.00000	0.00000	0.00000	0.00000	0.00000
Phosphorous	214.914	-0.22134	0.00000	0.00000	0.00000	0.00000
Potassium	766.49	0.22220	0.00000	0.00000	0.00000	0.00000
Selenium	196.026	0.00000	0.00000	0.00000	0.00000	0.00000
Silicon	251.611	0.00000	0.00000	0.00000	0.00000	0.00000
Silver	328.068	0.00000	0.00000	0.00000	0.00000	0.00000
Sodium	589.592	0.00000	0.00000	0.00000	0.00000	0.00000
Strontium	421.552	0.00000	0.00000	0.00000	0.00000	0.00000
Sulfur	181.975	0.00000	0.00000	0.00000	0.00000	0.00000
Thallium	190.801	0.00000	0.00000	0.00000	0.00000	0.00000
Tin	189.927	0.00000	0.00000	0.00000	0.00000	0.00000
Titanium	334.94	0.00000	0.00000	0.00000	0.00000	0.00000
Uranium	409.014	0.00000	0.00000	0.00000	0.00000	0.00000
Vanadium	292.402	0.00000	0.00000	0.00000	0.00000	0.00000
Zinc	213.857	-0.01674	0.00000	0.00000	0.00000	0.00000

METALS
-11-
Interelement Correction Factors

Lab Code: GELGEL Job No: **10-2093-1**

Contract: LANL01004

Instrument: OPTIMA4

Effective Dates: **25-MAR-10**

Interelement Correction Factors (apparent ppb analyte/ppm interferent)

Parmname	Wavelength	Boron	Cadmium	Chromium	Cobalt	Copper
Aluminum	396.153	0.00000	0.00000	0.00000	0.00000	0.00000
Antimony	206.836	0.00000	0.00000	14.9992	0.00000	0.00000
Arsenic	188.979	0.00000	0.00000	-9.49960	0.00000	0.00000
Barium	233.527	0.00000	0.00000	0.00000	0.00000	0.00000
Beryllium	313.107	0.00000	0.00000	0.00000	0.00000	0.00000
Boron	249.677	0.00000	0.00000	0.00000	3.47778	0.00000
Cadmium	226.502	0.00000	0.00000	0.00000	0.00000	0.00000
Chromium	267.716	0.00000	0.00000	0.00000	0.00000	0.00000
Cobalt	228.616	0.00000	0.00000	-0.18390	0.00000	0.00000
Copper	324.752	0.00000	0.00000	0.00000	-0.60088	0.00000
Lead	220.353	0.00000	0.00000	0.00000	0.04741	0.32747
Magnesium	279.077	0.00000	0.00000	0.00000	0.00000	0.00000
Manganese	257.61	0.00000	0.00000	0.00000	0.00000	0.00000
Molybdenum	202.031	0.00000	0.00000	0.00000	0.00000	0.00000
Phosphorous	214.914	0.00000	0.00000	0.00000	0.00000	10.9289
Potassium	766.49	0.00000	0.00000	0.00000	0.00000	0.00000
Selenium	196.026	0.00000	0.00000	0.00000	0.00000	0.00000
Silicon	251.611	0.00000	0.00000	0.00000	0.00000	0.00000
Silver	328.068	0.00000	0.00000	-0.07359	0.00000	0.00000
Sodium	589.592	0.00000	0.00000	0.00000	0.00000	0.00000
Strontium	421.552	0.00000	0.00000	0.00000	0.00000	0.00000
Sulfur	181.975	0.00000	0.00000	0.00000	0.00000	0.00000
Thallium	190.801	0.00000	0.00000	0.00000	5.02864	0.00000
Tin	189.927	0.00000	0.00000	0.00000	0.00000	0.00000
Titanium	334.94	0.00000	0.00000	0.33675	0.00000	0.00000
Uranium	409.014	0.00000	0.00000	1.18768	0.00000	0.00000
Vanadium	292.402	0.00000	0.00000	-4.30004	0.00000	0.00000
Zinc	213.857	0.00000	0.00000	0.03286	0.12442	0.79397

METALS
-11-
Interelement Correction Factors

Lab Code: GEL

GEL Job No: 10-2093-1

Contract: LANL01004

Instrument: OPTIMA4

Effective Dates: 25-MAR-10

Interelement Correction Factors (apparent ppb analyte/ppm interferent)

Parmname	Wavelength	Lead	Magnesium	Manganese	Molybdenum	Phosphorous
Aluminum	396.153	0.00000	0.00000	0.00000	46.4438	0.00000
Antimony	206.836	0.00000	0.00000	0.00000	-14.0269	0.00000
Arsenic	188.979	0.00000	0.00000	0.00000	-2.84596	0.00000
Barium	233.527	0.00000	0.00000	0.00000	-0.32136	0.00000
Beryllium	313.107	0.00000	0.00000	0.00000	0.00000	0.00000
Boron	249.677	0.00000	0.00000	0.00000	0.00000	0.00000
Cadmium	226.502	0.00000	0.00000	0.00000	0.00000	0.00000
Chromium	267.716	0.00000	0.01216	0.24903	0.00000	0.00000
Cobalt	228.616	0.00000	0.00000	0.00000	0.00000	0.00000
Copper	324.752	0.00000	-0.02702	0.00000	0.00000	0.00000
Lead	220.353	0.00000	0.00000	0.00000	-2.77286	0.00000
Magnesium	279.077	0.00000	0.00000	0.00000	-24.4630	0.00000
Manganese	257.61	0.00000	0.03966	0.00000	0.00000	0.00000
Molybdenum	202.031	0.00000	0.00000	0.00000	-0.01826	0.00000
Phosphorous	214.914	0.00000	0.00000	0.00000	10.3832	0.00000
Potassium	766.49	0.00000	0.07568	0.00000	0.00000	0.00000
Selenium	196.026	0.00000	0.00000	0.00000	0.00000	0.00000
Silicon	251.611	0.00000	0.00000	0.00000	13.3443	0.00000
Silver	328.068	0.00000	0.00000	0.28019	-0.03095	0.00000
Sodium	589.592	0.00000	0.00000	0.00000	0.00000	0.00000
Strontium	421.552	0.00000	0.00000	0.00000	0.00000	0.00000
Sulfur	181.975	0.00000	0.00000	0.00000	-8.43314	0.00000
Thallium	190.801	0.00000	0.00000	-2.58065	0.00000	0.00000
Tin	189.927	0.00000	0.00000	0.00000	0.00000	0.00000
Titanium	334.94	0.00000	0.08144	0.00000	0.00000	0.00000
Uranium	409.014	0.00000	0.00000	-6.48399	0.00000	0.00000
Vanadium	292.402	0.00000	0.00000	0.00000	-10.3466	0.00000
Zinc	213.857	0.00000	0.00000	0.06887	-0.04597	0.00000

METALS
-11-
Interelement Correction Factors

Lab Code: GEL

GEL Job No: 10-2093-1

Contract: LANL01004

Instrument: OPTIMA4

Effective Dates: 25-MAR-10

Interelement Correction Factors (apparent ppb analyte/ppm interferent)

Parmname	Wavelength	Potassium	Selenium	Silicon	Silver	Sodium
Aluminum	396.153	0.00000	0.00000	0.00000	0.00000	0.00000
Antimony	206.836	0.00000	0.00000	0.00000	0.00000	0.00000
Arsenic	188.979	0.00000	0.00000	0.00000	0.00000	0.00000
Barium	233.527	0.00000	0.00000	0.00000	0.00000	0.00000
Beryllium	313.107	0.00000	0.00000	0.00000	0.00000	0.00000
Boron	249.677	0.00000	0.00000	0.00000	0.00000	0.00000
Cadmium	226.502	0.00000	0.00000	0.00000	0.00000	0.00000
Chromium	267.716	0.00000	0.00000	0.00000	0.00000	0.00000
Cobalt	228.616	0.00000	0.00000	0.00000	0.00000	0.00000
Copper	324.752	0.00000	0.00000	0.00000	0.00000	0.00000
Lead	220.353	0.00000	0.00000	0.00000	0.00000	0.00000
Magnesium	279.077	0.00000	0.00000	0.00000	0.00000	0.00000
Manganese	257.61	0.00000	0.00000	0.00000	0.00000	0.00000
Molybdenum	202.031	0.00000	0.00000	0.00000	0.00000	0.00000
Phosphorous	214.914	0.00000	0.00000	0.00000	0.00000	0.00000
Potassium	766.49	0.00000	0.00000	0.00000	0.00000	0.16274
Selenium	196.026	0.00000	0.00000	0.00000	0.00000	0.00000
Silicon	251.611	0.00000	0.00000	0.00000	0.00000	0.00000
Silver	328.068	0.00000	0.00000	0.00000	0.00000	0.00000
Sodium	589.592	0.88937	0.00000	0.00000	0.00000	0.00000
Strontium	421.552	0.00000	0.00000	0.00000	0.00000	0.00000
Sulfur	181.975	0.00000	0.00000	0.00000	0.00000	0.00000
Thallium	190.801	0.00000	0.00000	0.00000	0.00000	0.00000
Tin	189.927	0.00000	0.00000	0.00000	0.00000	0.00000
Titanium	334.94	0.00000	0.00000	0.00000	0.00000	0.00000
Uranium	409.014	0.00000	0.00000	0.00000	0.00000	0.00000
Vanadium	292.402	0.00000	0.00000	0.00000	0.00000	0.00000
Zinc	213.857	0.00000	0.00000	0.00000	0.00000	0.00000

METALS
-11-
Interelement Correction Factors

Lab Code: GEL

GEL Job No: 10-2093-1

Contract: LANL01004

Instrument: OPTIMA4

Effective Dates: 25-MAR-10

Interelement Correction Factors (apparent ppb analyte/ppm interferent)

Parmname	Wavelength	Strontium	Sulfur	Thallium	Tin	Titanium
Aluminum	396.153	0.00000	0.00000	0.00000	0.00000	0.00000
Antimony	206.836	0.00000	0.00000	0.00000	-1.82716	0.00000
Arsenic	188.979	0.00000	0.00000	0.00000	0.00000	0.00000
Barium	233.527	0.00000	0.00000	0.00000	0.00000	0.00000
Beryllium	313.107	0.00000	0.00000	0.00000	0.00000	0.00000
Boron	249.677	0.00000	0.00000	0.00000	0.00000	0.00000
Cadmium	226.502	0.00000	0.00000	0.00000	0.00000	0.00000
Chromium	267.716	0.00000	0.00000	0.00000	0.00000	0.00000
Cobalt	228.616	0.00000	0.00000	0.00000	0.00000	0.00000
Copper	324.752	0.00000	0.00000	0.00000	0.00000	0.00000
Lead	220.353	0.00000	0.00000	0.00000	0.00000	-1.32991
Magnesium	279.077	0.00000	0.00000	0.00000	0.00000	0.00000
Manganese	257.61	0.00000	0.00000	0.00000	0.00000	0.00000
Molybdenum	202.031	0.00000	0.00000	0.00000	0.00000	0.00000
Phosphorous	214.914	0.00000	0.00000	0.00000	-8.61809	0.00000
Potassium	766.49	0.00000	0.00000	0.00000	0.00000	0.00000
Selenium	196.026	0.00000	0.00000	0.00000	0.00000	0.00000
Silicon	251.611	0.00000	0.00000	0.00000	6.59640	0.00000
Silver	328.068	0.00000	0.00000	0.00000	0.00000	0.00000
Sodium	589.592	0.00000	0.00000	0.00000	0.00000	0.00000
Strontium	421.552	0.00000	0.00000	0.00000	0.00000	0.00000
Sulfur	181.975	0.00000	0.00000	0.00000	0.00000	0.00000
Thallium	190.801	0.00000	0.00000	0.00000	0.00000	-10.0432
Tin	189.927	0.00000	0.00000	0.00000	0.00000	-3.37234
Titanium	334.94	0.00000	0.00000	0.00000	0.00000	0.00000
Uranium	409.014	0.00000	0.00000	0.00000	0.00000	0.00000
Vanadium	292.402	0.00000	0.00000	0.00000	0.00000	0.92753
Zinc	213.857	0.00000	0.00000	0.00000	0.00000	-0.56798

METALS
-11-
Interelement Correction Factors

Lab Code: GEL

GEL Job No: 10-2093-1

Contract: LANL01004

Instrument: OPTIMA4

Effective Dates: 25-MAR-10

Interelement Correction Factors (apparent ppb analyte/ppm interferent)

Parmname	Wavelength	Uranium	Vanadium	Zinc
Aluminum	396.153	0.00000	0.00000	0.00000
Antimony	206.836	0.00000	-1.62578	0.00000
Arsenic	188.979	0.00000	0.00000	0.00000
Barium	233.527	0.00000	-0.63442	0.00000
Beryllium	313.107	-0.30229	0.00000	0.00000
Boron	249.677	0.00000	0.00000	0.00000
Cadmium	226.502	0.00000	0.00000	0.00000
Chromium	267.716	0.78601	-0.47146	0.00000
Cobalt	228.616	0.00000	0.00000	0.00000
Copper	324.752	-0.82619	0.00000	0.00000
Lead	220.353	0.74521	0.00000	0.00000
Magnesium	279.077	0.00000	0.00000	0.00000
Manganese	257.61	0.00000	0.00000	0.00000
Molybdenum	202.031	0.00000	-0.33953	0.00000
Phosphorous	214.914	0.00000	0.00000	0.00000
Potassium	766.49	0.00000	0.00000	0.00000
Selenium	196.026	-0.96499	0.00000	0.00000
Silicon	251.611	0.00000	0.00000	0.00000
Silver	328.068	-1.22996	-11.9401	0.00000
Sodium	589.592	0.00000	0.00000	0.00000
Strontium	421.552	0.00000	0.00000	0.00000
Sulfur	181.975	0.00000	0.00000	0.00000
Thallium	190.801	0.00000	-7.37871	0.00000
Tin	189.927	0.00000	0.00000	0.00000
Titanium	334.94	0.40930	0.00000	0.00000
Uranium	409.014	0.00000	-57.5852	0.00000
Vanadium	292.402	-0.67226	0.00000	0.00000
Zinc	213.857	0.00000	0.00000	0.00000

METALS
-12-
Linear Ranges

SDG NO. 10-2093-1

Contract: LANL01004

Lab Code: GEL

Instrument ID ICPMS6

<u>Analyte</u>	<u>Integration Time (msec)</u>	<u>LDR</u>	<u>Units</u>	<u>Effective Date</u>
Potassium	1	50000	ug/L	01-FEB-10
Selenium	1000	500	ug/L	01-FEB-10
Silver	1000	250	ug/L	01-FEB-10
Sodium	1	50000	ug/L	01-FEB-10
Thallium	1000	500	ug/L	01-FEB-10
Uranium	1000	5000	ug/L	01-FEB-10
Vanadium	1000	100	ug/L	01-FEB-10
Zinc	1000	2500	ug/L	01-FEB-10
Aluminum	1	50000	ug/L	01-FEB-10
Antimony	1000	250	ug/L	01-FEB-10
Arsenic	1000	1000	ug/L	01-FEB-10
Barium	1000	1000	ug/L	01-FEB-10
Beryllium	1000	1000	ug/L	01-FEB-10
Cadmium	1000	1000	ug/L	01-FEB-10
Calcium	500	50000	ug/L	01-FEB-10
Chromium	1000	1000	ug/L	01-FEB-10
Cobalt	1000	1000	ug/L	01-FEB-10
Copper	1000	1000	ug/L	01-FEB-10
Iron	500	50000	ug/L	01-FEB-10
Lead	1000	5000	ug/L	01-FEB-10
Magnesium	1	50000	ug/L	01-FEB-10
Manganese	1000	1000	ug/L	01-FEB-10
Nickel	1000	1000	ug/L	01-FEB-10

METALS
-12-
Linear Ranges

SDG NO. 10-2093-1

Contract: LANL01004

Lab Code: GEL

Instrument ID OPTIMA4

<u>Analyte</u>	<u>Integration Time (sec)</u>	<u>LDR</u>	<u>Units</u>	<u>Effective Date</u>
Aluminum	20	500000	ug/L	01-FEB-10
Antimony	20	10000	ug/L	01-FEB-10
Arsenic	20	10000	ug/L	01-FEB-10
Barium	20	15000	ug/L	01-FEB-10
Beryllium	20	3000	ug/L	01-FEB-10
Cadmium	20	10000	ug/L	01-FEB-10
Calcium	20	500000	ug/L	01-FEB-10
Chromium	20	25000	ug/L	01-FEB-10
Cobalt	20	10000	ug/L	01-FEB-10
Copper	20	20000	ug/L	01-FEB-10
Iron	20	500000	ug/L	01-FEB-10
Lead	20	25000	ug/L	01-FEB-10
Magnesium	20	500000	ug/L	01-FEB-10
Manganese	20	10000	ug/L	01-FEB-10
Nickel	20	10000	ug/L	01-FEB-10
Potassium	20	300000	ug/L	01-FEB-10
Selenium	20	10000	ug/L	01-FEB-10
Silver	20	1000	ug/L	01-FEB-10
Sodium	20	500000	ug/L	01-FEB-10
Thallium	20	10000	ug/L	01-FEB-10
Uranium	20	15000	ug/L	01-FEB-10
Vanadium	20	10000	ug/L	01-FEB-10
Zinc	20	15000	ug/L	01-FEB-10

Raw Data

The autosampler is not connecting.

It is not possible to establish a connection to the autosampler.

Make sure that the autosampler is powered on and that the cable is connected. Then go to the Autosampler page in the Diagnostics window and click on the Reconnect button.
[0603]

=====

Reprocessing Begun

Logged In Analyst: optima4

Technique: ICP Continuous

Results Data Set (original): 032910B

Results Library (original): C:\pe\optima4\Results\Results.mdb

Results Data Set (reprocessed): 032910C

Results Library (reprocessed): C:\pe\optima4\Results\Results.mdb

=====

Method Loaded

Method Name: Gen Eng fast_new Si

Method Last Saved: 3/29/2010 19:12:39

IEC File: 031810.iec

MSF File:

Method Description:

Analyte	Calibration Equation	Processing	View	Internal Standard	IEC
Ag 328.068	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Al 396.153Radial	Lin Thru 0	Peak Area	Radial	Sc RADIAL	Yes
As 188.979	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
B 249.677	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Ba 233.527	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Be 313.107	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Ca 317.933Radial	Lin Thru 0	Peak Area	Radial	Sc RADIAL	No
Cd 226.502	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Co 228.616	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Cr 267.716	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Cu 324.752	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Fe 238.204 Radial	Lin Thru 0	Peak Area	Radial	Sc RADIAL	No
K 766.490 Radial	Lin Thru 0	Peak Area	Radial	Sc RADIAL	Yes
Mg 279.077 IEC	Lin Thru 0	Peak Area	Radial	Sc RADIAL	Yes
Mn 257.610	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Mo 202.031	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Na 589.592 Radial	Lin Thru 0	Peak Area	Radial	Sc RADIAL	Yes
Ni 231.604	Lin Thru 0	Peak Area	Axial	Sc 361.383	No
P 214.914	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Pb 220.353	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
S 181.975 Axial	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Sb 206.836	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Sc 361.383	Lin Thru 0	Peak Area	Axial	n/a	n/a
Sc RADIAL	Lin, Calc Int	Peak Area	Radial	n/a	n/a
Se 196.026	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
SiO2	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Si 251.611	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Sn 189.927	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Sr 421.552	Lin Thru 0	Peak Area	Radial	Sc RADIAL	Yes
Ti 334.940	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Tl 190.801	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
U 409.014	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
V 292.402	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes
Y 371.029	Lin, Calc Int	Peak Area	Axial	n/a	n/a
Zn 213.857	Lin Thru 0	Peak Area	Axial	Sc 361.383	Yes

=====

Sequence No.: 1

Autosampler Location: 8

Sample ID: S0

Date Collected: 3/29/2010 18:25:17

Analyst:

Data Type: Reprocessed on 3/29/2010 19:14:31

Logged In Analyst (Original) : optima4

Initial Sample Wt:

Initial Sample Vol:

Dilution:

Sample Prep Vol:

Replicate Data: S0

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Analysis Time
1	Sc 361.383	1675486.4	1675486.4	100.16 %	18:27:09
1	Sc RADIAL	146509.4	146509.4	101 %	18:25:47
1	Y 371.029	1022720.1	1022720.1	100.01 %	18:27:09
1	Ag 328.068†	2983.2	2978.4	[0.00] µg/L	18:27:11
1	Al 396.153Radial†	-35.1	-35.0	[0.00] µg/L	18:26:07
1	As 188.979†	-19.2	-19.2	[0.00] µg/L	18:27:31

1	B 249.677†	3447.9	3442.3	[0.00]	µg/L	18:27:11
1	Ba 233.527†	-170.9	-170.6	[0.00]	µg/L	18:27:31
1	Be 313.107†	-760.2	-759.0	[0.00]	µg/L	18:27:11
1	Ca 317.933Radial†	609.6	606.5	[0.00]	µg/L	18:26:07
1	Cd 226.502†	-94.3	-94.2	[0.00]	µg/L	18:27:31
1	Co 228.616†	-177.2	-176.9	[0.00]	µg/L	18:27:31
1	Cr 267.716†	191.1	190.8	[0.00]	µg/L	18:27:31
1	Cu 324.752†	2447.0	2443.1	[0.00]	µg/L	18:27:11
1	Fe 238.204 Radial†	120.7	120.1	[0.00]	µg/L	18:26:07
1	K 766.490 Radial†	1409.9	1402.7	[0.00]	µg/L	18:25:47
1	Mg 279.077 IEC†	182.4	181.4	[0.00]	µg/L	18:26:07
1	Mn 257.610†	83.5	83.4	[0.00]	µg/L	18:27:31
1	Mo 202.031†	-61.5	-61.4	[0.00]	µg/L	18:27:31
1	Na 589.592 Radial†	1727.7	1718.8	[0.00]	µg/L	18:25:47
1	Ni 231.604†	-12.7	-12.7	[0.00]	µg/L	18:27:31
1	P 214.914†	74.6	74.5	[0.00]	µg/L	18:27:31
1	Pb 220.353†	124.0	123.8	[0.00]	µg/L	18:27:31
1	S 181.975 Axial†	92.2	92.1	[0.00]	µg/L	18:27:31
1	Sb 206.836†	94.8	94.7	[0.00]	µg/L	18:27:31
1	Se 196.026†	10.9	10.9	[0.00]	µg/L	18:27:31
1	SiO2†	1567.1	1564.5	[0.00]	µg/L	18:27:31
1	Si 251.611†	683.3	682.2	[0.00]	µg/L	18:27:11
1	Sn 189.927†	-0.3	-0.3	[0.00]	µg/L	18:27:31
1	Sr 421.552†	-242.7	-241.5	[0.00]	µg/L	18:25:47
1	Ti 334.940†	661.0	659.9	[0.00]	µg/L	18:27:11
1	Tl 190.801†	-125.7	-125.5	[0.00]	µg/L	18:27:31
1	U 409.014†	-452.8	-452.0	[0.00]	µg/L	18:27:11
1	V 292.402†	515.3	514.5	[0.00]	µg/L	18:27:11
1	Zn 213.857†	458.0	457.2	[0.00]	µg/L	18:27:31
2	Sc 361.383	1673882.1	1673882.1	100.07	%	18:27:33
2	Sc RADIAL	143614.2	143614.2	98.5	%	18:26:09
2	Y 371.029	1022767.5	1022767.5	100.02	%	18:27:33
2	Ag 328.068†	3053.8	3051.7	[0.00]	µg/L	18:27:35
2	Al 396.153Radial†	-38.9	-39.5	[0.00]	µg/L	18:26:29
2	As 188.979†	-15.1	-15.1	[0.00]	µg/L	18:27:55
2	B 249.677†	3293.2	3291.1	[0.00]	µg/L	18:27:35
2	Ba 233.527†	-175.9	-175.8	[0.00]	µg/L	18:27:55
2	Be 313.107†	-530.4	-530.1	[0.00]	µg/L	18:27:35
2	Ca 317.933Radial†	602.3	611.3	[0.00]	µg/L	18:26:29
2	Cd 226.502†	-94.9	-94.9	[0.00]	µg/L	18:27:55
2	Co 228.616†	-169.1	-169.0	[0.00]	µg/L	18:27:55
2	Cr 267.716†	157.6	157.5	[0.00]	µg/L	18:27:55
2	Cu 324.752†	2326.2	2324.7	[0.00]	µg/L	18:27:35
2	Fe 238.204 Radial†	112.7	114.4	[0.00]	µg/L	18:26:29
2	K 766.490 Radial†	1475.1	1497.1	[0.00]	µg/L	18:26:09
2	Mg 279.077 IEC†	191.8	194.7	[0.00]	µg/L	18:26:29
2	Mn 257.610†	69.4	69.3	[0.00]	µg/L	18:27:55
2	Mo 202.031†	-55.1	-55.0	[0.00]	µg/L	18:27:55
2	Na 589.592 Radial†	1691.1	1716.3	[0.00]	µg/L	18:26:09
2	Ni 231.604†	-51.5	-51.5	[0.00]	µg/L	18:27:55
2	P 214.914†	99.0	98.9	[0.00]	µg/L	18:27:55
2	Pb 220.353†	108.5	108.4	[0.00]	µg/L	18:27:55
2	S 181.975 Axial†	90.3	90.2	[0.00]	µg/L	18:27:55
2	Sb 206.836†	81.0	81.0	[0.00]	µg/L	18:27:55
2	Se 196.026†	15.5	15.5	[0.00]	µg/L	18:27:55
2	SiO2†	1541.6	1540.6	[0.00]	µg/L	18:27:55
2	Si 251.611†	721.8	721.4	[0.00]	µg/L	18:27:35
2	Sn 189.927†	7.0	7.0	[0.00]	µg/L	18:27:55
2	Sr 421.552†	-264.2	-268.1	[0.00]	µg/L	18:26:09
2	Ti 334.940†	533.5	533.1	[0.00]	µg/L	18:27:35
2	Tl 190.801†	-121.5	-121.4	[0.00]	µg/L	18:27:55
2	U 409.014†	-565.6	-565.2	[0.00]	µg/L	18:27:35
2	V 292.402†	425.8	425.5	[0.00]	µg/L	18:27:35
2	Zn 213.857†	466.7	466.4	[0.00]	µg/L	18:27:55
3	Sc 361.383	1668955.0	1668955.0	99.772	%	18:27:57
3	Sc RADIAL	147139.1	147139.1	101	%	18:26:31
3	Y 371.029	1022257.2	1022257.2	99.968	%	18:27:57
3	Ag 328.068†	2864.4	2871.0	[0.00]	µg/L	18:27:59
3	Al 396.153Radial†	-21.4	-21.2	[0.00]	µg/L	18:26:51
3	As 188.979†	-8.4	-8.4	[0.00]	µg/L	18:28:20
3	B 249.677†	3326.1	3333.7	[0.00]	µg/L	18:27:59

3	Ba 233.527†	-178.4	-178.8	[0.00]	µg/L	18:28:20
3	Be 313.107†	-689.7	-691.3	[0.00]	µg/L	18:27:59
3	Ca 317.933Radial†	636.8	630.8	[0.00]	µg/L	18:26:51
3	Cd 226.502†	-94.0	-94.2	[0.00]	µg/L	18:28:20
3	Co 228.616†	-183.5	-183.9	[0.00]	µg/L	18:28:20
3	Cr 267.716†	132.1	132.4	[0.00]	µg/L	18:28:20
3	Cu 324.752†	2501.2	2506.9	[0.00]	µg/L	18:27:59
3	Fe 238.204 Radial†	106.3	105.3	[0.00]	µg/L	18:26:51
3	K 766.490 Radial†	1479.1	1465.2	[0.00]	µg/L	18:26:31
3	Mg 279.077 IEC†	185.6	183.9	[0.00]	µg/L	18:26:51
3	Mn 257.610†	87.1	87.3	[0.00]	µg/L	18:28:20
3	Mo 202.031†	-49.1	-49.2	[0.00]	µg/L	18:28:20
3	Na 589.592 Radial†	1664.8	1649.1	[0.00]	µg/L	18:26:31
3	Ni 231.604†	-58.4	-58.5	[0.00]	µg/L	18:28:20
3	P 214.914†	65.2	65.3	[0.00]	µg/L	18:28:20
3	Pb 220.353†	104.9	105.1	[0.00]	µg/L	18:28:20
3	S 181.975 Axial†	101.9	102.2	[0.00]	µg/L	18:28:20
3	Sb 206.836†	84.1	84.3	[0.00]	µg/L	18:28:20
3	Se 196.026†	6.3	6.3	[0.00]	µg/L	18:28:20
3	SiO2†	1609.7	1613.4	[0.00]	µg/L	18:28:20
3	Si 251.611†	624.2	625.6	[0.00]	µg/L	18:27:59
3	Sn 189.927†	-0.6	-0.6	[0.00]	µg/L	18:28:20
3	Sr 421.552†	-327.4	-324.4	[0.00]	µg/L	18:26:31
3	Ti 334.940†	714.3	716.0	[0.00]	µg/L	18:27:59
3	Tl 190.801†	-113.7	-113.9	[0.00]	µg/L	18:28:20
3	U 409.014†	-419.1	-420.1	[0.00]	µg/L	18:27:59
3	V 292.402†	354.6	355.5	[0.00]	µg/L	18:27:59
3	Zn 213.857†	468.5	469.6	[0.00]	µg/L	18:28:20

Mean Data: S0

Analyte	Mean Corrected Intensity	Std.Dev.	RSD	Calib Conc. Units
Sc 361.383	1672774.5	3403.67	0.20%	100.00 %
Sc RADIAL	145754.2	1879.88	1.29%	100 %
Y 371.029	1022581.6	281.95	0.03%	100.00 %
Ag 328.068†	2967.0	90.92	3.06%	[0.00] µg/L
Al 396.153Radial†	-31.9	9.54	29.92%	[0.00] µg/L
As 188.979†	-14.2	5.41	37.98%	[0.00] µg/L
B 249.677†	3355.7	78.00	2.32%	[0.00] µg/L
Ba 233.527†	-175.1	4.13	2.36%	[0.00] µg/L
Be 313.107†	-660.1	117.60	17.82%	[0.00] µg/L
Ca 317.933Radial†	616.2	12.87	2.09%	[0.00] µg/L
Cd 226.502†	-94.4	0.38	0.41%	[0.00] µg/L
Co 228.616†	-176.6	7.48	4.23%	[0.00] µg/L
Cr 267.716†	160.2	29.32	18.30%	[0.00] µg/L
Cu 324.752†	2424.9	92.45	3.81%	[0.00] µg/L
Fe 238.204 Radial†	113.3	7.45	6.58%	[0.00] µg/L
K 766.490 Radial†	1455.0	48.06	3.30%	[0.00] µg/L
Mg 279.077 IEC†	186.7	7.04	3.77%	[0.00] µg/L
Mn 257.610†	80.0	9.46	11.83%	[0.00] µg/L
Mo 202.031†	-55.2	6.06	10.98%	[0.00] µg/L
Na 589.592 Radial†	1694.7	39.52	2.33%	[0.00] µg/L
Ni 231.604†	-40.9	24.66	60.28%	[0.00] µg/L
P 214.914†	79.6	17.37	21.83%	[0.00] µg/L
Pb 220.353†	112.4	9.96	8.86%	[0.00] µg/L
S 181.975 Axial†	94.8	6.43	6.78%	[0.00] µg/L
Sb 206.836†	86.6	7.13	8.23%	[0.00] µg/L
Se 196.026†	10.9	4.59	42.08%	[0.00] µg/L
SiO2†	1572.9	37.13	2.36%	[0.00] µg/L
Si 251.611†	676.4	48.15	7.12%	[0.00] µg/L
Sn 189.927†	2.0	4.32	214.20%	[0.00] µg/L
Sr 421.552†	-278.0	42.30	15.22%	[0.00] µg/L
Ti 334.940†	636.3	93.67	14.72%	[0.00] µg/L
Tl 190.801†	-120.3	5.87	4.88%	[0.00] µg/L
U 409.014†	-479.1	76.26	15.92%	[0.00] µg/L
V 292.402†	431.8	79.70	18.46%	[0.00] µg/L
Zn 213.857†	464.4	6.40	1.38%	[0.00] µg/L

Sequence No.: 2
 Sample ID: S0.1
 Analyst:
 Logged In Analyst (Original) : optima4
 Initial Sample Wt:
 Dilution:

Autosampler Location: 2
 Date Collected: 3/29/2010 18:28:28
 Data Type: Reprocessed on 3/29/2010 19:14:33
 Initial Sample Vol:
 Sample Prep Vol:

Replicate Data: S0.1

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Analysis Time
1	Sc 361.383	1661946.1	1661946.1	99.353 %	18:29:20
1	Sc RADIAL	142262.8	142262.8	97.6 %	18:28:58
1	Y 371.029	1013636.7	1013636.7	99.125 %	18:29:20
1	Ag 328.068†	28004.5	25219.9	[100] µg/L	18:29:22
1	As 188.979†	214.7	230.4	[100] µg/L	18:29:42
1	B 249.677†	9080.8	5784.2	[100] µg/L	18:29:22
1	Ba 233.527†	21988.9	22307.2	[100] µg/L	18:29:22
1	Be 313.107†	303759.0	306398.2	[100] µg/L	18:29:20
1	Cd 226.502†	14418.1	14606.5	[100] µg/L	18:29:22
1	Co 228.616†	7233.5	7457.2	[100] µg/L	18:29:42
1	Cr 267.716†	11824.2	11741.0	[100] µg/L	18:29:22
1	Cu 324.752†	25515.5	23256.9	[100] µg/L	18:29:22
1	K 766.490 Radial†	3700.4	2336.2	[1000] µg/L	18:28:58
1	Mn 257.610†	75396.6	75807.8	[100] µg/L	18:29:22
1	Mo 202.031†	3080.8	3156.1	[100] µg/L	18:29:42
1	Ni 231.604†	8001.7	8094.7	[100] µg/L	18:29:22
1	P 214.914†	2111.9	2046.0	[500] µg/L	18:29:42
1	Pb 220.353†	1769.2	1668.3	[100] µg/L	18:29:42
1	S 181.975 Axial†	329.8	237.2	[200] µg/L	18:29:42
1	Sb 206.836†	823.1	741.9	[100] µg/L	18:29:42
1	Se 196.026†	270.2	261.0	[100] µg/L	18:29:42
1	SiO2†	11219.8	9720.0	[1069.5] µg/L	18:29:22
1	Si 251.611†	30808.9	30333.3	[500] µg/L	18:29:22
1	Sn 189.927†	1389.8	1396.8	[100] µg/L	18:29:42
1	Sr 421.552†	43261.6	44601.3	[100] µg/L	18:28:58
1	Ti 334.940†	97625.2	97625.0	[100] µg/L	18:29:22
1	Tl 190.801†	629.9	754.3	[100] µg/L	18:29:42
1	U 409.014†	1288.2	1775.7	[100] µg/L	18:29:22
1	V 292.402†	18219.3	17906.2	[100] µg/L	18:29:22
1	Zn 213.857†	16338.0	15980.0	[100] µg/L	18:29:22
2	Sc 361.383	1666549.8	1666549.8	99.628 %	18:29:44
2	Sc RADIAL	146980.5	146980.5	101 %	18:29:00
2	Y 371.029	1017353.0	1017353.0	99.489 %	18:29:44
2	Ag 328.068†	28245.8	25384.2	[100] µg/L	18:29:47
2	As 188.979†	216.8	231.9	[100] µg/L	18:30:07
2	B 249.677†	9095.6	5773.9	[100] µg/L	18:29:47
2	Ba 233.527†	22220.1	22478.2	[100] µg/L	18:29:47
2	Be 313.107†	301592.1	303378.7	[100] µg/L	18:29:44
2	Cd 226.502†	14444.4	14592.7	[100] µg/L	18:29:47
2	Co 228.616†	7194.5	7397.9	[100] µg/L	18:30:07
2	Cr 267.716†	11989.4	11874.0	[100] µg/L	18:29:47
2	Cu 324.752†	25454.5	23124.7	[100] µg/L	18:29:47
2	K 766.490 Radial†	3828.6	2341.7	[1000] µg/L	18:29:00
2	Mn 257.610†	75955.3	76159.0	[100] µg/L	18:29:47
2	Mo 202.031†	3072.9	3139.6	[100] µg/L	18:30:07
2	Ni 231.604†	7945.1	8015.7	[100] µg/L	18:29:47
2	P 214.914†	2095.0	2023.3	[500] µg/L	18:30:07
2	Pb 220.353†	1806.4	1700.7	[100] µg/L	18:30:07
2	S 181.975 Axial†	328.8	235.2	[200] µg/L	18:30:07
2	Sb 206.836†	831.1	747.6	[100] µg/L	18:30:07
2	Se 196.026†	268.7	258.8	[100] µg/L	18:30:07
2	SiO2†	11380.9	9850.6	[1069.5] µg/L	18:29:47
2	Si 251.611†	30908.3	30347.4	[500] µg/L	18:29:47
2	Sn 189.927†	1386.9	1390.0	[100] µg/L	18:30:07
2	Sr 421.552†	43897.3	43809.0	[100] µg/L	18:29:00
2	Ti 334.940†	97949.2	97678.7	[100] µg/L	18:29:47
2	Tl 190.801†	629.9	752.6	[100] µg/L	18:30:07
2	U 409.014†	1127.3	1610.7	[100] µg/L	18:29:47

2	V 292.402†	18287.8	17924.3	[100] µg/L	18:29:47
2	Zn 213.857†	16478.9	16076.1	[100] µg/L	18:29:47
3	Sc 361.383	1678711.7	1678711.7	100.35 %	18:30:09
3	Sc RADIAL	143945.0	143945.0	98.8 %	18:29:02
3	Y 371.029	1024374.9	1024374.9	100.18 %	18:30:09
3	Ag 328.068†	27960.9	24894.9	[100] µg/L	18:30:11
3	As 188.979†	221.3	234.7	[100] µg/L	18:30:31
3	B 249.677†	9088.4	5700.5	[100] µg/L	18:30:11
3	Ba 233.527†	21982.2	22079.5	[100] µg/L	18:30:11
3	Be 313.107†	305374.6	304954.6	[100] µg/L	18:30:09
3	Cd 226.502†	14449.3	14492.6	[100] µg/L	18:30:11
3	Co 228.616†	7225.7	7376.7	[100] µg/L	18:30:31
3	Cr 267.716†	11783.4	11581.4	[100] µg/L	18:30:11
3	Cu 324.752†	25635.6	23120.1	[100] µg/L	18:30:11
3	K 766.490 Radial†	3785.9	2378.5	[1000] µg/L	18:29:02
3	Mn 257.610†	75567.2	75219.9	[100] µg/L	18:30:11
3	Mo 202.031†	3088.5	3132.8	[100] µg/L	18:30:31
3	Ni 231.604†	7999.7	8012.3	[100] µg/L	18:30:11
3	P 214.914†	2091.9	2004.9	[500] µg/L	18:30:31
3	Pb 220.353†	1784.3	1665.6	[100] µg/L	18:30:31
3	S 181.975 Axial†	327.0	231.0	[200] µg/L	18:30:31
3	Sb 206.836†	817.3	727.8	[100] µg/L	18:30:31
3	Se 196.026†	251.7	239.9	[100] µg/L	18:30:31
3	SiO2†	11327.9	9715.0	[1069.5] µg/L	18:30:11
3	Si 251.611†	30819.3	30033.9	[500] µg/L	18:30:11
3	Sn 189.927†	1401.4	1394.4	[100] µg/L	18:30:31
3	Sr 421.552†	43851.5	44680.7	[100] µg/L	18:29:02
3	Ti 334.940†	97740.3	96758.3	[100] µg/L	18:30:11
3	Tl 190.801†	620.5	738.6	[100] µg/L	18:30:31
3	U 409.014†	1269.9	1744.5	[100] µg/L	18:30:11
3	V 292.402†	18059.5	17563.8	[100] µg/L	18:30:11
3	Zn 213.857†	16510.7	15987.9	[100] µg/L	18:30:11

Mean Data: S0.1

Analyte	Mean Corrected Intensity	Std.Dev.	RSD	Calib Conc. Units
Sc 361.383	1669069.2	8662.09	0.52%	99.778 %
Sc RADIAL	144396.1	2390.99	1.66%	99.1 %
Y 371.029	1018454.9	5453.26	0.54%	99.596 %
Ag 328.068†	25166.4	249.02	0.99%	[100] µg/L
As 188.979†	232.3	2.20	0.95%	[100] µg/L
B 249.677†	5752.9	45.63	0.79%	[100] µg/L
Ba 233.527†	22288.3	200.02	0.90%	[100] µg/L
Be 313.107†	304910.5	1510.27	0.50%	[100] µg/L
Cd 226.502†	14563.9	62.13	0.43%	[100] µg/L
Co 228.616†	7410.6	41.70	0.56%	[100] µg/L
Cr 267.716†	11732.1	146.47	1.25%	[100] µg/L
Cu 324.752†	23167.2	77.70	0.34%	[100] µg/L
K 766.490 Radial†	2352.1	22.98	0.98%	[1000] µg/L
Mn 257.610†	75728.9	474.50	0.63%	[100] µg/L
Mo 202.031†	3142.8	11.99	0.38%	[100] µg/L
Ni 231.604†	8040.9	46.63	0.58%	[100] µg/L
P 214.914†	2024.7	20.61	1.02%	[500] µg/L
Pb 220.353†	1678.2	19.56	1.17%	[100] µg/L
S 181.975 Axial†	234.4	3.15	1.34%	[200] µg/L
Sb 206.836†	739.1	10.21	1.38%	[100] µg/L
Se 196.026†	253.2	11.62	4.59%	[100] µg/L
SiO2†	9761.9	76.87	0.79%	[1069.5] µg/L
Si 251.611†	30238.2	177.02	0.59%	[500] µg/L
Sn 189.927†	1393.8	3.45	0.25%	[100] µg/L
Sr 421.552†	44363.6	481.98	1.09%	[100] µg/L
Ti 334.940†	97354.0	516.57	0.53%	[100] µg/L
Tl 190.801†	748.5	8.62	1.15%	[100] µg/L
U 409.014†	1710.3	87.69	5.13%	[100] µg/L
V 292.402†	17798.1	203.14	1.14%	[100] µg/L
Zn 213.857†	16014.7	53.32	0.33%	[100] µg/L

Sequence No.: 3
 Sample ID: S0.5
 Analyst:
 Logged In Analyst (Original) : optima4
 Initial Sample Wt:
 Dilution:

Autosampler Location: 3
 Date Collected: 3/29/2010 18:30:39
 Data Type: Reprocessed on 3/29/2010 19:14:34
 Initial Sample Vol:
 Sample Prep Vol:

Replicate Data: S0.5

Repl#	Analyte	Net Intensity	Corrected Intensity	Conc. Units	Analysis Time
1	Sc 361.383	1666330.4	1666330.4	99.615 %	18:31:37
1	Sc RADIAL	146255.9	146255.9	100 %	18:31:10
1	Y 371.029	1010770.4	1010770.4	98.845 %	18:31:37
1	Ag 328.068†	124810.0	122325.6	[500] µg/L	18:31:37
1	Al 396.153Radial†	22730.9	22684.8	[5000] µg/L	18:31:10
1	As 188.979†	1130.3	1148.9	[500] µg/L	18:31:57
1	B 249.677†	32443.2	29213.0	[500] µg/L	18:31:37
1	Ba 233.527†	108021.9	108614.7	[500] µg/L	18:31:37
1	Be 313.107†	1516563.3	1523088.3	[500] µg/L	18:31:37
1	Ca 317.933Radial†	86179.3	85267.4	[5000] µg/L	18:31:10
1	Cd 226.502†	71219.1	71589.0	[500] µg/L	18:31:37
1	Co 228.616†	35394.0	35707.4	[500] µg/L	18:31:57
1	Cr 267.716†	57615.1	57677.6	[500] µg/L	18:31:37
1	Cu 324.752†	116290.7	114315.5	[500] µg/L	18:31:37
1	K 766.490 Radial†	13629.8	12128.1	[5000] µg/L	18:31:10
1	Mg 279.077 IEC†	12468.2	12238.8	[5000] µg/L	18:31:10
1	Mn 257.610†	362696.8	364019.5	[500] µg/L	18:31:37
1	Mo 202.031†	15371.1	15485.8	[500] µg/L	18:31:57
1	Ni 231.604†	38767.1	38957.9	[500] µg/L	18:31:37
1	P 214.914†	10122.4	10082.0	[2500] µg/L	18:31:57
1	Pb 220.353†	8161.6	8080.8	[500] µg/L	18:31:57
1	S 181.975 Axial†	1278.6	1188.7	[1000] µg/L	18:31:57
1	Sb 206.836†	3687.2	3614.8	[500] µg/L	18:31:57
1	Se 196.026†	1225.0	1218.8	[500] µg/L	18:31:57
1	SiO2†	49926.4	48546.6	[5347.5] µg/L	18:31:37
1	Si 251.611†	150511.0	150416.7	[2500] µg/L	18:31:37
1	Sn 189.927†	6828.0	6852.4	[500] µg/L	18:31:57
1	Sr 421.552†	212817.9	212365.9	[500] µg/L	18:31:08
1	Ti 334.940†	484276.9	485513.3	[500] µg/L	18:31:37
1	Tl 190.801†	3503.2	3637.1	[500] µg/L	18:31:57
1	U 409.014†	6910.1	7415.9	[500] µg/L	18:31:37
1	V 292.402†	89155.4	89068.4	[500] µg/L	18:31:37
1	Zn 213.857†	79249.5	79091.5	[500] µg/L	18:31:37
2	Sc 361.383	1656377.5	1656377.5	99.020 %	18:32:00
2	Sc RADIAL	143364.9	143364.9	98.4 %	18:31:14
2	Y 371.029	1005040.5	1005040.5	98.285 %	18:32:00
2	Ag 328.068†	123893.4	122152.8	[500] µg/L	18:32:00
2	Al 396.153Radial†	22411.8	22817.2	[5000] µg/L	18:31:14
2	As 188.979†	1160.9	1186.7	[500] µg/L	18:32:21
2	B 249.677†	32166.0	29128.7	[500] µg/L	18:32:00
2	Ba 233.527†	106821.0	108053.5	[500] µg/L	18:32:00
2	Be 313.107†	1497872.7	1513360.7	[500] µg/L	18:32:00
2	Ca 317.933Radial†	83955.9	84739.0	[5000] µg/L	18:31:14
2	Cd 226.502†	70376.7	71167.8	[500] µg/L	18:32:00
2	Co 228.616†	35865.0	36396.7	[500] µg/L	18:32:21
2	Cr 267.716†	57094.1	57499.1	[500] µg/L	18:32:00
2	Cu 324.752†	115218.7	113934.4	[500] µg/L	18:32:00
2	K 766.490 Radial†	13146.4	11910.5	[5000] µg/L	18:31:14
2	Mg 279.077 IEC†	12081.5	12096.2	[5000] µg/L	18:31:14
2	Mn 257.610†	359096.8	362571.6	[500] µg/L	18:32:00
2	Mo 202.031†	15556.5	15765.7	[500] µg/L	18:32:21
2	Ni 231.604†	38151.2	38569.7	[500] µg/L	18:32:00
2	P 214.914†	10250.6	10272.5	[2500] µg/L	18:32:21
2	Pb 220.353†	8247.6	8216.9	[500] µg/L	18:32:21
2	S 181.975 Axial†	1295.5	1213.5	[1000] µg/L	18:32:21
2	Sb 206.836†	3729.7	3679.9	[500] µg/L	18:32:21
2	Se 196.026†	1259.6	1261.2	[500] µg/L	18:32:21
2	SiO2†	49488.1	48405.1	[5347.5] µg/L	18:32:00

2	Si 251.611†	149066.4	149865.6	[2500] µg/L	18:32:00
2	Sn 189.927†	6928.0	6994.5	[500] µg/L	18:32:21
2	Sr 421.552†	210571.1	214358.5	[500] µg/L	18:31:12
2	Ti 334.940†	480119.5	484236.0	[500] µg/L	18:32:00
2	Tl 190.801†	3520.8	3676.0	[500] µg/L	18:32:21
2	U 409.014†	6871.4	7418.6	[500] µg/L	18:32:00
2	V 292.402†	88228.0	88669.5	[500] µg/L	18:32:00
2	Zn 213.857†	78116.6	78425.5	[500] µg/L	18:32:00
3	Sc 361.383	1678591.9	1678591.9	100.35 %	18:32:24
3	Sc RADIAL	148088.8	148088.8	102 %	18:31:18
3	Y 371.029	1018746.9	1018746.9	99.625 %	18:32:24
3	Ag 328.068†	125886.3	122483.0	[500] µg/L	18:32:24
3	Al 396.153Radial†	22914.6	22585.2	[5000] µg/L	18:31:18
3	As 188.979†	1161.2	1171.4	[500] µg/L	18:32:44
3	B 249.677†	32821.8	29352.3	[500] µg/L	18:32:24
3	Ba 233.527†	108685.7	108484.1	[500] µg/L	18:32:24
3	Be 313.107†	1528160.6	1523524.6	[500] µg/L	18:32:24
3	Ca 317.933Radial†	86630.7	84648.8	[5000] µg/L	18:31:18
3	Cd 226.502†	72351.9	72195.6	[500] µg/L	18:32:24
3	Co 228.616†	36165.4	36216.7	[500] µg/L	18:32:44
3	Cr 267.716†	58224.7	57862.7	[500] µg/L	18:32:24
3	Cu 324.752†	117068.1	114237.5	[500] µg/L	18:32:24
3	K 766.490 Radial†	13544.3	11875.7	[5000] µg/L	18:31:18
3	Mg 279.077 IEC†	12711.0	12323.9	[5000] µg/L	18:31:18
3	Mn 257.610†	365977.4	364629.0	[500] µg/L	18:32:24
3	Mo 202.031†	15658.0	15658.9	[500] µg/L	18:32:44
3	Ni 231.604†	38949.9	38855.9	[500] µg/L	18:32:24
3	P 214.914†	10378.5	10262.9	[2500] µg/L	18:32:44
3	Pb 220.353†	8301.3	8160.1	[500] µg/L	18:32:44
3	S 181.975 Axial†	1298.3	1199.0	[1000] µg/L	18:32:44
3	Sb 206.836†	3757.3	3657.7	[500] µg/L	18:32:44
3	Se 196.026†	1268.4	1253.0	[500] µg/L	18:32:44
3	SiO2†	50453.3	48705.6	[5347.5] µg/L	18:32:24
3	Si 251.611†	151847.8	150645.2	[2500] µg/L	18:32:24
3	Sn 189.927†	6976.6	6950.4	[500] µg/L	18:32:44
3	Sr 421.552†	212729.2	209653.5	[500] µg/L	18:31:16
3	Ti 334.940†	487904.2	485577.0	[500] µg/L	18:32:24
3	Tl 190.801†	3573.5	3681.5	[500] µg/L	18:32:44
3	U 409.014†	7083.7	7538.2	[500] µg/L	18:32:24
3	V 292.402†	89928.1	89184.6	[500] µg/L	18:32:24
3	Zn 213.857†	79862.3	79121.1	[500] µg/L	18:32:24

Mean Data: S0.5

Analyte	Mean Corrected Intensity	Std.Dev.	RSD	Conc. Units	Calib
Sc 361.383	1667099.9	11127.18	0.67%	99.661 %	
Sc RADIAL	145903.2	2381.65	1.63%	100 %	
Y 371.029	1011519.3	6883.81	0.68%	98.918 %	
Ag 328.068†	122320.5	165.15	0.14%	[500] µg/L	
Al 396.153Radial†	22695.7	116.36	0.51%	[5000] µg/L	
As 188.979†	1169.0	19.01	1.63%	[500] µg/L	
B 249.677†	29231.4	112.94	0.39%	[500] µg/L	
Ba 233.527†	108384.1	293.66	0.27%	[500] µg/L	
Be 313.107†	1519991.2	5746.30	0.38%	[500] µg/L	
Ca 317.933Radial†	84885.1	334.21	0.39%	[5000] µg/L	
Cd 226.502†	71650.8	516.66	0.72%	[500] µg/L	
Co 228.616†	36106.9	357.49	0.99%	[500] µg/L	
Cr 267.716†	57679.8	181.81	0.32%	[500] µg/L	
Cu 324.752†	114162.5	201.35	0.18%	[500] µg/L	
K 766.490 Radial†	11971.4	136.75	1.14%	[5000] µg/L	
Mg 279.077 IEC†	12219.6	115.04	0.94%	[5000] µg/L	
Mn 257.610†	363740.0	1056.77	0.29%	[500] µg/L	
Mo 202.031†	15636.8	141.25	0.90%	[500] µg/L	
Ni 231.604†	38794.5	201.22	0.52%	[500] µg/L	
P 214.914†	10205.8	107.31	1.05%	[2500] µg/L	
Pb 220.353†	8152.6	68.35	0.84%	[500] µg/L	
S 181.975 Axial†	1200.4	12.45	1.04%	[1000] µg/L	
Sb 206.836†	3650.8	33.08	0.91%	[500] µg/L	
Se 196.026†	1244.3	22.47	1.81%	[500] µg/L	
SiO2†	48552.4	150.29	0.31%	[5347.5] µg/L	

Si 251.611†	150309.2	400.75	0.27%	[2500] µg/L
Sn 189.927†	6932.4	72.76	1.05%	[500] µg/L
Sr 421.552†	212126.0	2361.66	1.11%	[500] µg/L
Ti 334.940†	485108.8	756.53	0.16%	[500] µg/L
Tl 190.801†	3664.9	24.20	0.66%	[500] µg/L
U 409.014†	7457.6	69.86	0.94%	[500] µg/L
V 292.402†	88974.2	270.15	0.30%	[500] µg/L
Zn 213.857†	78879.4	393.36	0.50%	[500] µg/L

Sequence No.: 4
 Sample ID: SCAL
 Analyst:
 Logged In Analyst (Original) : optima4
 Initial Sample Wt:
 Dilution:

Autosampler Location: 4
 Date Collected: 3/29/2010 18:32:52
 Data Type: Reprocessed on 3/29/2010 19:14:34
 Initial Sample Vol:
 Sample Prep Vol:

Replicate Data: SCAL

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Analysis Time
1	Sc 361.383	1695274.3	1695274.3	101.35 %	18:33:51
1	Sc RADIAL	148093.8	148093.8	102 %	18:33:23
1	Y 371.029	1024428.2	1024428.2	100.18 %	18:33:51
1	Ag 328.068†	253437.3	247106.6	[1000] µg/L	18:33:51
1	Al 396.153Radial†	47074.8	46363.0	[10000] µg/L	18:33:23
1	As 188.979†	2423.7	2405.8	[1000] µg/L	18:33:53
1	B 249.677†	64171.5	59964.1	[1000] µg/L	18:33:51
1	Ba 233.527†	222696.0	219915.4	[1000] µg/L	18:33:51
1	Be 313.107†	3125497.2	3084675.4	[1000] µg/L	18:33:51
1	Ca 317.933Radial†	175989.6	172593.1	[10000] µg/L	18:33:23
1	Cd 226.502†	147319.9	145459.1	[1000] µg/L	18:33:51
1	Co 228.616†	73285.4	72489.3	[1000] µg/L	18:33:53
1	Cr 267.716†	118453.3	116720.9	[1000] µg/L	18:33:51
1	Cu 324.752†	236158.0	230598.8	[1000] µg/L	18:33:51
1	Fe 238.204 Radial†	153305.8	150770.6	[10000] µg/L	18:33:23
1	K 766.490 Radial†	26333.7	24462.7	[10000] µg/L	18:33:23
1	Mg 279.077 IEC†	25539.7	24949.5	[10000] µg/L	18:33:23
1	Mn 257.610†	742700.4	732763.2	[1000] µg/L	18:33:51
1	Mo 202.031†	31916.7	31548.3	[1000] µg/L	18:33:53
1	Na 589.592 Radial†	67840.0	65073.6	[10000] µg/L	18:33:23
1	Ni 231.604†	79543.1	78528.3	[1000] µg/L	18:33:51
1	P 214.914†	21051.1	20692.1	[5000] µg/L	18:33:53
1	Pb 220.353†	16751.4	16416.6	[1000] µg/L	18:33:53
1	S 181.975 Axial†	2600.1	2470.7	[2000] µg/L	18:33:53
1	Sb 206.836†	7615.0	7427.3	[1000] µg/L	18:33:53
1	Se 196.026†	2517.5	2473.2	[1000] µg/L	18:33:53
1	SiO2†	101024.7	98111.1	[10695] µg/L	18:33:51
1	Si 251.611†	307939.1	303175.7	[5000] µg/L	18:33:51
1	Sn 189.927†	14211.0	14020.4	[1000] µg/L	18:33:53
1	Sr 421.552†	434456.1	427870.5	[1000] µg/L	18:33:21
1	Ti 334.940†	997481.3	983606.3	[1000] µg/L	18:33:51
1	Tl 190.801†	7335.9	7358.9	[1000] µg/L	18:33:53
1	U 409.014†	16212.4	16476.3	[1000] µg/L	18:33:51
1	V 292.402†	183867.8	180995.7	[1000] µg/L	18:33:51
1	Zn 213.857†	161925.8	159312.2	[1000] µg/L	18:33:51
2	Sc 361.383	1690996.4	1690996.4	101.09 %	18:33:57
2	Sc RADIAL	145999.7	145999.7	100 %	18:33:27
2	Y 371.029	1021922.1	1021922.1	99.936 %	18:33:57
2	Ag 328.068†	252044.6	246361.5	[1000] µg/L	18:33:57
2	Al 396.153Radial†	46624.8	46578.3	[10000] µg/L	18:33:27
2	As 188.979†	2403.1	2391.4	[1000] µg/L	18:33:59
2	B 249.677†	63843.6	59800.0	[1000] µg/L	18:33:57
2	Ba 233.527†	221227.7	219018.9	[1000] µg/L	18:33:57
2	Be 313.107†	3107291.9	3074468.3	[1000] µg/L	18:33:57
2	Ca 317.933Radial†	173656.9	172748.8	[10000] µg/L	18:33:27
2	Cd 226.502†	146575.4	145090.3	[1000] µg/L	18:33:57
2	Co 228.616†	74805.8	74176.3	[1000] µg/L	18:33:59
2	Cr 267.716†	118015.5	116583.5	[1000] µg/L	18:33:57
2	Cu 324.752†	235118.6	230160.1	[1000] µg/L	18:33:57
2	Fe 238.204 Radial†	151211.1	150843.6	[10000] µg/L	18:33:27
2	K 766.490 Radial†	25931.4	24432.8	[10000] µg/L	18:33:27
2	Mg 279.077 IEC†	24969.0	24740.4	[10000] µg/L	18:33:27
2	Mn 257.610†	740445.3	732386.4	[1000] µg/L	18:33:57
2	Mo 202.031†	32495.1	32200.2	[1000] µg/L	18:33:59
2	Na 589.592 Radial†	67249.4	65441.6	[10000] µg/L	18:33:27
2	Ni 231.604†	79100.3	78288.9	[1000] µg/L	18:33:57
2	P 214.914†	21690.5	21377.2	[5000] µg/L	18:33:59
2	Pb 220.353†	17172.9	16875.4	[1000] µg/L	18:33:59

2	S 181.975 Axial†	2679.6	2555.9	[2000]	µg/L	18:33:59
2	Sb 206.836†	7635.7	7466.8	[1000]	µg/L	18:33:59
2	Se 196.026†	2666.5	2626.9	[1000]	µg/L	18:33:59
2	SiO2†	100664.8	98007.2	[10695]	µg/L	18:33:57
2	Si 251.611†	306502.8	302523.6	[5000]	µg/L	18:33:57
2	Sn 189.927†	14443.7	14286.0	[1000]	µg/L	18:33:59
2	Sr 421.552†	430963.7	430517.1	[1000]	µg/L	18:33:25
2	Ti 334.940†	993955.9	982608.8	[1000]	µg/L	18:33:57
2	Tl 190.801†	7531.3	7570.4	[1000]	µg/L	18:33:59
2	U 409.014†	16040.6	16346.9	[1000]	µg/L	18:33:57
2	V 292.402†	183235.5	180829.1	[1000]	µg/L	18:33:57
2	Zn 213.857†	161264.5	159062.3	[1000]	µg/L	18:33:57
3	Sc 361.383	1679595.4	1679595.4	100.41	%	18:34:04
3	Sc RADIAL	149693.3	149693.3	103	%	18:33:31
3	Y 371.029	1015550.9	1015550.9	99.312	%	18:34:04
3	Ag 328.068†	251016.5	247030.1	[1000]	µg/L	18:34:04
3	Al 396.153Radial†	47551.4	46332.0	[10000]	µg/L	18:33:31
3	As 188.979†	2421.2	2425.6	[1000]	µg/L	18:34:06
3	B 249.677†	63426.3	59813.0	[1000]	µg/L	18:34:04
3	Ba 233.527†	219963.3	219245.0	[1000]	µg/L	18:34:04
3	Be 313.107†	3093622.9	3081719.7	[1000]	µg/L	18:34:04
3	Ca 317.933Radial†	178184.0	172879.1	[10000]	µg/L	18:33:31
3	Cd 226.502†	145509.3	145012.8	[1000]	µg/L	18:34:04
3	Co 228.616†	73160.7	73040.2	[1000]	µg/L	18:34:06
3	Cr 267.716†	117369.2	116732.4	[1000]	µg/L	18:34:04
3	Cu 324.752†	233979.9	230604.8	[1000]	µg/L	18:34:04
3	Fe 238.204 Radial†	154947.1	150756.5	[10000]	µg/L	18:33:31
3	K 766.490 Radial†	26410.5	24260.6	[10000]	µg/L	18:33:31
3	Mg 279.077 IEC†	25740.2	24876.2	[10000]	µg/L	18:33:31
3	Mn 257.610†	735902.7	732834.1	[1000]	µg/L	18:34:04
3	Mo 202.031†	31675.9	31602.5	[1000]	µg/L	18:34:06
3	Na 589.592 Radial†	68591.3	65091.7	[10000]	µg/L	18:33:31
3	Ni 231.604†	78372.8	78095.4	[1000]	µg/L	18:34:04
3	P 214.914†	21100.1	20934.8	[5000]	µg/L	18:34:06
3	Pb 220.353†	16565.8	16386.1	[1000]	µg/L	18:34:06
3	S 181.975 Axial†	2538.8	2433.7	[2000]	µg/L	18:34:06
3	Sb 206.836†	7547.1	7429.8	[1000]	µg/L	18:34:06
3	Se 196.026†	2534.8	2513.6	[1000]	µg/L	18:34:06
3	SiO2†	99973.5	97994.7	[10695]	µg/L	18:34:04
3	Si 251.611†	304718.9	302805.0	[5000]	µg/L	18:34:04
3	Sn 189.927†	14107.2	14047.9	[1000]	µg/L	18:34:06
3	Sr 421.552†	434068.2	422924.1	[1000]	µg/L	18:33:29
3	Ti 334.940†	988596.9	983945.8	[1000]	µg/L	18:34:04
3	Tl 190.801†	7419.8	7510.0	[1000]	µg/L	18:34:06
3	U 409.014†	16237.0	16650.2	[1000]	µg/L	18:34:04
3	V 292.402†	181988.8	180817.9	[1000]	µg/L	18:34:04
3	Zn 213.857†	160057.9	158943.5	[1000]	µg/L	18:34:04

Mean Data: SCAL

Analyte	Mean Corrected Intensity	Std.Dev.	RSD	Calib Conc. Units
Sc 361.383	1688622.0	8104.65	0.48%	100.95 %
Sc RADIAL	147928.9	1852.30	1.25%	101 %
Y 371.029	1020633.7	4576.76	0.45%	99.810 %
Ag 328.068†	246832.7	409.85	0.17%	[1000] µg/L
Al 396.153Radial†	46424.4	134.12	0.29%	[10000] µg/L
As 188.979†	2407.6	17.16	0.71%	[1000] µg/L
B 249.677†	59859.0	91.23	0.15%	[1000] µg/L
Ba 233.527†	219393.1	466.22	0.21%	[1000] µg/L
Be 313.107†	3080287.8	5252.04	0.17%	[1000] µg/L
Ca 317.933Radial†	172740.3	143.17	0.08%	[10000] µg/L
Cd 226.502†	145187.4	238.43	0.16%	[1000] µg/L
Co 228.616†	73235.3	860.22	1.17%	[1000] µg/L
Cr 267.716†	116678.9	82.81	0.07%	[1000] µg/L
Cu 324.752†	230454.6	255.03	0.11%	[1000] µg/L
Fe 238.204 Radial†	150790.2	46.73	0.03%	[10000] µg/L
K 766.490 Radial†	24385.4	109.10	0.45%	[10000] µg/L
Mg 279.077 IEC†	24855.4	106.12	0.43%	[10000] µg/L
Mn 257.610†	732661.3	240.63	0.03%	[1000] µg/L
Mo 202.031†	31783.7	361.73	1.14%	[1000] µg/L

Na 589.592 Radial†	65202.3	207.44	0.32%	[10000]	µg/L
Ni 231.604†	78304.2	216.83	0.28%	[1000]	µg/L
P 214.914†	21001.4	347.34	1.65%	[5000]	µg/L
Pb 220.353†	16559.4	274.11	1.66%	[1000]	µg/L
S 181.975 Axial†	2486.8	62.65	2.52%	[2000]	µg/L
Sb 206.836†	7441.3	22.10	0.30%	[1000]	µg/L
Se 196.026†	2537.9	79.67	3.14%	[1000]	µg/L
SiO2†	98037.6	63.89	0.07%	[10695]	µg/L
Si 251.611†	302834.8	327.07	0.11%	[5000]	µg/L
Sn 189.927†	14118.1	146.08	1.03%	[1000]	µg/L
Sr 421.552†	427103.9	3854.12	0.90%	[1000]	µg/L
Ti 334.940†	983387.0	694.94	0.07%	[1000]	µg/L
Tl 190.801†	7479.8	108.97	1.46%	[1000]	µg/L
U 409.014†	16491.1	152.21	0.92%	[1000]	µg/L
V 292.402†	180880.9	99.54	0.06%	[1000]	µg/L
Zn 213.857†	159106.0	188.24	0.12%	[1000]	µg/L

Sequence No.: 5

Sample ID: S10

Analyst:

Logged In Analyst (Original) : optima4

Initial Sample Wt:

Dilution:

Autosampler Location: 5

Date Collected: 3/29/2010 18:34:14

Data Type: Reprocessed on 3/29/2010 19:14:35

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: S10

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Analysis Time
1	Sc 361.383	1647889.5	1647889.5	98.512 %	18:35:05
1	Sc RADIAL	147922.0	147922.0	101 %	18:34:43
1	Y 371.029	997984.1	997984.1	97.595 %	18:35:05
1	Al 396.153Radial†	231630.6	228268.0	[50000] µg/L	18:34:43
1	Ca 317.933Radial†	864405.0	851121.2	[50000] µg/L	18:34:43
1	Fe 238.204 Radial†	304562.8	299986.3	[20000] µg/L	18:34:43
1	Mg 279.077 IEC†	122786.4	120800.3	[50000] µg/L	18:34:43
1	Na 589.592 Radial†	134121.8	130461.6	[20000] µg/L	18:34:43
2	Sc 361.383	1646965.2	1646965.2	98.457 %	18:35:08
2	Sc RADIAL	147135.1	147135.1	101 %	18:34:45
2	Y 371.029	998151.2	998151.2	97.611 %	18:35:08
2	Al 396.153Radial†	231070.3	228933.5	[50000] µg/L	18:34:45
2	Ca 317.933Radial†	860622.6	851929.2	[50000] µg/L	18:34:45
2	Fe 238.204 Radial†	303079.0	300121.2	[20000] µg/L	18:34:45
2	Mg 279.077 IEC†	122393.7	121058.3	[50000] µg/L	18:34:45
2	Na 589.592 Radial†	133483.0	130535.5	[20000] µg/L	18:34:45
3	Sc 361.383	1642134.3	1642134.3	98.168 %	18:35:10
3	Sc RADIAL	146873.2	146873.2	101 %	18:34:47
3	Y 371.029	994617.7	994617.7	97.265 %	18:35:10
3	Al 396.153Radial†	231391.3	229660.2	[50000] µg/L	18:34:47
3	Ca 317.933Radial†	862939.8	855749.1	[50000] µg/L	18:34:47
3	Fe 238.204 Radial†	304238.1	301806.9	[20000] µg/L	18:34:47
3	Mg 279.077 IEC†	122676.5	121555.2	[50000] µg/L	18:34:47
3	Na 589.592 Radial†	134070.7	131354.5	[20000] µg/L	18:34:47

Mean Data: S10

Analyte	Mean Corrected Intensity	Std.Dev.	RSD	Calib. Conc. Units
Sc 361.383	1645663.0	3090.68	0.19%	98.379 %
Sc RADIAL	147310.1	545.84	0.37%	101 %
Y 371.029	996917.7	1993.60	0.20%	97.490 %
Al 396.153Radial†	228953.9	696.32	0.30%	[50000] µg/L
Ca 317.933Radial†	852933.2	2471.89	0.29%	[50000] µg/L
Fe 238.204 Radial†	300638.1	1014.46	0.34%	[20000] µg/L
Mg 279.077 IEC†	121137.9	383.71	0.32%	[50000] µg/L
Na 589.592 Radial†	130783.9	495.57	0.38%	[20000] µg/L

Calibration Summary

Analyte	Stds.	Equation	Intercept	Slope	Curvature	Corr. Coef.	Reslope
Ag 328.068	3	Lin Thru 0	0.0	246.4	0.00000	0.999992	
Al 396.153Radial	3	Lin Thru 0	0.0	4.581	0.00000	0.999996	
As 188.979	3	Lin Thru 0	0.0	2.393	0.00000	0.999929	
B 249.677	3	Lin Thru 0	0.0	59.56	0.00000	0.999952	
Ba 233.527	3	Lin Thru 0	0.0	218.9	0.00000	0.999987	
Be 313.107	3	Lin Thru 0	0.0	3072	0.00000	0.999986	
Ca 317.933Radial	3	Lin Thru 0	0.0	17.07	0.00000	0.999997	
Cd 226.502	3	Lin Thru 0	0.0	144.8	0.00000	0.999986	
Co 228.616	3	Lin Thru 0	0.0	73.04	0.00000	0.999984	
Cr 267.716	3	Lin Thru 0	0.0	116.4	0.00000	0.999990	
Cu 324.752	3	Lin Thru 0	0.0	230.0	0.00000	0.999993	
Fe 238.204 Radia	2	Lin Thru 0	0.0	15.04	0.00000	0.999999	
K 766.490 Radial	3	Lin Thru 0	0.0	2.429	0.00000	0.999970	
Mg 279.077 IEC	3	Lin Thru 0	0.0	2.425	0.00000	0.999987	
Mn 257.610	3	Lin Thru 0	0.0	731.8	0.00000	0.999991	
Mo 202.031	3	Lin Thru 0	0.0	31.68	0.00000	0.999979	

Na 589.592 Radia	2	Lin Thru 0	0.0	6.535	0.00000	0.999999
Ni 231.604	3	Lin Thru 0	0.0	78.18	0.00000	0.999990
P 214.914	3	Lin Thru 0	0.0	4.176	0.00000	0.999933
Pb 220.353	3	Lin Thru 0	0.0	16.51	0.00000	0.999980
S 181.975 Axial	3	Lin Thru 0	0.0	1.234	0.00000	0.999894
Sb 206.836	3	Lin Thru 0	0.0	7.413	0.00000	0.999972
Se 196.026	3	Lin Thru 0	0.0	2.528	0.00000	0.999970
SiO2	3	Lin Thru 0	0.0	9.149	0.00000	0.999993
Si 251.611	3	Lin Thru 0	0.0	60.48	0.00000	0.999996
Sn 189.927	3	Lin Thru 0	0.0	14.07	0.00000	0.999974
Sr 421.552	3	Lin Thru 0	0.0	426.7	0.00000	0.999990
Ti 334.940	3	Lin Thru 0	0.0	980.7	0.00000	0.999985
Tl 190.801	3	Lin Thru 0	0.0	7.450	0.00000	0.999968
U 409.014	3	Lin Thru 0	0.0	16.18	0.00000	0.999235
V 292.402	3	Lin Thru 0	0.0	180.3	0.00000	0.999978
Zn 213.857	3	Lin Thru 0	0.0	158.8	0.00000	0.999994

Sequence No.: 6

Sample ID: ICV

Analyst:

Logged In Analyst (Original) : optima4

Initial Sample Wt:

Dilution:

Autosampler Location: 9

Date Collected: 3/29/2010 18:35:18

Data Type: Reprocessed on 3/29/2010 19:14:36

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: ICV

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc 361.383	1701844.8	1701844.8	101.74 %		18:36:17
1	Sc RADIAL	151216.0	151216.0	104 %		18:35:50
1	Y 371.029	1036585.9	1036585.9	101.37 %		18:36:17
1	Ag 328.068†	65858.6	61766.5	256.87 µg/L	256.87 ppb	18:36:17
1	Al 396.153Radial†	24486.5	23634.0	5134.9 µg/L	5134.9 ppb	18:35:50
1	As 188.979†	1140.6	1135.4	481.67 µg/L	481.67 ppb	18:36:37
1	B 249.677†	34168.2	30228.9	505.75 µg/L	505.75 ppb	18:36:17
1	Ba 233.527†	112714.3	110964.0	507.33 µg/L	507.33 ppb	18:36:17
1	Be 313.107†	798269.6	785294.0	255.76 µg/L	255.76 ppb	18:36:17
1	Ca 317.933Radial†	89164.4	85327.7	4999.8 µg/L	4999.8 ppb	18:35:50
1	Cd 226.502†	72993.3	71840.9	495.79 µg/L	495.79 ppb	18:36:17
1	Co 228.616†	37444.2	36981.2	506.64 µg/L	506.64 ppb	18:36:17
1	Cr 267.716†	57873.1	56724.3	487.10 µg/L	487.10 ppb	18:36:17
1	Cu 324.752†	121386.5	116888.2	509.66 µg/L	509.66 ppb	18:36:17
1	Fe 238.204 Radial†	78431.6	75485.5	5018.5 µg/L	5018.5 ppb	18:35:50
1	K 766.490 Radial†	7725.2	5991.2	2463.6 µg/L	2463.6 ppb	18:35:50
1	Mg 279.077 IEC†	13310.9	12643.4	5221.4 µg/L	5221.4 ppb	18:35:50
1	Mn 257.610†	376288.9	369781.3	505.06 µg/L	505.06 ppb	18:36:17
1	Mo 202.031†	16673.6	16444.0	519.54 µg/L	519.54 ppb	18:36:37
1	Na 589.592 Radial†	18471.5	16109.6	2462.8 µg/L	2462.8 ppb	18:35:50
1	Ni 231.604†	39283.0	38652.9	494.42 µg/L	494.42 ppb	18:36:17
1	P 214.914†	10554.2	10294.3	2456.6 µg/L	2456.6 ppb	18:36:37
1	Pb 220.353†	8472.5	8215.3	499.30 µg/L	499.30 ppb	18:36:37
1	S 181.975 Axial†	3123.6	2975.4	2415.0 µg/L	2415.0 ppb	18:36:37
1	Sb 206.836†	3775.1	3624.0	490.49 µg/L	490.49 ppb	18:36:37
1	Se 196.026†	6364.3	6244.7	2470 µg/L	2470 ppb	18:36:37
1	SiO2†	99568.8	96295.2	10503 µg/L	10503 ppb	18:36:17
1	Si 251.611†	303093.3	297239.6	4904.5 µg/L	4904.5 ppb	18:36:17
1	Sn 189.927†	7432.7	7303.7	520.86 µg/L	520.86 ppb	18:36:37
1	Sr 421.552†	233447.1	225293.2	527.99 µg/L	527.99 ppb	18:35:48
1	Ti 334.940†	482527.6	473648.9	482.33 µg/L	482.33 ppb	18:36:17
1	Tl 190.801†	3799.6	3855.0	524.73 µg/L	524.73 ppb	18:36:37
1	U 409.014†	6773.0	7136.4	471.37 µg/L	471.37 ppb	18:36:17
1	V 292.402†	91625.4	89628.5	503.69 µg/L	503.69 ppb	18:36:17
1	Zn 213.857†	81346.1	79492.2	496.47 µg/L	496.47 ppb	18:36:17
2	Sc 361.383	1701980.9	1701980.9	101.75 %		18:36:40
2	Sc RADIAL	148848.9	148848.9	102 %		18:35:54
2	Y 371.029	1036246.9	1036246.9	101.34 %		18:36:40
2	Ag 328.068†	66063.0	61962.3	257.67 µg/L	257.67 ppb	18:36:40
2	Al 396.153Radial†	24189.6	23718.6	5153.2 µg/L	5153.2 ppb	18:35:54
2	As 188.979†	1141.1	1135.8	481.85 µg/L	481.85 ppb	18:37:00
2	B 249.677†	34342.1	30397.1	508.57 µg/L	508.57 ppb	18:36:40
2	Ba 233.527†	113003.6	111239.5	508.60 µg/L	508.60 ppb	18:36:40
2	Be 313.107†	803326.2	790201.1	257.35 µg/L	257.35 ppb	18:36:40
2	Ca 317.933Radial†	87776.3	85335.2	5000.3 µg/L	5000.3 ppb	18:35:54
2	Cd 226.502†	73305.6	72142.1	497.87 µg/L	497.87 ppb	18:36:40
2	Co 228.616†	37456.8	36990.6	506.77 µg/L	506.77 ppb	18:36:40
2	Cr 267.716†	58033.0	56876.9	488.42 µg/L	488.42 ppb	18:36:40
2	Cu 324.752†	121826.1	117310.6	511.48 µg/L	511.48 ppb	18:36:40
2	Fe 238.204 Radial†	77113.3	75396.8	5012.6 µg/L	5012.6 ppb	18:35:54
2	K 766.490 Radial†	7618.8	6005.4	2469.4 µg/L	2469.4 ppb	18:35:54
2	Mg 279.077 IEC†	12970.7	12514.3	5168.3 µg/L	5168.3 ppb	18:35:54
2	Mn 257.610†	377832.0	371268.3	507.10 µg/L	507.10 ppb	18:36:40
2	Mo 202.031†	16755.0	16522.7	522.02 µg/L	522.02 ppb	18:37:00
2	Na 589.592 Radial†	18069.9	15999.5	2445.9 µg/L	2445.9 ppb	18:35:54
2	Ni 231.604†	39447.3	38811.3	496.44 µg/L	496.44 ppb	18:36:40
2	P 214.914†	10626.3	10364.3	2473.3 µg/L	2473.3 ppb	18:37:00
2	Pb 220.353†	8494.9	8236.7	500.61 µg/L	500.61 ppb	18:37:00

2	S 181.975 Axial†	3125.4	2976.9	2416.3 µg/L	2416.3 ppb	18:37:00
2	Sb 206.836†	3806.5	3654.5	494.63 µg/L	494.63 ppb	18:37:00
2	Se 196.026†	6410.3	6289.4	2490 µg/L	2490 ppb	18:37:00
2	SiO2†	100159.6	96868.0	10565 µg/L	10565 ppb	18:36:40
2	Si 251.611†	304136.0	298240.5	4921.0 µg/L	4921.0 ppb	18:36:40
2	Sn 189.927†	7468.1	7337.9	523.29 µg/L	523.29 ppb	18:37:00
2	Sr 421.552†	233080.0	228512.0	535.53 µg/L	535.53 ppb	18:35:52
2	Ti 334.940†	484116.4	475172.5	483.90 µg/L	483.90 ppb	18:36:40
2	Tl 190.801†	3811.9	3866.8	526.34 µg/L	526.34 ppb	18:37:00
2	U 409.014†	6593.5	6959.4	460.57 µg/L	460.57 ppb	18:36:40
2	V 292.402†	92020.5	90009.6	505.83 µg/L	505.83 ppb	18:36:40
2	Zn 213.857†	81495.2	79632.3	497.34 µg/L	497.34 ppb	18:36:40
3	Sc 361.383	1720635.0	1720635.0	102.86 %		18:37:03
3	Sc RADIAL	149044.6	149044.6	102 %		18:35:58
3	Y 371.029	1046771.8	1046771.8	102.37 %		18:37:03
3	Ag 328.068†	66524.8	61707.3	256.63 µg/L	256.63 ppb	18:37:03
3	Al 396.153Radial†	24064.3	23565.0	5120.0 µg/L	5120.0 ppb	18:35:58
3	As 188.979†	1131.9	1114.6	473.00 µg/L	473.00 ppb	18:37:23
3	B 249.677†	34751.0	30428.7	509.10 µg/L	509.10 ppb	18:37:03
3	Ba 233.527†	114119.3	111120.0	508.05 µg/L	508.05 ppb	18:37:03
3	Be 313.107†	809136.9	787290.3	256.41 µg/L	256.41 ppb	18:37:03
3	Ca 317.933Radial†	87762.2	85208.6	4992.9 µg/L	4992.9 ppb	18:35:58
3	Cd 226.502†	74233.6	72263.2	498.71 µg/L	498.71 ppb	18:37:03
3	Co 228.616†	37810.4	36935.2	506.02 µg/L	506.02 ppb	18:37:03
3	Cr 267.716†	58579.7	56790.0	487.67 µg/L	487.67 ppb	18:37:03
3	Cu 324.752†	122627.9	116792.1	509.24 µg/L	509.24 ppb	18:37:03
3	Fe 238.204 Radial†	77211.6	75393.8	5012.4 µg/L	5012.4 ppb	18:35:58
3	K 766.490 Radial†	7631.8	6008.3	2470.6 µg/L	2470.6 ppb	18:35:58
3	Mg 279.077 IEC†	13062.0	12587.0	5198.1 µg/L	5198.1 ppb	18:35:58
3	Mn 257.610†	380724.0	370053.9	505.44 µg/L	505.44 ppb	18:37:03
3	Mo 202.031†	16767.7	16356.5	516.77 µg/L	516.77 ppb	18:37:23
3	Na 589.592 Radial†	18288.4	16189.9	2475.1 µg/L	2475.1 ppb	18:35:58
3	Ni 231.604†	39680.9	38618.1	493.97 µg/L	493.97 ppb	18:37:03
3	P 214.914†	10598.2	10223.8	2439.7 µg/L	2439.7 ppb	18:37:23
3	Pb 220.353†	8535.0	8185.1	497.46 µg/L	497.46 ppb	18:37:23
3	S 181.975 Axial†	3153.8	2971.2	2411.6 µg/L	2411.6 ppb	18:37:23
3	Sb 206.836†	3795.0	3602.8	487.58 µg/L	487.58 ppb	18:37:23
3	Se 196.026†	6408.5	6219.4	2460 µg/L	2460 ppb	18:37:23
3	SiO2†	100969.8	96588.4	10535 µg/L	10535 ppb	18:37:03
3	Si 251.611†	306927.5	297713.8	4912.4 µg/L	4912.4 ppb	18:37:03
3	Sn 189.927†	7476.5	7266.5	518.21 µg/L	518.21 ppb	18:37:23
3	Sr 421.552†	230245.5	225440.5	528.33 µg/L	528.33 ppb	18:35:56
3	Ti 334.940†	487355.2	473162.7	481.84 µg/L	481.84 ppb	18:37:03
3	Tl 190.801†	3807.3	3821.7	520.26 µg/L	520.26 ppb	18:37:23
3	U 409.014†	6788.8	7079.0	467.87 µg/L	467.87 ppb	18:37:03
3	V 292.402†	92755.7	89743.8	504.30 µg/L	504.30 ppb	18:37:03
3	Zn 213.857†	82290.5	79537.1	496.75 µg/L	496.75 ppb	18:37:03

Mean Data: ICV

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1708153.5	102.11 %	0.646			0.63%
Sc RADIAL	149703.2	103 %	0.9			0.88%
Y 371.029	1039868.2	101.69 %	0.585			0.58%
Ag 328.068†	61812.1	257.06 µg/L	0.547	257.06 ppb	0.547	0.21%
QC value within limits for Ag 328.068 Recovery = 102.82%						
Al 396.153Radial†	23639.2	5136.0 µg/L	16.67	5136.0 ppb	16.67	0.32%
QC value within limits for Al 396.153Radial Recovery = 102.72%						
As 188.979†	1128.6	478.84 µg/L	5.057	478.84 ppb	5.057	1.06%
QC value within limits for As 188.979 Recovery = 95.77%						
B 249.677†	30351.6	507.81 µg/L	1.804	507.81 ppb	1.804	0.36%
QC value within limits for B 249.677 Recovery = 101.56%						
Ba 233.527†	111107.9	507.99 µg/L	0.632	507.99 ppb	0.632	0.12%
QC value within limits for Ba 233.527 Recovery = 101.60%						
Be 313.107†	787595.1	256.51 µg/L	0.802	256.51 ppb	0.802	0.31%
QC value within limits for Be 313.107 Recovery = 102.60%						
Ca 317.933Radial†	85290.5	4997.7 µg/L	4.16	4997.7 ppb	4.16	0.08%
QC value within limits for Ca 317.933Radial Recovery = 99.95%						
Cd 226.502†	72082.0	497.46 µg/L	1.502	497.46 ppb	1.502	0.30%
QC value within limits for Cd 226.502 Recovery = 99.49%						

Co 228.616†	36969.0	506.48 µg/L	0.406	506.48 ppb	0.406	0.08%
QC value within limits for Co 228.616 Recovery = 101.30%						
Cr 267.716†	56797.1	487.73 µg/L	0.662	487.73 ppb	0.662	0.14%
QC value within limits for Cr 267.716 Recovery = 97.55%						
Cu 324.752†	116997.0	510.13 µg/L	1.195	510.13 ppb	1.195	0.23%
QC value within limits for Cu 324.752 Recovery = 102.03%						
Fe 238.204 Radial†	75425.3	5014.5 µg/L	3.46	5014.5 ppb	3.46	0.07%
QC value within limits for Fe 238.204 Radial Recovery = 100.29%						
K 766.490 Radial†	6001.6	2467.9 µg/L	3.77	2467.9 ppb	3.77	0.15%
QC value within limits for K 766.490 Radial Recovery = 98.71%						
Mg 279.077 IEC†	12581.6	5195.9 µg/L	26.65	5195.9 ppb	26.65	0.51%
QC value within limits for Mg 279.077 IEC Recovery = 103.92%						
Mn 257.610†	370367.8	505.87 µg/L	1.083	505.87 ppb	1.083	0.21%
QC value within limits for Mn 257.610 Recovery = 101.17%						
Mo 202.031†	16441.1	519.44 µg/L	2.624	519.44 ppb	2.624	0.51%
QC value within limits for Mo 202.031 Recovery = 103.89%						
Na 589.592 Radial†	16099.7	2461.3 µg/L	14.63	2461.3 ppb	14.63	0.59%
QC value within limits for Na 589.592 Radial Recovery = 98.45%						
Ni 231.604†	38694.1	494.94 µg/L	1.317	494.94 ppb	1.317	0.27%
QC value within limits for Ni 231.604 Recovery = 98.99%						
P 214.914†	10294.2	2456.5 µg/L	16.81	2456.5 ppb	16.81	0.68%
QC value within limits for P 214.914 Recovery = 98.26%						
Pb 220.353†	8212.4	499.12 µg/L	1.581	499.12 ppb	1.581	0.32%
QC value within limits for Pb 220.353 Recovery = 99.82%						
S 181.975 Axial†	2974.5	2414.3 µg/L	2.40	2414.3 ppb	2.40	0.10%
QC value within limits for S 181.975 Axial Recovery = 96.57%						
Sb 206.836†	3627.1	490.90 µg/L	3.546	490.90 ppb	3.546	0.72%
QC value within limits for Sb 206.836 Recovery = 98.18%						
Se 196.026†	6251.2	2470 µg/L	14.0	2470 ppb	14.0	0.57%
QC value within limits for Se 196.026 Recovery = 98.99%						
SiO2†	96583.8	10534 µg/L	31.3	10534 ppb	31.3	0.30%
QC value within limits for SiO2 Recovery = 98.50%						
Si 251.611†	297731.3	4912.6 µg/L	8.25	4912.6 ppb	8.25	0.17%
QC value within limits for Si 251.611 Recovery = 98.25%						
Sn 189.927†	7302.7	520.79 µg/L	2.541	520.79 ppb	2.541	0.49%
QC value within limits for Sn 189.927 Recovery = 104.16%						
Sr 421.552†	226415.3	530.62 µg/L	4.259	530.62 ppb	4.259	0.80%
QC value within limits for Sr 421.552 Recovery = 106.12%						
Ti 334.940†	473994.7	482.69 µg/L	1.073	482.69 ppb	1.073	0.22%
QC value within limits for Ti 334.940 Recovery = 96.54%						
Tl 190.801†	3847.8	523.78 µg/L	3.151	523.78 ppb	3.151	0.60%
QC value within limits for Tl 190.801 Recovery = 104.76%						
U 409.014†	7058.3	466.61 µg/L	5.511	466.61 ppb	5.511	1.18%
QC value within limits for U 409.014 Recovery = 93.32%						
V 292.402†	89793.9	504.61 µg/L	1.101	504.61 ppb	1.101	0.22%
QC value within limits for V 292.402 Recovery = 100.92%						
Zn 213.857†	79553.9	496.85 µg/L	0.443	496.85 ppb	0.443	0.09%
QC value within limits for Zn 213.857 Recovery = 99.37%						
All analyte(s) passed QC.						

Sequence No.: 7

Sample ID: ICB

Analyst:

Logged In Analyst (Original) : optima4

Initial Sample Wt:

Dilution:

Autosampler Location: 10

Date Collected: 3/29/2010 18:37:32

Data Type: Reprocessed on 3/29/2010 19:14:36

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: ICB

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc 361.383	1718110.5	1718110.5	102.71 %		18:39:24
1	Sc RADIAL	149870.1	149870.1	103 %		18:38:01
1	Y 371.029	1056124.6	1056124.6	103.28 %		18:39:24
1	Ag 328.068†	2764.1	-275.9	-1.1170 µg/L	-1.1170 ppb	18:39:26
1	Al 396.153Radial†	-34.1	-1.3	-0.3025 µg/L	-0.3025 ppb	18:38:21
1	As 188.979†	-13.9	0.8	0.3158 µg/L	0.3158 ppb	18:39:46
1	B 249.677†	3290.8	-151.7	-2.5477 µg/L	-2.5477 ppb	18:39:46
1	Ba 233.527†	-149.3	29.7	0.1352 µg/L	0.1352 ppb	18:39:46
1	Be 313.107†	-642.8	34.2	0.0134 µg/L	0.0134 ppb	18:39:26
1	Ca 317.933Radial†	601.2	-31.5	-1.8457 µg/L	-1.8457 ppb	18:38:21
1	Cd 226.502†	-82.2	14.4	0.0988 µg/L	0.0988 ppb	18:39:46
1	Co 228.616†	-179.0	2.3	0.0321 µg/L	0.0321 ppb	18:39:46
1	Cr 267.716†	164.4	-0.2	-0.0075 µg/L	-0.0075 ppb	18:39:46
1	Cu 324.752†	2372.4	-115.1	-0.4939 µg/L	-0.4939 ppb	18:39:26
1	Fe 238.204 Radial†	141.5	24.3	1.6170 µg/L	1.6170 ppb	18:38:21
1	K 766.490 Radial†	1569.1	71.0	29.223 µg/L	29.223 ppb	18:38:01
1	Mg 279.077 IEC†	162.3	-28.9	-11.902 µg/L	-11.902 ppb	18:38:21
1	Mn 257.610†	162.2	77.9	0.1069 µg/L	0.1069 ppb	18:39:46
1	Mo 202.031†	-48.8	7.7	0.2416 µg/L	0.2416 ppb	18:39:46
1	Na 589.592 Radial†	1595.3	-143.3	-21.948 µg/L	-21.948 ppb	18:38:01
1	Ni 231.604†	-74.2	-31.3	-0.4003 µg/L	-0.4003 ppb	18:39:46
1	P 214.914†	77.1	-4.5	-1.0788 µg/L	-1.0788 ppb	18:39:46
1	Pb 220.353†	105.8	-9.5	-0.5776 µg/L	-0.5776 ppb	18:39:46
1	S 181.975 Axial†	96.4	-1.0	-0.8082 µg/L	-0.8082 ppb	18:39:46
1	Sb 206.836†	76.9	-11.8	-1.5863 µg/L	-1.5863 ppb	18:39:46
1	Se 196.026†	30.3	18.6	7.35 µg/L	7.35 ppb	18:39:46
1	SiO2†	1615.4	-0.1	-0.0156 µg/L	-0.0156 ppb	18:39:46
1	Si 251.611†	756.3	60.0	0.9881 µg/L	0.9881 ppb	18:39:26
1	Sn 189.927†	2.2	0.2	0.0117 µg/L	0.0117 ppb	18:39:46
1	Sr 421.552†	-232.4	51.9	0.1217 µg/L	0.1217 ppb	18:38:01
1	Ti 334.940†	823.7	165.6	0.1667 µg/L	0.1667 ppb	18:39:26
1	Tl 190.801†	-129.5	-5.8	-0.7821 µg/L	-0.7821 ppb	18:39:46
1	U 409.014†	-365.4	123.4	7.5895 µg/L	7.5895 ppb	18:39:26
1	V 292.402†	336.7	-104.0	-0.5695 µg/L	-0.5695 ppb	18:39:26
1	Zn 213.857†	481.8	4.7	0.0326 µg/L	0.0326 ppb	18:39:46
2	Sc 361.383	1718304.1	1718304.1	102.72 %		18:39:48
2	Sc RADIAL	149819.8	149819.8	103 %		18:38:23
2	Y 371.029	1056622.1	1056622.1	103.33 %		18:39:48
2	Ag 328.068†	3062.4	14.3	0.0846 µg/L	0.0846 ppb	18:39:50
2	Al 396.153Radial†	-45.4	-12.3	-2.7171 µg/L	-2.7171 ppb	18:38:44
2	As 188.979†	-10.9	3.6	1.5162 µg/L	1.5162 ppb	18:40:10
2	B 249.677†	3277.0	-165.5	-2.7792 µg/L	-2.7792 ppb	18:40:10
2	Ba 233.527†	-168.1	11.4	0.0526 µg/L	0.0526 ppb	18:40:10
2	Be 313.107†	-415.9	255.2	0.0882 µg/L	0.0882 ppb	18:39:50
2	Ca 317.933Radial†	633.4	0.0	0.0016 µg/L	0.0016 ppb	18:38:44
2	Cd 226.502†	-115.3	-17.9	-0.1235 µg/L	-0.1235 ppb	18:40:10
2	Co 228.616†	-162.9	18.1	0.2472 µg/L	0.2472 ppb	18:40:10
2	Cr 267.716†	189.3	24.1	0.1939 µg/L	0.1939 ppb	18:40:10
2	Cu 324.752†	2490.6	-0.2	0.0132 µg/L	0.0132 ppb	18:39:50
2	Fe 238.204 Radial†	132.2	15.4	1.0215 µg/L	1.0215 ppb	18:38:44
2	K 766.490 Radial†	1519.5	23.3	9.5884 µg/L	9.5884 ppb	18:38:23
2	Mg 279.077 IEC†	195.8	3.8	1.5733 µg/L	1.5733 ppb	18:38:44
2	Mn 257.610†	168.0	83.5	0.1141 µg/L	0.1141 ppb	18:40:10
2	Mo 202.031†	-35.6	20.5	0.6489 µg/L	0.6489 ppb	18:40:10
2	Na 589.592 Radial†	1651.7	-87.8	-13.450 µg/L	-13.450 ppb	18:38:23
2	Ni 231.604†	-55.2	-12.8	-0.1641 µg/L	-0.1641 ppb	18:40:10
2	P 214.914†	83.6	1.8	0.4344 µg/L	0.4344 ppb	18:40:10
2	Pb 220.353†	94.6	-20.3	-1.2399 µg/L	-1.2399 ppb	18:40:10

2	S 181.975 Axial†	84.2	-12.9	-10.416 µg/L	-10.416 ppb	18:40:10
2	Sb 206.836†	72.7	-15.8	-2.1296 µg/L	-2.1296 ppb	18:40:10
2	Se 196.026†	25.1	13.5	5.37 µg/L	5.37 ppb	18:40:10
2	SiO2†	1629.2	13.2	1.4227 µg/L	1.4227 ppb	18:40:10
2	Si 251.611†	776.2	79.3	1.3023 µg/L	1.3023 ppb	18:39:50
2	Sn 189.927†	1.7	-0.4	-0.0258 µg/L	-0.0258 ppb	18:40:10
2	Sr 421.552†	-119.9	161.3	0.3781 µg/L	0.3781 ppb	18:38:23
2	Ti 334.940†	906.1	245.8	0.2435 µg/L	0.2435 ppb	18:39:50
2	Tl 190.801†	-120.0	3.5	0.4698 µg/L	0.4698 ppb	18:40:10
2	U 409.014†	-211.2	273.5	16.929 µg/L	16.929 ppb	18:39:50
2	V 292.402†	536.3	90.3	0.5193 µg/L	0.5193 ppb	18:39:50
2	Zn 213.857†	461.1	-15.5	-0.0967 µg/L	-0.0967 ppb	18:40:10
3	Sc 361.383	1698930.8	1698930.8	101.56 %		18:40:12
3	Sc RADIAL	152143.2	152143.2	104 %		18:38:46
3	Y 371.029	1045315.3	1045315.3	102.22 %		18:40:12
3	Ag 328.068†	3085.7	71.1	0.2837 µg/L	0.2837 ppb	18:40:14
3	Al 396.153Radial†	-62.8	-28.3	-6.2230 µg/L	-6.2230 ppb	18:39:06
3	As 188.979†	-25.2	-10.6	-4.4173 µg/L	-4.4173 ppb	18:40:34
3	B 249.677†	3266.7	-139.3	-2.3411 µg/L	-2.3411 ppb	18:40:34
3	Ba 233.527†	-163.9	13.7	0.0623 µg/L	0.0623 ppb	18:40:34
3	Be 313.107†	-627.7	42.1	0.0141 µg/L	0.0141 ppb	18:40:14
3	Ca 317.933Radial†	630.0	-12.6	-0.7399 µg/L	-0.7399 ppb	18:39:06
3	Cd 226.502†	-76.1	19.4	0.1339 µg/L	0.1339 ppb	18:40:34
3	Co 228.616†	-133.4	45.2	0.6195 µg/L	0.6195 ppb	18:40:34
3	Cr 267.716†	156.7	-5.9	-0.0523 µg/L	-0.0523 ppb	18:40:34
3	Cu 324.752†	2540.5	76.5	0.3341 µg/L	0.3341 ppb	18:40:14
3	Fe 238.204 Radial†	134.4	15.5	1.0313 µg/L	1.0313 ppb	18:39:06
3	K 766.490 Radial†	1520.9	2.1	0.8535 µg/L	0.8535 ppb	18:38:46
3	Mg 279.077 IEC†	186.1	-8.4	-3.4269 µg/L	-3.4269 ppb	18:39:06
3	Mn 257.610†	142.8	60.6	0.0829 µg/L	0.0829 ppb	18:40:34
3	Mo 202.031†	-28.7	26.9	0.8495 µg/L	0.8495 ppb	18:40:34
3	Na 589.592 Radial†	1594.0	-167.7	-25.662 µg/L	-25.662 ppb	18:38:46
3	Ni 231.604†	-74.3	-32.3	-0.4127 µg/L	-0.4127 ppb	18:40:34
3	P 214.914†	71.0	-9.6	-2.3151 µg/L	-2.3151 ppb	18:40:34
3	Pb 220.353†	138.9	24.3	1.4738 µg/L	1.4738 ppb	18:40:34
3	S 181.975 Axial†	87.7	-8.5	-6.8917 µg/L	-6.8917 ppb	18:40:34
3	Sb 206.836†	71.9	-15.8	-2.1234 µg/L	-2.1234 ppb	18:40:34
3	Se 196.026†	21.3	10.1	3.99 µg/L	3.99 ppb	18:40:34
3	SiO2†	1618.8	21.0	2.2686 µg/L	2.2686 ppb	18:40:34
3	Si 251.611†	788.9	100.3	1.6458 µg/L	1.6458 ppb	18:40:14
3	Sn 189.927†	6.3	4.2	0.2956 µg/L	0.2956 ppb	18:40:34
3	Sr 421.552†	-237.8	50.2	0.1176 µg/L	0.1176 ppb	18:38:46
3	Ti 334.940†	556.8	-88.1	-0.0902 µg/L	-0.0902 ppb	18:40:14
3	Tl 190.801†	-119.8	2.3	0.3073 µg/L	0.3073 ppb	18:40:34
3	U 409.014†	-464.1	22.2	1.3392 µg/L	1.3392 ppb	18:40:14
3	V 292.402†	338.6	-98.5	-0.5367 µg/L	-0.5367 ppb	18:40:14
3	Zn 213.857†	460.6	-10.9	-0.0662 µg/L	-0.0662 ppb	18:40:34

Mean Data: ICB

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1711781.8	102.33 %	0.665			0.65%
Sc RADIAL	150611.1	103 %	0.9			0.88%
Y 371.029	1052687.3	102.94 %	0.625			0.61%
Ag 328.068†	-63.5	-0.2496 µg/L	0.75780	-0.2496 ppb	0.75780	303.64%
QC value within limits for Ag 328.068 Recovery = Not calculated						
Al 396.153Radial†	-14.0	-3.0809 µg/L	2.97697	-3.0809 ppb	2.97697	96.63%
QC value within limits for Al 396.153Radial Recovery = Not calculated						
As 188.979†	-2.1	-0.8618 µg/L	3.13716	-0.8618 ppb	3.13716	364.04%
QC value within limits for As 188.979 Recovery = Not calculated						
B 249.677†	-152.2	-2.5560 µg/L	0.21918	-2.5560 ppb	0.21918	8.58%
QC value within limits for B 249.677 Recovery = Not calculated						
Ba 233.527†	18.2	0.0834 µg/L	0.04516	0.0834 ppb	0.04516	54.17%
QC value within limits for Ba 233.527 Recovery = Not calculated						
Be 313.107†	110.5	0.0386 µg/L	0.04296	0.0386 ppb	0.04296	111.35%
QC value within limits for Be 313.107 Recovery = Not calculated						
Ca 317.933Radial†	-14.7	-0.8613 µg/L	0.92961	-0.8613 ppb	0.92961	107.93%
QC value within limits for Ca 317.933Radial Recovery = Not calculated						
Cd 226.502†	5.3	0.0364 µg/L	0.13959	0.0364 ppb	0.13959	383.42%
QC value within limits for Cd 226.502 Recovery = Not calculated						

Co 228.616†	21.9	0.2996 µg/L	0.29720	0.2996 ppb	0.29720	99.21%
QC value within limits for Co 228.616 Recovery = Not calculated						
Cr 267.716†	6.0	0.0447 µg/L	0.13112	0.0447 ppb	0.13112	293.47%
QC value within limits for Cr 267.716 Recovery = Not calculated						
Cu 324.752†	-12.9	-0.0489 µg/L	0.41746	-0.0489 ppb	0.41746	854.27%
QC value within limits for Cu 324.752 Recovery = Not calculated						
Fe 238.204 Radial†	18.4	1.2233 µg/L	0.34099	1.2233 ppb	0.34099	27.88%
QC value within limits for Fe 238.204 Radial Recovery = Not calculated						
K 766.490 Radial†	32.1	13.222 µg/L	14.5294	13.222 ppb	14.5294	109.89%
QC value within limits for K 766.490 Radial Recovery = Not calculated						
Mg 279.077 IEC†	-11.2	-4.5853 µg/L	6.81203	-4.5853 ppb	6.81203	148.56%
QC value within limits for Mg 279.077 IEC Recovery = Not calculated						
Mn 257.610†	74.0	0.1013 µg/L	0.01630	0.1013 ppb	0.01630	16.09%
QC value within limits for Mn 257.610 Recovery = Not calculated						
Mo 202.031†	18.4	0.5800 µg/L	0.30975	0.5800 ppb	0.30975	53.40%
QC value within limits for Mo 202.031 Recovery = Not calculated						
Na 589.592 Radial†	-132.9	-20.353 µg/L	6.2604	-20.353 ppb	6.2604	30.76%
QC value within limits for Na 589.592 Radial Recovery = Not calculated						
Ni 231.604†	-25.5	-0.3257 µg/L	0.14010	-0.3257 ppb	0.14010	43.01%
QC value within limits for Ni 231.604 Recovery = Not calculated						
P 214.914†	-4.1	-0.9865 µg/L	1.37705	-0.9865 ppb	1.37705	139.59%
QC value within limits for P 214.914 Recovery = Not calculated						
Pb 220.353†	-1.8	-0.1146 µg/L	1.41489	-0.1146 ppb	1.41489	>999.9%
QC value within limits for Pb 220.353 Recovery = Not calculated						
S 181.975 Axial†	-7.5	-6.0387 µg/L	4.86046	-6.0387 ppb	4.86046	80.49%
QC value within limits for S 181.975 Axial Recovery = Not calculated						
Sb 206.836†	-14.5	-1.9465 µg/L	0.31193	-1.9465 ppb	0.31193	16.03%
QC value within limits for Sb 206.836 Recovery = Not calculated						
Se 196.026†	14.1	5.57 µg/L	1.688	5.57 ppb	1.688	30.30%
QC value within limits for Se 196.026 Recovery = Not calculated						
SiO2†	11.4	1.2252 µg/L	1.15483	1.2252 ppb	1.15483	94.25%
QC value within limits for SiO2 Recovery = Not calculated						
Si 251.611†	79.9	1.3121 µg/L	0.32896	1.3121 ppb	0.32896	25.07%
QC value within limits for Si 251.611 Recovery = Not calculated						
Sn 189.927†	1.3	0.0938 µg/L	0.17571	0.0938 ppb	0.17571	187.29%
QC value within limits for Sn 189.927 Recovery = Not calculated						
Sr 421.552†	87.8	0.2058 µg/L	0.14923	0.2058 ppb	0.14923	72.50%
QC value within limits for Sr 421.552 Recovery = Not calculated						
Ti 334.940†	107.7	0.1067 µg/L	0.17474	0.1067 ppb	0.17474	163.81%
QC value within limits for Ti 334.940 Recovery = Not calculated						
Tl 190.801†	0.0	-0.0017 µg/L	0.68072	-0.0017 ppb	0.68072	>999.9%
QC value within limits for Tl 190.801 Recovery = Not calculated						
U 409.014†	139.7	8.6193 µg/L	7.84577	8.6193 ppb	7.84577	91.03%
QC value within limits for U 409.014 Recovery = Not calculated						
V 292.402†	-37.4	-0.1957 µg/L	0.61936	-0.1957 ppb	0.61936	316.55%
QC value within limits for V 292.402 Recovery = Not calculated						
Zn 213.857†	-7.2	-0.0435 µg/L	0.06758	-0.0435 ppb	0.06758	155.53%
QC value within limits for Zn 213.857 Recovery = Not calculated						
All analyte(s) passed QC.						

Sequence No.: 8

Sample ID: PQL

Analyst:

Logged In Analyst (Original) : optima4

Initial Sample Wt:

Dilution:

Autosampler Location: 101

Date Collected: 3/29/2010 18:40:43

Data Type: Reprocessed on 3/29/2010 19:14:37

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: PQL

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc 361.383	1721442.6	1721442.6	102.91 %		18:41:40
1	Sc RADIAL	147903.8	147903.8	101 %		18:41:13
1	Y 371.029	1058404.9	1058404.9	103.50 %		18:41:40
1	Ag 328.068†	4025.6	944.7	3.9659 µg/L	3.9659 ppb	18:41:43
1	Al 396.153Radial†	922.6	941.1	204.98 µg/L	204.98 ppb	18:41:15
1	As 188.979†	70.2	82.5	34.551 µg/L	34.551 ppb	18:42:03
1	B 249.677†	6252.3	2719.8	45.645 µg/L	45.645 ppb	18:41:43
1	Ba 233.527†	968.6	1116.3	5.1042 µg/L	5.1042 ppb	18:42:03
1	Be 313.107†	14893.3	15132.4	4.9477 µg/L	4.9477 ppb	18:41:43
1	Ca 317.933Radial†	4243.5	3565.6	208.93 µg/L	208.93 ppb	18:41:15
1	Cd 226.502†	637.3	713.7	4.9197 µg/L	4.9197 ppb	18:42:03
1	Co 228.616†	202.6	373.5	5.1141 µg/L	5.1141 ppb	18:42:03
1	Cr 267.716†	729.0	548.1	4.6505 µg/L	4.6505 ppb	18:42:03
1	Cu 324.752†	4895.4	2332.1	10.224 µg/L	10.224 ppb	18:41:43
1	Fe 238.204 Radial†	1705.5	1567.4	104.21 µg/L	104.21 ppb	18:41:15
1	K 766.490 Radial†	1904.1	421.4	173.34 µg/L	173.34 ppb	18:41:13
1	Mg 279.077 IEC†	935.0	734.7	303.09 µg/L	303.09 ppb	18:41:15
1	Mn 257.610†	7824.8	7523.6	10.268 µg/L	10.268 ppb	18:41:43
1	Mo 202.031†	258.6	306.5	9.6870 µg/L	9.6870 ppb	18:42:03
1	Na 589.592 Radial†	3412.3	1667.9	255.06 µg/L	255.06 ppb	18:41:15
1	Ni 231.604†	353.8	384.7	4.9210 µg/L	4.9210 ppb	18:42:03
1	P 214.914†	701.3	601.9	143.99 µg/L	143.99 ppb	18:42:03
1	Pb 220.353†	285.3	164.8	9.9640 µg/L	9.9640 ppb	18:42:03
1	S 181.975 Axial†	217.5	116.6	94.518 µg/L	94.518 ppb	18:42:03
1	Sb 206.836†	151.7	60.8	8.2873 µg/L	8.2873 ppb	18:42:03
1	Se 196.026†	93.5	79.9	31.7 µg/L	31.7 ppb	18:42:03
1	SiO2†	3528.6	1856.0	202.45 µg/L	202.45 ppb	18:41:43
1	Si 251.611†	7008.2	6133.7	101.23 µg/L	101.23 ppb	18:41:43
1	Sn 189.927†	141.3	135.3	9.6379 µg/L	9.6379 ppb	18:42:03
1	Sr 421.552†	2328.3	2572.4	6.0274 µg/L	6.0274 ppb	18:41:15
1	Ti 334.940†	5694.2	4896.9	4.9428 µg/L	4.9428 ppb	18:41:43
1	Tl 190.801†	28.4	147.9	19.934 µg/L	19.934 ppb	18:42:03
1	U 409.014†	713.0	1172.0	72.715 µg/L	72.715 ppb	18:41:43
1	V 292.402†	1246.9	779.8	4.4736 µg/L	4.4736 ppb	18:41:43
1	Zn 213.857†	2077.4	1554.3	9.7365 µg/L	9.7365 ppb	18:42:03
2	Sc 361.383	1724623.2	1724623.2	103.10 %		18:42:05
2	Sc RADIAL	148676.2	148676.2	102 %		18:41:17
2	Y 371.029	1060877.7	1060877.7	103.75 %		18:42:05
2	Ag 328.068†	4441.5	1340.9	5.5444 µg/L	5.5444 ppb	18:42:07
2	Al 396.153Radial†	882.0	896.6	195.25 µg/L	195.25 ppb	18:41:19
2	As 188.979†	60.0	72.5	30.385 µg/L	30.385 ppb	18:42:27
2	B 249.677†	6195.0	2653.1	44.524 µg/L	44.524 ppb	18:42:07
2	Ba 233.527†	972.4	1118.3	5.1130 µg/L	5.1130 ppb	18:42:27
2	Be 313.107†	15035.6	15243.7	4.9775 µg/L	4.9775 ppb	18:42:07
2	Ca 317.933Radial†	4053.9	3358.0	196.76 µg/L	196.76 ppb	18:41:19
2	Cd 226.502†	642.0	717.1	4.9432 µg/L	4.9432 ppb	18:42:27
2	Co 228.616†	195.2	365.9	5.0104 µg/L	5.0104 ppb	18:42:27
2	Cr 267.716†	741.9	559.4	4.7640 µg/L	4.7640 ppb	18:42:27
2	Cu 324.752†	4804.6	2235.3	9.7851 µg/L	9.7851 ppb	18:42:07
2	Fe 238.204 Radial†	1689.7	1543.2	102.60 µg/L	102.60 ppb	18:41:19
2	K 766.490 Radial†	1941.0	447.8	184.20 µg/L	184.20 ppb	18:41:17
2	Mg 279.077 IEC†	934.9	729.8	301.08 µg/L	301.08 ppb	18:41:19
2	Mn 257.610†	7840.1	7524.4	10.269 µg/L	10.269 ppb	18:42:07
2	Mo 202.031†	268.7	315.9	9.9813 µg/L	9.9813 ppb	18:42:27
2	Na 589.592 Radial†	3585.8	1820.6	278.41 µg/L	278.41 ppb	18:41:19
2	Ni 231.604†	360.6	390.7	4.9969 µg/L	4.9969 ppb	18:42:27
2	P 214.914†	704.9	604.1	144.53 µg/L	144.53 ppb	18:42:27
2	Pb 220.353†	256.9	136.7	8.2831 µg/L	8.2831 ppb	18:42:27

2	S 181.975 Axial†	211.0	109.8	89.075 µg/L	89.075 ppb	18:42:27
2	Sb 206.836†	139.1	48.3	6.6025 µg/L	6.6025 ppb	18:42:27
2	Se 196.026†	85.2	71.7	28.4 µg/L	28.4 ppb	18:42:27
2	SiO2†	3666.3	1983.3	216.34 µg/L	216.34 ppb	18:42:07
2	Si 251.611†	6987.0	6100.5	100.67 µg/L	100.67 ppb	18:42:07
2	Sn 189.927†	148.9	142.4	10.142 µg/L	10.142 ppb	18:42:27
2	Sr 421.552†	2257.8	2491.4	5.8378 µg/L	5.8378 ppb	18:41:19
2	Ti 334.940†	5599.5	4794.8	4.8474 µg/L	4.8474 ppb	18:42:07
2	Tl 190.801†	28.5	147.9	19.938 µg/L	19.938 ppb	18:42:27
2	U 409.014†	356.1	824.5	51.229 µg/L	51.229 ppb	18:42:07
2	V 292.402†	1199.8	731.9	4.1969 µg/L	4.1969 ppb	18:42:07
2	Zn 213.857†	2110.9	1583.0	9.9172 µg/L	9.9172 ppb	18:42:27
3	Sc 361.383	1709181.0	1709181.0	102.18 %		18:42:29
3	Sc RADIAL	148765.1	148765.1	102 %		18:41:21
3	Y 371.029	1051117.1	1051117.1	102.79 %		18:42:29
3	Ag 328.068†	4096.5	1042.2	4.3518 µg/L	4.3518 ppb	18:42:31
3	Al 396.153Radial†	913.9	927.3	201.93 µg/L	201.93 ppb	18:41:23
3	As 188.979†	45.1	58.4	24.503 µg/L	24.503 ppb	18:42:51
3	B 249.677†	6365.0	2873.8	48.229 µg/L	48.229 ppb	18:42:31
3	Ba 233.527†	993.8	1147.7	5.2479 µg/L	5.2479 ppb	18:42:51
3	Be 313.107†	15404.4	15736.4	5.1406 µg/L	5.1406 ppb	18:42:31
3	Ca 317.933Radial†	4204.3	3503.0	205.26 µg/L	205.26 ppb	18:41:23
3	Cd 226.502†	656.9	737.3	5.0831 µg/L	5.0831 ppb	18:42:51
3	Co 228.616†	214.1	386.1	5.2868 µg/L	5.2868 ppb	18:42:51
3	Cr 267.716†	776.9	600.1	5.1070 µg/L	5.1070 ppb	18:42:51
3	Cu 324.752†	4905.4	2376.0	10.405 µg/L	10.405 ppb	18:42:31
3	Fe 238.204 Radial†	1701.7	1554.0	103.31 µg/L	103.31 ppb	18:41:23
3	K 766.490 Radial†	1863.7	371.0	152.58 µg/L	152.58 ppb	18:41:21
3	Mg 279.077 IEC†	946.2	740.4	305.43 µg/L	305.43 ppb	18:41:23
3	Mn 257.610†	7932.9	7683.9	10.487 µg/L	10.487 ppb	18:42:31
3	Mo 202.031†	276.9	326.2	10.308 µg/L	10.308 ppb	18:42:51
3	Na 589.592 Radial†	3380.4	1617.2	247.32 µg/L	247.32 ppb	18:41:23
3	Ni 231.604†	372.2	405.1	5.1823 µg/L	5.1823 ppb	18:42:51
3	P 214.914†	693.9	599.5	143.42 µg/L	143.42 ppb	18:42:51
3	Pb 220.353†	299.1	180.3	10.914 µg/L	10.914 ppb	18:42:51
3	S 181.975 Axial†	216.9	117.4	95.241 µg/L	95.241 ppb	18:42:51
3	Sb 206.836†	178.2	87.8	11.935 µg/L	11.935 ppb	18:42:51
3	Se 196.026†	84.3	71.6	28.4 µg/L	28.4 ppb	18:42:51
3	SiO2†	3665.9	2015.0	219.80 µg/L	219.80 ppb	18:42:31
3	Si 251.611†	7292.1	6460.4	106.62 µg/L	106.62 ppb	18:42:31
3	Sn 189.927†	146.0	140.9	10.035 µg/L	10.035 ppb	18:42:51
3	Sr 421.552†	2185.8	2419.5	5.6692 µg/L	5.6692 ppb	18:41:23
3	Ti 334.940†	5763.7	5004.6	5.0573 µg/L	5.0573 ppb	18:42:31
3	Tl 190.801†	37.2	156.7	21.117 µg/L	21.117 ppb	18:42:51
3	U 409.014†	504.2	972.6	60.421 µg/L	60.421 ppb	18:42:31
3	V 292.402†	1321.2	861.3	4.9254 µg/L	4.9254 ppb	18:42:31
3	Zn 213.857†	2122.4	1612.8	10.103 µg/L	10.103 ppb	18:42:51

Mean Data: PQL

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1718415.6	102.73 %	0.487			0.47%
Sc RADIAL	148448.4	102 %	0.3			0.32%
Y 371.029	1056799.9	103.35 %	0.496			0.48%
Ag 328.068†	1109.3	4.6207 µg/L	0.82285	4.6207 ppb	0.82285	17.81%
QC value within limits for Ag 328.068 Recovery = 92.41%						
Al 396.153Radial†	921.7	200.72 µg/L	4.978	200.72 ppb	4.978	2.48%
QC value within limits for Al 396.153Radial Recovery = 100.36%						
As 188.979†	71.1	29.813 µg/L	5.0483	29.813 ppb	5.0483	16.93%
QC value within limits for As 188.979 Recovery = 99.38%						
B 249.677†	2748.9	46.133 µg/L	1.8998	46.133 ppb	1.8998	4.12%
QC value within limits for B 249.677 Recovery = 92.27%						
Ba 233.527†	1127.4	5.1550 µg/L	0.08056	5.1550 ppb	0.08056	1.56%
QC value within limits for Ba 233.527 Recovery = 103.10%						
Be 313.107†	15370.8	5.0219 µg/L	0.10386	5.0219 ppb	0.10386	2.07%
QC value within limits for Be 313.107 Recovery = 100.44%						
Ca 317.933Radial†	3475.5	203.65 µg/L	6.241	203.65 ppb	6.241	3.06%
QC value within limits for Ca 317.933Radial Recovery = 101.83%						
Cd 226.502†	722.7	4.9820 µg/L	0.08834	4.9820 ppb	0.08834	1.77%
QC value within limits for Cd 226.502 Recovery = 99.64%						

Co 228.616†	375.2	5.1371 µg/L	0.13962	5.1371 ppb	0.13962	2.72%
QC value within limits for Co 228.616 Recovery = 102.74%						
Cr 267.716†	569.2	4.8405 µg/L	0.23770	4.8405 ppb	0.23770	4.91%
QC value within limits for Cr 267.716 Recovery = 96.81%						
Cu 324.752†	2314.5	10.138 µg/L	0.3187	10.138 ppb	0.3187	3.14%
QC value within limits for Cu 324.752 Recovery = 101.38%						
Fe 238.204 Radial†	1554.9	103.37 µg/L	0.806	103.37 ppb	0.806	0.78%
QC value within limits for Fe 238.204 Radial Recovery = 103.37%						
K 766.490 Radial†	413.4	170.04 µg/L	16.070	170.04 ppb	16.070	9.45%
QC value within limits for K 766.490 Radial Recovery = 113.36%						
Mg 279.077 IEC†	735.0	303.20 µg/L	2.180	303.20 ppb	2.180	0.72%
QC value within limits for Mg 279.077 IEC Recovery = 101.07%						
Mn 257.610†	7577.3	10.342 µg/L	0.1261	10.342 ppb	0.1261	1.22%
QC value within limits for Mn 257.610 Recovery = 103.42%						
Mo 202.031†	316.2	9.9921 µg/L	0.31074	9.9921 ppb	0.31074	3.11%
QC value within limits for Mo 202.031 Recovery = 99.92%						
Na 589.592 Radial†	1701.9	260.27 µg/L	16.186	260.27 ppb	16.186	6.22%
QC value within limits for Na 589.592 Radial Recovery = 86.76%						
Ni 231.604†	393.5	5.0334 µg/L	0.13439	5.0334 ppb	0.13439	2.67%
QC value within limits for Ni 231.604 Recovery = 100.67%						
P 214.914†	601.9	143.98 µg/L	0.554	143.98 ppb	0.554	0.38%
QC value within limits for P 214.914 Recovery = 95.99%						
Pb 220.353†	160.6	9.7204 µg/L	1.33235	9.7204 ppb	1.33235	13.71%
QC value within limits for Pb 220.353 Recovery = 97.20%						
S 181.975 Axial†	114.6	92.945 µg/L	3.3708	92.945 ppb	3.3708	3.63%
QC value within limits for S 181.975 Axial Recovery = 92.94%						
Sb 206.836†	65.6	8.9415 µg/L	2.72562	8.9415 ppb	2.72562	30.48%
QC value within limits for Sb 206.836 Recovery = 89.41%						
Se 196.026†	74.4	29.5 µg/L	1.90	29.5 ppb	1.90	6.42%
QC value within limits for Se 196.026 Recovery = 98.43%						
SiO2†	1951.4	212.86 µg/L	9.186	212.86 ppb	9.186	4.32%
QC value within limits for SiO2 Recovery = 99.94%						
Si 251.611†	6231.5	102.84 µg/L	3.285	102.84 ppb	3.285	3.19%
QC value within limits for Si 251.611 Recovery = 102.84%						
Sn 189.927†	139.6	9.9381 µg/L	0.26552	9.9381 ppb	0.26552	2.67%
QC value within limits for Sn 189.927 Recovery = 99.38%						
Sr 421.552†	2494.5	5.8448 µg/L	0.17922	5.8448 ppb	0.17922	3.07%
QC value within limits for Sr 421.552 Recovery = 116.90%						
Ti 334.940†	4898.8	4.9492 µg/L	0.10510	4.9492 ppb	0.10510	2.12%
QC value within limits for Ti 334.940 Recovery = 98.98%						
Tl 190.801†	150.8	20.330 µg/L	0.6817	20.330 ppb	0.6817	3.35%
QC value within limits for Tl 190.801 Recovery = 101.65%						
U 409.014†	989.7	61.455 µg/L	10.7804	61.455 ppb	10.7804	17.54%
QC value within limits for U 409.014 Recovery = 122.91%						
V 292.402†	791.0	4.5320 µg/L	0.36774	4.5320 ppb	0.36774	8.11%
QC value within limits for V 292.402 Recovery = 90.64%						
Zn 213.857†	1583.4	9.9190 µg/L	0.18336	9.9190 ppb	0.18336	1.85%
QC value within limits for Zn 213.857 Recovery = 99.19%						
All analyte(s) passed QC.						

Sequence No.: 9

Sample ID: ICSCA

Analyst:

Logged In Analyst (Original) : optima4

Initial Sample Wt:

Dilution:

Autosampler Location: 103

Date Collected: 3/29/2010 18:43:01

Data Type: Reprocessed on 3/29/2010 19:14:38

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: ICSCA

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc 361.383	1519975.5	1519975.5	90.866 %		18:44:01
1	Sc RADIAL	137750.3	137750.3	94.5 %		18:43:34
1	Y 371.029	919968.6	919968.6	89.965 %		18:44:01
1	Ag 328.068†	5916.7	3544.4	1.2267 µg/L	1.2267 ppb	18:44:01
1	Al 396.153Radial†	2228558.9	2358079.9	514740 µg/L	514740 ppb	18:43:31
1	As 188.979†	-88.3	-82.9	8.1301 µg/L	8.1301 ppb	18:44:21
1	B 249.677†	3032.6	-18.3	-0.3191 µg/L	-0.3191 ppb	18:44:01
1	Ba 233.527†	439.8	659.1	0.5804 µg/L	0.5804 ppb	18:44:21
1	Be 313.107†	-620.0	-22.3	0.0066 µg/L	0.0066 ppb	18:44:01
1	Ca 317.933Radial†	7783821.6	8235480.1	482560 µg/L	482560 ppb	18:43:31
1	Cd 226.502†	2257.8	2579.2	-2.2506 µg/L	-2.2506 ppb	18:44:21
1	Co 228.616†	76.3	260.5	-6.3814 µg/L	-6.3814 ppb	18:44:21
1	Cr 267.716†	306.4	176.9	2.2002 µg/L	2.2002 ppb	18:44:21
1	Cu 324.752†	-6875.9	-9992.0	-2.5122 µg/L	-2.5122 ppb	18:44:01
1	Fe 238.204 Radial†	2712004.8	2869471.1	190770 µg/L	190770 ppb	18:43:31
1	K 766.490 Radial†	1538.5	172.9	-171.54 µg/L	-171.54 ppb	18:43:34
1	Mg 279.077 IEC†	1111575.2	1175976.0	484700 µg/L	484700 ppb	18:43:31
1	Mn 257.610†	14620.3	16010.1	2.1476 µg/L	2.1476 ppb	18:44:01
1	Mo 202.031†	-501.7	-496.9	0.7251 µg/L	0.7251 ppb	18:44:01
1	Na 589.592 Radial†	1635.3	35.6	5.3873 µg/L	5.3873 ppb	18:43:34
1	Ni 231.604†	146.0	201.6	2.5791 µg/L	2.5791 ppb	18:44:21
1	P 214.914†	148.1	83.5	4.8563 µg/L	4.8563 ppb	18:44:21
1	Pb 220.353†	-247.5	-384.9	2.4276 µg/L	2.4276 ppb	18:44:21
1	S 181.975 Axial†	166.5	88.4	71.471 µg/L	71.471 ppb	18:44:21
1	Sb 206.836†	109.8	34.2	-1.4541 µg/L	-1.4541 ppb	18:44:21
1	Se 196.026†	-143.9	-169.3	-0.728 µg/L	-0.728 ppb	18:44:21
1	SiO2†	1500.4	78.4	8.9950 µg/L	8.9950 ppb	18:44:21
1	Si 251.611†	379.6	-258.7	-4.0756 µg/L	-4.0756 ppb	18:44:21
1	Sn 189.927†	17.0	16.7	1.2650 µg/L	1.2650 ppb	18:44:21
1	Sr 421.552†	1360.0	1717.1	0.2472 µg/L	0.2472 ppb	18:43:34
1	Ti 334.940†	20973.2	22445.2	-4.0421 µg/L	-4.0421 ppb	18:44:01
1	Tl 190.801†	-165.7	-62.0	-7.8287 µg/L	-7.8287 ppb	18:44:21
1	U 409.014†	239.9	743.1	25.180 µg/L	25.180 ppb	18:44:01
1	V 292.402†	5463.3	5580.7	0.4848 µg/L	0.4848 ppb	18:44:01
1	Zn 213.857†	3868.4	3792.8	7.6857 µg/L	7.6857 ppb	18:44:21
2	Sc 361.383	1532514.6	1532514.6	91.615 %		18:44:24
2	Sc RADIAL	139244.5	139244.5	95.5 %		18:43:38
2	Y 371.029	927898.5	927898.5	90.741 %		18:44:24
2	Ag 328.068†	5725.2	3282.1	0.2956 µg/L	0.2956 ppb	18:44:24
2	Al 396.153Radial†	2228857.8	2333088.7	509290 µg/L	509290 ppb	18:43:36
2	As 188.979†	-96.0	-90.5	4.5139 µg/L	4.5139 ppb	18:44:44
2	B 249.677†	3203.6	141.1	2.3574 µg/L	2.3574 ppb	18:44:24
2	Ba 233.527†	417.7	631.0	0.4768 µg/L	0.4768 ppb	18:44:44
2	Be 313.107†	-855.2	-273.4	-0.0781 µg/L	-0.0781 ppb	18:44:24
2	Ca 317.933Radial†	7791433.2	8155066.3	477850 µg/L	477850 ppb	18:43:36
2	Cd 226.502†	2233.3	2532.1	-2.3767 µg/L	-2.3767 ppb	18:44:44
2	Co 228.616†	66.6	249.3	-6.4368 µg/L	-6.4368 ppb	18:44:44
2	Cr 267.716†	246.3	108.6	1.6057 µg/L	1.6057 ppb	18:44:44
2	Cu 324.752†	-6872.9	-9926.8	-2.6212 µg/L	-2.6212 ppb	18:44:24
2	Fe 238.204 Radial†	2714288.8	2841068.4	188880 µg/L	188880 ppb	18:43:36
2	K 766.490 Radial†	1618.0	238.7	-142.04 µg/L	-142.04 ppb	18:43:38
2	Mg 279.077 IEC†	1114260.0	1166165.0	480660 µg/L	480660 ppb	18:43:36
2	Mn 257.610†	14586.8	15841.8	2.0830 µg/L	2.0830 ppb	18:44:24
2	Mo 202.031†	-508.1	-499.4	0.4957 µg/L	0.4957 ppb	18:44:24
2	Na 589.592 Radial†	1714.1	99.5	15.141 µg/L	15.141 ppb	18:43:38
2	Ni 231.604†	152.3	207.2	2.6500 µg/L	2.6500 ppb	18:44:44
2	P 214.914†	105.5	35.5	-6.5606 µg/L	-6.5606 ppb	18:44:44
2	Pb 220.353†	-290.5	-429.6	-0.5500 µg/L	-0.5500 ppb	18:44:44

2	S 181.975 Axial†	171.6	92.5	74.799 µg/L	74.799 ppb	18:44:44
2	Sb 206.836†	130.7	56.0	1.5606 µg/L	1.5606 ppb	18:44:44
2	Se 196.026†	-155.0	-180.1	-5.67 µg/L	-5.67 ppb	18:44:44
2	SiO2†	1504.6	69.4	8.0425 µg/L	8.0425 ppb	18:44:44
2	Si 251.611†	375.1	-267.0	-4.2014 µg/L	-4.2014 ppb	18:44:44
2	Sn 189.927†	-4.2	-6.6	-0.3924 µg/L	-0.3924 ppb	18:44:44
2	Sr 421.552†	1366.5	1708.4	0.2637 µg/L	0.2637 ppb	18:43:38
2	Ti 334.940†	21214.1	22519.4	-3.7556 µg/L	-3.7556 ppb	18:44:24
2	Tl 190.801†	-155.0	-48.9	-6.0537 µg/L	-6.0537 ppb	18:44:44
2	U 409.014†	96.2	584.1	15.646 µg/L	15.646 ppb	18:44:24
2	V 292.402†	5684.6	5773.1	1.8417 µg/L	1.8417 ppb	18:44:24
2	Zn 213.857†	3858.3	3747.0	7.5506 µg/L	7.5506 ppb	18:44:44
3	Sc 361.383	1531662.1	1531662.1	91.564 %		18:44:46
3	Sc RADIAL	139848.7	139848.7	95.9 %		18:43:42
3	Y 371.029	927170.5	927170.5	90.670 %		18:44:46
3	Ag 328.068†	5762.9	3326.8	0.5251 µg/L	0.5251 ppb	18:44:46
3	Al 396.153Radial†	2231390.2	2325648.7	507660 µg/L	507660 ppb	18:43:40
3	As 188.979†	-103.4	-98.7	0.8735 µg/L	0.8735 ppb	18:45:06
3	B 249.677†	3235.4	177.8	2.9710 µg/L	2.9710 ppb	18:44:46
3	Ba 233.527†	402.4	614.5	0.4137 µg/L	0.4137 ppb	18:45:06
3	Be 313.107†	-678.3	-80.7	-0.0209 µg/L	-0.0209 ppb	18:44:46
3	Ca 317.933Radial†	7787439.6	8115669.6	475540 µg/L	475540 ppb	18:43:40
3	Cd 226.502†	2245.5	2546.8	-2.1709 µg/L	-2.1709 ppb	18:45:06
3	Co 228.616†	93.2	278.4	-5.9871 µg/L	-5.9871 ppb	18:45:06
3	Cr 267.716†	275.9	141.1	1.8999 µg/L	1.8999 ppb	18:45:06
3	Cu 324.752†	-6732.3	-9777.4	-2.2074 µg/L	-2.2074 ppb	18:44:46
3	Fe 238.204 Radial†	2711795.4	2826195.2	187900 µg/L	187900 ppb	18:43:40
3	K 766.490 Radial†	1584.0	195.9	-158.63 µg/L	-158.63 ppb	18:43:42
3	Mg 279.077 IEC†	1112495.6	1159287.1	477830 µg/L	477830 ppb	18:43:40
3	Mn 257.610†	14462.2	15714.6	2.0242 µg/L	2.0242 ppb	18:44:46
3	Mo 202.031†	-593.4	-592.8	-2.5422 µg/L	-2.5422 ppb	18:44:46
3	Na 589.592 Radial†	1732.7	111.2	16.939 µg/L	16.939 ppb	18:43:42
3	Ni 231.604†	209.1	269.3	3.4450 µg/L	3.4450 ppb	18:45:06
3	P 214.914†	118.4	49.8	-2.8056 µg/L	-2.8056 ppb	18:45:06
3	Pb 220.353†	-264.9	-401.8	1.0704 µg/L	1.0704 ppb	18:45:06
3	S 181.975 Axial†	171.3	92.2	74.546 µg/L	74.546 ppb	18:45:06
3	Sb 206.836†	101.8	24.6	-2.6986 µg/L	-2.6986 ppb	18:45:06
3	Se 196.026†	-151.8	-176.7	-4.70 µg/L	-4.70 ppb	18:45:06
3	SiO2†	1457.7	19.2	2.6178 µg/L	2.6178 ppb	18:45:06
3	Si 251.611†	375.6	-266.2	-4.1555 µg/L	-4.1555 ppb	18:45:06
3	Sn 189.927†	9.2	8.1	0.6527 µg/L	0.6527 ppb	18:45:06
3	Sr 421.552†	1404.5	1741.8	0.3601 µg/L	0.3601 ppb	18:43:42
3	Ti 334.940†	21500.8	22845.3	-3.2450 µg/L	-3.2450 ppb	18:44:46
3	Tl 190.801†	-148.3	-41.6	-5.0807 µg/L	-5.0807 ppb	18:45:06
3	U 409.014†	-176.5	286.3	-2.6068 µg/L	-2.6068 ppb	18:44:46
3	V 292.402†	5753.1	5851.3	2.3911 µg/L	2.3911 ppb	18:44:46
3	Zn 213.857†	3845.3	3735.2	7.5699 µg/L	7.5699 ppb	18:45:06

Mean Data: ICSCA

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1528050.7	91.348 %	0.4188			0.46%
Sc RADIAL	138947.9	95.3 %	0.74			0.78%
Y 371.029	925012.6	90.459 %	0.4287			0.47%
Ag 328.068†	3384.5	0.6825 µg/L	0.48505	0.6825 ppb	0.48505	71.07%
QC value within limits for Ag 328.068 Recovery = Not calculated						
Al 396.153Radial†	2338939.1	510560 µg/L	3708.4	510560 ppb	3708.4	0.73%
QC value within limits for Al 396.153Radial Recovery = 102.11%						
As 188.979†	-90.7	4.5059 µg/L	3.62830	4.5059 ppb	3.62830	80.52%
QC value within limits for As 188.979 Recovery = Not calculated						
B 249.677†	100.2	1.6697 µg/L	1.74948	1.6697 ppb	1.74948	104.78%
QC value within limits for B 249.677 Recovery = Not calculated						
Ba 233.527†	634.8	0.4903 µg/L	0.08415	0.4903 ppb	0.08415	17.16%
QC value within limits for Ba 233.527 Recovery = Not calculated						
Be 313.107†	-125.5	-0.0308 µg/L	0.04321	-0.0308 ppb	0.04321	140.33%
QC value within limits for Be 313.107 Recovery = Not calculated						
Ca 317.933Radial†	8168738.7	478650 µg/L	3578.1	478650 ppb	3578.1	0.75%
QC value within limits for Ca 317.933Radial Recovery = 95.73%						
Cd 226.502†	2552.7	-2.2661 µg/L	0.10379	-2.2661 ppb	0.10379	4.58%
QC value within limits for Cd 226.502 Recovery = Not calculated						

Co 228.616†	262.7	-6.2685 µg/L	0.24520	-6.2685 ppb	0.24520	3.91%
QC value within limits for Co 228.616 Recovery = Not calculated						
Cr 267.716†	142.2	1.9019 µg/L	0.29723	1.9019 ppb	0.29723	15.63%
QC value within limits for Cr 267.716 Recovery = Not calculated						
Cu 324.752†	-9898.7	-2.4469 µg/L	0.21446	-2.4469 ppb	0.21446	8.76%
QC value within limits for Cu 324.752 Recovery = Not calculated						
Fe 238.204 Radial†	2845578.2	189180 µg/L	1461.8	189180 ppb	1461.8	0.77%
QC value within limits for Fe 238.204 Radial Recovery = 94.59%						
K 766.490 Radial†	202.5	-157.40 µg/L	14.790	-157.40 ppb	14.790	9.40%
QC value within limits for K 766.490 Radial Recovery = Not calculated						
Mg 279.077 IEC†	1167142.7	481060 µg/L	3456.9	481060 ppb	3456.9	0.72%
QC value within limits for Mg 279.077 IEC Recovery = 96.21%						
Mn 257.610†	15855.5	2.0849 µg/L	0.06170	2.0849 ppb	0.06170	2.96%
QC value within limits for Mn 257.610 Recovery = Not calculated						
Mo 202.031†	-529.7	-0.4405 µg/L	1.82378	-0.4405 ppb	1.82378	414.05%
QC value within limits for Mo 202.031 Recovery = Not calculated						
Na 589.592 Radial†	82.1	12.489 µg/L	6.2157	12.489 ppb	6.2157	49.77%
QC value within limits for Na 589.592 Radial Recovery = Not calculated						
Ni 231.604†	226.0	2.8914 µg/L	0.48079	2.8914 ppb	0.48079	16.63%
QC value within limits for Ni 231.604 Recovery = Not calculated						
P 214.914†	56.3	-1.5033 µg/L	5.81883	-1.5033 ppb	5.81883	387.07%
QC value within limits for P 214.914 Recovery = Not calculated						
Pb 220.353†	-405.4	0.9827 µg/L	1.49074	0.9827 ppb	1.49074	151.70%
QC value within limits for Pb 220.353 Recovery = Not calculated						
S 181.975 Axial†	91.0	73.605 µg/L	1.8528	73.605 ppb	1.8528	2.52%
QC value within limits for S 181.975 Axial Recovery = Not calculated						
Sb 206.836†	38.3	-0.8640 µg/L	2.19006	-0.8640 ppb	2.19006	253.47%
QC value within limits for Sb 206.836 Recovery = Not calculated						
Se 196.026†	-175.4	-3.70 µg/L	2.618	-3.70 ppb	2.618	70.77%
QC value within limits for Se 196.026 Recovery = Not calculated						
SiO2†	55.7	6.5518 µg/L	3.44005	6.5518 ppb	3.44005	52.51%
QC value within limits for SiO2 Recovery = Not calculated						
Si 251.611†	-264.0	-4.1441 µg/L	0.06368	-4.1441 ppb	0.06368	1.54%
QC value within limits for Si 251.611 Recovery = Not calculated						
Sn 189.927†	6.1	0.5084 µg/L	0.83805	0.5084 ppb	0.83805	164.84%
QC value within limits for Sn 189.927 Recovery = Not calculated						
Sr 421.552†	1722.4	0.2904 µg/L	0.06098	0.2904 ppb	0.06098	21.00%
QC value within limits for Sr 421.552 Recovery = Not calculated						
Ti 334.940†	22603.3	-3.6809 µg/L	0.40375	-3.6809 ppb	0.40375	10.97%
QC value within limits for Ti 334.940 Recovery = Not calculated						
Tl 190.801†	-50.8	-6.3210 µg/L	1.39339	-6.3210 ppb	1.39339	22.04%
QC value within limits for Tl 190.801 Recovery = Not calculated						
U 409.014†	537.8	12.740 µg/L	14.1197	12.740 ppb	14.1197	110.83%
QC value within limits for U 409.014 Recovery = Not calculated						
V 292.402†	5735.0	1.5725 µg/L	0.98127	1.5725 ppb	0.98127	62.40%
QC value within limits for V 292.402 Recovery = Not calculated						
Zn 213.857†	3758.3	7.6020 µg/L	0.07306	7.6020 ppb	0.07306	0.96%
QC value within limits for Zn 213.857 Recovery = Not calculated						
All analyte(s) passed QC.						

Sequence No.: 10

Sample ID: ICSAB

Analyst:

Logged In Analyst (Original) : optima4

Initial Sample Wt:

Dilution:

Autosampler Location: 104

Date Collected: 3/29/2010 18:45:15

Data Type: Reprocessed on 3/29/2010 19:14:39

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: ICSAB

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc 361.383	1510684.4	1510684.4	90.310 %		18:46:21
1	Sc RADIAL	137128.2	137128.2	94.1 %		18:45:49
1	Y 371.029	915417.0	915417.0	89.520 %		18:46:21
1	Ag 328.068†	64579.9	68542.0	271.32 µg/L	271.32 ppb	18:46:21
1	Al 396.153Radial†	2257035.7	2399046.7	523660 µg/L	523660 ppb	18:45:45
1	As 188.979†	1040.4	1166.3	536.34 µg/L	536.34 ppb	18:46:23
1	B 249.677†	30637.0	30568.6	511.66 µg/L	511.66 ppb	18:46:21
1	Ba 233.527†	99072.5	109877.7	499.99 µg/L	499.99 ppb	18:46:21
1	Be 313.107†	681148.0	754892.4	245.89 µg/L	245.89 ppb	18:46:21
1	Ca 317.933Radial†	7888724.1	8384349.0	491290 µg/L	491290 ppb	18:45:45
1	Cd 226.502†	63574.5	70490.2	466.80 µg/L	466.80 ppb	18:46:21
1	Co 228.616†	29268.7	32585.7	436.71 µg/L	436.71 ppb	18:46:23
1	Cr 267.716†	51261.8	56601.7	486.64 µg/L	486.64 ppb	18:46:23
1	Cu 324.752†	105042.3	113888.0	536.82 µg/L	536.82 ppb	18:46:21
1	Fe 238.204 Radial†	2714615.2	2885265.2	191820 µg/L	191820 ppb	18:45:47
1	K 766.490 Radial†	14492.6	13949.3	5495.4 µg/L	5495.4 ppb	18:45:49
1	Mg 279.077 IEC†	1107607.9	1177095.4	485180 µg/L	485180 ppb	18:45:49
1	Mn 257.610†	329092.8	364323.1	478.08 µg/L	478.08 ppb	18:46:21
1	Mo 202.031†	13229.8	14704.5	480.80 µg/L	480.80 ppb	18:46:23
1	Na 589.592 Radial†	34394.1	34862.9	5329.4 µg/L	5329.4 ppb	18:45:49
1	Ni 231.604†	31853.0	35311.6	451.68 µg/L	451.68 ppb	18:46:23
1	P 214.914†	9576.1	10524.0	2499.6 µg/L	2499.6 ppb	18:46:23
1	Pb 220.353†	6597.4	7192.9	463.36 µg/L	463.36 ppb	18:46:23
1	S 181.975 Axial†	3009.0	3237.0	2626.5 µg/L	2626.5 ppb	18:46:23
1	Sb 206.836†	3499.0	3787.8	505.98 µg/L	505.98 ppb	18:46:23
1	Se 196.026†	5309.9	5868.7	2390 µg/L	2390 ppb	18:46:23
1	SiO2†	92256.7	100582.6	10974 µg/L	10974 ppb	18:46:21
1	Si 251.611†	281270.8	310773.6	5129.3 µg/L	5129.3 ppb	18:46:21
1	Sn 189.927†	6022.0	6666.1	475.68 µg/L	475.68 ppb	18:46:23
1	Sr 421.552†	210049.1	223540.3	520.07 µg/L	520.07 ppb	18:45:49
1	Ti 334.940†	468269.2	517876.1	500.97 µg/L	500.97 ppb	18:46:21
1	Tl 190.801†	2818.9	3241.7	443.45 µg/L	443.45 ppb	18:46:23
1	U 409.014†	7133.6	8378.1	528.93 µg/L	528.93 ppb	18:46:21
1	V 292.402†	88326.4	97371.6	516.38 µg/L	516.38 ppb	18:46:21
1	Zn 213.857†	72620.0	79947.4	483.88 µg/L	483.88 ppb	18:46:21
2	Sc 361.383	1518034.6	1518034.6	90.750 %		18:46:26
2	Sc RADIAL	136837.3	136837.3	93.9 %		18:45:56
2	Y 371.029	919619.6	919619.6	89.931 %		18:46:26
2	Ag 328.068†	64494.6	68101.8	269.69 µg/L	269.69 ppb	18:46:26
2	Al 396.153Radial†	2229777.5	2375110.8	518440 µg/L	518440 ppb	18:45:52
2	As 188.979†	1016.8	1134.7	522.67 µg/L	522.67 ppb	18:46:28
2	B 249.677†	30917.4	30713.3	514.09 µg/L	514.09 ppb	18:46:26
2	Ba 233.527†	99392.7	109699.3	499.19 µg/L	499.19 ppb	18:46:26
2	Be 313.107†	684598.1	755042.2	245.93 µg/L	245.93 ppb	18:46:26
2	Ca 317.933Radial†	7784991.4	8291677.2	485860 µg/L	485860 ppb	18:45:52
2	Cd 226.502†	63805.9	70404.3	466.38 µg/L	466.38 ppb	18:46:26
2	Co 228.616†	29275.9	32436.7	434.76 µg/L	434.76 ppb	18:46:28
2	Cr 267.716†	50741.5	55753.6	479.35 µg/L	479.35 ppb	18:46:28
2	Cu 324.752†	105439.6	113762.6	535.91 µg/L	535.91 ppb	18:46:26
2	Fe 238.204 Radial†	2684811.7	2859651.8	190120 µg/L	190120 ppb	18:45:54
2	K 766.490 Radial†	14227.4	13699.5	5395.1 µg/L	5395.1 ppb	18:45:56
2	Mg 279.077 IEC†	1095117.9	1166293.6	480720 µg/L	480720 ppb	18:45:56
2	Mn 257.610†	330574.5	364191.4	478.08 µg/L	478.08 ppb	18:46:26
2	Mo 202.031†	13322.6	14735.9	481.64 µg/L	481.64 ppb	18:46:28
2	Na 589.592 Radial†	34233.3	34769.4	5315.2 µg/L	5315.2 ppb	18:45:56
2	Ni 231.604†	31592.4	34853.7	445.82 µg/L	445.82 ppb	18:46:28
2	P 214.914†	9407.5	10286.9	2442.8 µg/L	2442.8 ppb	18:46:28
2	Pb 220.353†	6453.4	6998.8	451.34 µg/L	451.34 ppb	18:46:28

2	S 181.975 Axial†	2940.7	3145.6	2552.4 µg/L	2552.4 ppb	18:46:28
2	Sb 206.836†	3475.9	3743.6	500.18 µg/L	500.18 ppb	18:46:28
2	Se 196.026†	5145.8	5659.4	2310 µg/L	2310 ppb	18:46:28
2	SiO2†	92799.3	100685.9	10985 µg/L	10985 ppb	18:46:26
2	Si 251.611†	282521.5	310643.8	5127.1 µg/L	5127.1 ppb	18:46:26
2	Sn 189.927†	5996.0	6605.2	471.35 µg/L	471.35 ppb	18:46:28
2	Sr 421.552†	208807.5	222692.2	518.13 µg/L	518.13 ppb	18:45:56
2	Ti 334.940†	470515.6	517840.9	501.16 µg/L	501.16 ppb	18:46:26
2	Tl 190.801†	2878.3	3292.0	450.21 µg/L	450.21 ppb	18:46:28
2	U 409.014†	7163.0	8372.3	528.73 µg/L	528.73 ppb	18:46:26
2	V 292.402†	88754.8	97370.2	516.63 µg/L	516.63 ppb	18:46:26
2	Zn 213.857†	72903.7	79870.6	483.58 µg/L	483.58 ppb	18:46:26
3	Sc 361.383	1509678.5	1509678.5	90.250 %		18:46:31
3	Sc RADIAL	138373.5	138373.5	94.9 %		18:46:03
3	Y 371.029	914674.1	914674.1	89.448 %		18:46:31
3	Ag 328.068†	64587.4	68598.0	271.77 µg/L	271.77 ppb	18:46:31
3	Al 396.153Radial†	2250390.9	2370456.7	517420 µg/L	517420 ppb	18:45:58
3	As 188.979†	1006.1	1129.0	520.40 µg/L	520.40 ppb	18:46:33
3	B 249.677†	30857.6	30835.5	516.13 µg/L	516.13 ppb	18:46:31
3	Ba 233.527†	99227.6	110122.6	501.13 µg/L	501.13 ppb	18:46:31
3	Be 313.107†	682431.3	756816.9	246.51 µg/L	246.51 ppb	18:46:31
3	Ca 317.933Radial†	7834035.4	8251280.0	483490 µg/L	483490 ppb	18:45:58
3	Cd 226.502†	63517.1	70473.5	466.87 µg/L	466.87 ppb	18:46:31
3	Co 228.616†	29487.3	32849.5	440.42 µg/L	440.42 ppb	18:46:33
3	Cr 267.716†	51368.6	56757.9	487.95 µg/L	487.95 ppb	18:46:33
3	Cu 324.752†	105432.6	114397.9	538.71 µg/L	538.71 ppb	18:46:31
3	Fe 238.204 Radial†	2714742.3	2859431.1	190100 µg/L	190100 ppb	18:46:01
3	K 766.490 Radial†	14507.9	13826.8	5448.0 µg/L	5448.0 ppb	18:46:03
3	Mg 279.077 IEC†	1111196.5	1170280.1	482370 µg/L	482370 ppb	18:46:03
3	Mn 257.610†	329292.9	364787.6	478.83 µg/L	478.83 ppb	18:46:31
3	Mo 202.031†	13311.3	14804.5	483.83 µg/L	483.83 ppb	18:46:33
3	Na 589.592 Radial†	34668.7	34823.2	5323.3 µg/L	5323.3 ppb	18:46:03
3	Ni 231.604†	31996.5	35494.2	454.01 µg/L	454.01 ppb	18:46:33
3	P 214.914†	9605.6	10563.7	2508.9 µg/L	2508.9 ppb	18:46:33
3	Pb 220.353†	6567.4	7164.5	461.32 µg/L	461.32 ppb	18:46:33
3	S 181.975 Axial†	2974.8	3201.4	2597.7 µg/L	2597.7 ppb	18:46:33
3	Sb 206.836†	3463.3	3750.8	501.08 µg/L	501.08 ppb	18:46:33
3	Se 196.026†	5291.7	5852.5	2380 µg/L	2380 ppb	18:46:33
3	SiO2†	92489.2	100908.3	11009 µg/L	11009 ppb	18:46:31
3	Si 251.611†	281639.3	311389.5	5139.4 µg/L	5139.4 ppb	18:46:31
3	Sn 189.927†	6087.5	6743.1	481.17 µg/L	481.17 ppb	18:46:33
3	Sr 421.552†	210738.5	222257.1	517.13 µg/L	517.13 ppb	18:46:03
3	Ti 334.940†	470683.6	520896.9	504.08 µg/L	504.08 ppb	18:46:31
3	Tl 190.801†	2864.6	3294.4	450.54 µg/L	450.54 ppb	18:46:33
3	U 409.014†	7145.1	8396.1	530.14 µg/L	530.14 ppb	18:46:31
3	V 292.402†	88390.3	97507.5	517.45 µg/L	517.45 ppb	18:46:31
3	Zn 213.857†	72542.0	79914.6	483.81 µg/L	483.81 ppb	18:46:31

Mean Data: ICSAB

Analyte	Mean Corrected Intensity	Conc. Units	Calib. Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1512799.2	90.437 %	0.2727			0.30%
Sc RADIAL	137446.3	94.3 %	0.56			0.59%
Y 371.029	916570.2	89.633 %	0.2608			0.29%
Ag 328.068†	68413.9	270.93 µg/L	1.098	270.93 ppb	1.098	0.41%
QC value within limits for Ag 328.068 Recovery = 108.37%						
Al 396.153Radial†	2381538.1	519840 µg/L	3348.7	519840 ppb	3348.7	0.64%
QC value within limits for Al 396.153Radial Recovery = 103.97%						
As 188.979†	1143.3	526.47 µg/L	8.621	526.47 ppb	8.621	1.64%
QC value within limits for As 188.979 Recovery = 105.29%						
B 249.677†	30705.8	513.96 µg/L	2.238	513.96 ppb	2.238	0.44%
QC value within limits for B 249.677 Recovery = 102.79%						
Ba 233.527†	109899.8	500.10 µg/L	0.973	500.10 ppb	0.973	0.19%
QC value within limits for Ba 233.527 Recovery = 100.02%						
Be 313.107†	755583.8	246.11 µg/L	0.349	246.11 ppb	0.349	0.14%
QC value within limits for Be 313.107 Recovery = 98.44%						
Ca 317.933Radial†	8309102.1	486880 µg/L	3997.7	486880 ppb	3997.7	0.82%
QC value within limits for Ca 317.933Radial Recovery = 97.38%						
Cd 226.502†	70456.0	466.68 µg/L	0.262	466.68 ppb	0.262	0.06%
QC value within limits for Cd 226.502 Recovery = 93.34%						

Co 228.616†	32623.9	437.30 µg/L	2.873	437.30 ppb	2.873	0.66%
QC value within limits for Co 228.616 Recovery = 87.46%						
Cr 267.716†	56371.1	484.65 µg/L	4.635	484.65 ppb	4.635	0.96%
QC value within limits for Cr 267.716 Recovery = 96.93%						
Cu 324.752†	114016.2	537.15 µg/L	1.432	537.15 ppb	1.432	0.27%
QC value within limits for Cu 324.752 Recovery = 107.43%						
Fe 238.204 Radial†	2868116.0	190680 µg/L	987.4	190680 ppb	987.4	0.52%
QC value within limits for Fe 238.204 Radial Recovery = 95.34%						
K 766.490 Radial†	13825.2	5446.2 µg/L	50.18	5446.2 ppb	50.18	0.92%
QC value within limits for K 766.490 Radial Recovery = 108.92%						
Mg 279.077 IEC†	1171223.1	482760 µg/L	2251.4	482760 ppb	2251.4	0.47%
QC value within limits for Mg 279.077 IEC Recovery = 96.55%						
Mn 257.610†	364434.0	478.33 µg/L	0.433	478.33 ppb	0.433	0.09%
QC value within limits for Mn 257.610 Recovery = 95.67%						
Mo 202.031†	14748.3	482.09 µg/L	1.569	482.09 ppb	1.569	0.33%
QC value within limits for Mo 202.031 Recovery = 96.42%						
Na 589.592 Radial†	34818.5	5322.6 µg/L	7.14	5322.6 ppb	7.14	0.13%
QC value within limits for Na 589.592 Radial Recovery = 106.45%						
Ni 231.604†	35219.8	450.50 µg/L	4.221	450.50 ppb	4.221	0.94%
QC value within limits for Ni 231.604 Recovery = 90.10%						
P 214.914†	10458.2	2483.8 µg/L	35.79	2483.8 ppb	35.79	1.44%
QC value within limits for P 214.914 Recovery = 99.35%						
Pb 220.353†	7118.7	458.68 µg/L	6.431	458.68 ppb	6.431	1.40%
QC value within limits for Pb 220.353 Recovery = 91.74%						
S 181.975 Axial†	3194.7	2592.2 µg/L	37.32	2592.2 ppb	37.32	1.44%
QC value within limits for S 181.975 Axial Recovery = 103.69%						
Sb 206.836†	3760.7	502.41 µg/L	3.120	502.41 ppb	3.120	0.62%
QC value within limits for Sb 206.836 Recovery = 100.48%						
Se 196.026†	5793.5	2360 µg/L	46.2	2360 ppb	46.2	1.96%
QC value within limits for Se 196.026 Recovery = 94.33%						
SiO2†	100725.6	10989 µg/L	18.1	10989 ppb	18.1	0.16%
QC value within limits for SiO2 Recovery = 102.75%						
Si 251.611†	310935.6	5131.9 µg/L	6.54	5131.9 ppb	6.54	0.13%
QC value within limits for Si 251.611 Recovery = 102.64%						
Sn 189.927†	6671.5	476.07 µg/L	4.919	476.07 ppb	4.919	1.03%
QC value within limits for Sn 189.927 Recovery = 95.21%						
Sr 421.552†	222829.9	518.44 µg/L	1.498	518.44 ppb	1.498	0.29%
QC value within limits for Sr 421.552 Recovery = 103.69%						
Ti 334.940†	518871.3	502.07 µg/L	1.741	502.07 ppb	1.741	0.35%
QC value within limits for Ti 334.940 Recovery = 100.41%						
Tl 190.801†	3276.0	448.07 µg/L	4.004	448.07 ppb	4.004	0.89%
QC value within limits for Tl 190.801 Recovery = 89.61%						
U 409.014†	8382.2	529.27 µg/L	0.763	529.27 ppb	0.763	0.14%
QC value within limits for U 409.014 Recovery = 105.85%						
V 292.402†	97416.4	516.82 µg/L	0.558	516.82 ppb	0.558	0.11%
QC value within limits for V 292.402 Recovery = 103.36%						
Zn 213.857†	79910.9	483.76 µg/L	0.156	483.76 ppb	0.156	0.03%
QC value within limits for Zn 213.857 Recovery = 96.75%						
All analyte(s) passed QC.						

Sequence No.: 11

Sample ID: LR1

Analyst:

Logged In Analyst (Original) : optima4

Initial Sample Wt:

Dilution:

Autosampler Location: 105

Date Collected: 3/29/2010 18:46:42

Data Type: Reprocessed on 3/29/2010 19:14:40

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: LR1

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc 361.383	1475217.1	1475217.1	88.190 %		18:47:41
1	Sc RADIAL	134988.0	134988.0	92.6 %		18:47:14
1	Y 371.029	890652.0	890652.0	87.098 %		18:47:41
1	Ag 328.068†	2600.2	-18.7	4.2300 µg/L	4.2300 ppb	18:47:41
1	Al 396.153Radial†	2173247.9	2346612.0	512240 µg/L	512240 ppb	18:47:12
1	As 188.979†	-221.7	-237.2	2.3463 µg/L	2.3463 ppb	18:47:43
1	B 249.677†	3640.1	771.9	12.918 µg/L	12.918 ppb	18:47:41
1	Ba 233.527†	451.6	687.2	-2.6252 µg/L	-2.6252 ppb	18:47:43
1	Be 313.107†	-13095.3	-14188.9	-0.0322 µg/L	-0.0322 ppb	18:47:41
1	Ca 317.933Radial†	7559025.2	8161296.1	478220 µg/L	478220 ppb	18:47:12
1	Cd 226.502†	5610.9	6456.7	-2.9745 µg/L	-2.9745 ppb	18:47:43
1	Co 228.616†	613.3	872.0	-11.650 µg/L	-11.650 ppb	18:47:43
1	Cr 267.716†	908.0	869.3	5.4318 µg/L	5.4318 ppb	18:47:43
1	Cu 324.752†	-17506.0	-22275.2	-5.5587 µg/L	-5.5587 ppb	18:47:43
1	Fe 238.204 Radial†	6300456.2	6802850.0	452280 µg/L	452280 ppb	18:47:12
1	K 766.490 Radial†	1898.7	595.1	-78.007 µg/L	-78.007 ppb	18:47:14
1	Mg 279.077 IEC†	1069506.5	1154620.7	475670 µg/L	475670 ppb	18:47:12
1	Mn 257.610†	14951.4	16873.6	2.9939 µg/L	2.9939 ppb	18:47:41
1	Mo 202.031†	-853.5	-912.6	-2.2055 µg/L	-2.2055 ppb	18:47:41
1	Na 589.592 Radial†	3064907.6	3307661.5	506110 µg/L	506110 ppb	18:47:12
1	Ni 231.604†	241.8	315.0	4.0298 µg/L	4.0298 ppb	18:47:43
1	P 214.914†	851.2	885.7	19.361 µg/L	19.361 ppb	18:47:43
1	Pb 220.353†	111.2	13.7	6.6643 µg/L	6.6643 ppb	18:47:43
1	S 181.975 Axial†	199.5	131.4	106.18 µg/L	106.18 ppb	18:47:43
1	Sb 206.836†	173.5	110.1	5.3162 µg/L	5.3162 ppb	18:47:43
1	Se 196.026†	-269.6	-316.6	46.3 µg/L	46.3 ppb	18:47:43
1	SiO2†	1875.2	553.5	61.247 µg/L	61.247 ppb	18:47:43
1	Si 251.611†	-2234.1	-3209.7	-52.717 µg/L	-52.717 ppb	18:47:43
1	Sn 189.927†	58.5	64.3	4.6670 µg/L	4.6670 ppb	18:47:43
1	Sr 421.552†	4787.3	5447.1	9.0235 µg/L	9.0235 ppb	18:47:14
1	Ti 334.940†	25472.1	28246.9	-3.7159 µg/L	-3.7159 ppb	18:47:41
1	Tl 190.801†	-294.1	-213.1	-27.836 µg/L	-27.836 ppb	18:47:43
1	U 409.014†	216123.9	245545.7	15094 µg/L	15094 ppb	18:47:41
1	V 292.402†	10776.3	11787.7	3.3989 µg/L	3.3989 ppb	18:47:43
1	Zn 213.857†	7832.8	8417.4	9.2023 µg/L	9.2023 ppb	18:47:43
2	Sc 361.383	1474797.5	1474797.5	88.165 %		18:47:46
2	Sc RADIAL	136487.8	136487.8	93.6 %		18:47:19
2	Y 371.029	890090.9	890090.9	87.044 %		18:47:46
2	Ag 328.068†	2591.0	-28.2	4.2336 µg/L	4.2336 ppb	18:47:46
2	Al 396.153Radial†	2181204.6	2329323.3	508460 µg/L	508460 ppb	18:47:17
2	As 188.979†	-251.7	-271.3	-12.460 µg/L	-12.460 ppb	18:47:48
2	B 249.677†	3729.3	874.2	14.628 µg/L	14.628 ppb	18:47:46
2	Ba 233.527†	527.6	773.5	-2.2009 µg/L	-2.2009 ppb	18:47:48
2	Be 313.107†	-13474.2	-14622.9	-0.1807 µg/L	-0.1807 ppb	18:47:46
2	Ca 317.933Radial†	7600178.4	8115555.5	475540 µg/L	475540 ppb	18:47:17
2	Cd 226.502†	5683.2	6540.6	-2.1393 µg/L	-2.1393 ppb	18:47:48
2	Co 228.616†	752.5	1030.1	-9.3590 µg/L	-9.3590 ppb	18:47:48
2	Cr 267.716†	724.6	661.7	3.6080 µg/L	3.6080 ppb	18:47:48
2	Cu 324.752†	-17459.2	-22227.9	-5.7811 µg/L	-5.7811 ppb	18:47:48
2	Fe 238.204 Radial†	6336284.1	6766355.5	449850 µg/L	449850 ppb	18:47:17
2	K 766.490 Radial†	1981.3	660.8	-49.077 µg/L	-49.077 ppb	18:47:19
2	Mg 279.077 IEC†	1076643.1	1149552.1	473590 µg/L	473590 ppb	18:47:17
2	Mn 257.610†	15045.5	16985.2	3.2356 µg/L	3.2356 ppb	18:47:46
2	Mo 202.031†	-881.3	-944.4	-3.3453 µg/L	-3.3453 ppb	18:47:46
2	Na 589.592 Radial†	3084400.4	3292112.6	503740 µg/L	503740 ppb	18:47:17
2	Ni 231.604†	341.9	428.7	5.4833 µg/L	5.4833 ppb	18:47:48
2	P 214.914†	888.6	928.3	30.390 µg/L	30.390 ppb	18:47:48
2	Pb 220.353†	63.3	-40.6	3.2317 µg/L	3.2317 ppb	18:47:48

2	S 181.975 Axial†	169.7	97.6	78.843 µg/L	78.843 ppb	18:47:48
2	Sb 206.836†	95.2	21.4	-6.5888 µg/L	-6.5888 ppb	18:47:48
2	Se 196.026†	-403.3	-468.4	-14.6 µg/L	-14.6 ppb	18:47:48
2	SiO2†	1816.0	486.9	54.020 µg/L	54.020 ppb	18:47:48
2	Si 251.611†	-2084.7	-3041.0	-49.906 µg/L	-49.906 ppb	18:47:48
2	Sn 189.927†	43.9	47.8	3.4920 µg/L	3.4920 ppb	18:47:48
2	Sr 421.552†	4824.6	5430.1	9.0047 µg/L	9.0047 ppb	18:47:19
2	Ti 334.940†	25083.7	27814.6	-4.0459 µg/L	-4.0459 ppb	18:47:46
2	Tl 190.801†	-241.3	-153.4	-19.840 µg/L	-19.840 ppb	18:47:48
2	U 409.014†	215721.0	245158.5	15071 µg/L	15071 ppb	18:47:46
2	V 292.402†	10612.7	11605.5	2.7405 µg/L	2.7405 ppb	18:47:48
2	Zn 213.857†	7898.7	8494.6	9.8973 µg/L	9.8973 ppb	18:47:48
3	Sc 361.383	1482973.9	1482973.9	88.654 %		18:47:51
3	Sc RADIAL	135581.7	135581.7	93.0 %		18:47:23
3	Y 371.029	894893.3	894893.3	87.513 %		18:47:51
3	Ag 328.068†	2907.1	312.1	5.3159 µg/L	5.3159 ppb	18:47:51
3	Al 396.153Radial†	2198157.6	2363115.2	515840 µg/L	515840 ppb	18:47:21
3	As 188.979†	-166.7	-173.8	30.035 µg/L	30.035 ppb	18:47:53
3	B 249.677†	3819.0	952.0	15.940 µg/L	15.940 ppb	18:47:51
3	Ba 233.527†	467.2	702.0	-2.6283 µg/L	-2.6283 ppb	18:47:53
3	Be 313.107†	-13583.2	-14661.6	-0.1997 µg/L	-0.1997 ppb	18:47:51
3	Ca 317.933Radial†	7679845.3	8255440.6	483730 µg/L	483730 ppb	18:47:21
3	Cd 226.502†	5523.3	6324.6	-4.4547 µg/L	-4.4547 ppb	18:47:53
3	Co 228.616†	665.1	926.8	-11.181 µg/L	-11.181 ppb	18:47:53
3	Cr 267.716†	895.3	849.6	5.3942 µg/L	5.3942 ppb	18:47:53
3	Cu 324.752†	-17409.5	-22062.6	-3.6839 µg/L	-3.6839 ppb	18:47:53
3	Fe 238.204 Radial†	6403813.8	6884172.5	457680 µg/L	457680 ppb	18:47:21
3	K 766.490 Radial†	2077.2	778.0	-6.1386 µg/L	-6.1386 ppb	18:47:23
3	Mg 279.077 IEC†	1090892.1	1172554.0	483060 µg/L	483060 ppb	18:47:21
3	Mn 257.610†	15096.7	16948.9	2.7894 µg/L	2.7894 ppb	18:47:51
3	Mo 202.031†	-879.5	-936.8	-2.6225 µg/L	-2.6225 ppb	18:47:51
3	Na 589.592 Radial†	3116499.7	3348632.9	512380 µg/L	512380 ppb	18:47:21
3	Ni 231.604†	249.4	322.2	4.1219 µg/L	4.1219 ppb	18:47:53
3	P 214.914†	734.4	748.9	-16.245 µg/L	-16.245 ppb	18:47:53
3	Pb 220.353†	-96.4	-221.1	-7.4793 µg/L	-7.4793 ppb	18:47:53
3	S 181.975 Axial†	169.9	96.8	78.205 µg/L	78.205 ppb	18:47:53
3	Sb 206.836†	73.9	-3.3	-10.074 µg/L	-10.074 ppb	18:47:53
3	Se 196.026†	-324.5	-376.9	24.3 µg/L	24.3 ppb	18:47:53
3	SiO2†	1980.5	661.1	72.973 µg/L	72.973 ppb	18:47:53
3	Si 251.611†	-1826.1	-2736.2	-44.905 µg/L	-44.905 ppb	18:47:53
3	Sn 189.927†	110.7	122.9	8.8298 µg/L	8.8298 ppb	18:47:53
3	Sr 421.552†	4811.0	5449.9	8.9869 µg/L	8.9869 ppb	18:47:23
3	Ti 334.940†	25226.4	27818.7	-4.5924 µg/L	-4.5924 ppb	18:47:51
3	Tl 190.801†	-184.7	-88.0	-11.070 µg/L	-11.070 ppb	18:47:53
3	U 409.014†	216613.9	244816.6	15048 µg/L	15048 ppb	18:47:51
3	V 292.402†	10498.6	11410.5	0.4086 µg/L	0.4086 ppb	18:47:53
3	Zn 213.857†	7725.4	8249.7	7.5805 µg/L	7.5805 ppb	18:47:53

Mean Data: LR1

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1477662.9	88.336 %	0.2752			0.31%
Sc RADIAL	135685.8	93.1 %	0.52			0.56%
Y 371.029	891878.7	87.218 %	0.2568			0.29%
Ag 328.068†	88.4	4.5932 µg/L	0.62588	4.5932 ppb	0.62588	13.63%
Al 396.153Radial†	2346350.2	512180 µg/L	3688.5	512180 ppb	3688.5	0.72%
QC value within limits for Al 396.153Radial Recovery = 102.44%						
As 188.979†	-227.4	6.6405 µg/L	21.57070	6.6405 ppb	21.57070	324.83%
B 249.677†	866.1	14.495 µg/L	1.5153	14.495 ppb	1.5153	10.45%
Ba 233.527†	720.9	-2.4848 µg/L	0.24586	-2.4848 ppb	0.24586	9.89%
Be 313.107†	-14491.1	-0.1375 µg/L	0.09171	-0.1375 ppb	0.09171	66.68%
Ca 317.933Radial†	8177430.7	479160 µg/L	4179.3	479160 ppb	4179.3	0.87%
QC value within limits for Ca 317.933Radial Recovery = 95.83%						
Cd 226.502†	6440.6	-3.1895 µg/L	1.17255	-3.1895 ppb	1.17255	36.76%
Co 228.616†	943.0	-10.730 µg/L	1.2103	-10.730 ppb	1.2103	11.28%
Cr 267.716†	793.5	4.8113 µg/L	1.04230	4.8113 ppb	1.04230	21.66%
Cu 324.752†	-22188.5	-5.0079 µg/L	1.15199	-5.0079 ppb	1.15199	23.00%
Fe 238.204 Radial†	6817792.7	453270 µg/L	4009.8	453270 ppb	4009.8	0.88%
QC value within limits for Fe 238.204 Radial Recovery = 90.65%						
K 766.490 Radial†	678.0	-44.408 µg/L	36.1609	-44.408 ppb	36.1609	81.43%

Mg 279.077 IEC†	1158908.9	477440 µg/L	4979.6	477440 ppb	4979.6	1.04%
QC value within limits for Mg 279.077 IEC Recovery = 95.49%						
Mn 257.610†	16935.9	3.0063 µg/L	0.22334	3.0063 ppb	0.22334	7.43%
Mo 202.031†	-931.3	-2.7244 µg/L	0.57668	-2.7244 ppb	0.57668	21.17%
Na 589.592 Radial†	3316135.7	507410 µg/L	4467.6	507410 ppb	4467.6	0.88%
QC value within limits for Na 589.592 Radial Recovery = 101.48%						
Ni 231.604†	355.3	4.5450 µg/L	0.81388	4.5450 ppb	0.81388	17.91%
P 214.914†	854.3	11.169 µg/L	24.3729	11.169 ppb	24.3729	218.22%
Pb 220.353†	-82.7	0.8056 µg/L	7.37729	0.8056 ppb	7.37729	915.80%
S 181.975 Axial†	108.6	87.742 µg/L	15.9697	87.742 ppb	15.9697	18.20%
Sb 206.836†	42.7	-3.7822 µg/L	8.06989	-3.7822 ppb	8.06989	213.36%
Se 196.026†	-387.3	18.7 µg/L	30.84	18.7 ppb	30.84	165.04%
SiO2†	567.2	62.747 µg/L	9.5648	62.747 ppb	9.5648	15.24%
Si 251.611†	-2995.6	-49.176 µg/L	3.9567	-49.176 ppb	3.9567	8.05%
Sn 189.927†	78.3	5.6629 µg/L	2.80476	5.6629 ppb	2.80476	49.53%
Sr 421.552†	5442.4	9.0050 µg/L	0.01831	9.0050 ppb	0.01831	0.20%
Ti 334.940†	27960.1	-4.1181 µg/L	0.44268	-4.1181 ppb	0.44268	10.75%
Tl 190.801†	-151.5	-19.582 µg/L	8.3859	-19.582 ppb	8.3859	42.82%
U 409.014†	245173.6	15071 µg/L	23.1	15071 ppb	23.1	0.15%
QC value within limits for U 409.014 Recovery = 100.47%						
V 292.402†	11601.2	2.1827 µg/L	1.57124	2.1827 ppb	1.57124	71.99%
Zn 213.857†	8387.2	8.8934 µg/L	1.18890	8.8934 ppb	1.18890	13.37%
All analyte(s) passed QC.						

Sequence No.: 12

Sample ID: LR2

Analyst:

Logged In Analyst (Original) : optima4

Initial Sample Wt:

Dilution:

Autosampler Location: 108

Date Collected: 3/29/2010 18:48:01

Data Type: Reprocessed on 3/29/2010 19:14:40

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: LR2

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc 361.383	1698380.4	1698380.4	101.53 %		18:49:13
1	Sc RADIAL	151205.1	151205.1	104 %		18:48:34
1	Y 371.029	1017103.0	1017103.0	99.464 %		18:49:13
1	Ag 328.068†	-18686.1	-21371.4	31.131 µg/L	31.131 ppb	18:49:15
1	Al 396.153Radial†	2338.4	2286.0	66.356 µg/L	66.356 ppb	18:48:36
1	As 188.979†	24060.3	23711.8	10160 µg/L	10160 ppb	18:49:15
1	B 249.677†	302290.6	294377.4	4910.3 µg/L	4910.3 ppb	18:49:13
1	Ba 233.527†	3091920.0	3045479.3	13922 µg/L	13922 ppb	18:49:13
1	Be 313.107†	8967503.4	8832963.6	2875.2 µg/L	2875.2 ppb	18:49:09
1	Ca 317.933Radial†	1386.8	720.6	42.226 µg/L	42.226 ppb	18:48:36
1	Cd 226.502†	1391850.4	1370960.3	9471.5 µg/L	9471.5 ppb	18:49:13
1	Co 228.616†	680530.5	670447.0	9197.3 µg/L	9197.3 ppb	18:49:13
1	Cr 267.716†	2796482.2	2754160.4	23659 µg/L	23659 ppb	18:49:13
1	Cu 324.752†	4652514.4	4579945.2	19914 µg/L	19914 ppb	18:49:13
1	Fe 238.204 Radial†	-1093.2	-1167.1	-77.594 µg/L	-77.594 ppb	18:48:36
1	K 766.490 Radial†	735082.9	707128.4	291110 µg/L	291110 ppb	18:48:34
1	Mg 279.077 IEC†	-573.2	-739.2	-76.817 µg/L	-76.817 ppb	18:48:36
1	Mn 257.610†	6850554.7	6747191.3	9219.6 µg/L	9219.6 ppb	18:49:13
1	Mo 202.031†	299568.0	295106.7	9318.7 µg/L	9318.7 ppb	18:49:15
1	Na 589.592 Radial†	4106.1	2263.3	87.417 µg/L	87.417 ppb	18:48:36
1	Ni 231.604†	759020.4	747617.8	9562.9 µg/L	9562.9 ppb	18:49:13
1	P 214.914†	61793.1	60781.8	14324 µg/L	14324 ppb	18:49:15
1	Pb 220.353†	385088.4	379170.1	22997 µg/L	22997 ppb	18:49:13
1	S 181.975 Axial†	62300.3	61266.2	49715 µg/L	49715 ppb	18:49:15
1	Sb 206.836†	72365.8	71188.1	9412.3 µg/L	9412.3 ppb	18:49:15
1	Se 196.026†	23983.3	23610.8	9340 µg/L	9340 ppb	18:49:15
1	SiO2†	927224.5	911672.2	99243 µg/L	99243 ppb	18:49:13
1	Si 251.611†	2845330.8	2801756.4	46140 µg/L	46140 ppb	18:49:13
1	Sn 189.927†	135952.5	133900.7	9552.3 µg/L	9552.3 ppb	18:49:15
1	Sr 421.552†	4291141.6	4136725.5	9695.4 µg/L	9695.4 ppb	18:48:32
1	Ti 334.940†	9795412.6	9647094.3	9829.2 µg/L	9829.2 ppb	18:49:09
1	Tl 190.801†	68839.1	67921.6	9266.8 µg/L	9266.8 ppb	18:49:15
1	U 409.014†	-6352.9	-5778.0	247.84 µg/L	247.84 ppb	18:49:15
1	V 292.402†	1822287.8	1794382.0	10142 µg/L	10142 ppb	18:49:13
1	Zn 213.857†	2271454.5	2236744.1	14006 µg/L	14006 ppb	18:49:13
2	Sc 361.383	1692355.1	1692355.1	101.17 %		18:49:22
2	Sc RADIAL	148148.5	148148.5	102 %		18:48:40
2	Y 371.029	1013670.4	1013670.4	99.129 %		18:49:22
2	Ag 328.068†	-18902.0	-21650.3	30.241 µg/L	30.241 ppb	18:49:25
2	Al 396.153Radial†	2166.1	2162.9	32.480 µg/L	32.480 ppb	18:48:43
2	As 188.979†	24382.8	24114.9	10329 µg/L	10329 ppb	18:49:25
2	B 249.677†	301947.2	295098.0	4922.4 µg/L	4922.4 ppb	18:49:22
2	Ba 233.527†	3087006.8	3051465.1	13949 µg/L	13949 ppb	18:49:22
2	Be 313.107†	8888938.4	8786753.2	2860.1 µg/L	2860.1 ppb	18:49:19
2	Ca 317.933Radial†	1193.0	557.5	32.668 µg/L	32.668 ppb	18:48:43
2	Cd 226.502†	1387271.1	1371314.7	9474.0 µg/L	9474.0 ppb	18:49:22
2	Co 228.616†	679503.2	671817.9	9216.1 µg/L	9216.1 ppb	18:49:22
2	Cr 267.716†	2791317.7	2758861.8	23700 µg/L	23700 ppb	18:49:22
2	Cu 324.752†	4645173.2	4589003.5	19954 µg/L	19954 ppb	18:49:22
2	Fe 238.204 Radial†	-1141.0	-1235.9	-82.165 µg/L	-82.165 ppb	18:48:43
2	K 766.490 Radial†	723724.6	710573.4	292530 µg/L	292530 ppb	18:48:40
2	Mg 279.077 IEC†	-594.9	-771.9	-86.616 µg/L	-86.616 ppb	18:48:43
2	Mn 257.610†	6838819.1	6759613.7	9236.6 µg/L	9236.6 ppb	18:49:22
2	Mo 202.031†	303352.5	299897.9	9470.0 µg/L	9470.0 ppb	18:49:25
2	Na 589.592 Radial†	3886.9	2129.3	65.648 µg/L	65.648 ppb	18:48:43
2	Ni 231.604†	757365.3	748643.5	9576.0 µg/L	9576.0 ppb	18:49:22
2	P 214.914†	62941.1	62133.3	14647 µg/L	14647 ppb	18:49:25
2	Pb 220.353†	383628.9	379077.8	22992 µg/L	22992 ppb	18:49:22

2	S 181.975 Axial†	63093.2	62268.3	50529 µg/L	50529 ppb	18:49:25
2	Sb 206.836†	73391.6	72455.9	9585.2 µg/L	9585.2 ppb	18:49:25
2	Se 196.026†	24264.9	23973.2	9480 µg/L	9480 ppb	18:49:25
2	SiO2†	925612.2	913330.0	99418 µg/L	99418 ppb	18:49:22
2	Si 251.611†	2841383.2	2807831.9	46237 µg/L	46237 ppb	18:49:22
2	Sn 189.927†	137626.2	136031.8	9703.7 µg/L	9703.7 ppb	18:49:25
2	Sr 421.552†	4251704.3	4183270.4	9804.5 µg/L	9804.5 ppb	18:48:38
2	Ti 334.940†	9732958.3	9619711.2	9801.3 µg/L	9801.3 ppb	18:49:19
2	Tl 190.801†	69796.1	69108.9	9426.0 µg/L	9426.0 ppb	18:49:25
2	U 409.014†	-6518.6	-5964.1	237.63 µg/L	237.63 ppb	18:49:25
2	V 292.402†	1819682.2	1798196.6	10165 µg/L	10165 ppb	18:49:22
2	Zn 213.857†	2265596.7	2238919.2	14019 µg/L	14019 ppb	18:49:22
3	Sc 361.383	1700875.8	1700875.8	101.68 %		18:49:32
3	Sc RADIAL	149241.8	149241.8	102 %		18:48:47
3	Y 371.029	1018743.4	1018743.4	99.625 %		18:49:32
3	Ag 328.068†	-19043.0	-21695.4	29.614 µg/L	29.614 ppb	18:49:34
3	Al 396.153Radial†	2183.6	2164.5	34.118 µg/L	34.118 ppb	18:48:49
3	As 188.979†	24384.9	23996.2	10278 µg/L	10278 ppb	18:49:34
3	B 249.677†	302272.0	293922.3	4902.7 µg/L	4902.7 ppb	18:49:32
3	Ba 233.527†	3092416.4	3041499.6	13904 µg/L	13904 ppb	18:49:32
3	Be 313.107†	8907241.5	8760739.0	2851.7 µg/L	2851.7 ppb	18:49:28
3	Ca 317.933Radial†	1218.9	574.2	33.647 µg/L	33.647 ppb	18:48:49
3	Cd 226.502†	1391102.2	1368213.3	9452.5 µg/L	9452.5 ppb	18:49:32
3	Co 228.616†	681435.9	670354.0	9196.0 µg/L	9196.0 ppb	18:49:32
3	Cr 267.716†	2794875.2	2748538.9	23611 µg/L	23611 ppb	18:49:32
3	Cu 324.752†	4650199.8	4570945.8	19875 µg/L	19875 ppb	18:49:32
3	Fe 238.204 Radial†	-1251.6	-1335.7	-88.800 µg/L	-88.800 ppb	18:48:49
3	K 766.490 Radial†	729684.2	711177.7	292780 µg/L	292780 ppb	18:48:47
3	Mg 279.077 IEC†	-664.5	-835.6	-113.55 µg/L	-113.55 ppb	18:48:49
3	Mn 257.610†	6850008.1	6736754.4	9205.4 µg/L	9205.4 ppb	18:49:32
3	Mo 202.031†	303976.8	299009.8	9441.9 µg/L	9441.9 ppb	18:49:34
3	Na 589.592 Radial†	3504.7	1728.1	4.0327 µg/L	4.0327 ppb	18:48:49
3	Ni 231.604†	758972.5	746473.9	9548.3 µg/L	9548.3 ppb	18:49:32
3	P 214.914†	62994.4	61874.1	14586 µg/L	14586 ppb	18:49:34
3	Pb 220.353†	384992.3	378519.2	22958 µg/L	22958 ppb	18:49:32
3	S 181.975 Axial†	63225.2	62085.8	50381 µg/L	50381 ppb	18:49:34
3	Sb 206.836†	73461.5	72161.1	9546.2 µg/L	9546.2 ppb	18:49:34
3	Se 196.026†	24345.1	23931.9	9470 µg/L	9470 ppb	18:49:34
3	SiO2†	927967.0	911062.6	99172 µg/L	99172 ppb	18:49:32
3	Si 251.611†	2848954.5	2801208.6	46128 µg/L	46128 ppb	18:49:32
3	Sn 189.927†	137708.4	135431.2	9660.9 µg/L	9660.9 ppb	18:49:34
3	Sr 421.552†	4283363.5	4183546.2	9805.1 µg/L	9805.1 ppb	18:48:45
3	Ti 334.940†	9739101.8	9577559.1	9758.3 µg/L	9758.3 ppb	18:49:28
3	Tl 190.801†	69743.1	68711.1	9371.9 µg/L	9371.9 ppb	18:49:34
3	U 409.014†	-6372.0	-5787.7	246.22 µg/L	246.22 ppb	18:49:34
3	V 292.402†	1821804.8	1791273.7	10126 µg/L	10126 ppb	18:49:32
3	Zn 213.857†	2271404.4	2233412.6	13985 µg/L	13985 ppb	18:49:32

Mean Data: LR2

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1697203.7	101.46 %	0.262			0.26%
Sc RADIAL	149531.8	103 %	1.1			1.04%
Y 371.029	1016505.6	99.406 %	0.2532			0.25%
Ag 328.068†	-21572.4	30.328 µg/L	0.7622	30.328 ppb	0.7622	2.51%
Al 396.153Radial†	2204.5	44.318 µg/L	19.1029	44.318 ppb	19.1029	43.10%
As 188.979†	23941.0	10256 µg/L	86.9	10256 ppb	86.9	0.85%
QC value within limits for As 188.979 Recovery = 102.56%						
B 249.677†	294465.9	4911.8 µg/L	9.92	4911.8 ppb	9.92	0.20%
QC value within limits for B 249.677 Recovery = 98.24%						
Ba 233.527†	3046148.0	13925 µg/L	22.9	13925 ppb	22.9	0.16%
QC value within limits for Ba 233.527 Recovery = 92.83%						
Be 313.107†	8793485.2	2862.3 µg/L	11.91	2862.3 ppb	11.91	0.42%
QC value within limits for Be 313.107 Recovery = 95.41%						
Ca 317.933Radial†	617.5	36.181 µg/L	5.2587	36.181 ppb	5.2587	14.53%
Cd 226.502†	1370162.8	9466.0 µg/L	11.73	9466.0 ppb	11.73	0.12%
QC value within limits for Cd 226.502 Recovery = 94.66%						
Co 228.616†	670873.0	9203.1 µg/L	11.25	9203.1 ppb	11.25	0.12%
QC value within limits for Co 228.616 Recovery = 92.03%						
Cr 267.716†	2753853.7	23657 µg/L	44.4	23657 ppb	44.4	0.19%

QC value within limits for Cr 267.716 Recovery = 94.63%							
Cu 324.752†	4579964.8	19914 µg/L	39.3	19914 ppb	39.3	0.20%	
QC value within limits for Cu 324.752 Recovery = 99.57%							
Fe 238.204 Radial†	-1246.2	-82.853 µg/L	5.6347	-82.853 ppb	5.6347	6.80%	
K 766.490 Radial†	709626.5	292140 µg/L	899.3	292140 ppb	899.3	0.31%	
QC value within limits for K 766.490 Radial Recovery = 97.38%							
Mg 279.077 IEC†	-782.2	-92.329 µg/L	19.0229	-92.329 ppb	19.0229	20.60%	
Mn 257.610†	6747853.1	9220.5 µg/L	15.64	9220.5 ppb	15.64	0.17%	
QC value within limits for Mn 257.610 Recovery = 92.21%							
Mo 202.031†	298004.8	9410.2 µg/L	80.46	9410.2 ppb	80.46	0.86%	
QC value within limits for Mo 202.031 Recovery = 94.10%							
Na 589.592 Radial†	2040.3	52.366 µg/L	43.2497	52.366 ppb	43.2497	82.59%	
Ni 231.604†	747578.4	9562.4 µg/L	13.88	9562.4 ppb	13.88	0.15%	
QC value within limits for Ni 231.604 Recovery = 95.62%							
P 214.914†	61596.4	14519 µg/L	171.5	14519 ppb	171.5	1.18%	
QC value within limits for P 214.914 Recovery = 96.79%							
Pb 220.353†	378922.4	22983 µg/L	21.3	22983 ppb	21.3	0.09%	
QC value within limits for Pb 220.353 Recovery = 91.93%							
S 181.975 Axial†	61873.4	50208 µg/L	433.1	50208 ppb	433.1	0.86%	
QC value within limits for S 181.975 Axial Recovery = 100.42%							
Sb 206.836†	71935.0	9514.6 µg/L	90.66	9514.6 ppb	90.66	0.95%	
QC value within limits for Sb 206.836 Recovery = 95.15%							
Se 196.026†	23838.7	9430 µg/L	78.5	9430 ppb	78.5	0.83%	
QC value within limits for Se 196.026 Recovery = 94.29%							
SiO2†	912021.6	99278 µg/L	126.7	99278 ppb	126.7	0.13%	
QC value within limits for SiO2 Recovery = 92.78%							
Si 251.611†	2803599.0	46168 µg/L	59.8	46168 ppb	59.8	0.13%	
QC value within limits for Si 251.611 Recovery = 92.34%							
Sn 189.927†	135121.2	9639.0 µg/L	78.05	9639.0 ppb	78.05	0.81%	
QC value within limits for Sn 189.927 Recovery = 96.39%							
Sr 421.552†	4167847.3	9768.3 µg/L	63.17	9768.3 ppb	63.17	0.65%	
QC value within limits for Sr 421.552 Recovery = 97.68%							
Ti 334.940†	9614788.2	9796.3 µg/L	35.71	9796.3 ppb	35.71	0.36%	
QC value within limits for Ti 334.940 Recovery = 97.96%							
Tl 190.801†	68580.5	9354.9 µg/L	80.95	9354.9 ppb	80.95	0.87%	
QC value within limits for Tl 190.801 Recovery = 93.55%							
U 409.014†	-5843.2	243.90 µg/L	5.490	243.90 ppb	5.490	2.25%	
V 292.402†	1794617.4	10145 µg/L	19.6	10145 ppb	19.6	0.19%	
QC value within limits for V 292.402 Recovery = 101.45%							
Zn 213.857†	2236358.7	14003 µg/L	17.3	14003 ppb	17.3	0.12%	
QC value within limits for Zn 213.857 Recovery = 93.36%							
All analyte(s) passed QC.							

Sequence No.: 13

Sample ID: CCV

Analyst:

Logged In Analyst (Original) : optima4

Initial Sample Wt:

Dilution:

Autosampler Location: 7

Date Collected: 3/29/2010 18:49:43

Data Type: Reprocessed on 3/29/2010 19:14:41

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCV

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc 361.383	1716469.7	1716469.7	102.61 %		18:50:43
1	Sc RADIAL	154139.7	154139.7	106 %		18:50:16
1	Y 371.029	1044074.8	1044074.8	102.10 %		18:50:43
1	Ag 328.068†	127602.5	121387.1	498.79 µg/L	498.79 ppb	18:50:43
1	Al 396.153Radial†	24715.7	23403.0	5085.7 µg/L	5085.7 ppb	18:50:16
1	As 188.979†	1226.4	1209.4	512.57 µg/L	512.57 ppb	18:51:03
1	B 249.677†	33333.5	29129.3	487.34 µg/L	487.34 ppb	18:50:43
1	Ba 233.527†	111436.2	108774.4	497.32 µg/L	497.32 ppb	18:50:43
1	Be 313.107†	1573483.9	1534088.7	499.51 µg/L	499.51 ppb	18:50:43
1	Ca 317.933Radial†	90206.4	84682.8	4962.0 µg/L	4962.0 ppb	18:50:16
1	Cd 226.502†	72401.2	70652.6	487.60 µg/L	487.60 ppb	18:50:43
1	Co 228.616†	36477.3	35725.3	489.45 µg/L	489.45 ppb	18:50:43
1	Cr 267.716†	59006.8	57344.5	492.41 µg/L	492.41 ppb	18:50:43
1	Cu 324.752†	119200.3	113741.0	495.97 µg/L	495.97 ppb	18:50:43
1	Fe 238.204 Radial†	78399.3	74021.0	4921.2 µg/L	4921.2 ppb	18:50:16
1	K 766.490 Radial†	15543.8	13243.2	5447.9 µg/L	5447.9 ppb	18:50:16
1	Mg 279.077 IEC†	13152.3	12250.1	5058.7 µg/L	5058.7 ppb	18:50:16
1	Mn 257.610†	370669.7	361153.8	493.28 µg/L	493.28 ppb	18:50:43
1	Mo 202.031†	15969.2	15617.9	493.45 µg/L	493.45 ppb	18:51:03
1	Na 589.592 Radial†	70596.7	65061.3	9950.4 µg/L	9950.4 ppb	18:50:16
1	Ni 231.604†	39349.5	38388.8	491.04 µg/L	491.04 ppb	18:50:43
1	P 214.914†	10515.6	10168.3	2426.7 µg/L	2426.7 ppb	18:51:03
1	Pb 220.353†	8561.1	8230.7	500.15 µg/L	500.15 ppb	18:51:03
1	S 181.975 Axial†	1372.2	1242.5	1010.8 µg/L	1010.8 ppb	18:51:03
1	Sb 206.836†	3825.6	3641.6	492.37 µg/L	492.37 ppb	18:51:03
1	Se 196.026†	1275.8	1232.4	490 µg/L	490 ppb	18:51:03
1	SiO2†	51362.9	48482.5	5278.0 µg/L	5278.0 ppb	18:50:43
1	Si 251.611†	154098.4	149499.2	2462.1 µg/L	2462.1 ppb	18:50:43
1	Sn 189.927†	7147.3	6963.3	496.69 µg/L	496.69 ppb	18:51:03
1	Sr 421.552†	225096.8	213129.1	499.48 µg/L	499.48 ppb	18:50:14
1	Ti 334.940†	496998.7	483710.6	492.59 µg/L	492.59 ppb	18:50:43
1	Tl 190.801†	3658.8	3685.9	502.16 µg/L	502.16 ppb	18:51:03
1	U 409.014†	7304.5	7597.6	499.58 µg/L	499.58 ppb	18:50:43
1	V 292.402†	91666.3	88901.0	499.43 µg/L	499.43 ppb	18:50:43
1	Zn 213.857†	80718.2	78199.0	488.38 µg/L	488.38 ppb	18:50:43
2	Sc 361.383	1735506.8	1735506.8	103.75 %		18:51:06
2	Sc RADIAL	152000.4	152000.4	104 %		18:50:20
2	Y 371.029	1054226.6	1054226.6	103.09 %		18:51:06
2	Ag 328.068†	129107.7	121473.9	499.12 µg/L	499.12 ppb	18:51:06
2	Al 396.153Radial†	24426.5	23454.6	5097.3 µg/L	5097.3 ppb	18:50:20
2	As 188.979†	1211.7	1182.2	501.18 µg/L	501.18 ppb	18:51:26
2	B 249.677†	33876.9	29296.7	490.15 µg/L	490.15 ppb	18:51:06
2	Ba 233.527†	112976.1	109067.5	498.66 µg/L	498.66 ppb	18:51:06
2	Be 313.107†	1597015.9	1539949.6	501.42 µg/L	501.42 ppb	18:51:06
2	Ca 317.933Radial†	89516.0	85221.3	4993.6 µg/L	4993.6 ppb	18:50:20
2	Cd 226.502†	73594.6	71028.9	490.19 µg/L	490.19 ppb	18:51:06
2	Co 228.616†	37103.5	35939.0	492.37 µg/L	492.37 ppb	18:51:06
2	Cr 267.716†	59788.6	57467.2	493.47 µg/L	493.47 ppb	18:51:06
2	Cu 324.752†	121059.6	114258.9	498.22 µg/L	498.22 ppb	18:51:06
2	Fe 238.204 Radial†	77655.1	74350.7	4943.1 µg/L	4943.1 ppb	18:50:20
2	K 766.490 Radial†	15260.2	13178.1	5421.1 µg/L	5421.1 ppb	18:50:20
2	Mg 279.077 IEC†	13002.7	12281.7	5071.5 µg/L	5071.5 ppb	18:50:20
2	Mn 257.610†	375944.4	362275.4	494.81 µg/L	494.81 ppb	18:51:06
2	Mo 202.031†	15890.3	15371.2	485.66 µg/L	485.66 ppb	18:51:26
2	Na 589.592 Radial†	70215.3	65635.2	10038 µg/L	10038 ppb	18:50:20
2	Ni 231.604†	40047.6	38641.0	494.26 µg/L	494.26 ppb	18:51:06
2	P 214.914†	10471.7	10013.6	2389.6 µg/L	2389.6 ppb	18:51:26
2	Pb 220.353†	8484.3	8065.2	490.12 µg/L	490.12 ppb	18:51:26

2	S 181.975 Axial†	1365.8	1221.6	993.82 µg/L	993.82 ppb	18:51:26
2	Sb 206.836†	3834.3	3609.1	487.85 µg/L	487.85 ppb	18:51:26
2	Se 196.026†	1280.6	1223.4	486 µg/L	486 ppb	18:51:26
2	SiO2†	52085.9	48630.3	5294.5 µg/L	5294.5 ppb	18:51:06
2	Si 251.611†	156279.7	149954.3	2469.8 µg/L	2469.8 ppb	18:51:06
2	Sn 189.927†	7113.5	6854.4	488.96 µg/L	488.96 ppb	18:51:26
2	Sr 421.552†	226242.9	217223.8	509.08 µg/L	509.08 ppb	18:50:18
2	Ti 334.940†	504866.7	485981.2	494.91 µg/L	494.91 ppb	18:51:06
2	Tl 190.801†	3631.8	3620.9	493.44 µg/L	493.44 ppb	18:51:26
2	U 409.014†	7123.0	7344.6	483.95 µg/L	483.95 ppb	18:51:06
2	V 292.402†	92685.9	88903.8	499.36 µg/L	499.36 ppb	18:51:06
2	Zn 213.857†	81781.8	78361.2	489.37 µg/L	489.37 ppb	18:51:06
3	Sc 361.383	1735485.3	1735485.3	103.75 %		18:51:29
3	Sc RADIAL	153403.0	153403.0	105 %		18:50:24
3	Y 371.029	1055021.0	1055021.0	103.17 %		18:51:29
3	Ag 328.068†	128496.4	120886.2	496.73 µg/L	496.73 ppb	18:51:29
3	Al 396.153Radial†	24553.1	23360.7	5076.8 µg/L	5076.8 ppb	18:50:24
3	As 188.979†	1228.3	1198.2	507.85 µg/L	507.85 ppb	18:51:49
3	B 249.677†	33764.7	29188.9	488.34 µg/L	488.34 ppb	18:51:29
3	Ba 233.527†	112730.4	108832.0	497.58 µg/L	497.58 ppb	18:51:29
3	Be 313.107†	1593609.1	1536684.9	500.35 µg/L	500.35 ppb	18:51:29
3	Ca 317.933Radial†	90597.1	85463.7	5007.8 µg/L	5007.8 ppb	18:50:24
3	Cd 226.502†	73406.3	70848.2	488.94 µg/L	488.94 ppb	18:51:29
3	Co 228.616†	37011.7	35850.9	491.16 µg/L	491.16 ppb	18:51:29
3	Cr 267.716†	59666.8	57350.6	492.47 µg/L	492.47 ppb	18:51:29
3	Cu 324.752†	120307.7	113535.5	495.08 µg/L	495.08 ppb	18:51:29
3	Fe 238.204 Radial†	78518.4	74490.1	4952.4 µg/L	4952.4 ppb	18:50:24
3	K 766.490 Radial†	15451.9	13226.5	5441.0 µg/L	5441.0 ppb	18:50:24
3	Mg 279.077 IEC†	13189.3	12345.0	5097.6 µg/L	5097.6 ppb	18:50:24
3	Mn 257.610†	374488.1	360876.2	492.90 µg/L	492.90 ppb	18:51:29
3	Mo 202.031†	15929.3	15408.9	486.85 µg/L	486.85 ppb	18:51:49
3	Na 589.592 Radial†	70596.2	65381.5	9999.4 µg/L	9999.4 ppb	18:50:24
3	Ni 231.604†	39740.3	38345.2	490.48 µg/L	490.48 ppb	18:51:29
3	P 214.914†	10488.7	10030.1	2393.6 µg/L	2393.6 ppb	18:51:49
3	Pb 220.353†	8512.5	8092.5	491.77 µg/L	491.77 ppb	18:51:49
3	S 181.975 Axial†	1342.5	1199.2	975.68 µg/L	975.68 ppb	18:51:49
3	Sb 206.836†	3856.9	3630.9	490.82 µg/L	490.82 ppb	18:51:49
3	Se 196.026†	1283.1	1225.8	487 µg/L	487 ppb	18:51:49
3	SiO2†	51906.7	48458.3	5275.6 µg/L	5275.6 ppb	18:51:29
3	Si 251.611†	155757.0	149452.4	2461.5 µg/L	2461.5 ppb	18:51:29
3	Sn 189.927†	7131.5	6871.8	490.19 µg/L	490.19 ppb	18:51:49
3	Sr 421.552†	223596.8	212726.1	498.53 µg/L	498.53 ppb	18:50:22
3	Ti 334.940†	502794.3	483989.7	492.88 µg/L	492.88 ppb	18:51:29
3	Tl 190.801†	3635.4	3624.3	493.87 µg/L	493.87 ppb	18:51:49
3	U 409.014†	7197.3	7416.4	488.32 µg/L	488.32 ppb	18:51:29
3	V 292.402†	92498.4	88724.2	498.37 µg/L	498.37 ppb	18:51:29
3	Zn 213.857†	81445.8	78038.4	487.36 µg/L	487.36 ppb	18:51:29

Mean Data: CCV

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1729154.0	103.37 %	0.657			0.64%
Sc RADIAL	153181.0	105 %	0.7			0.71%
Y 371.029	1051107.5	102.79 %	0.597			0.58%
Ag 328.068†	121249.1	498.21 µg/L	1.295	498.21 ppb	1.295	0.26%
QC value within limits for Ag 328.068 Recovery = 99.64%						
Al 396.153Radial†	23406.1	5086.6 µg/L	10.30	5086.6 ppb	10.30	0.20%
QC value within limits for Al 396.153Radial Recovery = 101.73%						
As 188.979†	1196.6	507.20 µg/L	5.724	507.20 ppb	5.724	1.13%
QC value within limits for As 188.979 Recovery = 101.44%						
B 249.677†	29205.0	488.61 µg/L	1.419	488.61 ppb	1.419	0.29%
QC value within limits for B 249.677 Recovery = 97.72%						
Ba 233.527†	108891.3	497.85 µg/L	0.708	497.85 ppb	0.708	0.14%
QC value within limits for Ba 233.527 Recovery = 99.57%						
Be 313.107†	1536907.7	500.43 µg/L	0.954	500.43 ppb	0.954	0.19%
QC value within limits for Be 313.107 Recovery = 100.09%						
Ca 317.933Radial†	85122.6	4987.8 µg/L	23.42	4987.8 ppb	23.42	0.47%
QC value within limits for Ca 317.933Radial Recovery = 99.76%						
Cd 226.502†	70843.2	488.91 µg/L	1.299	488.91 ppb	1.299	0.27%
QC value within limits for Cd 226.502 Recovery = 97.78%						

Co 228.616†	35838.4	490.99 µg/L	1.470	490.99 ppb	1.470	0.30%
QC value within limits for Co 228.616 Recovery = 98.20%						
Cr 267.716†	57387.4	492.78 µg/L	0.599	492.78 ppb	0.599	0.12%
QC value within limits for Cr 267.716 Recovery = 98.56%						
Cu 324.752†	113845.1	496.42 µg/L	1.617	496.42 ppb	1.617	0.33%
QC value within limits for Cu 324.752 Recovery = 99.28%						
Fe 238.204 Radial†	74287.3	4938.9 µg/L	16.02	4938.9 ppb	16.02	0.32%
QC value within limits for Fe 238.204 Radial Recovery = 98.78%						
K 766.490 Radial†	13215.9	5436.6 µg/L	13.92	5436.6 ppb	13.92	0.26%
QC value within limits for K 766.490 Radial Recovery = 108.73%						
Mg 279.077 IEC†	12292.3	5076.0 µg/L	19.85	5076.0 ppb	19.85	0.39%
QC value within limits for Mg 279.077 IEC Recovery = 101.52%						
Mn 257.610†	361435.1	493.67 µg/L	1.013	493.67 ppb	1.013	0.21%
QC value within limits for Mn 257.610 Recovery = 98.73%						
Mo 202.031†	15466.0	488.65 µg/L	4.194	488.65 ppb	4.194	0.86%
QC value within limits for Mo 202.031 Recovery = 97.73%						
Na 589.592 Radial†	65359.4	9996.0 µg/L	44.02	9996.0 ppb	44.02	0.44%
QC value within limits for Na 589.592 Radial Recovery = 99.96%						
Ni 231.604†	38458.3	491.93 µg/L	2.043	491.93 ppb	2.043	0.42%
QC value within limits for Ni 231.604 Recovery = 98.39%						
P 214.914†	10070.7	2403.3 µg/L	20.35	2403.3 ppb	20.35	0.85%
QC value within limits for P 214.914 Recovery = 96.13%						
Pb 220.353†	8129.5	494.02 µg/L	5.379	494.02 ppb	5.379	1.09%
QC value within limits for Pb 220.353 Recovery = 98.80%						
S 181.975 Axial†	1221.1	993.43 µg/L	17.559	993.43 ppb	17.559	1.77%
QC value within limits for S 181.975 Axial Recovery = 99.34%						
Sb 206.836†	3627.2	490.35 µg/L	2.300	490.35 ppb	2.300	0.47%
QC value within limits for Sb 206.836 Recovery = 98.07%						
Se 196.026†	1227.2	488 µg/L	1.8	488 ppb	1.8	0.38%
QC value within limits for Se 196.026 Recovery = 97.52%						
SiO2†	48523.7	5282.7 µg/L	10.27	5282.7 ppb	10.27	0.19%
QC value within limits for SiO2 Recovery = 98.79%						
Si 251.611†	149635.3	2464.5 µg/L	4.63	2464.5 ppb	4.63	0.19%
QC value within limits for Si 251.611 Recovery = 98.58%						
Sn 189.927†	6896.5	491.95 µg/L	4.158	491.95 ppb	4.158	0.85%
QC value within limits for Sn 189.927 Recovery = 98.39%						
Sr 421.552†	214359.7	502.36 µg/L	5.833	502.36 ppb	5.833	1.16%
QC value within limits for Sr 421.552 Recovery = 100.47%						
Ti 334.940†	484560.5	493.46 µg/L	1.265	493.46 ppb	1.265	0.26%
QC value within limits for Ti 334.940 Recovery = 98.69%						
Tl 190.801†	3643.7	496.49 µg/L	4.915	496.49 ppb	4.915	0.99%
QC value within limits for Tl 190.801 Recovery = 99.30%						
U 409.014†	7452.9	490.62 µg/L	8.063	490.62 ppb	8.063	1.64%
QC value within limits for U 409.014 Recovery = 98.12%						
V 292.402†	88843.0	499.05 µg/L	0.592	499.05 ppb	0.592	0.12%
QC value within limits for V 292.402 Recovery = 99.81%						
Zn 213.857†	78199.5	488.37 µg/L	1.004	488.37 ppb	1.004	0.21%
QC value within limits for Zn 213.857 Recovery = 97.67%						
All analyte(s) passed QC.						

Sequence No.: 14

Sample ID: CCB

Analyst:

Logged In Analyst (Original) : optima4

Initial Sample Wt:

Dilution:

Autosampler Location: 8

Date Collected: 3/29/2010 18:51:58

Data Type: Reprocessed on 3/29/2010 19:14:42

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCB

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc 361.383	1728897.1	1728897.1	103.36 %		18:53:35
1	Sc RADIAL	154974.9	154974.9	106 %		18:52:27
1	Y 371.029	1063835.8	1063835.8	104.03 %		18:53:35
1	Ag 328.068†	3134.9	66.1	0.2939 µg/L	0.2939 ppb	18:53:37
1	Al 396.153Radial†	-26.1	7.3	1.5617 µg/L	1.5617 ppb	18:52:47
1	As 188.979†	-6.1	8.3	3.4794 µg/L	3.4794 ppb	18:53:57
1	B 249.677†	3279.3	-182.9	-3.0715 µg/L	-3.0715 ppb	18:53:57
1	Ba 233.527†	-172.5	8.1	0.0372 µg/L	0.0372 ppb	18:53:57
1	Be 313.107†	-265.8	402.9	0.1379 µg/L	0.1379 ppb	18:53:37
1	Ca 317.933Radial†	701.7	43.7	2.5615 µg/L	2.5615 ppb	18:52:47
1	Cd 226.502†	-78.0	18.9	0.1302 µg/L	0.1302 ppb	18:53:57
1	Co 228.616†	-150.4	31.1	0.4253 µg/L	0.4253 ppb	18:53:57
1	Cr 267.716†	165.7	0.1	-0.0163 µg/L	-0.0163 ppb	18:53:57
1	Cu 324.752†	2708.5	195.7	0.8692 µg/L	0.8692 ppb	18:53:37
1	Fe 238.204 Radial†	162.5	39.6	2.6306 µg/L	2.6306 ppb	18:52:47
1	K 766.490 Radial†	1937.4	367.1	151.11 µg/L	151.11 ppb	18:52:27
1	Mg 279.077 IEC†	162.4	-33.9	-13.972 µg/L	-13.972 ppb	18:52:47
1	Mn 257.610†	174.4	88.7	0.1218 µg/L	0.1218 ppb	18:53:57
1	Mo 202.031†	-30.8	25.4	0.8010 µg/L	0.8010 ppb	18:53:57
1	Na 589.592 Radial†	2342.1	508.0	77.603 µg/L	77.603 ppb	18:52:27
1	Ni 231.604†	-58.4	-15.6	-0.1996 µg/L	-0.1996 ppb	18:53:57
1	P 214.914†	71.2	-10.7	-2.5700 µg/L	-2.5700 ppb	18:53:57
1	Pb 220.353†	154.2	36.7	2.2095 µg/L	2.2095 ppb	18:53:57
1	S 181.975 Axial†	101.6	3.4	2.7893 µg/L	2.7893 ppb	18:53:57
1	Sb 206.836†	90.3	0.8	0.1164 µg/L	0.1164 ppb	18:53:57
1	Se 196.026†	18.0	6.5	2.59 µg/L	2.59 ppb	18:53:57
1	SiO2†	1694.9	67.0	7.2702 µg/L	7.2702 ppb	18:53:57
1	Si 251.611†	856.4	152.3	2.4932 µg/L	2.4932 ppb	18:53:57
1	Sn 189.927†	32.2	29.2	2.0730 µg/L	2.0730 ppb	18:53:57
1	Sr 421.552†	-130.0	155.7	0.3650 µg/L	0.3650 ppb	18:52:27
1	Ti 334.940†	561.4	-93.1	-0.1029 µg/L	-0.1029 ppb	18:53:37
1	Tl 190.801†	-112.5	11.5	1.5393 µg/L	1.5393 ppb	18:53:57
1	U 409.014†	-122.5	360.6	22.274 µg/L	22.274 ppb	18:53:37
1	V 292.402†	422.0	-23.5	-0.1074 µg/L	-0.1074 ppb	18:53:37
1	Zn 213.857†	665.5	179.5	1.1304 µg/L	1.1304 ppb	18:53:57
2	Sc 361.383	1739415.6	1739415.6	103.98 %		18:53:59
2	Sc RADIAL	153949.0	153949.0	106 %		18:52:49
2	Y 371.029	1070599.7	1070599.7	104.70 %		18:53:59
2	Ag 328.068†	3011.7	-70.7	-0.2648 µg/L	-0.2648 ppb	18:54:01
2	Al 396.153Radial†	-22.1	11.0	2.3766 µg/L	2.3766 ppb	18:53:09
2	As 188.979†	-13.6	1.2	0.4948 µg/L	0.4948 ppb	18:54:21
2	B 249.677†	3226.1	-253.2	-4.2510 µg/L	-4.2510 ppb	18:54:21
2	Ba 233.527†	-183.8	-1.7	-0.0082 µg/L	-0.0082 ppb	18:54:21
2	Be 313.107†	-497.9	181.3	0.0661 µg/L	0.0661 ppb	18:54:01
2	Ca 317.933Radial†	683.5	30.9	1.8113 µg/L	1.8113 ppb	18:53:09
2	Cd 226.502†	-81.2	16.3	0.1120 µg/L	0.1120 ppb	18:54:21
2	Co 228.616†	-169.3	13.8	0.1886 µg/L	0.1886 ppb	18:54:21
2	Cr 267.716†	203.3	35.3	0.2845 µg/L	0.2845 ppb	18:54:21
2	Cu 324.752†	2932.9	395.7	1.7397 µg/L	1.7397 ppb	18:54:01
2	Fe 238.204 Radial†	156.9	35.2	2.3419 µg/L	2.3419 ppb	18:53:09
2	K 766.490 Radial†	1851.5	297.9	122.64 µg/L	122.64 ppb	18:52:49
2	Mg 279.077 IEC†	181.3	-15.0	-6.1810 µg/L	-6.1810 ppb	18:53:09
2	Mn 257.610†	185.1	98.0	0.1342 µg/L	0.1342 ppb	18:54:21
2	Mo 202.031†	-40.6	16.1	0.5093 µg/L	0.5093 ppb	18:54:21
2	Na 589.592 Radial†	2203.5	391.5	59.792 µg/L	59.792 ppb	18:52:49
2	Ni 231.604†	-87.1	-42.9	-0.5483 µg/L	-0.5483 ppb	18:54:21
2	P 214.914†	70.7	-11.6	-2.7920 µg/L	-2.7920 ppb	18:54:21
2	Pb 220.353†	120.5	3.4	0.1904 µg/L	0.1904 ppb	18:54:21

2	S 181.975 Axial†	93.2	-5.2	-4.2193 µg/L	-4.2193 ppb	18:54:21
2	Sb 206.836†	93.2	3.0	0.4017 µg/L	0.4017 ppb	18:54:21
2	Se 196.026†	16.5	5.0	1.99 µg/L	1.99 ppb	18:54:21
2	SiO2†	1661.9	25.3	2.7424 µg/L	2.7424 ppb	18:54:21
2	Si 251.611†	798.6	91.6	1.5029 µg/L	1.5029 ppb	18:54:21
2	Sn 189.927†	13.9	11.4	0.8082 µg/L	0.8082 ppb	18:54:21
2	Sr 421.552†	-162.3	124.3	0.2914 µg/L	0.2914 ppb	18:52:49
2	Ti 334.940†	589.0	-69.9	-0.0804 µg/L	-0.0804 ppb	18:54:01
2	Tl 190.801†	-123.3	1.7	0.2267 µg/L	0.2267 ppb	18:54:21
2	U 409.014†	-105.6	377.6	23.300 µg/L	23.300 ppb	18:54:01
2	V 292.402†	344.7	-100.3	-0.5347 µg/L	-0.5347 ppb	18:54:01
2	Zn 213.857†	642.6	153.6	0.9689 µg/L	0.9689 ppb	18:54:21
3	Sc 361.383	1736015.7	1736015.7	103.78 %		18:54:23
3	Sc RADIAL	153754.9	153754.9	105 %		18:53:11
3	Y 371.029	1068282.8	1068282.8	104.47 %		18:54:23
3	Ag 328.068†	2964.9	-110.2	-0.4509 µg/L	-0.4509 ppb	18:54:26
3	Al 396.153Radial†	-16.1	16.6	3.5986 µg/L	3.5986 ppb	18:53:31
3	As 188.979†	-20.3	-5.3	-2.2272 µg/L	-2.2272 ppb	18:54:46
3	B 249.677†	3208.4	-264.2	-4.4364 µg/L	-4.4364 ppb	18:54:46
3	Ba 233.527†	-175.6	5.8	0.0262 µg/L	0.0262 ppb	18:54:46
3	Be 313.107†	-146.9	518.6	0.1704 µg/L	0.1704 ppb	18:54:26
3	Ca 317.933Radial†	709.7	56.6	3.3147 µg/L	3.3147 ppb	18:53:31
3	Cd 226.502†	-66.7	30.1	0.2078 µg/L	0.2078 ppb	18:54:46
3	Co 228.616†	-149.7	32.3	0.4424 µg/L	0.4424 ppb	18:54:46
3	Cr 267.716†	183.5	16.6	0.1380 µg/L	0.1380 ppb	18:54:46
3	Cu 324.752†	2785.8	259.4	1.1323 µg/L	1.1323 ppb	18:54:26
3	Fe 238.204 Radial†	167.4	45.4	3.0195 µg/L	3.0195 ppb	18:53:31
3	K 766.490 Radial†	2004.9	445.6	183.43 µg/L	183.43 ppb	18:53:11
3	Mg 279.077 IEC†	164.0	-31.2	-12.871 µg/L	-12.871 ppb	18:53:31
3	Mn 257.610†	141.8	56.6	0.0779 µg/L	0.0779 ppb	18:54:46
3	Mo 202.031†	-43.5	13.3	0.4189 µg/L	0.4189 ppb	18:54:46
3	Na 589.592 Radial†	2025.0	224.9	34.251 µg/L	34.251 ppb	18:53:11
3	Ni 231.604†	-54.8	-11.9	-0.1527 µg/L	-0.1527 ppb	18:54:46
3	P 214.914†	63.8	-18.1	-4.3341 µg/L	-4.3341 ppb	18:54:46
3	Pb 220.353†	149.8	31.9	1.9285 µg/L	1.9285 ppb	18:54:46
3	S 181.975 Axial†	104.0	5.4	4.3655 µg/L	4.3655 ppb	18:54:46
3	Sb 206.836†	91.0	1.1	0.1457 µg/L	0.1457 ppb	18:54:46
3	Se 196.026†	19.4	7.7	3.06 µg/L	3.06 ppb	18:54:46
3	SiO2†	1644.1	11.4	1.2195 µg/L	1.2195 ppb	18:54:46
3	Si 251.611†	797.5	92.1	1.5112 µg/L	1.5112 ppb	18:54:46
3	Sn 189.927†	13.8	11.3	0.8038 µg/L	0.8038 ppb	18:54:46
3	Sr 421.552†	-194.0	94.1	0.2206 µg/L	0.2206 ppb	18:53:11
3	Ti 334.940†	849.4	182.1	0.1846 µg/L	0.1846 ppb	18:54:26
3	Tl 190.801†	-118.6	6.0	0.7978 µg/L	0.7978 ppb	18:54:46
3	U 409.014†	-409.0	85.0	5.2024 µg/L	5.2024 ppb	18:54:26
3	V 292.402†	290.0	-152.4	-0.8373 µg/L	-0.8373 ppb	18:54:26
3	Zn 213.857†	615.7	128.9	0.8114 µg/L	0.8114 ppb	18:54:46

Mean Data: CCB

Analyte	Mean Corrected Intensity	Conc. Units	Calib.	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1734776.2	103.71 %		0.321			0.31%
Sc RADIAL	154226.3	106 %		0.4			0.43%
Y 371.029	1067572.8	104.40 %		0.336			0.32%
Ag 328.068†	-38.3	-0.1406 µg/L		0.38763	-0.1406 ppb	0.38763	275.71%
QC value within limits for Ag 328.068 Recovery = Not calculated							
Al 396.153Radial†	11.6	2.5123 µg/L		1.02521	2.5123 ppb	1.02521	40.81%
QC value within limits for Al 396.153Radial Recovery = Not calculated							
As 188.979†	1.4	0.5823 µg/L		2.85430	0.5823 ppb	2.85430	490.14%
QC value within limits for As 188.979 Recovery = Not calculated							
B 249.677†	-233.4	-3.9196 µg/L		0.74029	-3.9196 ppb	0.74029	18.89%
QC value within limits for B 249.677 Recovery = Not calculated							
Ba 233.527†	4.1	0.0184 µg/L		0.02367	0.0184 ppb	0.02367	128.49%
QC value within limits for Ba 233.527 Recovery = Not calculated							
Be 313.107†	367.6	0.1248 µg/L		0.05339	0.1248 ppb	0.05339	42.78%
QC value within limits for Be 313.107 Recovery = Not calculated							
Ca 317.933Radial†	43.7	2.5625 µg/L		0.75170	2.5625 ppb	0.75170	29.33%
QC value within limits for Ca 317.933Radial Recovery = Not calculated							
Cd 226.502†	21.8	0.1500 µg/L		0.05085	0.1500 ppb	0.05085	33.90%
QC value within limits for Cd 226.502 Recovery = Not calculated							

Co 228.616†	25.7	0.3521 µg/L	0.14188	0.3521 ppb	0.14188	40.30%
QC value within limits for Co 228.616 Recovery = Not calculated						
Cr 267.716†	17.3	0.1354 µg/L	0.15041	0.1354 ppb	0.15041	111.10%
QC value within limits for Cr 267.716 Recovery = Not calculated						
Cu 324.752†	283.6	1.2471 µg/L	0.44643	1.2471 ppb	0.44643	35.80%
QC value within limits for Cu 324.752 Recovery = Not calculated						
Fe 238.204 Radial†	40.1	2.6640 µg/L	0.34002	2.6640 ppb	0.34002	12.76%
QC value within limits for Fe 238.204 Radial Recovery = Not calculated						
K 766.490 Radial†	370.2	152.39 µg/L	30.414	152.39 ppb	30.414	19.96%
QC value greater than the upper limit for K 766.490 Radial Recovery = Not calculated						
Mg 279.077 IEC†	-26.7	-11.008 µg/L	4.2166	-11.008 ppb	4.2166	38.30%
QC value within limits for Mg 279.077 IEC Recovery = Not calculated						
Mn 257.610†	81.1	0.1113 µg/L	0.02959	0.1113 ppb	0.02959	26.59%
QC value within limits for Mn 257.610 Recovery = Not calculated						
Mo 202.031†	18.3	0.5764 µg/L	0.19971	0.5764 ppb	0.19971	34.65%
QC value within limits for Mo 202.031 Recovery = Not calculated						
Na 589.592 Radial†	374.8	57.216 µg/L	21.7906	57.216 ppb	21.7906	38.09%
QC value within limits for Na 589.592 Radial Recovery = Not calculated						
Ni 231.604†	-23.5	-0.3002 µg/L	0.21614	-0.3002 ppb	0.21614	72.00%
QC value within limits for Ni 231.604 Recovery = Not calculated						
P 214.914†	-13.5	-3.2320 µg/L	0.96088	-3.2320 ppb	0.96088	29.73%
QC value within limits for P 214.914 Recovery = Not calculated						
Pb 220.353†	24.0	1.4428 µg/L	1.09369	1.4428 ppb	1.09369	75.80%
QC value within limits for Pb 220.353 Recovery = Not calculated						
S 181.975 Axial†	1.2	0.9785 µg/L	4.56987	0.9785 ppb	4.56987	467.04%
QC value within limits for S 181.975 Axial Recovery = Not calculated						
Sb 206.836†	1.6	0.2213 µg/L	0.15695	0.2213 ppb	0.15695	70.93%
QC value within limits for Sb 206.836 Recovery = Not calculated						
Se 196.026†	6.4	2.55 µg/L	0.537	2.55 ppb	0.537	21.07%
QC value within limits for Se 196.026 Recovery = Not calculated						
SiO2†	34.6	3.7440 µg/L	3.14725	3.7440 ppb	3.14725	84.06%
QC value within limits for SiO2 Recovery = Not calculated						
Si 251.611†	112.0	1.8358 µg/L	0.56935	1.8358 ppb	0.56935	31.01%
QC value within limits for Si 251.611 Recovery = Not calculated						
Sn 189.927†	17.3	1.2284 µg/L	0.73152	1.2284 ppb	0.73152	59.55%
QC value within limits for Sn 189.927 Recovery = Not calculated						
Sr 421.552†	124.7	0.2923 µg/L	0.07221	0.2923 ppb	0.07221	24.70%
QC value within limits for Sr 421.552 Recovery = Not calculated						
Ti 334.940†	6.3	0.0004 µg/L	0.15987	0.0004 ppb	0.15987	>999.9%
QC value within limits for Ti 334.940 Recovery = Not calculated						
Tl 190.801†	6.4	0.8546 µg/L	0.65815	0.8546 ppb	0.65815	77.01%
QC value within limits for Tl 190.801 Recovery = Not calculated						
U 409.014†	274.4	16.925 µg/L	10.1653	16.925 ppb	10.1653	60.06%
QC value within limits for U 409.014 Recovery = Not calculated						
V 292.402†	-92.1	-0.4931 µg/L	0.36672	-0.4931 ppb	0.36672	74.37%
QC value within limits for V 292.402 Recovery = Not calculated						
Zn 213.857†	154.0	0.9702 µg/L	0.15951	0.9702 ppb	0.15951	16.44%
QC value within limits for Zn 213.857 Recovery = Not calculated						
QC Failed. Continue with analysis.						

Sequence No.: 15

Sample ID: CCV

Analyst:

Logged In Analyst (Original) : optima4

Initial Sample Wt:

Dilution:

Autosampler Location: 7

Date Collected: 3/29/2010 18:57:39

Data Type: Reprocessed on 3/29/2010 19:14:43

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCV

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc 361.383	1742170.7	1742170.7	104.15 %		18:58:39
1	Sc RADIAL	154515.3	154515.3	106 %		18:58:11
1	Y 371.029	1059060.1	1059060.1	103.57 %		18:58:39
1	Ag 328.068†	129322.6	121204.2	498.05 µg/L	498.05 ppb	18:58:39
1	Al 396.153Radial†	24823.0	23447.4	5095.8 µg/L	5095.8 ppb	18:58:11
1	As 188.979†	1217.4	1183.1	501.56 µg/L	501.56 ppb	18:58:59
1	B 249.677†	33548.3	28856.2	482.76 µg/L	482.76 ppb	18:58:39
1	Ba 233.527†	113126.0	108794.9	497.41 µg/L	497.41 ppb	18:58:39
1	Be 313.107†	1604803.7	1541539.3	501.94 µg/L	501.94 ppb	18:58:39
1	Ca 317.933Radial†	90245.5	84512.4	4952.1 µg/L	4952.1 ppb	18:58:11
1	Cd 226.502†	73575.0	70738.7	488.19 µg/L	488.19 ppb	18:58:39
1	Co 228.616†	37114.9	35813.1	490.65 µg/L	490.65 ppb	18:58:39
1	Cr 267.716†	59986.2	57436.6	493.20 µg/L	493.20 ppb	18:58:39
1	Cu 324.752†	120959.5	113716.5	495.86 µg/L	495.86 ppb	18:58:39
1	Fe 238.204 Radial†	78194.0	73647.1	4896.3 µg/L	4896.3 ppb	18:58:11
1	K 766.490 Radial†	14176.6	11917.8	4902.2 µg/L	4902.2 ppb	18:58:11
1	Mg 279.077 IEC†	13187.4	12253.0	5059.7 µg/L	5059.7 ppb	18:58:11
1	Mn 257.610†	376145.4	361082.3	493.18 µg/L	493.18 ppb	18:58:39
1	Mo 202.031†	15919.4	15340.5	484.69 µg/L	484.69 ppb	18:58:59
1	Na 589.592 Radial†	70146.9	64474.8	9861.1 µg/L	9861.1 ppb	18:58:11
1	Ni 231.604†	39988.6	38436.6	491.65 µg/L	491.65 ppb	18:58:39
1	P 214.914†	10512.2	10013.9	2389.7 µg/L	2389.7 ppb	18:58:59
1	Pb 220.353†	8436.4	7988.0	485.43 µg/L	485.43 ppb	18:58:59
1	S 181.975 Axial†	1318.2	1170.9	952.74 µg/L	952.74 ppb	18:58:59
1	Sb 206.836†	3856.6	3616.3	488.81 µg/L	488.81 ppb	18:58:59
1	Se 196.026†	1269.9	1208.4	480 µg/L	480 ppb	18:58:59
1	SiO2†	51891.1	48251.3	5253.1 µg/L	5253.1 ppb	18:58:39
1	Si 251.611†	155814.4	148931.5	2452.9 µg/L	2452.9 ppb	18:58:39
1	Sn 189.927†	7088.8	6804.4	485.40 µg/L	485.40 ppb	18:58:59
1	Sr 421.552†	226055.0	213515.6	500.39 µg/L	500.39 ppb	18:58:09
1	Ti 334.940†	505203.6	484443.4	493.34 µg/L	493.34 ppb	18:58:39
1	Tl 190.801†	3627.2	3603.0	491.03 µg/L	491.03 ppb	18:58:59
1	U 409.014†	7391.3	7576.0	498.27 µg/L	498.27 ppb	18:58:39
1	V 292.402†	93133.5	88991.9	499.85 µg/L	499.85 ppb	18:58:39
1	Zn 213.857†	81243.9	77543.3	484.25 µg/L	484.25 ppb	18:58:39
2	Sc 361.383	1731918.8	1731918.8	103.54 %		18:59:02
2	Sc RADIAL	153334.6	153334.6	105 %		18:58:15
2	Y 371.029	1053099.9	1053099.9	102.98 %		18:59:02
2	Ag 328.068†	128679.2	121317.8	498.52 µg/L	498.52 ppb	18:59:02
2	Al 396.153Radial†	24533.3	23352.3	5074.9 µg/L	5074.9 ppb	18:58:15
2	As 188.979†	1225.6	1198.0	507.75 µg/L	507.75 ppb	18:59:22
2	B 249.677†	33340.5	28846.3	482.59 µg/L	482.59 ppb	18:59:02
2	Ba 233.527†	112441.8	108777.0	497.33 µg/L	497.33 ppb	18:59:02
2	Be 313.107†	1592364.8	1538646.2	501.00 µg/L	501.00 ppb	18:59:02
2	Ca 317.933Radial†	89792.3	84737.0	4965.2 µg/L	4965.2 ppb	18:58:15
2	Cd 226.502†	73051.4	70651.1	487.59 µg/L	487.59 ppb	18:59:02
2	Co 228.616†	36781.7	35702.2	489.13 µg/L	489.13 ppb	18:59:02
2	Cr 267.716†	59502.2	57310.0	492.11 µg/L	492.11 ppb	18:59:02
2	Cu 324.752†	119947.4	113426.4	494.60 µg/L	494.60 ppb	18:59:02
2	Fe 238.204 Radial†	77968.6	74000.8	4919.8 µg/L	4919.8 ppb	18:58:15
2	K 766.490 Radial†	14058.0	11908.0	4898.2 µg/L	4898.2 ppb	18:58:15
2	Mg 279.077 IEC†	13036.1	12205.0	5039.9 µg/L	5039.9 ppb	18:58:15
2	Mn 257.610†	373427.3	360594.9	492.52 µg/L	492.52 ppb	18:59:02
2	Mo 202.031†	15910.1	15421.9	487.26 µg/L	487.26 ppb	18:59:22
2	Na 589.592 Radial†	69792.3	64647.2	9887.5 µg/L	9887.5 ppb	18:58:15
2	Ni 231.604†	39642.4	38329.5	490.28 µg/L	490.28 ppb	18:59:02
2	P 214.914†	10490.2	10052.4	2398.9 µg/L	2398.9 ppb	18:59:22
2	Pb 220.353†	8461.2	8059.8	489.79 µg/L	489.79 ppb	18:59:22

2	S 181.975 Axial†	1332.4	1192.1	969.89 µg/L	969.89 ppb	18:59:22
2	Sb 206.836†	3845.4	3627.4	490.36 µg/L	490.36 ppb	18:59:22
2	Se 196.026†	1281.0	1226.3	487 µg/L	487 ppb	18:59:22
2	SiO2†	51762.5	48422.0	5271.6 µg/L	5271.6 ppb	18:59:02
2	Si 251.611†	154651.7	148694.0	2448.9 µg/L	2448.9 ppb	18:59:02
2	Sn 189.927†	7107.0	6862.3	489.51 µg/L	489.51 ppb	18:59:22
2	Sr 421.552†	226773.0	215840.0	505.83 µg/L	505.83 ppb	18:58:13
2	Ti 334.940†	500715.6	482980.0	491.85 µg/L	491.85 ppb	18:59:02
2	Tl 190.801†	3643.2	3639.1	495.88 µg/L	495.88 ppb	18:59:22
2	U 409.014†	7329.7	7558.5	497.20 µg/L	497.20 ppb	18:59:02
2	V 292.402†	92631.5	89036.3	500.12 µg/L	500.12 ppb	18:59:02
2	Zn 213.857†	80666.5	77447.4	483.65 µg/L	483.65 ppb	18:59:02
3	Sc 361.383	1731636.7	1731636.7	103.52 %		18:59:25
3	Sc RADIAL	154205.4	154205.4	106 %		18:58:20
3	Y 371.029	1052626.8	1052626.8	102.94 %		18:59:25
3	Ag 328.068†	128532.9	121196.7	498.02 µg/L	498.02 ppb	18:59:25
3	Al 396.153Radial†	24950.8	23615.3	5132.4 µg/L	5132.4 ppb	18:58:20
3	As 188.979†	1233.7	1206.0	511.11 µg/L	511.11 ppb	18:59:45
3	B 249.677†	33475.9	28982.3	484.88 µg/L	484.88 ppb	18:59:25
3	Ba 233.527†	112293.7	108651.6	496.76 µg/L	496.76 ppb	18:59:25
3	Be 313.107†	1590952.1	1537532.1	500.63 µg/L	500.63 ppb	18:59:25
3	Ca 317.933Radial†	90838.5	85244.0	4994.9 µg/L	4994.9 ppb	18:58:20
3	Cd 226.502†	73036.3	70648.1	487.56 µg/L	487.56 ppb	18:59:25
3	Co 228.616†	36829.8	35754.4	489.84 µg/L	489.84 ppb	18:59:25
3	Cr 267.716†	59440.0	57259.2	491.68 µg/L	491.68 ppb	18:59:25
3	Cu 324.752†	119916.0	113414.9	494.56 µg/L	494.56 ppb	18:59:25
3	Fe 238.204 Radial†	78885.0	74448.4	4949.6 µg/L	4949.6 ppb	18:58:20
3	K 766.490 Radial†	14076.3	11849.9	4874.3 µg/L	4874.3 ppb	18:58:20
3	Mg 279.077 IEC†	13322.3	12405.5	5122.6 µg/L	5122.6 ppb	18:58:20
3	Mn 257.610†	373424.5	360651.0	492.59 µg/L	492.59 ppb	18:59:25
3	Mo 202.031†	15880.4	15395.8	486.44 µg/L	486.44 ppb	18:59:45
3	Na 589.592 Radial†	70305.8	64758.0	9904.5 µg/L	9904.5 ppb	18:58:20
3	Ni 231.604†	39803.4	38491.3	492.35 µg/L	492.35 ppb	18:59:25
3	P 214.914†	10482.3	10046.4	2397.5 µg/L	2397.5 ppb	18:59:45
3	Pb 220.353†	8408.9	8010.6	486.81 µg/L	486.81 ppb	18:59:45
3	S 181.975 Axial†	1326.3	1186.4	965.31 µg/L	965.31 ppb	18:59:45
3	Sb 206.836†	3839.9	3622.7	489.73 µg/L	489.73 ppb	18:59:45
3	Se 196.026†	1268.7	1214.6	483 µg/L	483 ppb	18:59:45
3	SiO2†	51614.7	48287.3	5257.0 µg/L	5257.0 ppb	18:59:25
3	Si 251.611†	154566.1	148635.7	2448.0 µg/L	2448.0 ppb	18:59:25
3	Sn 189.927†	7092.3	6849.2	488.58 µg/L	488.58 ppb	18:59:45
3	Sr 421.552†	224060.1	212058.6	496.97 µg/L	496.97 ppb	18:58:17
3	Ti 334.940†	500694.3	483038.2	491.90 µg/L	491.90 ppb	18:59:25
3	Tl 190.801†	3646.3	3642.7	496.35 µg/L	496.35 ppb	18:59:45
3	U 409.014†	7327.6	7557.6	497.15 µg/L	497.15 ppb	18:59:25
3	V 292.402†	92621.5	89041.2	500.13 µg/L	500.13 ppb	18:59:25
3	Zn 213.857†	80736.0	77527.2	484.14 µg/L	484.14 ppb	18:59:25

Mean Data: CCV

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1735242.1	103.73 %	0.359			0.35%
Sc RADIAL	154018.4	106 %	0.4			0.40%
Y 371.029	1054928.9	103.16 %	0.351			0.34%
Ag 328.068†	121239.6	498.20 µg/L	0.276	498.20 ppb	0.276	0.06%
QC value within limits for Ag 328.068 Recovery = 99.64%						
Al 396.153Radial†	23471.7	5101.0 µg/L	29.08	5101.0 ppb	29.08	0.57%
QC value within limits for Al 396.153Radial Recovery = 102.02%						
As 188.979†	1195.7	506.81 µg/L	4.846	506.81 ppb	4.846	0.96%
QC value within limits for As 188.979 Recovery = 101.36%						
B 249.677†	28895.0	483.41 µg/L	1.273	483.41 ppb	1.273	0.26%
QC value within limits for B 249.677 Recovery = 96.68%						
Ba 233.527†	108741.2	497.17 µg/L	0.357	497.17 ppb	0.357	0.07%
QC value within limits for Ba 233.527 Recovery = 99.43%						
Be 313.107†	1539239.2	501.19 µg/L	0.673	501.19 ppb	0.673	0.13%
QC value within limits for Be 313.107 Recovery = 100.24%						
Ca 317.933Radial†	84831.1	4970.7 µg/L	21.96	4970.7 ppb	21.96	0.44%
QC value within limits for Ca 317.933Radial Recovery = 99.41%						
Cd 226.502†	70679.3	487.78 µg/L	0.358	487.78 ppb	0.358	0.07%
QC value within limits for Cd 226.502 Recovery = 97.56%						

Co 228.616†	35756.6	489.87 µg/L	0.760	489.87 ppb	0.760	0.16%
QC value within limits for Co 228.616 Recovery = 97.97%						
Cr 267.716†	57335.3	492.33 µg/L	0.783	492.33 ppb	0.783	0.16%
QC value within limits for Cr 267.716 Recovery = 98.47%						
Cu 324.752†	113519.3	495.01 µg/L	0.740	495.01 ppb	0.740	0.15%
QC value within limits for Cu 324.752 Recovery = 99.00%						
Fe 238.204 Radial†	74032.1	4921.9 µg/L	26.70	4921.9 ppb	26.70	0.54%
QC value within limits for Fe 238.204 Radial Recovery = 98.44%						
K 766.490 Radial†	11891.9	4891.6 µg/L	15.12	4891.6 ppb	15.12	0.31%
QC value within limits for K 766.490 Radial Recovery = 97.83%						
Mg 279.077 IEC†	12287.8	5074.1 µg/L	43.14	5074.1 ppb	43.14	0.85%
QC value within limits for Mg 279.077 IEC Recovery = 101.48%						
Mn 257.610†	360776.1	492.77 µg/L	0.365	492.77 ppb	0.365	0.07%
QC value within limits for Mn 257.610 Recovery = 98.55%						
Mo 202.031†	15386.1	486.13 µg/L	1.313	486.13 ppb	1.313	0.27%
QC value within limits for Mo 202.031 Recovery = 97.23%						
Na 589.592 Radial†	64626.7	9884.4 µg/L	21.84	9884.4 ppb	21.84	0.22%
QC value within limits for Na 589.592 Radial Recovery = 98.84%						
Ni 231.604†	38419.1	491.43 µg/L	1.053	491.43 ppb	1.053	0.21%
QC value within limits for Ni 231.604 Recovery = 98.29%						
P 214.914†	10037.5	2395.4 µg/L	4.95	2395.4 ppb	4.95	0.21%
QC value within limits for P 214.914 Recovery = 95.81%						
Pb 220.353†	8019.5	487.34 µg/L	2.227	487.34 ppb	2.227	0.46%
QC value within limits for Pb 220.353 Recovery = 97.47%						
S 181.975 Axial†	1183.1	962.65 µg/L	8.881	962.65 ppb	8.881	0.92%
QC value within limits for S 181.975 Axial Recovery = 96.26%						
Sb 206.836†	3622.2	489.63 µg/L	0.781	489.63 ppb	0.781	0.16%
QC value within limits for Sb 206.836 Recovery = 97.93%						
Se 196.026†	1216.4	483 µg/L	3.6	483 ppb	3.6	0.75%
QC value within limits for Se 196.026 Recovery = 96.66%						
SiO2†	48320.2	5260.6 µg/L	9.78	5260.6 ppb	9.78	0.19%
QC value within limits for SiO2 Recovery = 98.37%						
Si 251.611†	148753.7	2449.9 µg/L	2.62	2449.9 ppb	2.62	0.11%
QC value within limits for Si 251.611 Recovery = 98.00%						
Sn 189.927†	6838.6	487.83 µg/L	2.157	487.83 ppb	2.157	0.44%
QC value within limits for Sn 189.927 Recovery = 97.57%						
Sr 421.552†	213804.8	501.06 µg/L	4.470	501.06 ppb	4.470	0.89%
QC value within limits for Sr 421.552 Recovery = 100.21%						
Ti 334.940†	483487.2	492.36 µg/L	0.845	492.36 ppb	0.845	0.17%
QC value within limits for Ti 334.940 Recovery = 98.47%						
Tl 190.801†	3628.3	494.42 µg/L	2.943	494.42 ppb	2.943	0.60%
QC value within limits for Tl 190.801 Recovery = 98.88%						
U 409.014†	7564.0	497.54 µg/L	0.636	497.54 ppb	0.636	0.13%
QC value within limits for U 409.014 Recovery = 99.51%						
V 292.402†	89023.2	500.03 µg/L	0.157	500.03 ppb	0.157	0.03%
QC value within limits for V 292.402 Recovery = 100.01%						
Zn 213.857†	77506.0	484.01 µg/L	0.318	484.01 ppb	0.318	0.07%
QC value within limits for Zn 213.857 Recovery = 96.80%						
All analyte(s) passed QC.						

Sequence No.: 16

Sample ID: CCB

Analyst:

Logged In Analyst (Original) : optima4

Initial Sample Wt:

Dilution:

Autosampler Location: 8

Date Collected: 3/29/2010 18:59:54

Data Type: Reprocessed on 3/29/2010 19:14:44

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCB

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc 361.383	1743930.9	1743930.9	104.25 %		19:01:45
1	Sc RADIAL	157207.9	157207.9	108 %		19:00:23
1	Y 371.029	1072817.8	1072817.8	104.91 %		19:01:45
1	Ag 328.068†	2785.5	-295.2	-1.1824 µg/L	-1.1824 ppb	19:01:47
1	Al 396.153Radial†	-35.9	-1.4	-0.3269 µg/L	-0.3269 ppb	19:00:43
1	As 188.979†	-9.7	4.9	2.0592 µg/L	2.0592 ppb	19:02:07
1	B 249.677†	3169.2	-315.8	-5.3028 µg/L	-5.3028 ppb	19:02:07
1	Ba 233.527†	-172.8	9.3	0.0423 µg/L	0.0423 ppb	19:02:07
1	Be 313.107†	-580.2	103.6	0.0392 µg/L	0.0392 ppb	19:01:47
1	Ca 317.933Radial†	703.1	35.6	2.0888 µg/L	2.0888 ppb	19:00:43
1	Cd 226.502†	-117.2	-18.0	-0.1248 µg/L	-0.1248 ppb	19:02:07
1	Co 228.616†	-175.0	8.7	0.1195 µg/L	0.1195 ppb	19:02:07
1	Cr 267.716†	174.7	7.4	0.0489 µg/L	0.0489 ppb	19:02:07
1	Cu 324.752†	2833.3	292.9	1.2883 µg/L	1.2883 ppb	19:01:47
1	Fe 238.204 Radial†	147.5	23.5	1.5605 µg/L	1.5605 ppb	19:00:43
1	K 766.490 Radial†	1652.9	77.5	31.907 µg/L	31.907 ppb	19:00:23
1	Mg 279.077 IEC†	179.9	-19.9	-8.1726 µg/L	-8.1726 ppb	19:00:43
1	Mn 257.610†	174.5	87.4	0.1197 µg/L	0.1197 ppb	19:02:07
1	Mo 202.031†	-38.4	18.4	0.5797 µg/L	0.5797 ppb	19:02:07
1	Na 589.592 Radial†	1931.7	96.3	14.699 µg/L	14.699 ppb	19:00:23
1	Ni 231.604†	-49.3	-6.4	-0.0822 µg/L	-0.0822 ppb	19:02:07
1	P 214.914†	78.3	-4.5	-1.0824 µg/L	-1.0824 ppb	19:02:07
1	Pb 220.353†	116.5	-0.7	-0.0551 µg/L	-0.0551 ppb	19:02:07
1	S 181.975 Axial†	92.5	-6.1	-4.9234 µg/L	-4.9234 ppb	19:02:07
1	Sb 206.836†	87.4	-2.8	-0.3729 µg/L	-0.3729 ppb	19:02:07
1	Se 196.026†	21.5	9.7	3.85 µg/L	3.85 ppb	19:02:07
1	SiO2†	1662.9	22.2	2.3983 µg/L	2.3983 ppb	19:02:07
1	Si 251.611†	781.9	73.6	1.2037 µg/L	1.2037 ppb	19:02:07
1	Sn 189.927†	15.0	12.4	0.8828 µg/L	0.8828 ppb	19:02:07
1	Sr 421.552†	-145.8	142.8	0.3347 µg/L	0.3347 ppb	19:00:23
1	Ti 334.940†	822.4	152.5	0.1487 µg/L	0.1487 ppb	19:01:47
1	Tl 190.801†	-112.5	12.4	1.6651 µg/L	1.6651 ppb	19:02:07
1	U 409.014†	-191.3	295.6	18.231 µg/L	18.231 ppb	19:01:47
1	V 292.402†	340.4	-105.3	-0.5658 µg/L	-0.5658 ppb	19:01:47
1	Zn 213.857†	528.4	42.4	0.2666 µg/L	0.2666 ppb	19:02:07
2	Sc 361.383	1749880.6	1749880.6	104.61 %		19:02:09
2	Sc RADIAL	154607.9	154607.9	106 %		19:00:45
2	Y 371.029	1075429.4	1075429.4	105.17 %		19:02:09
2	Ag 328.068†	2854.9	-238.0	-0.9266 µg/L	-0.9266 ppb	19:02:11
2	Al 396.153Radial†	-53.8	-18.9	-4.1894 µg/L	-4.1894 ppb	19:01:05
2	As 188.979†	-8.5	6.1	2.5641 µg/L	2.5641 ppb	19:02:31
2	B 249.677†	3184.7	-311.3	-5.2277 µg/L	-5.2277 ppb	19:02:31
2	Ba 233.527†	-166.1	16.2	0.0743 µg/L	0.0743 ppb	19:02:31
2	Be 313.107†	-429.5	249.5	0.0921 µg/L	0.0921 ppb	19:02:11
2	Ca 317.933Radial†	674.2	19.4	1.1395 µg/L	1.1395 ppb	19:01:05
2	Cd 226.502†	-92.3	6.1	0.0422 µg/L	0.0422 ppb	19:02:31
2	Co 228.616†	-147.4	35.7	0.4889 µg/L	0.4889 ppb	19:02:31
2	Cr 267.716†	146.6	-20.1	-0.2010 µg/L	-0.2010 ppb	19:02:31
2	Cu 324.752†	2740.1	194.5	0.8753 µg/L	0.8753 ppb	19:02:11
2	Fe 238.204 Radial†	152.9	30.9	2.0532 µg/L	2.0532 ppb	19:01:05
2	K 766.490 Radial†	1696.1	144.0	59.261 µg/L	59.261 ppb	19:00:45
2	Mg 279.077 IEC†	164.9	-31.2	-12.828 µg/L	-12.828 ppb	19:01:05
2	Mn 257.610†	159.3	72.2	0.0992 µg/L	0.0992 ppb	19:02:31
2	Mo 202.031†	-10.4	45.2	1.4272 µg/L	1.4272 ppb	19:02:31
2	Na 589.592 Radial†	1913.7	109.4	16.687 µg/L	16.687 ppb	19:00:45
2	Ni 231.604†	-34.9	7.5	0.0960 µg/L	0.0960 ppb	19:02:31
2	P 214.914†	88.9	5.5	1.2769 µg/L	1.2769 ppb	19:02:31
2	Pb 220.353†	116.9	-0.7	-0.0641 µg/L	-0.0641 ppb	19:02:31

2	S 181.975 Axial†	98.1	-1.0	-0.8273 µg/L	-0.8273 ppb	19:02:31
2	Sb 206.836†	79.8	-10.4	-1.3806 µg/L	-1.3806 ppb	19:02:31
2	Se 196.026†	23.1	11.2	4.46 µg/L	4.46 ppb	19:02:31
2	SiO2†	1662.3	16.2	1.7388 µg/L	1.7388 ppb	19:02:31
2	Si 251.611†	771.7	61.4	0.9975 µg/L	0.9975 ppb	19:02:31
2	Sn 189.927†	-2.4	-4.3	-0.3060 µg/L	-0.3060 ppb	19:02:31
2	Sr 421.552†	-168.4	119.2	0.2795 µg/L	0.2795 ppb	19:00:45
2	Ti 334.940†	843.2	169.7	0.1595 µg/L	0.1595 ppb	19:02:11
2	Tl 190.801†	-115.5	9.9	1.3206 µg/L	1.3206 ppb	19:02:31
2	U 409.014†	109.4	583.7	36.043 µg/L	36.043 ppb	19:02:11
2	V 292.402†	368.0	-80.0	-0.4063 µg/L	-0.4063 ppb	19:02:11
2	Zn 213.857†	532.3	44.4	0.2783 µg/L	0.2783 ppb	19:02:31
3	Sc 361.383	1734424.8	1734424.8	103.69 %		19:02:33
3	Sc RADIAL	152171.1	152171.1	104 %		19:01:07
3	Y 371.029	1067156.7	1067156.7	104.36 %		19:02:33
3	Ag 328.068†	2902.9	-167.4	-0.6806 µg/L	-0.6806 ppb	19:02:36
3	Al 396.153Radial†	-58.9	-24.5	-5.3555 µg/L	-5.3555 ppb	19:01:27
3	As 188.979†	-18.7	-3.8	-1.5762 µg/L	-1.5762 ppb	19:02:56
3	B 249.677†	3166.5	-301.7	-5.0666 µg/L	-5.0666 ppb	19:02:56
3	Ba 233.527†	-187.7	-6.0	-0.0277 µg/L	-0.0277 ppb	19:02:56
3	Be 313.107†	-333.0	339.0	0.1115 µg/L	0.1115 ppb	19:02:36
3	Ca 317.933Radial†	709.2	63.1	3.6954 µg/L	3.6954 ppb	19:01:27
3	Cd 226.502†	-99.5	-1.5	-0.0105 µg/L	-0.0105 ppb	19:02:56
3	Co 228.616†	-170.8	11.9	0.1624 µg/L	0.1624 ppb	19:02:56
3	Cr 267.716†	184.7	17.9	0.1506 µg/L	0.1506 ppb	19:02:56
3	Cu 324.752†	2715.6	194.2	0.8472 µg/L	0.8472 ppb	19:02:36
3	Fe 238.204 Radial†	137.1	18.1	1.2007 µg/L	1.2007 ppb	19:01:27
3	K 766.490 Radial†	1528.8	9.4	3.8507 µg/L	3.8507 ppb	19:01:07
3	Mg 279.077 IEC†	173.3	-20.7	-8.5238 µg/L	-8.5238 ppb	19:01:27
3	Mn 257.610†	141.1	56.1	0.0769 µg/L	0.0769 ppb	19:02:56
3	Mo 202.031†	-52.8	4.2	0.1336 µg/L	0.1336 ppb	19:02:56
3	Na 589.592 Radial†	1839.9	67.6	10.341 µg/L	10.341 ppb	19:01:07
3	Ni 231.604†	-39.3	3.0	0.0386 µg/L	0.0386 ppb	19:02:56
3	P 214.914†	57.3	-24.3	-5.8246 µg/L	-5.8246 ppb	19:02:56
3	Pb 220.353†	120.4	3.6	0.2179 µg/L	0.2179 ppb	19:02:56
3	S 181.975 Axial†	88.1	-9.8	-7.9574 µg/L	-7.9574 ppb	19:02:56
3	Sb 206.836†	87.1	-2.6	-0.3549 µg/L	-0.3549 ppb	19:02:56
3	Se 196.026†	3.8	-7.2	-2.85 µg/L	-2.85 ppb	19:02:56
3	SiO2†	1649.9	18.4	1.9980 µg/L	1.9980 ppb	19:02:56
3	Si 251.611†	767.7	64.1	1.0530 µg/L	1.0530 ppb	19:02:56
3	Sn 189.927†	11.8	9.4	0.6667 µg/L	0.6667 ppb	19:02:56
3	Sr 421.552†	-198.5	87.9	0.2060 µg/L	0.2060 ppb	19:01:07
3	Ti 334.940†	650.8	-8.7	-0.0097 µg/L	-0.0097 ppb	19:02:36
3	Tl 190.801†	-110.3	13.9	1.8642 µg/L	1.8642 ppb	19:02:56
3	U 409.014†	-434.4	60.1	3.6852 µg/L	3.6852 ppb	19:02:36
3	V 292.402†	355.5	-88.9	-0.4890 µg/L	-0.4890 ppb	19:02:36
3	Zn 213.857†	538.0	54.5	0.3420 µg/L	0.3420 ppb	19:02:56

Mean Data: CCB

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1742745.4	104.18 %	0.466			0.45%
Sc RADIAL	154662.3	106 %	1.7			1.63%
Y 371.029	1071801.3	104.81 %	0.414			0.39%
Ag 328.068†	-233.5	-0.9298 µg/L	0.25091	-0.9298 ppb	0.25091	26.98%
QC value within limits for Ag 328.068 Recovery = Not calculated						
Al 396.153Radial†	-14.9	-3.2906 µg/L	2.63203	-3.2906 ppb	2.63203	79.99%
QC value within limits for Al 396.153Radial Recovery = Not calculated						
As 188.979†	2.4	1.0157 µg/L	2.25883	1.0157 ppb	2.25883	222.39%
QC value within limits for As 188.979 Recovery = Not calculated						
B 249.677†	-309.6	-5.1990 µg/L	0.12069	-5.1990 ppb	0.12069	2.32%
QC value within limits for B 249.677 Recovery = Not calculated						
Ba 233.527†	6.5	0.0297 µg/L	0.05216	0.0297 ppb	0.05216	175.89%
QC value within limits for Ba 233.527 Recovery = Not calculated						
Be 313.107†	230.7	0.0809 µg/L	0.03739	0.0809 ppb	0.03739	46.19%
QC value within limits for Be 313.107 Recovery = Not calculated						
Ca 317.933Radial†	39.4	2.3079 µg/L	1.29199	2.3079 ppb	1.29199	55.98%
QC value within limits for Ca 317.933Radial Recovery = Not calculated						
Cd 226.502†	-4.5	-0.0310 µg/L	0.08537	-0.0310 ppb	0.08537	275.14%
QC value within limits for Cd 226.502 Recovery = Not calculated						

Co 228.616†	18.8	0.2569 µg/L	0.20203	0.2569 ppb	0.20203	78.63%
QC value within limits for Co 228.616 Recovery = Not calculated						
Cr 267.716†	1.7	-0.0005 µg/L	0.18092	-0.0005 ppb	0.18092	>999.9%
QC value within limits for Cr 267.716 Recovery = Not calculated						
Cu 324.752†	227.2	1.0036 µg/L	0.24693	1.0036 ppb	0.24693	24.60%
QC value within limits for Cu 324.752 Recovery = Not calculated						
Fe 238.204 Radial†	24.1	1.6048 µg/L	0.42799	1.6048 ppb	0.42799	26.67%
QC value within limits for Fe 238.204 Radial Recovery = Not calculated						
K 766.490 Radial†	76.9	31.673 µg/L	27.7059	31.673 ppb	27.7059	87.48%
QC value within limits for K 766.490 Radial Recovery = Not calculated						
Mg 279.077 IEC†	-23.9	-9.8414 µg/L	2.59218	-9.8414 ppb	2.59218	26.34%
QC value within limits for Mg 279.077 IEC Recovery = Not calculated						
Mn 257.610†	71.9	0.0986 µg/L	0.02141	0.0986 ppb	0.02141	21.70%
QC value within limits for Mn 257.610 Recovery = Not calculated						
Mo 202.031†	22.6	0.7135 µg/L	0.65711	0.7135 ppb	0.65711	92.10%
QC value within limits for Mo 202.031 Recovery = Not calculated						
Na 589.592 Radial†	91.1	13.909 µg/L	3.2461	13.909 ppb	3.2461	23.34%
QC value within limits for Na 589.592 Radial Recovery = Not calculated						
Ni 231.604†	1.4	0.0175 µg/L	0.09096	0.0175 ppb	0.09096	520.03%
QC value within limits for Ni 231.604 Recovery = Not calculated						
P 214.914†	-7.8	-1.8767 µg/L	3.61681	-1.8767 ppb	3.61681	192.72%
QC value within limits for P 214.914 Recovery = Not calculated						
Pb 220.353†	0.8	0.0329 µg/L	0.16029	0.0329 ppb	0.16029	486.83%
QC value within limits for Pb 220.353 Recovery = Not calculated						
S 181.975 Axial†	-5.6	-4.5694 µg/L	3.57820	-4.5694 ppb	3.57820	78.31%
QC value within limits for S 181.975 Axial Recovery = Not calculated						
Sb 206.836†	-5.3	-0.7028 µg/L	0.58704	-0.7028 ppb	0.58704	83.53%
QC value within limits for Sb 206.836 Recovery = Not calculated						
Se 196.026†	4.6	1.82 µg/L	4.054	1.82 ppb	4.054	222.54%
QC value within limits for Se 196.026 Recovery = Not calculated						
SiO2†	19.0	2.0451 µg/L	0.33227	2.0451 ppb	0.33227	16.25%
QC value within limits for SiO2 Recovery = Not calculated						
Si 251.611†	66.3	1.0847 µg/L	0.10673	1.0847 ppb	0.10673	9.84%
QC value within limits for Si 251.611 Recovery = Not calculated						
Sn 189.927†	5.8	0.4145 µg/L	0.63329	0.4145 ppb	0.63329	152.78%
QC value within limits for Sn 189.927 Recovery = Not calculated						
Sr 421.552†	116.6	0.2734 µg/L	0.06458	0.2734 ppb	0.06458	23.62%
QC value within limits for Sr 421.552 Recovery = Not calculated						
Ti 334.940†	104.5	0.0995 µg/L	0.09469	0.0995 ppb	0.09469	95.16%
QC value within limits for Ti 334.940 Recovery = Not calculated						
Tl 190.801†	12.1	1.6167 µg/L	0.27502	1.6167 ppb	0.27502	17.01%
QC value within limits for Tl 190.801 Recovery = Not calculated						
U 409.014†	313.1	19.320 µg/L	16.2065	19.320 ppb	16.2065	83.89%
QC value within limits for U 409.014 Recovery = Not calculated						
V 292.402†	-91.4	-0.4870 µg/L	0.07980	-0.4870 ppb	0.07980	16.39%
QC value within limits for V 292.402 Recovery = Not calculated						
Zn 213.857†	47.1	0.2956 µg/L	0.04054	0.2956 ppb	0.04054	13.71%
QC value within limits for Zn 213.857 Recovery = Not calculated						
All analyte(s) passed QC.						

Sequence No.: 8

Sample ID: CCV

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 7

Date Collected: 3/29/2010 19:31:23

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCV

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	154889.6	154889.6	106 %		19:31:56
1	Al 396.153Radial†	25248.9	23791.6	5171.1 µg/L	5171.1 ppb	19:31:56
1	Ca 317.933Radial†	90787.7	84816.9	4969.9 µg/L	4969.9 ppb	19:31:56
1	Fe 238.204 Radial†	79020.5	74246.6	4936.2 µg/L	4936.2 ppb	19:31:56
1	K 766.490 Radial†	14072.9	11787.9	4848.7 µg/L	4848.7 ppb	19:31:56
1	Mg 279.077 IEC†	13305.1	12333.7	5092.8 µg/L	5092.8 ppb	19:31:56
1	Na 589.592 Radial†	70517.8	64663.9	9890.1 µg/L	9890.1 ppb	19:31:56
1	Sr 421.552†	229051.2	215819.7	505.79 µg/L	505.79 ppb	19:31:54
1	Sc 361.383	1743822.4	1743822.4	104.25 %		19:32:23
1	Y 371.029	1059163.2	1059163.2	103.58 %		19:32:23
1	Ag 328.068†	128580.1	120374.3	494.64 µg/L	494.64 ppb	19:32:23
1	As 188.979†	1249.3	1212.6	513.82 µg/L	513.82 ppb	19:32:43
1	B 249.677†	33313.2	28600.3	478.47 µg/L	478.47 ppb	19:32:23
1	Ba 233.527†	113123.6	108689.7	496.93 µg/L	496.93 ppb	19:32:23
1	Be 313.107†	1610699.9	1545735.8	503.30 µg/L	503.30 ppb	19:32:23
1	Cd 226.502†	72730.5	69861.7	482.13 µg/L	482.13 ppb	19:32:23
1	Co 228.616†	36860.0	35534.8	486.84 µg/L	486.84 ppb	19:32:23
1	Cr 267.716†	59413.7	56832.8	488.02 µg/L	488.02 ppb	19:32:23
1	Cu 324.752†	120074.9	112757.8	491.69 µg/L	491.69 ppb	19:32:23
1	Mn 257.610†	374470.1	359133.2	490.52 µg/L	490.52 ppb	19:32:23
1	Mo 202.031†	15834.2	15244.3	481.66 µg/L	481.66 ppb	19:32:43
1	Ni 231.604†	39808.6	38227.6	488.98 µg/L	488.98 ppb	19:32:23
1	P 214.914†	10378.9	9876.5	2356.8 µg/L	2356.8 ppb	19:32:43
1	Pb 220.353†	8316.1	7864.8	477.97 µg/L	477.97 ppb	19:32:43
1	S 181.975 Axial†	1303.7	1155.8	940.47 µg/L	940.47 ppb	19:32:43
1	Sb 206.836†	3839.6	3596.5	486.17 µg/L	486.17 ppb	19:32:43
1	Se 196.026†	1266.7	1204.2	478 µg/L	478 ppb	19:32:43
1	SiO2†	51618.1	47942.2	5219.4 µg/L	5219.4 ppb	19:32:23
1	Si 251.611†	154593.2	147618.3	2431.2 µg/L	2431.2 ppb	19:32:23
1	Sn 189.927†	7080.7	6790.2	484.38 µg/L	484.38 ppb	19:32:43
1	Ti 334.940†	502894.8	481769.2	490.61 µg/L	490.61 ppb	19:32:23
1	Tl 190.801†	3593.0	3566.9	486.15 µg/L	486.15 ppb	19:32:43
1	U 409.014†	7303.3	7484.9	492.46 µg/L	492.46 ppb	19:32:23
1	V 292.402†	92682.1	88474.1	496.92 µg/L	496.92 ppb	19:32:23
1	Zn 213.857†	80453.5	76711.2	479.02 µg/L	479.02 ppb	19:32:23
2	Sc RADIAL	155203.4	155203.4	106 %		19:32:01
2	Al 396.153Radial†	25234.3	23729.9	5157.5 µg/L	5157.5 ppb	19:32:01
2	Ca 317.933Radial†	90949.0	84795.6	4968.7 µg/L	4968.7 ppb	19:32:01
2	Fe 238.204 Radial†	79090.7	74162.2	4930.6 µg/L	4930.6 ppb	19:32:01
2	K 766.490 Radial†	13942.4	11638.6	4787.3 µg/L	4787.3 ppb	19:32:01
2	Mg 279.077 IEC†	13250.9	12257.5	5061.5 µg/L	5061.5 ppb	19:32:01
2	Na 589.592 Radial†	70292.0	64317.7	9837.2 µg/L	9837.2 ppb	19:32:01
2	Sr 421.552†	228066.3	214459.1	502.60 µg/L	502.60 ppb	19:31:59
2	Sc 361.383	1737215.7	1737215.7	103.85 %		19:32:47
2	Y 371.029	1054931.1	1054931.1	103.16 %		19:32:47
2	Ag 328.068†	128483.5	120750.5	496.17 µg/L	496.17 ppb	19:32:47
2	As 188.979†	1256.3	1223.9	518.55 µg/L	518.55 ppb	19:33:07
2	B 249.677†	33149.8	28564.4	477.87 µg/L	477.87 ppb	19:32:47
2	Ba 233.527†	112832.9	108822.5	497.54 µg/L	497.54 ppb	19:32:47
2	Be 313.107†	1606762.7	1547820.7	503.98 µg/L	503.98 ppb	19:32:47
2	Cd 226.502†	72368.9	69778.8	481.56 µg/L	481.56 ppb	19:32:47
2	Co 228.616†	36711.4	35526.2	486.72 µg/L	486.72 ppb	19:32:47
2	Cr 267.716†	59192.4	56836.4	488.05 µg/L	488.05 ppb	19:32:47
2	Cu 324.752†	119958.6	113083.9	493.10 µg/L	493.10 ppb	19:32:47
2	Mn 257.610†	372915.3	359002.2	490.34 µg/L	490.34 ppb	19:32:47
2	Mo 202.031†	15840.2	15307.8	483.66 µg/L	483.66 ppb	19:33:07
2	Ni 231.604†	39651.1	38221.1	488.89 µg/L	488.89 ppb	19:32:47
2	P 214.914†	10418.1	9952.1	2374.9 µg/L	2374.9 ppb	19:33:07
2	Pb 220.353†	8335.8	7914.1	480.97 µg/L	480.97 ppb	19:33:07

2	S 181.975 Axial†	1310.0	1166.6	949.21 µg/L	949.21 ppb	19:33:07
2	Sb 206.836†	3818.2	3589.9	485.30 µg/L	485.30 ppb	19:33:07
2	Se 196.026†	1256.0	1198.5	476 µg/L	476 ppb	19:33:07
2	SiO2†	51436.2	47955.4	5220.8 µg/L	5220.8 ppb	19:32:47
2	Si 251.611†	154237.0	147839.3	2434.9 µg/L	2434.9 ppb	19:32:47
2	Sn 189.927†	7075.7	6811.2	485.88 µg/L	485.88 ppb	19:33:07
2	Ti 334.940†	501670.2	482424.6	491.29 µg/L	491.29 ppb	19:32:47
2	Tl 190.801†	3598.0	3584.8	488.57 µg/L	488.57 ppb	19:33:07
2	U 409.014†	7114.9	7330.1	482.93 µg/L	482.93 ppb	19:32:47
2	V 292.402†	92447.3	88586.2	497.56 µg/L	497.56 ppb	19:32:47
2	Zn 213.857†	80237.4	76796.6	479.56 µg/L	479.56 ppb	19:32:47
3	Sc RADIAL	152343.2	152343.2	105 %		19:32:05
3	Al 396.153Radial†	24790.2	23749.9	5162.0 µg/L	5162.0 ppb	19:32:05
3	Ca 317.933Radial†	88711.7	84258.7	4937.2 µg/L	4937.2 ppb	19:32:05
3	Fe 238.204 Radial†	77301.6	73844.9	4909.5 µg/L	4909.5 ppb	19:32:05
3	K 766.490 Radial†	13851.3	11797.3	4852.6 µg/L	4852.6 ppb	19:32:05
3	Mg 279.077 IEC†	12897.2	12152.7	5018.2 µg/L	5018.2 ppb	19:32:05
3	Na 589.592 Radial†	69172.5	64486.0	9862.9 µg/L	9862.9 ppb	19:32:05
3	Sr 421.552†	226674.9	217149.0	508.90 µg/L	508.90 ppb	19:32:03
3	Sc 361.383	1739184.0	1739184.0	103.97 %		19:33:10
3	Y 371.029	1056341.4	1056341.4	103.30 %		19:33:10
3	Ag 328.068†	128938.9	121048.4	497.41 µg/L	497.41 ppb	19:33:10
3	As 188.979†	1242.3	1209.1	512.38 µg/L	512.38 ppb	19:33:30
3	B 249.677†	33322.5	28694.4	480.05 µg/L	480.05 ppb	19:33:10
3	Ba 233.527†	113432.0	109275.8	499.61 µg/L	499.61 ppb	19:33:10
3	Be 313.107†	1612377.9	1551470.5	505.17 µg/L	505.17 ppb	19:33:10
3	Cd 226.502†	72852.6	70165.2	484.23 µg/L	484.23 ppb	19:33:10
3	Co 228.616†	36901.2	35668.8	488.67 µg/L	488.67 ppb	19:33:10
3	Cr 267.716†	59397.9	56969.5	489.19 µg/L	489.19 ppb	19:33:10
3	Cu 324.752†	120225.9	113210.3	493.66 µg/L	493.66 ppb	19:33:10
3	Mn 257.610†	374839.5	360446.6	492.32 µg/L	492.32 ppb	19:33:10
3	Mo 202.031†	15729.4	15184.0	479.75 µg/L	479.75 ppb	19:33:30
3	Ni 231.604†	40031.5	38543.8	493.02 µg/L	493.02 ppb	19:33:10
3	P 214.914†	10307.1	9834.0	2346.7 µg/L	2346.7 ppb	19:33:30
3	Pb 220.353†	8288.5	7859.6	477.65 µg/L	477.65 ppb	19:33:30
3	S 181.975 Axial†	1283.8	1140.0	927.63 µg/L	927.63 ppb	19:33:30
3	Sb 206.836†	3807.3	3575.3	483.25 µg/L	483.25 ppb	19:33:30
3	Se 196.026†	1249.7	1191.1	473 µg/L	473 ppb	19:33:30
3	SiO2†	51607.6	48064.2	5232.9 µg/L	5232.9 ppb	19:33:10
3	Si 251.611†	155270.1	148664.8	2448.6 µg/L	2448.6 ppb	19:33:10
3	Sn 189.927†	7010.2	6740.5	480.86 µg/L	480.86 ppb	19:33:30
3	Ti 334.940†	504064.8	484181.1	493.08 µg/L	493.08 ppb	19:33:10
3	Tl 190.801†	3573.6	3557.4	484.91 µg/L	484.91 ppb	19:33:30
3	U 409.014†	7322.0	7521.5	494.86 µg/L	494.86 ppb	19:33:10
3	V 292.402†	92839.2	88862.3	499.06 µg/L	499.06 ppb	19:33:10
3	Zn 213.857†	80753.8	77205.9	482.11 µg/L	482.11 ppb	19:33:10

Mean Data: CCV

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1740074.0	104.02 %	0.203			0.19%
Sc RADIAL	154145.4	106 %	1.1			1.02%
Y 371.029	1056811.9	103.35 %	0.211			0.20%
Ag 328.068†	120724.4	496.07 µg/L	1.385	496.07 ppb	1.385	0.28%
QC value within limits for Ag 328.068 Recovery = 99.21%						
Al 396.153Radial†	23757.1	5163.5 µg/L	6.91	5163.5 ppb	6.91	0.13%
QC value within limits for Al 396.153Radial Recovery = 103.27%						
As 188.979†	1215.2	514.92 µg/L	3.230	514.92 ppb	3.230	0.63%
QC value within limits for As 188.979 Recovery = 102.98%						
B 249.677†	28619.7	478.80 µg/L	1.123	478.80 ppb	1.123	0.23%
QC value within limits for B 249.677 Recovery = 95.76%						
Ba 233.527†	108929.3	498.02 µg/L	1.404	498.02 ppb	1.404	0.28%
QC value within limits for Ba 233.527 Recovery = 99.60%						
Be 313.107†	1548342.3	504.15 µg/L	0.946	504.15 ppb	0.946	0.19%
QC value within limits for Be 313.107 Recovery = 100.83%						
Ca 317.933Radial†	84623.7	4958.6 µg/L	18.54	4958.6 ppb	18.54	0.37%
QC value within limits for Ca 317.933Radial Recovery = 99.17%						
Cd 226.502†	69935.2	482.64 µg/L	1.407	482.64 ppb	1.407	0.29%
QC value within limits for Cd 226.502 Recovery = 96.53%						
Co 228.616†	35576.6	487.41 µg/L	1.097	487.41 ppb	1.097	0.23%

QC value within limits for Co 228.616 Recovery = 97.48%

Cr 267.716†	56879.6	488.42 µg/L	0.666	488.42 ppb	0.666	0.14%
QC value within limits for Cr 267.716 Recovery = 97.68%						
Cu 324.752†	113017.4	492.82 µg/L	1.012	492.82 ppb	1.012	0.21%
QC value within limits for Cu 324.752 Recovery = 98.56%						
Fe 238.204 Radial†	74084.6	4925.4 µg/L	14.08	4925.4 ppb	14.08	0.29%
QC value within limits for Fe 238.204 Radial Recovery = 98.51%						
K 766.490 Radial†	11741.2	4829.6 µg/L	36.64	4829.6 ppb	36.64	0.76%
QC value within limits for K 766.490 Radial Recovery = 96.59%						
Mg 279.077 IEC†	12248.0	5057.5 µg/L	37.48	5057.5 ppb	37.48	0.74%
QC value within limits for Mg 279.077 IEC Recovery = 101.15%						
Mn 257.610†	359527.3	491.06 µg/L	1.093	491.06 ppb	1.093	0.22%
QC value within limits for Mn 257.610 Recovery = 98.21%						
Mo 202.031†	15245.4	481.69 µg/L	1.954	481.69 ppb	1.954	0.41%
QC value within limits for Mo 202.031 Recovery = 96.34%						
Na 589.592 Radial†	64489.2	9863.4 µg/L	26.47	9863.4 ppb	26.47	0.27%
QC value within limits for Na 589.592 Radial Recovery = 98.63%						
Ni 231.604†	38330.9	490.30 µg/L	2.360	490.30 ppb	2.360	0.48%
QC value within limits for Ni 231.604 Recovery = 98.06%						
P 214.914†	9887.5	2359.5 µg/L	14.32	2359.5 ppb	14.32	0.61%
QC value within limits for P 214.914 Recovery = 94.38%						
Pb 220.353†	7879.5	478.86 µg/L	1.831	478.86 ppb	1.831	0.38%
QC value within limits for Pb 220.353 Recovery = 95.77%						
S 181.975 Axial†	1154.1	939.11 µg/L	10.857	939.11 ppb	10.857	1.16%
QC value within limits for S 181.975 Axial Recovery = 93.91%						
Sb 206.836†	3587.2	484.91 µg/L	1.496	484.91 ppb	1.496	0.31%
QC value within limits for Sb 206.836 Recovery = 96.98%						
Se 196.026†	1197.9	476 µg/L	2.6	476 ppb	2.6	0.55%
QC value within limits for Se 196.026 Recovery = 95.20%						
SiO2†	47987.3	5224.4 µg/L	7.40	5224.4 ppb	7.40	0.14%
QC value within limits for SiO2 Recovery = 97.70%						
Si 251.611†	148040.8	2438.2 µg/L	9.16	2438.2 ppb	9.16	0.38%
QC value within limits for Si 251.611 Recovery = 97.53%						
Sn 189.927†	6780.7	483.70 µg/L	2.578	483.70 ppb	2.578	0.53%
QC value within limits for Sn 189.927 Recovery = 96.74%						
Sr 421.552†	215809.3	505.76 µg/L	3.152	505.76 ppb	3.152	0.62%
QC value within limits for Sr 421.552 Recovery = 101.15%						
Ti 334.940†	482791.6	491.66 µg/L	1.273	491.66 ppb	1.273	0.26%
QC value within limits for Ti 334.940 Recovery = 98.33%						
Tl 190.801†	3569.7	486.55 µg/L	1.860	486.55 ppb	1.860	0.38%
QC value within limits for Tl 190.801 Recovery = 97.31%						
U 409.014†	7445.5	490.08 µg/L	6.310	490.08 ppb	6.310	1.29%
QC value within limits for U 409.014 Recovery = 98.02%						
V 292.402†	88640.9	497.85 µg/L	1.100	497.85 ppb	1.100	0.22%
QC value within limits for V 292.402 Recovery = 99.57%						
Zn 213.857†	76904.5	480.23 µg/L	1.651	480.23 ppb	1.651	0.34%
QC value within limits for Zn 213.857 Recovery = 96.05%						

All analyte(s) passed QC.

Sequence No.: 9

Sample ID: CCB

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 8

Date Collected: 3/29/2010 19:33:37

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCB

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	154440.8	154440.8	106 %		19:34:06
1	Al 396.153Radial†	-43.3	-9.0	-2.0043 µg/L	-2.0043 ppb	19:34:26
1	Ca 317.933Radial†	696.6	41.2	2.4138 µg/L	2.4138 ppb	19:34:26
1	Fe 238.204 Radial†	166.8	44.1	2.9352 µg/L	2.9352 ppb	19:34:26
1	K 766.490 Radial†	1613.3	67.6	27.814 µg/L	27.814 ppb	19:34:06
1	Mg 279.077 IEC†	157.8	-37.7	-15.541 µg/L	-15.541 ppb	19:34:26
1	Na 589.592 Radial†	1722.8	-68.9	-10.561 µg/L	-10.561 ppb	19:34:06
1	Sr 421.552†	-120.8	163.9	0.3842 µg/L	0.3842 ppb	19:34:06
1	Sc 361.383	1731581.1	1731581.1	103.52 %		19:35:14
1	Y 371.029	1065562.9	1065562.9	104.20 %		19:35:14
1	Ag 328.068†	3216.9	140.6	0.5847 µg/L	0.5847 ppb	19:35:16
1	As 188.979†	-11.7	2.9	1.2300 µg/L	1.2300 ppb	19:35:36
1	B 249.677†	3120.0	-341.7	-5.7362 µg/L	-5.7362 ppb	19:35:36
1	Ba 233.527†	-175.6	5.4	0.0247 µg/L	0.0247 ppb	19:35:36
1	Be 313.107†	-246.2	422.2	0.1424 µg/L	0.1424 ppb	19:35:16
1	Cd 226.502†	-69.1	27.7	0.1908 µg/L	0.1908 ppb	19:35:36
1	Co 228.616†	-181.3	1.5	0.0198 µg/L	0.0198 ppb	19:35:36
1	Cr 267.716†	175.8	9.6	0.0693 µg/L	0.0693 ppb	19:35:36
1	Cu 324.752†	2669.4	153.9	0.6825 µg/L	0.6825 ppb	19:35:16
1	Mn 257.610†	196.9	110.2	0.1512 µg/L	0.1512 ppb	19:35:36
1	Mo 202.031†	-29.9	26.3	0.8305 µg/L	0.8305 ppb	19:35:36
1	Ni 231.604†	-61.5	-18.5	-0.2372 µg/L	-0.2372 ppb	19:35:36
1	P 214.914†	55.3	-26.1	-6.2662 µg/L	-6.2662 ppb	19:35:36
1	Pb 220.353†	115.1	-1.2	-0.0837 µg/L	-0.0837 ppb	19:35:36
1	S 181.975 Axial†	87.6	-10.2	-8.2246 µg/L	-8.2246 ppb	19:35:36
1	Sb 206.836†	73.1	-16.1	-2.1571 µg/L	-2.1571 ppb	19:35:36
1	Se 196.026†	13.4	2.0	0.826 µg/L	0.826 ppb	19:35:36
1	SiO2†	1671.5	41.8	4.5433 µg/L	4.5433 ppb	19:35:36
1	Si 251.611†	796.8	93.3	1.5290 µg/L	1.5290 ppb	19:35:36
1	Sn 189.927†	8.8	6.4	0.4582 µg/L	0.4582 ppb	19:35:36
1	Ti 334.940†	627.3	-30.4	-0.0364 µg/L	-0.0364 ppb	19:35:16
1	Tl 190.801†	-118.4	5.9	0.7913 µg/L	0.7913 ppb	19:35:36
1	U 409.014†	-222.3	264.4	16.308 µg/L	16.308 ppb	19:35:16
1	V 292.402†	354.1	-89.7	-0.4781 µg/L	-0.4781 ppb	19:35:16
1	Zn 213.857†	527.0	44.7	0.2818 µg/L	0.2818 ppb	19:35:36
2	Sc RADIAL	154279.9	154279.9	106 %		19:34:28
2	Al 396.153Radial†	-70.9	-35.1	-7.7094 µg/L	-7.7094 ppb	19:34:48
2	Ca 317.933Radial†	709.7	54.3	3.1826 µg/L	3.1826 ppb	19:34:48
2	Fe 238.204 Radial†	178.3	55.2	3.6708 µg/L	3.6708 ppb	19:34:48
2	K 766.490 Radial†	1463.8	-72.1	-29.690 µg/L	-29.690 ppb	19:34:28
2	Mg 279.077 IEC†	161.8	-33.8	-13.912 µg/L	-13.912 ppb	19:34:48
2	Na 589.592 Radial†	1747.5	-43.7	-6.6675 µg/L	-6.6675 ppb	19:34:28
2	Sr 421.552†	-216.0	73.9	0.1732 µg/L	0.1732 ppb	19:34:28
2	Sc 361.383	1751103.4	1751103.4	104.68 %		19:35:38
2	Y 371.029	1076583.0	1076583.0	105.28 %		19:35:38
2	Ag 328.068†	2689.9	-397.5	-1.6314 µg/L	-1.6314 ppb	19:35:40
2	As 188.979†	-19.4	-4.3	-1.7955 µg/L	-1.7955 ppb	19:36:00
2	B 249.677†	3164.1	-333.1	-5.5927 µg/L	-5.5927 ppb	19:36:00
2	Ba 233.527†	-177.8	5.3	0.0236 µg/L	0.0236 ppb	19:36:00
2	Be 313.107†	-520.5	162.9	0.0516 µg/L	0.0516 ppb	19:35:40
2	Cd 226.502†	-104.5	-5.4	-0.0378 µg/L	-0.0378 ppb	19:36:00
2	Co 228.616†	-170.5	13.7	0.1872 µg/L	0.1872 ppb	19:36:00
2	Cr 267.716†	176.6	8.5	0.0762 µg/L	0.0762 ppb	19:36:00
2	Cu 324.752†	2448.1	-86.2	-0.3785 µg/L	-0.3785 ppb	19:35:40
2	Mn 257.610†	240.0	149.3	0.2045 µg/L	0.2045 ppb	19:36:00
2	Mo 202.031†	-29.0	27.5	0.8664 µg/L	0.8664 ppb	19:36:00
2	Ni 231.604†	-48.2	-5.1	-0.0655 µg/L	-0.0655 ppb	19:36:00
2	P 214.914†	58.0	-24.2	-5.7906 µg/L	-5.7906 ppb	19:36:00
2	Pb 220.353†	124.4	6.4	0.3918 µg/L	0.3918 ppb	19:36:00

2	S 181.975 Axial†	90.4	-8.5	-6.8756 µg/L	-6.8756 ppb	19:36:00
2	Sb 206.836†	78.1	-12.0	-1.6140 µg/L	-1.6140 ppb	19:36:00
2	Se 196.026†	15.0	3.5	1.36 µg/L	1.36 ppb	19:36:00
2	SiO2†	1656.1	9.2	0.9709 µg/L	0.9709 ppb	19:36:00
2	Si 251.611†	759.0	48.7	0.7903 µg/L	0.7903 ppb	19:36:00
2	Sn 189.927†	8.2	5.8	0.4148 µg/L	0.4148 ppb	19:36:00
2	Ti 334.940†	745.1	75.4	0.0800 µg/L	0.0800 ppb	19:35:40
2	Tl 190.801†	-111.6	13.7	1.8304 µg/L	1.8304 ppb	19:36:00
2	U 409.014†	-582.4	-77.2	-4.8304 µg/L	-4.8304 ppb	19:35:40
2	V 292.402†	254.3	-188.9	-1.0423 µg/L	-1.0423 ppb	19:35:40
2	Zn 213.857†	524.9	37.0	0.2333 µg/L	0.2333 ppb	19:36:00
3	Sc RADIAL	154300.7	154300.7	106 %		19:34:50
3	Al 396.153Radial†	-22.9	10.3	2.2225 µg/L	2.2225 ppb	19:35:10
3	Ca 317.933Radial†	702.8	47.7	2.7963 µg/L	2.7963 ppb	19:35:10
3	Fe 238.204 Radial†	157.6	35.6	2.3638 µg/L	2.3638 ppb	19:35:10
3	K 766.490 Radial†	1363.4	-167.1	-68.805 µg/L	-68.805 ppb	19:34:50
3	Mg 279.077 IEC†	165.1	-30.7	-12.669 µg/L	-12.669 ppb	19:35:10
3	Na 589.592 Radial†	1617.5	-166.8	-25.467 µg/L	-25.467 ppb	19:34:50
3	Sr 421.552†	-166.5	120.7	0.2829 µg/L	0.2829 ppb	19:34:50
3	Sc 361.383	1756722.7	1756722.7	105.02 %		19:36:02
3	Y 371.029	1079825.4	1079825.4	105.60 %		19:36:02
3	Ag 328.068†	3226.0	104.8	0.4137 µg/L	0.4137 ppb	19:36:04
3	As 188.979†	-24.9	-9.5	-3.9669 µg/L	-3.9669 ppb	19:36:25
3	B 249.677†	3162.1	-344.7	-5.7874 µg/L	-5.7874 ppb	19:36:25
3	Ba 233.527†	-158.1	24.5	0.1116 µg/L	0.1116 ppb	19:36:25
3	Be 313.107†	-509.5	174.9	0.0572 µg/L	0.0572 ppb	19:36:04
3	Cd 226.502†	-104.2	-4.8	-0.0337 µg/L	-0.0337 ppb	19:36:25
3	Co 228.616†	-161.9	22.4	0.3068 µg/L	0.3068 ppb	19:36:25
3	Cr 267.716†	163.5	-4.5	-0.0399 µg/L	-0.0399 ppb	19:36:25
3	Cu 324.752†	2579.5	31.3	0.1372 µg/L	0.1372 ppb	19:36:04
3	Mn 257.610†	210.9	120.8	0.1656 µg/L	0.1656 ppb	19:36:25
3	Mo 202.031†	-42.5	14.8	0.4652 µg/L	0.4652 ppb	19:36:25
3	Ni 231.604†	-54.2	-10.7	-0.1372 µg/L	-0.1372 ppb	19:36:25
3	P 214.914†	63.9	-18.7	-4.4865 µg/L	-4.4865 ppb	19:36:25
3	Pb 220.353†	88.7	-28.0	-1.6935 µg/L	-1.6935 ppb	19:36:25
3	S 181.975 Axial†	84.6	-14.3	-11.562 µg/L	-11.562 ppb	19:36:25
3	Sb 206.836†	89.1	-1.8	-0.2346 µg/L	-0.2346 ppb	19:36:25
3	Se 196.026†	11.7	0.2	0.100 µg/L	0.100 ppb	19:36:25
3	SiO2†	1684.0	30.6	3.3325 µg/L	3.3325 ppb	19:36:25
3	Si 251.611†	773.1	59.7	0.9802 µg/L	0.9802 ppb	19:36:25
3	Sn 189.927†	5.3	3.0	0.2161 µg/L	0.2161 ppb	19:36:25
3	Ti 334.940†	867.2	189.4	0.1939 µg/L	0.1939 ppb	19:36:04
3	Tl 190.801†	-113.0	12.7	1.7012 µg/L	1.7012 ppb	19:36:25
3	U 409.014†	-487.5	14.9	0.8641 µg/L	0.8641 ppb	19:36:04
3	V 292.402†	257.1	-187.1	-1.0329 µg/L	-1.0329 ppb	19:36:04
3	Zn 213.857†	501.2	12.8	0.0813 µg/L	0.0813 ppb	19:36:25

Mean Data: CCB

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1746469.1	104.41 %	0.789			0.76%
Sc RADIAL	154340.5	106 %	0.1			0.06%
Y 371.029	1073990.4	105.03 %	0.731			0.70%
Ag 328.068†	-50.7	-0.2110 µg/L	1.23303	-0.2110 ppb	1.23303	584.39%
QC value within limits for Ag 328.068 Recovery = Not calculated						
Al 396.153Radial†	-11.3	-2.4971 µg/L	4.98426	-2.4971 ppb	4.98426	199.60%
QC value within limits for Al 396.153Radial Recovery = Not calculated						
As 188.979†	-3.6	-1.5108 µg/L	2.61013	-1.5108 ppb	2.61013	172.77%
QC value within limits for As 188.979 Recovery = Not calculated						
B 249.677†	-339.8	-5.7054 µg/L	0.10093	-5.7054 ppb	0.10093	1.77%
QC value within limits for B 249.677 Recovery = Not calculated						
Ba 233.527†	11.7	0.0533 µg/L	0.05049	0.0533 ppb	0.05049	94.76%
QC value within limits for Ba 233.527 Recovery = Not calculated						
Be 313.107†	253.3	0.0837 µg/L	0.05087	0.0837 ppb	0.05087	60.76%
QC value within limits for Be 313.107 Recovery = Not calculated						
Ca 317.933Radial†	47.7	2.7975 µg/L	0.38440	2.7975 ppb	0.38440	13.74%
QC value within limits for Ca 317.933Radial Recovery = Not calculated						
Cd 226.502†	5.8	0.0397 µg/L	0.13082	0.0397 ppb	0.13082	329.26%
QC value within limits for Cd 226.502 Recovery = Not calculated						
Co 228.616†	12.5	0.1713 µg/L	0.14419	0.1713 ppb	0.14419	84.18%

QC value within limits for Co 228.616 Recovery = Not calculated						
Cr 267.716†	4.5	0.0352 µg/L	0.06512	0.0352 ppb	0.06512	185.02%
QC value within limits for Cr 267.716 Recovery = Not calculated						
Cu 324.752†	33.0	0.1470 µg/L	0.53058	0.1470 ppb	0.53058	360.82%
QC value within limits for Cu 324.752 Recovery = Not calculated						
Fe 238.204 Radial†	45.0	2.9899 µg/L	0.65521	2.9899 ppb	0.65521	21.91%
QC value within limits for Fe 238.204 Radial Recovery = Not calculated						
K 766.490 Radial†	-57.2	-23.560 µg/L	48.6004	-23.560 ppb	48.6004	206.28%
QC value within limits for K 766.490 Radial Recovery = Not calculated						
Mg 279.077 IEC†	-34.1	-14.041 µg/L	1.4406	-14.041 ppb	1.4406	10.26%
QC value within limits for Mg 279.077 IEC Recovery = Not calculated						
Mn 257.610†	126.8	0.1738 µg/L	0.02760	0.1738 ppb	0.02760	15.88%
QC value within limits for Mn 257.610 Recovery = Not calculated						
Mo 202.031†	22.8	0.7207 µg/L	0.22201	0.7207 ppb	0.22201	30.81%
QC value within limits for Mo 202.031 Recovery = Not calculated						
Na 589.592 Radial†	-93.1	-14.232 µg/L	9.9226	-14.232 ppb	9.9226	69.72%
QC value within limits for Na 589.592 Radial Recovery = Not calculated						
Ni 231.604†	-11.5	-0.1466 µg/L	0.08623	-0.1466 ppb	0.08623	58.80%
QC value within limits for Ni 231.604 Recovery = Not calculated						
P 214.914†	-23.0	-5.5144 µg/L	0.92145	-5.5144 ppb	0.92145	16.71%
QC value within limits for P 214.914 Recovery = Not calculated						
Pb 220.353†	-7.6	-0.4618 µg/L	1.09284	-0.4618 ppb	1.09284	236.66%
QC value within limits for Pb 220.353 Recovery = Not calculated						
S 181.975 Axial†	-11.0	-8.8875 µg/L	2.41268	-8.8875 ppb	2.41268	27.15%
QC value within limits for S 181.975 Axial Recovery = Not calculated						
Sb 206.836†	-10.0	-1.3353 µg/L	0.99108	-1.3353 ppb	0.99108	74.22%
QC value within limits for Sb 206.836 Recovery = Not calculated						
Se 196.026†	1.9	0.763 µg/L	0.6334	0.763 ppb	0.6334	83.06%
QC value within limits for Se 196.026 Recovery = Not calculated						
SiO2†	27.2	2.9489 µg/L	1.81680	2.9489 ppb	1.81680	61.61%
QC value within limits for SiO2 Recovery = Not calculated						
Si 251.611†	67.2	1.0998 µg/L	0.38363	1.0998 ppb	0.38363	34.88%
QC value within limits for Si 251.611 Recovery = Not calculated						
Sn 189.927†	5.1	0.3630 µg/L	0.12911	0.3630 ppb	0.12911	35.56%
QC value within limits for Sn 189.927 Recovery = Not calculated						
Sr 421.552†	119.5	0.2801 µg/L	0.10556	0.2801 ppb	0.10556	37.69%
QC value within limits for Sr 421.552 Recovery = Not calculated						
Ti 334.940†	78.1	0.0792 µg/L	0.11512	0.0792 ppb	0.11512	145.40%
QC value within limits for Ti 334.940 Recovery = Not calculated						
Tl 190.801†	10.8	1.4410 µg/L	0.56631	1.4410 ppb	0.56631	39.30%
QC value within limits for Tl 190.801 Recovery = Not calculated						
U 409.014†	67.4	4.1140 µg/L	10.93772	4.1140 ppb	10.93772	265.87%
QC value within limits for U 409.014 Recovery = Not calculated						
V 292.402†	-155.2	-0.8511 µg/L	0.32304	-0.8511 ppb	0.32304	37.96%
QC value within limits for V 292.402 Recovery = Not calculated						
Zn 213.857†	31.5	0.1988 µg/L	0.10458	0.1988 ppb	0.10458	52.60%
QC value within limits for Zn 213.857 Recovery = Not calculated						
All analyte(s) passed QC.						

Sequence No.: 18

Sample ID: CCV

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 7

Date Collected: 3/29/2010 19:52:48

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCV

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	155882.7	155882.7	107 %		19:53:21
1	Al 396.153Radial†	25404.5	23785.7	5169.7 µg/L	5169.7 ppb	19:53:21
1	Ca 317.933Radial†	90923.1	84399.2	4945.4 µg/L	4945.4 ppb	19:53:21
1	Fe 238.204 Radial†	79031.3	73782.9	4905.3 µg/L	4905.3 ppb	19:53:21
1	K 766.490 Radial†	14120.7	11748.2	4832.4 µg/L	4832.4 ppb	19:53:21
1	Mg 279.077 IEC†	13276.7	12227.4	5049.1 µg/L	5049.1 ppb	19:53:21
1	Na 589.592 Radial†	70685.1	64397.5	9849.3 µg/L	9849.3 ppb	19:53:21
1	Sr 421.552†	229627.1	214985.0	503.83 µg/L	503.83 ppb	19:53:19
1	Sc 361.383	1753609.4	1753609.4	104.83 %		19:53:33
1	Y 371.029	1065335.0	1065335.0	104.18 %		19:53:33
1	Ag 328.068†	129859.6	120906.6	496.82 µg/L	496.82 ppb	19:53:33
1	As 188.979†	1259.2	1215.4	515.01 µg/L	515.01 ppb	19:53:54
1	B 249.677†	33439.0	28541.9	477.50 µg/L	477.50 ppb	19:53:33
1	Ba 233.527†	114213.7	109124.0	498.92 µg/L	498.92 ppb	19:53:33
1	Be 313.107†	1623855.4	1549661.7	504.58 µg/L	504.58 ppb	19:53:33
1	Cd 226.502†	73102.1	69826.8	481.89 µg/L	481.89 ppb	19:53:33
1	Co 228.616†	36982.2	35454.0	485.73 µg/L	485.73 ppb	19:53:33
1	Cr 267.716†	59867.3	56947.4	489.01 µg/L	489.01 ppb	19:53:33
1	Cu 324.752†	121039.4	113035.1	492.88 µg/L	492.88 ppb	19:53:33
1	Mn 257.610†	376767.1	359319.5	490.78 µg/L	490.78 ppb	19:53:33
1	Mo 202.031†	15963.8	15283.1	482.88 µg/L	482.88 ppb	19:53:54
1	Ni 231.604†	39977.6	38175.7	488.31 µg/L	488.31 ppb	19:53:33
1	P 214.914†	10457.3	9895.7	2361.5 µg/L	2361.5 ppb	19:53:54
1	Pb 220.353†	8391.8	7892.5	479.66 µg/L	479.66 ppb	19:53:54
1	S 181.975 Axial†	1293.9	1139.4	927.23 µg/L	927.23 ppb	19:53:54
1	Sb 206.836†	3874.2	3609.0	487.86 µg/L	487.86 ppb	19:53:54
1	Se 196.026†	1272.9	1203.3	478 µg/L	478 ppb	19:53:54
1	SiO2†	51967.3	47999.0	5225.6 µg/L	5225.6 ppb	19:53:33
1	Si 251.611†	156115.9	148243.1	2441.5 µg/L	2441.5 ppb	19:53:33
1	Sn 189.927†	7141.4	6810.1	485.80 µg/L	485.80 ppb	19:53:54
1	Ti 334.940†	507174.4	483159.2	492.04 µg/L	492.04 ppb	19:53:33
1	Tl 190.801†	3640.2	3592.7	489.65 µg/L	489.65 ppb	19:53:54
1	U 409.014†	7175.3	7323.6	482.62 µg/L	482.62 ppb	19:53:33
1	V 292.402†	93601.0	88854.5	499.04 µg/L	499.04 ppb	19:53:33
1	Zn 213.857†	81005.3	76806.8	479.63 µg/L	479.63 ppb	19:53:33
2	Sc RADIAL	156189.6	156189.6	107 %		19:53:25
2	Al 396.153Radial†	25453.6	23784.9	5169.5 µg/L	5169.5 ppb	19:53:25
2	Ca 317.933Radial†	91189.7	84480.9	4950.2 µg/L	4950.2 ppb	19:53:25
2	Fe 238.204 Radial†	79453.6	74031.8	4921.9 µg/L	4921.9 ppb	19:53:25
2	K 766.490 Radial†	14048.5	11654.9	4794.0 µg/L	4794.0 ppb	19:53:25
2	Mg 279.077 IEC†	13352.4	12273.6	5068.1 µg/L	5068.1 ppb	19:53:25
2	Na 589.592 Radial†	70950.0	64514.9	9867.3 µg/L	9867.3 ppb	19:53:25
2	Sr 421.552†	232352.0	217106.1	508.80 µg/L	508.80 ppb	19:53:23
2	Sc 361.383	1749571.1	1749571.1	104.59 %		19:53:57
2	Y 371.029	1062777.0	1062777.0	103.93 %		19:53:57
2	Ag 328.068†	129030.1	120399.3	494.76 µg/L	494.76 ppb	19:53:57
2	As 188.979†	1277.4	1235.6	523.42 µg/L	523.42 ppb	19:54:17
2	B 249.677†	33289.1	28472.2	476.33 µg/L	476.33 ppb	19:53:57
2	Ba 233.527†	113708.3	108892.2	497.86 µg/L	497.86 ppb	19:53:57
2	Be 313.107†	1621134.0	1550635.2	504.90 µg/L	504.90 ppb	19:53:57
2	Cd 226.502†	72772.0	69672.1	480.82 µg/L	480.82 ppb	19:53:57
2	Co 228.616†	36900.7	35457.5	485.78 µg/L	485.78 ppb	19:53:57
2	Cr 267.716†	59600.3	56824.0	487.94 µg/L	487.94 ppb	19:53:57
2	Cu 324.752†	120397.9	112688.2	491.39 µg/L	491.39 ppb	19:53:57
2	Mn 257.610†	375323.1	358768.5	490.02 µg/L	490.02 ppb	19:53:57
2	Mo 202.031†	15936.5	15292.2	483.17 µg/L	483.17 ppb	19:54:17
2	Ni 231.604†	39772.4	38067.5	486.93 µg/L	486.93 ppb	19:53:57
2	P 214.914†	10473.9	9934.6	2370.8 µg/L	2370.8 ppb	19:54:17
2	Pb 220.353†	8398.2	7917.1	481.14 µg/L	481.14 ppb	19:54:17

2	S 181.975 Axial†	1310.8	1158.5	942.63 µg/L	942.63 ppb	19:54:17
2	Sb 206.836†	3846.2	3590.8	485.41 µg/L	485.41 ppb	19:54:17
2	Se 196.026†	1265.1	1198.6	476 µg/L	476 ppb	19:54:17
2	SiO2†	51895.6	48044.8	5230.6 µg/L	5230.6 ppb	19:53:57
2	Si 251.611†	155321.7	147827.6	2434.7 µg/L	2434.7 ppb	19:53:57
2	Sn 189.927†	7131.0	6815.9	486.21 µg/L	486.21 ppb	19:54:17
2	Ti 334.940†	504709.9	481919.6	490.77 µg/L	490.77 ppb	19:53:57
2	Tl 190.801†	3621.3	3582.7	488.28 µg/L	488.28 ppb	19:54:17
2	U 409.014†	7284.6	7443.9	490.00 µg/L	490.00 ppb	19:53:57
2	V 292.402†	93209.2	88686.0	498.11 µg/L	498.11 ppb	19:53:57
2	Zn 213.857†	80533.7	76534.3	477.93 µg/L	477.93 ppb	19:53:57
3	Sc RADIAL	155078.4	155078.4	106 %		19:53:29
3	Al 396.153Radial†	25069.2	23593.8	5127.8 µg/L	5127.8 ppb	19:53:29
3	Ca 317.933Radial†	90380.5	84330.2	4941.4 µg/L	4941.4 ppb	19:53:29
3	Fe 238.204 Radial†	78812.3	73960.4	4917.1 µg/L	4917.1 ppb	19:53:29
3	K 766.490 Radial†	14162.7	11856.1	4876.9 µg/L	4876.9 ppb	19:53:29
3	Mg 279.077 IEC†	13255.0	12271.4	5067.2 µg/L	5067.2 ppb	19:53:29
3	Na 589.592 Radial†	70378.5	64452.3	9857.7 µg/L	9857.7 ppb	19:53:29
3	Sr 421.552†	229789.0	216250.9	506.80 µg/L	506.80 ppb	19:53:27
3	Sc 361.383	1754221.5	1754221.5	104.87 %		19:54:20
3	Y 371.029	1065517.6	1065517.6	104.20 %		19:54:20
3	Ag 328.068†	129249.8	120281.8	494.30 µg/L	494.30 ppb	19:54:20
3	As 188.979†	1278.2	1233.1	522.37 µg/L	522.37 ppb	19:54:40
3	B 249.677†	33485.8	28575.4	478.06 µg/L	478.06 ppb	19:54:20
3	Ba 233.527†	113649.5	108547.9	496.28 µg/L	496.28 ppb	19:54:20
3	Be 313.107†	1620552.1	1545971.4	503.38 µg/L	503.38 ppb	19:54:20
3	Cd 226.502†	72839.4	69552.0	479.99 µg/L	479.99 ppb	19:54:20
3	Co 228.616†	36967.6	35427.9	485.37 µg/L	485.37 ppb	19:54:20
3	Cr 267.716†	59675.2	56744.3	487.25 µg/L	487.25 ppb	19:54:20
3	Cu 324.752†	120775.4	112743.0	491.64 µg/L	491.64 ppb	19:54:20
3	Mn 257.610†	375706.0	358182.3	489.22 µg/L	489.22 ppb	19:54:20
3	Mo 202.031†	15964.1	15278.1	482.72 µg/L	482.72 ppb	19:54:40
3	Ni 231.604†	39857.9	38048.2	486.68 µg/L	486.68 ppb	19:54:20
3	P 214.914†	10507.5	9940.1	2372.1 µg/L	2372.1 ppb	19:54:40
3	Pb 220.353†	8449.2	7944.5	482.78 µg/L	482.78 ppb	19:54:40
3	S 181.975 Axial†	1329.7	1173.2	954.54 µg/L	954.54 ppb	19:54:40
3	Sb 206.836†	3845.9	3580.7	484.06 µg/L	484.06 ppb	19:54:40
3	Se 196.026†	1261.3	1191.8	474 µg/L	474 ppb	19:54:40
3	SiO2†	51759.5	47783.5	5202.0 µg/L	5202.0 ppb	19:54:20
3	Si 251.611†	155480.2	147585.0	2430.6 µg/L	2430.6 ppb	19:54:20
3	Sn 189.927†	7188.1	6852.4	488.80 µg/L	488.80 ppb	19:54:40
3	Ti 334.940†	505136.1	481046.7	489.87 µg/L	489.87 ppb	19:54:20
3	Tl 190.801†	3646.0	3597.0	490.19 µg/L	490.19 ppb	19:54:40
3	U 409.014†	7585.0	7711.9	506.54 µg/L	506.54 ppb	19:54:20
3	V 292.402†	93415.0	88646.0	497.89 µg/L	497.89 ppb	19:54:20
3	Zn 213.857†	80914.4	76693.2	478.93 µg/L	478.93 ppb	19:54:20

Mean Data: CCV

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1752467.3	104.76 %	0.151			0.14%
Sc RADIAL	155716.9	107 %	0.4			0.37%
Y 371.029	1064543.2	104.10 %	0.150			0.14%
Ag 328.068†	120529.2	495.29 µg/L	1.342	495.29 ppb	1.342	0.27%
QC value within limits for Ag 328.068 Recovery = 99.06%						
Al 396.153Radial†	23721.5	5155.7 µg/L	24.12	5155.7 ppb	24.12	0.47%
QC value within limits for Al 396.153Radial Recovery = 103.11%						
As 188.979†	1228.0	520.27 µg/L	4.583	520.27 ppb	4.583	0.88%
QC value within limits for As 188.979 Recovery = 104.05%						
B 249.677†	28529.8	477.29 µg/L	0.884	477.29 ppb	0.884	0.19%
QC value within limits for B 249.677 Recovery = 95.46%						
Ba 233.527†	108854.7	497.68 µg/L	1.325	497.68 ppb	1.325	0.27%
QC value within limits for Ba 233.527 Recovery = 99.54%						
Be 313.107†	1548756.1	504.29 µg/L	0.798	504.29 ppb	0.798	0.16%
QC value within limits for Be 313.107 Recovery = 100.86%						
Ca 317.933Radial†	84403.4	4945.7 µg/L	4.42	4945.7 ppb	4.42	0.09%
QC value within limits for Ca 317.933Radial Recovery = 98.91%						
Cd 226.502†	69683.6	480.90 µg/L	0.952	480.90 ppb	0.952	0.20%
QC value within limits for Cd 226.502 Recovery = 96.18%						
Co 228.616†	35446.5	485.63 µg/L	0.223	485.63 ppb	0.223	0.05%

QC value within limits for Co 228.616 Recovery = 97.13%					
Cr 267.716†	56838.6	488.07 µg/L	0.888	488.07 ppb	0.888 0.18%
QC value within limits for Cr 267.716 Recovery = 97.61%					
Cu 324.752†	112822.1	491.97 µg/L	0.803	491.97 ppb	0.803 0.16%
QC value within limits for Cu 324.752 Recovery = 98.39%					
Fe 238.204 Radial†	73925.1	4914.8 µg/L	8.52	4914.8 ppb	8.52 0.17%
QC value within limits for Fe 238.204 Radial Recovery = 98.30%					
K 766.490 Radial†	11753.1	4834.4 µg/L	41.46	4834.4 ppb	41.46 0.86%
QC value within limits for K 766.490 Radial Recovery = 96.69%					
Mg 279.077 IEC†	12257.5	5061.5 µg/L	10.75	5061.5 ppb	10.75 0.21%
QC value within limits for Mg 279.077 IEC Recovery = 101.23%					
Mn 257.610†	358756.8	490.01 µg/L	0.777	490.01 ppb	0.777 0.16%
QC value within limits for Mn 257.610 Recovery = 98.00%					
Mo 202.031†	15284.5	482.92 µg/L	0.226	482.92 ppb	0.226 0.05%
QC value within limits for Mo 202.031 Recovery = 96.58%					
Na 589.592 Radial†	64454.9	9858.1 µg/L	9.01	9858.1 ppb	9.01 0.09%
QC value within limits for Na 589.592 Radial Recovery = 98.58%					
Ni 231.604†	38097.1	487.31 µg/L	0.879	487.31 ppb	0.879 0.18%
QC value within limits for Ni 231.604 Recovery = 97.46%					
P 214.914†	9923.5	2368.1 µg/L	5.81	2368.1 ppb	5.81 0.25%
QC value within limits for P 214.914 Recovery = 94.72%					
Pb 220.353†	7918.0	481.20 µg/L	1.563	481.20 ppb	1.563 0.32%
QC value within limits for Pb 220.353 Recovery = 96.24%					
S 181.975 Axial†	1157.0	941.47 µg/L	13.693	941.47 ppb	13.693 1.45%
QC value within limits for S 181.975 Axial Recovery = 94.15%					
Sb 206.836†	3593.5	485.78 µg/L	1.923	485.78 ppb	1.923 0.40%
QC value within limits for Sb 206.836 Recovery = 97.16%					
Se 196.026†	1197.9	476 µg/L	2.3	476 ppb	2.3 0.48%
QC value within limits for Se 196.026 Recovery = 95.20%					
SiO2†	47942.4	5219.4 µg/L	15.27	5219.4 ppb	15.27 0.29%
QC value within limits for SiO2 Recovery = 97.60%					
Si 251.611†	147885.2	2435.6 µg/L	5.51	2435.6 ppb	5.51 0.23%
QC value within limits for Si 251.611 Recovery = 97.42%					
Sn 189.927†	6826.1	486.94 µg/L	1.623	486.94 ppb	1.623 0.33%
QC value within limits for Sn 189.927 Recovery = 97.39%					
Sr 421.552†	216114.0	506.48 µg/L	2.501	506.48 ppb	2.501 0.49%
QC value within limits for Sr 421.552 Recovery = 101.30%					
Ti 334.940†	482041.8	490.89 µg/L	1.088	490.89 ppb	1.088 0.22%
QC value within limits for Ti 334.940 Recovery = 98.18%					
Tl 190.801†	3590.8	489.38 µg/L	0.983	489.38 ppb	0.983 0.20%
QC value within limits for Tl 190.801 Recovery = 97.88%					
U 409.014†	7493.2	493.05 µg/L	12.247	493.05 ppb	12.247 2.48%
QC value within limits for U 409.014 Recovery = 98.61%					
V 292.402†	88728.8	498.35 µg/L	0.611	498.35 ppb	0.611 0.12%
QC value within limits for V 292.402 Recovery = 99.67%					
Zn 213.857†	76678.1	478.83 µg/L	0.858	478.83 ppb	0.858 0.18%
QC value within limits for Zn 213.857 Recovery = 95.77%					
All analyte(s) passed QC.					

Sequence No.: 19

Sample ID: CCB

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 8

Date Collected: 3/29/2010 19:54:47

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCB

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	157224.0	157224.0	108 %		19:55:16
1	Al 396.153Radial†	-32.4	1.9	0.3819 µg/L	0.3819 ppb	19:55:36
1	Ca 317.933Radial†	709.9	41.9	2.4560 µg/L	2.4560 ppb	19:55:36
1	Fe 238.204 Radial†	168.7	43.1	2.8662 µg/L	2.8662 ppb	19:55:36
1	K 766.490 Radial†	1483.0	-80.2	-33.015 µg/L	-33.015 ppb	19:55:16
1	Mg 279.077 IEC†	179.6	-20.2	-8.3135 µg/L	-8.3135 ppb	19:55:36
1	Na 589.592 Radial†	1705.0	-114.1	-17.428 µg/L	-17.428 ppb	19:55:16
1	Sr 421.552†	-122.3	164.6	0.3859 µg/L	0.3859 ppb	19:55:16
1	Sc 361.383	1744373.3	1744373.3	104.28 %		19:56:24
1	Y 371.029	1071958.2	1071958.2	104.83 %		19:56:24
1	Ag 328.068†	3041.9	-50.0	-0.2039 µg/L	-0.2039 ppb	19:56:26
1	As 188.979†	-16.7	-1.8	-0.7391 µg/L	-0.7391 ppb	19:56:46
1	B 249.677†	3115.7	-367.9	-6.1751 µg/L	-6.1751 ppb	19:56:46
1	Ba 233.527†	-172.9	9.3	0.0420 µg/L	0.0420 ppb	19:56:46
1	Be 313.107†	-510.3	170.7	0.0584 µg/L	0.0584 ppb	19:56:26
1	Cd 226.502†	-91.2	6.9	0.0476 µg/L	0.0476 ppb	19:56:46
1	Co 228.616†	-200.7	-15.9	-0.2172 µg/L	-0.2172 ppb	19:56:46
1	Cr 267.716†	193.2	25.0	0.2074 µg/L	0.2074 ppb	19:56:46
1	Cu 324.752†	2573.6	43.1	0.1952 µg/L	0.1952 ppb	19:56:26
1	Mn 257.610†	146.1	60.1	0.0824 µg/L	0.0824 ppb	19:56:46
1	Mo 202.031†	-38.9	17.9	0.5656 µg/L	0.5656 ppb	19:56:46
1	Ni 231.604†	-15.8	25.7	0.3290 µg/L	0.3290 ppb	19:56:46
1	P 214.914†	40.8	-40.5	-9.7010 µg/L	-9.7010 ppb	19:56:46
1	Pb 220.353†	105.0	-11.7	-0.7153 µg/L	-0.7153 ppb	19:56:46
1	S 181.975 Axial†	80.4	-17.8	-14.383 µg/L	-14.383 ppb	19:56:46
1	Sb 206.836†	78.7	-11.2	-1.5082 µg/L	-1.5082 ppb	19:56:46
1	Se 196.026†	26.3	14.3	5.65 µg/L	5.65 ppb	19:56:46
1	SiO2†	1648.2	7.7	0.8224 µg/L	0.8224 ppb	19:56:46
1	Si 251.611†	791.8	83.0	1.3617 µg/L	1.3617 ppb	19:56:46
1	Sn 189.927†	7.8	5.5	0.3882 µg/L	0.3882 ppb	19:56:46
1	Ti 334.940†	798.2	129.1	0.1285 µg/L	0.1285 ppb	19:56:26
1	Tl 190.801†	-105.6	19.0	2.5510 µg/L	2.5510 ppb	19:56:46
1	U 409.014†	-340.6	152.4	9.3589 µg/L	9.3589 ppb	19:56:26
1	V 292.402†	251.4	-190.7	-1.0454 µg/L	-1.0454 ppb	19:56:26
1	Zn 213.857†	524.6	38.6	0.2408 µg/L	0.2408 ppb	19:56:46
2	Sc RADIAL	153604.9	153604.9	105 %		19:55:38
2	Al 396.153Radial†	-40.7	-6.7	-1.5003 µg/L	-1.5003 ppb	19:55:58
2	Ca 317.933Radial†	698.2	46.3	2.7145 µg/L	2.7145 ppb	19:55:58
2	Fe 238.204 Radial†	160.1	38.6	2.5686 µg/L	2.5686 ppb	19:55:58
2	K 766.490 Radial†	1640.2	101.4	41.741 µg/L	41.741 ppb	19:55:38
2	Mg 279.077 IEC†	170.0	-25.4	-10.448 µg/L	-10.448 ppb	19:55:58
2	Na 589.592 Radial†	1652.3	-126.9	-19.447 µg/L	-19.447 ppb	19:55:38
2	Sr 421.552†	-170.5	116.2	0.2723 µg/L	0.2723 ppb	19:55:38
2	Sc 361.383	1769862.2	1769862.2	105.80 %		19:56:48
2	Y 371.029	1086957.3	1086957.3	106.30 %		19:56:48
2	Ag 328.068†	3055.4	-79.2	-0.3279 µg/L	-0.3279 ppb	19:56:50
2	As 188.979†	-3.9	10.5	4.3943 µg/L	4.3943 ppb	19:57:10
2	B 249.677†	3116.6	-410.1	-6.8860 µg/L	-6.8860 ppb	19:57:10
2	Ba 233.527†	-159.5	24.3	0.1105 µg/L	0.1105 ppb	19:57:10
2	Be 313.107†	-578.9	112.9	0.0378 µg/L	0.0378 ppb	19:56:50
2	Cd 226.502†	-100.7	-0.8	-0.0060 µg/L	-0.0060 ppb	19:57:10
2	Co 228.616†	-154.1	30.9	0.4233 µg/L	0.4233 ppb	19:57:10
2	Cr 267.716†	158.7	-10.2	-0.0909 µg/L	-0.0909 ppb	19:57:10
2	Cu 324.752†	2676.8	105.1	0.4602 µg/L	0.4602 ppb	19:56:50
2	Mn 257.610†	145.1	57.2	0.0785 µg/L	0.0785 ppb	19:57:10
2	Mo 202.031†	-36.1	21.0	0.6639 µg/L	0.6639 ppb	19:57:10
2	Ni 231.604†	-68.7	-24.1	-0.3078 µg/L	-0.3078 ppb	19:57:10
2	P 214.914†	59.6	-23.2	-5.5807 µg/L	-5.5807 ppb	19:57:10
2	Pb 220.353†	97.2	-20.5	-1.2440 µg/L	-1.2440 ppb	19:57:10

2	S 181.975 Axial†	84.9	-14.6	-11.787 µg/L	-11.787 ppb	19:57:10
2	Sb 206.836†	96.3	4.4	0.6052 µg/L	0.6052 ppb	19:57:10
2	Se 196.026†	0.8	-10.2	-4.02 µg/L	-4.02 ppb	19:57:10
2	SiO2†	1672.2	7.6	0.8120 µg/L	0.8120 ppb	19:57:10
2	Si 251.611†	794.7	74.7	1.2254 µg/L	1.2254 ppb	19:57:10
2	Sn 189.927†	4.2	1.9	0.1385 µg/L	0.1385 ppb	19:57:10
2	Ti 334.940†	903.8	217.9	0.2217 µg/L	0.2217 ppb	19:56:50
2	Tl 190.801†	-111.2	15.2	2.0307 µg/L	2.0307 ppb	19:57:10
2	U 409.014†	-447.5	56.1	3.4153 µg/L	3.4153 ppb	19:56:50
2	V 292.402†	287.1	-160.5	-0.8820 µg/L	-0.8820 ppb	19:56:50
2	Zn 213.857†	515.3	22.6	0.1440 µg/L	0.1440 ppb	19:57:10
3	Sc RADIAL	153703.8	153703.8	105 %		19:56:00
3	Al 396.153Radial†	-49.3	-14.8	-3.2844 µg/L	-3.2844 ppb	19:56:20
3	Ca 317.933Radial†	710.1	57.2	3.3512 µg/L	3.3512 ppb	19:56:20
3	Fe 238.204 Radial†	142.7	22.1	1.4665 µg/L	1.4665 ppb	19:56:20
3	K 766.490 Radial†	1683.5	141.5	58.243 µg/L	58.243 ppb	19:56:00
3	Mg 279.077 IEC†	155.1	-39.6	-16.319 µg/L	-16.319 ppb	19:56:20
3	Na 589.592 Radial†	1574.2	-202.0	-30.955 µg/L	-30.955 ppb	19:56:00
3	Sr 421.552†	-284.4	8.3	0.0193 µg/L	0.0193 ppb	19:56:00
3	Sc 361.383	1752547.4	1752547.4	104.77 %		19:57:12
3	Y 371.029	1077428.7	1077428.7	105.36 %		19:57:12
3	Ag 328.068†	3055.4	-50.7	-0.2129 µg/L	-0.2129 ppb	19:57:14
3	As 188.979†	-12.7	2.2	0.9041 µg/L	0.9041 ppb	19:57:35
3	B 249.677†	3085.6	-410.5	-6.8921 µg/L	-6.8921 ppb	19:57:35
3	Ba 233.527†	-169.6	13.1	0.0597 µg/L	0.0597 ppb	19:57:35
3	Be 313.107†	-482.0	200.1	0.0664 µg/L	0.0664 ppb	19:57:14
3	Cd 226.502†	-116.9	-17.2	-0.1188 µg/L	-0.1188 ppb	19:57:35
3	Co 228.616†	-195.4	-9.9	-0.1357 µg/L	-0.1357 ppb	19:57:35
3	Cr 267.716†	143.5	-23.2	-0.2031 µg/L	-0.2031 ppb	19:57:35
3	Cu 324.752†	2562.2	20.7	0.0929 µg/L	0.0929 ppb	19:57:14
3	Mn 257.610†	158.6	71.4	0.0982 µg/L	0.0982 ppb	19:57:35
3	Mo 202.031†	-25.3	31.1	0.9808 µg/L	0.9808 ppb	19:57:35
3	Ni 231.604†	-42.1	0.8	0.0099 µg/L	0.0099 ppb	19:57:35
3	P 214.914†	71.3	-11.5	-2.7700 µg/L	-2.7700 ppb	19:57:35
3	Pb 220.353†	104.0	-13.2	-0.8002 µg/L	-0.8002 ppb	19:57:35
3	S 181.975 Axial†	83.8	-14.8	-11.977 µg/L	-11.977 ppb	19:57:35
3	Sb 206.836†	75.3	-14.7	-1.9710 µg/L	-1.9710 ppb	19:57:35
3	Se 196.026†	23.6	11.6	4.60 µg/L	4.60 ppb	19:57:35
3	SiO2†	1653.5	5.4	0.5590 µg/L	0.5590 ppb	19:57:35
3	Si 251.611†	763.9	52.8	0.8589 µg/L	0.8589 ppb	19:57:35
3	Sn 189.927†	2.7	0.5	0.0386 µg/L	0.0386 ppb	19:57:35
3	Ti 334.940†	894.4	217.4	0.2215 µg/L	0.2215 ppb	19:57:14
3	Tl 190.801†	-118.7	7.0	0.9364 µg/L	0.9364 ppb	19:57:35
3	U 409.014†	-431.7	67.1	4.0863 µg/L	4.0863 ppb	19:57:14
3	V 292.402†	259.2	-184.4	-1.0115 µg/L	-1.0115 ppb	19:57:14
3	Zn 213.857†	491.0	4.2	0.0263 µg/L	0.0263 ppb	19:57:35

Mean Data: CCB

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1755594.3	104.95 %	0.778			0.74%
Sc RADIAL	154844.2	106 %	1.4			1.33%
Y 371.029	1078781.4	105.50 %	0.742			0.70%
Ag 328.068†	-60.0	-0.2482 µg/L	0.06913	-0.2482 ppb	0.06913	27.85%
QC value within limits for Ag 328.068 Recovery = Not calculated						
Al 396.153Radial†	-6.6	-1.4676 µg/L	1.83335	-1.4676 ppb	1.83335	124.92%
QC value within limits for Al 396.153Radial Recovery = Not calculated						
As 188.979†	3.6	1.5198 µg/L	2.62149	1.5198 ppb	2.62149	172.49%
QC value within limits for As 188.979 Recovery = Not calculated						
B 249.677†	-396.2	-6.6511 µg/L	0.41221	-6.6511 ppb	0.41221	6.20%
QC value within limits for B 249.677 Recovery = Not calculated						
Ba 233.527†	15.6	0.0707 µg/L	0.03556	0.0707 ppb	0.03556	50.28%
QC value within limits for Ba 233.527 Recovery = Not calculated						
Be 313.107†	161.2	0.0542 µg/L	0.01474	0.0542 ppb	0.01474	27.20%
QC value within limits for Be 313.107 Recovery = Not calculated						
Ca 317.933Radial†	48.5	2.8406 µg/L	0.46071	2.8406 ppb	0.46071	16.22%
QC value within limits for Ca 317.933Radial Recovery = Not calculated						
Cd 226.502†	-3.7	-0.0257 µg/L	0.08491	-0.0257 ppb	0.08491	330.30%
QC value within limits for Cd 226.502 Recovery = Not calculated						
Co 228.616†	1.7	0.0235 µg/L	0.34867	0.0235 ppb	0.34867	>999.9%

QC value within limits for Co 228.616	Recovery = Not calculated		
Cr 267.716†	-2.8 -0.0289 µg/L	0.21215 -0.0289 ppb	0.21215 734.89%
QC value within limits for Cr 267.716	Recovery = Not calculated		
Cu 324.752†	56.3 0.2495 µg/L	0.18957 0.2495 ppb	0.18957 75.99%
QC value within limits for Cu 324.752	Recovery = Not calculated		
Fe 238.204 Radial†	34.6 2.3004 µg/L	0.73735 2.3004 ppb	0.73735 32.05%
QC value within limits for Fe 238.204 Radial	Recovery = Not calculated		
K 766.490 Radial†	54.2 22.323 µg/L	48.6295 22.323 ppb	48.6295 217.84%
QC value within limits for K 766.490 Radial	Recovery = Not calculated		
Mg 279.077 IEC†	-28.4 -11.693 µg/L	4.1454 -11.693 ppb	4.1454 35.45%
QC value within limits for Mg 279.077 IEC	Recovery = Not calculated		
Mn 257.610†	62.9 0.0864 µg/L	0.01044 0.0864 ppb	0.01044 12.09%
QC value within limits for Mn 257.610	Recovery = Not calculated		
Mo 202.031†	23.4 0.7368 µg/L	0.21697 0.7368 ppb	0.21697 29.45%
QC value within limits for Mo 202.031	Recovery = Not calculated		
Na 589.592 Radial†	-147.6 -22.610 µg/L	7.2970 -22.610 ppb	7.2970 32.27%
QC value within limits for Na 589.592 Radial	Recovery = Not calculated		
Ni 231.604†	0.8 0.0104 µg/L	0.31844 0.0104 ppb	0.31844 >999.9%
QC value within limits for Ni 231.604	Recovery = Not calculated		
P 214.914†	-25.1 -6.0172 µg/L	3.48607 -6.0172 ppb	3.48607 57.93%
QC value within limits for P 214.914	Recovery = Not calculated		
Pb 220.353†	-15.2 -0.9198 µg/L	0.28391 -0.9198 ppb	0.28391 30.87%
QC value within limits for Pb 220.353	Recovery = Not calculated		
S 181.975 Axial†	-15.7 -12.716 µg/L	1.4469 -12.716 ppb	1.4469 11.38%
QC value within limits for S 181.975 Axial	Recovery = Not calculated		
Sb 206.836†	-7.2 -0.9580 µg/L	1.37341 -0.9580 ppb	1.37341 143.36%
QC value within limits for Sb 206.836	Recovery = Not calculated		
Se 196.026†	5.2 2.08 µg/L	5.305 2.08 ppb	5.305 255.01%
QC value within limits for Se 196.026	Recovery = Not calculated		
SiO2†	6.9 0.7311 µg/L	0.14916 0.7311 ppb	0.14916 20.40%
QC value within limits for SiO2	Recovery = Not calculated		
Si 251.611†	70.1 1.1487 µg/L	0.26000 1.1487 ppb	0.26000 22.64%
QC value within limits for Si 251.611	Recovery = Not calculated		
Sn 189.927†	2.6 0.1884 µg/L	0.18007 0.1884 ppb	0.18007 95.55%
QC value within limits for Sn 189.927	Recovery = Not calculated		
Sr 421.552†	96.4 0.2258 µg/L	0.18764 0.2258 ppb	0.18764 83.09%
QC value within limits for Sr 421.552	Recovery = Not calculated		
Ti 334.940†	188.1 0.1905 µg/L	0.05374 0.1905 ppb	0.05374 28.21%
QC value within limits for Ti 334.940	Recovery = Not calculated		
Tl 190.801†	13.7 1.8394 µg/L	0.82412 1.8394 ppb	0.82412 44.80%
QC value within limits for Tl 190.801	Recovery = Not calculated		
U 409.014†	91.9 5.6202 µg/L	3.25513 5.6202 ppb	3.25513 57.92%
QC value within limits for U 409.014	Recovery = Not calculated		
V 292.402†	-178.5 -0.9796 µg/L	0.08622 -0.9796 ppb	0.08622 8.80%
QC value within limits for V 292.402	Recovery = Not calculated		
Zn 213.857†	21.8 0.1370 µg/L	0.10743 0.1370 ppb	0.10743 78.42%
QC value within limits for Zn 213.857	Recovery = Not calculated		

All analyte(s) passed QC.

Sequence No.: 28

Sample ID: CCV

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 7

Date Collected: 3/29/2010 20:14:40

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCV

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	158830.4	158830.4	109 %		20:15:13
1	Al 396.153Radial†	25834.9	23739.9	5159.6 µg/L	5159.6 ppb	20:15:13
1	Ca 317.933Radial†	92141.6	83939.6	4918.5 µg/L	4918.5 ppb	20:15:13
1	Fe 238.204 Radial†	80227.4	73509.2	4887.1 µg/L	4887.1 ppb	20:15:13
1	K 766.490 Radial†	14250.9	11622.7	4780.8 µg/L	4780.8 ppb	20:15:13
1	Mg 279.077 IEC†	13509.5	12210.6	5042.2 µg/L	5042.2 ppb	20:15:13
1	Na 589.592 Radial†	71473.6	63894.6	9772.4 µg/L	9772.4 ppb	20:15:13
1	Sr 421.552†	233067.3	214157.3	501.89 µg/L	501.89 ppb	20:15:11
1	Sc 361.383	1758890.2	1758890.2	105.15 %		20:15:40
1	Y 371.029	1068006.2	1068006.2	104.44 %		20:15:40
1	Ag 328.068†	130795.7	121424.9	498.97 µg/L	498.97 ppb	20:15:40
1	As 188.979†	1305.1	1255.5	531.78 µg/L	531.78 ppb	20:16:00
1	B 249.677†	33757.2	28748.7	480.95 µg/L	480.95 ppb	20:15:40
1	Ba 233.527†	115387.0	109912.7	502.52 µg/L	502.52 ppb	20:15:40
1	Be 313.107†	1647211.3	1567223.6	510.30 µg/L	510.30 ppb	20:15:40
1	Cd 226.502†	73776.2	70258.5	484.88 µg/L	484.88 ppb	20:15:40
1	Co 228.616†	37405.4	35750.6	489.80 µg/L	489.80 ppb	20:15:40
1	Cr 267.716†	60425.3	57306.6	492.09 µg/L	492.09 ppb	20:15:40
1	Cu 324.752†	122063.0	113661.9	495.62 µg/L	495.62 ppb	20:15:40
1	Mn 257.610†	380412.8	361707.7	494.04 µg/L	494.04 ppb	20:15:40
1	Mo 202.031†	16080.3	15348.2	484.94 µg/L	484.94 ppb	20:16:00
1	Ni 231.604†	40320.7	38387.5	491.02 µg/L	491.02 ppb	20:15:40
1	P 214.914†	10614.3	10015.1	2390.0 µg/L	2390.0 ppb	20:16:00
1	Pb 220.353†	8478.6	7951.1	483.21 µg/L	483.21 ppb	20:16:00
1	S 181.975 Axial†	1339.7	1179.2	959.49 µg/L	959.49 ppb	20:16:00
1	Sb 206.836†	3893.5	3616.2	488.83 µg/L	488.83 ppb	20:16:00
1	Se 196.026†	1283.0	1209.3	480 µg/L	480 ppb	20:16:00
1	SiO2†	52444.4	48303.9	5258.8 µg/L	5258.8 ppb	20:15:40
1	Si 251.611†	157396.1	149013.5	2454.2 µg/L	2454.2 ppb	20:15:40
1	Sn 189.927†	7240.5	6884.0	491.06 µg/L	491.06 ppb	20:16:00
1	Ti 334.940†	511382.1	485708.4	494.63 µg/L	494.63 ppb	20:15:40
1	Tl 190.801†	3660.5	3601.6	490.88 µg/L	490.88 ppb	20:16:00
1	U 409.014†	7375.4	7493.4	493.30 µg/L	493.30 ppb	20:15:40
1	V 292.402†	94413.5	89359.2	501.88 µg/L	501.88 ppb	20:15:40
1	Zn 213.857†	81706.6	77241.8	482.36 µg/L	482.36 ppb	20:15:40
2	Sc RADIAL	157495.3	157495.3	108 %		20:15:18
2	Al 396.153Radial†	25706.5	23822.0	5177.5 µg/L	5177.5 ppb	20:15:18
2	Ca 317.933Radial†	91510.6	84072.4	4926.3 µg/L	4926.3 ppb	20:15:18
2	Fe 238.204 Radial†	79745.5	73687.3	4899.0 µg/L	4899.0 ppb	20:15:18
2	K 766.490 Radial†	14109.0	11602.1	4772.3 µg/L	4772.3 ppb	20:15:18
2	Mg 279.077 IEC†	13430.6	12242.7	5055.5 µg/L	5055.5 ppb	20:15:18
2	Na 589.592 Radial†	70962.0	63977.1	9785.1 µg/L	9785.1 ppb	20:15:18
2	Sr 421.552†	232192.9	215161.2	504.24 µg/L	504.24 ppb	20:15:16
2	Sc 361.383	1762035.0	1762035.0	105.34 %		20:16:04
2	Y 371.029	1068713.1	1068713.1	104.51 %		20:16:04
2	Ag 328.068†	130782.3	121190.1	498.00 µg/L	498.00 ppb	20:16:04
2	As 188.979†	1306.9	1255.0	531.56 µg/L	531.56 ppb	20:16:24
2	B 249.677†	33992.4	28914.7	483.74 µg/L	483.74 ppb	20:16:04
2	Ba 233.527†	115511.3	109834.8	502.16 µg/L	502.16 ppb	20:16:04
2	Be 313.107†	1645684.7	1562978.3	508.91 µg/L	508.91 ppb	20:16:04
2	Cd 226.502†	74022.3	70366.9	485.63 µg/L	485.63 ppb	20:16:04
2	Co 228.616†	37443.2	35723.0	489.42 µg/L	489.42 ppb	20:16:04
2	Cr 267.716†	60364.6	57146.4	490.71 µg/L	490.71 ppb	20:16:04
2	Cu 324.752†	122082.7	113473.4	494.80 µg/L	494.80 ppb	20:16:04
2	Mn 257.610†	380150.5	360813.0	492.82 µg/L	492.82 ppb	20:16:04
2	Mo 202.031†	16156.3	15393.1	486.35 µg/L	486.35 ppb	20:16:24
2	Ni 231.604†	40290.4	38290.3	489.78 µg/L	489.78 ppb	20:16:04
2	P 214.914†	10621.1	10003.5	2387.2 µg/L	2387.2 ppb	20:16:24
2	Pb 220.353†	8535.7	7990.8	485.62 µg/L	485.62 ppb	20:16:24

2	S 181.975 Axial†	1326.2	1164.2	947.33 µg/L	947.33 ppb	20:16:24
2	Sb 206.836†	3900.6	3616.4	488.88 µg/L	488.88 ppb	20:16:24
2	Se 196.026†	1284.8	1208.8	480 µg/L	480 ppb	20:16:24
2	SiO2†	52491.8	48259.9	5253.9 µg/L	5253.9 ppb	20:16:04
2	Si 251.611†	157382.7	148733.6	2449.6 µg/L	2449.6 ppb	20:16:04
2	Sn 189.927†	7227.9	6859.8	489.33 µg/L	489.33 ppb	20:16:24
2	Ti 334.940†	511020.6	484497.1	493.40 µg/L	493.40 ppb	20:16:04
2	Tl 190.801†	3689.6	3623.0	493.72 µg/L	493.72 ppb	20:16:24
2	U 409.014†	7356.3	7462.8	491.32 µg/L	491.32 ppb	20:16:04
2	V 292.402†	94327.3	89117.0	500.55 µg/L	500.55 ppb	20:16:04
2	Zn 213.857†	81870.2	77258.4	482.47 µg/L	482.47 ppb	20:16:04
3	Sc RADIAL	156537.6	156537.6	107 %		20:15:22
3	Al 396.153Radial†	25645.9	23911.1	5196.9 µg/L	5196.9 ppb	20:15:22
3	Ca 317.933Radial†	91188.8	84290.9	4939.1 µg/L	4939.1 ppb	20:15:22
3	Fe 238.204 Radial†	79529.7	73937.9	4915.6 µg/L	4915.6 ppb	20:15:22
3	K 766.490 Radial†	14092.0	11666.3	4798.7 µg/L	4798.7 ppb	20:15:22
3	Mg 279.077 IEC†	13237.8	12139.2	5012.8 µg/L	5012.8 ppb	20:15:22
3	Na 589.592 Radial†	70964.3	64381.0	9846.9 µg/L	9846.9 ppb	20:15:22
3	Sr 421.552†	233615.3	217800.3	510.43 µg/L	510.43 ppb	20:15:20
3	Sc 361.383	1760601.0	1760601.0	105.25 %		20:16:27
3	Y 371.029	1068160.3	1068160.3	104.46 %		20:16:27
3	Ag 328.068†	130523.2	121045.1	497.39 µg/L	497.39 ppb	20:16:27
3	As 188.979†	1312.2	1261.0	534.08 µg/L	534.08 ppb	20:16:47
3	B 249.677†	33684.6	28648.5	479.28 µg/L	479.28 ppb	20:16:27
3	Ba 233.527†	115155.8	109586.4	501.03 µg/L	501.03 ppb	20:16:27
3	Be 313.107†	1645527.7	1564101.6	509.28 µg/L	509.28 ppb	20:16:27
3	Cd 226.502†	73929.1	70335.6	485.41 µg/L	485.41 ppb	20:16:27
3	Co 228.616†	37338.0	35652.0	488.45 µg/L	488.45 ppb	20:16:27
3	Cr 267.716†	60447.8	57272.2	491.80 µg/L	491.80 ppb	20:16:27
3	Cu 324.752†	121740.8	113243.0	493.79 µg/L	493.79 ppb	20:16:27
3	Mn 257.610†	379672.2	360652.5	492.60 µg/L	492.60 ppb	20:16:27
3	Mo 202.031†	16168.3	15416.9	487.10 µg/L	487.10 ppb	20:16:47
3	Ni 231.604†	40268.9	38301.0	489.91 µg/L	489.91 ppb	20:16:27
3	P 214.914†	10675.3	10063.2	2401.6 µg/L	2401.6 ppb	20:16:47
3	Pb 220.353†	8520.4	7982.9	485.15 µg/L	485.15 ppb	20:16:47
3	S 181.975 Axial†	1321.3	1160.6	944.41 µg/L	944.41 ppb	20:16:47
3	Sb 206.836†	3929.7	3647.1	493.02 µg/L	493.02 ppb	20:16:47
3	Se 196.026†	1275.2	1200.7	477 µg/L	477 ppb	20:16:47
3	SiO2†	52357.5	48172.8	5244.4 µg/L	5244.4 ppb	20:16:27
3	Si 251.611†	157210.8	148692.0	2448.9 µg/L	2448.9 ppb	20:16:27
3	Sn 189.927†	7259.6	6895.4	491.87 µg/L	491.87 ppb	20:16:47
3	Ti 334.940†	509954.6	483879.4	492.77 µg/L	492.77 ppb	20:16:27
3	Tl 190.801†	3695.1	3631.0	494.80 µg/L	494.80 ppb	20:16:47
3	U 409.014†	7240.3	7358.2	484.82 µg/L	484.82 ppb	20:16:27
3	V 292.402†	94156.3	89027.6	500.06 µg/L	500.06 ppb	20:16:27
3	Zn 213.857†	81777.8	77234.0	482.31 µg/L	482.31 ppb	20:16:27

Mean Data: CCV

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1760508.7	105.24 %	0.094			0.09%
Sc RADIAL	157621.1	108 %	0.8			0.73%
Y 371.029	1068293.2	104.47 %	0.036			0.03%
Ag 328.068†	121220.0	498.12 µg/L	0.794	498.12 ppb	0.794	0.16%
QC value within limits for Ag 328.068 Recovery = 99.62%						
Al 396.153Radial†	23824.3	5178.0 µg/L	18.65	5178.0 ppb	18.65	0.36%
QC value within limits for Al 396.153Radial Recovery = 103.56%						
As 188.979†	1257.1	532.47 µg/L	1.398	532.47 ppb	1.398	0.26%
QC value within limits for As 188.979 Recovery = 106.49%						
B 249.677†	28770.7	481.32 µg/L	2.255	481.32 ppb	2.255	0.47%
QC value within limits for B 249.677 Recovery = 96.26%						
Ba 233.527†	109778.0	501.91 µg/L	0.779	501.91 ppb	0.779	0.16%
QC value within limits for Ba 233.527 Recovery = 100.38%						
Be 313.107†	1564767.8	509.50 µg/L	0.717	509.50 ppb	0.717	0.14%
QC value within limits for Be 313.107 Recovery = 101.90%						
Ca 317.933Radial†	84101.0	4928.0 µg/L	10.39	4928.0 ppb	10.39	0.21%
QC value within limits for Ca 317.933Radial Recovery = 98.56%						
Cd 226.502†	70320.3	485.30 µg/L	0.384	485.30 ppb	0.384	0.08%
QC value within limits for Cd 226.502 Recovery = 97.06%						
Co 228.616†	35708.6	489.22 µg/L	0.698	489.22 ppb	0.698	0.14%

QC value within limits for Co 228.616 Recovery = 97.84%							
Cr 267.716†	57241.7	491.53 µg/L	0.725	491.53 ppb	0.725	0.15%	
QC value within limits for Cr 267.716 Recovery = 98.31%							
Cu 324.752†	113459.4	494.74 µg/L	0.914	494.74 ppb	0.914	0.18%	
QC value within limits for Cu 324.752 Recovery = 98.95%							
Fe 238.204 Radial†	73711.5	4900.6 µg/L	14.32	4900.6 ppb	14.32	0.29%	
QC value within limits for Fe 238.204 Radial Recovery = 98.01%							
K 766.490 Radial†	11630.4	4783.9 µg/L	13.48	4783.9 ppb	13.48	0.28%	
QC value within limits for K 766.490 Radial Recovery = 95.68%							
Mg 279.077 IEC†	12197.5	5036.8 µg/L	21.85	5036.8 ppb	21.85	0.43%	
QC value within limits for Mg 279.077 IEC Recovery = 100.74%							
Mn 257.610†	361057.7	493.15 µg/L	0.777	493.15 ppb	0.777	0.16%	
QC value within limits for Mn 257.610 Recovery = 98.63%							
Mo 202.031†	15386.1	486.13 µg/L	1.101	486.13 ppb	1.101	0.23%	
QC value within limits for Mo 202.031 Recovery = 97.23%							
Na 589.592 Radial†	64084.3	9801.5 µg/L	39.82	9801.5 ppb	39.82	0.41%	
QC value within limits for Na 589.592 Radial Recovery = 98.01%							
Ni 231.604†	38326.3	490.24 µg/L	0.682	490.24 ppb	0.682	0.14%	
QC value within limits for Ni 231.604 Recovery = 98.05%							
P 214.914†	10027.2	2392.9 µg/L	7.59	2392.9 ppb	7.59	0.32%	
QC value within limits for P 214.914 Recovery = 95.72%							
Pb 220.353†	7974.9	484.66 µg/L	1.279	484.66 ppb	1.279	0.26%	
QC value within limits for Pb 220.353 Recovery = 96.93%							
S 181.975 Axial†	1168.0	950.41 µg/L	8.003	950.41 ppb	8.003	0.84%	
QC value within limits for S 181.975 Axial Recovery = 95.04%							
Sb 206.836†	3626.6	490.24 µg/L	2.403	490.24 ppb	2.403	0.49%	
QC value within limits for Sb 206.836 Recovery = 98.05%							
Se 196.026†	1206.3	479 µg/L	1.9	479 ppb	1.9	0.40%	
QC value within limits for Se 196.026 Recovery = 95.86%							
SiO2†	48245.5	5252.4 µg/L	7.33	5252.4 ppb	7.33	0.14%	
QC value within limits for SiO2 Recovery = 98.22%							
Si 251.611†	148813.1	2450.9 µg/L	2.90	2450.9 ppb	2.90	0.12%	
QC value within limits for Si 251.611 Recovery = 98.04%							
Sn 189.927†	6879.7	490.75 µg/L	1.293	490.75 ppb	1.293	0.26%	
QC value within limits for Sn 189.927 Recovery = 98.15%							
Sr 421.552†	215706.3	505.52 µg/L	4.410	505.52 ppb	4.410	0.87%	
QC value within limits for Sr 421.552 Recovery = 101.10%							
Ti 334.940†	484695.0	493.60 µg/L	0.946	493.60 ppb	0.946	0.19%	
QC value within limits for Ti 334.940 Recovery = 98.72%							
Tl 190.801†	3618.5	493.13 µg/L	2.027	493.13 ppb	2.027	0.41%	
QC value within limits for Tl 190.801 Recovery = 98.63%							
U 409.014†	7438.1	489.81 µg/L	4.433	489.81 ppb	4.433	0.91%	
QC value within limits for U 409.014 Recovery = 97.96%							
V 292.402†	89167.9	500.83 µg/L	0.945	500.83 ppb	0.945	0.19%	
QC value within limits for V 292.402 Recovery = 100.17%							
Zn 213.857†	77244.7	482.38 µg/L	0.080	482.38 ppb	0.080	0.02%	
QC value within limits for Zn 213.857 Recovery = 96.48%							
All analyte(s) passed QC.							

Sequence No.: 29

Sample ID: CCB

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 8

Date Collected: 3/29/2010 20:16:54

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCB

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	158157.7	158157.7	109 %		20:17:23
1	Al 396.153Radial†	-63.6	-26.8	-5.8638 µg/L	-5.8638 ppb	20:17:43
1	Ca 317.933Radial†	734.1	60.4	3.5365 µg/L	3.5365 ppb	20:17:43
1	Fe 238.204 Radial†	186.1	58.3	3.8728 µg/L	3.8728 ppb	20:17:43
1	K 766.490 Radial†	1649.8	65.4	26.926 µg/L	26.926 ppb	20:17:23
1	Mg 279.077 IEC†	176.6	-23.9	-9.8603 µg/L	-9.8603 ppb	20:17:43
1	Na 589.592 Radial†	1600.7	-219.6	-33.624 µg/L	-33.624 ppb	20:17:23
1	Sr 421.552†	-113.7	173.2	0.4058 µg/L	0.4058 ppb	20:17:23
1	Sc 361.383	1797162.4	1797162.4	107.44 %		20:18:45
1	Y 371.029	1101535.0	1101535.0	107.72 %		20:18:45
1	Ag 328.068†	3189.5	1.7	0.0181 µg/L	0.0181 ppb	20:18:47
1	As 188.979†	-18.7	-3.2	-1.3282 µg/L	-1.3282 ppb	20:19:07
1	B 249.677†	3164.5	-410.2	-6.8868 µg/L	-6.8868 ppb	20:19:07
1	Ba 233.527†	-166.3	20.3	0.0925 µg/L	0.0925 ppb	20:19:07
1	Be 313.107†	-796.9	-81.6	-0.0232 µg/L	-0.0232 ppb	20:18:47
1	Cd 226.502†	-88.5	12.1	0.0830 µg/L	0.0830 ppb	20:19:07
1	Co 228.616†	-182.6	6.7	0.0913 µg/L	0.0913 ppb	20:19:07
1	Cr 267.716†	146.8	-23.6	-0.2111 µg/L	-0.2111 ppb	20:19:07
1	Cu 324.752†	2533.1	-67.1	-0.2822 µg/L	-0.2822 ppb	20:18:47
1	Mn 257.610†	189.2	96.1	0.1316 µg/L	0.1316 ppb	20:19:07
1	Mo 202.031†	-43.6	14.6	0.4617 µg/L	0.4617 ppb	20:19:07
1	Ni 231.604†	-36.3	7.1	0.0912 µg/L	0.0912 ppb	20:19:07
1	P 214.914†	33.9	-48.0	-11.496 µg/L	-11.496 ppb	20:19:07
1	Pb 220.353†	106.6	-13.2	-0.8080 µg/L	-0.8080 ppb	20:19:07
1	S 181.975 Axial†	94.0	-7.3	-5.9118 µg/L	-5.9118 ppb	20:19:07
1	Sb 206.836†	77.5	-14.5	-1.9423 µg/L	-1.9423 ppb	20:19:07
1	Se 196.026†	26.1	13.3	5.29 µg/L	5.29 ppb	20:19:07
1	SiO2†	1703.2	12.4	1.3407 µg/L	1.3407 ppb	20:19:07
1	Si 251.611†	757.0	28.3	0.4592 µg/L	0.4592 ppb	20:19:07
1	Sn 189.927†	6.4	3.9	0.2796 µg/L	0.2796 ppb	20:19:07
1	Ti 334.940†	1092.2	380.2	0.3841 µg/L	0.3841 ppb	20:18:47
1	Tl 190.801†	-110.1	17.8	2.3981 µg/L	2.3981 ppb	20:19:07
1	U 409.014†	-322.2	179.2	11.064 µg/L	11.064 ppb	20:18:47
1	V 292.402†	429.3	-32.2	-0.1685 µg/L	-0.1685 ppb	20:18:47
1	Zn 213.857†	497.4	-1.5	-0.0099 µg/L	-0.0099 ppb	20:19:07
2	Sc RADIAL	155691.2	155691.2	107 %		20:17:45
2	Al 396.153Radial†	-30.3	3.5	0.7196 µg/L	0.7196 ppb	20:18:05
2	Ca 317.933Radial†	713.2	51.5	3.0148 µg/L	3.0148 ppb	20:18:05
2	Fe 238.204 Radial†	162.5	38.8	2.5826 µg/L	2.5826 ppb	20:18:05
2	K 766.490 Radial†	1523.5	-28.7	-11.809 µg/L	-11.809 ppb	20:17:45
2	Mg 279.077 IEC†	195.4	-3.7	-1.5189 µg/L	-1.5189 ppb	20:18:05
2	Na 589.592 Radial†	1538.6	-254.3	-38.906 µg/L	-38.906 ppb	20:17:45
2	Sr 421.552†	-172.2	116.8	0.2737 µg/L	0.2737 ppb	20:17:45
2	Sc 361.383	1776190.8	1776190.8	106.18 %		20:19:09
2	Y 371.029	1089581.5	1089581.5	106.55 %		20:19:09
2	Ag 328.068†	3209.2	55.3	0.2233 µg/L	0.2233 ppb	20:19:11
2	As 188.979†	-18.8	-3.4	-1.4319 µg/L	-1.4319 ppb	20:19:31
2	B 249.677†	3163.9	-376.0	-6.3128 µg/L	-6.3128 ppb	20:19:31
2	Ba 233.527†	-158.5	25.8	0.1177 µg/L	0.1177 ppb	20:19:31
2	Be 313.107†	-622.2	74.1	0.0253 µg/L	0.0253 ppb	20:19:11
2	Cd 226.502†	-71.9	26.7	0.1839 µg/L	0.1839 ppb	20:19:31
2	Co 228.616†	-183.6	3.7	0.0500 µg/L	0.0500 ppb	20:19:31
2	Cr 267.716†	166.1	-3.8	-0.0355 µg/L	-0.0355 ppb	20:19:31
2	Cu 324.752†	2626.6	48.8	0.2155 µg/L	0.2155 ppb	20:19:11
2	Mn 257.610†	203.0	111.2	0.1519 µg/L	0.1519 ppb	20:19:31
2	Mo 202.031†	-29.4	27.5	0.8686 µg/L	0.8686 ppb	20:19:31
2	Ni 231.604†	-58.1	-13.8	-0.1766 µg/L	-0.1766 ppb	20:19:31
2	P 214.914†	38.3	-43.5	-10.438 µg/L	-10.438 ppb	20:19:31
2	Pb 220.353†	142.1	21.4	1.2928 µg/L	1.2928 ppb	20:19:31

2	S 181.975 Axial†	84.7	-15.1	-12.191 µg/L	-12.191 ppb	20:19:31
2	Sb 206.836†	90.2	-1.7	-0.2231 µg/L	-0.2231 ppb	20:19:31
2	Se 196.026†	16.7	4.8	1.90 µg/L	1.90 ppb	20:19:31
2	SiO2†	1687.5	16.4	1.7745 µg/L	1.7745 ppb	20:19:31
2	Si 251.611†	744.1	24.4	0.3950 µg/L	0.3950 ppb	20:19:31
2	Sn 189.927†	-5.5	-7.2	-0.5152 µg/L	-0.5152 ppb	20:19:31
2	Ti 334.940†	590.2	-80.5	-0.0834 µg/L	-0.0834 ppb	20:19:11
2	Tl 190.801†	-116.1	11.0	1.4736 µg/L	1.4736 ppb	20:19:31
2	U 409.014†	-444.6	60.4	3.7028 µg/L	3.7028 ppb	20:19:11
2	V 292.402†	365.2	-87.9	-0.4766 µg/L	-0.4766 ppb	20:19:11
2	Zn 213.857†	508.8	14.8	0.0938 µg/L	0.0938 ppb	20:19:31
3	Sc RADIAL	155889.7	155889.7	107 %		20:18:07
3	Al 396.153Radial†	-21.6	11.7	2.4989 µg/L	2.4989 ppb	20:18:27
3	Ca 317.933Radial†	710.6	48.2	2.8268 µg/L	2.8268 ppb	20:18:27
3	Fe 238.204 Radial†	176.6	51.8	3.4464 µg/L	3.4464 ppb	20:18:27
3	K 766.490 Radial†	1522.8	-31.2	-12.835 µg/L	-12.835 ppb	20:18:07
3	Mg 279.077 IEC†	169.6	-28.1	-11.582 µg/L	-11.582 ppb	20:18:27
3	Na 589.592 Radial†	1514.3	-278.9	-42.658 µg/L	-42.658 ppb	20:18:07
3	Sr 421.552†	-115.2	170.3	0.3991 µg/L	0.3991 ppb	20:18:07
3	Sc 361.383	1775735.1	1775735.1	106.16 %		20:19:33
3	Y 371.029	1090212.1	1090212.1	106.61 %		20:19:33
3	Ag 328.068†	3310.5	151.5	0.6044 µg/L	0.6044 ppb	20:19:35
3	As 188.979†	-18.3	-3.0	-1.2478 µg/L	-1.2478 ppb	20:19:55
3	B 249.677†	3162.1	-376.9	-6.3290 µg/L	-6.3290 ppb	20:19:55
3	Ba 233.527†	-165.4	19.2	0.0872 µg/L	0.0872 ppb	20:19:55
3	Be 313.107†	-659.6	38.8	0.0140 µg/L	0.0140 ppb	20:19:35
3	Cd 226.502†	-97.0	3.1	0.0206 µg/L	0.0206 ppb	20:19:55
3	Co 228.616†	-161.6	24.4	0.3340 µg/L	0.3340 ppb	20:19:55
3	Cr 267.716†	177.4	6.9	0.0553 µg/L	0.0553 ppb	20:19:55
3	Cu 324.752†	2774.4	188.7	0.8244 µg/L	0.8244 ppb	20:19:35
3	Mn 257.610†	182.4	91.8	0.1259 µg/L	0.1259 ppb	20:19:55
3	Mo 202.031†	-25.4	31.3	0.9879 µg/L	0.9879 ppb	20:19:55
3	Ni 231.604†	-68.5	-23.6	-0.3019 µg/L	-0.3019 ppb	20:19:55
3	P 214.914†	51.6	-31.0	-7.4391 µg/L	-7.4391 ppb	20:19:55
3	Pb 220.353†	84.6	-32.7	-1.9844 µg/L	-1.9844 ppb	20:19:55
3	S 181.975 Axial†	85.3	-14.4	-11.697 µg/L	-11.697 ppb	20:19:55
3	Sb 206.836†	54.5	-35.3	-4.7507 µg/L	-4.7507 ppb	20:19:55
3	Se 196.026†	0.8	-10.1	-4.01 µg/L	-4.01 ppb	20:19:55
3	SiO2†	1675.1	5.1	0.5352 µg/L	0.5352 ppb	20:19:55
3	Si 251.611†	757.0	36.7	0.5978 µg/L	0.5978 ppb	20:19:55
3	Sn 189.927†	-6.1	-7.8	-0.5522 µg/L	-0.5522 ppb	20:19:55
3	Ti 334.940†	761.4	80.9	0.0816 µg/L	0.0816 ppb	20:19:35
3	Tl 190.801†	-108.3	18.3	2.4419 µg/L	2.4419 ppb	20:19:55
3	U 409.014†	-429.2	74.8	4.5456 µg/L	4.5456 ppb	20:19:35
3	V 292.402†	201.6	-241.9	-1.3288 µg/L	-1.3288 ppb	20:19:35
3	Zn 213.857†	514.6	20.3	0.1291 µg/L	0.1291 ppb	20:19:55

Mean Data: CCB

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1783029.4	106.59 %	0.732			0.69%
Sc RADIAL	156579.5	107 %	0.9			0.88%
Y 371.029	1093776.2	106.96 %	0.658			0.61%
Ag 328.068†	69.5	0.2819 µg/L	0.29754	0.2819 ppb	0.29754	105.55%
QC value within limits for Ag 328.068 Recovery = Not calculated						
Al 396.153Radial†	-3.9	-0.8818 µg/L	4.40531	-0.8818 ppb	4.40531	499.59%
QC value within limits for Al 396.153Radial Recovery = Not calculated						
As 188.979†	-3.2	-1.3360 µg/L	0.09228	-1.3360 ppb	0.09228	6.91%
QC value within limits for As 188.979 Recovery = Not calculated						
B 249.677†	-387.7	-6.5095 µg/L	0.32684	-6.5095 ppb	0.32684	5.02%
QC value within limits for B 249.677 Recovery = Not calculated						
Ba 233.527†	21.7	0.0991 µg/L	0.01628	0.0991 ppb	0.01628	16.43%
QC value within limits for Ba 233.527 Recovery = Not calculated						
Be 313.107†	10.4	0.0053 µg/L	0.02537	0.0053 ppb	0.02537	474.55%
QC value within limits for Be 313.107 Recovery = Not calculated						
Ca 317.933Radial†	53.3	3.1261 µg/L	0.36770	3.1261 ppb	0.36770	11.76%
QC value within limits for Ca 317.933Radial Recovery = Not calculated						
Cd 226.502†	13.9	0.0958 µg/L	0.08241	0.0958 ppb	0.08241	85.99%
QC value within limits for Cd 226.502 Recovery = Not calculated						
Co 228.616†	11.6	0.1584 µg/L	0.15343	0.1584 ppb	0.15343	96.85%

QC value within limits for Co 228.616	Recovery = Not calculated		
Cr 267.716†	-6.8 -0.0638 µg/L	0.13543 -0.0638 ppb	0.13543 212.32%
QC value within limits for Cr 267.716	Recovery = Not calculated		
Cu 324.752†	56.8 0.2526 µg/L	0.55423 0.2526 ppb	0.55423 219.45%
QC value within limits for Cu 324.752	Recovery = Not calculated		
Fe 238.204 Radial†	49.6 3.3006 µg/L	0.65736 3.3006 ppb	0.65736 19.92%
QC value within limits for Fe 238.204 Radial	Recovery = Not calculated		
K 766.490 Radial†	1.8 0.7609 µg/L	22.66551 0.7609 ppb	22.66551 >999.9%
QC value within limits for K 766.490 Radial	Recovery = Not calculated		
Mg 279.077 IEC†	-18.6 -7.6537 µg/L	5.38218 -7.6537 ppb	5.38218 70.32%
QC value within limits for Mg 279.077 IEC	Recovery = Not calculated		
Mn 257.610†	99.7 0.1365 µg/L	0.01367 0.1365 ppb	0.01367 10.02%
QC value within limits for Mn 257.610	Recovery = Not calculated		
Mo 202.031†	24.5 0.7728 µg/L	0.27588 0.7728 ppb	0.27588 35.70%
QC value within limits for Mo 202.031	Recovery = Not calculated		
Na 589.592 Radial†	-250.9 -38.396 µg/L	4.5384 -38.396 ppb	4.5384 11.82%
QC value within limits for Na 589.592 Radial	Recovery = Not calculated		
Ni 231.604†	-10.1 -0.1291 µg/L	0.20080 -0.1291 ppb	0.20080 155.54%
QC value within limits for Ni 231.604	Recovery = Not calculated		
P 214.914†	-40.8 -9.7910 µg/L	2.10426 -9.7910 ppb	2.10426 21.49%
QC value within limits for P 214.914	Recovery = Not calculated		
Pb 220.353†	-8.2 -0.4998 µg/L	1.66019 -0.4998 ppb	1.66019 332.15%
QC value within limits for Pb 220.353	Recovery = Not calculated		
S 181.975 Axial†	-12.3 -9.9332 µg/L	3.49134 -9.9332 ppb	3.49134 35.15%
QC value within limits for S 181.975 Axial	Recovery = Not calculated		
Sb 206.836†	-17.2 -2.3053 µg/L	2.28550 -2.3053 ppb	2.28550 99.14%
QC value within limits for Sb 206.836	Recovery = Not calculated		
Se 196.026†	2.7 1.06 µg/L	4.705 1.06 ppb	4.705 444.44%
QC value within limits for Se 196.026	Recovery = Not calculated		
SiO2†	11.3 1.2168 µg/L	0.62889 1.2168 ppb	0.62889 51.68%
QC value within limits for SiO2	Recovery = Not calculated		
Si 251.611†	29.8 0.4840 µg/L	0.10365 0.4840 ppb	0.10365 21.42%
QC value within limits for Si 251.611	Recovery = Not calculated		
Sn 189.927†	-3.7 -0.2626 µg/L	0.46990 -0.2626 ppb	0.46990 178.94%
QC value within limits for Sn 189.927	Recovery = Not calculated		
Sr 421.552†	153.4 0.3595 µg/L	0.07442 0.3595 ppb	0.07442 20.70%
QC value within limits for Sr 421.552	Recovery = Not calculated		
Ti 334.940†	126.9 0.1275 µg/L	0.23711 0.1275 ppb	0.23711 186.03%
QC value within limits for Ti 334.940	Recovery = Not calculated		
Tl 190.801†	15.7 2.1045 µg/L	0.54683 2.1045 ppb	0.54683 25.98%
QC value within limits for Tl 190.801	Recovery = Not calculated		
U 409.014†	104.8 6.4375 µg/L	4.02889 6.4375 ppb	4.02889 62.58%
QC value within limits for U 409.014	Recovery = Not calculated		
V 292.402†	-120.7 -0.6580 µg/L	0.60105 -0.6580 ppb	0.60105 91.35%
QC value within limits for V 292.402	Recovery = Not calculated		
Zn 213.857†	11.2 0.0710 µg/L	0.07224 0.0710 ppb	0.07224 101.73%
QC value within limits for Zn 213.857	Recovery = Not calculated		

All analyte(s) passed QC.

Sequence No.: 37

Sample ID: CCV

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 7

Date Collected: 3/29/2010 20:39:13

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCV

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	158480.3	158480.3	109 %		20:39:46
1	Al 396.153Radial†	25899.3	23851.4	5184.2 µg/L	5184.2 ppb	20:39:46
1	Ca 317.933Radial†	91372.8	83419.3	4888.0 µg/L	4888.0 ppb	20:39:46
1	Fe 238.204 Radial†	79864.5	73338.0	4875.8 µg/L	4875.8 ppb	20:39:46
1	K 766.490 Radial†	13976.2	11398.9	4688.7 µg/L	4688.7 ppb	20:39:46
1	Mg 279.077 IEC†	13513.6	12241.7	5054.9 µg/L	5054.9 ppb	20:39:46
1	Na 589.592 Radial†	70984.5	63589.7	9725.9 µg/L	9725.9 ppb	20:39:46
1	Sr 421.552†	231158.4	212874.2	498.88 µg/L	498.88 ppb	20:39:44
1	Sc 361.383	1746203.9	1746203.9	104.39 %		20:40:13
1	Y 371.029	1060403.2	1060403.2	103.70 %		20:40:13
1	Ag 328.068†	129222.9	120821.9	496.49 µg/L	496.49 ppb	20:40:13
1	As 188.979†	1283.9	1244.1	526.99 µg/L	526.99 ppb	20:40:33
1	B 249.677†	33276.5	28521.6	477.15 µg/L	477.15 ppb	20:40:13
1	Ba 233.527†	114363.4	109729.4	501.68 µg/L	501.68 ppb	20:40:13
1	Be 313.107†	1632572.9	1564581.9	509.43 µg/L	509.43 ppb	20:40:13
1	Cd 226.502†	72628.8	69669.1	480.81 µg/L	480.81 ppb	20:40:13
1	Co 228.616†	36875.4	35501.3	486.39 µg/L	486.39 ppb	20:40:13
1	Cr 267.716†	59790.0	57115.6	490.45 µg/L	490.45 ppb	20:40:13
1	Cu 324.752†	120808.8	113303.8	494.05 µg/L	494.05 ppb	20:40:13
1	Mn 257.610†	375213.3	359355.3	490.82 µg/L	490.82 ppb	20:40:13
1	Mo 202.031†	15789.8	15181.1	479.66 µg/L	479.66 ppb	20:40:33
1	Ni 231.604†	39738.4	38108.3	487.45 µg/L	487.45 ppb	20:40:13
1	P 214.914†	10363.4	9848.0	2350.1 µg/L	2350.1 ppb	20:40:33
1	Pb 220.353†	8305.0	7843.4	476.67 µg/L	476.67 ppb	20:40:33
1	S 181.975 Axial†	1299.5	1150.0	935.75 µg/L	935.75 ppb	20:40:33
1	Sb 206.836†	3827.9	3580.3	483.91 µg/L	483.91 ppb	20:40:33
1	Se 196.026†	1246.7	1183.4	470 µg/L	470 ppb	20:40:33
1	SiO2†	51835.7	48083.1	5234.9 µg/L	5234.9 ppb	20:40:13
1	Si 251.611†	155248.2	148043.5	2438.3 µg/L	2438.3 ppb	20:40:13
1	Sn 189.927†	7083.7	6783.8	483.93 µg/L	483.93 ppb	20:40:33
1	Ti 334.940†	505298.5	483413.9	492.29 µg/L	492.29 ppb	20:40:13
1	Tl 190.801†	3587.5	3556.9	484.85 µg/L	484.85 ppb	20:40:33
1	U 409.014†	7184.1	7361.1	484.98 µg/L	484.98 ppb	20:40:13
1	V 292.402†	93312.1	88956.4	499.59 µg/L	499.59 ppb	20:40:13
1	Zn 213.857†	80758.5	76898.2	480.22 µg/L	480.22 ppb	20:40:13
2	Sc RADIAL	157839.6	157839.6	108 %		20:39:50
2	Al 396.153Radial†	25654.3	23721.9	5156.0 µg/L	5156.0 ppb	20:39:50
2	Ca 317.933Radial†	90857.8	83284.8	4880.1 µg/L	4880.1 ppb	20:39:50
2	Fe 238.204 Radial†	79351.6	73162.6	4864.1 µg/L	4864.1 ppb	20:39:50
2	K 766.490 Radial†	14108.1	11572.9	4760.3 µg/L	4760.3 ppb	20:39:50
2	Mg 279.077 IEC†	13317.1	12110.8	5000.9 µg/L	5000.9 ppb	20:39:50
2	Na 589.592 Radial†	70889.1	63766.6	9752.9 µg/L	9752.9 ppb	20:39:50
2	Sr 421.552†	232019.8	214532.6	502.77 µg/L	502.77 ppb	20:39:48
2	Sc 361.383	1748401.5	1748401.5	104.52 %		20:40:36
2	Y 371.029	1060574.0	1060574.0	103.72 %		20:40:36
2	Ag 328.068†	128320.4	119802.8	492.33 µg/L	492.33 ppb	20:40:36
2	As 188.979†	1300.9	1258.8	533.09 µg/L	533.09 ppb	20:40:56
2	B 249.677†	33199.5	28407.7	475.25 µg/L	475.25 ppb	20:40:36
2	Ba 233.527†	113312.8	108586.5	496.46 µg/L	496.46 ppb	20:40:36
2	Be 313.107†	1626044.8	1556370.4	506.76 µg/L	506.76 ppb	20:40:36
2	Cd 226.502†	71814.6	68802.6	474.82 µg/L	474.82 ppb	20:40:36
2	Co 228.616†	36702.1	35291.2	483.50 µg/L	483.50 ppb	20:40:36
2	Cr 267.716†	59191.4	56470.8	484.90 µg/L	484.90 ppb	20:40:36
2	Cu 324.752†	120253.9	112627.4	491.11 µg/L	491.11 ppb	20:40:36
2	Mn 257.610†	372516.4	356323.3	486.68 µg/L	486.68 ppb	20:40:36
2	Mo 202.031†	15750.8	15124.7	477.88 µg/L	477.88 ppb	20:40:56
2	Ni 231.604†	39612.3	37939.8	485.29 µg/L	485.29 ppb	20:40:36
2	P 214.914†	10343.5	9816.5	2342.6 µg/L	2342.6 ppb	20:40:56
2	Pb 220.353†	8312.4	7840.4	476.48 µg/L	476.48 ppb	20:40:56

2	S 181.975 Axial†	1287.8	1137.3	925.44 µg/L	925.44 ppb	20:40:56
2	Sb 206.836†	3843.7	3590.8	485.39 µg/L	485.39 ppb	20:40:56
2	Se 196.026†	1243.8	1179.1	469 µg/L	469 ppb	20:40:56
2	SiO2†	51279.8	47488.8	5170.0 µg/L	5170.0 ppb	20:40:36
2	Si 251.611†	154265.1	146916.0	2419.7 µg/L	2419.7 ppb	20:40:36
2	Sn 189.927†	7111.0	6801.4	485.17 µg/L	485.17 ppb	20:40:56
2	Ti 334.940†	501677.3	479340.9	488.14 µg/L	488.14 ppb	20:40:36
2	Tl 190.801†	3591.8	3556.8	484.78 µg/L	484.78 ppb	20:40:56
2	U 409.014†	7373.9	7534.0	495.49 µg/L	495.49 ppb	20:40:36
2	V 292.402†	92934.7	88483.0	496.93 µg/L	496.93 ppb	20:40:36
2	Zn 213.857†	80169.9	76237.8	476.08 µg/L	476.08 ppb	20:40:36
3	Sc RADIAL	156089.6	156089.6	107 %		20:39:54
3	Al 396.153Radial†	25631.8	23966.5	5209.3 µg/L	5209.3 ppb	20:39:54
3	Ca 317.933Radial†	90218.0	83628.1	4900.2 µg/L	4900.2 ppb	20:39:54
3	Fe 238.204 Radial†	78756.2	73428.1	4881.8 µg/L	4881.8 ppb	20:39:54
3	K 766.490 Radial†	13885.5	11511.0	4734.8 µg/L	4734.8 ppb	20:39:54
3	Mg 279.077 IEC†	13155.9	12098.2	4995.8 µg/L	4995.8 ppb	20:39:54
3	Na 589.592 Radial†	70406.1	64049.4	9796.2 µg/L	9796.2 ppb	20:39:54
3	Sr 421.552†	227678.4	212880.7	498.90 µg/L	498.90 ppb	20:39:52
3	Sc 361.383	1750051.7	1750051.7	104.62 %		20:40:59
3	Y 371.029	1061656.2	1061656.2	103.82 %		20:40:59
3	Ag 328.068†	129101.5	120433.7	494.92 µg/L	494.92 ppb	20:40:59
3	As 188.979†	1318.4	1274.5	539.66 µg/L	539.66 ppb	20:41:19
3	B 249.677†	33442.7	28610.3	478.64 µg/L	478.64 ppb	20:40:59
3	Ba 233.527†	114533.5	109651.1	501.32 µg/L	501.32 ppb	20:40:59
3	Be 313.107†	1637681.6	1566026.4	509.91 µg/L	509.91 ppb	20:40:59
3	Cd 226.502†	72370.3	69269.0	478.04 µg/L	478.04 ppb	20:40:59
3	Co 228.616†	36966.6	35510.9	486.52 µg/L	486.52 ppb	20:40:59
3	Cr 267.716†	59644.0	56850.1	488.16 µg/L	488.16 ppb	20:40:59
3	Cu 324.752†	121321.2	113539.1	495.08 µg/L	495.08 ppb	20:40:59
3	Mn 257.610†	375810.6	359135.9	490.53 µg/L	490.53 ppb	20:40:59
3	Mo 202.031†	15874.8	15229.0	481.17 µg/L	481.17 ppb	20:41:19
3	Ni 231.604†	39836.0	38117.9	487.57 µg/L	487.57 ppb	20:40:59
3	P 214.914†	10423.7	9883.8	2358.6 µg/L	2358.6 ppb	20:41:19
3	Pb 220.353†	8358.7	7877.1	478.72 µg/L	478.72 ppb	20:41:19
3	S 181.975 Axial†	1303.9	1151.5	936.96 µg/L	936.96 ppb	20:41:19
3	Sb 206.836†	3860.5	3603.4	487.09 µg/L	487.09 ppb	20:41:19
3	Se 196.026†	1260.6	1194.1	474 µg/L	474 ppb	20:41:19
3	SiO2†	51807.0	47946.5	5219.9 µg/L	5219.9 ppb	20:40:59
3	Si 251.611†	155533.5	147989.2	2437.4 µg/L	2437.4 ppb	20:40:59
3	Sn 189.927†	7141.0	6823.7	486.76 µg/L	486.76 ppb	20:41:19
3	Ti 334.940†	505758.7	482789.5	491.66 µg/L	491.66 ppb	20:40:59
3	Tl 190.801†	3621.3	3581.7	488.18 µg/L	488.18 ppb	20:41:19
3	U 409.014†	7328.7	7484.2	492.60 µg/L	492.60 ppb	20:40:59
3	V 292.402†	93571.4	89007.7	499.88 µg/L	499.88 ppb	20:40:59
3	Zn 213.857†	80716.3	76687.7	478.89 µg/L	478.89 ppb	20:40:59

Mean Data: CCV

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1748219.0	104.51 %	0.115			0.11%
Sc RADIAL	157469.8	108 %	0.8			0.79%
Y 371.029	1060877.8	103.75 %	0.066			0.06%
Ag 328.068†	120352.8	494.58 µg/L	2.097	494.58 ppb	2.097	0.42%
QC value within limits for Ag 328.068 Recovery = 98.92%						
Al 396.153Radial†	23846.6	5183.2 µg/L	26.63	5183.2 ppb	26.63	0.51%
QC value within limits for Al 396.153Radial Recovery = 103.66%						
As 188.979†	1259.1	533.25 µg/L	6.336	533.25 ppb	6.336	1.19%
QC value within limits for As 188.979 Recovery = 106.65%						
B 249.677†	28513.2	477.02 µg/L	1.699	477.02 ppb	1.699	0.36%
QC value within limits for B 249.677 Recovery = 95.40%						
Ba 233.527†	109322.4	499.82 µg/L	2.918	499.82 ppb	2.918	0.58%
QC value within limits for Ba 233.527 Recovery = 99.96%						
Be 313.107†	1562326.2	508.70 µg/L	1.694	508.70 ppb	1.694	0.33%
QC value within limits for Be 313.107 Recovery = 101.74%						
Ca 317.933Radial†	83444.1	4889.5 µg/L	10.13	4889.5 ppb	10.13	0.21%
QC value within limits for Ca 317.933Radial Recovery = 97.79%						
Cd 226.502†	69246.9	477.89 µg/L	2.994	477.89 ppb	2.994	0.63%
QC value within limits for Cd 226.502 Recovery = 95.58%						
Co 228.616†	35434.5	485.47 µg/L	1.703	485.47 ppb	1.703	0.35%

QC value within limits for Co 228.616 Recovery = 97.09%						
Cr 267.716†	56812.2	487.84 µg/L	2.787	487.84 ppb	2.787	0.57%
QC value within limits for Cr 267.716 Recovery = 97.57%						
Cu 324.752†	113156.8	493.41 µg/L	2.057	493.41 ppb	2.057	0.42%
QC value within limits for Cu 324.752 Recovery = 98.68%						
Fe 238.204 Radial†	73309.6	4873.9 µg/L	8.98	4873.9 ppb	8.98	0.18%
QC value within limits for Fe 238.204 Radial Recovery = 97.48%						
K 766.490 Radial†	11494.3	4727.9 µg/L	36.31	4727.9 ppb	36.31	0.77%
QC value within limits for K 766.490 Radial Recovery = 94.56%						
Mg 279.077 IEC†	12150.2	5017.2 µg/L	32.78	5017.2 ppb	32.78	0.65%
QC value within limits for Mg 279.077 IEC Recovery = 100.34%						
Mn 257.610†	358271.5	489.35 µg/L	2.310	489.35 ppb	2.310	0.47%
QC value within limits for Mn 257.610 Recovery = 97.87%						
Mo 202.031†	15178.3	479.57 µg/L	1.650	479.57 ppb	1.650	0.34%
QC value within limits for Mo 202.031 Recovery = 95.91%						
Na 589.592 Radial†	63801.9	9758.3 µg/L	35.47	9758.3 ppb	35.47	0.36%
QC value within limits for Na 589.592 Radial Recovery = 97.58%						
Ni 231.604†	38055.3	486.77 µg/L	1.281	486.77 ppb	1.281	0.26%
QC value within limits for Ni 231.604 Recovery = 97.35%						
P 214.914†	9849.4	2350.4 µg/L	8.04	2350.4 ppb	8.04	0.34%
QC value within limits for P 214.914 Recovery = 94.02%						
Pb 220.353†	7853.6	477.29 µg/L	1.242	477.29 ppb	1.242	0.26%
QC value within limits for Pb 220.353 Recovery = 95.46%						
S 181.975 Axial†	1146.3	932.72 µg/L	6.328	932.72 ppb	6.328	0.68%
QC value within limits for S 181.975 Axial Recovery = 93.27%						
Sb 206.836†	3591.5	485.47 µg/L	1.590	485.47 ppb	1.590	0.33%
QC value within limits for Sb 206.836 Recovery = 97.09%						
Se 196.026†	1185.5	471 µg/L	3.0	471 ppb	3.0	0.65%
QC value within limits for Se 196.026 Recovery = 94.21%						
SiO2†	47839.5	5208.2 µg/L	33.99	5208.2 ppb	33.99	0.65%
QC value within limits for SiO2 Recovery = 97.40%						
Si 251.611†	147649.6	2431.8 µg/L	10.49	2431.8 ppb	10.49	0.43%
QC value within limits for Si 251.611 Recovery = 97.27%						
Sn 189.927†	6803.0	485.29 µg/L	1.421	485.29 ppb	1.421	0.29%
QC value within limits for Sn 189.927 Recovery = 97.06%						
Sr 421.552†	213429.2	500.18 µg/L	2.240	500.18 ppb	2.240	0.45%
QC value within limits for Sr 421.552 Recovery = 100.04%						
Ti 334.940†	481848.1	490.70 µg/L	2.236	490.70 ppb	2.236	0.46%
QC value within limits for Ti 334.940 Recovery = 98.14%						
Tl 190.801†	3565.2	485.94 µg/L	1.942	485.94 ppb	1.942	0.40%
QC value within limits for Tl 190.801 Recovery = 97.19%						
U 409.014†	7459.8	491.02 µg/L	5.432	491.02 ppb	5.432	1.11%
QC value within limits for U 409.014 Recovery = 98.20%						
V 292.402†	88815.7	498.80 µg/L	1.625	498.80 ppb	1.625	0.33%
QC value within limits for V 292.402 Recovery = 99.76%						
Zn 213.857†	76607.9	478.40 µg/L	2.115	478.40 ppb	2.115	0.44%
QC value within limits for Zn 213.857 Recovery = 95.68%						
All analyte(s) passed QC.						

Sequence No.: 38

Sample ID: CCB

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 8

Date Collected: 3/29/2010 20:41:27

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCB

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	159642.2	159642.2	110 %		20:41:56
1	Al 396.153Radial†	-31.9	2.8	0.5753 µg/L	0.5753 ppb	20:42:16
1	Ca 317.933Radial†	722.9	43.8	2.5682 µg/L	2.5682 ppb	20:42:16
1	Fe 238.204 Radial†	156.5	29.6	1.9698 µg/L	1.9698 ppb	20:42:16
1	K 766.490 Radial†	1376.5	-198.2	-81.588 µg/L	-81.588 ppb	20:41:56
1	Mg 279.077 IEC†	160.5	-40.1	-16.536 µg/L	-16.536 ppb	20:42:16
1	Na 589.592 Radial†	1426.6	-392.2	-59.938 µg/L	-59.938 ppb	20:41:56
1	Sr 421.552†	-236.3	62.2	0.1458 µg/L	0.1458 ppb	20:41:56
1	Sc 361.383	1761363.3	1761363.3	105.30 %		20:43:04
1	Y 371.029	1082249.7	1082249.7	105.84 %		20:43:04
1	Ag 328.068†	2961.0	-154.9	-0.6438 µg/L	-0.6438 ppb	20:43:06
1	As 188.979†	-17.6	-2.5	-1.0426 µg/L	-1.0426 ppb	20:43:26
1	B 249.677†	3116.7	-395.7	-6.6440 µg/L	-6.6440 ppb	20:43:26
1	Ba 233.527†	-177.6	6.4	0.0281 µg/L	0.0281 ppb	20:43:26
1	Be 313.107†	-787.6	-87.9	-0.0270 µg/L	-0.0270 ppb	20:43:06
1	Cd 226.502†	-97.6	1.7	0.0116 µg/L	0.0116 ppb	20:43:26
1	Co 228.616†	-177.8	7.8	0.1062 µg/L	0.1062 ppb	20:43:26
1	Cr 267.716†	140.3	-27.0	-0.2369 µg/L	-0.2369 ppb	20:43:26
1	Cu 324.752†	2779.8	215.1	0.9395 µg/L	0.9395 ppb	20:43:06
1	Mn 257.610†	177.4	88.5	0.1216 µg/L	0.1216 ppb	20:43:26
1	Mo 202.031†	-33.7	23.2	0.7311 µg/L	0.7311 ppb	20:43:26
1	Ni 231.604†	-52.7	-9.1	-0.1163 µg/L	-0.1163 ppb	20:43:26
1	P 214.914†	64.5	-18.3	-4.4052 µg/L	-4.4052 ppb	20:43:26
1	Pb 220.353†	118.6	0.2	0.0090 µg/L	0.0090 ppb	20:43:26
1	S 181.975 Axial†	91.5	-7.9	-6.4221 µg/L	-6.4221 ppb	20:43:26
1	Sb 206.836†	85.6	-5.4	-0.7134 µg/L	-0.7134 ppb	20:43:26
1	Se 196.026†	17.8	6.0	2.38 µg/L	2.38 ppb	20:43:26
1	SiO2†	1758.9	97.6	10.643 µg/L	10.643 ppb	20:43:26
1	Si 251.611†	831.5	113.3	1.8631 µg/L	1.8631 ppb	20:43:26
1	Sn 189.927†	4.0	1.8	0.1284 µg/L	0.1284 ppb	20:43:26
1	Ti 334.940†	1053.8	364.4	0.3709 µg/L	0.3709 ppb	20:43:06
1	Tl 190.801†	-105.5	20.1	2.6847 µg/L	2.6847 ppb	20:43:26
1	U 409.014†	-413.2	86.7	5.2550 µg/L	5.2550 ppb	20:43:06
1	V 292.402†	111.6	-325.8	-1.7979 µg/L	-1.7979 ppb	20:43:06
1	Zn 213.857†	508.2	18.2	0.1146 µg/L	0.1146 ppb	20:43:26
2	Sc RADIAL	156186.9	156186.9	107 %		20:42:18
2	Al 396.153Radial†	-15.2	17.7	3.8291 µg/L	3.8291 ppb	20:42:38
2	Ca 317.933Radial†	693.6	31.0	1.8191 µg/L	1.8191 ppb	20:42:38
2	Fe 238.204 Radial†	162.9	38.7	2.5747 µg/L	2.5747 ppb	20:42:38
2	K 766.490 Radial†	1472.5	-80.8	-33.270 µg/L	-33.270 ppb	20:42:18
2	Mg 279.077 IEC†	190.1	-9.2	-3.7954 µg/L	-3.7954 ppb	20:42:38
2	Na 589.592 Radial†	1486.0	-308.0	-47.099 µg/L	-47.099 ppb	20:42:18
2	Sr 421.552†	-366.4	-64.0	-0.1499 µg/L	-0.1499 ppb	20:42:18
2	Sc 361.383	1768341.2	1768341.2	105.71 %		20:43:28
2	Y 371.029	1086167.8	1086167.8	106.22 %		20:43:28
2	Ag 328.068†	2860.7	-260.9	-1.0681 µg/L	-1.0681 ppb	20:43:30
2	As 188.979†	-12.8	2.1	0.8941 µg/L	0.8941 ppb	20:43:50
2	B 249.677†	3095.0	-428.0	-7.1869 µg/L	-7.1869 ppb	20:43:50
2	Ba 233.527†	-192.4	-6.9	-0.0315 µg/L	-0.0315 ppb	20:43:50
2	Be 313.107†	-460.5	224.5	0.0719 µg/L	0.0719 ppb	20:43:30
2	Cd 226.502†	-94.7	4.9	0.0334 µg/L	0.0334 ppb	20:43:50
2	Co 228.616†	-140.7	43.5	0.5958 µg/L	0.5958 ppb	20:43:50
2	Cr 267.716†	149.4	-18.9	-0.1596 µg/L	-0.1596 ppb	20:43:50
2	Cu 324.752†	2666.0	97.1	0.4194 µg/L	0.4194 ppb	20:43:30
2	Mn 257.610†	165.4	76.4	0.1046 µg/L	0.1046 ppb	20:43:50
2	Mo 202.031†	-30.4	26.4	0.8348 µg/L	0.8348 ppb	20:43:50
2	Ni 231.604†	-24.5	17.7	0.2263 µg/L	0.2263 ppb	20:43:50
2	P 214.914†	45.9	-36.2	-8.6751 µg/L	-8.6751 ppb	20:43:50
2	Pb 220.353†	89.4	-27.9	-1.6824 µg/L	-1.6824 ppb	20:43:50

2	S 181.975 Axial†	94.2	-5.7	-4.6425 µg/L	-4.6425 ppb	20:43:50
2	Sb 206.836†	72.8	-17.8	-2.3809 µg/L	-2.3809 ppb	20:43:50
2	Se 196.026†	8.4	-3.0	-1.17 µg/L	-1.17 ppb	20:43:50
2	SiO2†	1693.5	29.1	3.1523 µg/L	3.1523 ppb	20:43:50
2	Si 251.611†	804.4	84.5	1.3841 µg/L	1.3841 ppb	20:43:50
2	Sn 189.927†	8.2	5.7	0.4069 µg/L	0.4069 ppb	20:43:50
2	Ti 334.940†	839.4	157.7	0.1627 µg/L	0.1627 ppb	20:43:30
2	Tl 190.801†	-101.0	24.8	3.3258 µg/L	3.3258 ppb	20:43:50
2	U 409.014†	-571.5	-61.5	-3.8245 µg/L	-3.8245 ppb	20:43:30
2	V 292.402†	384.6	-68.0	-0.3725 µg/L	-0.3725 ppb	20:43:30
2	Zn 213.857†	520.5	28.0	0.1740 µg/L	0.1740 ppb	20:43:50
3	Sc RADIAL	157025.4	157025.4	108 %		20:42:40
3	Al 396.153Radial†	-41.8	-6.9	-1.5626 µg/L	-1.5626 ppb	20:43:00
3	Ca 317.933Radial†	735.1	66.2	3.8771 µg/L	3.8771 ppb	20:43:00
3	Fe 238.204 Radial†	156.0	31.5	2.0942 µg/L	2.0942 ppb	20:43:00
3	K 766.490 Radial†	1504.7	-58.3	-23.989 µg/L	-23.989 ppb	20:42:40
3	Mg 279.077 IEC†	175.7	-23.6	-9.6897 µg/L	-9.6897 ppb	20:43:00
3	Na 589.592 Radial†	1490.0	-311.7	-47.668 µg/L	-47.668 ppb	20:42:40
3	Sr 421.552†	-200.3	92.1	0.2158 µg/L	0.2158 ppb	20:42:40
3	Sc 361.383	1802169.8	1802169.8	107.74 %		20:43:52
3	Y 371.029	1105477.1	1105477.1	108.11 %		20:43:52
3	Ag 328.068†	2995.0	-187.1	-0.7466 µg/L	-0.7466 ppb	20:43:54
3	As 188.979†	-15.0	0.3	0.1424 µg/L	0.1424 ppb	20:44:15
3	B 249.677†	3108.4	-470.5	-7.8995 µg/L	-7.8995 ppb	20:44:15
3	Ba 233.527†	-173.6	13.9	0.0633 µg/L	0.0633 ppb	20:44:15
3	Be 313.107†	-686.3	23.1	0.0136 µg/L	0.0136 ppb	20:43:54
3	Cd 226.502†	-87.9	12.8	0.0881 µg/L	0.0881 ppb	20:44:15
3	Co 228.616†	-169.8	19.0	0.2599 µg/L	0.2599 ppb	20:44:15
3	Cr 267.716†	170.2	-2.2	-0.0351 µg/L	-0.0351 ppb	20:44:15
3	Cu 324.752†	2724.0	103.6	0.4670 µg/L	0.4670 ppb	20:43:54
3	Mn 257.610†	180.6	87.6	0.1201 µg/L	0.1201 ppb	20:44:15
3	Mo 202.031†	-18.7	37.8	1.1943 µg/L	1.1943 ppb	20:44:15
3	Ni 231.604†	-67.6	-21.8	-0.2790 µg/L	-0.2790 ppb	20:44:15
3	P 214.914†	48.5	-34.6	-8.3057 µg/L	-8.3057 ppb	20:44:15
3	Pb 220.353†	111.7	-8.7	-0.5419 µg/L	-0.5419 ppb	20:44:15
3	S 181.975 Axial†	82.0	-18.7	-15.128 µg/L	-15.128 ppb	20:44:15
3	Sb 206.836†	86.7	-6.1	-0.8115 µg/L	-0.8115 ppb	20:44:15
3	Se 196.026†	20.9	8.5	3.37 µg/L	3.37 ppb	20:44:15
3	SiO2†	1699.8	4.9	0.5106 µg/L	0.5106 ppb	20:44:15
3	Si 251.611†	817.9	82.8	1.3569 µg/L	1.3569 ppb	20:44:15
3	Sn 189.927†	-7.0	-8.5	-0.6027 µg/L	-0.6027 ppb	20:44:15
3	Ti 334.940†	578.4	-99.5	-0.1088 µg/L	-0.1088 ppb	20:43:54
3	Tl 190.801†	-115.5	13.1	1.7476 µg/L	1.7476 ppb	20:44:15
3	U 409.014†	-166.7	324.4	19.989 µg/L	19.989 ppb	20:43:54
3	V 292.402†	270.2	-181.0	-0.9785 µg/L	-0.9785 ppb	20:43:54
3	Zn 213.857†	519.3	17.6	0.1119 µg/L	0.1119 ppb	20:44:15

Mean Data: CCB

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1777291.5	106.25 %	1.305			1.23%
Sc RADIAL	157618.2	108 %	1.2			1.14%
Y 371.029	1091298.2	106.72 %	1.216			1.14%
Ag 328.068†	-201.0	-0.8195 µg/L	0.22133	-0.8195 ppb	0.22133	27.01%
QC value within limits for Ag 328.068 Recovery = Not calculated						
Al 396.153Radial†	4.5	0.9472 µg/L	2.71501	0.9472 ppb	2.71501	286.62%
QC value within limits for Al 396.153Radial Recovery = Not calculated						
As 188.979†	-0.0	-0.0020 µg/L	0.97639	-0.0020 ppb	0.97639	>999.9%
QC value within limits for As 188.979 Recovery = Not calculated						
B 249.677†	-431.4	-7.2435 µg/L	0.62967	-7.2435 ppb	0.62967	8.69%
QC value within limits for B 249.677 Recovery = Not calculated						
Ba 233.527†	4.5	0.0200 µg/L	0.04797	0.0200 ppb	0.04797	240.04%
QC value within limits for Ba 233.527 Recovery = Not calculated						
Be 313.107†	53.2	0.0195 µg/L	0.04972	0.0195 ppb	0.04972	254.94%
QC value within limits for Be 313.107 Recovery = Not calculated						
Ca 317.933Radial†	47.0	2.7548 µg/L	1.04159	2.7548 ppb	1.04159	37.81%
QC value within limits for Ca 317.933Radial Recovery = Not calculated						
Cd 226.502†	6.5	0.0444 µg/L	0.03942	0.0444 ppb	0.03942	88.81%
QC value within limits for Cd 226.502 Recovery = Not calculated						
Co 228.616†	23.4	0.3206 µg/L	0.25038	0.3206 ppb	0.25038	78.09%

QC value within limits for Co 228.616 Recovery = Not calculated							
Cr 267.716†	-16.1	-0.1439 µg/L	0.10181	-0.1439 ppb	0.10181	70.75%	
QC value within limits for Cr 267.716 Recovery = Not calculated							
Cu 324.752†	138.6	0.6086 µg/L	0.28751	0.6086 ppb	0.28751	47.24%	
QC value within limits for Cu 324.752 Recovery = Not calculated							
Fe 238.204 Radial†	33.3	2.2129 µg/L	0.31946	2.2129 ppb	0.31946	14.44%	
QC value within limits for Fe 238.204 Radial Recovery = Not calculated							
K 766.490 Radial†	-112.4	-46.282 µg/L	30.9255	-46.282 ppb	30.9255	66.82%	
QC value within limits for K 766.490 Radial Recovery = Not calculated							
Mg 279.077 IEC†	-24.3	-10.007 µg/L	6.3764	-10.007 ppb	6.3764	63.72%	
QC value within limits for Mg 279.077 IEC Recovery = Not calculated							
Mn 257.610†	84.2	0.1154 µg/L	0.00942	0.1154 ppb	0.00942	8.16%	
QC value within limits for Mn 257.610 Recovery = Not calculated							
Mo 202.031†	29.2	0.9200 µg/L	0.24309	0.9200 ppb	0.24309	26.42%	
QC value within limits for Mo 202.031 Recovery = Not calculated							
Na 589.592 Radial†	-337.3	-51.568 µg/L	7.2542	-51.568 ppb	7.2542	14.07%	
QC value within limits for Na 589.592 Radial Recovery = Not calculated							
Ni 231.604†	-4.4	-0.0563 µg/L	0.25791	-0.0563 ppb	0.25791	457.85%	
QC value within limits for Ni 231.604 Recovery = Not calculated							
P 214.914†	-29.7	-7.1287 µg/L	2.36584	-7.1287 ppb	2.36584	33.19%	
QC value within limits for P 214.914 Recovery = Not calculated							
Pb 220.353†	-12.1	-0.7384 µg/L	0.86263	-0.7384 ppb	0.86263	116.82%	
QC value within limits for Pb 220.353 Recovery = Not calculated							
S 181.975 Axial†	-10.8	-8.7308 µg/L	5.61093	-8.7308 ppb	5.61093	64.27%	
QC value within limits for S 181.975 Axial Recovery = Not calculated							
Sb 206.836†	-9.7	-1.3019 µg/L	0.93572	-1.3019 ppb	0.93572	71.87%	
QC value within limits for Sb 206.836 Recovery = Not calculated							
Se 196.026†	3.8	1.53 µg/L	2.391	1.53 ppb	2.391	156.61%	
QC value within limits for Se 196.026 Recovery = Not calculated							
SiO2†	43.9	4.7687 µg/L	5.25620	4.7687 ppb	5.25620	110.22%	
QC value within limits for SiO2 Recovery = Not calculated							
Si 251.611†	93.5	1.5347 µg/L	0.28470	1.5347 ppb	0.28470	18.55%	
QC value within limits for Si 251.611 Recovery = Not calculated							
Sn 189.927†	-0.3	-0.0225 µg/L	0.52147	-0.0225 ppb	0.52147	>999.9%	
QC value within limits for Sn 189.927 Recovery = Not calculated							
Sr 421.552†	30.1	0.0706 µg/L	0.19411	0.0706 ppb	0.19411	275.10%	
QC value within limits for Sr 421.552 Recovery = Not calculated							
Ti 334.940†	140.8	0.1416 µg/L	0.24052	0.1416 ppb	0.24052	169.85%	
QC value within limits for Ti 334.940 Recovery = Not calculated							
Tl 190.801†	19.3	2.5860 µg/L	0.79369	2.5860 ppb	0.79369	30.69%	
QC value within limits for Tl 190.801 Recovery = Not calculated							
U 409.014†	116.5	7.1397 µg/L	12.01791	7.1397 ppb	12.01791	168.33%	
QC value within limits for U 409.014 Recovery = Not calculated							
V 292.402†	-191.6	-1.0496 µg/L	0.71539	-1.0496 ppb	0.71539	68.16%	
QC value within limits for V 292.402 Recovery = Not calculated							
Zn 213.857†	21.3	0.1335 µg/L	0.03514	0.1335 ppb	0.03514	26.32%	
QC value within limits for Zn 213.857 Recovery = Not calculated							
All analyte(s) passed QC.							

Sequence No.: 46

Sample ID: CCV

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 7

Date Collected: 3/29/2010 21:03:21

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCV

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	154851.7	154851.7	106 %		21:03:53
1	Al 396.153Radial†	25485.8	24020.4	5220.8 µg/L	5220.8 ppb	21:03:53
1	Ca 317.933Radial†	90010.8	84106.5	4928.3 µg/L	4928.3 ppb	21:03:53
1	Fe 238.204 Radial†	78533.5	73806.4	4906.9 µg/L	4906.9 ppb	21:03:53
1	K 766.490 Radial†	13939.7	11665.7	4798.5 µg/L	4798.5 ppb	21:03:53
1	Mg 279.077 IEC†	13229.3	12265.4	5064.8 µg/L	5064.8 ppb	21:03:53
1	Na 589.592 Radial†	69846.3	64048.1	9795.9 µg/L	9795.9 ppb	21:03:53
1	Sr 421.552†	228674.2	215517.6	505.08 µg/L	505.08 ppb	21:03:51
1	Sc 361.383	1713248.9	1713248.9	102.42 %		21:04:06
1	Y 371.029	1039105.6	1039105.6	101.62 %		21:04:06
1	Ag 328.068†	126578.4	120621.1	495.66 µg/L	495.66 ppb	21:04:06
1	As 188.979†	1286.8	1270.6	538.07 µg/L	538.07 ppb	21:04:26
1	B 249.677†	32552.7	28428.0	475.59 µg/L	475.59 ppb	21:04:06
1	Ba 233.527†	111768.2	109302.8	499.73 µg/L	499.73 ppb	21:04:06
1	Be 313.107†	1595894.5	1558852.6	507.57 µg/L	507.57 ppb	21:04:06
1	Cd 226.502†	71067.7	69483.2	479.52 µg/L	479.52 ppb	21:04:06
1	Co 228.616†	36010.7	35336.6	484.13 µg/L	484.13 ppb	21:04:06
1	Cr 267.716†	58430.3	56889.7	488.51 µg/L	488.51 ppb	21:04:06
1	Cu 324.752†	118439.2	113216.3	493.68 µg/L	493.68 ppb	21:04:06
1	Mn 257.610†	368025.4	359251.0	490.68 µg/L	490.68 ppb	21:04:06
1	Mo 202.031†	15706.6	15390.8	486.28 µg/L	486.28 ppb	21:04:26
1	Ni 231.604†	38854.0	37977.0	485.77 µg/L	485.77 ppb	21:04:06
1	P 214.914†	10314.2	9990.9	2384.3 µg/L	2384.3 ppb	21:04:26
1	Pb 220.353†	8262.0	7954.4	483.41 µg/L	483.41 ppb	21:04:26
1	S 181.975 Axial†	1274.3	1149.4	935.31 µg/L	935.31 ppb	21:04:26
1	Sb 206.836†	3786.5	3610.4	488.11 µg/L	488.11 ppb	21:04:26
1	Se 196.026†	1247.6	1207.2	480 µg/L	480 ppb	21:04:26
1	SiO2†	50572.1	47804.5	5204.1 µg/L	5204.1 ppb	21:04:06
1	Si 251.611†	152175.1	147903.7	2435.8 µg/L	2435.8 ppb	21:04:06
1	Sn 189.927†	7069.4	6900.4	492.22 µg/L	492.22 ppb	21:04:26
1	Ti 334.940†	495105.0	482772.1	491.64 µg/L	491.64 ppb	21:04:06
1	Tl 190.801†	3560.4	3596.6	490.17 µg/L	490.17 ppb	21:04:26
1	U 409.014†	7150.7	7460.8	491.07 µg/L	491.07 ppb	21:04:06
1	V 292.402†	91336.8	88747.2	498.49 µg/L	498.49 ppb	21:04:06
1	Zn 213.857†	78849.4	76522.2	477.86 µg/L	477.86 ppb	21:04:06
2	Sc RADIAL	153431.3	153431.3	105 %		21:03:57
2	Al 396.153Radial†	25174.7	23947.0	5204.9 µg/L	5204.9 ppb	21:03:57
2	Ca 317.933Radial†	89019.4	83949.0	4919.1 µg/L	4919.1 ppb	21:03:57
2	Fe 238.204 Radial†	77673.0	73673.3	4898.1 µg/L	4898.1 ppb	21:03:57
2	K 766.490 Radial†	13736.1	11593.9	4768.9 µg/L	4768.9 ppb	21:03:57
2	Mg 279.077 IEC†	13051.1	12211.4	5042.5 µg/L	5042.5 ppb	21:03:57
2	Na 589.592 Radial†	69569.0	64393.3	9848.8 µg/L	9848.8 ppb	21:03:57
2	Sr 421.552†	230380.7	219131.5	513.55 µg/L	513.55 ppb	21:03:55
2	Sc 361.383	1723240.0	1723240.0	103.02 %		21:04:29
2	Y 371.029	1044358.9	1044358.9	102.13 %		21:04:29
2	Ag 328.068†	127680.9	120974.7	497.13 µg/L	497.13 ppb	21:04:29
2	As 188.979†	1279.6	1256.3	532.10 µg/L	532.10 ppb	21:04:49
2	B 249.677†	32914.0	28594.4	478.37 µg/L	478.37 ppb	21:04:29
2	Ba 233.527†	112872.1	109741.6	501.74 µg/L	501.74 ppb	21:04:29
2	Be 313.107†	1612082.1	1565532.0	509.75 µg/L	509.75 ppb	21:04:29
2	Cd 226.502†	71525.6	69525.3	479.81 µg/L	479.81 ppb	21:04:29
2	Co 228.616†	36504.1	35611.7	487.90 µg/L	487.90 ppb	21:04:29
2	Cr 267.716†	58865.9	56981.8	489.29 µg/L	489.29 ppb	21:04:29
2	Cu 324.752†	119296.1	113377.7	494.39 µg/L	494.39 ppb	21:04:29
2	Mn 257.610†	370507.0	359576.6	491.13 µg/L	491.13 ppb	21:04:29
2	Mo 202.031†	15700.9	15296.3	483.30 µg/L	483.30 ppb	21:04:49
2	Ni 231.604†	39299.1	38189.1	488.48 µg/L	488.48 ppb	21:04:29
2	P 214.914†	10271.7	9891.3	2360.4 µg/L	2360.4 ppb	21:04:49
2	Pb 220.353†	8221.9	7868.7	478.21 µg/L	478.21 ppb	21:04:49

2	S 181.975 Axial†	1283.0	1150.6	936.30 µg/L	936.30 ppb	21:04:49
2	Sb 206.836†	3813.2	3614.9	488.65 µg/L	488.65 ppb	21:04:49
2	Se 196.026†	1244.9	1197.5	476 µg/L	476 ppb	21:04:49
2	SiO2†	51026.3	47959.1	5221.2 µg/L	5221.2 ppb	21:04:29
2	Si 251.611†	153367.0	148199.2	2440.8 µg/L	2440.8 ppb	21:04:29
2	Sn 189.927†	7028.6	6820.7	486.55 µg/L	486.55 ppb	21:04:49
2	Ti 334.940†	498901.8	483655.0	492.54 µg/L	492.54 ppb	21:04:29
2	Tl 190.801†	3590.9	3606.0	491.45 µg/L	491.45 ppb	21:04:49
2	U 409.014†	7310.8	7575.8	498.29 µg/L	498.29 ppb	21:04:29
2	V 292.402†	92221.6	89089.0	500.36 µg/L	500.36 ppb	21:04:29
2	Zn 213.857†	79595.3	76799.9	479.59 µg/L	479.59 ppb	21:04:29
3	Sc RADIAL	153860.9	153860.9	106 %		21:04:01
3	Al 396.153Radial†	25294.4	23993.6	5215.1 µg/L	5215.1 ppb	21:04:01
3	Ca 317.933Radial†	89754.2	84409.0	4946.0 µg/L	4946.0 ppb	21:04:01
3	Fe 238.204 Radial†	78247.7	74011.6	4920.6 µg/L	4920.6 ppb	21:04:01
3	K 766.490 Radial†	13894.4	11707.3	4815.6 µg/L	4815.6 ppb	21:04:01
3	Mg 279.077 IEC†	13234.5	12350.5	5099.8 µg/L	5099.8 ppb	21:04:01
3	Na 589.592 Radial†	69626.7	64263.4	9828.8 µg/L	9828.8 ppb	21:04:01
3	Sr 421.552†	228028.2	216291.8	506.89 µg/L	506.89 ppb	21:03:59
3	Sc 361.383	1732745.4	1732745.4	103.59 %		21:04:52
3	Y 371.029	1050125.7	1050125.7	102.69 %		21:04:52
3	Ag 328.068†	127692.6	120306.0	494.38 µg/L	494.38 ppb	21:04:52
3	As 188.979†	1285.3	1255.0	531.54 µg/L	531.54 ppb	21:05:12
3	B 249.677†	33066.4	28566.3	477.91 µg/L	477.91 ppb	21:04:52
3	Ba 233.527†	113084.6	109345.8	499.93 µg/L	499.93 ppb	21:04:52
3	Be 313.107†	1614930.2	1559697.0	507.85 µg/L	507.85 ppb	21:04:52
3	Cd 226.502†	71595.2	69211.7	477.64 µg/L	477.64 ppb	21:04:52
3	Co 228.616†	36541.6	35453.5	485.73 µg/L	485.73 ppb	21:04:52
3	Cr 267.716†	58957.8	56757.0	487.36 µg/L	487.36 ppb	21:04:52
3	Cu 324.752†	119675.9	113109.0	493.23 µg/L	493.23 ppb	21:04:52
3	Mn 257.610†	371477.0	358540.1	489.71 µg/L	489.71 ppb	21:04:52
3	Mo 202.031†	15758.3	15268.1	482.41 µg/L	482.41 ppb	21:05:12
3	Ni 231.604†	39365.4	38043.9	486.63 µg/L	486.63 ppb	21:04:52
3	P 214.914†	10350.1	9912.3	2365.5 µg/L	2365.5 ppb	21:05:12
3	Pb 220.353†	8278.4	7879.4	478.85 µg/L	478.85 ppb	21:05:12
3	S 181.975 Axial†	1296.2	1156.5	941.02 µg/L	941.02 ppb	21:05:12
3	Sb 206.836†	3820.2	3601.3	486.84 µg/L	486.84 ppb	21:05:12
3	Se 196.026†	1245.9	1191.9	474 µg/L	474 ppb	21:05:12
3	SiO2†	51139.5	47796.6	5203.5 µg/L	5203.5 ppb	21:04:52
3	Si 251.611†	153580.9	147589.1	2430.7 µg/L	2430.7 ppb	21:04:52
3	Sn 189.927†	7084.4	6837.2	487.72 µg/L	487.72 ppb	21:05:12
3	Ti 334.940†	499459.5	481536.7	490.37 µg/L	490.37 ppb	21:04:52
3	Tl 190.801†	3572.9	3569.5	486.51 µg/L	486.51 ppb	21:05:12
3	U 409.014†	7416.3	7638.8	501.99 µg/L	501.99 ppb	21:04:52
3	V 292.402†	92167.5	88545.7	497.33 µg/L	497.33 ppb	21:04:52
3	Zn 213.857†	79634.5	76413.9	477.17 µg/L	477.17 ppb	21:04:52

Mean Data: CCV

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1723078.1	103.01 %	0.583			0.57%
Sc RADIAL	154048.0	106 %	0.5			0.47%
Y 371.029	1044530.0	102.15 %	0.539			0.53%
Ag 328.068†	120633.9	495.73 µg/L	1.374	495.73 ppb	1.374	0.28%
QC value within limits for Ag 328.068 Recovery = 99.15%						
Al 396.153Radial†	23987.0	5213.6 µg/L	8.05	5213.6 ppb	8.05	0.15%
QC value within limits for Al 396.153Radial Recovery = 104.27%						
As 188.979†	1260.7	533.90 µg/L	3.620	533.90 ppb	3.620	0.68%
QC value within limits for As 188.979 Recovery = 106.78%						
B 249.677†	28529.6	477.29 µg/L	1.490	477.29 ppb	1.490	0.31%
QC value within limits for B 249.677 Recovery = 95.46%						
Ba 233.527†	109463.4	500.47 µg/L	1.106	500.47 ppb	1.106	0.22%
QC value within limits for Ba 233.527 Recovery = 100.09%						
Be 313.107†	1561360.5	508.39 µg/L	1.184	508.39 ppb	1.184	0.23%
QC value within limits for Be 313.107 Recovery = 101.68%						
Ca 317.933Radial†	84154.8	4931.1 µg/L	13.70	4931.1 ppb	13.70	0.28%
QC value within limits for Ca 317.933Radial Recovery = 98.62%						
Cd 226.502†	69406.7	478.99 µg/L	1.177	478.99 ppb	1.177	0.25%
QC value within limits for Cd 226.502 Recovery = 95.80%						
Co 228.616†	35467.2	485.92 µg/L	1.892	485.92 ppb	1.892	0.39%

QC value within limits for Co 228.616 Recovery = 97.18%							
Cr 267.716†	56876.2	488.38 µg/L	0.973	488.38 ppb	0.973	0.20%	
QC value within limits for Cr 267.716 Recovery = 97.68%							
Cu 324.752†	113234.3	493.76 µg/L	0.585	493.76 ppb	0.585	0.12%	
QC value within limits for Cu 324.752 Recovery = 98.75%							
Fe 238.204 Radial†	73830.5	4908.5 µg/L	11.33	4908.5 ppb	11.33	0.23%	
QC value within limits for Fe 238.204 Radial Recovery = 98.17%							
K 766.490 Radial†	11655.6	4794.3 µg/L	23.63	4794.3 ppb	23.63	0.49%	
QC value within limits for K 766.490 Radial Recovery = 95.89%							
Mg 279.077 IEC†	12275.8	5069.1 µg/L	28.89	5069.1 ppb	28.89	0.57%	
QC value within limits for Mg 279.077 IEC Recovery = 101.38%							
Mn 257.610†	359122.6	490.51 µg/L	0.726	490.51 ppb	0.726	0.15%	
QC value within limits for Mn 257.610 Recovery = 98.10%							
Mo 202.031†	15318.4	483.99 µg/L	2.029	483.99 ppb	2.029	0.42%	
QC value within limits for Mo 202.031 Recovery = 96.80%							
Na 589.592 Radial†	64235.0	9824.5 µg/L	26.69	9824.5 ppb	26.69	0.27%	
QC value within limits for Na 589.592 Radial Recovery = 98.25%							
Ni 231.604†	38070.0	486.96 µg/L	1.387	486.96 ppb	1.387	0.28%	
QC value within limits for Ni 231.604 Recovery = 97.39%							
P 214.914†	9931.5	2370.0 µg/L	12.59	2370.0 ppb	12.59	0.53%	
QC value within limits for P 214.914 Recovery = 94.80%							
Pb 220.353†	7900.8	480.16 µg/L	2.839	480.16 ppb	2.839	0.59%	
QC value within limits for Pb 220.353 Recovery = 96.03%							
S 181.975 Axial†	1152.2	937.54 µg/L	3.050	937.54 ppb	3.050	0.33%	
QC value within limits for S 181.975 Axial Recovery = 93.75%							
Sb 206.836†	3608.9	487.87 µg/L	0.930	487.87 ppb	0.930	0.19%	
QC value within limits for Sb 206.836 Recovery = 97.57%							
Se 196.026†	1198.9	476 µg/L	3.1	476 ppb	3.1	0.64%	
QC value within limits for Se 196.026 Recovery = 95.27%							
SiO2†	47853.4	5209.6 µg/L	10.06	5209.6 ppb	10.06	0.19%	
QC value within limits for SiO2 Recovery = 97.42%							
Si 251.611†	147897.3	2435.8 µg/L	5.04	2435.8 ppb	5.04	0.21%	
QC value within limits for Si 251.611 Recovery = 97.43%							
Sn 189.927†	6852.8	488.83 µg/L	2.990	488.83 ppb	2.990	0.61%	
QC value within limits for Sn 189.927 Recovery = 97.77%							
Sr 421.552†	216980.3	508.51 µg/L	4.460	508.51 ppb	4.460	0.88%	
QC value within limits for Sr 421.552 Recovery = 101.70%							
Ti 334.940†	482654.6	491.52 µg/L	1.088	491.52 ppb	1.088	0.22%	
QC value within limits for Ti 334.940 Recovery = 98.30%							
Tl 190.801†	3590.7	489.37 µg/L	2.564	489.37 ppb	2.564	0.52%	
QC value within limits for Tl 190.801 Recovery = 97.87%							
U 409.014†	7558.5	497.12 µg/L	5.554	497.12 ppb	5.554	1.12%	
QC value within limits for U 409.014 Recovery = 99.42%							
V 292.402†	88794.0	498.73 µg/L	1.529	498.73 ppb	1.529	0.31%	
QC value within limits for V 292.402 Recovery = 99.75%							
Zn 213.857†	76578.7	478.21 µg/L	1.247	478.21 ppb	1.247	0.26%	
QC value within limits for Zn 213.857 Recovery = 95.64%							
All analyte(s) passed QC.							

Sequence No.: 47
 Sample ID: CCB
 Analyst:
 Initial Sample Wt:
 Dilution:

Autosampler Location: 8
 Date Collected: 3/29/2010 21:05:20
 Data Type: Original
 Initial Sample Vol:
 Sample Prep Vol:

Replicate Data: CCB

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	154996.4	154996.4	106 %		21:05:49
1	Al 396.153Radial†	-63.3	-27.7	-6.1097 µg/L	-6.1097 ppb	21:06:09
1	Ca 317.933Radial†	693.4	35.9	2.1034 µg/L	2.1034 ppb	21:06:09
1	Fe 238.204 Radial†	151.1	28.8	1.9138 µg/L	1.9138 ppb	21:06:09
1	K 766.490 Radial†	1597.5	47.3	19.463 µg/L	19.463 ppb	21:05:49
1	Mg 279.077 IEC†	208.9	9.8	4.0702 µg/L	4.0702 ppb	21:06:09
1	Na 589.592 Radial†	1678.5	-116.3	-17.818 µg/L	-17.818 ppb	21:05:49
1	Sr 421.552†	-227.7	63.9	0.1497 µg/L	0.1497 ppb	21:05:49
1	Sc 361.383	1725992.9	1725992.9	103.18 %		21:06:57
1	Y 371.029	1059747.2	1059747.2	103.63 %		21:06:57
1	Ag 328.068†	3051.7	-9.4	-0.0382 µg/L	-0.0382 ppb	21:06:59
1	As 188.979†	-12.6	2.0	0.8526 µg/L	0.8526 ppb	21:07:19
1	B 249.677†	3056.4	-393.5	-6.6077 µg/L	-6.6077 ppb	21:07:19
1	Ba 233.527†	-168.8	11.5	0.0524 µg/L	0.0524 ppb	21:07:19
1	Be 313.107†	-508.1	167.7	0.0571 µg/L	0.0571 ppb	21:06:59
1	Cd 226.502†	-60.4	35.9	0.2479 µg/L	0.2479 ppb	21:07:19
1	Co 228.616†	-169.8	12.0	0.1644 µg/L	0.1644 ppb	21:07:19
1	Cr 267.716†	146.1	-18.7	-0.1673 µg/L	-0.1673 ppb	21:07:19
1	Cu 324.752†	2666.8	159.7	0.7014 µg/L	0.7014 ppb	21:06:59
1	Mn 257.610†	177.8	92.3	0.1259 µg/L	0.1259 ppb	21:07:19
1	Mo 202.031†	-5.1	50.3	1.5872 µg/L	1.5872 ppb	21:07:19
1	Ni 231.604†	-16.9	24.5	0.3133 µg/L	0.3133 ppb	21:07:19
1	P 214.914†	22.6	-57.6	-13.826 µg/L	-13.826 ppb	21:07:19
1	Pb 220.353†	90.0	-25.2	-1.5281 µg/L	-1.5281 ppb	21:07:19
1	S 181.975 Axial†	71.1	-25.9	-21.007 µg/L	-21.007 ppb	21:07:19
1	Sb 206.836†	85.9	-3.3	-0.4268 µg/L	-0.4268 ppb	21:07:19
1	Se 196.026†	19.1	7.6	3.00 µg/L	3.00 ppb	21:07:19
1	SiO2†	1671.8	47.4	5.1244 µg/L	5.1244 ppb	21:07:19
1	Si 251.611†	772.8	72.6	1.1761 µg/L	1.1761 ppb	21:07:19
1	Sn 189.927†	9.7	7.4	0.5233 µg/L	0.5233 ppb	21:07:19
1	Ti 334.940†	780.1	119.7	0.1184 µg/L	0.1184 ppb	21:06:59
1	Tl 190.801†	-117.8	6.2	0.8248 µg/L	0.8248 ppb	21:07:19
1	U 409.014†	-356.1	134.0	8.2316 µg/L	8.2316 ppb	21:06:59
1	V 292.402†	287.8	-152.9	-0.8274 µg/L	-0.8274 ppb	21:06:59
1	Zn 213.857†	507.5	27.4	0.1698 µg/L	0.1698 ppb	21:07:19
2	Sc RADIAL	152412.0	152412.0	105 %		21:06:11
2	Al 396.153Radial†	-24.5	8.4	1.8014 µg/L	1.8014 ppb	21:06:31
2	Ca 317.933Radial†	694.0	47.5	2.7825 µg/L	2.7825 ppb	21:06:31
2	Fe 238.204 Radial†	146.8	27.1	1.7992 µg/L	1.7992 ppb	21:06:31
2	K 766.490 Radial†	1385.9	-129.6	-53.361 µg/L	-53.361 ppb	21:06:11
2	Mg 279.077 IEC†	168.1	-25.9	-10.680 µg/L	-10.680 ppb	21:06:31
2	Na 589.592 Radial†	1601.9	-162.8	-24.860 µg/L	-24.860 ppb	21:06:11
2	Sr 421.552†	-193.2	93.2	0.2184 µg/L	0.2184 ppb	21:06:11
2	Sc 361.383	1730228.9	1730228.9	103.43 %		21:07:21
2	Y 371.029	1062056.7	1062056.7	103.86 %		21:07:21
2	Ag 328.068†	3294.6	218.2	0.8697 µg/L	0.8697 ppb	21:07:23
2	As 188.979†	-7.8	6.7	2.7923 µg/L	2.7923 ppb	21:07:43
2	B 249.677†	3121.5	-337.9	-5.6726 µg/L	-5.6726 ppb	21:07:43
2	Ba 233.527†	-196.4	-14.9	-0.0686 µg/L	-0.0686 ppb	21:07:43
2	Be 313.107†	-630.3	50.7	0.0170 µg/L	0.0170 ppb	21:07:23
2	Cd 226.502†	-85.2	12.1	0.0830 µg/L	0.0830 ppb	21:07:43
2	Co 228.616†	-178.5	4.0	0.0551 µg/L	0.0551 ppb	21:07:43
2	Cr 267.716†	146.8	-18.3	-0.1593 µg/L	-0.1593 ppb	21:07:43
2	Cu 324.752†	2640.7	128.1	0.5583 µg/L	0.5583 ppb	21:07:23
2	Mn 257.610†	136.5	52.0	0.0714 µg/L	0.0714 ppb	21:07:43
2	Mo 202.031†	-31.2	25.1	0.7914 µg/L	0.7914 ppb	21:07:43
2	Ni 231.604†	-64.5	-21.4	-0.2741 µg/L	-0.2741 ppb	21:07:43
2	P 214.914†	43.5	-37.5	-8.9955 µg/L	-8.9955 ppb	21:07:43
2	Pb 220.353†	100.4	-15.4	-0.9295 µg/L	-0.9295 ppb	21:07:43

2	S 181.975 Axial†	84.3	-13.3	-10.766 µg/L	-10.766 ppb	21:07:43
2	Sb 206.836†	56.9	-31.6	-4.2573 µg/L	-4.2573 ppb	21:07:43
2	Se 196.026†	21.3	9.7	3.82 µg/L	3.82 ppb	21:07:43
2	SiO2†	1625.1	-1.7	-0.2117 µg/L	-0.2117 ppb	21:07:43
2	Si 251.611†	795.8	92.9	1.5262 µg/L	1.5262 ppb	21:07:43
2	Sn 189.927†	2.5	0.4	0.0269 µg/L	0.0269 ppb	21:07:43
2	Ti 334.940†	1026.5	356.1	0.3635 µg/L	0.3635 ppb	21:07:23
2	Tl 190.801†	-125.8	-1.3	-0.1808 µg/L	-0.1808 ppb	21:07:43
2	U 409.014†	-469.0	25.7	1.5015 µg/L	1.5015 ppb	21:07:23
2	V 292.402†	173.5	-264.1	-1.4569 µg/L	-1.4569 ppb	21:07:23
2	Zn 213.857†	498.1	17.1	0.1092 µg/L	0.1092 ppb	21:07:43
3	Sc RADIAL	153579.1	153579.1	105 %		21:06:33
3	Al 396.153Radial†	-58.8	-23.9	-5.2607 µg/L	-5.2607 ppb	21:06:53
3	Ca 317.933Radial†	673.1	22.6	1.3237 µg/L	1.3237 ppb	21:06:53
3	Fe 238.204 Radial†	131.8	11.8	0.7823 µg/L	0.7823 ppb	21:06:53
3	K 766.490 Radial†	1453.7	-75.3	-31.005 µg/L	-31.005 ppb	21:06:33
3	Mg 279.077 IEC†	180.2	-15.7	-6.4370 µg/L	-6.4370 ppb	21:06:53
3	Na 589.592 Radial†	1585.7	-189.9	-29.024 µg/L	-29.024 ppb	21:06:33
3	Sr 421.552†	-259.8	31.4	0.0737 µg/L	0.0737 ppb	21:06:33
3	Sc 361.383	1727714.6	1727714.6	103.28 %		21:07:45
3	Y 371.029	1060914.8	1060914.8	103.75 %		21:07:45
3	Ag 328.068†	3064.7	0.2	-0.0004 µg/L	-0.0004 ppb	21:07:47
3	As 188.979†	-17.3	-2.5	-1.0488 µg/L	-1.0488 ppb	21:08:08
3	B 249.677†	3076.5	-377.0	-6.3309 µg/L	-6.3309 ppb	21:08:08
3	Ba 233.527†	-187.7	-6.7	-0.0307 µg/L	-0.0307 ppb	21:08:08
3	Be 313.107†	-530.7	146.3	0.0497 µg/L	0.0497 ppb	21:07:47
3	Cd 226.502†	-118.4	-20.2	-0.1396 µg/L	-0.1396 ppb	21:08:08
3	Co 228.616†	-159.8	21.9	0.3001 µg/L	0.3001 ppb	21:08:08
3	Cr 267.716†	166.1	0.6	-0.0009 µg/L	-0.0009 ppb	21:08:08
3	Cu 324.752†	2799.8	285.9	1.2487 µg/L	1.2487 ppb	21:07:47
3	Mn 257.610†	156.9	71.9	0.0985 µg/L	0.0985 ppb	21:08:08
3	Mo 202.031†	-29.4	26.7	0.8435 µg/L	0.8435 ppb	21:08:08
3	Ni 231.604†	-49.4	-6.9	-0.0885 µg/L	-0.0885 ppb	21:08:08
3	P 214.914†	34.7	-45.9	-11.027 µg/L	-11.027 ppb	21:08:08
3	Pb 220.353†	99.2	-16.4	-0.9975 µg/L	-0.9975 ppb	21:08:08
3	S 181.975 Axial†	91.1	-6.6	-5.3466 µg/L	-5.3466 ppb	21:08:08
3	Sb 206.836†	84.8	-4.6	-0.6054 µg/L	-0.6054 ppb	21:08:08
3	Se 196.026†	15.6	4.2	1.65 µg/L	1.65 ppb	21:08:08
3	SiO2†	1696.3	69.5	7.5803 µg/L	7.5803 ppb	21:08:08
3	Si 251.611†	783.8	82.5	1.3544 µg/L	1.3544 ppb	21:08:08
3	Sn 189.927†	-1.7	-3.7	-0.2629 µg/L	-0.2629 ppb	21:08:08
3	Ti 334.940†	938.9	272.7	0.2758 µg/L	0.2758 ppb	21:07:47
3	Tl 190.801†	-117.7	6.3	0.8448 µg/L	0.8448 ppb	21:08:08
3	U 409.014†	-379.0	112.2	6.8863 µg/L	6.8863 ppb	21:07:47
3	V 292.402†	296.9	-144.3	-0.7876 µg/L	-0.7876 ppb	21:07:47
3	Zn 213.857†	483.2	3.5	0.0213 µg/L	0.0213 ppb	21:08:08

Mean Data: CCB

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1727978.8	103.30 %	0.127			0.12%
Sc RADIAL	153662.5	105 %	0.9			0.84%
Y 371.029	1060906.2	103.75 %	0.113			0.11%
Ag 328.068†	69.6	0.2771 µg/L	0.51363	0.2771 ppb	0.51363	185.39%
QC value within limits for Ag 328.068 Recovery = Not calculated						
Al 396.153Radial†	-14.4	-3.1897 µg/L	4.34321	-3.1897 ppb	4.34321	136.17%
QC value within limits for Al 396.153Radial Recovery = Not calculated						
As 188.979†	2.1	0.8654 µg/L	1.92055	0.8654 ppb	1.92055	221.93%
QC value within limits for As 188.979 Recovery = Not calculated						
B 249.677†	-369.5	-6.2037 µg/L	0.48034	-6.2037 ppb	0.48034	7.74%
QC value within limits for B 249.677 Recovery = Not calculated						
Ba 233.527†	-3.3	-0.0156 µg/L	0.06185	-0.0156 ppb	0.06185	395.65%
QC value within limits for Ba 233.527 Recovery = Not calculated						
Be 313.107†	121.6	0.0413 µg/L	0.02134	0.0413 ppb	0.02134	51.70%
QC value within limits for Be 313.107 Recovery = Not calculated						
Ca 317.933Radial†	35.3	2.0699 µg/L	0.72997	2.0699 ppb	0.72997	35.27%
QC value within limits for Ca 317.933Radial Recovery = Not calculated						
Cd 226.502†	9.3	0.0638 µg/L	0.19446	0.0638 ppb	0.19446	304.95%
QC value within limits for Cd 226.502 Recovery = Not calculated						
Co 228.616†	12.7	0.1732 µg/L	0.12276	0.1732 ppb	0.12276	70.87%

Cr 267.716†	QC value within limits for Co 228.616	Recovery = Not calculated				
	-12.2	-0.1092 µg/L	0.09382	-0.1092 ppb	0.09382	85.93%
Cu 324.752†	QC value within limits for Cr 267.716	Recovery = Not calculated				
	191.2	0.8362 µg/L	0.36438	0.8362 ppb	0.36438	43.58%
Fe 238.204 Radial†	QC value within limits for Cu 324.752	Recovery = Not calculated				
	22.5	1.4984 µg/L	0.62279	1.4984 ppb	0.62279	41.56%
K 766.490 Radial†	QC value within limits for Fe 238.204 Radial	Recovery = Not calculated				
	-52.6	-21.634 µg/L	37.3056	-21.634 ppb	37.3056	172.44%
Mg 279.077 IEC†	QC value within limits for K 766.490 Radial	Recovery = Not calculated				
	-10.6	-4.3490 µg/L	7.59366	-4.3490 ppb	7.59366	174.61%
Mn 257.610†	QC value within limits for Mg 279.077 IEC	Recovery = Not calculated				
	72.1	0.0986 µg/L	0.02726	0.0986 ppb	0.02726	27.63%
Mo 202.031†	QC value within limits for Mn 257.610	Recovery = Not calculated				
	34.0	1.0741 µg/L	0.44518	1.0741 ppb	0.44518	41.45%
Na 589.592 Radial†	QC value within limits for Mo 202.031	Recovery = Not calculated				
	-156.3	-23.901 µg/L	5.6641	-23.901 ppb	5.6641	23.70%
Ni 231.604†	QC value within limits for Na 589.592 Radial	Recovery = Not calculated				
	-1.3	-0.0164 µg/L	0.30026	-0.0164 ppb	0.30026	>999.9%
P 214.914†	QC value within limits for Ni 231.604	Recovery = Not calculated				
	-47.0	-11.283 µg/L	2.4255	-11.283 ppb	2.4255	21.50%
Pb 220.353†	QC value within limits for P 214.914	Recovery = Not calculated				
	-19.0	-1.1517 µg/L	0.32775	-1.1517 ppb	0.32775	28.46%
S 181.975 Axial†	QC value within limits for Pb 220.353	Recovery = Not calculated				
	-15.3	-12.373 µg/L	7.9530	-12.373 ppb	7.9530	64.28%
Sb 206.836†	QC value within limits for S 181.975 Axial	Recovery = Not calculated				
	-13.2	-1.7632 µg/L	2.16182	-1.7632 ppb	2.16182	122.61%
Se 196.026†	QC value within limits for Sb 206.836	Recovery = Not calculated				
	7.1	2.83 µg/L	1.094	2.83 ppb	1.094	38.72%
SiO2†	QC value within limits for Se 196.026	Recovery = Not calculated				
	38.4	4.1643 µg/L	3.98373	4.1643 ppb	3.98373	95.66%
Si 251.611†	QC value within limits for SiO2	Recovery = Not calculated				
	82.7	1.3522 µg/L	0.17505	1.3522 ppb	0.17505	12.95%
Sn 189.927†	QC value within limits for Si 251.611	Recovery = Not calculated				
	1.3	0.0958 µg/L	0.39756	0.0958 ppb	0.39756	415.11%
Sr 421.552†	QC value within limits for Sn 189.927	Recovery = Not calculated				
	62.8	0.1473 µg/L	0.07240	0.1473 ppb	0.07240	49.16%
Ti 334.940†	QC value within limits for Sr 421.552	Recovery = Not calculated				
	249.5	0.2525 µg/L	0.12417	0.2525 ppb	0.12417	49.17%
Tl 190.801†	QC value within limits for Ti 334.940	Recovery = Not calculated				
	3.7	0.4963 µg/L	0.58643	0.4963 ppb	0.58643	118.16%
U 409.014†	QC value within limits for Tl 190.801	Recovery = Not calculated				
	90.6	5.5398 µg/L	3.56137	5.5398 ppb	3.56137	64.29%
V 292.402†	QC value within limits for U 409.014	Recovery = Not calculated				
	-187.1	-1.0240 µg/L	0.37548	-1.0240 ppb	0.37548	36.67%
Zn 213.857†	QC value within limits for V 292.402	Recovery = Not calculated				
	16.0	0.1001 µg/L	0.07465	0.1001 ppb	0.07465	74.57%
QC value within limits for Zn 213.857 Recovery = Not calculated						

All analyte(s) passed QC.

Sequence No.: 55

Sample ID: CCV

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 7

Date Collected: 3/29/2010 21:21:26

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCV

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	154714.0	154714.0	106 %		21:21:59
1	Al 396.153Radial†	25548.1	24100.5	5238.5 µg/L	5238.5 ppb	21:21:59
1	Ca 317.933Radial†	89497.2	83698.1	4904.3 µg/L	4904.3 ppb	21:21:59
1	Fe 238.204 Radial†	78346.3	73695.8	4899.6 µg/L	4899.6 ppb	21:21:59
1	K 766.490 Radial†	13948.1	11685.3	4806.5 µg/L	4806.5 ppb	21:21:59
1	Mg 279.077 IEC†	13187.8	12237.4	5053.2 µg/L	5053.2 ppb	21:21:59
1	Na 589.592 Radial†	69758.3	64023.7	9792.2 µg/L	9792.2 ppb	21:21:59
1	Sr 421.552†	228178.1	215241.9	504.43 µg/L	504.43 ppb	21:21:57
1	Sc 361.383	1735452.7	1735452.7	103.75 %		21:22:12
1	Y 371.029	1050791.1	1050791.1	102.76 %		21:22:12
1	Ag 328.068†	128429.5	120824.1	496.54 µg/L	496.54 ppb	21:22:12
1	As 188.979†	1304.3	1271.4	538.44 µg/L	538.44 ppb	21:22:32
1	B 249.677†	33357.7	28797.2	481.77 µg/L	481.77 ppb	21:22:12
1	Ba 233.527†	114396.7	110440.2	504.93 µg/L	504.93 ppb	21:22:12
1	Be 313.107†	1635862.4	1577441.1	513.62 µg/L	513.62 ppb	21:22:12
1	Cd 226.502†	72815.3	70279.9	485.02 µg/L	485.02 ppb	21:22:12
1	Co 228.616†	36981.4	35822.4	490.78 µg/L	490.78 ppb	21:22:12
1	Cr 267.716†	59642.9	57328.5	492.28 µg/L	492.28 ppb	21:22:12
1	Cu 324.752†	120492.9	113716.2	495.85 µg/L	495.85 ppb	21:22:12
1	Mn 257.610†	375406.7	361768.4	494.12 µg/L	494.12 ppb	21:22:12
1	Mo 202.031†	15724.6	15211.9	480.63 µg/L	480.63 ppb	21:22:32
1	Ni 231.604†	39726.7	38332.8	490.32 µg/L	490.32 ppb	21:22:12
1	P 214.914†	10354.3	9900.7	2362.7 µg/L	2362.7 ppb	21:22:32
1	Pb 220.353†	8256.8	7846.2	476.85 µg/L	476.85 ppb	21:22:32
1	S 181.975 Axial†	1288.8	1147.5	933.70 µg/L	933.70 ppb	21:22:32
1	Sb 206.836†	3841.8	3616.4	488.79 µg/L	488.79 ppb	21:22:32
1	Se 196.026†	1256.4	1200.2	477 µg/L	477 ppb	21:22:32
1	SiO2†	51655.1	48216.6	5249.4 µg/L	5249.4 ppb	21:22:12
1	Si 251.611†	155313.5	149027.7	2454.5 µg/L	2454.5 ppb	21:22:12
1	Sn 189.927†	7082.5	6824.6	486.84 µg/L	486.84 ppb	21:22:32
1	Ti 334.940†	504215.8	485369.0	494.29 µg/L	494.29 ppb	21:22:12
1	Tl 190.801†	3584.2	3575.1	487.32 µg/L	487.32 ppb	21:22:32
1	U 409.014†	7243.0	7460.5	491.31 µg/L	491.31 ppb	21:22:12
1	V 292.402†	93303.5	89501.9	502.63 µg/L	502.63 ppb	21:22:12
1	Zn 213.857†	80568.9	77194.6	482.06 µg/L	482.06 ppb	21:22:12
2	Sc RADIAL	155802.8	155802.8	107 %		21:22:03
2	Al 396.153Radial†	25671.7	24047.8	5226.9 µg/L	5226.9 ppb	21:22:03
2	Ca 317.933Radial†	90704.0	84237.8	4936.0 µg/L	4936.0 ppb	21:22:03
2	Fe 238.204 Radial†	79350.7	74119.7	4927.7 µg/L	4927.7 ppb	21:22:03
2	K 766.490 Radial†	14028.1	11668.4	4799.6 µg/L	4799.6 ppb	21:22:03
2	Mg 279.077 IEC†	13391.2	12340.9	5095.9 µg/L	5095.9 ppb	21:22:03
2	Na 589.592 Radial†	70468.8	64229.1	9823.6 µg/L	9823.6 ppb	21:22:03
2	Sr 421.552†	228226.2	213784.6	501.02 µg/L	501.02 ppb	21:22:01
2	Sc 361.383	1718458.2	1718458.2	102.73 %		21:22:35
2	Y 371.029	1040541.3	1040541.3	101.76 %		21:22:35
2	Ag 328.068†	127122.8	120776.3	496.30 µg/L	496.30 ppb	21:22:35
2	As 188.979†	1315.4	1294.6	548.12 µg/L	548.12 ppb	21:22:55
2	B 249.677†	32820.6	28592.4	478.34 µg/L	478.34 ppb	21:22:35
2	Ba 233.527†	112822.5	109998.3	502.91 µg/L	502.91 ppb	21:22:35
2	Be 313.107†	1612596.5	1570387.2	511.32 µg/L	511.32 ppb	21:22:35
2	Cd 226.502†	71251.1	69451.4	479.30 µg/L	479.30 ppb	21:22:35
2	Co 228.616†	36408.8	35617.5	487.97 µg/L	487.97 ppb	21:22:35
2	Cr 267.716†	58690.5	56970.0	489.20 µg/L	489.20 ppb	21:22:35
2	Cu 324.752†	118859.8	113275.1	493.93 µg/L	493.93 ppb	21:22:35
2	Mn 257.610†	369770.3	359860.3	491.51 µg/L	491.51 ppb	21:22:35
2	Mo 202.031†	15667.6	15306.3	483.62 µg/L	483.62 ppb	21:22:55
2	Ni 231.604†	39105.3	38106.6	487.43 µg/L	487.43 ppb	21:22:35
2	P 214.914†	10294.9	9941.7	2372.5 µg/L	2372.5 ppb	21:22:55
2	Pb 220.353†	8226.7	7895.5	479.85 µg/L	479.85 ppb	21:22:55

2	S 181.975 Axial†	1280.0	1151.2	936.74 µg/L	936.74 ppb	21:22:55
2	Sb 206.836†	3824.3	3636.0	491.52 µg/L	491.52 ppb	21:22:55
2	Se 196.026†	1243.4	1199.4	477 µg/L	477 ppb	21:22:55
2	SiO2†	50957.3	48029.8	5228.9 µg/L	5228.9 ppb	21:22:35
2	Si 251.611†	152847.9	148108.2	2439.3 µg/L	2439.3 ppb	21:22:35
2	Sn 189.927†	7068.4	6878.5	490.66 µg/L	490.66 ppb	21:22:55
2	Ti 334.940†	497011.6	483162.6	492.04 µg/L	492.04 ppb	21:22:35
2	Tl 190.801†	3575.6	3600.9	490.75 µg/L	490.75 ppb	21:22:55
2	U 409.014†	7042.3	7334.2	483.35 µg/L	483.35 ppb	21:22:35
2	V 292.402†	91957.7	89081.3	500.31 µg/L	500.31 ppb	21:22:35
2	Zn 213.857†	79391.5	76816.5	479.70 µg/L	479.70 ppb	21:22:35
3	Sc RADIAL	153629.1	153629.1	105 %		21:22:07
3	Al 396.153Radial†	25706.1	24420.3	5308.2 µg/L	5308.2 ppb	21:22:07
3	Ca 317.933Radial†	90217.9	84977.2	4979.3 µg/L	4979.3 ppb	21:22:07
3	Fe 238.204 Radial†	78896.4	74739.0	4968.9 µg/L	4968.9 ppb	21:22:07
3	K 766.490 Radial†	14006.0	11833.0	4867.3 µg/L	4867.3 ppb	21:22:07
3	Mg 279.077 IEC†	13233.2	12368.3	5107.1 µg/L	5107.1 ppb	21:22:07
3	Na 589.592 Radial†	70244.8	64949.4	9933.8 µg/L	9933.8 ppb	21:22:07
3	Sr 421.552†	231320.2	219741.0	514.98 µg/L	514.98 ppb	21:22:05
3	Sc 361.383	1729039.4	1729039.4	103.36 %		21:22:58
3	Y 371.029	1047411.6	1047411.6	102.43 %		21:22:58
3	Ag 328.068†	127427.9	120314.2	494.42 µg/L	494.42 ppb	21:22:58
3	As 188.979†	1312.7	1284.2	543.77 µg/L	543.77 ppb	21:23:18
3	B 249.677†	33004.1	28574.4	478.04 µg/L	478.04 ppb	21:22:58
3	Ba 233.527†	113024.4	109521.5	500.73 µg/L	500.73 ppb	21:22:58
3	Be 313.107†	1619574.1	1567531.4	510.39 µg/L	510.39 ppb	21:22:58
3	Cd 226.502†	71668.9	69431.2	479.16 µg/L	479.16 ppb	21:22:58
3	Co 228.616†	36487.7	35476.9	486.05 µg/L	486.05 ppb	21:22:58
3	Cr 267.716†	59071.0	56988.5	489.36 µg/L	489.36 ppb	21:22:58
3	Cu 324.752†	119482.8	113169.8	493.48 µg/L	493.48 ppb	21:22:58
3	Mn 257.610†	371130.6	358973.6	490.30 µg/L	490.30 ppb	21:22:58
3	Mo 202.031†	15756.3	15298.8	483.38 µg/L	483.38 ppb	21:23:18
3	Ni 231.604†	39442.5	38199.9	488.62 µg/L	488.62 ppb	21:22:58
3	P 214.914†	10384.3	9966.8	2378.5 µg/L	2378.5 ppb	21:23:18
3	Pb 220.353†	8281.8	7899.8	480.11 µg/L	480.11 ppb	21:23:18
3	S 181.975 Axial†	1288.9	1152.1	937.49 µg/L	937.49 ppb	21:23:18
3	Sb 206.836†	3835.5	3624.1	489.90 µg/L	489.90 ppb	21:23:18
3	Se 196.026†	1254.5	1202.8	478 µg/L	478 ppb	21:23:18
3	SiO2†	51174.5	47936.4	5218.7 µg/L	5218.7 ppb	21:22:58
3	Si 251.611†	153310.8	147645.6	2431.6 µg/L	2431.6 ppb	21:22:58
3	Sn 189.927†	7110.2	6876.8	490.54 µg/L	490.54 ppb	21:23:18
3	Ti 334.940†	498783.5	481916.1	490.77 µg/L	490.77 ppb	21:22:58
3	Tl 190.801†	3617.1	3619.7	493.26 µg/L	493.26 ppb	21:23:18
3	U 409.014†	7080.7	7329.4	482.98 µg/L	482.98 ppb	21:22:58
3	V 292.402†	92337.1	88900.5	499.30 µg/L	499.30 ppb	21:22:58
3	Zn 213.857†	79755.1	76695.4	478.93 µg/L	478.93 ppb	21:22:58

Mean Data: CCV

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1727650.1	103.28 %	0.513			0.50%
Sc RADIAL	154715.3	106 %	0.7			0.70%
Y 371.029	1046248.0	102.31 %	0.511			0.50%
Ag 328.068†	120638.2	495.75 µg/L	1.163	495.75 ppb	1.163	0.23%
QC value within limits for Ag 328.068 Recovery = 99.15%						
Al 396.153Radial†	24189.5	5257.9 µg/L	43.98	5257.9 ppb	43.98	0.84%
QC value within limits for Al 396.153Radial Recovery = 105.16%						
As 188.979†	1283.4	543.44 µg/L	4.846	543.44 ppb	4.846	0.89%
QC value within limits for As 188.979 Recovery = 108.69%						
B 249.677†	28654.7	479.38 µg/L	2.070	479.38 ppb	2.070	0.43%
QC value within limits for B 249.677 Recovery = 95.88%						
Ba 233.527†	109986.6	502.86 µg/L	2.100	502.86 ppb	2.100	0.42%
QC value within limits for Ba 233.527 Recovery = 100.57%						
Be 313.107†	1571786.6	511.78 µg/L	1.662	511.78 ppb	1.662	0.32%
QC value within limits for Be 313.107 Recovery = 102.36%						
Ca 317.933Radial†	84304.4	4939.9 µg/L	37.63	4939.9 ppb	37.63	0.76%
QC value within limits for Ca 317.933Radial Recovery = 98.80%						
Cd 226.502†	69720.8	481.16 µg/L	3.348	481.16 ppb	3.348	0.70%
QC value within limits for Cd 226.502 Recovery = 96.23%						
Co 228.616†	35638.9	488.27 µg/L	2.383	488.27 ppb	2.383	0.49%

QC value within limits for Co 228.616 Recovery = 97.65%						
Cr 267.716†	57095.7	490.28 µg/L	1.730	490.28 ppb	1.730	0.35%
QC value within limits for Cr 267.716 Recovery = 98.06%						
Cu 324.752†	113387.0	494.42 µg/L	1.260	494.42 ppb	1.260	0.25%
QC value within limits for Cu 324.752 Recovery = 98.88%						
Fe 238.204 Radial†	74184.8	4932.1 µg/L	34.88	4932.1 ppb	34.88	0.71%
QC value within limits for Fe 238.204 Radial Recovery = 98.64%						
K 766.490 Radial†	11728.9	4824.5 µg/L	37.26	4824.5 ppb	37.26	0.77%
QC value within limits for K 766.490 Radial Recovery = 96.49%						
Mg 279.077 IEC†	12315.5	5085.4 µg/L	28.47	5085.4 ppb	28.47	0.56%
QC value within limits for Mg 279.077 IEC Recovery = 101.71%						
Mn 257.610†	360200.8	491.98 µg/L	1.953	491.98 ppb	1.953	0.40%
QC value within limits for Mn 257.610 Recovery = 98.40%						
Mo 202.031†	15272.3	482.54 µg/L	1.658	482.54 ppb	1.658	0.34%
QC value within limits for Mo 202.031 Recovery = 96.51%						
Na 589.592 Radial†	64400.7	9849.8 µg/L	74.35	9849.8 ppb	74.35	0.75%
QC value within limits for Na 589.592 Radial Recovery = 98.50%						
Ni 231.604†	38213.1	488.79 µg/L	1.454	488.79 ppb	1.454	0.30%
QC value within limits for Ni 231.604 Recovery = 97.76%						
P 214.914†	9936.4	2371.2 µg/L	7.98	2371.2 ppb	7.98	0.34%
QC value within limits for P 214.914 Recovery = 94.85%						
Pb 220.353†	7880.5	478.93 µg/L	1.813	478.93 ppb	1.813	0.38%
QC value within limits for Pb 220.353 Recovery = 95.79%						
S 181.975 Axial†	1150.2	935.98 µg/L	2.006	935.98 ppb	2.006	0.21%
QC value within limits for S 181.975 Axial Recovery = 93.60%						
Sb 206.836†	3625.5	490.07 µg/L	1.373	490.07 ppb	1.373	0.28%
QC value within limits for Sb 206.836 Recovery = 98.01%						
Se 196.026†	1200.8	477 µg/L	0.7	477 ppb	0.7	0.15%
QC value within limits for Se 196.026 Recovery = 95.42%						
SiO2†	48060.9	5232.3 µg/L	15.67	5232.3 ppb	15.67	0.30%
QC value within limits for SiO2 Recovery = 97.85%						
Si 251.611†	148260.5	2441.8 µg/L	11.67	2441.8 ppb	11.67	0.48%
QC value within limits for Si 251.611 Recovery = 97.67%						
Sn 189.927†	6860.0	489.35 µg/L	2.170	489.35 ppb	2.170	0.44%
QC value within limits for Sn 189.927 Recovery = 97.87%						
Sr 421.552†	216255.8	506.81 µg/L	7.277	506.81 ppb	7.277	1.44%
QC value within limits for Sr 421.552 Recovery = 101.36%						
Ti 334.940†	483482.6	492.36 µg/L	1.782	492.36 ppb	1.782	0.36%
QC value within limits for Ti 334.940 Recovery = 98.47%						
Tl 190.801†	3598.6	490.44 µg/L	2.982	490.44 ppb	2.982	0.61%
QC value within limits for Tl 190.801 Recovery = 98.09%						
U 409.014†	7374.7	485.88 µg/L	4.704	485.88 ppb	4.704	0.97%
QC value within limits for U 409.014 Recovery = 97.18%						
V 292.402†	89161.2	500.74 µg/L	1.709	500.74 ppb	1.709	0.34%
QC value within limits for V 292.402 Recovery = 100.15%						
Zn 213.857†	76902.2	480.23 µg/L	1.635	480.23 ppb	1.635	0.34%
QC value within limits for Zn 213.857 Recovery = 96.05%						

All analyte(s) passed QC.

Sequence No.: 56

Sample ID: CCB

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 8

Date Collected: 3/29/2010 21:23:26

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCB

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	155306.1	155306.1	107 %		21:23:55
1	Al 396.153Radial†	-24.3	9.1	1.9543 µg/L	1.9543 ppb	21:24:15
1	Ca 317.933Radial†	683.7	25.5	1.4938 µg/L	1.4938 ppb	21:24:15
1	Fe 238.204 Radial†	158.4	35.3	2.3500 µg/L	2.3500 ppb	21:24:15
1	K 766.490 Radial†	1643.9	87.8	36.134 µg/L	36.134 ppb	21:23:55
1	Mg 279.077 IEC†	167.4	-29.6	-12.187 µg/L	-12.187 ppb	21:24:15
1	Na 589.592 Radial†	1516.3	-271.7	-41.602 µg/L	-41.602 ppb	21:23:55
1	Sr 421.552†	-242.4	50.5	0.1183 µg/L	0.1183 ppb	21:23:55
1	Sc 361.383	1748094.6	1748094.6	104.50 %		21:25:03
1	Y 371.029	1071566.5	1071566.5	104.79 %		21:25:03
1	Ag 328.068†	3427.1	312.3	1.2793 µg/L	1.2793 ppb	21:25:05
1	As 188.979†	-13.5	1.3	0.5449 µg/L	0.5449 ppb	21:25:25
1	B 249.677†	3112.2	-377.5	-6.3385 µg/L	-6.3385 ppb	21:25:25
1	Ba 233.527†	-154.2	27.5	0.1256 µg/L	0.1256 ppb	21:25:25
1	Be 313.107†	-701.4	-11.1	0.0002 µg/L	0.0002 ppb	21:25:05
1	Cd 226.502†	-80.7	17.1	0.1180 µg/L	0.1180 ppb	21:25:25
1	Co 228.616†	-180.0	4.3	0.0591 µg/L	0.0591 ppb	21:25:25
1	Cr 267.716†	154.7	-12.2	-0.1146 µg/L	-0.1146 ppb	21:25:25
1	Cu 324.752†	2711.0	169.4	0.7467 µg/L	0.7467 ppb	21:25:05
1	Mn 257.610†	174.7	87.2	0.1196 µg/L	0.1196 ppb	21:25:25
1	Mo 202.031†	-33.7	22.9	0.7232 µg/L	0.7232 ppb	21:25:25
1	Ni 231.604†	-63.8	-20.2	-0.2580 µg/L	-0.2580 ppb	21:25:25
1	P 214.914†	25.7	-55.0	-13.175 µg/L	-13.175 ppb	21:25:25
1	Pb 220.353†	88.4	-27.8	-1.6943 µg/L	-1.6943 ppb	21:25:25
1	S 181.975 Axial†	88.7	-10.0	-8.0713 µg/L	-8.0713 ppb	21:25:25
1	Sb 206.836†	103.6	12.5	1.6953 µg/L	1.6953 ppb	21:25:25
1	Se 196.026†	29.5	17.3	6.85 µg/L	6.85 ppb	21:25:25
1	SiO2†	1690.4	44.8	4.8636 µg/L	4.8636 ppb	21:25:25
1	Si 251.611†	812.1	100.8	1.6531 µg/L	1.6531 ppb	21:25:25
1	Sn 189.927†	9.4	7.0	0.4982 µg/L	0.4982 ppb	21:25:25
1	Ti 334.940†	734.9	66.9	0.0641 µg/L	0.0641 ppb	21:25:05
1	Tl 190.801†	-117.2	8.2	1.0976 µg/L	1.0976 ppb	21:25:25
1	U 409.014†	-286.2	205.2	12.661 µg/L	12.661 ppb	21:25:05
1	V 292.402†	393.2	-55.5	-0.2928 µg/L	-0.2928 ppb	21:25:05
1	Zn 213.857†	542.6	54.8	0.3462 µg/L	0.3462 ppb	21:25:25
2	Sc RADIAL	153477.3	153477.3	105 %		21:24:17
2	Al 396.153Radial†	-47.4	-13.1	-2.9442 µg/L	-2.9442 ppb	21:24:37
2	Ca 317.933Radial†	711.1	59.1	3.4638 µg/L	3.4638 ppb	21:24:37
2	Fe 238.204 Radial†	171.6	49.7	3.3060 µg/L	3.3060 ppb	21:24:37
2	K 766.490 Radial†	1553.5	20.3	8.3817 µg/L	8.3817 ppb	21:24:17
2	Mg 279.077 IEC†	185.8	-10.2	-4.1787 µg/L	-4.1787 ppb	21:24:37
2	Na 589.592 Radial†	1510.8	-259.9	-39.777 µg/L	-39.777 ppb	21:24:17
2	Sr 421.552†	-111.6	172.0	0.4031 µg/L	0.4031 ppb	21:24:17
2	Sc 361.383	1741520.5	1741520.5	104.11 %		21:25:27
2	Y 371.029	1067626.4	1067626.4	104.41 %		21:25:27
2	Ag 328.068†	3414.4	312.6	1.2772 µg/L	1.2772 ppb	21:25:29
2	As 188.979†	-19.8	-4.8	-1.9816 µg/L	-1.9816 ppb	21:25:49
2	B 249.677†	3071.8	-405.2	-6.8037 µg/L	-6.8037 ppb	21:25:49
2	Ba 233.527†	-157.9	23.4	0.1075 µg/L	0.1075 ppb	21:25:49
2	Be 313.107†	-655.5	30.5	0.0121 µg/L	0.0121 ppb	21:25:29
2	Cd 226.502†	-93.0	5.0	0.0343 µg/L	0.0343 ppb	21:25:49
2	Co 228.616†	-157.6	25.2	0.3454 µg/L	0.3454 ppb	21:25:49
2	Cr 267.716†	146.2	-19.8	-0.1753 µg/L	-0.1753 ppb	21:25:49
2	Cu 324.752†	2664.3	134.2	0.5901 µg/L	0.5901 ppb	21:25:29
2	Mn 257.610†	201.1	113.2	0.1548 µg/L	0.1548 ppb	21:25:49
2	Mo 202.031†	-3.9	51.4	1.6241 µg/L	1.6241 ppb	21:25:49
2	Ni 231.604†	-71.2	-27.4	-0.3510 µg/L	-0.3510 ppb	21:25:49
2	P 214.914†	49.3	-32.2	-7.7507 µg/L	-7.7507 ppb	21:25:49
2	Pb 220.353†	105.7	-10.9	-0.6592 µg/L	-0.6592 ppb	21:25:49

2	S 181.975 Axial†	91.8	-6.6	-5.3552 µg/L	-5.3552 ppb	21:25:49
2	Sb 206.836†	83.1	-6.8	-0.8931 µg/L	-0.8931 ppb	21:25:49
2	Se 196.026†	11.8	0.5	0.191 µg/L	0.191 ppb	21:25:49
2	SiO2†	1682.8	43.5	4.7163 µg/L	4.7163 ppb	21:25:49
2	Si 251.611†	832.1	122.9	2.0124 µg/L	2.0124 ppb	21:25:49
2	Sn 189.927†	-2.3	-4.2	-0.2990 µg/L	-0.2990 ppb	21:25:49
2	Ti 334.940†	806.8	138.6	0.1389 µg/L	0.1389 ppb	21:25:29
2	Tl 190.801†	-103.8	20.6	2.7680 µg/L	2.7680 ppb	21:25:49
2	U 409.014†	-377.6	116.4	7.1940 µg/L	7.1940 ppb	21:25:29
2	V 292.402†	451.2	1.6	0.0290 µg/L	0.0290 ppb	21:25:29
2	Zn 213.857†	515.7	30.9	0.1963 µg/L	0.1963 ppb	21:25:49
3	Sc RADIAL	150012.7	150012.7	103 %		21:24:39
3	Al 396.153Radial†	-29.8	2.9	0.5867 µg/L	0.5867 ppb	21:24:59
3	Ca 317.933Radial†	710.4	74.0	4.3369 µg/L	4.3369 ppb	21:24:59
3	Fe 238.204 Radial†	151.9	34.3	2.2797 µg/L	2.2797 ppb	21:24:59
3	K 766.490 Radial†	1399.3	-95.4	-39.262 µg/L	-39.262 ppb	21:24:39
3	Mg 279.077 IEC†	165.1	-26.3	-10.817 µg/L	-10.817 ppb	21:24:59
3	Na 589.592 Radial†	1639.2	-102.0	-15.574 µg/L	-15.574 ppb	21:24:39
3	Sr 421.552†	-287.8	-1.6	-0.0038 µg/L	-0.0038 ppb	21:24:39
3	Sc 361.383	1723128.2	1723128.2	103.01 %		21:25:51
3	Y 371.029	1057308.7	1057308.7	103.40 %		21:25:51
3	Ag 328.068†	3346.0	281.2	1.1646 µg/L	1.1646 ppb	21:25:53
3	As 188.979†	-18.6	-3.8	-1.5909 µg/L	-1.5909 ppb	21:26:14
3	B 249.677†	3052.0	-392.9	-6.5974 µg/L	-6.5974 ppb	21:26:14
3	Ba 233.527†	-170.9	9.2	0.0418 µg/L	0.0418 ppb	21:26:14
3	Be 313.107†	-474.6	199.4	0.0725 µg/L	0.0725 ppb	21:25:53
3	Cd 226.502†	-97.7	-0.4	-0.0033 µg/L	-0.0033 ppb	21:26:14
3	Co 228.616†	-155.6	25.6	0.3503 µg/L	0.3503 ppb	21:26:14
3	Cr 267.716†	182.3	16.7	0.1237 µg/L	0.1237 ppb	21:26:14
3	Cu 324.752†	2711.9	207.8	0.9243 µg/L	0.9243 ppb	21:25:53
3	Mn 257.610†	171.1	86.1	0.1180 µg/L	0.1180 ppb	21:26:14
3	Mo 202.031†	-16.8	38.9	1.2275 µg/L	1.2275 ppb	21:26:14
3	Ni 231.604†	-81.5	-38.2	-0.4887 µg/L	-0.4887 ppb	21:26:14
3	P 214.914†	37.1	-43.6	-10.455 µg/L	-10.455 ppb	21:26:14
3	Pb 220.353†	81.7	-33.1	-2.0187 µg/L	-2.0187 ppb	21:26:14
3	S 181.975 Axial†	91.8	-5.7	-4.6479 µg/L	-4.6479 ppb	21:26:14
3	Sb 206.836†	81.4	-7.6	-1.0134 µg/L	-1.0134 ppb	21:26:14
3	Se 196.026†	21.3	9.8	3.89 µg/L	3.89 ppb	21:26:14
3	SiO2†	1680.3	58.3	6.3388 µg/L	6.3388 ppb	21:26:14
3	Si 251.611†	807.9	107.9	1.7669 µg/L	1.7669 ppb	21:26:14
3	Sn 189.927†	3.7	1.6	0.1137 µg/L	0.1137 ppb	21:26:14
3	Ti 334.940†	1049.1	382.1	0.3802 µg/L	0.3802 ppb	21:25:53
3	Tl 190.801†	-103.5	19.8	2.6620 µg/L	2.6620 ppb	21:26:14
3	U 409.014†	-71.7	409.5	25.265 µg/L	25.265 ppb	21:25:53
3	V 292.402†	327.3	-114.1	-0.6031 µg/L	-0.6031 ppb	21:25:53
3	Zn 213.857†	513.6	34.2	0.2177 µg/L	0.2177 ppb	21:26:14

Mean Data: CCB

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1737581.1	103.87 %	0.774			0.74%
Sc RADIAL	152932.0	105 %	1.8			1.76%
Y 371.029	1065500.5	104.20 %	0.720			0.69%
Ag 328.068†	302.0	1.2404 µg/L	0.06566	1.2404 ppb	0.06566	5.29%
QC value within limits for Ag 328.068 Recovery = Not calculated						
Al 396.153Radial†	-0.4	-0.1344 µg/L	2.52760	-0.1344 ppb	2.52760	>999.9%
QC value within limits for Al 396.153Radial Recovery = Not calculated						
As 188.979†	-2.4	-1.0092 µg/L	1.36000	-1.0092 ppb	1.36000	134.76%
QC value within limits for As 188.979 Recovery = Not calculated						
B 249.677†	-391.9	-6.5799 µg/L	0.23305	-6.5799 ppb	0.23305	3.54%
QC value within limits for B 249.677 Recovery = Not calculated						
Ba 233.527†	20.0	0.0916 µg/L	0.04412	0.0916 ppb	0.04412	48.14%
QC value within limits for Ba 233.527 Recovery = Not calculated						
Be 313.107†	72.9	0.0283 µg/L	0.03879	0.0283 ppb	0.03879	137.14%
QC value within limits for Be 313.107 Recovery = Not calculated						
Ca 317.933Radial†	52.9	3.0982 µg/L	1.45639	3.0982 ppb	1.45639	47.01%
QC value within limits for Ca 317.933Radial Recovery = Not calculated						
Cd 226.502†	7.3	0.0497 µg/L	0.06207	0.0497 ppb	0.06207	124.90%
QC value within limits for Cd 226.502 Recovery = Not calculated						
Co 228.616†	18.4	0.2516 µg/L	0.16669	0.2516 ppb	0.16669	66.25%

QC value within limits for Co 228.616 Recovery = Not calculated					
Cr 267.716†	-5.1	-0.0554 µg/L	0.15802	-0.0554 ppb	0.15802 285.26%
QC value within limits for Cr 267.716 Recovery = Not calculated					
Cu 324.752†	170.5	0.7537 µg/L	0.16723	0.7537 ppb	0.16723 22.19%
QC value within limits for Cu 324.752 Recovery = Not calculated					
Fe 238.204 Radial†	39.8	2.6452 µg/L	0.57333	2.6452 ppb	0.57333 21.67%
QC value within limits for Fe 238.204 Radial Recovery = Not calculated					
K 766.490 Radial†	4.2	1.7511 µg/L	38.13273	1.7511 ppb	38.13273 >999.9%
QC value within limits for K 766.490 Radial Recovery = Not calculated					
Mg 279.077 IEC†	-22.0	-9.0611 µg/L	4.28341	-9.0611 ppb	4.28341 47.27%
QC value within limits for Mg 279.077 IEC Recovery = Not calculated					
Mn 257.610†	95.5	0.1308 µg/L	0.02079	0.1308 ppb	0.02079 15.90%
QC value within limits for Mn 257.610 Recovery = Not calculated					
Mo 202.031†	37.8	1.1916 µg/L	0.45152	1.1916 ppb	0.45152 37.89%
QC value within limits for Mo 202.031 Recovery = Not calculated					
Na 589.592 Radial†	-211.2	-32.318 µg/L	14.5288	-32.318 ppb	14.5288 44.96%
QC value within limits for Na 589.592 Radial Recovery = Not calculated					
Ni 231.604†	-28.6	-0.3659 µg/L	0.11605	-0.3659 ppb	0.11605 31.72%
QC value within limits for Ni 231.604 Recovery = Not calculated					
P 214.914†	-43.6	-10.460 µg/L	2.7120	-10.460 ppb	2.7120 25.93%
QC value within limits for P 214.914 Recovery = Not calculated					
Pb 220.353†	-23.9	-1.4574 µg/L	0.70999	-1.4574 ppb	0.70999 48.72%
QC value within limits for Pb 220.353 Recovery = Not calculated					
S 181.975 Axial†	-7.4	-6.0248 µg/L	1.80725	-6.0248 ppb	1.80725 30.00%
QC value within limits for S 181.975 Axial Recovery = Not calculated					
Sb 206.836†	-0.6	-0.0704 µg/L	1.53036	-0.0704 ppb	1.53036 >999.9%
QC value within limits for Sb 206.836 Recovery = Not calculated					
Se 196.026†	9.2	3.64 µg/L	3.337	3.64 ppb	3.337 91.59%
QC value within limits for Se 196.026 Recovery = Not calculated					
SiO2†	48.9	5.3062 µg/L	0.89725	5.3062 ppb	0.89725 16.91%
QC value within limits for SiO2 Recovery = Not calculated					
Si 251.611†	110.5	1.8108 µg/L	0.18363	1.8108 ppb	0.18363 10.14%
QC value within limits for Si 251.611 Recovery = Not calculated					
Sn 189.927†	1.5	0.1043 µg/L	0.39868	0.1043 ppb	0.39868 382.19%
QC value within limits for Sn 189.927 Recovery = Not calculated					
Sr 421.552†	73.6	0.1725 µg/L	0.20882	0.1725 ppb	0.20882 121.03%
QC value within limits for Sr 421.552 Recovery = Not calculated					
Ti 334.940†	195.9	0.1944 µg/L	0.16524	0.1944 ppb	0.16524 85.00%
QC value within limits for Ti 334.940 Recovery = Not calculated					
Tl 190.801†	16.2	2.1759 µg/L	0.93532	2.1759 ppb	0.93532 42.99%
QC value within limits for Tl 190.801 Recovery = Not calculated					
U 409.014†	243.7	15.040 µg/L	9.2675	15.040 ppb	9.2675 61.62%
QC value within limits for U 409.014 Recovery = Not calculated					
V 292.402†	-56.0	-0.2890 µg/L	0.31607	-0.2890 ppb	0.31607 109.37%
QC value within limits for V 292.402 Recovery = Not calculated					
Zn 213.857†	40.0	0.2534 µg/L	0.08112	0.2534 ppb	0.08112 32.01%
QC value within limits for Zn 213.857 Recovery = Not calculated					
All analyte(s) passed QC.					

Sequence No.: 64

Sample ID: CCV

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 7

Date Collected: 3/29/2010 21:41:23

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCV

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	155141.6	155141.6	106 %		21:41:56
1	Al 396.153Radial†	25732.1	24207.0	5261.9 µg/L	5261.9 ppb	21:41:56
1	Ca 317.933Radial†	90696.3	84592.2	4956.7 µg/L	4956.7 ppb	21:41:56
1	Fe 238.204 Radial†	79315.9	74403.3	4946.6 µg/L	4946.6 ppb	21:41:56
1	K 766.490 Radial†	13939.8	11641.4	4788.4 µg/L	4788.4 ppb	21:41:56
1	Mg 279.077 IEC†	13393.7	12396.6	5118.7 µg/L	5118.7 ppb	21:41:56
1	Na 589.592 Radial†	70468.0	64509.4	9866.5 µg/L	9866.5 ppb	21:41:56
1	Sr 421.552†	232398.2	218614.1	512.33 µg/L	512.33 ppb	21:41:53
1	Sc 361.383	1769586.3	1769586.3	105.79 %		21:42:08
1	Y 371.029	1071797.7	1071797.7	104.81 %		21:42:08
1	Ag 328.068†	129603.3	119545.9	491.31 µg/L	491.31 ppb	21:42:08
1	As 188.979†	1329.3	1270.8	538.12 µg/L	538.12 ppb	21:42:28
1	B 249.677†	33677.3	28479.2	476.45 µg/L	476.45 ppb	21:42:08
1	Ba 233.527†	115439.2	109298.8	499.71 µg/L	499.71 ppb	21:42:08
1	Be 313.107†	1651472.1	1561782.3	508.53 µg/L	508.53 ppb	21:42:08
1	Cd 226.502†	73101.7	69196.8	477.54 µg/L	477.54 ppb	21:42:08
1	Co 228.616†	37176.9	35319.6	483.89 µg/L	483.89 ppb	21:42:08
1	Cr 267.716†	60164.7	56712.9	486.98 µg/L	486.98 ppb	21:42:08
1	Cu 324.752†	121865.1	112773.1	491.76 µg/L	491.76 ppb	21:42:08
1	Mn 257.610†	378134.2	357367.0	488.10 µg/L	488.10 ppb	21:42:08
1	Mo 202.031†	15933.4	15116.9	477.64 µg/L	477.64 ppb	21:42:28
1	Ni 231.604†	40031.5	37882.3	484.56 µg/L	484.56 ppb	21:42:08
1	P 214.914†	10529.6	9874.0	2356.3 µg/L	2356.3 ppb	21:42:28
1	Pb 220.353†	8381.8	7810.8	474.69 µg/L	474.69 ppb	21:42:28
1	S 181.975 Axial†	1319.0	1152.0	937.38 µg/L	937.38 ppb	21:42:28
1	Sb 206.836†	3878.6	3579.8	483.87 µg/L	483.87 ppb	21:42:28
1	Se 196.026†	1271.4	1191.0	473 µg/L	473 ppb	21:42:28
1	SiO2†	52156.9	47730.6	5196.4 µg/L	5196.4 ppb	21:42:08
1	Si 251.611†	156637.6	147391.8	2427.5 µg/L	2427.5 ppb	21:42:08
1	Sn 189.927†	7201.5	6805.5	485.46 µg/L	485.46 ppb	21:42:28
1	Ti 334.940†	508354.7	479906.9	488.71 µg/L	488.71 ppb	21:42:08
1	Tl 190.801†	3635.0	3556.4	484.75 µg/L	484.75 ppb	21:42:28
1	U 409.014†	7495.6	7564.6	497.45 µg/L	497.45 ppb	21:42:08
1	V 292.402†	94313.8	88722.2	498.25 µg/L	498.25 ppb	21:42:08
1	Zn 213.857†	81212.0	76304.6	476.49 µg/L	476.49 ppb	21:42:08
2	Sc RADIAL	152571.4	152571.4	105 %		21:42:00
2	Al 396.153Radial†	25314.1	24214.9	5263.2 µg/L	5263.2 ppb	21:42:00
2	Ca 317.933Radial†	88626.2	84050.0	4925.0 µg/L	4925.0 ppb	21:42:00
2	Fe 238.204 Radial†	77784.9	74196.0	4932.8 µg/L	4932.8 ppb	21:42:00
2	K 766.490 Radial†	13885.1	11809.7	4857.7 µg/L	4857.7 ppb	21:42:00
2	Mg 279.077 IEC†	13015.3	12247.1	5057.3 µg/L	5057.3 ppb	21:42:00
2	Na 589.592 Radial†	69451.8	64653.8	9888.5 µg/L	9888.5 ppb	21:42:00
2	Sr 421.552†	226457.0	216616.4	507.65 µg/L	507.65 ppb	21:41:58
2	Sc 361.383	1736903.3	1736903.3	103.83 %		21:42:32
2	Y 371.029	1053285.4	1053285.4	103.00 %		21:42:32
2	Ag 328.068†	128049.4	120354.6	494.59 µg/L	494.59 ppb	21:42:32
2	As 188.979†	1336.9	1301.8	551.11 µg/L	551.11 ppb	21:42:52
2	B 249.677†	32949.6	28377.4	474.74 µg/L	474.74 ppb	21:42:32
2	Ba 233.527†	113487.1	109472.1	500.51 µg/L	500.51 ppb	21:42:32
2	Be 313.107†	1622396.8	1563155.8	508.97 µg/L	508.97 ppb	21:42:32
2	Cd 226.502†	71970.0	69407.2	478.99 µg/L	478.99 ppb	21:42:32
2	Co 228.616†	36579.3	35405.4	485.07 µg/L	485.07 ppb	21:42:32
2	Cr 267.716†	59093.3	56751.3	487.32 µg/L	487.32 ppb	21:42:32
2	Cu 324.752†	119729.1	112883.6	492.24 µg/L	492.24 ppb	21:42:32
2	Mn 257.610†	371985.4	358171.2	489.21 µg/L	489.21 ppb	21:42:32
2	Mo 202.031†	15973.6	15439.0	487.80 µg/L	487.80 ppb	21:42:52
2	Ni 231.604†	39464.7	38048.6	486.69 µg/L	486.69 ppb	21:42:32
2	P 214.914†	10515.6	10047.8	2397.9 µg/L	2397.9 ppb	21:42:52
2	Pb 220.353†	8420.5	7997.2	486.01 µg/L	486.01 ppb	21:42:52

2	S 181.975 Axial†	1316.9	1173.4	954.81 µg/L	954.81 ppb	21:42:52
2	Sb 206.836†	3875.7	3646.0	492.95 µg/L	492.95 ppb	21:42:52
2	Se 196.026†	1265.9	1208.2	480 µg/L	480 ppb	21:42:52
2	SiO2†	51399.8	47929.2	5217.7 µg/L	5217.7 ppb	21:42:32
2	Si 251.611†	153711.9	147360.2	2426.8 µg/L	2426.8 ppb	21:42:32
2	Sn 189.927†	7192.7	6925.1	493.97 µg/L	493.97 ppb	21:42:52
2	Ti 334.940†	500404.8	481292.9	490.13 µg/L	490.13 ppb	21:42:32
2	Tl 190.801†	3631.2	3617.4	492.94 µg/L	492.94 ppb	21:42:52
2	U 409.014†	7251.0	7462.4	491.17 µg/L	491.17 ppb	21:42:32
2	V 292.402†	92671.4	88818.0	498.89 µg/L	498.89 ppb	21:42:32
2	Zn 213.857†	79943.3	76527.3	477.88 µg/L	477.88 ppb	21:42:32
3	Sc RADIAL	153899.6	153899.6	106 %		21:42:04
3	Al 396.153Radial†	25427.3	24113.4	5241.3 µg/L	5241.3 ppb	21:42:04
3	Ca 317.933Radial†	89584.3	84226.7	4935.3 µg/L	4935.3 ppb	21:42:04
3	Fe 238.204 Radial†	78451.3	74185.8	4932.1 µg/L	4932.1 ppb	21:42:04
3	K 766.490 Radial†	13947.9	11754.7	4835.1 µg/L	4835.1 ppb	21:42:04
3	Mg 279.077 IEC†	13129.1	12247.5	5057.3 µg/L	5057.3 ppb	21:42:04
3	Na 589.592 Radial†	69867.9	64475.3	9861.2 µg/L	9861.2 ppb	21:42:04
3	Sr 421.552†	230570.5	218645.2	512.41 µg/L	512.41 ppb	21:42:02
3	Sc 361.383	1756529.9	1756529.9	105.01 %		21:42:55
3	Y 371.029	1063628.8	1063628.8	104.01 %		21:42:55
3	Ag 328.068†	129932.1	120769.6	496.30 µg/L	496.30 ppb	21:42:55
3	As 188.979†	1327.9	1278.8	541.51 µg/L	541.51 ppb	21:43:15
3	B 249.677†	33771.3	28805.3	481.91 µg/L	481.91 ppb	21:42:55
3	Ba 233.527†	115375.4	110049.1	503.14 µg/L	503.14 ppb	21:42:55
3	Be 313.107†	1656355.2	1578036.4	513.82 µg/L	513.82 ppb	21:42:55
3	Cd 226.502†	73621.8	70205.8	484.51 µg/L	484.51 ppb	21:42:55
3	Co 228.616†	37314.4	35711.8	489.27 µg/L	489.27 ppb	21:42:55
3	Cr 267.716†	60209.2	57178.1	490.99 µg/L	490.99 ppb	21:42:55
3	Cu 324.752†	121793.5	113561.3	495.18 µg/L	495.18 ppb	21:42:55
3	Mn 257.610†	379257.5	361093.6	493.20 µg/L	493.20 ppb	21:42:55
3	Mo 202.031†	15953.4	15247.9	481.77 µg/L	481.77 ppb	21:43:15
3	Ni 231.604†	40238.5	38360.8	490.68 µg/L	490.68 ppb	21:42:55
3	P 214.914†	10528.4	9946.8	2373.7 µg/L	2373.7 ppb	21:43:15
3	Pb 220.353†	8392.4	7879.8	478.89 µg/L	478.89 ppb	21:43:15
3	S 181.975 Axial†	1322.2	1164.3	947.34 µg/L	947.34 ppb	21:43:15
3	Sb 206.836†	3881.7	3610.0	487.96 µg/L	487.96 ppb	21:43:15
3	Se 196.026†	1265.3	1194.1	474 µg/L	474 ppb	21:43:15
3	SiO2†	52227.4	48164.2	5243.6 µg/L	5243.6 ppb	21:42:55
3	Si 251.611†	156492.0	148353.7	2443.4 µg/L	2443.4 ppb	21:42:55
3	Sn 189.927†	7205.6	6860.0	489.35 µg/L	489.35 ppb	21:43:15
3	Ti 334.940†	508571.1	483684.9	492.57 µg/L	492.57 ppb	21:42:55
3	Tl 190.801†	3639.0	3585.7	488.73 µg/L	488.73 ppb	21:43:15
3	U 409.014†	7286.8	7418.4	488.63 µg/L	488.63 ppb	21:42:55
3	V 292.402†	94216.9	89292.6	501.47 µg/L	501.47 ppb	21:42:55
3	Zn 213.857†	81432.1	77084.8	481.37 µg/L	481.37 ppb	21:42:55

Mean Data: CCV

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1754339.8	104.88 %	0.983			0.94%
Sc RADIAL	153870.9	106 %	0.9			0.84%
Y 371.029	1062904.0	103.94 %	0.907			0.87%
Ag 328.068†	120223.3	494.06 µg/L	2.537	494.06 ppb	2.537	0.51%
QC value within limits for Ag 328.068 Recovery = 98.81%						
Al 396.153Radial†	24178.4	5255.5 µg/L	12.29	5255.5 ppb	12.29	0.23%
QC value within limits for Al 396.153Radial Recovery = 105.11%						
As 188.979†	1283.8	543.58 µg/L	6.739	543.58 ppb	6.739	1.24%
QC value within limits for As 188.979 Recovery = 108.72%						
B 249.677†	28554.0	477.70 µg/L	3.745	477.70 ppb	3.745	0.78%
QC value within limits for B 249.677 Recovery = 95.54%						
Ba 233.527†	109606.6	501.12 µg/L	1.796	501.12 ppb	1.796	0.36%
QC value within limits for Ba 233.527 Recovery = 100.22%						
Be 313.107†	1567658.2	510.44 µg/L	2.933	510.44 ppb	2.933	0.57%
QC value within limits for Be 313.107 Recovery = 102.09%						
Ca 317.933Radial†	84289.7	4939.0 µg/L	16.20	4939.0 ppb	16.20	0.33%
QC value within limits for Ca 317.933Radial Recovery = 98.78%						
Cd 226.502†	69603.2	480.35 µg/L	3.678	480.35 ppb	3.678	0.77%
QC value within limits for Cd 226.502 Recovery = 96.07%						
Co 228.616†	35478.9	486.07 µg/L	2.825	486.07 ppb	2.825	0.58%

QC value within limits for Co 228.616 Recovery = 97.21%							
Cr 267.716†	56880.8	488.43 µg/L	2.221	488.43 ppb	2.221	0.45%	
QC value within limits for Cr 267.716 Recovery = 97.69%							
Cu 324.752†	113072.7	493.06 µg/L	1.852	493.06 ppb	1.852	0.38%	
QC value within limits for Cu 324.752 Recovery = 98.61%							
Fe 238.204 Radial†	74261.7	4937.2 µg/L	8.16	4937.2 ppb	8.16	0.17%	
QC value within limits for Fe 238.204 Radial Recovery = 98.74%							
K 766.490 Radial†	11735.3	4827.1 µg/L	35.34	4827.1 ppb	35.34	0.73%	
QC value within limits for K 766.490 Radial Recovery = 96.54%							
Mg 279.077 IEC†	12297.1	5077.8 µg/L	35.42	5077.8 ppb	35.42	0.70%	
QC value within limits for Mg 279.077 IEC Recovery = 101.56%							
Mn 257.610†	358877.3	490.17 µg/L	2.681	490.17 ppb	2.681	0.55%	
QC value within limits for Mn 257.610 Recovery = 98.03%							
Mo 202.031†	15267.9	482.40 µg/L	5.112	482.40 ppb	5.112	1.06%	
QC value within limits for Mo 202.031 Recovery = 96.48%							
Na 589.592 Radial†	64546.2	9872.1 µg/L	14.48	9872.1 ppb	14.48	0.15%	
QC value within limits for Na 589.592 Radial Recovery = 98.72%							
Ni 231.604†	38097.2	487.31 µg/L	3.107	487.31 ppb	3.107	0.64%	
QC value within limits for Ni 231.604 Recovery = 97.46%							
P 214.914†	9956.2	2376.0 µg/L	20.89	2376.0 ppb	20.89	0.88%	
QC value within limits for P 214.914 Recovery = 95.04%							
Pb 220.353†	7895.9	479.86 µg/L	5.722	479.86 ppb	5.722	1.19%	
QC value within limits for Pb 220.353 Recovery = 95.97%							
S 181.975 Axial†	1163.3	946.51 µg/L	8.747	946.51 ppb	8.747	0.92%	
QC value within limits for S 181.975 Axial Recovery = 94.65%							
Sb 206.836†	3611.9	488.26 µg/L	4.549	488.26 ppb	4.549	0.93%	
QC value within limits for Sb 206.836 Recovery = 97.65%							
Se 196.026†	1197.8	476 µg/L	3.6	476 ppb	3.6	0.76%	
QC value within limits for Se 196.026 Recovery = 95.19%							
SiO2†	47941.4	5219.2 µg/L	23.65	5219.2 ppb	23.65	0.45%	
QC value within limits for SiO2 Recovery = 97.60%							
Si 251.611†	147701.9	2432.6 µg/L	9.35	2432.6 ppb	9.35	0.38%	
QC value within limits for Si 251.611 Recovery = 97.30%							
Sn 189.927†	6863.5	489.59 µg/L	4.258	489.59 ppb	4.258	0.87%	
QC value within limits for Sn 189.927 Recovery = 97.92%							
Sr 421.552†	217958.6	510.80 µg/L	2.724	510.80 ppb	2.724	0.53%	
QC value within limits for Sr 421.552 Recovery = 102.16%							
Ti 334.940†	481628.2	490.47 µg/L	1.952	490.47 ppb	1.952	0.40%	
QC value within limits for Ti 334.940 Recovery = 98.09%							
Tl 190.801†	3586.5	488.81 µg/L	4.099	488.81 ppb	4.099	0.84%	
QC value within limits for Tl 190.801 Recovery = 97.76%							
U 409.014†	7481.8	492.42 µg/L	4.540	492.42 ppb	4.540	0.92%	
QC value within limits for U 409.014 Recovery = 98.48%							
V 292.402†	88944.2	499.54 µg/L	1.704	499.54 ppb	1.704	0.34%	
QC value within limits for V 292.402 Recovery = 99.91%							
Zn 213.857†	76638.9	478.58 µg/L	2.509	478.58 ppb	2.509	0.52%	
QC value within limits for Zn 213.857 Recovery = 95.72%							

All analyte(s) passed QC.

Sequence No.: 65

Sample ID: CCB

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 8

Date Collected: 3/29/2010 21:43:22

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCB

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	155956.8	155956.8	107 %		21:43:51
1	Al 396.153Radial†	-16.8	16.2	3.4619 µg/L	3.4619 ppb	21:44:11
1	Ca 317.933Radial†	700.6	38.5	2.2587 µg/L	2.2587 ppb	21:44:11
1	Fe 238.204 Radial†	158.1	34.5	2.2919 µg/L	2.2919 ppb	21:44:11
1	K 766.490 Radial†	1477.7	-74.0	-30.465 µg/L	-30.465 ppb	21:43:51
1	Mg 279.077 IEC†	161.1	-36.2	-14.868 µg/L	-14.868 ppb	21:44:11
1	Na 589.592 Radial†	1643.2	-159.1	-24.311 µg/L	-24.311 ppb	21:43:51
1	Sr 421.552†	-196.3	94.6	0.2216 µg/L	0.2216 ppb	21:43:51
1	Sc 361.383	1765629.9	1765629.9	105.55 %		21:45:13
1	Y 371.029	1081668.4	1081668.4	105.78 %		21:45:13
1	Ag 328.068†	3343.9	201.0	0.8287 µg/L	0.8287 ppb	21:45:15
1	As 188.979†	-0.7	13.6	5.6736 µg/L	5.6736 ppb	21:45:35
1	B 249.677†	3087.2	-430.8	-7.2342 µg/L	-7.2342 ppb	21:45:35
1	Ba 233.527†	-174.6	9.6	0.0437 µg/L	0.0437 ppb	21:45:35
1	Be 313.107†	-668.1	27.1	0.0159 µg/L	0.0159 ppb	21:45:15
1	Cd 226.502†	-91.4	7.8	0.0536 µg/L	0.0536 ppb	21:45:35
1	Co 228.616†	-169.6	15.9	0.2174 µg/L	0.2174 ppb	21:45:35
1	Cr 267.716†	125.9	-40.9	-0.3702 µg/L	-0.3702 ppb	21:45:35
1	Cu 324.752†	2790.6	219.0	0.9713 µg/L	0.9713 ppb	21:45:15
1	Mn 257.610†	190.9	100.8	0.1384 µg/L	0.1384 ppb	21:45:35
1	Mo 202.031†	-5.1	50.4	1.5908 µg/L	1.5908 ppb	21:45:35
1	Ni 231.604†	-58.3	-14.3	-0.1833 µg/L	-0.1833 ppb	21:45:35
1	P 214.914†	44.9	-37.1	-8.9068 µg/L	-8.9068 ppb	21:45:35
1	Pb 220.353†	100.6	-17.1	-1.0500 µg/L	-1.0500 ppb	21:45:35
1	S 181.975 Axial†	88.1	-11.4	-9.1903 µg/L	-9.1903 ppb	21:45:35
1	Sb 206.836†	84.0	-7.1	-0.9269 µg/L	-0.9269 ppb	21:45:35
1	Se 196.026†	15.6	3.8	1.54 µg/L	1.54 ppb	21:45:35
1	SiO2†	1680.5	19.3	2.0584 µg/L	2.0584 ppb	21:45:35
1	Si 251.611†	824.6	104.8	1.7121 µg/L	1.7121 ppb	21:45:35
1	Sn 189.927†	2.6	0.4	0.0311 µg/L	0.0311 ppb	21:45:35
1	Ti 334.940†	807.6	128.8	0.1231 µg/L	0.1231 ppb	21:45:15
1	Tl 190.801†	-115.4	11.0	1.4674 µg/L	1.4674 ppb	21:45:35
1	U 409.014†	-105.6	379.0	23.345 µg/L	23.345 ppb	21:45:15
1	V 292.402†	205.8	-236.8	-1.2834 µg/L	-1.2834 ppb	21:45:15
1	Zn 213.857†	546.7	53.5	0.3372 µg/L	0.3372 ppb	21:45:35
2	Sc RADIAL	155375.0	155375.0	107 %		21:44:13
2	Al 396.153Radial†	-68.3	-32.2	-7.0550 µg/L	-7.0550 ppb	21:44:33
2	Ca 317.933Radial†	709.4	49.3	2.8889 µg/L	2.8889 ppb	21:44:33
2	Fe 238.204 Radial†	170.5	46.7	3.1031 µg/L	3.1031 ppb	21:44:33
2	K 766.490 Radial†	1698.0	137.8	56.753 µg/L	56.753 ppb	21:44:13
2	Mg 279.077 IEC†	155.9	-40.4	-16.664 µg/L	-16.664 ppb	21:44:33
2	Na 589.592 Radial†	1687.7	-111.6	-17.120 µg/L	-17.120 ppb	21:44:13
2	Sr 421.552†	-289.5	6.4	0.0151 µg/L	0.0151 ppb	21:44:13
2	Sc 361.383	1758365.8	1758365.8	105.12 %		21:45:38
2	Y 371.029	1078074.0	1078074.0	105.43 %		21:45:38
2	Ag 328.068†	3122.4	3.3	0.0229 µg/L	0.0229 ppb	21:45:40
2	As 188.979†	-17.5	-2.4	-0.9870 µg/L	-0.9870 ppb	21:46:00
2	B 249.677†	3114.5	-392.8	-6.5943 µg/L	-6.5943 ppb	21:46:00
2	Ba 233.527†	-174.5	9.1	0.0411 µg/L	0.0411 ppb	21:46:00
2	Be 313.107†	-678.6	14.5	0.0087 µg/L	0.0087 ppb	21:45:40
2	Cd 226.502†	-106.7	-7.1	-0.0492 µg/L	-0.0492 ppb	21:46:00
2	Co 228.616†	-181.1	4.3	0.0589 µg/L	0.0589 ppb	21:46:00
2	Cr 267.716†	186.4	17.1	0.1365 µg/L	0.1365 ppb	21:46:00
2	Cu 324.752†	2877.2	312.3	1.3685 µg/L	1.3685 ppb	21:45:40
2	Mn 257.610†	194.2	104.8	0.1438 µg/L	0.1438 ppb	21:46:00
2	Mo 202.031†	-37.8	19.2	0.6071 µg/L	0.6071 ppb	21:46:00
2	Ni 231.604†	-60.1	-16.3	-0.2082 µg/L	-0.2082 ppb	21:46:00
2	P 214.914†	32.8	-48.4	-11.617 µg/L	-11.617 ppb	21:46:00
2	Pb 220.353†	87.7	-29.0	-1.7681 µg/L	-1.7681 ppb	21:46:00

2	S 181.975 Axial†	91.7	-7.6	-6.1290 µg/L	-6.1290 ppb	21:46:00
2	Sb 206.836†	84.8	-5.9	-0.7957 µg/L	-0.7957 ppb	21:46:00
2	Se 196.026†	18.7	6.9	2.73 µg/L	2.73 ppb	21:46:00
2	SiO2†	1682.8	28.0	3.0520 µg/L	3.0520 ppb	21:46:00
2	Si 251.611†	805.7	90.1	1.4833 µg/L	1.4833 ppb	21:46:00
2	Sn 189.927†	-1.8	-3.8	-0.2671 µg/L	-0.2671 ppb	21:46:00
2	Ti 334.940†	866.0	187.5	0.1872 µg/L	0.1872 ppb	21:45:40
2	Tl 190.801†	-106.3	19.2	2.5714 µg/L	2.5714 ppb	21:46:00
2	U 409.014†	-280.2	212.6	13.103 µg/L	13.103 ppb	21:45:40
2	V 292.402†	347.0	-101.7	-0.5490 µg/L	-0.5490 ppb	21:45:40
2	Zn 213.857†	514.2	24.8	0.1559 µg/L	0.1559 ppb	21:46:00
3	Sc RADIAL	154236.9	154236.9	106 %		21:44:35
3	Al 396.153Radial†	-27.1	6.3	1.3236 µg/L	1.3236 ppb	21:44:55
3	Ca 317.933Radial†	725.7	69.6	4.0774 µg/L	4.0774 ppb	21:44:55
3	Fe 238.204 Radial†	170.1	47.5	3.1556 µg/L	3.1556 ppb	21:44:55
3	K 766.490 Radial†	1418.1	-114.9	-47.294 µg/L	-47.294 ppb	21:44:35
3	Mg 279.077 IEC†	159.9	-35.5	-14.632 µg/L	-14.632 ppb	21:44:55
3	Na 589.592 Radial†	1547.3	-232.5	-35.541 µg/L	-35.541 ppb	21:44:35
3	Sr 421.552†	-316.6	-21.2	-0.0498 µg/L	-0.0498 ppb	21:44:35
3	Sc 361.383	1753936.7	1753936.7	104.85 %		21:46:02
3	Y 371.029	1074322.0	1074322.0	105.06 %		21:46:02
3	Ag 328.068†	3311.5	191.2	0.7816 µg/L	0.7816 ppb	21:46:04
3	As 188.979†	-21.8	-6.6	-2.7393 µg/L	-2.7393 ppb	21:46:24
3	B 249.677†	3129.0	-371.5	-6.2368 µg/L	-6.2368 ppb	21:46:24
3	Ba 233.527†	-162.2	20.3	0.0929 µg/L	0.0929 ppb	21:46:24
3	Be 313.107†	-901.0	-199.2	-0.0620 µg/L	-0.0620 ppb	21:46:04
3	Cd 226.502†	-95.1	3.7	0.0249 µg/L	0.0249 ppb	21:46:24
3	Co 228.616†	-174.5	10.2	0.1392 µg/L	0.1392 ppb	21:46:24
3	Cr 267.716†	174.7	6.4	0.0473 µg/L	0.0473 ppb	21:46:24
3	Cu 324.752†	2668.6	120.3	0.5307 µg/L	0.5307 ppb	21:46:04
3	Mn 257.610†	187.9	99.2	0.1361 µg/L	0.1361 ppb	21:46:24
3	Mo 202.031†	-24.5	31.8	1.0050 µg/L	1.0050 ppb	21:46:24
3	Ni 231.604†	-80.3	-35.6	-0.4559 µg/L	-0.4559 ppb	21:46:24
3	P 214.914†	36.8	-44.4	-10.662 µg/L	-10.662 ppb	21:46:24
3	Pb 220.353†	101.1	-16.0	-0.9738 µg/L	-0.9738 ppb	21:46:24
3	S 181.975 Axial†	84.3	-14.4	-11.695 µg/L	-11.695 ppb	21:46:24
3	Sb 206.836†	73.7	-16.4	-2.1934 µg/L	-2.1934 ppb	21:46:24
3	Se 196.026†	9.7	-1.7	-0.644 µg/L	-0.644 ppb	21:46:24
3	SiO2†	1725.4	72.7	7.9170 µg/L	7.9170 ppb	21:46:24
3	Si 251.611†	849.4	133.7	2.1983 µg/L	2.1983 ppb	21:46:24
3	Sn 189.927†	1.0	-1.1	-0.0738 µg/L	-0.0738 ppb	21:46:24
3	Ti 334.940†	975.6	294.1	0.2973 µg/L	0.2973 ppb	21:46:04
3	Tl 190.801†	-110.8	14.6	1.9610 µg/L	1.9610 ppb	21:46:24
3	U 409.014†	-341.5	153.4	9.4487 µg/L	9.4487 ppb	21:46:04
3	V 292.402†	361.9	-86.7	-0.4648 µg/L	-0.4648 ppb	21:46:04
3	Zn 213.857†	519.6	31.1	0.1983 µg/L	0.1983 ppb	21:46:24

Mean Data: CCB

Analyte	Mean Corrected Intensity	Conc. Units	Calib. Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1759310.8	105.17 %	0.353			0.34%
Sc RADIAL	155189.5	106 %	0.6			0.56%
Y 371.029	1078021.5	105.42 %	0.359			0.34%
Ag 328.068†	131.9	0.5444 µg/L	0.45227	0.5444 ppb	0.45227	83.07%
QC value within limits for Ag 328.068 Recovery = Not calculated						
Al 396.153Radial†	-3.2	-0.7565 µg/L	5.55848	-0.7565 ppb	5.55848	734.76%
QC value within limits for Al 396.153Radial Recovery = Not calculated						
As 188.979†	1.5	0.6491 µg/L	4.43866	0.6491 ppb	4.43866	683.80%
QC value within limits for As 188.979 Recovery = Not calculated						
B 249.677†	-398.4	-6.6884 µg/L	0.50530	-6.6884 ppb	0.50530	7.55%
QC value within limits for B 249.677 Recovery = Not calculated						
Ba 233.527†	13.0	0.0592 µg/L	0.02918	0.0592 ppb	0.02918	49.24%
QC value within limits for Ba 233.527 Recovery = Not calculated						
Be 313.107†	-52.5	-0.0125 µg/L	0.04303	-0.0125 ppb	0.04303	345.39%
QC value within limits for Be 313.107 Recovery = Not calculated						
Ca 317.933Radial†	52.5	3.0750 µg/L	0.92355	3.0750 ppb	0.92355	30.03%
QC value within limits for Ca 317.933Radial Recovery = Not calculated						
Cd 226.502†	1.5	0.0098 µg/L	0.05303	0.0098 ppb	0.05303	543.11%
QC value within limits for Cd 226.502 Recovery = Not calculated						
Co 228.616†	10.1	0.1385 µg/L	0.07927	0.1385 ppb	0.07927	57.23%

Cr	267.716†	QC value within limits for Co 228.616	Recovery = Not calculated			
		-5.8	-0.0621 µg/L	0.27051	-0.0621 ppb	0.27051 435.31%
Cu	324.752†	QC value within limits for Cr 267.716	Recovery = Not calculated			
		217.2	0.9568 µg/L	0.41909	0.9568 ppb	0.41909 43.80%
Fe	238.204 Radial†	QC value within limits for Cu 324.752	Recovery = Not calculated			
		42.9	2.8502 µg/L	0.48420	2.8502 ppb	0.48420 16.99%
K	766.490 Radial†	QC value within limits for Fe 238.204 Radial	Recovery = Not calculated			
		-17.0	-7.0019 µg/L	55.85109	-7.0019 ppb	55.85109 797.66%
Mg	279.077 IEC†	QC value within limits for K 766.490 Radial	Recovery = Not calculated			
		-37.4	-15.388 µg/L	1.1111	-15.388 ppb	1.1111 7.22%
Mn	257.610†	QC value within limits for Mg 279.077 IEC	Recovery = Not calculated			
		101.6	0.1394 µg/L	0.00394	0.1394 ppb	0.00394 2.82%
Mo	202.031†	QC value within limits for Mn 257.610	Recovery = Not calculated			
		33.8	1.0676 µg/L	0.49486	1.0676 ppb	0.49486 46.35%
Na	589.592 Radial†	QC value within limits for Mo 202.031	Recovery = Not calculated			
		-167.7	-25.657 µg/L	9.2837	-25.657 ppb	9.2837 36.18%
Ni	231.604†	QC value within limits for Na 589.592 Radial	Recovery = Not calculated			
		-22.1	-0.2825 µg/L	0.15069	-0.2825 ppb	0.15069 53.35%
P	214.914†	QC value within limits for Ni 231.604	Recovery = Not calculated			
		-43.3	-10.395 µg/L	1.3745	-10.395 ppb	1.3745 13.22%
Pb	220.353†	QC value within limits for P 214.914	Recovery = Not calculated			
		-20.7	-1.2640 µg/L	0.43823	-1.2640 ppb	0.43823 34.67%
S	181.975 Axial†	QC value within limits for Pb 220.353	Recovery = Not calculated			
		-11.1	-9.0047 µg/L	2.78752	-9.0047 ppb	2.78752 30.96%
Sb	206.836†	QC value within limits for S 181.975 Axial	Recovery = Not calculated			
		-9.8	-1.3053 µg/L	0.77187	-1.3053 ppb	0.77187 59.13%
Se	196.026†	QC value within limits for Sb 206.836	Recovery = Not calculated			
		3.0	1.21 µg/L	1.710	1.21 ppb	1.710 141.69%
SiO2†		QC value within limits for Se 196.026	Recovery = Not calculated			
		40.0	4.3425 µg/L	3.13523	4.3425 ppb	3.13523 72.20%
Si	251.611†	QC value within limits for SiO2	Recovery = Not calculated			
		109.6	1.7979 µg/L	0.36513	1.7979 ppb	0.36513 20.31%
Sn	189.927†	QC value within limits for Si 251.611	Recovery = Not calculated			
		-1.5	-0.1033 µg/L	0.15126	-0.1033 ppb	0.15126 146.44%
Sr	421.552†	QC value within limits for Sn 189.927	Recovery = Not calculated			
		26.6	0.0623 µg/L	0.14172	0.0623 ppb	0.14172 227.53%
Ti	334.940†	QC value within limits for Sr 421.552	Recovery = Not calculated			
		203.5	0.2025 µg/L	0.08808	0.2025 ppb	0.08808 43.49%
Tl	190.801†	QC value within limits for Ti 334.940	Recovery = Not calculated			
		14.9	1.9999 µg/L	0.55303	1.9999 ppb	0.55303 27.65%
U	409.014†	QC value within limits for Tl 190.801	Recovery = Not calculated			
		248.3	15.299 µg/L	7.2039	15.299 ppb	7.2039 47.09%
V	292.402†	QC value within limits for U 409.014	Recovery = Not calculated			
		-141.7	-0.7657 µg/L	0.45029	-0.7657 ppb	0.45029 58.81%
Zn	213.857†	QC value within limits for V 292.402	Recovery = Not calculated			
		36.5	0.2305 µg/L	0.09482	0.2305 ppb	0.09482 41.14%
		QC value within limits for Zn 213.857	Recovery = Not calculated			

All analyte(s) passed QC.

Sequence No.: 73

Sample ID: CCV

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 1

Date Collected: 3/29/2010 22:01:04

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCV

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	158049.5	158049.5	108 %		22:01:37
1	Al 396.153Radial†	26411.5	24388.7	5301.6 µg/L	5301.6 ppb	22:01:37
1	Ca 317.933Radial†	92553.1	84736.9	4965.2 µg/L	4965.2 ppb	22:01:37
1	Fe 238.204 Radial†	80932.2	74522.9	4954.5 µg/L	4954.5 ppb	22:01:37
1	K 766.490 Radial†	14535.0	11949.3	4915.2 µg/L	4915.2 ppb	22:01:37
1	Mg 279.077 IEC†	13642.6	12394.6	5117.9 µg/L	5117.9 ppb	22:01:37
1	Na 589.592 Radial†	72124.5	64818.9	9913.8 µg/L	9913.8 ppb	22:01:37
1	Sr 421.552†	236566.4	218441.0	511.93 µg/L	511.93 ppb	22:01:35
1	Sc 361.383	1796532.1	1796532.1	107.40 %		22:01:50
1	Y 371.029	1087433.5	1087433.5	106.34 %		22:01:50
1	Ag 328.068†	132761.6	120649.0	495.79 µg/L	495.79 ppb	22:01:50
1	As 188.979†	1379.4	1298.6	549.79 µg/L	549.79 ppb	22:02:10
1	B 249.677†	34327.9	28607.5	478.59 µg/L	478.59 ppb	22:01:50
1	Ba 233.527†	118329.1	110352.8	504.53 µg/L	504.53 ppb	22:01:50
1	Be 313.107†	1697099.0	1580851.1	514.73 µg/L	514.73 ppb	22:01:50
1	Cd 226.502†	75099.3	70020.3	483.23 µg/L	483.23 ppb	22:01:50
1	Co 228.616†	38144.6	35693.5	489.02 µg/L	489.02 ppb	22:01:50
1	Cr 267.716†	61551.1	57150.8	490.75 µg/L	490.75 ppb	22:01:50
1	Cu 324.752†	125230.0	114178.5	497.87 µg/L	497.87 ppb	22:01:50
1	Mn 257.610†	387183.9	360432.0	492.29 µg/L	492.29 ppb	22:01:50
1	Mo 202.031†	16175.9	15116.8	477.63 µg/L	477.63 ppb	22:02:10
1	Ni 231.604†	40995.7	38212.6	488.78 µg/L	488.78 ppb	22:01:50
1	P 214.914†	10701.6	9884.8	2358.9 µg/L	2358.9 ppb	22:02:10
1	Pb 220.353†	8517.0	7817.8	475.13 µg/L	475.13 ppb	22:02:10
1	S 181.975 Axial†	1332.8	1146.2	932.66 µg/L	932.66 ppb	22:02:10
1	Sb 206.836†	3939.5	3581.5	484.05 µg/L	484.05 ppb	22:02:10
1	Se 196.026†	1279.3	1180.3	469 µg/L	469 ppb	22:02:10
1	SiO2†	53216.1	47977.4	5223.3 µg/L	5223.3 ppb	22:01:50
1	Si 251.611†	160303.4	148584.2	2447.2 µg/L	2447.2 ppb	22:01:50
1	Sn 189.927†	7334.9	6827.6	487.05 µg/L	487.05 ppb	22:02:10
1	Ti 334.940†	519977.9	483521.9	492.40 µg/L	492.40 ppb	22:01:50
1	Tl 190.801†	3694.6	3560.4	485.32 µg/L	485.32 ppb	22:02:10
1	U 409.014†	7392.0	7361.9	485.07 µg/L	485.07 ppb	22:01:50
1	V 292.402†	96188.6	89130.7	500.52 µg/L	500.52 ppb	22:01:50
1	Zn 213.857†	83802.2	77564.9	484.40 µg/L	484.40 ppb	22:01:50
2	Sc RADIAL	156901.2	156901.2	108 %		22:01:41
2	Al 396.153Radial†	26045.7	24227.1	5266.1 µg/L	5266.1 ppb	22:01:41
2	Ca 317.933Radial†	91463.8	84349.6	4942.5 µg/L	4942.5 ppb	22:01:41
2	Fe 238.204 Radial†	80200.4	74389.3	4945.7 µg/L	4945.7 ppb	22:01:41
2	K 766.490 Radial†	14394.1	11916.4	4901.6 µg/L	4901.6 ppb	22:01:41
2	Mg 279.077 IEC†	13524.6	12377.1	5110.8 µg/L	5110.8 ppb	22:01:41
2	Na 589.592 Radial†	71678.0	64891.0	9924.8 µg/L	9924.8 ppb	22:01:41
2	Sr 421.552†	232732.3	216475.9	507.32 µg/L	507.32 ppb	22:01:39
2	Sc 361.383	1783616.2	1783616.2	106.63 %		22:02:13
2	Y 371.029	1079542.4	1079542.4	105.57 %		22:02:13
2	Ag 328.068†	131412.3	120278.7	494.27 µg/L	494.27 ppb	22:02:13
2	As 188.979†	1380.3	1308.7	554.01 µg/L	554.01 ppb	22:02:33
2	B 249.677†	34427.1	28932.0	484.03 µg/L	484.03 ppb	22:02:13
2	Ba 233.527†	116944.7	109852.3	502.24 µg/L	502.24 ppb	22:02:13
2	Be 313.107†	1678543.6	1574891.6	512.79 µg/L	512.79 ppb	22:02:13
2	Cd 226.502†	74410.0	69880.2	482.26 µg/L	482.26 ppb	22:02:13
2	Co 228.616†	37848.5	35673.1	488.73 µg/L	488.73 ppb	22:02:13
2	Cr 267.716†	60832.9	56892.2	488.54 µg/L	488.54 ppb	22:02:13
2	Cu 324.752†	123762.6	113646.6	495.55 µg/L	495.55 ppb	22:02:13
2	Mn 257.610†	383763.1	359834.4	491.48 µg/L	491.48 ppb	22:02:13
2	Mo 202.031†	16215.3	15262.8	482.24 µg/L	482.24 ppb	22:02:33
2	Ni 231.604†	40715.4	38226.1	488.96 µg/L	488.96 ppb	22:02:13
2	P 214.914†	10801.6	10050.8	2398.6 µg/L	2398.6 ppb	22:02:33
2	Pb 220.353†	8589.1	7942.9	482.72 µg/L	482.72 ppb	22:02:33

2	S 181.975 Axial†	1344.2	1165.8	948.58 µg/L	948.58 ppb	22:02:33
2	Sb 206.836†	3942.2	3610.6	488.08 µg/L	488.08 ppb	22:02:33
2	Se 196.026†	1283.6	1192.9	474 µg/L	474 ppb	22:02:33
2	SiO2†	52849.8	47992.6	5224.8 µg/L	5224.8 ppb	22:02:13
2	Si 251.611†	158621.6	148087.7	2438.9 µg/L	2438.9 ppb	22:02:13
2	Sn 189.927†	7373.6	6913.4	493.14 µg/L	493.14 ppb	22:02:33
2	Ti 334.940†	514397.9	481794.6	490.64 µg/L	490.64 ppb	22:02:13
2	Tl 190.801†	3715.3	3604.7	491.24 µg/L	491.24 ppb	22:02:33
2	U 409.014†	7243.6	7272.5	479.51 µg/L	479.51 ppb	22:02:13
2	V 292.402†	95349.6	88992.3	499.79 µg/L	499.79 ppb	22:02:13
2	Zn 213.857†	82609.2	77011.1	480.91 µg/L	480.91 ppb	22:02:13
3	Sc RADIAL	156463.7	156463.7	107 %		22:01:45
3	Al 396.153Radial†	25995.3	24247.8	5270.6 µg/L	5270.6 ppb	22:01:45
3	Ca 317.933Radial†	91157.7	84302.0	4939.7 µg/L	4939.7 ppb	22:01:45
3	Fe 238.204 Radial†	79790.6	74215.9	4934.1 µg/L	4934.1 ppb	22:01:45
3	K 766.490 Radial†	14295.4	11862.0	4879.2 µg/L	4879.2 ppb	22:01:45
3	Mg 279.077 IEC†	13441.9	12335.1	5093.5 µg/L	5093.5 ppb	22:01:45
3	Na 589.592 Radial†	71245.2	64673.9	9891.6 µg/L	9891.6 ppb	22:01:45
3	Sr 421.552†	235650.6	219799.0	515.11 µg/L	515.11 ppb	22:01:43
3	Sc 361.383	1779354.1	1779354.1	106.37 %		22:02:36
3	Y 371.029	1076400.2	1076400.2	105.26 %		22:02:36
3	Ag 328.068†	130833.4	120029.7	493.27 µg/L	493.27 ppb	22:02:36
3	As 188.979†	1382.7	1314.1	556.25 µg/L	556.25 ppb	22:02:57
3	B 249.677†	34071.7	28675.2	479.73 µg/L	479.73 ppb	22:02:36
3	Ba 233.527†	116809.2	109987.6	502.86 µg/L	502.86 ppb	22:02:36
3	Be 313.107†	1674596.4	1574951.7	512.81 µg/L	512.81 ppb	22:02:36
3	Cd 226.502†	73969.6	69633.4	480.55 µg/L	480.55 ppb	22:02:36
3	Co 228.616†	37628.2	35550.9	487.06 µg/L	487.06 ppb	22:02:36
3	Cr 267.716†	60619.6	56828.4	487.98 µg/L	487.98 ppb	22:02:36
3	Cu 324.752†	123542.2	113717.4	495.86 µg/L	495.86 ppb	22:02:36
3	Mn 257.610†	382395.5	359410.8	490.90 µg/L	490.90 ppb	22:02:36
3	Mo 202.031†	16173.8	15260.2	482.16 µg/L	482.16 ppb	22:02:57
3	Ni 231.604†	40421.3	38041.0	486.59 µg/L	486.59 ppb	22:02:36
3	P 214.914†	10736.5	10013.9	2389.8 µg/L	2389.8 ppb	22:02:57
3	Pb 220.353†	8554.5	7929.6	481.90 µg/L	481.90 ppb	22:02:57
3	S 181.975 Axial†	1335.2	1160.4	944.20 µg/L	944.20 ppb	22:02:57
3	Sb 206.836†	3941.0	3618.3	489.13 µg/L	489.13 ppb	22:02:57
3	Se 196.026†	1288.0	1199.9	477 µg/L	477 ppb	22:02:57
3	SiO2†	52993.8	48246.8	5252.6 µg/L	5252.6 ppb	22:02:36
3	Si 251.611†	158759.4	148573.6	2447.0 µg/L	2447.0 ppb	22:02:36
3	Sn 189.927†	7362.8	6919.8	493.59 µg/L	493.59 ppb	22:02:57
3	Ti 334.940†	513521.6	482126.3	490.98 µg/L	490.98 ppb	22:02:36
3	Tl 190.801†	3708.7	3606.8	491.53 µg/L	491.53 ppb	22:02:57
3	U 409.014†	7457.8	7490.2	492.90 µg/L	492.90 ppb	22:02:36
3	V 292.402†	94935.5	88817.2	498.83 µg/L	498.83 ppb	22:02:36
3	Zn 213.857†	82507.8	77101.4	481.50 µg/L	481.50 ppb	22:02:36

Mean Data: CCV

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1786500.8	106.80 %	0.535			0.50%
Sc RADIAL	157138.2	108 %	0.6			0.52%
Y 371.029	1081125.4	105.73 %	0.556			0.53%
Ag 328.068†	120319.2	494.45 µg/L	1.270	494.45 ppb	1.270	0.26%
QC value within limits for Ag 328.068 Recovery = 98.89%						
Al 396.153Radial†	24287.9	5279.4 µg/L	19.31	5279.4 ppb	19.31	0.37%
QC value within limits for Al 396.153Radial Recovery = 105.59%						
As 188.979†	1307.2	553.35 µg/L	3.278	553.35 ppb	3.278	0.59%
QC value greater than the upper limit for As 188.979 Recovery = 110.67%						
B 249.677†	28738.2	480.78 µg/L	2.873	480.78 ppb	2.873	0.60%
QC value within limits for B 249.677 Recovery = 96.16%						
Ba 233.527†	110064.3	503.21 µg/L	1.182	503.21 ppb	1.182	0.23%
QC value within limits for Ba 233.527 Recovery = 100.64%						
Be 313.107†	1576898.2	513.44 µg/L	1.114	513.44 ppb	1.114	0.22%
QC value within limits for Be 313.107 Recovery = 102.69%						
Ca 317.933Radial†	84462.8	4949.2 µg/L	13.98	4949.2 ppb	13.98	0.28%
QC value within limits for Ca 317.933Radial Recovery = 98.98%						
Cd 226.502†	69844.6	482.01 µg/L	1.352	482.01 ppb	1.352	0.28%
QC value within limits for Cd 226.502 Recovery = 96.40%						
Co 228.616†	35639.2	488.27 µg/L	1.056	488.27 ppb	1.056	0.22%

QC value within limits for Co 228.616 Recovery = 97.65%					
Cr 267.716†	56957.1	489.09 µg/L	1.468	489.09 ppb	1.468 0.30%
QC value within limits for Cr 267.716 Recovery = 97.82%					
Cu 324.752†	113847.5	496.43 µg/L	1.257	496.43 ppb	1.257 0.25%
QC value within limits for Cu 324.752 Recovery = 99.29%					
Fe 238.204 Radial†	74376.0	4944.8 µg/L	10.23	4944.8 ppb	10.23 0.21%
QC value within limits for Fe 238.204 Radial Recovery = 98.90%					
K 766.490 Radial†	11909.2	4898.7 µg/L	18.15	4898.7 ppb	18.15 0.37%
QC value within limits for K 766.490 Radial Recovery = 97.97%					
Mg 279.077 IEC†	12368.9	5107.4 µg/L	12.54	5107.4 ppb	12.54 0.25%
QC value within limits for Mg 279.077 IEC Recovery = 102.15%					
Mn 257.610†	359892.4	491.56 µg/L	0.701	491.56 ppb	0.701 0.14%
QC value within limits for Mn 257.610 Recovery = 98.31%					
Mo 202.031†	15213.3	480.68 µg/L	2.637	480.68 ppb	2.637 0.55%
QC value within limits for Mo 202.031 Recovery = 96.14%					
Na 589.592 Radial†	64794.6	9910.0 µg/L	16.90	9910.0 ppb	16.90 0.17%
QC value within limits for Na 589.592 Radial Recovery = 99.10%					
Ni 231.604†	38159.9	488.11 µg/L	1.320	488.11 ppb	1.320 0.27%
QC value within limits for Ni 231.604 Recovery = 97.62%					
P 214.914†	9983.2	2382.4 µg/L	20.89	2382.4 ppb	20.89 0.88%
QC value within limits for P 214.914 Recovery = 95.30%					
Pb 220.353†	7896.8	479.91 µg/L	4.167	479.91 ppb	4.167 0.87%
QC value within limits for Pb 220.353 Recovery = 95.98%					
S 181.975 Axial†	1157.5	941.82 µg/L	8.224	941.82 ppb	8.224 0.87%
QC value within limits for S 181.975 Axial Recovery = 94.18%					
Sb 206.836†	3603.5	487.09 µg/L	2.680	487.09 ppb	2.680 0.55%
QC value within limits for Sb 206.836 Recovery = 97.42%					
Se 196.026†	1191.0	473 µg/L	3.9	473 ppb	3.9 0.83%
QC value within limits for Se 196.026 Recovery = 94.65%					
SiO2†	48072.3	5233.6 µg/L	16.47	5233.6 ppb	16.47 0.31%
QC value within limits for SiO2 Recovery = 97.87%					
Si 251.611†	148415.2	2444.4 µg/L	4.72	2444.4 ppb	4.72 0.19%
QC value within limits for Si 251.611 Recovery = 97.78%					
Sn 189.927†	6886.9	491.26 µg/L	3.655	491.26 ppb	3.655 0.74%
QC value within limits for Sn 189.927 Recovery = 98.25%					
Sr 421.552†	218238.6	511.45 µg/L	3.916	511.45 ppb	3.916 0.77%
QC value within limits for Sr 421.552 Recovery = 102.29%					
Ti 334.940†	482481.0	491.34 µg/L	0.934	491.34 ppb	0.934 0.19%
QC value within limits for Ti 334.940 Recovery = 98.27%					
Tl 190.801†	3590.7	489.36 µg/L	3.506	489.36 ppb	3.506 0.72%
QC value within limits for Tl 190.801 Recovery = 97.87%					
U 409.014†	7374.9	485.83 µg/L	6.730	485.83 ppb	6.730 1.39%
QC value within limits for U 409.014 Recovery = 97.17%					
V 292.402†	88980.1	499.71 µg/L	0.850	499.71 ppb	0.850 0.17%
QC value within limits for V 292.402 Recovery = 99.94%					
Zn 213.857†	77225.8	482.27 µg/L	1.867	482.27 ppb	1.867 0.39%
QC value within limits for Zn 213.857 Recovery = 96.45%					
QC Failed. Continue with analysis.					

Sequence No.: 74

Sample ID: CCB

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 6

Date Collected: 3/29/2010 22:03:04

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCB

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	160449.4	160449.4	110 %		22:03:34
1	Al 396.153Radial†	-23.3	10.7	2.2857 µg/L	2.2857 ppb	22:03:54
1	Ca 317.933Radial†	663.3	-13.6	-0.7986 µg/L	-0.7986 ppb	22:03:54
1	Fe 238.204 Radial†	178.8	49.2	3.2692 µg/L	3.2692 ppb	22:03:54
1	K 766.490 Radial†	1550.2	-46.8	-19.248 µg/L	-19.248 ppb	22:03:34
1	Mg 279.077 IEC†	188.3	-15.6	-6.4221 µg/L	-6.4221 ppb	22:03:54
1	Na 589.592 Radial†	1720.0	-132.3	-20.226 µg/L	-20.226 ppb	22:03:34
1	Sr 421.552†	-107.7	180.2	0.4223 µg/L	0.4223 ppb	22:03:34
1	Sc 361.383	1782990.1	1782990.1	106.59 %		22:04:42
1	Y 371.029	1090676.4	1090676.4	106.66 %		22:04:42
1	Ag 328.068†	3540.4	354.5	1.4358 µg/L	1.4358 ppb	22:04:44
1	As 188.979†	-23.8	-8.1	-3.3731 µg/L	-3.3731 ppb	22:05:04
1	B 249.677†	3170.3	-381.3	-6.4031 µg/L	-6.4031 ppb	22:05:04
1	Ba 233.527†	-164.7	20.5	0.0937 µg/L	0.0937 ppb	22:05:04
1	Be 313.107†	-523.0	169.4	0.0564 µg/L	0.0564 ppb	22:04:44
1	Cd 226.502†	-92.5	7.6	0.0522 µg/L	0.0522 ppb	22:05:04
1	Co 228.616†	-166.7	20.2	0.2761 µg/L	0.2761 ppb	22:05:04
1	Cr 267.716†	144.9	-24.3	-0.2125 µg/L	-0.2125 ppb	22:05:04
1	Cu 324.752†	3308.1	678.7	2.9543 µg/L	2.9543 ppb	22:04:44
1	Mn 257.610†	226.5	132.5	0.1813 µg/L	0.1813 ppb	22:05:04
1	Mo 202.031†	-22.2	34.4	1.0857 µg/L	1.0857 ppb	22:05:04
1	Ni 231.604†	-71.5	-26.2	-0.3353 µg/L	-0.3353 ppb	22:05:04
1	P 214.914†	17.7	-63.0	-15.122 µg/L	-15.122 ppb	22:05:04
1	Pb 220.353†	110.9	-8.4	-0.5118 µg/L	-0.5118 ppb	22:05:04
1	S 181.975 Axial†	97.2	-3.6	-2.9298 µg/L	-2.9298 ppb	22:05:04
1	Sb 206.836†	92.1	-0.2	-0.0106 µg/L	-0.0106 ppb	22:05:04
1	Se 196.026†	10.0	-1.5	-0.603 µg/L	-0.603 ppb	22:05:04
1	SiO2†	1743.7	63.1	6.8545 µg/L	6.8545 ppb	22:05:04
1	Si 251.611†	838.2	110.0	1.8012 µg/L	1.8012 ppb	22:05:04
1	Sn 189.927†	10.0	7.4	0.5254 µg/L	0.5254 ppb	22:05:04
1	Ti 334.940†	839.9	151.6	0.1534 µg/L	0.1534 ppb	22:04:44
1	Tl 190.801†	-122.2	5.6	0.7511 µg/L	0.7511 ppb	22:05:04
1	U 409.014†	-437.1	69.0	4.2258 µg/L	4.2258 ppb	22:04:44
1	V 292.402†	331.6	-120.7	-0.6569 µg/L	-0.6569 ppb	22:04:44
1	Zn 213.857†	604.8	103.0	0.6478 µg/L	0.6478 ppb	22:05:04
2	Sc RADIAL	156747.2	156747.2	108 %		22:03:56
2	Al 396.153Radial†	-29.6	4.3	0.8879 µg/L	0.8879 ppb	22:04:16
2	Ca 317.933Radial†	666.7	3.7	0.2175 µg/L	0.2175 ppb	22:04:16
2	Fe 238.204 Radial†	175.2	49.7	3.3017 µg/L	3.3017 ppb	22:04:16
2	K 766.490 Radial†	1470.5	-87.7	-36.090 µg/L	-36.090 ppb	22:03:56
2	Mg 279.077 IEC†	169.6	-29.0	-11.920 µg/L	-11.920 ppb	22:04:16
2	Na 589.592 Radial†	1750.9	-66.6	-10.165 µg/L	-10.165 ppb	22:03:56
2	Sr 421.552†	-135.6	151.9	0.3559 µg/L	0.3559 ppb	22:03:56
2	Sc 361.383	1797191.3	1797191.3	107.44 %		22:05:06
2	Y 371.029	1098454.4	1098454.4	107.42 %		22:05:06
2	Ag 328.068†	3408.6	205.6	0.8469 µg/L	0.8469 ppb	22:05:08
2	As 188.979†	-12.7	2.4	1.0155 µg/L	1.0155 ppb	22:05:28
2	B 249.677†	3164.7	-410.0	-6.8848 µg/L	-6.8848 ppb	22:05:28
2	Ba 233.527†	-163.4	23.0	0.1052 µg/L	0.1052 ppb	22:05:28
2	Be 313.107†	-678.6	28.5	0.0135 µg/L	0.0135 ppb	22:05:08
2	Cd 226.502†	-87.1	13.3	0.0914 µg/L	0.0914 ppb	22:05:28
2	Co 228.616†	-175.3	13.5	0.1843 µg/L	0.1843 ppb	22:05:28
2	Cr 267.716†	187.5	14.3	0.1122 µg/L	0.1122 ppb	22:05:28
2	Cu 324.752†	3253.3	603.2	2.6341 µg/L	2.6341 ppb	22:05:08
2	Mn 257.610†	189.8	96.7	0.1326 µg/L	0.1326 ppb	22:05:28
2	Mo 202.031†	-18.9	37.7	1.1886 µg/L	1.1886 ppb	22:05:28
2	Ni 231.604†	-71.9	-26.0	-0.3327 µg/L	-0.3327 ppb	22:05:28
2	P 214.914†	32.5	-49.3	-11.863 µg/L	-11.863 ppb	22:05:28
2	Pb 220.353†	101.8	-17.6	-1.0762 µg/L	-1.0762 ppb	22:05:28

2	S 181.975 Axial†	94.3	-7.1	-5.7195 µg/L	-5.7195 ppb	22:05:28
2	Sb 206.836†	73.5	-18.2	-2.4456 µg/L	-2.4456 ppb	22:05:28
2	Se 196.026†	11.7	0.0	0.017 µg/L	0.017 ppb	22:05:28
2	SiO2†	1699.5	9.0	0.9499 µg/L	0.9499 ppb	22:05:28
2	Si 251.611†	884.5	146.9	2.4136 µg/L	2.4136 ppb	22:05:28
2	Sn 189.927†	-0.8	-2.7	-0.1939 µg/L	-0.1939 ppb	22:05:28
2	Ti 334.940†	738.9	51.4	0.0476 µg/L	0.0476 ppb	22:05:08
2	Tl 190.801†	-120.9	7.8	1.0385 µg/L	1.0385 ppb	22:05:28
2	U 409.014†	-272.9	225.1	13.889 µg/L	13.889 ppb	22:05:08
2	V 292.402†	392.8	-66.2	-0.3457 µg/L	-0.3457 ppb	22:05:08
2	Zn 213.857†	590.9	85.6	0.5385 µg/L	0.5385 ppb	22:05:28
3	Sc RADIAL	159177.1	159177.1	109 %		22:04:18
3	Al 396.153Radial†	-32.3	2.3	0.4484 µg/L	0.4484 ppb	22:04:38
3	Ca 317.933Radial†	661.7	-10.3	-0.6042 µg/L	-0.6042 ppb	22:04:38
3	Fe 238.204 Radial†	157.7	31.1	2.0666 µg/L	2.0666 ppb	22:04:38
3	K 766.490 Radial†	1654.5	60.0	24.710 µg/L	24.710 ppb	22:04:18
3	Mg 279.077 IEC†	173.1	-28.1	-11.572 µg/L	-11.572 ppb	22:04:38
3	Na 589.592 Radial†	1670.7	-164.9	-25.257 µg/L	-25.257 ppb	22:04:18
3	Sr 421.552†	-81.8	203.1	0.4761 µg/L	0.4761 ppb	22:04:18
3	Sc 361.383	1802721.6	1802721.6	107.77 %		22:05:30
3	Y 371.029	1101871.3	1101871.3	107.75 %		22:05:30
3	Ag 328.068†	3236.7	36.3	0.1614 µg/L	0.1614 ppb	22:05:33
3	As 188.979†	-14.2	1.1	0.4596 µg/L	0.4596 ppb	22:05:53
3	B 249.677†	3175.4	-409.2	-6.8698 µg/L	-6.8698 ppb	22:05:53
3	Ba 233.527†	-172.2	15.3	0.0698 µg/L	0.0698 ppb	22:05:53
3	Be 313.107†	-906.9	-181.5	-0.0538 µg/L	-0.0538 ppb	22:05:33
3	Cd 226.502†	-107.7	-5.6	-0.0386 µg/L	-0.0386 ppb	22:05:53
3	Co 228.616†	-189.6	0.7	0.0092 µg/L	0.0092 ppb	22:05:53
3	Cr 267.716†	175.9	3.0	0.0117 µg/L	0.0117 ppb	22:05:53
3	Cu 324.752†	3047.7	403.1	1.7668 µg/L	1.7668 ppb	22:05:33
3	Mn 257.610†	198.6	104.3	0.1430 µg/L	0.1430 ppb	22:05:53
3	Mo 202.031†	-19.7	36.9	1.1654 µg/L	1.1654 ppb	22:05:53
3	Ni 231.604†	-45.7	-1.5	-0.0189 µg/L	-0.0189 ppb	22:05:53
3	P 214.914†	24.9	-56.4	-13.551 µg/L	-13.551 ppb	22:05:53
3	Pb 220.353†	87.5	-31.3	-1.9030 µg/L	-1.9030 ppb	22:05:53
3	S 181.975 Axial†	90.3	-11.0	-8.9087 µg/L	-8.9087 ppb	22:05:53
3	Sb 206.836†	80.8	-11.6	-1.5550 µg/L	-1.5550 ppb	22:05:53
3	Se 196.026†	19.6	7.3	2.90 µg/L	2.90 ppb	22:05:53
3	SiO2†	1704.6	8.9	0.9407 µg/L	0.9407 ppb	22:05:53
3	Si 251.611†	850.1	112.5	1.8467 µg/L	1.8467 ppb	22:05:53
3	Sn 189.927†	-3.2	-5.0	-0.3566 µg/L	-0.3566 ppb	22:05:53
3	Ti 334.940†	849.3	151.7	0.1485 µg/L	0.1485 ppb	22:05:33
3	Tl 190.801†	-126.9	2.6	0.3427 µg/L	0.3427 ppb	22:05:53
3	U 409.014†	-211.7	282.7	17.431 µg/L	17.431 ppb	22:05:33
3	V 292.402†	343.3	-113.2	-0.6046 µg/L	-0.6046 ppb	22:05:33
3	Zn 213.857†	574.3	68.5	0.4296 µg/L	0.4296 ppb	22:05:53

Mean Data: CCB

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1794301.0	107.26 %	0.608			0.57%
Sc RADIAL	158791.2	109 %	1.3			1.18%
Y 371.029	1097000.7	107.28 %	0.561			0.52%
Ag 328.068†	198.8	0.8147 µg/L	0.63786	0.8147 ppb	0.63786	78.29%
QC value within limits for Ag 328.068 Recovery = Not calculated						
Al 396.153Radial†	5.8	1.2073 µg/L	0.95936	1.2073 ppb	0.95936	79.46%
QC value within limits for Al 396.153Radial Recovery = Not calculated						
As 188.979†	-1.5	-0.6327 µg/L	2.38947	-0.6327 ppb	2.38947	377.69%
QC value within limits for As 188.979 Recovery = Not calculated						
B 249.677†	-400.2	-6.7193 µg/L	0.27389	-6.7193 ppb	0.27389	4.08%
QC value within limits for B 249.677 Recovery = Not calculated						
Ba 233.527†	19.6	0.0896 µg/L	0.01809	0.0896 ppb	0.01809	20.20%
QC value within limits for Ba 233.527 Recovery = Not calculated						
Be 313.107†	5.5	0.0054 µg/L	0.05556	0.0054 ppb	0.05556	>999.9%
QC value within limits for Be 313.107 Recovery = Not calculated						
Ca 317.933Radial†	-6.7	-0.3951 µg/L	0.53934	-0.3951 ppb	0.53934	136.51%
QC value within limits for Ca 317.933Radial Recovery = Not calculated						
Cd 226.502†	5.1	0.0350 µg/L	0.06666	0.0350 ppb	0.06666	190.46%
QC value within limits for Cd 226.502 Recovery = Not calculated						
Co 228.616†	11.4	0.1565 µg/L	0.13561	0.1565 ppb	0.13561	86.64%

QC value within limits for Co 228.616 Recovery = Not calculated						
Cr 267.716†	-2.3	-0.0296 µg/L	0.16621	-0.0296 ppb	0.16621	562.40%
QC value within limits for Cr 267.716 Recovery = Not calculated						
Cu 324.752†	561.7	2.4517 µg/L	0.61441	2.4517 ppb	0.61441	25.06%
QC value within limits for Cu 324.752 Recovery = Not calculated						
Fe 238.204 Radial†	43.3	2.8792 µg/L	0.70386	2.8792 ppb	0.70386	24.45%
QC value within limits for Fe 238.204 Radial Recovery = Not calculated						
K 766.490 Radial†	-24.8	-10.209 µg/L	31.3914	-10.209 ppb	31.3914	307.48%
QC value within limits for K 766.490 Radial Recovery = Not calculated						
Mg 279.077 IEC†	-24.2	-9.9713 µg/L	3.07868	-9.9713 ppb	3.07868	30.88%
QC value within limits for Mg 279.077 IEC Recovery = Not calculated						
Mn 257.610†	111.1	0.1523 µg/L	0.02563	0.1523 ppb	0.02563	16.83%
QC value within limits for Mn 257.610 Recovery = Not calculated						
Mo 202.031†	36.3	1.1466 µg/L	0.05397	1.1466 ppb	0.05397	4.71%
QC value within limits for Mo 202.031 Recovery = Not calculated						
Na 589.592 Radial†	-121.3	-18.549 µg/L	7.6848	-18.549 ppb	7.6848	41.43%
QC value within limits for Na 589.592 Radial Recovery = Not calculated						
Ni 231.604†	-17.9	-0.2290 µg/L	0.18194	-0.2290 ppb	0.18194	79.46%
QC value within limits for Ni 231.604 Recovery = Not calculated						
P 214.914†	-56.3	-13.512 µg/L	1.6296	-13.512 ppb	1.6296	12.06%
QC value within limits for P 214.914 Recovery = Not calculated						
Pb 220.353†	-19.1	-1.1637 µg/L	0.69972	-1.1637 ppb	0.69972	60.13%
QC value within limits for Pb 220.353 Recovery = Not calculated						
S 181.975 Axial†	-7.2	-5.8527 µg/L	2.99169	-5.8527 ppb	2.99169	51.12%
QC value within limits for S 181.975 Axial Recovery = Not calculated						
Sb 206.836†	-10.0	-1.3371 µg/L	1.23203	-1.3371 ppb	1.23203	92.14%
QC value within limits for Sb 206.836 Recovery = Not calculated						
Se 196.026†	1.9	0.771 µg/L	1.8678	0.771 ppb	1.8678	242.41%
QC value within limits for Se 196.026 Recovery = Not calculated						
SiO2†	27.0	2.9150 µg/L	3.41170	2.9150 ppb	3.41170	117.04%
QC value within limits for SiO2 Recovery = Not calculated						
Si 251.611†	123.1	2.0205 µg/L	0.34120	2.0205 ppb	0.34120	16.89%
QC value within limits for Si 251.611 Recovery = Not calculated						
Sn 189.927†	-0.1	-0.0084 µg/L	0.46934	-0.0084 ppb	0.46934	>999.9%
QC value within limits for Sn 189.927 Recovery = Not calculated						
Sr 421.552†	178.4	0.4181 µg/L	0.06020	0.4181 ppb	0.06020	14.40%
QC value within limits for Sr 421.552 Recovery = Not calculated						
Ti 334.940†	118.2	0.1165 µg/L	0.05971	0.1165 ppb	0.05971	51.25%
QC value within limits for Ti 334.940 Recovery = Not calculated						
Tl 190.801†	5.3	0.7108 µg/L	0.34967	0.7108 ppb	0.34967	49.20%
QC value within limits for Tl 190.801 Recovery = Not calculated						
U 409.014†	192.3	11.848 µg/L	6.8347	11.848 ppb	6.8347	57.68%
QC value within limits for U 409.014 Recovery = Not calculated						
V 292.402†	-100.0	-0.5357 µg/L	0.16666	-0.5357 ppb	0.16666	31.11%
QC value within limits for V 292.402 Recovery = Not calculated						
Zn 213.857†	85.7	0.5387 µg/L	0.10910	0.5387 ppb	0.10910	20.25%
QC value within limits for Zn 213.857 Recovery = Not calculated						

All analyte(s) passed QC.

Sequence No.: 81

Sample ID: CCV

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 1

Date Collected: 3/29/2010 22:19:12

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCV

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	152312.7	152312.7	104 %		22:19:45
1	Al 396.153Radial†	25257.2	24201.5	5260.5 µg/L	5260.5 ppb	22:19:45
1	Ca 317.933Radial†	88990.6	84542.6	4953.8 µg/L	4953.8 ppb	22:19:45
1	Fe 238.204 Radial†	77715.5	74255.9	4936.8 µg/L	4936.8 ppb	22:19:45
1	K 766.490 Radial†	13912.9	11858.9	4877.9 µg/L	4877.9 ppb	22:19:45
1	Mg 279.077 IEC†	13152.4	12399.4	5120.0 µg/L	5120.0 ppb	22:19:45
1	Na 589.592 Radial†	69880.5	65176.8	9968.5 µg/L	9968.5 ppb	22:19:45
1	Sr 421.552†	228320.8	218767.5	512.69 µg/L	512.69 ppb	22:19:43
1	Sc 361.383	1737411.7	1737411.7	103.86 %		22:19:58
1	Y 371.029	1050981.5	1050981.5	102.78 %		22:19:58
1	Ag 328.068†	128476.0	120729.2	496.13 µg/L	496.13 ppb	22:19:58
1	As 188.979†	1340.1	1304.5	552.24 µg/L	552.24 ppb	22:20:18
1	B 249.677†	33219.3	28627.8	478.94 µg/L	478.94 ppb	22:19:58
1	Ba 233.527†	114183.4	110110.5	503.42 µg/L	503.42 ppb	22:19:58
1	Be 313.107†	1633886.1	1573760.5	512.42 µg/L	512.42 ppb	22:19:58
1	Cd 226.502†	72231.0	69638.2	480.59 µg/L	480.59 ppb	22:19:58
1	Co 228.616†	36690.0	35501.6	486.39 µg/L	486.39 ppb	22:19:58
1	Cr 267.716†	59371.2	57002.2	489.48 µg/L	489.48 ppb	22:19:58
1	Cu 324.752†	120429.1	113523.9	495.02 µg/L	495.02 ppb	22:19:58
1	Mn 257.610†	373880.7	359891.1	491.55 µg/L	491.55 ppb	22:19:58
1	Mo 202.031†	15806.6	15273.7	482.59 µg/L	482.59 ppb	22:20:18
1	Ni 231.604†	39682.8	38247.4	489.23 µg/L	489.23 ppb	22:19:58
1	P 214.914†	10452.4	9984.0	2382.6 µg/L	2382.6 ppb	22:20:18
1	Pb 220.353†	8370.1	7946.2	482.91 µg/L	482.91 ppb	22:20:18
1	S 181.975 Axial†	1298.7	1155.6	940.31 µg/L	940.31 ppb	22:20:18
1	Sb 206.836†	3840.2	3610.7	488.09 µg/L	488.09 ppb	22:20:18
1	Se 196.026†	1269.8	1211.6	481 µg/L	481 ppb	22:20:18
1	SiO2†	51583.1	48091.2	5235.5 µg/L	5235.5 ppb	22:19:58
1	Si 251.611†	154617.6	148188.9	2440.6 µg/L	2440.6 ppb	22:19:58
1	Sn 189.927†	7196.6	6926.8	494.09 µg/L	494.09 ppb	22:20:18
1	Ti 334.940†	501274.3	481988.9	490.84 µg/L	490.84 ppb	22:19:58
1	Tl 190.801†	3622.3	3607.9	491.69 µg/L	491.69 ppb	22:20:18
1	U 409.014†	7175.0	7387.1	486.68 µg/L	486.68 ppb	22:19:58
1	V 292.402†	93168.0	89270.1	501.35 µg/L	501.35 ppb	22:19:58
1	Zn 213.857†	80276.7	76825.8	479.74 µg/L	479.74 ppb	22:19:58
2	Sc RADIAL	154831.9	154831.9	106 %		22:19:49
2	Al 396.153Radial†	25587.3	24119.0	5242.1 µg/L	5242.1 ppb	22:19:49
2	Ca 317.933Radial†	90429.6	84511.6	4952.0 µg/L	4952.0 ppb	22:19:49
2	Fe 238.204 Radial†	79228.1	74469.7	4951.0 µg/L	4951.0 ppb	22:19:49
2	K 766.490 Radial†	14006.7	11730.5	4825.1 µg/L	4825.1 ppb	22:19:49
2	Mg 279.077 IEC†	13348.5	12379.3	5111.8 µg/L	5111.8 ppb	22:19:49
2	Na 589.592 Radial†	70589.6	64756.3	9904.2 µg/L	9904.2 ppb	22:19:49
2	Sr 421.552†	229160.8	216003.2	506.22 µg/L	506.22 ppb	22:19:47
2	Sc 361.383	1714461.6	1714461.6	102.49 %		22:20:21
2	Y 371.029	1037130.3	1037130.3	101.42 %		22:20:21
2	Ag 328.068†	127395.8	121331.1	498.59 µg/L	498.59 ppb	22:20:21
2	As 188.979†	1344.4	1326.0	561.27 µg/L	561.27 ppb	22:20:41
2	B 249.677†	32990.6	28832.7	482.36 µg/L	482.36 ppb	22:20:21
2	Ba 233.527†	113263.4	110684.5	506.05 µg/L	506.05 ppb	22:20:21
2	Be 313.107†	1625203.6	1586346.8	516.52 µg/L	516.52 ppb	22:20:21
2	Cd 226.502†	71591.7	69945.4	482.71 µg/L	482.71 ppb	22:20:21
2	Co 228.616†	36606.2	35892.7	491.75 µg/L	491.75 ppb	22:20:21
2	Cr 267.716†	58947.1	57353.6	492.50 µg/L	492.50 ppb	22:20:21
2	Cu 324.752†	119611.8	114278.5	498.30 µg/L	498.30 ppb	22:20:21
2	Mn 257.610†	371366.8	362257.0	494.79 µg/L	494.79 ppb	22:20:21
2	Mo 202.031†	15850.0	15519.8	490.36 µg/L	490.36 ppb	22:20:41
2	Ni 231.604†	39310.2	38395.3	491.12 µg/L	491.12 ppb	22:20:21
2	P 214.914†	10467.4	10133.3	2418.3 µg/L	2418.3 ppb	22:20:41
2	Pb 220.353†	8392.4	8075.9	490.79 µg/L	490.79 ppb	22:20:41

2	S 181.975 Axial†	1313.6	1186.9	965.72 µg/L	965.72 ppb	22:20:41
2	Sb 206.836†	3868.7	3688.0	498.60 µg/L	498.60 ppb	22:20:41
2	Se 196.026†	1246.3	1205.1	479 µg/L	479 ppb	22:20:41
2	SiO2†	51189.2	48371.7	5265.9 µg/L	5265.9 ppb	22:20:21
2	Si 251.611†	153640.7	149228.5	2457.6 µg/L	2457.6 ppb	22:20:21
2	Sn 189.927†	7204.7	7027.5	501.26 µg/L	501.26 ppb	22:20:41
2	Ti 334.940†	498506.7	485749.2	494.67 µg/L	494.67 ppb	22:20:21
2	Tl 190.801†	3638.8	3670.6	500.15 µg/L	500.15 ppb	22:20:41
2	U 409.014†	7086.3	7393.1	487.16 µg/L	487.16 ppb	22:20:21
2	V 292.402†	92241.8	89567.1	503.08 µg/L	503.08 ppb	22:20:21
2	Zn 213.857†	79665.1	77263.6	482.48 µg/L	482.48 ppb	22:20:21
3	Sc RADIAL	154090.6	154090.6	106 %		22:19:53
3	Al 396.153Radial†	25424.6	24080.9	5233.9 µg/L	5233.9 ppb	22:19:53
3	Ca 317.933Radial†	89815.0	84339.8	4941.9 µg/L	4941.9 ppb	22:19:53
3	Fe 238.204 Radial†	78583.1	74218.4	4934.3 µg/L	4934.3 ppb	22:19:53
3	K 766.490 Radial†	13957.7	11747.6	4832.1 µg/L	4832.1 ppb	22:19:53
3	Mg 279.077 IEC†	13296.6	12390.6	5116.5 µg/L	5116.5 ppb	22:19:53
3	Na 589.592 Radial†	70420.8	64916.2	9928.7 µg/L	9928.7 ppb	22:19:53
3	Sr 421.552†	227165.2	215153.4	504.22 µg/L	504.22 ppb	22:19:51
3	Sc 361.383	1727606.5	1727606.5	103.28 %		22:20:44
3	Y 371.029	1045815.5	1045815.5	102.27 %		22:20:44
3	Ag 328.068†	127723.5	120702.7	496.03 µg/L	496.03 ppb	22:20:44
3	As 188.979†	1349.6	1321.0	559.18 µg/L	559.18 ppb	22:21:05
3	B 249.677†	33234.8	28824.3	482.23 µg/L	482.23 ppb	22:20:44
3	Ba 233.527†	114068.8	110623.4	505.77 µg/L	505.77 ppb	22:20:44
3	Be 313.107†	1634139.1	1582933.7	515.41 µg/L	515.41 ppb	22:20:44
3	Cd 226.502†	72201.5	70004.3	483.12 µg/L	483.12 ppb	22:20:44
3	Co 228.616†	36622.8	35637.0	488.24 µg/L	488.24 ppb	22:20:44
3	Cr 267.716†	59398.0	57352.5	492.49 µg/L	492.49 ppb	22:20:44
3	Cu 324.752†	119868.0	113638.7	495.52 µg/L	495.52 ppb	22:20:44
3	Mn 257.610†	373060.7	361140.2	493.26 µg/L	493.26 ppb	22:20:44
3	Mo 202.031†	15888.1	15439.1	487.81 µg/L	487.81 ppb	22:21:05
3	Ni 231.604†	39594.7	38378.9	490.91 µg/L	490.91 ppb	22:20:44
3	P 214.914†	10522.4	10108.9	2412.5 µg/L	2412.5 ppb	22:21:05
3	Pb 220.353†	8403.6	8024.5	487.67 µg/L	487.67 ppb	22:21:05
3	S 181.975 Axial†	1310.6	1174.2	955.43 µg/L	955.43 ppb	22:21:05
3	Sb 206.836†	3889.0	3678.9	497.34 µg/L	497.34 ppb	22:21:05
3	Se 196.026†	1271.0	1219.8	485 µg/L	485 ppb	22:21:05
3	SiO2†	51423.3	48218.3	5249.2 µg/L	5249.2 ppb	22:20:44
3	Si 251.611†	154582.4	148999.8	2453.9 µg/L	2453.9 ppb	22:20:44
3	Sn 189.927†	7242.6	7010.7	500.07 µg/L	500.07 ppb	22:21:05
3	Ti 334.940†	501288.0	484741.5	493.64 µg/L	493.64 ppb	22:20:44
3	Tl 190.801†	3618.0	3623.5	493.81 µg/L	493.81 ppb	22:21:05
3	U 409.014†	7090.5	7344.5	484.10 µg/L	484.10 ppb	22:20:44
3	V 292.402†	92797.7	89420.5	502.24 µg/L	502.24 ppb	22:20:44
3	Zn 213.857†	80147.9	77139.7	481.71 µg/L	481.71 ppb	22:20:44

Mean Data: CCV

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1726493.3	103.21 %	0.688			0.67%
Sc RADIAL	153745.1	105 %	0.9			0.84%
Y 371.029	1044642.4	102.16 %	0.685			0.67%
Ag 328.068†	120921.0	496.92 µg/L	1.451	496.92 ppb	1.451	0.29%
QC value within limits for Ag 328.068 Recovery = 99.38%						
Al 396.153Radial†	24133.8	5245.5 µg/L	13.60	5245.5 ppb	13.60	0.26%
QC value within limits for Al 396.153Radial Recovery = 104.91%						
As 188.979†	1317.2	557.56 µg/L	4.727	557.56 ppb	4.727	0.85%
QC value greater than the upper limit for As 188.979 Recovery = 111.51%						
B 249.677†	28761.6	481.17 µg/L	1.939	481.17 ppb	1.939	0.40%
QC value within limits for B 249.677 Recovery = 96.23%						
Ba 233.527†	110472.8	505.08 µg/L	1.442	505.08 ppb	1.442	0.29%
QC value within limits for Ba 233.527 Recovery = 101.02%						
Be 313.107†	1581013.7	514.78 µg/L	2.119	514.78 ppb	2.119	0.41%
QC value within limits for Be 313.107 Recovery = 102.96%						
Ca 317.933Radial†	84464.7	4949.3 µg/L	6.40	4949.3 ppb	6.40	0.13%
QC value within limits for Ca 317.933Radial Recovery = 98.99%						
Cd 226.502†	69862.6	482.14 µg/L	1.358	482.14 ppb	1.358	0.28%
QC value within limits for Cd 226.502 Recovery = 96.43%						
Co 228.616†	35677.1	488.79 µg/L	2.721	488.79 ppb	2.721	0.56%

QC value within limits for Co 228.616 Recovery = 97.76%					
Cr 267.716†	57236.1	491.49 µg/L	1.741	491.49 ppb	1.741 0.35%
QC value within limits for Cr 267.716 Recovery = 98.30%					
Cu 324.752†	113813.7	496.28 µg/L	1.771	496.28 ppb	1.771 0.36%
QC value within limits for Cu 324.752 Recovery = 99.26%					
Fe 238.204 Radial†	74314.7	4940.7 µg/L	9.01	4940.7 ppb	9.01 0.18%
QC value within limits for Fe 238.204 Radial Recovery = 98.81%					
K 766.490 Radial†	11779.0	4845.0 µg/L	28.69	4845.0 ppb	28.69 0.59%
QC value within limits for K 766.490 Radial Recovery = 96.90%					
Mg 279.077 IEC†	12389.7	5116.1 µg/L	4.08	5116.1 ppb	4.08 0.08%
QC value within limits for Mg 279.077 IEC Recovery = 102.32%					
Mn 257.610†	361096.1	493.20 µg/L	1.617	493.20 ppb	1.617 0.33%
QC value within limits for Mn 257.610 Recovery = 98.64%					
Mo 202.031†	15410.9	486.92 µg/L	3.960	486.92 ppb	3.960 0.81%
QC value within limits for Mo 202.031 Recovery = 97.38%					
Na 589.592 Radial†	64949.8	9933.8 µg/L	32.45	9933.8 ppb	32.45 0.33%
QC value within limits for Na 589.592 Radial Recovery = 99.34%					
Ni 231.604†	38340.5	490.42 µg/L	1.037	490.42 ppb	1.037 0.21%
QC value within limits for Ni 231.604 Recovery = 98.08%					
P 214.914†	10075.4	2404.5 µg/L	19.15	2404.5 ppb	19.15 0.80%
QC value within limits for P 214.914 Recovery = 96.18%					
Pb 220.353†	8015.5	487.12 µg/L	3.967	487.12 ppb	3.967 0.81%
QC value within limits for Pb 220.353 Recovery = 97.42%					
S 181.975 Axial†	1172.2	953.82 µg/L	12.785	953.82 ppb	12.785 1.34%
QC value within limits for S 181.975 Axial Recovery = 95.38%					
Sb 206.836†	3659.2	494.68 µg/L	5.740	494.68 ppb	5.740 1.16%
QC value within limits for Sb 206.836 Recovery = 98.94%					
Se 196.026†	1212.2	482 µg/L	2.9	482 ppb	2.9 0.60%
QC value within limits for Se 196.026 Recovery = 96.33%					
SiO2†	48227.1	5250.2 µg/L	15.19	5250.2 ppb	15.19 0.29%
QC value within limits for SiO2 Recovery = 98.18%					
Si 251.611†	148805.7	2450.7 µg/L	8.96	2450.7 ppb	8.96 0.37%
QC value within limits for Si 251.611 Recovery = 98.03%					
Sn 189.927†	6988.3	498.47 µg/L	3.841	498.47 ppb	3.841 0.77%
QC value within limits for Sn 189.927 Recovery = 99.69%					
Sr 421.552†	216641.4	507.71 µg/L	4.429	507.71 ppb	4.429 0.87%
QC value within limits for Sr 421.552 Recovery = 101.54%					
Ti 334.940†	484159.9	493.05 µg/L	1.985	493.05 ppb	1.985 0.40%
QC value within limits for Ti 334.940 Recovery = 98.61%					
Tl 190.801†	3634.0	495.22 µg/L	4.399	495.22 ppb	4.399 0.89%
QC value within limits for Tl 190.801 Recovery = 99.04%					
U 409.014†	7374.9	485.98 µg/L	1.643	485.98 ppb	1.643 0.34%
QC value within limits for U 409.014 Recovery = 97.20%					
V 292.402†	89419.2	502.22 µg/L	0.868	502.22 ppb	0.868 0.17%
QC value within limits for V 292.402 Recovery = 100.44%					
Zn 213.857†	77076.4	481.31 µg/L	1.413	481.31 ppb	1.413 0.29%
QC value within limits for Zn 213.857 Recovery = 96.26%					
QC Failed. Continue with analysis.					

Sequence No.: 82

Sample ID: CCB

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 6

Date Collected: 3/29/2010 22:21:13

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCB

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	153048.9	153048.9	105 %		22:21:43
1	Al 396.153Radial†	-46.2	-12.1	-2.7027 µg/L	-2.7027 ppb	22:22:03
1	Ca 317.933Radial†	641.8	-5.0	-0.2911 µg/L	-0.2911 ppb	22:22:03
1	Fe 238.204 Radial†	160.0	39.1	2.6003 µg/L	2.6003 ppb	22:22:03
1	K 766.490 Radial†	1587.0	56.4	23.221 µg/L	23.221 ppb	22:21:43
1	Mg 279.077 IEC†	160.9	-33.5	-13.768 µg/L	-13.768 ppb	22:22:03
1	Na 589.592 Radial†	1749.0	-29.1	-4.4718 µg/L	-4.4718 ppb	22:21:43
1	Sr 421.552†	-135.3	149.1	0.3494 µg/L	0.3494 ppb	22:21:43
1	Sc 361.383	1742642.1	1742642.1	104.18 %		22:23:05
1	Y 371.029	1066501.3	1066501.3	104.29 %		22:23:05
1	Ag 328.068†	3331.6	231.0	0.9172 µg/L	0.9172 ppb	22:23:07
1	As 188.979†	-18.4	-3.4	-1.4062 µg/L	-1.4062 ppb	22:23:27
1	B 249.677†	3114.2	-366.4	-6.1519 µg/L	-6.1519 ppb	22:23:27
1	Ba 233.527†	-147.0	33.9	0.1544 µg/L	0.1544 ppb	22:23:27
1	Be 313.107†	-699.4	-11.3	-0.0042 µg/L	-0.0042 ppb	22:23:07
1	Cd 226.502†	-105.1	-6.5	-0.0448 µg/L	-0.0448 ppb	22:23:27
1	Co 228.616†	-157.7	25.3	0.3459 µg/L	0.3459 ppb	22:23:27
1	Cr 267.716†	174.6	7.4	0.0642 µg/L	0.0642 ppb	22:23:27
1	Cu 324.752†	2824.4	286.3	1.2434 µg/L	1.2434 ppb	22:23:07
1	Mn 257.610†	185.8	98.4	0.1350 µg/L	0.1350 ppb	22:23:27
1	Mo 202.031†	-12.5	43.2	1.3628 µg/L	1.3628 ppb	22:23:27
1	Ni 231.604†	-33.1	9.1	0.1168 µg/L	0.1168 ppb	22:23:27
1	P 214.914†	23.7	-56.8	-13.626 µg/L	-13.626 ppb	22:23:27
1	Pb 220.353†	94.6	-21.6	-1.3058 µg/L	-1.3058 ppb	22:23:27
1	S 181.975 Axial†	90.7	-7.8	-6.2749 µg/L	-6.2749 ppb	22:23:27
1	Sb 206.836†	85.8	-4.3	-0.5625 µg/L	-0.5625 ppb	22:23:27
1	Se 196.026†	15.2	3.7	1.47 µg/L	1.47 ppb	22:23:27
1	SiO2†	1707.1	65.8	7.1504 µg/L	7.1504 ppb	22:23:27
1	Si 251.611†	834.7	124.8	2.0451 µg/L	2.0451 ppb	22:23:27
1	Sn 189.927†	4.0	1.8	0.1301 µg/L	0.1301 ppb	22:23:27
1	Ti 334.940†	654.1	-8.5	-0.0069 µg/L	-0.0069 ppb	22:23:07
1	Tl 190.801†	-117.5	7.5	0.9902 µg/L	0.9902 ppb	22:23:27
1	U 409.014†	-528.2	-28.0	-1.8141 µg/L	-1.8141 ppb	22:23:07
1	V 292.402†	165.6	-272.9	-1.5009 µg/L	-1.5009 ppb	22:23:07
1	Zn 213.857†	513.9	28.9	0.1799 µg/L	0.1799 ppb	22:23:27
2	Sc RADIAL	151679.0	151679.0	104 %		22:22:05
2	Al 396.153Radial†	-28.1	4.8	0.9816 µg/L	0.9816 ppb	22:22:25
2	Ca 317.933Radial†	626.5	-14.1	-0.8283 µg/L	-0.8283 ppb	22:22:25
2	Fe 238.204 Radial†	161.3	41.8	2.7763 µg/L	2.7763 ppb	22:22:25
2	K 766.490 Radial†	1640.2	121.1	49.867 µg/L	49.867 ppb	22:22:05
2	Mg 279.077 IEC†	170.3	-23.0	-9.4578 µg/L	-9.4578 ppb	22:22:25
2	Na 589.592 Radial†	1597.3	-159.9	-24.506 µg/L	-24.506 ppb	22:22:05
2	Sr 421.552†	-216.8	69.7	0.1633 µg/L	0.1633 ppb	22:22:05
2	Sc 361.383	1717045.6	1717045.6	102.65 %		22:23:29
2	Y 371.029	1051770.0	1051770.0	102.85 %		22:23:29
2	Ag 328.068†	3191.7	142.4	0.5609 µg/L	0.5609 ppb	22:23:31
2	As 188.979†	-14.9	-0.3	-0.1085 µg/L	-0.1085 ppb	22:23:51
2	B 249.677†	3102.8	-332.9	-5.5892 µg/L	-5.5892 ppb	22:23:51
2	Ba 233.527†	-171.7	7.8	0.0352 µg/L	0.0352 ppb	22:23:51
2	Be 313.107†	-760.6	-80.9	-0.0263 µg/L	-0.0263 ppb	22:23:31
2	Cd 226.502†	-75.1	21.3	0.1466 µg/L	0.1466 ppb	22:23:51
2	Co 228.616†	-175.4	5.7	0.0784 µg/L	0.0784 ppb	22:23:51
2	Cr 267.716†	170.4	5.8	0.0490 µg/L	0.0490 ppb	22:23:51
2	Cu 324.752†	3002.5	500.2	2.1749 µg/L	2.1749 ppb	22:23:31
2	Mn 257.610†	187.0	102.2	0.1400 µg/L	0.1400 ppb	22:23:51
2	Mo 202.031†	-6.1	49.2	1.5540 µg/L	1.5540 ppb	22:23:51
2	Ni 231.604†	-67.8	-25.2	-0.3219 µg/L	-0.3219 ppb	22:23:51
2	P 214.914†	19.7	-60.4	-14.507 µg/L	-14.507 ppb	22:23:51
2	Pb 220.353†	107.1	-8.1	-0.4886 µg/L	-0.4886 ppb	22:23:51

2	S 181.975 Axial†	88.2	-8.9	-7.1659 µg/L	-7.1659 ppb	22:23:51
2	Sb 206.836†	81.5	-7.3	-0.9613 µg/L	-0.9613 ppb	22:23:51
2	Se 196.026†	13.5	2.2	0.889 µg/L	0.889 ppb	22:23:51
2	SiO2†	1716.0	98.9	10.765 µg/L	10.765 ppb	22:23:51
2	Si 251.611†	860.2	161.6	2.6514 µg/L	2.6514 ppb	22:23:51
2	Sn 189.927†	2.5	0.4	0.0292 µg/L	0.0292 ppb	22:23:51
2	Ti 334.940†	705.6	51.1	0.0527 µg/L	0.0527 ppb	22:23:31
2	Tl 190.801†	-114.7	8.6	1.1402 µg/L	1.1402 ppb	22:23:51
2	U 409.014†	-487.9	3.8	0.1533 µg/L	0.1533 ppb	22:23:31
2	V 292.402†	179.2	-257.2	-1.4109 µg/L	-1.4109 ppb	22:23:31
2	Zn 213.857†	508.9	31.4	0.1979 µg/L	0.1979 ppb	22:23:51
3	Sc RADIAL	151305.2	151305.2	104 %		22:22:27
3	Al 396.153Radial†	-37.6	-4.4	-1.0405 µg/L	-1.0405 ppb	22:22:47
3	Ca 317.933Radial†	634.0	-5.4	-0.3182 µg/L	-0.3182 ppb	22:22:47
3	Fe 238.204 Radial†	145.7	27.0	1.7971 µg/L	1.7971 ppb	22:22:47
3	K 766.490 Radial†	1457.1	-51.4	-21.154 µg/L	-21.154 ppb	22:22:27
3	Mg 279.077 IEC†	160.0	-32.5	-13.375 µg/L	-13.375 ppb	22:22:47
3	Na 589.592 Radial†	1632.9	-121.7	-18.602 µg/L	-18.602 ppb	22:22:27
3	Sr 421.552†	-158.8	125.0	0.2930 µg/L	0.2930 ppb	22:22:27
3	Sc 361.383	1696452.4	1696452.4	101.42 %		22:23:54
3	Y 371.029	1039324.0	1039324.0	101.64 %		22:23:54
3	Ag 328.068†	3361.8	347.9	1.3916 µg/L	1.3916 ppb	22:23:56
3	As 188.979†	-22.4	-7.8	-3.2622 µg/L	-3.2622 ppb	22:24:16
3	B 249.677†	3155.6	-244.2	-4.0995 µg/L	-4.0995 ppb	22:24:16
3	Ba 233.527†	-185.2	-7.6	-0.0344 µg/L	-0.0344 ppb	22:24:16
3	Be 313.107†	-556.9	110.9	0.0329 µg/L	0.0329 ppb	22:23:56
3	Cd 226.502†	-87.0	8.7	0.0596 µg/L	0.0596 ppb	22:24:16
3	Co 228.616†	-172.6	6.4	0.0881 µg/L	0.0881 ppb	22:24:16
3	Cr 267.716†	143.3	-18.9	-0.1543 µg/L	-0.1543 ppb	22:24:16
3	Cu 324.752†	2803.5	339.5	1.4669 µg/L	1.4669 ppb	22:23:56
3	Mn 257.610†	199.4	116.6	0.1599 µg/L	0.1599 ppb	22:24:16
3	Mo 202.031†	1.4	56.6	1.7870 µg/L	1.7870 ppb	22:24:16
3	Ni 231.604†	-50.6	-8.9	-0.1143 µg/L	-0.1143 ppb	22:24:16
3	P 214.914†	39.3	-40.8	-9.8087 µg/L	-9.8087 ppb	22:24:16
3	Pb 220.353†	108.5	-5.4	-0.3153 µg/L	-0.3153 ppb	22:24:16
3	S 181.975 Axial†	90.6	-5.5	-4.4474 µg/L	-4.4474 ppb	22:24:16
3	Sb 206.836†	74.1	-13.6	-1.8066 µg/L	-1.8066 ppb	22:24:16
3	Se 196.026†	28.5	17.2	6.79 µg/L	6.79 ppb	22:24:16
3	SiO2†	1717.2	120.3	13.094 µg/L	13.094 ppb	22:24:16
3	Si 251.611†	817.8	130.0	2.1214 µg/L	2.1214 ppb	22:24:16
3	Sn 189.927†	10.4	8.2	0.5861 µg/L	0.5861 ppb	22:24:16
3	Ti 334.940†	751.3	104.5	0.1120 µg/L	0.1120 ppb	22:23:56
3	Tl 190.801†	-109.7	12.1	1.6251 µg/L	1.6251 ppb	22:24:16
3	U 409.014†	-660.7	-172.4	-10.683 µg/L	-10.683 ppb	22:23:56
3	V 292.402†	331.5	-104.9	-0.5717 µg/L	-0.5717 ppb	22:23:56
3	Zn 213.857†	511.3	39.8	0.2498 µg/L	0.2498 ppb	22:24:16

Mean Data: CCB

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1718713.4	102.75 %	1.383			1.35%
Sc RADIAL	152011.1	104 %	0.6			0.60%
Y 371.029	1052531.7	102.93 %	1.330			1.29%
Ag 328.068†	240.4	0.9566 µg/L	0.41670	0.9566 ppb	0.41670	43.56%
QC value within limits for Ag 328.068 Recovery = Not calculated						
Al 396.153Radial†	-3.9	-0.9205 µg/L	1.84510	-0.9205 ppb	1.84510	200.44%
QC value within limits for Al 396.153Radial Recovery = Not calculated						
As 188.979†	-3.8	-1.5923 µg/L	1.58505	-1.5923 ppb	1.58505	99.54%
QC value within limits for As 188.979 Recovery = Not calculated						
B 249.677†	-314.5	-5.2802 µg/L	1.06050	-5.2802 ppb	1.06050	20.08%
QC value within limits for B 249.677 Recovery = Not calculated						
Ba 233.527†	11.4	0.0517 µg/L	0.09546	0.0517 ppb	0.09546	184.53%
QC value within limits for Ba 233.527 Recovery = Not calculated						
Be 313.107†	6.3	0.0008 µg/L	0.02989	0.0008 ppb	0.02989	>999.9%
QC value within limits for Be 313.107 Recovery = Not calculated						
Ca 317.933Radial†	-8.2	-0.4792 µg/L	0.30265	-0.4792 ppb	0.30265	63.16%
QC value within limits for Ca 317.933Radial Recovery = Not calculated						
Cd 226.502†	7.8	0.0538 µg/L	0.09583	0.0538 ppb	0.09583	178.12%
QC value within limits for Cd 226.502 Recovery = Not calculated						
Co 228.616†	12.5	0.1708 µg/L	0.15171	0.1708 ppb	0.15171	88.81%

Cr 267.716†	QC value within limits for Co 228.616	Recovery = Not calculated			
	-1.9	-0.0137 µg/L	0.12202	-0.0137 ppb	0.12202 890.26%
Cu 324.752†	QC value within limits for Cr 267.716	Recovery = Not calculated			
	375.3	1.6284 µg/L	0.48629	1.6284 ppb	0.48629 29.86%
Fe 238.204 Radial†	QC value within limits for Cu 324.752	Recovery = Not calculated			
	36.0	2.3913 µg/L	0.52198	2.3913 ppb	0.52198 21.83%
K 766.490 Radial†	QC value within limits for Fe 238.204 Radial	Recovery = Not calculated			
	42.0	17.311 µg/L	35.8774	17.311 ppb	35.8774 207.25%
Mg 279.077 IEC†	QC value within limits for K 766.490 Radial	Recovery = Not calculated			
	-29.7	-12.200 µg/L	2.3830	-12.200 ppb	2.3830 19.53%
Mn 257.610†	QC value within limits for Mg 279.077 IEC	Recovery = Not calculated			
	105.7	0.1449 µg/L	0.01317	0.1449 ppb	0.01317 9.09%
Mo 202.031†	QC value within limits for Mn 257.610	Recovery = Not calculated			
	49.7	1.5679 µg/L	0.21243	1.5679 ppb	0.21243 13.55%
Na 589.592 Radial†	QC value within limits for Mo 202.031	Recovery = Not calculated			
	-103.5	-15.860 µg/L	10.2945	-15.860 ppb	10.2945 64.91%
Ni 231.604†	QC value within limits for Na 589.592 Radial	Recovery = Not calculated			
	-8.3	-0.1065 µg/L	0.21945	-0.1065 ppb	0.21945 206.12%
P 214.914†	QC value within limits for Ni 231.604	Recovery = Not calculated			
	-52.7	-12.647 µg/L	2.4974	-12.647 ppb	2.4974 19.75%
Pb 220.353†	QC value within limits for P 214.914	Recovery = Not calculated			
	-11.7	-0.7032 µg/L	0.52900	-0.7032 ppb	0.52900 75.22%
S 181.975 Axial†	QC value within limits for Pb 220.353	Recovery = Not calculated			
	-7.4	-5.9627 µg/L	1.38586	-5.9627 ppb	1.38586 23.24%
Sb 206.836†	QC value within limits for S 181.975 Axial	Recovery = Not calculated			
	-8.4	-1.1101 µg/L	0.63531	-1.1101 ppb	0.63531 57.23%
Se 196.026†	QC value within limits for Sb 206.836	Recovery = Not calculated			
	7.7	3.05 µg/L	3.254	3.05 ppb	3.254 106.62%
SiO2†	QC value within limits for Se 196.026	Recovery = Not calculated			
	95.0	10.336 µg/L	2.9948	10.336 ppb	2.9948 28.97%
Si 251.611†	QC value within limits for SiO2	Recovery = Not calculated			
	138.8	2.2727 µg/L	0.33024	2.2727 ppb	0.33024 14.53%
Sn 189.927†	QC value within limits for Si 251.611	Recovery = Not calculated			
	3.5	0.2485 µg/L	0.29673	0.2485 ppb	0.29673 119.41%
Sr 421.552†	QC value within limits for Sn 189.927	Recovery = Not calculated			
	114.6	0.2685 µg/L	0.09545	0.2685 ppb	0.09545 35.54%
Ti 334.940†	QC value within limits for Sr 421.552	Recovery = Not calculated			
	49.0	0.0526 µg/L	0.05945	0.0526 ppb	0.05945 112.94%
Tl 190.801†	QC value within limits for Ti 334.940	Recovery = Not calculated			
	9.4	1.2518 µg/L	0.33186	1.2518 ppb	0.33186 26.51%
U 409.014†	QC value within limits for Tl 190.801	Recovery = Not calculated			
	-65.5	-4.1145 µg/L	5.77269	-4.1145 ppb	5.77269 140.30%
V 292.402†	QC value within limits for U 409.014	Recovery = Not calculated			
	-211.7	-1.1612 µg/L	0.51246	-1.1612 ppb	0.51246 44.13%
Zn 213.857†	QC value within limits for V 292.402	Recovery = Not calculated			
	33.4	0.2092 µg/L	0.03629	0.2092 ppb	0.03629 17.35%
	QC value within limits for Zn 213.857	Recovery = Not calculated			

All analyte(s) passed QC.

Sequence No.: 90

Sample ID: CCV

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 1

Date Collected: 3/29/2010 22:42:27

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCV

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	153670.6	153670.6	105 %		22:43:01
1	Al 396.153Radial†	25532.3	24248.9	5270.5 µg/L	5270.5 ppb	22:43:01
1	Ca 317.933Radial†	89233.6	84020.5	4923.2 µg/L	4923.2 ppb	22:43:01
1	Fe 238.204 Radial†	78366.9	74216.5	4934.2 µg/L	4934.2 ppb	22:43:01
1	K 766.490 Radial†	13951.5	11777.8	4844.6 µg/L	4844.6 ppb	22:43:01
1	Mg 279.077 IEC†	13259.2	12389.5	5116.1 µg/L	5116.1 ppb	22:43:01
1	Na 589.592 Radial†	70022.2	64720.3	9898.7 µg/L	9898.7 ppb	22:43:01
1	Sr 421.552†	229045.7	217524.4	509.78 µg/L	509.78 ppb	22:42:59
1	Sc 361.383	1713229.0	1713229.0	102.42 %		22:43:14
1	Y 371.029	1036548.2	1036548.2	101.37 %		22:43:14
1	Ag 328.068†	127511.9	121534.0	499.48 µg/L	499.48 ppb	22:43:14
1	As 188.979†	1343.6	1326.1	561.34 µg/L	561.34 ppb	22:43:34
1	B 249.677†	32986.3	28851.7	482.68 µg/L	482.68 ppb	22:43:14
1	Ba 233.527†	113774.1	111262.6	508.69 µg/L	508.69 ppb	22:43:14
1	Be 313.107†	1631598.6	1593731.7	518.93 µg/L	518.93 ppb	22:43:14
1	Cd 226.502†	71789.2	70188.4	484.39 µg/L	484.39 ppb	22:43:14
1	Co 228.616†	36461.6	35777.2	490.17 µg/L	490.17 ppb	22:43:14
1	Cr 267.716†	59082.6	57527.2	493.98 µg/L	493.98 ppb	22:43:14
1	Cu 324.752†	120035.3	114776.0	500.47 µg/L	500.47 ppb	22:43:14
1	Mn 257.610†	372176.7	363308.5	496.22 µg/L	496.22 ppb	22:43:14
1	Mo 202.031†	15824.6	15506.1	489.92 µg/L	489.92 ppb	22:43:34
1	Ni 231.604†	39287.7	38400.9	491.19 µg/L	491.19 ppb	22:43:14
1	P 214.914†	10456.8	10130.3	2417.6 µg/L	2417.6 ppb	22:43:34
1	Pb 220.353†	8326.6	8017.5	487.25 µg/L	487.25 ppb	22:43:34
1	S 181.975 Axial†	1304.8	1179.1	959.43 µg/L	959.43 ppb	22:43:34
1	Sb 206.836†	3849.6	3672.0	496.42 µg/L	496.42 ppb	22:43:34
1	Se 196.026†	1254.9	1214.3	483 µg/L	483 ppb	22:43:34
1	SiO2†	51326.3	48541.5	5284.5 µg/L	5284.5 ppb	22:43:14
1	Si 251.611†	154043.3	149729.5	2465.9 µg/L	2465.9 ppb	22:43:14
1	Sn 189.927†	7190.3	7018.5	500.63 µg/L	500.63 ppb	22:43:34
1	Ti 334.940†	500662.7	488204.2	497.17 µg/L	497.17 ppb	22:43:14
1	Tl 190.801†	3597.1	3632.4	495.09 µg/L	495.09 ppb	22:43:34
1	U 409.014†	7277.7	7584.9	499.24 µg/L	499.24 ppb	22:43:14
1	V 292.402†	92881.7	90256.7	506.92 µg/L	506.92 ppb	22:43:14
1	Zn 213.857†	79753.5	77405.8	483.38 µg/L	483.38 ppb	22:43:14
2	Sc RADIAL	153338.2	153338.2	105 %		22:43:05
2	Al 396.153Radial†	25484.3	24255.7	5272.5 µg/L	5272.5 ppb	22:43:05
2	Ca 317.933Radial†	89276.4	84244.7	4936.4 µg/L	4936.4 ppb	22:43:05
2	Fe 238.204 Radial†	78452.2	74458.8	4950.3 µg/L	4950.3 ppb	22:43:05
2	K 766.490 Radial†	14131.6	11977.7	4926.8 µg/L	4926.8 ppb	22:43:05
2	Mg 279.077 IEC†	13272.8	12429.7	5132.4 µg/L	5132.4 ppb	22:43:05
2	Na 589.592 Radial†	70049.9	64890.6	9924.7 µg/L	9924.7 ppb	22:43:05
2	Sr 421.552†	227233.2	216272.5	506.85 µg/L	506.85 ppb	22:43:03
2	Sc 361.383	1742064.1	1742064.1	104.14 %		22:43:37
2	Y 371.029	1053661.3	1053661.3	103.04 %		22:43:37
2	Ag 328.068†	128515.8	120437.1	494.94 µg/L	494.94 ppb	22:43:37
2	As 188.979†	1335.3	1296.4	548.84 µg/L	548.84 ppb	22:43:57
2	B 249.677†	33342.8	28660.9	479.49 µg/L	479.49 ppb	22:43:37
2	Ba 233.527†	114630.7	110246.4	504.04 µg/L	504.04 ppb	22:43:37
2	Be 313.107†	1643078.7	1578386.3	513.93 µg/L	513.93 ppb	22:43:37
2	Cd 226.502†	72541.4	69750.5	481.36 µg/L	481.36 ppb	22:43:37
2	Co 228.616†	36852.9	35563.7	487.24 µg/L	487.24 ppb	22:43:37
2	Cr 267.716†	59491.9	56965.4	489.16 µg/L	489.16 ppb	22:43:37
2	Cu 324.752†	120802.1	113572.4	495.23 µg/L	495.23 ppb	22:43:37
2	Mn 257.610†	375411.3	360399.5	492.25 µg/L	492.25 ppb	22:43:37
2	Mo 202.031†	15759.6	15187.9	479.88 µg/L	479.88 ppb	22:43:57
2	Ni 231.604†	39775.9	38234.8	489.07 µg/L	489.07 ppb	22:43:37
2	P 214.914†	10394.9	9901.9	2362.9 µg/L	2362.9 ppb	22:43:57
2	Pb 220.353†	8272.7	7831.2	475.94 µg/L	475.94 ppb	22:43:57

2	S 181.975 Axial†	1293.3	1147.1	933.39 µg/L	933.39 ppb	22:43:57
2	Sb 206.836†	3828.2	3589.3	485.17 µg/L	485.17 ppb	22:43:57
2	Se 196.026†	1246.5	1186.1	471 µg/L	471 ppb	22:43:57
2	SiO2†	51780.7	48148.3	5241.9 µg/L	5241.9 ppb	22:43:37
2	Si 251.611†	155219.0	148368.9	2443.6 µg/L	2443.6 ppb	22:43:37
2	Sn 189.927†	7132.8	6847.1	488.43 µg/L	488.43 ppb	22:43:57
2	Ti 334.940†	503531.9	482867.8	491.73 µg/L	491.73 ppb	22:43:37
2	Tl 190.801†	3581.7	3559.5	485.21 µg/L	485.21 ppb	22:43:57
2	U 409.014†	7146.8	7341.7	483.86 µg/L	483.86 ppb	22:43:37
2	V 292.402†	93375.5	89229.7	501.09 µg/L	501.09 ppb	22:43:37
2	Zn 213.857†	80733.7	77058.2	481.21 µg/L	481.21 ppb	22:43:37
3	Sc RADIAL	153918.1	153918.1	106 %		22:43:09
3	Al 396.153Radial†	25598.5	24272.6	5276.1 µg/L	5276.1 ppb	22:43:09
3	Ca 317.933Radial†	89923.4	84537.6	4953.5 µg/L	4953.5 ppb	22:43:09
3	Fe 238.204 Radial†	78639.1	74354.7	4943.4 µg/L	4943.4 ppb	22:43:09
3	K 766.490 Radial†	13877.1	11686.1	4806.8 µg/L	4806.8 ppb	22:43:09
3	Mg 279.077 IEC†	13270.8	12380.3	5112.0 µg/L	5112.0 ppb	22:43:09
3	Na 589.592 Radial†	70254.6	64833.6	9916.1 µg/L	9916.1 ppb	22:43:09
3	Sr 421.552†	228786.4	216929.5	508.39 µg/L	508.39 ppb	22:43:07
3	Sc 361.383	1738165.6	1738165.6	103.91 %		22:44:00
3	Y 371.029	1052043.8	1052043.8	102.88 %		22:44:00
3	Ag 328.068†	128389.3	120592.1	495.57 µg/L	495.57 ppb	22:44:00
3	As 188.979†	1343.6	1307.3	553.39 µg/L	553.39 ppb	22:44:20
3	B 249.677†	33214.1	28608.9	478.62 µg/L	478.62 ppb	22:44:00
3	Ba 233.527†	113962.7	109850.4	502.23 µg/L	502.23 ppb	22:44:00
3	Be 313.107†	1635274.2	1574414.0	512.64 µg/L	512.64 ppb	22:44:00
3	Cd 226.502†	72141.5	69521.9	479.78 µg/L	479.78 ppb	22:44:00
3	Co 228.616†	36635.4	35433.7	485.46 µg/L	485.46 ppb	22:44:00
3	Cr 267.716†	59220.7	56832.5	488.01 µg/L	488.01 ppb	22:44:00
3	Cu 324.752†	120354.6	113401.9	494.50 µg/L	494.50 ppb	22:44:00
3	Mn 257.610†	373061.4	358946.6	490.26 µg/L	490.26 ppb	22:44:00
3	Mo 202.031†	15720.2	15184.0	479.76 µg/L	479.76 ppb	22:44:20
3	Ni 231.604†	39617.8	38168.2	488.22 µg/L	488.22 ppb	22:44:00
3	P 214.914†	10370.4	9900.6	2362.7 µg/L	2362.7 ppb	22:44:20
3	Pb 220.353†	8273.8	7850.1	477.07 µg/L	477.07 ppb	22:44:20
3	S 181.975 Axial†	1305.4	1161.5	945.06 µg/L	945.06 ppb	22:44:20
3	Sb 206.836†	3838.2	3607.2	487.59 µg/L	487.59 ppb	22:44:20
3	Se 196.026†	1253.8	1195.7	475 µg/L	475 ppb	22:44:20
3	SiO2†	51493.2	47983.1	5223.9 µg/L	5223.9 ppb	22:44:00
3	Si 251.611†	154605.0	148112.3	2439.4 µg/L	2439.4 ppb	22:44:00
3	Sn 189.927†	7146.9	6876.0	490.48 µg/L	490.48 ppb	22:44:20
3	Ti 334.940†	501550.0	482044.9	490.89 µg/L	490.89 ppb	22:44:00
3	Tl 190.801†	3584.4	3569.9	486.57 µg/L	486.57 ppb	22:44:20
3	U 409.014†	7451.7	7650.5	502.82 µg/L	502.82 ppb	22:44:00
3	V 292.402†	92793.5	88870.7	499.10 µg/L	499.10 ppb	22:44:00
3	Zn 213.857†	80130.4	76651.4	478.65 µg/L	478.65 ppb	22:44:00

Mean Data: CCV

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1731152.9	103.49 %	0.935			0.90%
Sc RADIAL	153642.3	105 %	0.2			0.19%
Y 371.029	1047417.8	102.43 %	0.924			0.90%
Ag 328.068†	120854.4	496.66 µg/L	2.458	496.66 ppb	2.458	0.49%
QC value within limits for Ag 328.068 Recovery = 99.33%						
Al 396.153Radial†	24259.1	5273.0 µg/L	2.86	5273.0 ppb	2.86	0.05%
QC value within limits for Al 396.153Radial Recovery = 105.46%						
As 188.979†	1309.9	554.52 µg/L	6.329	554.52 ppb	6.329	1.14%
QC value greater than the upper limit for As 188.979 Recovery = 110.90%						
B 249.677†	28707.2	480.26 µg/L	2.138	480.26 ppb	2.138	0.45%
QC value within limits for B 249.677 Recovery = 96.05%						
Ba 233.527†	110453.1	504.99 µg/L	3.332	504.99 ppb	3.332	0.66%
QC value within limits for Ba 233.527 Recovery = 101.00%						
Be 313.107†	1582177.3	515.17 µg/L	3.321	515.17 ppb	3.321	0.64%
QC value within limits for Be 313.107 Recovery = 103.03%						
Ca 317.933Radial†	84267.6	4937.7 µg/L	15.19	4937.7 ppb	15.19	0.31%
QC value within limits for Ca 317.933Radial Recovery = 98.75%						
Cd 226.502†	69820.3	481.85 µg/L	2.340	481.85 ppb	2.340	0.49%
QC value within limits for Cd 226.502 Recovery = 96.37%						
Co 228.616†	35591.5	487.62 µg/L	2.378	487.62 ppb	2.378	0.49%

QC value within limits for Co 228.616 Recovery = 97.52%							
Cr 267.716†	57108.4	490.38 µg/L	3.167	490.38 ppb	3.167	0.65%	
QC value within limits for Cr 267.716 Recovery = 98.08%							
Cu 324.752†	113916.7	496.74 µg/L	3.258	496.74 ppb	3.258	0.66%	
QC value within limits for Cu 324.752 Recovery = 99.35%							
Fe 238.204 Radial†	74343.3	4942.6 µg/L	8.08	4942.6 ppb	8.08	0.16%	
QC value within limits for Fe 238.204 Radial Recovery = 98.85%							
K 766.490 Radial†	11813.8	4859.4 µg/L	61.38	4859.4 ppb	61.38	1.26%	
QC value within limits for K 766.490 Radial Recovery = 97.19%							
Mg 279.077 IEC†	12399.8	5120.2 µg/L	10.79	5120.2 ppb	10.79	0.21%	
QC value within limits for Mg 279.077 IEC Recovery = 102.40%							
Mn 257.610†	360884.9	492.91 µg/L	3.035	492.91 ppb	3.035	0.62%	
QC value within limits for Mn 257.610 Recovery = 98.58%							
Mo 202.031†	15292.7	483.19 µg/L	5.836	483.19 ppb	5.836	1.21%	
QC value within limits for Mo 202.031 Recovery = 96.64%							
Na 589.592 Radial†	64814.8	9913.2 µg/L	13.23	9913.2 ppb	13.23	0.13%	
QC value within limits for Na 589.592 Radial Recovery = 99.13%							
Ni 231.604†	38268.0	489.49 µg/L	1.533	489.49 ppb	1.533	0.31%	
QC value within limits for Ni 231.604 Recovery = 97.90%							
P 214.914†	9977.6	2381.1 µg/L	31.64	2381.1 ppb	31.64	1.33%	
QC value within limits for P 214.914 Recovery = 95.24%							
Pb 220.353†	7899.6	480.09 µg/L	6.228	480.09 ppb	6.228	1.30%	
QC value within limits for Pb 220.353 Recovery = 96.02%							
S 181.975 Axial†	1162.6	945.96 µg/L	13.047	945.96 ppb	13.047	1.38%	
QC value within limits for S 181.975 Axial Recovery = 94.60%							
Sb 206.836†	3622.8	489.72 µg/L	5.923	489.72 ppb	5.923	1.21%	
QC value within limits for Sb 206.836 Recovery = 97.94%							
Se 196.026†	1198.7	476 µg/L	5.7	476 ppb	5.7	1.19%	
QC value within limits for Se 196.026 Recovery = 95.26%							
SiO2†	48224.3	5250.1 µg/L	31.11	5250.1 ppb	31.11	0.59%	
QC value within limits for SiO2 Recovery = 98.18%							
Si 251.611†	148736.9	2449.7 µg/L	14.25	2449.7 ppb	14.25	0.58%	
QC value within limits for Si 251.611 Recovery = 97.99%							
Sn 189.927†	6913.8	493.18 µg/L	6.535	493.18 ppb	6.535	1.33%	
QC value within limits for Sn 189.927 Recovery = 98.64%							
Sr 421.552†	216908.8	508.34 µg/L	1.468	508.34 ppb	1.468	0.29%	
QC value within limits for Sr 421.552 Recovery = 101.67%							
Ti 334.940†	484372.3	493.26 µg/L	3.408	493.26 ppb	3.408	0.69%	
QC value within limits for Ti 334.940 Recovery = 98.65%							
Tl 190.801†	3587.3	488.96 µg/L	5.353	488.96 ppb	5.353	1.09%	
QC value within limits for Tl 190.801 Recovery = 97.79%							
U 409.014†	7525.7	495.31 µg/L	10.074	495.31 ppb	10.074	2.03%	
QC value within limits for U 409.014 Recovery = 99.06%							
V 292.402†	89452.4	502.37 µg/L	4.061	502.37 ppb	4.061	0.81%	
QC value within limits for V 292.402 Recovery = 100.47%							
Zn 213.857†	77038.5	481.08 µg/L	2.367	481.08 ppb	2.367	0.49%	
QC value within limits for Zn 213.857 Recovery = 96.22%							
QC Failed. Continue with analysis.							

Sequence No.: 91
 Sample ID: CCB
 Analyst:
 Initial Sample Wt:
 Dilution:

Autosampler Location: 6
 Date Collected: 3/29/2010 22:44:29
 Data Type: Original
 Initial Sample Vol:
 Sample Prep Vol:

Replicate Data: CCB

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	154912.0	154912.0	106 %		22:44:59
1	Al 396.153Radial†	-35.0	-1.1	-0.2804 µg/L	-0.2804 ppb	22:45:19
1	Ca 317.933Radial†	642.9	-11.3	-0.6631 µg/L	-0.6631 ppb	22:45:19
1	Fe 238.204 Radial†	163.6	40.6	2.6994 µg/L	2.6994 ppb	22:45:19
1	K 766.490 Radial†	1426.7	-112.7	-46.378 µg/L	-46.378 ppb	22:44:59
1	Mg 279.077 IEC†	180.0	-17.3	-7.1267 µg/L	-7.1267 ppb	22:45:19
1	Na 589.592 Radial†	1706.5	-89.1	-13.586 µg/L	-13.586 ppb	22:44:59
1	Sr 421.552†	-175.2	113.1	0.2652 µg/L	0.2652 ppb	22:44:59
1	Sc 361.383	1763263.5	1763263.5	105.41 %		22:46:07
1	Y 371.029	1078054.6	1078054.6	105.42 %		22:46:07
1	Ag 328.068†	3459.8	315.2	1.2970 µg/L	1.2970 ppb	22:46:09
1	As 188.979†	-24.9	-9.4	-3.9329 µg/L	-3.9329 ppb	22:46:29
1	B 249.677†	3110.0	-405.3	-6.8044 µg/L	-6.8044 ppb	22:46:29
1	Ba 233.527†	-155.7	27.4	0.1251 µg/L	0.1251 ppb	22:46:29
1	Be 313.107†	-549.3	139.0	0.0510 µg/L	0.0510 ppb	22:46:09
1	Cd 226.502†	-95.9	3.4	0.0231 µg/L	0.0231 ppb	22:46:29
1	Co 228.616†	-186.7	-0.5	-0.0073 µg/L	-0.0073 ppb	22:46:29
1	Cr 267.716†	177.6	8.2	0.0553 µg/L	0.0553 ppb	22:46:29
1	Cu 324.752†	2872.9	300.6	1.3229 µg/L	1.3229 ppb	22:46:09
1	Mn 257.610†	184.1	94.6	0.1296 µg/L	0.1296 ppb	22:46:29
1	Mo 202.031†	-26.2	30.4	0.9589 µg/L	0.9589 ppb	22:46:29
1	Ni 231.604†	-47.7	-4.3	-0.0553 µg/L	-0.0553 ppb	22:46:29
1	P 214.914†	31.9	-49.3	-11.833 µg/L	-11.833 ppb	22:46:29
1	Pb 220.353†	75.9	-40.5	-2.4620 µg/L	-2.4620 ppb	22:46:29
1	S 181.975 Axial†	96.5	-3.3	-2.6691 µg/L	-2.6691 ppb	22:46:29
1	Sb 206.836†	94.3	2.8	0.3918 µg/L	0.3918 ppb	22:46:29
1	Se 196.026†	22.1	10.1	4.01 µg/L	4.01 ppb	22:46:29
1	SiO2†	1729.5	67.9	7.3789 µg/L	7.3789 ppb	22:46:29
1	Si 251.611†	852.7	132.5	2.1731 µg/L	2.1731 ppb	22:46:29
1	Sn 189.927†	14.1	11.4	0.8115 µg/L	0.8115 ppb	22:46:29
1	Ti 334.940†	920.6	237.0	0.2344 µg/L	0.2344 ppb	22:46:09
1	Tl 190.801†	-118.0	8.4	1.1222 µg/L	1.1222 ppb	22:46:29
1	U 409.014†	-177.4	310.8	19.177 µg/L	19.177 ppb	22:46:09
1	V 292.402†	364.3	-86.2	-0.4555 µg/L	-0.4555 ppb	22:46:09
1	Zn 213.857†	511.7	21.0	0.1315 µg/L	0.1315 ppb	22:46:29
2	Sc RADIAL	153548.1	153548.1	105 %		22:45:21
2	Al 396.153Radial†	-31.3	2.2	0.4081 µg/L	0.4081 ppb	22:45:41
2	Ca 317.933Radial†	642.0	-6.8	-0.3982 µg/L	-0.3982 ppb	22:45:41
2	Fe 238.204 Radial†	145.2	24.6	1.6337 µg/L	1.6337 ppb	22:45:41
2	K 766.490 Radial†	1418.9	-108.1	-44.492 µg/L	-44.492 ppb	22:45:21
2	Mg 279.077 IEC†	174.6	-20.9	-8.5921 µg/L	-8.5921 ppb	22:45:41
2	Na 589.592 Radial†	1677.9	-102.0	-15.567 µg/L	-15.567 ppb	22:45:21
2	Sr 421.552†	-164.6	121.7	0.2853 µg/L	0.2853 ppb	22:45:21
2	Sc 361.383	1742152.7	1742152.7	104.15 %		22:46:31
2	Y 371.029	1065618.3	1065618.3	104.21 %		22:46:31
2	Ag 328.068†	3303.4	204.8	0.8259 µg/L	0.8259 ppb	22:46:34
2	As 188.979†	-13.5	1.3	0.5289 µg/L	0.5289 ppb	22:46:54
2	B 249.677†	3107.7	-371.7	-6.2409 µg/L	-6.2409 ppb	22:46:54
2	Ba 233.527†	-159.2	22.2	0.1013 µg/L	0.1013 ppb	22:46:54
2	Be 313.107†	-751.4	-61.3	-0.0185 µg/L	-0.0185 ppb	22:46:34
2	Cd 226.502†	-95.8	2.4	0.0166 µg/L	0.0166 ppb	22:46:54
2	Co 228.616†	-177.5	6.1	0.0840 µg/L	0.0840 ppb	22:46:54
2	Cr 267.716†	192.1	24.2	0.2038 µg/L	0.2038 ppb	22:46:54
2	Cu 324.752†	2839.7	301.7	1.3157 µg/L	1.3157 ppb	22:46:34
2	Mn 257.610†	146.4	60.5	0.0831 µg/L	0.0831 ppb	22:46:54
2	Mo 202.031†	-13.5	42.2	1.3326 µg/L	1.3326 ppb	22:46:54
2	Ni 231.604†	-63.6	-20.2	-0.2583 µg/L	-0.2583 ppb	22:46:54
2	P 214.914†	31.2	-49.6	-11.901 µg/L	-11.901 ppb	22:46:54
2	Pb 220.353†	82.8	-32.9	-1.9932 µg/L	-1.9932 ppb	22:46:54

2	S 181.975 Axial†	81.5	-16.6	-13.406 µg/L	-13.406 ppb	22:46:54
2	Sb 206.836†	82.0	-7.9	-1.0565 µg/L	-1.0565 ppb	22:46:54
2	Se 196.026†	7.9	-3.3	-1.32 µg/L	-1.32 ppb	22:46:54
2	SiO2†	1731.4	89.6	9.7506 µg/L	9.7506 ppb	22:46:54
2	Si 251.611†	850.1	139.9	2.2935 µg/L	2.2935 ppb	22:46:54
2	Sn 189.927†	5.1	2.9	0.2036 µg/L	0.2036 ppb	22:46:54
2	Ti 334.940†	788.8	121.0	0.1220 µg/L	0.1220 ppb	22:46:34
2	Tl 190.801†	-114.7	10.2	1.3610 µg/L	1.3610 ppb	22:46:54
2	U 409.014†	-416.9	78.8	4.8158 µg/L	4.8158 ppb	22:46:34
2	V 292.402†	274.8	-168.0	-0.9142 µg/L	-0.9142 ppb	22:46:34
2	Zn 213.857†	471.1	-12.1	-0.0756 µg/L	-0.0756 ppb	22:46:54
3	Sc RADIAL	154388.4	154388.4	106 %		22:45:43
3	Al 396.153Radial†	-29.7	3.8	0.7678 µg/L	0.7678 ppb	22:46:03
3	Ca 317.933Radial†	650.1	-2.5	-0.1455 µg/L	-0.1455 ppb	22:46:03
3	Fe 238.204 Radial†	160.3	38.1	2.5315 µg/L	2.5315 ppb	22:46:03
3	K 766.490 Radial†	1386.3	-146.2	-60.200 µg/L	-60.200 ppb	22:45:43
3	Mg 279.077 IEC†	169.5	-26.7	-10.958 µg/L	-10.958 ppb	22:46:03
3	Na 589.592 Radial†	1530.6	-249.7	-38.157 µg/L	-38.157 ppb	22:45:43
3	Sr 421.552†	-237.9	53.4	0.1250 µg/L	0.1250 ppb	22:45:43
3	Sc 361.383	1750459.2	1750459.2	104.64 %		22:46:56
3	Y 371.029	1070679.8	1070679.8	104.70 %		22:46:56
3	Ag 328.068†	3084.2	-19.7	-0.0766 µg/L	-0.0766 ppb	22:46:58
3	As 188.979†	-5.5	9.0	3.7759 µg/L	3.7759 ppb	22:47:18
3	B 249.677†	3100.0	-393.3	-6.6028 µg/L	-6.6028 ppb	22:47:18
3	Ba 233.527†	-155.7	26.3	0.1198 µg/L	0.1198 ppb	22:47:18
3	Be 313.107†	-710.6	-18.9	-0.0028 µg/L	-0.0028 ppb	22:46:58
3	Cd 226.502†	-91.7	6.8	0.0466 µg/L	0.0466 ppb	22:47:18
3	Co 228.616†	-175.2	9.2	0.1261 µg/L	0.1261 ppb	22:47:18
3	Cr 267.716†	129.8	-36.2	-0.3199 µg/L	-0.3199 ppb	22:47:18
3	Cu 324.752†	2844.0	292.9	1.2827 µg/L	1.2827 ppb	22:46:58
3	Mn 257.610†	164.1	76.9	0.1055 µg/L	0.1055 ppb	22:47:18
3	Mo 202.031†	-10.2	45.5	1.4349 µg/L	1.4349 ppb	22:47:18
3	Ni 231.604†	-50.8	-7.6	-0.0975 µg/L	-0.0975 ppb	22:47:18
3	P 214.914†	34.6	-46.5	-11.157 µg/L	-11.157 ppb	22:47:18
3	Pb 220.353†	85.4	-30.8	-1.8707 µg/L	-1.8707 ppb	22:47:18
3	S 181.975 Axial†	93.1	-5.9	-4.7394 µg/L	-4.7394 ppb	22:47:18
3	Sb 206.836†	89.1	-1.5	-0.1726 µg/L	-0.1726 ppb	22:47:18
3	Se 196.026†	18.1	6.3	2.52 µg/L	2.52 ppb	22:47:18
3	SiO2†	1733.5	83.7	9.1075 µg/L	9.1075 ppb	22:47:18
3	Si 251.611†	819.6	106.9	1.7472 µg/L	1.7472 ppb	22:47:18
3	Sn 189.927†	3.7	1.6	0.1115 µg/L	0.1115 ppb	22:47:18
3	Ti 334.940†	816.3	143.8	0.1431 µg/L	0.1431 ppb	22:46:58
3	Tl 190.801†	-122.0	3.7	0.4965 µg/L	0.4965 ppb	22:47:18
3	U 409.014†	-315.7	177.4	10.912 µg/L	10.912 ppb	22:46:58
3	V 292.402†	292.4	-152.4	-0.8252 µg/L	-0.8252 ppb	22:46:58
3	Zn 213.857†	509.1	22.1	0.1383 µg/L	0.1383 ppb	22:47:18

Mean Data: CCB

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1751958.5	104.73 %	0.636			0.61%
Sc RADIAL	154282.8	106 %	0.5			0.45%
Y 371.029	1071450.9	104.78 %	0.612			0.58%
Ag 328.068†	166.8	0.6821 µg/L	0.69799	0.6821 ppb	0.69799	102.33%
QC value within limits for Ag 328.068 Recovery = Not calculated						
Al 396.153Radial†	1.6	0.2985 µg/L	0.53261	0.2985 ppb	0.53261	178.41%
QC value within limits for Al 396.153Radial Recovery = Not calculated						
As 188.979†	0.3	0.1240 µg/L	3.87033	0.1240 ppb	3.87033	>999.9%
QC value within limits for As 188.979 Recovery = Not calculated						
B 249.677†	-390.1	-6.5494 µg/L	0.28549	-6.5494 ppb	0.28549	4.36%
QC value within limits for B 249.677 Recovery = Not calculated						
Ba 233.527†	25.3	0.1154 µg/L	0.01249	0.1154 ppb	0.01249	10.82%
QC value within limits for Ba 233.527 Recovery = Not calculated						
Be 313.107†	19.6	0.0099 µg/L	0.03648	0.0099 ppb	0.03648	368.40%
QC value within limits for Be 313.107 Recovery = Not calculated						
Ca 317.933Radial†	-6.9	-0.4023 µg/L	0.25879	-0.4023 ppb	0.25879	64.33%
QC value within limits for Ca 317.933Radial Recovery = Not calculated						
Cd 226.502†	4.2	0.0288 µg/L	0.01577	0.0288 ppb	0.01577	54.78%
QC value within limits for Cd 226.502 Recovery = Not calculated						
Co 228.616†	4.9	0.0676 µg/L	0.06820	0.0676 ppb	0.06820	100.91%

Cr 267.716†	QC value within limits for Co 228.616	Recovery = Not calculated		
	-1.3	-0.0203 µg/L	0.26989	-0.0203 ppb
			0.26989	>999.9%
Cu 324.752†	QC value within limits for Cr 267.716	Recovery = Not calculated		
	298.4	1.3071 µg/L	0.02146	1.3071 ppb
			0.02146	1.64%
Fe 238.204 Radial†	QC value within limits for Cu 324.752	Recovery = Not calculated		
	34.4	2.2882 µg/L	0.57300	2.2882 ppb
			0.57300	25.04%
K 766.490 Radial†	QC value within limits for Fe 238.204 Radial	Recovery = Not calculated		
	-122.3	-50.357 µg/L	8.5766	-50.357 ppb
			8.5766	17.03%
Mg 279.077 IEC†	QC value within limits for K 766.490 Radial	Recovery = Not calculated		
	-21.6	-8.8922 µg/L	1.93304	-8.8922 ppb
			1.93304	21.74%
Mn 257.610†	QC value within limits for Mg 279.077 IEC	Recovery = Not calculated		
	77.3	0.1060 µg/L	0.02325	0.1060 ppb
			0.02325	21.93%
Mo 202.031†	QC value within limits for Mn 257.610	Recovery = Not calculated		
	39.4	1.2422 µg/L	0.25054	1.2422 ppb
			0.25054	20.17%
Na 589.592 Radial†	QC value within limits for Mo 202.031	Recovery = Not calculated		
	-146.9	-22.437 µg/L	13.6499	-22.437 ppb
			13.6499	60.84%
Ni 231.604†	QC value within limits for Na 589.592 Radial	Recovery = Not calculated		
	-10.7	-0.1370 µg/L	0.10709	-0.1370 ppb
			0.10709	78.15%
P 214.914†	QC value within limits for Ni 231.604	Recovery = Not calculated		
	-48.5	-11.630 µg/L	0.4111	-11.630 ppb
			0.4111	3.54%
Pb 220.353†	QC value within limits for P 214.914	Recovery = Not calculated		
	-34.7	-2.1086 µg/L	0.31210	-2.1086 ppb
			0.31210	14.80%
S 181.975 Axial†	QC value within limits for Pb 220.353	Recovery = Not calculated		
	-8.6	-6.9382 µg/L	5.69617	-6.9382 ppb
			5.69617	82.10%
Sb 206.836†	QC value within limits for S 181.975 Axial	Recovery = Not calculated		
	-2.2	-0.2791 µg/L	0.73004	-0.2791 ppb
			0.73004	261.58%
Se 196.026†	QC value within limits for Sb 206.836	Recovery = Not calculated		
	4.4	1.74 µg/L	2.749	1.74 ppb
			2.749	158.29%
SiO2†	QC value within limits for Se 196.026	Recovery = Not calculated		
	80.4	8.7457 µg/L	1.22656	8.7457 ppb
			1.22656	14.02%
Si 251.611†	QC value within limits for SiO2	Recovery = Not calculated		
	126.4	2.0713 µg/L	0.28701	2.0713 ppb
			0.28701	13.86%
Sn 189.927†	QC value within limits for Si 251.611	Recovery = Not calculated		
	5.3	0.3755 µg/L	0.38038	0.3755 ppb
			0.38038	101.29%
Sr 421.552†	QC value within limits for Sn 189.927	Recovery = Not calculated		
	96.1	0.2252 µg/L	0.08730	0.2252 ppb
			0.08730	38.77%
Ti 334.940†	QC value within limits for Sr 421.552	Recovery = Not calculated		
	167.3	0.1665 µg/L	0.05972	0.1665 ppb
			0.05972	35.87%
Tl 190.801†	QC value within limits for Ti 334.940	Recovery = Not calculated		
	7.4	0.9932 µg/L	0.44647	0.9932 ppb
			0.44647	44.95%
U 409.014†	QC value within limits for Tl 190.801	Recovery = Not calculated		
	189.0	11.635 µg/L	7.2080	11.635 ppb
			7.2080	61.95%
V 292.402†	QC value within limits for U 409.014	Recovery = Not calculated		
	-135.5	-0.7316 µg/L	0.24321	-0.7316 ppb
			0.24321	33.24%
Zn 213.857†	QC value within limits for V 292.402	Recovery = Not calculated		
	10.3	0.0648 µg/L	0.12157	0.0648 ppb
			0.12157	187.70%

QC value within limits for Zn 213.857 Recovery = Not calculated

All analyte(s) passed QC.

Sequence No.: 92

Sample ID: 1202056877|959114|1

Analyst: HSC

Initial Sample Wt:

Dilution:

Autosampler Location: 412

Date Collected: 3/29/2010 22:47:26

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: 1202056877|959114|1

Repl#	Analyte	Net Intensity	Corrected Intensity	Conc. Units	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	153706.8	153706.8	105 %			22:47:58
1	Al 396.153Radial†	313.0	328.7	71.710 µg/L	71.710 ppb	71.710 ppb	22:48:00
1	Ca 317.933Radial†	1390.5	702.4	41.158 µg/L	41.158 ppb	41.158 ppb	22:48:00
1	Fe 238.204 Radial†	2558.9	2313.2	153.79 µg/L	153.79 ppb	153.79 ppb	22:48:00
1	K 766.490 Radial†	1427.1	-101.7	-41.901 µg/L	-41.901 ppb	-41.901 ppb	22:47:58
1	Mg 279.077 IEC†	229.3	30.8	12.569 µg/L	12.569 ppb	12.569 ppb	22:48:00
1	Na 589.592 Radial†	1689.6	-92.6	-14.125 µg/L	-14.125 ppb	-14.125 ppb	22:48:00
1	Sr 421.552†	40.3	316.2	0.7409 µg/L	0.7409 ppb	0.7409 ppb	22:48:00
1	Sc 361.383	1723755.6	1723755.6	103.05 %			22:48:12
1	Y 371.029	1051639.9	1051639.9	102.84 %			22:48:12
1	Ag 328.068†	2889.7	-162.8	-0.6433 µg/L	-0.6433 ppb	-0.6433 ppb	22:48:14
1	As 188.979†	-16.8	-2.1	-0.8147 µg/L	-0.8147 ppb	-0.8147 ppb	22:48:34
1	B 249.677†	3188.5	-261.5	-4.3903 µg/L	-4.3903 ppb	-4.3903 ppb	22:48:34
1	Ba 233.527†	222.9	391.4	1.7857 µg/L	1.7857 ppb	1.7857 ppb	22:48:34
1	Be 313.107†	-542.9	133.2	0.0503 µg/L	0.0503 ppb	0.0503 ppb	22:48:14
1	Cd 226.502†	-84.2	12.7	0.0716 µg/L	0.0716 ppb	0.0716 ppb	22:48:34
1	Co 228.616†	-164.2	17.3	0.2304 µg/L	0.2304 ppb	0.2304 ppb	22:48:34
1	Cr 267.716†	242.2	74.8	0.6282 µg/L	0.6282 ppb	0.6282 ppb	22:48:34
1	Cu 324.752†	2837.0	328.2	1.4686 µg/L	1.4686 ppb	1.4686 ppb	22:48:14
1	Mn 257.610†	2489.3	2335.7	3.1907 µg/L	3.1907 ppb	3.1907 ppb	22:48:34
1	Mo 202.031†	-34.8	21.4	0.6813 µg/L	0.6813 ppb	0.6813 ppb	22:48:34
1	Ni 231.604†	-35.8	6.2	0.0790 µg/L	0.0790 ppb	0.0790 ppb	22:48:34
1	P 214.914†	54.8	-26.4	-6.4254 µg/L	-6.4254 ppb	-6.4254 ppb	22:48:34
1	Pb 220.353†	84.5	-30.5	-1.8570 µg/L	-1.8570 ppb	-1.8570 ppb	22:48:34
1	S 181.975 Axial†	107.3	9.3	7.5032 µg/L	7.5032 ppb	7.5032 ppb	22:48:34
1	Sb 206.836†	81.0	-8.1	-1.0893 µg/L	-1.0893 ppb	-1.0893 ppb	22:48:34
1	Se 196.026†	16.7	5.3	2.15 µg/L	2.15 ppb	2.15 ppb	22:48:34
1	SiO2†	3155.2	1489.0	162.72 µg/L	162.72 ppb	162.72 ppb	22:48:14
1	Si 251.611†	5296.0	4463.0	73.780 µg/L	73.780 ppb	73.780 ppb	22:48:14
1	Sn 189.927†	15.0	12.5	0.8989 µg/L	0.8989 ppb	0.8989 ppb	22:48:34
1	Ti 334.940†	3887.8	3136.5	3.1887 µg/L	3.1887 ppb	3.1887 ppb	22:48:14
1	Tl 190.801†	-113.8	9.9	1.3656 µg/L	1.3656 ppb	1.3656 ppb	22:48:34
1	U 409.014†	-111.4	371.0	22.870 µg/L	22.870 ppb	22.870 ppb	22:48:14
1	V 292.402†	319.1	-122.2	-0.6798 µg/L	-0.6798 ppb	-0.6798 ppb	22:48:14
1	Zn 213.857†	901.1	410.0	2.5658 µg/L	2.5658 ppb	2.5658 ppb	22:48:34
2	Sc RADIAL	153549.1	153549.1	105 %			22:48:02
2	Al 396.153Radial†	416.1	426.9	93.135 µg/L	93.135 ppb	93.135 ppb	22:48:04
2	Ca 317.933Radial†	1354.7	669.7	39.244 µg/L	39.244 ppb	39.244 ppb	22:48:04
2	Fe 238.204 Radial†	2550.7	2307.9	153.44 µg/L	153.44 ppb	153.44 ppb	22:48:04
2	K 766.490 Radial†	1589.8	54.1	22.257 µg/L	22.257 ppb	22.257 ppb	22:48:02
2	Mg 279.077 IEC†	165.4	-29.6	-12.322 µg/L	-12.322 ppb	-12.322 ppb	22:48:04
2	Na 589.592 Radial†	1613.9	-162.8	-24.928 µg/L	-24.928 ppb	-24.928 ppb	22:48:04
2	Sr 421.552†	43.6	319.4	0.7482 µg/L	0.7482 ppb	0.7482 ppb	22:48:04
2	Sc 361.383	1738791.8	1738791.8	103.95 %			22:48:36
2	Y 371.029	1061047.8	1061047.8	103.76 %			22:48:36
2	Ag 328.068†	3212.1	123.1	0.5006 µg/L	0.5006 ppb	0.5006 ppb	22:48:38
2	As 188.979†	-17.9	-3.0	-1.1969 µg/L	-1.1969 ppb	-1.1969 ppb	22:48:58
2	B 249.677†	3168.0	-308.0	-5.1706 µg/L	-5.1706 ppb	-5.1706 ppb	22:48:58
2	Ba 233.527†	241.2	407.1	1.8579 µg/L	1.8579 ppb	1.8579 ppb	22:48:58
2	Be 313.107†	-674.6	11.1	0.0049 µg/L	0.0049 ppb	0.0049 ppb	22:48:38
2	Cd 226.502†	-88.4	9.3	0.0485 µg/L	0.0485 ppb	0.0485 ppb	22:48:58
2	Co 228.616†	-190.5	-6.6	-0.0970 µg/L	-0.0970 ppb	-0.0970 ppb	22:48:58
2	Cr 267.716†	251.2	81.5	0.7009 µg/L	0.7009 ppb	0.7009 ppb	22:48:58
2	Cu 324.752†	2974.1	436.3	1.9222 µg/L	1.9222 ppb	1.9222 ppb	22:48:38
2	Mn 257.610†	2509.4	2334.1	3.1895 µg/L	3.1895 ppb	3.1895 ppb	22:48:58
2	Mo 202.031†	-26.0	30.2	0.9602 µg/L	0.9602 ppb	0.9602 ppb	22:48:58
2	Ni 231.604†	-15.6	25.9	0.3314 µg/L	0.3314 ppb	0.3314 ppb	22:48:58
2	P 214.914†	46.8	-34.6	-8.3885 µg/L	-8.3885 ppb	-8.3885 ppb	22:48:58
2	Pb 220.353†	117.5	0.6	0.0417 µg/L	0.0417 ppb	0.0417 ppb	22:48:58

2	S 181.975 Axial†	115.7	16.5	13.373 µg/L	13.373 ppb	22:48:58
2	Sb 206.836†	76.2	-13.3	-1.7961 µg/L	-1.7961 ppb	22:48:58
2	Se 196.026†	15.8	4.3	1.76 µg/L	1.76 ppb	22:48:58
2	SiO2†	3200.0	1505.6	164.52 µg/L	164.52 ppb	22:48:38
2	Si 251.611†	5193.6	4320.1	71.412 µg/L	71.412 ppb	22:48:38
2	Sn 189.927†	18.2	15.5	1.1142 µg/L	1.1142 ppb	22:48:58
2	Ti 334.940†	4067.7	3276.9	3.3415 µg/L	3.3415 ppb	22:48:38
2	Tl 190.801†	-106.6	17.8	2.4275 µg/L	2.4275 ppb	22:48:58
2	U 409.014†	-425.6	69.7	4.2878 µg/L	4.2878 ppb	22:48:38
2	V 292.402†	429.3	-18.8	-0.1159 µg/L	-0.1159 ppb	22:48:38
2	Zn 213.857†	890.9	392.7	2.4549 µg/L	2.4549 ppb	22:48:58
3	Sc RADIAL	152226.6	152226.6	104 %		22:48:06
3	Al 396.153Radial†	306.6	325.4	70.998 µg/L	70.998 ppb	22:48:08
3	Ca 317.933Radial†	1361.4	687.3	40.274 µg/L	40.274 ppb	22:48:08
3	Fe 238.204 Radial†	2515.4	2295.1	152.59 µg/L	152.59 ppb	22:48:08
3	K 766.490 Radial†	1412.2	-102.8	-42.340 µg/L	-42.340 ppb	22:48:06
3	Mg 279.077 IEC†	219.9	23.9	9.7481 µg/L	9.7481 ppb	22:48:08
3	Na 589.592 Radial†	1622.2	-141.5	-21.620 µg/L	-21.620 ppb	22:48:08
3	Sr 421.552†	108.6	382.0	0.8950 µg/L	0.8950 ppb	22:48:08
3	Sc 361.383	1719221.7	1719221.7	102.78 %		22:49:00
3	Y 371.029	1049311.3	1049311.3	102.61 %		22:49:00
3	Ag 328.068†	3491.4	430.1	1.7468 µg/L	1.7468 ppb	22:49:02
3	As 188.979†	-0.1	14.1	5.9385 µg/L	5.9385 ppb	22:49:22
3	B 249.677†	3156.9	-284.0	-4.7691 µg/L	-4.7691 ppb	22:49:22
3	Ba 233.527†	223.1	392.1	1.7899 µg/L	1.7899 ppb	22:49:22
3	Be 313.107†	-943.9	-258.3	-0.0840 µg/L	-0.0840 ppb	22:49:02
3	Cd 226.502†	-103.4	-6.2	-0.0588 µg/L	-0.0588 ppb	22:49:22
3	Co 228.616†	-172.8	8.5	0.1100 µg/L	0.1100 ppb	22:49:22
3	Cr 267.716†	233.0	66.5	0.5755 µg/L	0.5755 ppb	22:49:22
3	Cu 324.752†	2667.4	170.4	0.7636 µg/L	0.7636 ppb	22:49:02
3	Mn 257.610†	2512.1	2364.2	3.2298 µg/L	3.2298 ppb	22:49:22
3	Mo 202.031†	-27.9	28.0	0.8908 µg/L	0.8908 ppb	22:49:22
3	Ni 231.604†	-49.8	-7.5	-0.0961 µg/L	-0.0961 ppb	22:49:22
3	P 214.914†	36.9	-43.6	-10.536 µg/L	-10.536 ppb	22:49:22
3	Pb 220.353†	92.4	-22.6	-1.3601 µg/L	-1.3601 ppb	22:49:22
3	S 181.975 Axial†	107.0	9.3	7.5567 µg/L	7.5567 ppb	22:49:22
3	Sb 206.836†	78.5	-10.3	-1.3771 µg/L	-1.3771 ppb	22:49:22
3	Se 196.026†	20.3	8.8	3.55 µg/L	3.55 ppb	22:49:22
3	SiO2†	3219.4	1559.5	170.40 µg/L	170.40 ppb	22:49:02
3	Si 251.611†	5299.9	4480.3	74.054 µg/L	74.054 ppb	22:49:02
3	Sn 189.927†	34.9	32.0	2.2845 µg/L	2.2845 ppb	22:49:22
3	Ti 334.940†	4036.6	3291.2	3.3560 µg/L	3.3560 ppb	22:49:02
3	Tl 190.801†	-109.3	14.0	1.9230 µg/L	1.9230 ppb	22:49:22
3	U 409.014†	-489.6	2.7	0.1754 µg/L	0.1754 ppb	22:49:02
3	V 292.402†	511.6	66.0	0.3503 µg/L	0.3503 ppb	22:49:02
3	Zn 213.857†	888.6	400.2	2.5056 µg/L	2.5056 ppb	22:49:22

Mean Data: 1202056877|959114|1

Analyte	Mean Corrected Intensity	Conc.	Calib. Units	Std.Dev.	Sample Conc.	Sample Units	Std.Dev.	RSD
Sc 361.383	1727256.4	103.26	%	0.612				0.59%
Sc RADIAL	153160.8	105	%	0.6				0.53%
Y 371.029	1053999.7	103.07	%	0.608				0.59%
Ag 328.068†	130.1	0.5347	µg/L	1.19545	0.5347	ppb	1.19545	223.56%
Al 396.153Radial†	360.3	78.614	µg/L	12.5802	78.614	ppb	12.5802	16.00%
As 188.979†	3.0	1.3090	µg/L	4.01385	1.3090	ppb	4.01385	306.64%
B 249.677†	-284.5	-4.7767	µg/L	0.39019	-4.7767	ppb	0.39019	8.17%
Ba 233.527†	396.9	1.8112	µg/L	0.04055	1.8112	ppb	0.04055	2.24%
Be 313.107†	-38.0	-0.0096	µg/L	0.06832	-0.0096	ppb	0.06832	711.49%
Ca 317.933Radial†	686.5	40.226	µg/L	0.9578	40.226	ppb	0.9578	2.38%
Cd 226.502†	5.3	0.0204	µg/L	0.06959	0.0204	ppb	0.06959	340.62%
Co 228.616†	6.4	0.0811	µg/L	0.16562	0.0811	ppb	0.16562	204.14%
Cr 267.716†	74.2	0.6349	µg/L	0.06298	0.6349	ppb	0.06298	9.92%
Cu 324.752†	311.7	1.3848	µg/L	0.58383	1.3848	ppb	0.58383	42.16%
Fe 238.204 Radial†	2305.4	153.27	µg/L	0.619	153.27	ppb	0.619	0.40%
K 766.490 Radial†	-50.1	-20.661	µg/L	37.1690	-20.661	ppb	37.1690	179.90%
Mg 279.077 IEC†	8.3	3.3317	µg/L	13.62925	3.3317	ppb	13.62925	409.08%
Mn 257.610†	2344.7	3.2033	µg/L	0.02292	3.2033	ppb	0.02292	0.72%
Mo 202.031†	26.5	0.8441	µg/L	0.14516	0.8441	ppb	0.14516	17.20%
Na 589.592 Radial†	-132.3	-20.225	µg/L	5.5348	-20.225	ppb	5.5348	27.37%

Ni 231.604†	8.2	0.1048 µg/L	0.21490	0.1048 ppb	0.21490	205.10%
P 214.914†	-34.9	-8.4499 µg/L	2.05586	-8.4499 ppb	2.05586	24.33%
Pb 220.353†	-17.5	-1.0584 µg/L	0.98464	-1.0584 ppb	0.98464	93.03%
S 181.975 Axial†	11.7	9.4776 µg/L	3.37359	9.4776 ppb	3.37359	35.60%
Sb 206.836†	-10.5	-1.4209 µg/L	0.35543	-1.4209 ppb	0.35543	25.01%
Se 196.026†	6.1	2.49 µg/L	0.944	2.49 ppb	0.944	37.92%
SiO2†	1518.1	165.88 µg/L	4.016	165.88 ppb	4.016	2.42%
Si 251.611†	4421.1	73.082 µg/L	1.4530	73.082 ppb	1.4530	1.99%
Sn 189.927†	20.0	1.4325 µg/L	0.74564	1.4325 ppb	0.74564	52.05%
Sr 421.552†	339.2	0.7947 µg/L	0.08696	0.7947 ppb	0.08696	10.94%
Ti 334.940†	3234.9	3.2954 µg/L	0.09270	3.2954 ppb	0.09270	2.81%
Tl 190.801†	13.9	1.9054 µg/L	0.53116	1.9054 ppb	0.53116	27.88%
U 409.014†	147.8	9.1110 µg/L	12.09158	9.1110 ppb	12.09158	132.71%
V 292.402†	-25.0	-0.1485 µg/L	0.51584	-0.1485 ppb	0.51584	347.44%
Zn 213.857†	401.0	2.5088 µg/L	0.05553	2.5088 ppb	0.05553	2.21%

Sequence No.: 93

Sample ID: 1202056882|959114|1

Analyst: HSC

Initial Sample Wt:

Dilution:

Autosampler Location: 413

Date Collected: 3/29/2010 22:49:31

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: 1202056882|959114|1

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	156540.3	156540.3	107 %		22:50:03
1	Al 396.153Radial†	504163.3	469456.9	102450 µg/L	102450 ppb	22:50:03
1	Ca 317.933Radial†	1954681.7	1819382.7	106610 µg/L	106610 ppb	22:50:00
1	Fe 238.204 Radial†	3217831.6	2996001.0	199180 µg/L	199180 ppb	22:50:00
1	K 766.490 Radial†	116415.7	106939.4	43977 µg/L	43977 ppb	22:50:03
1	Mg 279.077 IEC†	109432.9	101706.0	41777 µg/L	41777 ppb	22:50:03
1	Na 589.592 Radial†	81140.5	73855.0	11262 µg/L	11262 ppb	22:50:03
1	Sr 421.552†	1193276.2	1111334.3	2603.8 µg/L	2603.8 ppb	22:50:00
1	Sc 361.383	1741650.9	1741650.9	104.12 %		22:50:31
1	Y 371.029	1132485.7	1132485.7	110.75 %		22:50:31
1	Ag 328.068†	86352.2	79970.2	334.99 µg/L	334.99 ppb	22:50:31
1	As 188.979†	3058.9	2952.2	1304.9 µg/L	1304.9 ppb	22:50:33
1	B 249.677†	106142.1	98588.9	1651.7 µg/L	1651.7 ppb	22:50:31
1	Ba 233.527†	484373.9	465393.7	2124.5 µg/L	2124.5 ppb	22:50:31
1	Be 313.107†	2930802.2	2815559.0	916.44 µg/L	916.44 ppb	22:50:31
1	Cd 226.502†	101676.1	97749.6	654.77 µg/L	654.77 ppb	22:50:31
1	Co 228.616†	77188.1	74312.2	1009.6 µg/L	1009.6 ppb	22:50:31
1	Cr 267.716†	319865.5	307055.6	2643.2 µg/L	2643.2 ppb	22:50:31
1	Cu 324.752†	486244.4	464590.2	2050.2 µg/L	2050.2 ppb	22:50:31
1	Mn 257.610†	4428474.7	4253263.5	5809.6 µg/L	5809.6 ppb	22:50:31
1	Mo 202.031†	17301.4	16672.4	535.38 µg/L	535.38 ppb	22:50:33
1	Ni 231.604†	122128.6	117339.8	1500.9 µg/L	1500.9 ppb	22:50:31
1	P 214.914†	36583.9	35057.5	8264.9 µg/L	8264.9 ppb	22:50:33
1	Pb 220.353†	15335.6	14616.7	894.29 µg/L	894.29 ppb	22:50:33
1	S 181.975 Axial†	5332.9	5027.2	4077.4 µg/L	4077.4 ppb	22:50:33
1	Sb 206.836†	9521.4	9058.2	1190.8 µg/L	1190.8 ppb	22:50:33
1	Se 196.026†	7863.7	7541.8	3050 µg/L	3050 ppb	22:50:33
1	SiO2†	898794.5	861677.3	94151 µg/L	94151 ppb	22:50:31
1	Si 251.611†	2750796.7	2641335.6	43660 µg/L	43660 ppb	22:50:31
1	Sn 189.927†	16159.5	15518.5	1123.9 µg/L	1123.9 ppb	22:50:33
1	Ti 334.940†	6270682.0	6022061.5	6139.2 µg/L	6139.2 ppb	22:50:31
1	Tl 190.801†	9214.4	8970.3	1285.6 µg/L	1285.6 ppb	22:50:33
1	U 409.014†	-4404.7	-3751.4	-159.92 µg/L	-159.92 ppb	22:50:31
1	V 292.402†	254866.8	244355.8	1334.7 µg/L	1334.7 ppb	22:50:31
1	Zn 213.857†	1076563.6	1033524.7	6477.5 µg/L	6477.5 ppb	22:50:31
2	Sc RADIAL	158269.8	158269.8	109 %		22:50:07
2	Al 396.153Radial†	508681.2	468487.7	102240 µg/L	102240 ppb	22:50:07
2	Ca 317.933Radial†	1958528.7	1803036.5	105650 µg/L	105650 ppb	22:50:05
2	Fe 238.204 Radial†	3224602.5	2969495.0	197420 µg/L	197420 ppb	22:50:05
2	K 766.490 Radial†	117503.9	106757.0	43902 µg/L	43902 ppb	22:50:07
2	Mg 279.077 IEC†	110482.6	101559.2	41718 µg/L	41718 ppb	22:50:07
2	Na 589.592 Radial†	82008.2	73828.4	11258 µg/L	11258 ppb	22:50:07
2	Sr 421.552†	1197261.3	1102862.6	2584.0 µg/L	2584.0 ppb	22:50:05
2	Sc 361.383	1734836.2	1734836.2	103.71 %		22:50:37
2	Y 371.029	1128802.5	1128802.5	110.39 %		22:50:37
2	Ag 328.068†	86082.3	80035.7	335.28 µg/L	335.28 ppb	22:50:37
2	As 188.979†	3025.4	2931.4	1295.8 µg/L	1295.8 ppb	22:50:39
2	B 249.677†	105687.4	98550.9	1651.0 µg/L	1651.0 ppb	22:50:37
2	Ba 233.527†	482863.9	465765.1	2126.3 µg/L	2126.3 ppb	22:50:37
2	Be 313.107†	2921251.8	2817407.5	917.04 µg/L	917.04 ppb	22:50:37
2	Cd 226.502†	101330.7	97800.1	655.30 µg/L	655.30 ppb	22:50:37
2	Co 228.616†	76942.6	74366.6	1010.4 µg/L	1010.4 ppb	22:50:37
2	Cr 267.716†	318856.4	307289.4	2645.1 µg/L	2645.1 ppb	22:50:37
2	Cu 324.752†	484492.7	464735.7	2050.5 µg/L	2050.5 ppb	22:50:37
2	Mn 257.610†	4410520.4	4252659.2	5808.8 µg/L	5808.8 ppb	22:50:37
2	Mo 202.031†	17294.2	16730.7	537.15 µg/L	537.15 ppb	22:50:39
2	Ni 231.604†	121319.2	117020.1	1496.8 µg/L	1496.8 ppb	22:50:37
2	P 214.914†	36610.6	35221.3	8305.2 µg/L	8305.2 ppb	22:50:39
2	Pb 220.353†	15203.2	14546.9	890.12 µg/L	890.12 ppb	22:50:39

2	S 181.975 Axial†	5339.3	5053.5	4098.7 µg/L	4098.7 ppb	22:50:39
2	Sb 206.836†	9552.1	9123.8	1199.6 µg/L	1199.6 ppb	22:50:39
2	Se 196.026†	7957.3	7661.8	3100 µg/L	3100 ppb	22:50:39
2	SiO2†	895417.6	861812.2	94166 µg/L	94166 ppb	22:50:37
2	Si 251.611†	2740561.0	2641844.3	43668 µg/L	43668 ppb	22:50:37
2	Sn 189.927†	16036.5	15460.8	1119.9 µg/L	1119.9 ppb	22:50:39
2	Ti 334.940†	6252311.0	6028005.6	6145.2 µg/L	6145.2 ppb	22:50:37
2	Tl 190.801†	9228.0	9018.2	1292.1 µg/L	1292.1 ppb	22:50:39
2	U 409.014†	-4412.5	-3775.5	-161.09 µg/L	-161.09 ppb	22:50:37
2	V 292.402†	253787.1	244276.4	1334.6 µg/L	1334.6 ppb	22:50:37
2	Zn 213.857†	1071458.5	1032664.0	6472.3 µg/L	6472.3 ppb	22:50:37
3	Sc RADIAL	153966.6	153966.6	106 %		22:50:11
3	Al 396.153Radial†	495619.1	469215.3	102400 µg/L	102400 ppb	22:50:11
3	Ca 317.933Radial†	1927024.1	1823622.9	106860 µg/L	106860 ppb	22:50:09
3	Fe 238.204 Radial†	3171781.3	3002489.2	199620 µg/L	199620 ppb	22:50:09
3	K 766.490 Radial†	113991.2	106456.0	43778 µg/L	43778 ppb	22:50:11
3	Mg 279.077 IEC†	106515.6	100647.5	41340 µg/L	41340 ppb	22:50:11
3	Na 589.592 Radial†	79720.5	73773.6	11249 µg/L	11249 ppb	22:50:11
3	Sr 421.552†	1180516.8	1117827.5	2619.1 µg/L	2619.1 ppb	22:50:09
3	Sc 361.383	1722456.3	1722456.3	102.97 %		22:50:43
3	Y 371.029	1120682.5	1120682.5	109.59 %		22:50:43
3	Ag 328.068†	85548.8	80114.2	335.60 µg/L	335.60 ppb	22:50:43
3	As 188.979†	3056.3	2982.4	1317.7 µg/L	1317.7 ppb	22:50:45
3	B 249.677†	105167.8	98778.7	1654.8 µg/L	1654.8 ppb	22:50:43
3	Ba 233.527†	479911.5	466244.1	2128.4 µg/L	2128.4 ppb	22:50:43
3	Be 313.107†	2902704.2	2819639.9	917.77 µg/L	917.77 ppb	22:50:43
3	Cd 226.502†	100859.8	98045.1	656.76 µg/L	656.76 ppb	22:50:43
3	Co 228.616†	76505.8	74475.7	1011.8 µg/L	1011.8 ppb	22:50:43
3	Cr 267.716†	317200.6	307891.2	2650.4 µg/L	2650.4 ppb	22:50:43
3	Cu 324.752†	481922.0	465596.8	2054.6 µg/L	2054.6 ppb	22:50:43
3	Mn 257.610†	4390303.2	4263591.1	5823.8 µg/L	5823.8 ppb	22:50:43
3	Mo 202.031†	17355.0	16909.6	542.88 µg/L	542.88 ppb	22:50:45
3	Ni 231.604†	121051.6	117600.9	1504.3 µg/L	1504.3 ppb	22:50:43
3	P 214.914†	36481.1	35349.3	8334.4 µg/L	8334.4 ppb	22:50:45
3	Pb 220.353†	15338.2	14783.4	904.40 µg/L	904.40 ppb	22:50:45
3	S 181.975 Axial†	5432.3	5180.8	4201.9 µg/L	4201.9 ppb	22:50:45
3	Sb 206.836†	9519.1	9157.9	1204.2 µg/L	1204.2 ppb	22:50:45
3	Se 196.026†	8060.2	7816.8	3160 µg/L	3160 ppb	22:50:45
3	SiO2†	890711.6	863447.5	94344 µg/L	94344 ppb	22:50:43
3	Si 251.611†	2725175.7	2645895.5	43735 µg/L	43735 ppb	22:50:43
3	Sn 189.927†	16164.8	15696.5	1136.7 µg/L	1136.7 ppb	22:50:45
3	Ti 334.940†	6219089.5	6039072.3	6156.6 µg/L	6156.6 ppb	22:50:43
3	Tl 190.801†	9201.9	9056.8	1297.4 µg/L	1297.4 ppb	22:50:45
3	U 409.014†	-4231.3	-3630.1	-152.29 µg/L	-152.29 ppb	22:50:43
3	V 292.402†	252539.7	244823.7	1337.3 µg/L	1337.3 ppb	22:50:43
3	Zn 213.857†	1066957.6	1035718.3	6491.2 µg/L	6491.2 ppb	22:50:43

Mean Data: 1202056882|959114|1

Analyte	Mean Corrected Intensity	Conc. Units	Calib.	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1732981.1	103.60 %		0.582			0.56%
Sc RADIAL	156258.9	107 %		1.5			1.39%
Y 371.029	1127323.6	110.24 %		0.591			0.54%
Ag 328.068†	80040.1	335.29 µg/L		0.306	335.29 ppb	0.306	0.09%
Al 396.153Radial†	469053.3	102360 µg/L		110.1	102360 ppb	110.1	0.11%
As 188.979†	2955.3	1306.1 µg/L		10.98	1306.1 ppb	10.98	0.84%
B 249.677†	98639.5	1652.5 µg/L		2.05	1652.5 ppb	2.05	0.12%
Ba 233.527†	465801.0	2126.4 µg/L		1.95	2126.4 ppb	1.95	0.09%
Be 313.107†	2817535.5	917.08 µg/L		0.666	917.08 ppb	0.666	0.07%
Ca 317.933Radial†	1815347.3	106370 µg/L		637.0	106370 ppb	637.0	0.60%
Cd 226.502†	97864.9	655.61 µg/L		1.034	655.61 ppb	1.034	0.16%
Co 228.616†	74384.8	1010.6 µg/L		1.12	1010.6 ppb	1.12	0.11%
Cr 267.716†	307412.1	2646.2 µg/L		3.72	2646.2 ppb	3.72	0.14%
Cu 324.752†	464974.2	2051.8 µg/L		2.46	2051.8 ppb	2.46	0.12%
Fe 238.204 Radial†	2989328.4	198740 µg/L		1162.1	198740 ppb	1162.1	0.58%
K 766.490 Radial†	106717.5	43886 µg/L		100.5	43886 ppb	100.5	0.23%
Mg 279.077 IEC†	101304.2	41611 µg/L		236.9	41611 ppb	236.9	0.57%
Mn 257.610†	4256504.6	5814.1 µg/L		8.40	5814.1 ppb	8.40	0.14%
Mo 202.031†	16770.9	538.47 µg/L		3.919	538.47 ppb	3.919	0.73%
Na 589.592 Radial†	73819.0	11256 µg/L		6.3	11256 ppb	6.3	0.06%

Ni 231.604†	117320.3	1500.7 µg/L	3.72	1500.7 ppb	3.72	0.25%
P 214.914†	35209.4	8301.5 µg/L	34.92	8301.5 ppb	34.92	0.42%
Pb 220.353†	14649.0	896.27 µg/L	7.346	896.27 ppb	7.346	0.82%
S 181.975 Axial†	5087.2	4126.0 µg/L	66.56	4126.0 ppb	66.56	1.61%
Sb 206.836†	9113.3	1198.2 µg/L	6.84	1198.2 ppb	6.84	0.57%
Se 196.026†	7673.5	3100 µg/L	54.6	3100 ppb	54.6	1.76%
SiO2†	862312.3	94220 µg/L	107.5	94220 ppb	107.5	0.11%
Si 251.611†	2643025.1	43688 µg/L	41.2	43688 ppb	41.2	0.09%
Sn 189.927†	15558.6	1126.8 µg/L	8.76	1126.8 ppb	8.76	0.78%
Sr 421.552†	1110674.8	2602.3 µg/L	17.58	2602.3 ppb	17.58	0.68%
Ti 334.940†	6029713.1	6147.0 µg/L	8.82	6147.0 ppb	8.82	0.14%
Tl 190.801†	9015.1	1291.7 µg/L	5.93	1291.7 ppb	5.93	0.46%
U 409.014†	-3719.0	-157.77 µg/L	4.781	-157.77 ppb	4.781	3.03%
Concentration less than lower limit for U 409.014.						
V 292.402†	244485.3	1335.6 µg/L	1.56	1335.6 ppb	1.56	0.12%
Zn 213.857†	1033969.0	6480.3 µg/L	9.79	6480.3 ppb	9.79	0.15%

Sequence No.: 95

Sample ID: 1202056878|959114|1

Analyst: HSC

Initial Sample Wt:

Dilution:

Autosampler Location: 415

Date Collected: 3/29/2010 22:52:58

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: 1202056878|959114|1

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	156991.3	156991.3	108 %		22:53:29
1	Al 396.153Radial†	532899.0	494787.2	108010 µg/L	108010 ppb	22:53:27
1	Ca 317.933Radial†	530327.2	491751.5	28815 µg/L	28815 ppb	22:53:29
1	Fe 238.204 Radial†	2144947.4	1991303.9	132390 µg/L	132390 ppb	22:53:27
1	K 766.490 Radial†	42674.8	38165.3	15680 µg/L	15680 ppb	22:53:29
1	Mg 279.077 IEC†	51630.2	47747.9	19573 µg/L	19573 ppb	22:53:29
1	Na 589.592 Radial†	37188.4	32831.8	5009.7 µg/L	5009.7 ppb	22:53:29
1	Sr 421.552†	124602.5	115961.7	271.56 µg/L	271.56 ppb	22:53:29
1	Sc 361.383	1744488.8	1744488.8	104.29 %		22:53:42
1	Y 371.029	1178717.9	1178717.9	115.27 %		22:53:42
1	Ag 328.068†	3089.8	-4.2	0.1717 µg/L	0.1717 ppb	22:53:44
1	As 188.979†	12.7	26.5	41.592 µg/L	41.592 ppb	22:54:05
1	B 249.677†	4488.9	948.7	15.765 µg/L	15.765 ppb	22:53:44
1	Ba 233.527†	328800.4	315458.8	1439.6 µg/L	1439.6 ppb	22:53:44
1	Be 313.107†	45578.9	44365.3	14.356 µg/L	14.356 ppb	22:53:44
1	Cd 226.502†	1950.1	1964.3	-0.3216 µg/L	-0.3216 ppb	22:54:05
1	Co 228.616†	3364.9	3403.2	41.122 µg/L	41.122 ppb	22:54:05
1	Cr 267.716†	10916.0	10307.0	92.621 µg/L	92.621 ppb	22:54:05
1	Cu 324.752†	12208.4	9281.6	59.954 µg/L	59.954 ppb	22:53:44
1	Mn 257.610†	1792884.9	1719101.1	2347.9 µg/L	2347.9 ppb	22:53:42
1	Mo 202.031†	-139.9	-78.9	3.1825 µg/L	3.1825 ppb	22:54:05
1	Ni 231.604†	6079.7	5870.7	75.093 µg/L	75.093 ppb	22:54:05
1	P 214.914†	6946.3	6581.1	1509.5 µg/L	1509.5 ppb	22:54:05
1	Pb 220.353†	1358.8	1190.5	80.705 µg/L	80.705 ppb	22:54:05
1	S 181.975 Axial†	1610.0	1449.0	1174.0 µg/L	1174.0 ppb	22:54:05
1	Sb 206.836†	70.3	-19.2	-5.9710 µg/L	-5.9710 ppb	22:54:05
1	Se 196.026†	-112.1	-118.4	-1.19 µg/L	-1.19 ppb	22:54:05
1	SiO2†	867750.3	830505.0	90775 µg/L	90775 ppb	22:53:42
1	Si 251.611†	2654987.2	2545166.7	42084 µg/L	42084 ppb	22:53:42
1	Sn 189.927†	-12.4	-13.9	14.209 µg/L	14.209 ppb	22:54:05
1	Ti 334.940†	4610505.7	4420335.7	4506.6 µg/L	4506.6 ppb	22:53:42
1	Tl 190.801†	-529.6	-387.5	0.7915 µg/L	0.7915 ppb	22:54:05
1	U 409.014†	-5273.6	-4577.7	-283.26 µg/L	-283.26 ppb	22:53:44
1	V 292.402†	44064.5	41821.2	206.92 µg/L	206.92 ppb	22:53:44
1	Zn 213.857†	48938.0	46461.8	281.90 µg/L	281.90 ppb	22:53:44
2	Sc RADIAL	155773.1	155773.1	107 %		22:53:34
2	Al 396.153Radial†	535983.8	501542.9	109480 µg/L	109480 ppb	22:53:32
2	Ca 317.933Radial†	524186.5	489856.3	28703 µg/L	28703 ppb	22:53:34
2	Fe 238.204 Radial†	2152406.2	2013856.9	133890 µg/L	133890 ppb	22:53:32
2	K 766.490 Radial†	42324.5	38147.4	15672 µg/L	15672 ppb	22:53:34
2	Mg 279.077 IEC†	51103.8	47630.3	19524 µg/L	19524 ppb	22:53:34
2	Na 589.592 Radial†	36850.1	32785.3	5002.6 µg/L	5002.6 ppb	22:53:34
2	Sr 421.552†	123342.0	115687.0	270.92 µg/L	270.92 ppb	22:53:34
2	Sc 361.383	1734462.5	1734462.5	103.69 %		22:54:07
2	Y 371.029	1171047.6	1171047.6	114.52 %		22:54:07
2	Ag 328.068†	3159.7	80.3	0.5298 µg/L	0.5298 ppb	22:54:09
2	As 188.979†	24.1	37.5	46.559 µg/L	46.559 ppb	22:54:30
2	B 249.677†	4440.3	926.7	15.395 µg/L	15.395 ppb	22:54:09
2	Ba 233.527†	332095.2	320459.0	1462.4 µg/L	1462.4 ppb	22:54:09
2	Be 313.107†	46201.1	45218.0	14.630 µg/L	14.630 ppb	22:54:09
2	Cd 226.502†	1972.9	1997.1	-0.2525 µg/L	-0.2525 ppb	22:54:30
2	Co 228.616†	3372.3	3429.0	41.419 µg/L	41.419 ppb	22:54:30
2	Cr 267.716†	10955.1	10405.3	93.532 µg/L	93.532 ppb	22:54:30
2	Cu 324.752†	12370.0	9505.2	61.132 µg/L	61.132 ppb	22:54:09
2	Mn 257.610†	1772924.2	1709788.3	2335.2 µg/L	2335.2 ppb	22:54:07
2	Mo 202.031†	-142.1	-81.8	3.1502 µg/L	3.1502 ppb	22:54:30
2	Ni 231.604†	6077.3	5902.1	75.494 µg/L	75.494 ppb	22:54:30
2	P 214.914†	6933.6	6607.4	1515.1 µg/L	1515.1 ppb	22:54:30
2	Pb 220.353†	1397.7	1235.5	83.456 µg/L	83.456 ppb	22:54:30

2	S 181.975 Axial†	1606.9	1454.9	1178.7 µg/L	1178.7 ppb	22:54:30
2	Sb 206.836†	57.2	-31.5	-7.6633 µg/L	-7.6633 ppb	22:54:30
2	Se 196.026†	-97.9	-105.3	4.51 µg/L	4.51 ppb	22:54:30
2	SiO2†	858618.2	826507.7	90338 µg/L	90338 ppb	22:54:07
2	Si 251.611†	2624768.6	2530739.5	41845 µg/L	41845 ppb	22:54:07
2	Sn 189.927†	-7.0	-8.8	14.496 µg/L	14.496 ppb	22:54:30
2	Ti 334.940†	4560443.3	4397609.9	4483.4 µg/L	4483.4 ppb	22:54:07
2	Tl 190.801†	-543.1	-403.5	-1.5963 µg/L	-1.5963 ppb	22:54:30
2	U 409.014†	-5470.0	-4796.4	-297.03 µg/L	-297.03 ppb	22:54:09
2	V 292.402†	44356.7	42347.3	209.62 µg/L	209.62 ppb	22:54:09
2	Zn 213.857†	49319.1	47100.6	285.77 µg/L	285.77 ppb	22:54:09
3	Sc RADIAL	156720.5	156720.5	108 %		22:53:38
3	Al 396.153Radial†	532203.2	494994.8	108050 µg/L	108050 ppb	22:53:36
3	Ca 317.933Radial†	528226.0	490647.8	28750 µg/L	28750 ppb	22:53:38
3	Fe 238.204 Radial†	2141313.1	1991364.0	132390 µg/L	132390 ppb	22:53:36
3	K 766.490 Radial†	42807.8	38357.3	15759 µg/L	15759 ppb	22:53:38
3	Mg 279.077 IEC†	51381.3	47599.2	19512 µg/L	19512 ppb	22:53:38
3	Na 589.592 Radial†	37112.5	32820.9	5008.0 µg/L	5008.0 ppb	22:53:38
3	Sr 421.552†	124421.7	115993.4	271.63 µg/L	271.63 ppb	22:53:38
3	Sc 361.383	1745300.5	1745300.5	104.34 %		22:54:32
3	Y 371.029	1179003.4	1179003.4	115.30 %		22:54:32
3	Ag 328.068†	3160.1	61.7	0.4039 µg/L	0.4039 ppb	22:54:34
3	As 188.979†	13.3	27.0	41.806 µg/L	41.806 ppb	22:54:55
3	B 249.677†	4264.9	732.0	12.128 µg/L	12.128 ppb	22:54:34
3	Ba 233.527†	326901.4	313492.1	1430.6 µg/L	1430.6 ppb	22:54:34
3	Be 313.107†	45420.3	44192.9	14.296 µg/L	14.296 ppb	22:54:34
3	Cd 226.502†	1943.3	1957.0	-0.3727 µg/L	-0.3727 ppb	22:54:55
3	Co 228.616†	3360.2	3397.2	41.031 µg/L	41.031 ppb	22:54:55
3	Cr 267.716†	10862.6	10251.0	92.152 µg/L	92.152 ppb	22:54:55
3	Cu 324.752†	12062.4	9136.3	59.310 µg/L	59.310 ppb	22:54:34
3	Mn 257.610†	1788465.5	1714065.8	2341.0 µg/L	2341.0 ppb	22:54:32
3	Mo 202.031†	-142.3	-81.1	3.1101 µg/L	3.1101 ppb	22:54:55
3	Ni 231.604†	6052.8	5842.2	74.728 µg/L	74.728 ppb	22:54:55
3	P 214.914†	6869.0	6504.0	1491.1 µg/L	1491.1 ppb	22:54:55
3	Pb 220.353†	1336.6	1168.7	79.382 µg/L	79.382 ppb	22:54:55
3	S 181.975 Axial†	1597.1	1435.9	1163.3 µg/L	1163.3 ppb	22:54:55
3	Sb 206.836†	69.3	-20.2	-6.1029 µg/L	-6.1029 ppb	22:54:55
3	Se 196.026†	-104.5	-111.0	1.72 µg/L	1.72 ppb	22:54:55
3	SiO2†	865855.2	828301.8	90534 µg/L	90534 ppb	22:54:32
3	Si 251.611†	2649633.4	2538851.5	41980 µg/L	41980 ppb	22:54:32
3	Sn 189.927†	-8.3	-10.0	14.456 µg/L	14.456 ppb	22:54:55
3	Ti 334.940†	4601891.0	4410023.0	4496.1 µg/L	4496.1 ppb	22:54:32
3	Tl 190.801†	-537.6	-395.0	-0.3477 µg/L	-0.3477 ppb	22:54:55
3	U 409.014†	-5501.7	-4794.0	-296.78 µg/L	-296.78 ppb	22:54:34
3	V 292.402†	43728.7	41479.7	205.03 µg/L	205.03 ppb	22:54:34
3	Zn 213.857†	48489.9	46010.5	279.05 µg/L	279.05 ppb	22:54:34

Mean Data: 1202056878|959114|1

Analyte	Mean Corrected Intensity	Conc. Units	Calib. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1741417.2	104.10 %		0.361			0.35%
Sc RADIAL	156495.0	107 %		0.4			0.41%
Y 371.029	1176256.3	115.03 %		0.441			0.38%
Ag 328.068†	45.9	0.3685 µg/L		0.18165	0.3685 ppb	0.18165	49.30%
Al 396.153Radial†	497108.3	108510 µg/L		838.6	108510 ppb	838.6	0.77%
As 188.979†	30.3	43.319 µg/L		2.8076	43.319 ppb	2.8076	6.48%
B 249.677†	869.1	14.429 µg/L		2.0015	14.429 ppb	2.0015	13.87%
Ba 233.527†	316469.9	1444.2 µg/L		16.40	1444.2 ppb	16.40	1.14%
Be 313.107†	44592.1	14.427 µg/L		0.1778	14.427 ppb	0.1778	1.23%
Ca 317.933Radial†	490751.9	28756 µg/L		55.8	28756 ppb	55.8	0.19%
Cd 226.502†	1972.8	-0.3156 µg/L		0.06034	-0.3156 ppb	0.06034	19.12%
Co 228.616†	3409.8	41.190 µg/L		0.2033	41.190 ppb	0.2033	0.49%
Cr 267.716†	10321.1	92.768 µg/L		0.7020	92.768 ppb	0.7020	0.76%
Cu 324.752†	9307.7	60.132 µg/L		0.9240	60.132 ppb	0.9240	1.54%
Fe 238.204 Radial†	1998841.6	132890 µg/L		864.5	132890 ppb	864.5	0.65%
K 766.490 Radial†	38223.3	15704 µg/L		48.0	15704 ppb	48.0	0.31%
Mg 279.077 IEC†	47659.2	19536 µg/L		32.6	19536 ppb	32.6	0.17%
Mn 257.610†	1714318.4	2341.4 µg/L		6.37	2341.4 ppb	6.37	0.27%
Mo 202.031†	-80.6	3.1476 µg/L		0.03623	3.1476 ppb	0.03623	1.15%
Na 589.592 Radial†	32812.7	5006.8 µg/L		3.71	5006.8 ppb	3.71	0.07%

Ni 231.604†	5871.7	75.105 µg/L	0.3830	75.105 ppb	0.3830	0.51%
P 214.914†	6564.2	1505.2 µg/L	12.58	1505.2 ppb	12.58	0.84%
Pb 220.353†	1198.2	81.181 µg/L	2.0781	81.181 ppb	2.0781	2.56%
S 181.975 Axial†	1446.6	1172.0 µg/L	7.88	1172.0 ppb	7.88	0.67%
Sb 206.836†	-23.6	-6.5790 µg/L	0.94128	-6.5790 ppb	0.94128	14.31%
Se 196.026†	-111.6	1.68 µg/L	2.853	1.68 ppb	2.853	169.61%
SiO2†	828438.2	90549 µg/L	218.8	90549 ppb	218.8	0.24%
Si 251.611†	2538252.6	41970 µg/L	119.6	41970 ppb	119.6	0.28%
Sn 189.927†	-10.9	14.387 µg/L	0.1557	14.387 ppb	0.1557	1.08%
Sr 421.552†	115880.7	271.37 µg/L	0.395	271.37 ppb	0.395	0.15%
Ti 334.940†	4409322.9	4495.4 µg/L	11.60	4495.4 ppb	11.60	0.26%
Tl 190.801†	-395.3	-0.3842 µg/L	1.19432	-0.3842 ppb	1.19432	310.89%
U 409.014†	-4722.7	-292.35 µg/L	7.881	-292.35 ppb	7.881	2.70%
Concentration less than lower limit for U 409.014.						
V 292.402†	41882.7	207.19 µg/L	2.308	207.19 ppb	2.308	1.11%
Zn 213.857†	46524.3	282.24 µg/L	3.371	282.24 ppb	3.371	1.19%

Sequence No.: 96

Sample ID: 1202056880|959114|1

Analyst: HSC

Initial Sample Wt:

Dilution:

Autosampler Location: 416

Date Collected: 3/29/2010 22:55:03

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: 1202056880|959114|1

Repl#	Analyte	Net Intensity	Corrected Intensity	Conc. Units	Calib. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	152274.7	152274.7	104 %			22:55:34
1	Al 396.153Radial†	855266.5	818675.2	178690 µg/L		178690 ppb	22:55:32
1	Ca 317.933Radial†	656361.3	627639.2	36777 µg/L		36777 ppb	22:55:34
1	Fe 238.204 Radial†	2445145.4	2340329.1	155590 µg/L		155590 ppb	22:55:32
1	K 766.490 Radial†	61389.6	57305.8	23541 µg/L		23541 ppb	22:55:34
1	Mg 279.077 IEC†	72525.0	69232.8	28423 µg/L		28423 ppb	22:55:34
1	Na 589.592 Radial†	68335.9	63715.0	9728.2 µg/L		9728.2 ppb	22:55:34
1	Sr 421.552†	333993.6	319969.7	749.64 µg/L		749.64 ppb	22:55:34
1	Sc 361.383	1719268.3	1719268.3	102.78 %			22:55:49
1	Y 371.029	1161275.3	1161275.3	113.56 %			22:55:49
1	Ag 328.068†	111760.2	105770.9	435.44 µg/L		435.44 ppb	22:55:49
1	As 188.979†	1210.9	1192.4	539.99 µg/L		539.99 ppb	22:55:51
1	B 249.677†	30893.7	26702.6	446.67 µg/L		446.67 ppb	22:55:49
1	Ba 233.527†	457093.7	444907.6	2031.1 µg/L		2031.1 ppb	22:55:49
1	Be 313.107†	1507001.6	1466908.1	477.54 µg/L		477.54 ppb	22:55:49
1	Cd 226.502†	64719.7	63063.9	419.38 µg/L		419.38 ppb	22:55:49
1	Co 228.616†	35019.7	34249.3	462.91 µg/L		462.91 ppb	22:55:51
1	Cr 267.716†	70355.3	68292.5	591.14 µg/L		591.14 ppb	22:55:49
1	Cu 324.752†	135786.8	129689.8	587.59 µg/L		587.59 ppb	22:55:49
1	Mn 257.610†	2215486.3	2155493.3	2943.8 µg/L		2943.8 ppb	22:55:49
1	Mo 202.031†	14341.0	14008.4	449.11 µg/L		449.11 ppb	22:55:51
1	Ni 231.604†	45190.9	44009.7	562.94 µg/L		562.94 ppb	22:55:51
1	P 214.914†	9675.7	9334.5	2162.5 µg/L		2162.5 ppb	22:55:51
1	Pb 220.353†	8418.6	8078.5	503.96 µg/L		503.96 ppb	22:55:51
1	S 181.975 Axial†	7712.4	7409.0	6006.4 µg/L		6006.4 ppb	22:55:51
1	Sb 206.836†	2363.2	2212.7	294.77 µg/L		294.77 ppb	22:55:51
1	Se 196.026†	1111.0	1070.0	477 µg/L		477 ppb	22:55:51
1	SiO2†	913975.7	887686.4	97005 µg/L		97005 ppb	22:55:49
1	Si 251.611†	2795508.2	2719233.4	44953 µg/L		44953 ppb	22:55:49
1	Sn 189.927†	6784.3	6598.8	488.64 µg/L		488.64 ppb	22:55:51
1	Ti 334.940†	5834213.4	5675803.4	5785.9 µg/L		5785.9 ppb	22:55:49
1	Tl 190.801†	2934.4	2975.4	468.16 µg/L		468.16 ppb	22:55:51
1	U 409.014†	1750.1	2181.8	161.71 µg/L		161.71 ppb	22:55:49
1	V 292.402†	136559.8	132435.0	711.71 µg/L		711.71 ppb	22:55:49
1	Zn 213.857†	132628.6	128577.6	794.51 µg/L		794.51 ppb	22:55:49
2	Sc RADIAL	152809.6	152809.6	105 %			22:55:39
2	Al 396.153Radial†	853420.6	814049.2	177680 µg/L		177680 ppb	22:55:37
2	Ca 317.933Radial†	662541.6	631335.2	36994 µg/L		36994 ppb	22:55:39
2	Fe 238.204 Radial†	2434549.1	2322030.4	154380 µg/L		154380 ppb	22:55:37
2	K 766.490 Radial†	61752.2	57446.0	23599 µg/L		23599 ppb	22:55:39
2	Mg 279.077 IEC†	73214.3	69647.2	28595 µg/L		28595 ppb	22:55:39
2	Na 589.592 Radial†	68870.0	63995.5	9771.1 µg/L		9771.1 ppb	22:55:39
2	Sr 421.552†	337539.9	322233.4	754.94 µg/L		754.94 ppb	22:55:39
2	Sc 361.383	1750707.9	1750707.9	104.66 %			22:55:55
2	Y 371.029	1180983.6	1180983.6	115.49 %			22:55:55
2	Ag 328.068†	114066.1	106021.3	436.45 µg/L		436.45 ppb	22:55:55
2	As 188.979†	1239.3	1198.4	542.26 µg/L		542.26 ppb	22:55:57
2	B 249.677†	31559.2	26798.6	448.29 µg/L		448.29 ppb	22:55:55
2	Ba 233.527†	467203.3	446580.7	2038.7 µg/L		2038.7 ppb	22:55:55
2	Be 313.107†	1543276.9	1475237.5	480.25 µg/L		480.25 ppb	22:55:55
2	Cd 226.502†	66445.9	63582.5	423.09 µg/L		423.09 ppb	22:55:55
2	Co 228.616†	35571.9	34165.0	461.82 µg/L		461.82 ppb	22:55:57
2	Cr 267.716†	72017.6	68651.4	594.18 µg/L		594.18 ppb	22:55:55
2	Cu 324.752†	138957.3	130346.7	590.27 µg/L		590.27 ppb	22:55:55
2	Mn 257.610†	2264005.5	2163142.5	2954.3 µg/L		2954.3 ppb	22:55:55
2	Mo 202.031†	14562.1	13969.1	447.83 µg/L		447.83 ppb	22:55:57
2	Ni 231.604†	45792.2	43794.6	560.18 µg/L		560.18 ppb	22:55:57
2	P 214.914†	9866.4	9347.6	2166.2 µg/L		2166.2 ppb	22:55:57
2	Pb 220.353†	8550.1	8057.0	502.66 µg/L		502.66 ppb	22:55:57

2	S 181.975 Axial†	7907.4	7460.6	6048.2 µg/L	6048.2 ppb	22:55:57
2	Sb 206.836†	2439.9	2244.6	299.04 µg/L	299.04 ppb	22:55:57
2	Se 196.026†	1094.5	1034.8	463 µg/L	463 ppb	22:55:57
2	SiO2†	933993.9	890843.9	97351 µg/L	97351 ppb	22:55:55
2	Si 251.611†	2857650.7	2729765.0	45127 µg/L	45127 ppb	22:55:55
2	Sn 189.927†	6888.6	6579.9	487.35 µg/L	487.35 ppb	22:55:57
2	Ti 334.940†	5958897.9	5692999.1	5803.4 µg/L	5803.4 ppb	22:55:55
2	Tl 190.801†	3001.5	2988.2	470.10 µg/L	470.10 ppb	22:55:57
2	U 409.014†	1686.6	2090.6	156.45 µg/L	156.45 ppb	22:55:55
2	V 292.402†	139128.2	132503.0	712.26 µg/L	712.26 ppb	22:55:55
2	Zn 213.857†	135549.2	129050.8	797.62 µg/L	797.62 ppb	22:55:55
3	Sc RADIAL	153791.6	153791.6	106 %		22:55:43
3	Al 396.153Radial†	859718.8	814820.6	177840 µg/L	177840 ppb	22:55:41
3	Ca 317.933Radial†	663973.6	628657.2	36837 µg/L	36837 ppb	22:55:43
3	Fe 238.204 Radial†	2452785.3	2324486.1	154540 µg/L	154540 ppb	22:55:41
3	K 766.490 Radial†	61857.6	57169.9	23485 µg/L	23485 ppb	22:55:43
3	Mg 279.077 IEC†	73456.4	69430.8	28505 µg/L	28505 ppb	22:55:43
3	Na 589.592 Radial†	69130.5	63822.9	9744.8 µg/L	9744.8 ppb	22:55:43
3	Sr 421.552†	337787.3	320412.0	750.67 µg/L	750.67 ppb	22:55:43
3	Sc 361.383	1728119.0	1728119.0	103.31 %		22:56:01
3	Y 371.029	1166957.9	1166957.9	114.12 %		22:56:01
3	Ag 328.068†	112660.7	106085.6	436.71 µg/L	436.71 ppb	22:56:01
3	As 188.979†	1237.6	1212.2	548.07 µg/L	548.07 ppb	22:56:03
3	B 249.677†	31172.1	26818.1	448.62 µg/L	448.62 ppb	22:56:01
3	Ba 233.527†	460447.4	445876.2	2035.5 µg/L	2035.5 ppb	22:56:01
3	Be 313.107†	1521944.3	1473862.8	479.80 µg/L	479.80 ppb	22:56:01
3	Cd 226.502†	65582.0	63576.1	423.03 µg/L	423.03 ppb	22:56:01
3	Co 228.616†	35019.7	34074.7	460.58 µg/L	460.58 ppb	22:56:03
3	Cr 267.716†	71032.3	68597.2	593.73 µg/L	593.73 ppb	22:56:01
3	Cu 324.752†	137027.1	130213.8	589.70 µg/L	589.70 ppb	22:56:01
3	Mn 257.610†	2233191.2	2161591.3	2952.1 µg/L	2952.1 ppb	22:56:01
3	Mo 202.031†	14528.4	14118.4	452.54 µg/L	452.54 ppb	22:56:03
3	Ni 231.604†	45078.7	43675.9	558.67 µg/L	558.67 ppb	22:56:03
3	P 214.914†	9678.4	9288.9	2152.0 µg/L	2152.0 ppb	22:56:03
3	Pb 220.353†	8431.8	8049.3	502.21 µg/L	502.21 ppb	22:56:03
3	S 181.975 Axial†	7812.3	7467.3	6053.6 µg/L	6053.6 ppb	22:56:03
3	Sb 206.836†	2431.3	2266.8	302.10 µg/L	302.10 ppb	22:56:03
3	Se 196.026†	1040.0	995.8	448 µg/L	448 ppb	22:56:03
3	SiO2†	920640.3	889583.1	97213 µg/L	97213 ppb	22:56:01
3	Si 251.611†	2817190.4	2726291.0	45070 µg/L	45070 ppb	22:56:01
3	Sn 189.927†	6742.2	6524.2	483.39 µg/L	483.39 ppb	22:56:03
3	Ti 334.940†	5880893.9	5691916.7	5802.3 µg/L	5802.3 ppb	22:56:01
3	Tl 190.801†	2925.2	2951.8	465.21 µg/L	465.21 ppb	22:56:03
3	U 409.014†	1530.1	1960.2	148.34 µg/L	148.34 ppb	22:56:01
3	V 292.402†	137356.7	132525.9	712.40 µg/L	712.40 ppb	22:56:01
3	Zn 213.857†	133661.9	128916.9	796.78 µg/L	796.78 ppb	22:56:01

Mean Data: 1202056880|959114|1

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1732698.4	103.58 %	0.969			0.94%
Sc RADIAL	152958.6	105 %	0.5			0.50%
Y 371.029	1169739.0	114.39 %	0.992			0.87%
Ag 328.068†	105959.3	436.20 µg/L	0.671	436.20 ppb	0.671	0.15%
Al 396.153Radial†	815848.3	178070 µg/L	541.0	178070 ppb	541.0	0.30%
As 188.979†	1201.0	543.44 µg/L	4.163	543.44 ppb	4.163	0.77%
B 249.677†	26773.1	447.86 µg/L	1.042	447.86 ppb	1.042	0.23%
Ba 233.527†	445788.2	2035.1 µg/L	3.85	2035.1 ppb	3.85	0.19%
Be 313.107†	1472002.8	479.20 µg/L	1.452	479.20 ppb	1.452	0.30%
Ca 317.933Radial†	629210.5	36869 µg/L	111.9	36869 ppb	111.9	0.30%
Cd 226.502†	63407.5	421.84 µg/L	2.123	421.84 ppb	2.123	0.50%
Co 228.616†	34163.0	461.77 µg/L	1.166	461.77 ppb	1.166	0.25%
Cr 267.716†	68513.7	593.01 µg/L	1.641	593.01 ppb	1.641	0.28%
Cu 324.752†	130083.5	589.19 µg/L	1.412	589.19 ppb	1.412	0.24%
Fe 238.204 Radial†	2328948.5	154840 µg/L	660.3	154840 ppb	660.3	0.43%
K 766.490 Radial†	57307.2	23542 µg/L	56.8	23542 ppb	56.8	0.24%
Mg 279.077 IEC†	69436.9	28508 µg/L	86.0	28508 ppb	86.0	0.30%
Mn 257.610†	2160075.7	2950.1 µg/L	5.52	2950.1 ppb	5.52	0.19%
Mo 202.031†	14031.9	449.83 µg/L	2.438	449.83 ppb	2.438	0.54%
Na 589.592 Radial†	63844.5	9748.0 µg/L	21.62	9748.0 ppb	21.62	0.22%

Ni 231.604†	43826.7	560.59 µg/L	2.164	560.59 ppb	2.164	0.39%
P 214.914†	9323.6	2160.2 µg/L	7.38	2160.2 ppb	7.38	0.34%
Pb 220.353†	8061.6	502.94 µg/L	0.907	502.94 ppb	0.907	0.18%
S 181.975 Axial†	7445.6	6036.1 µg/L	25.85	6036.1 ppb	25.85	0.43%
Sb 206.836†	2241.4	298.64 µg/L	3.680	298.64 ppb	3.680	1.23%
Se 196.026†	1033.5	463 µg/L	14.9	463 ppb	14.9	3.22%
SiO2†	889371.1	97190 µg/L	173.7	97190 ppb	173.7	0.18%
Si 251.611†	2725096.5	45050 µg/L	88.7	45050 ppb	88.7	0.20%
Sn 189.927†	6567.6	486.46 µg/L	2.736	486.46 ppb	2.736	0.56%
Sr 421.552†	320871.7	751.75 µg/L	2.811	751.75 ppb	2.811	0.37%
Ti 334.940†	5686906.4	5797.2 µg/L	9.82	5797.2 ppb	9.82	0.17%
Tl 190.801†	2971.8	467.83 µg/L	2.465	467.83 ppb	2.465	0.53%
U 409.014†	2077.5	155.50 µg/L	6.738	155.50 ppb	6.738	4.33%
V 292.402†	132488.0	712.13 µg/L	0.366	712.13 ppb	0.366	0.05%
Zn 213.857†	128848.4	796.30 µg/L	1.610	796.30 ppb	1.610	0.20%

Sequence No.: 97

Sample ID: 1202056881|959114|1

Analyst: HSC

Initial Sample Wt:

Dilution:

Autosampler Location: 417

Date Collected: 3/29/2010 22:56:11

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: 1202056881|959114|1

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	153962.4	153962.4	106 %		22:56:43
1	Al 396.153Radial†	901543.0	853511.2	186290 µg/L	186290 ppb	22:56:40
1	Ca 317.933Radial†	639676.3	604957.2	35448 µg/L	35448 ppb	22:56:43
1	Fe 238.204 Radial†	2322942.0	2198986.5	146200 µg/L	146200 ppb	22:56:40
1	K 766.490 Radial†	62053.2	57290.0	23533 µg/L	23533 ppb	22:56:43
1	Mg 279.077 IEC†	73981.9	69851.1	28686 µg/L	28686 ppb	22:56:43
1	Na 589.592 Radial†	71197.8	65707.3	10033 µg/L	10033 ppb	22:56:43
1	Sr 421.552†	342567.7	324582.5	760.46 µg/L	760.46 ppb	22:56:43
1	Sc 361.383	1711574.5	1711574.5	102.32 %		22:56:57
1	Y 371.029	1144656.2	1144656.2	111.94 %		22:56:57
1	Ag 328.068†	113743.7	108198.2	445.27 µg/L	445.27 ppb	22:56:57
1	As 188.979†	1230.3	1216.7	548.08 µg/L	548.08 ppb	22:56:59
1	B 249.677†	31201.1	27138.2	453.92 µg/L	453.92 ppb	22:56:57
1	Ba 233.527†	456543.6	446369.1	2037.9 µg/L	2037.9 ppb	22:56:57
1	Be 313.107†	1532299.4	1498223.5	487.74 µg/L	487.74 ppb	22:56:57
1	Cd 226.502†	65553.9	64162.2	427.96 µg/L	427.96 ppb	22:56:57
1	Co 228.616†	36219.6	35575.1	481.55 µg/L	481.55 ppb	22:56:59
1	Cr 267.716†	70082.7	68333.7	591.08 µg/L	591.08 ppb	22:56:57
1	Cu 324.752†	137256.7	131720.3	595.08 µg/L	595.08 ppb	22:56:57
1	Mn 257.610†	2396999.8	2342581.7	3199.5 µg/L	3199.5 ppb	22:56:57
1	Mo 202.031†	14574.1	14298.9	457.92 µg/L	457.92 ppb	22:56:59
1	Ni 231.604†	45983.2	44981.7	575.37 µg/L	575.37 ppb	22:56:59
1	P 214.914†	9734.9	9434.7	2194.4 µg/L	2194.4 ppb	22:56:59
1	Pb 220.353†	8734.2	8423.7	525.55 µg/L	525.55 ppb	22:56:59
1	S 181.975 Axial†	7916.1	7641.8	6195.1 µg/L	6195.1 ppb	22:56:59
1	Sb 206.836†	2408.8	2267.6	302.37 µg/L	302.37 ppb	22:56:59
1	Se 196.026†	1107.6	1071.6	475 µg/L	475 ppb	22:56:59
1	SiO2†	950355.6	927239.0	101330 µg/L	101330 ppb	22:56:57
1	Si 251.611†	2906780.9	2840210.0	46953 µg/L	46953 ppb	22:56:57
1	Sn 189.927†	6812.4	6656.0	492.45 µg/L	492.45 ppb	22:56:59
1	Ti 334.940†	5732918.0	5602390.9	5710.9 µg/L	5710.9 ppb	22:56:57
1	Tl 190.801†	3041.8	3032.1	483.75 µg/L	483.75 ppb	22:56:59
1	U 409.014†	2085.8	2517.6	185.90 µg/L	185.90 ppb	22:56:57
1	V 292.402†	134985.7	131493.8	708.16 µg/L	708.16 ppb	22:56:57
1	Zn 213.857†	128602.5	125222.7	774.37 µg/L	774.37 ppb	22:56:57
2	Sc RADIAL	154224.9	154224.9	106 %		22:56:47
2	Al 396.153Radial†	899833.7	850442.9	185620 µg/L	185620 ppb	22:56:45
2	Ca 317.933Radial†	643817.4	607840.1	35617 µg/L	35617 ppb	22:56:47
2	Fe 238.204 Radial†	2307774.4	2180908.5	144990 µg/L	144990 ppb	22:56:45
2	K 766.490 Radial†	62735.8	57835.1	23758 µg/L	23758 ppb	22:56:47
2	Mg 279.077 IEC†	74687.3	70398.5	28913 µg/L	28913 ppb	22:56:47
2	Na 589.592 Radial†	71674.7	66043.3	10084 µg/L	10084 ppb	22:56:47
2	Sr 421.552†	343448.0	324862.4	761.11 µg/L	761.11 ppb	22:56:47
2	Sc 361.383	1727648.1	1727648.1	103.28 %		22:57:03
2	Y 371.029	1154511.5	1154511.5	112.90 %		22:57:03
2	Ag 328.068†	114185.8	107592.0	442.82 µg/L	442.82 ppb	22:57:03
2	As 188.979†	1221.4	1196.8	539.48 µg/L	539.48 ppb	22:57:05
2	B 249.677†	31498.2	27142.1	454.02 µg/L	454.02 ppb	22:57:03
2	Ba 233.527†	460200.0	445758.2	2035.1 µg/L	2035.1 ppb	22:57:03
2	Be 313.107†	1545668.3	1497234.9	487.42 µg/L	487.42 ppb	22:57:03
2	Cd 226.502†	66242.8	64233.2	428.57 µg/L	428.57 ppb	22:57:03
2	Co 228.616†	35885.5	34922.3	472.68 µg/L	472.68 ppb	22:57:05
2	Cr 267.716†	70754.4	68346.9	591.15 µg/L	591.15 ppb	22:57:03
2	Cu 324.752†	138117.3	131305.5	593.10 µg/L	593.10 ppb	22:57:03
2	Mn 257.610†	2415429.4	2338630.4	3194.1 µg/L	3194.1 ppb	22:57:03
2	Mo 202.031†	14353.6	13952.9	446.95 µg/L	446.95 ppb	22:57:05
2	Ni 231.604†	45168.2	43774.4	559.93 µg/L	559.93 ppb	22:57:05
2	P 214.914†	9611.6	9226.8	2145.4 µg/L	2145.4 ppb	22:57:05
2	Pb 220.353†	8732.7	8342.9	520.61 µg/L	520.61 ppb	22:57:05

2	S 181.975 Axial†	7772.1	7430.4	6023.7 µg/L	6023.7 ppb	22:57:05
2	Sb 206.836†	2400.1	2237.2	298.12 µg/L	298.12 ppb	22:57:05
2	Se 196.026†	1040.3	996.3	445 µg/L	445 ppb	22:57:05
2	SiO2†	958000.5	925999.6	101190 µg/L	101190 ppb	22:57:03
2	Si 251.611†	2929586.1	2835860.1	46882 µg/L	46882 ppb	22:57:03
2	Sn 189.927†	6787.6	6570.0	486.28 µg/L	486.28 ppb	22:57:05
2	Ti 334.940†	5770205.2	5586295.5	5694.6 µg/L	5694.6 ppb	22:57:03
2	Tl 190.801†	3017.1	3041.6	476.70 µg/L	476.70 ppb	22:57:05
2	U 409.014†	2073.2	2486.4	184.22 µg/L	184.22 ppb	22:57:03
2	V 292.402†	136273.8	131513.6	708.36 µg/L	708.36 ppb	22:57:03
2	Zn 213.857†	129838.2	125249.9	774.75 µg/L	774.75 ppb	22:57:03
3	Sc RADIAL	154858.0	154858.0	106 %		22:56:51
3	Al 396.153Radial†	907001.1	853712.5	186330 µg/L	186330 ppb	22:56:49
3	Ca 317.933Radial†	641913.2	603560.5	35366 µg/L	35366 ppb	22:56:51
3	Fe 238.204 Radial†	2340040.0	2202361.3	146420 µg/L	146420 ppb	22:56:49
3	K 766.490 Radial†	62482.9	57354.7	23560 µg/L	23560 ppb	22:56:51
3	Mg 279.077 IEC†	74369.6	69810.9	28669 µg/L	28669 ppb	22:56:51
3	Na 589.592 Radial†	71553.3	65652.1	10025 µg/L	10025 ppb	22:56:51
3	Sr 421.552†	343558.8	323639.8	758.25 µg/L	758.25 ppb	22:56:51
3	Sc 361.383	1734296.3	1734296.3	103.68 %		22:57:09
3	Y 371.029	1158763.8	1158763.8	113.32 %		22:57:09
3	Ag 328.068†	114971.2	107925.7	444.16 µg/L	444.16 ppb	22:57:09
3	As 188.979†	1255.9	1225.6	551.86 µg/L	551.86 ppb	22:57:11
3	B 249.677†	31556.7	27081.6	452.99 µg/L	452.99 ppb	22:57:09
3	Ba 233.527†	462786.9	446545.3	2038.7 µg/L	2038.7 ppb	22:57:09
3	Be 313.107†	1551309.1	1496938.6	487.32 µg/L	487.32 ppb	22:57:09
3	Cd 226.502†	66677.3	64406.5	429.62 µg/L	429.62 ppb	22:57:09
3	Co 228.616†	36357.0	35243.9	477.01 µg/L	477.01 ppb	22:57:11
3	Cr 267.716†	71208.1	68521.8	592.71 µg/L	592.71 ppb	22:57:09
3	Cu 324.752†	138907.3	131554.9	594.39 µg/L	594.39 ppb	22:57:09
3	Mn 257.610†	2430462.1	2344164.8	3201.6 µg/L	3201.6 ppb	22:57:09
3	Mo 202.031†	14664.8	14199.8	454.79 µg/L	454.79 ppb	22:57:11
3	Ni 231.604†	46036.2	44444.0	568.49 µg/L	568.49 ppb	22:57:11
3	P 214.914†	9647.2	9225.4	2144.2 µg/L	2144.2 ppb	22:57:11
3	Pb 220.353†	8845.0	8418.8	525.22 µg/L	525.22 ppb	22:57:11
3	S 181.975 Axial†	7934.8	7558.5	6127.6 µg/L	6127.6 ppb	22:57:11
3	Sb 206.836†	2420.6	2248.1	299.67 µg/L	299.67 ppb	22:57:11
3	Se 196.026†	1120.1	1069.4	474 µg/L	474 ppb	22:57:11
3	SiO2†	963572.6	927818.3	101390 µg/L	101390 ppb	22:57:09
3	Si 251.611†	2947179.9	2841956.2	46982 µg/L	46982 ppb	22:57:09
3	Sn 189.927†	6900.9	6654.0	492.27 µg/L	492.27 ppb	22:57:11
3	Ti 334.940†	5796127.5	5589881.3	5698.2 µg/L	5698.2 ppb	22:57:09
3	Tl 190.801†	2961.0	2976.3	467.97 µg/L	467.97 ppb	22:57:11
3	U 409.014†	2076.2	2481.7	183.63 µg/L	183.63 ppb	22:57:09
3	V 292.402†	136739.0	131456.5	707.91 µg/L	707.91 ppb	22:57:09
3	Zn 213.857†	130864.3	125757.6	777.76 µg/L	777.76 ppb	22:57:09

Mean Data: 1202056881|959114|1

Analyte	Mean Corrected Intensity	Conc. Units	Calib.	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1724506.3	103.09 %		0.698			0.68%
Sc RADIAL	154348.4	106 %		0.3			0.30%
Y 371.029	1152643.8	112.72 %		0.708			0.63%
Ag 328.068†	107905.3	444.08 µg/L		1.230	444.08 ppb	1.230	0.28%
Al 396.153Radial†	852555.5	186080 µg/L		399.7	186080 ppb	399.7	0.21%
As 188.979†	1213.1	546.48 µg/L		6.345	546.48 ppb	6.345	1.16%
B 249.677†	27120.6	453.64 µg/L		0.570	453.64 ppb	0.570	0.13%
Ba 233.527†	446224.2	2037.2 µg/L		1.88	2037.2 ppb	1.88	0.09%
Be 313.107†	1497465.7	487.50 µg/L		0.219	487.50 ppb	0.219	0.05%
Ca 317.933Radial†	605452.6	35477 µg/L		127.9	35477 ppb	127.9	0.36%
Cd 226.502†	64267.3	428.72 µg/L		0.839	428.72 ppb	0.839	0.20%
Co 228.616†	35247.1	477.08 µg/L		4.439	477.08 ppb	4.439	0.93%
Cr 267.716†	68400.8	591.65 µg/L		0.918	591.65 ppb	0.918	0.16%
Cu 324.752†	131526.9	594.19 µg/L		1.004	594.19 ppb	1.004	0.17%
Fe 238.204 Radial†	2194085.5	145870 µg/L		766.9	145870 ppb	766.9	0.53%
K 766.490 Radial†	57493.2	23617 µg/L		122.6	23617 ppb	122.6	0.52%
Mg 279.077 IEC†	70020.2	28756 µg/L		135.9	28756 ppb	135.9	0.47%
Mn 257.610†	2341792.3	3198.4 µg/L		3.90	3198.4 ppb	3.90	0.12%
Mo 202.031†	14150.5	453.22 µg/L		5.650	453.22 ppb	5.650	1.25%
Na 589.592 Radial†	65800.9	10047 µg/L		32.3	10047 ppb	32.3	0.32%

Ni 231.604†	44400.1	567.93 µg/L	7.736	567.93 ppb	7.736	1.36%
P 214.914†	9295.6	2161.3 µg/L	28.66	2161.3 ppb	28.66	1.33%
Pb 220.353†	8395.2	523.79 µg/L	2.766	523.79 ppb	2.766	0.53%
S 181.975 Axial†	7543.6	6115.5 µg/L	86.31	6115.5 ppb	86.31	1.41%
Sb 206.836†	2250.9	300.05 µg/L	2.148	300.05 ppb	2.148	0.72%
Se 196.026†	1045.8	464 µg/L	17.2	464 ppb	17.2	3.71%
SiO2†	927018.9	101300 µg/L	101.4	101300 ppb	101.4	0.10%
Si 251.611†	2839342.1	46939 µg/L	51.8	46939 ppb	51.8	0.11%
Sn 189.927†	6626.7	490.33 µg/L	3.511	490.33 ppb	3.511	0.72%
Sr 421.552†	324361.6	759.94 µg/L	1.500	759.94 ppb	1.500	0.20%
Ti 334.940†	5592832.6	5701.2 µg/L	8.58	5701.2 ppb	8.58	0.15%
Tl 190.801†	3037.0	476.14 µg/L	7.904	476.14 ppb	7.904	1.66%
U 409.014†	2495.2	184.58 µg/L	1.179	184.58 ppb	1.179	0.64%
V 292.402†	131488.0	708.14 µg/L	0.230	708.14 ppb	0.230	0.03%
Zn 213.857†	125410.1	775.63 µg/L	1.854	775.63 ppb	1.854	0.24%

Sequence No.: 98
 Sample ID: 1202056879|959114|5
 Analyst: HSC
 Initial Sample Wt:
 Dilution:

Autosampler Location: 418
 Date Collected: 3/29/2010 22:57:18
 Data Type: Original
 Initial Sample Vol:
 Sample Prep Vol:

Replicate Data: 1202056879|959114|5

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	154102.7	154102.7	106 %		22:57:49
1	Al 396.153Radial†	107633.2	101834.0	22229 µg/L	22229 ppb	22:57:49
1	Ca 317.933Radial†	114615.7	107790.2	6316.0 µg/L	6316.0 ppb	22:57:49
1	Fe 238.204 Radial†	459709.2	434691.2	28900 µg/L	28900 ppb	22:57:47
1	K 766.490 Radial†	10556.7	8529.8	3504.9 µg/L	3504.9 ppb	22:57:49
1	Mg 279.077 IEC†	11745.1	10922.1	4478.5 µg/L	4478.5 ppb	22:57:49
1	Na 589.592 Radial†	9237.2	7042.1	1074.4 µg/L	1074.4 ppb	22:57:49
1	Sr 421.552†	26897.8	25718.6	60.228 µg/L	60.228 ppb	22:57:49
1	Sc 361.383	1761156.6	1761156.6	105.28 %		22:58:02
1	Y 371.029	1092554.2	1092554.2	106.84 %		22:58:02
1	Ag 328.068†	3253.9	123.5	0.4566 µg/L	0.4566 ppb	22:58:04
1	As 188.979†	-15.3	-0.3	6.5335 µg/L	6.5335 ppb	22:58:24
1	B 249.677†	3398.1	-128.1	-2.1915 µg/L	-2.1915 ppb	22:58:04
1	Ba 233.527†	74675.8	71103.3	324.48 µg/L	324.48 ppb	22:58:04
1	Be 313.107†	9331.2	9523.0	3.0828 µg/L	3.0828 ppb	22:58:04
1	Cd 226.502†	333.3	411.0	-0.1932 µg/L	-0.1932 ppb	22:58:24
1	Co 228.616†	702.8	844.1	10.372 µg/L	10.372 ppb	22:58:24
1	Cr 267.716†	2418.7	2137.1	19.219 µg/L	19.219 ppb	22:58:24
1	Cu 324.752†	4583.7	1928.8	12.675 µg/L	12.675 ppb	22:58:04
1	Mn 257.610†	460084.1	436915.2	596.76 µg/L	596.76 ppb	22:58:02
1	Mo 202.031†	-65.3	-6.8	1.0241 µg/L	1.0241 ppb	22:58:24
1	Ni 231.604†	1275.6	1252.5	16.021 µg/L	16.021 ppb	22:58:24
1	P 214.914†	1490.1	1335.8	305.07 µg/L	305.07 ppb	22:58:24
1	Pb 220.353†	409.4	276.4	18.462 µg/L	18.462 ppb	22:58:24
1	S 181.975 Axial†	430.2	313.8	254.22 µg/L	254.22 ppb	22:58:24
1	Sb 206.836†	58.0	-31.6	-4.9746 µg/L	-4.9746 ppb	22:58:24
1	Se 196.026†	-8.2	-18.7	2.59 µg/L	2.59 ppb	22:58:24
1	SiO2†	180390.4	169764.9	18555 µg/L	18555 ppb	22:58:04
1	Si 251.611†	562405.2	533505.0	8821.4 µg/L	8821.4 ppb	22:58:02
1	Sn 189.927†	5.2	3.0	3.3525 µg/L	3.3525 ppb	22:58:24
1	Ti 334.940†	962628.4	913683.4	931.48 µg/L	931.48 ppb	22:58:02
1	Tl 190.801†	-194.6	-64.6	2.5059 µg/L	2.5059 ppb	22:58:24
1	U 409.014†	-1469.7	-916.9	-56.519 µg/L	-56.519 ppb	22:58:04
1	V 292.402†	8989.1	8106.2	39.546 µg/L	39.546 ppb	22:58:04
1	Zn 213.857†	10509.4	9517.6	57.548 µg/L	57.548 ppb	22:58:04
2	Sc RADIAL	156527.3	156527.3	107 %		22:57:53
2	Al 396.153Radial†	109574.3	102064.7	22279 µg/L	22279 ppb	22:57:53
2	Ca 317.933Radial†	117040.3	108368.7	6349.9 µg/L	6349.9 ppb	22:57:53
2	Fe 238.204 Radial†	459573.2	427829.5	28444 µg/L	28444 ppb	22:57:51
2	K 766.490 Radial†	10541.3	8360.8	3435.3 µg/L	3435.3 ppb	22:57:53
2	Mg 279.077 IEC†	11883.2	10878.6	4461.0 µg/L	4461.0 ppb	22:57:53
2	Na 589.592 Radial†	9242.3	6911.5	1054.5 µg/L	1054.5 ppb	22:57:53
2	Sr 421.552†	27400.3	25792.4	60.401 µg/L	60.401 ppb	22:57:53
2	Sc 361.383	1749389.0	1749389.0	104.58 %		22:58:26
2	Y 371.029	1085826.4	1085826.4	106.18 %		22:58:26
2	Ag 328.068†	3299.6	188.1	0.7431 µg/L	0.7431 ppb	22:58:28
2	As 188.979†	-4.1	10.4	10.886 µg/L	10.886 ppb	22:58:48
2	B 249.677†	3419.4	-86.0	-1.4836 µg/L	-1.4836 ppb	22:58:28
2	Ba 233.527†	75624.9	72487.9	330.81 µg/L	330.81 ppb	22:58:28
2	Be 313.107†	9171.1	9429.6	3.0514 µg/L	3.0514 ppb	22:58:28
2	Cd 226.502†	334.6	414.4	-0.1221 µg/L	-0.1221 ppb	22:58:48
2	Co 228.616†	681.8	828.5	10.189 µg/L	10.189 ppb	22:58:48
2	Cr 267.716†	2403.6	2138.1	19.216 µg/L	19.216 ppb	22:58:48
2	Cu 324.752†	4743.6	2111.0	13.398 µg/L	13.398 ppb	22:58:28
2	Mn 257.610†	453168.4	433241.9	591.75 µg/L	591.75 ppb	22:58:26
2	Mo 202.031†	-52.0	5.5	1.3967 µg/L	1.3967 ppb	22:58:48
2	Ni 231.604†	1283.6	1268.3	16.223 µg/L	16.223 ppb	22:58:48
2	P 214.914†	1509.4	1363.7	312.07 µg/L	312.07 ppb	22:58:48
2	Pb 220.353†	395.7	265.9	17.837 µg/L	17.837 ppb	22:58:48

2	S 181.975 Axial†	422.8	309.5	250.72 µg/L	250.72 ppb	22:58:48
2	Sb 206.836†	83.9	-6.4	-1.5691 µg/L	-1.5691 ppb	22:58:48
2	Se 196.026†	16.0	4.4	11.6 µg/L	11.6 ppb	22:58:48
2	SiO2†	182696.7	173122.6	18922 µg/L	18922 ppb	22:58:28
2	Si 251.611†	553853.5	528921.1	8745.6 µg/L	8745.6 ppb	22:58:26
2	Sn 189.927†	-8.3	-9.9	2.4108 µg/L	2.4108 ppb	22:58:48
2	Ti 334.940†	948573.5	906394.4	924.05 µg/L	924.05 ppb	22:58:26
2	Tl 190.801†	-213.3	-83.6	-0.1274 µg/L	-0.1274 ppb	22:58:48
2	U 409.014†	-1512.2	-966.8	-59.414 µg/L	-59.414 ppb	22:58:28
2	V 292.402†	9321.2	8481.2	41.707 µg/L	41.707 ppb	22:58:28
2	Zn 213.857†	10622.2	9692.5	58.692 µg/L	58.692 ppb	22:58:28
3	Sc RADIAL	153123.5	153123.5	105 %		22:57:57
3	Al 396.153Radial†	107138.4	102014.1	22268 µg/L	22268 ppb	22:57:57
3	Ca 317.933Radial†	113967.3	107866.2	6320.5 µg/L	6320.5 ppb	22:57:57
3	Fe 238.204 Radial†	462650.4	440271.4	29271 µg/L	29271 ppb	22:57:55
3	K 766.490 Radial†	10510.8	8549.9	3513.2 µg/L	3513.2 ppb	22:57:57
3	Mg 279.077 IEC†	11548.9	10806.4	4430.5 µg/L	4430.5 ppb	22:57:57
3	Na 589.592 Radial†	9144.0	7009.2	1069.4 µg/L	1069.4 ppb	22:57:57
3	Sr 421.552†	26759.9	25750.1	60.302 µg/L	60.302 ppb	22:57:57
3	Sc 361.383	1740300.9	1740300.9	104.04 %		22:58:51
3	Y 371.029	1080533.8	1080533.8	105.67 %		22:58:51
3	Ag 328.068†	3189.3	98.5	0.3890 µg/L	0.3890 ppb	22:58:53
3	As 188.979†	-11.9	2.8	7.9261 µg/L	7.9261 ppb	22:59:13
3	B 249.677†	3350.8	-134.9	-2.3054 µg/L	-2.3054 ppb	22:58:53
3	Ba 233.527†	75955.6	73183.5	333.98 µg/L	333.98 ppb	22:58:53
3	Be 313.107†	9459.7	9752.8	3.1625 µg/L	3.1625 ppb	22:58:53
3	Cd 226.502†	323.3	405.2	-0.2728 µg/L	-0.2728 ppb	22:59:13
3	Co 228.616†	695.5	845.1	10.375 µg/L	10.375 ppb	22:59:13
3	Cr 267.716†	2443.9	2188.9	19.665 µg/L	19.665 ppb	22:59:13
3	Cu 324.752†	4676.0	2069.7	13.354 µg/L	13.354 ppb	22:58:53
3	Mn 257.610†	453887.0	436195.5	595.78 µg/L	595.78 ppb	22:58:51
3	Mo 202.031†	-73.8	-15.7	0.7584 µg/L	0.7584 ppb	22:59:13
3	Ni 231.604†	1239.6	1232.4	15.764 µg/L	15.764 ppb	22:59:13
3	P 214.914†	1512.4	1374.1	314.01 µg/L	314.01 ppb	22:59:13
3	Pb 220.353†	405.7	277.5	18.504 µg/L	18.504 ppb	22:59:13
3	S 181.975 Axial†	419.2	308.1	249.60 µg/L	249.60 ppb	22:59:13
3	Sb 206.836†	68.9	-20.4	-3.4869 µg/L	-3.4869 ppb	22:59:13
3	Se 196.026†	-9.5	-20.1	2.17 µg/L	2.17 ppb	22:59:13
3	SiO2†	183703.0	175002.2	19128 µg/L	19128 ppb	22:58:53
3	Si 251.611†	554457.7	532267.5	8801.0 µg/L	8801.0 ppb	22:58:51
3	Sn 189.927†	14.9	12.3	4.0110 µg/L	4.0110 ppb	22:59:13
3	Ti 334.940†	948950.2	911493.1	929.25 µg/L	929.25 ppb	22:58:51
3	Tl 190.801†	-207.2	-78.9	0.5661 µg/L	0.5661 ppb	22:59:13
3	U 409.014†	-1176.1	-651.4	-40.130 µg/L	-40.130 ppb	22:58:53
3	V 292.402†	9131.1	8345.0	40.824 µg/L	40.824 ppb	22:58:53
3	Zn 213.857†	10654.1	9776.3	59.138 µg/L	59.138 ppb	22:58:53

Mean Data: 1202056879|959114|5

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1750282.2	104.63 %	0.625			0.60%
Sc RADIAL	154584.5	106 %	1.2			1.13%
Y 371.029	1086304.8	106.23 %	0.589			0.55%
Ag 328.068†	136.7	0.5296 µg/L	0.18797	0.5296 ppb	0.18797	35.50%
Al 396.153Radial†	101970.9	22259 µg/L	26.5	22259 ppb	26.5	0.12%
As 188.979†	4.3	8.4487 µg/L	2.22301	8.4487 ppb	2.22301	26.31%
B 249.677†	-116.4	-1.9935 µg/L	0.44526	-1.9935 ppb	0.44526	22.34%
Ba 233.527†	72258.3	329.76 µg/L	4.837	329.76 ppb	4.837	1.47%
Be 313.107†	9568.5	3.0989 µg/L	0.05727	3.0989 ppb	0.05727	1.85%
Ca 317.933Radial†	108008.4	6328.8 µg/L	18.42	6328.8 ppb	18.42	0.29%
Cd 226.502†	410.2	-0.1960 µg/L	0.07541	-0.1960 ppb	0.07541	38.47%
Co 228.616†	839.2	10.312 µg/L	0.1068	10.312 ppb	0.1068	1.04%
Cr 267.716†	2154.7	19.367 µg/L	0.2584	19.367 ppb	0.2584	1.33%
Cu 324.752†	2036.5	13.142 µg/L	0.4051	13.142 ppb	0.4051	3.08%
Fe 238.204 Radial†	434264.0	28871 µg/L	414.3	28871 ppb	414.3	1.44%
K 766.490 Radial†	8480.2	3484.5 µg/L	42.76	3484.5 ppb	42.76	1.23%
Mg 279.077 IEC†	10869.0	4456.7 µg/L	24.31	4456.7 ppb	24.31	0.55%
Mn 257.610†	435450.9	594.76 µg/L	2.659	594.76 ppb	2.659	0.45%
Mo 202.031†	-5.7	1.0597 µg/L	0.32063	1.0597 ppb	0.32063	30.26%
Na 589.592 Radial†	6987.6	1066.1 µg/L	10.36	1066.1 ppb	10.36	0.97%

Ni 231.604†	1251.1	16.003 µg/L	0.2303	16.003 ppb	0.2303	1.44%
P 214.914†	1357.9	310.39 µg/L	4.702	310.39 ppb	4.702	1.51%
Pb 220.353†	273.3	18.268 µg/L	0.3733	18.268 ppb	0.3733	2.04%
S 181.975 Axial†	310.4	251.51 µg/L	2.409	251.51 ppb	2.409	0.96%
Sb 206.836†	-19.5	-3.3435 µg/L	1.70727	-3.3435 ppb	1.70727	51.06%
Se 196.026†	-11.5	5.44 µg/L	5.301	5.44 ppb	5.301	97.50%
SiO2†	172629.9	18869 µg/L	290.0	18869 ppb	290.0	1.54%
Si 251.611†	531564.5	8789.3 µg/L	39.21	8789.3 ppb	39.21	0.45%
Sn 189.927†	1.8	3.2581 µg/L	0.80425	3.2581 ppb	0.80425	24.68%
Sr 421.552†	25753.7	60.310 µg/L	0.0867	60.310 ppb	0.0867	0.14%
Ti 334.940†	910523.6	928.26 µg/L	3.811	928.26 ppb	3.811	0.41%
Tl 190.801†	-75.7	0.9815 µg/L	1.36491	0.9815 ppb	1.36491	139.06%
U 409.014†	-845.0	-52.021 µg/L	10.3992	-52.021 ppb	10.3992	19.99%
Concentration less than lower limit for U 409.014.						
V 292.402†	8310.8	40.692 µg/L	1.0868	40.692 ppb	1.0868	2.67%
Zn 213.857†	9662.1	58.459 µg/L	0.8203	58.459 ppb	0.8203	1.40%

Sequence No.: 99

Sample ID: CCV

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 1

Date Collected: 3/29/2010 22:59:20

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCV

Repl#	Analyte	Net Intensity	Corrected Intensity	Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	153187.4	153187.4	105 %		22:59:54
1	Al 396.153Radial†	25521.6	24315.0	5285.2 µg/L	5285.2 ppb	22:59:54
1	Ca 317.933Radial†	89994.9	85011.8	4981.3 µg/L	4981.3 ppb	22:59:54
1	Fe 238.204 Radial†	79073.5	75123.3	4994.5 µg/L	4994.5 ppb	22:59:54
1	K 766.490 Radial†	14176.6	12033.7	4949.9 µg/L	4949.9 ppb	22:59:54
1	Mg 279.077 IEC†	13414.9	12577.3	5193.3 µg/L	5193.3 ppb	22:59:54
1	Na 589.592 Radial†	70293.6	65188.0	9970.2 µg/L	9970.2 ppb	22:59:54
1	Sr 421.552†	228379.3	217575.5	509.90 µg/L	509.90 ppb	22:59:51
1	Sc 361.383	1745783.8	1745783.8	104.36 %		23:00:20
1	Y 371.029	1054187.4	1054187.4	103.09 %		23:00:20
1	Ag 328.068†	129606.4	121219.2	498.16 µg/L	498.16 ppb	23:00:20
1	As 188.979†	1356.6	1314.1	556.30 µg/L	556.30 ppb	23:00:40
1	B 249.677†	33639.8	28877.3	483.11 µg/L	483.11 ppb	23:00:20
1	Ba 233.527†	115645.9	110984.6	507.42 µg/L	507.42 ppb	23:00:20
1	Be 313.107†	1663973.6	1595045.7	519.35 µg/L	519.35 ppb	23:00:20
1	Cd 226.502†	73436.0	70459.3	486.25 µg/L	486.25 ppb	23:00:20
1	Co 228.616†	37283.3	35900.7	491.85 µg/L	491.85 ppb	23:00:20
1	Cr 267.716†	60081.4	57408.5	492.96 µg/L	492.96 ppb	23:00:20
1	Cu 324.752†	121728.4	114212.8	498.03 µg/L	498.03 ppb	23:00:20
1	Mn 257.610†	378188.7	362292.8	494.83 µg/L	494.83 ppb	23:00:20
1	Mo 202.031†	15943.5	15331.9	484.43 µg/L	484.43 ppb	23:00:40
1	Ni 231.604†	40193.6	38553.6	493.15 µg/L	493.15 ppb	23:00:20
1	P 214.914†	10567.7	10046.2	2397.5 µg/L	2397.5 ppb	23:00:40
1	Pb 220.353†	8429.4	7964.5	484.02 µg/L	484.02 ppb	23:00:40
1	S 181.975 Axial†	1321.8	1171.7	953.34 µg/L	953.34 ppb	23:00:40
1	Sb 206.836†	3888.6	3639.3	491.93 µg/L	491.93 ppb	23:00:40
1	Se 196.026†	1285.4	1220.8	485 µg/L	485 ppb	23:00:40
1	SiO2†	52174.1	48419.3	5271.3 µg/L	5271.3 ppb	23:00:20
1	Si 251.611†	157031.6	149788.1	2467.0 µg/L	2467.0 ppb	23:00:20
1	Sn 189.927†	7242.6	6937.7	494.88 µg/L	494.88 ppb	23:00:40
1	Ti 334.940†	506991.5	485152.6	494.06 µg/L	494.06 ppb	23:00:20
1	Tl 190.801†	3627.5	3596.1	490.15 µg/L	490.15 ppb	23:00:40
1	U 409.014†	7292.7	7466.8	491.80 µg/L	491.80 ppb	23:00:20
1	V 292.402†	94247.3	89874.1	504.72 µg/L	504.72 ppb	23:00:20
1	Zn 213.857†	81526.3	77652.4	484.91 µg/L	484.91 ppb	23:00:20
2	Sc RADIAL	152753.8	152753.8	105 %		22:59:58
2	Al 396.153Radial†	25361.9	24231.6	5266.7 µg/L	5266.7 ppb	22:59:58
2	Ca 317.933Radial†	89359.1	84648.2	4960.0 µg/L	4960.0 ppb	22:59:58
2	Fe 238.204 Radial†	78661.4	74943.6	4982.5 µg/L	4982.5 ppb	22:59:58
2	K 766.490 Radial†	14004.3	11907.6	4898.0 µg/L	4898.0 ppb	22:59:58
2	Mg 279.077 IEC†	13300.6	12504.4	5163.4 µg/L	5163.4 ppb	22:59:58
2	Na 589.592 Radial†	69798.5	64905.4	9927.0 µg/L	9927.0 ppb	22:59:58
2	Sr 421.552†	228787.1	218581.4	512.26 µg/L	512.26 ppb	22:59:56
2	Sc 361.383	1730259.3	1730259.3	103.44 %		23:00:44
2	Y 371.029	1046508.0	1046508.0	102.34 %		23:00:44
2	Ag 328.068†	128748.1	121503.7	499.30 µg/L	499.30 ppb	23:00:44
2	As 188.979†	1365.2	1334.1	564.68 µg/L	564.68 ppb	23:01:04
2	B 249.677†	33448.5	28981.6	484.86 µg/L	484.86 ppb	23:00:44
2	Ba 233.527†	114240.3	110620.0	505.75 µg/L	505.75 ppb	23:00:44
2	Be 313.107†	1642115.1	1588218.9	517.13 µg/L	517.13 ppb	23:00:44
2	Cd 226.502†	72778.9	70455.4	486.23 µg/L	486.23 ppb	23:00:44
2	Co 228.616†	36814.1	35767.6	490.03 µg/L	490.03 ppb	23:00:44
2	Cr 267.716†	59621.8	57480.7	493.59 µg/L	493.59 ppb	23:00:44
2	Cu 324.752†	120547.8	114118.0	497.61 µg/L	497.61 ppb	23:00:44
2	Mn 257.610†	374569.2	362044.8	494.50 µg/L	494.50 ppb	23:00:44
2	Mo 202.031†	15997.4	15521.1	490.40 µg/L	490.40 ppb	23:01:04
2	Ni 231.604†	39787.6	38506.6	492.54 µg/L	492.54 ppb	23:00:44
2	P 214.914†	10598.8	10167.1	2426.4 µg/L	2426.4 ppb	23:01:04
2	Pb 220.353†	8438.9	8046.1	488.99 µg/L	488.99 ppb	23:01:04

2	S 181.975 Axial†	1326.3	1187.4	966.15 µg/L	966.15 ppb	23:01:04
2	Sb 206.836†	3908.3	3691.8	499.10 µg/L	499.10 ppb	23:01:04
2	Se 196.026†	1273.7	1220.5	485 µg/L	485 ppb	23:01:04
2	SiO2†	51794.9	48501.2	5280.0 µg/L	5280.0 ppb	23:00:44
2	Si 251.611†	155273.5	149438.5	2461.1 µg/L	2461.1 ppb	23:00:44
2	Sn 189.927†	7271.5	7027.9	501.29 µg/L	501.29 ppb	23:01:04
2	Ti 334.940†	502012.3	484697.4	493.59 µg/L	493.59 ppb	23:00:44
2	Tl 190.801†	3633.1	3632.7	495.06 µg/L	495.06 ppb	23:01:04
2	U 409.014†	7140.3	7382.2	486.53 µg/L	486.53 ppb	23:00:44
2	V 292.402†	93260.9	89730.7	503.99 µg/L	503.99 ppb	23:00:44
2	Zn 213.857†	80757.9	77610.5	484.66 µg/L	484.66 ppb	23:00:44
3	Sc RADIAL	153154.6	153154.6	105 %		23:00:02
3	Al 396.153Radial†	25368.9	24175.0	5254.4 µg/L	5254.4 ppb	23:00:02
3	Ca 317.933Radial†	89319.3	84387.2	4944.7 µg/L	4944.7 ppb	23:00:02
3	Fe 238.204 Radial†	78269.7	74374.5	4944.7 µg/L	4944.7 ppb	23:00:02
3	K 766.490 Radial†	14084.9	11949.3	4915.2 µg/L	4915.2 ppb	23:00:02
3	Mg 279.077 IEC†	13224.5	12398.9	5119.9 µg/L	5119.9 ppb	23:00:02
3	Na 589.592 Radial†	69824.0	64755.4	9904.0 µg/L	9904.0 ppb	23:00:02
3	Sr 421.552†	228293.2	217540.2	509.82 µg/L	509.82 ppb	23:00:00
3	Sc 361.383	1733972.1	1733972.1	103.66 %		23:01:07
3	Y 371.029	1048931.9	1048931.9	102.58 %		23:01:07
3	Ag 328.068†	129263.4	121734.2	500.23 µg/L	500.23 ppb	23:01:07
3	As 188.979†	1370.6	1336.4	565.64 µg/L	565.64 ppb	23:01:27
3	B 249.677†	33479.7	28942.4	484.20 µg/L	484.20 ppb	23:01:07
3	Ba 233.527†	114984.6	111101.5	507.95 µg/L	507.95 ppb	23:01:07
3	Be 313.107†	1650571.4	1592977.4	518.68 µg/L	518.68 ppb	23:01:07
3	Cd 226.502†	72958.6	70478.1	486.39 µg/L	486.39 ppb	23:01:07
3	Co 228.616†	36929.1	35802.4	490.51 µg/L	490.51 ppb	23:01:07
3	Cr 267.716†	59712.4	57444.7	493.28 µg/L	493.28 ppb	23:01:07
3	Cu 324.752†	120840.0	114150.3	497.74 µg/L	497.74 ppb	23:01:07
3	Mn 257.610†	375967.2	362618.1	495.28 µg/L	495.28 ppb	23:01:07
3	Mo 202.031†	15997.1	15487.8	489.34 µg/L	489.34 ppb	23:01:27
3	Ni 231.604†	39901.0	38533.6	492.89 µg/L	492.89 ppb	23:01:07
3	P 214.914†	10572.2	10119.5	2415.0 µg/L	2415.0 ppb	23:01:27
3	Pb 220.353†	8447.8	8037.2	488.45 µg/L	488.45 ppb	23:01:27
3	S 181.975 Axial†	1325.8	1184.2	963.54 µg/L	963.54 ppb	23:01:27
3	Sb 206.836†	3902.5	3678.1	497.24 µg/L	497.24 ppb	23:01:27
3	Se 196.026†	1282.6	1226.4	487 µg/L	487 ppb	23:01:27
3	SiO2†	51885.3	48481.2	5277.9 µg/L	5277.9 ppb	23:01:07
3	Si 251.611†	155674.6	149503.9	2462.2 µg/L	2462.2 ppb	23:01:07
3	Sn 189.927†	7251.3	6993.4	498.84 µg/L	498.84 ppb	23:01:27
3	Ti 334.940†	504044.2	485618.4	494.54 µg/L	494.54 ppb	23:01:07
3	Tl 190.801†	3649.3	3640.8	496.16 µg/L	496.16 ppb	23:01:27
3	U 409.014†	7071.7	7301.3	481.55 µg/L	481.55 ppb	23:01:07
3	V 292.402†	93512.7	89780.5	504.26 µg/L	504.26 ppb	23:01:07
3	Zn 213.857†	81160.7	77831.9	486.05 µg/L	486.05 ppb	23:01:07

Mean Data: CCV

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1736671.7	103.82 %	0.485			0.47%
Sc RADIAL	153031.9	105 %	0.2			0.16%
Y 371.029	1049875.8	102.67 %	0.384			0.37%
Ag 328.068†	121485.7	499.23 µg/L	1.038	499.23 ppb	1.038	0.21%
QC value within limits for Ag 328.068 Recovery = 99.85%						
Al 396.153Radial†	24240.5	5268.8 µg/L	15.50	5268.8 ppb	15.50	0.29%
QC value within limits for Al 396.153Radial Recovery = 105.38%						
As 188.979†	1328.2	562.21 µg/L	5.136	562.21 ppb	5.136	0.91%
QC value greater than the upper limit for As 188.979 Recovery = 112.44%						
B 249.677†	28933.8	484.06 µg/L	0.887	484.06 ppb	0.887	0.18%
QC value within limits for B 249.677 Recovery = 96.81%						
Ba 233.527†	110902.0	507.04 µg/L	1.147	507.04 ppb	1.147	0.23%
QC value within limits for Ba 233.527 Recovery = 101.41%						
Be 313.107†	1592080.7	518.39 µg/L	1.140	518.39 ppb	1.140	0.22%
QC value within limits for Be 313.107 Recovery = 103.68%						
Ca 317.933Radial†	84682.4	4962.0 µg/L	18.38	4962.0 ppb	18.38	0.37%
QC value within limits for Ca 317.933Radial Recovery = 99.24%						
Cd 226.502†	70464.3	486.29 µg/L	0.086	486.29 ppb	0.086	0.02%
QC value within limits for Cd 226.502 Recovery = 97.26%						
Co 228.616†	35823.6	490.80 µg/L	0.945	490.80 ppb	0.945	0.19%

QC value within limits for Co 228.616	Recovery = 98.16%			
Cr 267.716†	57444.6	493.28 µg/L	0.312	493.28 ppb 0.312 0.06%
QC value within limits for Cr 267.716	Recovery = 98.66%			
Cu 324.752†	114160.4	497.79 µg/L	0.215	497.79 ppb 0.215 0.04%
QC value within limits for Cu 324.752	Recovery = 99.56%			
Fe 238.204 Radial†	74813.8	4973.9 µg/L	25.99	4973.9 ppb 25.99 0.52%
QC value within limits for Fe 238.204 Radial	Recovery = 99.48%			
K 766.490 Radial†	11963.5	4921.0 µg/L	26.43	4921.0 ppb 26.43 0.54%
QC value within limits for K 766.490 Radial	Recovery = 98.42%			
Mg 279.077 IEC†	12493.5	5158.9 µg/L	36.92	5158.9 ppb 36.92 0.72%
QC value within limits for Mg 279.077 IEC	Recovery = 103.18%			
Mn 257.610†	362318.6	494.87 µg/L	0.394	494.87 ppb 0.394 0.08%
QC value within limits for Mn 257.610	Recovery = 98.97%			
Mo 202.031†	15446.9	488.06 µg/L	3.187	488.06 ppb 3.187 0.65%
QC value within limits for Mo 202.031	Recovery = 97.61%			
Na 589.592 Radial†	64949.6	9933.7 µg/L	33.59	9933.7 ppb 33.59 0.34%
QC value within limits for Na 589.592 Radial	Recovery = 99.34%			
Ni 231.604†	38531.3	492.86 µg/L	0.302	492.86 ppb 0.302 0.06%
QC value within limits for Ni 231.604	Recovery = 98.57%			
P 214.914†	10110.9	2413.0 µg/L	14.58	2413.0 ppb 14.58 0.60%
QC value within limits for P 214.914	Recovery = 96.52%			
Pb 220.353†	8015.9	487.15 µg/L	2.725	487.15 ppb 2.725 0.56%
QC value within limits for Pb 220.353	Recovery = 97.43%			
S 181.975 Axial†	1181.1	961.01 µg/L	6.770	961.01 ppb 6.770 0.70%
QC value within limits for S 181.975 Axial	Recovery = 96.10%			
Sb 206.836†	3669.7	496.09 µg/L	3.716	496.09 ppb 3.716 0.75%
QC value within limits for Sb 206.836	Recovery = 99.22%			
Se 196.026†	1222.6	486 µg/L	1.3	486 ppb 1.3 0.27%
QC value within limits for Se 196.026	Recovery = 97.15%			
SiO2†	48467.2	5276.4 µg/L	4.53	5276.4 ppb 4.53 0.09%
QC value within limits for SiO2	Recovery = 98.67%			
Si 251.611†	149576.8	2463.4 µg/L	3.14	2463.4 ppb 3.14 0.13%
QC value within limits for Si 251.611	Recovery = 98.54%			
Sn 189.927†	6986.3	498.34 µg/L	3.237	498.34 ppb 3.237 0.65%
QC value within limits for Sn 189.927	Recovery = 99.67%			
Sr 421.552†	217899.0	510.66 µg/L	1.386	510.66 ppb 1.386 0.27%
QC value within limits for Sr 421.552	Recovery = 102.13%			
Ti 334.940†	485156.2	494.06 µg/L	0.472	494.06 ppb 0.472 0.10%
QC value within limits for Ti 334.940	Recovery = 98.81%			
Tl 190.801†	3623.2	493.79 µg/L	3.199	493.79 ppb 3.199 0.65%
QC value within limits for Tl 190.801	Recovery = 98.76%			
U 409.014†	7383.4	486.63 µg/L	5.126	486.63 ppb 5.126 1.05%
QC value within limits for U 409.014	Recovery = 97.33%			
V 292.402†	89795.1	504.32 µg/L	0.371	504.32 ppb 0.371 0.07%
QC value within limits for V 292.402	Recovery = 100.86%			
Zn 213.857†	77698.3	485.21 µg/L	0.743	485.21 ppb 0.743 0.15%
QC value within limits for Zn 213.857	Recovery = 97.04%			
QC Failed. Continue with analysis.				

Sequence No.: 100

Sample ID: CCB

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 6

Date Collected: 3/29/2010 23:01:34

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCB

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	155434.4	155434.4	107 %		23:02:04
1	Al 396.153Radial†	-51.2	-16.1	-3.5513 µg/L	-3.5513 ppb	23:02:24
1	Ca 317.933Radial†	649.2	-7.4	-0.4325 µg/L	-0.4325 ppb	23:02:24
1	Fe 238.204 Radial†	156.2	33.2	2.2058 µg/L	2.2058 ppb	23:02:24
1	K 766.490 Radial†	1684.9	124.9	51.442 µg/L	51.442 ppb	23:02:04
1	Mg 279.077 IEC†	192.9	-5.7	-2.3512 µg/L	-2.3512 ppb	23:02:24
1	Na 589.592 Radial†	1531.9	-258.2	-39.556 µg/L	-39.556 ppb	23:02:04
1	Sr 421.552†	-266.4	28.1	0.0660 µg/L	0.0660 ppb	23:02:04
1	Sc 361.383	1773084.5	1773084.5	106.00 %		23:03:26
1	Y 371.029	1083665.8	1083665.8	105.97 %		23:03:26
1	Ag 328.068†	3188.1	40.7	0.1603 µg/L	0.1603 ppb	23:03:28
1	As 188.979†	-12.9	2.0	0.8500 µg/L	0.8500 ppb	23:03:48
1	B 249.677†	3155.7	-378.5	-6.3560 µg/L	-6.3560 ppb	23:03:48
1	Ba 233.527†	-168.6	16.0	0.0729 µg/L	0.0729 ppb	23:03:48
1	Be 313.107†	-602.7	91.5	0.0297 µg/L	0.0297 ppb	23:03:28
1	Cd 226.502†	-90.7	8.9	0.0609 µg/L	0.0609 ppb	23:03:48
1	Co 228.616†	-165.9	20.1	0.2751 µg/L	0.2751 ppb	23:03:48
1	Cr 267.716†	163.5	-6.0	-0.0511 µg/L	-0.0511 ppb	23:03:48
1	Cu 324.752†	2830.0	245.1	1.0654 µg/L	1.0654 ppb	23:03:28
1	Mn 257.610†	187.4	96.8	0.1324 µg/L	0.1324 ppb	23:03:48
1	Mo 202.031†	-32.8	24.3	0.7669 µg/L	0.7669 ppb	23:03:48
1	Ni 231.604†	-57.6	-13.4	-0.1720 µg/L	-0.1720 ppb	23:03:48
1	P 214.914†	34.6	-46.9	-11.266 µg/L	-11.266 ppb	23:03:48
1	Pb 220.353†	92.6	-25.1	-1.5171 µg/L	-1.5171 ppb	23:03:48
1	S 181.975 Axial†	93.3	-6.8	-5.4826 µg/L	-5.4826 ppb	23:03:48
1	Sb 206.836†	100.9	8.6	1.1678 µg/L	1.1678 ppb	23:03:48
1	Se 196.026†	13.1	1.4	0.557 µg/L	0.557 ppb	23:03:48
1	SiO2†	1733.6	62.6	6.8345 µg/L	6.8345 ppb	23:03:48
1	Si 251.611†	908.9	181.1	2.9879 µg/L	2.9879 ppb	23:03:28
1	Sn 189.927†	-7.8	-9.4	-0.6637 µg/L	-0.6637 ppb	23:03:48
1	Ti 334.940†	999.5	306.7	0.3130 µg/L	0.3130 ppb	23:03:28
1	Tl 190.801†	-111.5	15.1	2.0276 µg/L	2.0276 ppb	23:03:48
1	U 409.014†	-514.2	-6.0	-0.3902 µg/L	-0.3902 ppb	23:03:28
1	V 292.402†	390.8	-63.1	-0.3432 µg/L	-0.3432 ppb	23:03:28
1	Zn 213.857†	504.5	11.6	0.0731 µg/L	0.0731 ppb	23:03:48
2	Sc RADIAL	154078.8	154078.8	106 %		23:02:26
2	Al 396.153Radial†	-47.5	-13.0	-2.8946 µg/L	-2.8946 ppb	23:02:46
2	Ca 317.933Radial†	651.0	-0.4	-0.0219 µg/L	-0.0219 ppb	23:02:46
2	Fe 238.204 Radial†	154.8	33.2	2.2069 µg/L	2.2069 ppb	23:02:46
2	K 766.490 Radial†	1545.5	7.0	2.8751 µg/L	2.8751 ppb	23:02:26
2	Mg 279.077 IEC†	165.9	-29.7	-12.225 µg/L	-12.225 ppb	23:02:46
2	Na 589.592 Radial†	1707.0	-80.0	-12.240 µg/L	-12.240 ppb	23:02:26
2	Sr 421.552†	-357.1	-59.8	-0.1402 µg/L	-0.1402 ppb	23:02:26
2	Sc 361.383	1744785.0	1744785.0	104.30 %		23:03:50
2	Y 371.029	1066249.8	1066249.8	104.27 %		23:03:50
2	Ag 328.068†	3202.9	103.6	0.4168 µg/L	0.4168 ppb	23:03:52
2	As 188.979†	-24.6	-9.4	-3.9138 µg/L	-3.9138 ppb	23:04:12
2	B 249.677†	3188.7	-298.6	-5.0148 µg/L	-5.0148 ppb	23:04:12
2	Ba 233.527†	-157.1	24.4	0.1114 µg/L	0.1114 ppb	23:04:12
2	Be 313.107†	-703.8	-14.6	-0.0039 µg/L	-0.0039 ppb	23:03:52
2	Cd 226.502†	-119.9	-20.6	-0.1424 µg/L	-0.1424 ppb	23:04:12
2	Co 228.616†	-137.8	44.5	0.6093 µg/L	0.6093 ppb	23:04:12
2	Cr 267.716†	196.6	28.2	0.2400 µg/L	0.2400 ppb	23:04:12
2	Cu 324.752†	2589.8	58.0	0.2551 µg/L	0.2551 ppb	23:03:52
2	Mn 257.610†	196.2	108.1	0.1482 µg/L	0.1482 ppb	23:04:12
2	Mo 202.031†	-24.7	31.6	0.9959 µg/L	0.9959 ppb	23:04:12
2	Ni 231.604†	-50.1	-7.1	-0.0910 µg/L	-0.0910 ppb	23:04:12
2	P 214.914†	27.6	-53.1	-12.727 µg/L	-12.727 ppb	23:04:12
2	Pb 220.353†	102.2	-14.5	-0.8747 µg/L	-0.8747 ppb	23:04:12

2	S 181.975 Axial†	102.1	3.0	2.4780 µg/L	2.4780 ppb	23:04:12
2	Sb 206.836†	86.8	-3.5	-0.4576 µg/L	-0.4576 ppb	23:04:12
2	Se 196.026†	28.9	16.8	6.65 µg/L	6.65 ppb	23:04:12
2	SiO2†	1738.7	94.1	10.252 µg/L	10.252 ppb	23:04:12
2	Si 251.611†	925.9	211.3	3.4804 µg/L	3.4804 ppb	23:03:52
2	Sn 189.927†	2.9	0.7	0.0523 µg/L	0.0523 ppb	23:04:12
2	Ti 334.940†	1025.7	347.0	0.3535 µg/L	0.3535 ppb	23:03:52
2	Tl 190.801†	-111.6	13.3	1.7870 µg/L	1.7870 ppb	23:04:12
2	U 409.014†	-449.9	47.7	2.9140 µg/L	2.9140 ppb	23:03:52
2	V 292.402†	335.3	-110.4	-0.5996 µg/L	-0.5996 ppb	23:03:52
2	Zn 213.857†	495.5	10.6	0.0670 µg/L	0.0670 ppb	23:04:12
3	Sc RADIAL	153417.2	153417.2	105 %		23:02:48
3	Al 396.153Radial†	-43.3	-9.2	-2.0663 µg/L	-2.0663 ppb	23:03:08
3	Ca 317.933Radial†	638.3	-9.8	-0.5721 µg/L	-0.5721 ppb	23:03:08
3	Fe 238.204 Radial†	157.4	36.2	2.4086 µg/L	2.4086 ppb	23:03:08
3	K 766.490 Radial†	1629.7	93.3	38.407 µg/L	38.407 ppb	23:02:48
3	Mg 279.077 IEC†	176.0	-19.5	-8.0003 µg/L	-8.0003 ppb	23:03:08
3	Na 589.592 Radial†	1673.7	-104.6	-16.036 µg/L	-16.036 ppb	23:02:48
3	Sr 421.552†	-102.9	180.2	0.4224 µg/L	0.4224 ppb	23:02:48
3	Sc 361.383	1744530.6	1744530.6	104.22 %		23:04:15
3	Y 371.029	1066508.8	1066508.8	104.30 %		23:04:15
3	Ag 328.068†	3132.1	36.2	0.1410 µg/L	0.1410 ppb	23:04:17
3	As 188.979†	-26.4	-11.1	-4.6173 µg/L	-4.6173 ppb	23:04:37
3	B 249.677†	3123.5	-360.6	-6.0559 µg/L	-6.0559 ppb	23:04:37
3	Ba 233.527†	-146.6	34.5	0.1572 µg/L	0.1572 ppb	23:04:37
3	Be 313.107†	-721.4	-31.6	-0.0085 µg/L	-0.0085 ppb	23:04:17
3	Cd 226.502†	-107.7	-8.9	-0.0617 µg/L	-0.0617 ppb	23:04:37
3	Co 228.616†	-161.1	22.1	0.3028 µg/L	0.3028 ppb	23:04:37
3	Cr 267.716†	126.1	-39.3	-0.3430 µg/L	-0.3430 ppb	23:04:37
3	Cu 324.752†	2834.0	292.6	1.2771 µg/L	1.2771 ppb	23:04:17
3	Mn 257.610†	184.8	97.2	0.1331 µg/L	0.1331 ppb	23:04:37
3	Mo 202.031†	-21.1	35.0	1.1038 µg/L	1.1038 ppb	23:04:37
3	Ni 231.604†	-44.5	-1.8	-0.0230 µg/L	-0.0230 ppb	23:04:37
3	P 214.914†	38.2	-42.9	-10.301 µg/L	-10.301 ppb	23:04:37
3	Pb 220.353†	87.9	-28.2	-1.7095 µg/L	-1.7095 ppb	23:04:37
3	S 181.975 Axial†	83.2	-15.1	-12.203 µg/L	-12.203 ppb	23:04:37
3	Sb 206.836†	88.6	-1.7	-0.2140 µg/L	-0.2140 ppb	23:04:37
3	Se 196.026†	16.2	4.6	1.83 µg/L	1.83 ppb	23:04:37
3	SiO2†	1727.7	83.7	9.1129 µg/L	9.1129 ppb	23:04:37
3	Si 251.611†	815.2	105.3	1.7226 µg/L	1.7226 ppb	23:04:17
3	Sn 189.927†	10.3	7.9	0.5602 µg/L	0.5602 ppb	23:04:37
3	Ti 334.940†	751.1	83.8	0.0838 µg/L	0.0838 ppb	23:04:17
3	Tl 190.801†	-126.3	-0.8	-0.1124 µg/L	-0.1124 ppb	23:04:37
3	U 409.014†	-400.2	95.3	5.8276 µg/L	5.8276 ppb	23:04:17
3	V 292.402†	244.7	-197.2	-1.0803 µg/L	-1.0803 ppb	23:04:17
3	Zn 213.857†	492.6	7.9	0.0488 µg/L	0.0488 ppb	23:04:37

Mean Data: CCB

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1754133.4	104.86 %	0.981			0.94%
Sc RADIAL	154310.2	106 %	0.7			0.67%
Y 371.029	1072141.4	104.85 %	0.976			0.93%
Ag 328.068†	60.2	0.2394 µg/L	0.15400	0.2394 ppb	0.15400	64.34%
QC value within limits for Ag 328.068 Recovery = Not calculated						
Al 396.153Radial†	-12.8	-2.8374 µg/L	0.74415	-2.8374 ppb	0.74415	26.23%
QC value within limits for Al 396.153Radial Recovery = Not calculated						
As 188.979†	-6.1	-2.5604 µg/L	2.97431	-2.5604 ppb	2.97431	116.17%
QC value within limits for As 188.979 Recovery = Not calculated						
B 249.677†	-345.9	-5.8089 µg/L	0.70385	-5.8089 ppb	0.70385	12.12%
QC value within limits for B 249.677 Recovery = Not calculated						
Ba 233.527†	25.0	0.1138 µg/L	0.04218	0.1138 ppb	0.04218	37.06%
QC value within limits for Ba 233.527 Recovery = Not calculated						
Be 313.107†	15.1	0.0058 µg/L	0.02083	0.0058 ppb	0.02083	361.45%
QC value within limits for Be 313.107 Recovery = Not calculated						
Ca 317.933Radial†	-5.8	-0.3422 µg/L	0.28598	-0.3422 ppb	0.28598	83.58%
QC value within limits for Ca 317.933Radial Recovery = Not calculated						
Cd 226.502†	-6.9	-0.0477 µg/L	0.10238	-0.0477 ppb	0.10238	214.53%
QC value within limits for Cd 226.502 Recovery = Not calculated						
Co 228.616†	28.9	0.3958 µg/L	0.18544	0.3958 ppb	0.18544	46.86%

QC value within limits for Co 228.616 Recovery = Not calculated					
Cr 267.716†	-5.7	-0.0513 µg/L	0.29150	-0.0513 ppb	0.29150 567.93%
QC value within limits for Cr 267.716 Recovery = Not calculated					
Cu 324.752†	198.6	0.8659 µg/L	0.53941	0.8659 ppb	0.53941 62.30%
QC value within limits for Cu 324.752 Recovery = Not calculated					
Fe 238.204 Radial†	34.2	2.2738 µg/L	0.11675	2.2738 ppb	0.11675 5.13%
QC value within limits for Fe 238.204 Radial Recovery = Not calculated					
K 766.490 Radial†	75.1	30.908 µg/L	25.1368	30.908 ppb	25.1368 81.33%
QC value within limits for K 766.490 Radial Recovery = Not calculated					
Mg 279.077 IEC†	-18.3	-7.5254 µg/L	4.95395	-7.5254 ppb	4.95395 65.83%
QC value within limits for Mg 279.077 IEC Recovery = Not calculated					
Mn 257.610†	100.7	0.1379 µg/L	0.00890	0.1379 ppb	0.00890 6.45%
QC value within limits for Mn 257.610 Recovery = Not calculated					
Mo 202.031†	30.3	0.9555 µg/L	0.17201	0.9555 ppb	0.17201 18.00%
QC value within limits for Mo 202.031 Recovery = Not calculated					
Na 589.592 Radial†	-147.6	-22.611 µg/L	14.7972	-22.611 ppb	14.7972 65.44%
QC value within limits for Na 589.592 Radial Recovery = Not calculated					
Ni 231.604†	-7.5	-0.0953 µg/L	0.07457	-0.0953 ppb	0.07457 78.22%
QC value within limits for Ni 231.604 Recovery = Not calculated					
P 214.914†	-47.6	-11.432 µg/L	1.2217	-11.432 ppb	1.2217 10.69%
QC value within limits for P 214.914 Recovery = Not calculated					
Pb 220.353†	-22.6	-1.3671 µg/L	0.43713	-1.3671 ppb	0.43713 31.98%
QC value within limits for Pb 220.353 Recovery = Not calculated					
S 181.975 Axial†	-6.3	-5.0693 µg/L	7.34945	-5.0693 ppb	7.34945 144.98%
QC value within limits for S 181.975 Axial Recovery = Not calculated					
Sb 206.836†	1.1	0.1654 µg/L	0.87661	0.1654 ppb	0.87661 530.04%
QC value within limits for Sb 206.836 Recovery = Not calculated					
Se 196.026†	7.6	3.01 µg/L	3.211	3.01 ppb	3.211 106.64%
QC value within limits for Se 196.026 Recovery = Not calculated					
SiO2†	80.1	8.7333 µg/L	1.74025	8.7333 ppb	1.74025 19.93%
QC value within limits for SiO2 Recovery = Not calculated					
Si 251.611†	165.9	2.7303 µg/L	0.90677	2.7303 ppb	0.90677 33.21%
QC value within limits for Si 251.611 Recovery = Not calculated					
Sn 189.927†	-0.3	-0.0171 µg/L	0.61490	-0.0171 ppb	0.61490 >999.9%
QC value within limits for Sn 189.927 Recovery = Not calculated					
Sr 421.552†	49.5	0.1161 µg/L	0.28462	0.1161 ppb	0.28462 245.24%
QC value within limits for Sr 421.552 Recovery = Not calculated					
Ti 334.940†	245.8	0.2501 µg/L	0.14545	0.2501 ppb	0.14545 58.15%
QC value within limits for Ti 334.940 Recovery = Not calculated					
Tl 190.801†	9.2	1.2341 µg/L	1.17229	1.2341 ppb	1.17229 94.99%
QC value within limits for Tl 190.801 Recovery = Not calculated					
U 409.014†	45.7	2.7838 µg/L	3.11096	2.7838 ppb	3.11096 111.75%
QC value within limits for U 409.014 Recovery = Not calculated					
V 292.402†	-123.5	-0.6744 µg/L	0.37421	-0.6744 ppb	0.37421 55.49%
QC value within limits for V 292.402 Recovery = Not calculated					
Zn 213.857†	10.0	0.0630 µg/L	0.01264	0.0630 ppb	0.01264 20.07%
QC value within limits for Zn 213.857 Recovery = Not calculated					

All analyte(s) passed QC.

Sequence No.: 108

Sample ID: CCV

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 1

Date Collected: 3/29/2010 23:19:12

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCV

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	154136.4	154136.4	106 %		23:19:45
1	Al 396.153Radial†	25647.9	24285.0	5278.5 µg/L	5278.5 ppb	23:19:45
1	Ca 317.933Radial†	90627.7	85083.0	4985.5 µg/L	4985.5 ppb	23:19:45
1	Fe 238.204 Radial†	79120.2	74704.2	4966.6 µg/L	4966.6 ppb	23:19:45
1	K 766.490 Radial†	14323.3	12089.4	4972.8 µg/L	4972.8 ppb	23:19:45
1	Mg 279.077 IEC†	13368.7	12455.0	5143.0 µg/L	5143.0 ppb	23:19:45
1	Na 589.592 Radial†	70549.2	65017.9	9944.2 µg/L	9944.2 ppb	23:19:45
1	Sr 421.552†	227955.0	215836.4	505.82 µg/L	505.82 ppb	23:19:43
1	Sc 361.383	1718341.7	1718341.7	102.72 %		23:19:58
1	Y 371.029	1038520.8	1038520.8	101.56 %		23:19:58
1	Ag 328.068†	127024.8	120689.3	495.96 µg/L	495.96 ppb	23:19:58
1	As 188.979†	1330.3	1309.3	554.29 µg/L	554.29 ppb	23:20:18
1	B 249.677†	32912.7	28684.3	479.88 µg/L	479.88 ppb	23:19:58
1	Ba 233.527†	113367.1	110535.8	505.37 µg/L	505.37 ppb	23:19:58
1	Be 313.107†	1628068.3	1585555.0	516.26 µg/L	516.26 ppb	23:19:58
1	Cd 226.502†	71621.3	69816.4	481.82 µg/L	481.82 ppb	23:19:58
1	Co 228.616†	36326.5	35539.8	486.91 µg/L	486.91 ppb	23:19:58
1	Cr 267.716†	59120.7	57392.7	492.84 µg/L	492.84 ppb	23:19:58
1	Cu 324.752†	119452.9	113860.4	496.48 µg/L	496.48 ppb	23:19:58
1	Mn 257.610†	371120.9	361199.5	493.34 µg/L	493.34 ppb	23:19:58
1	Mo 202.031†	15768.0	15405.0	486.73 µg/L	486.73 ppb	23:20:18
1	Ni 231.604†	39236.7	38237.2	489.10 µg/L	489.10 ppb	23:19:58
1	P 214.914†	10424.7	10068.7	2402.9 µg/L	2402.9 ppb	23:20:18
1	Pb 220.353†	8314.7	7981.8	485.09 µg/L	485.09 ppb	23:20:18
1	S 181.975 Axial†	1298.5	1169.2	951.40 µg/L	951.40 ppb	23:20:18
1	Sb 206.836†	3855.1	3666.2	495.59 µg/L	495.59 ppb	23:20:18
1	Se 196.026†	1258.8	1214.5	483 µg/L	483 ppb	23:20:18
1	SiO2†	51076.3	48149.0	5241.7 µg/L	5241.7 ppb	23:19:58
1	Si 251.611†	153567.5	148818.8	2450.9 µg/L	2450.9 ppb	23:19:58
1	Sn 189.927†	7143.2	6951.8	495.88 µg/L	495.88 ppb	23:20:18
1	Ti 334.940†	498664.1	484804.1	493.71 µg/L	493.71 ppb	23:19:58
1	Tl 190.801†	3600.2	3625.0	494.03 µg/L	494.03 ppb	23:20:18
1	U 409.014†	6923.6	7219.1	476.32 µg/L	476.32 ppb	23:19:58
1	V 292.402†	92215.1	89337.9	501.76 µg/L	501.76 ppb	23:19:58
1	Zn 213.857†	79897.0	77313.8	482.81 µg/L	482.81 ppb	23:19:58
2	Sc RADIAL	152383.6	152383.6	105 %		23:19:49
2	Al 396.153Radial†	25403.6	24330.3	5288.3 µg/L	5288.3 ppb	23:19:49
2	Ca 317.933Radial†	89336.3	84833.6	4970.9 µg/L	4970.9 ppb	23:19:49
2	Fe 238.204 Radial†	78325.9	74805.1	4973.3 µg/L	4973.3 ppb	23:19:49
2	K 766.490 Radial†	14050.2	11983.9	4929.4 µg/L	4929.4 ppb	23:19:49
2	Mg 279.077 IEC†	13136.7	12378.5	5111.5 µg/L	5111.5 ppb	23:19:49
2	Na 589.592 Radial†	69754.8	65025.4	9945.3 µg/L	9945.3 ppb	23:19:49
2	Sr 421.552†	229433.2	219729.8	514.95 µg/L	514.95 ppb	23:19:47
2	Sc 361.383	1706795.5	1706795.5	102.03 %		23:20:21
2	Y 371.029	1031761.7	1031761.7	100.90 %		23:20:21
2	Ag 328.068†	126284.7	120800.5	496.45 µg/L	496.45 ppb	23:20:21
2	As 188.979†	1338.5	1326.0	561.27 µg/L	561.27 ppb	23:20:41
2	B 249.677†	32737.1	28728.9	480.62 µg/L	480.62 ppb	23:20:21
2	Ba 233.527†	112574.8	110505.9	505.23 µg/L	505.23 ppb	23:20:21
2	Be 313.107†	1615813.9	1584266.5	515.85 µg/L	515.85 ppb	23:20:21
2	Cd 226.502†	70950.5	69630.7	480.53 µg/L	480.53 ppb	23:20:21
2	Co 228.616†	36281.3	35734.7	489.58 µg/L	489.58 ppb	23:20:21
2	Cr 267.716†	58468.1	57142.5	490.67 µg/L	490.67 ppb	23:20:21
2	Cu 324.752†	118730.4	113938.9	496.84 µg/L	496.84 ppb	23:20:21
2	Mn 257.610†	368844.5	361412.5	493.63 µg/L	493.63 ppb	23:20:21
2	Mo 202.031†	15740.2	15481.6	489.15 µg/L	489.15 ppb	23:20:41
2	Ni 231.604†	38994.0	38257.6	489.36 µg/L	489.36 ppb	23:20:21
2	P 214.914†	10374.8	10088.4	2407.6 µg/L	2407.6 ppb	23:20:41
2	Pb 220.353†	8268.2	7990.9	485.63 µg/L	485.63 ppb	23:20:41

2	S 181.975 Axial†	1289.1	1168.5	950.85 µg/L	950.85 ppb	23:20:41
2	Sb 206.836†	3830.6	3667.6	495.84 µg/L	495.84 ppb	23:20:41
2	Se 196.026†	1246.5	1210.8	481 µg/L	481 ppb	23:20:41
2	SiO2†	50868.9	48282.0	5256.2 µg/L	5256.2 ppb	23:20:21
2	Si 251.611†	152572.9	148855.3	2451.5 µg/L	2451.5 ppb	23:20:21
2	Sn 189.927†	7087.8	6944.5	495.36 µg/L	495.36 ppb	23:20:41
2	Ti 334.940†	495538.2	485024.4	493.93 µg/L	493.93 ppb	23:20:21
2	Tl 190.801†	3597.6	3646.2	496.87 µg/L	496.87 ppb	23:20:41
2	U 409.014†	7226.1	7561.2	497.52 µg/L	497.52 ppb	23:20:21
2	V 292.402†	91787.2	89525.8	502.84 µg/L	502.84 ppb	23:20:21
2	Zn 213.857†	79187.7	77144.8	481.75 µg/L	481.75 ppb	23:20:21
3	Sc RADIAL	151273.8	151273.8	104 %		23:19:53
3	Al 396.153Radial†	25453.8	24556.9	5338.2 µg/L	5338.2 ppb	23:19:53
3	Ca 317.933Radial†	88670.2	84818.7	4970.0 µg/L	4970.0 ppb	23:19:53
3	Fe 238.204 Radial†	77670.3	74723.0	4967.8 µg/L	4967.8 ppb	23:19:53
3	K 766.490 Radial†	14141.9	12170.9	5006.4 µg/L	5006.4 ppb	23:19:53
3	Mg 279.077 IEC†	13129.4	12463.7	5146.4 µg/L	5146.4 ppb	23:19:53
3	Na 589.592 Radial†	69306.4	65082.8	9954.1 µg/L	9954.1 ppb	23:19:53
3	Sr 421.552†	228139.7	220093.5	515.80 µg/L	515.80 ppb	23:19:51
3	Sc 361.383	1748522.6	1748522.6	104.53 %		23:20:44
3	Y 371.029	1056889.5	1056889.5	103.36 %		23:20:44
3	Ag 328.068†	129108.4	120548.2	495.40 µg/L	495.40 ppb	23:20:44
3	As 188.979†	1335.1	1291.5	546.81 µg/L	546.81 ppb	23:21:04
3	B 249.677†	33757.7	28939.6	484.16 µg/L	484.16 ppb	23:20:44
3	Ba 233.527†	115066.6	110256.8	504.09 µg/L	504.09 ppb	23:20:44
3	Be 313.107†	1654579.2	1583560.9	515.61 µg/L	515.61 ppb	23:20:44
3	Cd 226.502†	73134.2	70060.3	483.50 µg/L	483.50 ppb	23:20:44
3	Co 228.616†	37181.3	35747.1	489.75 µg/L	489.75 ppb	23:20:44
3	Cr 267.716†	59785.9	57035.7	489.77 µg/L	489.77 ppb	23:20:44
3	Cu 324.752†	121249.3	113571.8	495.23 µg/L	495.23 ppb	23:20:44
3	Mn 257.610†	377108.6	360691.8	492.65 µg/L	492.65 ppb	23:20:44
3	Mo 202.031†	15828.9	15198.4	480.21 µg/L	480.21 ppb	23:21:04
3	Ni 231.604†	40152.2	38453.7	491.87 µg/L	491.87 ppb	23:20:44
3	P 214.914†	10441.2	9909.3	2364.7 µg/L	2364.7 ppb	23:21:04
3	Pb 220.353†	8353.9	7879.6	478.88 µg/L	478.88 ppb	23:21:04
3	S 181.975 Axial†	1305.7	1154.3	939.27 µg/L	939.27 ppb	23:21:04
3	Sb 206.836†	3855.8	3602.1	486.88 µg/L	486.88 ppb	23:21:04
3	Se 196.026†	1256.0	1190.7	473 µg/L	473 ppb	23:21:04
3	SiO2†	52044.0	48216.6	5249.4 µg/L	5249.4 ppb	23:20:44
3	Si 251.611†	156313.0	148865.0	2451.9 µg/L	2451.9 ppb	23:20:44
3	Sn 189.927†	7153.9	6841.9	488.06 µg/L	488.06 ppb	23:21:04
3	Ti 334.940†	506029.3	483471.1	492.35 µg/L	492.35 ppb	23:20:44
3	Tl 190.801†	3606.4	3570.4	486.68 µg/L	486.68 ppb	23:21:04
3	U 409.014†	7134.5	7304.5	481.66 µg/L	481.66 ppb	23:20:44
3	V 292.402†	94029.7	89524.4	502.72 µg/L	502.72 ppb	23:20:44
3	Zn 213.857†	81320.7	77333.4	482.92 µg/L	482.92 ppb	23:20:44

Mean Data: CCV

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1724553.3	103.10 %	1.288			1.25%
Sc RADIAL	152597.9	105 %	1.0			0.95%
Y 371.029	1042390.7	101.94 %	1.272			1.25%
Ag 328.068†	120679.3	495.94 µg/L	0.522	495.94 ppb	0.522	0.11%
QC value within limits for Ag 328.068 Recovery = 99.19%						
Al 396.153Radial†	24390.7	5301.7 µg/L	32.00	5301.7 ppb	32.00	0.60%
QC value within limits for Al 396.153Radial Recovery = 106.03%						
As 188.979†	1308.9	554.12 µg/L	7.234	554.12 ppb	7.234	1.31%
QC value greater than the upper limit for As 188.979 Recovery = 110.82%						
B 249.677†	28784.3	481.55 µg/L	2.286	481.55 ppb	2.286	0.47%
QC value within limits for B 249.677 Recovery = 96.31%						
Ba 233.527†	110432.8	504.90 µg/L	0.701	504.90 ppb	0.701	0.14%
QC value within limits for Ba 233.527 Recovery = 100.98%						
Be 313.107†	1584460.8	515.91 µg/L	0.328	515.91 ppb	0.328	0.06%
QC value within limits for Be 313.107 Recovery = 103.18%						
Ca 317.933Radial†	84911.8	4975.5 µg/L	8.70	4975.5 ppb	8.70	0.17%
QC value within limits for Ca 317.933Radial Recovery = 99.51%						
Cd 226.502†	69835.8	481.95 µg/L	1.489	481.95 ppb	1.489	0.31%
QC value within limits for Cd 226.502 Recovery = 96.39%						
Co 228.616†	35673.9	488.75 µg/L	1.591	488.75 ppb	1.591	0.33%

QC value within limits for Co 228.616 Recovery = 97.75%							
Cr 267.716†	57190.3	491.09 µg/L	1.578	491.09 ppb	1.578	0.32%	
QC value within limits for Cr 267.716 Recovery = 98.22%							
Cu 324.752†	113790.4	496.18 µg/L	0.844	496.18 ppb	0.844	0.17%	
QC value within limits for Cu 324.752 Recovery = 99.24%							
Fe 238.204 Radial†	74744.1	4969.2 µg/L	3.57	4969.2 ppb	3.57	0.07%	
QC value within limits for Fe 238.204 Radial Recovery = 99.38%							
K 766.490 Radial†	12081.4	4969.5 µg/L	38.58	4969.5 ppb	38.58	0.78%	
QC value within limits for K 766.490 Radial Recovery = 99.39%							
Mg 279.077 IEC†	12432.4	5133.6 µg/L	19.23	5133.6 ppb	19.23	0.37%	
QC value within limits for Mg 279.077 IEC Recovery = 102.67%							
Mn 257.610†	361101.2	493.21 µg/L	0.507	493.21 ppb	0.507	0.10%	
QC value within limits for Mn 257.610 Recovery = 98.64%							
Mo 202.031†	15361.7	485.37 µg/L	4.625	485.37 ppb	4.625	0.95%	
QC value within limits for Mo 202.031 Recovery = 97.07%							
Na 589.592 Radial†	65042.1	9947.8 µg/L	5.41	9947.8 ppb	5.41	0.05%	
QC value within limits for Na 589.592 Radial Recovery = 99.48%							
Ni 231.604†	38316.2	490.11 µg/L	1.529	490.11 ppb	1.529	0.31%	
QC value within limits for Ni 231.604 Recovery = 98.02%							
P 214.914†	10022.2	2391.7 µg/L	23.50	2391.7 ppb	23.50	0.98%	
QC value within limits for P 214.914 Recovery = 95.67%							
Pb 220.353†	7950.8	483.20 µg/L	3.751	483.20 ppb	3.751	0.78%	
QC value within limits for Pb 220.353 Recovery = 96.64%							
S 181.975 Axial†	1164.0	947.18 µg/L	6.849	947.18 ppb	6.849	0.72%	
QC value within limits for S 181.975 Axial Recovery = 94.72%							
Sb 206.836†	3645.3	492.77 µg/L	5.101	492.77 ppb	5.101	1.04%	
QC value within limits for Sb 206.836 Recovery = 98.55%							
Se 196.026†	1205.3	479 µg/L	5.1	479 ppb	5.1	1.06%	
QC value within limits for Se 196.026 Recovery = 95.79%							
SiO2†	48215.9	5249.1 µg/L	7.25	5249.1 ppb	7.25	0.14%	
QC value within limits for SiO2 Recovery = 98.16%							
Si 251.611†	148846.4	2451.4 µg/L	0.46	2451.4 ppb	0.46	0.02%	
QC value within limits for Si 251.611 Recovery = 98.06%							
Sn 189.927†	6912.8	493.10 µg/L	4.370	493.10 ppb	4.370	0.89%	
QC value within limits for Sn 189.927 Recovery = 98.62%							
Sr 421.552†	218553.2	512.19 µg/L	5.531	512.19 ppb	5.531	1.08%	
QC value within limits for Sr 421.552 Recovery = 102.44%							
Ti 334.940†	484433.2	493.33 µg/L	0.856	493.33 ppb	0.856	0.17%	
QC value within limits for Ti 334.940 Recovery = 98.67%							
Tl 190.801†	3613.9	492.52 µg/L	5.258	492.52 ppb	5.258	1.07%	
QC value within limits for Tl 190.801 Recovery = 98.50%							
U 409.014†	7361.6	485.16 µg/L	11.027	485.16 ppb	11.027	2.27%	
QC value within limits for U 409.014 Recovery = 97.03%							
V 292.402†	89462.7	502.44 µg/L	0.589	502.44 ppb	0.589	0.12%	
QC value within limits for V 292.402 Recovery = 100.49%							
Zn 213.857†	77264.0	482.49 µg/L	0.648	482.49 ppb	0.648	0.13%	
QC value within limits for Zn 213.857 Recovery = 96.50%							
QC Failed. Continue with analysis.							

Sequence No.: 109

Sample ID: CCB

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 6

Date Collected: 3/29/2010 23:21:12

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCB

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	154345.7	154345.7	106 %		23:21:42
1	Al 396.153Radial†	-6.9	25.4	5.4993 µg/L	5.4993 ppb	23:22:02
1	Ca 317.933Radial†	672.1	18.5	1.0834 µg/L	1.0834 ppb	23:22:02
1	Fe 238.204 Radial†	187.1	63.4	4.2178 µg/L	4.2178 ppb	23:22:02
1	K 766.490 Radial†	1653.7	106.6	43.891 µg/L	43.891 ppb	23:21:42
1	Mg 279.077 IEC†	187.6	-9.5	-3.8883 µg/L	-3.8883 ppb	23:22:02
1	Na 589.592 Radial†	1576.9	-205.6	-31.494 µg/L	-31.494 ppb	23:21:42
1	Sr 421.552†	-216.9	73.1	0.1714 µg/L	0.1714 ppb	23:21:42
1	Sc 361.383	1744594.7	1744594.7	104.29 %		23:22:50
1	Y 371.029	1066117.2	1066117.2	104.26 %		23:22:50
1	Ag 328.068†	3419.8	312.0	1.2788 µg/L	1.2788 ppb	23:22:52
1	As 188.979†	-13.4	1.4	0.5838 µg/L	0.5838 ppb	23:23:12
1	B 249.677†	3118.6	-365.4	-6.1363 µg/L	-6.1363 ppb	23:23:12
1	Ba 233.527†	-165.9	16.0	0.0725 µg/L	0.0725 ppb	23:23:12
1	Be 313.107†	-693.3	-4.6	0.0041 µg/L	0.0041 ppb	23:22:52
1	Cd 226.502†	-87.2	10.8	0.0738 µg/L	0.0738 ppb	23:23:12
1	Co 228.616†	-161.0	22.2	0.3042 µg/L	0.3042 ppb	23:23:12
1	Cr 267.716†	163.4	-3.5	-0.0453 µg/L	-0.0453 ppb	23:23:12
1	Cu 324.752†	2554.7	24.6	0.1231 µg/L	0.1231 ppb	23:22:52
1	Mn 257.610†	272.5	181.3	0.2479 µg/L	0.2479 ppb	23:23:12
1	Mo 202.031†	-31.7	24.8	0.7836 µg/L	0.7836 ppb	23:23:12
1	Ni 231.604†	-48.3	-5.4	-0.0688 µg/L	-0.0688 ppb	23:23:12
1	P 214.914†	32.3	-48.6	-11.656 µg/L	-11.656 ppb	23:23:12
1	Pb 220.353†	80.7	-35.0	-2.1336 µg/L	-2.1336 ppb	23:23:12
1	S 181.975 Axial†	94.0	-4.7	-3.7789 µg/L	-3.7789 ppb	23:23:12
1	Sb 206.836†	77.0	-12.8	-1.7137 µg/L	-1.7137 ppb	23:23:12
1	Se 196.026†	8.9	-2.4	-0.921 µg/L	-0.921 ppb	23:23:12
1	SiO2†	1705.7	62.6	6.8216 µg/L	6.8216 ppb	23:23:12
1	Si 251.611†	894.1	180.9	2.9798 µg/L	2.9798 ppb	23:22:52
1	Sn 189.927†	2.8	0.6	0.0455 µg/L	0.0455 ppb	23:23:12
1	Ti 334.940†	969.2	293.0	0.2915 µg/L	0.2915 ppb	23:22:52
1	Tl 190.801†	-123.6	1.8	0.2358 µg/L	0.2358 ppb	23:23:12
1	U 409.014†	-185.5	301.2	18.564 µg/L	18.564 ppb	23:22:52
1	V 292.402†	291.9	-151.9	-0.8231 µg/L	-0.8231 ppb	23:22:52
1	Zn 213.857†	511.2	25.7	0.1620 µg/L	0.1620 ppb	23:23:12
2	Sc RADIAL	153540.0	153540.0	105 %		23:22:04
2	Al 396.153Radial†	-62.1	-27.0	-5.9210 µg/L	-5.9210 ppb	23:22:24
2	Ca 317.933Radial†	679.6	29.0	1.6973 µg/L	1.6973 ppb	23:22:24
2	Fe 238.204 Radial†	188.0	65.2	4.3352 µg/L	4.3352 ppb	23:22:24
2	K 766.490 Radial†	1646.4	107.9	44.427 µg/L	44.427 ppb	23:22:04
2	Mg 279.077 IEC†	158.0	-36.7	-15.119 µg/L	-15.119 ppb	23:22:24
2	Na 589.592 Radial†	1599.5	-176.3	-27.023 µg/L	-27.023 ppb	23:22:04
2	Sr 421.552†	-265.3	26.1	0.0613 µg/L	0.0613 ppb	23:22:04
2	Sc 361.383	1765889.6	1765889.6	105.57 %		23:23:14
2	Y 371.029	1078417.8	1078417.8	105.46 %		23:23:14
2	Ag 328.068†	3351.5	207.7	0.8714 µg/L	0.8714 ppb	23:23:16
2	As 188.979†	-7.9	6.7	2.8228 µg/L	2.8228 ppb	23:23:36
2	B 249.677†	3111.0	-408.7	-6.8623 µg/L	-6.8623 ppb	23:23:36
2	Ba 233.527†	-163.4	20.3	0.0928 µg/L	0.0928 ppb	23:23:36
2	Be 313.107†	-604.1	87.9	0.0354 µg/L	0.0354 ppb	23:23:16
2	Cd 226.502†	-96.7	2.8	0.0187 µg/L	0.0187 ppb	23:23:36
2	Co 228.616†	-177.5	8.5	0.1163 µg/L	0.1163 ppb	23:23:36
2	Cr 267.716†	183.6	13.6	0.0998 µg/L	0.0998 ppb	23:23:36
2	Cu 324.752†	2609.4	47.0	0.2231 µg/L	0.2231 ppb	23:23:16
2	Mn 257.610†	280.3	185.5	0.2541 µg/L	0.2541 ppb	23:23:36
2	Mo 202.031†	-45.5	12.1	0.3817 µg/L	0.3817 ppb	23:23:36
2	Ni 231.604†	-58.4	-14.4	-0.1841 µg/L	-0.1841 ppb	23:23:36
2	P 214.914†	42.0	-39.8	-9.5428 µg/L	-9.5428 ppb	23:23:36
2	Pb 220.353†	75.9	-40.5	-2.4705 µg/L	-2.4705 ppb	23:23:36

2	S 181.975 Axial†	93.6	-6.1	-4.9583 µg/L	-4.9583 ppb	23:23:36
2	Sb 206.836†	72.9	-17.5	-2.3614 µg/L	-2.3614 ppb	23:23:36
2	Se 196.026†	12.6	1.0	0.433 µg/L	0.433 ppb	23:23:36
2	SiO2†	1700.2	37.7	4.1002 µg/L	4.1002 ppb	23:23:36
2	Si 251.611†	818.2	98.7	1.6238 µg/L	1.6238 ppb	23:23:16
2	Sn 189.927†	9.6	7.1	0.5049 µg/L	0.5049 ppb	23:23:36
2	Ti 334.940†	981.8	293.6	0.2914 µg/L	0.2914 ppb	23:23:16
2	Tl 190.801†	-108.9	17.2	2.3083 µg/L	2.3083 ppb	23:23:36
2	U 409.014†	-120.2	365.3	22.575 µg/L	22.575 ppb	23:23:16
2	V 292.402†	468.2	11.6	0.0833 µg/L	0.0833 ppb	23:23:16
2	Zn 213.857†	496.0	5.4	0.0348 µg/L	0.0348 ppb	23:23:36
3	Sc RADIAL	153171.1	153171.1	105 %		23:22:26
3	Al 396.153Radial†	-25.1	8.0	1.7102 µg/L	1.7102 ppb	23:22:46
3	Ca 317.933Radial†	656.9	8.9	0.5193 µg/L	0.5193 ppb	23:22:46
3	Fe 238.204 Radial†	208.0	84.6	5.6278 µg/L	5.6278 ppb	23:22:46
3	K 766.490 Radial†	1550.8	20.7	8.5363 µg/L	8.5363 ppb	23:22:26
3	Mg 279.077 IEC†	175.6	-19.6	-8.0671 µg/L	-8.0671 ppb	23:22:46
3	Na 589.592 Radial†	1513.4	-254.6	-38.970 µg/L	-38.970 ppb	23:22:26
3	Sr 421.552†	-202.7	85.1	0.1995 µg/L	0.1995 ppb	23:22:26
3	Sc 361.383	1729956.0	1729956.0	103.42 %		23:23:39
3	Y 371.029	1058943.9	1058943.9	103.56 %		23:23:39
3	Ag 328.068†	3273.0	197.7	0.8051 µg/L	0.8051 ppb	23:23:41
3	As 188.979†	-19.7	-4.8	-1.9868 µg/L	-1.9868 ppb	23:24:01
3	B 249.677†	3141.9	-317.6	-5.3328 µg/L	-5.3328 ppb	23:24:01
3	Ba 233.527†	-150.9	29.2	0.1330 µg/L	0.1330 ppb	23:24:01
3	Be 313.107†	-661.5	20.4	0.0091 µg/L	0.0091 ppb	23:23:41
3	Cd 226.502†	-86.1	11.1	0.0762 µg/L	0.0762 ppb	23:24:01
3	Co 228.616†	-170.6	11.6	0.1590 µg/L	0.1590 ppb	23:24:01
3	Cr 267.716†	152.9	-12.4	-0.1130 µg/L	-0.1130 ppb	23:24:01
3	Cu 324.752†	2631.1	119.2	0.5258 µg/L	0.5258 ppb	23:23:41
3	Mn 257.610†	268.4	179.6	0.2457 µg/L	0.2457 ppb	23:24:01
3	Mo 202.031†	-29.2	27.0	0.8519 µg/L	0.8519 ppb	23:24:01
3	Ni 231.604†	-67.5	-24.4	-0.3117 µg/L	-0.3117 ppb	23:24:01
3	P 214.914†	41.0	-39.9	-9.5795 µg/L	-9.5795 ppb	23:24:01
3	Pb 220.353†	109.7	-6.4	-0.3889 µg/L	-0.3889 ppb	23:24:01
3	S 181.975 Axial†	96.4	-1.7	-1.3370 µg/L	-1.3370 ppb	23:24:01
3	Sb 206.836†	87.9	-1.7	-0.2168 µg/L	-0.2168 ppb	23:24:01
3	Se 196.026†	9.9	-1.3	-0.511 µg/L	-0.511 ppb	23:24:01
3	SiO2†	1682.8	54.3	5.9216 µg/L	5.9216 ppb	23:24:01
3	Si 251.611†	803.9	101.0	1.6624 µg/L	1.6624 ppb	23:23:41
3	Sn 189.927†	-7.9	-9.7	-0.6878 µg/L	-0.6878 ppb	23:24:01
3	Ti 334.940†	739.1	78.3	0.0772 µg/L	0.0772 ppb	23:23:41
3	Tl 190.801†	-133.0	-8.3	-1.1198 µg/L	-1.1198 ppb	23:24:01
3	U 409.014†	-358.2	132.8	8.1685 µg/L	8.1685 ppb	23:23:41
3	V 292.402†	332.1	-110.7	-0.6012 µg/L	-0.6012 ppb	23:23:41
3	Zn 213.857†	499.0	18.1	0.1151 µg/L	0.1151 ppb	23:24:01

Mean Data: CCB

Analyte	Mean Corrected Intensity	Conc. Units	Calib.	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1746813.4	104.43 %		1.080			1.03%
Sc RADIAL	153685.6	105 %		0.4			0.39%
Y 371.029	1067826.3	104.42 %		0.963			0.92%
Ag 328.068†	239.2	0.9851 µg/L		0.25651	0.9851 ppb	0.25651	26.04%
QC value within limits for Ag 328.068 Recovery = Not calculated							
Al 396.153Radial†	2.1	0.4295 µg/L		5.81688	0.4295 ppb	5.81688	>999.9%
QC value within limits for Al 396.153Radial Recovery = Not calculated							
As 188.979†	1.1	0.4733 µg/L		2.40671	0.4733 ppb	2.40671	508.55%
QC value within limits for As 188.979 Recovery = Not calculated							
B 249.677†	-363.9	-6.1105 µg/L		0.76505	-6.1105 ppb	0.76505	12.52%
QC value within limits for B 249.677 Recovery = Not calculated							
Ba 233.527†	21.8	0.0995 µg/L		0.03078	0.0995 ppb	0.03078	30.95%
QC value within limits for Ba 233.527 Recovery = Not calculated							
Be 313.107†	34.6	0.0162 µg/L		0.01682	0.0162 ppb	0.01682	103.65%
QC value within limits for Be 313.107 Recovery = Not calculated							
Ca 317.933Radial†	18.8	1.1000 µg/L		0.58920	1.1000 ppb	0.58920	53.56%
QC value within limits for Ca 317.933Radial Recovery = Not calculated							
Cd 226.502†	8.2	0.0562 µg/L		0.03251	0.0562 ppb	0.03251	57.82%
QC value within limits for Cd 226.502 Recovery = Not calculated							
Co 228.616†	14.1	0.1932 µg/L		0.09852	0.1932 ppb	0.09852	51.00%

Cr	267.716†	QC value within limits for Co 228.616	Recovery = Not calculated			
		-0.8	-0.0195 µg/L	0.10874	-0.0195 ppb	0.10874 557.14%
Cu	324.752†	QC value within limits for Cr 267.716	Recovery = Not calculated			
		63.6	0.2907 µg/L	0.20967	0.2907 ppb	0.20967 72.13%
Fe	238.204 Radial†	QC value within limits for Cu 324.752	Recovery = Not calculated			
		71.1	4.7269 µg/L	0.78237	4.7269 ppb	0.78237 16.55%
K	766.490 Radial†	QC value within limits for Fe 238.204 Radial	Recovery = Not calculated			
		78.4	32.285 µg/L	20.5687	32.285 ppb	20.5687 63.71%
Mg	279.077 IEC†	QC value within limits for K 766.490 Radial	Recovery = Not calculated			
		-21.9	-9.0247 µg/L	5.67609	-9.0247 ppb	5.67609 62.90%
Mn	257.610†	QC value within limits for Mg 279.077 IEC	Recovery = Not calculated			
		182.1	0.2492 µg/L	0.00435	0.2492 ppb	0.00435 1.75%
Mo	202.031†	QC value within limits for Mn 257.610	Recovery = Not calculated			
		21.3	0.6724 µg/L	0.25409	0.6724 ppb	0.25409 37.79%
Na	589.592 Radial†	QC value within limits for Mo 202.031	Recovery = Not calculated			
		-212.2	-32.496 µg/L	6.0363	-32.496 ppb	6.0363 18.58%
Ni	231.604†	QC value within limits for Na 589.592 Radial	Recovery = Not calculated			
		-14.7	-0.1882 µg/L	0.12151	-0.1882 ppb	0.12151 64.57%
P	214.914†	QC value within limits for Ni 231.604	Recovery = Not calculated			
		-42.8	-10.260 µg/L	1.2097	-10.260 ppb	1.2097 11.79%
Pb	220.353†	QC value within limits for P 214.914	Recovery = Not calculated			
		-27.3	-1.6643 µg/L	1.11729	-1.6643 ppb	1.11729 67.13%
S	181.975 Axial†	QC value within limits for Pb 220.353	Recovery = Not calculated			
		-4.2	-3.3581 µg/L	1.84693	-3.3581 ppb	1.84693 55.00%
Sb	206.836†	QC value within limits for S 181.975 Axial	Recovery = Not calculated			
		-10.7	-1.4306 µg/L	1.09994	-1.4306 ppb	1.09994 76.88%
Se	196.026†	QC value within limits for Sb 206.836	Recovery = Not calculated			
		-0.9	-0.333 µg/L	0.6940	-0.333 ppb	0.6940 208.39%
SiO2†		QC value within limits for Se 196.026	Recovery = Not calculated			
		51.5	5.6145 µg/L	1.38643	5.6145 ppb	1.38643 24.69%
Si	251.611†	QC value within limits for SiO2	Recovery = Not calculated			
		126.8	2.0887 µg/L	0.77200	2.0887 ppb	0.77200 36.96%
Sn	189.927†	QC value within limits for Si 251.611	Recovery = Not calculated			
		-0.7	-0.0458 µg/L	0.60155	-0.0458 ppb	0.60155 >999.9%
Sr	421.552†	QC value within limits for Sn 189.927	Recovery = Not calculated			
		61.5	0.1441 µg/L	0.07307	0.1441 ppb	0.07307 50.72%
Ti	334.940†	QC value within limits for Sr 421.552	Recovery = Not calculated			
		221.6	0.2200 µg/L	0.12370	0.2200 ppb	0.12370 56.22%
Tl	190.801†	QC value within limits for Ti 334.940	Recovery = Not calculated			
		3.5	0.4748 µg/L	1.72648	0.4748 ppb	1.72648 363.65%
U	409.014†	QC value within limits for Tl 190.801	Recovery = Not calculated			
		266.4	16.436 µg/L	7.4353	16.436 ppb	7.4353 45.24%
V	292.402†	QC value within limits for U 409.014	Recovery = Not calculated			
		-83.7	-0.4470 µg/L	0.47245	-0.4470 ppb	0.47245 105.69%
Zn	213.857†	QC value within limits for V 292.402	Recovery = Not calculated			
		16.4	0.1040 µg/L	0.06433	0.1040 ppb	0.06433 61.87%

QC value within limits for Zn 213.857 Recovery = Not calculated

All analyte(s) passed QC.

Sequence No.: 110

Sample ID: 248118001|959114|1

Analyst: HSC

Initial Sample Wt:

Dilution:

Autosampler Location: 426

Date Collected: 3/29/2010 23:24:08

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: 248118001|959114|1

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	154062.9	154062.9	106 %		23:24:39
1	Al 396.153Radial†	82625.8	78201.6	17070 µg/L	17070 ppb	23:24:39
1	Ca 317.933Radial†	62846.4	58840.8	3447.8 µg/L	3447.8 ppb	23:24:41
1	Fe 238.204 Radial†	1148351.1	1086306.4	72221 µg/L	72221 ppb	23:24:39
1	K 766.490 Radial†	10741.4	8707.1	3579.5 µg/L	3579.5 ppb	23:24:41
1	Mg 279.077 IEC†	7152.5	6580.1	2651.2 µg/L	2651.2 ppb	23:24:41
1	Na 589.592 Radial†	16613.6	14022.8	2142.5 µg/L	2142.5 ppb	23:24:41
1	Sr 421.552†	18462.7	17745.0	41.562 µg/L	41.562 ppb	23:24:41
1	Sc 361.383	1743840.6	1743840.6	104.25 %		23:24:53
1	Y 371.029	1364727.8	1364727.8	133.46 %		23:24:53
1	Ag 328.068†	3106.3	12.6	-1.4387 µg/L	-1.4387 ppb	23:24:56
1	As 188.979†	-0.7	13.6	22.080 µg/L	22.080 ppb	23:25:16
1	B 249.677†	3463.8	-33.0	-0.5893 µg/L	-0.5893 ppb	23:24:56
1	Ba 233.527†	45889.2	44194.1	201.00 µg/L	201.00 ppb	23:24:56
1	Be 313.107†	23295.4	23006.2	7.3827 µg/L	7.3827 ppb	23:24:56
1	Cd 226.502†	978.6	1033.2	-0.4504 µg/L	-0.4504 ppb	23:25:16
1	Co 228.616†	574.0	727.2	6.3911 µg/L	6.3911 ppb	23:25:16
1	Cr 267.716†	2704.1	2433.7	22.693 µg/L	22.693 ppb	23:24:56
1	Cu 324.752†	5130.0	2496.1	21.158 µg/L	21.158 ppb	23:24:56
1	Mn 257.610†	2991254.8	2869273.2	3920.4 µg/L	3920.4 ppb	23:24:53
1	Mo 202.031†	-18.3	37.7	4.1118 µg/L	4.1118 ppb	23:24:56
1	Ni 231.604†	1661.9	1635.1	20.914 µg/L	20.914 ppb	23:25:16
1	P 214.914†	2487.9	2306.9	507.05 µg/L	507.05 ppb	23:25:16
1	Pb 220.353†	737.9	595.4	37.624 µg/L	37.624 ppb	23:25:16
1	S 181.975 Axial†	107.3	8.1	6.6079 µg/L	6.6079 ppb	23:25:16
1	Sb 206.836†	62.7	-26.5	-4.8058 µg/L	-4.8058 ppb	23:25:16
1	Se 196.026†	-67.5	-75.7	-5.23 µg/L	-5.23 ppb	23:25:16
1	SiO2†	595451.2	569612.2	62259 µg/L	62259 ppb	23:24:53
1	Si 251.611†	1818447.1	1743664.1	28831 µg/L	28831 ppb	23:24:53
1	Sn 189.927†	84.8	79.4	12.179 µg/L	12.179 ppb	23:25:16
1	Ti 334.940†	1982454.2	1901027.6	1938.5 µg/L	1938.5 ppb	23:24:53
1	Tl 190.801†	-399.9	-263.3	-5.4380 µg/L	-5.4380 ppb	23:25:16
1	U 409.014†	-6424.5	-5683.6	-339.25 µg/L	-339.25 ppb	23:24:53
1	V 292.402†	9693.9	8867.0	35.773 µg/L	35.773 ppb	23:24:56
1	Zn 213.857†	77561.5	73936.3	458.76 µg/L	458.76 ppb	23:24:56
2	Sc RADIAL	154593.2	154593.2	106 %		23:24:43
2	Al 396.153Radial†	82873.8	78167.3	17063 µg/L	17063 ppb	23:24:43
2	Ca 317.933Radial†	62778.0	58572.4	3432.1 µg/L	3432.1 ppb	23:24:45
2	Fe 238.204 Radial†	1152458.3	1086452.2	72231 µg/L	72231 ppb	23:24:43
2	K 766.490 Radial†	10854.7	8779.1	3609.2 µg/L	3609.2 ppb	23:24:45
2	Mg 279.077 IEC†	7066.2	6475.5	2608.1 µg/L	2608.1 ppb	23:24:45
2	Na 589.592 Radial†	16857.7	14199.1	2169.4 µg/L	2169.4 ppb	23:24:45
2	Sr 421.552†	18365.5	17593.4	41.207 µg/L	41.207 ppb	23:24:45
2	Sc 361.383	1731749.0	1731749.0	103.53 %		23:25:18
2	Y 371.029	1357248.3	1357248.3	132.73 %		23:25:18
2	Ag 328.068†	3314.6	234.7	-0.5512 µg/L	-0.5512 ppb	23:25:20
2	As 188.979†	6.5	20.5	24.963 µg/L	24.963 ppb	23:25:40
2	B 249.677†	3494.1	19.5	0.2913 µg/L	0.2913 ppb	23:25:20
2	Ba 233.527†	45701.6	44320.3	201.58 µg/L	201.58 ppb	23:25:20
2	Be 313.107†	23540.5	23398.9	7.5054 µg/L	7.5054 ppb	23:25:20
2	Cd 226.502†	986.2	1047.0	-0.3556 µg/L	-0.3556 ppb	23:25:40
2	Co 228.616†	588.3	744.8	6.6326 µg/L	6.6326 ppb	23:25:40
2	Cr 267.716†	2479.9	2235.2	21.002 µg/L	21.002 ppb	23:25:20
2	Cu 324.752†	5206.6	2604.4	21.615 µg/L	21.615 ppb	23:25:20
2	Mn 257.610†	2975383.0	2873976.7	3926.8 µg/L	3926.8 ppb	23:25:18
2	Mo 202.031†	91.5	143.6	7.4547 µg/L	7.4547 ppb	23:25:20
2	Ni 231.604†	1670.0	1654.0	21.157 µg/L	21.157 ppb	23:25:40
2	P 214.914†	2474.5	2310.6	507.90 µg/L	507.90 ppb	23:25:40
2	Pb 220.353†	710.9	574.3	36.370 µg/L	36.370 ppb	23:25:40

2	S 181.975 Axial†	115.3	16.5	13.411 µg/L	13.411 ppb	23:25:40
2	Sb 206.836†	72.9	-16.2	-3.3376 µg/L	-3.3376 ppb	23:25:40
2	Se 196.026†	-41.6	-51.1	4.49 µg/L	4.49 ppb	23:25:40
2	SiO2†	591955.0	570223.2	62326 µg/L	62326 ppb	23:25:18
2	Si 251.611†	1808131.6	1745879.5	28868 µg/L	28868 ppb	23:25:18
2	Sn 189.927†	84.3	79.4	12.203 µg/L	12.203 ppb	23:25:40
2	Ti 334.940†	1974028.4	1906166.7	1943.7 µg/L	1943.7 ppb	23:25:18
2	Tl 190.801†	-387.2	-253.7	-4.0787 µg/L	-4.0787 ppb	23:25:40
2	U 409.014†	-6664.7	-5958.6	-356.16 µg/L	-356.16 ppb	23:25:18
2	V 292.402†	9767.4	9002.9	36.537 µg/L	36.537 ppb	23:25:20
2	Zn 213.857†	77645.3	74536.6	462.54 µg/L	462.54 ppb	23:25:20
3	Sc RADIAL	154904.6	154904.6	106 %		23:24:47
3	Al 396.153Radial†	82680.4	77828.2	16989 µg/L	16989 ppb	23:24:47
3	Ca 317.933Radial†	61904.3	57631.3	3376.9 µg/L	3376.9 ppb	23:24:49
3	Fe 238.204 Radial†	1151394.9	1083267.3	72019 µg/L	72019 ppb	23:24:47
3	K 766.490 Radial†	10741.1	8651.6	3556.7 µg/L	3556.7 ppb	23:24:49
3	Mg 279.077 IEC†	6987.7	6388.2	2572.3 µg/L	2572.3 ppb	23:24:49
3	Na 589.592 Radial†	16532.6	13861.3	2117.8 µg/L	2117.8 ppb	23:24:49
3	Sr 421.552†	18236.0	17436.8	40.841 µg/L	40.841 ppb	23:24:49
3	Sc 361.383	1770092.8	1770092.8	105.82 %		23:25:43
3	Y 371.029	1384229.0	1384229.0	135.37 %		23:25:43
3	Ag 328.068†	3187.0	44.7	-1.3319 µg/L	-1.3319 ppb	23:25:45
3	As 188.979†	-0.7	13.5	22.026 µg/L	22.026 ppb	23:26:05
3	B 249.677†	3491.6	-56.1	-0.9763 µg/L	-0.9763 ppb	23:25:45
3	Ba 233.527†	46072.3	43714.3	198.81 µg/L	198.81 ppb	23:25:45
3	Be 313.107†	23647.9	23007.8	7.3805 µg/L	7.3805 ppb	23:25:45
3	Cd 226.502†	1007.5	1046.5	-0.3370 µg/L	-0.3370 ppb	23:26:05
3	Co 228.616†	581.6	726.3	6.3868 µg/L	6.3868 ppb	23:26:05
3	Cr 267.716†	2698.7	2390.1	22.315 µg/L	22.315 ppb	23:25:45
3	Cu 324.752†	5342.2	2623.6	21.673 µg/L	21.673 ppb	23:25:45
3	Mn 257.610†	3051898.5	2884027.5	3940.6 µg/L	3940.6 ppb	23:25:43
3	Mo 202.031†	90.6	140.8	7.3573 µg/L	7.3573 ppb	23:25:45
3	Ni 231.604†	1653.5	1603.5	20.511 µg/L	20.511 ppb	23:26:05
3	P 214.914†	2495.8	2279.1	500.46 µg/L	500.46 ppb	23:26:05
3	Pb 220.353†	720.6	568.6	36.023 µg/L	36.023 ppb	23:26:05
3	S 181.975 Axial†	105.4	4.8	3.8879 µg/L	3.8879 ppb	23:26:05
3	Sb 206.836†	69.4	-21.0	-4.0138 µg/L	-4.0138 ppb	23:26:05
3	Se 196.026†	-35.5	-44.5	7.05 µg/L	7.05 ppb	23:26:05
3	SiO2†	607702.9	572719.1	62598 µg/L	62598 ppb	23:25:43
3	Si 251.611†	1856843.3	1754079.1	29003 µg/L	29003 ppb	23:25:43
3	Sn 189.927†	84.0	77.4	12.059 µg/L	12.059 ppb	23:26:05
3	Ti 334.940†	2019200.6	1907550.2	1945.1 µg/L	1945.1 ppb	23:25:43
3	Tl 190.801†	-393.4	-251.5	-3.7461 µg/L	-3.7461 ppb	23:26:05
3	U 409.014†	-6678.3	-5832.0	-348.30 µg/L	-348.30 ppb	23:25:43
3	V 292.402†	9684.7	8720.4	35.012 µg/L	35.012 ppb	23:25:45
3	Zn 213.857†	78252.2	73485.6	455.95 µg/L	455.95 ppb	23:25:45

Mean Data: 248118001|959114|1

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1748560.8	104.53 %	1.172			1.12%
Sc RADIAL	154520.3	106 %	0.3			0.28%
Y 371.029	1368735.0	133.85 %	1.362			1.02%
Ag 328.068†	97.3	-1.1073 µg/L	0.48453	-1.1073 ppb	0.48453	43.76%
Al 396.153Radial†	78065.7	17041 µg/L	45.1	17041 ppb	45.1	0.26%
As 188.979†	15.9	23.023 µg/L	1.6804	23.023 ppb	1.6804	7.30%
B 249.677†	-23.2	-0.4248 µg/L	0.64963	-0.4248 ppb	0.64963	152.93%
Ba 233.527†	44076.2	200.46 µg/L	1.459	200.46 ppb	1.459	0.73%
Be 313.107†	23137.6	7.4229 µg/L	0.07150	7.4229 ppb	0.07150	0.96%
Ca 317.933Radial†	58348.2	3419.0 µg/L	37.22	3419.0 ppb	37.22	1.09%
Cd 226.502†	1042.2	-0.3810 µg/L	0.06078	-0.3810 ppb	0.06078	15.95%
Co 228.616†	732.8	6.4702 µg/L	0.14070	6.4702 ppb	0.14070	2.17%
Cr 267.716†	2353.0	22.003 µg/L	0.8876	22.003 ppb	0.8876	4.03%
Cu 324.752†	2574.7	21.482 µg/L	0.2823	21.482 ppb	0.2823	1.31%
Fe 238.204 Radial†	1085342.0	72157 µg/L	119.6	72157 ppb	119.6	0.17%
K 766.490 Radial†	8712.6	3581.8 µg/L	26.30	3581.8 ppb	26.30	0.73%
Mg 279.077 IEC†	6481.3	2610.5 µg/L	39.49	2610.5 ppb	39.49	1.51%
Mn 257.610†	2875759.1	3929.3 µg/L	10.30	3929.3 ppb	10.30	0.26%
Mo 202.031†	107.4	6.3079 µg/L	1.90249	6.3079 ppb	1.90249	30.16%
Na 589.592 Radial†	14027.7	2143.2 µg/L	25.83	2143.2 ppb	25.83	1.21%

Ni 231.604†	1630.9	20.861 µg/L	0.3263	20.861 ppb	0.3263	1.56%
P 214.914†	2298.9	505.14 µg/L	4.070	505.14 ppb	4.070	0.81%
Pb 220.353†	579.4	36.672 µg/L	0.8423	36.672 ppb	0.8423	2.30%
S 181.975 Axial†	9.8	7.9688 µg/L	4.90514	7.9688 ppb	4.90514	61.55%
Sb 206.836†	-21.3	-4.0524 µg/L	0.73485	-4.0524 ppb	0.73485	18.13%
Se 196.026†	-57.1	2.10 µg/L	6.476	2.10 ppb	6.476	307.70%
SiO2†	570851.5	62394 µg/L	179.9	62394 ppb	179.9	0.29%
Si 251.611†	1747874.3	28901 µg/L	90.7	28901 ppb	90.7	0.31%
Sn 189.927†	78.7	12.147 µg/L	0.0767	12.147 ppb	0.0767	0.63%
Sr 421.552†	17591.7	41.204 µg/L	0.3609	41.204 ppb	0.3609	0.88%
Ti 334.940†	1904914.8	1942.4 µg/L	3.51	1942.4 ppb	3.51	0.18%
Tl 190.801†	-256.1	-4.4209 µg/L	0.89637	-4.4209 ppb	0.89637	20.28%
U 409.014†	-5824.7	-347.90 µg/L	8.462	-347.90 ppb	8.462	2.43%
Concentration less than lower limit for U 409.014.						
V 292.402†	8863.4	35.774 µg/L	0.7623	35.774 ppb	0.7623	2.13%
Zn 213.857†	73986.2	459.08 µg/L	3.307	459.08 ppb	3.307	0.72%

Sequence No.: 111

Sample ID: 248118002|959114|1

Analyst: HSC

Initial Sample Wt:

Dilution:

Autosampler Location: 427

Date Collected: 3/29/2010 23:26:12

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: 248118002|959114|1

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	153694.2	153694.2	105 %		23:26:41
1	Al 396.153Radial†	89313.9	84731.8	18496 µg/L	18496 ppb	23:26:41
1	Ca 317.933Radial†	73078.9	68687.4	4024.8 µg/L	4024.8 ppb	23:26:43
1	Fe 238.204 Radial†	1111070.2	1053558.1	70044 µg/L	70044 ppb	23:26:41
1	K 766.490 Radial†	11092.5	9064.4	3726.2 µg/L	3726.2 ppb	23:26:43
1	Mg 279.077 IEC†	7958.2	7360.4	2974.8 µg/L	2974.8 ppb	23:26:43
1	Na 589.592 Radial†	16510.0	13962.3	2133.1 µg/L	2133.1 ppb	23:26:43
1	Sr 421.552†	20411.0	19634.5	45.987 µg/L	45.987 ppb	23:26:43
1	Sc 361.383	1774288.9	1774288.9	106.07 %		23:27:10
1	Y 371.029	1380436.3	1380436.3	135.00 %		23:27:10
1	Ag 328.068†	2924.0	-210.4	-2.3702 µg/L	-2.3702 ppb	23:27:12
1	As 188.979†	1.2	15.4	22.386 µg/L	22.386 ppb	23:27:32
1	B 249.677†	3404.7	-145.8	-2.4849 µg/L	-2.4849 ppb	23:27:12
1	Ba 233.527†	50548.6	47831.6	217.64 µg/L	217.64 ppb	23:27:12
1	Be 313.107†	22857.2	22209.6	7.1190 µg/L	7.1190 ppb	23:27:12
1	Cd 226.502†	964.7	1003.9	-0.4196 µg/L	-0.4196 ppb	23:27:32
1	Co 228.616†	642.7	782.6	7.2800 µg/L	7.2800 ppb	23:27:32
1	Cr 267.716†	3337.9	2986.7	27.371 µg/L	27.371 ppb	23:27:12
1	Cu 324.752†	5237.9	2513.3	20.913 µg/L	20.913 ppb	23:27:12
1	Mn 257.610†	3059520.9	2884393.1	3941.0 µg/L	3941.0 ppb	23:27:10
1	Mo 202.031†	47.8	100.3	6.0063 µg/L	6.0063 ppb	23:27:12
1	Ni 231.604†	2368.7	2274.1	29.088 µg/L	29.088 ppb	23:27:32
1	P 214.914†	2458.1	2237.9	492.29 µg/L	492.29 ppb	23:27:32
1	Pb 220.353†	749.2	593.9	37.563 µg/L	37.563 ppb	23:27:32
1	S 181.975 Axial†	125.4	23.4	18.952 µg/L	18.952 ppb	23:27:32
1	Sb 206.836†	63.6	-26.7	-4.8591 µg/L	-4.8591 ppb	23:27:32
1	Se 196.026†	-50.2	-58.3	0.898 µg/L	0.898 ppb	23:27:32
1	SiO2†	645051.5	606572.6	66299 µg/L	66299 ppb	23:27:10
1	Si 251.611†	1968662.3	1855350.6	30678 µg/L	30678 ppb	23:27:10
1	Sn 189.927†	70.4	64.4	10.751 µg/L	10.751 ppb	23:27:32
1	Ti 334.940†	1905323.4	1795675.6	1831.0 µg/L	1831.0 ppb	23:27:10
1	Tl 190.801†	-379.1	-237.1	-2.9541 µg/L	-2.9541 ppb	23:27:32
1	U 409.014†	-6785.9	-5918.6	-353.14 µg/L	-353.14 ppb	23:27:10
1	V 292.402†	9824.3	8830.3	36.047 µg/L	36.047 ppb	23:27:12
1	Zn 213.857†	74627.6	69893.4	433.44 µg/L	433.44 ppb	23:27:12
2	Sc RADIAL	155141.0	155141.0	106 %		23:26:45
2	Al 396.153Radial†	89514.3	84130.2	18364 µg/L	18364 ppb	23:26:45
2	Ca 317.933Radial†	74070.8	68973.0	4041.5 µg/L	4041.5 ppb	23:26:47
2	Fe 238.204 Radial†	1118029.0	1050269.8	69826 µg/L	69826 ppb	23:26:45
2	K 766.490 Radial†	11220.4	9086.5	3735.3 µg/L	3735.3 ppb	23:26:47
2	Mg 279.077 IEC†	8100.4	7423.6	3001.1 µg/L	3001.1 ppb	23:26:47
2	Na 589.592 Radial†	16653.8	13951.5	2131.4 µg/L	2131.4 ppb	23:26:47
2	Sr 421.552†	20538.4	19573.7	45.844 µg/L	45.844 ppb	23:26:47
2	Sc 361.383	1750408.6	1750408.6	104.64 %		23:27:34
2	Y 371.029	1364236.0	1364236.0	133.41 %		23:27:34
2	Ag 328.068†	3387.8	270.5	-0.4123 µg/L	-0.4123 ppb	23:27:36
2	As 188.979†	2.1	16.3	22.717 µg/L	22.717 ppb	23:27:56
2	B 249.677†	3435.2	-72.9	-1.2617 µg/L	-1.2617 ppb	23:27:36
2	Ba 233.527†	51074.7	48984.5	222.91 µg/L	222.91 ppb	23:27:36
2	Be 313.107†	23112.7	22747.7	7.2925 µg/L	7.2925 ppb	23:27:36
2	Cd 226.502†	935.6	988.5	-0.5027 µg/L	-0.5027 ppb	23:27:56
2	Co 228.616†	656.4	803.9	7.5884 µg/L	7.5884 ppb	23:27:56
2	Cr 267.716†	3309.8	3002.7	27.503 µg/L	27.503 ppb	23:27:36
2	Cu 324.752†	5334.2	2672.7	21.570 µg/L	21.570 ppb	23:27:36
2	Mn 257.610†	3026757.9	2892435.1	3952.0 µg/L	3952.0 ppb	23:27:34
2	Mo 202.031†	64.3	116.7	6.5167 µg/L	6.5167 ppb	23:27:36
2	Ni 231.604†	2353.4	2290.0	29.291 µg/L	29.291 ppb	23:27:56
2	P 214.914†	2452.4	2264.1	498.68 µg/L	498.68 ppb	23:27:56
2	Pb 220.353†	703.3	559.7	35.500 µg/L	35.500 ppb	23:27:56

2	S 181.975 Axial†	108.2	8.5	6.9580 µg/L	6.9580 ppb	23:27:56
2	Sb 206.836†	72.6	-17.3	-3.5708 µg/L	-3.5708 ppb	23:27:56
2	Se 196.026†	-48.0	-56.8	1.42 µg/L	1.42 ppb	23:27:56
2	SiO2†	636950.2	607127.4	66359 µg/L	66359 ppb	23:27:34
2	Si 251.611†	1944177.2	1857272.6	30710 µg/L	30710 ppb	23:27:34
2	Sn 189.927†	84.8	79.0	11.806 µg/L	11.806 ppb	23:27:56
2	Ti 334.940†	1884041.8	1799844.4	1835.3 µg/L	1835.3 ppb	23:27:34
2	Tl 190.801†	-397.0	-259.0	-5.8240 µg/L	-5.8240 ppb	23:27:56
2	U 409.014†	-6789.0	-6008.8	-358.51 µg/L	-358.51 ppb	23:27:34
2	V 292.402†	9940.0	9067.3	37.394 µg/L	37.394 ppb	23:27:36
2	Zn 213.857†	75757.4	71933.0	446.30 µg/L	446.30 ppb	23:27:36
3	Sc RADIAL	155349.8	155349.8	107 %		23:26:49
3	Al 396.153Radial†	90166.2	84628.7	18473 µg/L	18473 ppb	23:26:49
3	Ca 317.933Radial†	72796.3	67683.6	3966.0 µg/L	3966.0 ppb	23:26:51
3	Fe 238.204 Radial†	1126402.0	1056713.8	70254 µg/L	70254 ppb	23:26:49
3	K 766.490 Radial†	11014.4	8879.1	3649.9 µg/L	3649.9 ppb	23:26:51
3	Mg 279.077 IEC†	8055.0	7370.8	2978.9 µg/L	2978.9 ppb	23:26:51
3	Na 589.592 Radial†	16393.3	13686.0	2090.9 µg/L	2090.9 ppb	23:26:51
3	Sr 421.552†	20278.1	19303.6	45.211 µg/L	45.211 ppb	23:26:51
3	Sc 361.383	1750763.4	1750763.4	104.66 %		23:27:59
3	Y 371.029	1364009.6	1364009.6	133.39 %		23:27:59
3	Ag 328.068†	3149.5	42.2	-1.3302 µg/L	-1.3302 ppb	23:28:01
3	As 188.979†	15.8	29.3	28.274 µg/L	28.274 ppb	23:28:21
3	B 249.677†	3332.5	-171.7	-2.9206 µg/L	-2.9206 ppb	23:28:01
3	Ba 233.527†	50841.9	48752.2	221.85 µg/L	221.85 ppb	23:28:01
3	Be 313.107†	22960.1	22597.5	7.2447 µg/L	7.2447 ppb	23:28:01
3	Cd 226.502†	967.0	1018.3	-0.3417 µg/L	-0.3417 ppb	23:28:21
3	Co 228.616†	660.1	807.3	7.6125 µg/L	7.6125 ppb	23:28:21
3	Cr 267.716†	3410.9	3098.7	28.343 µg/L	28.343 ppb	23:28:01
3	Cu 324.752†	5415.7	2749.6	21.969 µg/L	21.969 ppb	23:28:01
3	Mn 257.610†	3017561.3	2883062.0	3939.2 µg/L	3939.2 ppb	23:27:59
3	Mo 202.031†	29.9	83.8	5.4965 µg/L	5.4965 ppb	23:28:01
3	Ni 231.604†	2385.7	2320.4	29.680 µg/L	29.680 ppb	23:28:21
3	P 214.914†	2460.9	2271.7	500.24 µg/L	500.24 ppb	23:28:21
3	Pb 220.353†	696.9	553.5	35.107 µg/L	35.107 ppb	23:28:21
3	S 181.975 Axial†	108.9	9.3	7.5309 µg/L	7.5309 ppb	23:28:21
3	Sb 206.836†	60.4	-29.0	-5.1837 µg/L	-5.1837 ppb	23:28:21
3	Se 196.026†	-53.9	-62.4	-0.649 µg/L	-0.649 ppb	23:28:21
3	SiO2†	635560.9	605676.6	66201 µg/L	66201 ppb	23:27:59
3	Si 251.611†	1939411.2	1852342.5	30628 µg/L	30628 ppb	23:27:59
3	Sn 189.927†	88.6	82.6	12.048 µg/L	12.048 ppb	23:28:21
3	Ti 334.940†	1880304.4	1795908.7	1831.3 µg/L	1831.3 ppb	23:27:59
3	Tl 190.801†	-378.6	-241.4	-3.5253 µg/L	-3.5253 ppb	23:28:21
3	U 409.014†	-6730.6	-5951.6	-355.16 µg/L	-355.16 ppb	23:27:59
3	V 292.402†	9964.1	9088.4	37.442 µg/L	37.442 ppb	23:28:01
3	Zn 213.857†	75299.9	71481.2	443.41 µg/L	443.41 ppb	23:28:01

Mean Data: 248118002|959114|1

Analyte	Mean Corrected Intensity	Conc. Units	Calib.	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1758486.9	105.12 %		0.818			0.78%
Sc RADIAL	154728.3	106 %		0.6			0.58%
Y 371.029	1369560.6	133.93 %		0.921			0.69%
Ag 328.068†	34.1	-1.3709 µg/L		0.97955	-1.3709 ppb	0.97955	71.45%
Al 396.153Radial†	84496.9	18444 µg/L		70.3	18444 ppb	70.3	0.38%
As 188.979†	20.3	24.459 µg/L		3.3081	24.459 ppb	3.3081	13.52%
B 249.677†	-130.1	-2.2224 µg/L		0.86005	-2.2224 ppb	0.86005	38.70%
Ba 233.527†	48522.8	220.80 µg/L		2.787	220.80 ppb	2.787	1.26%
Be 313.107†	22518.2	7.2187 µg/L		0.08961	7.2187 ppb	0.08961	1.24%
Ca 317.933Radial†	68448.0	4010.8 µg/L		39.68	4010.8 ppb	39.68	0.99%
Cd 226.502†	1003.6	-0.4213 µg/L		0.08053	-0.4213 ppb	0.08053	19.11%
Co 228.616†	797.9	7.4936 µg/L		0.18537	7.4936 ppb	0.18537	2.47%
Cr 267.716†	3029.4	27.739 µg/L		0.5272	27.739 ppb	0.5272	1.90%
Cu 324.752†	2645.2	21.484 µg/L		0.5334	21.484 ppb	0.5334	2.48%
Fe 238.204 Radial†	1053513.9	70041 µg/L		214.2	70041 ppb	214.2	0.31%
K 766.490 Radial†	9010.0	3703.8 µg/L		46.90	3703.8 ppb	46.90	1.27%
Mg 279.077 IEC†	7384.9	2984.9 µg/L		14.14	2984.9 ppb	14.14	0.47%
Mn 257.610†	2886630.1	3944.1 µg/L		6.93	3944.1 ppb	6.93	0.18%
Mo 202.031†	100.2	6.0065 µg/L		0.51013	6.0065 ppb	0.51013	8.49%
Na 589.592 Radial†	13866.6	2118.5 µg/L		23.91	2118.5 ppb	23.91	1.13%

Ni 231.604†	2294.8	29.353 µg/L	0.3009	29.353 ppb	0.3009	1.03%
P 214.914†	2257.9	497.07 µg/L	4.211	497.07 ppb	4.211	0.85%
Pb 220.353†	569.0	36.057 µg/L	1.3191	36.057 ppb	1.3191	3.66%
S 181.975 Axial†	13.7	11.147 µg/L	6.7654	11.147 ppb	6.7654	60.69%
Sb 206.836†	-24.3	-4.5379 µg/L	0.85307	-4.5379 ppb	0.85307	18.80%
Se 196.026†	-59.1	0.556 µg/L	1.0753	0.556 ppb	1.0753	193.49%
SiO2†	606458.8	66286 µg/L	80.0	66286 ppb	80.0	0.12%
Si 251.611†	1854988.6	30672 µg/L	41.1	30672 ppb	41.1	0.13%
Sn 189.927†	75.3	11.535 µg/L	0.6895	11.535 ppb	0.6895	5.98%
Sr 421.552†	19503.9	45.681 µg/L	0.4126	45.681 ppb	0.4126	0.90%
Ti 334.940†	1797142.9	1832.5 µg/L	2.39	1832.5 ppb	2.39	0.13%
Tl 190.801†	-245.8	-4.1011 µg/L	1.51912	-4.1011 ppb	1.51912	37.04%
U 409.014†	-5959.7	-355.60 µg/L	2.716	-355.60 ppb	2.716	0.76%
Concentration less than lower limit for U 409.014.						
V 292.402†	8995.4	36.961 µg/L	0.7922	36.961 ppb	0.7922	2.14%
Zn 213.857†	71102.5	441.05 µg/L	6.747	441.05 ppb	6.747	1.53%

Sequence No.: 112

Sample ID: 248118003|959114|1

Analyst: HSC

Initial Sample Wt:

Dilution:

Autosampler Location: 428

Date Collected: 3/29/2010 23:28:29

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: 248118003|959114|1

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	154978.8	154978.8	106 %		23:29:01
1	Al 396.153Radial†	118144.9	111144.6	24261 µg/L	24261 ppb	23:29:01
1	Ca 317.933Radial†	103691.7	96903.7	5678.1 µg/L	5678.1 ppb	23:29:01
1	Fe 238.204 Radial†	1163044.9	1093705.6	72713 µg/L	72713 ppb	23:28:59
1	K 766.490 Radial†	13780.3	11505.0	4729.2 µg/L	4729.2 ppb	23:29:01
1	Mg 279.077 IEC†	12064.5	11159.7	4539.1 µg/L	4539.1 ppb	23:29:01
1	Na 589.592 Radial†	17230.6	14510.3	2216.0 µg/L	2216.0 ppb	23:29:01
1	Sr 421.552†	22066.9	21031.4	49.248 µg/L	49.248 ppb	23:29:01
1	Sc 361.383	1750164.5	1750164.5	104.63 %		23:29:13
1	Y 371.029	1362072.2	1362072.2	133.20 %		23:29:13
1	Ag 328.068†	3078.6	-24.6	-1.4976 µg/L	-1.4976 ppb	23:29:15
1	As 188.979†	6.2	20.2	25.090 µg/L	25.090 ppb	23:29:35
1	B 249.677†	3415.0	-91.7	-1.5914 µg/L	-1.5914 ppb	23:29:15
1	Ba 233.527†	66297.9	63541.3	289.38 µg/L	289.38 ppb	23:29:15
1	Be 313.107†	29521.2	28875.9	9.2901 µg/L	9.2901 ppb	23:29:15
1	Cd 226.502†	995.1	1045.5	-0.4192 µg/L	-0.4192 ppb	23:29:35
1	Co 228.616†	953.2	1087.7	11.390 µg/L	11.390 ppb	23:29:35
1	Cr 267.716†	4180.4	3835.3	34.824 µg/L	34.824 ppb	23:29:15
1	Cu 324.752†	6675.1	3955.1	27.617 µg/L	27.617 ppb	23:29:15
1	Mn 257.610†	2737291.9	2616172.4	3574.5 µg/L	3574.5 ppb	23:29:13
1	Mo 202.031†	175.6	223.1	10.019 µg/L	10.019 ppb	23:29:15
1	Ni 231.604†	1282.9	1267.0	16.207 µg/L	16.207 ppb	23:29:35
1	P 214.914†	2934.5	2725.2	608.34 µg/L	608.34 ppb	23:29:35
1	Pb 220.353†	1169.7	1005.5	62.881 µg/L	62.881 ppb	23:29:35
1	S 181.975 Axial†	154.6	53.0	42.963 µg/L	42.963 ppb	23:29:35
1	Sb 206.836†	65.5	-24.0	-4.6200 µg/L	-4.6200 ppb	23:29:35
1	Se 196.026†	-46.9	-55.7	2.85 µg/L	2.85 ppb	23:29:35
1	SiO2†	744365.1	709877.4	77590 µg/L	77590 ppb	23:29:13
1	Si 251.611†	2267988.6	2167024.7	35831 µg/L	35831 ppb	23:29:13
1	Sn 189.927†	51.7	47.4	9.8236 µg/L	9.8236 ppb	23:29:35
1	Ti 334.940†	1964624.1	1877114.6	1914.0 µg/L	1914.0 ppb	23:29:13
1	Tl 190.801†	-393.9	-256.2	-5.6035 µg/L	-5.6035 ppb	23:29:35
1	U 409.014†	-6634.3	-5861.8	-352.21 µg/L	-352.21 ppb	23:29:13
1	V 292.402†	10802.9	9893.4	41.516 µg/L	41.516 ppb	23:29:15
1	Zn 213.857†	66223.9	62831.1	388.93 µg/L	388.93 ppb	23:29:15
2	Sc RADIAL	154778.9	154778.9	106 %		23:29:05
2	Al 396.153Radial†	118006.7	111157.9	24264 µg/L	24264 ppb	23:29:05
2	Ca 317.933Radial†	103321.0	96680.4	5665.1 µg/L	5665.1 ppb	23:29:05
2	Fe 238.204 Radial†	1155245.5	1087773.3	72319 µg/L	72319 ppb	23:29:03
2	K 766.490 Radial†	13739.2	11483.1	4720.2 µg/L	4720.2 ppb	23:29:05
2	Mg 279.077 IEC†	12104.0	11211.6	4560.8 µg/L	4560.8 ppb	23:29:05
2	Na 589.592 Radial†	17241.4	14541.4	2220.8 µg/L	2220.8 ppb	23:29:05
2	Sr 421.552†	22192.9	21176.9	49.589 µg/L	49.589 ppb	23:29:05
2	Sc 361.383	1771897.0	1771897.0	105.93 %		23:29:37
2	Y 371.029	1377303.9	1377303.9	134.69 %		23:29:37
2	Ag 328.068†	3171.6	27.2	-1.3138 µg/L	-1.3138 ppb	23:29:40
2	As 188.979†	3.0	17.0	23.667 µg/L	23.667 ppb	23:30:00
2	B 249.677†	3474.1	-76.0	-1.3262 µg/L	-1.3262 ppb	23:29:40
2	Ba 233.527†	65632.6	62136.1	282.97 µg/L	282.97 ppb	23:29:40
2	Be 313.107†	29294.9	28316.2	9.1048 µg/L	9.1048 ppb	23:29:40
2	Cd 226.502†	1017.1	1054.6	-0.3152 µg/L	-0.3152 ppb	23:30:00
2	Co 228.616†	941.0	1064.9	11.093 µg/L	11.093 ppb	23:30:00
2	Cr 267.716†	4084.6	3695.8	33.616 µg/L	33.616 ppb	23:29:40
2	Cu 324.752†	6585.7	3792.4	26.844 µg/L	26.844 ppb	23:29:40
2	Mn 257.610†	2782458.2	2626723.4	3588.9 µg/L	3588.9 ppb	23:29:37
2	Mo 202.031†	194.9	239.2	10.513 µg/L	10.513 ppb	23:29:40
2	Ni 231.604†	1267.9	1237.9	15.834 µg/L	15.834 ppb	23:30:00
2	P 214.914†	2891.2	2649.9	590.57 µg/L	590.57 ppb	23:30:00
2	Pb 220.353†	1191.4	1012.3	63.319 µg/L	63.319 ppb	23:30:00

2	S 181.975 Axial†	160.0	56.2	45.589 µg/L	45.589 ppb	23:30:00
2	Sb 206.836†	65.3	-25.0	-4.7196 µg/L	-4.7196 ppb	23:30:00
2	Se 196.026†	-52.5	-60.4	0.822 µg/L	0.822 ppb	23:30:00
2	SiO2†	756310.6	712428.6	77869 µg/L	77869 ppb	23:29:37
2	Si 251.611†	2305812.3	2176145.4	35982 µg/L	35982 ppb	23:29:37
2	Sn 189.927†	49.4	44.6	9.6380 µg/L	9.6380 ppb	23:30:00
2	Ti 334.940†	1992495.3	1880395.8	1917.3 µg/L	1917.3 ppb	23:29:37
2	Tl 190.801†	-369.9	-228.9	-1.8868 µg/L	-1.8868 ppb	23:30:00
2	U 409.014†	-6890.3	-6025.7	-362.21 µg/L	-362.21 ppb	23:29:37
2	V 292.402†	10737.5	9705.0	40.524 µg/L	40.524 ppb	23:29:40
2	Zn 213.857†	65785.2	61640.7	381.48 µg/L	381.48 ppb	23:29:40
3	Sc RADIAL	156925.9	156925.9	108 %		23:29:09
3	Al 396.153Radial†	119975.3	111466.0	24331 µg/L	24331 ppb	23:29:09
3	Ca 317.933Radial†	105550.5	97420.1	5708.4 µg/L	5708.4 ppb	23:29:09
3	Fe 238.204 Radial†	1171069.1	1087586.1	72307 µg/L	72307 ppb	23:29:07
3	K 766.490 Radial†	14042.1	11587.5	4763.1 µg/L	4763.1 ppb	23:29:09
3	Mg 279.077 IEC†	12320.1	11256.4	4579.3 µg/L	4579.3 ppb	23:29:09
3	Na 589.592 Radial†	17432.7	14497.0	2214.0 µg/L	2214.0 ppb	23:29:09
3	Sr 421.552†	22466.3	21144.9	49.513 µg/L	49.513 ppb	23:29:09
3	Sc 361.383	1766827.4	1766827.4	105.62 %		23:30:02
3	Y 371.029	1374515.2	1374515.2	134.42 %		23:30:02
3	Ag 328.068†	3397.1	249.2	-0.4168 µg/L	-0.4168 ppb	23:30:04
3	As 188.979†	3.0	17.1	23.673 µg/L	23.673 ppb	23:30:24
3	B 249.677†	3513.0	-29.7	-0.5491 µg/L	-0.5491 ppb	23:30:04
3	Ba 233.527†	64990.6	61706.0	281.00 µg/L	281.00 ppb	23:30:04
3	Be 313.107†	28855.0	27979.0	8.9948 µg/L	8.9948 ppb	23:30:04
3	Cd 226.502†	997.7	1039.0	-0.4212 µg/L	-0.4212 ppb	23:30:24
3	Co 228.616†	942.3	1068.8	11.144 µg/L	11.144 ppb	23:30:24
3	Cr 267.716†	4067.5	3690.7	33.573 µg/L	33.573 ppb	23:30:04
3	Cu 324.752†	6668.8	3889.0	27.262 µg/L	27.262 ppb	23:30:04
3	Mn 257.610†	2771979.8	2624340.0	3585.6 µg/L	3585.6 ppb	23:30:02
3	Mo 202.031†	185.0	230.4	10.234 µg/L	10.234 ppb	23:30:04
3	Ni 231.604†	1271.9	1245.1	15.927 µg/L	15.927 ppb	23:30:24
3	P 214.914†	2924.1	2688.9	599.94 µg/L	599.94 ppb	23:30:24
3	Pb 220.353†	1193.4	1017.5	63.637 µg/L	63.637 ppb	23:30:24
3	S 181.975 Axial†	159.3	56.0	45.460 µg/L	45.460 ppb	23:30:24
3	Sb 206.836†	55.2	-34.4	-5.9858 µg/L	-5.9858 ppb	23:30:24
3	Se 196.026†	-32.8	-42.0	8.11 µg/L	8.11 ppb	23:30:24
3	SiO2†	753120.5	711457.1	77763 µg/L	77763 ppb	23:30:02
3	Si 251.611†	2294710.8	2171880.9	35912 µg/L	35912 ppb	23:30:02
3	Sn 189.927†	57.3	52.2	10.175 µg/L	10.175 ppb	23:30:24
3	Ti 334.940†	1986598.1	1880209.8	1917.1 µg/L	1917.1 ppb	23:30:02
3	Tl 190.801†	-382.6	-241.9	-3.6424 µg/L	-3.6424 ppb	23:30:24
3	U 409.014†	-6886.8	-6041.1	-363.19 µg/L	-363.19 ppb	23:30:02
3	V 292.402†	10664.4	9664.9	40.300 µg/L	40.300 ppb	23:30:04
3	Zn 213.857†	65215.8	61279.8	379.21 µg/L	379.21 ppb	23:30:04

Mean Data: 248118003|959114|1

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1762963.0	105.39 %	0.680			0.64%
Sc RADIAL	155561.2	107 %	0.8			0.76%
Y 371.029	1371297.1	134.10 %	0.793			0.59%
Ag 328.068†	83.9	-1.0761 µg/L	0.57826	-1.0761 ppb	0.57826	53.74%
Al 396.153Radial†	111256.2	24286 µg/L	39.7	24286 ppb	39.7	0.16%
As 188.979†	18.1	24.143 µg/L	0.8201	24.143 ppb	0.8201	3.40%
B 249.677†	-65.8	-1.1556 µg/L	0.54169	-1.1556 ppb	0.54169	46.88%
Ba 233.527†	62461.1	284.45 µg/L	4.382	284.45 ppb	4.382	1.54%
Be 313.107†	28390.4	9.1299 µg/L	0.14924	9.1299 ppb	0.14924	1.63%
Ca 317.933Radial†	97001.4	5683.9 µg/L	22.23	5683.9 ppb	22.23	0.39%
Cd 226.502†	1046.4	-0.3852 µg/L	0.06066	-0.3852 ppb	0.06066	15.75%
Co 228.616†	1073.8	11.209 µg/L	0.1590	11.209 ppb	0.1590	1.42%
Cr 267.716†	3740.6	34.005 µg/L	0.7104	34.005 ppb	0.7104	2.09%
Cu 324.752†	3878.8	27.241 µg/L	0.3867	27.241 ppb	0.3867	1.42%
Fe 238.204 Radial†	1089688.3	72446 µg/L	231.4	72446 ppb	231.4	0.32%
K 766.490 Radial†	11525.2	4737.5 µg/L	22.64	4737.5 ppb	22.64	0.48%
Mg 279.077 IEC†	11209.2	4559.7 µg/L	20.13	4559.7 ppb	20.13	0.44%
Mn 257.610†	2622411.9	3583.0 µg/L	7.56	3583.0 ppb	7.56	0.21%
Mo 202.031†	230.9	10.255 µg/L	0.2476	10.255 ppb	0.2476	2.41%
Na 589.592 Radial†	14516.2	2216.9 µg/L	3.51	2216.9 ppb	3.51	0.16%

Ni 231.604†	1250.0	15.989 µg/L	0.1940	15.989 ppb	0.1940	1.21%
P 214.914†	2688.0	599.62 µg/L	8.886	599.62 ppb	8.886	1.48%
Pb 220.353†	1011.8	63.279 µg/L	0.3795	63.279 ppb	0.3795	0.60%
S 181.975 Axial†	55.1	44.670 µg/L	1.4805	44.670 ppb	1.4805	3.31%
Sb 206.836†	-27.8	-5.1084 µg/L	0.76147	-5.1084 ppb	0.76147	14.91%
Se 196.026†	-52.7	3.93 µg/L	3.763	3.93 ppb	3.763	95.81%
SiO2†	711254.4	77740 µg/L	140.7	77740 ppb	140.7	0.18%
Si 251.611†	2171683.6	35908 µg/L	75.5	35908 ppb	75.5	0.21%
Sn 189.927†	48.1	9.8790 µg/L	0.27295	9.8790 ppb	0.27295	2.76%
Sr 421.552†	21117.7	49.450 µg/L	0.1792	49.450 ppb	0.1792	0.36%
Ti 334.940†	1879240.1	1916.1 µg/L	1.88	1916.1 ppb	1.88	0.10%
Tl 190.801†	-242.3	-3.7109 µg/L	1.85931	-3.7109 ppb	1.85931	50.10%
U 409.014†	-5976.2	-359.21 µg/L	6.079	-359.21 ppb	6.079	1.69%
Concentration less than lower limit for U 409.014.						
V 292.402†	9754.4	40.780 µg/L	0.6472	40.780 ppb	0.6472	1.59%
Zn 213.857†	61917.2	383.21 µg/L	5.084	383.21 ppb	5.084	1.33%

Sequence No.: 113

Sample ID: 248118004|959114|1

Analyst: HSC

Initial Sample Wt:

Dilution:

Autosampler Location: 429

Date Collected: 3/29/2010 23:30:33

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: 248118004|959114|1

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	158556.4	158556.4	109 %		23:31:05
1	Al 396.153Radial†	642477.1	590633.8	128930 µg/L	128930 ppb	23:31:05
1	Ca 317.933Radial†	819073.2	752323.1	44083 µg/L	44083 ppb	23:31:05
1	Fe 238.204 Radial†	1974927.2	1815353.6	120690 µg/L	120690 ppb	23:31:02
1	K 766.490 Radial†	49299.3	43863.7	18018 µg/L	18018 ppb	23:31:05
1	Mg 279.077 IEC†	76846.8	70455.4	28946 µg/L	28946 ppb	23:31:05
1	Na 589.592 Radial†	12140.7	9465.7	1432.3 µg/L	1432.3 ppb	23:31:05
1	Sr 421.552†	151230.1	139297.5	326.13 µg/L	326.13 ppb	23:31:05
1	Sc 361.383	1765974.7	1765974.7	105.57 %		23:31:18
1	Y 371.029	1593014.4	1593014.4	155.78 %		23:31:18
1	Ag 328.068†	3267.5	128.0	-0.8949 µg/L	-0.8949 ppb	23:31:20
1	As 188.979†	74.5	84.8	63.324 µg/L	63.324 ppb	23:31:40
1	B 249.677†	5175.0	1546.2	25.861 µg/L	25.861 ppb	23:31:20
1	Ba 233.527†	179173.4	169892.5	774.68 µg/L	774.68 ppb	23:31:20
1	Be 313.107†	90567.8	86448.1	28.009 µg/L	28.009 ppb	23:31:20
1	Cd 226.502†	1654.3	1661.4	-1.1744 µg/L	-1.1744 ppb	23:31:40
1	Co 228.616†	1982.0	2054.0	22.606 µg/L	22.606 ppb	23:31:40
1	Cr 267.716†	10858.8	10125.5	90.281 µg/L	90.281 ppb	23:31:40
1	Cu 324.752†	21006.4	17472.9	93.975 µg/L	93.975 ppb	23:31:20
1	Mn 257.610†	2910278.1	2756606.8	3765.3 µg/L	3765.3 ppb	23:31:18
1	Mo 202.031†	-180.1	-115.4	1.7180 µg/L	1.7180 ppb	23:31:40
1	Ni 231.604†	7596.6	7236.6	92.565 µg/L	92.565 ppb	23:31:40
1	P 214.914†	7721.5	7234.4	1678.3 µg/L	1678.3 ppb	23:31:40
1	Pb 220.353†	2138.7	1913.4	121.39 µg/L	121.39 ppb	23:31:40
1	S 181.975 Axial†	583.7	458.1	371.12 µg/L	371.12 ppb	23:31:40
1	Sb 206.836†	95.2	3.5	-2.9719 µg/L	-2.9719 ppb	23:31:40
1	Se 196.026†	-88.0	-94.3	4.16 µg/L	4.16 ppb	23:31:40
1	SiO2†	1162788.6	1099849.1	120210 µg/L	120210 ppb	23:31:18
1	Si 251.611†	3547078.2	3359203.0	55544 µg/L	55544 ppb	23:31:18
1	Sn 189.927†	133.7	124.7	11.707 µg/L	11.707 ppb	23:31:40
1	Ti 334.940†	874035.8	827271.8	842.49 µg/L	842.49 ppb	23:31:18
1	Tl 190.801†	-307.2	-170.6	-3.5772 µg/L	-3.5772 ppb	23:31:40
1	U 409.014†	-7921.6	-7024.4	-425.33 µg/L	-425.33 ppb	23:31:18
1	V 292.402†	33399.1	31204.6	153.17 µg/L	153.17 ppb	23:31:20
1	Zn 213.857†	80902.5	76168.5	468.03 µg/L	468.03 ppb	23:31:20
2	Sc RADIAL	159251.6	159251.6	109 %		23:31:09
2	Al 396.153Radial†	644428.1	589841.3	128760 µg/L	128760 ppb	23:31:09
2	Ca 317.933Radial†	820686.4	750512.7	43977 µg/L	43977 ppb	23:31:09
2	Fe 238.204 Radial†	1931908.0	1768055.3	117550 µg/L	117550 ppb	23:31:07
2	K 766.490 Radial†	49325.2	43689.6	17947 µg/L	17947 ppb	23:31:09
2	Mg 279.077 IEC†	76662.6	69978.3	28752 µg/L	28752 ppb	23:31:09
2	Na 589.592 Radial†	12293.5	9556.8	1446.3 µg/L	1446.3 ppb	23:31:09
2	Sr 421.552†	151573.2	139004.6	325.45 µg/L	325.45 ppb	23:31:09
2	Sc 361.383	1767742.8	1767742.8	105.68 %		23:31:43
2	Y 371.029	1597912.4	1597912.4	156.26 %		23:31:43
2	Ag 328.068†	2992.3	-135.5	-1.9130 µg/L	-1.9130 ppb	23:31:45
2	As 188.979†	73.2	83.5	62.073 µg/L	62.073 ppb	23:32:05
2	B 249.677†	5315.1	1673.8	28.003 µg/L	28.003 ppb	23:31:45
2	Ba 233.527†	180665.5	171134.7	780.40 µg/L	780.40 ppb	23:31:45
2	Be 313.107†	91785.1	87514.2	28.360 µg/L	28.360 ppb	23:31:45
2	Cd 226.502†	1690.7	1694.3	-0.6168 µg/L	-0.6168 ppb	23:32:05
2	Co 228.616†	2015.5	2083.8	23.183 µg/L	23.183 ppb	23:32:05
2	Cr 267.716†	10938.7	10190.8	90.722 µg/L	90.722 ppb	23:32:05
2	Cu 324.752†	21076.5	17519.3	93.725 µg/L	93.725 ppb	23:31:45
2	Mn 257.610†	2923739.4	2766587.5	3778.9 µg/L	3778.9 ppb	23:31:43
2	Mo 202.031†	-157.8	-94.1	2.2629 µg/L	2.2629 ppb	23:32:05
2	Ni 231.604†	7609.0	7241.1	92.622 µg/L	92.622 ppb	23:32:05
2	P 214.914†	7755.8	7259.6	1686.4 µg/L	1686.4 ppb	23:32:05
2	Pb 220.353†	2173.0	1943.8	123.32 µg/L	123.32 ppb	23:32:05

2	S 181.975 Axial†	579.9	453.9	367.71 µg/L	367.71 ppb	23:32:05
2	Sb 206.836†	76.5	-14.3	-5.3233 µg/L	-5.3233 ppb	23:32:05
2	Se 196.026†	-86.3	-92.6	3.76 µg/L	3.76 ppb	23:32:05
2	SiO2†	1168103.8	1103777.0	120640 µg/L	120640 ppb	23:31:43
2	Si 251.611†	3565167.9	3372960.2	55771 µg/L	55771 ppb	23:31:43
2	Sn 189.927†	142.7	133.0	12.312 µg/L	12.312 ppb	23:32:05
2	Ti 334.940†	879119.8	831254.5	846.56 µg/L	846.56 ppb	23:31:43
2	Tl 190.801†	-301.9	-165.4	-2.7838 µg/L	-2.7838 ppb	23:32:05
2	U 409.014†	-7699.6	-6806.9	-411.01 µg/L	-411.01 ppb	23:31:43
2	V 292.402†	33681.9	31440.6	154.99 µg/L	154.99 ppb	23:31:45
2	Zn 213.857†	81672.4	76820.3	472.47 µg/L	472.47 ppb	23:31:45
3	Sc RADIAL	158363.0	158363.0	109 %		23:31:13
3	Al 396.153Radial†	642890.1	591735.3	129170 µg/L	129170 ppb	23:31:13
3	Ca 317.933Radial†	821290.4	755283.4	44256 µg/L	44256 ppb	23:31:13
3	Fe 238.204 Radial†	1964608.4	1808073.7	120210 µg/L	120210 ppb	23:31:11
3	K 766.490 Radial†	49635.3	44228.3	18168 µg/L	18168 ppb	23:31:13
3	Mg 279.077 IEC†	76742.9	70446.0	28943 µg/L	28943 ppb	23:31:13
3	Na 589.592 Radial†	12378.2	9697.9	1467.7 µg/L	1467.7 ppb	23:31:13
3	Sr 421.552†	151475.1	139692.7	327.06 µg/L	327.06 ppb	23:31:13
3	Sc 361.383	1778673.4	1778673.4	106.33 %		23:32:08
3	Y 371.029	1606322.8	1606322.8	157.09 %		23:32:08
3	Ag 328.068†	3087.0	-63.9	-1.7027 µg/L	-1.7027 ppb	23:32:10
3	As 188.979†	88.7	97.6	68.584 µg/L	68.584 ppb	23:32:30
3	B 249.677†	5226.1	1559.3	26.080 µg/L	26.080 ppb	23:32:10
3	Ba 233.527†	176413.9	166085.6	757.29 µg/L	757.29 ppb	23:32:10
3	Be 313.107†	88823.8	84195.5	27.283 µg/L	27.283 ppb	23:32:10
3	Cd 226.502†	1653.7	1649.6	-1.2052 µg/L	-1.2052 ppb	23:32:30
3	Co 228.616†	2012.1	2068.9	22.817 µg/L	22.817 ppb	23:32:30
3	Cr 267.716†	10927.2	10116.4	90.164 µg/L	90.164 ppb	23:32:30
3	Cu 324.752†	20521.6	16874.9	91.324 µg/L	91.324 ppb	23:32:10
3	Mn 257.610†	2937328.0	2762365.0	3773.1 µg/L	3773.1 ppb	23:32:08
3	Mo 202.031†	-177.0	-111.3	1.8281 µg/L	1.8281 ppb	23:32:30
3	Ni 231.604†	7601.1	7189.4	91.961 µg/L	91.961 ppb	23:32:30
3	P 214.914†	7736.5	7196.3	1669.6 µg/L	1669.6 ppb	23:32:30
3	Pb 220.353†	2133.8	1894.4	120.26 µg/L	120.26 ppb	23:32:30
3	S 181.975 Axial†	567.0	438.5	355.20 µg/L	355.20 ppb	23:32:30
3	Sb 206.836†	80.7	-10.8	-4.8969 µg/L	-4.8969 ppb	23:32:30
3	Se 196.026†	-73.8	-80.3	9.56 µg/L	9.56 ppb	23:32:30
3	SiO2†	1173240.3	1101814.9	120430 µg/L	120430 ppb	23:32:08
3	Si 251.611†	3580839.7	3366966.8	55672 µg/L	55672 ppb	23:32:08
3	Sn 189.927†	123.5	114.1	10.966 µg/L	10.966 ppb	23:32:30
3	Ti 334.940†	883728.3	830476.4	845.75 µg/L	845.75 ppb	23:32:08
3	Tl 190.801†	-324.0	-184.4	-5.3989 µg/L	-5.3989 ppb	23:32:30
3	U 409.014†	-7584.6	-6653.9	-402.52 µg/L	-402.52 ppb	23:32:08
3	V 292.402†	32773.6	30390.5	148.74 µg/L	148.74 ppb	23:32:10
3	Zn 213.857†	79302.4	74116.5	455.17 µg/L	455.17 ppb	23:32:10

Mean Data: 248118004|959114|1

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1770797.0	105.86 %	0.411			0.39%
Sc RADIAL	158723.7	109 %	0.3			0.29%
Y 371.029	1599083.2	156.38 %	0.658			0.42%
Internal Standard Check greater than the upper limit for Y 371.029. Recovery = 156.4%						
Ag 328.068†	-23.8	-1.5035 µg/L	0.53750	-1.5035 ppb	0.53750	35.75%
Al 396.153Radial†	590736.8	128950 µg/L	207.6	128950 ppb	207.6	0.16%
As 188.979†	88.6	64.661 µg/L	3.4551	64.661 ppb	3.4551	5.34%
B 249.677†	1593.1	26.648 µg/L	1.1781	26.648 ppb	1.1781	4.42%
Ba 233.527†	169037.6	770.79 µg/L	12.033	770.79 ppb	12.033	1.56%
Be 313.107†	86052.6	27.884 µg/L	0.5495	27.884 ppb	0.5495	1.97%
Ca 317.933Radial†	752706.4	44105 µg/L	141.1	44105 ppb	141.1	0.32%
Cd 226.502†	1668.5	-0.9988 µg/L	0.33120	-0.9988 ppb	0.33120	33.16%
Co 228.616†	2068.9	22.869 µg/L	0.2921	22.869 ppb	0.2921	1.28%
Cr 267.716†	10144.2	90.389 µg/L	0.2942	90.389 ppb	0.2942	0.33%
Cu 324.752†	17289.0	93.008 µg/L	1.4637	93.008 ppb	1.4637	1.57%
Fe 238.204 Radial†	1797160.9	119480 µg/L	1693.2	119480 ppb	1693.2	1.42%
K 766.490 Radial†	43927.2	18045 µg/L	113.1	18045 ppb	113.1	0.63%
Mg 279.077 IEC†	70293.2	28880 µg/L	111.0	28880 ppb	111.0	0.38%
Mn 257.610†	2761853.1	3772.4 µg/L	6.85	3772.4 ppb	6.85	0.18%
Mo 202.031†	-106.9	1.9363 µg/L	0.28812	1.9363 ppb	0.28812	14.88%

Na 589.592 Radial†	9573.5	1448.8 µg/L	17.83	1448.8 ppb	17.83	1.23%
Ni 231.604†	7222.4	92.383 µg/L	0.3663	92.383 ppb	0.3663	0.40%
P 214.914†	7230.1	1678.1 µg/L	8.42	1678.1 ppb	8.42	0.50%
Pb 220.353†	1917.2	121.66 µg/L	1.549	121.66 ppb	1.549	1.27%
S 181.975 Axial†	450.1	364.68 µg/L	8.384	364.68 ppb	8.384	2.30%
Sb 206.836†	-7.2	-4.3974 µg/L	1.25275	-4.3974 ppb	1.25275	28.49%
Se 196.026†	-89.0	5.82 µg/L	3.239	5.82 ppb	3.239	55.61%
SiO2†	1101813.6	120430 µg/L	214.7	120430 ppb	214.7	0.18%
Concentration greater than upper limit for SiO2.						
Si 251.611†	3366376.7	55663 µg/L	114.0	55663 ppb	114.0	0.20%
Concentration greater than upper limit for Si 251.611.						
Sn 189.927†	123.9	11.662 µg/L	0.6740	11.662 ppb	0.6740	5.78%
Sr 421.552†	139331.6	326.21 µg/L	0.808	326.21 ppb	0.808	0.25%
Ti 334.940†	829667.6	844.93 µg/L	2.154	844.93 ppb	2.154	0.25%
Tl 190.801†	-173.5	-3.9200 µg/L	1.34081	-3.9200 ppb	1.34081	34.20%
U 409.014†	-6828.4	-412.95 µg/L	11.525	-412.95 ppb	11.525	2.79%
Concentration less than lower limit for U 409.014.						
V 292.402†	31011.9	152.30 µg/L	3.213	152.30 ppb	3.213	2.11%
Zn 213.857†	75701.7	465.22 µg/L	8.981	465.22 ppb	8.981	1.93%
Internal Standard Check failed. Continue with analysis.						

Sequence No.: 114

Sample ID: 248118005|959114|1

Analyst: HSC

Initial Sample Wt:

Dilution:

Autosampler Location: 430

Date Collected: 3/29/2010 23:32:37

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: 248118005|959114|1

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	154520.2	154520.2	106 %		23:33:06
1	Al 396.153Radial†	79758.5	75265.6	16429 µg/L	16429 ppb	23:33:06
1	Ca 317.933Radial†	54522.9	50813.6	2977.5 µg/L	2977.5 ppb	23:33:08
1	Fe 238.204 Radial†	1195928.2	1127969.7	74991 µg/L	74991 ppb	23:33:06
1	K 766.490 Radial†	14630.8	12345.8	5077.5 µg/L	5077.5 ppb	23:33:08
1	Mg 279.077 IEC†	5171.3	4691.2	1870.1 µg/L	1870.1 ppb	23:33:08
1	Na 589.592 Radial†	28523.6	25210.7	3853.0 µg/L	3853.0 ppb	23:33:08
1	Sr 421.552†	14009.6	13492.9	31.600 µg/L	31.600 ppb	23:33:08
1	Sc 361.383	1743284.8	1743284.8	104.22 %		23:33:34
1	Y 371.029	1492078.5	1492078.5	145.91 %		23:33:34
1	Ag 328.068†	2807.0	-273.6	-3.3362 µg/L	-3.3362 ppb	23:33:37
1	As 188.979†	22.8	36.1	32.177 µg/L	32.177 ppb	23:33:57
1	B 249.677†	3381.0	-111.4	-1.9081 µg/L	-1.9081 ppb	23:33:37
1	Ba 233.527†	74361.5	71528.9	325.84 µg/L	325.84 ppb	23:33:37
1	Be 313.107†	30803.5	30217.7	9.6908 µg/L	9.6908 ppb	23:33:37
1	Cd 226.502†	1027.1	1080.0	-0.4195 µg/L	-0.4195 ppb	23:33:37
1	Co 228.616†	625.8	777.1	7.0538 µg/L	7.0538 ppb	23:33:57
1	Cr 267.716†	3226.3	2935.5	26.737 µg/L	26.737 ppb	23:33:37
1	Cu 324.752†	6696.6	4000.8	27.974 µg/L	27.974 ppb	23:33:37
1	Mn 257.610†	4440066.7	4260400.1	5821.3 µg/L	5821.3 ppb	23:33:34
1	Mo 202.031†	169.9	218.2	9.9043 µg/L	9.9043 ppb	23:33:37
1	Ni 231.604†	1490.0	1470.6	18.811 µg/L	18.811 ppb	23:33:57
1	P 214.914†	2940.7	2742.2	609.13 µg/L	609.13 ppb	23:33:57
1	Pb 220.353†	1466.4	1294.7	80.449 µg/L	80.449 ppb	23:33:57
1	S 181.975 Axial†	112.3	13.0	10.573 µg/L	10.573 ppb	23:33:57
1	Sb 206.836†	59.9	-29.2	-5.1840 µg/L	-5.1840 ppb	23:33:57
1	Se 196.026†	-38.4	-47.8	6.66 µg/L	6.66 ppb	23:33:57
1	SiO2†	645279.5	617607.1	67505 µg/L	67505 ppb	23:33:34
1	Si 251.611†	1977961.6	1897282.9	31371 µg/L	31371 ppb	23:33:34
1	Sn 189.927†	70.6	65.7	12.459 µg/L	12.459 ppb	23:33:57
1	Ti 334.940†	2359890.2	2263803.7	2308.5 µg/L	2308.5 ppb	23:33:34
1	Tl 190.801†	-486.4	-346.5	-8.0117 µg/L	-8.0117 ppb	23:33:57
1	U 409.014†	-8623.0	-7795.1	-458.24 µg/L	-458.24 ppb	23:33:34
1	V 292.402†	9095.8	8296.0	31.812 µg/L	31.812 ppb	23:33:37
1	Zn 213.857†	91207.2	87053.7	541.13 µg/L	541.13 ppb	23:33:37
2	Sc RADIAL	152361.4	152361.4	105 %		23:33:10
2	Al 396.153Radial†	79273.2	75867.4	16561 µg/L	16561 ppb	23:33:10
2	Ca 317.933Radial†	54329.0	51356.8	3009.3 µg/L	3009.3 ppb	23:33:12
2	Fe 238.204 Radial†	1184354.2	1132881.2	75318 µg/L	75318 ppb	23:33:10
2	K 766.490 Radial†	14561.9	12475.4	5130.8 µg/L	5130.8 ppb	23:33:12
2	Mg 279.077 IEC†	5138.9	4729.4	1885.5 µg/L	1885.5 ppb	23:33:12
2	Na 589.592 Radial†	28571.0	25637.3	3918.3 µg/L	3918.3 ppb	23:33:12
2	Sr 421.552†	13915.3	13589.9	31.828 µg/L	31.828 ppb	23:33:12
2	Sc 361.383	1742349.7	1742349.7	104.16 %		23:33:59
2	Y 371.029	1490021.7	1490021.7	145.71 %		23:33:59
2	Ag 328.068†	3014.5	-72.9	-2.5157 µg/L	-2.5157 ppb	23:34:02
2	As 188.979†	19.0	32.5	30.704 µg/L	30.704 ppb	23:34:22
2	B 249.677†	3196.9	-286.5	-4.8469 µg/L	-4.8469 ppb	23:34:02
2	Ba 233.527†	75305.7	72473.6	330.15 µg/L	330.15 ppb	23:34:02
2	Be 313.107†	30887.6	30314.3	9.7243 µg/L	9.7243 ppb	23:34:02
2	Cd 226.502†	1132.2	1181.4	0.2467 µg/L	0.2467 ppb	23:34:02
2	Co 228.616†	637.3	788.4	7.1957 µg/L	7.1957 ppb	23:34:22
2	Cr 267.716†	3069.8	2787.0	25.471 µg/L	25.471 ppb	23:34:02
2	Cu 324.752†	6618.7	3929.5	27.717 µg/L	27.717 ppb	23:34:02
2	Mn 257.610†	4423739.2	4247011.2	5803.0 µg/L	5803.0 ppb	23:33:59
2	Mo 202.031†	159.9	208.7	9.6184 µg/L	9.6184 ppb	23:34:02
2	Ni 231.604†	1476.1	1458.1	18.651 µg/L	18.651 ppb	23:34:22
2	P 214.914†	2928.4	2731.9	606.49 µg/L	606.49 ppb	23:34:22
2	Pb 220.353†	1472.8	1301.6	80.852 µg/L	80.852 ppb	23:34:22

2	S 181.975 Axial†	99.3	0.5	0.4704 µg/L	0.4704 ppb	23:34:22
2	Sb 206.836†	64.2	-25.0	-4.6183 µg/L	-4.6183 ppb	23:34:22
2	Se 196.026†	-38.2	-47.6	6.85 µg/L	6.85 ppb	23:34:22
2	SiO2†	642737.2	615498.7	67274 µg/L	67274 ppb	23:33:59
2	Si 251.611†	1971567.2	1892162.5	31287 µg/L	31287 ppb	23:33:59
2	Sn 189.927†	71.0	66.1	12.467 µg/L	12.467 ppb	23:34:22
2	Ti 334.940†	2352871.4	2258280.6	2302.8 µg/L	2302.8 ppb	23:33:59
2	Tl 190.801†	-460.5	-321.8	-4.8142 µg/L	-4.8142 ppb	23:34:22
2	U 409.014†	-8503.1	-7684.4	-451.61 µg/L	-451.61 ppb	23:33:59
2	V 292.402†	9020.0	8228.0	31.384 µg/L	31.384 ppb	23:34:02
2	Zn 213.857†	92616.7	88453.9	549.91 µg/L	549.91 ppb	23:34:02
3	Sc RADIAL	152581.8	152581.8	105 %		23:33:14
3	Al 396.153Radial†	79043.7	75538.6	16489 µg/L	16489 ppb	23:33:14
3	Ca 317.933Radial†	53889.5	50861.9	2980.3 µg/L	2980.3 ppb	23:33:16
3	Fe 238.204 Radial†	1183208.1	1130149.9	75136 µg/L	75136 ppb	23:33:14
3	K 766.490 Radial†	14535.6	12430.2	5112.3 µg/L	5112.3 ppb	23:33:16
3	Mg 279.077 IEC†	5080.2	4666.2	1859.7 µg/L	1859.7 ppb	23:33:16
3	Na 589.592 Radial†	28170.6	25215.4	3853.7 µg/L	3853.7 ppb	23:33:16
3	Sr 421.552†	13785.3	13446.4	31.491 µg/L	31.491 ppb	23:33:16
3	Sc 361.383	1747994.6	1747994.6	104.50 %		23:34:24
3	Y 371.029	1492452.6	1492452.6	145.95 %		23:34:24
3	Ag 328.068†	3167.0	63.7	-1.9394 µg/L	-1.9394 ppb	23:34:26
3	As 188.979†	24.9	38.1	33.021 µg/L	33.021 ppb	23:34:47
3	B 249.677†	3424.6	-78.5	-1.3550 µg/L	-1.3550 ppb	23:34:26
3	Ba 233.527†	76221.7	73116.8	333.09 µg/L	333.09 ppb	23:34:26
3	Be 313.107†	31267.9	30582.5	9.8102 µg/L	9.8102 ppb	23:34:26
3	Cd 226.502†	1136.2	1181.7	0.2680 µg/L	0.2680 ppb	23:34:26
3	Co 228.616†	637.9	787.0	7.1893 µg/L	7.1893 ppb	23:34:47
3	Cr 267.716†	3166.9	2870.4	26.192 µg/L	26.192 ppb	23:34:26
3	Cu 324.752†	6766.3	4050.3	28.212 µg/L	28.212 ppb	23:34:26
3	Mn 257.610†	4421815.6	4231455.0	5781.8 µg/L	5781.8 ppb	23:34:24
3	Mo 202.031†	194.3	241.1	10.634 µg/L	10.634 ppb	23:34:26
3	Ni 231.604†	1480.4	1457.6	18.645 µg/L	18.645 ppb	23:34:47
3	P 214.914†	2933.4	2727.6	605.55 µg/L	605.55 ppb	23:34:47
3	Pb 220.353†	1510.4	1333.0	82.748 µg/L	82.748 ppb	23:34:47
3	S 181.975 Axial†	113.4	13.6	11.121 µg/L	11.121 ppb	23:34:47
3	Sb 206.836†	51.5	-37.3	-6.2696 µg/L	-6.2696 ppb	23:34:47
3	Se 196.026†	-46.9	-55.8	3.55 µg/L	3.55 ppb	23:34:47
3	SiO2†	643453.5	614191.4	67131 µg/L	67131 ppb	23:34:24
3	Si 251.611†	1970691.2	1885211.6	31172 µg/L	31172 ppb	23:34:24
3	Sn 189.927†	57.9	53.3	11.523 µg/L	11.523 ppb	23:34:47
3	Ti 334.940†	2350006.9	2248244.5	2292.6 µg/L	2292.6 ppb	23:34:24
3	Tl 190.801†	-467.2	-326.8	-5.6229 µg/L	-5.6229 ppb	23:34:47
3	U 409.014†	-8603.9	-7754.6	-455.95 µg/L	-455.95 ppb	23:34:24
3	V 292.402†	9356.2	8521.7	33.063 µg/L	33.063 ppb	23:34:26
3	Zn 213.857†	93716.7	89219.4	554.74 µg/L	554.74 ppb	23:34:26

Mean Data: 248118005|959114|1

Analyte	Mean Corrected Intensity	Conc. Units	Calib.	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1744543.0	104.29 %		0.181			0.17%
Sc RADIAL	153154.5	105 %		0.8			0.78%
Y 371.029	1491517.6	145.86 %		0.128			0.09%
Ag 328.068†	-94.3	-2.5971 µg/L		0.70192	-2.5971 ppb	0.70192	27.03%
Al 396.153Radial†	75557.2	16493 µg/L		65.8	16493 ppb	65.8	0.40%
As 188.979†	35.5	31.967 µg/L		1.1722	31.967 ppb	1.1722	3.67%
B 249.677†	-158.8	-2.7034 µg/L		1.87688	-2.7034 ppb	1.87688	69.43%
Ba 233.527†	72373.1	329.69 µg/L		3.648	329.69 ppb	3.648	1.11%
Be 313.107†	30371.5	9.7418 µg/L		0.06163	9.7418 ppb	0.06163	0.63%
Ca 317.933Radial†	51010.8	2989.0 µg/L		17.62	2989.0 ppb	17.62	0.59%
Cd 226.502†	1147.7	0.0317 µg/L		0.39093	0.0317 ppb	0.39093	>999.9%
Co 228.616†	784.2	7.1463 µg/L		0.08012	7.1463 ppb	0.08012	1.12%
Cr 267.716†	2864.3	26.133 µg/L		0.6350	26.133 ppb	0.6350	2.43%
Cu 324.752†	3993.5	27.968 µg/L		0.2472	27.968 ppb	0.2472	0.88%
Fe 238.204 Radial†	1130333.6	75149 µg/L		163.6	75149 ppb	163.6	0.22%
K 766.490 Radial†	12417.1	5106.9 µg/L		27.07	5106.9 ppb	27.07	0.53%
Mg 279.077 IEC†	4695.6	1871.8 µg/L		13.02	1871.8 ppb	13.02	0.70%
Mn 257.610†	4246288.8	5802.0 µg/L		19.79	5802.0 ppb	19.79	0.34%
Mo 202.031†	222.7	10.052 µg/L		0.5237	10.052 ppb	0.5237	5.21%
Na 589.592 Radial†	25354.5	3875.0 µg/L		37.46	3875.0 ppb	37.46	0.97%

Ni 231.604†	1462.1	18.702 µg/L	0.0944	18.702 ppb	0.0944	0.50%
P 214.914†	2733.9	607.05 µg/L	1.857	607.05 ppb	1.857	0.31%
Pb 220.353†	1309.8	81.350 µg/L	1.2275	81.350 ppb	1.2275	1.51%
S 181.975 Axial†	9.0	7.3880 µg/L	5.99705	7.3880 ppb	5.99705	81.17%
Sb 206.836†	-30.5	-5.3573 µg/L	0.83918	-5.3573 ppb	0.83918	15.66%
Se 196.026†	-50.4	5.69 µg/L	1.855	5.69 ppb	1.855	32.64%
SiO2†	615765.7	67303 µg/L	188.4	67303 ppb	188.4	0.28%
Si 251.611†	1891552.3	31276 µg/L	100.2	31276 ppb	100.2	0.32%
Sn 189.927†	61.7	12.150 µg/L	0.5425	12.150 ppb	0.5425	4.46%
Sr 421.552†	13509.7	31.640 µg/L	0.1715	31.640 ppb	0.1715	0.54%
Ti 334.940†	2256776.3	2301.3 µg/L	8.04	2301.3 ppb	8.04	0.35%
Tl 190.801†	-331.7	-6.1496 µg/L	1.66251	-6.1496 ppb	1.66251	27.03%
U 409.014†	-7744.7	-455.27 µg/L	3.367	-455.27 ppb	3.367	0.74%
Concentration less than lower limit for U 409.014.						
V 292.402†	8348.6	32.087 µg/L	0.8721	32.087 ppb	0.8721	2.72%
Zn 213.857†	88242.3	548.59 µg/L	6.902	548.59 ppb	6.902	1.26%

Sequence No.: 115

Sample ID: 248118006|959114|1

Analyst: HSC

Initial Sample Wt:

Dilution:

Autosampler Location: 431

Date Collected: 3/29/2010 23:34:55

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: 248118006|959114|1

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	155017.7	155017.7	106 %		23:35:26
1	Al 396.153Radial†	174786.7	164373.7	35880 µg/L	35880 ppb	23:35:26
1	Ca 317.933Radial†	141635.3	132555.3	7767.2 µg/L	7767.2 ppb	23:35:26
1	Fe 238.204 Radial†	1624772.4	1527566.9	101560 µg/L	101560 ppb	23:35:24
1	K 766.490 Radial†	17119.5	14641.5	6017.0 µg/L	6017.0 ppb	23:35:26
1	Mg 279.077 IEC†	20203.4	18809.4	7668.4 µg/L	7668.4 ppb	23:35:26
1	Na 589.592 Radial†	26864.5	23564.4	3600.3 µg/L	3600.3 ppb	23:35:26
1	Sr 421.552†	39619.5	37529.9	87.899 µg/L	87.899 ppb	23:35:26
1	Sc 361.383	1757854.0	1757854.0	105.09 %		23:35:39
1	Y 371.029	1415789.6	1415789.6	138.45 %		23:35:39
1	Ag 328.068†	2789.9	-312.2	-2.5582 µg/L	-2.5582 ppb	23:35:39
1	As 188.979†	12.9	26.5	34.659 µg/L	34.659 ppb	23:35:59
1	B 249.677†	3511.7	-13.9	-0.2810 µg/L	-0.2810 ppb	23:35:39
1	Ba 233.527†	147105.8	140161.0	639.06 µg/L	639.06 ppb	23:35:39
1	Be 313.107†	34586.2	33572.4	10.795 µg/L	10.795 ppb	23:35:39
1	Cd 226.502†	1458.4	1482.2	-0.4176 µg/L	-0.4176 ppb	23:35:59
1	Co 228.616†	860.1	995.1	8.9707 µg/L	8.9707 ppb	23:35:59
1	Cr 267.716†	10144.2	9493.0	84.453 µg/L	84.453 ppb	23:35:59
1	Cu 324.752†	8456.4	5622.2	39.085 µg/L	39.085 ppb	23:35:39
1	Mn 257.610†	2769877.9	2635736.7	3601.0 µg/L	3601.0 ppb	23:35:39
1	Mo 202.031†	222.5	267.0	12.616 µg/L	12.616 ppb	23:35:59
1	Ni 231.604†	4586.8	4405.7	56.354 µg/L	56.354 ppb	23:35:59
1	P 214.914†	3721.2	3461.5	767.54 µg/L	767.54 ppb	23:35:59
1	Pb 220.353†	1007.9	846.7	54.119 µg/L	54.119 ppb	23:35:59
1	S 181.975 Axial†	933.1	793.1	642.66 µg/L	642.66 ppb	23:35:59
1	Sb 206.836†	86.7	-4.1	-3.0185 µg/L	-3.0185 ppb	23:35:59
1	Se 196.026†	-74.0	-81.4	2.63 µg/L	2.63 ppb	23:35:59
1	SiO2†	847580.5	804985.1	87985 µg/L	87985 ppb	23:35:39
1	Si 251.611†	2579195.9	2453687.3	40571 µg/L	40571 ppb	23:35:39
1	Sn 189.927†	52.0	47.5	12.393 µg/L	12.393 ppb	23:35:59
1	Ti 334.940†	2756033.7	2622006.2	2673.3 µg/L	2673.3 ppb	23:35:39
1	Tl 190.801†	-443.8	-302.0	-3.7819 µg/L	-3.7819 ppb	23:35:59
1	U 409.014†	-7986.4	-7120.8	-434.22 µg/L	-434.22 ppb	23:35:39
1	V 292.402†	17884.7	16587.3	73.529 µg/L	73.529 ppb	23:35:59
1	Zn 213.857†	86613.1	81956.6	506.62 µg/L	506.62 ppb	23:35:39
2	Sc RADIAL	155147.2	155147.2	106 %		23:35:31
2	Al 396.153Radial†	174606.7	164067.4	35814 µg/L	35814 ppb	23:35:31
2	Ca 317.933Radial†	141680.8	132486.8	7763.2 µg/L	7763.2 ppb	23:35:31
2	Fe 238.204 Radial†	1625305.7	1526792.2	101510 µg/L	101510 ppb	23:35:28
2	K 766.490 Radial†	17081.1	14591.9	5996.6 µg/L	5996.6 ppb	23:35:31
2	Mg 279.077 IEC†	20228.6	18817.2	7671.7 µg/L	7671.7 ppb	23:35:31
2	Na 589.592 Radial†	26766.0	23450.8	3582.9 µg/L	3582.9 ppb	23:35:31
2	Sr 421.552†	39471.1	37359.4	87.500 µg/L	87.500 ppb	23:35:31
2	Sc 361.383	1761128.9	1761128.9	105.28 %		23:36:02
2	Y 371.029	1419225.4	1419225.4	138.79 %		23:36:02
2	Ag 328.068†	3343.4	208.6	-0.4520 µg/L	-0.4520 ppb	23:36:02
2	As 188.979†	9.3	23.1	33.199 µg/L	33.199 ppb	23:36:22
2	B 249.677†	3710.5	168.6	2.7828 µg/L	2.7828 ppb	23:36:02
2	Ba 233.527†	147314.1	140098.5	638.77 µg/L	638.77 ppb	23:36:02
2	Be 313.107†	34297.1	33236.5	10.685 µg/L	10.685 ppb	23:36:02
2	Cd 226.502†	1480.3	1500.4	-0.2860 µg/L	-0.2860 ppb	23:36:22
2	Co 228.616†	878.6	1011.1	9.1925 µg/L	9.1925 ppb	23:36:22
2	Cr 267.716†	10092.6	9426.0	83.876 µg/L	83.876 ppb	23:36:22
2	Cu 324.752†	8638.1	5779.9	39.761 µg/L	39.761 ppb	23:36:02
2	Mn 257.610†	2776504.8	2637129.9	3602.9 µg/L	3602.9 ppb	23:36:02
2	Mo 202.031†	199.8	245.0	11.920 µg/L	11.920 ppb	23:36:22
2	Ni 231.604†	4631.2	4439.8	56.790 µg/L	56.790 ppb	23:36:22
2	P 214.914†	3710.6	3444.9	763.56 µg/L	763.56 ppb	23:36:22
2	Pb 220.353†	1032.0	867.8	55.398 µg/L	55.398 ppb	23:36:22

2	S 181.975 Axial†	930.6	789.1	639.38 µg/L	639.38 ppb	23:36:22
2	Sb 206.836†	65.2	-24.7	-5.7969 µg/L	-5.7969 ppb	23:36:22
2	Se 196.026†	-59.7	-67.7	8.03 µg/L	8.03 ppb	23:36:22
2	SiO2†	849425.2	805237.4	88013 µg/L	88013 ppb	23:36:02
2	Si 251.611†	2584888.0	2454529.9	40585 µg/L	40585 ppb	23:36:02
2	Sn 189.927†	40.6	36.6	11.630 µg/L	11.630 ppb	23:36:22
2	Ti 334.940†	2765666.9	2626279.3	2677.7 µg/L	2677.7 ppb	23:36:02
2	Tl 190.801†	-430.2	-288.3	-1.9011 µg/L	-1.9011 ppb	23:36:22
2	U 409.014†	-8031.6	-7149.6	-436.00 µg/L	-436.00 ppb	23:36:02
2	V 292.402†	17840.4	16513.5	73.113 µg/L	73.113 ppb	23:36:22
2	Zn 213.857†	86612.5	81802.8	505.65 µg/L	505.65 ppb	23:36:02
3	Sc RADIAL	157457.1	157457.1	108 %		23:35:35
3	Al 396.153Radial†	177346.0	164196.8	35842 µg/L	35842 ppb	23:35:35
3	Ca 317.933Radial†	144218.6	132883.4	7786.4 µg/L	7786.4 ppb	23:35:35
3	Fe 238.204 Radial†	1612428.6	1492472.3	99225 µg/L	99225 ppb	23:35:33
3	K 766.490 Radial†	17567.1	14806.5	6084.9 µg/L	6084.9 ppb	23:35:35
3	Mg 279.077 IEC†	20595.1	18877.7	7698.6 µg/L	7698.6 ppb	23:35:35
3	Na 589.592 Radial†	27265.1	23543.9	3597.1 µg/L	3597.1 ppb	23:35:35
3	Sr 421.552†	40117.1	37413.4	87.626 µg/L	87.626 ppb	23:35:35
3	Sc 361.383	1771483.3	1771483.3	105.90 %		23:36:25
3	Y 371.029	1426243.6	1426243.6	139.47 %		23:36:25
3	Ag 328.068†	3075.2	-63.2	-1.5401 µg/L	-1.5401 ppb	23:36:25
3	As 188.979†	11.5	25.1	33.526 µg/L	33.526 ppb	23:36:45
3	B 249.677†	3638.2	79.8	1.2911 µg/L	1.2911 ppb	23:36:25
3	Ba 233.527†	148107.6	140029.9	638.49 µg/L	638.49 ppb	23:36:25
3	Be 313.107†	34505.8	33243.2	10.688 µg/L	10.688 ppb	23:36:25
3	Cd 226.502†	1476.0	1488.1	-0.1310 µg/L	-0.1310 ppb	23:36:45
3	Co 228.616†	890.9	1017.9	9.4042 µg/L	9.4042 ppb	23:36:45
3	Cr 267.716†	10147.6	9421.9	83.759 µg/L	83.759 ppb	23:36:45
3	Cu 324.752†	8670.2	5762.2	39.354 µg/L	39.354 ppb	23:36:25
3	Mn 257.610†	2796465.2	2640563.2	3607.6 µg/L	3607.6 ppb	23:36:25
3	Mo 202.031†	222.2	265.1	12.464 µg/L	12.464 ppb	23:36:45
3	Ni 231.604†	4653.8	4435.4	56.734 µg/L	56.734 ppb	23:36:45
3	P 214.914†	3743.1	3454.9	767.53 µg/L	767.53 ppb	23:36:45
3	Pb 220.353†	1044.4	873.8	55.840 µg/L	55.840 ppb	23:36:45
3	S 181.975 Axial†	927.7	781.2	633.00 µg/L	633.00 ppb	23:36:45
3	Sb 206.836†	67.3	-23.1	-5.5401 µg/L	-5.5401 ppb	23:36:45
3	Se 196.026†	-67.2	-74.3	4.60 µg/L	4.60 ppb	23:36:45
3	SiO2†	855210.4	805984.4	88094 µg/L	88094 ppb	23:36:25
3	Si 251.611†	2604224.6	2458438.2	40650 µg/L	40650 ppb	23:36:25
3	Sn 189.927†	49.7	44.9	12.223 µg/L	12.223 ppb	23:36:45
3	Ti 334.940†	2780898.1	2625307.2	2676.7 µg/L	2676.7 ppb	23:36:25
3	Tl 190.801†	-472.7	-326.1	-6.9641 µg/L	-6.9641 ppb	23:36:45
3	U 409.014†	-8058.4	-7130.3	-434.25 µg/L	-434.25 ppb	23:36:25
3	V 292.402†	17958.6	16526.1	73.554 µg/L	73.554 ppb	23:36:45
3	Zn 213.857†	87474.4	82135.8	507.99 µg/L	507.99 ppb	23:36:25

Mean Data: 248118006|959114|1

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1763488.8	105.42 %	0.425			0.40%
Sc RADIAL	155874.0	107 %	0.9			0.88%
Y 371.029	1420419.5	138.91 %	0.521			0.38%
Ag 328.068†	-55.6	-1.5167 µg/L	1.05328	-1.5167 ppb	1.05328	69.44%
Al 396.153Radial†	164212.6	35845 µg/L	33.6	35845 ppb	33.6	0.09%
As 188.979†	24.9	33.795 µg/L	0.7666	33.795 ppb	0.7666	2.27%
B 249.677†	78.2	1.2643 µg/L	1.53207	1.2643 ppb	1.53207	121.18%
Ba 233.527†	140096.5	638.77 µg/L	0.284	638.77 ppb	0.284	0.04%
Be 313.107†	33350.7	10.723 µg/L	0.0627	10.723 ppb	0.0627	0.58%
Ca 317.933Radial†	132641.9	7772.2 µg/L	12.42	7772.2 ppb	12.42	0.16%
Cd 226.502†	1490.3	-0.2782 µg/L	0.14346	-0.2782 ppb	0.14346	51.57%
Co 228.616†	1008.0	9.1892 µg/L	0.21676	9.1892 ppb	0.21676	2.36%
Cr 267.716†	9447.0	84.029 µg/L	0.3712	84.029 ppb	0.3712	0.44%
Cu 324.752†	5721.4	39.400 µg/L	0.3406	39.400 ppb	0.3406	0.86%
Fe 238.204 Radial†	1515610.5	100760 µg/L	1332.5	100760 ppb	1332.5	1.32%
K 766.490 Radial†	14680.0	6032.8 µg/L	46.23	6032.8 ppb	46.23	0.77%
Mg 279.077 IEC†	18834.8	7679.6 µg/L	16.55	7679.6 ppb	16.55	0.22%
Mn 257.610†	2637809.9	3603.8 µg/L	3.40	3603.8 ppb	3.40	0.09%
Mo 202.031†	259.0	12.333 µg/L	0.3660	12.333 ppb	0.3660	2.97%
Na 589.592 Radial†	23519.7	3593.4 µg/L	9.24	3593.4 ppb	9.24	0.26%

Ni 231.604†	4427.0	56.626 µg/L	0.2374	56.626 ppb	0.2374	0.42%
P 214.914†	3453.8	766.21 µg/L	2.296	766.21 ppb	2.296	0.30%
Pb 220.353†	862.7	55.119 µg/L	0.8936	55.119 ppb	0.8936	1.62%
S 181.975 Axial†	787.8	638.35 µg/L	4.909	638.35 ppb	4.909	0.77%
Sb 206.836†	-17.3	-4.7852 µg/L	1.53534	-4.7852 ppb	1.53534	32.09%
Se 196.026†	-74.5	5.09 µg/L	2.733	5.09 ppb	2.733	53.75%
SiO2†	805402.3	88031 µg/L	56.8	88031 ppb	56.8	0.06%
Si 251.611†	2455551.8	40602 µg/L	41.9	40602 ppb	41.9	0.10%
Sn 189.927†	43.0	12.082 µg/L	0.4007	12.082 ppb	0.4007	3.32%
Sr 421.552†	37434.2	87.675 µg/L	0.2042	87.675 ppb	0.2042	0.23%
Ti 334.940†	2624530.9	2675.9 µg/L	2.28	2675.9 ppb	2.28	0.09%
Tl 190.801†	-305.5	-4.2157 µg/L	2.55923	-4.2157 ppb	2.55923	60.71%
U 409.014†	-7133.5	-434.82 µg/L	1.017	-434.82 ppb	1.017	0.23%
Concentration less than lower limit for U 409.014.						
V 292.402†	16542.3	73.398 µg/L	0.2477	73.398 ppb	0.2477	0.34%
Zn 213.857†	81965.1	506.75 µg/L	1.174	506.75 ppb	1.174	0.23%

Sequence No.: 116

Sample ID: 248118007|959114|1

Analyst: HSC

Initial Sample Wt:

Dilution:

Autosampler Location: 432

Date Collected: 3/29/2010 23:36:53

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: 248118007|959114|1

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	156050.6	156050.6	107 %		23:37:24
1	Al 396.153Radial†	372507.7	347961.1	75956 µg/L	75956 ppb	23:37:22
1	Ca 317.933Radial†	317127.7	295587.1	17320 µg/L	17320 ppb	23:37:24
1	Fe 238.204 Radial†	1956153.8	1826971.4	121460 µg/L	121460 ppb	23:37:22
1	K 766.490 Radial†	44797.3	40386.5	16604 µg/L	16604 ppb	23:37:24
1	Mg 279.077 IEC†	50013.7	46527.0	19079 µg/L	19079 ppb	23:37:24
1	Na 589.592 Radial†	36707.0	32590.3	4972.0 µg/L	4972.0 ppb	23:37:24
1	Sr 421.552†	99364.4	93086.2	218.03 µg/L	218.03 ppb	23:37:24
1	Sc 361.383	1765259.5	1765259.5	105.53 %		23:37:37
1	Y 371.029	1256899.6	1256899.6	122.91 %		23:37:37
1	Ag 328.068†	3207.3	72.2	-0.1955 µg/L	-0.1955 ppb	23:37:37
1	As 188.979†	20.0	33.2	41.798 µg/L	41.798 ppb	23:37:57
1	B 249.677†	4276.8	697.1	11.524 µg/L	11.524 ppb	23:37:37
1	Ba 233.527†	214371.8	203315.5	927.37 µg/L	927.37 ppb	23:37:37
1	Be 313.107†	37842.5	36519.9	11.768 µg/L	11.768 ppb	23:37:37
1	Cd 226.502†	1780.8	1781.9	-0.4325 µg/L	-0.4325 ppb	23:37:57
1	Co 228.616†	3783.2	3761.6	46.092 µg/L	46.092 ppb	23:37:57
1	Cr 267.716†	8997.9	8366.2	75.255 µg/L	75.255 ppb	23:37:57
1	Cu 324.752†	14148.5	10982.4	65.651 µg/L	65.651 ppb	23:37:37
1	Mn 257.610†	3040617.9	2881234.6	3936.0 µg/L	3936.0 ppb	23:37:37
1	Mo 202.031†	-79.9	-20.5	4.5719 µg/L	4.5719 ppb	23:37:57
1	Ni 231.604†	6157.6	5875.9	75.160 µg/L	75.160 ppb	23:37:57
1	P 214.914†	4981.3	4640.7	1045.1 µg/L	1045.1 ppb	23:37:57
1	Pb 220.353†	1792.5	1586.2	100.21 µg/L	100.21 ppb	23:37:57
1	S 181.975 Axial†	763.8	629.0	509.60 µg/L	509.60 ppb	23:37:57
1	Sb 206.836†	70.7	-19.7	-5.4562 µg/L	-5.4562 ppb	23:37:57
1	Se 196.026†	-82.1	-88.7	6.68 µg/L	6.68 ppb	23:37:57
1	SiO2†	1056232.1	999321.4	109230 µg/L	109230 ppb	23:37:37
1	Si 251.611†	3209813.3	3040969.1	50282 µg/L	50282 ppb	23:37:37
1	Sn 189.927†	62.7	57.4	11.901 µg/L	11.901 ppb	23:37:57
1	Ti 334.940†	2401224.0	2274783.2	2318.6 µg/L	2318.6 ppb	23:37:37
1	Tl 190.801†	-415.9	-273.8	-2.1209 µg/L	-2.1209 ppb	23:37:57
1	U 409.014†	-7283.5	-6422.8	-387.16 µg/L	-387.16 ppb	23:37:37
1	V 292.402†	37338.6	34950.6	172.45 µg/L	172.45 ppb	23:37:37
1	Zn 213.857†	63465.2	59675.7	364.45 µg/L	364.45 ppb	23:37:37
2	Sc RADIAL	154463.8	154463.8	106 %		23:37:29
2	Al 396.153Radial†	371034.4	350145.2	76432 µg/L	76432 ppb	23:37:27
2	Ca 317.933Radial†	311365.1	293192.3	17180 µg/L	17180 ppb	23:37:29
2	Fe 238.204 Radial†	1945538.3	1835724.3	122050 µg/L	122050 ppb	23:37:27
2	K 766.490 Radial†	44086.7	40145.8	16505 µg/L	16505 ppb	23:37:29
2	Mg 279.077 IEC†	49044.4	46092.3	18900 µg/L	18900 ppb	23:37:29
2	Na 589.592 Radial†	36295.3	32554.0	4966.5 µg/L	4966.5 ppb	23:37:29
2	Sr 421.552†	97934.5	92690.4	217.11 µg/L	217.11 ppb	23:37:29
2	Sc 361.383	1769577.2	1769577.2	105.79 %		23:38:00
2	Y 371.029	1258615.6	1258615.6	123.08 %		23:38:00
2	Ag 328.068†	2822.6	-298.8	-1.7291 µg/L	-1.7291 ppb	23:38:00
2	As 188.979†	25.4	38.3	44.061 µg/L	44.061 ppb	23:38:20
2	B 249.677†	4357.4	763.3	12.636 µg/L	12.636 ppb	23:38:00
2	Ba 233.527†	214488.1	202929.8	925.60 µg/L	925.60 ppb	23:38:00
2	Be 313.107†	37909.0	36495.3	11.755 µg/L	11.755 ppb	23:38:00
2	Cd 226.502†	1788.5	1785.0	-0.4717 µg/L	-0.4717 ppb	23:38:20
2	Co 228.616†	3793.9	3762.9	46.078 µg/L	46.078 ppb	23:38:20
2	Cr 267.716†	8987.9	8336.0	75.029 µg/L	75.029 ppb	23:38:20
2	Cu 324.752†	14086.5	10891.0	65.322 µg/L	65.322 ppb	23:38:00
2	Mn 257.610†	3047418.6	2880633.0	3935.1 µg/L	3935.1 ppb	23:38:00
2	Mo 202.031†	-61.7	-3.1	5.1393 µg/L	5.1393 ppb	23:38:20
2	Ni 231.604†	6166.3	5869.9	75.082 µg/L	75.082 ppb	23:38:20
2	P 214.914†	4969.3	4617.9	1039.4 µg/L	1039.4 ppb	23:38:20
2	Pb 220.353†	1815.8	1604.1	101.32 µg/L	101.32 ppb	23:38:20

2	S 181.975 Axial†	734.2	599.2	485.50 µg/L	485.50 ppb	23:38:20
2	Sb 206.836†	71.9	-18.7	-5.3218 µg/L	-5.3218 ppb	23:38:20
2	Se 196.026†	-96.7	-102.3	1.48 µg/L	1.48 ppb	23:38:20
2	SiO2†	1058321.3	998854.2	109180 µg/L	109180 ppb	23:38:00
2	Si 251.611†	3214808.3	3038269.5	50237 µg/L	50237 ppb	23:38:00
2	Sn 189.927†	79.3	73.0	13.013 µg/L	13.013 ppb	23:38:20
2	Ti 334.940†	2408306.7	2275926.6	2319.8 µg/L	2319.8 ppb	23:38:00
2	Tl 190.801†	-419.6	-276.3	-2.4587 µg/L	-2.4587 ppb	23:38:20
2	U 409.014†	-7553.0	-6660.7	-402.05 µg/L	-402.05 ppb	23:38:00
2	V 292.402†	37270.4	34799.8	171.51 µg/L	171.51 ppb	23:38:00
2	Zn 213.857†	63776.6	59823.4	365.33 µg/L	365.33 ppb	23:38:00
3	Sc RADIAL	156169.6	156169.6	107 %		23:37:33
3	Al 396.153Radial†	372420.2	347614.3	75880 µg/L	75880 ppb	23:37:31
3	Ca 317.933Radial†	312694.5	291223.9	17064 µg/L	17064 ppb	23:37:33
3	Fe 238.204 Radial†	1949906.8	1819748.8	120980 µg/L	120980 ppb	23:37:31
3	K 766.490 Radial†	44388.5	39973.1	16434 µg/L	16434 ppb	23:37:33
3	Mg 279.077 IEC†	49346.5	45868.8	18808 µg/L	18808 ppb	23:37:33
3	Na 589.592 Radial†	36466.1	32339.3	4933.7 µg/L	4933.7 ppb	23:37:33
3	Sr 421.552†	98475.8	92186.2	215.93 µg/L	215.93 ppb	23:37:33
3	Sc 361.383	1755861.0	1755861.0	104.97 %		23:38:23
3	Y 371.029	1249742.4	1249742.4	122.21 %		23:38:23
3	Ag 328.068†	2970.4	-137.2	-1.0264 µg/L	-1.0264 ppb	23:38:23
3	As 188.979†	37.4	49.9	48.670 µg/L	48.670 ppb	23:38:43
3	B 249.677†	4491.5	923.3	15.323 µg/L	15.323 ppb	23:38:23
3	Ba 233.527†	213179.3	203266.8	927.16 µg/L	927.16 ppb	23:38:23
3	Be 313.107†	37526.6	36411.0	11.737 µg/L	11.737 ppb	23:38:23
3	Cd 226.502†	1772.9	1783.4	-0.3710 µg/L	-0.3710 ppb	23:38:43
3	Co 228.616†	3750.9	3750.0	45.958 µg/L	45.958 ppb	23:38:43
3	Cr 267.716†	8952.6	8368.7	75.248 µg/L	75.248 ppb	23:38:43
3	Cu 324.752†	14090.8	10999.2	65.660 µg/L	65.660 ppb	23:38:23
3	Mn 257.610†	3030773.3	2887278.5	3944.2 µg/L	3944.2 ppb	23:38:23
3	Mo 202.031†	-65.1	-6.8	4.9815 µg/L	4.9815 ppb	23:38:43
3	Ni 231.604†	6162.5	5911.8	75.619 µg/L	75.619 ppb	23:38:43
3	P 214.914†	4948.2	4634.5	1043.9 µg/L	1043.9 ppb	23:38:43
3	Pb 220.353†	1845.4	1645.6	103.82 µg/L	103.82 ppb	23:38:43
3	S 181.975 Axial†	733.6	604.1	489.42 µg/L	489.42 ppb	23:38:43
3	Sb 206.836†	81.0	-9.5	-4.0701 µg/L	-4.0701 ppb	23:38:43
3	Se 196.026†	-73.0	-80.5	9.78 µg/L	9.78 ppb	23:38:43
3	SiO2†	1051136.7	999824.5	109280 µg/L	109280 ppb	23:38:23
3	Si 251.611†	3193980.8	3042166.7	50302 µg/L	50302 ppb	23:38:23
3	Sn 189.927†	66.7	61.5	12.207 µg/L	12.207 ppb	23:38:43
3	Ti 334.940†	2392147.3	2278315.6	2322.2 µg/L	2322.2 ppb	23:38:23
3	Tl 190.801†	-415.3	-275.4	-2.2815 µg/L	-2.2815 ppb	23:38:43
3	U 409.014†	-6988.9	-6179.1	-371.98 µg/L	-371.98 ppb	23:38:23
3	V 292.402†	37031.5	34847.3	171.96 µg/L	171.96 ppb	23:38:23
3	Zn 213.857†	63493.5	60024.6	366.70 µg/L	366.70 ppb	23:38:23

Mean Data: 248118007|959114|1

Analyte	Mean Corrected Intensity	Conc. Units	Calib.	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1763565.9	105.43 %		0.419			0.40%
Sc RADIAL	155561.3	107 %		0.7			0.61%
Y 371.029	1255085.9	122.74 %		0.460			0.37%
Ag 328.068†	-121.3	-0.9837 µg/L		0.76770	-0.9837 ppb	0.76770	78.04%
Al 396.153Radial†	348573.6	76089 µg/L		299.5	76089 ppb	299.5	0.39%
As 188.979†	40.5	44.843 µg/L		3.5021	44.843 ppb	3.5021	7.81%
B 249.677†	794.6	13.161 µg/L		1.9532	13.161 ppb	1.9532	14.84%
Ba 233.527†	203170.7	926.71 µg/L		0.965	926.71 ppb	0.965	0.10%
Be 313.107†	36475.4	11.753 µg/L		0.0156	11.753 ppb	0.0156	0.13%
Ca 317.933Radial†	293334.4	17188 µg/L		128.0	17188 ppb	128.0	0.74%
Cd 226.502†	1783.4	-0.4250 µg/L		0.05076	-0.4250 ppb	0.05076	11.94%
Co 228.616†	3758.2	46.042 µg/L		0.0737	46.042 ppb	0.0737	0.16%
Cr 267.716†	8357.0	75.177 µg/L		0.1289	75.177 ppb	0.1289	0.17%
Cu 324.752†	10957.5	65.544 µg/L		0.1926	65.544 ppb	0.1926	0.29%
Fe 238.204 Radial†	1827481.5	121500 µg/L		531.9	121500 ppb	531.9	0.44%
K 766.490 Radial†	40168.5	16514 µg/L		85.4	16514 ppb	85.4	0.52%
Mg 279.077 IEC†	46162.7	18929 µg/L		137.9	18929 ppb	137.9	0.73%
Mn 257.610†	2883048.7	3938.4 µg/L		5.03	3938.4 ppb	5.03	0.13%
Mo 202.031†	-10.1	4.8976 µg/L		0.29283	4.8976 ppb	0.29283	5.98%
Na 589.592 Radial†	32494.6	4957.4 µg/L		20.69	4957.4 ppb	20.69	0.42%

Ni 231.604†	5885.9	75.287 µg/L	0.2899	75.287 ppb	0.2899	0.39%
P 214.914†	4631.0	1042.8 µg/L	3.04	1042.8 ppb	3.04	0.29%
Pb 220.353†	1611.9	101.78 µg/L	1.847	101.78 ppb	1.847	1.81%
S 181.975 Axial†	610.8	494.84 µg/L	12.933	494.84 ppb	12.933	2.61%
Sb 206.836†	-16.0	-4.9494 µg/L	0.76442	-4.9494 ppb	0.76442	15.44%
Se 196.026†	-90.5	5.98 µg/L	4.193	5.98 ppb	4.193	70.16%
SiO2†	999333.4	109230 µg/L	53.1	109230 ppb	53.1	0.05%
Concentration greater than upper limit for SiO2.						
Si 251.611†	3040468.4	50274 µg/L	33.0	50274 ppb	33.0	0.07%
Concentration greater than upper limit for Si 251.611.						
Sn 189.927†	63.9	12.374 µg/L	0.5746	12.374 ppb	0.5746	4.64%
Sr 421.552†	92654.2	217.02 µg/L	1.056	217.02 ppb	1.056	0.49%
Ti 334.940†	2276341.8	2320.2 µg/L	1.84	2320.2 ppb	1.84	0.08%
Tl 190.801†	-275.2	-2.2870 µg/L	0.16896	-2.2870 ppb	0.16896	7.39%
U 409.014†	-6420.9	-387.06 µg/L	15.036	-387.06 ppb	15.036	3.88%
Concentration less than lower limit for U 409.014.						
V 292.402†	34865.9	171.97 µg/L	0.468	171.97 ppb	0.468	0.27%
Zn 213.857†	59841.2	365.50 µg/L	1.132	365.50 ppb	1.132	0.31%

Sequence No.: 117

Sample ID: CCV

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 1

Date Collected: 3/29/2010 23:38:52

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCV

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	152247.4	152247.4	104 %		23:39:26
1	Al 396.153Radial†	25276.5	24230.4	5266.9 µg/L	5266.9 ppb	23:39:26
1	Ca 317.933Radial†	88743.8	84342.8	4942.1 µg/L	4942.1 ppb	23:39:26
1	Fe 238.204 Radial†	78145.1	74699.0	4966.3 µg/L	4966.3 ppb	23:39:26
1	K 766.490 Radial†	13940.6	11891.1	4891.2 µg/L	4891.2 ppb	23:39:26
1	Mg 279.077 IEC†	13088.8	12343.9	5097.0 µg/L	5097.0 ppb	23:39:26
1	Na 589.592 Radial†	69529.9	64869.8	9921.6 µg/L	9921.6 ppb	23:39:26
1	Sr 421.552†	225990.5	216630.3	507.69 µg/L	507.69 ppb	23:39:24
1	Sc 361.383	1749225.5	1749225.5	104.57 %		23:39:53
1	Y 371.029	1057003.0	1057003.0	103.37 %		23:39:53
1	Ag 328.068†	129381.3	120759.6	496.28 µg/L	496.28 ppb	23:39:53
1	As 188.979†	1338.5	1294.2	547.95 µg/L	547.95 ppb	23:40:13
1	B 249.677†	33465.2	28646.9	479.25 µg/L	479.25 ppb	23:39:53
1	Ba 233.527†	115295.3	110431.3	504.89 µg/L	504.89 ppb	23:39:53
1	Be 313.107†	1653761.8	1582143.2	515.15 µg/L	515.15 ppb	23:39:53
1	Cd 226.502†	73121.3	70019.9	483.22 µg/L	483.22 ppb	23:39:53
1	Co 228.616†	37068.3	35624.8	488.07 µg/L	488.07 ppb	23:39:53
1	Cr 267.716†	59777.7	57004.8	489.50 µg/L	489.50 ppb	23:39:53
1	Cu 324.752†	121302.7	113576.2	495.26 µg/L	495.26 ppb	23:39:53
1	Mn 257.610†	377418.5	360843.1	492.86 µg/L	492.86 ppb	23:39:53
1	Mo 202.031†	15830.2	15193.6	480.06 µg/L	480.06 ppb	23:40:13
1	Ni 231.604†	39955.6	38250.3	489.27 µg/L	489.27 ppb	23:39:53
1	P 214.914†	10436.6	9900.9	2362.7 µg/L	2362.7 ppb	23:40:13
1	Pb 220.353†	8369.6	7891.4	479.58 µg/L	479.58 ppb	23:40:13
1	S 181.975 Axial†	1317.0	1164.6	947.59 µg/L	947.59 ppb	23:40:13
1	Sb 206.836†	3863.6	3608.1	487.70 µg/L	487.70 ppb	23:40:13
1	Se 196.026†	1247.3	1181.9	470 µg/L	470 ppb	23:40:13
1	SiO2†	51937.1	48094.3	5236.0 µg/L	5236.0 ppb	23:39:53
1	Si 251.611†	156292.1	148784.9	2450.5 µg/L	2450.5 ppb	23:39:53
1	Sn 189.927†	7149.3	6834.8	487.56 µg/L	487.56 ppb	23:40:13
1	Ti 334.940†	506642.1	483862.6	492.75 µg/L	492.75 ppb	23:39:53
1	Tl 190.801†	3599.1	3562.1	485.57 µg/L	485.57 ppb	23:40:13
1	U 409.014†	7328.1	7486.9	492.92 µg/L	492.92 ppb	23:39:53
1	V 292.402†	94058.4	89515.7	502.68 µg/L	502.68 ppb	23:39:53
1	Zn 213.857†	81063.1	77055.7	481.19 µg/L	481.19 ppb	23:39:53
2	Sc RADIAL	152182.5	152182.5	104 %		23:39:30
2	Al 396.153Radial†	25491.9	24447.0	5314.3 µg/L	5314.3 ppb	23:39:30
2	Ca 317.933Radial†	88400.0	84049.7	4925.0 µg/L	4925.0 ppb	23:39:30
2	Fe 238.204 Radial†	77685.7	74290.9	4939.1 µg/L	4939.1 ppb	23:39:30
2	K 766.490 Radial†	13882.1	11840.7	4870.5 µg/L	4870.5 ppb	23:39:30
2	Mg 279.077 IEC†	13076.1	12337.1	5094.2 µg/L	5094.2 ppb	23:39:30
2	Na 589.592 Radial†	69140.4	64525.1	9868.8 µg/L	9868.8 ppb	23:39:30
2	Sr 421.552†	225899.0	216634.9	507.70 µg/L	507.70 ppb	23:39:28
2	Sc 361.383	1756606.4	1756606.4	105.01 %		23:40:16
2	Y 371.029	1062553.1	1062553.1	103.91 %		23:40:16
2	Ag 328.068†	130340.9	121153.5	497.87 µg/L	497.87 ppb	23:40:16
2	As 188.979†	1330.2	1281.0	542.40 µg/L	542.40 ppb	23:40:36
2	B 249.677†	33839.7	28869.1	482.97 µg/L	482.97 ppb	23:40:16
2	Ba 233.527†	115935.0	110577.2	505.55 µg/L	505.55 ppb	23:40:16
2	Be 313.107†	1662354.9	1583681.1	515.65 µg/L	515.65 ppb	23:40:16
2	Cd 226.502†	73603.1	70184.9	484.37 µg/L	484.37 ppb	23:40:16
2	Co 228.616†	37410.1	35801.4	490.49 µg/L	490.49 ppb	23:40:16
2	Cr 267.716†	60118.4	57089.0	490.22 µg/L	490.22 ppb	23:40:16
2	Cu 324.752†	121758.4	113522.7	495.02 µg/L	495.02 ppb	23:40:16
2	Mn 257.610†	379503.4	361312.1	493.50 µg/L	493.50 ppb	23:40:16
2	Mo 202.031†	15835.0	15134.5	478.19 µg/L	478.19 ppb	23:40:36
2	Ni 231.604†	40393.9	38507.0	492.55 µg/L	492.55 ppb	23:40:16
2	P 214.914†	10445.1	9867.0	2354.6 µg/L	2354.6 ppb	23:40:36
2	Pb 220.353†	8314.6	7805.3	474.37 µg/L	474.37 ppb	23:40:36

2	S 181.975 Axial†	1291.1	1134.6	923.30 µg/L	923.30 ppb	23:40:36
2	Sb 206.836†	3853.2	3582.6	484.22 µg/L	484.22 ppb	23:40:36
2	Se 196.026†	1258.4	1187.4	472 µg/L	472 ppb	23:40:36
2	SiO2†	52352.2	48280.9	5256.5 µg/L	5256.5 ppb	23:40:16
2	Si 251.611†	157154.2	148977.8	2453.8 µg/L	2453.8 ppb	23:40:16
2	Sn 189.927†	7151.6	6808.3	485.68 µg/L	485.68 ppb	23:40:36
2	Ti 334.940†	509514.0	484561.7	493.46 µg/L	493.46 ppb	23:40:16
2	Tl 190.801†	3622.1	3569.5	486.57 µg/L	486.57 ppb	23:40:36
2	U 409.014†	7240.4	7374.0	485.99 µg/L	485.99 ppb	23:40:16
2	V 292.402†	94556.0	89611.6	503.19 µg/L	503.19 ppb	23:40:16
2	Zn 213.857†	81581.6	77223.8	482.23 µg/L	482.23 ppb	23:40:16
3	Sc RADIAL	152804.0	152804.0	105 %		23:39:34
3	Al 396.153Radial†	25361.2	24223.0	5264.8 µg/L	5264.8 ppb	23:39:34
3	Ca 317.933Radial†	88520.1	83820.0	4911.5 µg/L	4911.5 ppb	23:39:34
3	Fe 238.204 Radial†	77911.4	74203.5	4933.3 µg/L	4933.3 ppb	23:39:34
3	K 766.490 Radial†	14047.5	11944.4	4913.2 µg/L	4913.2 ppb	23:39:34
3	Mg 279.077 IEC†	13041.4	12253.0	5059.8 µg/L	5059.8 ppb	23:39:34
3	Na 589.592 Radial†	69331.6	64438.2	9855.5 µg/L	9855.5 ppb	23:39:34
3	Sr 421.552†	228055.6	217811.9	510.46 µg/L	510.46 ppb	23:39:32
3	Sc 361.383	1727263.3	1727263.3	103.26 %		23:40:39
3	Y 371.029	1044625.3	1044625.3	102.16 %		23:40:39
3	Ag 328.068†	128251.0	121238.1	498.21 µg/L	498.21 ppb	23:40:39
3	As 188.979†	1354.1	1325.6	561.10 µg/L	561.10 ppb	23:41:00
3	B 249.677†	33217.5	28813.9	482.04 µg/L	482.04 ppb	23:40:39
3	Ba 233.527†	113939.6	110520.3	505.30 µg/L	505.30 ppb	23:40:39
3	Be 313.107†	1635537.5	1584602.5	515.95 µg/L	515.95 ppb	23:40:39
3	Cd 226.502†	72123.9	69943.1	482.70 µg/L	482.70 ppb	23:40:39
3	Co 228.616†	36825.6	35840.5	491.03 µg/L	491.03 ppb	23:40:39
3	Cr 267.716†	59335.4	57303.3	492.07 µg/L	492.07 ppb	23:40:39
3	Cu 324.752†	119991.5	113781.3	496.14 µg/L	496.14 ppb	23:40:39
3	Mn 257.610†	373454.9	361593.7	493.88 µg/L	493.88 ppb	23:40:39
3	Mo 202.031†	15974.6	15525.8	490.54 µg/L	490.54 ppb	23:41:00
3	Ni 231.604†	39576.7	38369.1	490.79 µg/L	490.79 ppb	23:40:39
3	P 214.914†	10571.9	10158.8	2424.5 µg/L	2424.5 ppb	23:41:00
3	Pb 220.353†	8432.7	8054.2	489.48 µg/L	489.48 ppb	23:41:00
3	S 181.975 Axial†	1312.9	1176.7	957.45 µg/L	957.45 ppb	23:41:00
3	Sb 206.836†	3890.3	3681.0	497.66 µg/L	497.66 ppb	23:41:00
3	Se 196.026†	1268.6	1217.7	484 µg/L	484 ppb	23:41:00
3	SiO2†	51486.2	48289.2	5256.9 µg/L	5256.9 ppb	23:40:39
3	Si 251.611†	154556.3	149004.3	2453.9 µg/L	2453.9 ppb	23:40:39
3	Sn 189.927†	7248.5	7017.9	500.58 µg/L	500.58 ppb	23:41:00
3	Ti 334.940†	501274.5	484824.8	493.73 µg/L	493.73 ppb	23:40:39
3	Tl 190.801†	3659.3	3664.1	499.26 µg/L	499.26 ppb	23:41:00
3	U 409.014†	7080.4	7336.1	483.61 µg/L	483.61 ppb	23:40:39
3	V 292.402†	92863.7	89502.4	502.72 µg/L	502.72 ppb	23:40:39
3	Zn 213.857†	80355.3	77356.0	483.07 µg/L	483.07 ppb	23:40:39

Mean Data: CCV

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1744365.0	104.28 %	0.912			0.88%
Sc RADIAL	152411.3	105 %	0.2			0.22%
Y 371.029	1054727.1	103.14 %	0.898			0.87%
Ag 328.068†	121050.4	497.45 µg/L	1.032	497.45 ppb	1.032	0.21%
QC value within limits for Ag 328.068 Recovery = 99.49%						
Al 396.153Radial†	24300.1	5282.0 µg/L	27.97	5282.0 ppb	27.97	0.53%
QC value within limits for Al 396.153Radial Recovery = 105.64%						
As 188.979†	1300.3	550.48 µg/L	9.602	550.48 ppb	9.602	1.74%
QC value greater than the upper limit for As 188.979 Recovery = 110.10%						
B 249.677†	28776.6	481.42 µg/L	1.937	481.42 ppb	1.937	0.40%
QC value within limits for B 249.677 Recovery = 96.28%						
Ba 233.527†	110509.6	505.25 µg/L	0.336	505.25 ppb	0.336	0.07%
QC value within limits for Ba 233.527 Recovery = 101.05%						
Be 313.107†	1583475.6	515.59 µg/L	0.403	515.59 ppb	0.403	0.08%
QC value within limits for Be 313.107 Recovery = 103.12%						
Ca 317.933Radial†	84070.8	4926.2 µg/L	15.35	4926.2 ppb	15.35	0.31%
QC value within limits for Ca 317.933Radial Recovery = 98.52%						
Cd 226.502†	70049.3	483.43 µg/L	0.854	483.43 ppb	0.854	0.18%
QC value within limits for Cd 226.502 Recovery = 96.69%						
Co 228.616†	35755.6	489.87 µg/L	1.574	489.87 ppb	1.574	0.32%

QC value within limits for Co 228.616 Recovery = 97.97%							
Cr 267.716†	57132.4	490.60 µg/L	1.325	490.60 ppb	1.325	0.27%	
QC value within limits for Cr 267.716 Recovery = 98.12%							
Cu 324.752†	113626.8	495.47 µg/L	0.590	495.47 ppb	0.590	0.12%	
QC value within limits for Cu 324.752 Recovery = 99.09%							
Fe 238.204 Radial†	74397.8	4946.2 µg/L	17.58	4946.2 ppb	17.58	0.36%	
QC value within limits for Fe 238.204 Radial Recovery = 98.92%							
K 766.490 Radial†	11892.1	4891.6 µg/L	21.36	4891.6 ppb	21.36	0.44%	
QC value within limits for K 766.490 Radial Recovery = 97.83%							
Mg 279.077 IEC†	12311.3	5083.7 µg/L	20.70	5083.7 ppb	20.70	0.41%	
QC value within limits for Mg 279.077 IEC Recovery = 101.67%							
Mn 257.610†	361249.7	493.41 µg/L	0.519	493.41 ppb	0.519	0.11%	
QC value within limits for Mn 257.610 Recovery = 98.68%							
Mo 202.031†	15284.7	482.93 µg/L	6.658	482.93 ppb	6.658	1.38%	
QC value within limits for Mo 202.031 Recovery = 96.59%							
Na 589.592 Radial†	64611.1	9882.0 µg/L	34.93	9882.0 ppb	34.93	0.35%	
QC value within limits for Na 589.592 Radial Recovery = 98.82%							
Ni 231.604†	38375.5	490.87 µg/L	1.644	490.87 ppb	1.644	0.33%	
QC value within limits for Ni 231.604 Recovery = 98.17%							
P 214.914†	9975.6	2380.6 µg/L	38.21	2380.6 ppb	38.21	1.61%	
QC value within limits for P 214.914 Recovery = 95.22%							
Pb 220.353†	7917.0	481.14 µg/L	7.675	481.14 ppb	7.675	1.60%	
QC value within limits for Pb 220.353 Recovery = 96.23%							
S 181.975 Axial†	1158.6	942.78 µg/L	17.573	942.78 ppb	17.573	1.86%	
QC value within limits for S 181.975 Axial Recovery = 94.28%							
Sb 206.836†	3623.9	489.86 µg/L	6.973	489.86 ppb	6.973	1.42%	
QC value within limits for Sb 206.836 Recovery = 97.97%							
Se 196.026†	1195.7	475 µg/L	7.6	475 ppb	7.6	1.60%	
QC value within limits for Se 196.026 Recovery = 95.02%							
SiO2†	48221.4	5249.8 µg/L	11.92	5249.8 ppb	11.92	0.23%	
QC value within limits for SiO2 Recovery = 98.17%							
Si 251.611†	148922.3	2452.7 µg/L	1.92	2452.7 ppb	1.92	0.08%	
QC value within limits for Si 251.611 Recovery = 98.11%							
Sn 189.927†	6887.0	491.27 µg/L	8.114	491.27 ppb	8.114	1.65%	
QC value within limits for Sn 189.927 Recovery = 98.25%							
Sr 421.552†	217025.7	508.61 µg/L	1.596	508.61 ppb	1.596	0.31%	
QC value within limits for Sr 421.552 Recovery = 101.72%							
Ti 334.940†	484416.4	493.31 µg/L	0.510	493.31 ppb	0.510	0.10%	
QC value within limits for Ti 334.940 Recovery = 98.66%							
Tl 190.801†	3598.6	490.47 µg/L	7.634	490.47 ppb	7.634	1.56%	
QC value within limits for Tl 190.801 Recovery = 98.09%							
U 409.014†	7399.0	487.51 µg/L	4.839	487.51 ppb	4.839	0.99%	
QC value within limits for U 409.014 Recovery = 97.50%							
V 292.402†	89543.2	502.87 µg/L	0.285	502.87 ppb	0.285	0.06%	
QC value within limits for V 292.402 Recovery = 100.57%							
Zn 213.857†	77211.8	482.16 µg/L	0.944	482.16 ppb	0.944	0.20%	
QC value within limits for Zn 213.857 Recovery = 96.43%							
QC Failed. Continue with analysis.							

Sequence No.: 118

Sample ID: CCB

Analyst:

Initial Sample Wt:

Dilution:

Autosampler Location: 6

Date Collected: 3/29/2010 23:41:07

Data Type: Original

Initial Sample Vol:

Sample Prep Vol:

Replicate Data: CCB

Repl#	Analyte	Net Intensity	Corrected Intensity	Calib. Conc. Units	Sample Conc. Units	Analysis Time
1	Sc RADIAL	154154.1	154154.1	106 %		23:41:37
1	Al 396.153Radial†	-32.2	1.4	0.2551 µg/L	0.2551 ppb	23:41:57
1	Ca 317.933Radial†	665.8	13.3	0.7790 µg/L	0.7790 ppb	23:41:57
1	Fe 238.204 Radial†	199.1	75.0	4.9873 µg/L	4.9873 ppb	23:41:57
1	K 766.490 Radial†	1540.7	1.8	0.7423 µg/L	0.7423 ppb	23:41:37
1	Mg 279.077 IEC†	174.0	-22.1	-9.0967 µg/L	-9.0967 ppb	23:41:57
1	Na 589.592 Radial†	1654.0	-130.8	-20.020 µg/L	-20.020 ppb	23:41:37
1	Sr 421.552†	-155.4	131.1	0.3072 µg/L	0.3072 ppb	23:41:37
1	Sc 361.383	1757280.2	1757280.2	105.05 %		23:42:45
1	Y 371.029	1074756.8	1074756.8	105.10 %		23:42:45
1	Ag 328.068†	3145.9	27.6	0.1143 µg/L	0.1143 ppb	23:42:47
1	As 188.979†	-19.8	-4.6	-1.9026 µg/L	-1.9026 ppb	23:43:07
1	B 249.677†	3123.1	-382.7	-6.4271 µg/L	-6.4271 ppb	23:43:07
1	Ba 233.527†	-170.5	12.8	0.0586 µg/L	0.0586 ppb	23:43:07
1	Be 313.107†	-683.8	9.2	0.0042 µg/L	0.0042 ppb	23:42:47
1	Cd 226.502†	-90.7	8.0	0.0549 µg/L	0.0549 ppb	23:43:07
1	Co 228.616†	-158.9	25.3	0.3467 µg/L	0.3467 ppb	23:43:07
1	Cr 267.716†	176.9	8.1	0.0668 µg/L	0.0668 ppb	23:43:07
1	Cu 324.752†	2694.2	139.7	0.6114 µg/L	0.6114 ppb	23:42:47
1	Mn 257.610†	288.6	194.8	0.2665 µg/L	0.2665 ppb	23:43:07
1	Mo 202.031†	-22.6	33.7	1.0627 µg/L	1.0627 ppb	23:43:07
1	Ni 231.604†	-45.3	-2.2	-0.0280 µg/L	-0.0280 ppb	23:43:07
1	P 214.914†	17.9	-62.5	-14.985 µg/L	-14.985 ppb	23:43:07
1	Pb 220.353†	92.5	-24.4	-1.4794 µg/L	-1.4794 ppb	23:43:07
1	S 181.975 Axial†	98.7	-0.9	-0.7053 µg/L	-0.7053 ppb	23:43:07
1	Sb 206.836†	75.3	-15.0	-2.0094 µg/L	-2.0094 ppb	23:43:07
1	Se 196.026†	6.9	-4.3	-1.71 µg/L	-1.71 ppb	23:43:07
1	SiO2†	1703.5	48.7	5.2848 µg/L	5.2848 ppb	23:43:07
1	Si 251.611†	851.4	134.1	2.1981 µg/L	2.1981 ppb	23:43:07
1	Sn 189.927†	14.3	11.6	0.8211 µg/L	0.8211 ppb	23:43:07
1	Ti 334.940†	553.8	-109.2	-0.1122 µg/L	-0.1122 ppb	23:42:47
1	Tl 190.801†	-101.4	23.8	3.1904 µg/L	3.1904 ppb	23:43:07
1	U 409.014†	-434.8	65.2	4.0149 µg/L	4.0149 ppb	23:42:47
1	V 292.402†	413.9	-37.8	-0.1965 µg/L	-0.1965 ppb	23:42:47
1	Zn 213.857†	503.9	15.3	0.0954 µg/L	0.0954 ppb	23:43:07
2	Sc RADIAL	153227.7	153227.7	105 %		23:41:59
2	Al 396.153Radial†	-66.3	-31.2	-6.8637 µg/L	-6.8637 ppb	23:42:19
2	Ca 317.933Radial†	638.9	-8.4	-0.4934 µg/L	-0.4934 ppb	23:42:19
2	Fe 238.204 Radial†	205.8	82.5	5.4854 µg/L	5.4854 ppb	23:42:19
2	K 766.490 Radial†	1536.3	6.4	2.6229 µg/L	2.6229 ppb	23:41:59
2	Mg 279.077 IEC†	203.7	7.1	2.9505 µg/L	2.9505 ppb	23:42:19
2	Na 589.592 Radial†	1675.6	-100.9	-15.435 µg/L	-15.435 ppb	23:41:59
2	Sr 421.552†	-270.6	20.6	0.0483 µg/L	0.0483 ppb	23:41:59
2	Sc 361.383	1774132.2	1774132.2	106.06 %		23:43:09
2	Y 371.029	1084939.0	1084939.0	106.10 %		23:43:09
2	Ag 328.068†	3370.5	210.9	0.8421 µg/L	0.8421 ppb	23:43:11
2	As 188.979†	-16.0	-0.8	-0.3415 µg/L	-0.3415 ppb	23:43:31
2	B 249.677†	3102.4	-430.6	-7.2306 µg/L	-7.2306 ppb	23:43:31
2	Ba 233.527†	-158.2	25.9	0.1182 µg/L	0.1182 ppb	23:43:31
2	Be 313.107†	-751.9	-48.8	-0.0172 µg/L	-0.0172 ppb	23:43:11
2	Cd 226.502†	-98.1	1.9	0.0124 µg/L	0.0124 ppb	23:43:31
2	Co 228.616†	-144.4	40.4	0.5536 µg/L	0.5536 ppb	23:43:31
2	Cr 267.716†	168.8	-1.1	-0.0061 µg/L	-0.0061 ppb	23:43:31
2	Cu 324.752†	2681.7	103.6	0.4481 µg/L	0.4481 ppb	23:43:11
2	Mn 257.610†	284.9	188.6	0.2576 µg/L	0.2576 ppb	23:43:31
2	Mo 202.031†	-23.9	32.6	1.0304 µg/L	1.0304 ppb	23:43:31
2	Ni 231.604†	-58.3	-14.0	-0.1793 µg/L	-0.1793 ppb	23:43:31
2	P 214.914†	21.4	-59.4	-14.233 µg/L	-14.233 ppb	23:43:31
2	Pb 220.353†	44.3	-70.6	-4.2735 µg/L	-4.2735 ppb	23:43:31

2	S 181.975 Axial†	86.8	-13.0	-10.528 µg/L	-10.528 ppb	23:43:31
2	Sb 206.836†	76.6	-14.4	-1.9323 µg/L	-1.9323 ppb	23:43:31
2	Se 196.026†	30.5	17.9	7.06 µg/L	7.06 ppb	23:43:31
2	SiO2†	1731.9	60.1	6.5380 µg/L	6.5380 ppb	23:43:31
2	Si 251.611†	830.1	106.3	1.7426 µg/L	1.7426 ppb	23:43:31
2	Sn 189.927†	5.8	3.4	0.2428 µg/L	0.2428 ppb	23:43:31
2	Ti 334.940†	935.8	246.0	0.2523 µg/L	0.2523 ppb	23:43:11
2	Tl 190.801†	-121.7	5.6	0.7453 µg/L	0.7453 ppb	23:43:31
2	U 409.014†	-580.6	-68.3	-4.2602 µg/L	-4.2602 ppb	23:43:11
2	V 292.402†	326.3	-124.2	-0.6822 µg/L	-0.6822 ppb	23:43:11
2	Zn 213.857†	505.8	12.5	0.0790 µg/L	0.0790 ppb	23:43:31
3	Sc RADIAL	154277.1	154277.1	106 %		23:42:21
3	Al 396.153Radial†	-69.9	-34.2	-7.5057 µg/L	-7.5057 ppb	23:42:41
3	Ca 317.933Radial†	649.4	-2.7	-0.1580 µg/L	-0.1580 ppb	23:42:41
3	Fe 238.204 Radial†	174.9	51.9	3.4517 µg/L	3.4517 ppb	23:42:41
3	K 766.490 Radial†	1726.4	176.0	72.477 µg/L	72.477 ppb	23:42:21
3	Mg 279.077 IEC†	174.5	-21.8	-8.9549 µg/L	-8.9549 ppb	23:42:41
3	Na 589.592 Radial†	1592.5	-190.2	-29.164 µg/L	-29.164 ppb	23:42:21
3	Sc 421.552†	-251.6	40.3	0.0944 µg/L	0.0944 ppb	23:42:21
3	Sc 361.383	1738323.9	1738323.9	103.92 %		23:43:34
3	Y 371.029	1063504.2	1063504.2	104.00 %		23:43:34
3	Ag 328.068†	3360.1	266.4	1.0882 µg/L	1.0882 ppb	23:43:36
3	As 188.979†	-17.2	-2.3	-0.9662 µg/L	-0.9662 ppb	23:43:56
3	B 249.677†	3142.6	-331.6	-5.5673 µg/L	-5.5673 ppb	23:43:56
3	Ba 233.527†	-143.2	37.2	0.1697 µg/L	0.1697 ppb	23:43:56
3	Be 313.107†	-470.7	207.2	0.0725 µg/L	0.0725 ppb	23:43:36
3	Cd 226.502†	-86.5	11.2	0.0766 µg/L	0.0766 ppb	23:43:56
3	Co 228.616†	-181.3	2.1	0.0292 µg/L	0.0292 ppb	23:43:56
3	Cr 267.716†	145.3	-20.4	-0.1886 µg/L	-0.1886 ppb	23:43:56
3	Cu 324.752†	2780.2	250.5	1.1033 µg/L	1.1033 ppb	23:43:36
3	Mn 257.610†	273.3	183.0	0.2504 µg/L	0.2504 ppb	23:43:56
3	Mo 202.031†	-22.8	33.3	1.0497 µg/L	1.0497 ppb	23:43:56
3	Ni 231.604†	-56.4	-13.4	-0.1715 µg/L	-0.1715 ppb	23:43:56
3	P 214.914†	10.1	-69.9	-16.767 µg/L	-16.767 ppb	23:43:56
3	Pb 220.353†	80.3	-35.2	-2.1405 µg/L	-2.1405 ppb	23:43:56
3	S 181.975 Axial†	83.6	-14.4	-11.650 µg/L	-11.650 ppb	23:43:56
3	Sb 206.836†	84.1	-5.7	-0.7585 µg/L	-0.7585 ppb	23:43:56
3	Se 196.026†	23.6	11.8	4.67 µg/L	4.67 ppb	23:43:56
3	SiO2†	1739.0	100.6	10.968 µg/L	10.968 ppb	23:43:56
3	Si 251.611†	803.4	96.7	1.5871 µg/L	1.5871 ppb	23:43:56
3	Sn 189.927†	-1.0	-3.0	-0.2114 µg/L	-0.2114 ppb	23:43:56
3	Ti 334.940†	745.5	81.1	0.0766 µg/L	0.0766 ppb	23:43:36
3	Tl 190.801†	-124.1	0.8	0.1061 µg/L	0.1061 ppb	23:43:56
3	U 409.014†	-215.2	272.0	16.743 µg/L	16.743 ppb	23:43:36
3	V 292.402†	242.1	-198.9	-1.0823 µg/L	-1.0823 ppb	23:43:36
3	Zn 213.857†	492.4	9.5	0.0594 µg/L	0.0594 ppb	23:43:56

Mean Data: CCB

Analyte	Mean Corrected Intensity	Calib. Conc. Units	Std.Dev.	Sample Conc. Units	Std.Dev.	RSD
Sc 361.383	1756578.8	105.01 %	1.071			1.02%
Sc RADIAL	153886.3	106 %	0.4			0.37%
Y 371.029	1074400.0	105.07 %	1.049			1.00%
Ag 328.068†	168.3	0.6816 µg/L	0.50645	0.6816 ppb	0.50645	74.31%
QC value within limits for Ag 328.068 Recovery = Not calculated						
Al 396.153Radial†	-21.3	-4.7047 µg/L	4.30734	-4.7047 ppb	4.30734	91.55%
QC value within limits for Al 396.153Radial Recovery = Not calculated						
As 188.979†	-2.6	-1.0701 µg/L	0.78570	-1.0701 ppb	0.78570	73.42%
QC value within limits for As 188.979 Recovery = Not calculated						
B 249.677†	-381.6	-6.4083 µg/L	0.83185	-6.4083 ppb	0.83185	12.98%
QC value within limits for B 249.677 Recovery = Not calculated						
Ba 233.527†	25.3	0.1155 µg/L	0.05561	0.1155 ppb	0.05561	48.15%
QC value within limits for Ba 233.527 Recovery = Not calculated						
Be 313.107†	55.9	0.0199 µg/L	0.04685	0.0199 ppb	0.04685	235.93%
QC value within limits for Be 313.107 Recovery = Not calculated						
Ca 317.933Radial†	0.7	0.0425 µg/L	0.65946	0.0425 ppb	0.65946	>999.9%
QC value within limits for Ca 317.933Radial Recovery = Not calculated						
Cd 226.502†	7.0	0.0480 µg/L	0.03261	0.0480 ppb	0.03261	67.99%
QC value within limits for Cd 226.502 Recovery = Not calculated						
Co 228.616†	22.6	0.3098 µg/L	0.26415	0.3098 ppb	0.26415	85.26%

QC value within limits for Co 228.616 Recovery = Not calculated						
Cr 267.716†	-4.4	-0.0426 µg/L	0.13154	-0.0426 ppb	0.13154	308.49%
QC value within limits for Cr 267.716 Recovery = Not calculated						
Cu 324.752†	164.6	0.7209 µg/L	0.34103	0.7209 ppb	0.34103	47.31%
QC value within limits for Cu 324.752 Recovery = Not calculated						
Fe 238.204 Radial†	69.8	4.6415 µg/L	1.06002	4.6415 ppb	1.06002	22.84%
QC value within limits for Fe 238.204 Radial Recovery = Not calculated						
K 766.490 Radial†	61.4	25.281 µg/L	40.8842	25.281 ppb	40.8842	161.72%
QC value within limits for K 766.490 Radial Recovery = Not calculated						
Mg 279.077 IEC†	-12.3	-5.0337 µg/L	6.91491	-5.0337 ppb	6.91491	137.37%
QC value within limits for Mg 279.077 IEC Recovery = Not calculated						
Mn 257.610†	188.8	0.2582 µg/L	0.00805	0.2582 ppb	0.00805	3.12%
QC value within limits for Mn 257.610 Recovery = Not calculated						
Mo 202.031†	33.2	1.0476 µg/L	0.01628	1.0476 ppb	0.01628	1.55%
QC value within limits for Mo 202.031 Recovery = Not calculated						
Na 589.592 Radial†	-140.6	-21.540 µg/L	6.9896	-21.540 ppb	6.9896	32.45%
QC value within limits for Na 589.592 Radial Recovery = Not calculated						
Ni 231.604†	-9.9	-0.1262 µg/L	0.08520	-0.1262 ppb	0.08520	67.49%
QC value within limits for Ni 231.604 Recovery = Not calculated						
P 214.914†	-63.9	-15.328 µg/L	1.3013	-15.328 ppb	1.3013	8.49%
QC value within limits for P 214.914 Recovery = Not calculated						
Pb 220.353†	-43.4	-2.6311 µg/L	1.46023	-2.6311 ppb	1.46023	55.50%
QC value within limits for Pb 220.353 Recovery = Not calculated						
S 181.975 Axial†	-9.4	-7.6280 µg/L	6.02136	-7.6280 ppb	6.02136	78.94%
QC value within limits for S 181.975 Axial Recovery = Not calculated						
Sb 206.836†	-11.7	-1.5667 µg/L	0.70103	-1.5667 ppb	0.70103	44.74%
QC value within limits for Sb 206.836 Recovery = Not calculated						
Se 196.026†	8.4	3.34 µg/L	4.535	3.34 ppb	4.535	135.78%
QC value within limits for Se 196.026 Recovery = Not calculated						
SiO2†	69.8	7.5968 µg/L	2.98577	7.5968 ppb	2.98577	39.30%
QC value within limits for SiO2 Recovery = Not calculated						
Si 251.611†	112.4	1.8426 µg/L	0.31750	1.8426 ppb	0.31750	17.23%
QC value within limits for Si 251.611 Recovery = Not calculated						
Sn 189.927†	4.0	0.2842 µg/L	0.51748	0.2842 ppb	0.51748	182.09%
QC value within limits for Sn 189.927 Recovery = Not calculated						
Sr 421.552†	64.0	0.1500 µg/L	0.13814	0.1500 ppb	0.13814	92.12%
QC value within limits for Sr 421.552 Recovery = Not calculated						
Ti 334.940†	72.6	0.0722 µg/L	0.18230	0.0722 ppb	0.18230	252.47%
QC value within limits for Ti 334.940 Recovery = Not calculated						
Tl 190.801†	10.1	1.3473 µg/L	1.62792	1.3473 ppb	1.62792	120.83%
QC value within limits for Tl 190.801 Recovery = Not calculated						
U 409.014†	89.6	5.4993 µg/L	10.58022	5.4993 ppb	10.58022	192.39%
QC value within limits for U 409.014 Recovery = Not calculated						
V 292.402†	-120.3	-0.6537 µg/L	0.44357	-0.6537 ppb	0.44357	67.86%
QC value within limits for V 292.402 Recovery = Not calculated						
Zn 213.857†	12.4	0.0779 µg/L	0.01801	0.0779 ppb	0.01801	23.11%
QC value within limits for Zn 213.857 Recovery = Not calculated						

All analyte(s) passed QC.

ICPMS #6 Daily Performance Report

Sample ID: Sample

Sample Date/Time: Wednesday, March 24, 2010 02:25:40

Sample Description:

Method File: C:\elandata\Method\Daily2.mth

Dataset File: c:\elandata\Dataset\default\Sample.1799

Tuning File: c:\elandata\Tuning\default2.tun

Optimization File: c:\elandata\Optimize\default.dac

Dual Detector Mode: Pulse

Acq. Dead Time(ns): 35

Current Dead Time (ns): 35

Number of Replicates: 5

Summary

Analyte	Mass	Meas. Intens.	Mean	Net Intens.	Mean	Net Intens.	SD	Net Intens.	RSD
Be	9.0		1960.5		1960.535		50.160		2.6
Mg	24.0		18238.6		18238.636		157.642		0.9
Co	58.9		26360.7		26360.699		121.159		0.5
Rh	102.9		49939.1		49939.138		319.670		0.6
In	114.9		59742.3		59742.266		511.459		0.9
Pb	208.0		29263.3		29263.344		310.071		1.1
[> Ba	137.9		51164.7		51164.674		342.892		0.7
[Ba++	69.0		1582.2		0.031		0.001		2.3
[> Ce	139.9		66984.3		66984.282		548.113		0.8
[CeO	155.9		980.7		0.015		0.000		2.4
Bkgd	220.0		29.5		29.500		3.162		10.7

Current Optimization File Data

Current Value	Description
0.83	Nebulizer Gas Flow
8.75	Lens Voltage
1450.00	ICP RF Power
-1800.00	Analog Stage Voltage
900.00	Pulse Stage Voltage
30.00	Discriminator Threshold
-6.00	AC Rod Offset

Current Autolens Data

Analyte	Mass	Num of Pts	DAC Value	Maximum Intensity
Be	9	21	7.0	2131.8
Co	59	21	7.5	26323.6
In	115	21	8.3	56990.8

ICPMS #6 Instrument Tuning Report

File Name: default2.tun
File Path: c:\elandata\Tuning

Analyte	Exact Mass	Meas. Mass	Mass DAC	Res. DAC	Meas. Pk. Width
He	3.0	3.0	591	2080	0.650
Be	9.0	9.0	2026	2080	0.701
Mg	24.0	23.9	5678	2120	0.660
Mg	25.0	25.0	5922	2080	0.759
Mg	26.0	26.0	6155	2120	0.730
Co	58.9	59.0	14164	2170	0.668
Rh	102.9	103.0	24873	2230	0.725
In	114.9	114.9	27778	2260	0.713
Ce	139.9	140.0	33862	2280	0.769
Pb	206.0	205.9	49936	2420	0.779
Pb	207.0	207.0	50147	2385	0.743
Pb	208.0	208.0	50439	2430	0.734
U	238.1	238.0	57729	2470	0.727

ICPMS#6 - Summary Report

Sample ID: Blank

Sample Date/Time: Wednesday, March 24, 2010 15:58:42

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\beniasset1.mth

Dataset File: C:\elandata\Dataset\100323\Blank.201

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[Be	9		ug/L			11
> Sc	45		ug/L		947107	
[Ni	60		ug/L		101	
[> Ge	74		ug/L		167037	
As	75		ug/L		319	
Se	77		ug/L		5187	
Se	82		ug/L		-11	
[Kr	83		ug/L		110	
[> Lu	175		ug/L		102819	
[Tl	205		ug/L		167	

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Be	9	Linear Thru Zero	1.0000
Sc	45	Linear Thru Zero	
Ni	60	Linear Thru Zero	1.0000
Ge	74	Linear Thru Zero	
As	75	Linear Thru Zero	1.0000
Se	77	Linear Thru Zero	
Se	82	Linear Thru Zero	0.9999
Kr	83	Linear Thru Zero	
Lu	175	Linear Thru Zero	
Tl	205	Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[Be	9					
> Sc	45					
[Ni	60					
[> Ge	74					
As	75					
Se	77					
Se	82					
[Kr	83					
[> Lu	175					
[Tl	205					

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: Standard 1

Sample Date/Time: Wednesday, March 24, 2010 16:02:44

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\benlassetl.mth

Dataset File: C:\elandata\Dataset\100323\Standard 1.202

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[Be 9	10.000	ug/L	1.731	2064	0.002
>	Sc 45		ug/L		962124	962123.799
[Ni 60	10.000	ug/L	0.562	5358	0.005
>	Ge 74		ug/L		168454	168453.807
	As 75	10.000	ug/L	6.673	5444	0.030
	Se 77		ug/L		6854	0.010
	Se 82	10.000	ug/L	6.006	395	0.002
[Kr 83		ug/L		112	0.000
>	Lu 175		ug/L		102403	102402.739
[Tl 205	10.000	ug/L	1.354	36107	0.351

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Be	9Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ni	60Linear Thru Zero	1.0000
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	1.0000
Kr	83Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000

QC Calculated Values

Analyte Mass	QC Std	% Recovery	Int Std	% Recovery	Spike	% Recovery	Dilution	% Dil	Duplicate	Rel. % Difference
[Be	9								
>	Sc	45								
[Ni	60								
>	Ge	74								
	As	75								
	Se	77								
	Se	82								
[Kr	83								
>	Lu	175								
[Tl	205								

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: Standard 1

ICPMS#6 - Summary Report

Sample ID: Standard 2

Sample Date/Time: Wednesday, March 24, 2010 16:06:44

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\beniassetl.mth

Dataset File: C:\elandata\Dataset\100323\Standard 2.203

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[Be	9	100.023 ug/L	0.743	21003	0.022
>	Sc	45	ug/L		960946	960946.402
[Ni	60	100.037 ug/L	0.864	54601	0.057
>	Ge	74	ug/L		170378	170377.518
	As	75	100.036 ug/L	3.119	54039	0.315
	Se	77	ug/L		10172	0.029
	Se	82	100.060 ug/L	3.931	4350	0.026
[Kr	83	ug/L		105	-0.000
>	Lu	175	ug/L		103331	103331.127
[Tl	205	99.987 ug/L	1.784	358056	3.464

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Be	9Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ni	60Linear Thru Zero	1.0000
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	1.0000
Kr	83Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000

QC Calculated Values

	Analyte Mass	QC Std	% Recovery	Int Std	% Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[Be	9							
>	Sc	45							
[Ni	60							
>	Ge	74							
	As	75							
	Se	77							
	Se	82							
[Kr	83							
>	Lu	175							
[Tl	205							

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: Standard 2

Report Date/Time: Wednesday, March 24, 2010 16:07:22

ICPMS#6 - Summary Report

Sample ID: QC Std 1

Sample Date/Time: Wednesday, March 24, 2010 16:10:45

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\beniasset1.mth

Dataset File: C:\elandata\Dataset\100323\QC Std 1.204

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[Be	9	50.580 ug/L	1.501	10888	0.011
>	Sc	45	ug/L		984611	984610.629
[Ni	60	51.493 ug/L	0.960	28847	0.029
>	Ge	74	ug/L		173187	173186.886
	As	75	51.401 ug/L	0.722	28396	0.162
	Se	77	ug/L		8915	0.020
	Se	82	51.917 ug/L	2.191	2290	0.013
[Kr	83	ug/L		129	0.000
>	Lu	175	ug/L		103697	103696.709
[Tl	205	50.416 ug/L	1.101	181301	1.747

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Be	9Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ni	60Linear Thru Zero	1.0000
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	1.0000
Kr	83Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000

QC Calculated Values

	Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[Be	9	101.161			
>	Sc	45		104.0		
[Ni	60	102.986			
>	Ge	74		103.7		
	As	75	102.802			
	Se	77				
	Se	82	103.834			
[Kr	83				
>	Lu	175		100.9		
[Tl	205	100.832			

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 1

ICPMS#6 - Summary Report

Sample ID: QC Std 2

Sample Date/Time: Wednesday, March 24, 2010 16:14:48

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\beniassetl.mth

Dataset File: C:\elandata\Dataset\100323\QC Std 2.205

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[Be	9	0.007	ug/L	364.026	12	0.000
> Sc	45		ug/L		962655	962654.980
[Ni	60	0.011	ug/L	255.267	109	0.000
> Ge	74		ug/L		173338	173338.416
As	75	0.322	ug/L	101.556	508	0.001
Se	77		ug/L		5987	0.003
Se	82	-0.282	ug/L	147.971	-24	-0.000
[Kr	83		ug/L		117	0.000
> Lu	175		ug/L		102774	102774.476
[Tl	205	0.156	ug/L	10.213	724	0.005

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Be	9	Linear Thru Zero	1.0000
Sc	45	Linear Thru Zero	
Ni	60	Linear Thru Zero	1.0000
Ge	74	Linear Thru Zero	
As	75	Linear Thru Zero	1.0000
Se	77	Linear Thru Zero	
Se	82	Linear Thru Zero	1.0000
Kr	83	Linear Thru Zero	
Lu	175	Linear Thru Zero	
Tl	205	Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[Be	9					
> Sc	45		101.6			
[Ni	60					
> Ge	74		103.8			
As	75					
Se	77					
Se	82					
[Kr	83					
> Lu	175		100.0			
[Tl	205					

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 2

Report Date/Time: Wednesday, March 24, 2010 16:15:28

ICPMS#6 - Summary Report

Sample ID: QC Std 3

Sample Date/Time: Wednesday, March 24, 2010 16:18:51

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\beniasset1.mth

Dataset File: C:\elandata\Dataset\100323\QC Std 3.206

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Be	9	0.591	ug/L	3.472	137	0.000
> Sc	45		ug/L		979072	979072.007
Ni	60	2.295	ug/L	2.065	1378	0.001
> Ge	74		ug/L		174310	174310.083
As	75	5.680	ug/L	4.911	3455	0.018
Se	77		ug/L		7335	0.011
Se	82	5.473	ug/L	7.392	233	0.001
Kr	83		ug/L		113	-0.000
> Lu	175		ug/L		104013	104013.371
Tl	205	1.159	ug/L	1.982	4344	0.040

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Be	9	Linear Thru Zero	1.0000
Sc	45	Linear Thru Zero	
Ni	60	Linear Thru Zero	1.0000
Ge	74	Linear Thru Zero	
As	75	Linear Thru Zero	1.0000
Se	77	Linear Thru Zero	
Se	82	Linear Thru Zero	1.0000
Kr	83	Linear Thru Zero	
Lu	175	Linear Thru Zero	
Tl	205	Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
Be	9	118.114				
> Sc	45		103.4			
Ni	60	114.750				
> Ge	74		104.4			
As	75	113.602				
Se	77					
Se	82	109.460				
Kr	83					
> Lu	175		101.2			
Tl	205	115.863				

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: QC Std 4

Sample Date/Time: Wednesday, March 24, 2010 16:22:53

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\beniassetl.mth

Dataset File: C:\elandata\Dataset\100323\QC Std 4.207

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Be	9	0.103	ug/L	10.976	33	0.000
> Sc	45		ug/L		987090	987090.063
Ni	60	2.446	ug/L	3.997	1475	0.001
> Ge	74		ug/L		170475	170474.667
As	75	0.011	ug/L	8218.996	332	0.000
Se	77		ug/L		8047	0.016
Se	82	-1.619	ug/L	26.261	-81	-0.000
Kr	83		ug/L		189	0.000
> Lu	175		ug/L		102816	102816.094
Tl	205	0.022	ug/L	10.014	244	0.001

Calibration

Analyte	Mass Curve Type	Correlation Coefficient
Be	9Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ni	60Linear Thru Zero	1.0000
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	1.0000
Kr	83Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel.	% Difference
Be	9						
> Sc	45		104.2				
Ni	60	90.611					
> Ge	74		102.1				
As	75						
Se	77						
Se	82						
Kr	83						
> Lu	175		100.0				
Tl	205						

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 4

Report Date/Time: Wednesday, March 24, 2010 16:23:31

ICPMS#6 - Summary Report

Sample ID: QC Std 5

Sample Date/Time: Wednesday, March 24, 2010 16:26:55

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\beniasset1.mth

Dataset File: C:\elandata\Dataset\100323\QC Std 5.208

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[Be 9	20.027	ug/L	3.893	4312	0.004
>	Sc 45		ug/L		984145	984144.841
[Ni 60	22.093	ug/L	2.659	12426	0.013
>	Ge 74		ug/L		170325	170325.468
	As 75	21.757	ug/L	3.997	12005	0.069
	Se 77		ug/L		8746	0.020
	Se 82	20.015	ug/L	3.340	861	0.005
[Kr 83		ug/L		180	0.000
>	Lu 175		ug/L		102833	102832.808
[Tl 205	19.684	ug/L	0.498	70296	0.682

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Be	9Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ni	60Linear Thru Zero	1.0000
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	1.0000
Kr	83Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000

QC Calculated Values

	Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[Be 9	100.134				
>	Sc 45		103.9			
[Ni 60	97.327				
>	Ge 74		102.0			
	As 75	108.785				
	Se 77					
	Se 82	100.073				
[Kr 83					
>	Lu 175		100.0			
[Tl 205	98.421				

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 5

ICPMS#6 - Summary Report

Sample ID: QC Std 6

Sample Date/Time: Wednesday, March 24, 2010 16:30:56

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\beniasset1.mth

Dataset File: C:\elandata\Dataset\100323\QC Std 6.209

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[Be	9	49.349	ug/L	1.105	10630	0.011
> Sc	45		ug/L		985262	985261.517
[Ni	60	51.290	ug/L	0.971	28756	0.029
> Ge	74		ug/L		175525	175524.929
[As	75	50.380	ug/L	2.085	28209	0.159
Se	77		ug/L		9536	0.023
Se	82	51.877	ug/L	1.235	2319	0.013
[Kr	83		ug/L		110	-0.000
> Lu	175		ug/L		103888	103888.456
[Tl	205	50.052	ug/L	0.751	180310	1.734

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Be	9	Linear Thru Zero	1.0000
Sc	45	Linear Thru Zero	
Ni	60	Linear Thru Zero	1.0000
Ge	74	Linear Thru Zero	
As	75	Linear Thru Zero	1.0000
Se	77	Linear Thru Zero	
Se	82	Linear Thru Zero	1.0000
Kr	83	Linear Thru Zero	
Lu	175	Linear Thru Zero	
Tl	205	Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[Be	9	98.698				
> Sc	45		104.0			
[Ni	60	102.581				
> Ge	74		105.1			
[As	75	100.760				
Se	77					
Se	82	103.754				
[Kr	83					
> Lu	175		101.0			
[Tl	205	100.104				

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 6

ICPMS#6 - Summary Report

Sample ID: QC Std 7

Sample Date/Time: Wednesday, March 24, 2010 16:34:59

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\beniasset1.mth

Dataset File: C:\elandata\Dataset\100323\QC Std 7.210

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[Be	9	0.003	ug/L	418.493	12	0.000
[> Sc	45		ug/L		981333	981333.371
[Ni	60	0.006	ug/L	292.423	108	0.000
[> Ge	74		ug/L		174317	174316.876
As	75	0.026	ug/L	893.056	346	0.000
Se	77		ug/L		6724	0.008
Se	82	-0.027	ug/L	701.307	-12	-0.000
[Kr	83		ug/L		113	-0.000
[> Lu	175		ug/L		103996	103995.571
[Tl	205	0.155	ug/L	2.929	726	0.005

Calibration

Analyte	Mass Curve Type	Correlation Coefficient
Be	9Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ni	60Linear Thru Zero	1.0000
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	1.0000
Kr	83Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel.	% Difference
[Be	9						
[> Sc	45		103.6				
[Ni	60						
[> Ge	74		104.4				
As	75						
Se	77						
Se	82						
[Kr	83						
[> Lu	175		101.1				
[Tl	205						

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 7

ICPMS#6 - Summary Report

Sample ID: 1202056883

Sample Date/Time: Wednesday, March 24, 2010 16:39:02

Sample Type:

Sample Description: LANL 6020 MB

Number of Replicates: 3

Batch ID: 959116[2]rmj

Method File: c:\elandata\Method\beniassetl.mth

Dataset File: C:\elandata\Dataset\100323\1202056883.211

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[Be 9	-0.017	ug/L	89.782	8	-0.000
>	Sc 45		ug/L		1023163	1023163.221
[Ni 60	0.096	ug/L	5.846	165	0.000
>	Ge 74		ug/L		181254	181254.467
	As 75	-0.161	ug/L	24.062	254	-0.001
	Se 77		ug/L		5887	0.001
	Se 82	0.099	ug/L	399.554	-7	0.000
[Kr 83		ug/L		116	-0.000
>	Lu 175		ug/L		109749	109748.788
[Tl 205	0.081	ug/L	4.899	488	0.003

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Be	9Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ni	60Linear Thru Zero	1.0000
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	1.0000
Kr	83Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000

QC Calculated Values

	Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[Be 9					
>	Sc 45		108.0			
[Ni 60					
>	Ge 74		108.5			
	As 75					
	Se 77					
	Se 82					
[Kr 83					
>	Lu 175		106.7			
[Tl 205					

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: 1202056888

Sample Date/Time: Wednesday, March 24, 2010 16:43:03

Sample Type:

Sample Description: LANL 6020 LCS

Number of Replicates: 3

Batch ID: 959116|40|rmj

Method File: c:\elandata\Method\beniassetl.mth

Dataset File: C:\elandata\Dataset\100323\1202056888.212

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[Be 9	24.107	ug/L	0.273	5255	0.005
>	Sc 45		ug/L		995843	995842.528
[Ni 60	42.881	ug/L	1.526	24313	0.024
>	Ge 74		ug/L		176888	176887.568
	As 75	33.310	ug/L	3.072	18909	0.105
	Se 77		ug/L		10562	0.029
	Se 82	90.084	ug/L	0.682	4066	0.023
[Kr 83		ug/L		111	-0.000
>	Lu 175		ug/L		106852	106851.600
[Tl 205	36.992	ug/L	1.895	137087	1.282

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Be	9Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ni	60Linear Thru Zero	1.0000
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	1.0000
Kr	83Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000

QC Calculated Values

Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel. % Difference
[Be 9				
>	Sc 45	105.1			
[Ni 60				
>	Ge 74	105.9			
	As 75				
	Se 77				
	Se 82				
[Kr 83				
>	Lu 175	103.9			
[Tl 205				

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: QC Std 6

Sample Date/Time: Wednesday, March 24, 2010 16:47:04

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\beniasset1.mth

Dataset File: C:\elandata\Dataset\100323\QC Std 6.213

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[Be 9	49.744	ug/L	0.607	10739	0.011
>	Sc 45		ug/L		987456	987456.377
[Ni 60	51.781	ug/L	1.339	29090	0.029
>	Ge 74		ug/L		176574	176573.999
	As 75	50.170	ug/L	1.539	28266	0.158
	Se 77		ug/L		9464	0.023
	Se 82	51.931	ug/L	2.178	2335	0.013
[Kr 83		ug/L		112	-0.000
>	Lu 175		ug/L		104198	104197.519
[Tl 205	50.745	ug/L	1.832	183307	1.758

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Be	9Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ni	60Linear Thru Zero	1.0000
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	1.0000
Kr	83Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000

QC Calculated Values

	Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[Be 9	99.488				
>	Sc 45		104.3			
[Ni 60	103.562				
>	Ge 74		105.7			
	As 75	100.341				
	Se 77					
	Se 82	103.862				
[Kr 83					
>	Lu 175		101.3			
[Tl 205	101.491				

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: QC Std 7

Sample Date/Time: Wednesday, March 24, 2010 16:51:07

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\beniassetl.mth

Dataset File: C:\elandata\Dataset\100323\QC Std 7.214

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[Be	9	0.003	ug/L	556.862	12	0.000
> Sc	45		ug/L		975851	975850.541
[Ni	60	0.001	ug/L	1339.344	105	0.000
> Ge	74		ug/L		174852	174852.034
[As	75	0.564	ug/L	83.958	644	0.002
Se	77		ug/L		6809	0.008
Se	82	1.187	ug/L	27.378	42	0.000
[Kr	83		ug/L		124	0.000
> Lu	175		ug/L		103423	103422.503
[Tl	205	0.192	ug/L	4.777	856	0.007

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Be	9	Linear Thru Zero	1.0000
Sc	45	Linear Thru Zero	
Ni	60	Linear Thru Zero	1.0000
Ge	74	Linear Thru Zero	
As	75	Linear Thru Zero	1.0000
Se	77	Linear Thru Zero	
Se	82	Linear Thru Zero	1.0000
Kr	83	Linear Thru Zero	
Lu	175	Linear Thru Zero	
Tl	205	Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std	% Recovery	Int Std	% Recovery	Spike	% Recovery	Dilution	% Dil	Duplicate	Rel. % Difference
[Be	9										
> Sc	45				103.0						
[Ni	60										
> Ge	74				104.7						
As	75										
Se	77										
Se	82										
[Kr	83										
> Lu	175				100.6						
[Tl	205										

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: 1202056884

Sample Date/Time: Wednesday, March 24, 2010 16:59:12

Sample Type:

Sample Description: LANL 6020 DUP

Number of Replicates: 3

Batch ID: 959116|2|rmj

Method File: c:\elandata\Method\benlassetl.mth

Dataset File: C:\elandata\Dataset\100323\1202056884.216

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Be	9	5.145	ug/L	2.168	1167	0.001
> Sc	45		ug/L		1028718	1028717.607
Ni	60	38.172	ug/L	1.683	22370	0.022
> Ge	74		ug/L		167653	167653.206
As	75	9.509	ug/L	7.776	5348	0.030
Se	77		ug/L		4544	-0.004
Se	82	-0.049	ug/L	997.446	-13	-0.000
Kr	83		ug/L		220	0.001
> Lu	175		ug/L		111692	111692.393
Tl	205	0.920	ug/L	1.435	3743	0.032

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Be	9	Linear Thru Zero	1.0000
Sc	45	Linear Thru Zero	
Ni	60	Linear Thru Zero	1.0000
Ge	74	Linear Thru Zero	
As	75	Linear Thru Zero	1.0000
Se	77	Linear Thru Zero	
Se	82	Linear Thru Zero	1.0000
Kr	83	Linear Thru Zero	
Lu	175	Linear Thru Zero	
Tl	205	Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
Be	9					
> Sc	45		108.6			
Ni	60					
> Ge	74		100.4			
As	75					
Se	77					
Se	82					
Kr	83					
> Lu	175		108.6			
Tl	205					

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: 1202056884

Report Date/Time: Wednesday, March 24, 2010 16:59:50

ICPMS#6 - Summary Report

Sample ID: 1202056886

Sample Date/Time: Wednesday, March 24, 2010 17:03:13

Sample Type:

Sample Description: LANL 6020 MS

Number of Replicates: 3

Batch ID: 959116|2|rmj

Method File: c:\elandata\Method\beniassetl.mth

Dataset File: C:\elandata\Dataset\100323\1202056886.217

Concentration Results

Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[Be 9	29.756	ug/L	1.023	6602	0.006
[> Sc 45		ug/L		1014211	1014211.090
[Ni 60	60.960	ug/L	2.203	35155	0.035
[> Ge 74		ug/L		166511	166511.176
As 75	45.854	ug/L	1.684	24387	0.145
Se 77		ug/L		4769	-0.002
Se 82	7.452	ug/L	11.540	307	0.002
[Kr 83		ug/L		202	0.001
[> Lu 175		ug/L		111237	111236.842
[Tl 205	46.441	ug/L	1.063	179151	1.609

Calibration

Analyte	Mass Curve Type	Correlation Coefficient
Be	9Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ni	60Linear Thru Zero	1.0000
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	1.0000
Kr	83Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000

QC Calculated Values

Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[Be 9					
[> Sc 45		107.1			
[Ni 60					
[> Ge 74		99.7			
As 75					
Se 77					
Se 82					
[Kr 83					
[> Lu 175		108.2			
[Tl 205					

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: 1202056887

Sample Date/Time: Wednesday, March 24, 2010 17:07:15

Sample Type:

Sample Description: LANL 6020 MSD

Number of Replicates: 3

Batch ID: 959116|2|rmj

Method File: c:\elandata\Method\beniassetl.mth

Dataset File: C:\elandata\Dataset\100323\1202056887.218

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Be	9	28.429	ug/L	1.696	6364	0.006
> Sc	45		ug/L		1023059	1023058.689
Ni	60	57.938	ug/L	1.630	33713	0.033
> Ge	74		ug/L		168277	168277.308
As	75	44.357	ug/L	2.078	23853	0.140
Se	77		ug/L		4756	-0.003
Se	82	7.174	ug/L	8.893	298	0.002
Kr	83		ug/L		210	0.001
> Lu	175		ug/L		109881	109880.506
Tl	205	45.427	ug/L	1.580	173080	1.574

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Be	9	Linear Thru Zero	1.0000
Sc	45	Linear Thru Zero	
Ni	60	Linear Thru Zero	1.0000
Ge	74	Linear Thru Zero	
As	75	Linear Thru Zero	1.0000
Se	77	Linear Thru Zero	
Se	82	Linear Thru Zero	1.0000
Kr	83	Linear Thru Zero	
Lu	175	Linear Thru Zero	
Tl	205	Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std	% Recovery	Int Std	% Recovery	Spike %	Recovery	Dilution %	Dil	Duplicate	Rel. % Difference
Be	9										
> Sc	45				108.0						
Ni	60										
> Ge	74				100.7						
As	75										
Se	77										
Se	82										
Kr	83										
> Lu	175				106.9						
Tl	205										

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: 1202056887

ICPMS#6 - Summary Report

Sample ID: 1202056885

Sample Date/Time: Wednesday, March 24, 2010 17:11:18

Sample Type:

Sample Description: LANL 6020 SDILT

Number of Replicates: 3

Batch ID: 959116|10|rmj

Method File: c:\elandata\Method\beniassetl.mth

Dataset File: C:\elandata\Dataset\100323\1202056885.219

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[Be 9	1.042	ug/L	5.992	231	0.000
>	Sc 45		ug/L		967317	967316.637
[Ni 60	7.952	ug/L	2.309	4464	0.005
>	Ge 74		ug/L		168625	168625.198
	As 75	2.087	ug/L	27.604	1431	0.007
	Se 77		ug/L		5725	0.003
	Se 82	0.236	ug/L	78.974	-0	0.000
[Kr 83		ug/L		128	0.000
>	Lu 175		ug/L		104214	104213.517
[Tl 205	0.309	ug/L	7.228	1283	0.011

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Be	9Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ni	60Linear Thru Zero	1.0000
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	1.0000
Kr	83Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000

QC Calculated Values

Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[Be 9				
>	Sc 45	102.1			
[Ni 60				
>	Ge 74	101.0			
	As 75				
	Se 77				
	Se 82				
[Kr 83				
>	Lu 175	101.4			
[Tl 205				

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: 1202056885

Report Date/Time: Wednesday, March 24, 2010 17:11:57

ICPMS#6 - Summary Report

Sample ID: QC Std 6

Sample Date/Time: Wednesday, March 24, 2010 17:27:24

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\beniassetl.mth

Dataset File: C:\elandata\Dataset\100323\QC Std 6.223

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[Be	9	52.518	ug/L	1.120	10788	0.011
[> Sc	45		ug/L		939488	939488.196
[Ni	60	51.465	ug/L	2.110	27507	0.029
[> Ge	74		ug/L		166588	166587.528
As	75	51.759	ug/L	1.284	27498	0.163
Se	77		ug/L		8029	0.017
Se	82	52.571	ug/L	1.571	2230	0.013
[Kr	83		ug/L		117	0.000
[> Lu	175		ug/L		102528	102528.330
[Tl	205	50.535	ug/L	1.691	179649	1.751

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Be	9	Linear Thru Zero	1.0000
Sc	45	Linear Thru Zero	
Ni	60	Linear Thru Zero	1.0000
Ge	74	Linear Thru Zero	
As	75	Linear Thru Zero	1.0000
Se	77	Linear Thru Zero	
Se	82	Linear Thru Zero	1.0000
Kr	83	Linear Thru Zero	
Lu	175	Linear Thru Zero	
Tl	205	Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[Be	9	105.036				
[> Sc	45		99.2			
[Ni	60	102.931				
[> Ge	74		99.7			
As	75	103.518				
Se	77					
Se	82	105.141				
[Kr	83					
[> Lu	175		99.7			
[Tl	205	101.069				

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 6

Report Date/Time: Wednesday, March 24, 2010 17:28:02

ICPMS#6 - Summary Report

Sample ID: QC Std 7

Sample Date/Time: Wednesday, March 24, 2010 17:31:26

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\beniassetl.mth

Dataset File: C:\elandata\Dataset\100323\QC Std 7.224

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[Be 9	0.017	ug/L	81.777	14	0.000
>	Sc 45		ug/L		916851	916850.916
[Ni 60	0.006	ug/L	141.395	101	0.000
>	Ge 74		ug/L		164077	164077.276
[As 75	-0.580	ug/L	20.697	13	-0.002
	Se 77		ug/L		5736	0.004
	Se 82	-0.149	ug/L	471.759	-17	-0.000
[Kr 83		ug/L		118	0.000
>	Lu 175		ug/L		101651	101651.083
[Tl 205	0.138	ug/L	8.217	651	0.005

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Be	9Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ni	60Linear Thru Zero	1.0000
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	1.0000
Kr	83Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000

QC Calculated Values

	Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel.	% Difference
[Be 9						
>	Sc 45			96.8			
[Ni 60						
>	Ge 74			98.2			
	As 75						
	Se 77						
	Se 82						
[Kr 83						
>	Lu 175			98.9			
[Tl 205						

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 7

ICPMS#6 - Summary Report

Sample ID: 248118001

Sample Date/Time: Wednesday, March 24, 2010 17:51:38

Sample Type:

Sample Description: LANL 6020

Number of Replicates: 3

Batch ID: 959116|2|rmj

Method File: c:\elandata\Method\beniasset1.mth

Dataset File: C:\elandata\Dataset\100323\248118001.229

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[Be	9	2.641	ug/L	10.370	577	0.001
> Sc	45		ug/L		982428	982427.638
[Ni	60	9.660	ug/L	3.401	5484	0.005
> Ge	74		ug/L		166264	166263.899
[As	75	3.430	ug/L	29.016	2122	0.011
Se	77		ug/L		4102	-0.006
Se	82	0.918	ug/L	66.983	28	0.000
[Kr	83		ug/L		181	0.000
> Lu	175		ug/L		116693	116692.515
[Tl	205	0.086	ug/L	11.507	535	0.003

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Be	9	Linear Thru Zero	1.0000
Sc	45	Linear Thru Zero	
Ni	60	Linear Thru Zero	1.0000
Ge	74	Linear Thru Zero	
As	75	Linear Thru Zero	1.0000
Se	77	Linear Thru Zero	
Se	82	Linear Thru Zero	1.0000
Kr	83	Linear Thru Zero	
Lu	175	Linear Thru Zero	
Tl	205	Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[Be	9					
> Sc	45		103.7			
[Ni	60					
> Ge	74		99.5			
[As	75					
Se	77					
Se	82					
[Kr	83					
> Lu	175		113.5			
[Tl	205					

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: 248118001

ICPMS#6 - Summary Report

Sample ID: 248118002

Sample Date/Time: Wednesday, March 24, 2010 17:55:40

Sample Type:

Sample Description: LANL 6020

Number of Replicates: 3

Batch ID: 959116|2|rmj

Method File: c:\elandata\Method\beniassetl.mth

Dataset File: C:\elandata\Dataset\100323\248118002.230

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[Be	9	2.756 ug/L	3.885	597	0.001
>	Sc	45	ug/L		974231	974230.605
[Ni	60	10.496 ug/L	1.030	5901	0.006
>	Ge	74	ug/L		167113	167113.488
	As	75	4.326 ug/L	7.295	2598	0.014
	Se	77	ug/L		3984	-0.007
	Se	82	1.433 ug/L	64.200	51	0.000
[Kr	83	ug/L		184	0.000
>	Lu	175	ug/L		116808	116808.098
[Tl	205	0.086 ug/L	8.592	539	0.003

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Be	9Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ni	60Linear Thru Zero	1.0000
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	1.0000
Kr	83Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000

QC Calculated Values

Analyte Mass	QC Std	% Recovery	Int Std	% Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[Be	9						
>	Sc	45		102.9				
[Ni	60						
>	Ge	74		100.0				
	As	75						
	Se	77						
	Se	82						
[Kr	83						
>	Lu	175		113.6				
[Tl	205						

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: 248118003

Sample Date/Time: Wednesday, March 24, 2010 17:59:42

Sample Type:

Sample Description: LANL 6020

Number of Replicates: 3

Batch ID: 959116[2]rmj

Method File: c:\elandata\Method\beniassetl.mth

Dataset File: C:\elandata\Dataset\100323\248118003.231

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[Be	9	3.162 ug/L	2.399	687	0.001
>	Sc	45	ug/L		978685	978685.438
[Ni	60	7.936 ug/L	0.777	4508	0.004
>	Ge	74	ug/L		168878	168877.729
	As	75	3.222 ug/L	9.261	2039	0.010
	Se	77	ug/L		4030	-0.007
	Se	82	0.817 ug/L	46.826	25	0.000
[Kr	83	ug/L		170	0.000
>	Lu	175	ug/L		117387	117386.541
[Tl	205	0.120 ug/L	7.789	678	0.004

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Be	9Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ni	60Linear Thru Zero	1.0000
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	1.0000
Kr	83Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000

QC Calculated Values

	Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel. % Difference
[Be	9				
>	Sc	45		103.3		
[Ni	60				
>	Ge	74		101.1		
	As	75				
	Se	77				
	Se	82				
[Kr	83				
>	Lu	175		114.2		
[Tl	205				

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: 248118003

ICPMS#6 - Summary Report

Sample ID: 248118004

Sample Date/Time: Wednesday, March 24, 2010 18:03:44

Sample Type:

Sample Description: LANL 6020

Number of Replicates: 3

Batch ID: 959116|2|rmj

Method File: c:\elandata\Method\beniassetl.mth

Dataset File: C:\elandata\Dataset\100323\248118004.232

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[Be 9	13.152	ug/L	3.506	2981	0.003
>	Sc 45		ug/L		1034083	1034082.567
[Ni 60	51.949	ug/L	1.334	30564	0.029
>	Ge 74		ug/L		165930	165930.431
	As 75	10.097	ug/L	2.982	5601	0.032
	Se 77		ug/L		4305	-0.005
	Se 82	0.535	ug/L	119.011	13	0.000
[Kr 83		ug/L		278	0.001
>	Lu 175		ug/L		121408	121407.598
[Tl 205	0.742	ug/L	0.872	3317	0.026

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Be	9Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ni	60Linear Thru Zero	1.0000
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	1.0000
Kr	83Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000

QC Calculated Values

Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[Be 9					
> Sc 45		109.2			
[Ni 60					
> Ge 74		99.3			
As 75					
Se 77					
Se 82					
[Kr 83					
> Lu 175		118.1			
[Tl 205					

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: 248118004

ICPMS#6 - Summary Report

Sample ID: 248118005

Sample Date/Time: Wednesday, March 24, 2010 18:07:46

Sample Type:

Sample Description: LANL 6020

Number of Replicates: 3

Batch ID: 959116[2]rmj

Method File: c:\elandata\Method\beniassetl.mth

Dataset File: C:\elandata\Dataset\100323\248118005.233

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[Be	9	2.790 ug/L	3.307	606	0.001
>	Sc	45	ug/L		975570	975570.449
[Ni	60	9.730 ug/L	0.833	5485	0.006
>	Ge	74	ug/L		165987	165986.690
	As	75	3.018 ug/L	20.123	1896	0.010
	Se	77	ug/L		4000	-0.007
	Se	82	1.005 ug/L	65.287	33	0.000
[Kr	83	ug/L		185	0.000
>	Lu	175	ug/L		117926	117925.588
[Tl	205	0.089 ug/L	8.918	557	0.003

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Be	9Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ni	60Linear Thru Zero	1.0000
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	1.0000
Kr	83Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000

QC Calculated Values

Analyte Mass	QC Std	% Recovery	Int Std	% Recovery	Spike %	Recovery	Dilution %	Dil	Duplicate Rel.	% Difference
[Be	9								
>	Sc	45			103.0					
[Ni	60								
>	Ge	74			99.4					
	As	75								
	Se	77								
	Se	82								
[Kr	83								
>	Lu	175			114.7					
[Tl	205								

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: 248118006

Sample Date/Time: Wednesday, March 24, 2010 18:11:48

Sample Type:

Sample Description: LANL 6020

Number of Replicates: 3

Batch ID: 959116|2|rmj

Method File: c:\elandata\Method\beniassetl.mth

Dataset File: C:\elandata\Dataset\100323\248118006.234

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Be	9	3.324	ug/L	4.096	722	0.001
> Sc	45		ug/L		979485	979485.464
[Ni	60	14.665	ug/L	2.251	8248	0.008
> Ge	74		ug/L		165668	165667.512
[As	75	4.166	ug/L	10.644	2494	0.013
Se	77		ug/L		3909	-0.007
Se	82	1.373	ug/L	26.816	48	0.000
[Kr	83		ug/L		180	0.000
> Lu	175		ug/L		116086	116085.588
[Tl	205	0.167	ug/L	0.558	860	0.006

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Be	9	Linear Thru Zero	1.0000
Sc	45	Linear Thru Zero	
Ni	60	Linear Thru Zero	1.0000
Ge	74	Linear Thru Zero	
As	75	Linear Thru Zero	1.0000
Se	77	Linear Thru Zero	
Se	82	Linear Thru Zero	1.0000
Kr	83	Linear Thru Zero	
Lu	175	Linear Thru Zero	
Tl	205	Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
Be	9					
> Sc	45		103.4			
[Ni	60					
> Ge	74		99.2			
As	75					
Se	77					
Se	82					
[Kr	83					
> Lu	175		112.9			
[Tl	205					

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: 248118006

Report Date/Time: Wednesday, March 24, 2010 18:12:27

ICPMS#6 - Summary Report

Sample ID: 248118007

Sample Date/Time: Wednesday, March 24, 2010 18:15:51

Sample Type:

Sample Description: LANL 6020

Number of Replicates: 3

Batch ID: 959116[2]rmj

Method File: c:\elandata\Method\beniasset1.mth

Dataset File: C:\elandata\Dataset\100323\248118007.235

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Be	9	4.681	ug/L	4.173	1048	0.001
> Sc	45		ug/L		1014502	1014501.721
[Ni	60	37.004	ug/L	2.307	21389	0.021
> Ge	74		ug/L		166891	166890.604
As	75	9.262	ug/L	7.730	5192	0.029
Se	77		ug/L		3886	-0.008
Se	82	-0.478	ug/L	72.859	-31	-0.000
[Kr	83		ug/L		210	0.001
> Lu	175		ug/L		112842	112841.710
[Tl	205	0.672	ug/L	2.832	2808	0.023

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Be	9	Linear Thru Zero	1.0000
Sc	45	Linear Thru Zero	
Ni	60	Linear Thru Zero	1.0000
Ge	74	Linear Thru Zero	
As	75	Linear Thru Zero	1.0000
Se	77	Linear Thru Zero	
Se	82	Linear Thru Zero	1.0000
Kr	83	Linear Thru Zero	
Lu	175	Linear Thru Zero	
Tl	205	Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[Be	9					
> Sc	45		107.1			
[Ni	60					
> Ge	74		99.9			
As	75					
Se	77					
Se	82					
[Kr	83					
> Lu	175		109.7			
[Tl	205					

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: 248118007

Report Date/Time: Wednesday, March 24, 2010 18:16:30

ICPMS#6 - Summary Report

Sample ID: QC Std 6

Sample Date/Time: Wednesday, March 24, 2010 18:19:53

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\benlasset1.mth

Dataset File: C:\elandata\Dataset\100323\QC Std 6.236

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Be	9	53.112	ug/L	0.824	10710	0.012
> Sc	45		ug/L		922377	922376.875
Ni	60	51.918	ug/L	0.552	27248	0.029
> Ge	74		ug/L		165241	165240.813
As	75	50.263	ug/L	3.689	26499	0.158
Se	77		ug/L		7388	0.014
Se	82	51.178	ug/L	1.064	2153	0.013
Kr	83		ug/L		123	0.000
> Lu	175		ug/L		101398	101397.933
Tl	205	51.003	ug/L	1.484	179327	1.767

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Be	9Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ni	60Linear Thru Zero	1.0000
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	1.0000
Kr	83Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
Be	9	106.223				
> Sc	45		97.4			
Ni	60	103.836				
> Ge	74		98.9			
As	75	100.527				
Se	77					
Se	82	102.355				
Kr	83					
> Lu	175		98.6			
Tl	205	102.006				

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

Sample ID: QC Std 6

Report Date/Time: Wednesday, March 24, 2010 18:20:31

ICPMS#6 - Summary Report

Sample ID: QC Std 7

Sample Date/Time: Wednesday, March 24, 2010 18:23:55

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\beniasset1.mth

Dataset File: C:\elandata\Dataset\100323\QC Std 7.237

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
Be	9	0.005	ug/L	359.144	11	0.000
> Sc	45		ug/L		913027	913027.117
[Ni	60	0.015	ug/L	221.492	105	0.000
> Ge	74		ug/L		163996	163996.362
As	75	0.266	ug/L	78.867	450	0.001
Se	77		ug/L		5205	0.001
Se	82	-0.085	ug/L	380.048	-14	-0.000
[Kr	83		ug/L		107	-0.000
> Lu	175		ug/L		102339	102338.735
[Tl	205	0.135	ug/L	5.052	645	0.005

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Be	9Linear Thru Zero	1.0000
Sc	45Linear Thru Zero	
Ni	60Linear Thru Zero	1.0000
Ge	74Linear Thru Zero	
As	75Linear Thru Zero	1.0000
Se	77Linear Thru Zero	
Se	82Linear Thru Zero	1.0000
Kr	83Linear Thru Zero	
Lu	175Linear Thru Zero	
Tl	205Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
Be	9					
> Sc	45		96.4			
[Ni	60					
> Ge	74		98.2			
As	75					
Se	77					
Se	82					
[Kr	83					
> Lu	175		99.5			
[Tl	205					

QC Out Of Limits

Measurement Type Analyte

MassOut of Limits Message

QC Action

QC Action Line: No QC out of limits detected

ICPMS #6 Daily Performance Report

Sample ID: Sample

Sample Date/Time: Thursday, March 25, 2010 22:43:40

Sample Description:

Method File: C:\elandata\Method\Daily2.mth

Dataset File: c:\elandata\Dataset\100318\Sample.306

Tuning File: c:\elandata\Tuning\default2.tun

Optimization File: c:\elandata\Optimize\default.dac

Dual Detector Mode: Pulse

Acq. Dead Time(ns): 35

Current Dead Time (ns): 35

Number of Replicates: 5

Summary

Analyte	Mass	Meas. Intens. Mean	Net Intens. Mean	Net Intens. SD	Net Intens. RSD
Be	9.0	2316.0	2315.988	46.340	2.0
Mg	24.0	26605.8	26605.757	397.514	1.5
Co	58.9	35612.5	35612.535	243.017	0.7
Rh	102.9	71318.6	71318.603	927.372	1.3
In	114.9	76348.1	76348.091	817.381	1.1
Pb	208.0	42447.4	42447.374	415.016	1.0
[> Ba	137.9	70551.7	70551.711	1034.013	1.5
[Ba++	69.0	1910.1	0.027	0.001	1.9
[> Ce	139.9	91805.9	91805.864	795.215	0.9
[CeO	155.9	1832.9	0.020	0.000	1.5
Bkgd	220.0	17.8	17.800	2.308	13.0

Current Optimization File Data

Current Value	Description
0.80	Nebulizer Gas Flow
8.75	Lens Voltage
1450.00	ICP RF Power
-1800.00	Analog Stage Voltage
900.00	Pulse Stage Voltage
30.00	Discriminator Threshold
-6.00	AC Rod Offset

Current Autolens Data

Analyte	Mass	Num of Pts	DAC Value	Maximum Intensity
Be	9	21	7.3	2985.0
Co	59	21	8.0	34103.7
In	115	21	9.0	77537.2

ICPMS #6 Instrument Tuning Report

File Name: default2.tun
File Path: c:\elandata\Tuning

Analyte	Exact Mass	Meas. Mass	Mass DAC	Res. DAC	Meas. Pk. Width
He	3.0	3.0	584	2080	0.655
Be	9.0	9.1	2055	2080	0.676
Mg	24.0	24.0	5674	2120	0.601
Mg	25.0	25.0	5930	2080	0.677
Mg	26.0	25.9	6152	2120	0.713
Co	58.9	58.9	14160	2170	0.657
Rh	102.9	102.9	24847	2230	0.706
In	114.9	115.0	27789	2260	0.699
Ce	139.9	139.9	33848	2280	0.755
Pb	206.0	206.0	49948	2420	0.746
Pb	207.0	207.0	50135	2385	0.711
Pb	208.0	208.0	50439	2430	0.727
U	238.1	238.1	57729	2470	0.712

ICPMS#6 - Summary Report

Sample ID: Blank

Sample Date/Time: Thursday, March 25, 2010 23:39:49

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\lu.mth

Dataset File: C:\elandata\Dataset\100325\Blank.007

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[> Lu	175		ug/L		99203	
[U	238		ug/L		26	

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[> Lu	175					
[U	238					

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: Standard 1

Sample Date/Time: Thursday, March 25, 2010 23:42:53

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\U.mth

Dataset File: C:\elandata\Dataset\100325\Standard 1.008

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175	ug/L		100494	100493.600
[U	238	10.000 ug/L	1.205	53935	0.536

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	1.0000

QC Calculated Values

	Analyte Mass	QC Std	% Recovery	Int Std	% Recovery	Spike	% Recov	Dilution	% Di	Duplicate	Rel. % Difference
[>	Lu	175									
[U	238									

QC Out Of Limits

Measurement Type	Analyte	Mass Out of Limits	Message
------------------	---------	--------------------	---------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: Standard 2

Sample Date/Time: Thursday, March 25, 2010 23:45:55

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\w.mth

Dataset File: C:\elandata\Dataset\100325\Standard 2.009

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175	ug/L		99977	99976.627
[U	238	100.007 ug/L	0.802	540187	5.403

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	1.0000

QC Calculated Values

	Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[>	Lu	175				
[U	238				

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: QC Std 1

Sample Date/Time: Thursday, March 25, 2010 23:48:58

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\w.mth

Dataset File: C:\elandata\Dataset\100325\QC Std 1.010

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[> Lu	175		ug/L		98148	98147.755
[U	238	54.121	ug/L	0.090	287013	2.924

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[> Lu	175			98.9		
[U	238	108.242				

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: QC Std 2

Sample Date/Time: Thursday, March 25, 2010 23:52:03

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\w.mth

Dataset File: C:\elandata\Dataset\100325\QC Std 2.011

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[> Lu	175		ug/L		96948	96947.556
[U	238	0.011	ug/L	17.119	84	0.001

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[> Lu	175			97.7		
[U	238					

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: QC Std 3

Sample Date/Time: Thursday, March 25, 2010 23:55:08

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\lu.mth

Dataset File: C:\elandata\Dataset\100325\QC Std 3.012

Concentration Results

Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[> Lu 175		ug/L		99178	99177.738
[U 238	0.218	ug/L	1.805	1193	0.012

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	1.0000

QC Calculated Values

Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[> Lu 175			100.0		
[U 238	108.910				

QC Out Of Limits

Measurement Type	Analyte	MassOut of Limits Message
------------------	---------	---------------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: QC Std 4

Sample Date/Time: Thursday, March 25, 2010 23:58:12

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\w.mth

Dataset File: C:\elandata\Dataset\100325\QC Std 4.013

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[> Lu	175		ug/L		98268	98267.831
[U	238	0.005	ug/L	36.082	54	0.000

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[> Lu	175		99.1				
[U	238						

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: QC Std 5

Sample Date/Time: Friday, March 26, 2010 00:01:16

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\l.u.mth

Dataset File: C:\elandata\Dataset\100325\QC Std 5.014

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175	ug/L		98559	98559.477
[U	238	ug/L	0.314	115886	1.176

Calibration

Analyte	Mass Curve Type	Correlation Coefficient
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	1.0000

QC Calculated Values

	Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[>	Lu	175		99.4		
[U	238	108.792			

QC Out Of Limits

Measurement Type	Analyte	Mass Out of Limits Message
------------------	---------	----------------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: QC Std 6

Sample Date/Time: Friday, March 26, 2010 00:04:20

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\l.u.mth

Dataset File: C:\elandata\Dataset\100325\QC Std 6.015

Concentration Results

Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[> Lu 175		ug/L		98667	98666.564
[U 238	53.804	ug/L	0.812	286821	2.907

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	1.0000

QC Calculated Values

Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[> Lu 175			99.5		
[U 238	107.608				

QC Out Of Limits

Measurement Type	Analyte	MassOut of Limits Message
------------------	---------	---------------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: QC Std 7

Sample Date/Time: Friday, March 26, 2010 00:07:24

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\w.mth

Dataset File: C:\elandata\Dataset\100325\QC Std 7.016

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu 175		ug/L		98475	98475.259
[U 238	0.008	ug/L	17.468	69	0.000

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	1.0000

QC Calculated Values

	Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[>	Lu 175			99.3		
[U 238					

QC Out Of Limits

Measurement Type	Analyte	MassOut of Limits Message
------------------	---------	---------------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: QC Std 6

Sample Date/Time: Friday, March 26, 2010 00:32:02

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\w.mth

Dataset File: C:\elandata\Dataset\100325\QC Std 6.024

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175	ug/L		97410	97409.634
[U	238	54.025 ug/L	0.622	284341	2.919

Calibration

Analyte	Mass Curve Type	Correlation Coefficient
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	1.0000

QC Calculated Values

	Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[>	Lu	175		98.2		
[U	238	108.049			

QC Out Of Limits

Measurement Type	Analyte	Mass Out of Limits Message
------------------	---------	----------------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: QC Std 7

Sample Date/Time: Friday, March 26, 2010 00:35:07

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\w.mth

Dataset File: C:\elandata\Dataset\100325\QC Std 7.025

Concentration Results

Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[> Lu 175		ug/L		96914	96914.274
[U 238	0.012	ug/L	10.073	87	0.001

Calibration

Analyte	Mass Curve Type	Correlation Coefficient
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	1.0000

QC Calculated Values

Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel.	% Difference
[> Lu 175			97.7			
[U 238						

QC Out Of Limits

Measurement Type	Analyte	Mass Out of Limits Message
------------------	---------	----------------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: 1202056883

Sample Date/Time: Friday, March 26, 2010 00:38:13

Sample Type:

Sample Description: LANL 6020 MB

Number of Replicates: 3

Batch ID: 959116[2]rmj

Method File: c:\elandata\Method\lu.mth

Dataset File: C:\elandata\Dataset\100325\1202056883.026

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175	ug/L		97967	97967.083
[U	238	0.007 ug/L	16.969	61	0.000

Calibration

Analyte	Mass Curve Type	Correlation Coefficient
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	1.0000

QC Calculated Values

	Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[>	Lu	175		98.8		
[U	238				

QC Out Of Limits

Measurement Type Analyte Mass Out of Limits Message

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: 1202056888

Sample Date/Time: Friday, March 26, 2010 00:41:16

Sample Type:

Sample Description: LANL 6020 LCS

Number of Replicates: 3

Batch ID: 959116|40|rmj

Method File: c:\elandata\Method\w.mth

Dataset File: C:\elandata\Dataset\100325\1202056888.027

Concentration Results

Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[> Lu 175		ug/L		100155	100155.215
[U 238	0.616	ug/L	1.792	3357	0.033

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	1.0000

QC Calculated Values

Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dil	Duplicate Rel. % Difference
[> Lu 175		101.0			
[U 238					

QC Out Of Limits

Measurement Type	Analyte	Mass Out of Limits Message
------------------	---------	----------------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: 1202056884

Sample Date/Time: Friday, March 26, 2010 00:47:22

Sample Type:

Sample Description: LANL 6020 DUP

Number of Replicates: 3

Batch ID: 959116[2]rmj

Method File: c:\elandata\Method\l.u.mth

Dataset File: C:\elandata\Dataset\100325\1202056884.029

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175	ug/L		105661	105660.701
[U	238	24.291 ug/L	1.113	138690	1.312

Calibration

Analyte	Mass Curve Type	Correlation Coefficient
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	1.0000

QC Calculated Values

	Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[>	Lu	175		106.5		
[U	238				

QC Out Of Limits

Measurement Type	Analyte	Mass Out of Limits Message
------------------	---------	----------------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: 1202056886

Sample Date/Time: Friday, March 26, 2010 00:50:26

Sample Type:

Sample Description: LANL 6020 MS

Number of Replicates: 3

Batch ID: 959116|2|rmj

Method File: c:\elandata\Method\lu.mth

Dataset File: C:\elandata\Dataset\100325\1202056886.030

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175	ug/L		106328	106328.324
[U	238	45.722 ug/L	0.838	262671	2.470

Calibration

Analyte	Mass Curve Type	Correlation Coefficient
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	1.0000

QC Calculated Values

	Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[>	Lu	175		107.2		
[U	238				

QC Out Of Limits

Measurement Type	Analyte	Mass Out of Limits Message
------------------	---------	----------------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: 1202056887

Sample Date/Time: Friday, March 26, 2010 00:53:30

Sample Type:

Sample Description: LANL 6020 MSD

Number of Replicates: 3

Batch ID: 959116|2|rm|

Method File: c:\elandata\Method\w.mth

Dataset File: C:\elandata\Dataset\100325\1202056887.031

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175	ug/L		105688	105688.255
[U	238	43.816 ug/L	0.166	250218	2.367

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	1.0000

QC Calculated Values

	Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[>	Lu	175		106.5		
[U	238				

QC Out Of Limits

Measurement Type Analyte MassOut of Limits Message

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: 1202056885

Sample Date/Time: Friday, March 26, 2010 00:56:35

Sample Type:

Sample Description: LANL 6020 SDILT

Number of Replicates: 3

Batch ID: 959116|10|rmj

Method File: c:\elandata\Method\w.mth

Dataset File: C:\elandata\Dataset\100325\1202056885.032

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
>	Lu	175	ug/L		101976	101975.710
L	U	238	4.001 ug/L	0.368	22069	0.216

Calibration

Analyte	Mass Curve Type	Correlation Coefficient
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	1.0000

QC Calculated Values

	Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
>	Lu	175		102.8		
L	U	238				

QC Out Of Limits

Measurement Type	Analyte	Mass Out of Limits Message
------------------	---------	----------------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: QC Std 6

Sample Date/Time: Friday, March 26, 2010 01:02:42

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\l.u.mth

Dataset File: C:\elandata\Dataset\100325\QC Std 6.034

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[> Lu	175		ug/L		98702	98702.149
[U	238	53.844	ug/L	1.297	287135	2.909

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recov	Dilution % Dif	Duplicate Rel. % Difference
[> Lu	175			99.5		
[U	238	107.688				

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: QC Std 7

Sample Date/Time: Friday, March 26, 2010 01:05:47

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\lu.mth

Dataset File: C:\elandata\Dataset\100325\QC Std 7.035

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175	ug/L		97284	97284.462
[U	238	0.009 ug/L	25.453	71	0.000

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	1.0000

QC Calculated Values

	Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[>	Lu	175		98.1		
[U	238				

QC Out Of Limits

Measurement Type	Analyte	MassOut of Limits Message
------------------	---------	---------------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: 248118001

Sample Date/Time: Friday, March 26, 2010 01:27:17

Sample Type:

Sample Description: LANL 6020

Number of Replicates: 3

Batch ID: 959116[2|rm]

Method File: c:\elandata\Method\w.mth

Dataset File: C:\elandata\Dataset\100325\248118001.042

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[> Lu	175		ug/L		109410	109410.465
[U	238	3.161	ug/L	2.002	18713	0.171

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[> Lu	175		110.3			
[U	238					

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: 248118002

Sample Date/Time: Friday, March 26, 2010 01:30:21

Sample Type:

Sample Description: LANL 6020

Number of Replicates: 3

Batch ID: 959116|2|rmj

Method File: c:\elandata\Method\w.mth

Dataset File: C:\elandata\Dataset\100325\248118002.043

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175	ug/L		111155	111155.219
[U	238	3.383 ug/L	1.354	20347	0.183

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	1.0000

QC Calculated Values

	Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[>	Lu	175		112.0		
[U	238				

QC Out Of Limits

Measurement Type	Analyte	Mass Out of Limits Message
------------------	---------	----------------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: 248118003

Sample Date/Time: Friday, March 26, 2010 01:33:25

Sample Type:

Sample Description: LANL 6020

Number of Replicates: 3

Batch ID: 959116|2|rmj

Method File: c:\elandata\Method\w.mth

Dataset File: C:\elandata\Dataset\100325\248118003.044

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175	ug/L		107609	107609.179
[U	238	2.936 ug/L	0.738	17099	0.159

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	1.0000

QC Calculated Values

	Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[>	Lu	175		108.5		
[U	238				

QC Out Of Limits

Measurement Type	Analyte	MassOut of Limits Message
------------------	---------	---------------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: QC Std 6

Sample Date/Time: Friday, March 26, 2010 01:36:29

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\w.mth

Dataset File: C:\elandata\Dataset\100325\QC Std 6.045

Concentration Results

Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
> Lu 175		ug/L		98026	98025.507
[U 238	53.622	ug/L	0.367	284017	2.897

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	1.0000

QC Calculated Values

Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
> Lu 175		98.8			
[U 238	107.245				

QC Out Of Limits

Measurement Type	Analyte	MassOut of Limits Message
------------------	---------	---------------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: QC Std 7

Sample Date/Time: Friday, March 26, 2010 01:39:34

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\w.mth

Dataset File: C:\elandata\Dataset\100325\QC Std 7.046

Concentration Results

Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[> Lu 175		ug/L		98590	98590.024
[U 238	0.008	ug/L	18.318	69	0.000

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	1.0000

QC Calculated Values

Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[> Lu 175			99.4		
[U 238					

QC Out Of Limits

Measurement Type	Analyte	Mass Out of Limits Message
------------------	---------	----------------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: 248118004

Sample Date/Time: Friday, March 26, 2010 01:42:39

Sample Type:

Sample Description: LANL 6020

Number of Replicates: 3

Batch ID: 959116|2|rmj

Method File: c:\elandata\Method\w.mth

Dataset File: C:\elandata\Dataset\100325\248118004.047

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175	ug/L		114874	114874.213
[U	238	6.678 ug/L	0.530	41474	0.361

Calibration

Analyte	Mass Curve Type	Correlation Coefficient
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	1.0000

QC Calculated Values

	Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel.	% Difference
[>	Lu	175		115.8			
[U	238					

QC Out Of Limits

Measurement Type	Analyte	Mass Out of Limits Message
------------------	---------	----------------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: 248118005

Sample Date/Time: Friday, March 26, 2010 01:45:44

Sample Type:

Sample Description: LANL 6020

Number of Replicates: 3

Batch ID: 959116|2|rmj

Method File: c:\elandata\Method\w.mth

Dataset File: C:\elandata\Dataset\100325\248118005.048

Concentration Results

Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[> Lu 175		ug/L		112181	112180.553
[U 238	3.890	ug/L	1.174	23606	0.210

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	1.0000

QC Calculated Values

Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[> Lu 175		113.1			
[U 238					

QC Out Of Limits

Measurement Type	Analyte	MassOut of Limits Message
------------------	---------	---------------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: 248118006

Sample Date/Time: Friday, March 26, 2010 01:48:48

Sample Type:

Sample Description: LANL 6020

Number of Replicates: 3

Batch ID: 959116|2|rmj

Method File: c:\elandata\Method\w.mth

Dataset File: C:\elandata\Dataset\100325\248118006.049

Concentration Results

Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[> Lu 175		ug/L		111483	111482.766
[U 238	3.323	ug/L	1.023	20040	0.180

Calibration

Analyte	Mass Curve Type	Correlation Coefficient
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	1.0000

QC Calculated Values

Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[> Lu 175		112.4			
[U 238					

QC Out Of Limits

Measurement Type	Analyte	Mass Out of Limits Message
------------------	---------	----------------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: 248118007
Sample Date/Time: Friday, March 26, 2010 01:51:52
Sample Type:
Sample Description: LANL 6020
Number of Replicates: 3
Batch ID: 959116|2|rmj
Method File: c:\elandata\Method\l.u.mth
Dataset File: C:\elandata\Dataset\100325\248118007.050

Concentration Results

Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[> Lu 175		ug/L		107898	107897.687
[U 238	3.729	ug/L	0.735	21766	0.201

Calibration

Analyte	Mass Curve Type	Correlation Coefficient
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	1.0000

QC Calculated Values

Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[> Lu 175		108.8			
[U 238					

QC Out Of Limits

Measurement Type	Analyte	Mass Out of Limits Message
------------------	---------	----------------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: QC Std 6

Sample Date/Time: Friday, March 26, 2010 01:54:55

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\w.mth

Dataset File: C:\elandata\Dataset\100325\QC Std 6.051

Concentration Results

	Analyte Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[>	Lu	175	ug/L		99711	99711.459
[U	238	53.804 ug/L	0.596	289869	2.907

Calibration

Analyte	MassCurve Type	Correlation Coefficient
Lu	175Linear Thru Zero	
U	238Linear Thru Zero	1.0000

QC Calculated Values

	Analyte Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dif	Duplicate Rel. % Difference
[>	Lu	175		100.5		
[U	238	107.608			

QC Out Of Limits

Measurement Type	Analyte	Mass Out of Limits Message
------------------	---------	----------------------------

QC Action

QC Action Line: No QC out of limits detected

ICPMS#6 - Summary Report

Sample ID: QC Std 7

Sample Date/Time: Friday, March 26, 2010 01:58:00

Sample Type:

Sample Description:

Number of Replicates: 3

Batch ID:

Method File: c:\elandata\Method\w.mth

Dataset File: C:\elandata\Dataset\100325\QC Std 7.052

Concentration Results

Analyte	Mass	Conc. Mean	Report Unit	Conc. RSD	Meas. Intens. Mean	Net Intens. Mean
[> Lu	175		ug/L		97411	97411.000
[U	238	0.011	ug/L	27.009	81	0.001

Calibration

Analyte	Mass	Curve Type	Correlation Coefficient
Lu	175	Linear Thru Zero	
U	238	Linear Thru Zero	1.0000

QC Calculated Values

Analyte	Mass	QC Std % Recovery	Int Std % Recovery	Spike % Recovery	Dilution % Dil	Duplicate Rel. % Difference
[> Lu	175			98.2		
[U	238					

QC Out Of Limits

Measurement Type	Analyte	Mass	Out of Limits Message
------------------	---------	------	-----------------------

QC Action

QC Action Line: No QC out of limits detected

Method Name: SOIL
 Method Description: 7471A, ILM04 ANALYST JXL1
 Element: Hg

Date: 03/10/2010
 Technique: FI-MHS
 Calibration Type:
 Hg, Calc. Intercept : Linear
 Wavelength: 253.7 nm
 Sample Info Name: 031010S1.SIF Results Data Set Name: 031010S1

Element: Hg Seq. No.: 1 AS Loc.: 1 Date: 03/10/2010
 Sample ID: Calib Blank

Repl #	SampleConc µg/L	StndConc µg/L	Blncorr Signal	Peak Height	Time	Peak Stored
1			0.0034	0.0034	11:24:32	No
2			0.0034	0.0034	11:25:08	No
Mean:			0.0034			
SD :			0.0000			
%RSD:			1.3036			

Auto-zero performed.

Element: Hg Seq. No.: 2 AS Loc.: 2 Date: 03/10/2010
 Sample ID: S0.2

Repl #	SampleConc µg/L	StndConc µg/L	Blncorr Signal	Peak Height	Time	Peak Stored
1			0.0022	0.0057	11:26:31	No
2			0.0022	0.0056	11:27:05	No
Mean:			0.0022			
SD :			0.0001			
%RSD:			2.2945			

[Hg] Standard number 1 applied. [0.200]
 Correlation Coefficient: 1.00000 Slope: 0.01100
 Intercept : 0.00000

Element: Hg Seq. No.: 3 AS Loc.: 3 Date: 03/10/2010
 Sample ID: S0.5

Repl #	SampleConc µg/L	StndConc µg/L	Blncorr Signal	Peak Height	Time	Peak Stored
1			0.0054	0.0089	11:28:28	No
2			0.0052	0.0086	11:29:02	No
Mean:			0.0053			
SD :			0.0002			
%RSD:			3.6849			

[Hg] Standard number 2 applied. [0.500]
 Correlation Coefficient: 0.99986 Slope: 0.01060
 Intercept : 0.00003

Element: Hg Seq. No.: 4 AS Loc.: 4 Date: 03/10/2010
 Sample ID: S2.0

Repl #	SampleConc µg/L	StndConc µg/L	Blncorr Signal	Peak Height	Time	Peak Stored
1			0.0218	0.0252	11:30:27	No
2			0.0211	0.0245	11:31:01	No
Mean:			0.0214			
SD :			0.0005			
%RSD:			2.3140			

[Hg] Standard number 3 applied. [2.000]

Correlation Coefficient: 0.99999
Intercept : 0.00001

Slope: 0.01071

=====

Element: Hg Seq. No.: 5 AS Loc.: 5 Date: 03/10/2010
Sample ID: S5.0

Repl #	SampleConc µg/L	StndConc µg/L	BlkCorr Signal	Peak Height	Time	Peak Stored
1			0.0551	0.0585	11:32:26	No
2			0.0548	0.0582	11:33:01	No
Mean:			0.0550			
SD :			0.0002			
%RSD:			0.3529			

[Hg] Standard number 4 applied. [5.000]

Correlation Coefficient: 0.99995

Slope: 0.01099

Intercept : -0.00014

=====

Element: Hg Seq. No.: 6 AS Loc.: 6 Date: 03/10/2010
Sample ID: S10

Repl #	SampleConc µg/L	StndConc µg/L	BlkCorr Signal	Peak Height	Time	Peak Stored
1			0.1104	0.1138	11:34:28	No
2			0.1066	0.1101	11:35:03	No
Mean:			0.1085			
SD :			0.0026			
%RSD:			2.4402			

[Hg] Standard number 5 applied. [10.00]


Correlation Coefficient: 0.99997

Slope: 0.01088

Intercept : -0.00001

Calibration data for Hg

Standard ID	Mean Signal (Pk Height)	Entered Concentration (µg/L)	Calculated Concentration (µg/L)	Standard Deviation	%RSD
Calib Blank	0.0034	---	----	----	----
S0.2	0.0022	0.200	0.204	0.0001	2.3
S0.5	0.0053	0.500	0.489	0.0002	3.7
S2.0	0.0214	2.000	1.973	0.0005	2.3
S5.0	0.0550	5.000	5.054	0.0002	0.4
S10	0.1085	10.000	9.979	0.0026	2.4
Correlation Coefficient: 0.99997		Slope:	0.01088	Intercept:	0.0000

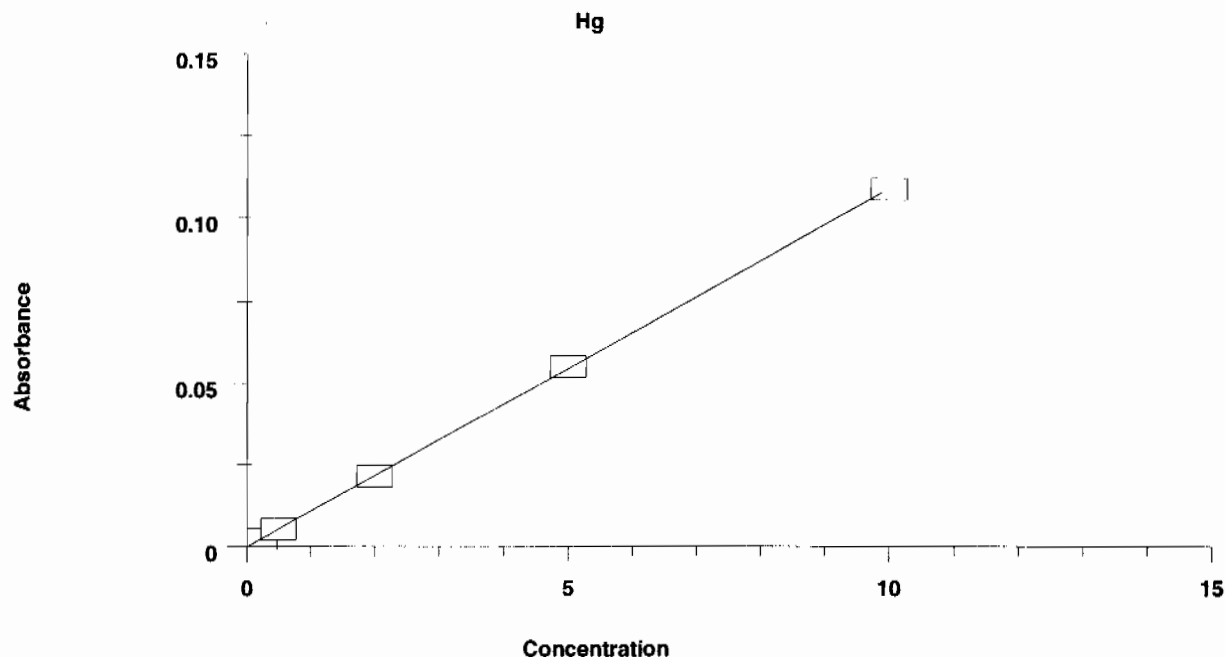

=====
 Element: Hg Seq. No.: 7 AS Loc.: 9 Date: 03/10/2010
 Sample ID: ICV
 =====

Repl #	SampleConc µg/L	StdConc µg/L	BlkCorr Signal	Peak Height	Time	Peak Stored
1	5.283	5.283	0.0574	0.0609	11:36:31	No
2	5.297	5.297	0.0576	0.0610	11:37:06	No
Mean:	5.290	5.290	0.0575			
SD :	0.0104	0.0104	0.0001			
%RSD:	0.2	0.2	0.1961			

QC value within specified limits.

=====
 Element: Hg Seq. No.: 8 AS Loc.: 10 Date: 03/10/2010
 Sample ID: ICB
 =====

Repl #	SampleConc µg/L	StdConc µg/L	BlkCorr Signal	Peak Height	Time	Peak Stored
1	-0.093	-0.093	-0.0010	0.0024	11:38:29	No
2	-0.096	-0.096	-0.0011	0.0024	11:39:03	No
Mean:	-0.095	-0.095	-0.0010			
SD :	0.0021	0.0021	0.0000			
%RSD:	2.2	2.2	2.1790			

QC value within specified limits.

=====
 Element: Hg Seq. No.: 9 AS Loc.: 11 Date: 03/10/2010
 Sample ID: CRDL
 =====

Repl #	SampleConc µg/L	StdConc µg/L	BlkCorr Signal	Peak Height	Time	Peak Stored
1	0.219	0.219	0.0024	0.0058	11:40:27	No
2	0.202	0.202	0.0022	0.0056	11:41:02	No
Mean:	0.210	0.210	0.0023			
SD :	0.0120	0.0120	0.0001			
%RSD:	5.7	5.7	5.7195			

QC value within specified limits.

=====

Element: Hg Seq. No.: 10 AS Loc.: 7 Date: 03/10/2010
 Sample ID: CCV

Repl #	SampleConc µg/L	StndConc µg/L	BlncCorr Signal	Peak Height	Time	Peak Stored
1	5.274	5.274	0.0574	0.0608	11:42:28	No
2	5.053	5.053	0.0549	0.0584	11:43:02	No
Mean:	5.164	5.164	0.0561			
SD :	0.1562	0.1562	0.0017			
%RSD:	3.0	3.0	3.0253			

QC value within specified limits.

=====

Element: Hg Seq. No.: 11 AS Loc.: 8 Date: 03/10/2010
 Sample ID: CCB

Repl #	SampleConc µg/L	StndConc µg/L	BlncCorr Signal	Peak Height	Time	Peak Stored
1	-0.002	-0.002	0.0000	0.0034	11:44:30	No
2	-0.001	-0.001	0.0000	0.0034	11:45:04	No
Mean:	-0.002	-0.002	0.0000			
SD :	0.0012	0.0012	0.0000			
%RSD:	78.7	78.7	43.6378			

QC value within specified limits.

=====

Element: Hg Seq. No.: 12 AS Loc.: 12 Date: 03/10/2010
 Sample ID: 1202056179|i||958757|MB

Repl #	SampleConc µg/L	StndConc µg/L	BlncCorr Signal	Peak Height	Time	Peak Stored
1	-0.056	-0.056	-0.0006	0.0028	11:46:31	No
2	-0.082	-0.082	-0.0009	0.0025	11:47:06	No
Mean:	-0.069	-0.069	-0.0008			
SD :	0.0181	0.0181	0.0002			
%RSD:	26.3	26.3	25.8466			

=====

Element: Hg Seq. No.: 13 AS Loc.: 13 Date: 03/10/2010
 Sample ID: 1202056180|i|10|LCS

Repl #	SampleConc µg/L	StndConc µg/L	BlncCorr Signal	Peak Height	Time	Peak Stored
1	3.686	3.686	0.0401	0.0435	11:48:31	No
2	3.631	3.631	0.0395	0.0429	11:49:06	No
Mean:	3.658	3.658	0.0398			
SD :	0.0388	0.0388	0.0004			
%RSD:	1.1	1.1	1.0601			

=====

Element: Hg Seq. No.: 14 AS Loc.: 14 Date: 03/10/2010
 Sample ID: 248068001|i|||

Repl #	SampleConc µg/L	StndConc µg/L	BlncCorr Signal	Peak Height	Time	Peak Stored
1	0.013	0.013	0.0001	0.0035	11:50:32	No
2	0.022	0.022	0.0002	0.0036	11:51:07	No
Mean:	0.017	0.017	0.0002			
SD :	0.0062	0.0062	0.0001			
%RSD:	35.5	35.5	38.2585			

=====

Element: Hg Seq. No.: 15 AS Loc.: 15 Date: 03/10/2010
 Sample ID: 1202056181|i|||DUP

Repl #	SampleConc µg/L	StdConc µg/L	BlkCorr Signal	Peak Height	Time	Peak Stored
1	-0.035	-0.035	-0.0004	0.0030	11:52:33	No
2	-0.035	-0.035	-0.0004	0.0030	11:53:08	No
Mean:	-0.035	-0.035	-0.0004			
SD :	0.0000	0.0000	0.0000			
%RSD:						

=====

Element: Hg Seq. No.: 16 AS Loc.: 16 Date: 03/10/2010
Sample ID: 1202056182|i|||MS

Repl #	SampleConc µg/L	StdConc µg/L	BlkCorr Signal	Peak Height	Time	Peak Stored
1	2.093	2.093	0.0228	0.0262	11:54:36	No
2	2.071	2.071	0.0225	0.0259	11:55:11	No
Mean:	2.082	2.082	0.0226			
SD :	0.0159	0.0159	0.0002			
%RSD:	0.8	0.8	0.7658			

=====

Element: Hg Seq. No.: 17 AS Loc.: 17 Date: 03/10/2010
Sample ID: 1202056184|i|||MSD

Repl #	SampleConc µg/L	StdConc µg/L	BlkCorr Signal	Peak Height	Time	Peak Stored
1	2.151	2.151	0.0234	0.0268	11:56:35	No
2	2.086	2.086	0.0227	0.0261	11:57:10	No
Mean:	2.119	2.119	0.0230			
SD :	0.0462	0.0462	0.0005			
%RSD:	2.2	2.2	2.1814			

=====

Element: Hg Seq. No.: 18 AS Loc.: 18 Date: 03/10/2010
Sample ID: 1202056183|i|5||SDILT

Repl #	SampleConc µg/L	StdConc µg/L	BlkCorr Signal	Peak Height	Time	Peak Stored
1	-0.111	-0.111	-0.0012	0.0022	11:58:32	No
2	-0.114	-0.114	-0.0012	0.0022	11:59:06	No
Mean:	-0.112	-0.112	-0.0012			
SD :	0.0015	0.0015	0.0000			
%RSD:	1.4	1.4	1.3550			

=====

Element: Hg Seq. No.: 19 AS Loc.: 19 Date: 03/10/2010
Sample ID: 248068002|i|||

Repl #	SampleConc µg/L	StdConc µg/L	BlkCorr Signal	Peak Height	Time	Peak Stored
1	0.261	0.261	0.0028	0.0062	12:00:28	No
2	0.260	0.260	0.0028	0.0062	12:01:03	No
Mean:	0.261	0.261	0.0028			
SD :	0.0008	0.0008	0.0000			
%RSD:	0.3	0.3	0.2969			

=====

Element: Hg Seq. No.: 20 AS Loc.: 20 Date: 03/10/2010
Sample ID: 248110001|i|||

Repl #	SampleConc µg/L	StdConc µg/L	BlkCorr Signal	Peak Height	Time	Peak Stored
1	0.257	0.257	0.0028	0.0062	12:02:25	No
2	0.247	0.247	0.0027	0.0061	12:03:00	No
Mean:	0.252	0.252	0.0027			
SD :	0.0077	0.0077	0.0001			

%RSD: 3.1 3.1 3.0785

=====
 Element: Hg Seq. No.: 21 AS Loc.: 21 Date: 03/10/2010
 Sample ID: 248110002|i|||

Repl #	SampleConc µg/L	StdndConc µg/L	BlncCorr Signal	Peak Height	Time	Peak Stored
1	0.233	0.233	0.0025	0.0059	12:04:22	No
2	0.243	0.243	0.0026	0.0060	12:04:57	No
Mean:	0.238	0.238	0.0026			
SD :	0.0070	0.0070	0.0001			
%RSD:	2.9	2.9	2.9532			

=====
 Element: Hg Seq. No.: 22 AS Loc.: 7 Date: 03/10/2010
 Sample ID: CCV

Repl #	SampleConc µg/L	StdndConc µg/L	BlncCorr Signal	Peak Height	Time	Peak Stored
1	5.122	5.122	0.0557	0.0591	12:06:22	No
2	5.174	5.174	0.0563	0.0597	12:06:57	No
Mean:	5.148	5.148	0.0560			
SD :	0.0365	0.0365	0.0004			
%RSD:	0.7	0.7	0.7088			

QC value within specified limits.

=====
 Element: Hg Seq. No.: 23 AS Loc.: 8 Date: 03/10/2010
 Sample ID: CCB

Repl #	SampleConc µg/L	StdndConc µg/L	BlncCorr Signal	Peak Height	Time	Peak Stored
1	-0.038	-0.038	-0.0004	0.0030	12:08:25	No
2	-0.032	-0.032	-0.0004	0.0030	12:09:00	No
Mean:	-0.035	-0.035	-0.0004			
SD :	0.0042	0.0042	0.0000			
%RSD:	11.9	11.9	11.5118			

QC value within specified limits.

=====
 Element: Hg Seq. No.: 24 AS Loc.: 22 Date: 03/10/2010
 Sample ID: 248110003|i|||

Repl #	SampleConc µg/L	StdndConc µg/L	BlncCorr Signal	Peak Height	Time	Peak Stored
1	0.259	0.259	0.0028	0.0062	12:10:25	No
2	0.268	0.268	0.0029	0.0063	12:11:00	No
Mean:	0.264	0.264	0.0029			
SD :	0.0065	0.0065	0.0001			
%RSD:	2.5	2.5	2.4719			

=====
 Element: Hg Seq. No.: 25 AS Loc.: 23 Date: 03/10/2010
 Sample ID: 248110004|i|||

Repl #	SampleConc µg/L	StdndConc µg/L	BlncCorr Signal	Peak Height	Time	Peak Stored
1	0.060	0.060	0.0006	0.0041	12:12:24	No
2	0.079	0.079	0.0008	0.0043	12:12:59	No
Mean:	0.069	0.069	0.0007			
SD :	0.0130	0.0130	0.0001			
%RSD:	18.7	18.7	18.9955			

=====
 Element: Hg Seq. No.: 26 AS Loc.: 24 Date: 03/10/2010
 Sample ID: 248110005|i|||

%RSD: 60.8 60.8 59.9339

=====
 Element: Hg Seq. No.: 32 AS Loc.: 30 Date: 03/10/2010
 Sample ID: 248118003|i|||

Repl #	SampleConc µg/L	StdConc µg/L	BlncCorr Signal	Peak Height	Time	Peak Stored
1	0.010	0.010	0.0001	0.0035	12:26:22	No
2	-0.047	-0.047	-0.0005	0.0029	12:26:57	No
Mean:	-0.018	-0.018	-0.0002			
SD :	0.0401	0.0401	0.0004			
%RSD:	218.6	218.6	204.8136			

=====
 Element: Hg Seq. No.: 33 AS Loc.: 31 Date: 03/10/2010
 Sample ID: 248118004|i|||

Repl #	SampleConc µg/L	StdConc µg/L	BlncCorr Signal	Peak Height	Time	Peak Stored
1	0.477	0.477	0.0052	0.0086	12:28:24	No
2	0.695	0.695	0.0075	0.0110	12:28:59	No
Mean:	0.586	0.586	0.0064			
SD :	0.1541	0.1541	0.0017			
%RSD:	26.3	26.3	26.3746			

=====
 Element: Hg Seq. No.: 34 AS Loc.: 7 Date: 03/10/2010
 Sample ID: CCV

Repl #	SampleConc µg/L	StdConc µg/L	BlncCorr Signal	Peak Height	Time	Peak Stored
1	3.238	3.238	0.0352	0.0386	12:30:26	No
2	3.176	3.176	0.0345	0.0379	12:31:01	No
Mean:	3.207	3.207	0.0349			
SD :	0.0433	0.0433	0.0005			
%RSD:	1.3	1.3	1.3501			

QC failed, value less than lower limit for Hg.
 Current analysis method being continued.

=====
 Element: Hg Seq. No.: 35 AS Loc.: 8 Date: 03/10/2010
 Sample ID: CCB

Repl #	SampleConc µg/L	StdConc µg/L	BlncCorr Signal	Peak Height	Time	Peak Stored
1	-0.170	-0.170	-0.0019	0.0016	12:32:29	No
2	-0.111	-0.111	-0.0012	0.0022	12:33:03	No
Mean:	-0.140	-0.140	-0.0015			
SD :	0.0412	0.0412	0.0004			
%RSD:	29.4	29.4	29.1117			

QC value within specified limits.

=====
 Element: Hg Seq. No.: 36 AS Loc.: 32 Date: 03/10/2010
 Sample ID: 248118005|i|||

Repl #	SampleConc µg/L	StdConc µg/L	BlncCorr Signal	Peak Height	Time	Peak Stored
1	-0.170	-0.170	-0.0019	0.0016	12:34:27	No
2	-0.075	-0.075	-0.0008	0.0026	12:35:03	No
Mean:	-0.123	-0.123	-0.0013			
SD :	0.0669	0.0669	0.0007			
%RSD:	54.6	54.6	54.0576			

=====
 Element: Hg Seq. No.: 37 AS Loc.: 33 Date: 03/10/2010

SD : 0.8334 0.8334 0.0091
 %RSD: 111.7 111.7 111.8433

=====
 Element: Hg Seq. No.: 43 AS Loc.: 39 Date: 03/10/2010
 Sample ID: 1202056102|i||MS

Repl #	SampleConc µg/L	StdndConc µg/L	BlndCorr Signal	Peak Height	Time	Peak Stored
1	2.719	2.719	0.0296	0.0330	12:48:03	No
2	2.588	2.588	0.0281	0.0315	12:48:38	No
Mean:	2.653	2.653	0.0288			
SD :	0.0924	0.0924	0.0010			
%RSD:	3.5	3.5	3.4851			

=====
 Element: Hg Seq. No.: 44 AS Loc.: 40 Date: 03/10/2010
 Sample ID: 1202056104|i||MSD

Repl #	SampleConc µg/L	StdndConc µg/L	BlndCorr Signal	Peak Height	Time	Peak Stored
1	2.725	2.725	0.0296	0.0330	12:50:02	No
2	2.603	2.603	0.0283	0.0317	12:50:37	No
Mean:	2.664	2.664	0.0290			
SD :	0.0861	0.0861	0.0009			
%RSD:	3.2	3.2	3.2322			

=====
 Element: Hg Seq. No.: 45 AS Loc.: 41 Date: 03/10/2010
 Sample ID: 1202056103|i|5||SDILT

Repl #	SampleConc µg/L	StdndConc µg/L	BlndCorr Signal	Peak Height	Time	Peak Stored
1	0.023	0.023	0.0002	0.0036	12:52:01	No
2	-0.006	-0.006	-0.0001	0.0033	12:52:36	No
Mean:	0.009	0.009	0.0001			
SD :	0.0199	0.0199	0.0002			
%RSD:	233.2	233.2	272.7061			

=====
 Element: Hg Seq. No.: 46 AS Loc.: 7 Date: 03/10/2010
 Sample ID: CCV

Repl #	SampleConc µg/L	StdndConc µg/L	BlndCorr Signal	Peak Height	Time	Peak Stored
1	3.971	3.971	0.0432	0.0466	12:54:02	No
2	3.875	3.875	0.0421	0.0456	12:54:37	No
Mean:	3.923	3.923	0.0427			
SD :	0.0678	0.0678	0.0007			
%RSD:	1.7	1.7	1.7290			

QC failed, value less than lower limit for Hg.
 Current analysis method being continued.

=====
 Element: Hg Seq. No.: 47 AS Loc.: 8 Date: 03/10/2010
 Sample ID: CCB

Repl #	SampleConc µg/L	StdndConc µg/L	BlndCorr Signal	Peak Height	Time	Peak Stored
1	-0.107	-0.107	-0.0012	0.0022	12:56:06	No
2	-0.111	-0.111	-0.0012	0.0022	12:56:41	No
Mean:	-0.109	-0.109	-0.0012			
SD :	0.0031	0.0031	0.0000			
%RSD:	2.8	2.8	2.8075			

QC value within specified limits.

Element: Hg Seq. No.: 48 AS Loc.: 42 Date: 03/10/2010
 Sample ID: 247806002|i|||

Repl #	SampleConc µg/L	StdndConc µg/L	BlkCorr Signal	Peak Height	Time	Peak Stored
1	-0.020	-0.020	-0.0002	0.0032	12:58:06	No
2	-0.033	-0.033	-0.0004	0.0030	12:58:42	No
Mean:	-0.027	-0.027	-0.0003			
SD :	0.0090	0.0090	0.0001			
%RSD:	33.7	33.7	32.2087			

Element: Hg Seq. No.: 49 AS Loc.: 43 Date: 03/10/2010
 Sample ID: 247806003|i|||

Repl #	SampleConc µg/L	StdndConc µg/L	BlkCorr Signal	Peak Height	Time	Peak Stored
1	0.181	0.181	0.0020	0.0054	13:00:06	No
2	0.151	0.151	0.0016	0.0050	13:00:41	No
Mean:	0.166	0.166	0.0018			
SD :	0.0214	0.0214	0.0002			
%RSD:	12.9	12.9	12.9601			

Element: Hg Seq. No.: 50 AS Loc.: 44 Date: 03/10/2010
 Sample ID: 247806004|i|||

Repl #	SampleConc µg/L	StdndConc µg/L	BlkCorr Signal	Peak Height	Time	Peak Stored
--------	--------------------	-------------------	-------------------	----------------	------	----------------

Element: Hg Seq. No.: 50 AS Loc.: 7 Date: 03/10/2010
 Sample ID: CCV

Repl #	SampleConc µg/L	StdndConc µg/L	BlkCorr Signal	Peak Height	Time	Peak Stored
1	5.005	5.005	0.0544	0.0578	13:05:31	No
2	4.892	4.892	0.0532	0.0566	13:06:06	No
Mean:	4.949	4.949	0.0538			
SD :	0.0796	0.0796	0.0009			
%RSD:	1.6	1.6	1.6094			

QC value within specified limits.

Element: Hg Seq. No.: 51 AS Loc.: 8 Date: 03/10/2010
 Sample ID: CCB

Repl #	SampleConc µg/L	StdndConc µg/L	BlkCorr Signal	Peak Height	Time	Peak Stored
1	-0.089	-0.089	-0.0010	0.0024	13:07:34	No
2	-0.083	-0.083	-0.0009	0.0025	13:08:08	No
Mean:	-0.086	-0.086	-0.0010			
SD :	0.0043	0.0043	0.0000			
%RSD:	5.0	5.0	4.9353			

QC value within specified limits.

Element: Hg Seq. No.: 52 AS Loc.: 22 Date: 03/10/2010
 Sample ID: 248110003|i||958757|

Repl #	SampleConc µg/L	StdndConc µg/L	BlkCorr Signal	Peak Height	Time	Peak Stored
1	0.205	0.205	0.0022	0.0056	13:09:34	No
2	0.196	0.196	0.0021	0.0055	13:10:09	No
Mean:	0.201	0.201	0.0022			
SD :	0.0063	0.0063	0.0001			
%RSD:	3.1	3.1	3.1572			

=====

Element: Hg Seq. No.: 53 AS Loc.: 23 Date: 03/10/2010
 Sample ID: 248110004|i|||

Repl #	SampleConc µg/L	StdndConc µg/L	BlnkCorr Signal	Peak Height	Time	Peak Stored
1	0.016	0.016	0.0002	0.0036	13:11:33	No
2	0.024	0.024	0.0002	0.0037	13:12:08	No
Mean:	0.020	0.020	0.0002			
SD :	0.0058	0.0058	0.0001			
%RSD:	29.2	29.2	31.1504			

=====

Element: Hg Seq. No.: 54 AS Loc.: 24 Date: 03/10/2010
 Sample ID: 248110005|i|||

Repl #	SampleConc µg/L	StdndConc µg/L	BlnkCorr Signal	Peak Height	Time	Peak Stored
1	0.134	0.134	0.0014	0.0049	13:13:32	No
2	0.131	0.131	0.0014	0.0048	13:14:07	No
Mean:	0.133	0.133	0.0014			
SD :	0.0017	0.0017	0.0000			
%RSD:	1.3	1.3	1.2712			

=====

Element: Hg Seq. No.: 55 AS Loc.: 25 Date: 03/10/2010
 Sample ID: 248110006|i|||

Repl #	SampleConc µg/L	StdndConc µg/L	BlnkCorr Signal	Peak Height	Time	Peak Stored
1	0.220	0.220	0.0024	0.0058	13:15:31	No
2	0.228	0.228	0.0025	0.0059	13:16:06	No
Mean:	0.224	0.224	0.0024			
SD :	0.0056	0.0056	0.0001			
%RSD:	2.5	2.5	2.5247			

=====

Element: Hg Seq. No.: 56 AS Loc.: 26 Date: 03/10/2010
 Sample ID: 248110007|i|||

Repl #	SampleConc µg/L	StdndConc µg/L	BlnkCorr Signal	Peak Height	Time	Peak Stored
1	0.205	0.205	0.0022	0.0056	13:17:31	No
2	0.212	0.212	0.0023	0.0057	13:18:06	No
Mean:	0.209	0.209	0.0023			
SD :	0.0050	0.0050	0.0001			
%RSD:	2.4	2.4	2.4058			

=====

Element: Hg Seq. No.: 57 AS Loc.: 27 Date: 03/10/2010
 Sample ID: 248110008|i|||

Repl #	SampleConc µg/L	StdndConc µg/L	BlnkCorr Signal	Peak Height	Time	Peak Stored
1	0.231	0.231	0.0025	0.0059	13:19:32	No
2	0.226	0.226	0.0024	0.0059	13:20:06	No
Mean:	0.229	0.229	0.0025			
SD :	0.0037	0.0037	0.0000			
%RSD:	1.6	1.6	1.6134			

=====

Element: Hg Seq. No.: 58 AS Loc.: 28 Date: 03/10/2010
 Sample ID: 248118001|i|||

Repl #	SampleConc µg/L	StdndConc µg/L	BlnkCorr Signal	Peak Height	Time	Peak Stored
1	-0.019	-0.019	-0.0002	0.0032	13:21:32	No
2	-0.023	-0.023	-0.0003	0.0032	13:22:07	No
Mean:	-0.021	-0.021	-0.0002			

SD : 0.0025 0.0025 0.0000
 %RSD: 12.0 12.0 11.2962

=====
 Element: Hg Seq. No.: 59 AS Loc.: 29 Date: 03/10/2010
 Sample ID: 248118002|i|||

Repl #	SampleConc µg/L	StdConc µg/L	Blncorr Signal	Peak Height	Time	Peak Stored
1	-0.028	-0.028	-0.0003	0.0031	13:23:33	No
2	-0.033	-0.033	-0.0004	0.0030	13:24:08	No
Mean:	-0.030	-0.030	-0.0003			
SD :	0.0033	0.0033	0.0000			
%RSD:	10.7	10.7	10.2525			

=====
 Element: Hg Seq. No.: 60 AS Loc.: 30 Date: 03/10/2010
 Sample ID: 248118003|i|||

Repl #	SampleConc µg/L	StdConc µg/L	Blncorr Signal	Peak Height	Time	Peak Stored
1	0.052	0.052	0.0006	0.0040	13:25:35	No
2	0.035	0.035	0.0004	0.0038	13:26:10	No
Mean:	0.044	0.044	0.0005			
SD :	0.0119	0.0119	0.0001			
%RSD:	27.2	27.2	27.9535			

=====
 Element: Hg Seq. No.: 61 AS Loc.: 31 Date: 03/10/2010
 Sample ID: 248118004|i|||

Repl #	SampleConc µg/L	StdConc µg/L	Blncorr Signal	Peak Height	Time	Peak Stored
1	0.965	0.965	0.0105	0.0139	13:27:37	No
2	0.942	0.942	0.0102	0.0136	13:28:11	No
Mean:	0.953	0.953	0.0104			
SD :	0.0162	0.0162	0.0002			
%RSD:	1.7	1.7	1.6982			

=====
 Element: Hg Seq. No.: 62 AS Loc.: 7 Date: 03/10/2010
 Sample ID: CCV

Repl #	SampleConc µg/L	StdConc µg/L	Blncorr Signal	Peak Height	Time	Peak Stored
1	4.923	4.923	0.0535	0.0569	13:29:38	No
2	4.958	4.958	0.0539	0.0573	13:30:13	No
Mean:	4.940	4.940	0.0537			
SD :	0.0249	0.0249	0.0003			
%RSD:	0.5	0.5	0.5048			

QC value within specified limits.

=====
 Element: Hg Seq. No.: 63 AS Loc.: 8 Date: 03/10/2010
 Sample ID: CCB

Repl #	SampleConc µg/L	StdConc µg/L	Blncorr Signal	Peak Height	Time	Peak Stored
1	-0.061	-0.061	-0.0007	0.0027	13:31:41	No
2	-0.068	-0.068	-0.0008	0.0027	13:32:17	No
Mean:	-0.065	-0.065	-0.0007			
SD :	0.0052	0.0052	0.0001			
%RSD:	8.0	8.0	7.8955			

QC value within specified limits.

=====
 Element: Hg Seq. No.: 64 AS Loc.: 32 Date: 03/10/2010

Sample ID: 248118005|i|||

Repl #	SampleConc µg/L	StdndConc µg/L	BlndCorr Signal	Peak Height	Time	Peak Stored
1	-0.037	-0.037	-0.0004	0.0030	13:33:41	No
2	-0.056	-0.056	-0.0006	0.0028	13:34:16	No
Mean:	-0.046	-0.046	-0.0005			
SD :	0.0133	0.0133	0.0001			
%RSD:	28.7	28.7	27.9598			

=====

Element: Hg Seq. No.: 65 AS Loc.: 33 Date: 03/10/2010

Sample ID: 248118006|i|||

Repl #	SampleConc µg/L	StdndConc µg/L	BlndCorr Signal	Peak Height	Time	Peak Stored
1	-0.013	-0.013	-0.0002	0.0033	13:35:36	No
2	-0.008	-0.008	-0.0001	0.0033	13:36:11	No
Mean:	-0.010	-0.010	-0.0001			
SD :	0.0035	0.0035	0.0000			
%RSD:	33.8	33.8	30.1963			

=====

Element: Hg Seq. No.: 66 AS Loc.: 34 Date: 03/10/2010

Sample ID: 248118007|i|||

Repl #	SampleConc µg/L	StdndConc µg/L	BlndCorr Signal	Peak Height	Time	Peak Stored
1	-0.017	-0.017	-0.0002	0.0032	13:37:31	No
2	0.001	0.001	0.0000	0.0034	13:38:06	No
Mean:	-0.008	-0.008	-0.0001			
SD :	0.0127	0.0127	0.0001			
%RSD:	151.7	151.7	132.2214			

=====

Element: Hg Seq. No.: 67 AS Loc.: 35 Date: 03/10/2010

Sample ID: 1202056099|i||958718|MB

Repl #	SampleConc µg/L	StdndConc µg/L	BlndCorr Signal	Peak Height	Time	Peak Stored
1	-0.138	-0.138	-0.0015	0.0019	13:39:27	No
2	-0.143	-0.143	-0.0016	0.0018	13:40:01	No
Mean:	-0.141	-0.141	-0.0015			
SD :	0.0039	0.0039	0.0000			
%RSD:	2.8	2.8	2.7559			

=====

Element: Hg Seq. No.: 68 AS Loc.: 36 Date: 03/10/2010

Sample ID: 1202056100|i|10||LCS

Repl #	SampleConc µg/L	StdndConc µg/L	BlndCorr Signal	Peak Height	Time	Peak Stored
1	3.416	3.416	0.0371	0.0406	13:41:23	No
2	3.310	3.310	0.0360	0.0394	13:41:58	No
Mean:	3.363	3.363	0.0366			
SD :	0.0754	0.0754	0.0008			
%RSD:	2.2	2.2	2.2423			

=====

Element: Hg Seq. No.: 69 AS Loc.: 37 Date: 03/10/2010

Sample ID: 247806001|i|||

Repl #	SampleConc µg/L	StdndConc µg/L	BlndCorr Signal	Peak Height	Time	Peak Stored
1	1.286	1.286	0.0140	0.0174	13:43:20	No
2	1.257	1.257	0.0137	0.0171	13:43:55	No
Mean:	1.271	1.271	0.0138			

SD : 0.0204 0.0204 0.0002
 %RSD: 1.6 1.6 1.6054

=====
 Element: Hg Seq. No.: 70 AS Loc.: 38 Date: 03/10/2010
 Sample ID: 1202056101|i|||DUP
 =====

Repl #	SampleConc µg/L	StdConc µg/L	BlkCorr Signal	Peak Height	Time	Peak Stored
1	1.651	1.651	0.0179	0.0214	13:45:17	No
2	1.662	1.662	0.0181	0.0215	13:45:52	No
Mean:	1.657	1.657	0.0180			
SD :	0.0076	0.0076	0.0001			
%RSD:	0.5	0.5	0.4599			

=====
 Element: Hg Seq. No.: 71 AS Loc.: 39 Date: 03/10/2010
 Sample ID: 1202056102|i|||MS
 =====

Repl #	SampleConc µg/L	StdConc µg/L	BlkCorr Signal	Peak Height	Time	Peak Stored
1	3.547	3.547	0.0386	0.0420	13:47:15	No
2	3.540	3.540	0.0385	0.0419	13:47:50	No
Mean:	3.544	3.544	0.0385			
SD :	0.0055	0.0055	0.0001			
%RSD:	0.2	0.2	0.1560			

=====
 Element: Hg Seq. No.: 72 AS Loc.: 40 Date: 03/10/2010
 Sample ID: 1202056104|i|||MSD
 =====

Repl #	SampleConc µg/L	StdConc µg/L	BlkCorr Signal	Peak Height	Time	Peak Stored
1	3.568	3.568	0.0388	0.0422	13:49:14	No
2	3.559	3.559	0.0387	0.0421	13:49:49	No
Mean:	3.563	3.563	0.0387			
SD :	0.0069	0.0069	0.0001			
%RSD:	0.2	0.2	0.1941			

=====
 Element: Hg Seq. No.: 73 AS Loc.: 41 Date: 03/10/2010
 Sample ID: 1202056103|i|5||SDILT
 =====

Repl #	SampleConc µg/L	StdConc µg/L	BlkCorr Signal	Peak Height	Time	Peak Stored
1	-0.073	-0.073	-0.0008	0.0026	13:51:13	No
2	-0.085	-0.085	-0.0009	0.0025	13:51:48	No
Mean:	-0.079	-0.079	-0.0009			
SD :	0.0090	0.0090	0.0001			
%RSD:	11.4	11.4	11.2520			

=====
 Element: Hg Seq. No.: 74 AS Loc.: 7 Date: 03/10/2010
 Sample ID: CCV
 =====

Repl #	SampleConc µg/L	StdConc µg/L	BlkCorr Signal	Peak Height	Time	Peak Stored
1	5.012	5.012	0.0545	0.0579	13:53:14	No
2	4.896	4.896	0.0532	0.0566	13:53:50	No
Mean:	4.954	4.954	0.0539			
SD :	0.0823	0.0823	0.0009			
%RSD:	1.7	1.7	1.6623			

QC value within specified limits.

=====
 Element: Hg Seq. No.: 75 AS Loc.: 8 Date: 03/10/2010
 Sample ID: CCB
 =====

```

-----
Repl  SampleConc  StndConc  BlnkCorr  Peak      Time      Peak
#      µg/L      µg/L      Signal    Height    Stored
1      -0.080    -0.080    -0.0009   0.0025    13:55:18  No
2      -0.085    -0.085    -0.0009   0.0025    13:55:53  No
Mean:   -0.082    -0.082    -0.0009
SD :    0.0034    0.0034    0.0000
%RSD:    4.1      4.1      4.0323
QC value within specified limits.

```

```

=====
Element: Hg      Seq. No.: 76      AS Loc.: 42      Date: 03/10/2010
Sample ID: 247806002|i|||

```

```

-----
Repl  SampleConc  StndConc  BlnkCorr  Peak      Time      Peak
#      µg/L      µg/L      Signal    Height    Stored
1      -0.008    -0.008    -0.0001   0.0033    13:57:19  No
2      -0.008    -0.008    -0.0001   0.0033    13:57:54  No
Mean:   -0.008    -0.008    -0.0001
SD :    0.0000    0.0000    0.0000
%RSD:    0.4      0.4      0.3271

```

```

=====
Element: Hg      Seq. No.: 77      AS Loc.: 43      Date: 03/10/2010
Sample ID: 247806003|i|||

```

```

-----
Repl  SampleConc  StndConc  BlnkCorr  Peak      Time      Peak
#      µg/L      µg/L      Signal    Height    Stored
1      0.273     0.273     0.0030    0.0064    13:59:19  No
2      0.256     0.256     0.0028    0.0062    13:59:53  No
Mean:   0.265     0.265     0.0029
SD :    0.0120    0.0120    0.0001
%RSD:    4.5      4.5      4.5599

```

```

=====
Element: Hg      Seq. No.: 78      AS Loc.: 44      Date: 03/10/2010
Sample ID: 247806004|i|||

```

```

-----
Repl  SampleConc  StndConc  BlnkCorr  Peak      Time      Peak
#      µg/L      µg/L      Signal    Height    Stored
1      17.96     17.96     0.1953    0.1987    14:01:19  No
Sample absorbance is greater than that of the highest standard.
2      17.70     17.70     0.1924    0.1959    14:01:54  No
Sample absorbance is greater than that of the highest standard.
Mean:   17.83     17.83     0.1939
SD :    0.1847    0.1847    0.0020
%RSD:    1.0      1.0      1.0364
Sample absorbance is greater than that of the highest standard.

```

```

=====
Element: Hg      Seq. No.: 79      AS Loc.: 45      Date: 03/10/2010
Sample ID: 247806005|i|||

```

```

-----
Repl  SampleConc  StndConc  BlnkCorr  Peak      Time      Peak
#      µg/L      µg/L      Signal    Height    Stored
1      0.705     0.705     0.0077    0.0111    14:03:20  No
2      0.676     0.676     0.0073    0.0108    14:03:55  No
Mean:   0.691     0.691     0.0075
SD :    0.0203    0.0203    0.0002
%RSD:    2.9      2.9      2.9494

```

```

=====
Element: Hg      Seq. No.: 80      AS Loc.: 46      Date: 03/10/2010
Sample ID: 247806006|i|||

```

```

-----
Repl  SampleConc  StndConc  BlnkCorr  Peak      Time      Peak
#      µg/L      µg/L      Signal    Height    Stored

```

Miscellaneous

Prep Logbook

Acid Digestion of Sediments, Sludges, and Soils

Batch ID: 959115.0 Verified by: Lab SOP: GL-MA-E-009 REV# 19
Analyst: Barry Audain Instrument: Sartorius Balance B-001
Method: SW846 3050B

Sample ID	Run Date	Initial Weight (g)	Final Volume (mL)	Prep Factor (mL/g)	pH Check
1202056883 MB	03-MAR-2010 18:14:00	0.521	50	95.96929	1
1202056888 LCS	03-MAR-2010 18:14:00	0.578	50	86.50519	
248110001	03-MAR-2010 18:14:00	0.534	50	93.63296	
1202056884 DUP (248110001)	03-MAR-2010 18:14:00	0.556	50	89.92806	
1202056885 SDILT (248110001)	03-MAR-2010 18:14:00	0.534	50	93.63296	
1202056886 MS (248110001)	03-MAR-2010 18:14:00	0.526	50	95.05703	
1202056887 MSD (248110001)	03-MAR-2010 18:14:00	0.502	50	99.60159	
248110002	03-MAR-2010 18:14:00	0.503	50	99.40358	
248110003	03-MAR-2010 18:14:00	0.511	50	97.84736	
248110004	03-MAR-2010 18:14:00	0.569	50	87.87346	
248110005	03-MAR-2010 18:14:00	0.519	50	96.33911	
248110006	03-MAR-2010 18:14:00	0.518	50	96.5251	
248110007	03-MAR-2010 18:14:00	0.505	50	99.0099	
248110008	03-MAR-2010 18:14:00	0.527	50	94.87666	
248118001	03-MAR-2010 18:14:00	0.53	50	94.33962	
248118002	03-MAR-2010 18:14:00	0.585	50	85.47009	
248118003	03-MAR-2010 18:14:00	0.516	50	96.89922	
248118004	03-MAR-2010 18:14:00	0.574	50	87.10801	
248118005	03-MAR-2010 18:14:00	0.576	50	86.80556	
248118006	03-MAR-2010 18:14:00	0.512	50	97.65625	
248118007	03-MAR-2010 18:14:00	0.584	50	85.61644	

Type	Sample Id	Description	Serial Number	Spike Amt	Units	Comments:
LCS	1202056888	Metals Soil LCS SRM ICPMS	U1062540-MS	.578	g	
MS	1202056886	ICP-MS Spike for soil products.	U1090827-A	.5	mL	sample#248110001 is a brown rocky soil.
MS	1202056886	ICP-MS Spike for Soil Products	U1090827-B	.5	mL	
MSD	1202056887	ICP-MS Spike for soil products.	U1090827-A	.5	mL	
MSD	1202056887	ICP-MS Spike for Soil Products	U1090827-B	.5	mL	
REGNT All		Hydrogen Peroxide 30%	1250038-02	1.5	mL	
REGNT All		Nitric Acid CONC.	1277919	.5	mL	

Prep Logbook

Mercury Analysis Using the Perkin Elmer Automated Mercury Analyzer

Batch ID: 958755.0 Verified by: _____
Analyst: Lamanuel Hightower
Method: SW846 7471A Prep
Lab SOP: GL-MA-E-010 REV# 23
Instrument: Sartorius Balance B-001

Sample ID	Run Date	Matrix	Initial Weight (g)	Final Volume (mL)	Prep Factor (mL/g)	pH Check 1	Type	Sample Id	Description	Serial Number	Spike Amount	Spike Units
1202056179 MB	10-MAR-2010 09:00:00	Soil	0.547	30	54.84461		LCS	1202056180	Metals LCS Soil SRM	U1031809A	.209	g
1202056180 LCS	10-MAR-2010 09:00:00	Soil	0.209	30	143.54067		MS	1202056182	Mercury soil working intermediate standard for MS	WHG100310-14	.3	mL
248068001	10-MAR-2010 09:00:00	Soil	0.552	30	54.34783		MSD	1202056184	Mercury soil working intermediate standard for MS	WHG100310-14	.3	mL
1202056181 DUP (248068001)	10-MAR-2010 09:00:00	Soil	0.585	30	51.28205							
1202056182 MS (248068001)	10-MAR-2010 09:00:00	Soil	0.505	30	59.40594							
1202056184 MSD (248068001)	10-MAR-2010 09:00:00	Soil	0.528	30	56.81818							
1202056183 SDILT (248068001)	10-MAR-2010 09:00:00	Soil	0.552	30	54.34783							
248068002	10-MAR-2010 09:00:00	Soil	0.525	30	57.14286							
248110001	10-MAR-2010 09:00:00	Soil	0.512	30	58.59375							
248110002	10-MAR-2010 09:00:00	Soil	0.593	30	50.59022							
248110003	10-MAR-2010 09:00:00	Soil	0.521	30	57.58157							
248110004	10-MAR-2010 09:00:00	Soil	0.527	30	56.926							
248110005	10-MAR-2010 09:00:00	Soil	0.557	30	53.85996							
248110006	10-MAR-2010 09:00:00	Soil	0.509	30	58.9391							
248110007	10-MAR-2010 09:00:00	Soil	0.558	30	53.76344							
248110008	10-MAR-2010 09:00:00	Soil	0.517	30	58.02708							
248118001	10-MAR-2010 09:00:00	Soil	0.558	30	53.76344							
248118002	10-MAR-2010 09:00:00	Soil	0.545	30	55.04587							
248118003	10-MAR-2010 09:00:00	Soil	0.588	30	51.02041							
248118004	10-MAR-2010 09:00:00	Soil	0.599	30	50.08347							
248118005	10-MAR-2010 09:00:00	Soil	0.535	30	56.07477							
248118006	10-MAR-2010 09:00:00	Soil	0.563	30	53.28597							
248118007	10-MAR-2010 09:00:00	Soil	0.554	30	54.15162							

Reagent/Solvent Lot ID **Description** **Amount** **Comments:**
 1255532-C Hg reducing agent 2 mL Sample 248068001 is a powder like brown soil.

Analytical Logbook version 1 11-04-2002

GEL Laboratories LLC

Prep Logbook

Batch ID: 958755.0
Analyst: Lamanuel Hightower
Method: SW846 7471A Prep
Lab SOP: GL-MA-E-010 REV# 23
Instrument: Sartorius Balance B-001

Verified by:
Type **Sample Id** **Description** **Serial Number** **Spike Amount** **Spike Units**
 LCS 1202056180 Metals LCS Soil SRM UF031809A .209 g
 MS 1202056182 Mercury soil working intermediate WHG100310-14 .3 mL
 MSD 1202056184 Mercury soil working intermediate WHG100310-14 .3 mL
 standard for MS
 standard for MS

pH Check 1

Sample ID	Run Date	Matrix	Initial Weight (g)	Final Volume (mL)	Prep Factor (mL/g)
-----------	----------	--------	--------------------	-------------------	--------------------

1255532-C	Hg reducing agent	2 mL			
1274391-1	NITRIC ACID	.375 mL			
1277235-A	Hydrochloric Acid Conc.	1.125 mL			
1277238-C	5% KMnO4 solution	7.5 mL			
WHG100310-07	Mercury Working Standard 1st Source CAL S 0.2/CRA	30 uL			
WHG100310-08	Mercury Working Standard 1st Source CAL S 0.5	75 uL			
WHG100310-09	Mercury Working 1st Source CAL S 2.0	300 uL			
WHG100310-10	Mercury Working 1st Source CAL S 5.0/CCV	750 uL			
WHG100310-11	Mercury Working 1st Source CAL S 10.0	1.5 mL			
WHG100310-12	Mercury Working 2nd Source S 5.0/ICV	750 uL			

Digestion Start Date: 10-MAR-10 09:00:00
 Digestion End Date: 10-MAR-10 09:30:00

Prep Logbook

Acid Digestion of Sediments, Sludges, and Soils

Batch ID: 959113.0
Analyst: Anthony Green
Method: SW846 3050B
Lab SOP: GL-MA-E-009 REV# 19
Instrument: BAL-001

Verified by:

Type	Sample Id	Description	Serial Number	Spike Amount	Spike Units
LCS	1202056882	Metals Soil LCS SRM ICP/Hg	U1062540-1	.548	g
MS	1202056880	Metals Spike Mix I	U11268741-01	.25	mL
MS	1202056880	Metals Spike Mix II	U11268744-06	.25	mL
MSD	1202056881	Metals Spike Mix I	U11268741-01	.25	mL
MSD	1202056881	Metals Spike Mix II	U11268744-06	.25	mL

Sample ID	Run Date	Matrix	Initial Weight (g)	Final Volume (mL)	Prep Factor (mL/g)	pH Check I
1202056877 MB	09-MAR-2010 10:00:00	Soil	0.549	50	91.07468	
1202056882 LCS	09-MAR-2010 10:00:00	Soil	0.548	50	91.24088	
248110001	09-MAR-2010 10:00:00	Soil	0.533	50	93.80863	
1202056878 DUP (248110001)	09-MAR-2010 10:00:00	Soil	0.527	50	94.87666	
1202056879 SDILT (248110001)	09-MAR-2010 10:00:00	Soil	0.533	50	93.80863	
1202056880 MS (248110001)	09-MAR-2010 10:00:00	Soil	0.513	50	97.46589	
1202056881 MSD (248110001)	09-MAR-2010 10:00:00	Soil	0.52	50	96.15385	
248110002	09-MAR-2010 10:00:00	Soil	0.533	50	93.80863	
248110003	09-MAR-2010 10:00:00	Soil	0.566	50	88.33922	
248110004	09-MAR-2010 10:00:00	Soil	0.527	50	94.87666	
248110005	09-MAR-2010 10:00:00	Soil	0.533	50	93.80863	
248110006	09-MAR-2010 10:00:00	Soil	0.511	50	97.84736	
248110007	09-MAR-2010 10:00:00	Soil	0.515	50	97.08738	
248110008	09-MAR-2010 10:00:00	Soil	0.536	50	93.28358	
248118001	09-MAR-2010 10:00:00	Soil	0.506	50	98.81423	
248118002	09-MAR-2010 10:00:00	Soil	0.521	50	95.96929	
248118003	09-MAR-2010 10:00:00	Soil	0.51	50	98.03922	
248118004	09-MAR-2010 10:00:00	Soil	0.551	50	90.7441	
248118005	09-MAR-2010 10:00:00	Soil	0.594	50	84.17508	
248118006	09-MAR-2010 10:00:00	Soil	0.524	50	95.41985	
248118007	09-MAR-2010 10:00:00	Soil	0.59	50	84.74576	

Reagent/Solvent Lot ID **Description** **Amount** **Comments:**

Analytical Logbook version 1 11-04-2002

GEL Laboratories LLC

Prep Logbook

Batch ID: 959113.0
Analyst: Anthony Green
Method: SW846 3050B
Lab SOP: GL-MA-E-009 REV# 19
Instrument: BAL-001

Type	Sample Id	Description	Serial Number	Spike Amount	Spike Units
LCS	1202056882	Metals Soil LCS SRM ICP/Hg	U1062540-1	.548	g
MS	1202056880	Metals Spike Mix I	U11268741-01	.25	mL
MS	1202056880	Metals Spike Mix II	U11268744-06	.25	mL
MSD	1202056881	Metals Spike Mix I	U11268741-01	.25	mL
MSD	1202056881	Metals Spike Mix II	U11268744-06	.25	mL

Sample ID	Run Date	Matrix	Initial Weight (g)	Final Volume (mL)	Prep Factor (mL/g)	pH Check 1
-----------	----------	--------	--------------------	-------------------	--------------------	------------

1277916	HYDROCHLORIC ACID	10 mL				
1277919	Nitric Acid CONC.	1.25 mL				

Sample 248110001 consist of brown, rocky soil.

DATA EXCEPTION REPORT

Mo. Day Yr. 26-MAR-10	Division: Industrial	Quality Criteria: Specifications	Type: Process
Instrument Type: ICP/MS	Test / Method: SW846 3050B/6020	Matrix Type: Solid	Client Code: LANL
Batch ID: 959116	Sample Numbers: See Below		

Potentially affected work order(s)(SDG): 248110(10-2090-1), 248118(10-2093-1)

Application Issues:

Failed Recovery for MS/PS

Failed Recovery for MSD/PSD

Specification and Requirements Exception Description:	DER Disposition:
1. Failed Recovery for MS/PS: QC 1202056886MS	The matrix spike and matrix spike duplicate recovery failed outside of the control limits for Se due to possible matrix interferences and/or sample non-homogeneity. Per GEL's accredited methods and SOPs, a corrective action is not required and the data is qualified and reported.
2. Failed Recovery for MSD/PSD: QC 1202056887MSD	

Originator's Name:

Rose Jenkins 27-MAR-10

Data Validator/Group Leader:

Jamie Johnson 27-MAR-10

DATA EXCEPTION REPORT

Mo. Day Yr. 30-MAR-10	Division: Industrial	Quality Criteria: Specifications	Type: Process
Instrument Type: ICP	Test / Method: SW846 3050B/6010B	Matrix Type: Solid	Client Code: LANL
Batch ID: 959114	Sample Numbers: See Below		

Potentially affected work order(s)(SDG): 248110(10-2090-1),248118(10-2093-1)

Application Issues:

Failed RPD for DUP
Failed Recovery for MSD/PSD
Failed Recovery for LCS/LCSD
Failed Recovery for MS/PS

**Specification and Requirements
Exception Description:**

DER Disposition:

1. Failed Recovery for MS/PS:

QC 1202056880MS

2. Failed RPD for DUP:

QC 1202056878DUP

3. Failed Recovery for LCS/LCSD:

QC 1202056882LCS

4. Failed Recovery for MSD/PSD:

QC 1202056881MSD

1./4. The matrix spike and matrix spike duplicate recovery failed outside of the control limits for antimony and potassium due to possible matrix interferences and/or non-homogeneity. Per GEL's accredited methods and SOPs, a corrective action is not required and the data is qualified and reported.

2. The sample and sample duplicate % RPD failed outside the control limits for manganese due to possible sample non-homogeneity and/or matrix interference. Per GEL's accredited methods and SOPs, a corrective action is not required and the data is qualified and reported.

3. Silver and/or antimony did not meet the recovery acceptance criteria for the LCS. Per the DOE-AL statement of work, page forty, silver and antimony are exempt from the re-digestion requirement for LCS failures.

Originator's Name:

Helen Camello 30-MAR-10

Data Validator/Group Leader:

Kristen Parson 31-MAR-10

Standard Logbook

Serial ID: UHG1167639-01 **Opened:** 13-AUG-09 **Amount :** 125 mL
Name: MHGSTOCK1 **Received:** 13-AUG-09 **Catalog Number :** PLHG4-2Y
Type: Source Material **Expires:** 13-AUG-10 **Lot Number :** 15-37HG
Employee: Bryan Davis **Solvent :** 10% HNO3
Supplier: Spex
Description: Mercury Source Standard #1 1,000 mg/L
Comments: None

Analyte	Concentration	Analyte	Concentration
Mercury	1000 mg/L		

Serial ID: UHG1167641-02 **Opened:** 13-AUG-09 **Amount :** 100 mL
Name: MHGSTOCK2 **Received:** 13-AUG-09 **Catalog Number :** AHG1KN-100
Type: Source Material **Expires:** 13-AUG-10 **Lot Number :** 4905530
Employee: Bryan Davis **Solvent :** 3% HNO3
Supplier: Ricca Chemical Company
Description: Mercury Source Standard #2 1,000 mg/L
Comments: None

Analyte	Concentration	Analyte	Concentration
Mercury	999.7 mg/L		

Serial ID: UI031809A **Opened:** 18-MAR-09 **Catalog Number :** 540
Name: METALSOILSRM **Received:** 18-MAR-09 **Lot Number :** D061-540
Type: Source Material **Expires:** 10-OCT-10
Employee: Jamie Johnson
Supplier: ERA
Description: Metals LCS Soil SRM
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	10600 mg/kg	Antimony	126 mg/kg
Arsenic	225 mg/kg	Barium	565 mg/kg
Beryllium	162 mg/kg	Boron	107 mg/kg
Cadmium	69.1 mg/kg	Calcium	10000 mg/kg
Chromium	124 mg/kg	Cobalt	115 mg/kg
Copper	66.7 mg/kg	Iron	17600 mg/kg
Lead	223 mg/kg	Magnesium	4260 mg/kg
Manganese	368 mg/kg	Mercury	5.15 mg/kg
Molybdenum	107 mg/kg	Nickel	172 mg/kg
Potassium	4090 mg/kg	Selenium	147 mg/kg
Silver	35.2 mg/kg	Sodium	538 mg/kg
Strontium	117 mg/kg	Thallium	173 mg/kg
Tin	164 mg/kg	Titanium	381 mg/kg
Vanadium	93.9 mg/kg	Zinc	349 mg/kg

Standard Logbook

Serial ID: UI062540-I **Opened:** 12-JUN-09 **Amount :** 80 g
Name: ICP SOIL SRM **Received:** 12-JUN-09 **Lot Number :** D062-540
Type: Source Material **Expires:** 31-JAN-12
Employee: Bryan Davis
Supplier: ERA
Description: Metals Soil LCS SRM ICP/Hg
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	10500 mg/kg	Antimony	173 mg/kg
Arsenic	104 mg/kg	Barium	198 mg/kg
Beryllium	77.6 mg/kg	Boron	141 mg/kg
Cadmium	60.7 mg/kg	Calcium	9870 mg/kg
Chromium	236 mg/kg	Cobalt	91.2 mg/kg
Copper	174 mg/kg	Iron	18000 mg/kg
Lead	86 mg/kg	Magnesium	4000 mg/kg
Manganese	558 mg/kg	Mercury	8.46 mg/kg
Molybdenum	48.6 mg/kg	Nickel	134 mg/kg
Phosphorous	736 mg/kg	Potassium	4300 mg/kg
Selenium	286 mg/kg	Silica	2591 mg/kg
Silicon	1211 mg/kg	Silver	30.1 mg/kg
Sodium	1020 mg/kg	Strontium	227 mg/kg
Sulfur	385 mg/kg	Thallium	121 mg/kg
Tin	104 mg/kg	Titanium	462 mg/kg
Vanadium	115 mg/kg	Zinc	594 mg/kg

Serial ID: UI062540-MS **Opened:** 12-JUN-09 **Lot Number :** D062-540
Name: ICPMS SOIL SRM **Received:** 12-JUN-09
Type: Source Material **Expires:** 31-JAN-12
Employee: Bryan Davis
Supplier: ERA
Description: Metals Soil LCS SRM ICPMS
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	10500 mg/kg	Antimony	67.4 mg/kg
Arsenic	104 mg/kg	Barium	198 mg/kg
Beryllium	77.6 mg/kg	Boron	141 mg/kg
Cadmium	60.6 mg/kg	Calcium	9870 mg/kg
Chromium	236 mg/kg	Cobalt	91.2 mg/kg
Copper	174 mg/kg	Iron	18000 mg/kg
Lead	86 mg/kg	Lithium	10.6 mg/kg
Magnesium	4000 mg/kg	Manganese	558 mg/kg
Mercury	8.46 mg/kg	Molybdenum	48.6 mg/kg
Nickel	134 mg/kg	Phosphorous	755 mg/kg
Potassium	4300 mg/kg	Selenium	286 mg/kg
Silver	30.1 mg/kg	Sodium	1020 mg/kg

Standard Logbook

Analyte	Concentration	Analyte	Concentration
Strontium	227 mg/kg	Thallium	121 mg/kg
Thorium	9.84 mg/kg	Tin	104 mg/kg
Titanium	462 mg/kg	Uranium	2.13 mg/kg
Uranium-235	.0153 mg/kg	Uranium-238	2.11 mg/kg
Vanadium	92.4 mg/kg	Zinc	594 mg/kg
Zirconium	10.6 mg/kg		

Serial ID: UI090421-40 **Opened:** 09-OCT-09 **Amount :** 250 mL
Name: TRACE ICP Na-1000SOUR **Received:** 21-APR-09 **Catalog Number :** HP100052-1
Type: Source Material **Expires:** 09-OCT-10 **Lot Number :** 0830227
Employee: Helen Camello **Solvent :** 1%HNO3
Supplier: ENVIRONMENTAL EXPRESS
Description: Sodium 1000 +/- 3 ug/mL in 1% HNO3
Comments: None

Analyte	Concentration	Analyte	Concentration
Sodium	1000 ug/mL		

Serial ID: UI090422-40 **Opened:** 04-MAY-09 **Amount :** 500 mL
Name: TRACE ICP ICSA SOLN A **Received:** 22-APR-09 **Catalog Number :** 160005-01-03
Type: Source Material **Expires:** 04-MAY-10 **Lot Number :** 1013357
Employee: Helen Camello **Solvent :** 5%HNO3
Supplier: o2si
Description: TRACE ICP ICSA SOLN A mg/L +/- 0.5% IN 5% HNO3
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	5000 mg/L	Calcium	5000 mg/L
Iron	2000 mg/L	Magnesium	5000 mg/L

Serial ID: UI090612-02 **Opened:** 12-JUN-09 **Catalog Number :** 060074-06-01
Name: ICPMS Tungsten - 10mg/L **Received:** 12-JUN-09 **Lot Number :** 1016377
Type: Source Material **Expires:** 12-JUN-10 **Solvent :** 2% HNO3
Employee: Paul Boyd
Supplier: O2SI
Description: ICPMS Tungsten standard SPIKE - 10mg/L
Comments: None

Analyte	Concentration	Analyte	Concentration
Tungsten	10 mg/L		

Standard Logbook

Serial ID: UI090701-09 **Opened:** 01-JUL-09 **Amount :** 250 mL
Name: ICP-MS CRDL Master #1 **Received:** 01-JUL-09 **Catalog Number :** 160044-09-02
Type: Source Material **Expires:** 01-JUL-10 **Lot Number :** 1016477
Employee: Paul Boyd **Solvent :** +/- 0.5% IN 2% HNO3
Supplier: 02SI
Description: ICPMS CRDL Master Soln #1
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	15 mg/L	Arsenic	5 mg/L
Barium	2 mg/L	Beryllium	.5 mg/L
Boron	15 mg/L	Cadmium	1 mg/L
Calcium	100 mg/L	Chromium	3 mg/L
Cobalt	1 mg/L	Copper	1 mg/L
Iron	25 mg/L	Lead	2 mg/L
Lithium	10 mg/L	Magnesium	15 mg/L
Manganese	5 mg/L	Nickel	2 mg/L
Phosphorous	50 mg/L	Potassium	300 mg/L
Selenium	5 mg/L	Sodium	250 mg/L
Strontium	10 mg/L	Thallium	1 mg/L
Thorium	1 mg/L	Uranium	.2 mg/L
Vanadium	10 mg/L	Zinc	10 mg/L

Serial ID: UI090701-10 **Opened:** 01-JUL-09 **Amount :** 250 mL
Name: ICP-MS CRDL Master #2 **Received:** 01-JUL-09 **Catalog Number :** 160044-08-02
Type: Source Material **Expires:** 01-JUL-10 **Lot Number :** 1016476
Employee: Paul Boyd **Solvent :** +/- 0.5% IN 2% HNO3
Supplier: 02SI
Description: ICPMS CRDL Soln #2
Comments: None

Analyte	Concentration	Analyte	Concentration
Antimony	2 mg/L	Molybdenum	.5 mg/L
Silver	1 mg/L	Tin	2 mg/L
Titanium	10 mg/L	Tungsten	5 mg/L
Zirconium	2 mg/L		

Serial ID: UI090701-40 **Opened:** 01-JUL-09 **Amount :** 500 mL
Name: TRACE ICP Stock PQL St **Received:** 30-JUN-09 **Catalog Number :** 160543-01-03
Type: Source Material **Expires:** 01-JUL-10 **Lot Number :** 1016475
Employee: Helen Camello **Solvent :** +/-0.5%in2%HNO3+TrHF
Supplier: 02si
Description: TRACE ICP Stock PQL Standard
Comments: None

Analyte	Concentration	Analyte	Concentration
---------	---------------	---------	---------------

Standard Logbook

Analyte	Concentration	Analyte	Concentration
Aluminum	100 mg/L	Antimony	5 mg/L
Arsenic	15 mg/L	Barium	2.5 mg/L
Beryllium	2.5 mg/L	Boron	25 mg/L
Cadmium	2.5 mg/L	Calcium	100 mg/L
Chromium	2.5 mg/L	Cobalt	2.5 mg/L
Copper	5 mg/L	Iron	50 mg/L
Lead	5 mg/L	Magnesium	150 mg/L
Manganese	5 mg/L	Molybdenum	5 mg/L
Nickel	2.5 mg/L	Phosphorous	75 mg/L
Potassium	75 mg/L	Selenium	15 mg/L
Silicon	50 mg/L	Silver	2.5 mg/L
Sodium	150 mg/L	Strontium	2.5 mg/L
Sulfur	50 mg/L	Thallium	10 mg/L
Tin	5 mg/L	Titanium	2.5 mg/L
Uranium	25 mg/L	Vanadium	2.5 mg/L
Zinc	5 mg/L		

Serial ID: UI090827-A **Opened:** 27-AUG-09 **Catalog Number :** 160067-03
Name: ICP-MS DOE SOIL SPIKE **Received:** 27-AUG-09 **Lot Number :** 1015749
Type: Source Material **Expires:** 27-AUG-10
Employee: Francena Armstrong
Supplier: 02si
Description: ICP-MS Spike for soil products.
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	200 mg/L	Arsenic	8 mg/L
Barium	5 mg/L	Beryllium	5 mg/L
Boron	10 mg/L	Cadmium	1 mg/L
Calcium	200 mg/L	Chromium	5 mg/L
Cobalt	5 mg/L	Copper	5 mg/L
Iron	200 mg/L	Lead	20 mg/L
Lithium	5 mg/L	Magnesium	200 mg/L
Manganese	5 mg/L	Nickel	5 mg/L
Phosphorus, Total as P	200 mg/L	Potassium	200 mg/L
Selenium	2 mg/L	Sodium	200 mg/L
Strontium	5 mg/L	Thallium	10 mg/L
Thorium	5 mg/L	Uranium	5 mg/L
Uranium-235	.036 mg/L	Uranium-238	4.964 mg/L
Vanadium	5 mg/L	Zinc	5 mg/L

Standard Logbook

Serial ID: UI090827-B **Opened:** 27-AUG-09 **Catalog Number :** 160067-03
Name: ICP-MS DOE SOIL SPIKE **Received:** 27-AUG-09 **Lot Number :** 1015749
Type: Source Material **Expires:** 27-AUG-10
Employee: Francena Armstrong
Supplier: 02si
Description: ICP-MS Spike for Soil Products
Comments: None

Analyte	Concentration	Analyte	Concentration
Antimony	20 mg/L	Molybdenum	5 mg/L
Silicon	200 mg/L	Silver	5 mg/L
Tin	5 mg/L	Zirconium	5 mg/L

Serial ID: UI090925-40 **Opened:** 23-OCT-09 **Amount :** 500 mL
Name: SECOND SOURCE STD -1 **Received:** 25-SEP-09 **Catalog Number :** SGELMX38-500N
Type: Source Material **Expires:** 30-SEP-10 **Lot Number :** 4909129
Employee: Helen Camello **Solvent :** 5%HNO3
Supplier: SPECTRO PURE
Description: SECOND SOURCE STD #1A 5%HNO3
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	1000 mg/L	Arsenic	100 mg/L
Barium	100 mg/L	Boron	100 mg/L
Cadmium	100 mg/L	Calcium	1000 mg/L
Chromium	100 mg/L	Cobalt	100 mg/L
Copper	100 mg/L	Iron	1000 mg/L
Lead	100 mg/L	Phosphorous	500 mg/L
Potassium	500 mg/L	Selenium	500 mg/L
Sodium	500 mg/L	Strontium	100 mg/L

Serial ID: UI090925-41 **Opened:** 23-OCT-09 **Amount :** 500 mL
Name: SECOND SOURCE STD -1 **Received:** 25-SEP-09 **Catalog Number :** SGELMX39-500B
Type: Source Material **Expires:** 30-SEP-10 **Lot Number :** 4909130
Employee: Helen Camello **Solvent :** 5%HNO3,TR,HF
Supplier: SPECTRO PURE
Description: SECOND SOURCE STD #1B
Comments: None

Analyte	Concentration	Analyte	Concentration
Antimony	100 mg/L	Beryllium	50 mg/L
Magnesium	1000 mg/L	Manganese	100 mg/L
Molybdenum	100 mg/L	Nickel	100 mg/L
Silver	50 mg/L	Sulfur	500 mg/L
Thallium	100 mg/L	Tin	100 mg/L
Titanium	100 mg/L	Uranium	100 mg/L

Standard Logbook

Analyte	Concentration	Analyte	Concentration
Vanadium	100 mg/L	Zinc	100 mg/L

Serial ID: UI091015-42 **Opened:** 28-OCT-09 **Amount :** 500 mL
Name: SI 1000mg/L **Received:** 15-OCT-09 **Catalog Number :** 060014-02-03
Type: Source Material **Expires:** 28-OCT-10 **Lot Number :** 1017581
Employee: Helen Camello **Solvent :** 0.3%H2O(NH4)2SiF6
Supplier: o2si
Description: Silicon 1000mg/L+/-0.3%in H2O(NH4)2SiF6
Comments: None

Analyte	Concentration	Analyte	Concentration
Silica	2139 mg/L	Silicon	1000 mg/L

Serial ID: UI091102-40 **Opened:** 16-NOV-09 **Amount :** 500 mL
Name: TRACE CALSTD#1A SOUF **Received:** 02-NOV-09 **Catalog Number :** HP2270-1-500
Type: Source Material **Expires:** 31-OCT-10 **Lot Number :** 0930215
Employee: Helen Camello **Solvent :** HNO3
Supplier: Environmental Express
Description: Trace Calibration Std #1A
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	2000 mg/L	Arsenic	200 mg/L
Barium	200 mg/L	Beryllium	200 mg/L
Boron	200 mg/L	Cadmium	200 mg/L
Calcium	2000 mg/L	Chromium	200 mg/L
Cobalt	200 mg/L	Copper	200 mg/L
Iron	2000 mg/L	Lead	200 mg/L
Magnesium	2000 mg/L	Manganese	200 mg/L
Nickel	200 mg/L	Phosphorous	1000 mg/L
Potassium	2000 mg/L	Selenium	200 mg/L
Sodium	2000 mg/L	Strontium	200 mg/L
Thallium	200 mg/L	Uranium	200 mg/L
Vanadium	200 mg/L	Zinc	200 mg/L

Serial ID: UI091102-41 **Opened:** 16-NOV-09 **Amount :** 500 mL
Name: TRACE CALSTD#1B SOUF **Received:** 02-NOV-09 **Catalog Number :** HP2270-2-500
Type: Source Material **Expires:** 31-OCT-10 **Lot Number :** 0930216
Employee: Helen Camello **Solvent :** HNO3
Supplier: Environmental Express
Description: Trace Calibration Standard #1B
Comments: None

Analyte	Concentration	Analyte	Concentration
----------------	----------------------	----------------	----------------------

Standard Logbook

Analyte	Concentration	Analyte	Concentration
Antimony	200 mg/L	Molybdenum	200 mg/L
Silver	200 mg/L	Sulfur	400 mg/L
Tin	200 mg/L	Titanium	200 mg/L

Serial ID: UI091102-42 **Opened:** 17-NOV-09 **Amount :** 200 mL
Name: SILICON **Received:** 02-NOV-09 **Catalog Number :** HP100050-4F
Type: Source Material **Expires:** 17-NOV-10 **Lot Number :** 0921924
Employee: Helen Camello **Solvent :** H2O/tr HF
Supplier: ENVIRONMENTAL EXPRESS
Description: SILICON 1000mg/L H2O/tr HF
Comments: None

Analyte	Concentration	Analyte	Concentration
Silica	2139 mg/L	Silicon	1000 mg/L

Serial ID: UI091217-12 **Opened:** 17-DEC-09 **Amount :** 250 mL
Name: ICP-MS ICSAB Master B **Received:** 17-DEC-09 **Catalog Number :** 160033-02
Type: Source Material **Expires:** 17-DEC-10 **Lot Number :** 1018212
Employee: Paul Boyd **Solvent :** +/- 0.5% in 2% HNO3
Supplier: 02Si
Description: ICPMS ICSAB Master B
Comments: None

Analyte	Concentration	Analyte	Concentration
Arsenic	2 mg/L	Barium	2 mg/L
Beryllium	2 mg/L	Boron	2 mg/L
Cadmium	2 mg/L	Chromium	2 mg/L
Cobalt	2 mg/L	Copper	2 mg/L
Lead	2 mg/L	Lithium	2 mg/L
Manganese	2 mg/L	Nickel	2 mg/L
Selenium	2 mg/L	Strontium	2 mg/L
Thallium	2 mg/L	Thorium	2 mg/L
Uranium	2 mg/L	Vanadium	2 mg/L
Zinc	2 mg/L		

Serial ID: UI091217-13 **Opened:** 17-DEC-09 **Amount :** 250 mL
Name: ICP-MS ICSAB Master C **Received:** 17-DEC-09 **Catalog Number :** 160033-03
Type: Source Material **Expires:** 17-DEC-10 **Lot Number :** 1016926
Employee: Paul Boyd **Solvent :** +/- 0.5% in 2% HNO3
Supplier: 02Si
Description: ICPMS ICSAB Master C
Comments: None

Analyte	Concentration	Analyte	Concentration
---------	---------------	---------	---------------

Standard Logbook

Analyte	Concentration	Analyte	Concentration
Antimony	2 mg/L	Silver	2 mg/L
Tin	2 mg/L	Tungsten	2 mg/L
Zirconium	2 mg/L		

Serial ID: UI100310-48 **Opened:** 19-MAR-10 **Amount :** 1000 mL
Name: Trace ICP ICSA **Received:** 12-MAR-10 **Catalog Number :** 160005-02
Type: Source Material **Expires:** 19-MAR-11 **Lot Number :** 1019141
Employee: Helen Camello **Solvent :** 3% HCl + 1% HNO3
Supplier: o2si
Description: Trace ICP Interferent Check Standard A
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	500000 UG/L	Calcium	500000 UG/L
Iron	200000 UG/L	Magnesium	500000 UG/L

Serial ID: UI100310-49.11 **Opened:** 29-MAR-10 **Amount :** 100 ml
Name: Trace ICP ICSAB **Received:** 12-MAR-10 **Catalog Number :** 160066-04
Type: Source Material **Expires:** 30-MAR-10 **Lot Number :** 1019142
Employee: Helen Camello **Solvent :** 3% HCl + 1% HNO3
Supplier: o2si
Description: Trace ICP Inteferent Check Standard AB
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	500000 ug/L	Antimony	500 ug/L
Arsenic	500 ug/L	Barium	500 ug/L
Beryllium	250 ug/L	Boron	500 ug/L
Cadmium	500 ug/L	Calcium	500000 ug/L
Chromium	500 ug/L	Cobalt	500 ug/L
Copper	500 ug/L	Iron	200000 ug/L
Lead	500 ug/L	Magnesium	500000 ug/L
Manganese	500 ug/L	Molybdenum	500 ug/L
Nickel	500 ug/L	Phosphorous	2500 ug/L
Potassium	5000 ug/L	Selenium	2500 ug/L
Silica	10696.5 ug/L	Silicon	5000 ug/L
Silver	250 ug/L	Sodium	5000 ug/L
Strontium	500 ug/L	Sulfur	2500 ug/L
Thallium	500 ug/L	Tin	500 ug/L
Titanium	500 ug/L	Uranium	500 ug/L
Vanadium	500 ug/L	Zinc	500 ug/L

Standard Logbook

Serial ID: UI100317-06 **Opened:** 17-MAR-10 **Amount :** 250 mL
Name: ICP-MS ICV/CCV Master A **Received:** 17-MAR-10 **Catalog Number :** 160055-01
Type: Source Material **Expires:** 17-MAR-11 **Lot Number :** 1019161
Employee: Paul Boyd **Solvent :** +/- 0.5% in 5% HNO3 100 cm2
Supplier: 02SI
Description: ICPMS ICV/CCV SOLN A - 10ppm
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	2020 mg/L	Calcium	2000 mg/L
Iron	2000 mg/L	Magnesium	2000 mg/L
Phosphorous	2000 mg/L	Potassium	2000 mg/L
Sodium	2000 mg/L		

Serial ID: UI100317-07 **Opened:** 17-MAR-10 **Amount :** 250 mL
Name: ICP-MS ICV/CCV Master B **Received:** 17-MAR-10 **Catalog Number :** 160054-02
Type: Source Material **Expires:** 17-MAR-11 **Lot Number :** 1019162
Employee: Paul Boyd **Solvent :** +/- 0.5% in 5% HNO3 100 cm2
Supplier: 02SI
Description: ICPMS ICV/CCV Soln B - 10ppm
Comments: None

Analyte	Concentration	Analyte	Concentration
Arsenic	20 mg/L	Barium	20 mg/L
Beryllium	20 mg/L	Boron	40 mg/L
Cadmium	20 mg/L	Chromium	20 mg/L
Cobalt	20 mg/L	Copper	20 mg/L
Lead	20 mg/L	Lithium	20 mg/L
Manganese	20 mg/L	Nickel	20 mg/L
Selenium	20 mg/L	Strontium	20 mg/L
Thallium	20 mg/L	Thorium	20 mg/L
Uranium	20 mg/L	Vanadium	20 mg/L
Zinc	20 mg/L		

Serial ID: UI100317-08 **Opened:** 17-MAR-10 **Amount :** 250 mL
Name: ICP-MS ICV/CCV Master C **Received:** 17-MAR-10 **Catalog Number :** 160054-03
Type: Source Material **Expires:** 17-MAR-11 **Lot Number :** 1019163
Employee: Paul Boyd **Solvent :** +/- 0.5% in 5% HNO3 100 cm2
Supplier: 02SI
Description: ICPMS ICV/CCV Soln C - 10ppm
Comments: None

Analyte	Concentration	Analyte	Concentration
Antimony	20 mg/L	Molybdenum	20 mg/L
Silver	20 mg/L	Tin	20 mg/L
Titanium	20 mg/L	Tungsten	20 mg/L

Standard Logbook

Analyte	Concentration	Analyte	Concentration
Zirconium	20 mg/L		

Serial ID: UI100318-11 **Opened:** 18-MAR-10 **Amount :** 1000 mL
Name: ICP-MS ICSA Master A **Received:** 18-MAR-10 **Catalog Number :** 160013-01-01L
Type: Source Material **Expires:** 18-MAR-11 **Lot Number :** 1018321
Employee: Paul Boyd **Solvent :** 2% HNO3
Supplier: Q2SI
Description: ICP-MS ICSA Master A
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	1000 mg/L	Calcium	1000 mg/L
Carbon	2000 mg/L	Chloride	10000 mg/L
Iron	1000 mg/L	Magnesium	1000 mg/L
Molybdenum	20 mg/L	Phosphorous	1000 mg/L
Potassium	1000 mg/L	Sodium	1000 mg/L
Sulfur	1000 mg/L	Titanium	20 mg/L

Serial ID: UI100325-40 **Opened:** 25-MAR-10 **Amount :** 500 mL
Name: ICP HIGH RANGE STD-A **Received:** 25-MAR-10 **Catalog Number :** 160211-05-03
Type: Source Material **Expires:** 25-MAR-11 **Lot Number :** 1019348
Employee: Helen Camello **Solvent :** +/-0.5%in2%HNO3
Supplier: Q2SI
Description: ICP HIGH RANGE STD SOLUTION A
Comments: None

Analyte	Concentration	Analyte	Concentration
Antimony	10000 ug/L	Arsenic	10000 ug/L
Barium	15000 ug/L	Beryllium	3000 ug/L
Boron	5000 ug/L	Cadmium	10000 ug/L
Chromium	25000 ug/L	Cobalt	10000 ug/L
Copper	20000 ug/L	Lead	25000 ug/L
Manganese	10000 ug/L	Molybdenum	10000 ug/L
Nickel	10000 ug/L	Phosphorous	15000 ug/L
Potassium	300000 ug/L	Selenium	10000 ug/L
Silica	107000 ug/L	Silicon	50000 ug/L
Silver	1000 ug/L	Strontium	10000 ug/L
Sulfur	50000 ug/L	Thallium	10000 ug/L
Tin	10000 ug/L	Titanium	10000 ug/L
Vanadium	10000 ug/L	Zinc	15000 ug/L

Standard Logbook

Serial ID: UI100325-41 **Opened:** 25-MAR-10 **Amount :** 500 mL
Name: ICP HIGH RANGE STD B **Received:** 25-MAR-10 **Catalog Number :** 160211-05-03
Type: Source Material **Expires:** 25-MAR-11 **Lot Number :** 1019348
Employee: Helen Camello **Solvent :** +/-0.5%in2%HNO3
Supplier: 02SI
Description: ICP HIGH RANGE STD SOLUTION B
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	500000 ug/L	Calcium	500000 ug/L
Iron	500000 ug/L	Magnesium	500000 ug/L
Sodium	500000 ug/L	Uranium	15000 ug/L

Serial ID: UI1268741-01 **Opened:** 11-FEB-10 **Lot Number :** 1018514
Name: METALSPIKE-1 **Received:** 11-FEB-10
Type: Source Material **Expires:** 11-FEB-11
Employee: Bryan Davis
Supplier: OS2I
Description: Metals Spike Mix I
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	1000 ug/mL	Arsenic	100 ug/mL
Barium	100 ug/mL	Beryllium	100 ug/mL
Boron	100 ug/mL	Cadmium	100 ug/mL
Calcium	1000 ug/mL	Cobalt	100 ug/mL
Iron	1000 ug/mL	Lead	100 ug/mL
Magnesium	1000 ug/mL	Phosphorous	100 ug/mL
Potassium	1000 ug/mL	Silver	100 ug/mL
Sodium	1000 ug/mL	Strontium	100 ug/mL

Serial ID: UI1268744-06 **Opened:** 11-FEB-10 **Lot Number :** 1018515
Name: METALSPIKE-2 **Received:** 11-FEB-10
Type: Source Material **Expires:** 11-FEB-11
Employee: Bryan Davis
Supplier: OS2I
Description: Metals Spike Mix II
Comments: None

Analyte	Concentration	Analyte	Concentration
Antimony	100 ug/mL	Chromium	100 ug/mL
Copper	100 ug/mL	Manganese	100 ug/mL
Molybdenum	100 ug/mL	Nickel	100 ug/mL
Selenium	100 ug/mL	Silica	2141 ug/mL
Silicon	1000 ug/mL	Sulfur	1000 ug/mL
Thallium	100 ug/mL	Tin	100 ug/mL

Standard Logbook

Analyte	Concentration	Analyte	Concentration
Titanium	100 ug/mL	Uranium	100 ug/mL
Uranium-235	.72 ug/mL	Uranium-238	99.28 ug/mL
Vanadium	100 ug/mL	Zinc	100 ug/mL

Serial ID: UMS100226-01 **Opened:** 26-FEB-10 **Amount :** 250 mL
Name: ICPMSCaSPIKEB **Received:** 26-FEB-10 **Catalog Number :** ZGEL-100-250
Type: Source Material **Expires:** 26-FEB-11 **Lot Number :** 21-104JB
Employee: Paul Boyd
Supplier: SPEX
Description: ICPMS Calibration Standard Solution B
Comments: None

Analyte	Concentration	Analyte	Concentration
Arsenic	10 mg/L	Barium	10 mg/L
Beryllium	10 mg/L	Boron	20 mg/L
Cadmium	10 mg/L	Chromium	10 mg/L
Cobalt	10 mg/L	Copper	10 mg/L
Lead	10 mg/L	Lithium	10 mg/L
Manganese	10 mg/L	Nickel	10 mg/L
Selenium	10 mg/L	Silver	10 mg/L
Strontium	10 mg/L	Thallium	10 mg/L
Thorium	10 mg/L	Uranium	10 mg/L
Vanadium	10 mg/L	Zinc	10 mg/L

Serial ID: UMS100226-02 **Opened:** 26-FEB-10 **Catalog Number :** ZGEL-102-250
Name: ICPMSCaSPIKEA **Received:** 26-FEB-10 **Lot Number :** 21-103JB
Type: Source Material **Expires:** 26-FEB-11
Employee: Paul Boyd
Supplier: SPEX
Description: ICPMS Calibration Standard Solution A
Comments: None

Analyte	Concentration	Analyte	Concentration
Aluminum	1000 mg/L	Calcium	1000 mg/L
Iron	1000 mg/L	Magnesium	1000 mg/L
Phosphorous	1000 mg/L	Potassium	1000 mg/L
Sodium	1000 mg/L		

Serial ID: UMS100226-03 **Opened:** 26-FEB-10 **Amount :** 250 ml
Name: ICPMSCaSPIKEC **Received:** 26-FEB-10 **Catalog Number :** ZGEL-101-250
Type: Source Material **Expires:** 26-FEB-11 **Lot Number :** 21-102JB
Employee: Paul Boyd
Supplier: SPEX
Description: ICPMS Calibration Standard Solution C

Standard Logbook

Comments: None

Analyte	Concentration	Analyte	Concentration
Antimony	10 mg/L	Molybdenum	10 mg/L
Tin	10 mg/L	Titanium	10 mg/L
Zirconium	10 mg/L		

Serial ID: IHG100309-01 Opened: 09-MAR-10 Instrument Id : Mercury
 Name: MHGINTER1 Received: 09-MAR-10 Pipet Id : Minou1
 Type: Intermediate Expires: 10-MAR-10 Solvent : 1mL HNO3 + TypeI H2O
 Employee: Tara Griffin
 Supplier: GEL
 Description: Mercury Intermediate 1st Source 200 ug/L
 Comments: Prepare fresh daily

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UHG1167639-01	Mercury	1000 mg/L	.05 mL	250 mL	200 ug/L

Serial ID: IHG100309-02 Opened: 09-MAR-10 Pipet Id : Minou1
 Name: MHGINTER2 Received: 09-MAR-10 Solvent : 2% HNO3-1274391
 Type: Intermediate Expires: 10-MAR-10
 Employee: Tara Griffin
 Supplier: GEL
 Description: Mercury Intermediate 2nd Source 200 ug/L
 Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UHG1167641-02	Mercury	999.7 mg/L	.05 mL	250 mL	200 ug/L

Serial ID: IHG100310-01 Opened: 10-MAR-10 Instrument Id : Mercury
 Name: MHGINTER1 Received: 10-MAR-10 Pipet Id : Minou1
 Type: Intermediate Expires: 11-MAR-10 Solvent : 1mL HNO3 + TypeI H2O
 Employee: Tara Griffin
 Supplier: GEL
 Description: Mercury Intermediate 1st Source 200 ug/L
 Comments: Prepare fresh daily

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UHG1167639-01	Mercury	1000 mg/L	.05 mL	250 mL	200 ug/L

Serial ID: IHG100310-02 Opened: 10-MAR-10 Pipet Id : Minou1
 Name: MHGINTER2 Received: 10-MAR-10 Solvent : 2% HNO3-1274391
 Type: Intermediate Expires: 11-MAR-10
 Employee: Tara Griffin
 Supplier: GEL

Standard Logbook

Description: Mercury Intermediate 2nd Source 200 ug/L

Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UHG1167641-02	Mercury	999.7 mg/L	.05 mL	250 mL	200 ug/L

Serial ID: WHG100309-07 Opened: 09-MAR-10 Pipet Id : Hg1289245
 Name: MHGWORKCALS0.2CRA Received: 09-MAR-10 Solvent : 2% HNO3-1274391
 Type: Working Expires: 16-MAR-10
 Employee: Tara Griffin
 Supplier: GEL
 Description: Mercury Working Standard 1st Source CAL S 0.2/CRA
 Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
IHG100309-01	Mercury	200 ug/L	30 uL	30 mL	.2 ug/L

Serial ID: WHG100309-08 Opened: 09-MAR-10 Pipet Id : Hg1289245
 Name: MHGWORKCALS0.5 Received: 09-MAR-10 Solvent : 2% HNO3-1274391
 Type: Working Expires: 16-MAR-10
 Employee: Tara Griffin Verified: 20-JUL-07
 Supplier: GEL
 Description: Mercury Working Standard 1st Source CAL S 0.5
 Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
IHG100309-01	Mercury	200 ug/L	75 uL	30 mL	.5 ug/L

Serial ID: WHG100309-09 Opened: 09-MAR-10 Pipet Id : Hg1289245
 Name: MHGWORKCALS2.0 Received: 09-MAR-10 Solvent : 2% HNO3-1274391
 Type: Working Expires: 16-MAR-10
 Employee: Tara Griffin Verified: 20-JUL-07
 Supplier: GEL
 Description: Mercury Working 1st Source CAL S 2.0
 Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
IHG100309-01	Mercury	200 ug/L	300 uL	30 mL	2 ug/L

Serial ID: WHG100309-10 Opened: 09-MAR-10 Pipet Id : Hg1289245
 Name: MHGWORKCALS5.0CCV Received: 09-MAR-10 Solvent : 2% HNO3-1274391
 Type: Working Expires: 16-MAR-10
 Employee: Tara Griffin Verified: 20-JUL-07
 Supplier: GEL
 Description: Mercury Working 1st Source CAL S 5.0/CCV

Standard Logbook

Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
IHG100309-01	Mercury	200 ug/L	750 uL	30 mL	5 ug/L

Serial ID: WHG100309-11 Opened: 09-MAR-10 Pipet Id : Hg1289245
 Name: MHGWORKCALS10.0 Received: 09-MAR-10 Solvent : 2% HNO3-1274391
 Type: Working Expires: 16-MAR-10
 Employee: Tara Griffin
 Supplier: GEL
 Description: Mercury Working 1st Source CAL S 10.0
 Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
IHG100309-01	Mercury	200 ug/L	1.5 mL	30 mL	10 ug/L

Serial ID: WHG100309-12 Opened: 09-MAR-10 Pipet Id : Hg1289245
 Name: MHGWORKS5.0ICV Received: 09-MAR-10 Solvent : 2% HNO3-1274391
 Type: Working Expires: 16-MAR-10
 Employee: Tara Griffin Verified: 20-JUL-07
 Supplier: GEL
 Description: Mercury Working 2nd Source S 5.0/ICV
 Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
IHG100309-02	Mercury	200 ug/L	750 uL	30 mL	5 ug/L

Serial ID: WHG100310-07 Opened: 10-MAR-10 Pipet Id : Hg1289245
 Name: MHGWORKCALS0.2CRA Received: 10-MAR-10 Solvent : 2% HNO3-1274391
 Type: Working Expires: 17-MAR-10
 Employee: Tara Griffin
 Supplier: GEL
 Description: Mercury Working Standard 1st Source CAL S 0.2/CRA
 Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
IHG100310-01	Mercury	200 ug/L	30 uL	30 mL	.2 ug/L

Serial ID: WHG100310-08 Opened: 10-MAR-10 Pipet Id : Hg1289245
 Name: MHGWORKCALS0.5 Received: 10-MAR-10 Solvent : 2% HNO3-1274391
 Type: Working Expires: 17-MAR-10
 Employee: Tara Griffin Verified: 20-JUL-07
 Supplier: GEL
 Description: Mercury Working Standard 1st Source CAL S 0.5
 Comments: None

Standard Logbook

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
IHG100310-01	Mercury	200 ug/L	75 uL	30 mL	.5 ug/L

Serial ID: WHG100310-09 Opened: 10-MAR-10 Pipet Id : Hg1289245
 Name: MHGWORKCALS2.0 Received: 10-MAR-10 Solvent : 2% HNO3-1274391
 Type: Working Expires: 17-MAR-10
 Employee: Tara Griffin Verified: 20-JUL-07
 Supplier: GEL
 Description: Mercury Working 1st Source CAL S 2.0
 Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
IHG100310-01	Mercury	200 ug/L	300 uL	30 mL	2 ug/L

Serial ID: WHG100310-10 Opened: 10-MAR-10 Pipet Id : Hg1289245
 Name: MHGWORKCALS5.0CCV Received: 10-MAR-10 Solvent : 2% HNO3-1274391
 Type: Working Expires: 17-MAR-10
 Employee: Tara Griffin Verified: 20-JUL-07
 Supplier: GEL
 Description: Mercury Working 1st Source CAL S 5.0/CCV
 Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
IHG100310-01	Mercury	200 ug/L	750 uL	30 mL	5 ug/L

Serial ID: WHG100310-11 Opened: 10-MAR-10 Pipet Id : Hg1289245
 Name: MHGWORKCALS10.0 Received: 10-MAR-10 Solvent : 2% HNO3-1274391
 Type: Working Expires: 17-MAR-10
 Employee: Tara Griffin
 Supplier: GEL
 Description: Mercury Working 1st Source CAL S 10.0
 Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
IHG100310-01	Mercury	200 ug/L	1.5 mL	30 mL	10 ug/L

Serial ID: WHG100310-12 Opened: 10-MAR-10 Pipet Id : Hg1289245
 Name: MHGWORKS5.0ICV Received: 10-MAR-10 Solvent : 2% HNO3-1274391
 Type: Working Expires: 17-MAR-10
 Employee: Tara Griffin Verified: 20-JUL-07
 Supplier: GEL
 Description: Mercury Working 2nd Source S 5.0/ICV
 Comments: None

Standard Logbook

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
IHG100310-02	Mercury	200 ug/L	750 uL	30 mL	5 ug/L

Serial ID: WHG100310-14 **Opened:** 10-MAR-10 **Pipet Id :** Hq1289245
Name: MHGSOILMSSPIKE **Received:** 10-MAR-10 **Solvent :** 2% HNO3-1274391
Type: Working **Expires:** 17-MAR-10
Employee: Tara Griffin **Verified:** 20-JUL-07
Supplier: GEL
Description: Mercury soil working intermediate standard for MS
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UHG1167639-01	Mercury	1000 mg/L	.05 mL	250 mL	200 ug/L

Serial ID: WI100329-42 **Opened:** 29-MAR-10 **Balance Id :** 216
Name: TRACE ICP 0.1 PPM STD. **Received:** 02-NOV-09 **Pipet Id :** 3581809
Type: Working **Expires:** 30-MAR-10 **Solvent :** 3%HCL and 1%HNO3 -1293083
Employee: Helen Camello
Supplier: GEL
Description: TRACE ICP 0.1 PPM CALIBRATION STD.
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
WI100329-44	Aluminum	10000 ug/L	10 mL	100 mL	1000 ug/L
WI100329-44	Antimony	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Arsenic	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Barium	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Beryllium	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Boron	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Cadmium	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Calcium	10000 ug/L	10 mL	100 mL	1000 ug/L
WI100329-44	Chromium	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Cobalt	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Copper	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Iron	10000 ug/L	10 mL	100 mL	1000 ug/L
WI100329-44	Lead	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Magnesium	10000 ug/L	10 mL	100 mL	1000 ug/L
WI100329-44	Manganese	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Molybdenum	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Nickel	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Phosphorous	5000 ug/L	10 mL	100 mL	500 ug/L
WI100329-44	Potassium	10000 ug/L	10 mL	100 mL	1000 ug/L
WI100329-44	Selenium	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Silica	10698 ug/L	10 mL	100 mL	1069 ug/L
WI100329-44	Silicon	5000 ug/L	10 mL	100 mL	500 ug/L
WI100329-44	Silver	1000 ug/L	10 mL	100 mL	100 ug/L

Standard Logbook

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
WI100329-44	Sodium	10000 ug/L	10 mL	100 mL	1000 ug/L
WI100329-44	Strontium	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Sulfur	2000 ug/L	10 mL	100 mL	200 ug/L
WI100329-44	Thallium	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Tin	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Titanium	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Uranium	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Vanadium	1000 ug/L	10 mL	100 mL	100 ug/L
WI100329-44	Zinc	1000 ug/L	10 mL	100 mL	100 ug/L

Serial ID: WI100329-43 **Opened:** 29-MAR-10 **Balance Id :** 216
Name: TRACE ICP 0.5/CCV STD. **Received:** 02-NOV-09 **Pipet Id :** 3581809
Type: Working **Expires:** 30-MAR-10 **Solvent :** 3%HCL and 1%HNO3 -1293083
Employee: Helen Camello
Supplier: GEL
Description: TRACE ICP 0.5/CCV CALIBRATION STD.
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI090421-40	Sodium	1000 ug/mL	5 mL	1000 mL	5000 UG/L
UI091015-42	Silica	2139 mg/L	2.5 mL	1000 mL	5348.25 UG/L
UI091015-42	Silicon	1000 mg/L	2.5 mL	1000 mL	2500 UG/L
UI091102-40	Aluminum	2000 mg/L	2.5 mL	1000 mL	5000 UG/L
UI091102-40	Arsenic	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Barium	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Beryllium	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Boron	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Cadmium	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Calcium	2000 mg/L	2.5 mL	1000 mL	5000 UG/L
UI091102-40	Chromium	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Cobalt	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Copper	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Iron	2000 mg/L	2.5 mL	1000 mL	5000 UG/L
UI091102-40	Lead	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Magnesium	2000 mg/L	2.5 mL	1000 mL	5000 UG/L
UI091102-40	Manganese	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Nickel	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Phosphorous	1000 mg/L	2.5 mL	1000 mL	2500 UG/L
UI091102-40	Potassium	2000 mg/L	2.5 mL	1000 mL	5000 UG/L
UI091102-40	Selenium	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Sodium	2000 mg/L	2.5 mL	1000 mL	5000 UG/L
UI091102-40	Strontium	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Thallium	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Uranium	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-40	Vanadium	200 mg/L	2.5 mL	1000 mL	500 UG/L

Standard Logbook

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI091102-40	Zinc	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-41	Antimony	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-41	Molybdenum	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-41	Silver	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-41	Sulfur	400 mg/L	2.5 mL	1000 mL	1000 UG/L
UI091102-41	Tin	200 mg/L	2.5 mL	1000 mL	500 UG/L
UI091102-41	Titanium	200 mg/L	2.5 mL	1000 mL	500 UG/L

Serial ID: WI100329-44 **Opened:** 29-MAR-10 **Balance Id :** 216
Name: TRACE ICP SCAL 1.0 **Received:** 02-NOV-09 **Pipet Id :** 3581809
Type: Working **Expires:** 30-MAR-10 **Solvent :** 3%HCL and 1 %HNO3-1293083
Employee: Helen Camello
Supplier: o2si
Description: Trace ICP Calibration Standard 1.0ppm
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI091015-42	Silica	2139 mg/L	2.5 mL	500 mL	10698 ug/L
UI091015-42	Silicon	1000 mg/L	2.5 mL	500 mL	5000 ug/L
UI091102-40	Aluminum	2000 mg/L	2.5 mL	500 mL	10000 ug/L
UI091102-40	Arsenic	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Barium	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Beryllium	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Boron	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Cadmium	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Calcium	2000 mg/L	2.5 mL	500 mL	10000 ug/L
UI091102-40	Chromium	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Cobalt	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Copper	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Iron	2000 mg/L	2.5 mL	500 mL	10000 ug/L
UI091102-40	Lead	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Magnesium	2000 mg/L	2.5 mL	500 mL	10000 ug/L
UI091102-40	Manganese	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Nickel	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Phosphorous	1000 mg/L	2.5 mL	500 mL	5000 ug/L
UI091102-40	Potassium	2000 mg/L	2.5 mL	500 mL	10000 ug/L
UI091102-40	Selenium	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Sodium	2000 mg/L	2.5 mL	500 mL	10000 ug/L
UI091102-40	Strontium	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Thallium	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Uranium	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Vanadium	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-40	Zinc	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-41	Antimony	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-41	Molybdenum	200 mg/L	2.5 mL	500 mL	1000 ug/L

Standard Logbook

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI091102-41	Silver	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-41	Sulfur	400 mg/L	2.5 mL	500 mL	2000 ug/L
UI091102-41	Tin	200 mg/L	2.5 mL	500 mL	1000 ug/L
UI091102-41	Titanium	200 mg/L	2.5 mL	500 mL	1000 ug/L

Serial ID: WI100329-45 **Opened:** 29-MAR-10 **Balance Id :** 216
Name: TRACE ICP S-10 STD **Received:** 22-APR-09 **Pipet Id :** 3581809
Type: Working **Expires:** 30-MAR-10 **Solvent :** 3%HCL and 1%HNO3 -1293083
Employee: Helen Camello
Supplier: GEL
Description: TRACE ICP S-10 CALIBRATION STD.
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI090421-40	Sodium	1000 ug/mL	10 mL	500 mL	20000 UG/L
UI090422-40	Aluminum	5000 mg/L	5 mL	500 mL	50000 UG/L
UI090422-40	Calcium	5000 mg/L	5 mL	500 mL	50000 UG/L
UI090422-40	Iron	2000 mg/L	5 mL	500 mL	20000 UG/L
UI090422-40	Magnesium	5000 mg/L	5 mL	500 mL	50000 UG/L

Serial ID: WI100329-46 **Opened:** 29-MAR-10 **Balance Id :** 216
Name: ICP TRACE ICV **Received:** 25-SEP-09 **Pipet Id :** 3581809
Type: Working **Expires:** 30-MAR-10 **Solvent :** 3%HCL AND 1%HNO3-1293083
Employee: Helen Camello
Supplier: GEL
Description: Initial Calibration Verification ICP Trace Metals
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI090925-40	Aluminum	1000 mg/L	2.5 mL	500 mL	5000 ug/L
UI090925-40	Arsenic	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-40	Barium	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-40	Boron	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-40	Cadmium	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-40	Calcium	1000 mg/L	2.5 mL	500 mL	5000 ug/L
UI090925-40	Chromium	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-40	Cobalt	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-40	Copper	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-40	Iron	1000 mg/L	2.5 mL	500 mL	5000 ug/L
UI090925-40	Lead	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-40	Phosphorous	500 mg/L	2.5 mL	500 mL	2500 ug/L
UI090925-40	Potassium	500 mg/L	2.5 mL	500 mL	2500 ug/L
UI090925-40	Selenium	500 mg/L	2.5 mL	500 mL	2500 ug/L
UI090925-40	Sodium	500 mg/L	2.5 mL	500 mL	2500 ug/L
UI090925-40	Strontium	100 mg/L	2.5 mL	500 mL	500 ug/L

Standard Logbook

Parent Material	Analyte	Parent Conc.	Alliquot	Final Vol.	Final Conc.
UI090925-41	Antimony	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-41	Beryllium	50 mg/L	2.5 mL	500 mL	250 ug/L
UI090925-41	Magnesium	1000 mg/L	2.5 mL	500 mL	5000 ug/L
UI090925-41	Manganese	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-41	Molybdenum	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-41	Nickel	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-41	Silver	50 mg/L	2.5 mL	500 mL	250 ug/L
UI090925-41	Sulfur	500 mg/L	2.5 mL	500 mL	2500 ug/L
UI090925-41	Thallium	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-41	Tin	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-41	Titanium	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-41	Uranium	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-41	Vanadium	100 mg/L	2.5 mL	500 mL	500 ug/L
UI090925-41	Zinc	100 mg/L	2.5 mL	500 mL	500 ug/L
UI091102-42	Silica	2139 mg/L	2.5 mL	500 mL	10695 ug/L
UI091102-42	Silicon	1000 mg/L	2.5 mL	500 mL	5000 ug/L

Serial ID: WI100329-47 **Opened:** 29-MAR-10 **Balance Id :** 216
Name: PQL Working Standard **Received:** 30-JUN-09 **Pipet Id :** 3581809
Type: Working **Expires:** 30-MAR-10 **Solvent :** 3%HCL &1%HNO3-1293083
Employee: Helen Camello
Supplier: 02si
Description: PQL Working Standard
Comments: None

Parent Material	Analyte	Parent Conc.	Alliquot	Final Vol.	Final Conc.
UI090701-40	Aluminum	100 mg/L	2 mL	1000 mL	200 ug/L
UI090701-40	Antimony	5 mg/L	2 mL	1000 mL	10 ug/L
UI090701-40	Arsenic	15 mg/L	2 mL	1000 mL	15 ug/L
UI090701-40	Barium	2.5 mg/L	2 mL	1000 mL	5 ug/L
UI090701-40	Beryllium	2.5 mg/L	2 mL	1000 mL	5 ug/L
UI090701-40	Boron	25 mg/L	2 mL	1000 mL	50 ug/L
UI090701-40	Cadmium	2.5 mg/L	2 mL	1000 mL	5 ug/L
UI090701-40	Calcium	100 mg/L	2 mL	1000 mL	100 ug/L
UI090701-40	Chromium	2.5 mg/L	2 mL	1000 mL	5 ug/L
UI090701-40	Cobalt	2.5 mg/L	2 mL	1000 mL	5 ug/L
UI090701-40	Copper	5 mg/L	2 mL	1000 mL	10 ug/L
UI090701-40	Iron	50 mg/L	2 mL	1000 mL	100 ug/L
UI090701-40	Lead	5 mg/L	2 mL	1000 mL	10 ug/L
UI090701-40	Magnesium	150 mg/L	2 mL	1000 mL	300 ug/L
UI090701-40	Manganese	5 mg/L	2 mL	1000 mL	10 ug/L
UI090701-40	Molybdenum	5 mg/L	2 mL	1000 mL	10 ug/L
UI090701-40	Nickel	2.5 mg/L	2 mL	1000 mL	5 ug/L
UI090701-40	Phosphorous	75 mg/L	2 mL	1000 mL	150 ug/L
UI090701-40	Potassium	75 mg/L	2 mL	1000 mL	150 ug/L

Standard Logbook

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI090701-40	Selenium	15 mg/L	2 mL	1000 mL	15 ug/L
UI090701-40	Silicon	50 mg/L	2 mL	1000 mL	100 ug/L
UI090701-40	Silver	2.5 mg/L	2 mL	1000 mL	5 ug/L
UI090701-40	Sodium	150 mg/L	2 mL	1000 mL	150 ug/L
UI090701-40	Strontium	2.5 mg/L	2 mL	1000 mL	5 ug/L
UI090701-40	Sulfur	50 mg/L	2 mL	1000 mL	100 ug/L
UI090701-40	Thallium	10 mg/L	2 mL	1000 mL	20 ug/L
UI090701-40	Tin	5 mg/L	2 mL	1000 mL	10 ug/L
UI090701-40	Titanium	2.5 mg/L	2 mL	1000 mL	5 ug/L
UI090701-40	Uranium	25 mg/L	2 mL	1000 mL	50 ug/L
UI090701-40	Vanadium	2.5 mg/L	2 mL	1000 mL	5 ug/L
UI090701-40	Zinc	5 mg/L	2 mL	1000 mL	10 ug/L

Serial ID: WMS100323-04AB **Opened:** 23-MAR-10 **Balance Id :** 40245216
Name: ICPMS Cal Standard 10 **Received:** 23-MAR-10 **Pipet Id :** 3541598
Type: Working **Expires:** 24-MAR-10 **Solvent :** 2%HNO3/1%HCl - 1289731
Employee: Rose Jenkins
Supplier: GEL
Description: ICPMS Calibration Standard (10 ppb)
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
WMS100323-04B	Aluminum	10000 ug/l	5 mL	50 mL	1000 ug/l
WMS100323-04B	Antimony	100 ug/l	5 mL	50 mL	10 ug/l
WMS100323-04B	Arsenic	100 ug/l	5 mL	50 mL	10 ug/l
WMS100323-04B	Barium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100323-04B	Beryllium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100323-04B	Boron	200 ug/l	5 mL	50 mL	20 ug/l
WMS100323-04B	Cadmium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100323-04B	Calcium	10000 ug/l	5 mL	50 mL	1000 ug/l
WMS100323-04B	Chromium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100323-04B	Cobalt	100 ug/l	5 mL	50 mL	10 ug/l
WMS100323-04B	Copper	100 ug/l	5 mL	50 mL	10 ug/l
WMS100323-04B	Iron	10000 ug/l	5 mL	50 mL	1000 ug/l
WMS100323-04B	Lead	100 ug/l	5 mL	50 mL	10 ug/l
WMS100323-04B	Lithium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100323-04B	Magnesium	10000 ug/l	5 mL	50 mL	1000 ug/l
WMS100323-04B	Manganese	100 ug/l	5 mL	50 mL	10 ug/l
WMS100323-04B	Molybdenum	100 ug/l	5 mL	50 mL	10 ug/l
WMS100323-04B	Nickel	100 ug/l	5 mL	50 mL	10 ug/l
WMS100323-04B	Phosphorous	10000 ug/l	5 mL	50 mL	1000 ug/l
WMS100323-04B	Potassium	10000 ug/l	5 mL	50 mL	1000 ug/l
WMS100323-04B	Selenium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100323-04B	Silver	100 ug/l	5 mL	50 mL	10 ug/l
WMS100323-04B	Sodium	10000 ug/l	5 mL	50 mL	1000 ug/l

Standard Logbook

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
WMS100323-04B	Strontium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100323-04B	Thallium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100323-04B	Thorium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100323-04B	Tin	100 ug/l	5 mL	50 mL	10 ug/l
WMS100323-04B	Titanium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100323-04B	Tungsten	100 ug/L	5 mL	50 mL	10 ug/L
WMS100323-04B	Uranium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100323-04B	Vanadium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100323-04B	Zinc	100 ug/l	5 mL	50 mL	10 ug/l
WMS100323-04B	Zirconium	100 ug/l	5 mL	50 mL	10 ug/l

Serial ID: WMS100323-04B **Opened:** 23-MAR-10 **Amount :** 50 mL
Name: ICPMS Cal Standard 100 **Received:** 23-MAR-10 **Balance Id :** 40245216
Type: Working **Expires:** 24-MAR-10 **Pipet Id :** 1758088
Employee: Rose Jenkins **Solvent :** 2%HNO3/1%HCl- 1289731
Supplier: GEL
Description: ICPMS Calibration Standard (100 ppb)
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI090612-02	Tungsten	10 mg/L	.5 mL	50 mL	100 ug/L
UMS100226-01	Arsenic	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Barium	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Beryllium	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Boron	20 mg/L	.5	50 mL	200 ug/l
UMS100226-01	Cadmium	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Chromium	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Cobalt	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Copper	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Lead	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Lithium	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Manganese	10 mg/l	.5	50 mL	100 ug/l
UMS100226-01	Nickel	10 mg/l	.5	50 mL	100 ug/l
UMS100226-01	Selenium	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Silver	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Strontium	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Thallium	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Thorium	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Uranium	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Vanadium	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Zinc	10 mg/L	.5	50 mL	100 ug/l
UMS100226-02	Aluminum	1000 mg/L	.5	50 mL	10000 ug/l
UMS100226-02	Calcium	1000 mg/L	.5	50 mL	10000 ug/l
UMS100226-02	Iron	1000 mg/L	.5	50 mL	10000 ug/l
UMS100226-02	Magnesium	1000 mg/L	.5	50 mL	10000 ug/l

Standard Logbook

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UMS100226-02	Phosphorous	1000 mg/L	.5	50 mL	10000 ug/l
UMS100226-02	Potassium	1000 mg/L	.5	50 mL	10000 ug/l
UMS100226-02	Sodium	1000 mg/L	.5	50 mL	10000 ug/l
UMS100226-03	Antimony	10 mg/L	.5	50 mL	100 ug/l
UMS100226-03	Molybdenum	10 mg/L	.5	50 mL	100 ug/l
UMS100226-03	Tin	10 mg/L	.5	50 mL	100 ug/l
UMS100226-03	Titanium	10 mg/L	.5	50 mL	100 ug/l
UMS100226-03	Zirconium	10 mg/L	.5	50 mL	100 ug/l

Serial ID: WMS100323-05B **Opened:** 23-MAR-10 **Balance Id :** 40245216
Name: ICPMS ICV **Received:** 23-MAR-10 **Pipet Id :** 1758088
Type: Working **Expires:** 24-MAR-10 **Solvent :** 2%HNO3/1%HCl- 1289731
Employee: Rose Jenkins
Supplier: GEL
Description: ICPMS ICV
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI100317-06	Aluminum	2020 mg/L	.125 mL	50 mL	5050 ug/L
UI100317-06	Calcium	2000 mg/L	.125 mL	50 mL	5000 ug/L
UI100317-06	Iron	2000 mg/L	.125 mL	50 mL	5000 ug/L
UI100317-06	Magnesium	2000 mg/L	.125 mL	50 mL	5000 ug/L
UI100317-06	Phosphorous	2000 mg/L	.125 mL	50 mL	5000 ug/L
UI100317-06	Potassium	2000 mg/L	.125 mL	50 mL	5000 ug/L
UI100317-06	Sodium	2000 mg/L	.125 mL	50 mL	5000 ug/L
UI100317-07	Arsenic	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Barium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Beryllium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Boron	40 mg/L	.125 mL	50 mL	100 ug/L
UI100317-07	Cadmium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Chromium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Cobalt	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Copper	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Lead	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Lithium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Manganese	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Nickel	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Selenium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Strontium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Thallium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Thorium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Uranium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Vanadium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Zinc	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-08	Antimony	20 mg/L	.125 mL	50 mL	50 ug/L

Standard Logbook

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI100317-08	Molybdenum	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-08	Silver	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-08	Tin	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-08	Titanium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-08	Tungsten	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-08	Zirconium	20 mg/L	.125 mL	50 mL	50 ug/L

Serial ID: WMS100323-06B **Opened:** 23-MAR-10 **Balance Id :** 40245216
Name: ICPMS CRDL **Received:** 23-MAR-10 **Pipet Id :** 3820544
Type: Working **Expires:** 24-MAR-10 **Solvent :** 2%HNO3/1%HCl - 1289731
Employee: Rose Jenkins **Verified:** 06-MAR-10
Supplier: GEL
Description: ICPMS CRDL
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI090701-09	Aluminum	15 mg/L	.05 mL	50 mL	15 ug/L
UI090701-09	Arsenic	5 mg/L	.05 mL	50 mL	5 ug/L
UI090701-09	Barium	2 mg/L	.05 mL	50 mL	2 ug/L
UI090701-09	Beryllium	.5 mg/L	.05 mL	50 mL	.5 ug/L
UI090701-09	Boron	15 mg/L	.05 mL	50 mL	15 ug/L
UI090701-09	Cadmium	1 mg/L	.05 mL	50 mL	1 ug/L
UI090701-09	Calcium	100 mg/L	.05 mL	50 mL	100 ug/L
UI090701-09	Chromium	3 mg/L	.05 mL	50 mL	3 ug/L
UI090701-09	Cobalt	1 mg/L	.05 mL	50 mL	1 ug/L
UI090701-09	Copper	1 mg/L	.05 mL	50 mL	1 ug/L
UI090701-09	Iron	25 mg/L	.05 mL	50 mL	25 ug/L
UI090701-09	Lead	2 mg/L	.05 mL	50 mL	2 ug/L
UI090701-09	Lithium	10 mg/L	.05 mL	50 mL	10 ug/L
UI090701-09	Magnesium	15 mg/L	.05 mL	50 mL	15 ug/L
UI090701-09	Manganese	5 mg/L	.05 mL	50 mL	5 ug/L
UI090701-09	Nickel	2 mg/L	.05 mL	50 mL	2 ug/L
UI090701-09	Phosphorous	50 mg/L	.05 mL	50 mL	50 ug/L
UI090701-09	Potassium	300 mg/L	.05 mL	50 mL	300 ug/L
UI090701-09	Selenium	5 mg/L	.05 mL	50 mL	5 ug/L
UI090701-09	Sodium	250 mg/L	.05 mL	50 mL	250 ug/L
UI090701-09	Strontium	10 mg/L	.05 mL	50 mL	10 ug/L
UI090701-09	Thallium	1 mg/L	.05 mL	50 mL	1 ug/L
UI090701-09	Thorium	1 mg/L	.05 mL	50 mL	1 ug/L
UI090701-09	Uranium	.2 mg/L	.05 mL	50 mL	.2 ug/L
UI090701-09	Vanadium	10 mg/L	.05 mL	50 mL	10 ug/L
UI090701-09	Zinc	10 mg/L	.05 mL	50 mL	10 ug/L
UI090701-10	Antimony	2 mg/L	.05 mL	50 mL	2 ug/L
UI090701-10	Molybdenum	.5 mg/L	.05 mL	50 mL	.5 ug/L
UI090701-10	Silver	1 mg/L	.05 mL	50 mL	1 ug/L

Standard Logbook

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI090701-10	Tin	2 mg/L	.05 mL	50 mL	5 ug/L
UI090701-10	Titanium	10 mg/L	.05 mL	50 mL	10 ug/L
UI090701-10	Tungsten	5 mg/L	.05 mL	50 mL	5 ug/L
UI090701-10	Zirconium	2 mg/L	.05 mL	50 mL	2 ug/L

Serial ID: WMS100323-07B **Opened:** 23-MAR-10 **Balance Id :** 40245216
Name: ICPMS ICSA **Received:** 23-MAR-10 **Lot Number :** 1010773
Type: Working **Expires:** 24-MAR-10 **Pipet Id :** 3541598
Employee: Rose Jenkins **Solvent :** 2%HNO3/1%HCl - 1289731
Supplier: GEL
Description: ICPMS ICSA
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI100318-11	Aluminum	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Calcium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Chloride	10000 mg/L	5 mL	50 mL	1000000 ug/L
UI100318-11	Iron	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Magnesium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Molybdenum	20 mg/L	5 mL	50 mL	2000 ug/L
UI100318-11	Phosphorous	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Potassium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Sodium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Sulfur	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Titanium	20 mg/L	5 mL	50 mL	2000 ug/L

Serial ID: WMS100323-08B **Opened:** 23-MAR-10 **Balance Id :** 40245216
Name: ICPMS ICSAB **Received:** 23-MAR-10 **Pipet Id :** 3541598/1758088
Type: Working **Expires:** 24-MAR-10 **Solvent :** 2%HNO3/1%HCl- 1289731
Employee: Rose Jenkins
Supplier: GEL
Description: ICPMS ICSAB
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI091217-12	Arsenic	2 mg/L	.5 mL	50 mL	20 ug/L
UI091217-12	Barium	2 mg/L	.5 mL	50 mL	20 ug/L
UI091217-12	Beryllium	2 mg/L	.5 mL	50 mL	20 ug/L
UI091217-12	Boron	2 mg/L	.5 mL	50 mL	20 ug/L
UI091217-12	Cadmium	2 mg/L	.5 mL	50 mL	20.2 ug/L
UI091217-12	Chromium	2 mg/L	.5 mL	50 mL	22.2 ug/L
UI091217-12	Cobalt	2 mg/L	.5 mL	50 mL	20.4 ug/L
UI091217-12	Copper	2 mg/L	.5 mL	50 mL	23.4 ug/L
UI091217-12	Lead	2 mg/L	.5 mL	50 mL	20 ug/L
UI091217-12	Lithium	2 mg/L	.5 mL	50 mL	20 ug/L

Standard Logbook

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI091217-12	Manganese	2 mg/L	.5 mL	50 mL	22.7 ug/L
UI091217-12	Nickel	2 mg/L	.5 mL	50 mL	22.4 ug/L
UI091217-12	Selenium	2 mg/L	.5 mL	50 mL	20 ug/L
UI091217-12	Strontium	2 mg/L	.5 mL	50 mL	20 ug/L
UI091217-12	Thallium	2 mg/L	.5 mL	50 mL	20 ug/L
UI091217-12	Thorium	2 mg/L	.5 mL	50 mL	20 ug/L
UI091217-12	Uranium	2 mg/L	.5 mL	50 mL	20 ug/L
UI091217-12	Vanadium	2 mg/L	.5 mL	50 mL	20 ug/L
UI091217-12	Zinc	2 mg/L	.5 mL	50 mL	27 ug/L
UI091217-13	Antimony	2 mg/L	.5 mL	50 mL	20.5 ug/L
UI091217-13	Silver	2 mg/L	.5 mL	50 mL	20 ug/L
UI091217-13	Tin	2 mg/L	.5 mL	50 mL	20 ug/L
UI091217-13	Tungsten	2 mg/L	.5 mL	50 mL	20 ug/L
UI091217-13	Zirconium	2 mg/L	.5 mL	50 mL	20 ug/L
UI100318-11	Aluminum	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Calcium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Chloride	10000 mg/L	5 mL	50 mL	1000000 ug/L
UI100318-11	Iron	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Magnesium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Molybdenum	20 mg/L	5 mL	50 mL	2000 ug/L
UI100318-11	Phosphorous	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Potassium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Sodium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Sulfur	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Titanium	20 mg/L	5 mL	50 mL	2000 ug/L

Serial ID: WMS100325-04AB **Opened:** 25-MAR-10 **Balance Id :** 40245216
Name: ICPMS Cal Standard 10 **Received:** 25-MAR-10 **Pipet Id :** 3541598
Type: Working **Expires:** 26-MAR-10 **Solvent :** 2%HNO3/1%HCl - 1289731
Employee: Rose Jenkins
Supplier: GEL
Description: ICPMS Calibration Standard (10 ppb)
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
WMS100325-04B	Aluminum	10000 ug/l	5 mL	50 mL	1000 ug/l
WMS100325-04B	Antimony	100 ug/l	5 mL	50 mL	10 ug/l
WMS100325-04B	Arsenic	100 ug/l	5 mL	50 mL	10 ug/l
WMS100325-04B	Barium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100325-04B	Beryllium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100325-04B	Boron	200 ug/l	5 mL	50 mL	20 ug/l
WMS100325-04B	Cadmium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100325-04B	Calcium	10000 ug/l	5 mL	50 mL	1000 ug/l
WMS100325-04B	Chromium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100325-04B	Cobalt	100 ug/l	5 mL	50 mL	10 ug/l

Standard Logbook

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
WMS100325-04B	Copper	100 ug/l	5 mL	50 mL	10 ug/l
WMS100325-04B	Iron	10000 ug/l	5 mL	50 mL	1000 ug/l
WMS100325-04B	Lead	100 ug/l	5 mL	50 mL	10 ug/l
WMS100325-04B	Lithium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100325-04B	Magnesium	10000 ug/l	5 mL	50 mL	1000 ug/l
WMS100325-04B	Manganese	100 ug/l	5 mL	50 mL	10 ug/l
WMS100325-04B	Molybdenum	100 ug/l	5 mL	50 mL	10 ug/l
WMS100325-04B	Nickel	100 ug/l	5 mL	50 mL	10 ug/l
WMS100325-04B	Phosphorous	10000 ug/l	5 mL	50 mL	1000 ug/l
WMS100325-04B	Potassium	10000 ug/l	5 mL	50 mL	1000 ug/l
WMS100325-04B	Selenium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100325-04B	Silver	100 ug/l	5 mL	50 mL	10 ug/l
WMS100325-04B	Sodium	10000 ug/l	5 mL	50 mL	1000 ug/l
WMS100325-04B	Strontium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100325-04B	Thallium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100325-04B	Thorium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100325-04B	Tin	100 ug/l	5 mL	50 mL	10 ug/l
WMS100325-04B	Titanium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100325-04B	Tungsten	100 ug/L	5 mL	50 mL	10 ug/L
WMS100325-04B	Uranium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100325-04B	Vanadium	100 ug/l	5 mL	50 mL	10 ug/l
WMS100325-04B	Zinc	100 ug/l	5 mL	50 mL	10 ug/l
WMS100325-04B	Zirconium	100 ug/l	5 mL	50 mL	10 ug/l

Serial ID: WMS100325-04B Opened: 25-MAR-10 Amount : 50 mL
 Name: ICPMS Cal Standard 100 Received: 25-MAR-10 Balance Id : 40245216
 Type: Working Expires: 26-MAR-10 Pipet Id : 1758088
 Employee: Rose Jenkins Solvent : 2%HNO3/1%HCl- 1289731
 Supplier: GEL
 Description: ICPMS Calibration Standard (100 ppb)
 Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI090612-02	Tungsten	10 mg/L	.5 mL	50 mL	100 ug/L
UMS100226-01	Arsenic	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Barium	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Beryllium	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Boron	20 mg/L	.5	50 mL	200 ug/l
UMS100226-01	Cadmium	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Chromium	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Cobalt	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Copper	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Lead	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Lithium	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Manganese	10 mg/L	.5	50 mL	100 ug/l

Standard Logbook

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UMS100226-01	Nickel	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Selenium	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Silver	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Strontium	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Thallium	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Thorium	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Uranium	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Vanadium	10 mg/L	.5	50 mL	100 ug/l
UMS100226-01	Zinc	10 mg/L	.5	50 mL	100 ug/l
UMS100226-02	Aluminum	1000 mg/L	.5	50 mL	10000 ug/l
UMS100226-02	Calcium	1000 mg/L	.5	50 mL	10000 ug/l
UMS100226-02	Iron	1000 mg/L	.5	50 mL	10000 ug/l
UMS100226-02	Magnesium	1000 mg/L	.5	50 mL	10000 ug/l
UMS100226-02	Phosphorous	1000 mg/L	.5	50 mL	10000 ug/l
UMS100226-02	Potassium	1000 mg/L	.5	50 mL	10000 ug/l
UMS100226-02	Sodium	1000 mg/L	.5	50 mL	10000 ug/l
UMS100226-03	Antimony	10 mg/L	.5	50 mL	100 ug/l
UMS100226-03	Molybdenum	10 mg/L	.5	50 mL	100 ug/l
UMS100226-03	Tin	10 mg/L	.5	50 mL	100 ug/l
UMS100226-03	Titanium	10 mg/L	.5	50 mL	100 ug/l
UMS100226-03	Zirconium	10 mg/L	.5	50 mL	100 ug/l

Serial ID: WMS100325-05B **Opened:** 25-MAR-10 **Balance Id :** 40245216
Name: ICPMS ICV **Received:** 25-MAR-10 **Pipet Id :** 1758088
Type: Working **Expires:** 26-MAR-10 **Solvent :** 2%HNO3/1%HCl- 1289731
Employee: Rose Jenkins
Supplier: GEL
Description: ICPMS ICV
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI100317-06	Aluminum	2020 mg/L	.125 mL	50 mL	5050 ug/L
UI100317-06	Calcium	2000 mg/L	.125 mL	50 mL	5000 ug/L
UI100317-06	Iron	2000 mg/L	.125 mL	50 mL	5000 ug/L
UI100317-06	Magnesium	2000 mg/L	.125 mL	50 mL	5000 ug/L
UI100317-06	Phosphorous	2000 mg/L	.125 mL	50 mL	5000 ug/L
UI100317-06	Potassium	2000 mg/L	.125 mL	50 mL	5000 ug/L
UI100317-06	Sodium	2000 mg/L	.125 mL	50 mL	5000 ug/L
UI100317-07	Arsenic	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Barium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Beryllium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Boron	40 mg/L	.125 mL	50 mL	100 ug/L
UI100317-07	Cadmium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Chromium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Cobalt	20 mg/L	.125 mL	50 mL	50 ug/L

Standard Logbook

Parent Material	Analyte	Parent Conc.	Allquot	Final Vol.	Final Conc.
UI100317-07	Copper	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Lead	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Lithium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Manganese	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Nickel	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Selenium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Strontium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Thallium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Thorium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Uranium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Vanadium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-07	Zinc	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-08	Antimony	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-08	Molybdenum	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-08	Silver	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-08	Tin	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-08	Titanium	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-08	Tungsten	20 mg/L	.125 mL	50 mL	50 ug/L
UI100317-08	Zirconium	20 mg/L	.125 mL	50 mL	50 ug/L

Serial ID: WMS100325-06B **Opened:** 25-MAR-10 **Balance Id :** 40245216
Name: ICPMS CRDL **Received:** 25-MAR-10 **Pipet Id :** 3820544
Type: Working **Expires:** 26-MAR-10 **Solvent :** 2%HNO3/1%HCl - 1289731
Employee: Rose Jenkins **Verified:** 06-MAR-10
Supplier: GEL
Description: ICPMS CRDL
Comments: None

Parent Material	Analyte	Parent Conc.	Allquot	Final Vol.	Final Conc.
UI090701-09	Aluminum	15 mg/L	.05 mL	50 mL	15 ug/L
UI090701-09	Arsenic	5 mg/L	.05 mL	50 mL	5 ug/L
UI090701-09	Barium	2 mg/L	.05 mL	50 mL	2 ug/L
UI090701-09	Beryllium	.5 mg/L	.05 mL	50 mL	.5 ug/L
UI090701-09	Boron	15 mg/L	.05 mL	50 mL	15 ug/L
UI090701-09	Cadmium	1 mg/L	.05 mL	50 mL	1 ug/L
UI090701-09	Calcium	100 mg/L	.05 mL	50 mL	100 ug/L
UI090701-09	Chromium	3 mg/L	.05 mL	50 mL	3 ug/L
UI090701-09	Cobalt	1 mg/L	.05 mL	50 mL	1 ug/L
UI090701-09	Copper	1 mg/L	.05 mL	50 mL	1 ug/L
UI090701-09	Iron	25 mg/L	.05 mL	50 mL	25 ug/L
UI090701-09	Lead	2 mg/L	.05 mL	50 mL	2 ug/L
UI090701-09	Lithium	10 mg/L	.05 mL	50 mL	10 ug/L
UI090701-09	Magnesium	15 mg/L	.05 mL	50 mL	15 ug/L
UI090701-09	Manganese	5 mg/L	.05 mL	50 mL	5 ug/L
UI090701-09	Nickel	2 mg/L	.05 mL	50 mL	2 ug/L

Standard Logbook

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI090701-09	Phosphorous	50 mg/L	.05 mL	50 mL	50 ug/L
UI090701-09	Potassium	300 mg/L	.05 mL	50 mL	300 ug/L
UI090701-09	Selenium	5 mg/L	.05 mL	50 mL	5 ug/L
UI090701-09	Sodium	250 mg/L	.05 mL	50 mL	250 ug/L
UI090701-09	Strontium	10 mg/L	.05 mL	50 mL	10 ug/L
UI090701-09	Thallium	1 mg/L	.05 mL	50 mL	1 ug/L
UI090701-09	Thorium	1 mg/L	.05 mL	50 mL	1 ug/L
UI090701-09	Uranium	.2 mg/L	.05 mL	50 mL	.2 ug/L
UI090701-09	Vanadium	10 mg/L	.05 mL	50 mL	10 ug/L
UI090701-09	Zinc	10 mg/L	.05 mL	50 mL	10 ug/L
UI090701-10	Antimony	2 mg/L	.05 mL	50 mL	2 ug/L
UI090701-10	Molybdenum	.5 mg/L	.05 mL	50 mL	.5 ug/L
UI090701-10	Silver	1 mg/L	.05 mL	50 mL	1 ug/L
UI090701-10	Tin	2 mg/L	.05 mL	50 mL	5 ug/L
UI090701-10	Titanium	10 mg/L	.05 mL	50 mL	10 ug/L
UI090701-10	Tungsten	5 mg/L	.05 mL	50 mL	5 ug/L
UI090701-10	Zirconium	2 mg/L	.05 mL	50 mL	2 ug/L

Serial ID: WMS100325-07B **Opened:** 25-MAR-10 **Balance Id :** 40245216
Name: ICPMS ICSA **Received:** 25-MAR-10 **Lot Number :** 1010773
Type: Working **Expires:** 26-MAR-10 **Pipet Id :** 3541598
Employee: Rose Jenkins **Solvent :** 2%HNO3/1%HCl - 1289731
Supplier: GEL
Description: ICPMS ICSA
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
UI100318-11	Aluminum	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Calcium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Chloride	10000 mg/L	5 mL	50 mL	1000000 ug/L
UI100318-11	Iron	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Magnesium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Molybdenum	20 mg/L	5 mL	50 mL	2000 ug/L
UI100318-11	Phosphorous	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Potassium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Sodium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Sulfur	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Titanium	20 mg/L	5 mL	50 mL	2000 ug/L

Serial ID: WMS100325-08B **Opened:** 25-MAR-10 **Balance Id :** 40245216
Name: ICPMS ICSAB **Received:** 25-MAR-10 **Pipet Id :** 3541598/1758088
Type: Working **Expires:** 26-MAR-10 **Solvent :** 2%HNO3/1%HCl- 1289731
Employee: Rose Jenkins
Supplier: GEL
Description: ICPMS ICSAB

Standard Logbook

Comments: None

Parent Material	Analyte	Parent Conc.	Alliquot	Final Vol.	Final Conc.
UI091217-12	Arsenic	2 mg/L	.5 mL	50 mL	20 ug/L
UI091217-12	Barium	2 mg/L	.5 mL	50 mL	20 ug/L
UI091217-12	Beryllium	2 mg/L	.5 mL	50 mL	20 ug/L
UI091217-12	Boron	2 mg/L	.5 mL	50 mL	20 ug/L
UI091217-12	Cadmium	2 mg/L	.5 mL	50 mL	20.2 ug/L
UI091217-12	Chromium	2 mg/L	.5 mL	50 mL	22.2 ug/L
UI091217-12	Cobalt	2 mg/L	.5 mL	50 mL	20.4 ug/L
UI091217-12	Copper	2 mg/L	.5 mL	50 mL	23.4 ug/L
UI091217-12	Lead	2 mg/L	.5 mL	50 mL	20 ug/L
UI091217-12	Lithium	2 mg/L	.5 mL	50 mL	20 ug/L
UI091217-12	Manganese	2 mg/L	.5 mL	50 mL	22.7 ug/L
UI091217-12	Nickel	2 mg/L	.5 mL	50 mL	22.4 ug/L
UI091217-12	Selenium	2 mg/L	.5 mL	50 mL	20 ug/L
UI091217-12	Strontium	2 mg/L	.5 mL	50 mL	20 ug/L
UI091217-12	Thallium	2 mg/L	.5 mL	50 mL	20 ug/L
UI091217-12	Thorium	2 mg/L	.5 mL	50 mL	20 ug/L
UI091217-12	Uranium	2 mg/L	.5 mL	50 mL	20 ug/L
UI091217-12	Vanadium	2 mg/L	.5 mL	50 mL	20 ug/L
UI091217-12	Zinc	2 mg/L	.5 mL	50 mL	27 ug/L
UI091217-13	Antimony	2 mg/L	.5 mL	50 mL	20.5 ug/L
UI091217-13	Silver	2 mg/L	.5 mL	50 mL	20 ug/L
UI091217-13	Tin	2 mg/L	.5 mL	50 mL	20 ug/L
UI091217-13	Tungsten	2 mg/L	.5 mL	50 mL	20 ug/L
UI091217-13	Zirconium	2 mg/L	.5 mL	50 mL	20 ug/L
UI100318-11	Aluminum	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Calcium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Chloride	10000 mg/L	5 mL	50 mL	1000000 ug/L
UI100318-11	Iron	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Magnesium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Molybdenum	20 mg/L	5 mL	50 mL	2000 ug/L
UI100318-11	Phosphorous	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Potassium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Sodium	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Sulfur	1000 mg/L	5 mL	50 mL	100000 ug/L
UI100318-11	Titanium	20 mg/L	5 mL	50 mL	2000 ug/L

Serial ID: 1100721TCLP Opened: 16-APR-09 Lot Number : H02026 L
 Name: I-HNO3 Received: 02-APR-09
 Type: Reagent/Solvent Expires: 02-APR-10
 Employee: Clifford Postell
 Supplier: BAKER
 Description: Nitric Acid CONC.
 Comments: None

Standard Logbook

Serial ID: 1156689-A **Opened:** 20-JUL-09 **Lot Number :** 41226920
Name: B-KMnO4(VWR)-MER **Received:** 20-JUL-09
Type: Reagent/Solvent **Expires:** 20-JUL-10
Employee: Tara Griffin **Verified:** 07-AUG-07
Supplier: VWR
Description: Potassium Permanganate
Comments: None

Serial ID: 1228372-A **Opened:** 12-NOV-09 **Lot Number :** 49215936
Name: B-NH2OH.HCl-MER **Received:** 12-NOV-09
Type: Reagent/Solvent **Expires:** 12-NOV-10
Employee: Tara Griffin
Supplier: Fisher Scientific
Description: Hydroxylamine Hydrochloride
Comments: None

Serial ID: 1250038-02 **Opened:** 04-JAN-10 **Lot Number :** ZU74081198 mL
Name: B-H2O2 **Received:** 04-JAN-10
Type: Reagent/Solvent **Expires:** 04-JAN-11
Employee: Bryan Davis
Supplier: EM SCIENCE
Description: Hydrogen Peroxide 30%
Comments: None

Serial ID: 1255532-C **Opened:** 15-JAN-10 **Balance Id :** BAL-002
Name: B-NaCl.NH2OH.HCl-MER **Received:** 15-JAN-10
Type: Reagent/Solvent **Expires:** 15-JUL-10
Employee: Tara Griffin
Supplier: GEL
Description: Hg reducing agent
Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
1228372-A	B-NH2OH.HCl-MER	N/A	120 g	1000 mL	N/A

Serial ID: 1274391-1 **Opened:** 24-FEB-10 **Instrument Id :** MERCURY
Name: B-HNO3-MER **Received:** 24-FEB-10 **Lot Number :** H44025
Type: Reagent/Solvent **Expires:** 24-FEB-11
Employee: Tara Griffin
Supplier: Mallinckrodt Chemicals
Description: NITRIC ACID
Comments: None

Standard Logbook

Serial ID: 1277235-A Opened: 01-MAR-10 Lot Number : J02039
 Name: B-HCl-MER Received: 01-MAR-10
 Type: Reagent/Solvent Expires: 01-MAR-11
 Employee: Tara Griffin
 Supplier: J T Baker
 Description: Hydrochloric Acid Conc.
 Comments: None

Serial ID: 1277238-C Opened: 01-MAR-10 Balance Id : BAL-002
 Name: B-KMnO4-MER Received: 01-MAR-10
 Type: Reagent/Solvent Expires: 20-JUL-10
 Employee: Tara Griffin
 Supplier: GEL
 Description: 5% KMnO4 solution
 Comments: None

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
1156689-A	B-KMnO4(VWR)-MER	Crystals	50 g	1000 mL	3%

Serial ID: 1277916 Opened: 02-MAR-10 Lot Number : J02039
 Name: I-HCL Received: 02-MAR-10 Preservative Id : 5 none
 Type: Reagent/Solvent Expires: 02-MAR-11
 Employee: Francena Armstrong
 Supplier: J.T. BAKER
 Description: HYDROCHLORIC ACID
 Comments: None

Serial ID: 1277919 Opened: 02-MAR-10 Lot Number : J 04043 L
 Name: I-HNO3 Received: 02-MAR-10
 Type: Reagent/Solvent Expires: 02-MAR-11
 Employee: Francena Armstrong
 Supplier: BAKER
 Description: Nitric Acid CONC.
 Comments: None

Serial ID: 1289731 Opened: 22-MAR-10 Solvent : Type I Water
 Name: B-2%HNO3/1%HCl-ICPMS Received: 22-MAR-10
 Type: Reagent/Solvent Expires: 29-MAR-10
 Employee: Paul Boyd
 Supplier: GEL
 Description: 2%HNO3/1%HCl Solution (Type I Water)
 Comments: None

Standard Logbook

Parent Material	Analyte	Parent Conc.	Aliquot	Final Vol.	Final Conc.
1100721TCLP	I-HNO3	69.0-70.0	180 mL	9 l	N/A
1277916	I-HCL	36.5-38.0	90 mL	9 l	N/A

Serial ID: 1293083 Opened: 29-MAR-10 Amount : 20 L
Name: B-ICP-RINSE SOLN Received: 29-MAR-10 Lot Number : H04040+G34050
Type: Reagent/Solvent Expires: 04-APR-10 Solvent : 3%HCL+1%HNO3
Employee: Helen Camello
Supplier: GEL
Description: 3%HCL+1%HNO3 RINSE SOLN.
Comments: None

General Chemistry

Analysis

Case Narrative

**General Chemistry Narrative
Los Alamos National Laboratory (LANL)
SDG 10-2093**

Method/Analysis Information

Product: Cyanide, Total

Analytical Batch: 959217 **Method:** SW9012A Cyanide and Total

Prep Batch : 959216 **Method:** SSW846 9010B Prep

Sample Analysis

The following samples were analyzed using the analytical protocol as established in SW846 9012A:

Sample ID	Client ID
248117001	RE36-10-8458
1202057161	Method Blank (MB)
1202057162	248188001(RE11-10-1654) Sample Duplicate (DUP)
1202057163	248044005(CAPA-10-13085) Sample Duplicate (DUP)
1202057164	248188001(RE11-10-1654) Matrix Spike (MS)
1202057165	248044005(CAPA-10-13085) Matrix Spike (MS)
1202057166	248188001(RE11-10-1654) Matrix Spike Duplicate (MSD)
1202057167	248044005(CAPA-10-13085) Matrix Spike Duplicate (MSD)
1202057168	Laboratory Control Sample (LCS)

The samples in this SDG were analyzed on an "as received" basis.

SOP Reference

Procedure for preparation, analysis and reporting of analytical data are controlled by GEL Laboratories LLC as Standard Operating Procedure (SOP). The data discussed in this narrative has been analyzed in accordance with GL-GC-E-095 REV# 12.

Preparation/Analytical Method Verification

The SOP stated above has been prepared based on technical research and testing conducted by GEL Laboratories, LLC. and with guidance from the regulatory documents listed in this "Method/Analysis Information" section.

Calibration Information

The Flow Injection analysis was performed on a Lachat QuickChem FIA+ 8000 Series.

Initial Calibration

All initial calibration requirements have been met for this SDG.

Continuing Calibration Blanks

All continuing calibration blanks (CCBs) associated with reported data from this batch were within acceptance limits.

Calibration Verification Information (CCV)

All continuing calibration verification standards (CCVs) associated with reported data from this batch were within acceptance limits.

Y Intercept Rule

The absolute value of the intercept is less than 3 times the MDL.

Quality Control (QC) Information**Method Blank (MB) Statement**

The MB analyzed with this SDG met the acceptance criteria.

Laboratory Control Sample (LCS) Recovery

The LCS spike recovery met the acceptance limits.

Quality Control (QC) Designation

The following samples were selected for QC analysis: 248044005 (CAPA-10-13085) and 248188001 (RE11-10-1654).

Matrix Spike (MS)/Post Spike (PS) Recovery Statement

The MS/PS recoveries for this sample set were within the required acceptance limits.

Matrix Spike Duplicate (MSD) Recovery Statement

The MSD recoveries for this sample set were within the required acceptance limits.

MS/MSD Relative Percent Difference (RPD) Statement

The RPDs between the spike and spike duplicate met the acceptance limits.

Duplicate Relative Percent Difference (RPD) Statement

The values for the sample and duplicate are less than the Practical Quantitation Limit (PQL); therefore, the RPD is not applicable. 1202057163 (CAPA-10-13085).

Technical Information

GEL assigns holding times based on the date and time of sample collection. Those holding times expressed in hours are calculated in the AlphaLims system by hours. Those holding times expressed as days expire at midnight on the day of expiration.

Holding Times

All samples in this SDG met the specified holding time.

Sample Preservation/Integrity

All the samples from this sample group met the preservation and integrity requirements of the method.

Sample Dilutions

The samples in this SDG did not require dilutions.

Sample Re-analysis

The following sample was re-analyzed due to instrument failure: 1202057164 (RE11-10-1654).

Miscellaneous Information

Data Exception (DER) Documentation

A DER was not required for this SDG.

Additional Comments

Additional comments were not required for this SDG.

Electronic Packaging Comment

This data package was generated using an electronic data processing program referred to as virtual packaging. In an effort to increase quality and efficiency, the laboratory has developed systems to generate all data packages electronically. The following change from traditional packages should be noted:

Analyst/peer reviewer initials and dates are not present on the electronic data files. Presently, all initials and dates are present on the original raw data. These hard copies are temporarily stored in the laboratory. The data validator will always sign and date the case narrative. Data that are not generated electronically, such as hand written pages, will be scanned and inserted into the electronic package.

Method/Analysis Information

Product: Nitrate Nitrite by Cadmium Reduction

Analytical Batch: 959199

Method: EPA 353.2 Nitrogen and Nitrate/Nitrite

Sample Analysis

The following samples were analyzed using the analytical protocol as established in EPA 353.2:

Sample ID	Client ID
248117001	RE36-10-8458
1202057088	Method Blank (MB)
1202057090	248108001(RE15-10-8407) Sample Duplicate (DUP)
1202057093	248108001(RE15-10-8407) Post Spike (PS)
1202057095	Laboratory Control Sample (LCS)
1202059915	248044005(CAPA-10-13085) Sample Duplicate (DUP)
1202059916	248044005(CAPA-10-13085) Post Spike (PS)

The samples in this SDG were analyzed on an "as received" basis.

SOP Reference

Procedure for preparation, analysis and reporting of analytical data are controlled by GEL Laboratories LLC as Standard Operating Procedure (SOP). The data discussed in this narrative has been analyzed in accordance with GL-GC-E-128 REV# 5.

Preparation/Analytical Method Verification

The SOP stated above has been prepared based on technical research and testing conducted by GEL Laboratories, LLC. and with guidance from the regulatory documents listed in this "Method/Analysis Information" section.

Calibration Information

The Nutrient analysis was performed on a Lachat QuickChem FIA+ 8500 Series.

Continuing Calibration Blanks

All continuing calibration blanks (CCBs) associated with reported data from this batch were within acceptance limits.

Y Intercept Rule

The absolute value of the intercept is less than 3 times the MDL.

Quality Control (QC) Information

Method Blank (MB) Statement

The MB analyzed with this SDG met the acceptance criteria.

Laboratory Control Sample (LCS) Recovery

The LCS spike recovery met the acceptance limits.

Quality Control (QC) Designation

The following samples were selected for QC analysis: 248044005 (CAPA-10-13085) and 248108001 (RE15-10-8407).

Matrix Spike (MS)/Post Spike (PS) Recovery Statement

The MS/PS recoveries for this sample set were within the required acceptance limits.

Duplicate Relative Percent Difference (RPD) Statement

The values for the sample and duplicate are less than the Practical Quantitation Limit (PQL); therefore, the RPD is not applicable. 1202057090 (RE15-10-8407).

Technical Information

GEL assigns holding times based on the date and time of sample collection. Those holding times expressed in hours are calculated in the AlphaLims system by hours. Those holding times expressed as days expire at midnight on the day of expiration.

Holding Times

All samples in this SDG met the specified holding time.

Sample Preservation/Integrity

All the samples from this sample group met the preservation and integrity requirements of the method.

Sample Dilutions

The following samples in this sample group were diluted due to matrix interference: 1202057090 (RE15-10-8407), 1202057093 (RE15-10-8407), 1202059915 (CAPA-10-13085), 1202059916 (CAPA-10-13085) and 248117001 (RE36-10-8458).

Sample Re-analysis

The samples in this SDG did not require re-analysis.

Miscellaneous Information

Data Exception (DER) Documentation

A DER was not required for this SDG.

Additional Comments

Additional comments were not required for this SDG.

Electronic Packaging Comment

This data package was generated using an electronic data processing program referred to as virtual packaging. In an effort to increase quality and efficiency, the laboratory has developed systems to generate all data packages electronically. The following change from traditional packages should be noted:

Analyst/peer reviewer initials and dates are not present on the electronic data files. Presently, all initials and dates are present on the original raw data. These hard copies are temporarily stored in the laboratory. The data validator will always sign and date the case narrative. Data that are not generated electronically, such as hand written pages, will be scanned and inserted into the electronic package.

Certification Statement

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless otherwise noted in the analytical case narrative.

Review Validation:

GEL requires all analytical data to be verified by a qualified data validator. In addition, all data designated for CLP or CLP-like packaging will receive a third level validation upon completion of the data package.

The following data validator verified the information presented in this case narrative:

Reviewer: _____

Nick A. Emme

Date: _____

3-23-10

Sample Data Summary

GEL LABORATORIES LLC

2040 Savage Road Charleston SC 29407 - (843) 556-8171 - www.gel.com

Certificate of Analysis Report for

LANL010 Los Alamos National Laboratory (72733-001-09)

Client SDG: 10-2093 GEL Work Order: 248117

The Qualifiers in this report are defined as follows:


- * Indicates that a quality control analyte recovery is outside of specified acceptance criteria.
- ** Indicates the analyte is a surrogate compound.

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless qualified on the Certificate of Analysis.

The designation ND, if present, appears in the result column when the analyte concentration is not detected above the detection limit.

This data report has been prepared and reviewed in accordance with GEL Laboratories LLC standard operating procedures. Please direct any questions to your Project Manager, Valerie Davis.

Reviewed by

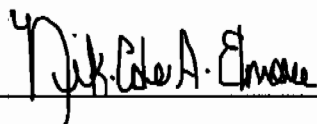

3-23-10

GEL LABORATORIES LLC

2040 Savage Road Charleston SC 29407 - (843) 556-8171 - www.gel.com

Certificate of Analysis

Company : Los Alamos National Laboratory
Address : PO Box 1663
TA-03, SM271, Drop Pt. 02U, Rm111
Los Alamos, New Mexico 87545
Contact: Ms. Joylene Valdez
Project: **LANL ER Project**

Report Date: March 23, 2010

Client SDG: 10-2093

Client Sample ID: RE36-10-8458
Sample ID: 248117001
Matrix: W
Collect Date: 22-FEB-10 12:00
Receive Date: 26-FEB-10
Collector: Client

Project: LANL01004
Client ID: LANL010

Parameter	Qualifier	Result	DL	RL	Units	DF	Analyst	Date	Time	Batch	Method
Flow Injection Analysis											
<i>SW9012A Cyanide, Total "As Received"</i>											
Cyanide, Total	U	ND	1.66	5.00	ug/L	1	AXC2	03/08/10	1512	959217	1
Nutrient Analysis											
<i>EPA 353.2 Nitrogen, Nitrate/Nitrite "As Received"</i>											
Nitrogen, Nitrate/Nitrite	U	ND	0.050	0.250	mg/L	5	AXH3	03/03/10	1229	959199	2

The following Prep Methods were performed

Method	Description	Analyst	Date	Time	Prep Batch
SW846 9010B Prep	SW846 9010B Prep	AXS5	03/08/10	1241	959216

The following Analytical Methods were performed

Method	Description	Analyst Comments
1	SW846 9012A	
2	EPA 353.2	

Quality Control Summary

GEL LABORATORIES LLC

2040 Savage Road Charleston, SC 29407 - (843) 556-8171 - www.gel.com

QC Summary

Report Date: March 23, 2010

Page 1 of 2

Los Alamos National Laboratory
PO Box 1663
TA-03, SM271, Drop Pt. 02U, Rm111
Los Alamos, New Mexico

Contact: Ms. Joylené Valdez

Workorder: 248117

Paramname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
Flow Injection Analysis											
Batch	959217										
QC1202057162 248188001 DUP											
Cyanide, Total		U	ND	U	ND	ug/L	N/A		AXC2	03/08/10	15:24
QC1202057163 248044005 DUP											
Cyanide, Total		U	ND	U	ND	ug/L	N/A			03/08/10	15:07
QC1202057168 LCS											
Cyanide, Total	50.0				49.3	ug/L	98.6	(90%-110%)		03/08/10	15:05
QC1202057161 MB											
Cyanide, Total			U		5.00	ug/L				03/08/10	15:05
QC1202057164 248188001 MS											
Cyanide, Total	100	U	ND		106	ug/L	106	(60%-144%)		03/08/10	15:37
QC1202057165 248044005 MS											
Cyanide, Total	100	U	ND		101	ug/L	101	(60%-144%)		03/08/10	15:08
QC1202057166 248188001 MSD											
Cyanide, Total	100	U	ND		110	ug/L	3.70	110 (0%-20%)		03/08/10	15:30
QC1202057167 248044005 MSD											
Cyanide, Total	100	U	ND		105	ug/L	3.88	105 (0%-20%)		03/08/10	15:09
Nutrient Analysis											
Batch	959199										
QC1202057090 248108001 DUP											
Nitrogen, Nitrate/Nitrite		U	ND	J	0.123	mg/L	200	(+/-0.500)	AXH3	03/03/10	12:45
QC1202059915 248044005 DUP											
Nitrogen, Nitrate/Nitrite		U	ND	U	ND	mg/L	N/A			03/03/10	12:06
QC1202057095 LCS											
Nitrogen, Nitrate/Nitrite	1.00				1.00	mg/L	100	(90%-110%)		03/03/10	11:44
QC1202057088 MB											
Nitrogen, Nitrate/Nitrite			J		0.0116	mg/L				03/03/10	11:43
QC1202057093 248108001 PS											
Nitrogen, Nitrate/Nitrite	1.00	U	ND		1.10	mg/L	109	(90%-110%)		03/03/10	12:47
QC1202059916 248044005 PS											
Nitrogen, Nitrate/Nitrite	1.00	U	ND		1.04	mg/L	103	(90%-110%)		03/03/10	12:12

Notes:

RER is calculated at the 95% confidence level (2-sigma).

The Qualifiers in this report are defined as follows:

- ** Analyte is a surrogate compound
- < Result is less than value reported
- > Result is greater than value reported
- A The TIC is a suspected aldol-condensation product
- B For General Chemistry and Organic analysis the target analyte was detected in the associated blank.
- C Analyte has been confirmed by GC/MS analysis
- D Results are reported from a diluted aliquot of the sample

GEL LABORATORIES LLC

2040 Savage Road Charleston, SC 29407 - (843) 556-8171 - www.gel.com

QC Summary

Workorder: 248117

Page 2 of 2

Parmname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
E	General Chemistry--	Concentration of the target analyte exceeds the instrument calibration range									
E	Metals--	%difference of sample and SD is >10%. Sample concentration must meet flagging criteria									
E	Organics--	Concentration of the target analyte exceeds the instrument calibration range									
F	Estimated Value										
H	Analytical holding time was exceeded										
J	Value is estimated										
M	Matrix Related Failure										
N	Organics--	Presumptive evidence based on mass spectral library search to make a tentative identification of the analyte (TIC). Quantitation is based on nearest internal standard response factor									
N/A	RPD or %Recovery limits do not apply.										
ND	Analyte concentration is not detected above the detection limit										
NJ	Consult Case Narrative, Data Summary package, or Project Manager concerning this qualifier										
P	Organics--	The concentrations between the primary and confirmation columns/detectors is >40% different. For HPLC, difference is also <70%									
R	Sample results are rejected										
U	Analyte was analyzed for, but not detected above the MDL, MDA, or LOD.										
X	Consult Case Narrative, Data Summary package, or Project Manager concerning this qualifier										
Y	QC Samples were not spiked with this compound										
Z	Paint Filter Test--	Particulates passed through the filter, however no free liquids were observed.									
^	RPD of sample and duplicate evaluated using +/-RL. Concentrations are <5X the RL. Qualifier Not Applicable for Radiochemistry.										
d	5-day BOD--	The 2:1 depletion requirement was not met for this sample									
h	Preparation or preservation holding time was exceeded										

N/A indicates that spike recovery limits do not apply when sample concentration exceeds spike conc. by a factor of 4 or more.

^ The Relative Percent Difference (RPD) obtained from the sample duplicate (DUP) is evaluated against the acceptance criteria when the sample is greater than five times (5X) the contract required detection limit (RL). In cases where either the sample or duplicate value is less than 5X the RL, a control limit of +/- the RL is used to evaluate the DUP result.

* Indicates that a Quality Control parameter was not within specifications.

For PS, PSD, and SDILT results, the values listed are the measured amounts, not final concentrations.

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless qualified on the QC Summary.

Instrument QC Data Summary

INITIAL AND CONTINUING CALIBRATION VERIFICATION

Report Run On: 23-MAR-2010 17:28

GEL Laboratories LLC

Contract: LANL01004

SDG #: 10-2093

Flow Injection Analysis

Method: SW846 9012A

Concentration Units:ug/L

Instrument: Lachat QuickChem FIA+ 8000 Series

Parmname: Cyanide, Total

Sample Type	Run Date	Data File	Result	Nominal	Recovery	Limits	Within Limits
ICV	08-MAR-2010 10:32:54	OM_3-8-2010_10-24-48	147	150	98	(90%-110%)	Yes
CCV	08-MAR-2010 15:01:26	OM_3-8-2010_14-58-05	103	100	103	(90%-110%)	Yes
CCV	08-MAR-2010 15:13:54	OM_3-8-2010_14-58-05	106	100	106	(90%-110%)	Yes
CCV	08-MAR-2010 15:26:19	OM_3-8-2010_14-58-05	109	100	109	(90%-110%)	Yes
CCV	08-MAR-2010 15:38:47	OM_3-8-2010_14-58-05	104	100	104	(90%-110%)	Yes

Sample Type	Run Date	Data File	Result	Limits	Within Limits
ICB	08-MAR-2010 10:34:44	OM_3-8-2010_10-24-48	-1.65	10	Yes
CCB	08-MAR-2010 15:03:15	OM_3-8-2010_14-58-05	-1.49	10	Yes
CCB	08-MAR-2010 15:15:44	OM_3-8-2010_14-58-05	-1.84	10	Yes
CCB	08-MAR-2010 15:28:11	OM_3-8-2010_14-58-05	-1.78	10	Yes
CCB	08-MAR-2010 15:40:39	OM_3-8-2010_14-58-05	-0.768	10	Yes

INITIAL AND CONTINUING CALIBRATION VERIFICATION

Report Run On: 23-MAR-2010 17:28

GEL Laboratories LLC

Contract: LANL01004

SDG #: 10-2093

Nutrient Analysis

Method: EPA 353.2

Concentration Units:mg/L

Instrument: Lachat Quickchem FIA+ 8500 Series

Parmname: Nitrogen, Nitrate/Nitrite

Sample Type	Run Date	Data File	Result	Nominal	Recovery	Limits	Within Limits
ICV	03-MAR-2010 10:40:18	OM_3-3-2010_10-30-06	0.983	1	98.3	(90%-110%)	Yes
CCV	03-MAR-2010 11:34:09	OM_3-3-2010_10-30-06	0.985	1	98.5	(90%-110%)	Yes
CCV	03-MAR-2010 11:50:55	OM_3-3-2010_10-30-06	0.968	1	96.8	(90%-110%)	Yes
CCV	03-MAR-2010 12:07:39	OM_3-3-2010_10-30-06	0.981	1	98.1	(90%-110%)	Yes
CCV	03-MAR-2010 12:24:25	OM_3-3-2010_10-30-06	1.01	1	101	(90%-110%)	Yes
CCV	03-MAR-2010 12:41:09	OM_3-3-2010_10-30-06	1.02	1	102	(90%-110%)	Yes
CCV	03-MAR-2010 12:57:55	OM_3-3-2010_10-30-06	1.01	1	101	(90%-110%)	Yes

Sample Type	Run Date	Data File	Result	Limits	Within Limits
ICB	03-MAR-2010 10:42:40	OM_3-3-2010_10-30-06	0.00396	0.05	Yes
CCB	03-MAR-2010 11:36:31	OM_3-3-2010_10-30-06	0.00385	0.05	Yes
CCB	03-MAR-2010 11:53:16	OM_3-3-2010_10-30-06	0.00438	0.05	Yes
CCB	03-MAR-2010 12:10:01	OM_3-3-2010_10-30-06	0.00404	0.05	Yes
CCB	03-MAR-2010 12:26:48	OM_3-3-2010_10-30-06	0.00458	0.05	Yes
CCB	03-MAR-2010 12:43:31	OM_3-3-2010_10-30-06	0.00556	0.05	Yes
CCB	03-MAR-2010 13:00:17	OM_3-3-2010_10-30-06	0.00422	0.05	Yes

Cyanide, Total

Prep Logbook

Cyanide Sample Distillation

Batch ID: 959216.0
Analyst: Alan Stanley
Method: SW846 9010B Prep EPA 335.4
Lab SOP: GL-GC-E-067 REV# 13
Instrument: Sartorius Balance B-001

Verified by:

Sample ID	Type	Sample Id	Description	Serial Number	Spike Amount	Spike Units
1202057168	LCS	1202057168	Secondary source standard for CN and phenol. Used to spike LCS, MS, ICV	URF1269274-02	.0125	mL
1202057164	MS	1202057164	Secondary source standard for CN and phenol. Used to spike LCS, MS, ICV	URF1269274-02	.025	mL
1202057165	MS	1202057165	Secondary source standard for CN and phenol. Used to spike LCS, MS, ICV	URF1269274-02	.025	mL
1202057166	MSD	1202057166	Secondary source standard for CN and phenol. Used to spike LCS, MS, ICV	URF1269274-02	.025	mL
1202057167	MSD	1202057167	Secondary source standard for CN and phenol. Used to spike LCS, MS, ICV	URF1269274-02	.025	mL

Sample ID	Run Date	Matrix	Initial Volume (mL)	Final Volume (mL)	Prep Factor (mL/mL)	pH Check
1202057161 MB	08-MAR-2010 12:41:00	Water	25	25	1	>12
1202057168 LCS	08-MAR-2010 12:41:00	Water	25	25	1	>12
248044005	08-MAR-2010 12:41:00	Ground Water	25	25	1	>12
1202057163 DUP (248044005)	08-MAR-2010 12:41:00	Ground Water	25	25	1	>12
1202057165 MS (248044005)	08-MAR-2010 12:41:00	Ground Water	25	25	1	>12
1202057167 MSD (248044005)	08-MAR-2010 12:41:00	Ground Water	25	25	1	>12
248044006	08-MAR-2010 12:41:00	Ground Water	25	25	1	>12
248108001	08-MAR-2010 12:41:00	Water	25	25	1	>12
248117001	08-MAR-2010 12:41:00	Water	25	25	1	>12
248127002	08-MAR-2010 12:41:00	Water	25	25	1	>12
248162001	08-MAR-2010 12:41:00	Water	25	25	1	>12
248162002	08-MAR-2010 12:41:00	Water	25	25	1	>12
248162003	08-MAR-2010 12:41:00	Water	25	25	1	>12
248162004	08-MAR-2010 12:41:00	Water	25	25	1	>12
248164002	08-MAR-2010 12:41:00	Ground Water	25	25	1	>12
248168006	08-MAR-2010 12:41:00	Water	25	25	1	>12
248169004	08-MAR-2010 12:41:00	Water	25	25	1	>12
248188001	08-MAR-2010 12:41:00	Water	25	25	1	>12
1202057162 DUP (248188001)	08-MAR-2010 12:41:00	Water	25	25	1	>12
1202057164 MS (248188001)	08-MAR-2010 12:41:00	Water	25	25	1	>12

Analytical Logbook version 1 11-04-2002

GEL Laboratories LLC

Prep Logbook

Batch ID: 959216.0
Analyst: Alan Stanley
Method: SW846 9010B Prep EPA 335.4
Lab SOP: GL-GC-E-067 REV# 13
Instrument: Sartorius Balance B-001

Type	Sample Id	Description	Serial Number	Spike Amount	Spike Units
LCS	1202057168	Secondary source standard for CN and phenol. Used to spike LCS, MS, ICV	URF1269274-02	.0125	mL
MS	1202057164	Secondary source standard for CN and phenol. Used to spike LCS, MS, ICV	URF1269274-02	.025	mL
MS	1202057165	Secondary source standard for CN and phenol. Used to spike LCS, MS, ICV	URF1269274-02	.025	mL
MSD	1202057166	Secondary source standard for CN and phenol. Used to spike LCS, MS, ICV	URF1269274-02	.025	mL
MSD	1202057167	Secondary source standard for CN and phenol. Used to spike LCS, MS, ICV	URF1269274-02	.025	mL

pH Check

Sample ID	Run Date	Matrix	Initial Volume (mL)	Final Volume (mL)	Prep Factor (mL/mL)	pH
1202057166 MSD (248188001)	08-MAR-2010 12:41:00	Water	25	25	1	>12
248199001	08-MAR-2010 12:41:00	Water	25	25	1	>12
248238001	08-MAR-2010 12:41:00	Water	25	25	1	>12
248238002	08-MAR-2010 12:41:00	Water	25	25	1	>12
248242001	08-MAR-2010 12:41:00	Water	25	25	1	>12
248245001	08-MAR-2010 12:41:00	Water	25	25	1	>12
248257001	08-MAR-2010 12:41:00	Water	25	25	1	>12
248257002	08-MAR-2010 12:41:00	Water	25	25	1	>12

Comments:

Reagent/Solvent Lot ID	Description	Amount
1260189-C	50% H2SO4 CN Prep	2.5 mL
1270661-C	Bismuth Nitrate Solution	1.25 mL
1270663-C	0.8N H3NO3S	1.25 mL
1270669-C	51% MgCl2 Soln	1 mL
1273851-C	0.25N Sodium Hydroxide Solution	25 mL
WCN100308-07	150 ppb CN Distilled ICV Standard	.0375 mL

This is runlog Lachat1

Sample ID	Batch	Dilution	Analyst	Runtime	Dataset
200 ppb		1	axc2	3/8/2010 10:25:45	OM_3-8-2010_10-24-48
150 ppb		1	axc2	3/8/2010 10:26:37	OM_3-8-2010_10-24-48
100 ppb		1	axc2	3/8/2010 10:27:29	OM_3-8-2010_10-24-48
50 ppb		1	axc2	3/8/2010 10:28:22	OM_3-8-2010_10-24-48
10 ppb		1	axc2	3/8/2010 10:29:15	OM_3-8-2010_10-24-48
CRDL 5.0 ppb		1	axc2	3/8/2010 10:30:09	OM_3-8-2010_10-24-48
ICAL-00		1	axc2	3/8/2010 10:31:03	OM_3-8-2010_10-24-48
ICV		1	axc2	3/8/2010 10:32:54	OM_3-8-2010_10-24-48
ICB		1	axc2	3/8/2010 10:34:44	OM_3-8-2010_10-24-48
CRDL		1	axc2	3/8/2010 10:36:34	OM_3-8-2010_10-24-48
1202054789	958168	1	axc2	3/8/2010 10:38:23	OM_3-8-2010_10-24-48
1202054796	958168	1	axc2	3/8/2010 10:39:17	OM_3-8-2010_10-24-48
248010001	958168	1	axc2	3/8/2010 10:40:10	OM_3-8-2010_10-24-48
1202054790	958168	1	axc2	3/8/2010 10:41:03	OM_3-8-2010_10-24-48
1202054792	958168	1	axc2	3/8/2010 10:41:56	OM_3-8-2010_10-24-48
1202054794	958168	1	axc2	3/8/2010 10:42:48	OM_3-8-2010_10-24-48
248010002	958168	1	axc2	3/8/2010 10:43:42	OM_3-8-2010_10-24-48
248019001	958168	1	axc2	3/8/2010 10:44:34	OM_3-8-2010_10-24-48
248019002	958168	1	axc2	3/8/2010 10:45:26	OM_3-8-2010_10-24-48
248023002	958168	1	axc2	3/8/2010 10:46:19	OM_3-8-2010_10-24-48
CCV		1	axc2	3/8/2010 10:47:11	OM_3-8-2010_10-24-48
CCB		1	axc2	3/8/2010 10:49:01	OM_3-8-2010_10-24-48
248024001	958168	1	axc2	3/8/2010 10:50:50	OM_3-8-2010_10-24-48
248024003	958168	1	axc2	3/8/2010 10:51:41	OM_3-8-2010_10-24-48
248044002	958168	1	axc2	3/8/2010 10:52:34	OM_3-8-2010_10-24-48
1202054791	958168	1	axc2	3/8/2010 10:53:25	OM_3-8-2010_10-24-48
1202054793	958168	1	axc2	3/8/2010 10:54:17	OM_3-8-2010_10-24-48
1202054795	958168	1	axc2	3/8/2010 10:55:10	OM_3-8-2010_10-24-48
248401005	958168	1	axc2	3/8/2010 10:56:04	OM_3-8-2010_10-24-48
248516001	958168	1	axc2	3/8/2010 10:56:58	OM_3-8-2010_10-24-48
248516002	958168	1	axc2	3/8/2010 10:57:51	OM_3-8-2010_10-24-48
248518001	958168	1	axc2	3/8/2010 10:58:44	OM_3-8-2010_10-24-48
CCV		1	axc2	3/8/2010 10:59:36	OM_3-8-2010_10-24-48
CCB		1	axc2	3/8/2010 11:01:27	OM_3-8-2010_10-24-48
248533001	958168	1	axc2	3/8/2010 11:03:16	OM_3-8-2010_10-24-48
248548001	958168	1	axc2	3/8/2010 11:04:09	OM_3-8-2010_10-24-48
248548003	958168	1	axc2	3/8/2010 11:05:01	OM_3-8-2010_10-24-48
248551001	958168	1	axc2	3/8/2010 11:05:54	OM_3-8-2010_10-24-48
248551002	958168	1	axc2	3/8/2010 11:06:46	OM_3-8-2010_10-24-48
248555002	958168	1	axc2	3/8/2010 11:07:39	OM_3-8-2010_10-24-48
1202059721	960271	1	axc2	3/8/2010 11:08:31	OM_3-8-2010_10-24-48
1202059731	960271	1	axc2	3/8/2010 11:09:23	OM_3-8-2010_10-24-48
248072001	960271	1	axc2	3/8/2010 11:10:15	OM_3-8-2010_10-24-48
1202059722	960271	1	axc2	3/8/2010 11:11:06	OM_3-8-2010_10-24-48
CCV		1	axc2	3/8/2010 11:11:59	OM_3-8-2010_10-24-48
CCB		1	axc2	3/8/2010 11:13:49	OM_3-8-2010_10-24-48
1202059725	960271	1	axc2	3/8/2010 11:15:40	OM_3-8-2010_10-24-48
1202059728	960271	1	axc2	3/8/2010 11:16:33	OM_3-8-2010_10-24-48
248072002	960271	1	axc2	3/8/2010 11:17:27	OM_3-8-2010_10-24-48
248072003	960271	1	axc2	3/8/2010 11:18:21	OM_3-8-2010_10-24-48
248097001	960271	1	axc2	3/8/2010 11:19:14	OM_3-8-2010_10-24-48
1202059724	960271	1	axc2	3/8/2010 11:20:07	OM_3-8-2010_10-24-48
1202059727	960271	1	axc2	3/8/2010 11:21:00	OM_3-8-2010_10-24-48
1202059730	960271	1	axc2	3/8/2010 11:21:53	OM_3-8-2010_10-24-48
248097002	960271	1	axc2	3/8/2010 11:22:47	OM_3-8-2010_10-24-48
248097003	960271	1	axc2	3/8/2010 11:23:38	OM_3-8-2010_10-24-48
CCV		1	axc2	3/8/2010 11:24:31	OM_3-8-2010_10-24-48
CCB		1	axc2	3/8/2010 11:26:21	OM_3-8-2010_10-24-48

248097004	960271	1	axc2	3/8/2010	11:28:09	OM_3-8-2010_10-24-48
248298001	960271	1	axc2	3/8/2010	11:29:02	OM_3-8-2010_10-24-48
248298002	960271	1	axc2	3/8/2010	11:29:53	OM_3-8-2010_10-24-48
248298003	960271	1	axc2	3/8/2010	11:30:46	OM_3-8-2010_10-24-48
248303001	960271	1	axc2	3/8/2010	11:31:38	OM_3-8-2010_10-24-48
248337001	960271	1	axc2	3/8/2010	11:32:32	OM_3-8-2010_10-24-48
248375001	960271	1	axc2	3/8/2010	11:33:26	OM_3-8-2010_10-24-48
248375002	960271	1	axc2	3/8/2010	11:34:19	OM_3-8-2010_10-24-48
248397001	960271	1	axc2	3/8/2010	11:35:14	OM_3-8-2010_10-24-48
248397002	960271	1	axc2	3/8/2010	11:36:06	OM_3-8-2010_10-24-48
CCV		1	axc2	3/8/2010	11:37:00	OM_3-8-2010_10-24-48
CCB		1	axc2	3/8/2010	11:38:51	OM_3-8-2010_10-24-48
248407001	960271	1	axc2	3/8/2010	11:40:39	OM_3-8-2010_10-24-48
1202059723	960271	1	axc2	3/8/2010	11:41:33	OM_3-8-2010_10-24-48
1202059726	960271	1	axc2	3/8/2010	11:42:26	OM_3-8-2010_10-24-48
1202059729	960271	1	axc2	3/8/2010	11:43:19	OM_3-8-2010_10-24-48
248419001	960271	1	axc2	3/8/2010	11:44:11	OM_3-8-2010_10-24-48
248419002	960271	1	axc2	3/8/2010	11:45:04	OM_3-8-2010_10-24-48
1202053300	957584	1	axc2	3/8/2010	11:45:57	OM_3-8-2010_10-24-48
1202053310	957584	1	axc2	3/8/2010	11:46:49	OM_3-8-2010_10-24-48
247829002	957584	1	axc2	3/8/2010	11:47:41	OM_3-8-2010_10-24-48
1202053302	957584	1	axc2	3/8/2010	11:48:33	OM_3-8-2010_10-24-48
CCV		1	axc2	3/8/2010	11:49:26	OM_3-8-2010_10-24-48
CCB		1	axc2	3/8/2010	11:51:15	OM_3-8-2010_10-24-48
1202053305	957584	1	axc2	3/8/2010	11:53:05	OM_3-8-2010_10-24-48
1202053308	957584	1	axc2	3/8/2010	11:54:00	OM_3-8-2010_10-24-48
247865010	957584	1	axc2	3/8/2010	11:54:55	OM_3-8-2010_10-24-48
247865012	957584	1	axc2	3/8/2010	11:55:48	OM_3-8-2010_10-24-48
1202053303	957584	1	axc2	3/8/2010	11:56:41	OM_3-8-2010_10-24-48
1202053306	957584	1	axc2	3/8/2010	11:57:35	OM_3-8-2010_10-24-48
1202053309	957584	1	axc2	3/8/2010	11:58:28	OM_3-8-2010_10-24-48
247865013	957584	1	axc2	3/8/2010	11:59:21	OM_3-8-2010_10-24-48
247865014	957584	1	axc2	3/8/2010	12:00:15	OM_3-8-2010_10-24-48
247865015	957584	1	axc2	3/8/2010	12:01:07	OM_3-8-2010_10-24-48
CCV		1	axc2	3/8/2010	12:02:00	OM_3-8-2010_10-24-48
CCB		1	axc2	3/8/2010	12:03:51	OM_3-8-2010_10-24-48
247865016	957584	1	axc2	3/8/2010	12:05:41	OM_3-8-2010_10-24-48
247865017	957584	1	axc2	3/8/2010	12:06:33	OM_3-8-2010_10-24-48
247865018	957584	1	axc2	3/8/2010	12:07:25	OM_3-8-2010_10-24-48
247865019	957584	1	axc2	3/8/2010	12:08:18	OM_3-8-2010_10-24-48
247865020	957584	1	axc2	3/8/2010	12:09:10	OM_3-8-2010_10-24-48
247866001	957584	1	axc2	3/8/2010	12:10:05	OM_3-8-2010_10-24-48
247919001	957584	1	axc2	3/8/2010	12:10:59	OM_3-8-2010_10-24-48
247919002	957584	1	axc2	3/8/2010	12:11:53	OM_3-8-2010_10-24-48
247922004	957584	1	axc2	3/8/2010	12:12:48	OM_3-8-2010_10-24-48
1202053301	957584	1	axc2	3/8/2010	12:13:41	OM_3-8-2010_10-24-48
CCV		1	axc2	3/8/2010	12:14:34	OM_3-8-2010_10-24-48
CCB		1	axc2	3/8/2010	12:16:24	OM_3-8-2010_10-24-48
1202053304	957584	1	axc2	3/8/2010	12:18:14	OM_3-8-2010_10-24-48
1202053307	957584	1	axc2	3/8/2010	12:19:07	OM_3-8-2010_10-24-48
248164004	957584	1	axc2	3/8/2010	12:20:01	OM_3-8-2010_10-24-48
248382002	957584	1	axc2	3/8/2010	12:20:54	OM_3-8-2010_10-24-48
248382003	957584	1	axc2	3/8/2010	12:21:47	OM_3-8-2010_10-24-48
248401002	957584	1	axc2	3/8/2010	12:22:40	OM_3-8-2010_10-24-48
248401004	957584	1	axc2	3/8/2010	12:23:33	OM_3-8-2010_10-24-48
CCV		1	axc2	3/8/2010	12:24:25	OM_3-8-2010_10-24-48
CCB		1	axc2	3/8/2010	12:26:15	OM_3-8-2010_10-24-48

Original Run Filename: OM_3-8-2010_10-24-48.OMN created 3/8/2010 10:24:48
 Original Run Author's Signature: [axc2]
 Current Run Filename: OM_3-8-2010_10-24-48.OMN last modified 3/8/2010 12:27:20
 Current Run Author's Signature: [axc2]
 Description: GL-GC-E-095 EPA 335.1, 335.3, 335.4, 9012A, CLP335.2-M
 Liquid LCS nominal 50 ug/L

Sample	Rep.	Cup No.	Channel 1		Detection Time	ADF	MDF	Description
			TCYANIDE	Area				
			Conc. (ug/L)	(Vs)				
WCN100308-01	1	S1	200	10.4	3/8/2010@10:25:45			200 ppb
WCN100308-02	1	S2	150	7.82	3/8/2010@10:26:37			150 ppb
WCN100308-03	1	S3	100	5.36	3/8/2010@10:27:29			100 ppb
WCN100308-04	1	S4	50.0	2.85	3/8/2010@10:28:22			50 ppb
WCN100308-05	1	S5	10.0	0.644	3/8/2010@10:29:15			10 ppb
WCN100308-06	1	S6	5.00	0.400	3/8/2010@10:30:09			CRDL 5.0 ppb
WCN100308-08	1	S7	0.00	-0.0189	3/8/2010@10:31:03			0.0 ppb
DQM Test: Minimum Correlation Coefficient								
			Result:	0.99976 > 0.99500				
			Message	Pass				
			Action	Continue				
WCN100308-07	1	S8	147	7.72	3/8/2010@10:32:54			ICV
		Known Conc:	150					
DQM Test: > + Percent Relative Difference								
			Result:	-2.1 < 10.0				
			Message	ICV Passed				
			Action	Continue				
DQM Test: < - Percent Relative Difference								
			Result:	-2.1 < 10.0				
			Message	ICV Passed				
			Action	Continue				
		Calibration:	Table/Fig. 1					
WCN100308-08	1	S7	-1.65	0.0363	3/8/2010@10:34:44			ICB/CCB
		Known Conc:	0.00					
DQM Test: > + Concentration Limit								
			Result:	-1.65 < 5.01				
			Message	ICB/CCB Passed				
			Action	Continue				
DQM Test: < - Concentration Limit								
			Result:	-1.65 > -5.01				
			Message	ICB/CCB Passed				
			Action	Continue				
WCN100308-06	1	S6	5.25	0.393	3/8/2010@10:36:34			CRDL
		Known Conc:	5.00					
DQM Test: > + Concentration Limit								
			Result:	5.25 < 7.50				
			Message	CRDL Passed				
			Action	Continue				
DQM Test: < - Concentration Limit								
			Result:	5.25 > 2.50				
			Message	Pass				
			Action	None				
1202054789 958168 MB	1	1	-1.83	0.0269	3/8/2010@10:38:23			
1202054796 LCS	1	2	50.4	2.73	3/8/2010@10:39:17			
248010001	1	3	-1.53	0.0427	3/8/2010@10:40:10			
1202054790 DUP	1	4	-1.69	0.0344	3/8/2010@10:41:03			
1202054792 MS	1	5	114	6.01	3/8/2010@10:41:56			
1202054794 MSD	1	6	111	5.86	3/8/2010@10:42:48			
248010002	1	7	-1.44	0.0471	3/8/2010@10:43:42			
248019001	1	8	-1.39	0.0498	3/8/2010@10:44:34			
248019002	1	9	-1.40	0.0491	3/8/2010@10:45:26			
248023002	1	10	-1.75	0.0312	3/8/2010@10:46:19			
WCN100308-03	1	S3	105	5.54	3/8/2010@10:47:11			CCV
		Known Conc:	100					
DQM Test: > + Percent Relative Difference								
			Result:	4.8 < 10.0				

Message			CCV Passed					
Action			Continue					
DQM Test: < - Percent Relative Difference								
Result:			4.8 < 10.0					
Message			CCV Passed					
Action			Continue					
WCN100308-08	1	S7	-1.67	0.0352	3/8/2010@10:49:01			CCB
Known Conc:			0.00					
DQM Test: > + Concentration Limit								
Result:			-1.67 < 5.00					
Message			CCB Passed					
Action			Continue					
DQM Test: < - Concentration Limit								
Result:			-1.67 > -5.00					
Message			CCB Passed					
Action			Continue					
248024001	1	11	-2.29	0.00319	3/8/2010@10:50:50			
248024003	1	12	-0.940	0.0730	3/8/2010@10:51:41			
248044002	1	13	-1.78	0.0297	3/8/2010@10:52:34			
1202054791 DUP	1	14	-1.89	0.0237	3/8/2010@10:53:25			
1202054793 MS	1	15	113	5.97	3/8/2010@10:54:17			
1202054795 MSD	1	16	94.5	5.01	3/8/2010@10:55:10			
248401005	1	17	-2.36	-4.50e-4	3/8/2010@10:56:04			
248516001	1	18	-1.70	0.0336	3/8/2010@10:56:58			
248516002	1	19	-2.03	0.0168	3/8/2010@10:57:51			
248518001	1	20	-2.35	3.13e-4	3/8/2010@10:58:44			
WCN100308-03	1	S3	107	5.64	3/8/2010@10:59:36			CCV
Known Conc:			100					
DQM Test: > + Percent Relative Difference								
Result:			6.6 < 10.0					
Message			CCV Passed					
Action			Continue					
DQM Test: < - Percent Relative Difference								
Result:			6.6 < 10.0					
Message			CCV Passed					
Action			Continue					
WCN100308-08	1	S7	-1.82	0.0275	3/8/2010@11:01:27			CCB
Known Conc:			0.00					
DQM Test: > + Concentration Limit								
Result:			-1.82 < 5.00					
Message			CCB Passed					
Action			Continue					
DQM Test: < - Concentration Limit								
Result:			-1.82 > -5.00					
Message			CCB Passed					
Action			Continue					
248533001	1	21	-1.85	0.0260	3/8/2010@11:03:16			
248548001	1	22	-2.24	0.00579	3/8/2010@11:04:09			
248548003	1	23	-1.45	0.0465	3/8/2010@11:05:01			
248551001	1	24	-0.552	0.0931	3/8/2010@11:05:54			
248551002	1	25	-1.81	0.0281	3/8/2010@11:06:46			
248555002	1	26	-1.99	0.0185	3/8/2010@11:07:39			
1202059721 960271 MB	1	27	-1.70	0.0339	3/8/2010@11:08:31			
1202059731 LCS	1	28	49.0	2.66	3/8/2010@11:09:23			
248072001	1	29	-2.36	-5.25e-4	3/8/2010@11:10:15			
1202059722 DUP	1	30	-1.95	0.0206	3/8/2010@11:11:06			
WCN100308-03	1	S3	105	5.54	3/8/2010@11:11:59			CCV
Known Conc:			100					
DQM Test: > + Percent Relative Difference								
Result:			4.7 < 10.0					
Message			CCV Passed					
Action			Continue					
DQM Test: < - Percent Relative Difference								
Result:			4.7 < 10.0					
Message			CCV Passed					
Action			Continue					
WCN100308-08	1	S7	-1.72	0.0325	3/8/2010@11:13:49			CCB
Known Conc:			0.00					

DQM Test: > + Concentration Limit						
Result:		-1.72 < 5.00				
Message		CCB Passed				
Action		Continue				
DQM Test: < - Concentration Limit						
Result:		-1.72 > -5.00				
Message		CCB Passed				
Action		Continue				
1202059725 MS	1	31	102	5.41	3/8/2010@11:15:40	
1202059728 MSD	1	32	101	5.33	3/8/2010@11:16:33	
248072002	1	33	-1.30	0.0543	3/8/2010@11:17:27	
248072003	1	34	-2.90	-0.0286	3/8/2010@11:18:21	
248097001	1	35	-1.88	0.0245	3/8/2010@11:19:14	
1202059724 DUP	1	36	-1.58	0.0398	3/8/2010@11:20:07	
1202059727 MS	1	37	100	5.32	3/8/2010@11:21:00	
1202059730 MSD	1	38	102	5.39	3/8/2010@11:21:53	
248097002	1	39	12.3	0.757	3/8/2010@11:22:47	
248097003	1	40	-1.04	0.0680	3/8/2010@11:23:38	
WCN100308-03	1	S3	106	5.63	3/8/2010@11:24:31	CCV
Known Conc:		100				
DQM Test: > + Percent Relative Difference						
Result:		6.4 < 10.0				
Message		CCV Passed				
Action		Continue				
DQM Test: < - Percent Relative Difference						
Result:		6.4 < 10.0				
Message		CCV Passed				
Action		Continue				
WCN100308-08	1	S7	-1.68	0.0346	3/8/2010@11:26:21	CCB
Known Conc:		0.00				
DQM Test: > + Concentration Limit						
Result:		-1.68 < 5.00				
Message		CCB Passed				
Action		Continue				
DQM Test: < - Concentration Limit						
Result:		-1.68 > -5.00				
Message		CCB Passed				
Action		Continue				
248097004	1	41	-0.871	0.0766	3/8/2010@11:28:09	
248298001	1	42	-1.67	0.0350	3/8/2010@11:29:02	
248298002	1	43	-1.93	0.0216	3/8/2010@11:29:53	
248298003	1	44	-0.109	0.116	3/8/2010@11:30:46	
248303001	1	45	2.92	0.273	3/8/2010@11:31:38	
248337001	1	46	-2.49	-0.00692	3/8/2010@11:32:32	
248375001	1	47	-2.35	1.70e-4	3/8/2010@11:33:26	
248375002	1	48	-2.05	0.0157	3/8/2010@11:34:19	
248397001	1	49	-1.87	0.0247	3/8/2010@11:35:14	
248397002	1	50	-2.17	0.00925	3/8/2010@11:36:06	
WCN100308-03	1	S3	106	5.62	3/8/2010@11:37:00	CCV
Known Conc:		100				
DQM Test: > + Percent Relative Difference						
Result:		6.2 < 10.0				
Message		CCV Passed				
Action		Continue				
DQM Test: < - Percent Relative Difference						
Result:		6.2 < 10.0				
Message		CCV Passed				
Action		Continue				
WCN100308-08	1	S7	-2.34	8.36e-4	3/8/2010@11:38:51	CCB
Known Conc:		0.00				
DQM Test: > + Concentration Limit						
Result:		-2.34 < 5.00				
Message		CCB Passed				
Action		Continue				
DQM Test: < - Concentration Limit						
Result:		-2.34 > -5.00				
Message		CCB Passed				
Action		Continue				

248407001	1	51	-1.69	0.0345	3/8/2010@11:40:39		
1202059723 DUP	1	52	-2.37	-0.00102	3/8/2010@11:41:33		
1202059726 MS	1	53	104	5.51	3/8/2010@11:42:26		
1202059729 MSD	1	54	82.4	4.39	3/8/2010@11:43:19		
248419001	1	55	-1.45	0.0465	3/8/2010@11:44:11		
248419002	1	56	-1.82	0.0276	3/8/2010@11:45:04		
1202053300 957584 MB	1	57	-1.77	0.0301	3/8/2010@11:45:57		
1202053310 LCS	1	58	52.0	2.81	3/8/2010@11:46:49		
247829002	1	59	-1.36	0.0515	3/8/2010@11:47:41		
1202053302 DUP	1	60	-1.35	0.0518	3/8/2010@11:48:33		
WCN100308-03	1	S3	107	5.65	3/8/2010@11:49:26		CCV
Known Conc:			100				
DQM Test: > + Percent Relative Difference							
Result:			6.9 < 10.0				
Message			CCV Passed				
Action			Continue				
DQM Test: < - Percent Relative Difference							
Result:			6.9 < 10.0				
Message			CCV Passed				
Action			Continue				
WCN100308-08	1	S7	-1.71	0.0332	3/8/2010@11:51:15		CCB
Known Conc:			0.00				
DQM Test: > + Concentration Limit							
Result:			-1.71 < 5.00				
Message			CCB Passed				
Action			Continue				
DQM Test: < - Concentration Limit							
Result:			-1.71 > -5.00				
Message			CCB Passed				
Action			Continue				
1202053305 MS	1	61	108	5.71	3/8/2010@11:53:05		
1202053308 MSD	1	62	108	5.72	3/8/2010@11:54:00		
247865010	1	63	-1.12	0.0636	3/8/2010@11:54:55		
247865012	1	64	-1.20	0.0593	3/8/2010@11:55:48		
1202053303 DUP	1	65	-1.53	0.0427	3/8/2010@11:56:41		
1202053306 MS	1	66	86.3	4.59	3/8/2010@11:57:35		
1202053309 MSD	1	67	102	5.39	3/8/2010@11:58:28		
247865013	1	68	-1.42	0.0483	3/8/2010@11:59:21		
247865014	1	69	-1.44	0.0472	3/8/2010@12:00:15		
247865015	1	70	-1.50	0.0439	3/8/2010@12:01:07		
WCN100308-03	1	S3	106	5.63	3/8/2010@12:02:00		CCV
Known Conc:			100				
DQM Test: > + Percent Relative Difference							
Result:			6.4 < 10.0				
Message			CCV Passed				
Action			Continue				
DQM Test: < - Percent Relative Difference							
Result:			6.4 < 10.0				
Message			CCV Passed				
Action			Continue				
WCN100308-08	1	S7	-1.63	0.0372	3/8/2010@12:03:51		CCB
Known Conc:			0.00				
DQM Test: > + Concentration Limit							
Result:			-1.63 < 5.00				
Message			CCB Passed				
Action			Continue				
DQM Test: < - Concentration Limit							
Result:			-1.63 > -5.00				
Message			CCB Passed				
Action			Continue				
247865016	1	71	-1.63	0.0374	3/8/2010@12:05:41		
247865017	1	72	-1.38	0.0501	3/8/2010@12:06:33		
247865018	1	73	-2.31	0.00203	3/8/2010@12:07:25		
247865019	1	74	-1.70	0.0337	3/8/2010@12:08:18		
247865020	1	75	-1.21	0.0589	3/8/2010@12:09:10		
247866001	1	76	-1.82	0.0273	3/8/2010@12:10:05		
247919001	1	77	-1.59	0.0392	3/8/2010@12:10:59		
247919002	1	78	-1.41	0.0486	3/8/2010@12:11:53		

247922004	1	79	0.739	0.160	3/8/2010@12:12:48		
1202053301 DUP	1	80	0.641	0.155	3/8/2010@12:13:41		
WCN100308-03	1	S3	107	5.65	3/8/2010@12:14:34		CCV
Known Conc:			100				
DQM Test: > + Percent Relative Difference							
Result:			6.8 < 10.0				
Message			CCV Passed				
Action			Continue				
DQM Test: < - Percent Relative Difference							
Result:			6.8 < 10.0				
Message			CCV Passed				
Action			Continue				
WCN100308-08	1	S7	-1.86	0.0256	3/8/2010@12:16:24		CCB
Known Conc:			0.00				
DQM Test: > + Concentration Limit							
Result:			-1.86 < 5.00				
Message			CCB Passed				
Action			Continue				
DQM Test: < - Concentration Limit							
Result:			-1.86 > -5.00				
Message			CCB Passed				
Action			Continue				
1202053304 MS	1	81	98.2	5.21	3/8/2010@12:18:14		
1202053307 MSD	1	82	98.4	5.21	3/8/2010@12:19:07		
248164004	1	83	-1.49	0.0445	3/8/2010@12:20:01		
248382002	1	84	-1.58	0.0400	3/8/2010@12:20:54		
248382003	1	85	-1.82	0.0273	3/8/2010@12:21:47		
248401002	1	86	-1.52	0.0428	3/8/2010@12:22:40		
248401004	1	87	-1.38	0.0501	3/8/2010@12:23:33		
WCN100308-03	1	S3	106	5.59	3/8/2010@12:24:25		CCV
Known Conc:			100				
DQM Test: > + Percent Relative Difference							
Result:			5.8 < 10.0				
Message			CCV Passed				
Action			Continue				
DQM Test: < - Percent Relative Difference							
Result:			5.8 < 10.0				
Message			CCV Passed				
Action			Continue				
WCN100308-08	1	S7	-1.71	0.0334	3/8/2010@12:26:15		CCB
Known Conc:			0.00				
DQM Test: > + Concentration Limit							
Result:			-1.71 < 5.00				
Message			CCB Passed				
Action			Continue				
DQM Test: < - Concentration Limit							
Result:			-1.71 > -5.00				
Message			CCB Passed				
Action			Continue				

Analyte Properties Table for OM_3-8-2010_10-24-48.OMN

Property	Channel 1
	TCYANIDE
Concentration Units	ug/L
Calibration Fit Type	First Order
Clear Calibration	True
Force Through Zero	False
Calibration Weighting	None
Auto Dilution Trigger	True
% of High Standard	100
Quik Chem Method	10-204-00-1-A
Chemistry	Direct/Bipolar
Calibration by Height	False
Inject to Peak Start	22
Peak Base Width	39

Channel 1: Current View


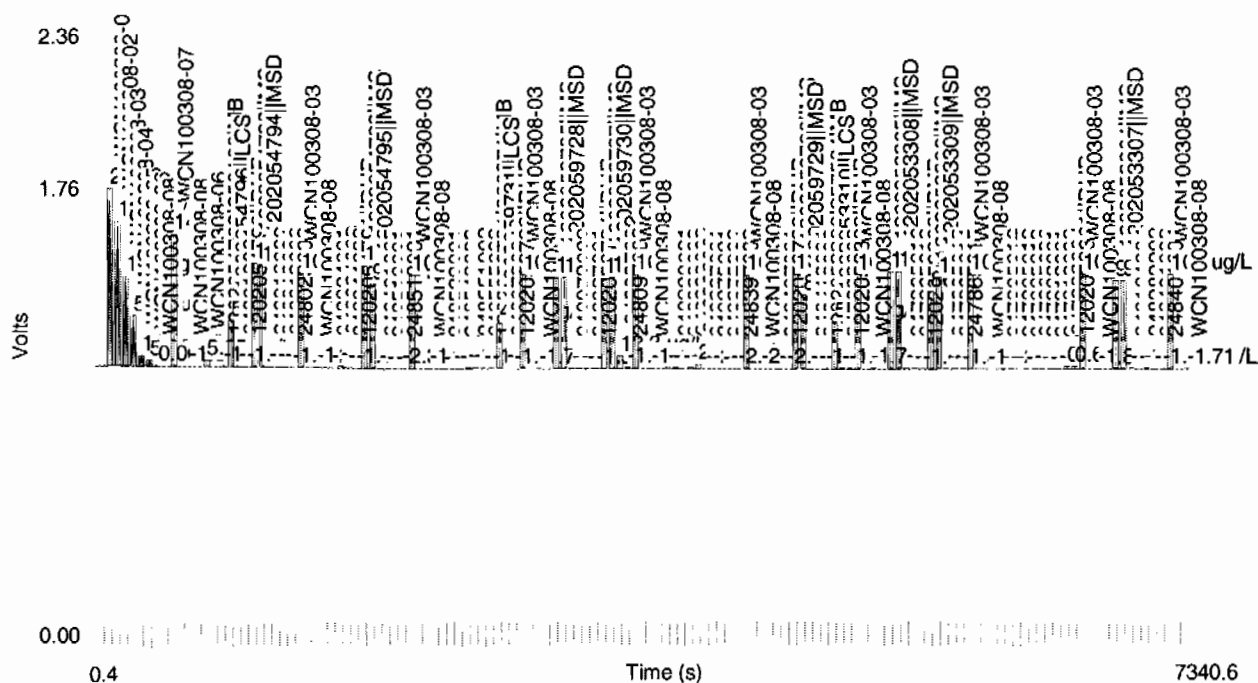


Table 1: TCYANIDE

	Conc. (ug/L)	Rep	Peak Area (Volt-s)	Peak Height (Volts)	% Residual	Detection Date	Detection Time
1	200	1	10.4	0.692	0.2	3/8/2010	10:26:48
2	150	1	7.82	0.567	0.7	3/8/2010	10:27:40
3	100	1	5.36	0.353	-1.3	3/8/2010	10:28:32
4	50.0	1	2.85	0.199	-5.1	3/8/2010	10:29:25
5	10.0	1	0.644	0.0420	-0.6	3/8/2010	10:30:18
6	5.00	1	0.400	0.0240	-4.6	3/8/2010	10:31:12
7	0.00	1	-0.0189	-0.00306		3/8/2010	10:32:06

Figure 1: TCYANIDE

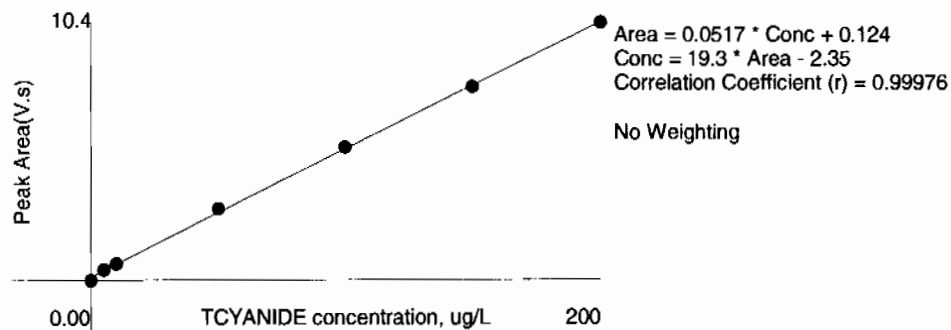

This is runlog Lachat1

Sample ID	Batch	Dilution	Analyst	Runtime	Dataset
CCV		1	axc2	3/8/2010 15:01:26	OM_3-8-2010_14-58-05
CCB		1	axc2	3/8/2010 15:03:15	OM_3-8-2010_14-58-05
1202057161	959217	1	axc2	3/8/2010 15:05:05	OM_3-8-2010_14-58-05
1202057168	959217	1	axc2	3/8/2010 15:05:58	OM_3-8-2010_14-58-05
248044005	959217	1	axc2	3/8/2010 15:06:52	OM_3-8-2010_14-58-05
1202057163	959217	1	axc2	3/8/2010 15:07:45	OM_3-8-2010_14-58-05
1202057165	959217	1	axc2	3/8/2010 15:08:38	OM_3-8-2010_14-58-05
1202057167	959217	1	axc2	3/8/2010 15:09:31	OM_3-8-2010_14-58-05
248044006	959217	1	axc2	3/8/2010 15:10:24	OM_3-8-2010_14-58-05
248108001	959217	1	axc2	3/8/2010 15:11:16	OM_3-8-2010_14-58-05
248117001	959217	1	axc2	3/8/2010 15:12:08	OM_3-8-2010_14-58-05
248127002	959217	1	axc2	3/8/2010 15:13:02	OM_3-8-2010_14-58-05
CCV		1	axc2	3/8/2010 15:13:54	OM_3-8-2010_14-58-05
CCB		1	axc2	3/8/2010 15:15:44	OM_3-8-2010_14-58-05
248162001	959217	1	axc2	3/8/2010 15:17:33	OM_3-8-2010_14-58-05
248162002	959217	1	axc2	3/8/2010 15:18:25	OM_3-8-2010_14-58-05
248162003	959217	1	axc2	3/8/2010 15:19:17	OM_3-8-2010_14-58-05
248162004	959217	1	axc2	3/8/2010 15:20:09	OM_3-8-2010_14-58-05
248164002	959217	1	axc2	3/8/2010 15:21:00	OM_3-8-2010_14-58-05
248168006	959217	1	axc2	3/8/2010 15:21:55	OM_3-8-2010_14-58-05
248169004	959217	1	axc2	3/8/2010 15:22:48	OM_3-8-2010_14-58-05
248188001	959217	1	axc2	3/8/2010 15:23:41	OM_3-8-2010_14-58-05
1202057162	959217	1	axc2	3/8/2010 15:24:34	OM_3-8-2010_14-58-05
1202057164*	959217	1	axc2	3/8/2010 15:25:27	OM_3-8-2010_14-58-05
CCV		1	axc2	3/8/2010 15:26:19	OM_3-8-2010_14-58-05
CCB		1	axc2	3/8/2010 15:28:11	OM_3-8-2010_14-58-05
1202057166	959217	1	axc2	3/8/2010 15:30:01	OM_3-8-2010_14-58-05
248199001	959217	1	axc2	3/8/2010 15:30:54	OM_3-8-2010_14-58-05
248238001	959217	1	axc2	3/8/2010 15:31:46	OM_3-8-2010_14-58-05
248238002	959217	1	axc2	3/8/2010 15:32:39	OM_3-8-2010_14-58-05
1202057164*	959217	1	axc2	3/8/2010 15:33:32	OM_3-8-2010_14-58-05
248242001	959217	1	axc2	3/8/2010 15:34:25	OM_3-8-2010_14-58-05
248245001	959217	1	axc2	3/8/2010 15:35:17	OM_3-8-2010_14-58-05
248257001	959217	1	axc2	3/8/2010 15:36:09	OM_3-8-2010_14-58-05
248257002	959217	1	axc2	3/8/2010 15:37:01	OM_3-8-2010_14-58-05
1202057164	959217	1	axc2	3/8/2010 15:37:54	OM_3-8-2010_14-58-05
CCV		1	axc2	3/8/2010 15:38:47	OM_3-8-2010_14-58-05
CCB		1	axc2	3/8/2010 15:40:39	OM_3-8-2010_14-58-05
1202057112	959204	1	axc2	3/8/2010 15:42:28	OM_3-8-2010_14-58-05
1202057119	959204	25	axc2	3/8/2010 15:43:18	OM_3-8-2010_14-58-05
248110001	959204	1	axc2	3/8/2010 15:44:13	OM_3-8-2010_14-58-05
248110002	959204	1	axc2	3/8/2010 15:45:07	OM_3-8-2010_14-58-05
248110003	959204	1	axc2	3/8/2010 15:46:00	OM_3-8-2010_14-58-05
248110004	959204	1	axc2	3/8/2010 15:46:54	OM_3-8-2010_14-58-05
248110005	959204	1	axc2	3/8/2010 15:47:47	OM_3-8-2010_14-58-05
248110006	959204	1	axc2	3/8/2010 15:48:41	OM_3-8-2010_14-58-05
248110007	959204	1	axc2	3/8/2010 15:49:33	OM_3-8-2010_14-58-05
248110008	959204	1	axc2	3/8/2010 15:50:26	OM_3-8-2010_14-58-05
CCV		1	axc2	3/8/2010 15:51:19	OM_3-8-2010_14-58-05
CCB		1	axc2	3/8/2010 15:53:09	OM_3-8-2010_14-58-05
248118001	959204	1	axc2	3/8/2010 15:54:59	OM_3-8-2010_14-58-05
248118002	959204	1	axc2	3/8/2010 15:55:52	OM_3-8-2010_14-58-05
248118003	959204	1	axc2	3/8/2010 15:56:45	OM_3-8-2010_14-58-05
248118004	959204	1	axc2	3/8/2010 15:57:37	OM_3-8-2010_14-58-05
248118005	959204	1	axc2	3/8/2010 15:58:28	OM_3-8-2010_14-58-05
248118006	959204	1	axc2	3/8/2010 15:59:22	OM_3-8-2010_14-58-05
248118007	959204	1	axc2	3/8/2010 16:00:13	OM_3-8-2010_14-58-05
248189001	959204	1	axc2	3/8/2010 16:01:07	OM_3-8-2010_14-58-05

1202057113	959204	1	axc2	3/8/2010	16:02:01	OM_3-8-2010_14-58-05
1202057115	959204	1	axc2	3/8/2010	16:02:55	OM_3-8-2010_14-58-05
CCV		1	axc2	3/8/2010	16:03:48	OM_3-8-2010_14-58-05
CCB		1	axc2	3/8/2010	16:05:39	OM_3-8-2010_14-58-05
1202057117	959204	1	axc2	3/8/2010	16:07:29	OM_3-8-2010_14-58-05
248189002	959204	1	axc2	3/8/2010	16:08:23	OM_3-8-2010_14-58-05
1202057114	959204	1	axc2	3/8/2010	16:09:16	OM_3-8-2010_14-58-05
1202057116	959204	1	axc2	3/8/2010	16:10:09	OM_3-8-2010_14-58-05
1202057118	959204	1	axc2	3/8/2010	16:11:02	OM_3-8-2010_14-58-05
1202054781	958165	1	axc2	3/8/2010	16:11:55	OM_3-8-2010_14-58-05
1202054788	958165	25	axc2	3/8/2010	16:12:47	OM_3-8-2010_14-58-05
247918001	958165	1	axc2	3/8/2010	16:13:39	OM_3-8-2010_14-58-05
247918002	958165	1	axc2	3/8/2010	16:14:33	OM_3-8-2010_14-58-05
247918003	958165	1	axc2	3/8/2010	16:15:25	OM_3-8-2010_14-58-05
CCV		1	axc2	3/8/2010	16:16:17	OM_3-8-2010_14-58-05
CCB		1	axc2	3/8/2010	16:18:09	OM_3-8-2010_14-58-05
247918004	958165	1	axc2	3/8/2010	16:19:58	OM_3-8-2010_14-58-05
1202054782	958165	1	axc2	3/8/2010	16:20:49	OM_3-8-2010_14-58-05
1202054784	958165	1	axc2	3/8/2010	16:21:44	OM_3-8-2010_14-58-05
1202054786	958165	1	axc2	3/8/2010	16:22:39	OM_3-8-2010_14-58-05
247918005	958165	1	axc2	3/8/2010	16:23:32	OM_3-8-2010_14-58-05
1202054783	958165	1	axc2	3/8/2010	16:24:26	OM_3-8-2010_14-58-05
1202054785	958165	1	axc2	3/8/2010	16:25:20	OM_3-8-2010_14-58-05
1202054787	958165	1	axc2	3/8/2010	16:26:12	OM_3-8-2010_14-58-05
247918006	958165	1	axc2	3/8/2010	16:27:06	OM_3-8-2010_14-58-05
247918007	958165	1	axc2	3/8/2010	16:28:00	OM_3-8-2010_14-58-05
CCV		1	axc2	3/8/2010	16:28:51	OM_3-8-2010_14-58-05
CCB		1	axc2	3/8/2010	16:30:42	OM_3-8-2010_14-58-05
248009001	958165	1	axc2	3/8/2010	16:32:32	OM_3-8-2010_14-58-05
248009002	958165	1	axc2	3/8/2010	16:33:25	OM_3-8-2010_14-58-05
248009003	958165	1	axc2	3/8/2010	16:34:17	OM_3-8-2010_14-58-05
248009004	958165	1	axc2	3/8/2010	16:35:10	OM_3-8-2010_14-58-05
248009005	958165	1	axc2	3/8/2010	16:36:03	OM_3-8-2010_14-58-05
248025001	958165	1	axc2	3/8/2010	16:36:55	OM_3-8-2010_14-58-05
248025002	958165	1	axc2	3/8/2010	16:37:48	OM_3-8-2010_14-58-05
248025004	958165	1	axc2	3/8/2010	16:38:42	OM_3-8-2010_14-58-05
248025006	958165	1	axc2	3/8/2010	16:39:36	OM_3-8-2010_14-58-05
248422001	958165	1	axc2	3/8/2010	16:40:31	OM_3-8-2010_14-58-05
CCV		1	axc2	3/8/2010	16:41:23	OM_3-8-2010_14-58-05
CCB		1	axc2	3/8/2010	16:43:15	OM_3-8-2010_14-58-05
248422002	958165	1	axc2	3/8/2010	16:45:06	OM_3-8-2010_14-58-05
1202061930	961278	1	axc2	3/8/2010	16:46:01	OM_3-8-2010_14-58-05
1202061932	961278	1	axc2	3/8/2010	16:46:53	OM_3-8-2010_14-58-05
247819001	961278	1	axc2	3/8/2010	16:47:47	OM_3-8-2010_14-58-05
1202061931	961278	1	axc2	3/8/2010	16:48:41	OM_3-8-2010_14-58-05
CCV		1	axc2	3/8/2010	16:49:33	OM_3-8-2010_14-58-05
CCB		1	axc2	3/8/2010	16:51:24	OM_3-8-2010_14-58-05

Original Run Filename: OM_3-8-2010_14-58-05.OMN created 3/8/2010 14:58:05
 Original Run Author's Signature: [axc2]
 Current Run Filename: OM_3-8-2010_14-58-05.OMN last modified 3/8/2010 16:52:28
 Current Run Author's Signature: [axc2]
 Description: GL-GC-E-095 EPA 335.1, 335.3, 335.4, 9012A, CLP335.2-M
 Liquid LCS nominal 50 ug/L

Sample	Rep.	Cup No.	Channel 1 TCYANIDE		Detection Time	ADF	MDF	Description
			Conc. (ug/L)	Area (Vs)				
WCN100308-03	1	S3	103	5.47	3/8/2010@15:01:26			CCV
Known Conc:			100					
DQM Test: > + Percent Relative Difference								
Result:			3.3 < 10.0					
Message			CCV Passed					
Action			Continue					
DQM Test: < - Percent Relative Difference								
Result:			3.3 < 10.0					
Message			CCV Passed					
Action			Continue					
Calibration:			Table/Fig. 1					
WCN100308-08	1	S7	-1.49	0.0446	3/8/2010@15:03:15			CCB
Known Conc:			0.00					
DQM Test: > + Concentration Limit								
Result:			-1.49 < 5.00					
Message			CCB Passed					
Action			Continue					
DQM Test: < - Concentration Limit								
Result:			-1.49 > -5.00					
Message			CCB Passed					
Action			Continue					
1202057161 959217 MB	1	1	-2.52	-0.00888	3/8/2010@15:05:05			
1202057168 LCS	1	2	49.3	2.67	3/8/2010@15:05:58			
248044005	1	3	-2.52	-0.00856	3/8/2010@15:06:52			
1202057163 DUP	1	4	-2.04	0.0161	3/8/2010@15:07:45			
1202057165 MS	1	5	101	5.35	3/8/2010@15:08:38			
1202057167 MSD	1	6	105	5.56	3/8/2010@15:09:31			
248044006	1	7	-1.95	0.0206	3/8/2010@15:10:24			
248108001	1	8	-2.52	-0.00848	3/8/2010@15:11:16			
248117001	1	9	-2.48	-0.00645	3/8/2010@15:12:08			
248127002	1	10	-0.731	0.0839	3/8/2010@15:13:02			
WCN100308-03	1	S3	106	5.63	3/8/2010@15:13:54			CCV
Known Conc:			100					
DQM Test: > + Percent Relative Difference								
Result:			6.4 < 10.0					
Message			CCV Passed					
Action			Continue					
DQM Test: < - Percent Relative Difference								
Result:			6.4 < 10.0					
Message			CCV Passed					
Action			Continue					
WCN100308-08	1	S7	-1.84	0.0265	3/8/2010@15:15:44			CCB
Known Conc:			0.00					
DQM Test: > + Concentration Limit								
Result:			-1.84 < 5.00					
Message			CCB Passed					
Action			Continue					
DQM Test: < - Concentration Limit								
Result:			-1.84 > -5.00					
Message			CCB Passed					
Action			Continue					
248162001	1	11	-2.35	1.80e-4	3/8/2010@15:17:33			
248162002	1	12	-2.05	0.0154	3/8/2010@15:18:25			
248162003	1	13	-2.14	0.0108	3/8/2010@15:19:17			
248162004	1	14	-2.03	0.0167	3/8/2010@15:20:09			
248164002	1	15	-1.57	0.0404	3/8/2010@15:21:00			

248168006	1	16	-1.99	0.0187	3/8/2010@15:21:55		
248169004	1	17	-1.56	0.0412	3/8/2010@15:22:48		
248188001	1	18	-2.03	0.0168	3/8/2010@15:23:41		
1202057162 DUP	1	19	-2.31	0.00215	3/8/2010@15:24:34		
1202057164 MS	1	20	70.7	3.78	3/8/2010@15:25:27		
WCN100308-03	1	S3	109	5.76	3/8/2010@15:26:19		CCV
Known Conc:			100				
DQM Test: > + Percent Relative Difference							
Result:			9.0 < 10.0				
Message			CCV Passed				
Action			Continue				
DQM Test: < - Percent Relative Difference							
Result:			9.0 < 10.0				
Message			CCV Passed				
Action			Continue				
WCN100308-08	1	S7	-1.78	0.0295	3/8/2010@15:28:11		CCB
Known Conc:			0.00				
DQM Test: > + Concentration Limit							
Result:			-1.78 < 5.00				
Message			CCB Passed				
Action			Continue				
DQM Test: < - Concentration Limit							
Result:			-1.78 > -5.00				
Message			CCB Passed				
Action			Continue				
1202057166 MSD	1	21	110	5.81	3/8/2010@15:30:01		
248199001	1	22	-1.68	0.0348	3/8/2010@15:30:54		
248238001	1	23	-1.98	0.0191	3/8/2010@15:31:46		
248238002	1	24	-1.94	0.0214	3/8/2010@15:32:39		
1202057164 MS	1	20	71.8	3.84	3/8/2010@15:33:32		
248242001	1	25	-1.93	0.0217	3/8/2010@15:34:25		
248245001	1	26	-2.35	1.99e-4	3/8/2010@15:35:17		
248257001	1	27	-2.49	-0.00739	3/8/2010@15:36:09		
248257002	1	28	-1.86	0.0256	3/8/2010@15:37:01		
1202057164 MS	1	20	106	5.61	3/8/2010@15:37:54		
WCN100308-03	1	S3	104	5.52	3/8/2010@15:38:47		CCV
Known Conc:			100				
DQM Test: > + Percent Relative Difference							
Result:			4.3 < 10.0				
Message			CCV Passed				
Action			Continue				
DQM Test: < - Percent Relative Difference							
Result:			4.3 < 10.0				
Message			CCV Passed				
Action			Continue				
WCN100308-08	1	S7	-0.768	0.0819	3/8/2010@15:40:39		CCB
Known Conc:			0.00				
DQM Test: > + Concentration Limit							
Result:			-0.768 < 5.00				
Message			CCB Passed				
Action			Continue				
DQM Test: < - Concentration Limit							
Result:			-0.768 > -5.00				
Message			CCB Passed				
Action			Continue				
1202057112 959204 MB	1	29	-2.19	0.00819	3/8/2010@15:42:28		
1202057119 LCS	1	30	31.1	1.73	3/8/2010@15:43:18	25.00	
248110001	1	31	-0.304	0.106	3/8/2010@15:44:13		
248110002	1	32	-1.46	0.0463	3/8/2010@15:45:07		
248110003	1	33	-2.31	0.00237	3/8/2010@15:46:00		
248110004	1	34	-2.16	0.00990	3/8/2010@15:46:54		
248110005	1	35	-0.698	0.0856	3/8/2010@15:47:47		
248110006	1	36	-1.47	0.0458	3/8/2010@15:48:41		
248110007	1	37	-1.24	0.0576	3/8/2010@15:49:33		
248110008	1	38	-0.761	0.0823	3/8/2010@15:50:26		
WCN100308-03	1	S3	106	5.60	3/8/2010@15:51:19		CCV
Known Conc:			100				
DQM Test: > + Percent Relative Difference							

		Result:	5.9 < 10.0					
		Message	CCV Passed					
		Action	Continue					
DQM Test: < - Percent Relative Difference								
		Result:	5.9 < 10.0					
		Message	CCV Passed					
		Action	Continue					
WCN100308-08	1	S7	-1.95	0.0205	3/8/2010@15:53:09			CCB
		Known Conc:	0.00					
DQM Test: > + Concentration Limit								
		Result:	-1.95 < 5.00					
		Message	CCB Passed					
		Action	Continue					
DQM Test: < - Concentration Limit								
		Result:	-1.95 > -5.00					
		Message	CCB Passed					
		Action	Continue					
248118001	1	39	0.0365	0.124	3/8/2010@15:54:59			
248118002	1	40	-2.19	0.00813	3/8/2010@15:55:52			
248118003	1	41	-0.754	0.0827	3/8/2010@15:56:45			
248118004	1	42	-1.55	0.0414	3/8/2010@15:57:37			
248118005	1	43	-1.86	0.0257	3/8/2010@15:58:28			
248118006	1	44	-0.195	0.112	3/8/2010@15:59:22			
248118007	1	45	-2.48	-0.00657	3/8/2010@16:00:13			
248189001	1	46	1.50	0.200	3/8/2010@16:01:07			
1202057113 DUP	1	47	1.10	0.179	3/8/2010@16:02:01			
1202057115 MS	1	48	98.4	5.21	3/8/2010@16:02:55			
WCN100308-03	1	S3	106	5.63	3/8/2010@16:03:48			CCV
		Known Conc:	100					
DQM Test: > + Percent Relative Difference								
		Result:	6.5 < 10.0					
		Message	CCV Passed					
		Action	Continue					
DQM Test: < - Percent Relative Difference								
		Result:	6.5 < 10.0					
		Message	CCV Passed					
		Action	Continue					
WCN100308-08	1	S7	-2.33	0.00121	3/8/2010@16:05:39			CCB
		Known Conc:	0.00					
DQM Test: > + Concentration Limit								
		Result:	-2.33 < 5.00					
		Message	CCB Passed					
		Action	Continue					
DQM Test: < - Concentration Limit								
		Result:	-2.33 > -5.00					
		Message	CCB Passed					
		Action	Continue					
1202057117 MSD	1	49	97.7	5.18	3/8/2010@16:07:29			
248189002	1	50	0.509	0.148	3/8/2010@16:08:23			
1202057114 DUP	1	51	0.322	0.138	3/8/2010@16:09:16			
1202057116 MS	1	52	93.9	4.98	3/8/2010@16:10:09			
1202057118 MSD	1	53	93.9	4.98	3/8/2010@16:11:02			
1202054781 958165 MB	1	54	-2.89	-0.0281	3/8/2010@16:11:55			
1202054788 LCS	1	55	20.3	1.17	3/8/2010@16:12:47		25.00	
247918001	1	56	-1.17	0.0613	3/8/2010@16:13:39			
247918002	1	57	-1.63	0.0371	3/8/2010@16:14:33			
247918003	1	58	-2.35	2.32e-4	3/8/2010@16:15:25			
WCN100308-03	1	S3	106	5.59	3/8/2010@16:16:17			CCV
		Known Conc:	100					
DQM Test: > + Percent Relative Difference								
		Result:	5.7 < 10.0					
		Message	CCV Passed					
		Action	Continue					
DQM Test: < - Percent Relative Difference								
		Result:	5.7 < 10.0					
		Message	CCV Passed					
		Action	Continue					
WCN100308-08	1	S7	-2.61	-0.0134	3/8/2010@16:18:09			CCB

Known Conc:			0.00					
DQM Test: > + Concentration Limit								
Result:			-2.61 < 5.00					
Message			CCB Passed					
Action			Continue					
DQM Test: < - Concentration Limit								
Result:			-2.61 > -5.00					
Message			CCB Passed					
Action			Continue					
247918004	1	59	-1.83	0.0268	3/8/2010@16:19:58			
1202054782	DUP	1	60	-1.86	0.0252	3/8/2010@16:20:49		
1202054784	MS	1	61	88.6	4.71	3/8/2010@16:21:44		
1202054786	MSD	1	62	102	5.39	3/8/2010@16:22:39		
247918005	1	63	-1.63	0.0372	3/8/2010@16:23:32			
1202054783	DUP	1	64	-2.35	2.22e-4	3/8/2010@16:24:26		
1202054785	MS	1	65	103	5.44	3/8/2010@16:25:20		
1202054787	MSD	1	66	99.0	5.24	3/8/2010@16:26:12		
247918006	1	67	-0.953	0.0724	3/8/2010@16:27:06			
247918007	1	68	0.145	0.129	3/8/2010@16:28:00			
WCN100308-03	1	S3	105	5.54	3/8/2010@16:28:51			CCV
Known Conc:			100					
DQM Test: > + Percent Relative Difference								
Result:			4.6 < 10.0					
Message			CCV Passed					
Action			Continue					
DQM Test: < - Percent Relative Difference								
Result:			4.6 < 10.0					
Message			CCV Passed					
Action			Continue					
WCN100308-08	1	S7	-2.34	4.90e-4	3/8/2010@16:30:42			CCB
Known Conc:			0.00					
DQM Test: > + Concentration Limit								
Result:			-2.34 < 5.00					
Message			CCB Passed					
Action			Continue					
DQM Test: < - Concentration Limit								
Result:			-2.34 > -5.00					
Message			CCB Passed					
Action			Continue					
248009001	1	69	-2.44	-0.00446	3/8/2010@16:32:32			
248009002	1	70	-1.42	0.0484	3/8/2010@16:33:25			
248009003	1	71	2.15	0.233	3/8/2010@16:34:17			
248009004	1	72	-1.18	0.0606	3/8/2010@16:35:10			
248009005	1	73	-2.05	0.0157	3/8/2010@16:36:03			
248025001	1	74	-2.44	-0.00448	3/8/2010@16:36:55			
248025002	1	75	-1.60	0.0388	3/8/2010@16:37:48			
248025004	1	76	-0.787	0.0809	3/8/2010@16:38:42			
248025006	1	77	-0.371	0.102	3/8/2010@16:39:36			
248422001	1	78	-2.28	0.00369	3/8/2010@16:40:31			
WCN100308-03	1	S3	102	5.40	3/8/2010@16:41:23			CCV
Known Conc:			100					
DQM Test: > + Percent Relative Difference								
Result:			2.0 < 10.0					
Message			CCV Passed					
Action			Continue					
DQM Test: < - Percent Relative Difference								
Result:			2.0 < 10.0					
Message			CCV Passed					
Action			Continue					
WCN100308-08	1	S7	-2.30	0.00277	3/8/2010@16:43:15			CCB
Known Conc:			0.00					
DQM Test: > + Concentration Limit								
Result:			-2.30 < 5.00					
Message			CCB Passed					
Action			Continue					
DQM Test: < - Concentration Limit								
Result:			-2.30 > -5.00					
Message			CCB Passed					

		Action	Continue					
248422002	1	79	-1.20	0.0595	3/8/2010@16:45:06			
1202061930 961278 MB	1	80	-1.83	0.0272	3/8/2010@16:46:01			
1202061932 LCS	1	81	-1.96	0.0203	3/8/2010@16:46:53			
247819001	1	82	110	5.83	3/8/2010@16:47:47			
1202061931 DUP	1	83	184	9.64	3/8/2010@16:48:41			
WCN100308-03	1	S3	106	5.59	3/8/2010@16:49:33			CCV
Known Conc:		100						
DQM Test: > + Percent Relative Difference								
Result:		5.7 < 10.0						
Message		CCV Passed						
Action		Continue						
DQM Test: < - Percent Relative Difference								
Result:		5.7 < 10.0						
Message		CCV Passed						
Action		Continue						
WCN100308-08	1	S7	-2.34	3.67e-4	3/8/2010@16:51:24			CCB
Known Conc:		0.00						
DQM Test: > + Concentration Limit								
Result:		-2.34 < 5.00						
Message		CCB Passed						
Action		Continue						
DQM Test: < - Concentration Limit								
Result:		-2.34 > -5.00						
Message		CCB Passed						
Action		Continue						

Analyte Properties Table for OM_3-8-2010_14-58-05.OMN

Property	Channel 1 TCYANIDE
Concentration Units	ug/L
Calibration Fit Type	First Order
Clear Calibration	True
Force Through Zero	False
Calibration Weighting	None
Auto Dilution Trigger	True
% of High Standard	100
Quik Chem Method	10-204-00-1-A
Chemistry	Direct/Bipolar
Calibration by Height	False
Inject to Peak Start	22
Peak Base Width	39

Channel 1: Current View


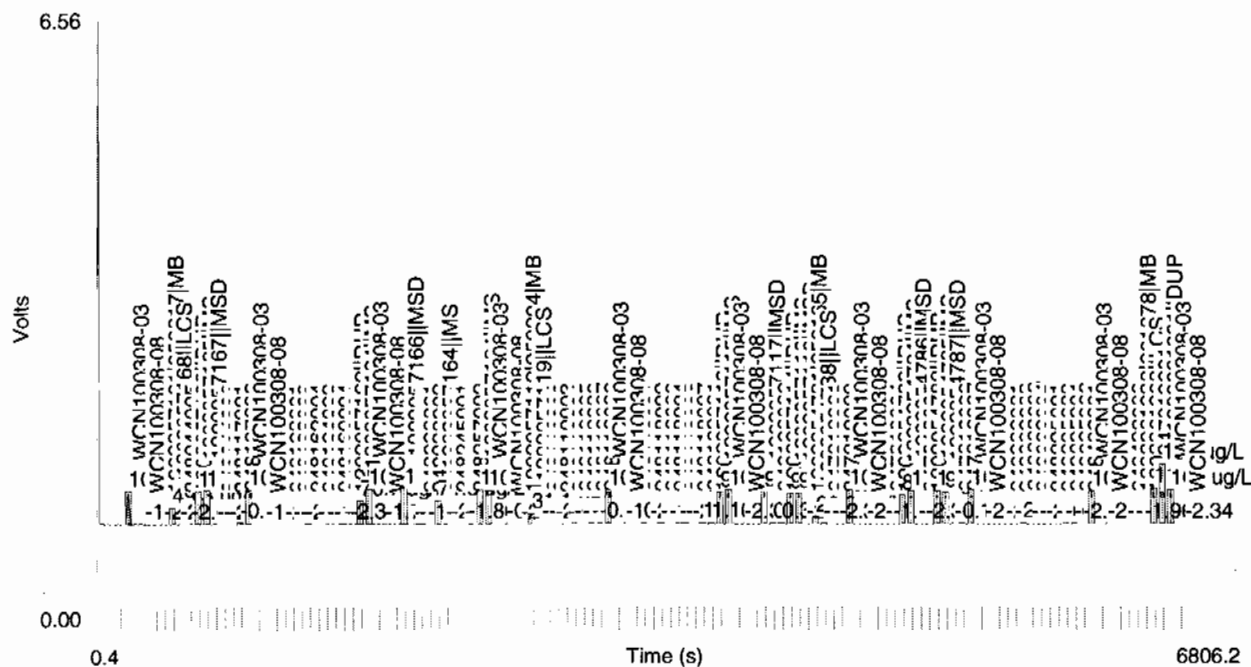


Table 1: TCYANIDE

	Conc. (ug/L)	Rep	Peak Area (Volt-s)	Peak Height (Volts)	% Residual	Detection Date	Detection Time
1	200	1	10.4	0.692	0.2	3/8/2010	10:26:48
2	150	1	7.82	0.567	0.7	3/8/2010	10:27:40
3	100	1	5.36	0.353	-1.3	3/8/2010	10:28:32
4	50.0	1	2.85	0.199	-5.1	3/8/2010	10:29:25
5	10.0	1	0.644	0.0420	-0.6	3/8/2010	10:30:18
6	5.00	1	0.400	0.0240	-4.6	3/8/2010	10:31:12
7	0.00	1	-0.0189	-0.00306		3/8/2010	10:32:06

Figure 1: TCYANIDE

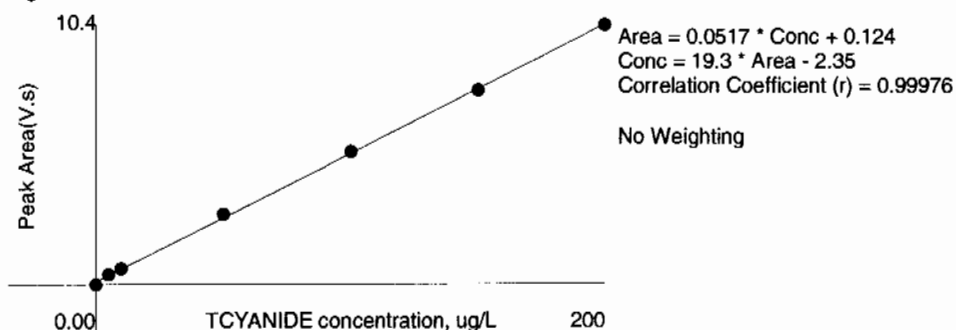

Nitrate Nitrite by Cadmium Reduction

This is runlog lachat3

Sample ID	Batch	Dilution	Analyst	Runtime	Dataset
1.5 PPM		1	axh3	3/3/2010 10:31:50	OM_3-3-2010_10-30-06
1.0 PPM		1	axh3	3/3/2010 10:33:02	OM_3-3-2010_10-30-06
0.5 ppm		1	axh3	3/3/2010 10:34:15	OM_3-3-2010_10-30-06
0.1 ppm		1	axh3	3/3/2010 10:35:29	OM_3-3-2010_10-30-06
0.05 ppm		1	axh3	3/3/2010 10:36:42	OM_3-3-2010_10-30-06
ICAL-00		1	axh3	3/3/2010 10:37:56	OM_3-3-2010_10-30-06
1.0 ppm ICB		1	axh3	3/3/2010 10:40:18	OM_3-3-2010_10-30-06
ICB		1	axh3	3/3/2010 10:42:40	OM_3-3-2010_10-30-06
Nitrate 1.0 ppm		1	axh3	3/3/2010 10:44:59	OM_3-3-2010_10-30-06
Nitrite 1.0 ppm		1	axh3	3/3/2010 10:47:19	OM_3-3-2010_10-30-06
1202054725	958150	1	axh3	3/3/2010 10:49:40	OM_3-3-2010_10-30-06
1202054732	958150	1	axh3	3/3/2010 10:50:53	OM_3-3-2010_10-30-06
247793001	958150	5	axh3	3/3/2010 10:52:06	OM_3-3-2010_10-30-06
1202054726	958150	5	axh3	3/3/2010 10:53:20	OM_3-3-2010_10-30-06
1202054729	958150	5	axh3	3/3/2010 10:54:32	OM_3-3-2010_10-30-06
247997001	958150	5	axh3	3/3/2010 10:55:44	OM_3-3-2010_10-30-06
248001001	958150	5	axh3	3/3/2010 10:56:57	OM_3-3-2010_10-30-06
248019001	958150	5	axh3	3/3/2010 10:58:10	OM_3-3-2010_10-30-06
248023001	958150	5	axh3	3/3/2010 10:59:22	OM_3-3-2010_10-30-06
248024002	958150	10	axh3	3/3/2010 11:00:34	OM_3-3-2010_10-30-06
1.0 ppm CCV		1	axh3	3/3/2010 11:01:46	OM_3-3-2010_10-30-06
CCB		1	axh3	3/3/2010 11:04:08	OM_3-3-2010_10-30-06
248024004	958150	10	axh3	3/3/2010 11:05:20	OM_3-3-2010_10-30-06
248038001	958150	5	axh3	3/3/2010 11:06:32	OM_3-3-2010_10-30-06
248038002	958150	5	axh3	3/3/2010 11:07:44	OM_3-3-2010_10-30-06
248039001	958150	5	axh3	3/3/2010 11:08:55	OM_3-3-2010_10-30-06
248044001*	958150	5	axh3	3/3/2010 11:10:07	OM_3-3-2010_10-30-06
1202054727	958150	5	axh3	3/3/2010 11:11:20	OM_3-3-2010_10-30-06
1202054730	958150	5	axh3	3/3/2010 11:12:34	OM_3-3-2010_10-30-06
248044003	958150	5	axh3	3/3/2010 11:13:47	OM_3-3-2010_10-30-06
248046001	958150	5	axh3	3/3/2010 11:14:59	OM_3-3-2010_10-30-06
248046002	958150	5	axh3	3/3/2010 11:16:12	OM_3-3-2010_10-30-06
1.0 ppm CCV		1	axh3	3/3/2010 11:17:24	OM_3-3-2010_10-30-06
CCB		1	axh3	3/3/2010 11:19:46	OM_3-3-2010_10-30-06
248044001	958150	5	axh3	3/3/2010 11:22:05	OM_3-3-2010_10-30-06
248053001	958150	5	axh3	3/3/2010 11:23:18	OM_3-3-2010_10-30-06
248053002	958150	5	axh3	3/3/2010 11:24:30	OM_3-3-2010_10-30-06
248053003	958150	5	axh3	3/3/2010 11:25:43	OM_3-3-2010_10-30-06
248074001	958150	5	axh3	3/3/2010 11:26:55	OM_3-3-2010_10-30-06
1202054728	958150	5	axh3	3/3/2010 11:28:07	OM_3-3-2010_10-30-06
1202054731	958150	5	axh3	3/3/2010 11:29:19	OM_3-3-2010_10-30-06
248074002	958150	5	axh3	3/3/2010 11:30:31	OM_3-3-2010_10-30-06
248074003	958150	5	axh3	3/3/2010 11:31:43	OM_3-3-2010_10-30-06
247793001	958150	10	axh3	3/3/2010 11:32:57	OM_3-3-2010_10-30-06
1.0 ppm CCV		1	axh3	3/3/2010 11:34:09	OM_3-3-2010_10-30-06
CCB		1	axh3	3/3/2010 11:36:31	OM_3-3-2010_10-30-06
1202054726	958150	10	axh3	3/3/2010 11:38:51	OM_3-3-2010_10-30-06
1202054729	958150	10	axh3	3/3/2010 11:40:03	OM_3-3-2010_10-30-06
248039001	958150	10	axh3	3/3/2010 11:41:15	OM_3-3-2010_10-30-06
248046001	958150	10	axh3	3/3/2010 11:42:28	OM_3-3-2010_10-30-06
1202057088	959199	1	axh3	3/3/2010 11:43:39	OM_3-3-2010_10-30-06
1202057095	959199	1	axh3	3/3/2010 11:44:50	OM_3-3-2010_10-30-06
247853003	959199	5	axh3	3/3/2010 11:46:04	OM_3-3-2010_10-30-06
1202057089	959199	5	axh3	3/3/2010 11:47:17	OM_3-3-2010_10-30-06
1202057092	959199	5	axh3	3/3/2010 11:48:30	OM_3-3-2010_10-30-06
247853006	959199	25	axh3	3/3/2010 11:49:43	OM_3-3-2010_10-30-06
1.0 ppm CCV		1	axh3	3/3/2010 11:50:55	OM_3-3-2010_10-30-06
CCB		1	axh3	3/3/2010 11:53:16	OM_3-3-2010_10-30-06

247853009	959199	5	axh3	3/3/2010	11:55:37	OM_3-3-2010_10-30-06
247853012	959199	10	axh3	3/3/2010	11:56:49	OM_3-3-2010_10-30-06
247853015	959199	10	axh3	3/3/2010	11:58:02	OM_3-3-2010_10-30-06
247853018	959199	50	axh3	3/3/2010	11:59:14	OM_3-3-2010_10-30-06
247966003	959199	5	axh3	3/3/2010	12:00:27	OM_3-3-2010_10-30-06
1202057096	959199	5	axh3	3/3/2010	12:01:39	OM_3-3-2010_10-30-06
1202057097	959199	5	axh3	3/3/2010	12:02:51	OM_3-3-2010_10-30-06
247966011	959199	5	axh3	3/3/2010	12:04:03	OM_3-3-2010_10-30-06
248044005	959199	5	axh3	3/3/2010	12:05:15	OM_3-3-2010_10-30-06
1202059915	959199	5	axh3	3/3/2010	12:06:27	OM_3-3-2010_10-30-06
1.0 ppm CCV		1	axh3	3/3/2010	12:07:39	OM_3-3-2010_10-30-06
CCB		1	axh3	3/3/2010	12:10:01	OM_3-3-2010_10-30-06
1202059916	959199	5	axh3	3/3/2010	12:12:21	OM_3-3-2010_10-30-06
248072001	959199	5	axh3	3/3/2010	12:13:31	OM_3-3-2010_10-30-06
1202057091	959199	5	axh3	3/3/2010	12:14:43	OM_3-3-2010_10-30-06
1202057094	959199	5	axh3	3/3/2010	12:15:56	OM_3-3-2010_10-30-06
248072002	959199	5	axh3	3/3/2010	12:17:09	OM_3-3-2010_10-30-06
248072003	959199	5	axh3	3/3/2010	12:18:23	OM_3-3-2010_10-30-06
248103003	959199	5	axh3	3/3/2010	12:19:36	OM_3-3-2010_10-30-06
248108001	959199	5	axh3	3/3/2010	12:20:48	OM_3-3-2010_10-30-06
1202057090	959199	5	axh3	3/3/2010	12:22:01	OM_3-3-2010_10-30-06
1202057093	959199	5	axh3	3/3/2010	12:23:13	OM_3-3-2010_10-30-06
1.0 ppm CCV		1	axh3	3/3/2010	12:24:25	OM_3-3-2010_10-30-06
CCB		1	axh3	3/3/2010	12:26:48	OM_3-3-2010_10-30-06
248117001	959199	5	axh3	3/3/2010	12:29:08	OM_3-3-2010_10-30-06
248126003	959199	5	axh3	3/3/2010	12:30:20	OM_3-3-2010_10-30-06
248127001	959199	5	axh3	3/3/2010	12:31:32	OM_3-3-2010_10-30-06
248199001	959199	5	axh3	3/3/2010	12:32:44	OM_3-3-2010_10-30-06
248238001	959199	5	axh3	3/3/2010	12:33:56	OM_3-3-2010_10-30-06
248238002	959199	5	axh3	3/3/2010	12:35:08	OM_3-3-2010_10-30-06
247966003	959199	5	axh3	3/3/2010	12:36:20	OM_3-3-2010_10-30-06
1202057096	959199	5	axh3	3/3/2010	12:37:32	OM_3-3-2010_10-30-06
1202057097	959199	5	axh3	3/3/2010	12:38:45	OM_3-3-2010_10-30-06
248108001	959199	10	axh3	3/3/2010	12:39:57	OM_3-3-2010_10-30-06
1.0 ppm CCV		1	axh3	3/3/2010	12:41:09	OM_3-3-2010_10-30-06
CCB		1	axh3	3/3/2010	12:43:31	OM_3-3-2010_10-30-06
1202057090	959199	10	axh3	3/3/2010	12:45:52	OM_3-3-2010_10-30-06
1202057093	959199	10	axh3	3/3/2010	12:47:05	OM_3-3-2010_10-30-06
1202058290	959715	1	axh3	3/3/2010	12:48:17	OM_3-3-2010_10-30-06
1202058297	959715	1	axh3	3/3/2010	12:49:29	OM_3-3-2010_10-30-06
248044006	959715	5	axh3	3/3/2010	12:50:42	OM_3-3-2010_10-30-06
1202058291	959715	5	axh3	3/3/2010	12:51:54	OM_3-3-2010_10-30-06
1202058294	959715	5	axh3	3/3/2010	12:53:07	OM_3-3-2010_10-30-06
248164001	959715	5	axh3	3/3/2010	12:54:19	OM_3-3-2010_10-30-06
248164003	959715	5	axh3	3/3/2010	12:55:31	OM_3-3-2010_10-30-06
248261001	959715	5	axh3	3/3/2010	12:56:43	OM_3-3-2010_10-30-06
1.0 ppm CCV		1	axh3	3/3/2010	12:57:55	OM_3-3-2010_10-30-06
CCB		1	axh3	3/3/2010	13:00:17	OM_3-3-2010_10-30-06
1202058292	959715	5	axh3	3/3/2010	13:02:37	OM_3-3-2010_10-30-06
1202058295	959715	5	axh3	3/3/2010	13:03:49	OM_3-3-2010_10-30-06
248298001	959715	5	axh3	3/3/2010	13:05:01	OM_3-3-2010_10-30-06
1202058293	959715	5	axh3	3/3/2010	13:06:15	OM_3-3-2010_10-30-06
1202058296	959715	5	axh3	3/3/2010	13:07:28	OM_3-3-2010_10-30-06
248298002	959715	5	axh3	3/3/2010	13:08:41	OM_3-3-2010_10-30-06
248298003	959715	5	axh3	3/3/2010	13:09:53	OM_3-3-2010_10-30-06
248382001	959715	5	axh3	3/3/2010	13:11:06	OM_3-3-2010_10-30-06
248382004	959715	5	axh3	3/3/2010	13:12:19	OM_3-3-2010_10-30-06
248401001	959715	5	axh3	3/3/2010	13:13:31	OM_3-3-2010_10-30-06
1.0 ppm CCV		1	axh3	3/3/2010	13:14:44	OM_3-3-2010_10-30-06
CCB		1	axh3	3/3/2010	13:17:05	OM_3-3-2010_10-30-06

248401003	959715	5	axh3	3/3/2010	13:19:26	OM_3-3-2010_10-30-06
248401006	959715	5	axh3	3/3/2010	13:20:37	OM_3-3-2010_10-30-06
248407001	959715	5	axh3	3/3/2010	13:21:49	OM_3-3-2010_10-30-06
248419001	959715	5	axh3	3/3/2010	13:23:01	OM_3-3-2010_10-30-06
248419002	959715	5	axh3	3/3/2010	13:24:13	OM_3-3-2010_10-30-06
1.0 ppm CCV		1	axh3	3/3/2010	13:26:33	OM_3-3-2010_10-30-06
CCB		1	axh3	3/3/2010	13:28:56	OM_3-3-2010_10-30-06

Original Run Filename: OM_3-3-2010_10-30-06.OMN created 3/3/2010 10:30:06
 Original Run Author's Signature: [lachat]
 Current Run Filename: OM_3-3-2010_10-30-06.OMN last modified 3/3/2010 13:30:17
 Current Run Author's Signature: [lachat]
 Description: EPA 353.2
 Cadmium Colum 9056CAJ
 LCS nominal 1.0 mg/L

Sample	Rep.	Cup No.	Channel 1		Detection Time	ADF	MDF	Description
			NO3 + NO2 Conc. (mg/L)	Area (Vs)				
WTR100303-26	1	S9	1.50	14.8	3/3/2010@10:31:50			1.5 PPM
WTR100303-25	1	S10	1.00	9.68	3/3/2010@10:33:02			1.0 PPM
WTR100303-24	1	S11	0.500	4.89	3/3/2010@10:34:15			0.5 ppm
WTR100303-23	1	S12	0.100	1.02	3/3/2010@10:35:29			0.1 ppm
WTR100303-21	1	S13	0.0500	0.312	3/3/2010@10:36:42			0.05 ppm
0.0ppm	1	S15	0.00	-0.0280	3/3/2010@10:37:56			0.0 ppm
DQM Test: Minimum Correlation Coefficient								
Result:			0.99989 > 0.99500					
Message			Calibration Passed					
Action			Continue					
WTR100303-27 ICV	1	S16	0.983	9.62	3/3/2010@10:40:18			1.0 ppm ICV
Known Conc:			1.00					
DQM Test: > + Concentration Limit								
Result:			0.983 < 1.10					
Message			ICV Passed					
Action			Continue					
DQM Test: < - Concentration Limit								
Result:			0.983 > 0.894					
Message			ICV Passed					
Action			Continue					
Calibration:			Table/Fig. 1					
ICB	1	S15	0.00396	-0.0247	3/3/2010@10:42:40			ICB
Known Conc:			0.00					
DQM Test: > + Concentration Limit								
Result:			0.00396 < 0.0500					
Message			ICB Passed					
Action			Continue					
DQM Test: < - Concentration Limit								
Result:			0.00396 > -0.0500					
Message			ICB Passed					
Action			Continue					
WTR100303-22	1	S1	0.943	9.22	3/3/2010@10:44:59			Nitrate 1.0 ppm
Known Conc:			1.00					
DQM Test: > + Concentration Limit								
Result:			0.943 < 1.10					
Message			Nitrate Standard Passed					
Action			Continue					
DQM Test: < - Concentration Limit								
Result:			0.943 > 0.894					
Message			Nitrate Standard Passed					
Action			Continue					
WTR100303-28	1	S2	0.937	9.17	3/3/2010@10:47:19			Nitrite 1.0 ppm
Known Conc:			1.00					
DQM Test: > + Concentration Limit								
Result:			0.937 < 1.10					
Message			Nitrite Standard Passed					
Action			Continue					
DQM Test: < - Concentration Limit								
Result:			0.937 > 0.894					
Message			Nitrite Standard Passed					
Action			Continue					
1202054725 958150 MB	1	1	0.0124	0.0582	3/3/2010@10:49:40			
1202054732 LCS	1	2	0.986	9.65	3/3/2010@10:50:53			
247793001	1	3	-0.0329	-0.388	3/3/2010@10:52:06		5.00	
1202054726 DUP	1	4	-0.0360	-0.419	3/3/2010@10:53:20		5.00	
1202054729 PS	1	5	0.348	3.36	3/3/2010@10:54:32		5.00	


247997001	1	6	0.0124	0.0585	3/3/2010@10:55:44	5.00	
248001001	1	7	0.0131	0.0653	3/3/2010@10:56:57	5.00	
248019001	1	8	0.196	1.87	3/3/2010@10:58:10	5.00	
248023001	1	9	0.0844	0.767	3/3/2010@10:59:22	5.00	
248024002	1	10	0.425	4.12	3/3/2010@11:00:34	10.00	
WTR100303-25 CCV	1	S10	0.983	9.62	3/3/2010@11:01:46		1.0 ppm CCV
Known Conc:			1.00				
DQM Test: > + Concentration Limit							
Result:			0.983 < 1.10				
Message			CCV Passed				
Action			Continue				
DQM Test: < - Concentration Limit							
Result:			0.983 > 0.894				
Message			CCV Passed				
Action			Continue				
CCB	1	S15	0.00204	-0.0437	3/3/2010@11:04:08		CCB
Known Conc:			0.00				
DQM Test: > + Concentration Limit							
Result:			0.00204 < 0.0500				
Message			CCB Passed				
Action			Continue				
DQM Test: < - Concentration Limit							
Result:			0.00204 > -0.0500				
Message			CCB Passed				
Action			Continue				
248024004	1	11	0.430	4.17	3/3/2010@11:05:20	10.00	
248038001	1	12	0.0214	0.147	3/3/2010@11:06:32	5.00	
248038002	1	13	0.0741	0.666	3/3/2010@11:07:44	5.00	
248039001	1	14	-0.0529	-0.584	3/3/2010@11:08:55	5.00	
248044001	1	15	2.97	29.2	3/3/2010@11:10:07	5.00	
1202054727 DUP	1	16	0.0856	0.779	3/3/2010@11:11:20	5.00	
1202054730 PS	1	17	1.05	10.3	3/3/2010@11:12:34	5.00	
248044003	1	18	0.0366	0.297	3/3/2010@11:13:47	5.00	
248046001	1	19	-0.0557	-0.613	3/3/2010@11:14:59	5.00	
248046002	1	20	-0.0479	-0.535	3/3/2010@11:16:12	5.00	
WTR100303-25 CCV	1	S10	1.00	9.80	3/3/2010@11:17:24		1.0 ppm CCV
Known Conc:			1.00				
DQM Test: > + Concentration Limit							
Result:			1.00 < 1.10				
Message			CCV Passed				
Action			Continue				
DQM Test: < - Concentration Limit							
Result:			1.00 > 0.894				
Message			CCV Passed				
Action			Continue				
CCB	1	S15	0.00357	-0.0286	3/3/2010@11:19:46		CCB
Known Conc:			0.00				
DQM Test: > + Concentration Limit							
Result:			0.00357 < 0.0500				
Message			CCB Passed				
Action			Continue				
DQM Test: < - Concentration Limit							
Result:			0.00357 > -0.0500				
Message			CCB Passed				
Action			Continue				
248044001	1	15	0.0892	0.815	3/3/2010@11:22:05	5.00	
248053001	1	21	0.0149	0.0826	3/3/2010@11:23:18	5.00	
248053002	1	22	0.0149	0.0834	3/3/2010@11:24:30	5.00	
248053003	1	23	0.0120	0.0547	3/3/2010@11:25:43	5.00	
248074001	1	24	0.393	3.81	3/3/2010@11:26:55	5.00	
1202054728 DUP	1	25	0.388	3.76	3/3/2010@11:28:07	5.00	
1202054731 PS	1	26	1.39	13.6	3/3/2010@11:29:19	5.00	
248074002	1	27	0.131	1.23	3/3/2010@11:30:31	5.00	
248074003	1	28	0.276	2.66	3/3/2010@11:31:43	5.00	
247793001	1	3	0.00533	-0.0112	3/3/2010@11:32:57	10.00	
WTR100303-25 CCV	1	S10	0.985	9.64	3/3/2010@11:34:09		1.0 ppm CCV
Known Conc:			1.00				
DQM Test: > + Concentration Limit							

		Result:	0.985 < 1.10				
		Message	CCV Passed				
		Action	Continue				
DQM Test: < - Concentration Limit							
		Result:	0.985 > 0.894				
		Message	CCV Passed				
		Action	Continue				
CCB	1	S15	0.00385	-0.0258	3/3/2010@11:36:31		CCB
		Known Conc:	0.00				
DQM Test: > + Concentration Limit							
		Result:	0.00385 < 0.0500				
		Message	CCB Passed				
		Action	Continue				
DQM Test: < - Concentration Limit							
		Result:	0.00385 > -0.0500				
		Message	CCB Passed				
		Action	Continue				
1202054726	DUP	1	4	0.0111	0.0460	3/3/2010@11:38:51	10.00
1202054729	PS	1	5	1.01	9.86	3/3/2010@11:40:03	10.00
248039001		1	14	-0.0350	-0.408	3/3/2010@11:41:15	10.00
248046001		1	19	-0.0330	-0.389	3/3/2010@11:42:28	10.00
1202057088	959199 MB	1	29	0.0116	0.0509	3/3/2010@11:43:39	
1202057095	LCS	1	30	1.00	9.79	3/3/2010@11:44:50	
247853003		1	31	0.0341	0.272	3/3/2010@11:46:04	5.00
1202057089	DUP	1	32	0.0331	0.263	3/3/2010@11:47:17	5.00
1202057092	PS	1	33	1.02	10.0	3/3/2010@11:48:30	5.00
247853006		1	34	0.196	1.87	3/3/2010@11:49:43	25.00
WTR100303-25	CCV	1	S10	0.968	9.47	3/3/2010@11:50:55	1.0 ppm CCV
		Known Conc:	1.00				
DQM Test: > + Concentration Limit							
		Result:	0.968 < 1.10				
		Message	CCV Passed				
		Action	Continue				
DQM Test: < - Concentration Limit							
		Result:	0.968 > 0.894				
		Message	CCV Passed				
		Action	Continue				
CCB	1	S15	0.00438	-0.0206	3/3/2010@11:53:16		CCB
		Known Conc:	0.00				
DQM Test: > + Concentration Limit							
		Result:	0.00438 < 0.0500				
		Message	CCB Passed				
		Action	Continue				
DQM Test: < - Concentration Limit							
		Result:	0.00438 > -0.0500				
		Message	CCB Passed				
		Action	Continue				
247853009		1	35	0.0177	0.110	3/3/2010@11:55:37	5.00
247853012		1	36	0.204	1.94	3/3/2010@11:56:49	10.00
247853015		1	37	0.219	2.09	3/3/2010@11:58:02	10.00
247853018		1	38	0.268	2.58	3/3/2010@11:59:14	50.00
247966003		1	39	-0.0241	-0.301	3/3/2010@12:00:27	5.00
1202057096	DUP	1	40	-0.0245	-0.305	3/3/2010@12:01:39	5.00
1202057097	PS	1	41	0.767	7.49	3/3/2010@12:02:51	5.00
247966011		1	42	-0.0241	-0.301	3/3/2010@12:04:03	5.00
248044005		1	43	0.00946	0.0294	3/3/2010@12:05:15	5.00
1202059915	DUP	1	89	0.00965	0.0313	3/3/2010@12:06:27	5.00
WTR100303-25	CCV	1	S10	0.981	9.60	3/3/2010@12:07:39	1.0 ppm CCV
		Known Conc:	1.00				
DQM Test: > + Concentration Limit							
		Result:	0.981 < 1.10				
		Message	CCV Passed				
		Action	Continue				
DQM Test: < - Concentration Limit							
		Result:	0.981 > 0.894				
		Message	CCV Passed				
		Action	Continue				
CCB	1	S15	0.00404	-0.0239	3/3/2010@12:10:01		CCB

Known Conc:		0.00					
DQM Test: > + Concentration Limit							
Result:		0.00404 < 0.0500					
Message		CCB Passed					
Action		Continue					
DQM Test: < - Concentration Limit							
Result:		0.00404 > -0.0500					
Message		CCB Passed					
Action		Continue					
1202059916 PS	1	90	1.04	10.2	3/3/2010@12:12:21	5.00	
248072001	1	44	0.170	1.61	3/3/2010@12:13:31	5.00	
1202057091 DUP	1	45	0.165	1.56	3/3/2010@12:14:43	5.00	
1202057094 PS	1	46	1.18	11.6	3/3/2010@12:15:56	5.00	
248072002	1	47	0.165	1.56	3/3/2010@12:17:09	5.00	
248072003	1	48	0.184	1.75	3/3/2010@12:18:23	5.00	
248103003	1	49	0.00535	-0.0110	3/3/2010@12:19:36	5.00	
248108001	1	50	-0.0372	-0.430	3/3/2010@12:20:48	5.00	
1202057090 DUP	1	51	-0.0370	-0.429	3/3/2010@12:22:01	5.00	
1202057093 PS	1	52	0.357	3.45	3/3/2010@12:23:13	5.00	
WTR100303-25 CCV	1	S10	1.01	9.89	3/3/2010@12:24:25		1.0 ppm CCV
Known Conc:		1.00					
DQM Test: > + Concentration Limit							
Result:		1.01 < 1.10					
Message		CCV Passed					
Action		Continue					
DQM Test: < - Concentration Limit							
Result:		1.01 > 0.894					
Message		CCV Passed					
Action		Continue					
CCB	1	S15	0.00458	-0.0186	3/3/2010@12:26:48		CCB
Known Conc:		0.00					
DQM Test: > + Concentration Limit							
Result:		0.00458 < 0.0500					
Message		CCB Passed					
Action		Continue					
DQM Test: < - Concentration Limit							
Result:		0.00458 > -0.0500					
Message		CCB Passed					
Action		Continue					
248117001	1	53	-0.0357	-0.415	3/3/2010@12:29:08	5.00	
248126003	1	54	0.138	1.29	3/3/2010@12:30:20	5.00	
248127001	1	55	0.126	1.17	3/3/2010@12:31:32	5.00	
248199001	1	56	-0.0330	-0.389	3/3/2010@12:32:44	5.00	
248238001	1	57	0.0119	0.0531	3/3/2010@12:33:56	5.00	
248238002	1	58	0.0133	0.0676	3/3/2010@12:35:08	5.00	
247966003	1	39	-0.0228	-0.288	3/3/2010@12:36:20	5.00	
1202057096 DUP	1	40	-0.0241	-0.301	3/3/2010@12:37:32	5.00	
1202057097 PS	1	41	0.737	7.19	3/3/2010@12:38:45	5.00	
248108001	1	50	0.00805	0.0156	3/3/2010@12:39:57	10.00	
WTR100303-25 CCV	1	S10	1.02	10.0	3/3/2010@12:41:09		1.0 ppm CCV
Known Conc:		1.00					
DQM Test: > + Concentration Limit							
Result:		1.02 < 1.10					
Message		CCV Passed					
Action		Continue					
DQM Test: < - Concentration Limit							
Result:		1.02 > 0.894					
Message		CCV Passed					
Action		Continue					
CCB	1	S15	0.00556	-0.00893	3/3/2010@12:43:31		CCB
Known Conc:		0.00					
DQM Test: > + Concentration Limit							
Result:		0.00556 < 0.0500					
Message		CCB Passed					
Action		Continue					
DQM Test: < - Concentration Limit							
Result:		0.00556 > -0.0500					
Message		CCB Passed					


- 5 -

		DQM Test: > + Concentration Limit						
Result:		0.994 < 1.10						
Message		CCV Passed						
Action		Continue						
		DQM Test: < - Concentration Limit						
Result:		0.994 > 0.894						
Message		CCV Passed						
Action		Continue						
CCB	1	S15	0.00455	-0.0189	3/3/2010@13:28:56			CCB
Known Conc:		0.00						
		DQM Test: > + Concentration Limit						
Result:		0.00455 < 0.0500						
Message		CCB Passed						
Action		Continue						
		DQM Test: < - Concentration Limit						
Result:		0.00455 > -0.0500						
Message		CCB Passed						
Action		Continue						

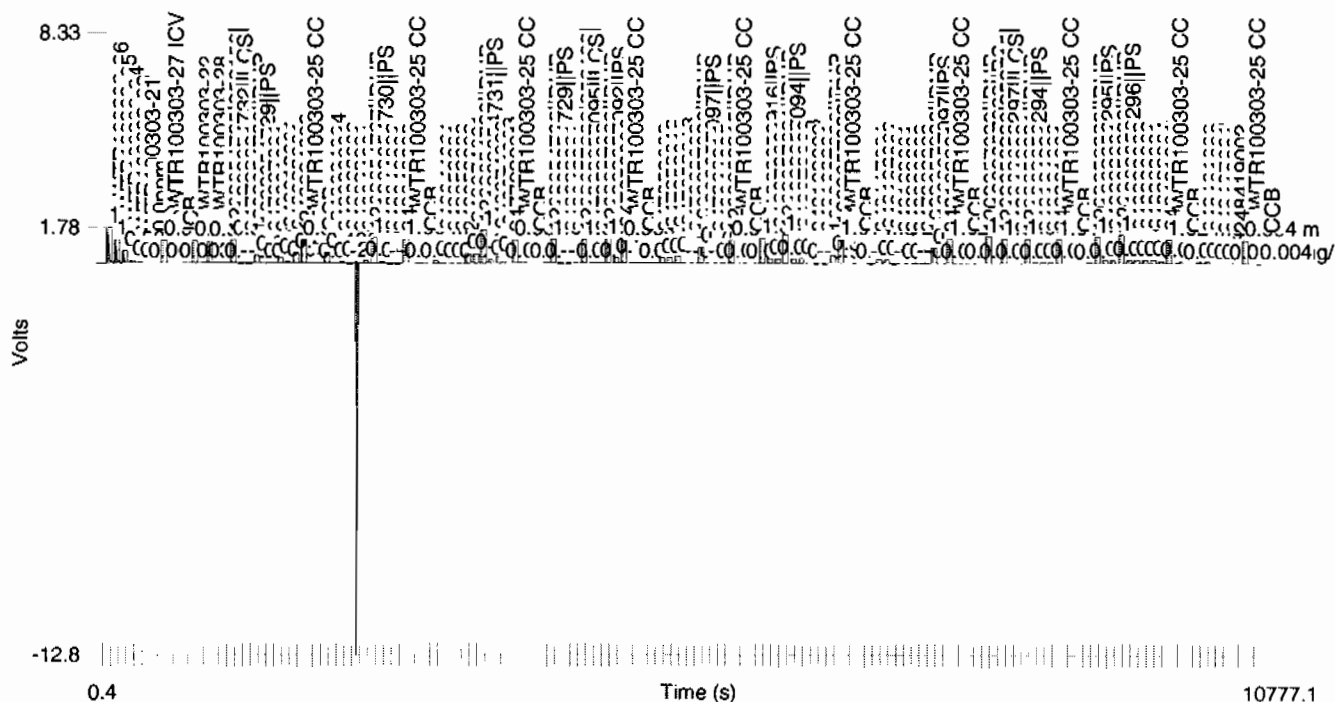Channel 1 (NO₃ + NO₂) : Current ViewTable 1: NO₃ + NO₂

	Conc. (mg/L)	Rep	Peak Area (Volt-s)	Peak Height (Volts)	% Residual	Detection Date	Detection Time
1	1.50	1	14.8	1.22	-0.4	3/3/2010	10:33:10
2	1.00	1	9.68	0.804	1.1	3/3/2010	10:34:23
3	0.500	1	4.89	0.403	-0.6	3/3/2010	10:35:35
4	0.100	1	1.02	0.0833	-10.8	3/3/2010	10:36:48
5	0.0500	1	0.312	0.0247	27.4	3/3/2010	10:38:02
6	0.00	1	-0.0280	-0.00133		3/3/2010	10:39:16

Figure 1: NO3 + NO2

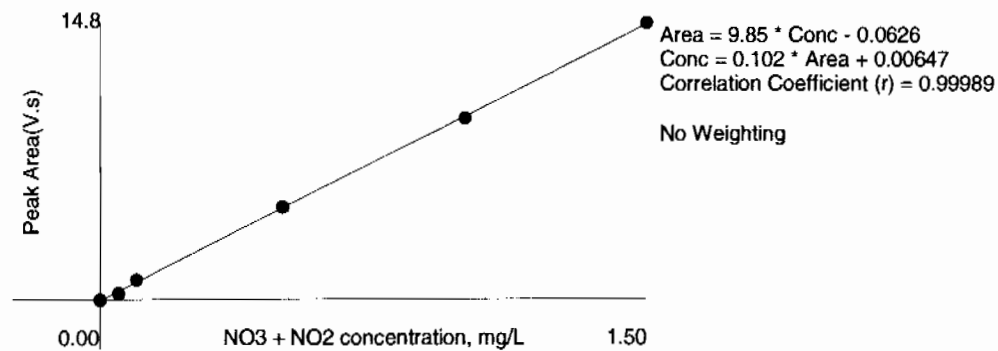

General Chemistry Analysis

Case Narrative

**General Chemistry Narrative
Los Alamos National Laboratory (LANL)
SDG 10-2093-1**

Method/Analysis Information

Product: pH
Analytical Batch: 959805 **Method:** SW9045C pH

Sample Analysis

The following samples were analyzed using the analytical protocol as established in SW846 9045C/9045D:

Sample ID	Client ID
248118001	RE36-10-8448
248118002	RE36-10-8456
248118003	RE36-10-8451
248118004	RE36-10-8450
248118005	RE36-10-8449
248118006	RE36-10-8453
248118007	RE36-10-8452
1202058593	248025004(CAPU-10-12541) Sample Duplicate (DUP)
1202058594	248110008(RE15-10-8397) Sample Duplicate (DUP)
1202058595	Laboratory Control Sample (LCS)

The samples in this SDG were analyzed on an "as received" basis.

SOP Reference

Procedure for preparation, analysis and reporting of analytical data are controlled by GEL Laboratories LLC as Standard Operating Procedure (SOP). The data discussed in this narrative has been analyzed in accordance with GL-GC-E-008 REV# 17.

Preparation/Analytical Method Verification

The SOP stated above has been prepared based on technical research and testing conducted by GEL Laboratories, LLC. and with guidance from the regulatory documents listed in this "Method/Analysis Information" section.

Calibration Information

The Electrode analysis was performed on a PerpHect pH Meter Orion 370.

Initial Calibration

All initial calibration requirements have been met for this SDG.

Calibration Verification Information (CCV)

All continuing calibration verification standards (CCVs) associated with reported data from this batch were within acceptance limits.

Quality Control (QC) Information

Laboratory Control Sample (LCS) Recovery

The LCS spike recovery met the acceptance limits.

Quality Control (QC) Designation

The following samples were selected for QC analysis: 248025004 (CAPU-10-12541) and 248110008 (RE15-10-8397).

Duplicate Relative Percent Difference (RPD) Statement

The RPD between the sample and its duplicate met the acceptance limits.

Technical Information

GEL assigns holding times based on the date and time of sample collection. Those holding times expressed in hours are calculated in the AlphaLims system by hours. Those holding times expressed as days expire at midnight on the day of expiration.

Holding Times

The following samples from this sample group were received by the lab outside of the method specified holding time: 248118001 (RE36-10-8448), 248118002 (RE36-10-8456), 248118003 (RE36-10-8451), 248118004 (RE36-10-8450), 248118005 (RE36-10-8449), 248118006 (RE36-10-8453) and 248118007 (RE36-10-8452).

Sample Re-analysis

The samples in this SDG did not require re-analysis.

Miscellaneous Information

Data Exception (DER) Documentation

A DER was not required for this SDG.

Additional Comments

Additional comments were not required for this SDG.

Electronic Packaging Comment

This data package was generated using an electronic data processing program referred to as virtual packaging. In an effort to increase quality and efficiency, the laboratory has developed systems to generate all data packages electronically. The following change from traditional packages should be noted: Analyst/peer reviewer initials and dates are not present on the electronic data files. Presently, all initials and dates are present on the original raw data. These hard copies are temporarily stored in the laboratory. The data validator will always sign and date the case narrative. Data that are not generated electronically, such as hand written pages, will be scanned and inserted into the electronic package.

Method/Analysis Information

Product: Cyanide, Total
Analytical Batch: 959204 **Method:** SW9012A Cyanide and Total
Prep Batch : 959203 **Method:** SSW846 9010B Prep

Sample Analysis

The following samples were analyzed using the analytical protocol as established in SW846 9012A:

Sample ID	Client ID
248118001	RE36-10-8448
248118002	RE36-10-8456
248118003	RE36-10-8451
248118004	RE36-10-8450
248118005	RE36-10-8449
248118006	RE36-10-8453
248118007	RE36-10-8452
1202057112	Method Blank (MB)
1202057113	248189001(RE11-10-1651) Sample Duplicate (DUP)
1202057114	248189002(RE11-10-1652) Sample Duplicate (DUP)
1202057115	248189001(RE11-10-1651) Matrix Spike (MS)
1202057116	248189002(RE11-10-1652) Matrix Spike (MS)
1202057117	248189001(RE11-10-1651) Matrix Spike Duplicate (MSD)
1202057118	248189002(RE11-10-1652) Matrix Spike Duplicate (MSD)
1202057119	Laboratory Control Sample (LCS)

The samples in this SDG were analyzed on a "dry weight" basis.

SOP Reference

Procedure for preparation, analysis and reporting of analytical data are controlled by GEL Laboratories LLC as Standard Operating Procedure (SOP). The data discussed in this narrative has been analyzed in accordance with GL-GC-E-095 REV# 12.

Preparation/Analytical Method Verification

The SOP stated above has been prepared based on technical research and testing conducted by GEL Laboratories, LLC. and with guidance from the regulatory documents listed in this "Method/Analysis Information" section.

Calibration Information

The Flow Injection analysis was performed on a Lachat QuickChem FIA+ 8000 Series.

Initial Calibration

All initial calibration requirements have been met for this SDG.

Continuing Calibration Blanks

All continuing calibration blanks (CCBs) associated with reported data from this batch were within acceptance limits.

Calibration Verification Information (CCV)

All continuing calibration verification standards (CCVs) associated with reported data from this batch were within acceptance limits.

Y Intercept Rule

The absolute value of the intercept is less than 3 times the MDL.

Quality Control (QC) Information**Method Blank (MB) Statement**

The MB analyzed with this SDG met the acceptance criteria.

Laboratory Control Sample (LCS) Recovery

The LCS spike recovery met the acceptance limits.

Quality Control (QC) Designation

The following samples were selected for QC analysis: 248189001 (RE11-10-1651) and 248189002 (RE11-10-1652).

Matrix Spike (MS)/Post Spike (PS) Recovery Statement

The MS/PS recoveries for this sample set were within the required acceptance limits.

Matrix Spike Duplicate (MSD) Recovery Statement

The MSD recoveries for this sample set were within the required acceptance limits.

MS/MSD Relative Percent Difference (RPD) Statement

The RPDs between the spike and spike duplicate met the acceptance limits.

Duplicate Relative Percent Difference (RPD) Statement

The values for the sample and duplicate are less than the Practical Quantitation Limit (PQL); therefore, the RPD is not applicable. 1202057114 (RE11-10-1652).

Technical Information

GEL assigns holding times based on the date and time of sample collection. Those holding times expressed in hours are calculated in the AlphaLims system by hours. Those holding times expressed as days expire at midnight on the day of expiration.

Holding Times

All samples in this SDG met the specified holding time.

Sample Preservation/Integrity

All the samples from this sample group met the preservation and integrity requirements of the method.

Sample Dilutions

The following sample in this sample group was diluted due to high concentration: 1202057119 (LCS).

Sample Re-analysis

The samples in this SDG did not require re-analysis.

Miscellaneous Information

Data Exception (DER) Documentation

A DER was not required for this SDG.

Additional Comments

Additional comments were not required for this SDG.

Electronic Packaging Comment

This data package was generated using an electronic data processing program referred to as virtual packaging. In an effort to increase quality and efficiency, the laboratory has developed systems to generate all data packages electronically. The following change from traditional packages should be noted:

Analyst/peer reviewer initials and dates are not present on the electronic data files. Presently, all initials and dates are present on the original raw data. These hard copies are temporarily stored in the laboratory. The data validator will always sign and date the case narrative. Data that are not generated electronically, such as hand written pages, will be scanned and inserted into the electronic package.

Method/Analysis Information

Product: Ion Chromatography
Analytical Batch: 962078 **Method:** EPA 300.0 Nitrate in Soil
Prep Batch : 962077 **Method:** EPA 300.0 PREP

Sample Analysis

The following samples were analyzed using the analytical protocol as established in EPA 300.0:

Sample ID	Client ID
248118001	RE36-10-8448
248118002	RE36-10-8456
248118003	RE36-10-8451
248118004	RE36-10-8450
248118005	RE36-10-8449
248118006	RE36-10-8453
248118007	RE36-10-8452
1202063606	Method Blank (MB)
1202063607	248110001(RE15-10-8404) Sample Duplicate (DUP)
1202063608	248118007(RE36-10-8452) Sample Duplicate (DUP)
1202063609	248110001(RE15-10-8404) Matrix Spike (MS)
1202063610	248118007(RE36-10-8452) Matrix Spike (MS)
1202063611	248110001(RE15-10-8404) Matrix Spike Duplicate (MSD)
1202063612	248118007(RE36-10-8452) Matrix Spike Duplicate (MSD)
1202063613	Laboratory Control Sample (LCS)

The samples in this SDG were analyzed on a "dry weight" basis.

SOP Reference

Procedure for preparation, analysis and reporting of analytical data are controlled by GEL Laboratories LLC as Standard Operating Procedure (SOP). The data discussed in this narrative has been analyzed in accordance with GL-GC-E-086 REV# 17.

Preparation/Analytical Method Verification

The SOP stated above has been prepared based on technical research and testing conducted by GEL Laboratories, LLC. and with guidance from the regulatory documents listed in this "Method/Analysis Information" section.

Calibration Information

The Ion Chromatography analysis was performed on a Dionex ICS-3000 Ion Chromatograph.

Initial Calibration

All initial calibration requirements have been met for this SDG.

Continuing Calibration Blanks

All continuing calibration blanks (CCBs) associated with reported data from this batch were within acceptance limits.

Calibration Verification Information (CCV)

All continuing calibration verification standards (CCVs) associated with reported data from this batch were within acceptance limits.

Y Intercept Rule

The absolute value of the intercept is less than 3 times the MDL.

Quality Control (QC) Information**Method Blank (MB) Statement**

The MB analyzed with this SDG met the acceptance criteria.

Laboratory Control Sample (LCS) Recovery

The LCS spike recovery met the acceptance limits.

Quality Control (QC) Designation

The following samples were selected for QC analysis: 248110001 (RE15-10-8404) and 248118007 (RE36-10-8452).

Matrix Spike (MS)/Post Spike (PS) Recovery Statement

The spike recovery falls outside of the GEL acceptance limits but within the client specified limits. 1202063609 (RE15-10-8404).

Matrix Spike Duplicate (MSD) Recovery Statement

The spike duplicate recovery falls outside of the GEL acceptance limits but within the client specified limits. 1202063611 (RE15-10-8404).

MS/MSD Relative Percent Difference (RPD) Statement

The RPDs between the spike and spike duplicate met the acceptance limits.

Duplicate Relative Percent Difference (RPD) Statement

The RPD between the sample and its duplicate met the acceptance limits.

Technical Information

GEL assigns holding times based on the date and time of sample collection. Those holding times expressed in hours are calculated in the AlphaLims system by hours. Those holding times expressed as days expire at midnight on the day of expiration.

Holding Times

All samples in this SDG met the specified holding time.

Sample Dilutions

The samples in this SDG did not require dilutions.

Sample Re-analysis

The samples in this SDG did not require re-analysis.

Miscellaneous Information**Data Exception (DER) Documentation**

The following DER was generated for this SDG: 808585 1202063609 (RE15-10-8404), 1202063611 (RE15-10-8404), 248118001 (RE36-10-8448), 248118002 (RE36-10-8456), 248118003 (RE36-10-8451), 248118004 (RE36-10-8450), 248118005 (RE36-10-8449), 248118006 (RE36-10-8453) and 248118007 (RE36-10-8452).

Manual Integrations

Manual integrations were not required for the samples in this SDG.

Additional Comments

Additional comments were not required for this SDG.

Electronic Packaging Comment

This data package was generated using an electronic data processing program referred to as virtual packaging. In an effort to increase quality and efficiency, the laboratory has developed systems to generate all data packages electronically. The following change from traditional packages should be noted:

Analyst/peer reviewer initials and dates are not present on the electronic data files. Presently, all initials and dates are present on the original raw data. These hard copies are temporarily stored in the laboratory. The data validator will always sign and date the case narrative. Data that are not generated electronically, such as hand written pages, will be scanned and inserted into the electronic package.

Certification Statement

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless otherwise noted in the analytical case narrative.

Review Validation:

GEL requires all analytical data to be verified by a qualified data validator. In addition, all data designated for CLP or CLP-like packaging will receive a third level validation upon completion of the data package.

The following data validator verified the information presented in this case narrative:

Reviewer: Nick-Cole A. Emore Date: 3.24.10

Sample Data Summary

GEL LABORATORIES LLC

2040 Savage Road Charleston SC 29407 - (843) 556-8171 - www.gel.com

Certificate of Analysis Report for

LANL010 Los Alamos National Laboratory (72733-001-09)

Client SDG: 10-2093-1 GEL Work Order: 248118

The Qualifiers in this report are defined as follows:

- * Indicates that a quality control analyte recovery is outside of specified acceptance criteria.
- ** Indicates the analyte is a surrogate compound.

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless qualified on the Certificate of Analysis.

The designation ND, if present, appears in the result column when the analyte concentration is not detected above the detection limit.

This data report has been prepared and reviewed in accordance with GEL Laboratories LLC standard operating procedures. Please direct any questions to your Project Manager, Valerie Davis.

Reviewed by

4 Nick-Cole A. Elmore 3.24.10

GEL LABORATORIES LLC

2040 Savage Road Charleston SC 29407 - (843) 556-8171 - www.gel.com

Certificate of Analysis

Company : Los Alamos National Laboratory
Address : PO Box 1663
TA-03, SM271, Drop Pt. 02U, Rm111
Los Alamos, New Mexico 87545
Contact: Ms. Joylene Valdez
Project: LANL ER Project

Report Date: March 24, 2010

Client SDG: 10-2093-1

Client Sample ID: RE36-10-8448
Sample ID: 248118001
Matrix: R
Collect Date: 22-FEB-10 12:00
Receive Date: 26-FEB-10
Collector: Client
Moisture: 2.66%

Project: LANL01004
Client ID: LANL010

Parameter	Qualifier	Result	DL	RL	Units	DF	Analyst	Date	Time	Batch	Method
Electrode Analysis											
<i>SW9045C pH "As Received"</i>											
pH at Temp 19.8C	H	8.45	0.010	0.100	SU	1	LXA1	03/02/10	1250	959805	1
Flow Injection Analysis											
<i>SW9012A Cyanide, Total "Dry Weight Corrected"</i>											
Cyanide, Total	U	ND	64.7	238	ug/kg	1	AXC2	03/08/10	1554	959204	2
Ion Chromatography											
<i>EPA 300.0 Nitrate in Soil "Dry Weight Corrected"</i>											
Nitrate-N	U	ND	0.308	1.03	mg/kg	1	MAR1	03/21/10	1440	962078	3

The following Prep Methods were performed

Method	Description	Analyst	Date	Time	Prep Batch
EPA 300.0 PREP	EPA 300.0 Total Anions in Soil	MAR1	03/19/10	1315	962077
SW846 9010B Prep	SW846 9010B Prep	AXS5	03/08/10	1243	959203

The following Analytical Methods were performed

Method	Description	Analyst Comments
1	SW846 9045C/9045D	
2	SW846 9012A	
3	EPA 300.0	

GEL LABORATORIES LLC

2040 Savage Road Charleston SC 29407 - (843) 556-8171 - www.gel.com

Certificate of Analysis

Company : Los Alamos National Laboratory
Address : PO Box 1663
TA-03, SM271, Drop Pt. 02U, Rm111
Los Alamos, New Mexico 87545
Contact: Ms. Joylene Valdez
Project: LANL ER Project

Report Date: March 24, 2010

Client SDG: 10-2093-1

Client Sample ID: RE36-10-8456
Sample ID: 248118002
Matrix: R
Collect Date: 22-FEB-10 12:00
Receive Date: 26-FEB-10
Collector: Client
Moisture: 2.81%

Project: LANL01004
Client ID: LANL010

Parameter	Qualifier	Result	DL	RL	Units	DF	Analyst	Date	Time	Batch	Method
Electrode Analysis											
<i>SW9045C pH "As Received"</i>											
pH at Temp 19.7C	H	8.26	0.010	0.100	SU	1	LXA1	03/02/10	1250	959805	1
Flow Injection Analysis											
<i>SW9012A Cyanide, Total "Dry Weight Corrected"</i>											
Cyanide, Total	U	ND	66.0	243	ug/kg	1	AXC2	03/08/10	1555	959204	2
Ion Chromatography											
<i>EPA 300.0 Nitrate in Soil "Dry Weight Corrected"</i>											
Nitrate-N	U	ND	0.309	1.03	mg/kg	1	MAR1	03/21/10	1507	962078	3

The following Prep Methods were performed

Method	Description	Analyst	Date	Time	Prep Batch
EPA 300.0 PREP	EPA 300.0 Total Anions in Soil	MAR1	03/19/10	1315	962077
SW846 9010B Prep	SW846 9010B Prep	AXS5	03/08/10	1243	959203

The following Analytical Methods were performed

Method	Description	Analyst Comments
1	SW846 9045C/9045D	
2	SW846 9012A	
3	EPA 300.0	

GEL LABORATORIES LLC

2040 Savage Road Charleston SC 29407 - (843) 556-8171 - www.gel.com

Certificate of Analysis

Company : Los Alamos National Laboratory
Address : PO Box 1663
TA-03, SM271, Drop Pt. 02U, Rm111
Los Alamos, New Mexico 87545
Contact: Ms. Joylene Valdez
Project: LANL ER Project

Report Date: March 24, 2010

Client SDG: 10-2093-1

Client Sample ID: RE36-10-8451
Sample ID: 248118003
Matrix: R
Collect Date: 22-FEB-10 12:00
Receive Date: 26-FEB-10
Collector: Client
Moisture: 3.01%

Project: LANL01004
Client ID: LANL010

Parameter	Qualifier	Result	DL	RL	Units	DF	Analyst	Date	Time	Batch	Method
Electrode Analysis											
<i>SW9045C pH "As Received"</i>											
pH at Temp 20.0C	H	7.92	0.010	0.100	SU	1	LXA1	03/02/10	1250	959805	1
Flow Injection Analysis											
<i>SW9012A Cyanide, Total "Dry Weight Corrected"</i>											
Cyanide, Total	U	ND	68.7	253	ug/kg	1	AXC2	03/08/10	1556	959204	2
Ion Chromatography											
<i>EPA 300.0 Nitrate in Soil "Dry Weight Corrected"</i>											
Nitrate-N	U	ND	0.309	1.03	mg/kg	1	MAR1	03/21/10	1534	962078	3

The following Prep Methods were performed

Method	Description	Analyst	Date	Time	Prep Batch
EPA 300.0 PREP	EPA 300.0 Total Anions in Soil	MAR1	03/19/10	1315	962077
SW846 9010B Prep	SW846 9010B Prep	AXS5	03/08/10	1243	959203

The following Analytical Methods were performed

Method	Description	Analyst Comments
1	SW846 9045C/9045D	
2	SW846 9012A	
3	EPA 300.0	

GEL LABORATORIES LLC

2040 Savage Road Charleston SC 29407 - (843) 556-8171 - www.gel.com

Certificate of Analysis

Company : Los Alamos National Laboratory
Address : PO Box 1663
TA-03, SM271, Drop Pt. 02U, Rm111
Los Alamos, New Mexico 87545
Contact: Ms. Joylene Valdez
Project: LANL ER Project

Report Date: March 24, 2010

Client SDG: 10-2093-1

Client Sample ID: RE36-10-8450
Sample ID: 248118004
Matrix: R
Collect Date: 22-FEB-10 12:00
Receive Date: 26-FEB-10
Collector: Client
Moisture: 14.9%

Project: LANL01004
Client ID: LANL010

Parameter	Qualifier	Result	DL	RL	Units	DF	Analyst	Date	Time	Batch	Method
Electrode Analysis											
<i>SW9045C pH "As Received"</i>											
pH at Temp 19.9C	H	8.07	0.010	0.100	SU	1	LXA1	03/02/10	1250	959805	1
Flow Injection Analysis											
<i>SW9012A Cyanide, Total "Dry Weight Corrected"</i>											
Cyanide, Total	U	ND	79.9	294	ug/kg	1	AXC2	03/08/10	1557	959204	2
Ion Chromatography											
<i>EPA 300.0 Nitrate in Soil "Dry Weight Corrected"</i>											
Nitrate-N	U	ND	0.353	1.18	mg/kg	1	MAR1	03/21/10	1601	962078	3

The following Prep Methods were performed

Method	Description	Analyst	Date	Time	Prep Batch
EPA 300.0 PREP	EPA 300.0 Total Anions in Soil	MAR1	03/19/10	1315	962077
SW846 9010B Prep	SW846 9010B Prep	AXS5	03/08/10	1243	959203

The following Analytical Methods were performed

Method	Description	Analyst Comments
1	SW846 9045C/9045D	
2	SW846 9012A	
3	EPA 300.0	

GEL LABORATORIES LLC

2040 Savage Road Charleston SC 29407 - (843) 556-8171 - www.gel.com

Certificate of Analysis

Company : Los Alamos National Laboratory
Address : PO Box 1663
TA-03, SM271, Drop Pt. 02U, Rm111
Los Alamos, New Mexico 87545
Contact: Ms. Joylene Valdez
Project: LANL ER Project

Report Date: March 24, 2010

Client SDG: 10-2093-1

Client Sample ID: RE36-10-8449
Sample ID: 248118005
Matrix: R
Collect Date: 22-FEB-10 12:00
Receive Date: 26-FEB-10
Collector: Client
Moisture: 1.76%

Project: LANL01004
Client ID: LANL010

Parameter	Qualifier	Result	DL	RL	Units	DF	Analyst	Date	Time	Batch	Method
Electrode Analysis											
<i>SW9045C pH "As Received"</i>											
pH at Temp 20.0C	H	8.62	0.010	0.100	SU	1	LXA1	03/02/10	1250	959805	1
Flow Injection Analysis											
<i>SW9012A Cyanide, Total "Dry Weight Corrected"</i>											
Cyanide, Total	U	ND	66.6	245	ug/kg	1	AXC2	03/08/10	1558	959204	2
Ion Chromatography											
<i>EPA 300.0 Nitrate in Soil "Dry Weight Corrected"</i>											
Nitrate-N	U	ND	0.305	1.02	mg/kg	1	MAR1	03/21/10	1627	962078	3

The following Prep Methods were performed

Method	Description	Analyst	Date	Time	Prep Batch
EPA 300.0 PREP	EPA 300.0 Total Anions in Soil	MAR1	03/19/10	1315	962077
SW846 9010B Prep	SW846 9010B Prep	AXS5	03/08/10	1243	959203

The following Analytical Methods were performed

Method	Description	Analyst Comments
1	SW846 9045C/9045D	
2	SW846 9012A	
3	EPA 300.0	

GEL LABORATORIES LLC

2040 Savage Road Charleston SC 29407 - (843) 556-8171 - www.gel.com

Certificate of Analysis

Company : Los Alamos National Laboratory
Address : PO Box 1663
TA-03, SM271, Drop Pt. 02U, Rm111
Los Alamos, New Mexico 87545
Contact: Ms. Joylene Valdez
Project: LANL ER Project

Report Date: March 24, 2010

Client SDG: 10-2093-1

Client Sample ID: RE36-10-8453
Sample ID: 248118006
Matrix: R
Collect Date: 22-FEB-10 12:00
Receive Date: 26-FEB-10
Collector: Client
Moisture: 4.28%

Project: LANL01004
Client ID: LANL010

Parameter	Qualifier	Result	DL	RL	Units	DF	Analyst	Date	Time	Batch	Method
Electrode Analysis											
<i>SW9045C pH "As Received"</i>											
pH at Temp 20.1C	H	8.60	0.010	0.100	SU	1	LXA1	03/02/10	1252	959805	1
Flow Injection Analysis											
<i>SW9012A Cyanide, Total "Dry Weight Corrected"</i>											
Cyanide, Total	U	ND	61.2	225	ug/kg	1	AXC2	03/08/10	1559	959204	2
Ion Chromatography											
<i>EPA 300.0 Nitrate in Soil "Dry Weight Corrected"</i>											
Nitrate-N	U	ND	0.313	1.04	mg/kg	1	MAR103/21/10	1748	962078		3

The following Prep Methods were performed

Method	Description	Analyst	Date	Time	Prep Batch
EPA 300.0 PREP	EPA 300.0 Total Anions in Soil	MAR1	03/19/10	1315	962077
SW846 9010B Prep	SW846 9010B Prep	AXS5	03/08/10	1243	959203

The following Analytical Methods were performed

Method	Description	Analyst Comments
1	SW846 9045C/9045D	
2	SW846 9012A	
3	EPA 300.0	

GEL LABORATORIES LLC

2040 Savage Road Charleston SC 29407 - (843) 556-8171 - www.gel.com

Certificate of Analysis

Company : Los Alamos National Laboratory
Address : PO Box 1663
TA-03, SM271, Drop Pt. 02U, Rm111
Los Alamos, New Mexico 87545
Contact: Ms. Joylene Valdez
Project: LANL ER Project

Report Date: March 24, 2010

Client SDG: 10-2093-1

Client Sample ID: RE36-10-8452
Sample ID: 248118007
Matrix: R
Collect Date: 22-FEB-10 12:00
Receive Date: 26-FEB-10
Collector: Client
Moisture: 7.14%

Project: LANL01004
Client ID: LANL010

Parameter	Qualifier	Result	DL	RL	Units	DF	Analyst	Date	Time	Batch	Method
Electrode Analysis											
<i>SW9045C pH "As Received"</i>											
pH at Temp 20.1C	H	8.23	0.010	0.100	SU	1	LXA1	03/02/10	1253	959805	1
Flow Injection Analysis											
<i>SW9012A Cyanide, Total "Dry Weight Corrected"</i>											
Cyanide, Total	U	ND	63.1	232	ug/kg	1	AXC2	03/08/10	1600	959204	2
Ion Chromatography											
<i>EPA 300.0 Nitrate in Soil "Dry Weight Corrected"</i>											
Nitrate-N	U	ND	0.323	1.08	mg/kg	1	MAR103/21/10	1815	962078		3

The following Prep Methods were performed

Method	Description	Analyst	Date	Time	Prep Batch
EPA 300.0 PREP	EPA 300.0 Total Anions in Soil	MAR1	03/19/10	1315	962077
SW846 9010B Prep	SW846 9010B Prep	AXS5	03/08/10	1243	959203

The following Analytical Methods were performed

Method	Description	Analyst Comments
1	SW846 9045C/9045D	
2	SW846 9012A	
3	EPA 300.0	

Quality Control Summary

GEL LABORATORIES LLC

2040 Savage Road Charleston, SC 29407 - (843) 556-8171 - www.gel.com

QC Summary

Report Date: March 24, 2010

Page 1 of 3

Los Alamos National Laboratory
PO Box 1663
TA-03, SM271, Drop Pt. 02U, Rm111
Los Alamos, New Mexico
Contact: Ms. Joylene Valdez

Workorder: 248118

Parmname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
Electrode Analysis											
Batch	959805										
QC1202058593	248025004	DUP									
pH		H	9.76	H	9.73	SU	0.308	(0%-10%)	LXA1	03/02/10	12:50
QC1202058594	248110008	DUP									
pH		H	8.67	H	8.57	SU	1.16	(0%-10%)		03/02/10	12:50
QC1202058595	LCS										
pH	7.00				6.99	SU	99.9	(95%-105%)		03/02/10	12:50
Flow Injection Analysis											
Batch	959204										
QC1202057113	248189001	DUP									
Cyanide, Total		J	86.4	U	ND	ug/kg	200 ^		AXC2	03/08/10	16:02
QC1202057114	248189002	DUP									
Cyanide, Total		U	ND	U	ND	ug/kg	N/A			03/08/10	16:09
QC1202057119	LCS										
Cyanide, Total	67900				77800	ug/kg	115	(32%-157%)		03/08/10	15:43
QC1202057112	MB										
Cyanide, Total				U	250	ug/kg				03/08/10	15:42
QC1202057115	248189001	MS									
Cyanide, Total	5560	J	86.4		5470	ug/kg	96.8	(26%-158%)		03/08/10	16:02
QC1202057116	248189002	MS									
Cyanide, Total	6600	U	ND		6200	ug/kg	93.4	(26%-158%)		03/08/10	16:10
QC1202057117	248189001	MSD									
Cyanide, Total	5870	J	86.4		5730	ug/kg	4.60	(0%-30%)		03/08/10	16:07
QC1202057118	248189002	MSD									
Cyanide, Total	6150	U	ND		5770	ug/kg	7.14	(0%-30%)		03/08/10	16:11
Ion Chromatography											
Batch	962078										
QC1202063607	248110001	DUP									
Nitrate-N			1.62		1.60	mg/kg	1.10 ^	(+/-1.10)	MAR1	03/20/10	11:37
QC1202063608	248118007	DUP									
Nitrate-N		U	ND	U	ND	mg/kg	N/A			03/21/10	18:42
QC1202063613	LCS										
Nitrate-N	50.0				46.9	mg/kg	93.9	(90%-110%)		03/20/10	10:43
QC1202063606	MB										
Nitrate-N				U	1.00	mg/kg				03/20/10	10:16
QC1202063609	248110001	MS									
Nitrate-N	55.2		1.62		50.5	mg/kg	88.5 *	(90%-110%)		03/20/10	12:04
QC1202063610	248118007	MS									
Nitrate-N	53.8	U	ND		49.2	mg/kg	91.3	(90%-110%)		03/21/10	19:09
QC1202063611	248110001	MSD									
Nitrate-N	55.2		1.62		50.4	mg/kg	0.287	(0%-20%)		03/20/10	12:31
QC1202063612	248118007	MSD									
Nitrate-N	53.8	U	ND		49.3	mg/kg	0.262	(0%-20%)		03/21/10	19:36

GEL LABORATORIES LLC

2040 Savage Road Charleston, SC 29407 - (843) 556-8171 - www.gel.com

QC Summary

Workorder: 248118

Page 2 of 3

Parmname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
----------	-----	--------	------	----	-------	------	------	-------	-------	------	------

Notes:

RER is calculated at the 95% confidence level (2-sigma).

The Qualifiers in this report are defined as follows:

- ** Analyte is a surrogate compound
- < Result is less than value reported
- > Result is greater than value reported
- A The TIC is a suspected aldol-condensation product
- B For General Chemistry and Organic analysis the target analyte was detected in the associated blank.
- BD Results are either below the MDC or tracer recovery is low
- C Analyte has been confirmed by GC/MS analysis
- D Results are reported from a diluted aliquot of the sample
- E General Chemistry--Concentration of the target analyte exceeds the instrument calibration range
- E Metals--%difference of sample and SD is >10%. Sample concentration must meet flagging criteria
- E Organics--Concentration of the target analyte exceeds the instrument calibration range
- F Estimated Value
- H Analytical holding time was exceeded
- J Value is estimated
- M M if above MDC and less than LLD
- M Matrix Related Failure
- N Organics--Presumptive evidence based on mass spectral library search to make a tentative identification of the analyte (TIC). Quantitation is based on nearest internal standard response factor
- N/A RPD or %Recovery limits do not apply.
- ND Analyte concentration is not detected above the detection limit
- NJ Consult Case Narrative, Data Summary package, or Project Manager concerning this qualifier
- P Organics--The concentrations between the primary and confirmation columns/detectors is >40% different. For HPLC, difference is also <70%
- R Sample results are rejected
- U Analyte was analyzed for, but not detected above the MDL, MDA, or LOD.
- UI Gamma Spectroscopy--Uncertain identification
- UJ Gamma Spectroscopy--Uncertain identification
- X Consult Case Narrative, Data Summary package, or Project Manager concerning this qualifier
- Y QC Samples were not spiked with this compound
- Z Paint Filter Test--Particulates passed through the filter, however no free liquids were observed.
- ^ RPD of sample and duplicate evaluated using +/-RL. Concentrations are <5X the RL. Qualifier Not Applicable for Radiochemistry.
- d 5-day BOD--The 2:1 depletion requirement was not met for this sample
- h Preparation or preservation holding time was exceeded

GEL LABORATORIES LLC

2040 Savage Road Charleston, SC 29407 - (843) 556-8171 - www.gel.com

QC Summary

Workorder: 248118

Page 3 of 3

Parmname	NOM	Sample	Qual	QC	Units	RPD%	REC%	Range	Anlst	Date	Time
----------	-----	--------	------	----	-------	------	------	-------	-------	------	------

N/A indicates that spike recovery limits do not apply when sample concentration exceeds spike conc. by a factor of 4 or more.

^ The Relative Percent Difference (RPD) obtained from the sample duplicate (DUP) is evaluated against the acceptance criteria when the sample is greater than five times (5X) the contract required detection limit (RL). In cases where either the sample or duplicate value is less than 5X the RL, a control limit of +/- the RL is used to evaluate the DUP result.

* Indicates that a Quality Control parameter was not within specifications.

For PS, PSD, and SDILT results, the values listed are the measured amounts, not final concentrations.

Where the analytical method has been performed under NELAP certification, the analysis has met all of the requirements of the NELAC standard unless qualified on the QC Summary.

Instrument QC Data Summary

INITIAL AND CONTINUING CALIBRATION VERIFICATION

Report Run On: 24-MAR-2010 12:19

GEL Laboratories LLC

Contract: LANL01004

SDG #: 10-2093-1

Flow Injection Analysis

Method: SW846 9012A

Concentration Units:ug/L

Instrument: Lachat QuickChem FIA+ 8000 Series

Parmname: Cyanide, Total

Sample Type	Run Date	Data File	Result	Nominal	Recovery	Limits	Within Limits
ICV	08-MAR-2010 10:32:54	OM_3-8-2010_10-24-48	147	150	98	(90%-110%)	Yes
CCV	08-MAR-2010 15:38:47	OM_3-8-2010_14-58-05	104	100	104	(90%-110%)	Yes
CCV	08-MAR-2010 15:51:19	OM_3-8-2010_14-58-05	106	100	106	(90%-110%)	Yes
CCV	08-MAR-2010 16:03:48	OM_3-8-2010_14-58-05	106	100	106	(90%-110%)	Yes
CCV	08-MAR-2010 16:16:17	OM_3-8-2010_14-58-05	106	100	106	(90%-110%)	Yes

Sample Type	Run Date	Data File	Result	Limits	Within Limits
ICB	08-MAR-2010 10:34:44	OM_3-8-2010_10-24-48	-1.65	10	Yes
CCB	08-MAR-2010 15:40:39	OM_3-8-2010_14-58-05	-0.768	10	Yes
CCB	08-MAR-2010 15:53:09	OM_3-8-2010_14-58-05	-1.95	10	Yes
CCB	08-MAR-2010 16:05:39	OM_3-8-2010_14-58-05	-2.33	10	Yes
CCB	08-MAR-2010 16:18:09	OM_3-8-2010_14-58-05	-2.61	10	Yes

INITIAL AND CONTINUING CALIBRATION VERIFICATION

Report Run On: 24-MAR-2010 12:19

GEL Laboratories LLC

Contract: LANL01004

SDG #: 10-2093-1

Ion Chromatography

Method: EPA 300.0

Concentration Units:mg/L

Instrument: Dionex ICS-3000 Ion Chromatograph

Parmname: Nitrate-N

Sample Type	Run Date	Data File	Result	Nominal	Recovery	Limits	Within Limits
ICV	19-MAR-2010 10:31:00	100319	4.6689	5	93.4	(90%-110%)	Yes
CCV	20-MAR-2010 09:23:00	100319	7.2587	7.5	96.8	(90%-110%)	Yes
CCV	20-MAR-2010 14:45:00	100319	4.674	5	93.5	(90%-110%)	Yes
ICV	21-MAR-2010 11:32:00	100321	4.6626	5	93.3	(90%-110%)	Yes
CCV	21-MAR-2010 16:54:00	100321	7.264	7.5	96.9	(90%-110%)	Yes
CCV	21-MAR-2010 20:03:00	100321	4.7008	5	94	(90%-110%)	Yes

Sample Type	Run Date	Data File	Result	Limits	Within Limits
ICB	19-MAR-2010 10:58:00	100319	0	0.1	Yes
CCB	20-MAR-2010 09:49:00	100319	0	0.1	Yes
CCB	20-MAR-2010 15:12:00	100319	0	0.1	Yes
ICB	21-MAR-2010 12:53:00	100321	0	0.1	Yes
CCB	21-MAR-2010 17:21:00	100321	0	0.1	Yes
CCB	21-MAR-2010 20:30:00	100321	0	0.1	Yes

Cyanide, Total

Prep Logbook

Cyanide Sample Distillation

Batch ID:	959203.0	Verified by:		Type	Sample Id	Description	Serial Number	Spike Amount	Spike Units
Analyst:	Alan Stanley			LCS	1202057119	Total Cyanide Solid LCS	URF1200957-01	.25	g
Method:	SW846 9010B Prep			MS	1202057115	Secondary source standard for CN and phenol. Used to spike LCS, MS, ICV	URF1269274-02	.025	mL
Lab SOP:	GL-GC-E-067 REV# 13			MS	1202057116	Secondary source standard for CN and phenol. Used to spike LCS, MS, ICV	URF1269274-02	.025	mL
Instrument:	Sartorius Balance B-001			MSD	1202057117	Secondary source standard for CN and phenol. Used to spike LCS, MS, ICV	URF1269274-02	.025	mL
				MSD	1202057118	Secondary source standard for CN and phenol. Used to spike LCS, MS, ICV	URF1269274-02	.025	mL

Sample ID	Run Date	Matrix	Initial Weight (g)	Final Volume (mL)	Prep Factor (mL/g)	pH Check 1
1202057112 MB	08-MAR-2010 12:43:00	Soil	0.5	25	50	>12
1202057119 LCS	08-MAR-2010 12:43:00	Soil	0.25	25	100	>12
248110001	08-MAR-2010 12:43:00	Soil	0.52	25	48.07692	>12
248110002	08-MAR-2010 12:43:00	Soil	0.5	25	50	>12
248110003	08-MAR-2010 12:43:00	Soil	0.51	25	49.01961	>12
248110004	08-MAR-2010 12:43:00	Soil	0.51	25	49.01961	>12
248110005	08-MAR-2010 12:43:00	Soil	0.53	25	47.16981	>12
248110006	08-MAR-2010 12:43:00	Soil	0.51	25	49.01961	>12
248110007	08-MAR-2010 12:43:00	Soil	0.56	25	44.64286	>12
248110008	08-MAR-2010 12:43:00	Soil	0.51	25	49.01961	>12
248118001	08-MAR-2010 12:43:00	Soil	0.54	25	46.2963	>12
248118002	08-MAR-2010 12:43:00	Soil	0.53	25	47.16981	>12
248118003	08-MAR-2010 12:43:00	Soil	0.51	25	49.01961	>12
248118004	08-MAR-2010 12:43:00	Soil	0.5	25	50	>12
248118005	08-MAR-2010 12:43:00	Soil	0.52	25	48.07692	>12
248118006	08-MAR-2010 12:43:00	Soil	0.58	25	43.10345	>12
248118007	08-MAR-2010 12:43:00	Soil	0.58	25	43.10345	>12
248189001	08-MAR-2010 12:43:00	Soil	0.56	25	44.64286	>12
1202057113 DUP (248189001)	08-MAR-2010 12:43:00	Soil	0.55	25	45.45455	>12
1202057115 MS (248189001)	08-MAR-2010 12:43:00	Soil	0.58	25	43.10345	>12
1202057117 MSD (248189001)	08-MAR-2010 12:43:00	Soil	0.55	25	45.45455	>12

Analytical Logbook version 1 11-04-2002

GEL Laboratories LLC

Prep Logbook

Batch ID: 959203.0
Analyst: Alan Stanley
Method: SW846 9010B Prep
Lab SOP: GL-GC-E-067 REV# 13
Instrument: Sartorius Balance B-001

Type	Sample Id	Description	Serial Number	Spike Amount	Spike Units
LCS	1202057119	Total Cyanide Solid LCS	URF1200957-01	.25	g
MS	1202057115	Secondary source standard for CN and phenol. Used to spike LCS, MS, ICV	URF1269274-02	.025	mL
MS	1202057116	Secondary source standard for CN and phenol. Used to spike LCS, MS, ICV	URF1269274-02	.025	mL
MSD	1202057117	Secondary source standard for CN and phenol. Used to spike LCS, MS, ICV	URF1269274-02	.025	mL
MSD	1202057118	Secondary source standard for CN and phenol. Used to spike LCS, MS, ICV	URF1269274-02	.025	mL

Sample ID	Run Date	Matrix	Initial Weight (g)	Final Volume (mL)	Prep Factor (mL/g)	pH Check 1
248189002	08-MAR-2010 12:43:00	Soil	0.53	25	47.16981	>12
1202057114 DUP (248189002)	08-MAR-2010 12:43:00	Soil	0.58	25	43.10345	>12
1202057116 MS (248189002)	08-MAR-2010 12:43:00	Soil	0.54	25	46.2963	>12
1202057118 MSD (248189002)	08-MAR-2010 12:43:00	Soil	0.58	25	43.10345	>12

Reagent/Solvent Lot ID Description Amount Comments:

1260189-C	50% H2SO4 CN Prep	2.5 mL	
1270661-C	Bismuth Nitrate Solution	1.25 mL	
1270663-C	0.8N H3NO3S	1.25 mL	
1270669-C	51% MgCl2 Soln	1 mL	
1273851-C	0.25N Sodium Hydroxide Solution	25 mL	
WCN100308-07	150 ppb CN Distilled ICV Standard	.0375 mL	

This is runlog Lachat1

Sample ID	Batch	Dilution	Analyst	Runtime	Dataset
200 ppb		1	axc2	3/8/2010 10:25:45	OM_3-8-2010_10-24-48
150 ppb		1	axc2	3/8/2010 10:26:37	OM_3-8-2010_10-24-48
100 ppb		1	axc2	3/8/2010 10:27:29	OM_3-8-2010_10-24-48
50 ppb		1	axc2	3/8/2010 10:28:22	OM_3-8-2010_10-24-48
10 ppb		1	axc2	3/8/2010 10:29:15	OM_3-8-2010_10-24-48
CRDL 5.0 ppb		1	axc2	3/8/2010 10:30:09	OM_3-8-2010_10-24-48
ICAL-00		1	axc2	3/8/2010 10:31:03	OM_3-8-2010_10-24-48
ICV		1	axc2	3/8/2010 10:32:54	OM_3-8-2010_10-24-48
ICB		1	axc2	3/8/2010 10:34:44	OM_3-8-2010_10-24-48
CRDL		1	axc2	3/8/2010 10:36:34	OM_3-8-2010_10-24-48
1202054789	958168	1	axc2	3/8/2010 10:38:23	OM_3-8-2010_10-24-48
1202054796	958168	1	axc2	3/8/2010 10:39:17	OM_3-8-2010_10-24-48
248010001	958168	1	axc2	3/8/2010 10:40:10	OM_3-8-2010_10-24-48
1202054790	958168	1	axc2	3/8/2010 10:41:03	OM_3-8-2010_10-24-48
1202054792	958168	1	axc2	3/8/2010 10:41:56	OM_3-8-2010_10-24-48
1202054794	958168	1	axc2	3/8/2010 10:42:48	OM_3-8-2010_10-24-48
248010002	958168	1	axc2	3/8/2010 10:43:42	OM_3-8-2010_10-24-48
248019001	958168	1	axc2	3/8/2010 10:44:34	OM_3-8-2010_10-24-48
248019002	958168	1	axc2	3/8/2010 10:45:26	OM_3-8-2010_10-24-48
248023002	958168	1	axc2	3/8/2010 10:46:19	OM_3-8-2010_10-24-48
CCV		1	axc2	3/8/2010 10:47:11	OM_3-8-2010_10-24-48
CCB		1	axc2	3/8/2010 10:49:01	OM_3-8-2010_10-24-48
248024001	958168	1	axc2	3/8/2010 10:50:50	OM_3-8-2010_10-24-48
248024003	958168	1	axc2	3/8/2010 10:51:41	OM_3-8-2010_10-24-48
248044002	958168	1	axc2	3/8/2010 10:52:34	OM_3-8-2010_10-24-48
1202054791	958168	1	axc2	3/8/2010 10:53:25	OM_3-8-2010_10-24-48
1202054793	958168	1	axc2	3/8/2010 10:54:17	OM_3-8-2010_10-24-48
1202054795	958168	1	axc2	3/8/2010 10:55:10	OM_3-8-2010_10-24-48
248401005	958168	1	axc2	3/8/2010 10:56:04	OM_3-8-2010_10-24-48
248516001	958168	1	axc2	3/8/2010 10:56:58	OM_3-8-2010_10-24-48
248516002	958168	1	axc2	3/8/2010 10:57:51	OM_3-8-2010_10-24-48
248518001	958168	1	axc2	3/8/2010 10:58:44	OM_3-8-2010_10-24-48
CCV		1	axc2	3/8/2010 10:59:36	OM_3-8-2010_10-24-48
CCB		1	axc2	3/8/2010 11:01:27	OM_3-8-2010_10-24-48
248533001	958168	1	axc2	3/8/2010 11:03:16	OM_3-8-2010_10-24-48
248548001	958168	1	axc2	3/8/2010 11:04:09	OM_3-8-2010_10-24-48
248548003	958168	1	axc2	3/8/2010 11:05:01	OM_3-8-2010_10-24-48
248551001	958168	1	axc2	3/8/2010 11:05:54	OM_3-8-2010_10-24-48
248551002	958168	1	axc2	3/8/2010 11:06:46	OM_3-8-2010_10-24-48
248555002	958168	1	axc2	3/8/2010 11:07:39	OM_3-8-2010_10-24-48
1202059721	960271	1	axc2	3/8/2010 11:08:31	OM_3-8-2010_10-24-48
1202059731	960271	1	axc2	3/8/2010 11:09:23	OM_3-8-2010_10-24-48
248072001	960271	1	axc2	3/8/2010 11:10:15	OM_3-8-2010_10-24-48
1202059722	960271	1	axc2	3/8/2010 11:11:06	OM_3-8-2010_10-24-48
CCV		1	axc2	3/8/2010 11:11:59	OM_3-8-2010_10-24-48
CCB		1	axc2	3/8/2010 11:13:49	OM_3-8-2010_10-24-48
1202059725	960271	1	axc2	3/8/2010 11:15:40	OM_3-8-2010_10-24-48
1202059728	960271	1	axc2	3/8/2010 11:16:33	OM_3-8-2010_10-24-48
248072002	960271	1	axc2	3/8/2010 11:17:27	OM_3-8-2010_10-24-48
248072003	960271	1	axc2	3/8/2010 11:18:21	OM_3-8-2010_10-24-48
248097001	960271	1	axc2	3/8/2010 11:19:14	OM_3-8-2010_10-24-48
1202059724	960271	1	axc2	3/8/2010 11:20:07	OM_3-8-2010_10-24-48
1202059727	960271	1	axc2	3/8/2010 11:21:00	OM_3-8-2010_10-24-48
1202059730	960271	1	axc2	3/8/2010 11:21:53	OM_3-8-2010_10-24-48
248097002	960271	1	axc2	3/8/2010 11:22:47	OM_3-8-2010_10-24-48
248097003	960271	1	axc2	3/8/2010 11:23:38	OM_3-8-2010_10-24-48
CCV		1	axc2	3/8/2010 11:24:31	OM_3-8-2010_10-24-48
CCB		1	axc2	3/8/2010 11:26:21	OM_3-8-2010_10-24-48

248097004	960271	1	axc2	3/8/2010	11:28:09	OM_3-8-2010_10-24-48
248298001	960271	1	axc2	3/8/2010	11:29:02	OM_3-8-2010_10-24-48
248298002	960271	1	axc2	3/8/2010	11:29:53	OM_3-8-2010_10-24-48
248298003	960271	1	axc2	3/8/2010	11:30:46	OM_3-8-2010_10-24-48
248303001	960271	1	axc2	3/8/2010	11:31:38	OM_3-8-2010_10-24-48
248337001	960271	1	axc2	3/8/2010	11:32:32	OM_3-8-2010_10-24-48
248375001	960271	1	axc2	3/8/2010	11:33:26	OM_3-8-2010_10-24-48
248375002	960271	1	axc2	3/8/2010	11:34:19	OM_3-8-2010_10-24-48
248397001	960271	1	axc2	3/8/2010	11:35:14	OM_3-8-2010_10-24-48
248397002	960271	1	axc2	3/8/2010	11:36:06	OM_3-8-2010_10-24-48
CCV		1	axc2	3/8/2010	11:37:00	OM_3-8-2010_10-24-48
CCB		1	axc2	3/8/2010	11:38:51	OM_3-8-2010_10-24-48
248407001	960271	1	axc2	3/8/2010	11:40:39	OM_3-8-2010_10-24-48
1202059723	960271	1	axc2	3/8/2010	11:41:33	OM_3-8-2010_10-24-48
1202059726	960271	1	axc2	3/8/2010	11:42:26	OM_3-8-2010_10-24-48
1202059729	960271	1	axc2	3/8/2010	11:43:19	OM_3-8-2010_10-24-48
248419001	960271	1	axc2	3/8/2010	11:44:11	OM_3-8-2010_10-24-48
248419002	960271	1	axc2	3/8/2010	11:45:04	OM_3-8-2010_10-24-48
1202053300	957584	1	axc2	3/8/2010	11:45:57	OM_3-8-2010_10-24-48
1202053310	957584	1	axc2	3/8/2010	11:46:49	OM_3-8-2010_10-24-48
247829002	957584	1	axc2	3/8/2010	11:47:41	OM_3-8-2010_10-24-48
1202053302	957584	1	axc2	3/8/2010	11:48:33	OM_3-8-2010_10-24-48
CCV		1	axc2	3/8/2010	11:49:26	OM_3-8-2010_10-24-48
CCB		1	axc2	3/8/2010	11:51:15	OM_3-8-2010_10-24-48
1202053305	957584	1	axc2	3/8/2010	11:53:05	OM_3-8-2010_10-24-48
1202053308	957584	1	axc2	3/8/2010	11:54:00	OM_3-8-2010_10-24-48
247865010	957584	1	axc2	3/8/2010	11:54:55	OM_3-8-2010_10-24-48
247865012	957584	1	axc2	3/8/2010	11:55:48	OM_3-8-2010_10-24-48
1202053303	957584	1	axc2	3/8/2010	11:56:41	OM_3-8-2010_10-24-48
1202053306	957584	1	axc2	3/8/2010	11:57:35	OM_3-8-2010_10-24-48
1202053309	957584	1	axc2	3/8/2010	11:58:28	OM_3-8-2010_10-24-48
247865013	957584	1	axc2	3/8/2010	11:59:21	OM_3-8-2010_10-24-48
247865014	957584	1	axc2	3/8/2010	12:00:15	OM_3-8-2010_10-24-48
247865015	957584	1	axc2	3/8/2010	12:01:07	OM_3-8-2010_10-24-48
CCV		1	axc2	3/8/2010	12:02:00	OM_3-8-2010_10-24-48
CCB		1	axc2	3/8/2010	12:03:51	OM_3-8-2010_10-24-48
247865016	957584	1	axc2	3/8/2010	12:05:41	OM_3-8-2010_10-24-48
247865017	957584	1	axc2	3/8/2010	12:06:33	OM_3-8-2010_10-24-48
247865018	957584	1	axc2	3/8/2010	12:07:25	OM_3-8-2010_10-24-48
247865019	957584	1	axc2	3/8/2010	12:08:18	OM_3-8-2010_10-24-48
247865020	957584	1	axc2	3/8/2010	12:09:10	OM_3-8-2010_10-24-48
247866001	957584	1	axc2	3/8/2010	12:10:05	OM_3-8-2010_10-24-48
247919001	957584	1	axc2	3/8/2010	12:10:59	OM_3-8-2010_10-24-48
247919002	957584	1	axc2	3/8/2010	12:11:53	OM_3-8-2010_10-24-48
247922004	957584	1	axc2	3/8/2010	12:12:48	OM_3-8-2010_10-24-48
1202053301	957584	1	axc2	3/8/2010	12:13:41	OM_3-8-2010_10-24-48
CCV		1	axc2	3/8/2010	12:14:34	OM_3-8-2010_10-24-48
CCB		1	axc2	3/8/2010	12:16:24	OM_3-8-2010_10-24-48
1202053304	957584	1	axc2	3/8/2010	12:18:14	OM_3-8-2010_10-24-48
1202053307	957584	1	axc2	3/8/2010	12:19:07	OM_3-8-2010_10-24-48
248164004	957584	1	axc2	3/8/2010	12:20:01	OM_3-8-2010_10-24-48
248382002	957584	1	axc2	3/8/2010	12:20:54	OM_3-8-2010_10-24-48
248382003	957584	1	axc2	3/8/2010	12:21:47	OM_3-8-2010_10-24-48
248401002	957584	1	axc2	3/8/2010	12:22:40	OM_3-8-2010_10-24-48
248401004	957584	1	axc2	3/8/2010	12:23:33	OM_3-8-2010_10-24-48
CCV		1	axc2	3/8/2010	12:24:25	OM_3-8-2010_10-24-48
CCB		1	axc2	3/8/2010	12:26:15	OM_3-8-2010_10-24-48

Author: axc2

Date : 3/8/2010

Original Run Filename: OM_3-8-2010_10-24-48.OMN created 3/8/2010 10:24:48
 Original Run Author's Signature: [axc2]
 Current Run Filename: OM_3-8-2010_10-24-48.OMN last modified 3/8/2010 12:27:20
 Current Run Author's Signature: [axc2]
 Description: GL-GC-E-095 EPA 335.1, 335.3, 335.4, 9012A, CLP335.2-M
 Liquid LCS nominal 50 ug/L

Sample	Rep.	Cup No.	Channel 1 TCYANIDE		Detection Time	ADF	MDF	Description
			Conc. (ug/L)	Area (Vs)				
WCN100308-01	1	S1	200	10.4	3/8/2010@10:25:45			200 ppb
WCN100308-02	1	S2	150	7.82	3/8/2010@10:26:37			150 ppb
WCN100308-03	1	S3	100	5.36	3/8/2010@10:27:29			100 ppb
WCN100308-04	1	S4	50.0	2.85	3/8/2010@10:28:22			50 ppb
WCN100308-05	1	S5	10.0	0.644	3/8/2010@10:29:15			10 ppb
WCN100308-06	1	S6	5.00	0.400	3/8/2010@10:30:09			CRDL 5.0 ppb
WCN100308-08	1	S7	0.00	-0.0189	3/8/2010@10:31:03			0.0 ppb
DQM Test: Minimum Correlation Coefficient								
Result:			0.99976 > 0.99500					
Message			Pass					
Action			Continue					
WCN100308-07	1	S8	147	7.72	3/8/2010@10:32:54			ICV
Known Conc:			150					
DQM Test: > + Percent Relative Difference								
Result:			-2.1 < 10.0					
Message			ICV Passed					
Action			Continue					
DQM Test: < - Percent Relative Difference								
Result:			-2.1 < 10.0					
Message			ICV Passed					
Action			Continue					
Calibration:			Table/Fig. 1					
WCN100308-08	1	S7	-1.65	0.0363	3/8/2010@10:34:44			ICB/CCB
Known Conc:			0.00					
DQM Test: > + Concentration Limit								
Result:			-1.65 < 5.01					
Message			ICB/CCB Passed					
Action			Continue					
DQM Test: < - Concentration Limit								
Result:			-1.65 > -5.01					
Message			ICB/CCB Passed					
Action			Continue					
WCN100308-06	1	S6	5.25	0.393	3/8/2010@10:36:34			CRDL
Known Conc:			5.00					
DQM Test: > + Concentration Limit								
Result:			5.25 < 7.50					
Message			CRDL Passed					
Action			Continue					
DQM Test: < - Concentration Limit								
Result:			5.25 > 2.50					
Message			Pass					
Action			None					
1202054789 958168 MB	1	1	-1.83	0.0269	3/8/2010@10:38:23			
1202054796 LCS	1	2	50.4	2.73	3/8/2010@10:39:17			
248010001	1	3	-1.53	0.0427	3/8/2010@10:40:10			
1202054790 DUP	1	4	-1.69	0.0344	3/8/2010@10:41:03			
1202054792 MS	1	5	114	6.01	3/8/2010@10:41:56			
1202054794 MSD	1	6	111	5.86	3/8/2010@10:42:48			
248010002	1	7	-1.44	0.0471	3/8/2010@10:43:42			
248019001	1	8	-1.39	0.0498	3/8/2010@10:44:34			
248019002	1	9	-1.40	0.0491	3/8/2010@10:45:26			
248023002	1	10	-1.75	0.0312	3/8/2010@10:46:19			
WCN100308-03	1	S3	105	5.54	3/8/2010@10:47:11			CCV
Known Conc:			100					
DQM Test: > + Percent Relative Difference								
Result:			4.8 < 10.0					

Message			CCV Passed					
Action			Continue					
DQM Test: < - Percent Relative Difference								
Result:			4.8 < 10.0					
Message			CCV Passed					
Action			Continue					
WCN100308-08	1	S7	-1.67	0.0352	3/8/2010@10:49:01			CCB
Known Conc:			0.00					
DQM Test: > + Concentration Limit								
Result:			-1.67 < 5.00					
Message			CCB Passed					
Action			Continue					
DQM Test: < - Concentration Limit								
Result:			-1.67 > -5.00					
Message			CCB Passed					
Action			Continue					
248024001	1	11	-2.29	0.00319	3/8/2010@10:50:50			
248024003	1	12	-0.940	0.0730	3/8/2010@10:51:41			
248044002	1	13	-1.78	0.0297	3/8/2010@10:52:34			
1202054791 DUP	1	14	-1.89	0.0237	3/8/2010@10:53:25			
1202054793 MS	1	15	113	5.97	3/8/2010@10:54:17			
1202054795 MSD	1	16	94.5	5.01	3/8/2010@10:55:10			
248401005	1	17	-2.36	-4.50e-4	3/8/2010@10:56:04			
248516001	1	18	-1.70	0.0336	3/8/2010@10:56:58			
248516002	1	19	-2.03	0.0168	3/8/2010@10:57:51			
248518001	1	20	-2.35	3.13e-4	3/8/2010@10:58:44			
WCN100308-03	1	S3	107	5.64	3/8/2010@10:59:36			CCV
Known Conc:			100					
DQM Test: > + Percent Relative Difference								
Result:			6.6 < 10.0					
Message			CCV Passed					
Action			Continue					
DQM Test: < - Percent Relative Difference								
Result:			6.6 < 10.0					
Message			CCV Passed					
Action			Continue					
WCN100308-08	1	S7	-1.82	0.0275	3/8/2010@11:01:27			CCB
Known Conc:			0.00					
DQM Test: > + Concentration Limit								
Result:			-1.82 < 5.00					
Message			CCB Passed					
Action			Continue					
DQM Test: < - Concentration Limit								
Result:			-1.82 > -5.00					
Message			CCB Passed					
Action			Continue					
248533001	1	21	-1.85	0.0260	3/8/2010@11:03:16			
248548001	1	22	-2.24	0.00579	3/8/2010@11:04:09			
248548003	1	23	-1.45	0.0465	3/8/2010@11:05:01			
248551001	1	24	-0.552	0.0931	3/8/2010@11:05:54			
248551002	1	25	-1.81	0.0281	3/8/2010@11:06:46			
248555002	1	26	-1.99	0.0185	3/8/2010@11:07:39			
1202059721 960271 MB	1	27	-1.70	0.0339	3/8/2010@11:08:31			
1202059731 LCS	1	28	49.0	2.66	3/8/2010@11:09:23			
248072001	1	29	-2.36	-5.25e-4	3/8/2010@11:10:15			
1202059722 DUP	1	30	-1.95	0.0206	3/8/2010@11:11:06			
WCN100308-03	1	S3	105	5.54	3/8/2010@11:11:59			CCV
Known Conc:			100					
DQM Test: > + Percent Relative Difference								
Result:			4.7 < 10.0					
Message			CCV Passed					
Action			Continue					
DQM Test: < - Percent Relative Difference								
Result:			4.7 < 10.0					
Message			CCV Passed					
Action			Continue					
WCN100308-08	1	S7	-1.72	0.0325	3/8/2010@11:13:49			CCB
Known Conc:			0.00					

DQM Test: > + Concentration Limit						
Result:		-1.72 < 5.00				
Message		CCB Passed				
Action		Continue				
DQM Test: < - Concentration Limit						
Result:		-1.72 > -5.00				
Message		CCB Passed				
Action		Continue				
1202059725	MS	1	31	102	5.41	3/8/2010@11:15:40
1202059728	MSD	1	32	101	5.33	3/8/2010@11:16:33
248072002		1	33	-1.30	0.0543	3/8/2010@11:17:27
248072003		1	34	-2.90	-0.0286	3/8/2010@11:18:21
248097001		1	35	-1.88	0.0245	3/8/2010@11:19:14
1202059724	DUP	1	36	-1.58	0.0398	3/8/2010@11:20:07
1202059727	MS	1	37	100	5.32	3/8/2010@11:21:00
1202059730	MSD	1	38	102	5.39	3/8/2010@11:21:53
248097002		1	39	12.3	0.757	3/8/2010@11:22:47
248097003		1	40	-1.04	0.0680	3/8/2010@11:23:38
WCN100308-03		1	S3	106	5.63	3/8/2010@11:24:31
Known Conc:				100		CCV
DQM Test: > + Percent Relative Difference						
Result:		6.4 < 10.0				
Message		CCV Passed				
Action		Continue				
DQM Test: < - Percent Relative Difference						
Result:		6.4 < 10.0				
Message		CCV Passed				
Action		Continue				
WCN100308-08		1	S7	-1.68	0.0346	3/8/2010@11:26:21
Known Conc:				0.00		CCB
DQM Test: > + Concentration Limit						
Result:		-1.68 < 5.00				
Message		CCB Passed				
Action		Continue				
DQM Test: < - Concentration Limit						
Result:		-1.68 > -5.00				
Message		CCB Passed				
Action		Continue				
248097004		1	41	-0.871	0.0766	3/8/2010@11:28:09
248298001		1	42	-1.67	0.0350	3/8/2010@11:29:02
248298002		1	43	-1.93	0.0216	3/8/2010@11:29:53
248298003		1	44	-0.109	0.116	3/8/2010@11:30:46
248303001		1	45	2.92	0.273	3/8/2010@11:31:38
248337001		1	46	-2.49	-0.00692	3/8/2010@11:32:32
248375001		1	47	-2.35	1.70e-4	3/8/2010@11:33:26
248375002		1	48	-2.05	0.0157	3/8/2010@11:34:19
248397001		1	49	-1.87	0.0247	3/8/2010@11:35:14
248397002		1	50	-2.17	0.00925	3/8/2010@11:36:06
WCN100308-03		1	S3	106	5.62	3/8/2010@11:37:00
Known Conc:				100		CCV
DQM Test: > + Percent Relative Difference						
Result:		6.2 < 10.0				
Message		CCV Passed				
Action		Continue				
DQM Test: < - Percent Relative Difference						
Result:		6.2 < 10.0				
Message		CCV Passed				
Action		Continue				
WCN100308-08		1	S7	-2.34	8.36e-4	3/8/2010@11:38:51
Known Conc:				0.00		CCB
DQM Test: > + Concentration Limit						
Result:		-2.34 < 5.00				
Message		CCB Passed				
Action		Continue				
DQM Test: < - Concentration Limit						
Result:		-2.34 > -5.00				
Message		CCB Passed				
Action		Continue				

248407001	1	51	-1.69	0.0345	3/8/2010@11:40:39		
1202059723 DUP	1	52	-2.37	-0.00102	3/8/2010@11:41:33		
1202059726 MS	1	53	104	5.51	3/8/2010@11:42:26		
1202059729 MSD	1	54	82.4	4.39	3/8/2010@11:43:19		
248419001	1	55	-1.45	0.0465	3/8/2010@11:44:11		
248419002	1	56	-1.82	0.0276	3/8/2010@11:45:04		
1202053300 957584 MB	1	57	-1.77	0.0301	3/8/2010@11:45:57		
1202053310 LCS	1	58	52.0	2.81	3/8/2010@11:46:49		
247829002	1	59	-1.36	0.0515	3/8/2010@11:47:41		
1202053302 DUP	1	60	-1.35	0.0518	3/8/2010@11:48:33		
WCN100308-03	1	S3	107	5.65	3/8/2010@11:49:26		CCV
Known Conc:			100				
DQM Test: > + Percent Relative Difference							
Result:			6.9 < 10.0				
Message			CCV Passed				
Action			Continue				
DQM Test: < - Percent Relative Difference							
Result:			6.9 < 10.0				
Message			CCV Passed				
Action			Continue				
WCN100308-08	1	S7	-1.71	0.0332	3/8/2010@11:51:15		CCB
Known Conc:			0.00				
DQM Test: > + Concentration Limit							
Result:			-1.71 < 5.00				
Message			CCB Passed				
Action			Continue				
DQM Test: < - Concentration Limit							
Result:			-1.71 > -5.00				
Message			CCB Passed				
Action			Continue				
1202053305 MS	1	61	108	5.71	3/8/2010@11:53:05		
1202053308 MSD	1	62	108	5.72	3/8/2010@11:54:00		
247865010	1	63	-1.12	0.0636	3/8/2010@11:54:55		
247865012	1	64	-1.20	0.0593	3/8/2010@11:55:48		
1202053303 DUP	1	65	-1.53	0.0427	3/8/2010@11:56:41		
1202053306 MS	1	66	86.3	4.59	3/8/2010@11:57:35		
1202053309 MSD	1	67	102	5.39	3/8/2010@11:58:28		
247865013	1	68	-1.42	0.0483	3/8/2010@11:59:21		
247865014	1	69	-1.44	0.0472	3/8/2010@12:00:15		
247865015	1	70	-1.50	0.0439	3/8/2010@12:01:07		
WCN100308-03	1	S3	106	5.63	3/8/2010@12:02:00		CCV
Known Conc:			100				
DQM Test: > + Percent Relative Difference							
Result:			6.4 < 10.0				
Message			CCV Passed				
Action			Continue				
DQM Test: < - Percent Relative Difference							
Result:			6.4 < 10.0				
Message			CCV Passed				
Action			Continue				
WCN100308-08	1	S7	-1.63	0.0372	3/8/2010@12:03:51		CCB
Known Conc:			0.00				
DQM Test: > + Concentration Limit							
Result:			-1.63 < 5.00				
Message			CCB Passed				
Action			Continue				
DQM Test: < - Concentration Limit							
Result:			-1.63 > -5.00				
Message			CCB Passed				
Action			Continue				
247865016	1	71	-1.63	0.0374	3/8/2010@12:05:41		
247865017	1	72	-1.38	0.0501	3/8/2010@12:06:33		
247865018	1	73	-2.31	0.00203	3/8/2010@12:07:25		
247865019	1	74	-1.70	0.0337	3/8/2010@12:08:18		
247865020	1	75	-1.21	0.0589	3/8/2010@12:09:10		
247866001	1	76	-1.82	0.0273	3/8/2010@12:10:05		
247919001	1	77	-1.59	0.0392	3/8/2010@12:10:59		
247919002	1	78	-1.41	0.0486	3/8/2010@12:11:53		

247922004	1	79	0.739	0.160	3/8/2010@12:12:48		
1202053301 DUP	1	80	0.641	0.155	3/8/2010@12:13:41		
WCN100308-03	1	S3	107	5.65	3/8/2010@12:14:34		CCV
Known Conc:			100				
DQM Test: > + Percent Relative Difference							
Result:			6.8 < 10.0				
Message			CCV Passed				
Action			Continue				
DQM Test: < - Percent Relative Difference							
Result:			6.8 < 10.0				
Message			CCV Passed				
Action			Continue				
WCN100308-08	1	S7	-1.86	0.0256	3/8/2010@12:16:24		CCB
Known Conc:			0.00				
DQM Test: > + Concentration Limit							
Result:			-1.86 < 5.00				
Message			CCB Passed				
Action			Continue				
DQM Test: < - Concentration Limit							
Result:			-1.86 > -5.00				
Message			CCB Passed				
Action			Continue				
1202053304 MS	1	81	98.2	5.21	3/8/2010@12:18:14		
1202053307 MSD	1	82	98.4	5.21	3/8/2010@12:19:07		
248164004	1	83	-1.49	0.0445	3/8/2010@12:20:01		
248382002	1	84	-1.58	0.0400	3/8/2010@12:20:54		
248382003	1	85	-1.82	0.0273	3/8/2010@12:21:47		
248401002	1	86	-1.52	0.0428	3/8/2010@12:22:40		
248401004	1	87	-1.38	0.0501	3/8/2010@12:23:33		
WCN100308-03	1	S3	106	5.59	3/8/2010@12:24:25		CCV
Known Conc:			100				
DQM Test: > + Percent Relative Difference							
Result:			5.8 < 10.0				
Message			CCV Passed				
Action			Continue				
DQM Test: < - Percent Relative Difference							
Result:			5.8 < 10.0				
Message			CCV Passed				
Action			Continue				
WCN100308-08	1	S7	-1.71	0.0334	3/8/2010@12:26:15		CCB
Known Conc:			0.00				
DQM Test: > + Concentration Limit							
Result:			-1.71 < 5.00				
Message			CCB Passed				
Action			Continue				
DQM Test: < - Concentration Limit							
Result:			-1.71 > -5.00				
Message			CCB Passed				
Action			Continue				

Analyte Properties Table for OM_3-8-2010_10-24-48.OMN

Property	Channel 1 TCYANIDE
Concentration Units	ug/L
Calibration Fit Type	First Order
Clear Calibration	True
Force Through Zero	False
Calibration Weighting	None
Auto Dilution Trigger	True
% of High Standard	100
Quik Chem Method	10-204-00-1-A
Chemistry	Direct/Bipolar
Calibration by Height	False
Inject to Peak Start	22
Peak Base Width	39

Channel 1: Current View


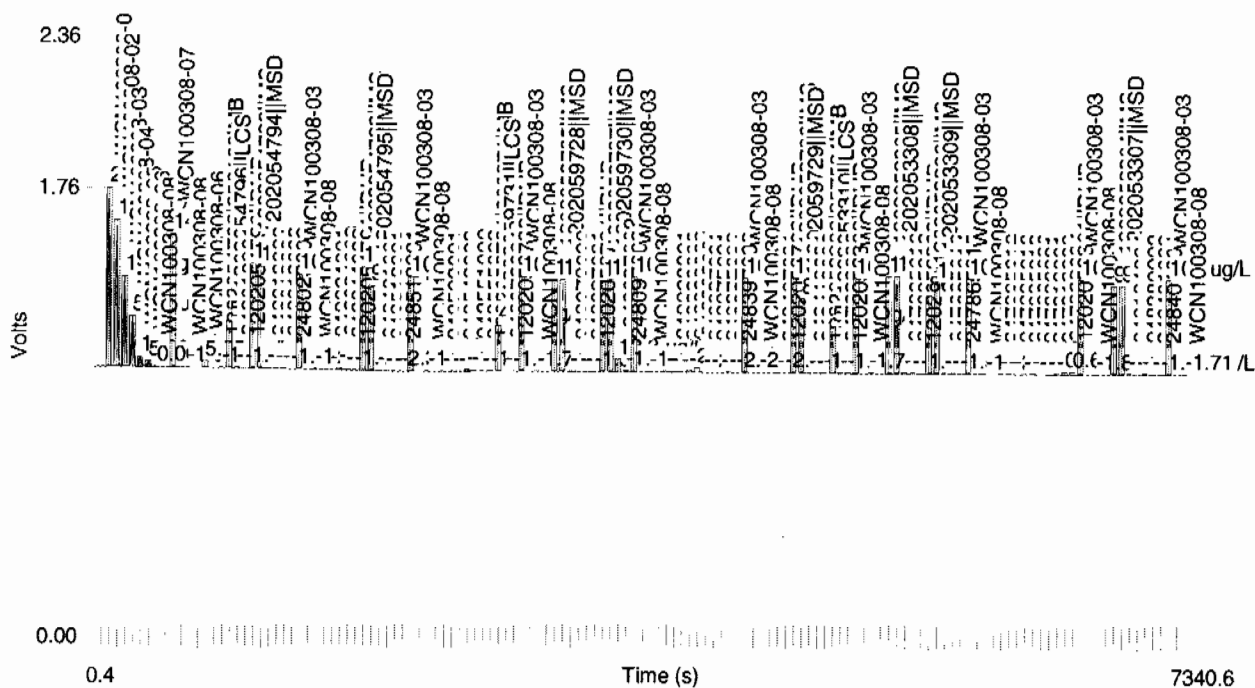


Table 1: TCYANIDE

	Conc. (ug/L)	Rep	Peak Area (Volt-s)	Peak Height (Volts)	% Residual	Detection Date	Detection Time
1	200	1	10.4	0.692	0.2	3/8/2010	10:26:48
2	150	1	7.82	0.567	0.7	3/8/2010	10:27:40
3	100	1	5.36	0.353	-1.3	3/8/2010	10:28:32
4	50.0	1	2.85	0.199	-5.1	3/8/2010	10:29:25
5	10.0	1	0.644	0.0420	-0.6	3/8/2010	10:30:18
6	5.00	1	0.400	0.0240	-4.6	3/8/2010	10:31:12
7	0.00	1	-0.0189	-0.00306		3/8/2010	10:32:06

Figure 1: TCYANIDE

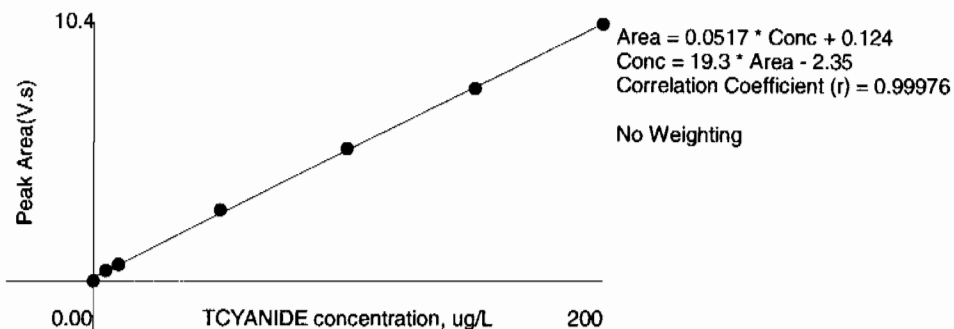

This is runlog Lachat1

Sample ID	Batch	Dilution	Analyst	Runtime	Dataset
CCV		1	axc2	3/8/2010 15:01:26	OM_3-8-2010_14-58-05
CCB		1	axc2	3/8/2010 15:03:15	OM_3-8-2010_14-58-05
1202057161	959217	1	axc2	3/8/2010 15:05:05	OM_3-8-2010_14-58-05
1202057168	959217	1	axc2	3/8/2010 15:05:58	OM_3-8-2010_14-58-05
248044005	959217	1	axc2	3/8/2010 15:06:52	OM_3-8-2010_14-58-05
1202057163	959217	1	axc2	3/8/2010 15:07:45	OM_3-8-2010_14-58-05
1202057165	959217	1	axc2	3/8/2010 15:08:38	OM_3-8-2010_14-58-05
1202057167	959217	1	axc2	3/8/2010 15:09:31	OM_3-8-2010_14-58-05
248044006	959217	1	axc2	3/8/2010 15:10:24	OM_3-8-2010_14-58-05
248108001	959217	1	axc2	3/8/2010 15:11:16	OM_3-8-2010_14-58-05
248117001	959217	1	axc2	3/8/2010 15:12:08	OM_3-8-2010_14-58-05
248127002	959217	1	axc2	3/8/2010 15:13:02	OM_3-8-2010_14-58-05
CCV		1	axc2	3/8/2010 15:13:54	OM_3-8-2010_14-58-05
CCB		1	axc2	3/8/2010 15:15:44	OM_3-8-2010_14-58-05
248162001	959217	1	axc2	3/8/2010 15:17:33	OM_3-8-2010_14-58-05
248162002	959217	1	axc2	3/8/2010 15:18:25	OM_3-8-2010_14-58-05
248162003	959217	1	axc2	3/8/2010 15:19:17	OM_3-8-2010_14-58-05
248162004	959217	1	axc2	3/8/2010 15:20:09	OM_3-8-2010_14-58-05
248164002	959217	1	axc2	3/8/2010 15:21:00	OM_3-8-2010_14-58-05
248168006	959217	1	axc2	3/8/2010 15:21:55	OM_3-8-2010_14-58-05
248169004	959217	1	axc2	3/8/2010 15:22:48	OM_3-8-2010_14-58-05
248188001	959217	1	axc2	3/8/2010 15:23:41	OM_3-8-2010_14-58-05
1202057162	959217	1	axc2	3/8/2010 15:24:34	OM_3-8-2010_14-58-05
1202057164*	959217	1	axc2	3/8/2010 15:25:27	OM_3-8-2010_14-58-05
CCV		1	axc2	3/8/2010 15:26:19	OM_3-8-2010_14-58-05
CCB		1	axc2	3/8/2010 15:28:11	OM_3-8-2010_14-58-05
1202057166	959217	1	axc2	3/8/2010 15:30:01	OM_3-8-2010_14-58-05
248199001	959217	1	axc2	3/8/2010 15:30:54	OM_3-8-2010_14-58-05
248238001	959217	1	axc2	3/8/2010 15:31:46	OM_3-8-2010_14-58-05
248238002	959217	1	axc2	3/8/2010 15:32:39	OM_3-8-2010_14-58-05
1202057164*	959217	1	axc2	3/8/2010 15:33:32	OM_3-8-2010_14-58-05
248242001	959217	1	axc2	3/8/2010 15:34:25	OM_3-8-2010_14-58-05
248245001	959217	1	axc2	3/8/2010 15:35:17	OM_3-8-2010_14-58-05
248257001	959217	1	axc2	3/8/2010 15:36:09	OM_3-8-2010_14-58-05
248257002	959217	1	axc2	3/8/2010 15:37:01	OM_3-8-2010_14-58-05
1202057164	959217	1	axc2	3/8/2010 15:37:54	OM_3-8-2010_14-58-05
CCV		1	axc2	3/8/2010 15:38:47	OM_3-8-2010_14-58-05
CCB		1	axc2	3/8/2010 15:40:39	OM_3-8-2010_14-58-05
1202057112	959204	1	axc2	3/8/2010 15:42:28	OM_3-8-2010_14-58-05
1202057119	959204	25	axc2	3/8/2010 15:43:18	OM_3-8-2010_14-58-05
248110001	959204	1	axc2	3/8/2010 15:44:13	OM_3-8-2010_14-58-05
248110002	959204	1	axc2	3/8/2010 15:45:07	OM_3-8-2010_14-58-05
248110003	959204	1	axc2	3/8/2010 15:46:00	OM_3-8-2010_14-58-05
248110004	959204	1	axc2	3/8/2010 15:46:54	OM_3-8-2010_14-58-05
248110005	959204	1	axc2	3/8/2010 15:47:47	OM_3-8-2010_14-58-05
248110006	959204	1	axc2	3/8/2010 15:48:41	OM_3-8-2010_14-58-05
248110007	959204	1	axc2	3/8/2010 15:49:33	OM_3-8-2010_14-58-05
248110008	959204	1	axc2	3/8/2010 15:50:26	OM_3-8-2010_14-58-05
CCV		1	axc2	3/8/2010 15:51:19	OM_3-8-2010_14-58-05
CCB		1	axc2	3/8/2010 15:53:09	OM_3-8-2010_14-58-05
248118001	959204	1	axc2	3/8/2010 15:54:59	OM_3-8-2010_14-58-05
248118002	959204	1	axc2	3/8/2010 15:55:52	OM_3-8-2010_14-58-05
248118003	959204	1	axc2	3/8/2010 15:56:45	OM_3-8-2010_14-58-05
248118004	959204	1	axc2	3/8/2010 15:57:37	OM_3-8-2010_14-58-05
248118005	959204	1	axc2	3/8/2010 15:58:28	OM_3-8-2010_14-58-05
248118006	959204	1	axc2	3/8/2010 15:59:22	OM_3-8-2010_14-58-05
248118007	959204	1	axc2	3/8/2010 16:00:13	OM_3-8-2010_14-58-05
248189001	959204	1	axc2	3/8/2010 16:01:07	OM_3-8-2010_14-58-05

1202057113	959204	1	axc2	3/8/2010	16:02:01	OM_3-8-2010_14-58-05
1202057115	959204	1	axc2	3/8/2010	16:02:55	OM_3-8-2010_14-58-05
CCV		1	axc2	3/8/2010	16:03:48	OM_3-8-2010_14-58-05
CCB		1	axc2	3/8/2010	16:05:39	OM_3-8-2010_14-58-05
1202057117	959204	1	axc2	3/8/2010	16:07:29	OM_3-8-2010_14-58-05
248189002	959204	1	axc2	3/8/2010	16:08:23	OM_3-8-2010_14-58-05
1202057114	959204	1	axc2	3/8/2010	16:09:16	OM_3-8-2010_14-58-05
1202057116	959204	1	axc2	3/8/2010	16:10:09	OM_3-8-2010_14-58-05
1202057118	959204	1	axc2	3/8/2010	16:11:02	OM_3-8-2010_14-58-05
1202054781	958165	1	axc2	3/8/2010	16:11:55	OM_3-8-2010_14-58-05
1202054788	958165	25	axc2	3/8/2010	16:12:47	OM_3-8-2010_14-58-05
247918001	958165	1	axc2	3/8/2010	16:13:39	OM_3-8-2010_14-58-05
247918002	958165	1	axc2	3/8/2010	16:14:33	OM_3-8-2010_14-58-05
247918003	958165	1	axc2	3/8/2010	16:15:25	OM_3-8-2010_14-58-05
CCV		1	axc2	3/8/2010	16:16:17	OM_3-8-2010_14-58-05
CCB		1	axc2	3/8/2010	16:18:09	OM_3-8-2010_14-58-05
247918004	958165	1	axc2	3/8/2010	16:19:58	OM_3-8-2010_14-58-05
1202054782	958165	1	axc2	3/8/2010	16:20:49	OM_3-8-2010_14-58-05
1202054784	958165	1	axc2	3/8/2010	16:21:44	OM_3-8-2010_14-58-05
1202054786	958165	1	axc2	3/8/2010	16:22:39	OM_3-8-2010_14-58-05
247918005	958165	1	axc2	3/8/2010	16:23:32	OM_3-8-2010_14-58-05
1202054783	958165	1	axc2	3/8/2010	16:24:26	OM_3-8-2010_14-58-05
1202054785	958165	1	axc2	3/8/2010	16:25:20	OM_3-8-2010_14-58-05
1202054787	958165	1	axc2	3/8/2010	16:26:12	OM_3-8-2010_14-58-05
247918006	958165	1	axc2	3/8/2010	16:27:06	OM_3-8-2010_14-58-05
247918007	958165	1	axc2	3/8/2010	16:28:00	OM_3-8-2010_14-58-05
CCV		1	axc2	3/8/2010	16:28:51	OM_3-8-2010_14-58-05
CCB		1	axc2	3/8/2010	16:30:42	OM_3-8-2010_14-58-05
248009001	958165	1	axc2	3/8/2010	16:32:32	OM_3-8-2010_14-58-05
248009002	958165	1	axc2	3/8/2010	16:33:25	OM_3-8-2010_14-58-05
248009003	958165	1	axc2	3/8/2010	16:34:17	OM_3-8-2010_14-58-05
248009004	958165	1	axc2	3/8/2010	16:35:10	OM_3-8-2010_14-58-05
248009005	958165	1	axc2	3/8/2010	16:36:03	OM_3-8-2010_14-58-05
248025001	958165	1	axc2	3/8/2010	16:36:55	OM_3-8-2010_14-58-05
248025002	958165	1	axc2	3/8/2010	16:37:48	OM_3-8-2010_14-58-05
248025004	958165	1	axc2	3/8/2010	16:38:42	OM_3-8-2010_14-58-05
248025006	958165	1	axc2	3/8/2010	16:39:36	OM_3-8-2010_14-58-05
248422001	958165	1	axc2	3/8/2010	16:40:31	OM_3-8-2010_14-58-05
CCV		1	axc2	3/8/2010	16:41:23	OM_3-8-2010_14-58-05
CCB		1	axc2	3/8/2010	16:43:15	OM_3-8-2010_14-58-05
248422002	958165	1	axc2	3/8/2010	16:45:06	OM_3-8-2010_14-58-05
1202061930	961278	1	axc2	3/8/2010	16:46:01	OM_3-8-2010_14-58-05
1202061932	961278	1	axc2	3/8/2010	16:46:53	OM_3-8-2010_14-58-05
247819001	961278	1	axc2	3/8/2010	16:47:47	OM_3-8-2010_14-58-05
1202061931	961278	1	axc2	3/8/2010	16:48:41	OM_3-8-2010_14-58-05
CCV		1	axc2	3/8/2010	16:49:33	OM_3-8-2010_14-58-05
CCB		1	axc2	3/8/2010	16:51:24	OM_3-8-2010_14-58-05

Original Run Filename: OM_3-8-2010_14-58-05.OMN created 3/8/2010 14:58:05
 Original Run Author's Signature: [axc2]
 Current Run Filename: OM_3-8-2010_14-58-05.OMN last modified 3/8/2010 16:52:28
 Current Run Author's Signature: [axc2]
 Description: GL-GC-E-095 EPA 335.1, 335.3, 335.4, 9012A, CLP335.2-M
 Liquid LCS nominal 50 ug/L

Sample	Rep.	Cup No.	Channel 1		Detection Time	ADF	MDF	Description
			TCYANIDE	Area (Vs)				
WCN100308-03	1	S3	103	5.47	3/8/2010@15:01:26			CCV
Known Conc:			100					
DQM Test: > + Percent Relative Difference								
Result:			3.3 < 10.0					
Message:			CCV Passed					
Action:			Continue					
DQM Test: < - Percent Relative Difference								
Result:			3.3 < 10.0					
Message:			CCV Passed					
Action:			Continue					
Calibration:			Table/Fig. 1					
WCN100308-08	1	S7	-1.49	0.0446	3/8/2010@15:03:15			CCB
Known Conc:			0.00					
DQM Test: > + Concentration Limit								
Result:			-1.49 < 5.00					
Message:			CCB Passed					
Action:			Continue					
DQM Test: < - Concentration Limit								
Result:			-1.49 > -5.00					
Message:			CCB Passed					
Action:			Continue					
1202057161 959217 MB	1	1	-2.52	-0.00888	3/8/2010@15:05:05			
1202057168 LCS	1	2	49.3	2.67	3/8/2010@15:05:58			
248044005	1	3	-2.52	-0.00856	3/8/2010@15:06:52			
1202057163 DUP	1	4	-2.04	0.0161	3/8/2010@15:07:45			
1202057165 MS	1	5	101	5.35	3/8/2010@15:08:38			
1202057167 MSD	1	6	105	5.56	3/8/2010@15:09:31			
248044006	1	7	-1.95	0.0206	3/8/2010@15:10:24			
248108001	1	8	-2.52	-0.00848	3/8/2010@15:11:16			
248117001	1	9	-2.48	-0.00645	3/8/2010@15:12:08			
248127002	1	10	-0.731	0.0839	3/8/2010@15:13:02			
WCN100308-03	1	S3	106	5.63	3/8/2010@15:13:54			CCV
Known Conc:			100					
DQM Test: > + Percent Relative Difference								
Result:			6.4 < 10.0					
Message:			CCV Passed					
Action:			Continue					
DQM Test: < - Percent Relative Difference								
Result:			6.4 < 10.0					
Message:			CCV Passed					
Action:			Continue					
WCN100308-08	1	S7	-1.84	0.0265	3/8/2010@15:15:44			CCB
Known Conc:			0.00					
DQM Test: > + Concentration Limit								
Result:			-1.84 < 5.00					
Message:			CCB Passed					
Action:			Continue					
DQM Test: < - Concentration Limit								
Result:			-1.84 > -5.00					
Message:			CCB Passed					
Action:			Continue					
248162001	1	11	-2.35	1.80e-4	3/8/2010@15:17:33			
248162002	1	12	-2.05	0.0154	3/8/2010@15:18:25			
248162003	1	13	-2.14	0.0108	3/8/2010@15:19:17			
248162004	1	14	-2.03	0.0167	3/8/2010@15:20:09			
248164002	1	15	-1.57	0.0404	3/8/2010@15:21:00			

248168006	1	16	-1.99	0.0187	3/8/2010@15:21:55		
248169004	1	17	-1.56	0.0412	3/8/2010@15:22:48		
248188001	1	18	-2.03	0.0168	3/8/2010@15:23:41		
1202057162 DUP	1	19	-2.31	0.00215	3/8/2010@15:24:34		
1202057164 MS	1	20	70.7	3.78	3/8/2010@15:25:27		
WCN100308-03	1	S3	109	5.76	3/8/2010@15:26:19		CCV
Known Conc:			100				
DQM Test: > + Percent Relative Difference							
Result:			9.0 < 10.0				
Message			CCV Passed				
Action			Continue				
DQM Test: < - Percent Relative Difference							
Result:			9.0 < 10.0				
Message			CCV Passed				
Action			Continue				
WCN100308-08	1	S7	-1.78	0.0295	3/8/2010@15:28:11		CCB
Known Conc:			0.00				
DQM Test: > + Concentration Limit							
Result:			-1.78 < 5.00				
Message			CCB Passed				
Action			Continue				
DQM Test: < - Concentration Limit							
Result:			-1.78 > -5.00				
Message			CCB Passed				
Action			Continue				
1202057166 MSD	1	21	110	5.81	3/8/2010@15:30:01		
248199001	1	22	-1.68	0.0348	3/8/2010@15:30:54		
248238001	1	23	-1.98	0.0191	3/8/2010@15:31:46		
248238002	1	24	-1.94	0.0214	3/8/2010@15:32:39		
1202057164 MS	1	20	71.8	3.84	3/8/2010@15:33:32		
248242001	1	25	-1.93	0.0217	3/8/2010@15:34:25		
248245001	1	26	-2.35	1.99e-4	3/8/2010@15:35:17		
248257001	1	27	-2.49	-0.00739	3/8/2010@15:36:09		
248257002	1	28	-1.86	0.0256	3/8/2010@15:37:01		
1202057164 MS	1	20	106	5.61	3/8/2010@15:37:54		
WCN100308-03	1	S3	104	5.52	3/8/2010@15:38:47		CCV
Known Conc:			100				
DQM Test: > + Percent Relative Difference							
Result:			4.3 < 10.0				
Message			CCV Passed				
Action			Continue				
DQM Test: < - Percent Relative Difference							
Result:			4.3 < 10.0				
Message			CCV Passed				
Action			Continue				
WCN100308-08	1	S7	-0.768	0.0819	3/8/2010@15:40:39		CCB
Known Conc:			0.00				
DQM Test: > + Concentration Limit							
Result:			-0.768 < 5.00				
Message			CCB Passed				
Action			Continue				
DQM Test: < - Concentration Limit							
Result:			-0.768 > -5.00				
Message			CCB Passed				
Action			Continue				
1202057112 959204 MB	1	29	-2.19	0.00819	3/8/2010@15:42:28		
1202057119 LCS	1	30	31.1	1.73	3/8/2010@15:43:18	25.00	
248110001	1	31	-0.304	0.106	3/8/2010@15:44:13		
248110002	1	32	-1.46	0.0463	3/8/2010@15:45:07		
248110003	1	33	-2.31	0.00237	3/8/2010@15:46:00		
248110004	1	34	-2.16	0.00990	3/8/2010@15:46:54		
248110005	1	35	-0.698	0.0856	3/8/2010@15:47:47		
248110006	1	36	-1.47	0.0458	3/8/2010@15:48:41		
248110007	1	37	-1.24	0.0576	3/8/2010@15:49:33		
248110008	1	38	-0.761	0.0823	3/8/2010@15:50:26		
WCN100308-03	1	S3	106	5.60	3/8/2010@15:51:19		CCV
Known Conc:			100				
DQM Test: > + Percent Relative Difference							

			Result:	5.9 < 10.0				
			Message	CCV Passed				
			Action	Continue				
DQM Test: < - Percent Relative Difference								
			Result:	5.9 < 10.0				
			Message	CCV Passed				
			Action	Continue				
WCN100308-08	1	S7		-1.95	0.0205	3/8/2010@15:53:09		CCB
			Known Conc:	0.00				
DQM Test: > + Concentration Limit								
			Result:	-1.95 < 5.00				
			Message	CCB Passed				
			Action	Continue				
DQM Test: < - Concentration Limit								
			Result:	-1.95 > -5.00				
			Message	CCB Passed				
			Action	Continue				
248118001	1	39		0.0365	0.124	3/8/2010@15:54:59		
248118002	1	40		-2.19	0.00813	3/8/2010@15:55:52		
248118003	1	41		-0.754	0.0827	3/8/2010@15:56:45		
248118004	1	42		-1.55	0.0414	3/8/2010@15:57:37		
248118005	1	43		-1.86	0.0257	3/8/2010@15:58:28		
248118006	1	44		-0.195	0.112	3/8/2010@15:59:22		
248118007	1	45		-2.48	-0.00657	3/8/2010@16:00:13		
248189001	1	46		1.50	0.200	3/8/2010@16:01:07		
1202057113 DUP	1	47		1.10	0.179	3/8/2010@16:02:01		
1202057115 MS	1	48		98.4	5.21	3/8/2010@16:02:55		
WCN100308-03	1	S3		106	5.63	3/8/2010@16:03:48		CCV
			Known Conc:	100				
DQM Test: > + Percent Relative Difference								
			Result:	6.5 < 10.0				
			Message	CCV Passed				
			Action	Continue				
DQM Test: < - Percent Relative Difference								
			Result:	6.5 < 10.0				
			Message	CCV Passed				
			Action	Continue				
WCN100308-08	1	S7		-2.33	0.00121	3/8/2010@16:05:39		CCB
			Known Conc:	0.00				
DQM Test: > + Concentration Limit								
			Result:	-2.33 < 5.00				
			Message	CCB Passed				
			Action	Continue				
DQM Test: < - Concentration Limit								
			Result:	-2.33 > -5.00				
			Message	CCB Passed				
			Action	Continue				
1202057117 MSD	1	49		97.7	5.18	3/8/2010@16:07:29		
248189002	1	50		0.509	0.148	3/8/2010@16:08:23		
1202057114 DUP	1	51		0.322	0.138	3/8/2010@16:09:16		
1202057116 MS	1	52		93.9	4.98	3/8/2010@16:10:09		
1202057118 MSD	1	53		93.9	4.98	3/8/2010@16:11:02		
1202054781 958165 MB	1	54		-2.89	-0.0281	3/8/2010@16:11:55		
1202054788 LCS	1	55		20.3	1.17	3/8/2010@16:12:47	25.00	
247918001	1	56		-1.17	0.0613	3/8/2010@16:13:39		
247918002	1	57		-1.63	0.0371	3/8/2010@16:14:33		
247918003	1	58		-2.35	2.32e-4	3/8/2010@16:15:25		
WCN100308-03	1	S3		106	5.59	3/8/2010@16:16:17		CCV
			Known Conc:	100				
DQM Test: > + Percent Relative Difference								
			Result:	5.7 < 10.0				
			Message	CCV Passed				
			Action	Continue				
DQM Test: < - Percent Relative Difference								
			Result:	5.7 < 10.0				
			Message	CCV Passed				
			Action	Continue				
WCN100308-08	1	S7		-2.61	-0.0134	3/8/2010@16:18:09		CCB

Known Conc:			0.00					
DQM Test: > + Concentration Limit								
Result:			-2.61 < 5.00					
Message			CCB Passed					
Action			Continue					
DQM Test: < - Concentration Limit								
Result:			-2.61 > -5.00					
Message			CCB Passed					
Action			Continue					
247918004	1	59	-1.83	0.0268	3/8/2010@16:19:58			
1202054782	DUP	1	60	-1.86	0.0252	3/8/2010@16:20:49		
1202054784	MS	1	61	88.6	4.71	3/8/2010@16:21:44		
1202054786	MSD	1	62	102	5.39	3/8/2010@16:22:39		
247918005		1	63	-1.63	0.0372	3/8/2010@16:23:32		
1202054783	DUP	1	64	-2.35	2.22e-4	3/8/2010@16:24:26		
1202054785	MS	1	65	103	5.44	3/8/2010@16:25:20		
1202054787	MSD	1	66	99.0	5.24	3/8/2010@16:26:12		
247918006		1	67	-0.953	0.0724	3/8/2010@16:27:06		
247918007		1	68	0.145	0.129	3/8/2010@16:28:00		
WCN100308-03	1	S3	105	5.54	3/8/2010@16:28:51			CCV
Known Conc:			100					
DQM Test: > + Percent Relative Difference								
Result:			4.6 < 10.0					
Message			CCV Passed					
Action			Continue					
DQM Test: < - Percent Relative Difference								
Result:			4.6 < 10.0					
Message			CCV Passed					
Action			Continue					
WCN100308-08	1	S7	-2.34	4.90e-4	3/8/2010@16:30:42			CCB
Known Conc:			0.00					
DQM Test: > + Concentration Limit								
Result:			-2.34 < 5.00					
Message			CCB Passed					
Action			Continue					
DQM Test: < - Concentration Limit								
Result:			-2.34 > -5.00					
Message			CCB Passed					
Action			Continue					
248009001	1	69	-2.44	-0.00446	3/8/2010@16:32:32			
248009002	1	70	-1.42	0.0484	3/8/2010@16:33:25			
248009003	1	71	2.15	0.233	3/8/2010@16:34:17			
248009004	1	72	-1.18	0.0606	3/8/2010@16:35:10			
248009005	1	73	-2.05	0.0157	3/8/2010@16:36:03			
248025001	1	74	-2.44	-0.00448	3/8/2010@16:36:55			
248025002	1	75	-1.60	0.0388	3/8/2010@16:37:48			
248025004	1	76	-0.787	0.0809	3/8/2010@16:38:42			
248025006	1	77	-0.371	0.102	3/8/2010@16:39:36			
248422001	1	78	-2.28	0.00369	3/8/2010@16:40:31			
WCN100308-03	1	S3	102	5.40	3/8/2010@16:41:23			CCV
Known Conc:			100					
DQM Test: > + Percent Relative Difference								
Result:			2.0 < 10.0					
Message			CCV Passed					
Action			Continue					
DQM Test: < - Percent Relative Difference								
Result:			2.0 < 10.0					
Message			CCV Passed					
Action			Continue					
WCN100308-08	1	S7	-2.30	0.00277	3/8/2010@16:43:15			CCB
Known Conc:			0.00					
DQM Test: > + Concentration Limit								
Result:			-2.30 < 5.00					
Message			CCB Passed					
Action			Continue					
DQM Test: < - Concentration Limit								
Result:			-2.30 > -5.00					
Message			CCB Passed					

		Action	Continue					
248422002	1	79	-1.20	0.0595	3/8/2010@16:45:06			
1202061930 961278 MB	1	80	-1.83	0.0272	3/8/2010@16:46:01			
1202061932 LCS	1	81	-1.96	0.0203	3/8/2010@16:46:53			
247819001	1	82	110	5.83	3/8/2010@16:47:47			
1202061931 DUP	1	83	184	9.64	3/8/2010@16:48:41			
WCN100308-03	1	S3	106	5.59	3/8/2010@16:49:33			CCV
Known Conc:		100						
DQM Test: > + Percent Relative Difference								
Result:		5.7 < 10.0						
Message		CCV Passed						
Action		Continue						
DQM Test: < - Percent Relative Difference								
Result:		5.7 < 10.0						
Message		CCV Passed						
Action		Continue						
WCN100308-08	1	S7	-2.34	3.67e-4	3/8/2010@16:51:24			CCB
Known Conc:		0.00						
DQM Test: > + Concentration Limit								
Result:		-2.34 < 5.00						
Message		CCB Passed						
Action		Continue						
DQM Test: < - Concentration Limit								
Result:		-2.34 > -5.00						
Message		CCB Passed						
Action		Continue						

Analyte Properties Table for OM_3-8-2010_14-58-05.OMN

Property	Channel 1
	TCYANIDE
Concentration Units	ug/L
Calibration Fit Type	First Order
Clear Calibration	True
Force Through Zero	False
Calibration Weighting	None
Auto Dilution Trigger	True
% of High Standard	100
Quik Chem Method	10-204-00-1-A
Chemistry	Direct/Bipolar
Calibration by Height	False
Inject to Peak Start	22
Peak Base Width	39

Channel 1: Current View


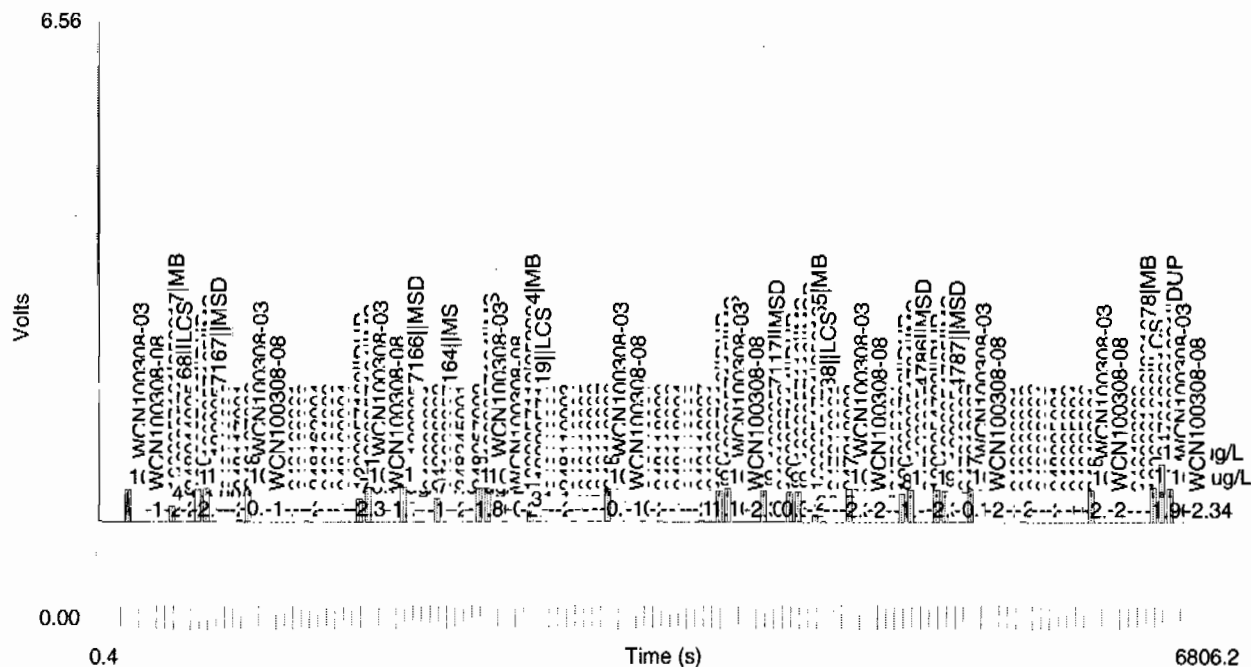


Table 1: TCYANIDE

	Conc. (ug/L)	Rep	Peak Area (Volt-s)	Peak Height (Volts)	% Residual	Detection Date	Detection Time
1	200	1	10.4	0.692	0.2	3/8/2010	10:26:48
2	150	1	7.82	0.567	0.7	3/8/2010	10:27:40
3	100	1	5.36	0.353	-1.3	3/8/2010	10:28:32
4	50.0	1	2.85	0.199	-5.1	3/8/2010	10:29:25
5	10.0	1	0.644	0.0420	-0.6	3/8/2010	10:30:18
6	5.00	1	0.400	0.0240	-4.6	3/8/2010	10:31:12
7	0.00	1	-0.0189	-0.00306		3/8/2010	10:32:06

Figure 1: TCYANIDE

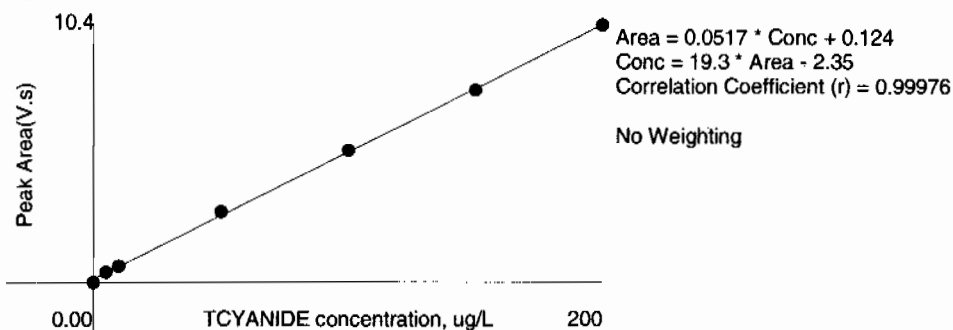

Ion Chromatography

Prep Logbook

Ion Chromatography (IC)

Batch ID:	962077.0	Verified by:		Type	Sample Id	Description	Serial Number	Spike Amount	Spike Units
Analyst:	Mary Sherwood			LCS	1202063613	GEL-ANION-4C Spiking Solution	UIC100224SPK	.8	mL
Method:	EPA 300.0 PREP			MS	1202063609	GEL-ANION-4C Spiking Solution	UIC100224SPK	.8	mL
Lab SOP:	GL-GC-E-086 REV# 17			MS	1202063610	GEL-ANION-4C Spiking Solution	UIC100224SPK	.8	mL
Instrument:	Sartorius Balance B-001			MSD	1202063611	GEL-ANION-4C Spiking Solution	UIC100224SPK	.8	mL
				MSD	1202063612	GEL-ANION-4C Spiking Solution	UIC100224SPK	.8	mL

Sample ID	Run Date	Matrix	Initial Weight (g)	Final Volume (mL)	Prep Factor (mL/g)	pH Check 1
1202063606 MB	19-MAR-2010 13:15:00	Soil	4	40	10	
1202063613 LCS	19-MAR-2010 13:15:00	Soil	4	40	10	
248110001	19-MAR-2010 13:15:00	Soil	4	40	10	
1202063607 DUP (248110001)	19-MAR-2010 13:15:00	Soil	4	40	10	
1202063609 MS (248110001)	19-MAR-2010 13:15:00	Soil	4	40	10	
1202063611 MSD (248110001)	19-MAR-2010 13:15:00	Soil	4	40	10	
248110002	19-MAR-2010 13:15:00	Soil	4	40	10	
248110003	19-MAR-2010 13:15:00	Soil	4	40	10	
248110004	19-MAR-2010 13:15:00	Soil	4	40	10	
248110005	19-MAR-2010 13:15:00	Soil	4	40	10	
248110006	19-MAR-2010 13:15:00	Soil	4	40	10	
248110007	19-MAR-2010 13:15:00	Soil	4	40	10	
248110008	19-MAR-2010 13:15:00	Soil	4	40	10	
248118001	19-MAR-2010 13:15:00	Soil	4	40	10	
248118002	19-MAR-2010 13:15:00	Soil	4	40	10	
248118003	19-MAR-2010 13:15:00	Soil	4	40	10	
248118004	19-MAR-2010 13:15:00	Soil	4	40	10	
248118005	19-MAR-2010 13:15:00	Soil	4	40	10	
248118006	19-MAR-2010 13:15:00	Soil	4	40	10	
248118007	19-MAR-2010 13:15:00	Soil	4	40	10	
1202063608 DUP (248118007)	19-MAR-2010 13:15:00	Soil	4	40	10	
1202063610 MS (248118007)	19-MAR-2010 13:15:00	Soil	4	40	10	
1202063612 MSD (248118007)	19-MAR-2010 13:15:00	Soil	4	40	10	

Analytical Logbook version 1 11-04-2002

GEL Laboratories LLC

Prep Logbook

Batch ID: 962077.0
Analyst: Mary Sherwood
Method: EPA 300.0 PREP
Lab SOP: GL-GC-E-086 REV# 17
Instrument: Sartorius Balance B-001

Type	Sample Id	Description	Serial Number	Spike Amount	Spike Units
LCS	1202063613	GEL-ANION-4C Spiking Solution	UIC100224SPK	.8	mL
MS	1202063609	GEL-ANION-4C Spiking Solution	UIC100224SPK	.8	mL
MS	1202063610	GEL-ANION-4C Spiking Solution	UIC100224SPK	.8	mL
MSD	1202063611	GEL-ANION-4C Spiking Solution	UIC100224SPK	.8	mL
MSD	1202063612	GEL-ANION-4C Spiking Solution	UIC100224SPK	.8	mL

Sample ID	Run Date	Matrix	Initial Weight (g)	Final Volume (mL)	Prep Factor (mL/g)	pH Check 1
-----------	----------	--------	--------------------	-------------------	--------------------	------------


Reagent/Solvent Lot ID **Description** **Amount** **Comments:**

This is runlog for Sequence 100312.seq for IC6

Sample ID	Run Time	Batch	Dilution	Dataset	Analyst
BLK	03/12/10 11:16		1	100312	MAR1
BLK	03/12/10 11:44		1	100312	MAR1
ICAL-07	03/12/10 12:13		1	100312	MAR1
ICAL-06	03/12/10 12:42		1	100312	MAR1
ICAL-05	03/12/10 13:11		1	100312	MAR1
ICAL-04	03/12/10 13:40		1	100312	MAR1
ICAL-03	03/12/10 14:08		1	100312	MAR1
ICAL-02	03/12/10 14:37		1	100312	MAR1
ICAL-01	03/12/10 15:06		1	100312	MAR1
ICV	03/12/10 15:35		1	100312	MAR1
ICB	03/12/10 16:04		1	100312	MAR1
1202063659	03/12/10 16:33	962090	1	100312	MAR1
1202063663	03/12/10 17:02	962090	1	100312	MAR1
248065001	03/12/10 17:31	962090	1	100312	MAR1
1202063660	03/12/10 18:00	962090	1	100312	MAR1
1202063661	03/12/10 18:29	962090	1	100312	MAR1
1202063662	03/12/10 18:58	962090	1	100312	MAR1
248065002	03/12/10 19:27	962090	1	100312	MAR1
248065003	03/12/10 19:55	962090	1	100312	MAR1
248065004	03/12/10 20:24	962090	1	100312	MAR1
248065005	03/12/10 20:53	962090	1	100312	MAR1
CVH	03/12/10 21:22		1	100312	MAR1
CCB	03/12/10 21:51		1	100312	MAR1
248065006	03/12/10 22:20	962090	1	100312	MAR1
248065007	03/12/10 22:49	962090	1	100312	MAR1
248065008	03/12/10 23:18	962090	1	100312	MAR1
248068001	03/12/10 23:47	962090	1	100312	MAR1

10 AUTOCAL7


Sample Name:	AUTOCAL7	Injection Volume:	1.0
Vial Number:	3	Channel:	CD_1
Sample Type:	standard	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100312an	Sample Amount:	1.0000
Recording Time:	3/12/2010 12:13	Analyst:	MAR1
Run Time (min):	26.00	Column:	AS23-001528; GL GCED86;300;9056

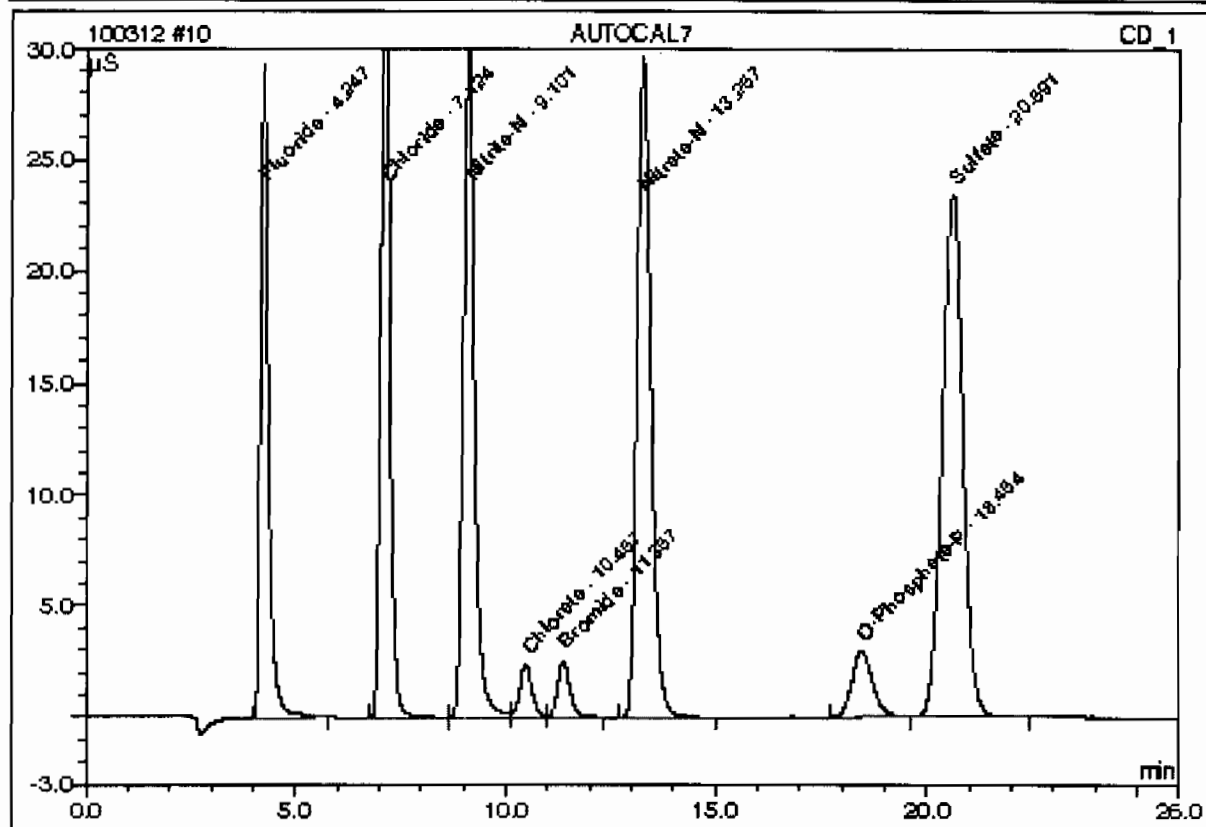

No.	Ret.Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area µS*min	Rel.Area %
1	4.25	Fluoride	10.0000	10.0082		6.22157	11.84
2	7.12	Chloride	20.0000	20.0326		9.47163	18.02
3	9.10	Nitrite-N	10.0000	10.0084		9.13994	17.39
4	10.47	Chlorate	5.0000	5.0492		0.79245	1.51
5	11.37	Bromide	5.0000	5.0195		0.84636	1.61
6	13.26	Nitrate-N	10.0000	10.0123		11.22910	21.36
7	18.45	O-Phosphate-P	5.0000	5.0489		1.68651	3.17
8	20.59	Sulfate	40.0000	40.0441		13.19754	25.11
Total:				105.2231	0.000	52.585	100.00

11 AUTOCAL6


Sample Name:	AUTOCAL6	Injection Volume:	1.0
Vial Number:	4	Channel:	CD_1
Sample Type:	standard	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100312an	Sample Amount:	1.0000
Recording Time:	3/12/2010 12:42	Analyst:	MAR1
Run Time (min):	26.00	Column:	AS23-001528; GL GCE086;300;9056

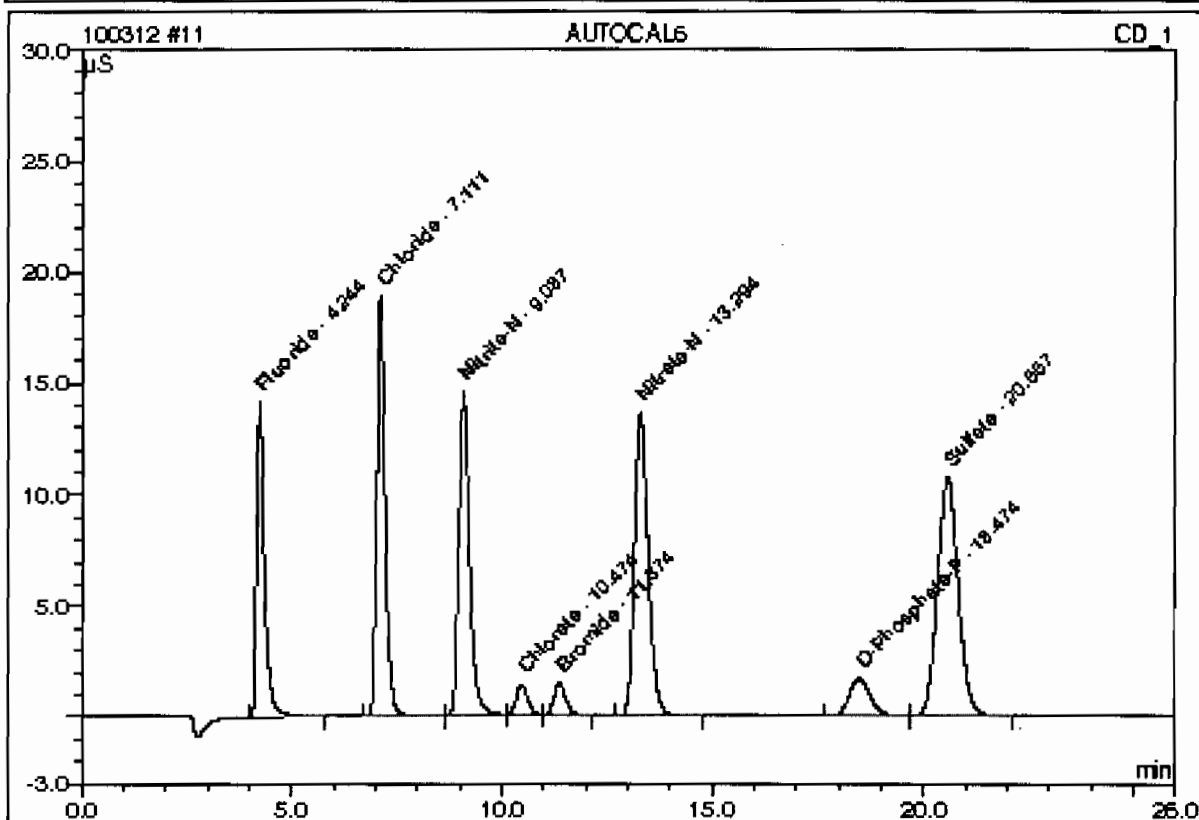

No.	Ret. Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area μS*min	Rel. Area %
1	4.24	Fluoride	5.0000	4.8561		2.99032	12.03
2	7.11	Chloride	10.0000	9.3413		4.33873	17.48
3	9.09	Nitrate-N	5.0000	4.8263		4.34814	17.50
4	10.47	Chlorate	3.0000	2.9358		0.46050	1.85
5	11.37	Bromide	3.0000	2.9362		0.49122	1.98
6	13.29	Nitrate-N	5.0000	4.6985		5.14610	20.71
7	18.47	O-Phosphate-P	3.0000	2.9248		0.95491	3.84
8	20.57	Sulfate	20.0000	18.9050		6.12051	24.63
Total:				51.4240	0.000	24.850	100.00

12 AUTOCAL5


Sample Name:	AUTOCAL5	Injection Volume:	1.0
Vial Number:	5	Channel:	CD_1
Sample Type:	standard	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100312an	Sample Amount:	1.0000
Recording Time:	3/12/2010 13:11	Analyst:	MAR1
Run Time (min):	26.00	Column:	AS23-001528; GL GCE086;300;0056

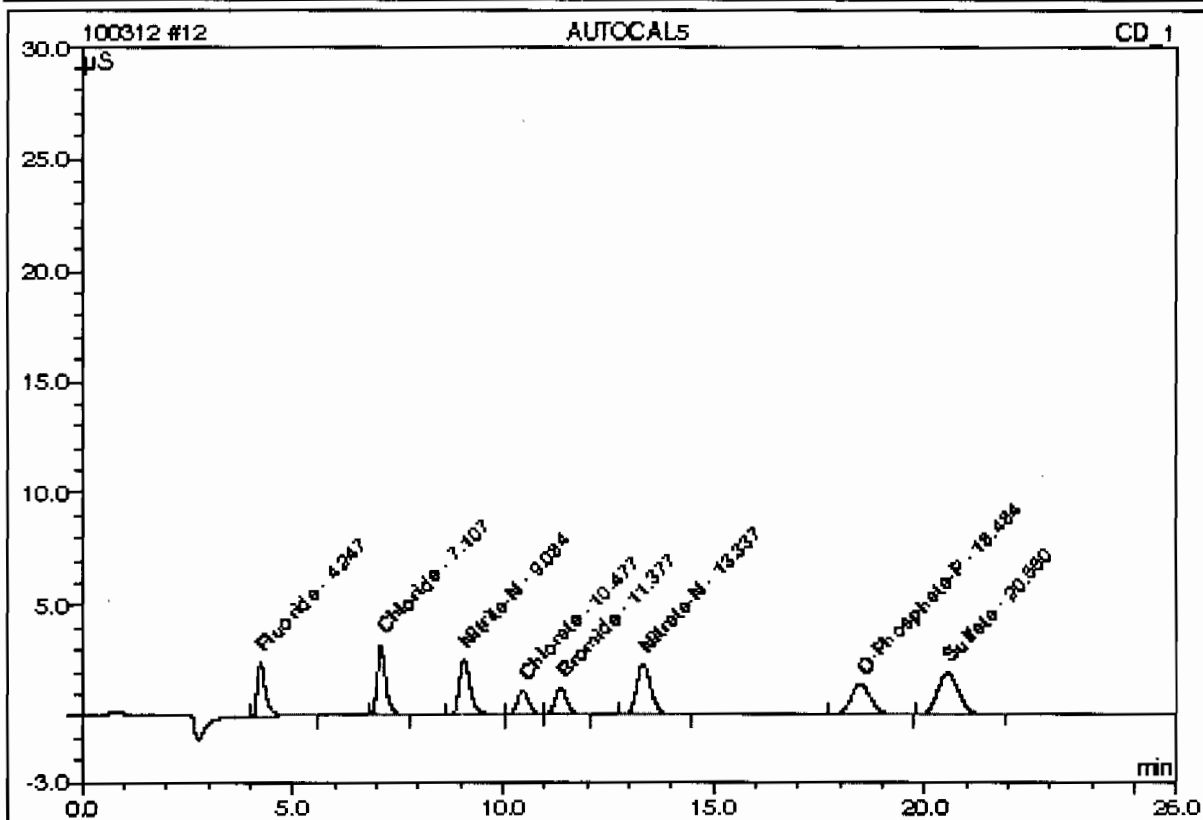

No.	Ret.Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area μS*min	Rel.Area %
1	4.25	Fluoride	1.0000	0.9247		0.54471	9.60
2	7.11	Chloride	2.0000	1.7462		0.75932	13.38
3	9.08	Nitrite-N	1.0000	0.9359		0.79384	13.99
4	10.48	Chlorate	2.5000	2.3846		0.36888	6.50
5	11.38	Bromide	2.5000	2.4488		0.40750	7.18
6	13.34	Nitrate-N	1.0000	0.9150		0.90731	15.99
7	18.48	O-Phosphate-P	2.5000	2.4403		0.78917	13.90
8	20.55	Sulfate	4.0000	3.6492		1.10495	19.47
Total:				15.4446	0.000	5.676	100.00

13 AUTOCAL4


Sample Name:	AUTOCAL4	Injection Volume:	1.0
Vial Number:	6	Channel:	CD_1
Sample Type:	standard	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100312an	Sample Amount:	1.0000
Recording Time:	3/12/2010 13:40	Analyst:	MAR1
Run Time (min):	26.00	Column:	AS23-001528; GLGCED86;300;9056

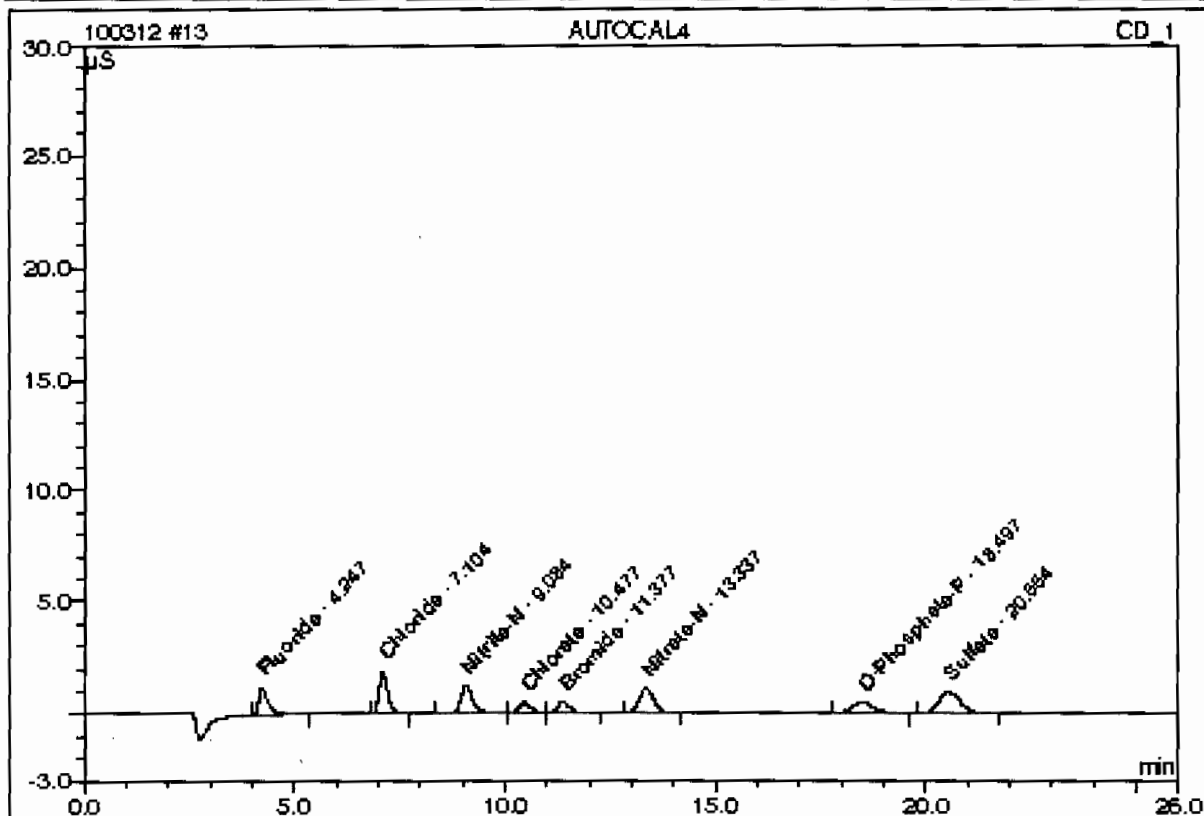

No.	Ret. Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area µS*min	Rel. Area %
1	4.25	Fluoride	0.5000	0.5181		0.29079	10.43
2	7.10	Chloride	1.0000	1.0724		0.44828	16.11
3	9.08	Nitrite-N	0.5000	0.5242		0.41773	14.98
4	10.48	Chlorate	1.0000	1.0431		0.15901	5.70
5	11.38	Bromide	1.0000	1.0406		0.17190	6.16
6	13.34	Nitrate-N	0.5000	0.5021		0.43247	15.51
7	18.50	O-Phosphate-P	1.0000	0.9735		0.29999	10.76
8	20.55	Sulfate	2.0000	2.0444		0.56783	20.36
Total:				7.7184	0.000	2.789	100.00

14 AUTOCAL3


Sample Name:	AUTOCAL3	Injection Volume:	1.0
Vial Number:	7	Channel:	CD_1
Sample Type:	standard	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100312an	Sample Amount:	1.0000
Recording Time:	3/12/2010 14:08	Analyst:	MAR1
Run Time (min):	26.00	Column:	AS23-001528; GL GC ED86;300;9056

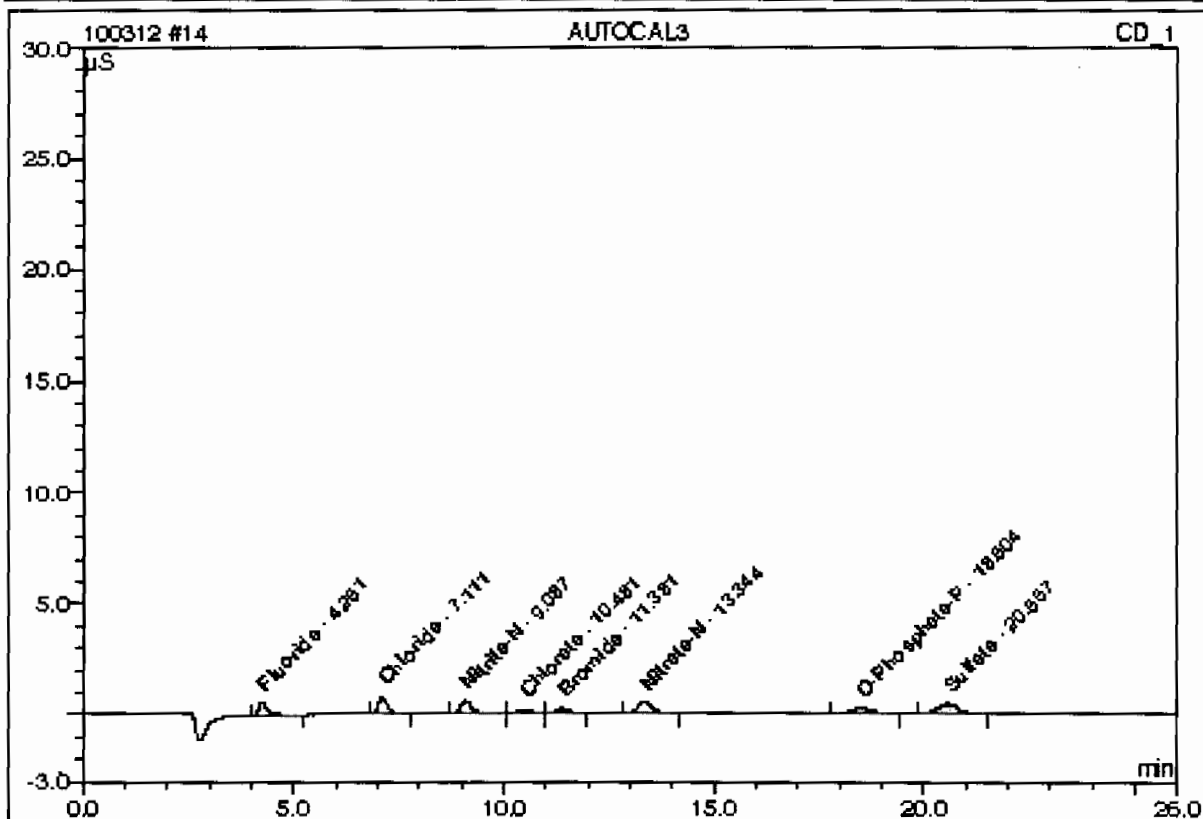

No.	Ret. Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area µS*min	Rel. Area %
1	4.25	Fluoride	0.2500	0.2767		0.13273	10.36
2	7.11	Chloride	0.5000	0.6177		0.19612	15.31
3	9.09	Nitrate-N	0.2500	0.2802		0.18850	14.72
4	10.48	Chlorate	0.5000	0.4873		0.07006	5.47
5	11.38	Bromide	0.5000	0.4930		0.07924	6.19
6	13.34	Nitrate-N	0.2500	0.3124		0.20857	16.29
7	18.50	O-Phosphate-P	0.5000	0.4938		0.13887	10.84
8	20.57	Sulfate	1.0000	1.2082		0.26661	20.82
Total:				4.1694	0.000	1.281	100.00

15 AUTOCAL2


Sample Name:	AUTOCAL2	Injection Volume:	1.0
Vial Number:	8	Channel:	CD_1
Sample Type:	standard	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100312an	Sample Amount:	1.0000
Recording Time:	3/12/2010 14:37	Analyst:	MAR1
Run Time (min):	26.00	Column:	AS23-001528; GL GC ED86;300;9056

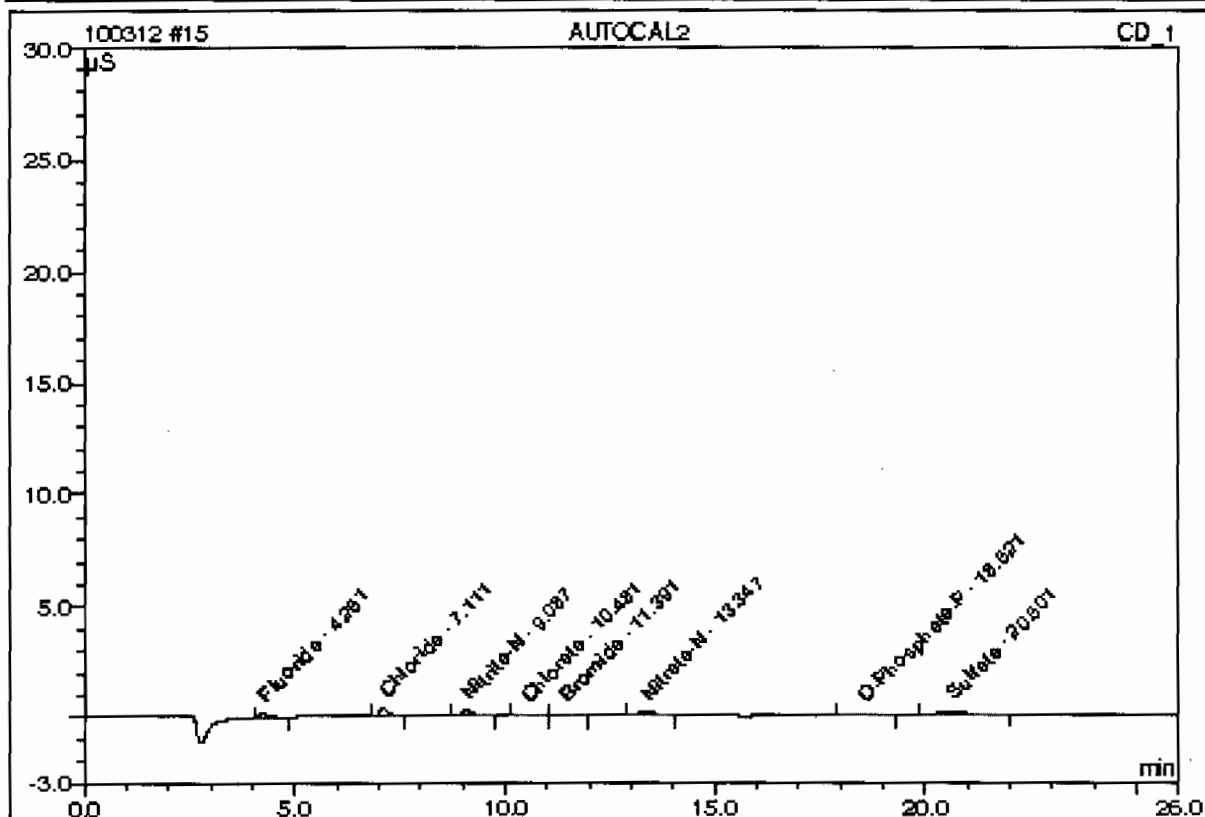

No.	Ret. Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area µS*min	Rel. Area %
1	4.25	Fluoride	0.1000	0.1393		0.05352	9.78
2	7.11	Chloride	0.2000	0.3635		0.09592	17.52
3	9.09	Nitrate-N	0.1000	0.1457		0.07635	13.95
4	10.48	Chlorate	0.2000	0.2155		0.02807	5.13
5	11.39	Bromide	0.2000	0.2128		0.03286	6.00
6	13.35	Nitrate-N	0.1000	0.1770		0.07876	14.39
7	18.52	O-Phosphate-P	0.2000	0.2166		0.04829	8.82
8	20.60	Sulfate	0.4000	0.7224		0.13373	24.43
Total:				2.1926	0.000	0.548	100.00

16 AUTOCAL1

Sample Name:	AUTOCAL1	Injection Volume:	1.0
Vial Number:	9	Channel:	CD_1
Sample Type:	standard	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100312an	Sample Amount:	1.0000
Recording Time:	3/12/2010 15:06	Analyst:	MAR1
Run Time (min):	26.00	Column:	AS23-001528; GL GC E086; 300; 9056

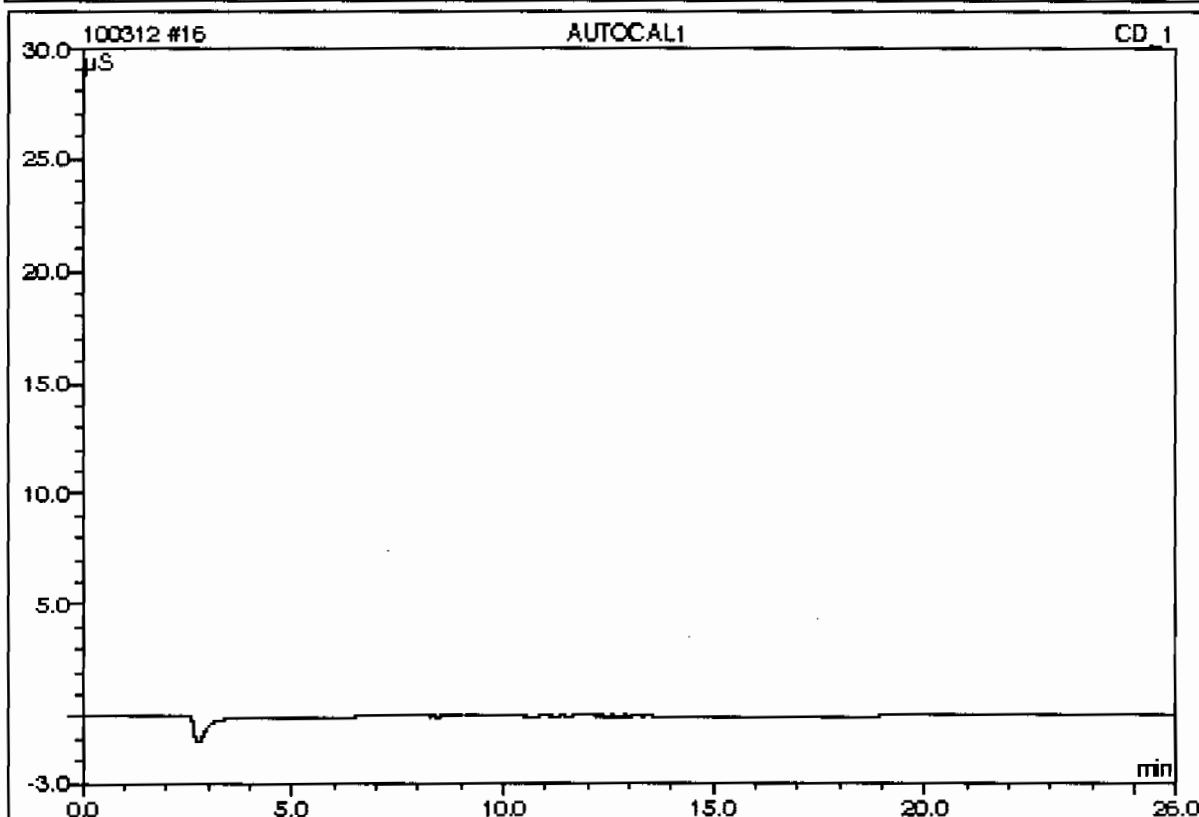

No.	Ret. Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area µS*min	Rel. Area %
n.a.	n.a.	Fluoride	0.0000	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Chloride	0.0000	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Nitrite-N	0.0000	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Chlorate	0.0000	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Bromide	0.0000	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Nitrate-N	0.0000	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	O-Phosphate-P	0.0000	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Sulfate	0.0000	n.a.	n.a.	n.a.	n.a.
Total:				0.0000	0.000	0.000	0.00

16 AUTOCAL1

Sample Name: AUTOCAL1

Vial Number: 9

Sample Type: standard

Control Program: AS23

Quantif. Method: 100312an

Recording Time: 3/12/2010 15:06

Run Time (min): 26.00

Injection Volume: 1.0

Channel: CD_1







Dilution Factor: 1.0000



Sample Weight: 1.0000

Sample Amount: 1.0000

Analyst: MAR1

Column: AS23-002712; GL GCED86;300;9056

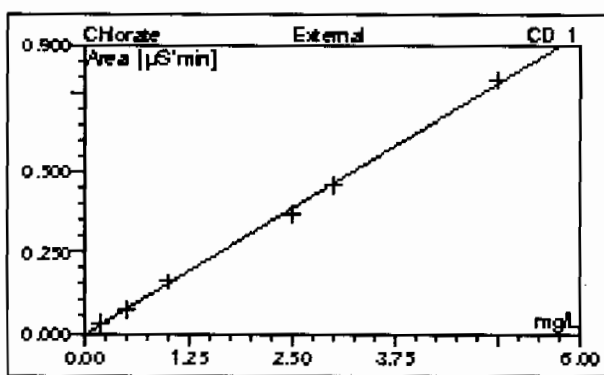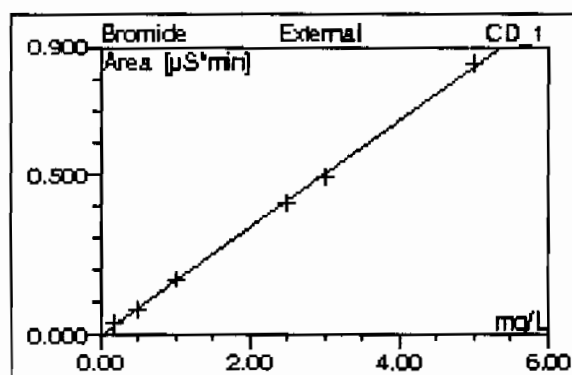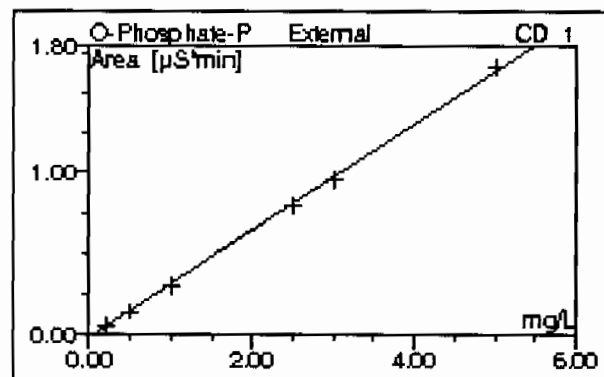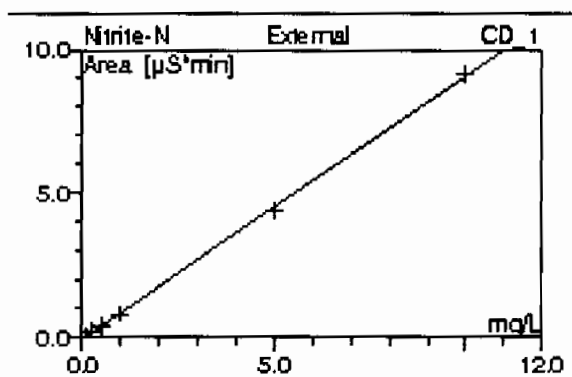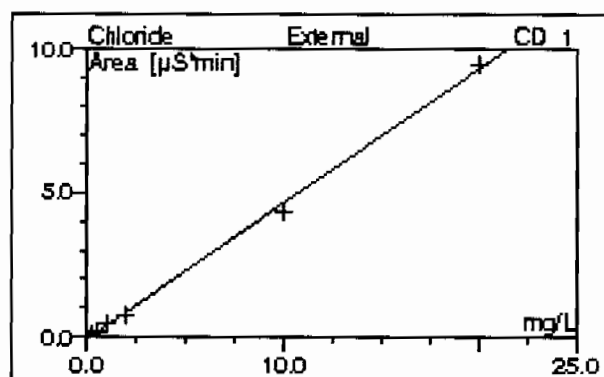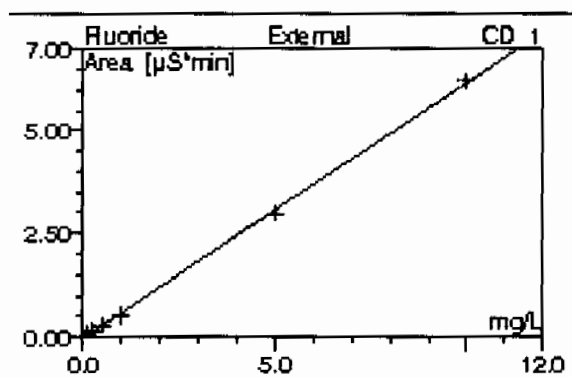


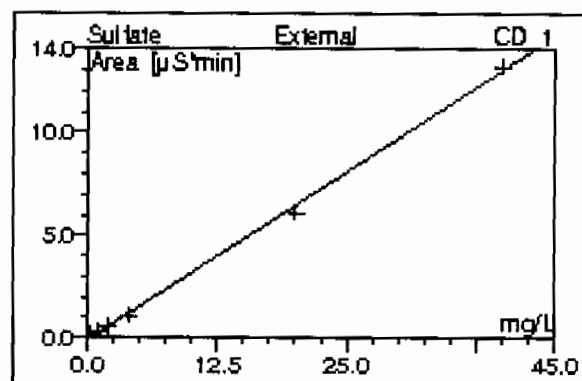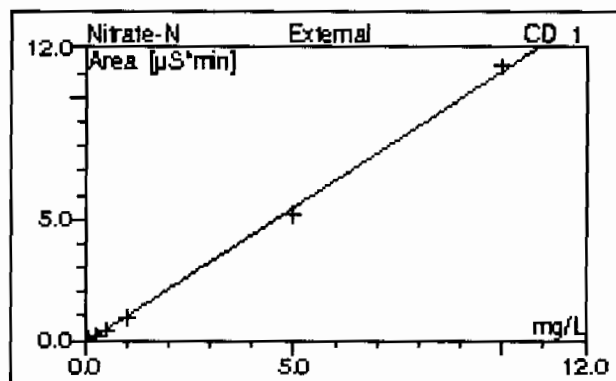

No. CD_1	Ret.Time CD_1 min	Peak Name CD_1	Cal.Type CD_1	Coeff.Det. CD_1 %	Offset CD_1	Slope CD_1	Curve CD_1
n.a.	n.a.	Fluoride	OLO#	99.9627	-0.0330	0.6210	0.0000
n.a.	n.a.	Chloride	OLO#	99.8225	-0.0749	0.4699	0.0000
n.a.	n.a.	Nitrite-N	OLO#	99.9452	-0.0564	0.9115	0.0000
n.a.	n.a.	Chlorate	OLO#	99.8605	-0.0058	0.1574	0.0000
n.a.	n.a.	Bromide	OLO#	99.9304	-0.0029	0.1680	0.0000
n.a.	n.a.	Nitrate-N	OLO#	99.8475	-0.1191	1.1179	0.0000
n.a.	n.a.	O-Phosphate-P	OLO#	99.9176	-0.0239	0.3332	0.0000
n.a.	n.a.	Sulfate	OLO#	99.8762	-0.1033	0.3281	0.0000
Average:				99.8953	-0.0524	0.5134	0.0000

17 WIC100312-02ICV


Sample Name:	WIC100312-02ICV	Injection Volume:	1.0
Vial Number:	10	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100312an	Sample Amount:	1.0000
Recording Time:	3/12/2010 15:35	Analyst:	MAR1
Run Time (min):	26.00	Column:	AS23-001528; GL GCED86;300;9056

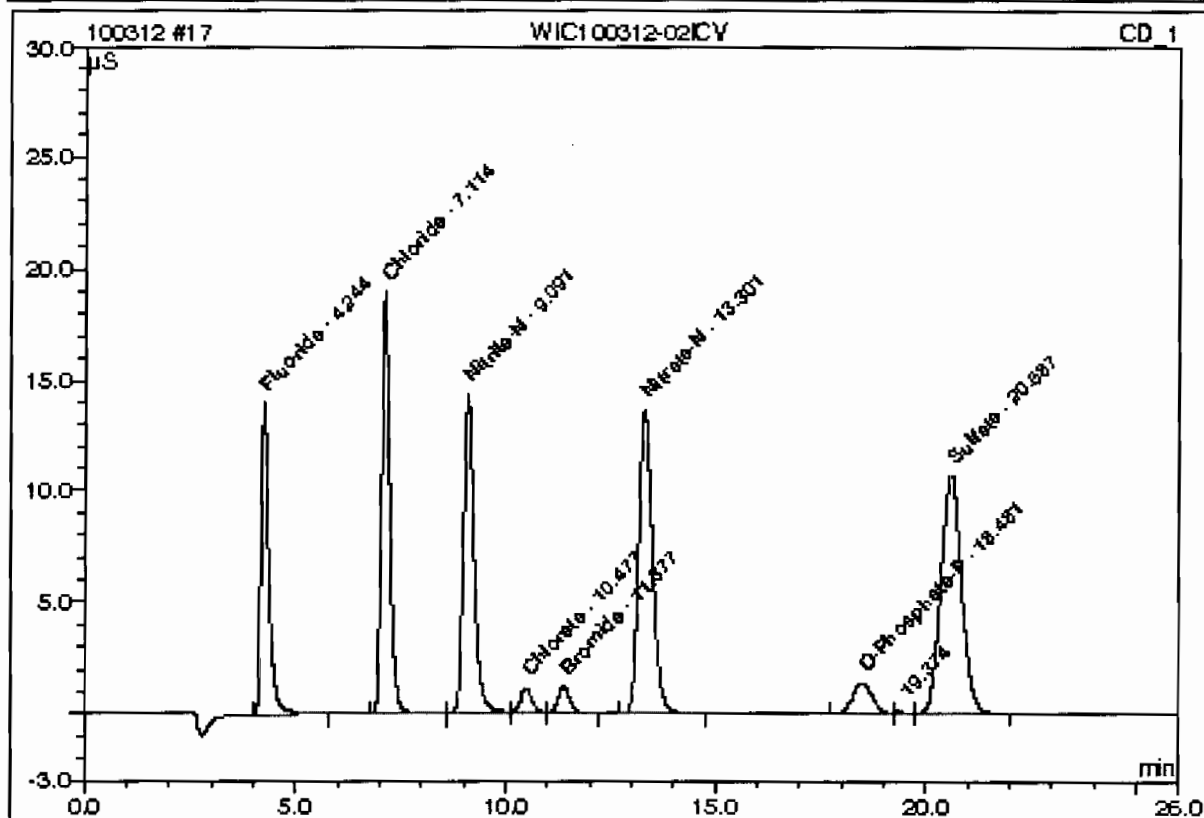

No.	Ret.Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area µS*min	Rel.Area %
1	4.24	Fluoride	n.a.	4.8260		2.96419	12.10
2	7.11	Chloride	n.a.	9.4396		4.36065	17.80
3	9.09	Nitrite-N	n.a.	4.7879		4.30795	17.58
4	10.48	Chlorate	n.a.	2.5037		0.38815	1.58
5	11.38	Bromide	n.a.	2.5123		0.41911	1.71
6	13.30	Nitrate-N	n.a.	4.7318		5.17038	21.10
7	18.48	O-Phosphate-P	n.a.	2.4304		0.78590	3.21
9	20.59	Sulfate	n.a.	18.8328		6.07580	24.80
Total:				50.0645	0.000	24.472	99.88

18 ICB

Sample Name:	ICB	Injection Volume:	1.0
Vial Number:	11	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100312an	Sample Amount:	1.0000
Recording Time:	3/12/2010 16:04	Analyst:	MAR1
Run Time (min):	26.00	Column:	AS23-001528; GL GCED86;300;9056

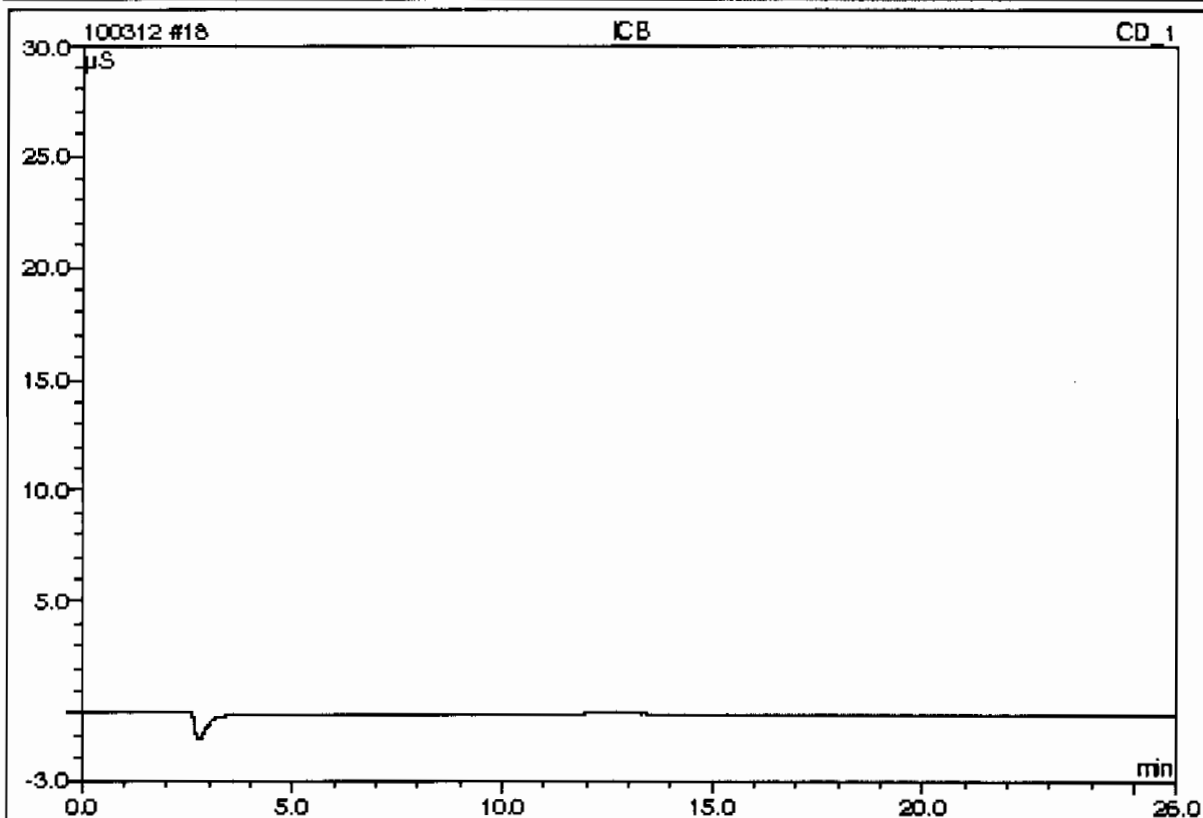

No.	Ret. Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area µS*min	Rel. Area %
n.a.	n.a.	Fluoride	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Chloride	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Nitrite-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Chlorate	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Bromide	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Nitrate-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	O-Phosphate-P	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Sulfate	n.a.	n.a.	n.a.	n.a.	n.a.
Total:				0.0000	0.000	0.000	0.00


This is runlog for Sequence 100319.seq for IC6

Sample ID	Run Time	Batch	Dilution	Dataset	Analyst
BLK	03/19/10 09:38		1	100319	MAR1
BLK	03/19/10 10:04		1	100319	MAR1
ICV	03/19/10 10:31		1	100319	MAR1
ICB	03/19/10 10:58		1	100319	MAR1
1202063590	03/19/10 11:25	962073	1	100319	MAR1
1202063597	03/19/10 11:52	962073	1	100319	MAR1
248025001	03/19/10 12:19	962073	1	100319	MAR1
1202063591	03/19/10 12:45	962073	1	100319	MAR1
1202063593	03/19/10 13:12	962073	1	100319	MAR1
1202063595	03/19/10 13:39	962073	1	100319	MAR1
248025002	03/19/10 14:06	962073	1	100319	MAR1
248025003	03/19/10 14:33	962073	1	100319	MAR1
248025004	03/19/10 15:00	962073	1	100319	MAR1
248025005	03/19/10 15:26	962073	1	100319	MAR1
CVH	03/19/10 15:53		1	100319	MAR1
CCB	03/19/10 16:20		1	100319	MAR1
248025006	03/19/10 16:47	962073	1	100319	MAR1
248025007	03/19/10 17:14	962073	1	100319	MAR1
248041001	03/19/10 17:41	962073	1	100319	MAR1
248041002	03/19/10 18:08	962073	1	100319	MAR1
248041003	03/19/10 18:35	962073	1	100319	MAR1
248041004	03/19/10 19:01	962073	1	100319	MAR1
248041005	03/19/10 19:28	962073	1	100319	MAR1
1202063592	03/19/10 19:55	962073	1	100319	MAR1
1202063594	03/19/10 20:22	962073	1	100319	MAR1
1202063596	03/19/10 20:49	962073	1	100319	MAR1
CCV	03/19/10 21:16		1	100319	MAR1
CCB	03/19/10 21:43		1	100319	MAR1

1202063582	03/19/10 22:10 962071 1	100319	MAR1
1202063589	03/19/10 22:37 962071 1	100319	MAR1
248000001	03/19/10 23:04 962071 1	100319	MAR1
1202063583	03/19/10 23:30 962071 1	100319	MAR1
1202063585	03/19/10 23:57 962071 1	100319	MAR1

16 WIC100319-02ICV


Sample Name:	WIC100319-02ICV	Injection Volume:	1.0
Vial Number:	3	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100311an	Sample Amount:	1.0000
Recording Time:	3/19/2010 10:31	Analyst:	MAR1
Run Time (min):	24.00	Column:	AS23-001528; GL GC E086;300;9056

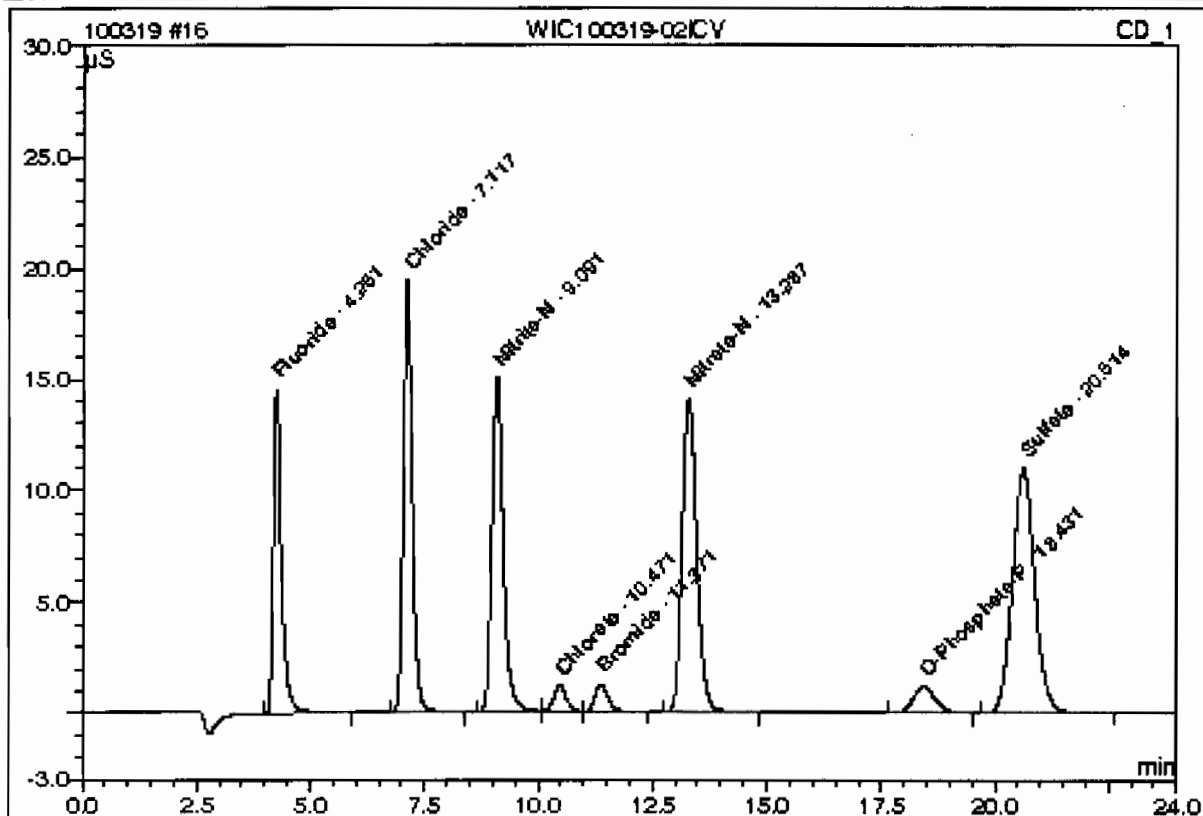

No.	Ret. Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area µS*min	Rel. Area %
1	4.25	Fluoride	n.a.	4.8208		3.08031	12.21
2	7.12	Chloride	n.a.	9.2239		4.42948	17.67
3	9.09	Nitrite-N	n.a.	4.8059		4.46472	17.81
4	10.47	Chlorate	n.a.	2.6276		0.41076	1.64
5	11.37	Bromide	n.a.	2.6109		0.43832	1.75
6	13.29	Nitrate-N	n.a.	4.6689		5.28947	21.10
7	18.43	O-Phosphate-P	n.a.	2.0940		0.66759	2.66
8	20.61	Sulfate	n.a.	18.8821		6.31278	25.18
Total:				49.7341	0.000	25.073	100.00

17 ICB

Sample Name:	ICB	Injection Volume:	1.0
Vial Number:	4	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100311an	Sample Amount:	1.0000
Recording Time:	3/19/2010 10:58	Analyst:	MAR1
Run Time (min):	24.00	Column:	AS23-001528; GL GCE086;300;9056

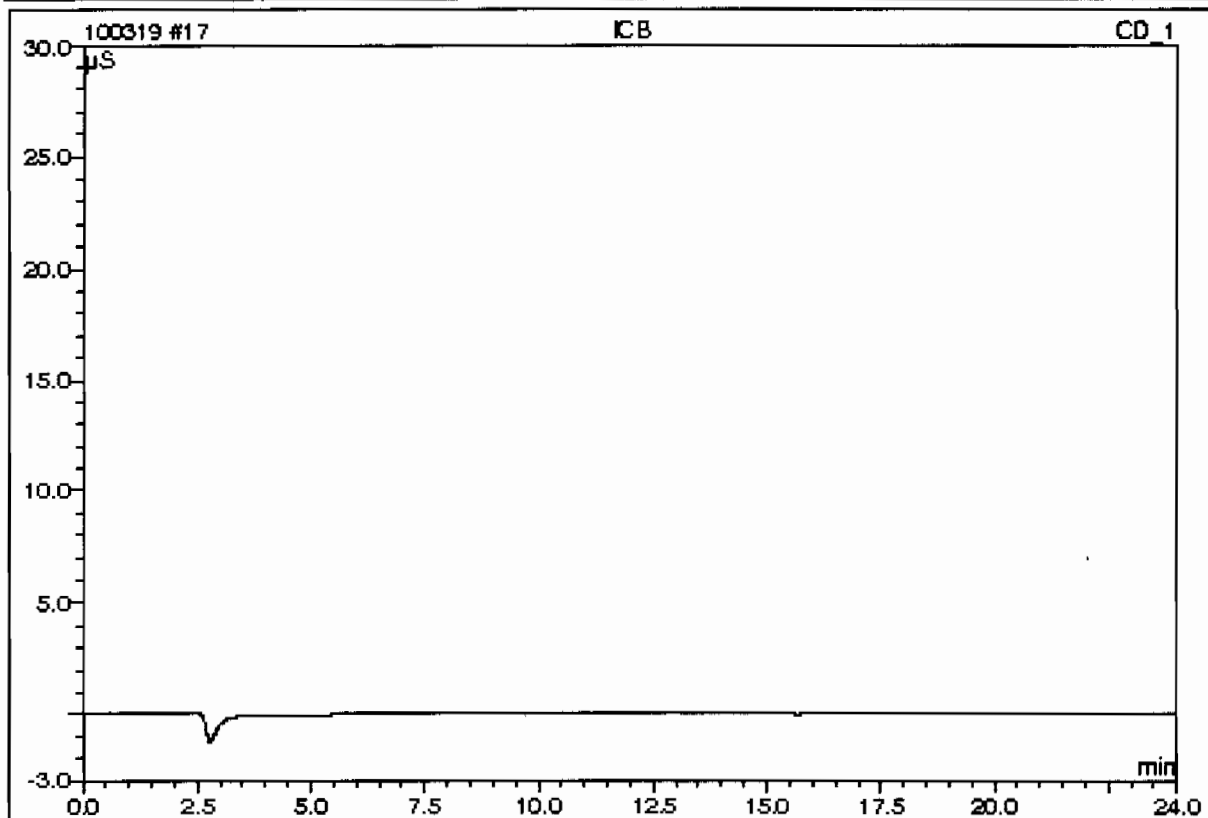

No.	Ret. Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area µS*min	Rel. Area %
n.a.	n.a.	Fluoride	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Chloride	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Nitrite-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Chlorate	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Bromide	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Nitrate-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	O-Phosphate-P	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Sulfate	n.a.	n.a.	n.a.	n.a.	n.a.
Total:				0.0000	0.000	0.000	0.00


This is runlog for Sequence 100319.seq for IC6

Sample ID	Run Time	Batch	Dilution	Dataset	Analyst
1202063587	03/20/10 00:24	962071	1	100319	MAR1
248000002	03/20/10 00:51	962071	1	100319	MAR1
248000003	03/20/10 01:18	962071	1	100319	MAR1
248000004	03/20/10 01:45	962071	1	100319	MAR1
248000005	03/20/10 02:12	962071	1	100319	MAR1
CVH	03/20/10 02:39		1	100319	MAR1
CCB	03/20/10 03:06		1	100319	MAR1
248002001	03/20/10 03:33	962071	1	100319	MAR1
248002002	03/20/10 04:00	962071	1	100319	MAR1
248002003	03/20/10 04:27	962071	1	100319	MAR1
248002004	03/20/10 04:53	962071	1	100319	MAR1
248002005	03/20/10 05:20	962071	1	100319	MAR1
248002006	03/20/10 05:47	962071	1	100319	MAR1
CCV	03/20/10 06:14		1	100319	MAR1
CCB	03/20/10 06:41		1	100319	MAR1
248002007	03/20/10 07:08	962071	1	100319	MAR1
248002008	03/20/10 07:35	962071	1	100319	MAR1
1202063584	03/20/10 08:02	962071	1	100319	MAR1
1202063586	03/20/10 08:29	962071	1	100319	MAR1
1202063588	03/20/10 08:56	962071	1	100319	MAR1
CVH	03/20/10 09:23		1	100319	MAR1
CCB	03/20/10 09:49		1	100319	MAR1
1202063606	03/20/10 10:16	962078	1	100319	MAR1
1202063613	03/20/10 10:43	962078	1	100319	MAR1
248110001	03/20/10 11:10	962078	1	100319	MAR1
1202063607	03/20/10 11:37	962078	1	100319	MAR1
1202063609	03/20/10 12:04	962078	1	100319	MAR1
1202063611	03/20/10 12:31	962078	1	100319	MAR1

248110002	03/20/10 12:58 962078 1	100319	MAR1
248110003	03/20/10 13:25 962078 1	100319	MAR1
248110004	03/20/10 13:52 962078 1	100319	MAR1
248110005	03/20/10 14:19 962078 1	100319	MAR1
CCV	03/20/10 14:45 1	100319	MAR1
CCB	03/20/10 15:12 1	100319	MAR1
248110006	03/20/10 15:39 962078 1	100319	MAR1
248110007	03/20/10 16:06 962078 1	100319	MAR1
248110008	03/20/10 16:33 962078 1	100319	MAR1
248118001	03/20/10 17:00 962078 1	100319	MAR1
248118002	03/20/10 17:01 962078 1	100319	MAR1
248118003	03/20/10 17:01 962078 1	100319	MAR1
248118004	03/20/10 17:01 962078 1	100319	MAR1
248118005	03/20/10 17:01 962078 1	100319	MAR1
CVH	03/20/10 17:01 1	100319	MAR1
CCB	03/20/10 17:01 1	100319	MAR1
248118006	03/20/10 17:01 962078 1	100319	MAR1
248118007	03/20/10 17:01 962078 1	100319	MAR1
1202063608	03/20/10 17:01 962078 1	100319	MAR1
1202063610	03/20/10 17:02 962078 1	100319	MAR1
1202063612	03/20/10 17:02 962078 1	100319	MAR1
CCV	03/20/10 17:02 1	100319	MAR1
CCB	03/20/10 17:02 1	100319	MAR1

67 WIC100319-02CVH


Sample Name:	WIC100319-02CVH	Injection Volume:	1.0
Vial Number:	4	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100311an	Sample Amount:	1.0000
Recording Time:	3/20/2010 9:23	Analyst:	MAR1
Run Time (min):	24.00	Column:	AS23-001528; GL GCED86;300;9056

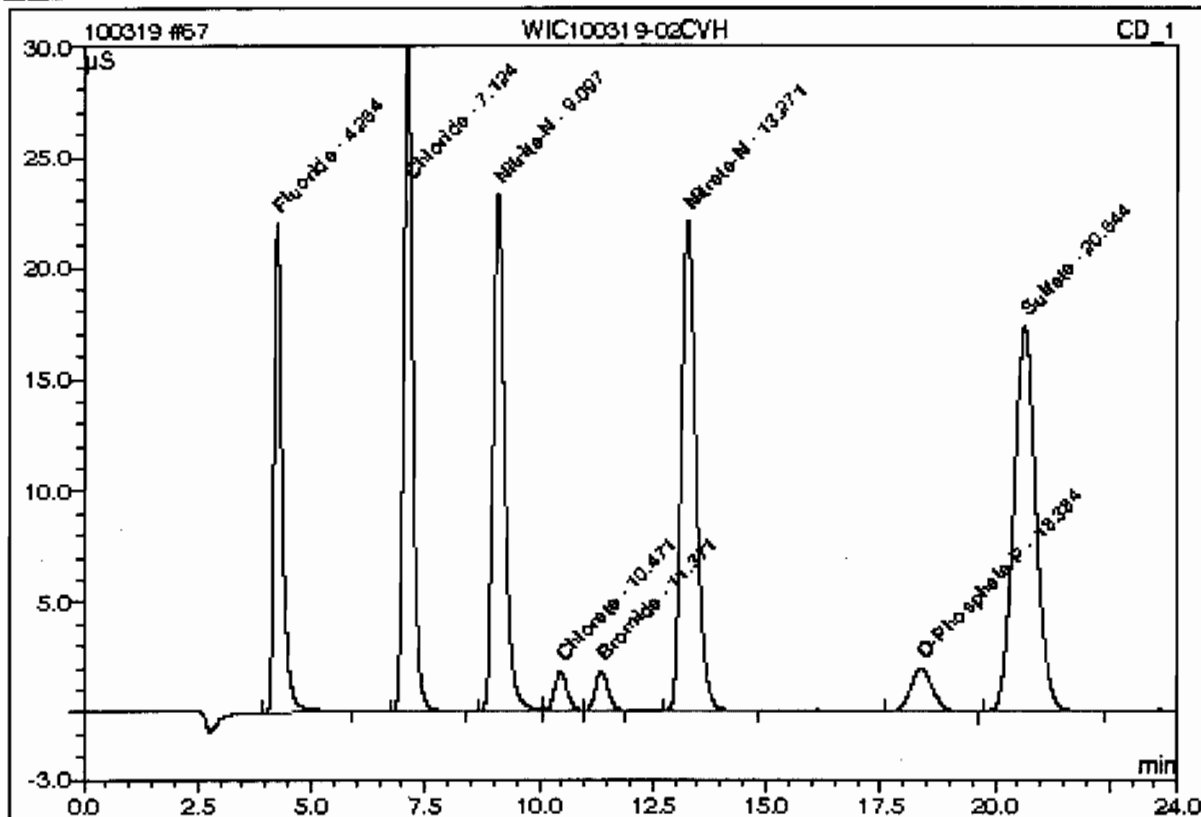

No.	Ret. Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area µS*min	Rel. Area %
1	4.25	Fluoride	n.a.	7.3290		4.87235	12.03
2	7.12	Chloride	n.a.	14.4082		8.96312	17.93
3	9.10	Nitrite-N	n.a.	7.3580		8.87612	17.71
4	10.47	Chlorate	n.a.	3.7179		0.58307	1.50
5	11.37	Bromide	n.a.	3.5255		0.59305	1.53
6	13.27	Nitrate-N	n.a.	7.2587		8.30240	21.38
7	18.38	O-Phosphate-P	n.a.	3.3396		1.07784	2.78
8	20.84	Sulfate	n.a.	29.0187		9.78237	25.14
Total:				75.9556	0.000	38.830	100.00

68 CCB


Sample Name:	CCB	Injection Volume:	1.0
Vial Number:	5	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100311an	Sample Amount:	1.0000
Recording Time:	3/20/2010 9:49	Analyst:	MAR1
Run Time (min):	24.00	Column:	AS23-001528; GL GCE086;300;9056

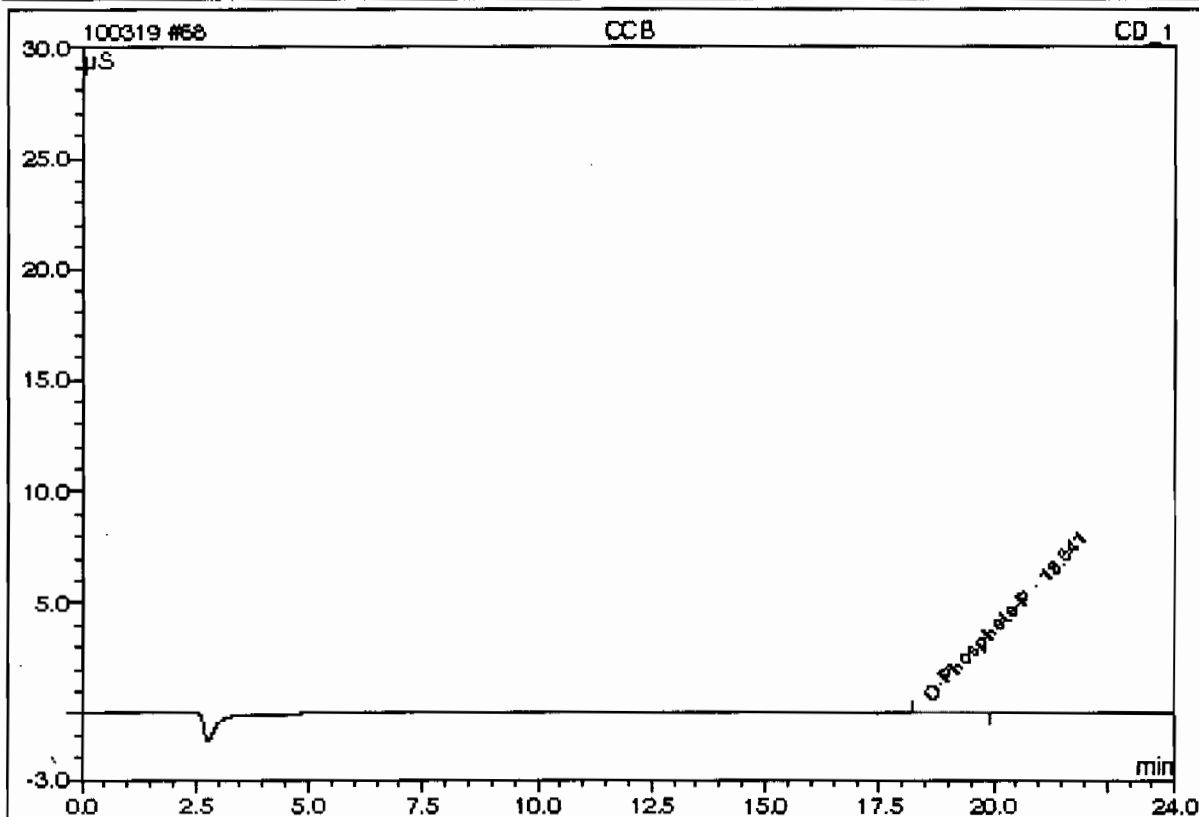

No.	Ret.Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area µS*min	Rel.Area %
n.a.	n.a.	Fluoride	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Chloride	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Nitrite-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Chlorate	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Bromide	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Nitrate-N	n.a.	n.a.	n.a.	n.a.	n.a.
1	18.54	O-Phosphate-P	n.a.	0.1971		0.04281	100.00
n.a.	n.a.	Sulfate	n.a.	n.a.	n.a.	n.a.	n.a.
Total:				0.1971	0.000	0.043	100.00

69 1202063606/962078/1/1/MB


Sample Name:	1202063606/962078/1/1/MB	Injection Volume:	1.0
Vial Number:	6	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100311an	Sample Amount:	1.0000
Recording Time:	3/20/2010 10:16	Analyst:	MAR1
Run Time (min):	24.00	Column:	AS23-001528; GL GC E086;300;9056

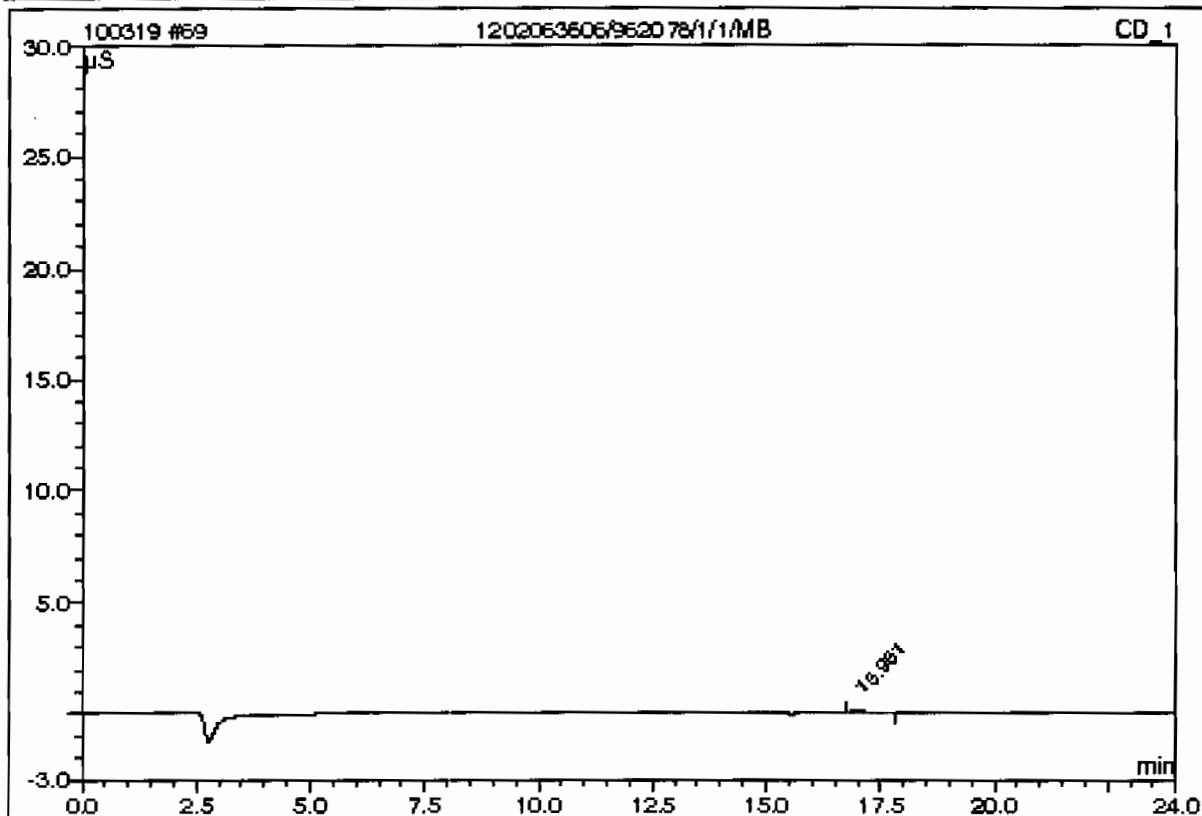

No.	Ret. Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area µS*min	Rel. Area %
n.a.	n.a.	Fluoride	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Chloride	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Nitrite-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Chlorate	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Bromide	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Nitrate-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	O-Phosphate-P	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Sulfate	n.a.	n.a.	n.a.	n.a.	n.a.
Total:				0.0000	0.000	0.000	0.00

70 1202063613/962078/1/1/LCS


Sample Name:	1202063613/962078/1/1/LCS	Injection Volume:	1.0
Vial Number:	7	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100311an	Sample Amount:	1.0000
Recording Time:	3/20/2010 10:43	Analyst:	MAR1
Run Time (min):	24.00	Column:	AS23-001528; GLGCED86;300;9056

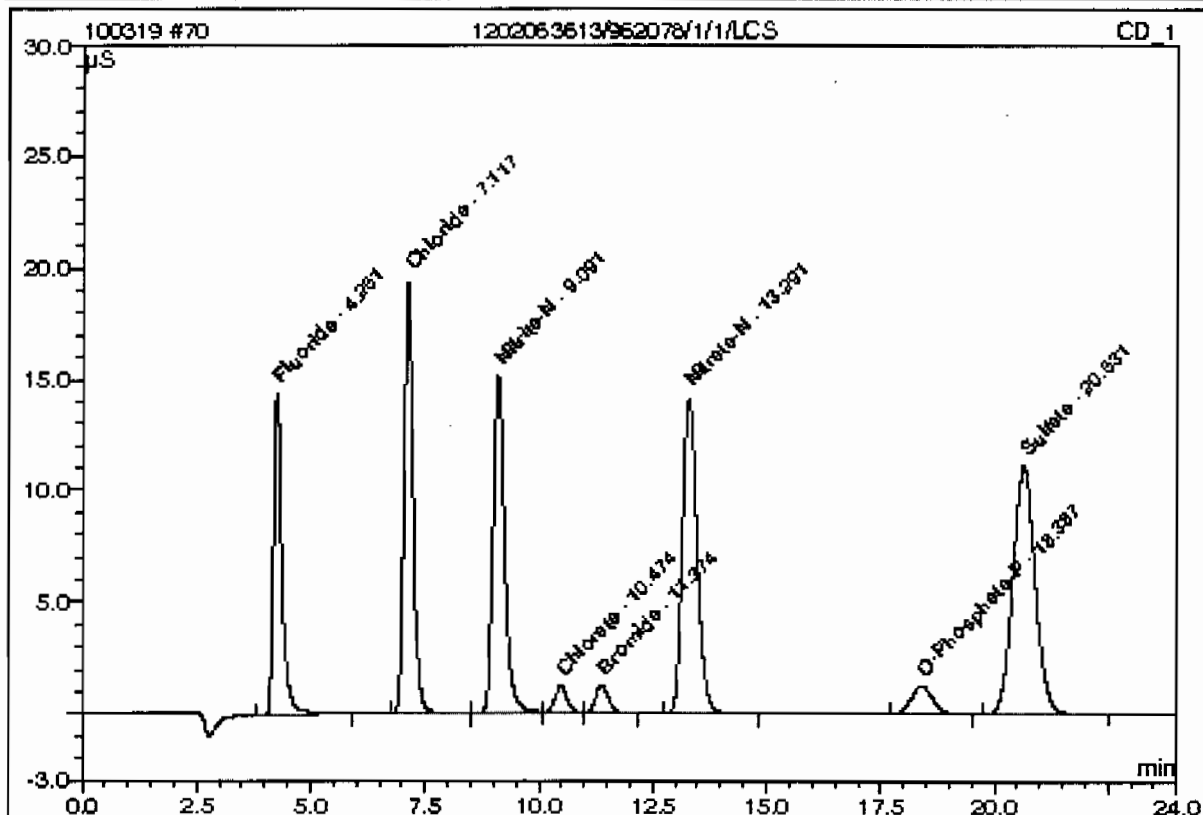

No.	Ret.Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area μS*min	Rel.Area %
1	4.25	Fluoride	n.a.	4.8365		3.07043	12.17
2	7.12	Chloride	n.a.	9.2872		4.46043	17.68
3	9.09	Nitrite-N	n.a.	4.8533		4.50947	17.87
4	10.47	Chlorate	n.a.	2.5722		0.40200	1.59
5	11.37	Bromide	n.a.	2.5390		0.42617	1.69
6	13.29	Nitrate-N	n.a.	4.6930		5.31756	21.08
7	18.39	O-Phosphate-P	n.a.	2.2134		0.70692	2.80
8	20.63	Sulfate	n.a.	18.9569		6.33821	25.12
Total:				49.9516	0.000	25.231	100.00

71 248110001/962078/1/1/


Sample Name:	248110001/962078/1/1/	Injection Volume:	1.0
Vial Number:	8	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100311an	Sample Amount:	1.0000
Recording Time:	3/20/2010 11:10	Analyst:	MAR1
Run Time (min):	24.00	Column:	AS23-001528; GL GC E086;300;9056

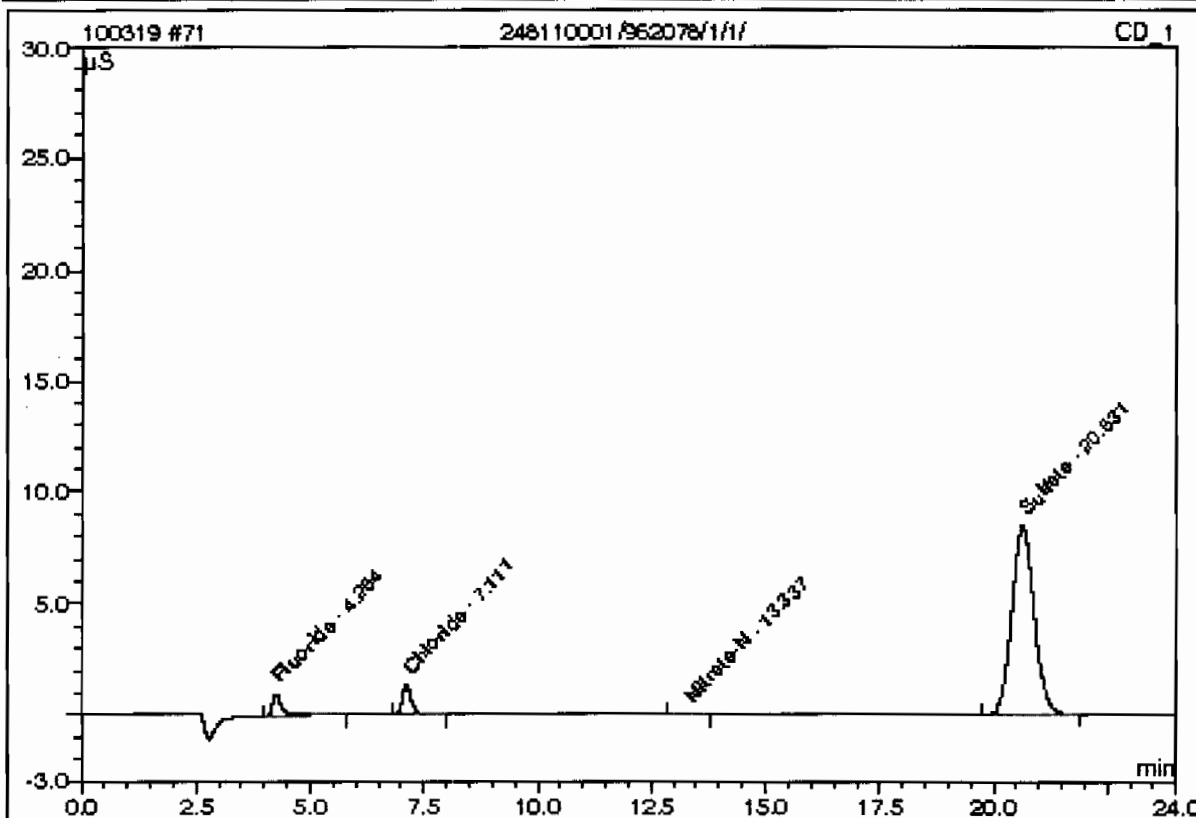

No.	Ret. Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area µS*min	Rel. Area %
1	4.25	Fluoride	n.a.	0.4335		0.24086	4.42
2	7.11	Chloride	n.a.	0.8072		0.31618	5.81
n.a.	n.a.	Nitrite-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Chlorate	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Bromide	n.a.	n.a.	n.a.	n.a.	n.a.
3	13.34	Nitrate-N	n.a.	0.1469		0.02874	0.53
n.a.	n.a.	O-Phosphate-P	n.a.	n.a.	n.a.	n.a.	n.a.
4	20.83	Sulfate	n.a.	14.6016		4.85607	89.24
Total:				15.9892	0.000	5.442	100.00

72 1202063607/962078/1/1/DUP


Sample Name:	1202063607/962078/1/1/DUP	Injection Volume:	1.0
Vial Number:	9	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100311an	Sample Amount:	1.0000
Recording Time:	3/20/2010 11:37	Analyst:	MAR1
Run Time (min):	24.00	Column:	AS23-001528; GL GCE086;300;9056

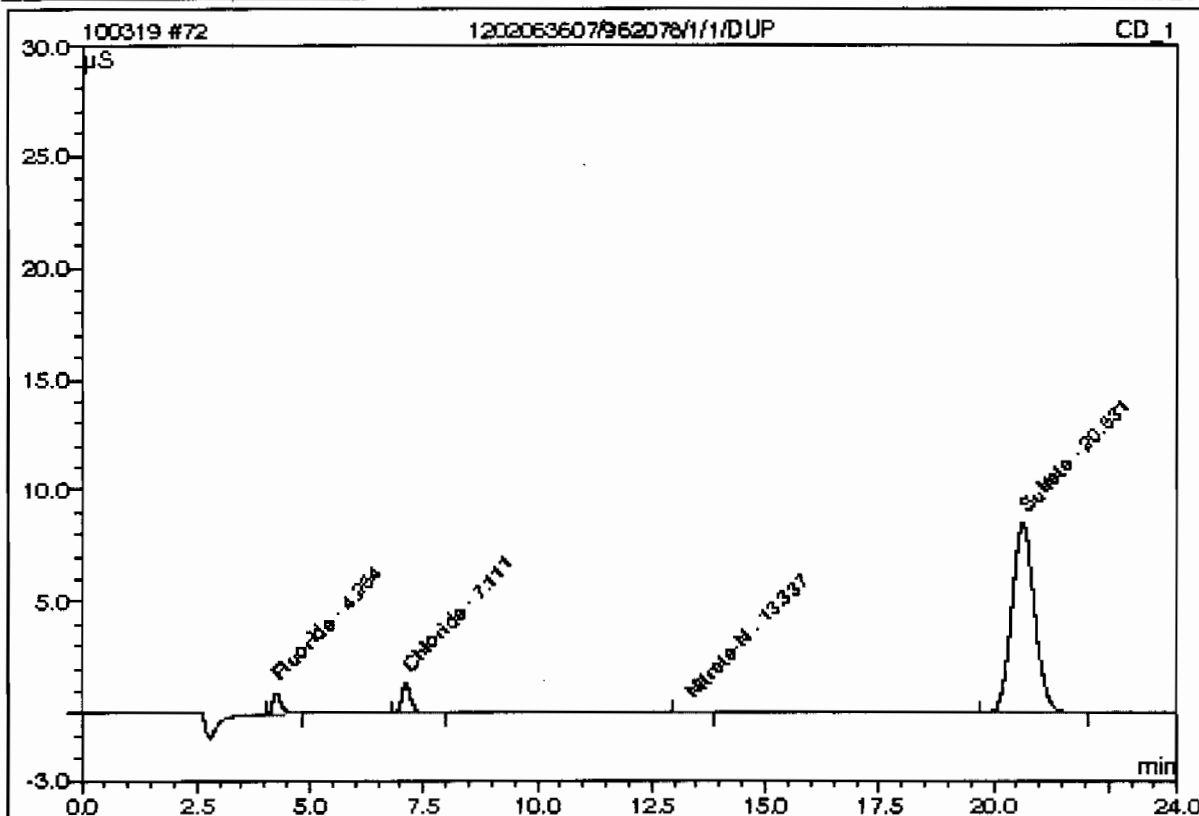

No.	Ret. Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area µS*min	Rel. Area %
1	4.25	Fluoride	n.a.	0.3872		0.21093	3.89
2	7.11	Chloride	n.a.	0.8086		0.31689	5.84
n.a.	n.a.	Nitrite-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Chlorate	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Bromide	n.a.	n.a.	n.a.	n.a.	n.a.
3	13.34	Nitrate-N	n.a.	0.1453		0.02685	0.50
n.a.	n.a.	O-Phosphate-P	n.a.	n.a.	n.a.	n.a.	n.a.
4	20.63	Sulfate	n.a.	14.6387		4.86868	89.77
Total:				15.9798	0.000	5.423	100.00

73 1202063609/962078/1/1/MS


Sample Name:	1202063609/962078/1/1/MS	Injection Volume:	1.0
Vial Number:	10	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100311an	Sample Amount:	1.0000
Recording Time:	3/20/2010 12:04	Analyst:	MAR1
Run Time (min):	24.00	Column:	AS23-001528; GL GCE086;300;0056

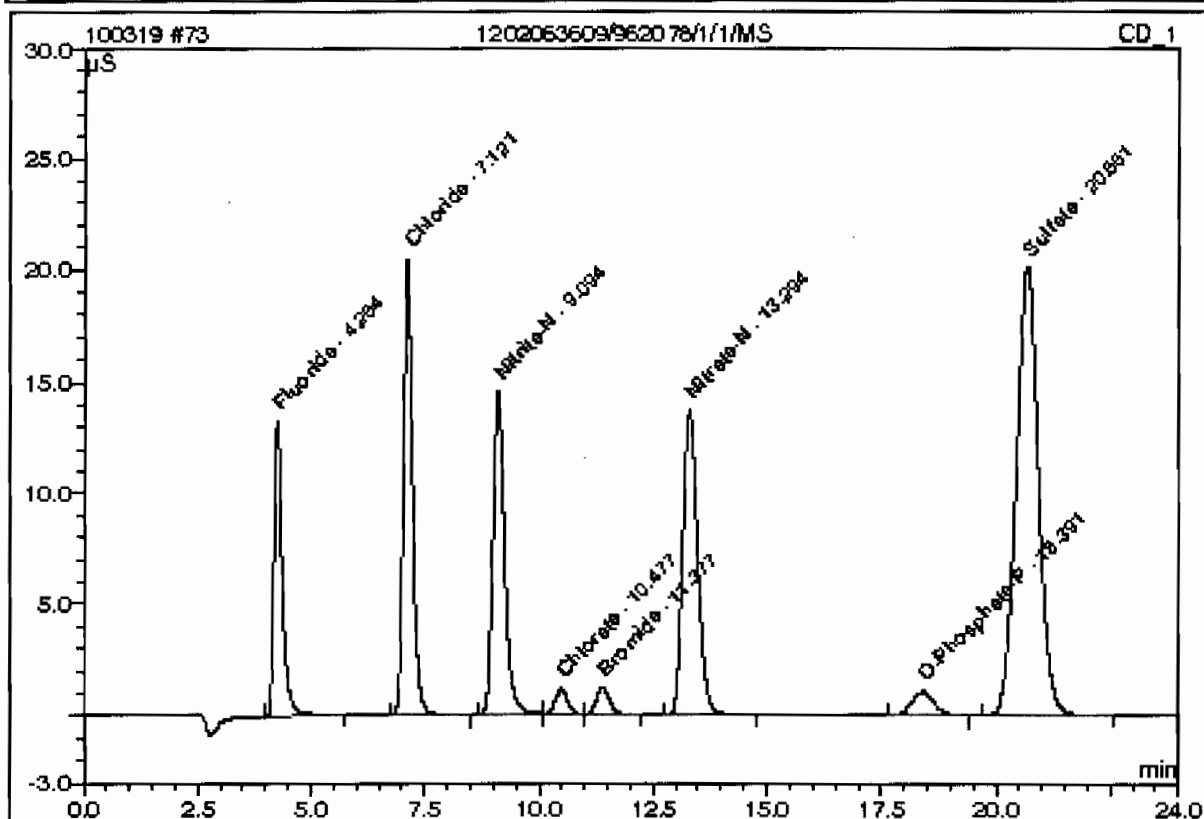

No.	Ret. Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area $\mu\text{S} \cdot \text{min}$	Rel. Area %
1	4.25	Fluoride	n.a.	4.4862		2.84527	9.54
2	7.12	Chloride	n.a.	9.7889		4.70560	15.78
3	9.09	Nitrite-N	n.a.	4.6833		4.34887	14.58
4	10.48	Chlorate	n.a.	2.4844		0.38812	1.30
5	11.38	Bromide	n.a.	2.4647		0.41359	1.39
6	13.29	Nitrate-N	n.a.	4.5734		5.17835	17.36
7	18.39	O-Phosphate-P	n.a.	1.8588		0.59013	1.98
8	20.66	Sulfate	n.a.	33.6981		11.35485	38.07
Total:				64.0379	0.000	29.825	100.00

74 1202063611/962078/1/1/MSD


Sample Name:	1202063611/962078/1/1/MSD	Injection Volume:	1.0
Vial Number:	11	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100311an	Sample Amount:	1.0000
Recording Time:	3/20/2010 12:31	Analyst:	MAR1
Run Time (min):	24.00	Column:	AS23-001528; GL GC E086; 300; 9056

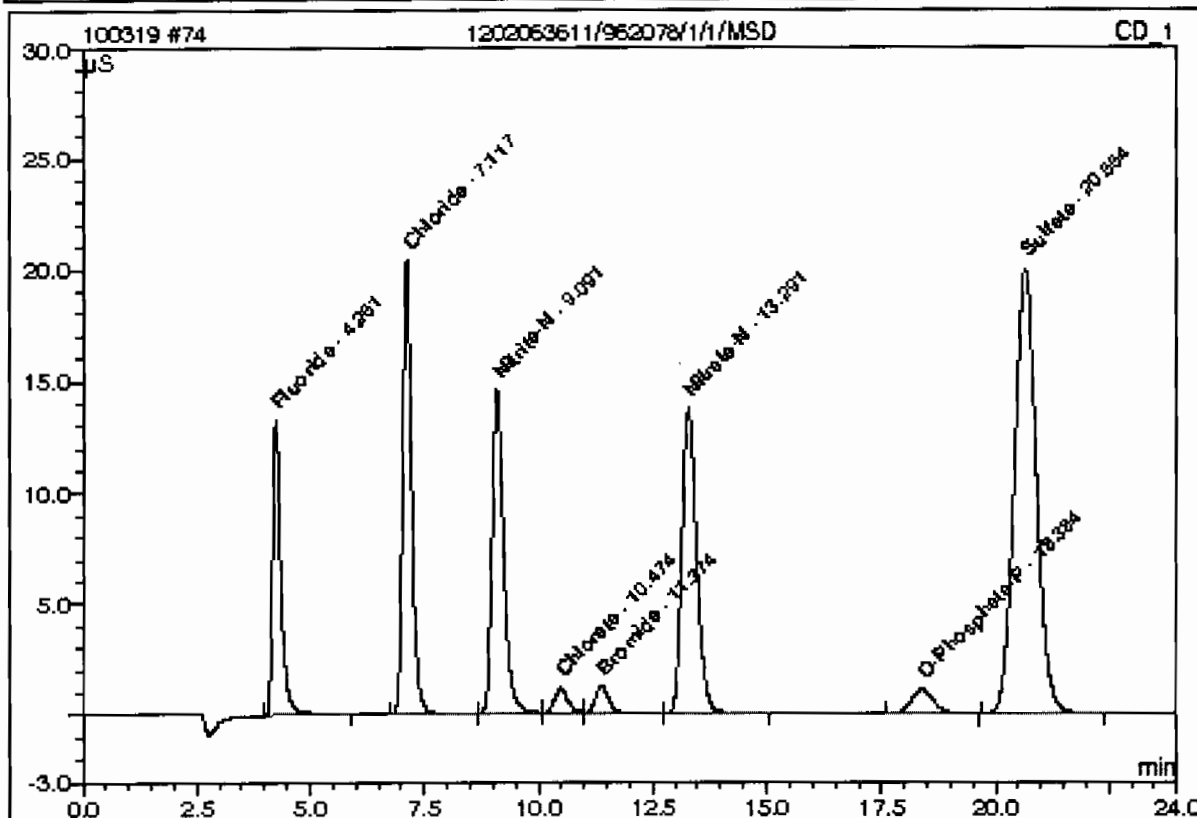

No.	Ret. Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area µS*min	Rel. Area %
1	4.25	Fluoride	n.a.	4.4666		2.83271	9.53
2	7.12	Chloride	n.a.	9.7497		4.68648	15.76
3	9.09	Nitrite-N	n.a.	4.6627		4.32934	14.56
4	10.47	Chlorate	n.a.	2.6137		0.40855	1.37
5	11.37	Bromide	n.a.	2.5883		0.43451	1.46
6	13.29	Nitrate-N	n.a.	4.5603		5.16310	17.36
7	18.38	O-Phosphate-P	n.a.	1.8877		0.59962	2.02
8	20.65	Sulfate	n.a.	33.4826		11.28152	37.94
Total:				64.0117	0.000	29.736	100.00

79 WIC100319-02CCV


Sample Name:	WIC100319-02CCV	Injection Volume:	1.0
Vial Number:	16	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100311an	Sample Amount:	1.0000
Recording Time:	3/20/2010 14:45	Analyst:	MAR1
Run Time (min):	24.00	Column:	AS23-001528; GL GCE086;300;9056

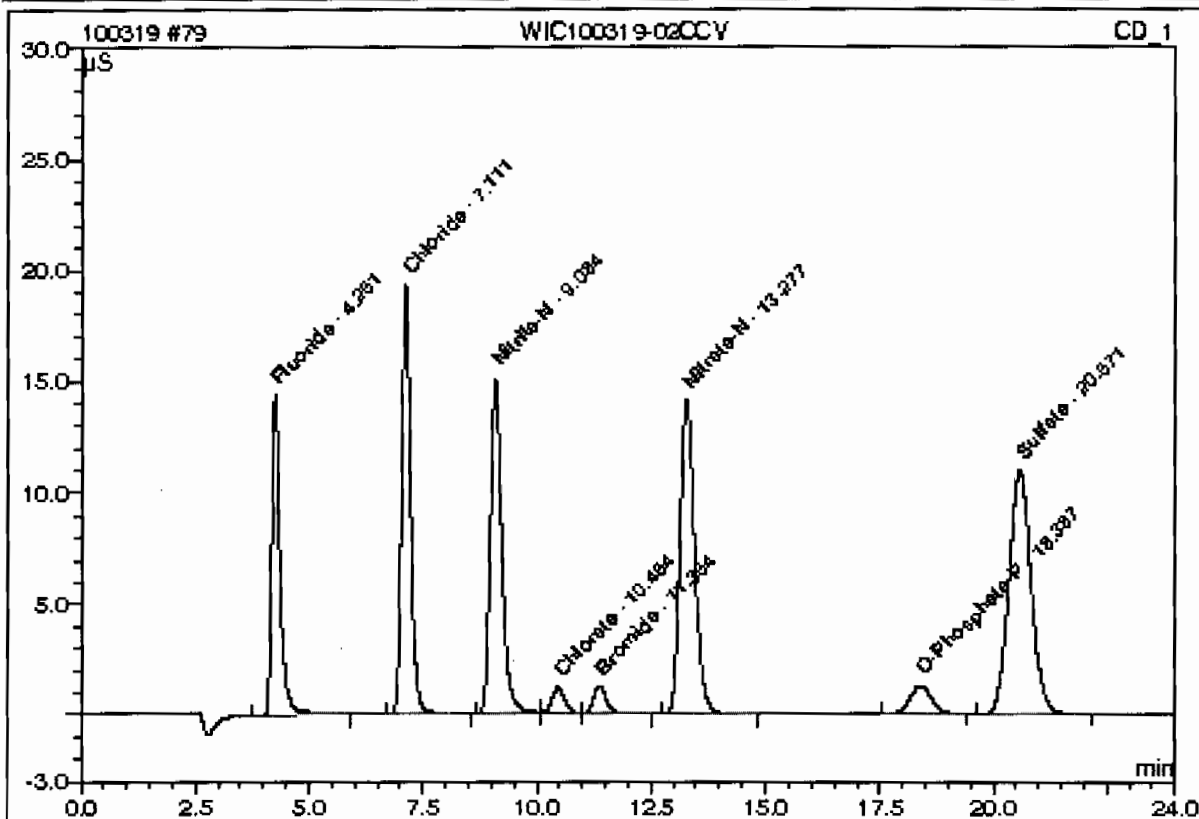

No.	Ret.Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area µS*min	Rel.Area %
1	4.25	Fluoride	n.a.	4.7969		3.04496	12.14
2	7.11	Chloride	n.a.	9.2285		4.43174	17.67
3	9.08	Nitrite-N	n.a.	4.8195		4.47753	17.85
4	10.46	Chlorate	n.a.	2.5794		0.40314	1.61
5	11.36	Bromide	n.a.	2.5729		0.43189	1.72
6	13.28	Nitrate-N	n.a.	4.6740		5.29541	21.11
7	18.39	O-Phosphate-P	n.a.	2.2344		0.71382	2.85
8	20.57	Sulfate	n.a.	18.7945		6.28296	25.05
Total:				49.7000	0.000	25.081	100.00

80 CCB

Sample Name:	CCB	Injection Volume:	1.0
Vial Number:	17	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100311an	Sample Amount:	1.0000
Recording Time:	3/20/2010 15:12	Analyst:	MAR1
Run Time (min):	24.00	Column:	AS23-001528; GL GC E086;300;9056

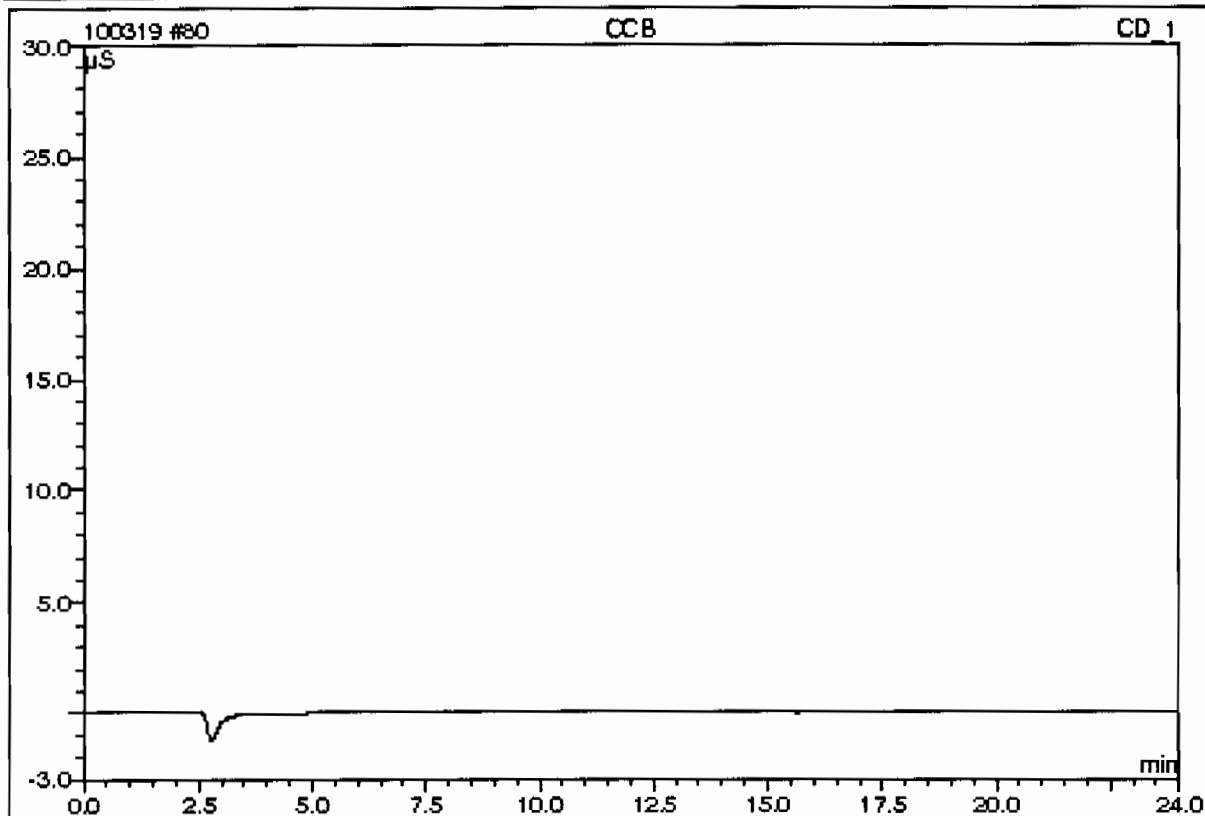


No.	Ret. Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area µS*min	Rel. Area %
n.a.	n.a.	Fluoride	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Chloride	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Nitrite-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Chlorate	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Bromide	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Nitrate-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	O-Phosphate-P	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Sulfate	n.a.	n.a.	n.a.	n.a.	n.a.
Total:				0.0000	0.000	0.000	0.00

This is runlog for Sequence 100321.seq for IC6

Sample ID	Run Time	Batch	Dilution	Dataset	Analyst
BLK	03/21/10 11:06		1	100321	MAR1
ICV	03/21/10 11:32		1	100321	MAR1
ICB	03/21/10 12:53		1	100321	MAR1
248110006	03/21/10 13:19	962078	1	100321	MAR1
248110007	03/21/10 13:46	962078	1	100321	MAR1
248110008	03/21/10 14:13	962078	1	100321	MAR1
248118001	03/21/10 14:40	962078	1	100321	MAR1
248118002	03/21/10 15:07	962078	1	100321	MAR1
248118003	03/21/10 15:34	962078	1	100321	MAR1
248118004	03/21/10 16:01	962078	1	100321	MAR1
248118005	03/21/10 16:27	962078	1	100321	MAR1
CVH	03/21/10 16:54		1	100321	MAR1
CCB	03/21/10 17:21		1	100321	MAR1
248118006	03/21/10 17:48	962078	1	100321	MAR1
248118007	03/21/10 18:15	962078	1	100321	MAR1
1202063608	03/21/10 18:42	962078	1	100321	MAR1
1202063610	03/21/10 19:09	962078	1	100321	MAR1
1202063612	03/21/10 19:36	962078	1	100321	MAR1
CCV	03/21/10 20:03		1	100321	MAR1
CCB	03/21/10 20:30		1	100321	MAR1
1202073527	03/21/10 20:57	966227	1	100321	MAR1
1202073534	03/21/10 21:23	966227	1	100321	MAR1
248386003	03/21/10 21:50	966227	1	100321	MAR1
248386004	03/21/10 22:17	966227	1	100321	MAR1
1202073529	03/21/10 22:44	966227	1	100321	MAR1
1202073531	03/21/10 23:11	966227	1	100321	MAR1
1202073533	03/21/10 23:38	966227	1	100321	MAR1

15 WIC100321-02ICV


Sample Name:	WIC100321-02ICV	Injection Volume:	1.0
Vial Number:	2	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100311an	Sample Amount:	1.0000
Recording Time:	3/21/2010 11:32	Analyst:	MAR1
Run Time (min):	24.00	Column:	AS23-001528; GL GCE086;300;9056

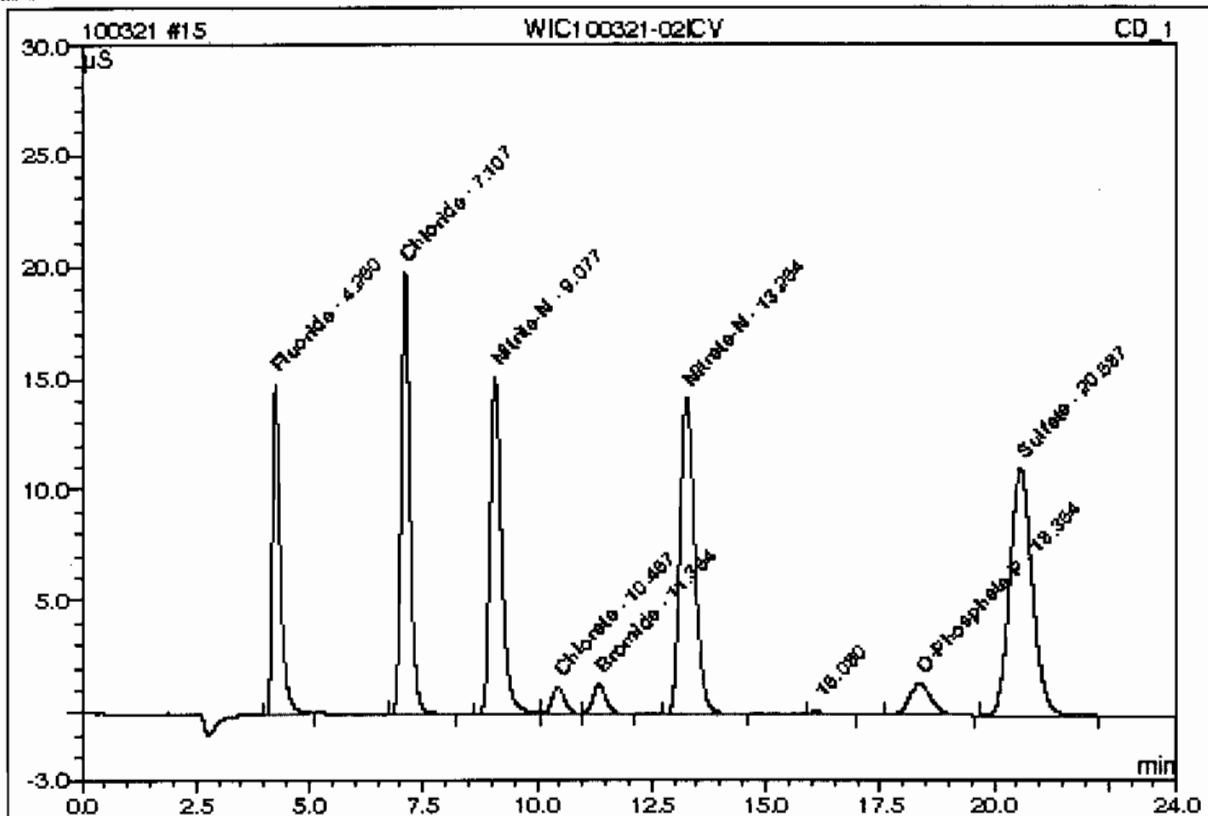

No.	Ret.Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area µS*min	Rel.Area %
1	4.25	Fluoride	n.a.	4.7492		3.01433	12.02
2	7.11	Chloride	n.a.	9.2029		4.41923	17.62
3	9.08	Nitrite-N	n.a.	4.7889		4.44859	17.74
4	10.46	Chlorate	n.a.	2.5430		0.39737	1.58
5	11.35	Bromide	n.a.	2.5104		0.42132	1.68
6	13.26	Nitrate-N	n.a.	4.6626		5.28214	21.06
8	18.36	O-Phosphate-P	n.a.	2.4391		0.78126	3.11
9	20.59	Sulfate	n.a.	18.7738		6.27592	25.02
Total:				49.6699	0.000	25.040	99.83

16 ICB


Sample Name:	ICB	Injection Volume:	1.0
Vial Number:	3	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight	1.0000
Quantif. Method:	100311an	Sample Amount:	1.0000
Recording Time:	3/21/2010 12:53	Analyst:	MAR1
Run Time (min):	24.00	Column:	AS23-001528; GL GCE086;300;9056

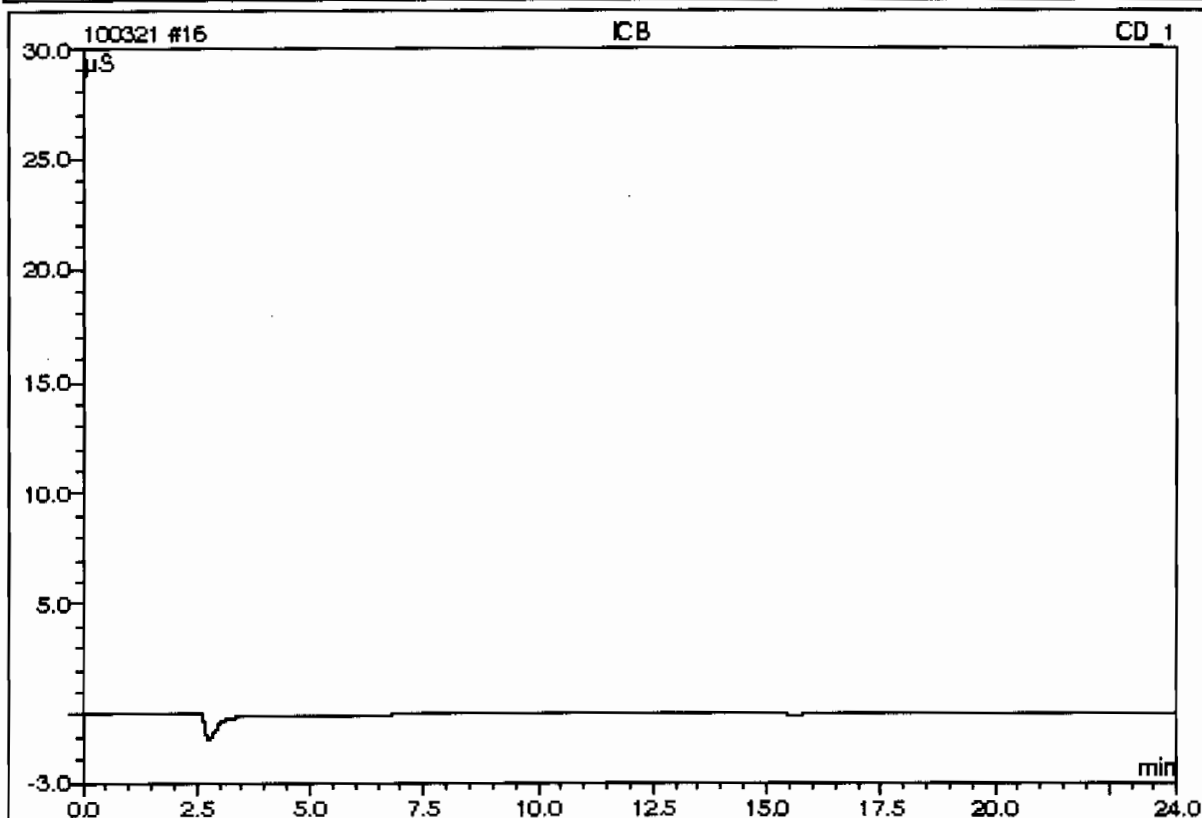

No.	Ret. Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area μS*min	Rel. Area %
n.a.	n.a.	Fluoride	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Chloride	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Nitrite-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Chlorate	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Bromide	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Nitrate-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	O-Phosphate-P	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Sulfate	n.a.	n.a.	n.a.	n.a.	n.a.
Total:				0.0000	0.000	0.000	0.00

20 248118001/962078/1/1/


Sample Name:	248118001/962078/1/1/	Injection Volume:	1.0
Vial Number:	7	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100311an	Sample Amount:	1.0000
Recording Time:	3/21/2010 14:40	Analyst:	MAR1
Run Time (min):	24.00	Column:	AS23-001528; GL GCE086;300;9056

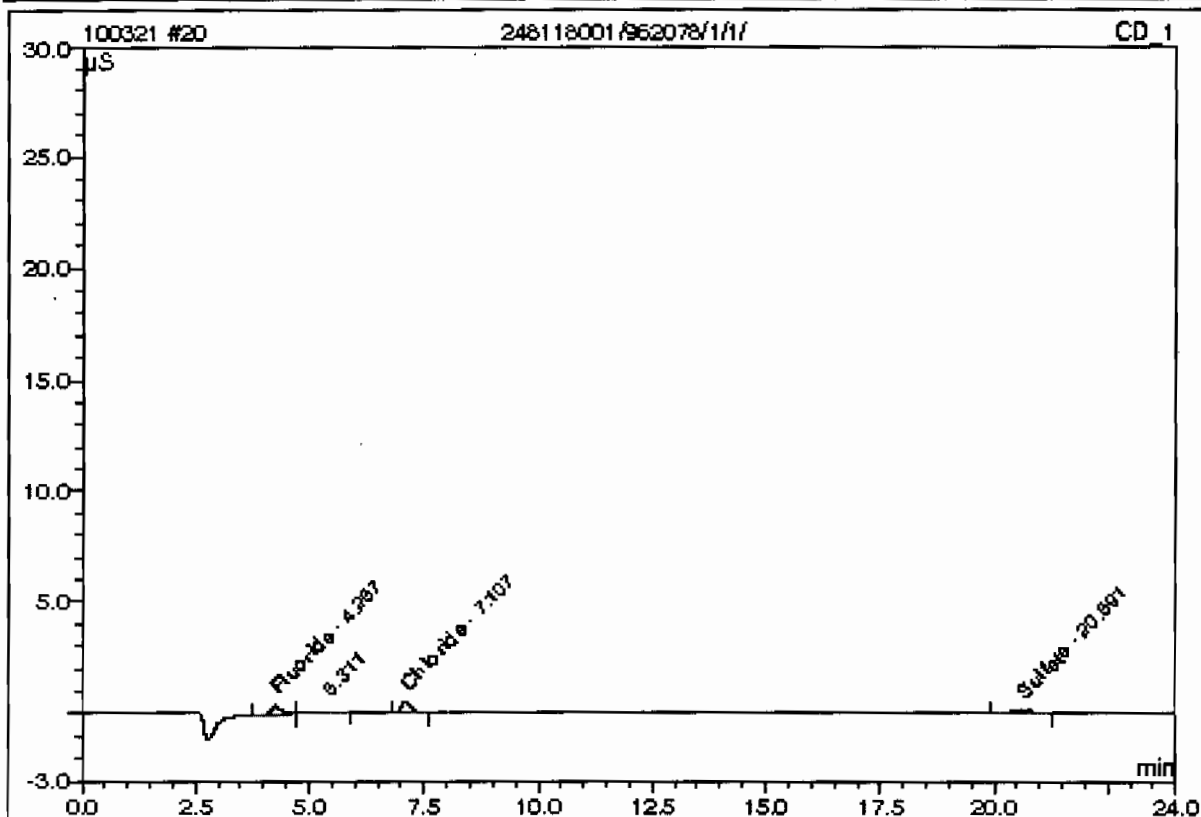

No.	Ret. Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area µS*min	Rel. Area %
1	4.26	Fluoride	n.a.	0.1948		0.08724	26.77
3	7.11	Chloride	n.a.	0.4168		0.12542	38.49
n.a.	n.a.	Nitrite-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Chlorate	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Bromide	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Nitrate-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	O-Phosphate-P	n.a.	n.a.	n.a.	n.a.	n.a.
4	20.59	Sulfate	n.a.	0.5467		0.07300	22.40
Total:				1.1583	0.000	0.286	87.66

21 248118002/962078/1/1/


Sample Name:	248118002/962078/1/1/	Injection Volume:	1.0
Vial Number:	8	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100311an	Sample Amount:	1.0000
Recording Time:	3/21/2010 15:07	Analyst:	MAR1
Run Time (min):	24.00	Column:	AS23-001528; GL GCE086;300;9056

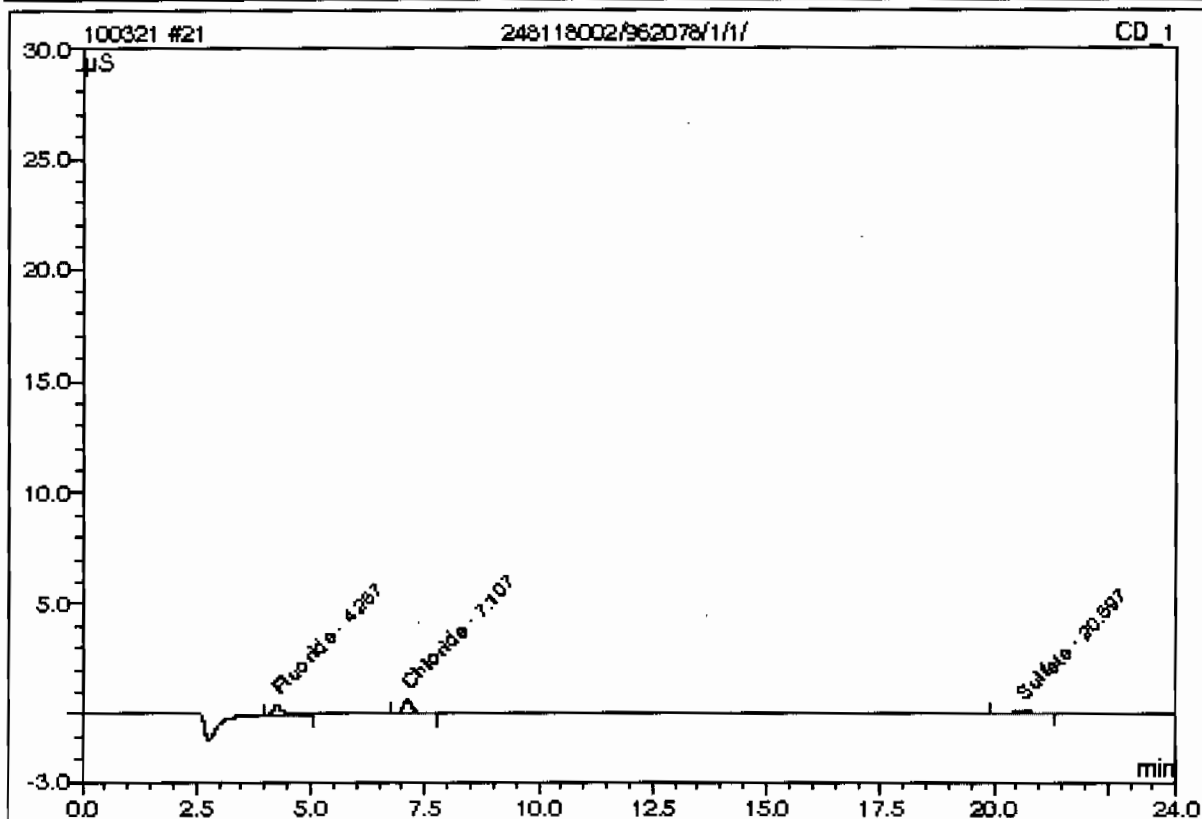

No.	Ret.Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area µS*min	Rel.Area %
1	4.26	Fluoride	n.a.	0.2097		0.09685	31.32
2	7.11	Chloride	n.a.	0.4475		0.14042	45.40
n.a.	n.a.	Nitrite-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Chlorate	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Bromide	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Nitrate-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	O-Phosphate-P	n.a.	n.a.	n.a.	n.a.	n.a.
3	20.60	Sulfate	n.a.	0.5437		0.07199	23.28
Total:				1.2010	0.000	0.309	100.00

22 248118003/962078/1/1/


Sample Name:	248118003/962078/1/1/	Injection Volume:	1.0
Vial Number:	9	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100311an	Sample Amount:	1.0000
Recording Time:	3/21/2010 15:34	Analyst:	MAR1
Run Time (min):	24.00	Column:	AS23-001528; GL GCE086;300;9056

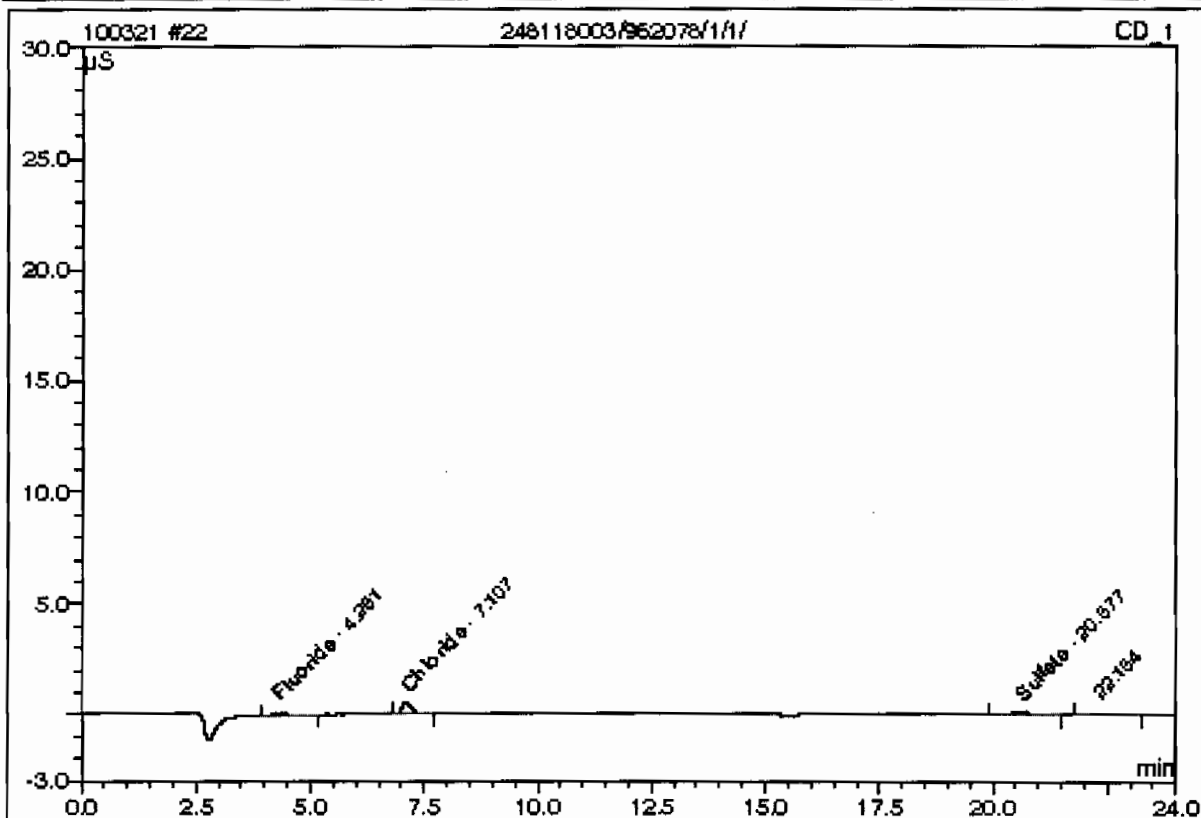

No.	Ret. Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area µS*min	Rel. Area %
1	4.26	Fluoride	n.a.	0.1188		0.03840	13.34
2	7.11	Chloride	n.a.	0.4359		0.13471	46.81
n.a.	n.a.	Nitrite-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Chlorate	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Bromide	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Nitrate-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	O-Phosphate-P	n.a.	n.a.	n.a.	n.a.	n.a.
3	20.58	Sulfate	n.a.	0.5906		0.08795	30.58
Total:				1.1452	0.000	0.261	90.70

23 248118004/962078/1/1/


Sample Name:	248118004/962078/1/1/	Injection Volume:	1.0
Vial Number:	10	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100311an	Sample Amount:	1.0000
Recording Time:	3/21/2010 16:01	Analyst:	MAR1
Run Time (min):	24.00	Column:	AS23-001528; GLGCED86;300;9056

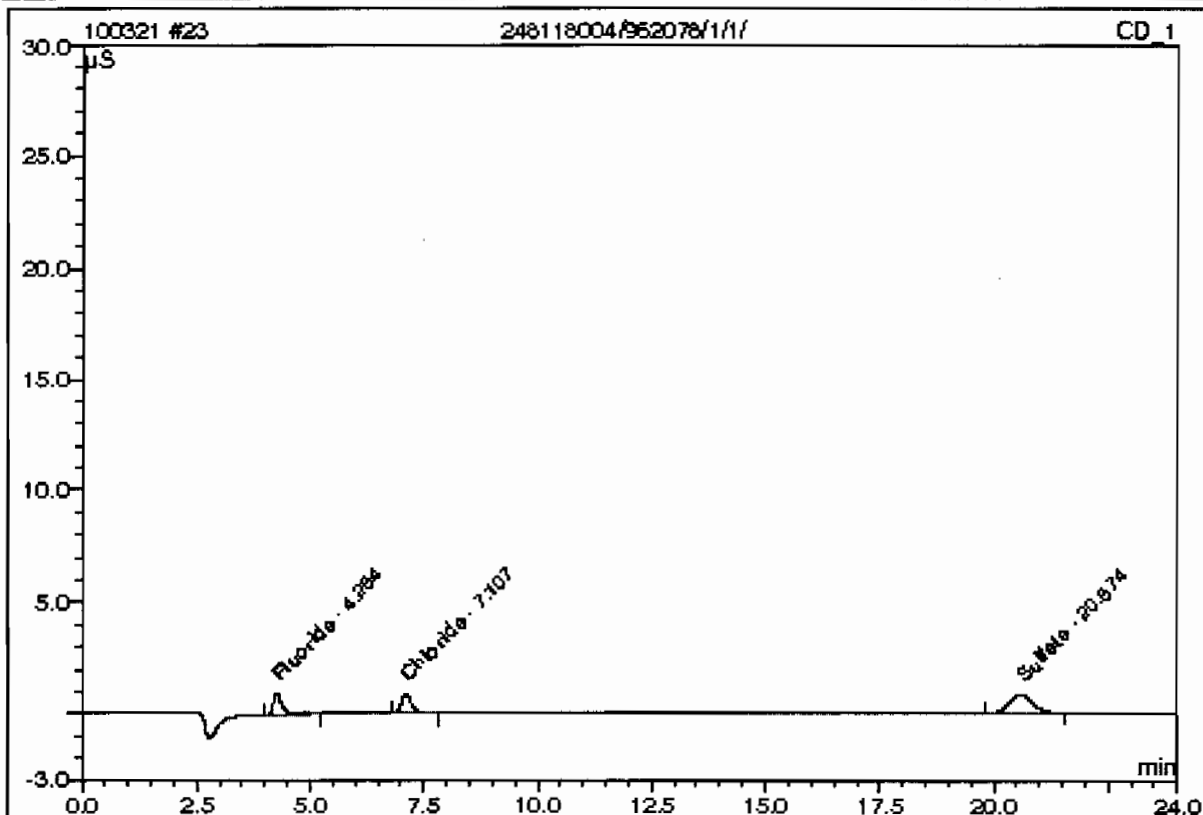

No.	Ret. Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area µS*min	Rel. Area %
1	4.25	Fluoride	n.a.	0.4044		0.22195	23.04
2	7.11	Chloride	n.a.	0.6191		0.22429	23.28
n.a.	n.a.	Nitrite-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Chlorate	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Bromide	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Nitrate-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	O-Phosphate-P	n.a.	n.a.	n.a.	n.a.	n.a.
3	20.57	Sulfate	n.a.	1.8517		0.51711	53.68
Total:				2.8752	0.000	0.963	100.00

24 248118005/962078/1/1/


Sample Name:	248118005/962078/1/1/	Injection Volume:	1.0
Vial Number:	11	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight	1.0000
Quantif. Method:	100311an	Sample Amount:	1.0000
Recording Time:	3/21/2010 16:27	Analyst:	MAR1
Run Time (min):	24.00	Column:	AS23-001528; GL GCE086;300;9056

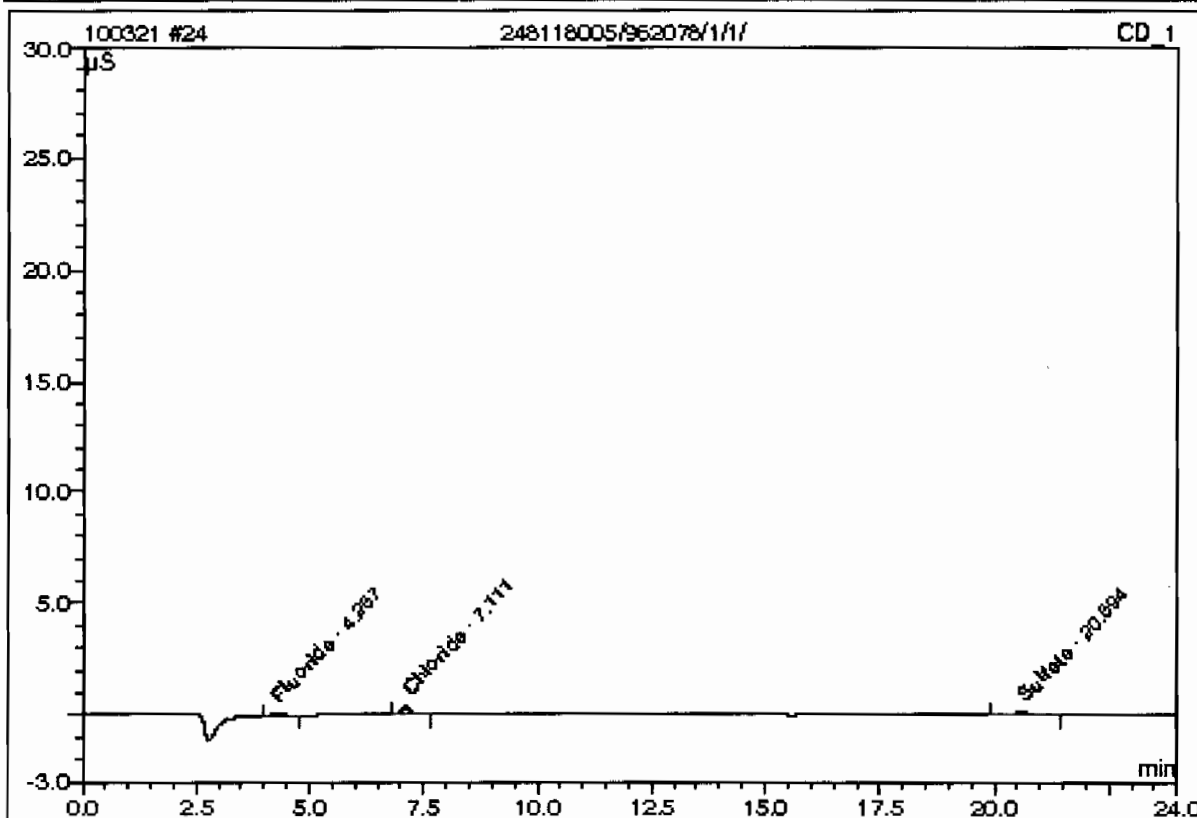

No.	Ret. Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area µS*min	Rel. Area %
1	4.26	Fluoride	n.a.	0.1004		0.02655	14.53
2	7.11	Chloride	n.a.	0.3474		0.09149	50.06
n.a.	n.a.	Nitrite-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Chlorate	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Bromide	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Nitrate-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	O-Phosphate-P	n.a.	n.a.	n.a.	n.a.	n.a.
3	20.59	Sulfate	n.a.	0.5224		0.06473	35.42
Total:				0.9701	0.000	0.183	100.00

25 WIC100321-02CVH


Sample Name:	WIC100321-02CVH	Injection Volume:	1.0
Vial Number:	12	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100311an	Sample Amount:	1.0000
Recording Time:	3/21/2010 16:54	Analyst:	MAR1
Run Time (min):	24.00	Column:	AS23-001528; GL GC E086;300;0056

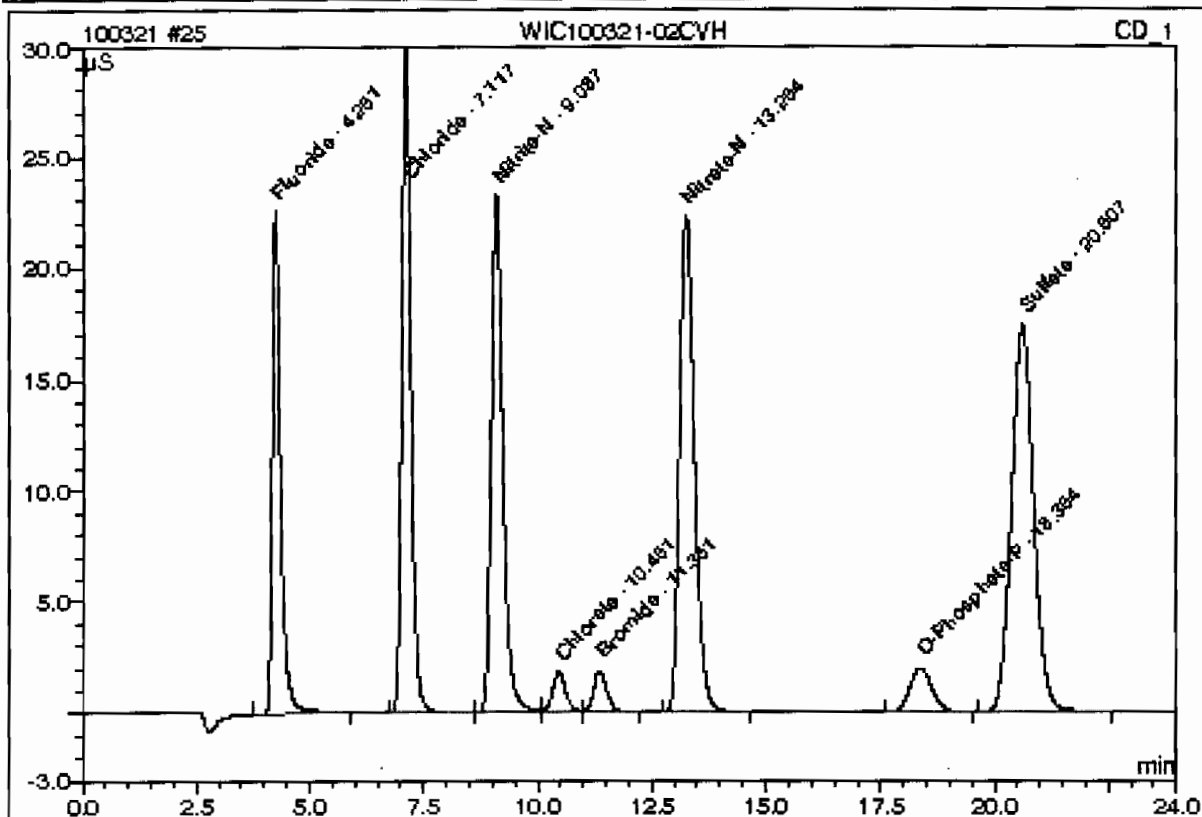

No.	Ret. Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area μS*min	Rel. Area %
1	4.25	Fluoride	n.a.	7.3711		4.69937	12.06
2	7.12	Chloride	n.a.	14.4763		6.99638	17.96
3	9.09	Nitrite-N	n.a.	7.3083		6.82919	17.53
4	10.46	Chlorate	n.a.	3.8025		0.59645	1.53
5	11.36	Bromide	n.a.	3.6702		0.61755	1.59
6	13.25	Nitrate-N	n.a.	7.2640		8.30849	21.33
7	18.36	O-Phosphate-P	n.a.	3.4291		1.10731	2.84
8	20.61	Sulfate	n.a.	29.1400		9.80365	25.16
Total:				76.4615	0.000	38.958	100.00

26 CCB


Sample Name:	CCB	Injection Volume:	1.0
Vial Number:	13	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100311an	Sample Amount:	1.0000
Recording Time:	3/21/2010 17:21	Analyst:	MAR1
Run Time (min):	24.00	Column:	AS23-001528; GL GC E086;300;9056

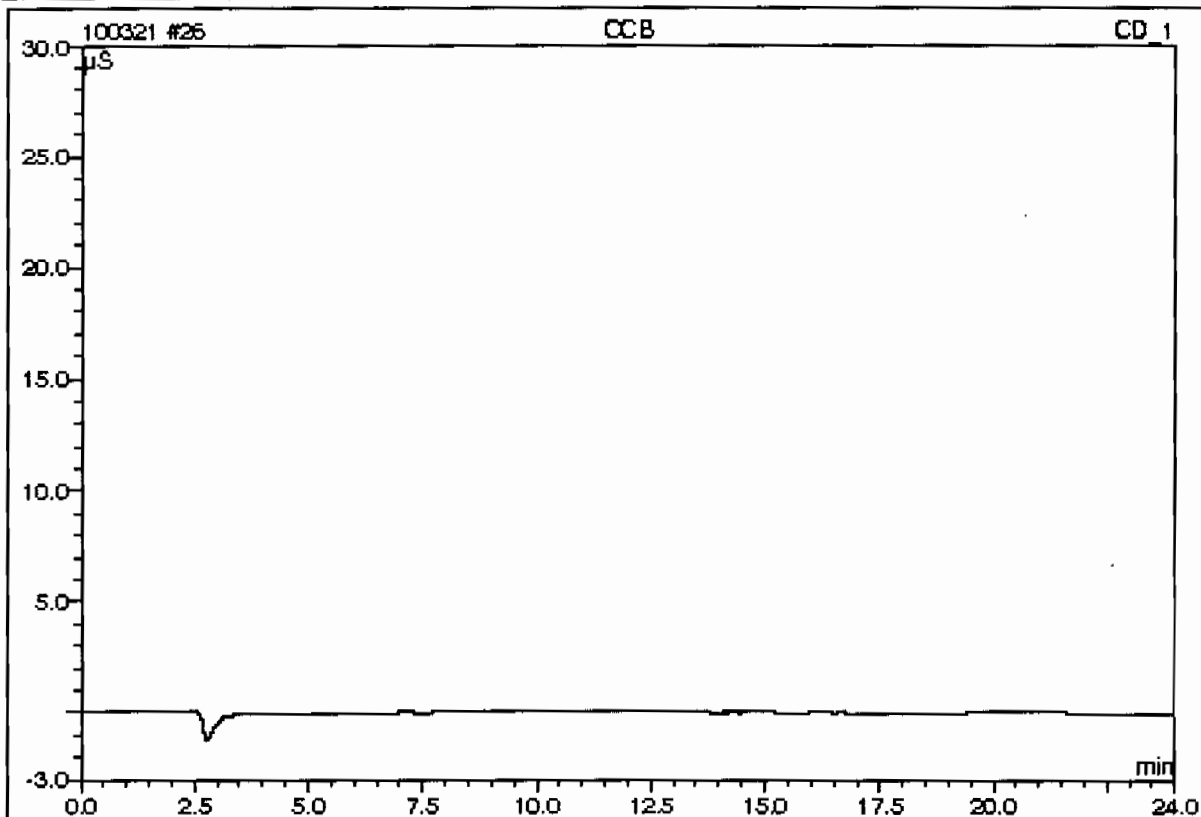

No.	Ret. Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area µS*min	Rel. Area %
n.a.	n.a.	Fluoride	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Chloride	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Nitrite-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Chlorate	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Bromide	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Nitrate-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	O-Phosphate-P	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Sulfate	n.a.	n.a.	n.a.	n.a.	n.a.
Total:				0.0000	0.000	0.000	0.00

27 248118006/962078/1/1/


Sample Name:	248118006/962078/1/1/	Injection Volume:	1.0
Vial Number:	14	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100311an	Sample Amount:	1.0000
Recording Time:	3/21/2010 17:48	Analyst:	MAR1
Run Time (min):	24.00	Column:	AS23-001528; GL GCE086;300;9056

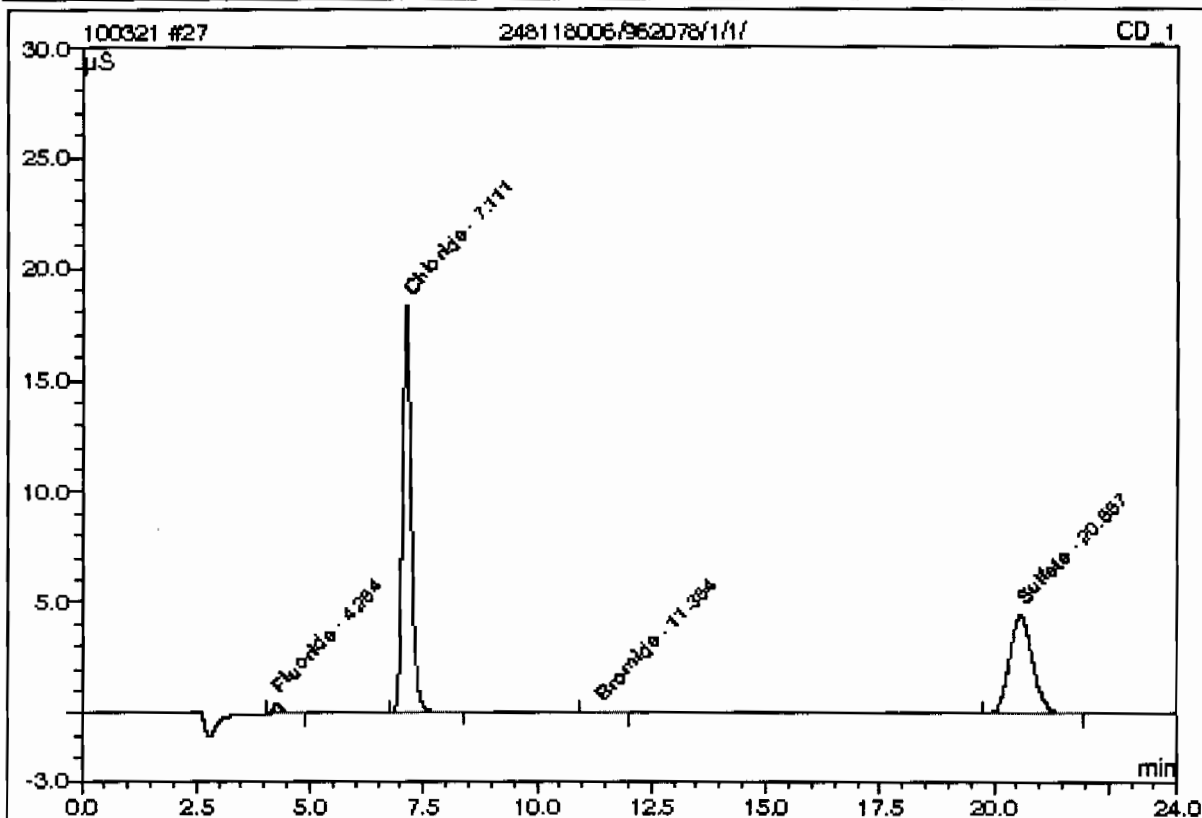

No.	Ret.Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area µS*min	Rel.Area %
1	4.25	Fluoride	n.a.	0.2045		0.09351	1.38
2	7.11	Chloride	n.a.	8.5608		4.10544	60.50
n.a.	n.a.	Nitrite-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Chlorate	n.a.	n.a.	n.a.	n.a.	n.a.
3	11.36	Bromide	n.a.	0.1125		0.01563	0.23
n.a.	n.a.	Nitrate-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	O-Phosphate-P	n.a.	n.a.	n.a.	n.a.	n.a.
4	20.57	Sulfate	n.a.	7.8868		2.57094	37.89
Total:				16.7646	0.000	6.786	100.00

28 248118007/962078/1/1/


Sample Name:	248118007/962078/1/1/	Injection Volume:	1.0
Vial Number:	15	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100311an	Sample Amount:	1.0000
Recording Time:	3/21/2010 18:15	Analyst:	MAR1
Run Time (min):	24.00	Column:	AS23-001528; GL GC E086;300;9056

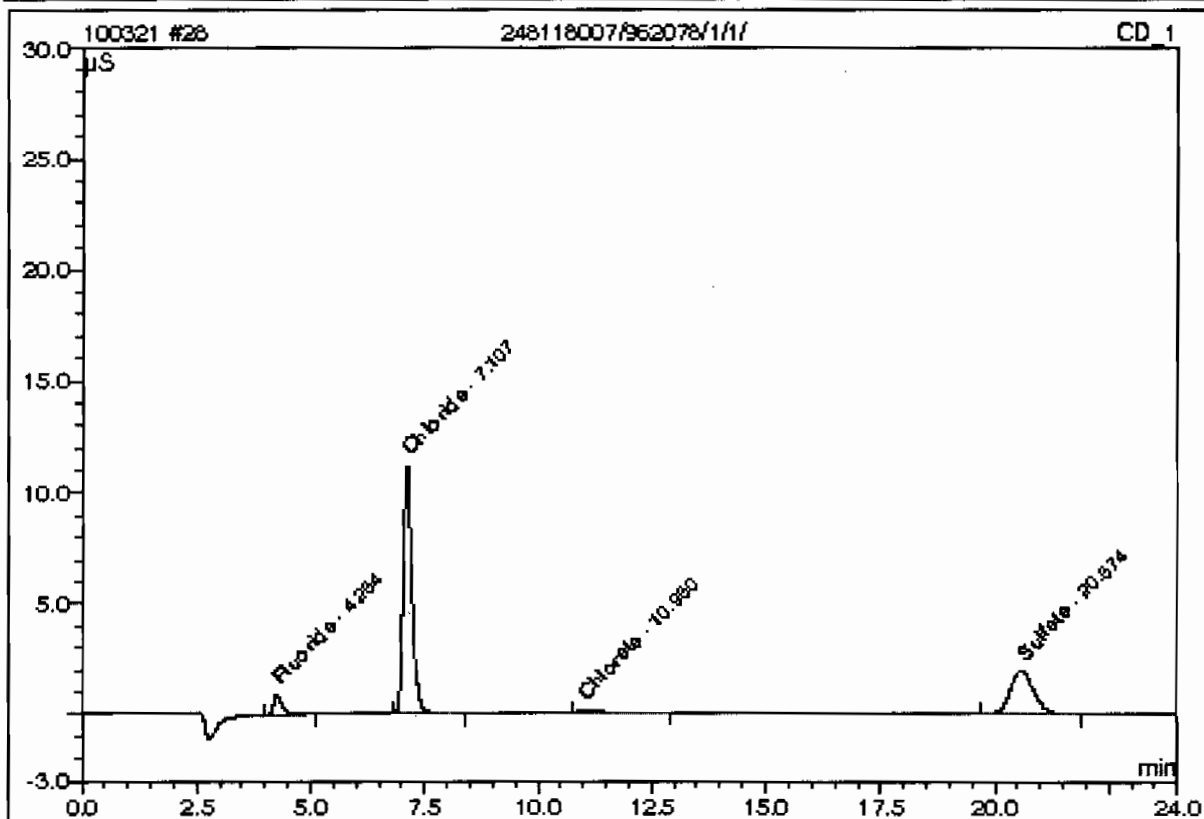

No.	Ret. Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area $\mu S \cdot min$	Rel. Area %
1	4.25	Fluoride	n.a.	0.3767		0.20414	5.08
2	7.11	Chloride	n.a.	5.3730		2.54754	63.35
n.a.	n.a.	Nitrite-N	n.a.	n.a.	n.a.	n.a.	n.a.
3	10.96	Chlorate	n.a.	0.7110		0.10783	2.68
n.a.	n.a.	Bromide	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Nitrate-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	O-Phosphate-P	n.a.	n.a.	n.a.	n.a.	n.a.
4	20.57	Sulfate	n.a.	3.7454		1.16158	28.89
Total:				10.2061	0.000	4.021	100.00

29 1202063608/962078/1/1/DUP


Sample Name:	1202063608/962078/1/1/DUP	Injection Volume:	1.0
Vial Number:	16	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100311an	Sample Amount:	1.0000
Recording Time:	3/21/2010 18:42	Analyst:	MAR1
Run Time (min):	24.00	Column:	AS23-001528; GL GC E086;300;9056

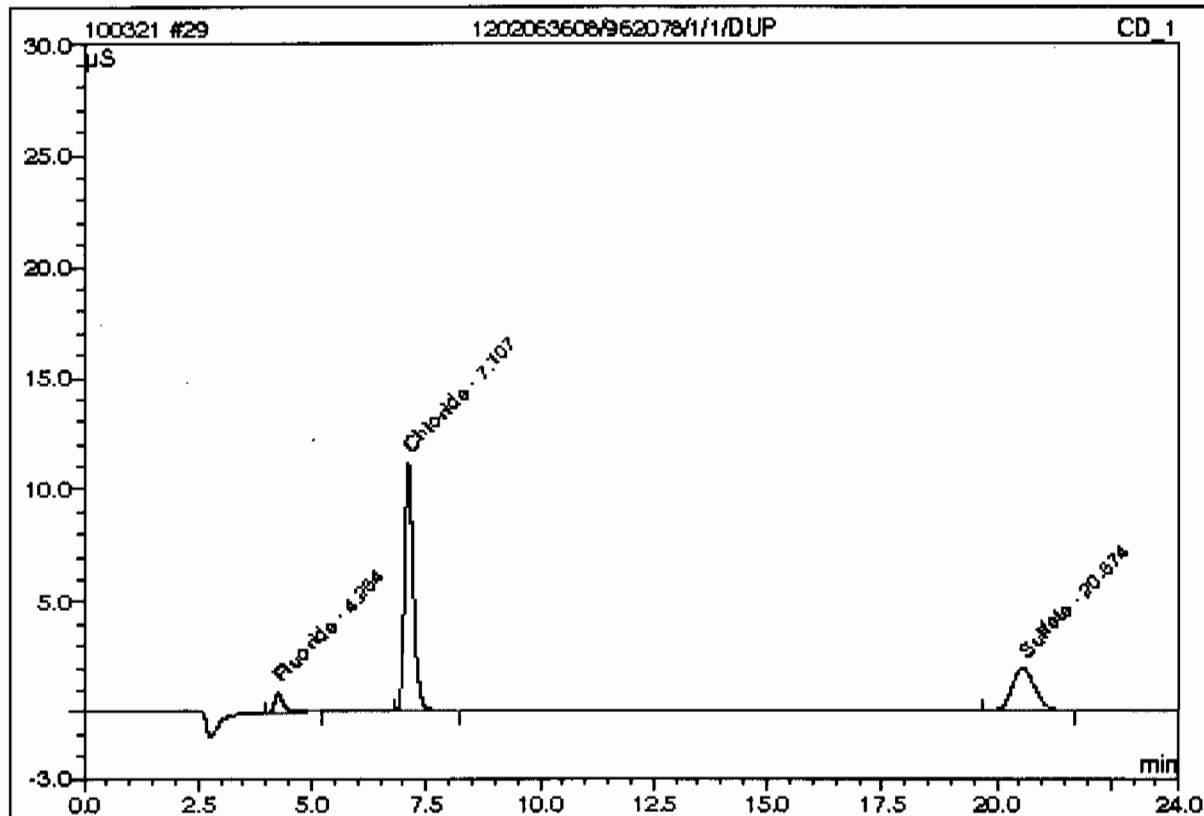

No.	Ret. Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area μS*min	Rel. Area %
1	4.25	Fluoride	n.a.	0.3654		0.19687	5.08
2	7.11	Chloride	n.a.	5.3381		2.53047	65.25
n.a.	n.a.	Nitrite-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Chlorate	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Bromide	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Nitrate-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	O-Phosphate-P	n.a.	n.a.	n.a.	n.a.	n.a.
3	20.57	Sulfate	n.a.	3.7138		1.15080	29.67
Total:				9.4172	0.000	3.878	100.00

30 1202063610/962078/1/1/MS


Sample Name:	1202063610/962078/1/1/MS	Injection Volume:	1.0
Vial Number:	17	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100311an	Sample Amount:	1.0000
Recording Time:	3/21/2010 19:09	Analyst:	MAR1
Run Time (min):	24.00	Column:	AS23-001528; GLGCED86;300;9056

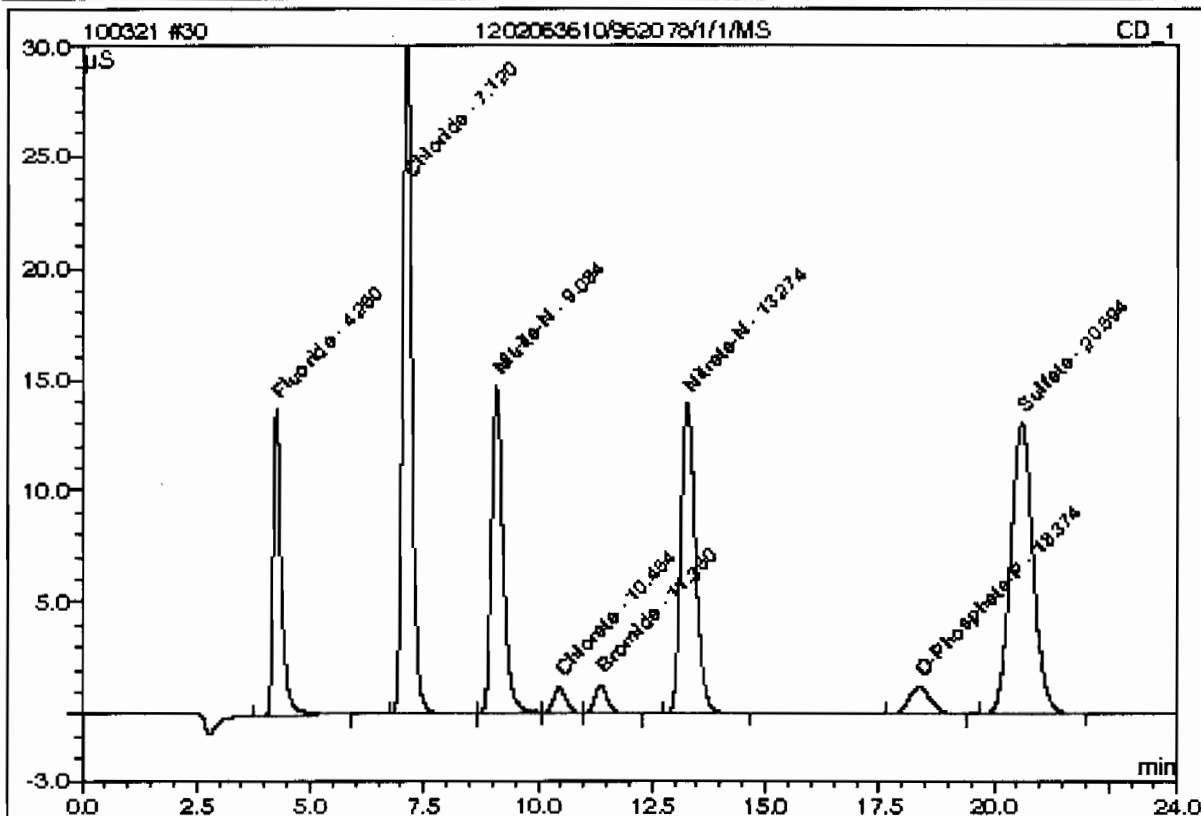

No.	Ret. Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area μS*min	Rel. Area %
1	4.25	Fluoride	n.a.	4.5224		2.86855	10.01
2	7.12	Chloride	n.a.	15.3139		7.40574	25.84
3	9.08	Nitrate-N	n.a.	4.6616		4.32829	15.10
4	10.48	Chlorate	n.a.	2.5114		0.39239	1.37
5	11.36	Bromide	n.a.	2.5615		0.42996	1.50
6	13.27	Nitrate-N	n.a.	4.5667		5.17054	18.04
7	18.37	O-Phosphate-P	n.a.	2.0973		0.66866	2.33
8	20.59	Sulfate	n.a.	22.0533		7.39198	25.80
Total:				58.2880	0.000	28.856	100.00

31 1202063612/962078/1/1/MSD


Sample Name:	1202063612/962078/1/1/MSD	Injection Volume:	1.0
Vial Number:	18	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100311an	Sample Amount:	1.0000
Recording Time:	3/21/2010 19:36	Analyst:	MAR1
Run Time (min):	24.00	Column:	AS23-001528; GL GCED86;300;0056

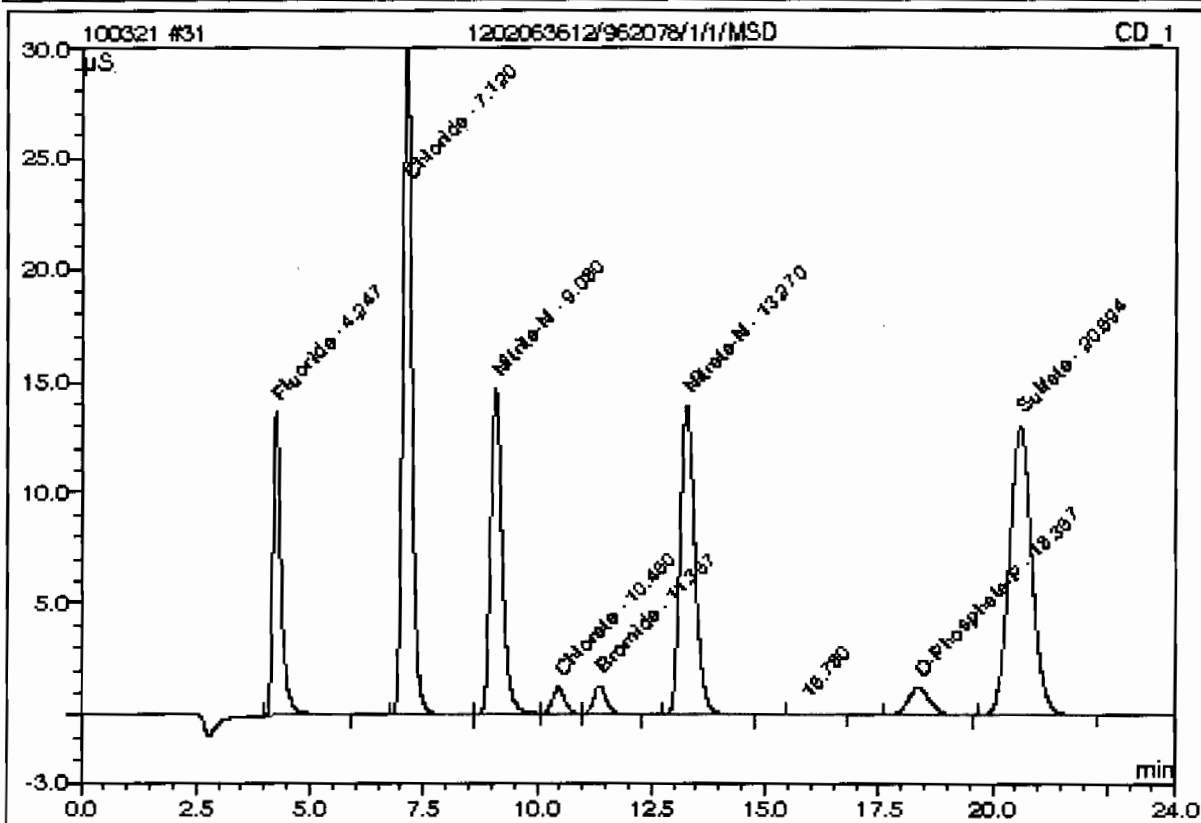

No.	Ret. Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area μS*min	Rel. Area %
1	4.25	Fluoride	n.a.	4.5127		2.86229	9.96
2	7.12	Chloride	n.a.	15.3448		7.42071	25.82
3	9.08	Nitrite-N	n.a.	4.6800		4.34569	15.12
4	10.48	Chlorate	n.a.	2.4932		0.38950	1.36
5	11.36	Bromide	n.a.	2.5637		0.43034	1.50
6	13.27	Nitrate-N	n.a.	4.5787		5.18456	18.04
8	18.37	O-Phosphate-P	n.a.	2.1274		0.67858	2.36
9	20.59	Sulfate	n.a.	22.0554		7.39267	25.72
Total:				58.3556	0.000	28.704	99.86

32 WIC100321-02CCV


Sample Name:	WIC100321-02CCV	Injection Volume:	1.0
Vial Number:	19	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100311an	Sample Amount:	1.0000
Recording Time:	3/21/2010 20:03	Analyst:	MAR1
Run Time (min):	24.00	Column:	AS23-001528; GL GC E086;300;9056

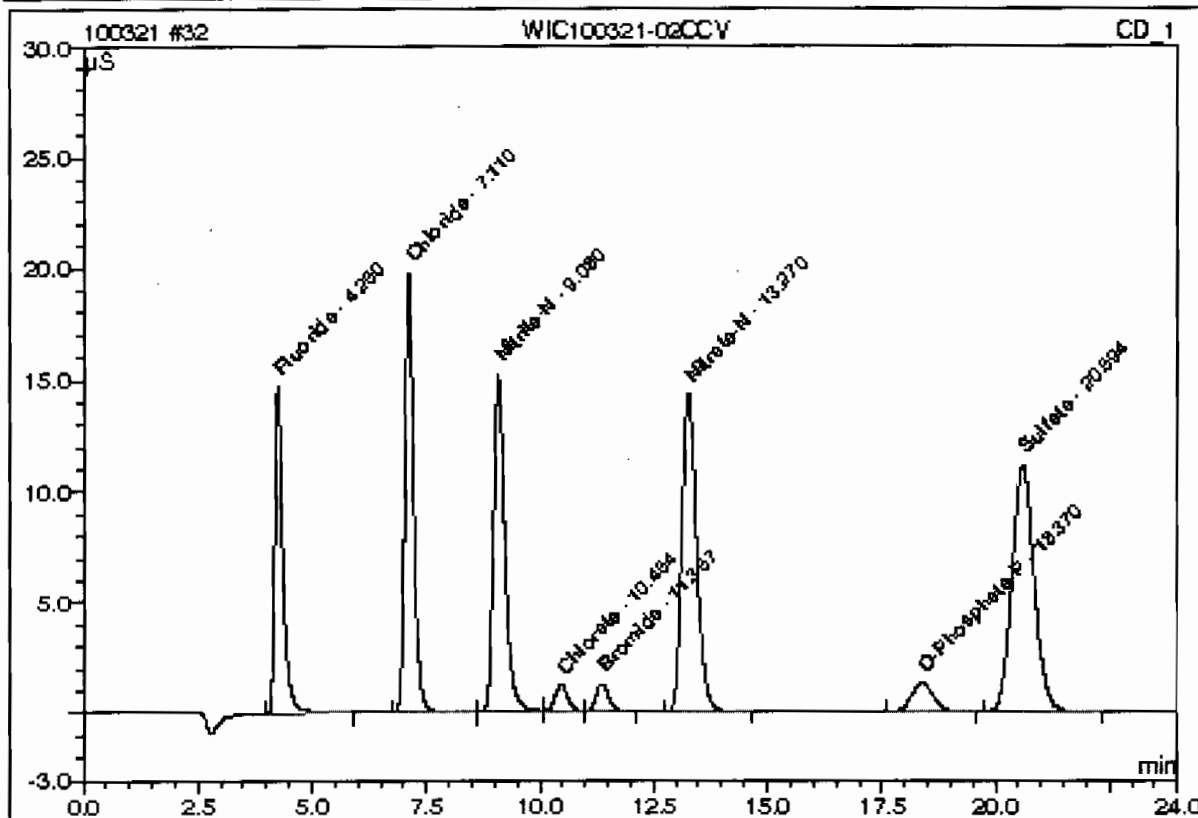

No.	Ret.Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area μS*min	Rel.Area %
1	4.25	Fluoride	n.a.	4.8444		3.07550	12.18
2	7.11	Chloride	n.a.	9.3012		4.46730	17.69
3	9.08	Nitrate-N	n.a.	4.8256		4.48329	17.75
4	10.46	Chlorate	n.a.	2.5695		0.40158	1.59
5	11.36	Bromide	n.a.	2.5245		0.42371	1.68
6	13.27	Nitrate-N	n.a.	4.7008		5.32661	21.09
7	18.37	O-Phosphate-P	n.a.	2.3245		0.74351	2.94
8	20.59	Sulfate	n.a.	18.9499		6.33585	25.09
Total:				50.0406	0.000	25.257	100.00

33 CCB


Sample Name:	CCB	Injection Volume:	1.0
Vial Number:	20	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100311an	Sample Amount:	1.0000
Recording Time:	3/21/2010 20:30	Analyst:	MAR1
Run Time (min):	24.00	Column:	AS23-001528; GL GCE086;300;9056

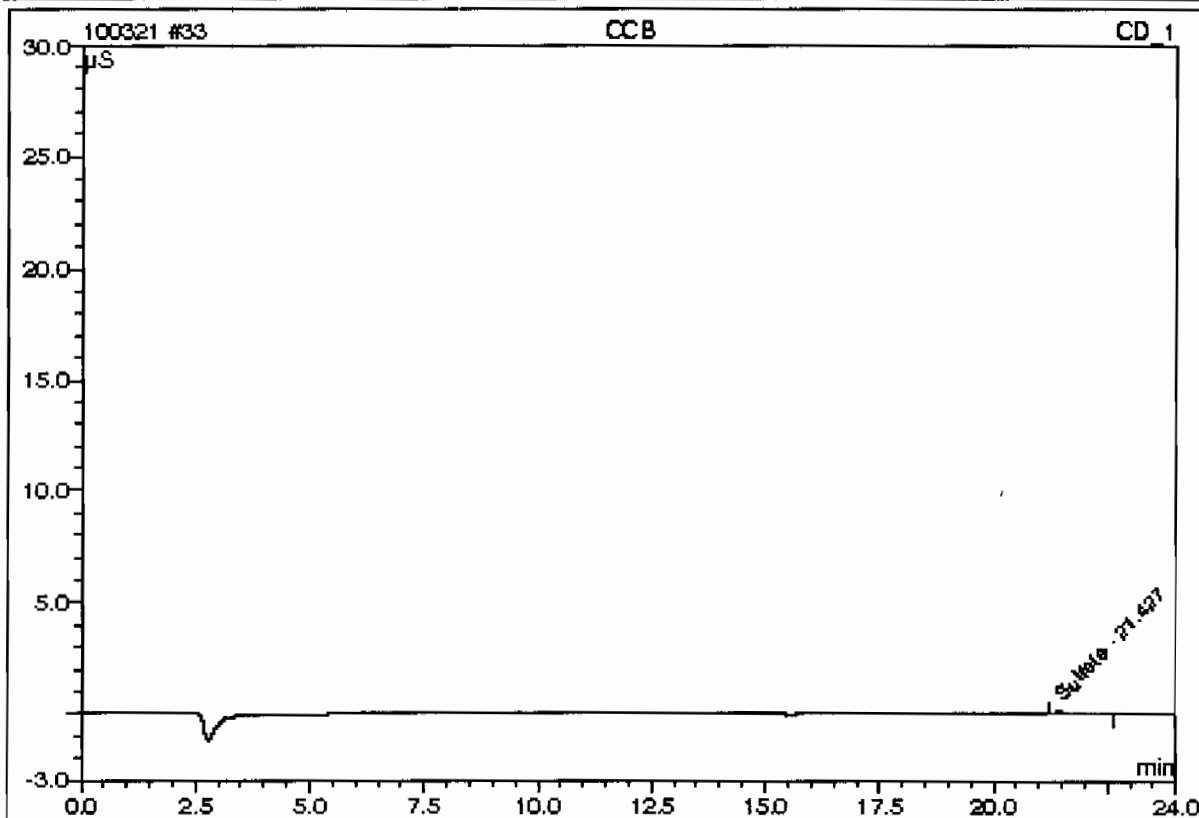

No.	Ret. Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area µS*min	Rel. Area %
n.a.	n.a.	Fluoride	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Chloride	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Nitrite-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Chlorate	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Bromide	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Nitrate-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	O-Phosphate-P	n.a.	n.a.	n.a.	n.a.	n.a.
1	21.43	Sulfate	n.a.	0.4804		0.05046	100.00
Total:				0.4804	0.000	0.050	100.00

33 CCB

Sample Name:	CCB	Injection Volume:	1.0
Vial Number:	20	Channel:	CD_1
Sample Type:	unknown	Dilution Factor:	1.0000
Control Program:	AS23	Sample Weight:	1.0000
Quantif. Method:	100311an	Sample Amount:	1.0000
Recording Time:	3/21/2010 20:30	Analyst:	MAR1
Run Time (min):	24.00	Column:	AS23-001528; GL GCE086;300;0056

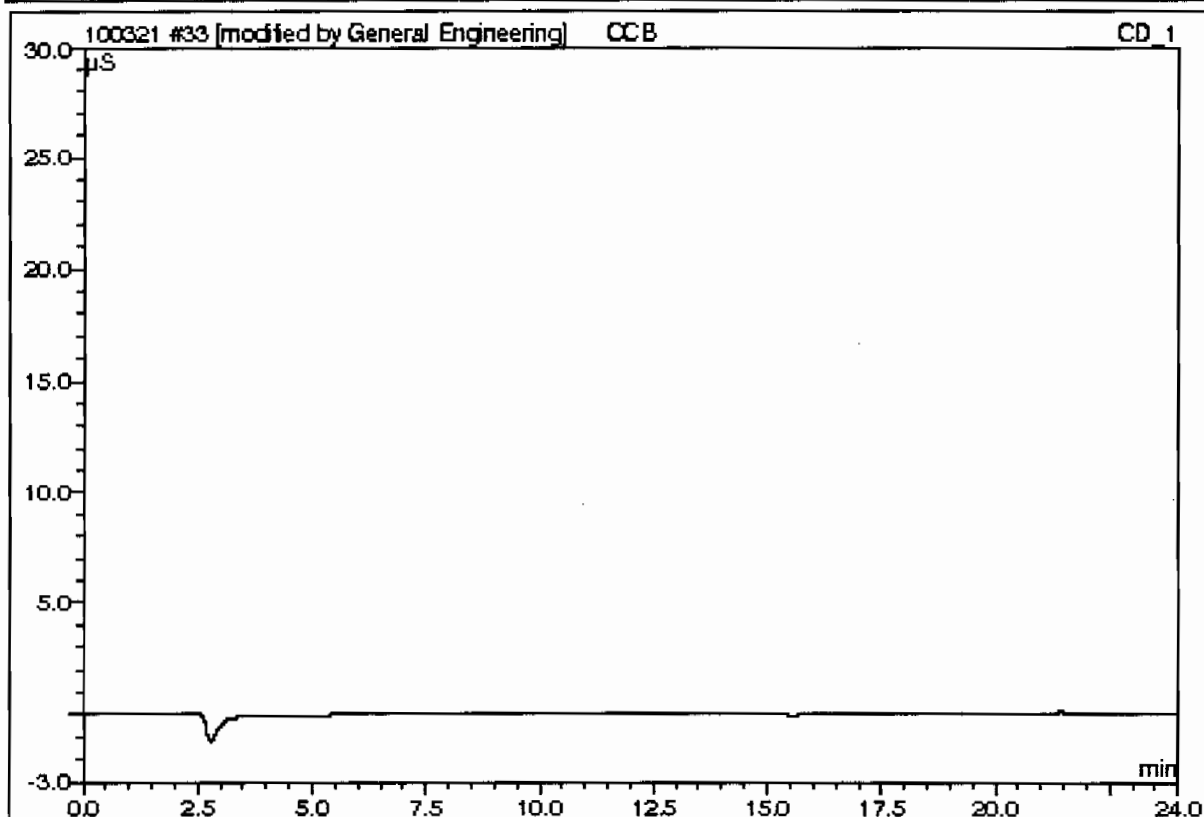

No.	Ret. Time min	Peak Name	Concentration mg/L	Amount mg/L	Modified?	Area µS*min	Rel. Area %
n.a.	n.a.	Fluoride	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Chloride	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Nitrite-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Chlorate	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Bromide	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Nitrate-N	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	O-Phosphate-P	n.a.	n.a.	n.a.	n.a.	n.a.
n.a.	n.a.	Sulfate	n.a.	n.a.	n.a.	n.a.	n.a.
Total:				0.0000	0.000	0.000	0.00

pH

pH / Corrosivity LogBook

Analyst: LXA1
 Batch: 959805
 Lab SOP: GL-GC-E-008 REV# 17
 Description: pH
 Method: SW846 9045C/9045D

Sample id	Parent Sample Id	Matrix	Start Time	Stop Time	Run Date	Parname	Initial W(g)	Final Vol(mL)	Ph	Temp	Nc(mg/L)	Recovery(%)	Rpd(%)
1202058595 LCS		Soil	11:10	11:15	02-MAR-10 12:50	pH	20	20	6.99	20.4°C	7	99.857	
1202058595 LCS		Soil	11:10	11:15	02-MAR-10 12:50	pH 2	20	20	6.99	20.4°C	7	99.857	
248025003		Soil	11:10	11:15	02-MAR-10 12:50	pH	20	20	9.77	20.4°C			
248025003		Soil	11:10	11:15	02-MAR-10 12:50	pH 2	20	20	9.77	20.4°C			
248025004		Soil	11:10	11:15	02-MAR-10 12:50	pH	20	20	9.76	20.0°C			
248025004		Soil	11:10	11:15	02-MAR-10 12:50	pH 2	20	20	9.76	20.0°C			
1202058593 DUP	248025004	Soil	11:10	11:15	02-MAR-10 12:50	pH	20	20	9.73	19.8°C			.308
1202058593 DUP	248025004	Soil	11:10	11:15	02-MAR-10 12:50	pH 2	20	20	9.72	19.9°C			.411
248025005		Soil	11:10	11:15	02-MAR-10 12:50	pH	20	20	9.82	19.8°C			
248025005		Soil	11:10	11:15	02-MAR-10 12:50	pH 2	20	20	9.82	19.8°C			
CCV			11:10	11:15	02-MAR-10 12:50	pH	20	20	7.02	19.4°C	7	100.286	
CCV			11:10	11:15	02-MAR-10 12:50	pH 2	20	20	7.02	19.4°C	7	100.286	
248025006		Soil	11:10	11:15	02-MAR-10 12:50	pH	20	20	8.22	19.7°C			
248025006		Soil	11:10	11:15	02-MAR-10 12:50	pH 2	20	20	8.22	19.7°C			
248025007		Soil	11:10	11:15	02-MAR-10 12:50	pH	20	20	11.93	19.5°C			
248025007		Soil	11:10	11:15	02-MAR-10 12:50	pH 2	20	20	11.93	19.5°C			
248110001		Soil	11:10	11:15	02-MAR-10 12:50	pH	20	20	8.61	19.3°C			
248110001		Soil	11:10	11:15	02-MAR-10 12:50	pH 2	20	20	8.59	19.3°C			
248110002		Soil	11:10	11:15	02-MAR-10 12:50	pH	20	20	8.41	19.4°C			
248110002		Soil	11:10	11:15	02-MAR-10 12:50	pH 2	20	20	8.41	19.4°C			
248110003		Soil	11:10	11:15	02-MAR-10 12:50	pH	20	20	8.8	19.3°C			
248110003		Soil	11:10	11:15	02-MAR-10 12:50	pH 2	20	20	8.79	19.3°C			
CCV			11:10	11:15	02-MAR-10 12:50	pH	20	20	7.01	19.2°C	7	100.143	
CCV			11:10	11:15	02-MAR-10 12:50	pH 2	20	20	7.01	19.2°C	7	100.143	
248110004		Soil	11:10	11:15	02-MAR-10 12:50	pH	20	20	9.09	19.4°C			
248110004		Soil	11:10	11:15	02-MAR-10 12:50	pH 2	20	20	9.09	19.4°C			
248110005		Soil	11:10	11:15	02-MAR-10 12:50	pH	20	20	8.32	19.3°C			
248110005		Soil	11:10	11:15	02-MAR-10 12:50	pH 2	20	20	8.32	19.3°C			

GEL Laboratories LLC

Page# _____

pH / Corrosivity LogBook

Analyst: LXA1
 Batch: 959805
 Lab SOP: GL-GC-E-008 REV# 17
 Description: pH
 Method: SW846 9045C/9045D

Description
 PH 7 BUFFER FOR PH
 LCS BUFFER SOLUTION

Type Sample Id Serial Number
 CCV 240 IMM091029-PH
 LCS 1202058595 IMM100209-01

Sample id	Parent Sample Id	Matrix	Start Time	Stop Time	Run Date	Paramname	Initial Wt(g)	Final Vol(mL)	Ph	Temp	Nc(mg/L)	Recovery(%)	Rpd(%)
248110006		Soil	11:10	11:15	02-MAR-10 12:50	pH	20	20	8.91	19.2°C			
248110006		Soil	11:10	11:15	02-MAR-10 12:50	pH 2	20	20	8.89	19.2°C			
248110007		Soil	11:10	11:15	02-MAR-10 12:50	pH	20	20	8.59	19.2°C			
248110007		Soil	11:10	11:15	02-MAR-10 12:50	pH 2	20	20	8.59	19.2°C			
248110008		Soil	11:10	11:15	02-MAR-10 12:50	pH	20	20	8.67	19.1°C			
248110008		Soil	11:10	11:15	02-MAR-10 12:50	pH 2	20	20	8.66	19.1°C			
CCV			11:10	11:15	02-MAR-10 12:50	pH	20	20	7.02	19.2°C	7	100.286	
CCV			11:10	11:15	02-MAR-10 12:50	pH 2	20	20	7.01	19.2°C	7	100.143	
1202058594 DUP	248110008	Soil	11:10	11:15	02-MAR-10 12:50	pH	20	20	8.57	19.7°C			1.16
1202058594 DUP	248110008	Soil	11:10	11:15	02-MAR-10 12:50	pH 2	20	20	8.57	19.7°C			1.045
248118001		Soil	11:10	11:15	02-MAR-10 12:50	pH	20	20	8.45	19.8°C			
248118001		Soil	11:10	11:15	02-MAR-10 12:50	pH 2	20	20	8.45	19.8°C			
248118002		Soil	11:10	11:15	02-MAR-10 12:50	pH	20	20	8.26	19.7°C			
248118002		Soil	11:10	11:15	02-MAR-10 12:50	pH 2	20	20	8.26	19.7°C			
248118003		Soil	11:10	11:15	02-MAR-10 12:50	pH	20	20	7.92	20.0°C			
248118003		Soil	11:10	11:15	02-MAR-10 12:50	pH 2	20	20	7.92	20.0°C			
248118004		Soil	11:10	11:15	02-MAR-10 12:50	pH	20	20	8.07	19.9°C			
248118004		Soil	11:10	11:15	02-MAR-10 12:50	pH 2	20	20	8.07	19.9°C			
CCV			11:10	11:15	02-MAR-10 12:50	pH	20	20	7.01	19.6°C	7	100.143	
CCV			11:10	11:15	02-MAR-10 12:50	pH 2	20	20	7.01	19.6°C	7	100.143	
248118005		Soil	11:10	11:15	02-MAR-10 12:50	pH	20	20	8.62	20.0°C			
248118005		Soil	11:10	11:15	02-MAR-10 12:50	pH 2	20	20	8.62	20.0°C			
248118006		Soil	11:10	11:15	02-MAR-10 12:52	pH	20	20	8.6	20.1°C			
248118006		Soil	11:10	11:15	02-MAR-10 12:52	pH 2	20	20	8.6	20.1°C			
248118007		Soil	11:10	11:15	02-MAR-10 12:53	pH	20	20	8.23	20.1°C			
248118007		Soil	11:10	11:15	02-MAR-10 12:53	pH 2	20	20	8.23	20.1°C			
CCV			11:10	11:15	02-MAR-10 12:55	pH	20	20	7.02	20.0°C	7	100.286	
CCV			11:10	11:15	02-MAR-10 12:55	pH 2	20	20	7.02	20.0°C	7	100.286	

GEL Laboratories LLC

Page#

pH / Corrosivity LogBook

Calibration Information:

Run Date: 02-MAR-10 11:20
Instrument: PHX370
Analyst: LXA1

Comments:

Standard	Observed	Theoretical	C	%Recovery
11:20 IMM100302-PH1	4.01	4 SU	20.4	100.25
11:20 IMM100302-PH2	7.02	7 SU	20.4	100.29
11:20 UPH100302-PH3	10.01	10 SU	20.4	100.1
11:20 UPH100302-PH4	2.04	2 SU	20.4	102
11:20 UPH100302-PH5	12.01	12 SU	20.4	100.08
11:20 IMM100302-PH6	7.02	7 SU	20.4	100.29

Miscellaneous

DATA EXCEPTION REPORT

Mo. Day Yr.
23-MAR-10

Division:
Industrial

Quality Criteria:
Specifications

Type:
Process

Instrument Type:
IC

Test / Method:
EPA 300.0

Matrix Type:
Solid

Client Code:
LANL

Batch ID:
962078

Sample Numbers:
See Below

Potentially affected work order(s)(SDG): 248110(10-2090-1), 248118(10-2093-1)

Application Issues:

Failed Recovery for MS/PS

Container scanning event for custody missed

Failed Recovery for MSD/PSD

**Specification and Requirements
Exception Description:**

DER Disposition:

1. Failed Recovery for MS/MSD:

QC 1202063609MS, 1202063611MSD

2. Container scanning event for custody missed:

248110 001,002,003,004,005,006,007,008

248118 001,002,003,004,005,006,007

1. The spike recovery falls outside of the GEL acceptance limits but within the client specified limits.

2. The following samples were not scanned to batch prior to initial run. However, the samples were in the custody of analyst during analysis.

Originator's Name:

Mary Sherwood 23-MAR-10

Data Validator/Group Leader:

Elzbieta Szulc 24-MAR-10